





TEST SETUP PHOTOGRAPHS





| | | | | | |
|--------------------------------------|---|---|--|---|---------------------------------|
| FCC ID: S8QEC-S10 |  PCTEST ENGINEERING LABORATORY, INC. | FCC Pt. 15C / RSS-210 MEASUREMENT REPORT (CERTIFICATION) | |  OLYMPUS "See More. See Better." | Reviewed by: Quality Manager |
| Test Report S/N: 0Y1105100855.S8Q | Test Dates: May 10, 2011 | EUT Type: Olympus Capsule Endoscope System | | | Page 1 of 5 |







| | | | | | |
|---|---|---|--|---|--|
| FCC ID: S8QEC-S10 |  PCTEST ENGINEERING LABORATORY, INC. | FCC Pt. 15C / RSS-210 MEASUREMENT REPORT (CERTIFICATION) | |  OLYMPUS "See More. See Future." | Reviewed by: Quality Manager |
| Test Report S/N: 0Y1105100855.S8Q | Test Dates: May 10, 2011 | EUT Type: Olympus Capsule Endoscope System | | | Page 2 of 5 |




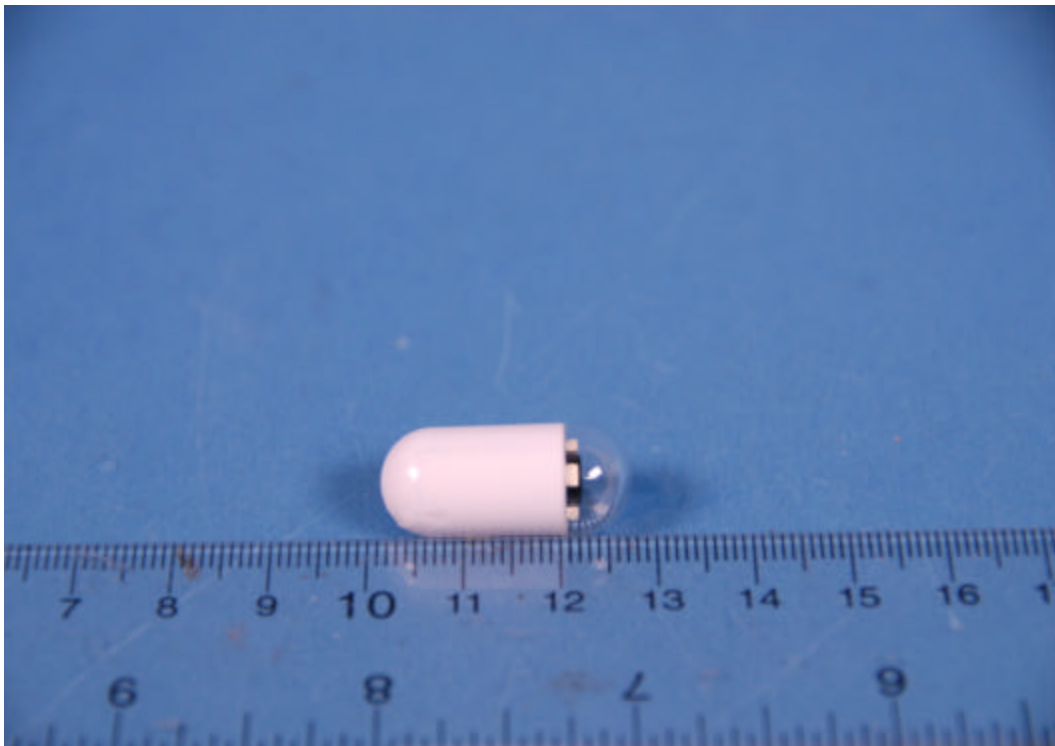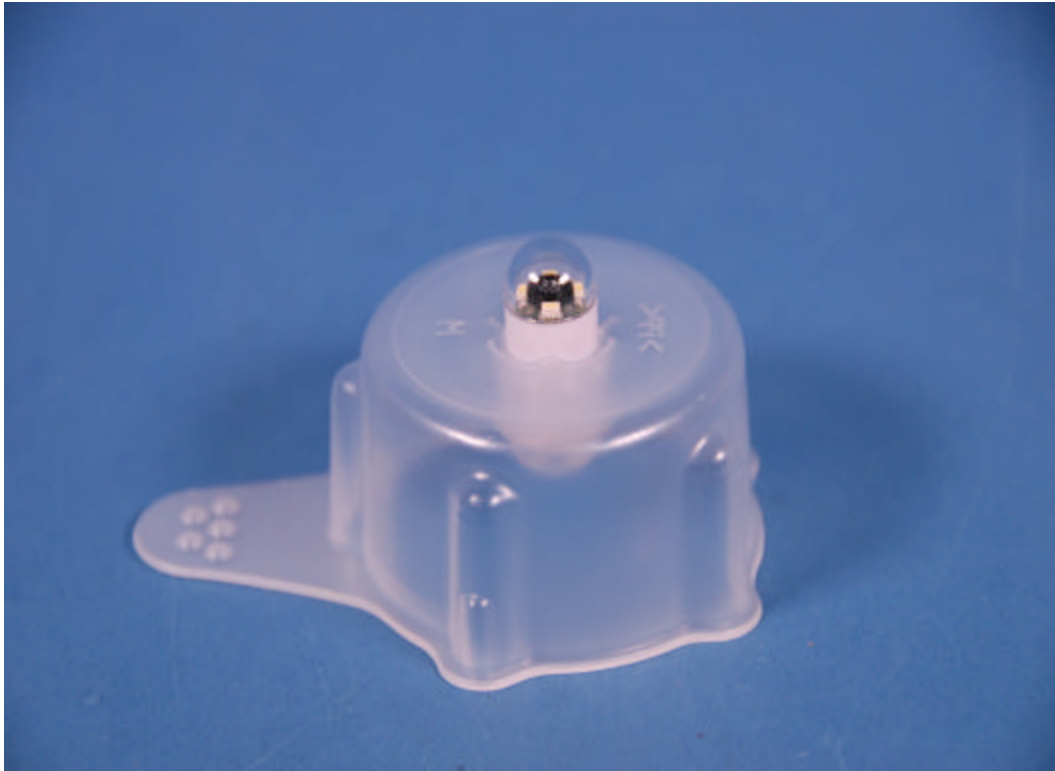

| | | | | | |
|--------------------------------------|---|---|--|---|---------------------------------|
| FCC ID: S8QEC-S10 |  PCTEST ENGINEERING LABORATORY, INC. | FCC Pt. 15C / RSS-210 MEASUREMENT REPORT (CERTIFICATION) | |  OLYMPUS "See More. See Future." | Reviewed by: Quality Manager |
| Test Report S/N: 0Y1105100855.S8Q | Test Dates: May 10, 2011 | EUT Type: Olympus Capsule Endoscope System | | | Page 3 of 5 |

1.0 EUT PHOTOGRAPHS

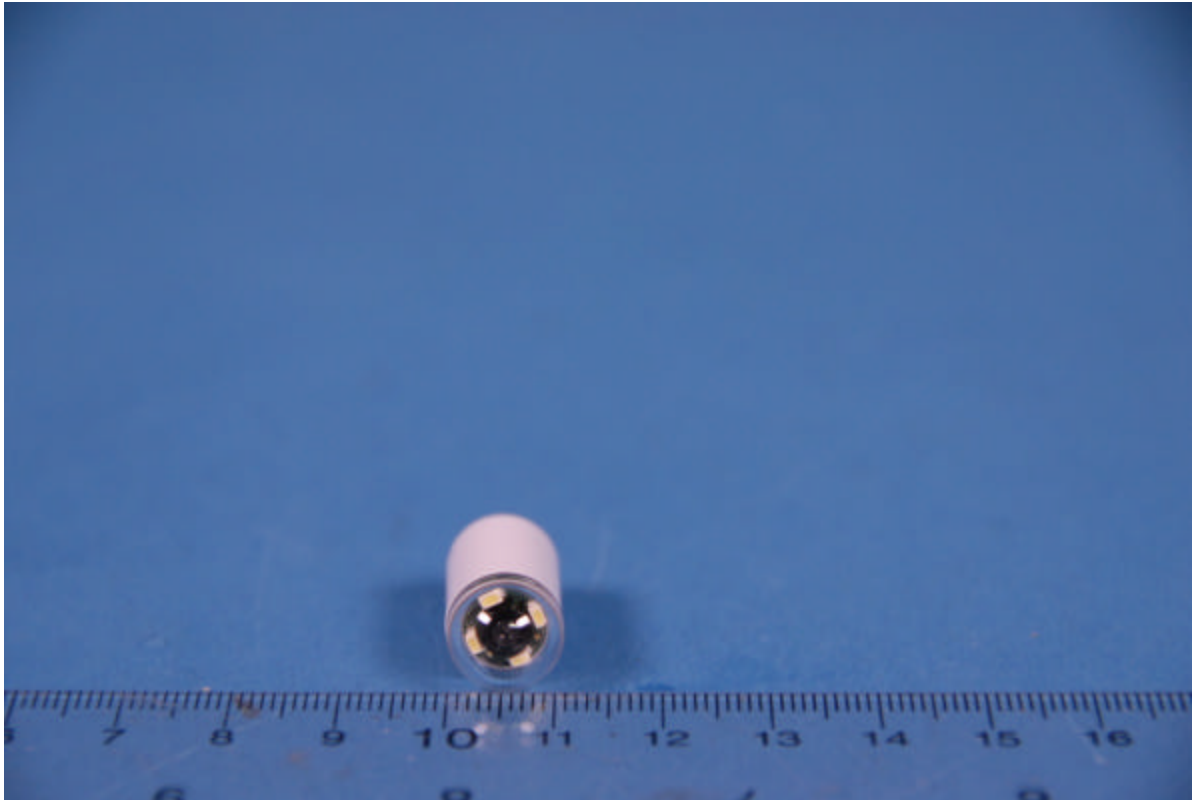

| | | | | |
|--------------------------------------|---|---|---|---------------------------------|
| FCC ID: S8QEC-S10 |  PCTEST ENGINEERING LABORATORY, INC. | FCC Pt. 15C / RSS-210 MEASUREMENT REPORT (CERTIFICATION) |  OLYMPUS "See Vision. See Future." | Reviewed by: Quality Manager |
| Test Report S/N: 0Y1105100855.S8Q | Test Dates: May 10, 2011 | EUT Type: Olympus Capsule Endoscope System | Page 4 of 5 | |



| | | | | | |
|--------------------------------------|---|---|--|---|---------------------------------|
| FCC ID: S8QEC-S10 |  PCTEST ENGINEERING LABORATORY, INC. | FCC Pt. 15C / RSS-210 MEASUREMENT REPORT (CERTIFICATION) | |  OLYMPUS "See More. See Future." | Reviewed by: Quality Manager |
| Test Report S/N: 0Y1105100855.S8Q | Test Dates: May 10, 2011 | EUT Type: Olympus Capsule Endoscope System | | | Page 5 of 5 |