



Valued Quality. Delivered.

Report No.: 17031394HKG-001
Page 1 of 41

Specific Absorption Rate (SAR) Evaluation Report

For

Watch Walkie Talkie

Model Number: 2720022
Brand Name: Watch WalkieTalkie

FCC ID: SF8KDWT2017

Prepared for

King Da Plastic Electronic Ltd.
No.49 Pu Xia Road, Heng Gang Jie Dao,
Long Gang Qu, Shenzhen City, China.

Prepared and Checked by:

Approved by:

Chan Chun Foo, Bike
Senior Lead Engineer
Date: May 12, 2017

Chan Chi Hung, Terry
Assistant Manager
Date: May 12, 2017

- Intertek's standard Terms and Conditions can be obtained at our website: <http://www.intertek.com/terms/>.
- This report shall not be reproduced, except in full.
- Only the original copy of this report is valid.
- This report is for the exclusive use of Intertek's Client and is provided pursuant to the agreement between Intertek and its Client. Intertek's responsibility and liability are limited to the terms and conditions of the agreement. Intertek assumes no liability to any party, other than to the Client in accordance with the agreement, for any loss, expense or damage occasioned by the use of this report. Only the Client is authorized to permit copying or distribution of this report and then only in its entirety. Any use of the Intertek name or one of its marks for the sale or advertisement of the tested material, product or service must first be approved in writing by Intertek. The observations and test results in this report are relevant only to the sample tested. This report by itself does not imply that the material, product, or service is or has ever been under an Intertek certification program.
- © 2016 Intertek

Intertek Testing Services Hong Kong Ltd.

2/F., Garment Centre, 576 Castle Peak Road, Kowloon, Hong Kong.
Tel: (852) 2173 8888 Fax: (852) 2785 5487 Website: www.hk.intertek-etlsemko.com



Valued Quality. Delivered.

Report No.: 17031394HKG-001
Page 2 of 41

Table of Contents

| | |
|---|----|
| 1 Test Result Summary..... | 3 |
| 2 General Information..... | 4 |
| 3 SAR Measurement System Description..... | 7 |
| 4 Tissue Verificaiton | 16 |
| 5 SAR Measurement System Verification..... | 19 |
| 6 SAR Evaluation | 21 |
| 7 Test Equipment List..... | 32 |
| 8 Measurement Uncertainty | 33 |
| 9 E-Field Probe and Dipole Antenna Calibration | 33 |
| APPENDIX A – System Check Data..... | 34 |
| APPENDIX B – SAR Evaluation Data..... | 36 |
| APPENDIX C – E-Field Probe and Dipole Antenna Calibration | 40 |
| APPENDIX D – SAR System Validation | 41 |



Valued Quality. Delivered.

1. Test Result Summary

| | |
|--------------------------|--|
| Applicant | : King Da Plastic Electronic Ltd. |
| Applicant Address | : No.49 Pu Xia Road, Heng Gang Jie Dao, Long Gang Qu, Shenzhen City, China. |
| Model | : 2720022 |
| Brand Name | : Watch WalkieTalkie |
| Serial Number | : N/A |
| FCC ID | : SF8KDWT2017 |
| Test Device | : Production Unit |
| Exposure Category | : General Population/Uncontrolled Exposure |
| Date of Test | : April 21, 2017 to April 24, 2017 |
| Place of Testing | : Intertek Testing Services Hong Kong Unit 3, G/F, World-Wide Industrial Centre, 43-47 Shan Mei Street, Fo Tan, Sha Tin. |
| Environmental Conditions | : Temperature: +18 to 25°C Humidity 25 to 75% |
| Test Specification | : ANSI/IEEE C95.1 IEEE Std 1528: 2013 FCC KDB Publication 447498 D01 v06 FCC KDB Publication 865664 D01 v01r04 FCC KDB Publication 865664 D02 v01r02 |

The maximum spatial peak SAR value for the sample device averaged over 1g was found to be:

| Band | Operating Mode | TX Frequency (MHz) | Highest Reported SAR | |
|------|----------------|---------------------|----------------------|--------------------------|
| | | | 1g Next to mouth | 10g extremity Wrist-Worn |
| GMRS | Voice | 462.5625 – 462.7125 | 0.034 W/kg | 0.030 W/kg |

This wireless portable device has been shown to be capable of compliance for localized specific absorption rate (SAR) for uncontrolled environment / general population exposure limits specified in ANSI/IEEE C95.1.



Valued Quality. Delivered.


Report No.: 17031394HKG-001
Page 4 of 41

2. General Information

2.1. Description of Equipment under test (EUT)

| | |
|-----------------------------------|---|
| Manufacturer | : King Da Plastic Electronic Ltd. |
| Manufacturer Address | : No.49 Pu Xia Road, Heng Gang Jie Dao, Long Gang Qu, Shenzhen City, China. |
| Device dimension (L x W) | : 250 (mm) x 48 (mm) |
| Device thickness | : 33 (mm) |
| Antenna Gain | : +2.05 dBi |
| Operating Configuration(s) / mode | : Next to mouth (Voice call) Wrist-worn (Voice call) |
| Tx Frequency | : 462.5625 MHz to 462.7125 MHz |
| Duty Cycle | : 100% |
| H/W Version | : N/A |
| S/W Version | : N/A |
| Battery Type | : 3 x 1.5 V AAA Alkaline Battery |
| Body-worn Accessories | : N/A |

2.2. EUT Antenna Locations

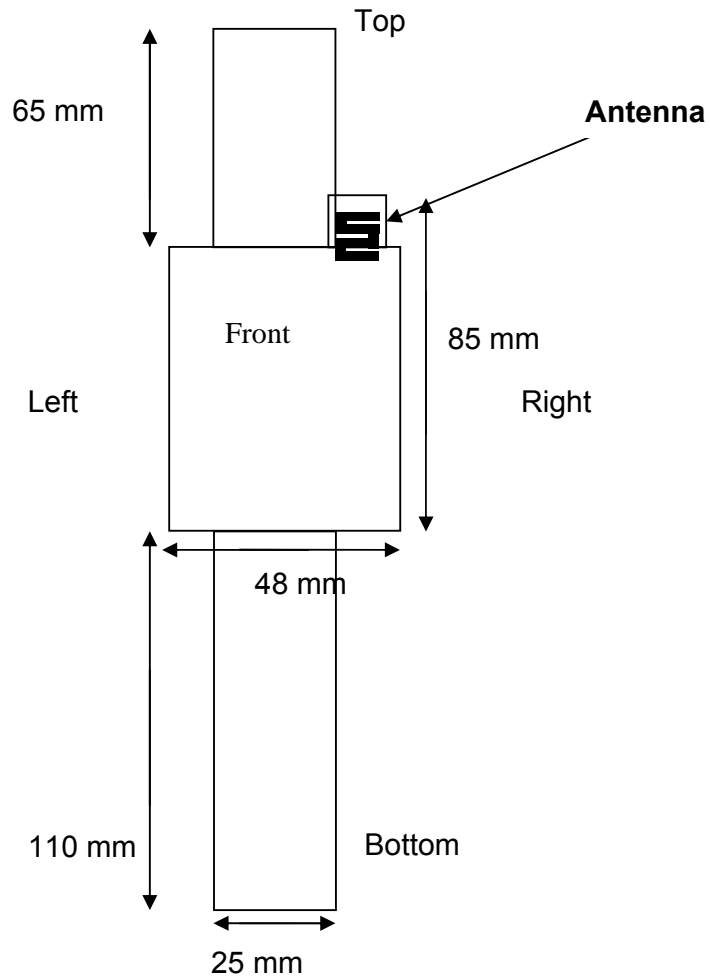

Details of antenna specification are shown in separate antenna dimension document.



Valued Quality. Delivered.

Report No.: 17031394HKG-001
Page 6 of 41

2.3. Nominal and Maximum Output Power Specifications

The EUT operates using the following maximum and nominal output power specifications. SAR values were scaled to the maximum allowed power to determine compliance per KDB Publication 447498.

| Band | Operating Mode | TX Frequency (MHz) | Output Power | |
|------|----------------|---------------------|--------------|---------|
| | | | Nominal | Maximum |
| GMRS | Voice | 462.5625 - 462.7125 | 7 dBm | 9 dBm |

3. SAR Measurement System Description

SAR is related to the rate at which energy is absorbed per unit mass in object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and occupational/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of given mass density (ρ). The equation description is as below:

$$SAR = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dV} \right)$$

SAR is expressed in units of Watts per kilogram (W/Kg)
SAR can be obtained using either of the following equations:

$$SAR = \frac{\sigma E^2}{\rho}$$

$$SAR = c_h \left. \frac{dT}{dt} \right|_{t=0}$$

Where

SAR is the specific absorption rate in watts per kilogram;
E is the r.m.s. value of the electric field strength in the tissue in volts per meter;
 σ is the conductivity of the tissue in siemens per metre;
 ρ is the density of the tissue in kilograms per cubic metre;
 c_h is the heat capacity of the tissue in joules per kilogram and Kelvin;

$\left. \frac{dT}{dt} \right|_{t=0}$ is the initial time derivative of temperature in the tissue in kelvins per second

An SAR measurement system usually consists of a small diameter isotropic electric field probe, a multiple axis probe positioning system, a test device holder, one or more phantom models, the field probe instrumentation, a computer and other electronic equipment for controlling the probe and making the measurements. Other supporting equipment, such as a network analyzer, power meters and RF signal generators, are also required to measure the dielectric parameters of the simulated tissue media and to verify the measurement accuracy of the SAR system.

The SAR measurement system being used is COMOSAR system, which consists following items for performing compliance tests

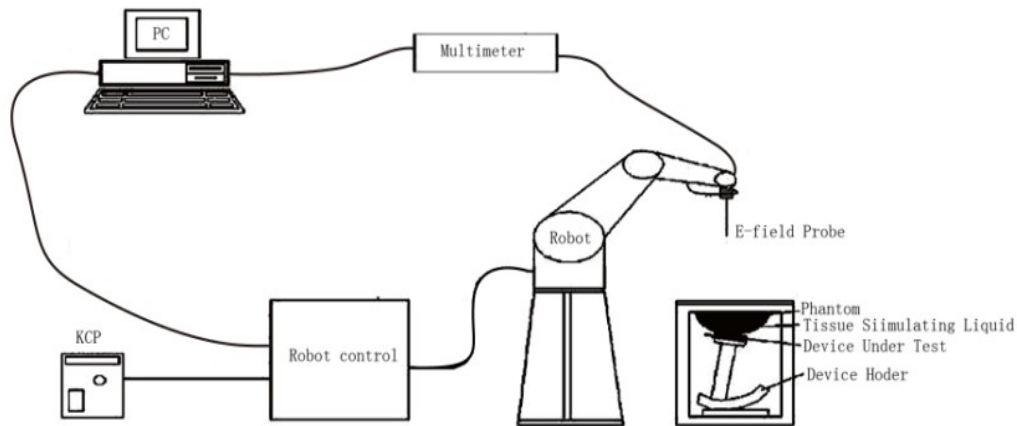


Figure 1: Schematic diagram of the SAR measurement system

- The PC. It controls most of the bench devices and stores measurement data. A computer running WinXP and the Opensar software
- The E-Field probe. The probe is a 3-axis system made of 3 distinct dipoles. Each dipole returns a voltage in function of the ambient electric field.
- The Keithley multimeter measures each probe dipole voltages.
- The SAM phantom simulates a human head. The measurement of the electric field is made inside the phantom.
- The liquids simulate the dielectric properties of the human head tissues
- The network emulator controls the mobile phone under test.
- The validation dipoles are used to measure a reference SAR. They are used to periodically check the bench to make sure that there is no drift of the system characteristics over time.
- The phantom, the device holder and other accessories according to the targeted measurement.

Robot

The COMOSAR system uses the KUKA robot from SATIMO SA (France). For the 6-axis controller COMOSAR system, the KUKA robot controller version from SATIMO is used.


The XL robot series have many features that are important for our application:

- High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- 6-axis controller



COMOSAR E-Field Probe

The SAR measurement is conducted with the dissymmetric probe manufactured by SATIMO. The probe is specially designed and calibrated for use in liquid with high permittivity. The dissymmetric probe has special calibration in liquid at different frequency. SATIMO conducts the probe calibration in compliance with international and national standards (e.g. IEEE Std 1528-2013 and relevant KDB files). The calibration data are in Appendix C.


| | | |
|----------------------|---|--|
| Model | SSE2 | |
| Manufacture | MVG | |
| Frequency | 0.45GHz-6GHz Linearity:±0.08dB |  |
| Dynamic Range | 0.01W/Kg-100W/Kg Linearity:±0.08dB | |
| Dimensions | Overall length:330mm Length of individual dipoles:2mm Maximum external diameter:8mm Probe Tip external diameter:2.5mm Distance between dipoles/ probe extremity:1mm | |

Video Positioning System

The video positioning system is used in OpenSAR to check the probe. Which is composed of a camera, LED, mirror and mechanical parts. The camera is piloted by the main computer with firewire link.

During the process, the actual position of the probe tip with respect to the robot arm is measured, as well as the probe length and the horizontal probe offset. The software then corrects all movements, such that the robot coordinates are valid for the probe tip.

The repeatability of this process is better than 0.1 mm. If a position has been taught with an aligned probe, the same position will be reached with another aligned probe within 0.1 mm, even if the other probe has different dimensions. During probe rotations, the probe tip will keep its actual position.

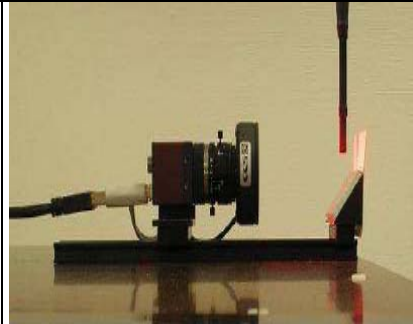

SAM Twin Phantom

The SAM twin phantom is a fiberglass shell phantom with $2\text{mm} \pm 0.2\text{ mm}$ shell thickness (except the ear region where shell thickness increases to $6\text{mm} \pm 0.2\text{ mm}$), relative permittivity $\epsilon_r = 3.4$ and loss tangent $\delta = 0.02$. It has three measurement areas:

- Left head
- Right head
- Flat phantom



The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

Elliptical Phantom

The elliptical phantom is a fiberglass shell phantom with

- $2\text{mm} \pm 0.2\text{ mm}$ shell thickness
- relative permittivity $\epsilon_r = 3.4$
- loss tangent $\delta = 0.02$




Device Holder

The COMOSAR device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation center for both scales is the ear reference point (EPR).

Thus the device needs no repositioning when changing the angles.

The COMOSAR device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity $\epsilon_r = 3.7$ and loss tangent $\delta = 0.005$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.

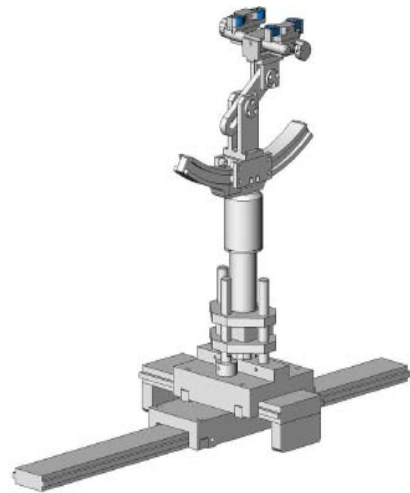

During measurement, the system first does an area (2D) scan at a fixed depth within the liquid from the inside wall of the phantom scanning area is greater than the projection of EUT and antenna.

Area Scan Parameters extracted from KDB 865664

| | ≤ 3 GHz | > 3 GHz |
|--|---|---|
| Maximum distance from closest measurement point (geometric center of probe sensors) to phantom surface | 5 mm ± 1 mm | $\frac{1}{2} \cdot \delta \cdot \ln(2)$ mm ± 0.5 mm |
| Maximum probe angle from probe axis to phantom surface normal at the measurement location | 30° ± 1° | 20° ± 1° |
| Maximum area scan spatial resolution: Δx_{Area} , Δy_{Area} | ≤ 2 GHz: ≤ 15 mm 2 – 3 GHz: ≤ 12 mm | 3 – 4 GHz: ≤ 12 mm 4 – 6 GHz: ≤ 10 mm |
| | When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be ≤ the corresponding x or y dimension of the test device with at least one measurement point on the test device. | |

When the maximum SAR point has been found, the system will then carry out a zoom (3D) scan centered at that point to determine volume averaged SAR level.

Zoom Scan Parameters extracted from KDB 865664

| | | | |
|--|------------------------------------|--|---|
| Maximum zoom scan spatial resolution: $\Delta x_{Zoom}, \Delta y_{Zoom}$ | | ≤ 2 GHz: ≤ 8 mm 2 – 3 GHz: ≤ 5 mm* | 3 – 4 GHz: ≤ 5 mm* 4 – 6 GHz: ≤ 4 mm* |
| Maximum zoom scan spatial resolution, normal to phantom surface | uniform grid: $\Delta z_{Zoom}(n)$ | ≤ 5 mm | 3 – 4 GHz: ≤ 4 mm 4 – 5 GHz: ≤ 3 mm 5 – 6 GHz: ≤ 2 mm |
| | graded grid | $\Delta z_{Zoom}(1)$: between 1 st two points closest to phantom surface | ≤ 4 mm |
| | | $\Delta z_{Zoom}(n>1)$: between subsequent points | $\leq 1.5 \cdot \Delta z_{Zoom}(n-1)$ mm |
| Minimum zoom scan volume | x, y, z | ≥ 30 mm | 3 – 4 GHz: ≥ 28 mm 4 – 5 GHz: ≥ 25 mm 5 – 6 GHz: ≥ 22 mm |
| <p>Note: δ is the penetration depth of a plane-wave at normal incidence to the tissue medium; see IEEE Std 1528-2013 for details.</p> <p>* When zoom scan is required and the <i>reported</i> SAR from the <i>area scan based 1-g SAR estimation</i> procedures of KDB Publication 447498 is ≤ 1.4 W/kg, ≤ 8 mm, ≤ 7 mm and ≤ 5 mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.</p> | | | |

4. Tissue Verification

For SAR measurement of field distribution inside phantom, homogeneous tissue simulating liquid as below liquid recipes were filled to a depth of 15cm ± 0.5cm for below 3GHz measurement and of 10cm ± 0.5cm for above 3GHz.

Head Tissue Recipes

| Frequency | Ingredients | | | | | |
|-----------|------------------|------|-----------------|-------|-------|-------------|
| | De-ionized Water | Salt | 1,2 propanediol | DGBE | DGMH | Triton X100 |
| 450 MHz | 33.5% | 3.4% | 63.1% | | | |
| 750 MHz | 34.2% | 1.4% | 64.4% | | | |
| 900 MHz | 35.3% | 1.0% | 63.7% | | | |
| 1800 MHz | 55.2% | 0.6% | | 13.8% | | 30.4% |
| 1900 MHz | 55.3% | 0.5% | | 13.8% | | 30.4% |
| 2000 MHz | 55.3% | 0.4% | | 13.8% | | 30.5% |
| 2450 MHz | 55.7% | 0.3% | | 18.7% | | 25.3% |
| 5000 MHz | 65.3% | | | | 17.2% | 17.5% |

Body Tissue Recipes

| Frequency | Ingredients | | | | | |
|-----------|------------------|------|-----------------|------|-------|-------------|
| | De-ionized Water | Salt | 1,2 propanediol | DGBE | DGMH | Triton X100 |
| 450 MHz | 52.4% | 1.9% | 45.7% | | | |
| 750 MHz | 55.4% | 1.3% | 43.3% | | | |
| 900 MHz | 52.9% | 1.0% | 46.1% | | | |
| 1800 MHz | 70.8% | 0.5% | | 8.7% | | 20.0% |
| 1900 MHz | 70.1% | 0.4% | | 8.9% | | 20.6% |
| 2000 MHz | 70.2% | 0.3% | | 8.6% | | 20.9% |
| 2450 MHz | 70.8% | 0.3% | | 8.7% | | 20.2% |
| 5000 MHz | 77.8% | | | | 11.7% | 11.5% |

The head tissue dielectric parameters recommended by the IEEE Std 1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in a human head. For other head and body tissue parameters, they are recommended by KDB 865664.

| Target Frequency | head | | body | |
|------------------|--------------|----------------|--------------|----------------|
| | ϵ_r | σ (S/m) | ϵ_r | σ (S/m) |
| 300 | 45.3 | 0.87 | 58.2 | 0.92 |
| 450 | 43.5 | 0.87 | 56.7 | 0.94 |
| 835 | 41.5 | 0.90 | 55.2 | 0.97 |
| 900 | 41.5 | 0.97 | 55.0 | 1.05 |
| 915 | 41.5 | 1.01 | 55.0 | 1.06 |
| 1450 | 40.5 | 1.20 | 54.0 | 1.30 |
| 1610 | 40.3 | 1.29 | 53.8 | 1.40 |
| 1800 – 2000 | 40.0 | 1.40 | 53.3 | 1.52 |
| 2450 | 39.2 | 1.80 | 52.7 | 1.95 |
| 3000 | 38.5 | 2.40 | 52.0 | 2.73 |
| 5800 | 35.3 | 5.27 | 48.2 | 6.00 |

(ϵ_r = relative permittivity, σ = conductivity and $\rho = 1000$ kg/m³)

When a transmission band overlaps with one of the target frequencies, the tissue dielectric parameters of the tissue medium at the middle of a device transmission band should be within $\pm 5\%$ of the parameters specified at that target frequency.



Valued Quality. Delivered.

Report No.: 17031394HKG-001
Page 18 of 41

The dielectric parameters of the liquids were verified prior to the SAR evaluation using SATIMO Dielectric Probe Kit and R&S Network Analyzer ZVL6.

The dielectric parameters were:

Head Liquid

| Freq. (MHz) | Temp. (°C) | ϵ_r / Relative Permittivity | | | σ / Conductivity | | | ρ^{**} (kg/m ³) |
|-------------|------------|--------------------------------------|---------|------------------------|-------------------------|---------|------------------------|----------------------------------|
| | | measured | Target* | Δ ($\pm 5\%$) | measured | Target* | Δ ($\pm 5\%$) | |
| 450 | 20.5 | 43.94 | 43.50 | 1.01 | 0.88 | 0.87 | 1.15 | 1000 |
| 460 | 20.5 | 42.69 | 43.50 | -1.86 | 0.85 | 0.87 | -2.30 | 1000 |

* Target values refer to KDB 865664

** Worst-case assumption

Note:

1. Date of tissue verification measurement: April 21, 2017
2. Ambient temperature: 21.0 deg C
3. The temperature condition is within +/- 2 deg. C during the SAR measurements.

Body Liquid

| Freq. (MHz) | Temp. (°C) | ϵ_r / Relative Permittivity | | | σ / Conductivity | | | ρ^{**} (kg/m ³) |
|-------------|------------|--------------------------------------|---------|------------------------|-------------------------|---------|------------------------|----------------------------------|
| | | measured | Target* | Δ ($\pm 5\%$) | measured | Target* | Δ ($\pm 5\%$) | |
| 450 | 20.9 | 54.14 | 56.70 | -4.51 | 0.95 | 0.94 | 1.06 | 1000 |
| 460 | 20.9 | 56.44 | 56.70 | -0.46 | 0.92 | 0.94 | -2.13 | 1000 |

* Target values refer to KDB 865664

** Worst-case assumption


Note:

1. Date of tissue verification measurement: April 24, 2017
2. Ambient temperature: 21.5 deg C
3. The temperature condition is within +/- 2 deg. C during the SAR measurements.


5. SAR Measurement System Verification

Each SATIMO system is equipped with one or more system check kits. These units, together with the predefined measurement procedures within the SATIMO software, enable user to conduct the system check. System kit includes a dipole, and dipole device holder.

The system check verifies that the system operates within its specifications. It's performed daily or before every SAR measurement. The system check uses normal SAR measurement in the flat section of the phantom with a matched dipole at a specified distance. The system check setup is shown as below.

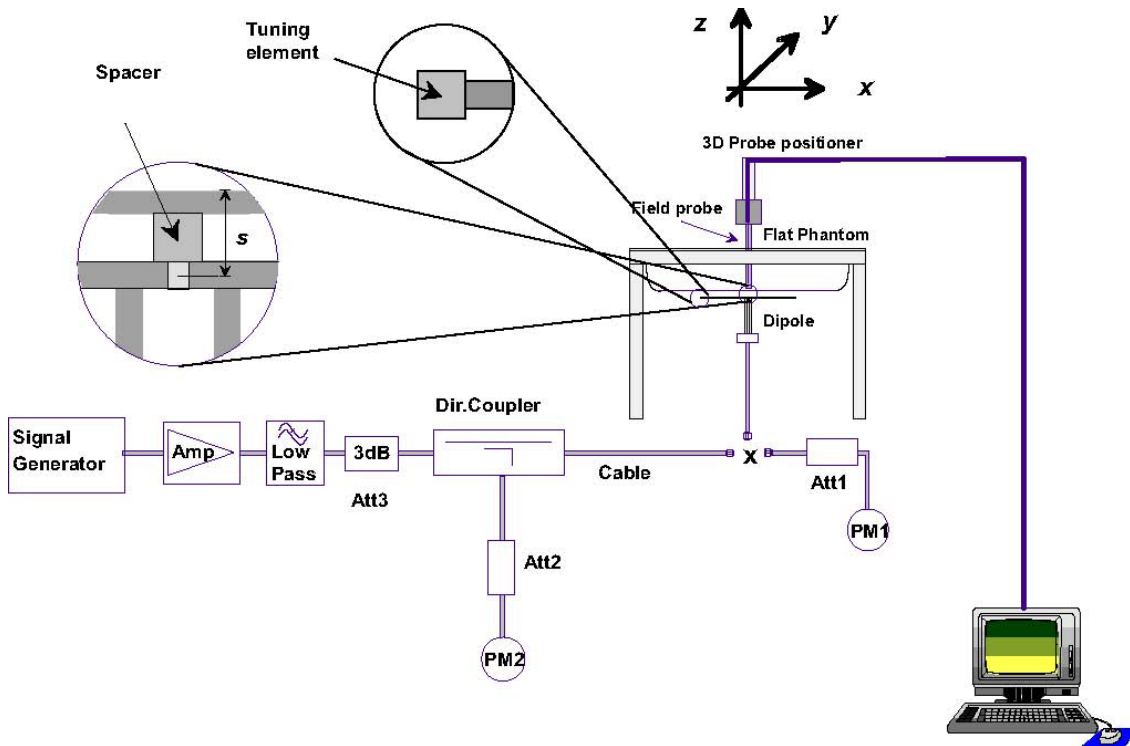

Validation Dipole

| | |
|---|---|
|  | <p>The dipoles used is based on the IEEE Std 1528, and is complied with mechanical and electrical specifications in line with the requirements of both FCC and KDB requirement.</p> |
|---|---|

System check results

| System Verification | | | | | | | | |
|---------------------|-------------|-------------|---------------|---------------------------|---------------------------------|-----------------------------------|-------------------------------------|------------------|
| Date | Freq. (MHz) | Liquid Type | System Diople | Serial No. | Target SAR _{1g} (W/kg) | Measured SAR _{1g} (W/kg) | Normalized SAR _{1g} (W/kg) | Deviation (±10%) |
| Apr 21, 2017 | 450 | Head | 450MHz | SN 26/16 DIP 0G450-420 | 4.77 | 0.470 | 4.70 | 1.47 |

* the target was quoted from dipole calibration report
* Input power level = 20dBm (0.1W)

SAR_{1g} ambient measured value < 12 mW/kg

| System Verification | | | | | | | | |
|---------------------|-------------|-------------|---------------|---------------------------|----------------------------------|------------------------------------|--------------------------------------|------------------|
| Date | Freq. (MHz) | Liquid Type | System Diople | Serial No. | Target SAR _{10g} (W/kg) | Measured SAR _{10g} (W/kg) | Normalized SAR _{10g} (W/kg) | Deviation (±10%) |
| Apr 24, 2017 | 450 | Body | 450MHz | SN 26/16 DIP 0G450-420 | 3.22 | 0.303 | 3.03 | -5.90 |

* the target was quoted from dipole calibration report
* Input power level = 20dBm (0.1W)

SAR_{10g} ambient measured value < 12 mW/kg

Details of System Verification plots are shown in the Appendix A - plot 1 and 2.



Valued Quality. Delivered.

Report No.: 17031394HKG-001
Page 21 of 41

6. SAR Evaluation


6.1. Device test positions relative to the head

This practice specifies two handset test positions against the head phantom—the “cheek” position and the “tilt” position. These two test positions are defined in the following subclauses. The handset should be tested in both positions on left and right sides of the SAM phantom. If handset construction is such that the handset positioning procedures described below to represent normal use conditions cannot be used, e.g., some asymmetric handsets, alternative alignment procedures should be adapted with all details provided in the test report. These alternative procedures should replicate intended use conditions as closely as possible according to the intent of the procedures described in this subclause.


Definition of the cheek position

The cheek position is established as follows:

1. Ready the handset for talk operation, if necessary. For example, for handsets with a cover piece (flip cover), open the cover. If the handset can transmit with the cover closed, both configurations must be tested.
2. Define two imaginary lines on the handset—the vertical centerline and the horizontal line. The vertical centerline passes through two points on the front side of the handset—the midpoint of the width w_t of the handset at the level of the acoustic output (point A in below figure), and the midpoint of the width w_b of the bottom of the handset (point B). The horizontal line is perpendicular to the vertical centerline and passes through the center of the acoustic output (see below left figure). The two lines intersect at point A. Note that for many handsets, point A coincides with the center of the acoustic output; however, the acoustic output may be located elsewhere on the horizontal line. Also note that the vertical centerline is not necessarily parallel to the front face of the handset (see right figure), especially for clamshell handsets, handsets with flip covers, and other irregularly-shaped handsets.
3. Position the handset close to the surface of the phantom such that point A is on the (virtual) extension of the line passing through points RE and LE on the phantom (see the figure as next page), such that the plane defined by the vertical centerline and the horizontal line of the handset is approximately parallel to the sagittal plane of the phantom.
4. Translate the handset towards the phantom along the line passing through RE and LE until handset point A touches the pinna at the ERP.

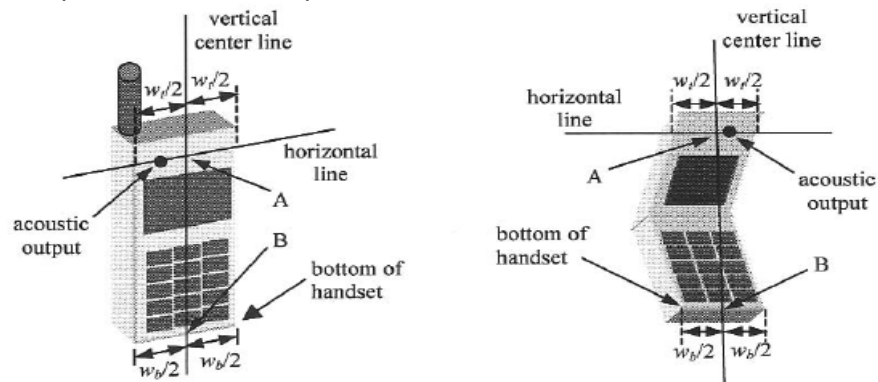


5. While maintaining the handset in this plane, rotate it around the LE-RE line until the vertical centerline is in the plane normal to the plane containing B-M and N-F lines, i.e., the Reference Plane.
6. Rotate the handset around the vertical centerline until the handset (horizontal line) is parallel to the N-F line.
7. While maintaining the vertical centerline in the Reference Plane, keeping point A on the line passing through RE and LE, and maintaining the handset contact with the pinna, rotate the handset about the N-F line until any point on the handset is in contact with a phantom point below the pinna on the cheek.

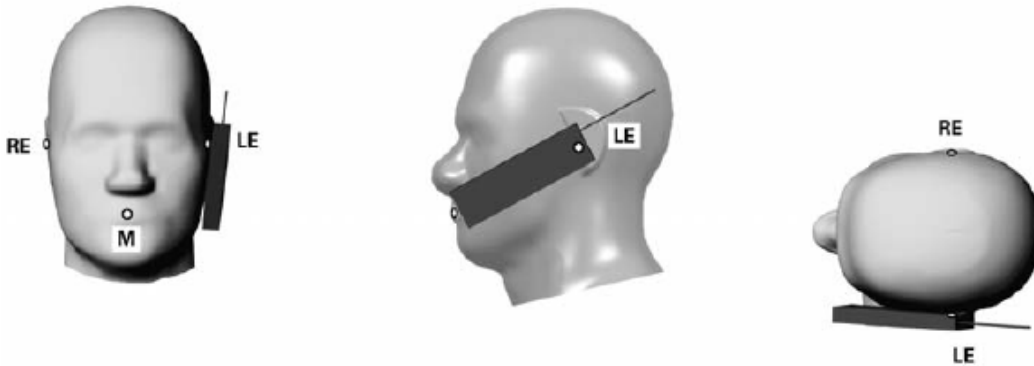

Definition of the tilt position

The tilt position is established as follows:

1. Repeat steps to place the device in the cheek position.
2. While maintaining the orientation of the handset, move the handset away from the pinna along the line passing through RE and LE far enough to allow a rotation of the handset away from the cheek by 15° .
3. Rotate the handset around the horizontal line by 15° .
4. While maintaining the orientation of the handset, move the handset towards the phantom on the line passing through RE and LE until any part of the handset touches the ear. The tilt position is obtained when the contact point is on the pinna. See the figure as below. If contact occurs at any location other than the pinna, e.g., the antenna at the back of the phantom head, the angle of the handset should be reduced.
5. In this case, the tilt position is obtained if any point on the handset is in contact with the pinna and a second point on the handset is in contact with the phantom, e.g., the antenna with the back of the head.

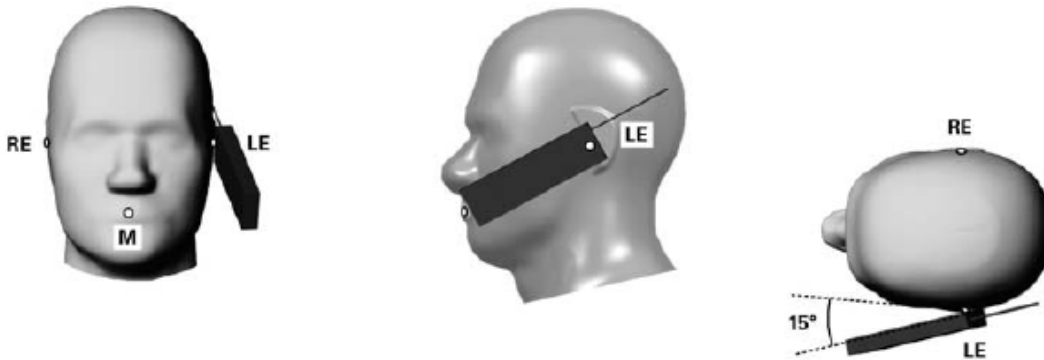

6.2. Device test positions relative to body-worn accessory

Body-worn operating configurations are tested with the belt-clips and holsters attached to the device and positioned against a flat phantom in a normal use configuration. Per FCC KDB Publication 648474, Body-worn accessory exposure is typically related to voice mode operations when handsets are carried in body worn accessories. The body-worn accessory procedures in FCC KDB Publication 447498 should be used to test for body-worn accessory SAR compliance, without a headset connected to it. This enables the test results for such configuration to be compatible with that required for hotspot mode when the body-worn accessory test separation distance is greater than or equal to that required for hotspot mode, when applicable. When the reported SAR for a body-worn accessory, measured without a headset connected to the handset, is $>1.2\text{W/kg}$, the highest reported SAR configuration for that wireless mode and frequency band should be reported for that body-worn accessory with a headset attached to the handset.


SAR evaluation is required for body-worn accessories supplied with the host device. The test configurations must be conservative for supporting the body-worn accessory use conditions expected by users. Body-worn accessories that do not contain metallic or conductive components may be tested according to worst-case exposure configurations, typically according to the smallest test separation distance required for the group of body-worn accessories with similar operating and exposure characteristics. All body-worn accessories containing metallic components, either supplied with the product or available as an option from the device manufacturer, must be tested in conjunction with the host device to demonstrate compliance

Body-worn accessories may not always be supplied or available as options for some devices intended to be authorized for body-worn use. In this case, a test configuration with a separation distance between the back of the device and the flat phantom is used. Test position spacing was documented. Transmitters that are designed to operate in front of a person's face, as in push-to-talk configurations, are tested for SAR compliance with the front of the device positioned to face the flat phantom in head fluid.

6.3. General Device Setup

The device was test in unmodulated continuous transmit operation (Continuous wave mode at 100% duty cycle) with the PTT transmit key constantly depressed.

During testing, the device was evaluated with a new alkaline battery, power saving function disabled and was configured to operate at maximum output power. A receive antenna and a spectrum analyzer were placed with a distance > 50cm away from the device to monitor the transmission states.

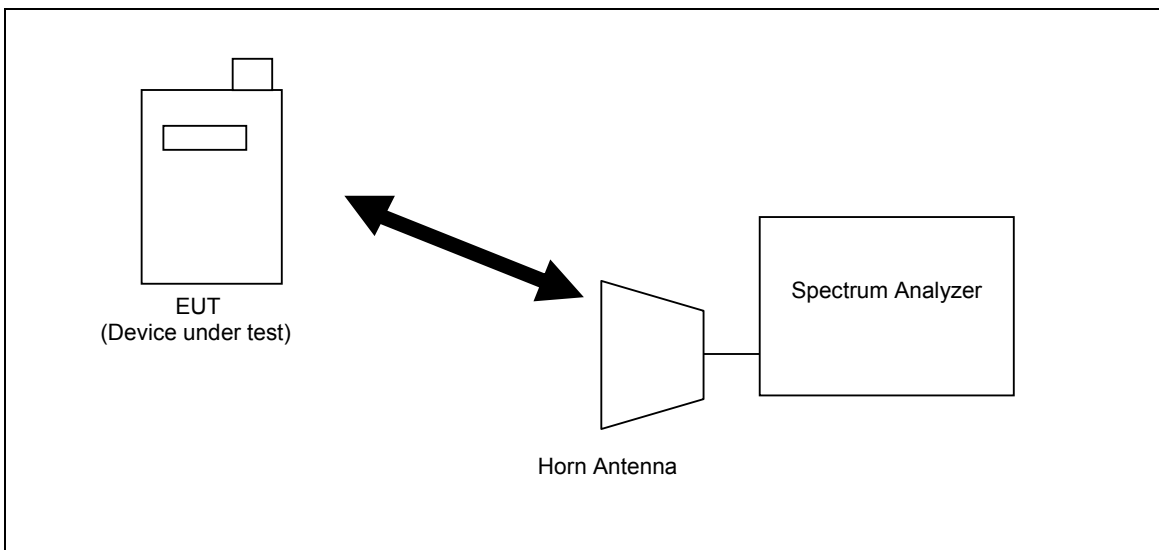

6.4. RF Output Power Measurements

| Channel | Frequency (MHz) | Measured Time-average Conducted Power (dBm) (100% Duty Cycle) |
|---------|-----------------|---|
| 1 | 462.5625 | 8.60 |
| 2 | 462.5875 | 8.60 |
| 3 | 462.6125 | 8.59 |
| 4 | 462.6375 | 8.60 |
| 5 | 462.6625 | 8.58 |
| 6 | 462.6875 | 8.58 |
| 7 | 462.7125 | 8.57 |

Note:

1. Time Average power (dBm) = Peak power (dBm) + Time Average factor.
2. Time Average factor = $10 \cdot \log(\text{duty cycle})$
3. Per KDB 447498, the tested device was within the specified tune-up tolerances range, but not more than 2dB lower than the maximum tune-up tolerance limit.
4. Per KDB 447498, when antenna port was not available on the device to support conducted power measurement and test software was used to establish transmitter power levels, the power level was verified separately according to design and component specifications and product development information specified by the manufacturer.

6.5. Exposure Conditions

Next to mouth Exposure Conditions

| Test Configurations | Distance to phantom | Operation Mode | SAR Required | Note |
|---------------------|---------------------|----------------|--------------|------|
| Front | 10 mm | Voice | Yes | |
| Front with earphone | 10 mm | Voice | Yes | |

Note:

1. Per KDB 447498 D01, next to the mouth use is evaluated with the front of the device positioned at 10mm from a flat phantom and the wrist bands should be strapped together.

Wrist-Worn Exposure Conditions

| Test Configurations | Distance to phantom | Operation Mode | SAR Required | Note |
|---------------------|---------------------|----------------|--------------|----------------------------|
| Back | 0 mm | Voice | Yes | Plastic wrist band removed |
| Back with earphone | 0 mm | Voice | Yes | Plastic wrist band removed |

Note:

1. Per KDB 447498 D01, wrist-worn exposure is evaluated with the back of the device positioned in direct contact against a flat phantom.
2. Per KDB 447498 D01, 10-g extremity SAR applied for wrist-worn condition.
3. Destructive modification on plastic wrist bands removal was applied in order to perform more conservative SAR measurement.



Valued Quality. Delivered.

Report No.: 17031394HKG-001
Page 29 of 41

6.6. Test Result

The results on the following page(s) were obtained when the device was tested in the condition described in this report. Detailed measurement data and plots, which reveal information about the location of the maximum SAR with respect to the device, are reported in Appendix B.

Next to mouth SAR

| Measurement Result | | | | | | | | | | | |
|--------------------|-------------|----------|-------|--------------------------|-----------------------------|----------------------|---------------|-----------------------------------|----------------|-----------------------------------|------|
| Chan | Freq. (MHz) | Battery | Mode | Test Position | Maximum Allowed Power (dBm) | Measured Power (dBm) | SAR Drift (%) | Measured SAR _{1g} (W/kg) | Scaling factor | Reported SAR _{1g} (W/kg) | Plot |
| 4 | 462.6375 | Alkaline | Voice | Front 10mm | 9 | 8.60 | -4.94 | 0.028 | 1.096 | 0.031 | 1 |
| 4 | 462.6375 | Alkaline | Voice | Front 10mm with earphone | 9 | 8.60 | -0.62 | 0.031 | 1.096 | 0.034 | 2 |

Note:

1. Brand new batteries were used at the beginning of each SAR measurement.
2. There was no power reduction used for any band/mode implemented in this device.
3. Reported SAR results were scaled to the maximum allowed power with the scaling factor equation $-10^{[(\text{Maximum power} - \text{measured power}) / 10]}$.
4. Per KDB 447498 D01, when the maximum output power variation across the required test channels was < 0.5 dB, measurement on middle channel was required.
5. Per KDB 447498 D01, next to the mouth use is evaluated with the front of the device positioned at 10 mm from a flat phantom filled with head tissue equivalent medium.
6. Per KDB 865664 D01, repeated measurement was not required when the original highest measured SAR was < 0.8 W/kg



Valued Quality. Delivered.

6.6 Test Result (Cont'd)

10g-extremity Wrist-Worn SAR

| Measurement Result | | | | | | | | | | | |
|--------------------|-------------|----------|-------|------------------------|-----------------------------|----------------------|---------------|------------------------------------|----------------|------------------------------------|------|
| Chan | Freq. (MHz) | Battery | Mode | Test Position | Maximum Allowed Power (dBm) | Measured Power (dBm) | SAR Drift (%) | Measured SAR _{10g} (W/kg) | Scaling factor | Reported SAR _{10g} (W/kg) | Plot |
| 4 | 462.6375 | Alkaline | Voice | Back 0mm | 9 | 8.60 | -1.81 | 0.024 | 1.096 | 0.026 | 3 |
| 4 | 462.6375 | Alkaline | Voice | Back 0mm with earphone | 9 | 8.60 | -4.02 | 0.027 | 1.096 | 0.030 | 4 |

Note:

1. Brand new batteries were used at the beginning of each SAR measurement.
2. There was no power reduction used for any band/mode implemented in this device.
3. Reported SAR results were scaled to the maximum allowed power with the scaling factor equation $-10^{[(\text{Maximum power} - \text{measured power}) / 10]}$.
4. Per KDB 447498 D01, when the maximum output power variation across the required test channels was < 0.5 dB, measurement on middle channel was required.
5. Per KDB 447498 D01, 10-g extremity SAR applied for wrist-worn condition.
6. Per KDB 865664 D01, repeated measurement was not required when the original highest measured SAR was < 0.8 W/kg.

6.7. SAR Limits

The following FCC limits (Std. C95.1-1992) for SAR apply to devices operate in General Population/Uncontrolled Exposure and Controlled environment:

General Population / Uncontrolled Environments:

Defined as location where there is the exposure of individuals who have no knowledge or control of their exposure.

| EXPOSURE (General Population/Uncontrolled Exposure environment) | SAR (W/kg) |
|--|---------------|
| Spatial Peak SAR (Head)* | 1.60 |
| Spatial Peak SAR (Partial Body)* | 1.60 |
| Spatial Peak SAR (Whole Body)* | 0.08 |
| Spatial Peak SAR (Hands / Wrists / Feet / Ankles)** | 4.00 |

Occupational / Controlled Environments:

Defined as location where there is the exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation)

| EXPOSURE (Occupational/Controlled Exposure environment) | SAR (W/kg) |
|--|---------------|
| Spatial Peak SAR (Head)* | 8.00 |
| Spatial Peak SAR (Partial Body)* | 8.00 |
| Spatial Peak SAR (Whole Body)* | 0.40 |
| Spatial Peak SAR (Hands / Wrists / Feet / Ankles)** | 20.00 |

Notes:

- * The Spatial Peak value of the SAR averaged over any 1 gram of tissue. (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time
- ** The Spatial Peak value of the SAR averaged over any 10 gram of tissue. (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time



Valued Quality. Delivered.

Report No.: 17031394HKG-001
Page 32 of 41

7. Test Equipment List

| Equipment | Registration No. | Manufacturer | Model No. | Calibration Date | Calibration Due Date |
|---------------------------------------|------------------|-----------------|---|--------------------|----------------------|
| SAR System | EW-3211 | MVG | SATIMO System (OpenSAR Software V4_02_34) | N/A | N/A |
| Phantom | EW-3211 | SATIMO | COMOSAR SAM PHANTOM | N/A | N/A |
| Digital Multimeter | EW-3206 | KEITHLEY | 2000 | 17 Aug, 2016 | 17 Aug, 2017 |
| SAR Probe | EW-3210 | MVG | SSE2 (SN 08/16 EPGO283) | 05 Jul, 2016 | 05 Jul, 2017 |
| SAR Dipole | EW-3212 | MVG | SN 26/16 DIP 0G450-420 | 05 Jul, 2016 | 05 Jul, 2019 |
| Dielectric Probe for SAR Test | EW-3213 | EW-3213 | Liquid Measurement Kit (SN 24/16 OCPG 76) | 05 Jul, 2016 | 05 Jul, 2017 |
| Head Liquid Tissue | N/A | MVG | Head Liquid 450MHz | Refer to Section 4 | |
| Body Liquid Tissue | N/A | MVG | Body Liquid 450MHz | Refer to Section 4 | |
| Network Analyzer | EW-3192 | Rhode & Schwarz | ZVL6 | 27 Jul, 2016 | 05 Jul, 2017 |
| Signal Generator (250kHz to 40GHz) | EW-1983 | AGILENTTECH | E8247C | 25 May, 2016 | 25 May, 2017 |
| Spectrum Analyzer | EW-2466 | ROHDESCHWARZ | FSP30 | 23 Dec, 2016 | 27 Nov, 2017 |
| Dual-directional coupler (0.1-2.0)GHz | EW-3189 | KEYSIGHT | 778D | 23 Aug, 2016 | 23 Aug, 2017 |
| RF Power Meter | EW-2270 | AGILENTTECH | N1911A | 08 Jan, 2017 | 08 Jan, 2018 |
| SAR RF Amplifier for SAR System | EW-3275 | SATIMO | MVG | 04 Jan, 2017 | 04 Jan, 2018 |



Valued Quality. Delivered.

Report No.: 17031394HKG-001
Page 33 of 41

8. Measurement Uncertainty

Per FCC KDB 865884, the extensive SAR measurement uncertainty analysis was not required when the highest measured SAR was $< 1.5\text{W/kg}$ for all frequency band.

9. E-Field Probe and Dipole Antenna Calibration


Probe calibration factors and dipole antenna calibration are included in Appendix C.

APPENDIX A – System Check Data

Plot #1

Operating Frequency : 450MHz
Test Date: 21 Apr 2017

| | |
|------------------------------------|---|
| Medium (Liquid Type) | : 450 Head |
| Relative permittivity ϵ_r | : 43.939 |
| Conductivity σ : | : 0.878 |
| Probe | : Model: SSE2; Serial No.: SN 08/16 EPGO283 |
| Crest factor | : 1.0 |
| Conversion Factor | : 1.51 |
| Area Scan | : dx=8mm, dy=8mm |
| Zoom Scan | : 5x5x7, dx=8mm dy=8mm dz=5mm |
| Phantom | : SAM phantom |
| Device Position | : Dipole |
| SAR Drift (%) | : 1.01% |
| Maximum location | : X=0.00, Y=7.00 |
| SAR Peak (W/kg) | : 0.72 W/kg |
| SAR 10g (W/kg) | : 0.310 W/kg |
| SAR 1g (W/kg) | : 0.470 W/kg |

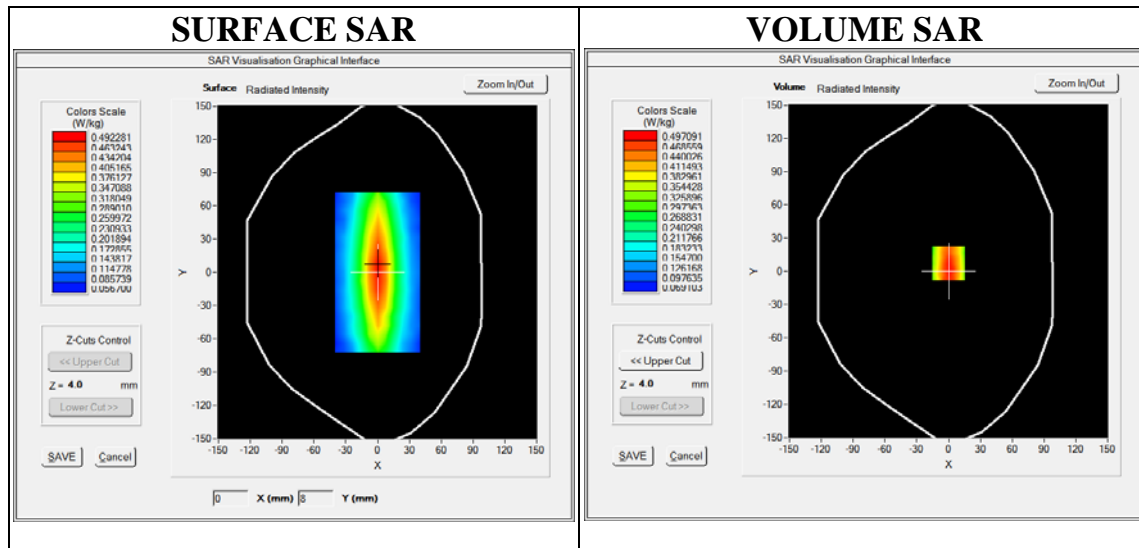


APPENDIX A – System Check Data (Cont'd)

Plot #2

Operating Frequency : 450MHz
Test Date: 24 Apr 2017

| | |
|------------------------------------|---|
| Medium (Liquid Type) | : 450 Body |
| Relative permittivity ϵ_r | : 54.139 |
| Conductivity σ : | : 0.955 |
| Probe | : Model: SSE2; Serial No.: SN 08/16 EPGO283 |
| Crest factor | : 1.0 |
| Conversion Factor | : 1.56 |
| Area Scan | : dx=8mm, dy=8mm |
| Zoom Scan | : 5x5x7, dx=8mm dy=8mm dz=5mm |
| Phantom | : SAM phantom |
| Device Position | : Dipole |
| SAR Drift (%) | : -4.32% |
| Maximum location | : X=1.00, Y=0.00 |
| SAR Peak (W/kg) | : 0.80 W/kg |
| SAR 10g (W/kg) | : 0.303 W/kg |
| SAR 1g (W/kg) | : 0.488 W/kg |

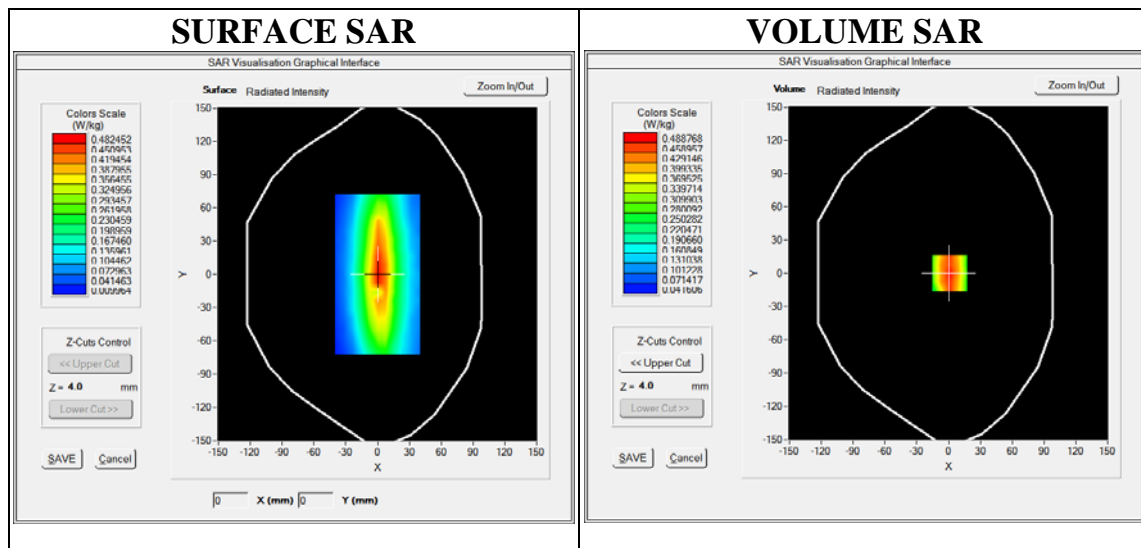


APPENDIX B – SAR Evaluation Data

Plot #1

Operating Frequency : 462.6375MHz
Product Description: Watch WalkieTalkie
Model: 2720022
Test Date: 21 Apr 2017

| | |
|------------------------------------|---|
| Medium (Liquid Type) | : 450 Head |
| Relative permittivity ϵ_r | : 42.693 |
| Conductivity σ : | : 0.846 |
| Probe | : Model: SSE2; Serial No.: SN 08/16 EPGO283 |
| Crest factor | : 1.00 |
| Conversion Factor | : 1.51 |
| Area Scan | : dx=8mm, dy=8mm |
| Zoom Scan | : 5x5x7,dx=8mm dy=8mm dz=5mm |
| Phantom | : SAM phantom |
| Device Position | : Front 10mm Separation |
| SAR Drift (%) | : -4.94% |
| Maximum location | : X=0.00, Y=10.00 |
| SAR Peak (W/kg) | : 0.06 W/kg |
| SAR 10g (W/kg) | : 0.019 W/kg |
| SAR 1g (W/kg) | : 0.028 W/kg |

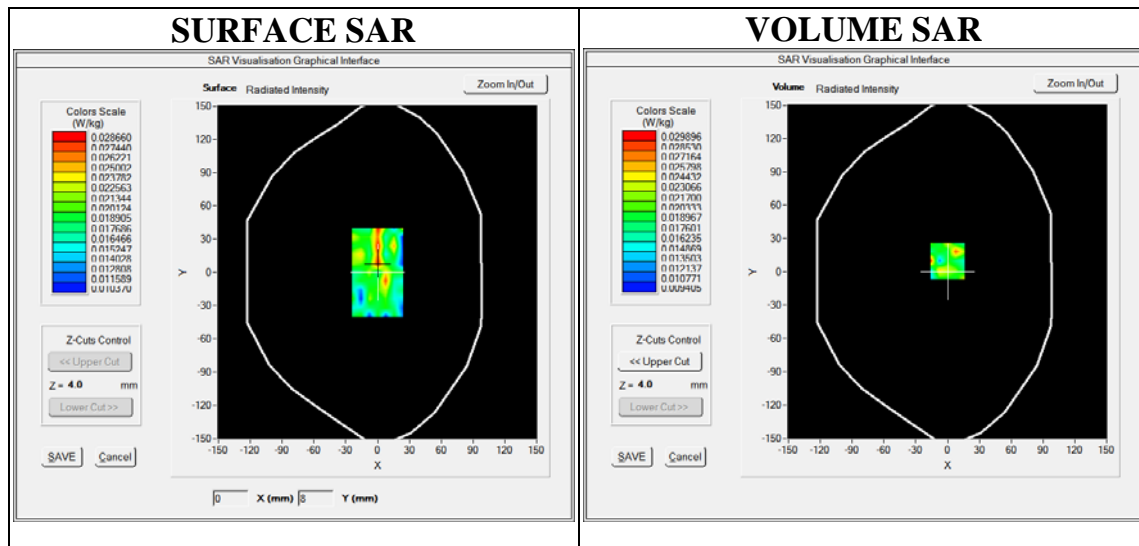


APPENDIX B – SAR Evaluation Data (Cont'd)

Plot #2

Operating Frequency : 462.6375MHz
Product Description: Watch WalkieTalkie
Model: 2720022
Test Date: 21 Apr 2017

| | |
|------------------------------------|---|
| Medium (Liquid Type) | : 450 Head |
| Relative permittivity ϵ_r | : 42.693 |
| Conductivity σ : | : 0.846 |
| Probe | : Model: SSE2; Serial No.: SN 08/16 EPGO283 |
| Crest factor | : 1.00 |
| Conversion Factor | : 1.51 |
| Area Scan | : dx=8mm, dy=8mm |
| Zoom Scan | : 5x5x7, dx=8mm dy=8mm dz=5mm |
| Phantom | : SAM phantom |
| Device Position | : Front 10mm Separation with earphone |
| SAR Drift (%) | : -0.62% |
| Maximum location | : X=8.00, Y=-9.00 |
| SAR Peak (W/kg) | : 0.07 W/kg |
| SAR 10g (W/kg) | : 0.021 W/kg |
| SAR 1g (W/kg) | : 0.031 W/kg |

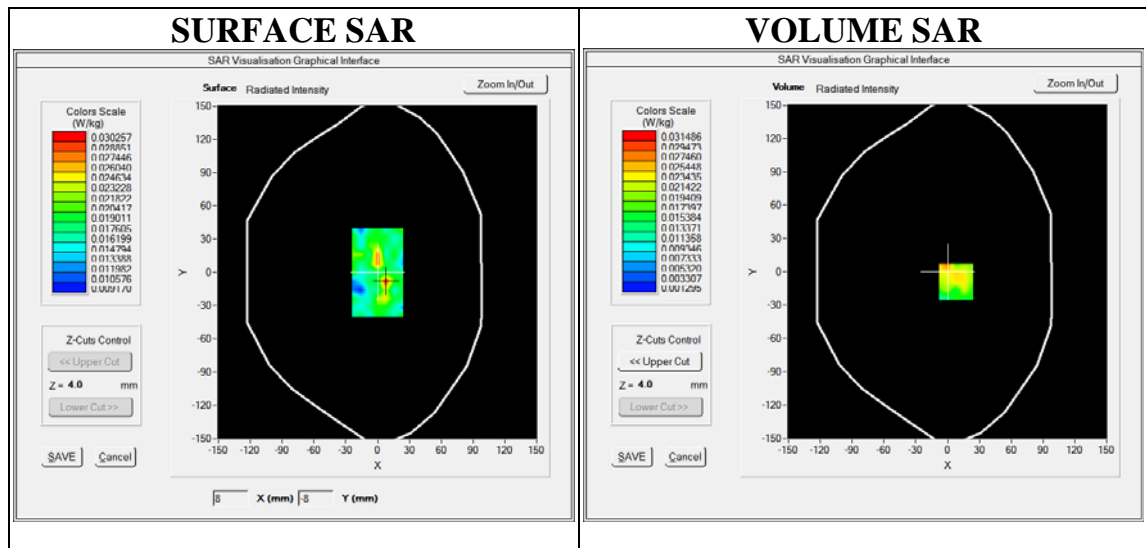


APPENDIX B – SAR Evaluation Data (Cont'd)

Plot #3

Operating Frequency : 462.6375MHz
Product Description: Watch WalkieTalkie
Model: 2720022
Test Date: 24 Apr 2017

| | |
|------------------------------------|---|
| Medium (Liquid Type) | : 450 Body |
| Relative permittivity ϵ_r | : 56.441 |
| Conductivity σ : | : 0.916 |
| Probe | : Model: SSE2; Serial No.: SN 08/16 EPGO283 |
| Crest factor | : 1.00 |
| Conversion Factor | : 1.56 |
| Area Scan | : dx=8mm, dy=8mm |
| Zoom Scan | : 5x5x7, dx=8mm dy=8mm dz=5mm |
| Phantom | : SAM phantom |
| Device Position | : Back 0mm Separation |
| SAR Drift (%) | : -1.81% |
| Maximum location | : X=0.00, Y=40.00 |
| SAR Peak (W/kg) | : 0.07 W/kg |
| SAR 10g (W/kg) | : 0.024 W/kg |
| SAR 1g (W/kg) | : 0.026 W/kg |

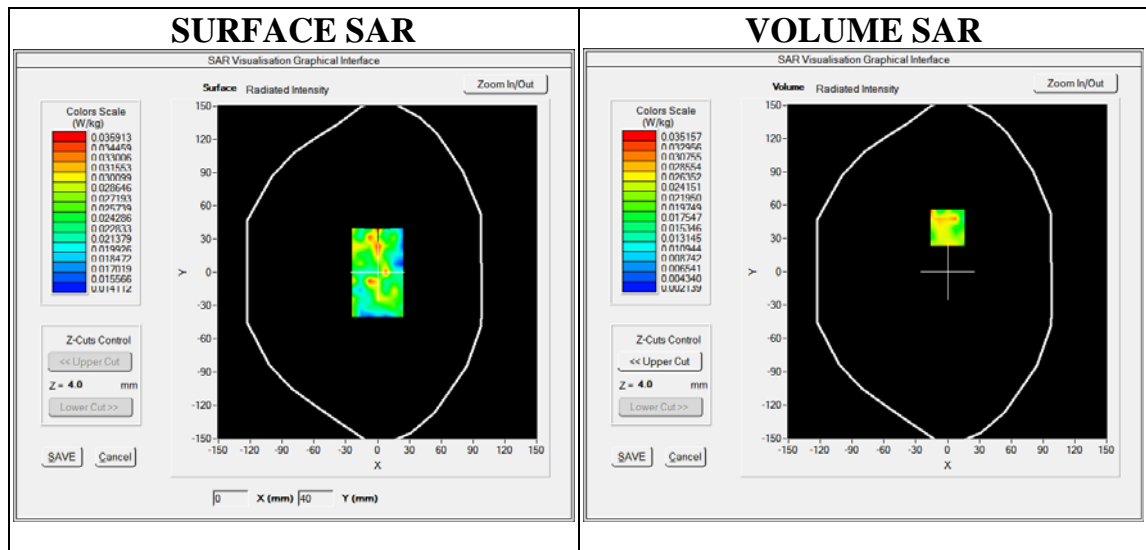


APPENDIX B – SAR Evaluation Data (Cont'd)

Plot #4

Operating Frequency : 462.6375MHz
Product Description: Watch WalkieTalkie
Model: 2720022
Test Date: 24 Apr 2017

| | |
|------------------------------------|---|
| Medium (Liquid Type) | : 450 Body |
| Relative permittivity ϵ_r | : 56.441 |
| Conductivity σ : | : 0.916 |
| Probe | : Model: SSE2; Serial No.: SN 08/16 EPGO283 |
| Crest factor | : 1.00 |
| Conversion Factor | : 1.56 |
| Area Scan | : dx=8mm, dy=8mm |
| Zoom Scan | : 5x5x7, dx=8mm dy=8mm dz=5mm |
| Phantom | : SAM phantom |
| Device Position | : Back 0mm Separation with earphone |
| SAR Drift (%) | : -4.02% |
| Maximum location | : X=-7.00, Y=8.00 |
| SAR Peak (W/kg) | : 0.15 W/kg |
| SAR 10g (W/kg) | : 0.027 W/kg |
| SAR 1g (W/kg) | : 0.032 W/kg |

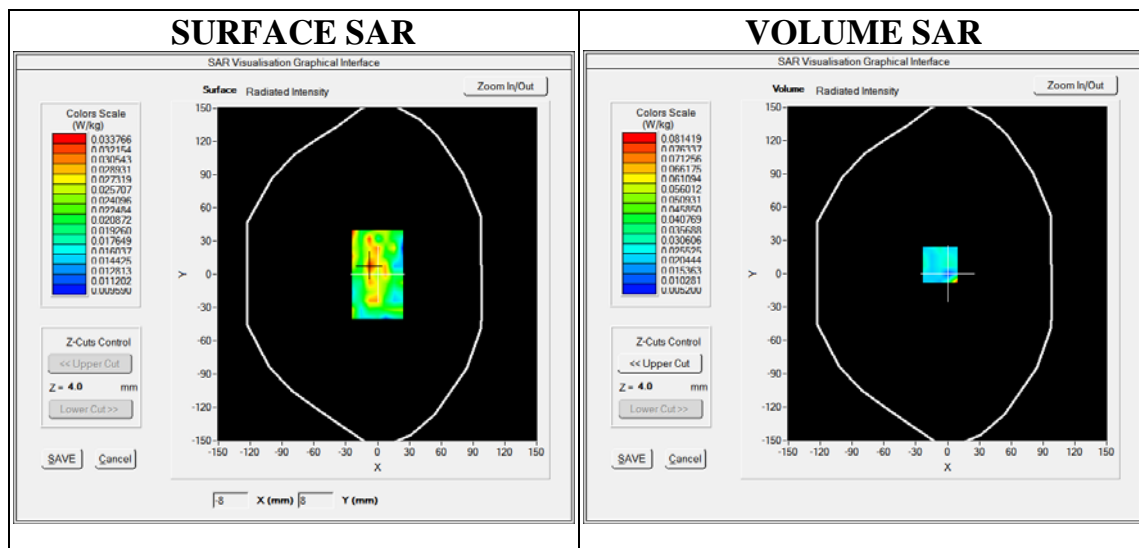



Valued Quality. Delivered.

Report No.: 17031394HKG-001
Page 40 of 41

APPENDIX C – E-Field Probe and Dipole Antenna Calibration



COMOSAR E-Field Probe Calibration Report

Ref : ACR.190.2.16.SATU.B

INTERTEK TESTING SERVICES HONG KONG LIMITED

WORKSHOP NO. 3 G/F, WORLD-WIDE INDUSTRIAL
CENTRE, 43-47 SHAN MEI STREET,
FO TAN, SHA TIN, N.T. HONG KONG
MVG COMOSAR DOSIMETRIC E-FIELD PROBE
SERIAL NO.: SN 08/16 EPGO283

Calibrated at MVG US
2105 Barrett Park Dr. - Kennesaw, GA 30144



Calibration Date: 7/5/2016

Summary:

This document presents the method and results from an accredited COMOSAR Dosimetric E-Field Probe calibration performed in MVG USA using the CALISAR / CALIBAIR test bench, for use with a COMOSAR system only. All calibration results are traceable to national metrology institutions.



| | <i>Name</i> | <i>Function</i> | <i>Date</i> | <i>Signature</i> |
|----------------------|---------------|-----------------|-------------|----------------------|
| <i>Prepared by :</i> | Jérôme LUC | Product Manager | 7/8/2016 | <i>JS</i> |
| <i>Checked by :</i> | Jérôme LUC | Product Manager | 7/8/2016 | <i>JS</i> |
| <i>Approved by :</i> | Kim RUTKOWSKI | Quality Manager | 7/8/2016 | <i>Kim Rutkowski</i> |

| | <i>Customer Name</i> |
|-----------------------|---|
| <i>Distribution :</i> | Intertek Testing Services Hong Kong Limited |

| <i>Issue</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|----------------------|
| A | 7/8/2016 | Initial release |
| B | 8/8/2016 | Add 1900 MHz factor |
| | | |
| | | |



TABLE OF CONTENTS

1 Device Under Test 4

2 Product Description 4

 2.1 General Information 4

3 Measurement Method 4

 3.1 Linearity 4

 3.2 Sensitivity 5

 3.3 Lower Detection Limit 5

 3.4 Isotropy 5

 3.5 Boundary Effect 5

4 Measurement Uncertainty 5

5 Calibration Measurement Results 6

 5.1 Sensitivity in air 6

 5.2 Linearity 7

 5.3 Sensitivity in liquid 7

 5.4 Isotropy 8

6 List of Equipment 10

1 DEVICE UNDER TEST

| Device Under Test | |
|--|---|
| Device Type | COMOSAR DOSIMETRIC E FIELD PROBE |
| Manufacturer | MVG |
| Model | SSE2 |
| Serial Number | SN 08/16 EPGO283 |
| Product Condition (new / used) | New |
| Frequency Range of Probe | 0.7 GHz-6GHz |
| Resistance of Three Dipoles at Connector | Dipole 1: R1=0.192 MΩ Dipole 2: R2=0.203 MΩ Dipole 3: R3=0.200 MΩ |

A yearly calibration interval is recommended.

2 PRODUCT DESCRIPTION

2.1 GENERAL INFORMATION

MVG's COMOSAR E field Probes are built in accordance to the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards.



Figure 1 – MVG COMOSAR Dosimetric E field Dipole

| | |
|--|--------|
| Probe Length | 330 mm |
| Length of Individual Dipoles | 2 mm |
| Maximum external diameter | 8 mm |
| Probe Tip External Diameter | 2.5 mm |
| Distance between dipoles / probe extremity | 1 mm |

3 MEASUREMENT METHOD

The IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards provide recommended practices for the probe calibrations, including the performance characteristics of interest and methods by which to assess their affect. All calibrations / measurements performed meet the fore mentioned standards.

3.1 LINEARITY

The evaluation of the linearity was done in free space using the waveguide, performing a power sweep to cover the SAR range 0.01W/kg to 100W/kg.

3.2 SENSITIVITY

The sensitivity factors of the three dipoles were determined using a two step calibration method (air and tissue simulating liquid) using waveguides as outlined in the standards.

3.3 LOWER DETECTION LIMIT

The lower detection limit was assessed using the same measurement set up as used for the linearity measurement. The required lower detection limit is 10 mW/kg.

3.4 ISOTROPY

The axial isotropy was evaluated by exposing the probe to a reference wave from a standard dipole with the dipole mounted under the flat phantom in the test configuration suggested for system validations and checks. The probe was rotated along its main axis from 0 - 360 degrees in 15 degree steps. The hemispherical isotropy is determined by inserting the probe in a thin plastic box filled with tissue-equivalent liquid, with the plastic box illuminated with the fields from a half wave dipole. The dipole is rotated about its axis (0°–180°) in 15° increments. At each step the probe is rotated about its axis (0°–360°).

3.5 BOUNDARY EFFECT

The boundary effect is defined as the deviation between the SAR measured data and the expected exponential decay in the liquid when the probe is oriented normal to the interface. To evaluate this effect, the liquid filled flat phantom is exposed to fields from either a reference dipole or waveguide. With the probe normal to the phantom surface, the peak spatial average SAR is measured and compared to the analytical value at the surface.

4 **MEASUREMENT UNCERTAINTY**

The guidelines outlined in the IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty associated with an E-field probe calibration using the waveguide technique. All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

| Uncertainty analysis of the probe calibration in waveguide | | | | | |
|--|-----------------------|--------------------------|------------|----|--------------------------|
| ERROR SOURCES | Uncertainty value (%) | Probability Distribution | Divisor | ci | Standard Uncertainty (%) |
| Incident or forward power | 3.00% | Rectangular | $\sqrt{3}$ | 1 | 1.732% |
| Reflected power | 3.00% | Rectangular | $\sqrt{3}$ | 1 | 1.732% |
| Liquid conductivity | 5.00% | Rectangular | $\sqrt{3}$ | 1 | 2.887% |
| Liquid permittivity | 4.00% | Rectangular | $\sqrt{3}$ | 1 | 2.309% |
| Field homogeneity | 3.00% | Rectangular | $\sqrt{3}$ | 1 | 1.732% |
| Field probe positioning | 5.00% | Rectangular | $\sqrt{3}$ | 1 | 2.887% |

| | | | | | |
|--|-------|-------------|------------|---|--------|
| Field probe linearity | 3.00% | Rectangular | $\sqrt{3}$ | 1 | 1.732% |
| Combined standard uncertainty | | | | | 5.831% |
| Expanded uncertainty 95 % confidence level k = 2 | | | | | 12.0% |

5 CALIBRATION MEASUREMENT RESULTS

| Calibration Parameters | |
|------------------------|-------|
| Liquid Temperature | 21 °C |
| Lab Temperature | 21 °C |
| Lab Humidity | 45 % |


5.1 SENSITIVITY IN AIR

| Normx dipole 1 ($\mu\text{V}/(\text{V}/\text{m})^2$) | Normy dipole 2 ($\mu\text{V}/(\text{V}/\text{m})^2$) | Normz dipole 3 ($\mu\text{V}/(\text{V}/\text{m})^2$) |
|---|---|---|
| 0.81 | 0.59 | 0.66 |


| DCP dipole 1 (mV) | DCP dipole 2 (mV) | DCP dipole 3 (mV) |
|----------------------|----------------------|----------------------|
| 93 | 91 | 96 |

Calibration curves $e_i=f(V)$ ($i=1,2,3$) allow to obtain H-field value using the formula:

$$E = \sqrt{E_1^2 + E_2^2 + E_3^2}$$

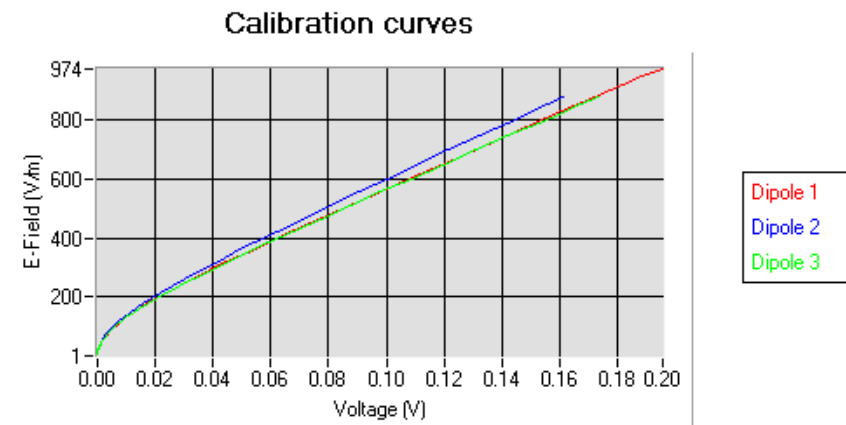

5.2 LINEARITY

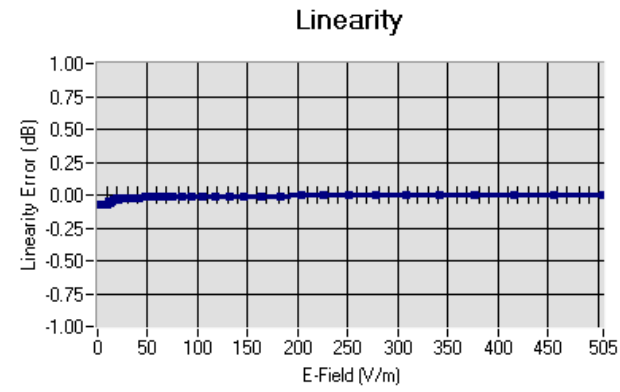

Linearity: $\pm 1.79\%$ ($\pm 0.08\text{dB}$)

5.3 SENSITIVITY IN LIQUID


| Liquid | Frequency (MHz +/- 100MHz) | Permittivity | Epsilon (S/m) | ConvF |
|--------|----------------------------------|--------------|---------------|-------|
| HL450 | 450 | 42.17 | 0.86 | 1.51 |
| BL450 | 450 | 57.65 | 0.95 | 1.56 |
| HL750 | 750 | 40.03 | 0.93 | 1.45 |
| BL750 | 750 | 56.83 | 1.00 | 1.50 |
| HL850 | 835 | 42.19 | 0.90 | 1.59 |
| BL850 | 835 | 54.67 | 1.01 | 1.63 |
| HL900 | 900 | 42.08 | 1.01 | 1.53 |
| BL900 | 900 | 55.25 | 1.08 | 1.59 |
| HL1800 | 1800 | 41.68 | 1.46 | 1.75 |
| BL1800 | 1800 | 53.86 | 1.46 | 1.81 |
| HL1900 | 1900 | 40.95 | 1.43 | 2.02 |
| BL1900 | 1900 | 53.32 | 1.49 | 2.11 |
| HL2000 | 2000 | 38.26 | 1.38 | 1.90 |
| BL2000 | 2000 | 52.70 | 1.51 | 1.97 |
| HL2300 | 2300 | 39.44 | 1.62 | 2.13 |
| BL2300 | 2300 | 54.52 | 1.77 | 2.20 |
| HL2450 | 2450 | 37.50 | 1.80 | 2.08 |
| BL2450 | 2450 | 53.22 | 1.89 | 2.14 |
| HL5200 | 5200 | 35.64 | 4.67 | 1.84 |
| BL5200 | 5200 | 48.64 | 5.51 | 1.90 |
| HL5400 | 5400 | 36.44 | 4.87 | 1.97 |
| BL5400 | 5400 | 46.52 | 5.77 | 2.04 |
| HL5600 | 5600 | 36.66 | 5.17 | 1.99 |
| BL5600 | 5600 | 46.79 | 5.77 | 2.04 |
| HL5800 | 5800 | 35.31 | 5.31 | 1.83 |
| BL5800 | 5800 | 47.04 | 6.10 | 1.90 |

LOWER DETECTION LIMIT: 9mW/kg

5.4 ISOTROPY


HL900 MHz

- Axial isotropy: 0.04 dB
- Hemispherical isotropy: 0.06 dB

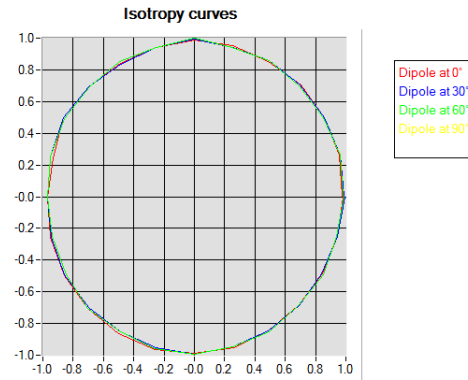


HL1800 MHz

- Axial isotropy: 0.05 dB
- Hemispherical isotropy: 0.06 dB

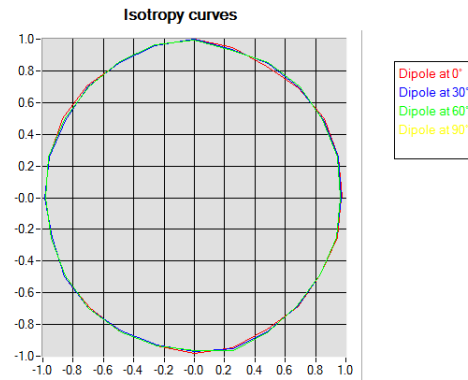

HL5600 MHz

- Axial isotropy: 0.05 dB
- Hemispherical isotropy: 0.08 dB

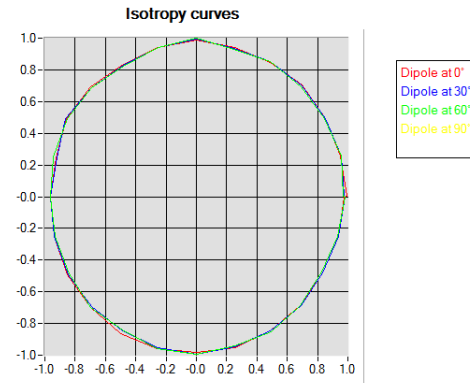



6 LIST OF EQUIPMENT

| Equipment Summary Sheet | | | | |
|-------------------------------|----------------------|--------------------|---|---|
| Equipment Description | Manufacturer / Model | Identification No. | Current Calibration Date | Next Calibration Date |
| Flat Phantom | MVG | SN-20/09-SAM71 | Validated. No cal required. | Validated. No cal required. |
| COMOSAR Test Bench | Version 3 | NA | Validated. No cal required. | Validated. No cal required. |
| Network Analyzer | Rhode & Schwarz ZVA | SN100132 | 02/2016 | 02/2019 |
| Reference Probe | MVG | EP 94 SN 37/08 | 10/2015 | 10/2016 |
| Multimeter | Keithley 2000 | 1188656 | 12/2013 | 12/2016 |
| Signal Generator | Agilent E4438C | MY49070581 | 12/2013 | 12/2016 |
| Amplifier | Aethercomm | SN 046 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter | HP E4418A | US38261498 | 12/2013 | 12/2016 |
| Power Sensor | HP ECP-E26A | US37181460 | 12/2013 | 12/2016 |
| Directional Coupler | Narda 4216-20 | 01386 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Waveguide | Mega Industries | 069Y7-158-13-712 | Validated. No cal required. | Validated. No cal required. |
| Waveguide Transition | Mega Industries | 069Y7-158-13-701 | Validated. No cal required. | Validated. No cal required. |
| Waveguide Termination | Mega Industries | 069Y7-158-13-701 | Validated. No cal required. | Validated. No cal required. |
| Temperature / Humidity Sensor | Control Company | 150798832 | 10/2015 | 10/2017 |



SAR Reference Dipole Calibration Report

Ref : ACR.221.1.16.SATU.A

INTERTEK TESTING SERVICES HONG KONG LIMITED

**WORKSHOP NO. 3 G/F, WORLD-WIDE INDUSTRIAL
CENTRE, 43-47 SHAN MEI STREET,
FO TAN, SHA TIN, N.T. HONG KONG**

MVG COMOSAR REFERENCE DIPOLE

FREQUENCY: 450 MHZ

SERIAL NO.: SN 26/16 DIP 0G450-420

Calibrated at MVG US

2105 Barrett Park Dr. - Kennesaw, GA 30144



Calibration Date: 7/5/2016

Summary:

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



| | <i>Name</i> | <i>Function</i> | <i>Date</i> | <i>Signature</i> |
|----------------------|---------------|-----------------|-------------|----------------------|
| <i>Prepared by :</i> | Jérôme LUC | Product Manager | 8/8/2016 | <i>JS</i> |
| <i>Checked by :</i> | Jérôme LUC | Product Manager | 8/8/2016 | <i>JS</i> |
| <i>Approved by :</i> | Kim RUTKOWSKI | Quality Manager | 8/8/2016 | <i>Kim Rutkowski</i> |

| | <i>Customer Name</i> |
|-----------------------|---|
| <i>Distribution :</i> | Intertek Testing Services Hong Kong Limited |

| <i>Issue</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|----------------------|
| A | 8/8/2016 | Initial release |
| | | |
| | | |
| | | |



TABLE OF CONTENTS

1 Introduction..... 4

2 Device Under Test 4

3 Product Description 4

 3.1 General Information 4

4 Measurement Method 5

 4.1 Return Loss Requirements 5

 4.2 Mechanical Requirements 5

5 Measurement Uncertainty 5

 5.1 Return Loss 5

 5.2 Dimension Measurement 5

 5.3 Validation Measurement 5

6 Calibration Measurement Results 6

 6.1 Return Loss and Impedance In Head Liquid 6

 6.2 Return Loss and Impedance In Body Liquid 6

 6.3 Mechanical Dimensions 6

7 Validation measurement 7

 7.1 Head Liquid Measurement 7

 7.2 SAR Measurement Result With Head Liquid 8

 7.3 Body Liquid Measurement 9

 7.4 SAR Measurement Result With Body Liquid 10

8 List of Equipment 11

1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEEE 1528, FCC KDBs and CEI/IEC 62209 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

2 DEVICE UNDER TEST

| Device Under Test | |
|--------------------------------|----------------------------------|
| Device Type | COMOSAR 450 MHz REFERENCE DIPOLE |
| Manufacturer | MVG |
| Model | SID450 |
| Serial Number | SN 26/16 DIP 0G450-420 |
| Product Condition (new / used) | New |

A yearly calibration interval is recommended.

3 PRODUCT DESCRIPTION

3.1 GENERAL INFORMATION

MVG’s COMOSAR Validation Dipoles are built in accordance to the IEEE 1528, FCC KDBs and CEI/IEC 62209 standards. The product is designed for use with the COMOSAR test bench only.



Figure 1 – MVG COMOSAR Validation Dipole

4 MEASUREMENT METHOD

The IEEE 1528, FCC KDBs and CEI/IEC 62209 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards.

4.2 MECHANICAL REQUIREMENTS

The IEEE Std. 1528 and CEI/IEC 62209 standards specify the mechanical components and dimensions of the validation dipoles, with the dimensions frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness.

5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz | 0.1 dB |

5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 3 - 300 | 0.05 mm |

5.3 VALIDATION MEASUREMENT


The guidelines outlined in the IEEE 1528, FCC KDBs, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g | 20.3 % |

| | |
|------|--------|
| 10 g | 20.1 % |
|------|--------|


6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

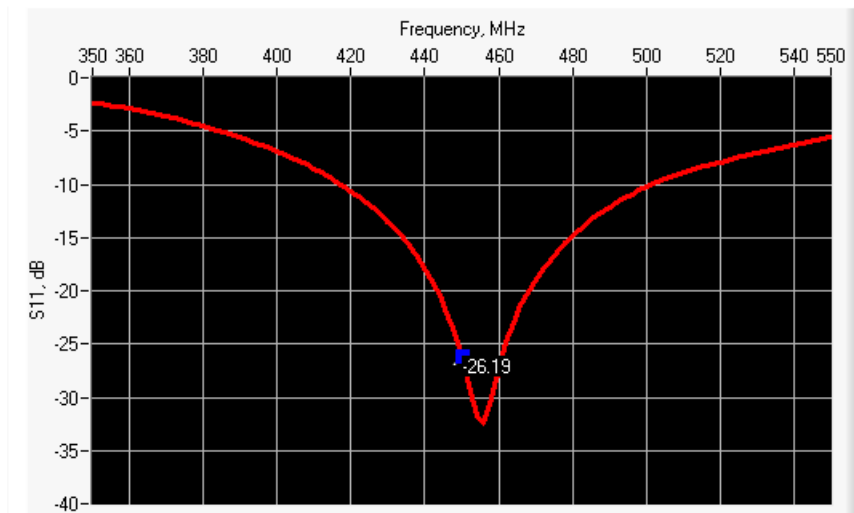

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance |
|-----------------|------------------|------------------|-----------------|
| 450 | -26.19 | -20 | 45.2 Ω + 1.2 jΩ |

6.2 RETURN LOSS AND IMPEDANCE IN BODY LIQUID

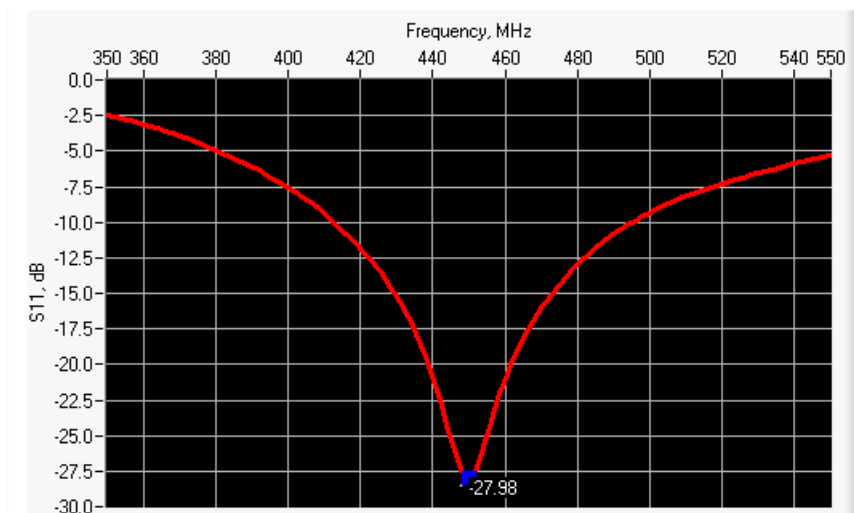

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance |
|-----------------|------------------|------------------|-----------------|
| 450 | -27.98 | -20 | 47.1 Ω - 2.8 jΩ |

6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm | | h mm | | d mm | |
|---------------|-------------|----------|-------------|----------|------------|----------|
| | required | measured | required | measured | required | measured |
| 300 | 420.0 ±1 %. | | 250.0 ±1 %. | | 6.35 ±1 %. | |



| | | | | | | |
|------|-------------|------|-------------|------|------------|------|
| 450 | 290.0 ±1 %. | PASS | 166.7 ±1 %. | PASS | 6.35 ±1 %. | PASS |
| 750 | 176.0 ±1 %. | | 100.0 ±1 %. | | 6.35 ±1 %. | |
| 835 | 161.0 ±1 %. | | 89.8 ±1 %. | | 3.6 ±1 %. | |
| 900 | 149.0 ±1 %. | | 83.3 ±1 %. | | 3.6 ±1 %. | |
| 1450 | 89.1 ±1 %. | | 51.7 ±1 %. | | 3.6 ±1 %. | |
| 1500 | 80.5 ±1 %. | | 50.0 ±1 %. | | 3.6 ±1 %. | |
| 1640 | 79.0 ±1 %. | | 45.7 ±1 %. | | 3.6 ±1 %. | |
| 1750 | 75.2 ±1 %. | | 42.9 ±1 %. | | 3.6 ±1 %. | |
| 1800 | 72.0 ±1 %. | | 41.7 ±1 %. | | 3.6 ±1 %. | |
| 1900 | 68.0 ±1 %. | | 39.5 ±1 %. | | 3.6 ±1 %. | |
| 1950 | 66.3 ±1 %. | | 38.5 ±1 %. | | 3.6 ±1 %. | |
| 2000 | 64.5 ±1 %. | | 37.5 ±1 %. | | 3.6 ±1 %. | |
| 2100 | 61.0 ±1 %. | | 35.7 ±1 %. | | 3.6 ±1 %. | |
| 2300 | 55.5 ±1 %. | | 32.6 ±1 %. | | 3.6 ±1 %. | |
| 2450 | 51.5 ±1 %. | | 30.4 ±1 %. | | 3.6 ±1 %. | |
| 2600 | 48.5 ±1 %. | | 28.8 ±1 %. | | 3.6 ±1 %. | |
| 3000 | 41.5 ±1 %. | | 25.0 ±1 %. | | 3.6 ±1 %. | |
| 3500 | 37.0 ±1 %. | | 26.4 ±1 %. | | 3.6 ±1 %. | |
| 3700 | 34.7 ±1 %. | | 26.4 ±1 %. | | 3.6 ±1 %. | |

7 VALIDATION MEASUREMENT

The IEEE Std. 1528, FCC KDBs and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

7.1 HEAD LIQUID MEASUREMENT

| Frequency MHz | Relative permittivity (ϵ_r') | | Conductivity (σ) S/m | |
|------------------|---|----------|-------------------------------|----------|
| | required | measured | required | measured |
| 300 | 45.3 ±5 % | | 0.87 ±5 % | |
| 450 | 43.5 ±5 % | PASS | 0.87 ±5 % | PASS |
| 750 | 41.9 ±5 % | | 0.89 ±5 % | |
| 835 | 41.5 ±5 % | | 0.90 ±5 % | |
| 900 | 41.5 ±5 % | | 0.97 ±5 % | |
| 1450 | 40.5 ±5 % | | 1.20 ±5 % | |
| 1500 | 40.4 ±5 % | | 1.23 ±5 % | |
| 1640 | 40.2 ±5 % | | 1.31 ±5 % | |
| 1750 | 40.1 ±5 % | | 1.37 ±5 % | |



| | | | | |
|------|-----------|--|-----------|--|
| 1800 | 40.0 ±5 % | | 1.40 ±5 % | |
| 1900 | 40.0 ±5 % | | 1.40 ±5 % | |
| 1950 | 40.0 ±5 % | | 1.40 ±5 % | |
| 2000 | 40.0 ±5 % | | 1.40 ±5 % | |
| 2100 | 39.8 ±5 % | | 1.49 ±5 % | |
| 2300 | 39.5 ±5 % | | 1.67 ±5 % | |
| 2450 | 39.2 ±5 % | | 1.80 ±5 % | |
| 2600 | 39.0 ±5 % | | 1.96 ±5 % | |
| 3000 | 38.5 ±5 % | | 2.40 ±5 % | |
| 3500 | 37.9 ±5 % | | 2.91 ±5 % | |


7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

| | |
|---|--|
| Software | OPENSAR V4 |
| Phantom | SN 20/09 SAM71 |
| Probe | SN 18/11 EPG122 |
| Liquid | Head Liquid Values: eps' : 42.2 sigma : 0.86 |
| Distance between dipole center and liquid | 15.0 mm |
| Area scan resolution | dx=8mm/dy=8mm |
| Zoon Scan Resolution | dx=8mm/dy=8mm/dz=5mm |
| Frequency | 450 MHz |
| Input power | 20 dBm |
| Liquid Temperature | 21 °C |
| Lab Temperature | 21 °C |
| Lab Humidity | 45 % |

| Frequency MHz | 1 g SAR (W/kg/W) | | 10 g SAR (W/kg/W) | |
|---------------|------------------|-------------|-------------------|-------------|
| | required | measured | required | measured |
| 300 | 2.85 | | 1.94 | |
| 450 | 4.58 | 4.77 (0.48) | 3.06 | 3.03 (0.30) |
| 750 | 8.49 | | 5.55 | |
| 835 | 9.56 | | 6.22 | |
| 900 | 10.9 | | 6.99 | |
| 1450 | 29 | | 16 | |
| 1500 | 30.5 | | 16.8 | |
| 1640 | 34.2 | | 18.4 | |
| 1750 | 36.4 | | 19.3 | |
| 1800 | 38.4 | | 20.1 | |

| | | | | |
|------|------|--|------|--|
| 1900 | 39.7 | | 20.5 | |
| 1950 | 40.5 | | 20.9 | |
| 2000 | 41.1 | | 21.1 | |
| 2100 | 43.6 | | 21.9 | |
| 2300 | 48.7 | | 23.3 | |
| 2450 | 52.4 | | 24 | |
| 2600 | 55.3 | | 24.6 | |
| 3000 | 63.8 | | 25.7 | |
| 3500 | 67.1 | | 25 | |

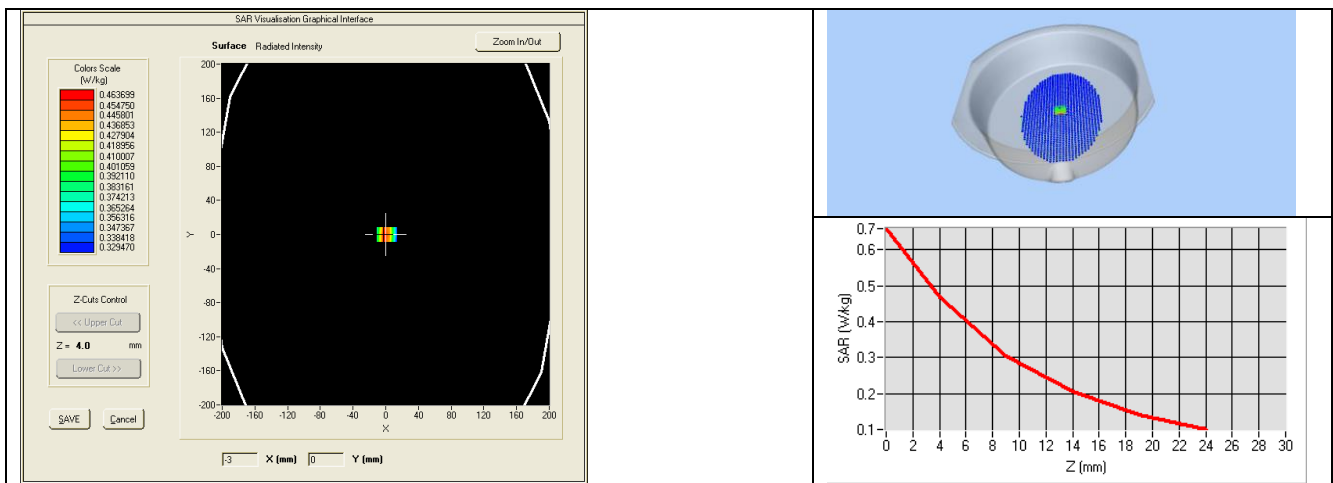

7.3 BODY LIQUID MEASUREMENT



| Frequency MHz | Relative permittivity (ϵ_r') | | Conductivity (σ) S/m | |
|---------------|---|----------|-------------------------------|----------|
| | required | measured | required | measured |
| 150 | 61.9 ± 5 % | | 0.80 ± 5 % | |
| 300 | 58.2 ± 5 % | | 0.92 ± 5 % | |
| 450 | 56.7 ± 5 % | PASS | 0.94 ± 5 % | PASS |
| 750 | 55.5 ± 5 % | | 0.96 ± 5 % | |
| 835 | 55.2 ± 5 % | | 0.97 ± 5 % | |
| 900 | 55.0 ± 5 % | | 1.05 ± 5 % | |
| 915 | 55.0 ± 5 % | | 1.06 ± 5 % | |
| 1450 | 54.0 ± 5 % | | 1.30 ± 5 % | |
| 1610 | 53.8 ± 5 % | | 1.40 ± 5 % | |
| 1800 | 53.3 ± 5 % | | 1.52 ± 5 % | |
| 1900 | 53.3 ± 5 % | | 1.52 ± 5 % | |
| 2000 | 53.3 ± 5 % | | 1.52 ± 5 % | |
| 2100 | 53.2 ± 5 % | | 1.62 ± 5 % | |
| 2450 | 52.7 ± 5 % | | 1.95 ± 5 % | |

| | | | | |
|------|------------|--|------------|--|
| 2600 | 52.5 ±5 % | | 2.16 ±5 % | |
| 3000 | 52.0 ±5 % | | 2.73 ±5 % | |
| 3500 | 51.3 ±5 % | | 3.31 ±5 % | |
| 5200 | 49.0 ±10 % | | 5.30 ±10 % | |
| 5300 | 48.9 ±10 % | | 5.42 ±10 % | |
| 5400 | 48.7 ±10 % | | 5.53 ±10 % | |
| 5500 | 48.6 ±10 % | | 5.65 ±10 % | |
| 5600 | 48.5 ±10 % | | 5.77 ±10 % | |
| 5800 | 48.2 ±10 % | | 6.00 ±10 % | |

7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

| | |
|---|--|
| Software | OPENSAR V4 |
| Phantom | SN 20/09 SAM71 |
| Probe | SN 18/11 EPG122 |
| Liquid | Body Liquid Values: eps' : 57.6 sigma : 0.95 |
| Distance between dipole center and liquid | 15.0 mm |
| Area scan resolution | dx=8mm/dy=8mm |
| Zoon Scan Resolution | dx=8mm/dy=8mm/dz=5mm |
| Frequency | 450 MHz |
| Input power | 20 dBm |
| Liquid Temperature | 21 °C |
| Lab Temperature | 21 °C |
| Lab Humidity | 45 % |

| Frequency MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|---------------|------------------|-------------------|
| | measured | measured |
| 450 | 4.88 (0.49) | 3.22 (0.32) |

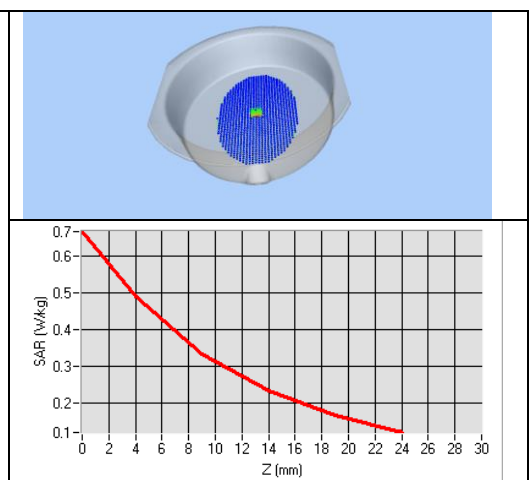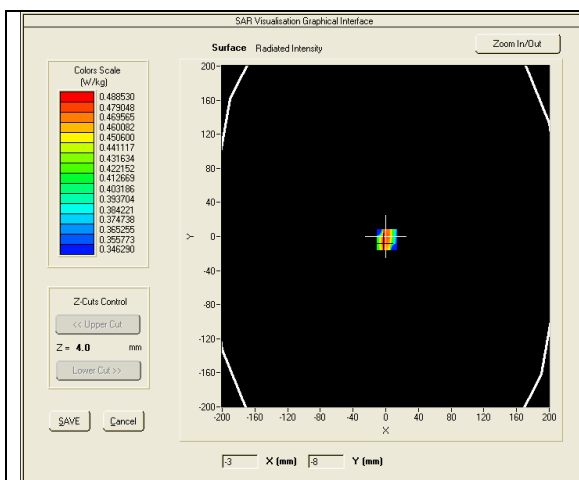



8 LIST OF EQUIPMENT

| Equipment Summary Sheet | | | | |
|---------------------------------|----------------------|--------------------|---|---|
| Equipment Description | Manufacturer / Model | Identification No. | Current Calibration Date | Next Calibration Date |
| SAM Phantom | MVG | SN-20/09-SAM71 | Validated. No cal required. | Validated. No cal required. |
| COMOSAR Test Bench | Version 3 | NA | Validated. No cal required. | Validated. No cal required. |
| Network Analyzer | Rhode & Schwarz ZVA | SN100132 | 02/2016 | 02/2019 |
| Calipers | Carrera | CALIPER-01 | 12/2013 | 12/2016 |
| Reference Probe | MVG | EPG122 SN 18/11 | 10/2015 | 10/2016 |
| Multimeter | Keithley 2000 | 1188656 | 12/2013 | 12/2016 |
| Signal Generator | Agilent E4438C | MY49070581 | 12/2013 | 12/2016 |
| Amplifier | Aethercomm | SN 046 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter | HP E4418A | US38261498 | 12/2013 | 12/2016 |
| Power Sensor | HP ECP-E26A | US37181460 | 12/2013 | 12/2016 |
| Directional Coupler | Narda 4216-20 | 01386 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature and Humidity Sensor | Control Company | 150798832 | 10/2015 | 10/2017 |

APPENDIX D – SAR System Validation

Per KDB 865664, SAR system validation status should be documented to confirm measurement accuracy. SAR measurement systems are validated according to procedures in KDB 865664. The validation status is documented according to the validation date(s), measurement frequencies, SAR probe and tissue dielectric parameters. When multiple SAR system is used, the validation status of each SAR system is needed to be documented separately according to the associated system components.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probe and tissue dielectric parameters are shown as below.

| Date | Probe S/N | Tested Freq. (MHz) | Tissue Type | Cond. | Perm | CW Validation | | | Mod. Validation | | |
|------------|-----------|--------------------|-------------|-------|------|---------------|-----------------|----------------|-----------------|-------------|-----------------------------|
| | | | | | | Sensitivity | Probe Linearity | Probe Isotropy | Mod. Type | Duty Factor | Peak to average power ratio |
| 19/09/2016 | EPGO 283 | 1900 | Head | 40.97 | 1.41 | PASS | PASS | PASS | GFSK | PASS | PASS |
| 19/09/2016 | EPGO 283 | 1900 | Body | 53.68 | 1.59 | PASS | PASS | PASS | GFSK | PASS | PASS |
| 30/09/2016 | EPGO 283 | 2450 | Head | 39.62 | 1.76 | PASS | PASS | PASS | OFDM | N/A | PASS |
| 30/09/2016 | EPGO 283 | 2450 | Body | 50.24 | 1.89 | PASS | PASS | PASS | OFDM | N/A | PASS |
| 30/09/2016 | EPGO 283 | 2450 | Head | 39.62 | 1.76 | PASS | PASS | PASS | DSSS | PASS | N/A |
| 30/09/2016 | EPGO 283 | 2450 | Body | 50.24 | 1.89 | PASS | PASS | PASS | DSSS | PASS | N/A |
| 11/10/2016 | EPGO 283 | 450 | Head | 41.84 | 0.88 | PASS | PASS | PASS | FM | PASS | PASS |
| 11/10/2016 | EPGO 283 | 450 | Body | 58.30 | 0.96 | PASS | PASS | PASS | FM | PASS | PASS |
| 14/10/2016 | EPGO 283 | 1800 | Head | 38.27 | 1.46 | PASS | PASS | PASS | GFSK | PASS | PASS |
| 14/10/2016 | EPGO 283 | 1800 | Body | 52.77 | 1.55 | PASS | PASS | PASS | GFSK | PASS | PASS |
| 24/10/2016 | EPGO 283 | 2450 | Head | 39.03 | 1.78 | PASS | PASS | PASS | FHSS | PASS | PASS |
| 24/10/2016 | EPGO 283 | 2450 | Body | 51.23 | 1.95 | PASS | PASS | PASS | FHSS | PASS | PASS |