Test Laboratory: SGS-SAR Lab

#### Haier i701 WCDMA1900 9400CH Back side 15mm

### DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, WCDMA (0); Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: MSL1900; Medium parameters used: f = 1880 MHz;  $\sigma = 1.493$  S/m;  $\varepsilon_r = 52.273$ ;  $\rho = 1000$ 

 $kg/m^3$ 

Phantom section: Flat Section

## DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(8.2, 8.2, 8.2); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = -14.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

## **Configuration/Body/Area Scan (8x13x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 0.439 W/kg


## **Configuration/Body/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 8.443 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 0.699 W/kg

SAR(1 g) = 0.435 W/kg; SAR(10 g) = 0.255 W/kg

Maximum value of SAR (measured) = 0.464 W/kg

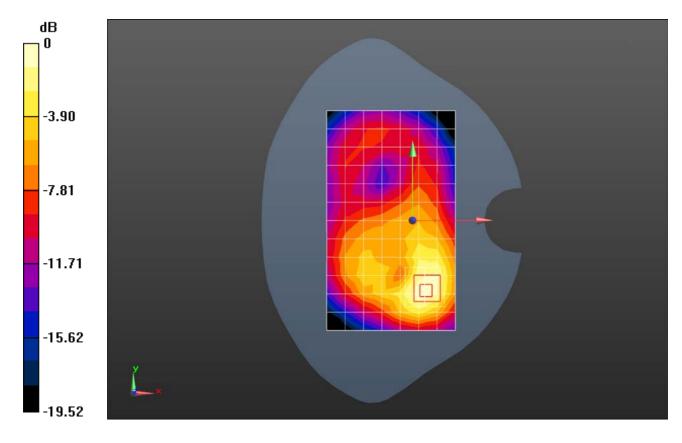

Test Laboratory: SGS-SAR Lab

#### Haier i701 WCDMA1900 9400CH Back side 10mm

DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, WCDMA (0); Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: MSL1900; Medium parameters used: f = 1880 MHz;  $\sigma = 1.493$  S/m;  $\varepsilon_r = 52.273$ ;  $\rho = 1000$ 

 $kg/m^3$ 

Phantom section: Flat Section

## DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(8.2, 8.2, 8.2); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = -14.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Configuration/Body/Area Scan (8x13x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 0.847 W/kg


**Configuration/Body/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 10.59 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 1.36 W/kg

SAR(1 g) = 0.806 W/kg; SAR(10 g) = 0.456 W/kg

Maximum value of SAR (measured) = 0.846 W/kg

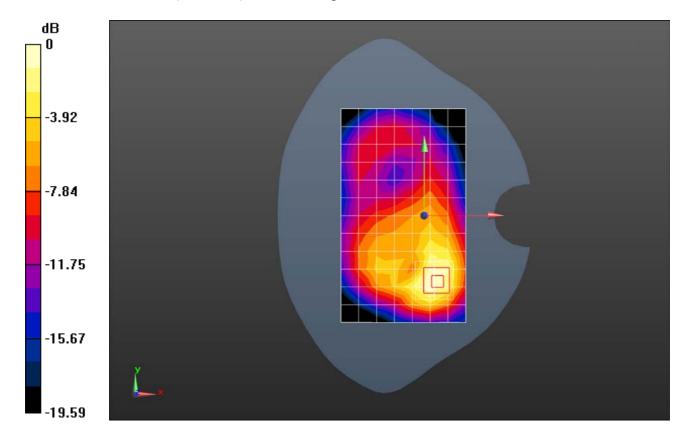

0 dB = 0.846 W/kg = -0.73 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band2 20MHz Bandwidth QPSK 1RB 0Offset 19100CH Left touch cheek

## DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 20MHz (0); Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL1900; Medium parameters used: f = 1900 MHz;  $\sigma = 1.437$  S/m;  $\varepsilon_r = 40.578$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Left Section

### DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(8.49, 8.49, 8.49); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Configuration/Head/Area Scan (8x13x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 0.206 W/kg


**Configuration/Head/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 3.351 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 0.277 W/kg

SAR(1 g) = 0.182 W/kg; SAR(10 g) = 0.114 W/kg

Maximum value of SAR (measured) = 0.193 W/kg

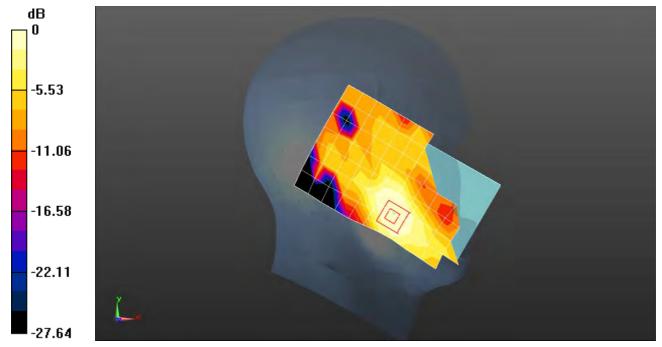

0 dB = 0.193 W/kg = -7.14 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band2 20MHz Bandwidth QPSK 1RB 0Offset 19100CH Front side 15mm

## DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 20MHz (0); Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: MSL1900; Medium parameters used: f = 1900 MHz;  $\sigma = 1.523$  S/m;  $\varepsilon_r = 52.205$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Flat Section

### DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(8.2, 8.2, 8.2); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Configuration/Body/Area Scan (9x16x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.389 W/kg


**Configuration/Body/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 6.616 V/m; Power Drift = 0.13 dB

Peak SAR (extrapolated) = 2.47 W/kg

SAR(1 g) = 0.410 W/kg; SAR(10 g) = 0.223 W/kg

Maximum value of SAR (measured) = 0.486 W/kg

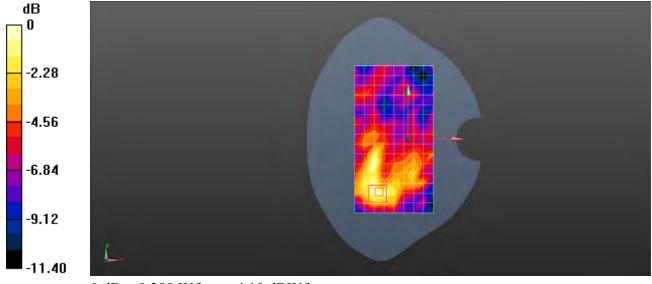

0 dB = 0.389 W/kg = -4.10 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band2 20MHz Bandwidth QPSK 1RB 0Offset 19100CH Back side 10mm

### DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 20MHz (0); Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: MSL1900; Medium parameters used: f = 1900 MHz;  $\sigma = 1.523$  S/m;  $\varepsilon_r = 52.205$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Flat Section

### DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(8.2, 8.2, 8.2); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Configuration/Body/Area Scan (9x16x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.925 W/kg


**Configuration/Body/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 12.12 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 1.51 W/kg

SAR(1 g) = 0.901 W/kg; SAR(10 g) = 0.520 W/kg

Maximum value of SAR (measured) = 1.02 W/kg

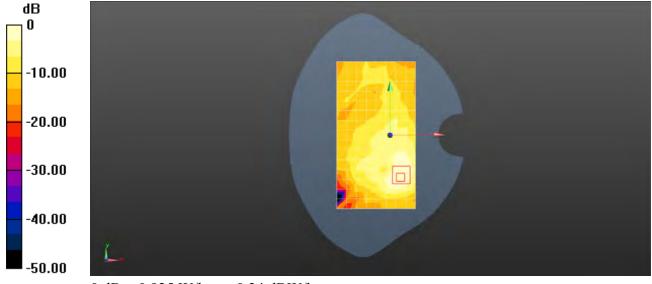

0 dB = 0.925 W/kg = -0.34 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band4 20MHz Bandwidth QPSK 1RB 0Offset 20050CH Right touch cheek

DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 20MHz (0); Frequency: 1720 MHz; Duty Cycle: 1:1

Medium: HSL1800; Medium parameters used: f = 1720 MHz;  $\sigma = 1.318$  S/m;  $\varepsilon_r = 40.663$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Right Section

### DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(8.77, 8.77, 8.77); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Configuration/Head/Area Scan (8x13x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 0.0601 W/kg


**Configuration/Head/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 1.206 V/m; Power Drift = 0.20 dB

Peak SAR (extrapolated) = 0.102 W/kg

SAR(1 g) = 0.056 W/kg; SAR(10 g) = 0.031 W/kg

Maximum value of SAR (measured) = 0.0651 W/kg

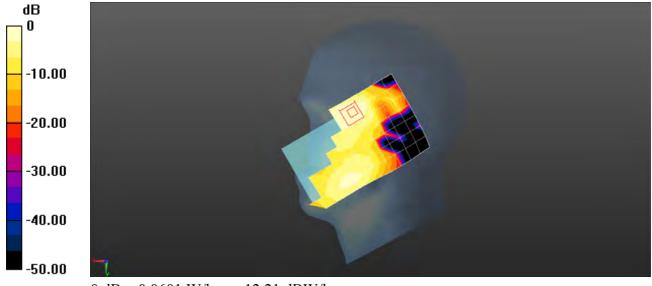

0 dB = 0.0601 W/kg = -12.21 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band4 20MHz Bandwidth QPSK 1RB 0Offset 20050CH Back side 15mm

#### DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 20MHz (0); Frequency: 1720 MHz; Duty Cycle: 1:1

Medium: MSL1750;Medium parameters used: f = 1720 MHz;  $\sigma = 1.461$  S/m;  $\epsilon_r = 54.721$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

### DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(8.49, 8.49, 8.49); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Configuration/Body/Area Scan (9x16x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.305 W/kg


**Configuration/Body/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 7.997 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 0.442 W/kg

SAR(1 g) = 0.262 W/kg; SAR(10 g) = 0.157 W/kg

Maximum value of SAR (measured) = 0.288 W/kg

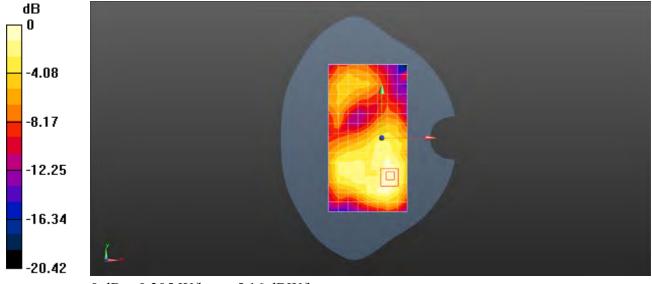

0 dB = 0.305 W/kg = -5.16 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band4 20MHz Bandwidth QPSK 50RB 0Offset 20175CH Back side 10mm

### DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 20MHz (0); Frequency: 1732.5 MHz; Duty Cycle: 1:1

Medium: MSL1750; Medium parameters used: f = 1732.5 MHz;  $\sigma = 1.472$  S/m;  $\varepsilon_r = 54.659$ ;  $\rho = 1000$ 

 $kg/m^3$ 

Phantom section: Flat Section

### DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(8.49, 8.49, 8.49); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Configuration/Body/Area Scan (9x16x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.545 W/kg


**Configuration/Body/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 8.900 V/m; Power Drift = -0.19 dB

Peak SAR (extrapolated) = 1.07 W/kg

SAR(1 g) = 0.576 W/kg; SAR(10 g) = 0.315 W/kg

Maximum value of SAR (measured) = 0.652 W/kg

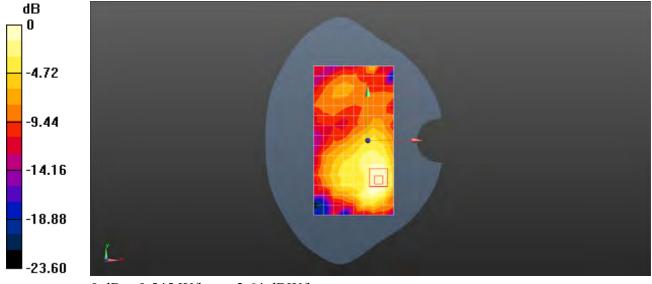

0 dB = 0.545 W/kg = -2.64 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band7 20MHz Bandwidth QPSK 1RB 0Offset 21100CH Right touch cheek

DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 20MHz (0); Frequency: 2510 MHz; Duty Cycle: 1:1

Medium: HSL2600; Medium parameters used: f = 2510 MHz;  $\sigma = 1.832$  S/m;  $\epsilon_r = 38.417$ ;  $\rho = 1000$ 

 $kg/m^3$ 

Phantom section: Right Section

### DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(7.35, 7.35, 7.35); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Configuration/Head/Area Scan (7x12x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 0.0277 W/kg


**Configuration/Head/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 1.299 V/m; Power Drift = 0.15 dB

Peak SAR (extrapolated) = 0.165 W/kg

SAR(1 g) = 0.0256 W/kg; SAR(10 g) = 0.011 W/kg

Maximum value of SAR (measured) = 0.0281 W/kg

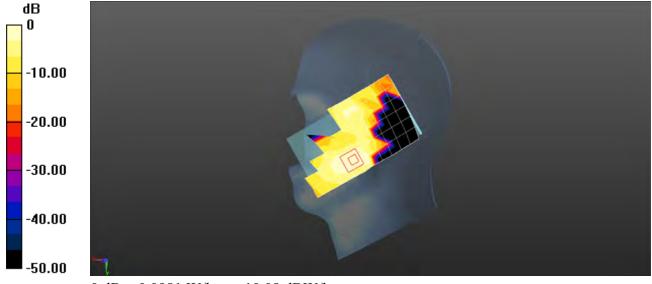

0 dB = 0.0981 W/kg = -10.08 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band7 20MHz Bandwidth QPSK 1RB 0Offset 21100CH Front side 15mm

#### DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 20MHz (0); Frequency: 2535 MHz; Duty Cycle: 1:1

Medium: MSL2600; Medium parameters used: f = 2535 MHz;  $\sigma = 2.085$  S/m;  $\varepsilon_r = 53.223$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Flat Section

### DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(7.63, 7.63, 7.63); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Configuration/Body/Area Scan (9x16x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.118 W/kg


**Configuration/Body/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 3.468 V/m; Power Drift = -0.18 dB

Peak SAR (extrapolated) = 0.184 W/kg

SAR(1 g) = 0.108 W/kg; SAR(10 g) = 0.060 W/kg

Maximum value of SAR (measured) = 0.117 W/kg

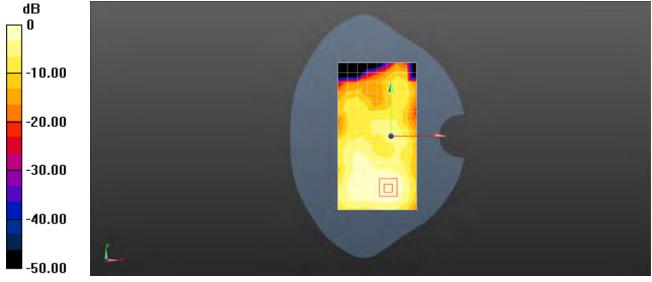

0 dB = 0.118 W/kg = -9.28 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band7 20MHz Bandwidth QPSK 1RB 0Offset 21100CH Back side 10mm

#### DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 20MHz (0); Frequency: 2535 MHz; Duty Cycle: 1:1

Medium: MSL2600; Medium parameters used: f = 2535 MHz;  $\sigma = 2.085$  S/m;  $\varepsilon_r = 53.223$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Flat Section

### DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(7.63, 7.63, 7.63); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)


**Configuration/Body/Area Scan (9x16x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.290 W/kg

**Configuration/Body/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 3.357 V/m; Power Drift = 0.10 dB

Peak SAR (extrapolated) = 0.591 W/kg

SAR(1 g) = 0.259 W/kg; SAR(10 g) = 0.124 W/kg

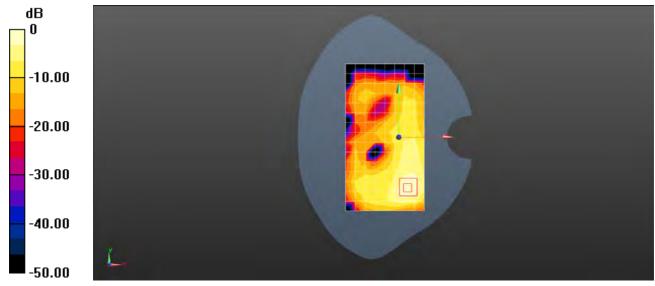

0 dB = 0.290 W/kg = -5.38 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band17 10MHz Bandwidth QPSK 1RB 0Offset 23780CH Left Touch Cheek

DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 10MHZ (0); Frequency: 709 MHz; Duty Cycle: 1:1

Medium: HSL750;Medium parameters used: f = 709 MHz;  $\sigma = 0.847$  S/m;  $\varepsilon_r = 42.426$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Left Section

## DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(10.67, 10.67, 10.67); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Configuration/Head/Area Scan (8x13x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 0.0148 W/kg


**Configuration/Head/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 0.7010 V/m; Power Drift = 2.02 dB

Peak SAR (extrapolated) = 0.0170 W/kg

SAR(1 g) = 0.014 W/kg; SAR(10 g) = 0.011 W/kg

Maximum value of SAR (measured) = 0.0150 W/kg

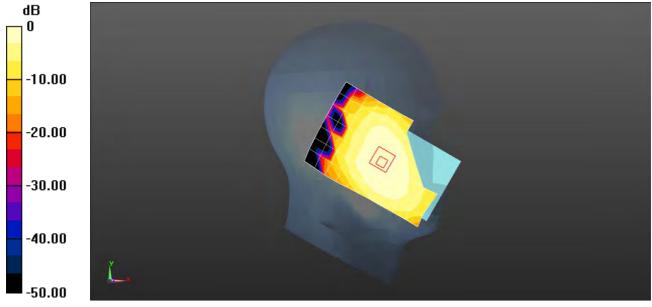

0 dB = 0.0148 W/kg = -18.29 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band17 10MHz Bandwidth QPSK 1RB 0Offset 23780CH Back side 15mm

DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 10MHZ (0); Frequency: 709 MHz; Duty Cycle: 1:1

Medium: MSL750;Medium parameters used: f = 709 MHz;  $\sigma = 0.903$  S/m;  $\varepsilon_r = 56.495$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Flat Section

## DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(10.41, 10.41, 10.41); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = -14.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)


**Configuration/Body/Area Scan (8x13x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 0.0368 W/kg

**Configuration/Body/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.291 V/m; Power Drift = 0.09 dB

Peak SAR (extrapolated) = 0.0440 W/kg

SAR(1 g) = 0.035 W/kg; SAR(10 g) = 0.028 W/kgMaximum value of SAR (measured) = 0.0369 W/kg

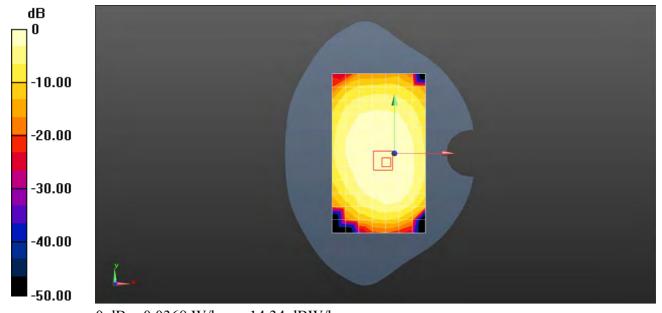

0 dB = 0.0368 W/kg = -14.34 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 LTE Band17 10MHz Bandwidth QPSK 1RB 0Offset 23780CH Back side 10mm

### DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, LTE-FDD BW 10MHZ (0); Frequency: 709 MHz; Duty Cycle: 1:1

Medium: MSL750;Medium parameters used: f = 709 MHz;  $\sigma = 0.903$  S/m;  $\varepsilon_r = 56.495$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Flat Section

## DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(10.41, 10.41, 10.41); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = -14.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)


**Configuration/Body/Area Scan (8x13x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 0.0488 W/kg

## **Configuration/Body/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 7.044 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 0.0660 W/kg

SAR(1 g) = 0.047 W/kg; SAR(10 g) = 0.035 W/kgMaximum value of SAR (measured) = 0.0493 W/kg

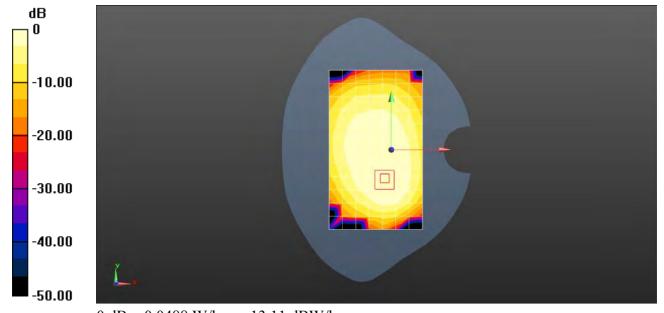

0 dB = 0.0488 W/kg = -13.11 dBW/kg

Test Laboratory: SGS-SAR Lab

## Haier i701 WIFI 802.11b 1CH Right tilted 15 degree

### DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, WI-FI(2.4GHz) (0); Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: HSL2450; Medium parameters used: f = 2412 MHz;  $\sigma = 1.727$  S/m;  $\epsilon_r = 38.717$ ;  $\rho = 1000$ 

 $kg/m^3$ 

Phantom section: Right Section

## DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(7.65, 7.65, 7.65); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

## Configuration/Head/Area Scan (10x16x1): Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.154 W/kg


## **Configuration/Head/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 10.38 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 0.390 W/kg

SAR(1 g) = 0.173 W/kg; SAR(10 g) = 0.082 W/kg

Maximum value of SAR (measured) = 0.193 W/kg

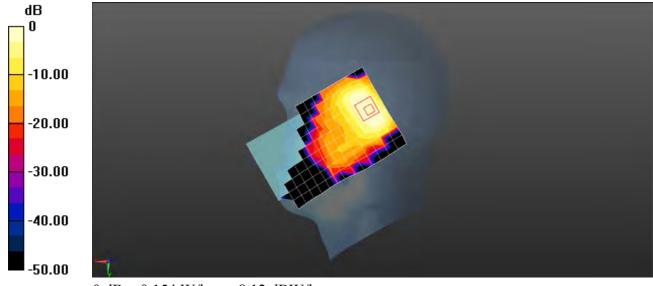

0 dB = 0.154 W/kg = -8.12 dBW/kg

Test Laboratory: SGS-SAR Lab

### Haier i701 WIFI 802.11b 1CH Back Side 15mm

### DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, WI-FI(2.4GHz) (0); Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: MSL2450; Medium parameters used: f = 2412 MHz;  $\sigma = 1.905$  S/m;  $\epsilon_r = 51.831$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Flat Section

## DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(7.7, 7.7, 7.7); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V4.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Configuration/Body/Area Scan (9x16x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.0337 W/kg


**Configuration/Body/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 0.3910 V/m; Power Drift = 0.18 dB

Peak SAR (extrapolated) = 0.0540 W/kg

SAR(1 g) = 0.030 W/kg; SAR(10 g) = 0.015 W/kg

Maximum value of SAR (measured) = 0.0336 W/kg

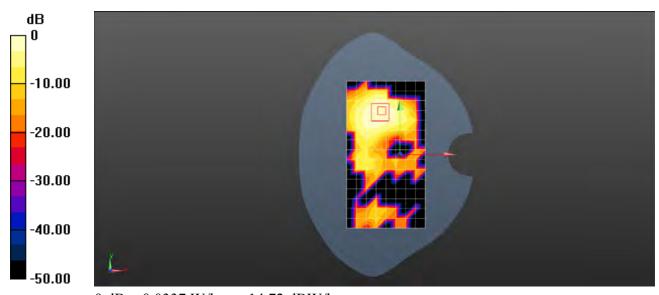

0 dB = 0.0337 W/kg = -14.72 dBW/kg

Test Laboratory: SGS-SAR Lab

#### Haier i701 WIFI 802.11b 1CH Back side 10mm

#### DUT: Haier-i701; Type: Mobile Phone; Serial: FINJSGKN9999999

Communication System: UID 0, WI-FI(2.4GHz) (0); Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: MSL2450; Medium parameters used: f = 2412 MHz;  $\sigma = 1.905$  S/m;  $\varepsilon_r = 51.831$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Flat Section

## DASY 5 Configuration:

- Probe: EX3DV4 SN3962; ConvF(7.7, 7.7, 7.7); Calibrated: 2015-11-27;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE3 Sn569; Calibrated: 2015-11-24
- Phantom: SAM 1; Type: SAM V.0; Serial: TP-1283
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

## **Configuration/Body/Area Scan (9x16x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.0802 W/kg


## **Configuration/Body/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 0.1490 V/m; Power Drift = 0.11 dB

Peak SAR (extrapolated) = 0.162 W/kg

SAR(1 g) = 0.078 W/kg; SAR(10 g) = 0.036 W/kg

Maximum value of SAR (measured) = 0.0921 W/kg

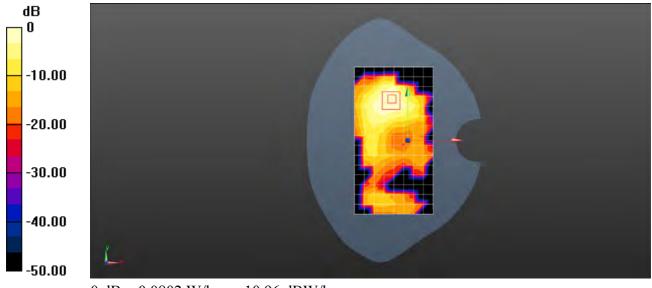

0 dB = 0.0802 W/kg = -10.96 dBW/kg



Report No.: SZEM160300168001

# **Appendix C**

## **Calibration certificate**

1. Dipole
D750V3-SN 1126(2014-09-19)
D835V2-SN 4d105(2013-11-25)
D1800V2-SN 2d070(2013-11-27)
D1900V2-SN 5d028(2013-11-27)
D2450V2-SN 733(2013-11-26)
D2600V2-SN 1093(2014-09-23)
2. DAE
DAE3-SN 569(2015-11-24)
3. Probe
EX3DV4-SN 3962(2015-11-27)

## Calibration Laboratory of Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura **Swiss Calibration Service** 

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Lenovo (Auden)

Accreditation No.: SCS 108

Certificate No: D750V3-1126 Sep14

## CALIBRATION CERTIFICATE

Object D750V3 - SN: 1126

Calibration procedure(s) QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

Calibration date: September 19, 2014

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22  $\pm$  3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	US37292783	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01828)	Oct-14
Reference 20 dB Attenuator	SN: 5058 (20k)	03-Apr-14 (No. 217-01918)	Apr-15
Type-N mismatch combination	SN: 5047.2 / 06327	03-Apr-14 (No. 217-01921)	Apr-15
Reference Probe ES3DV3	SN: 3205	30-Dec-13 (No. ES3-3205_Dec13)	Dec-14
DAE4	SN: 601	18-Aug-14 (No. DAE4-601_Aug14)	Aug-15
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14
	Name	Function	Signature
Calibrated by:	Michael Weber	Laboratory Technician	MILL

Technical Manager

Issued: September 22, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Katja Pokovic

Certificate No: D750V3-1126\_Sep14

Approved by:

Page 1 of 8

## Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

Service suisse d'étalonnage

C Servizio svizzero di taratura **Swiss Calibration Service** 

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL

tissue simulating liquid

ConvF

sensitivity in TSL / NORM x,y,z

N/A

not applicable or not measured

## Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)",

February 2005

c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation:

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.

Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.

Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.

Electrical Delay: One-way delay between the SMA connector and the antenna feed point.

No uncertainty required.

SAR measured: SAR measured at the stated antenna input power.

SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.

 SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

## **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz ± 1 MHz	

## **Head TSL parameters**

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.0 ± 6 %	0.91 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		1

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.10 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	8.26 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.37 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	5.41 W/kg ± 16.5 % (k=2)

## **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.5	0.96 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.0 ± 6 %	0.98 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

## SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.20 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	8.65 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.46 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	5.76 W/kg ± 16.5 % (k=2)

## Appendix (Additional assessments outside the scope of SCS108)

## **Antenna Parameters with Head TSL**

Impedance, transformed to feed point	53.1 Ω - 1.4 jΩ	
Return Loss	- 29.5 dB	

## Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.7 Ω - 3.2 jΩ	
Return Loss	- 29.1 dB	

## General Antenna Parameters and Design

Electrical Delay (one direction)	1.034 ns	

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	June 23, 2014

Certificate No: D750V3-1126\_Sep14

## **DASY5 Validation Report for Head TSL**

Date: 19.09.2014

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1126

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: f = 750 MHz;  $\sigma = 0.91 \text{ S/m}$ ;  $\varepsilon_r = 42$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

### DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(6.37, 6.37, 6.37); Calibrated: 30.12.2013;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 18.08.2014

Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

## Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 53.42 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.12 W/kg


SAR(1 g) = 2.1 W/kg; SAR(10 g) = 1.37 W/kg

Maximum value of SAR (measured) = 2.43 W/kg

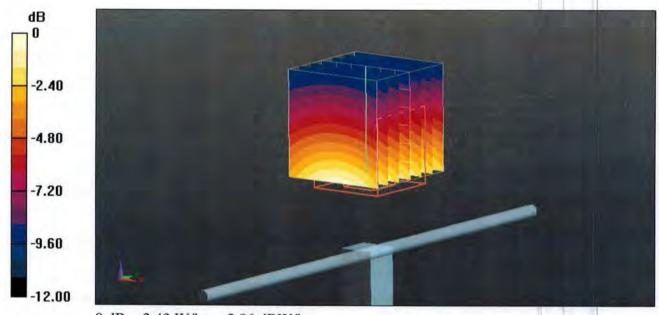

0 dB = 2.43 W/kg = 3.86 dBW/kg

## Impedance Measurement Plot for Head TSL

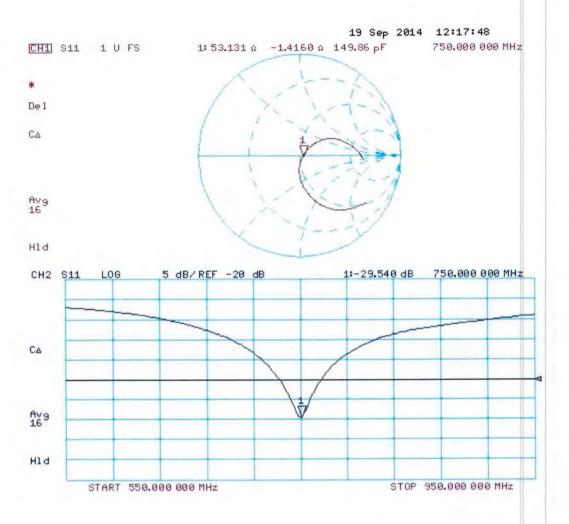

## **DASY5 Validation Report for Body TSL**

Date: 19.09.2014

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1126

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: f = 750 MHz;  $\sigma = 0.98 \text{ S/m}$ ;  $\varepsilon_r = 55$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

### DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(6.13, 6.13, 6.13); Calibrated: 30.12.2013;

• Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 18.08.2014

Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

## Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 53.03 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.20 W/kg

SAR(1 g) = 2.2 W/kg; SAR(10 g) = 1.46 W/kg


Maximum value of SAR (measured) = 2.56 W/kg

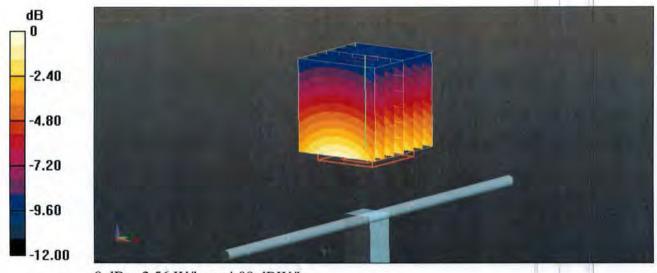

0 dB = 2.56 W/kg = 4.08 dBW/kg

Certificate No: D750V3-1126\_Sep14

## Impedance Measurement Plot for Body TSL

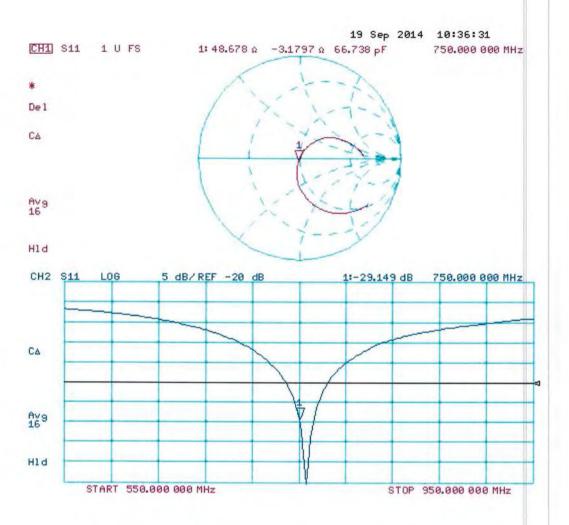




## SGS-CSTC Standards Technical Services Co., Ltd. Shenzhen Branch

Dipole Calibration for Impedance and Return-loss						
Model NO.:	D750V3	Serial NO.:	1126	Measurement Date:	2015-09-18	
Target Value: Measured Value:		sured Value:				
Liquid Type	Impedance	Return Loss	Impedance	Return Loss	verdict	
Head	53.1Ω-1.4jΩ	-29.5dB	49.6Ω+3.5jΩ	-29.4dB	Complied	
Body	48.7Ω-3.2jΩ	-29.1dB	46.7Ω+1.1jΩ	-29.3dB	Complied	

Remark: According to KDB 865664 D01,instead of the typical annual calibration recommended by measurement standards, longer calibration intervals of up to three years may be considered when it is demonstrated that the SAR target, impedance and return loss of a dipole have remain stable according to the following requirements:

- 1) The most recent return-loss result, measured at least annually, deviates by less than 20% from the previous measurement and meeting the required 20 dB minimum return-loss requirement.
- 2) The most recent measurement of the real and imaginary parts of the impedance, measured at least annually, deviates by less than 5  $\Omega$  from the previous measurement.

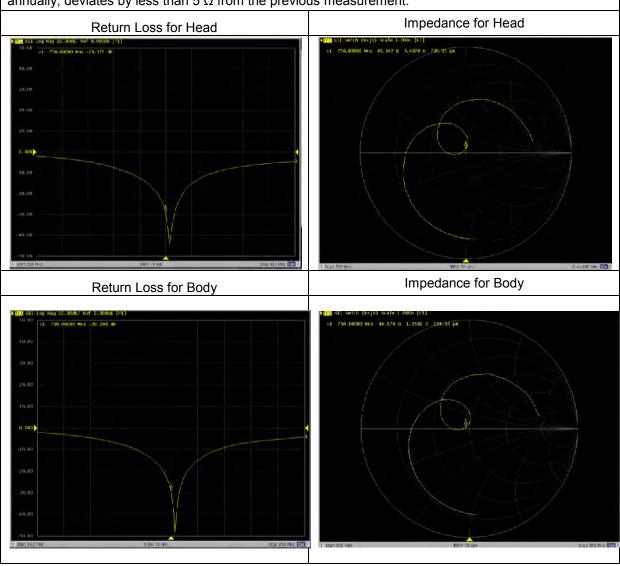

## Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage

Servizio svizzero di taratura Swiss Calibration Service

Certificate No: D835V2-4d105\_Nov13

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

SGS-SZ (Auden)

**CALIBRATION CERTIFICATE** 

Object D835V2 - SN: 4d105

Calibration procedure(s) QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

Calibration date: November 25, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards

GB37480704	00 0 1 10 (11 017 01007)	0.111
0007400704	09-Oct-13 (No. 217-01827)	Oct-14
US37292783	09-Oct-13 (No. 217-01827)	Oct-14
MY41092317	09-Oct-13 (No. 217-01828)	Oct-14
SN: 5058 (20k)	04-Apr-13 (No. 217-01736)	Apr-14
SN: 5047.3 / 06327	04-Apr-13 (No. 217-01739)	Apr-14
SN: 3205	28-Dec-12 (No. ES3-3205_Dec12)	Dec-13
SN: 601	25-Apr-13 (No. DAE4-601_Apr13)	Apr-14
ID#	Check Date (in house)	Scheduled Check
100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-15
US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14
Name	Function	Signature
Israe El-Naouq	Laboratory Technician	Deran Granera
Katja Pokovic	Technical Manager	Pour.
	MY41092317 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # 100005 US37390585 S4206 Name Israe El-Naouq	MY41092317 09-Oct-13 (No. 217-01828) SN: 5058 (20k) 04-Apr-13 (No. 217-01736) SN: 5047.3 / 06327 04-Apr-13 (No. 217-01739) SN: 3205 28-Dec-12 (No. ES3-3205_Dec12) SN: 601 25-Apr-13 (No. DAE4-601_Apr13)  ID # Check Date (in house)  100005 04-Aug-99 (in house check Oct-13) US37390585 S4206 18-Oct-01 (in house check Oct-13)  Name Function Israe El-Naouq Laboratory Technician

Cal Date (Certificate No.)

Issued: November 26, 2013

Scheduled Calibration

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## Calibration Laboratory of Schmid & Partner

Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

## Glossary:

TSL

tissue simulating liquid

ConvF

sensitivity in TSL / NORM x,y,z

N/A not applicable or not measured

## Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### **Additional Documentation:**

Certificate No: D835V2-4d105\_Nov13

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

## **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, $dy$ , $dz = 5 mm$	
Frequency	835 MHz ± 1 MHz	

## **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.8 ± 6 %	0.94 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.50 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.64 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.61 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.26 W/kg ± 16.5 % (k=2)

## **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.7 ± 6 %	1.01 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

## SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.39 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.28 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.55 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.06 W/kg ± 16.5 % (k=2)

Certificate No: D835V2-4d105\_Nov13 Page 3 of 8

## **Appendix**

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.4 Ω - 4.1 jΩ	
Return Loss	- 27.3 dB	

## Antenna Parameters with Body TSL

Impedance, transformed to feed point	46.9 Ω - 6.0 jΩ	
Return Loss	- 23.1 dB	

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.395 ns
Electrical Delay (one direction)	1.333 115

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	May 26, 2010

Certificate No: D835V2-4d105\_Nov13 Page 4 of 8

### **DASY5 Validation Report for Head TSL**

Date: 25.11.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d105

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: f = 835 MHz;  $\sigma = 0.94 \text{ S/m}$ ;  $\varepsilon_r = 40.8$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

## DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(6.05, 6.05, 6.05); Calibrated: 28.12.2012;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 25.04.2013

Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

## Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.324 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 3.80 W/kg


SAR(1 g) = 2.5 W/kg; SAR(10 g) = 1.61 W/kg

Maximum value of SAR (measured) = 2.92 W/kg

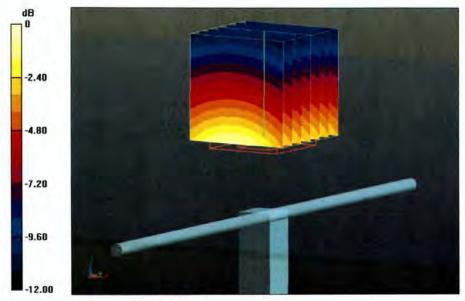

0 dB = 2.92 W/kg = 4.65 dBW/kg

## Impedance Measurement Plot for Head TSL

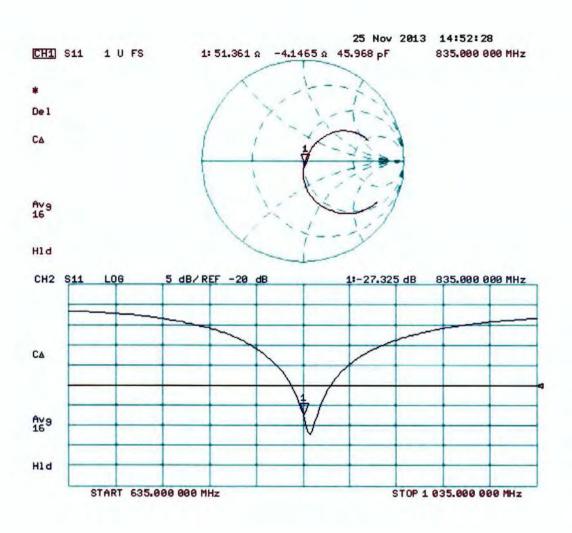

## **DASY5 Validation Report for Body TSL**

Date: 25.11.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d105

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: f = 835 MHz;  $\sigma = 1.007$  S/m;  $\varepsilon_r = 54.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

## DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(6.04, 6.04, 6.04); Calibrated: 28.12.2012;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 25.04.2013

Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

## Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 54.53 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 3.53 W/kg


SAR(1 g) = 2.39 W/kg; SAR(10 g) = 1.55 W/kg

Maximum value of SAR (measured) = 2.78 W/kg

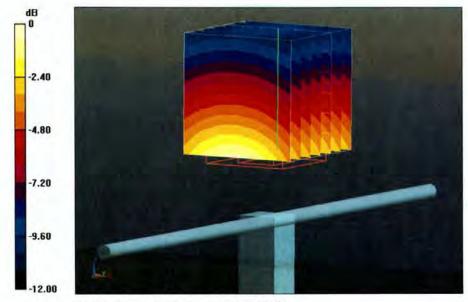

0 dB = 2.78 W/kg = 4.44 dBW/kg

## Impedance Measurement Plot for Body TSL

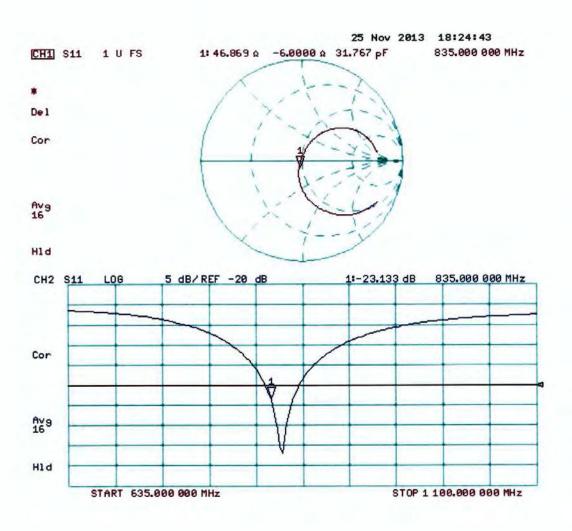


# SGS-CSTC Standards Technical Services Co., Ltd. Shenzhen Branch

Dipole Calibration for Impedance and Return-loss						
Model NO.:	D835V2	Serial NO.:	4d015	Measurement Date:	2015-11-25	
	Target \	/alue:	Measured Value:			
Liquid Type	Impedance	Return Loss	Impedance	Return Loss	verdict	
Head	51.4Ω-4.1jΩ	-27.3dB	51.4Ω-3.3jΩ	-27.7dB	Complied	
Body	46.9Ω-6.0jΩ	-23.1dB	46.9Ω-6.6jΩ	-23.7dB	Complied	

Remark: According to KDB 865664 D01,instead of the typical annual calibration recommended by measurement standards, longer calibration intervals of up to three years may be considered when it is demonstrated that the SAR target, impedance and return loss of a dipole have remain stable according to the following requirements:

- 1) The most recent return-loss result, measured at least annually, deviates by less than 20% from the previous measurement and meeting the required 20 dB minimum return-loss requirement.
- 2) The most recent measurement of the real and imaginary parts of the impedance, measured at least annually, deviates by less than 5  $\Omega$  from the previous measurement.

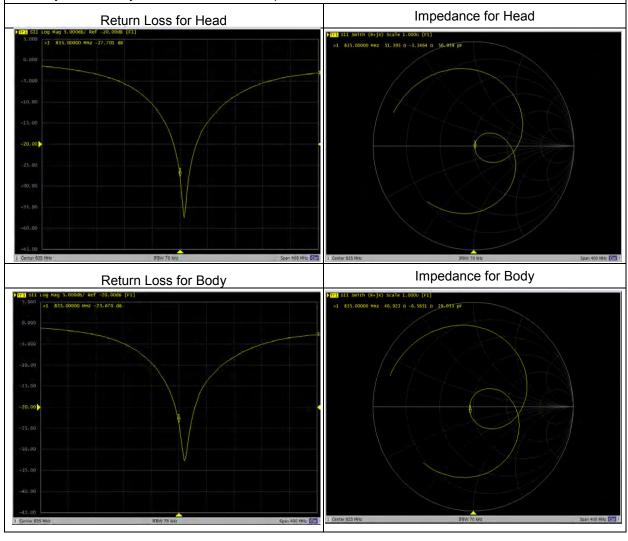

## Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

SGS-SZ (Auden)

Certificate No: D1800V2-2d070\_Nov13

Accreditation No.: SCS 108

## **CALIBRATION CERTIFICATE**

Object D1800V2 - SN: 2d070

Calibration procedure(s) QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

Calibration date: November 27, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	US37292783	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01828)	Oct-14
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-13 (No. 217-01736)	Apr-14
Type-N mismatch combination	SN: 5047.3 / 06327	04-Apr-13 (No. 217-01739)	Apr-14
Reference Probe ES3DV3	SN: 3205	28-Dec-12 (No. ES3-3205_Dec12)	Dec-13
DAE4	SN: 601	25-Apr-13 (No. DAE4-601_Apr13)	Apr-14
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-15
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14
	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	110=

Issued: November 27, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Katja Pokovic

Approved by:

Technical Manager

## Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

### Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### **Additional Documentation:**

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, $dy$ , $dz = 5 mm$	
Frequency	1800 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.42 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.79 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	38.8 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.11 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	20.3 W/kg ± 16.5 % (k=2)

## **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.8 ± 6 %	1.53 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	) <del></del> )	

## SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.72 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	38.6 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.13 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.4 W/kg ± 16.5 % (k=2)

Certificate No: D1800V2-2d070\_Nov13

## **Appendix**

### **Antenna Parameters with Head TSL**

Impedance, transformed to feed point	48.4 Ω - 5.0 jΩ	
Return Loss	- 25.5 dB	

### **Antenna Parameters with Body TSL**

Impedance, transformed to feed point	$45.3 \Omega - 4.3 j\Omega$	
Return Loss	- 23.5 dB	

## General Antenna Parameters and Design

1.212 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG	
Manufactured on	May 26, 2003	

Certificate No: D1800V2-2d070\_Nov13

## **DASY5 Validation Report for Head TSL**

Date: 27.11.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d070

Communication System: UID 0 - CW; Frequency: 1800 MHz

Medium parameters used: f = 1800 MHz;  $\sigma = 1.42 \text{ S/m}$ ;  $\varepsilon_r = 39.8$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(5.04, 5.04, 5.04); Calibrated: 28.12.2012;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 25.04.2013

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

## Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.789 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 17.9 W/kg


SAR(1 g) = 9.79 W/kg; SAR(10 g) = 5.11 W/kg

Maximum value of SAR (measured) = 12.0 W/kg

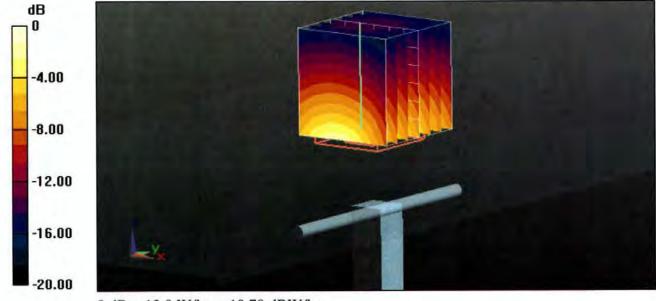

0 dB = 12.0 W/kg = 10.79 dBW/kg

## Impedance Measurement Plot for Head TSL

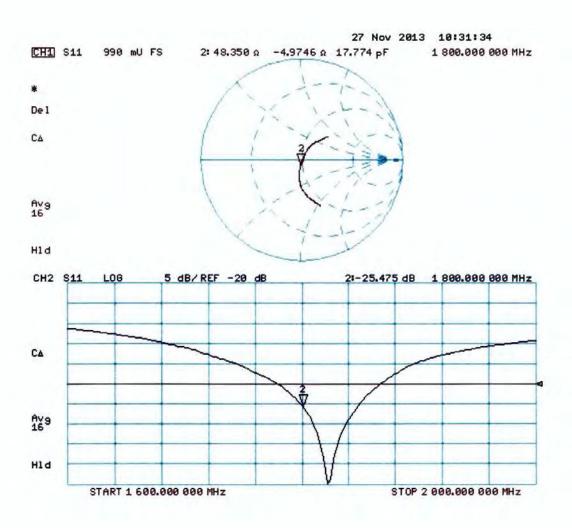

### **DASY5 Validation Report for Body TSL**

Date: 25.11.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d070

Communication System: UID 0 - CW; Frequency: 1800 MHz

Medium parameters used: f = 1800 MHz;  $\sigma = 1.53 \text{ S/m}$ ;  $\varepsilon_r = 52.8$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.73, 4.73, 4.73); Calibrated: 28.12.2012;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 25.04.2013

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

## Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 92.707 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 17.3 W/kg


SAR(1 g) = 9.72 W/kg; SAR(10 g) = 5.13 W/kg

Maximum value of SAR (measured) = 12.2 W/kg



0 dB = 12.2 W/kg = 10.86 dBW/kg

## Impedance Measurement Plot for Body TSL

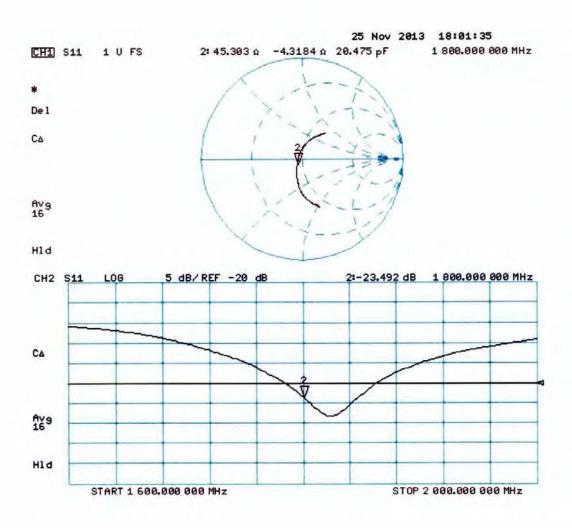




## SGS-CSTC Standards Technical Services Co., Ltd. Shenzhen Branch

Dipole Calibration for Impedance and Return-loss					
Model NO.:	D1800V2	Serial NO.:	2d070	Measurement Date:	2015-11-25
Liquid Type	Target \	/alue:	Measured Value:		verdict
Liquid Type	Impedance	Return Loss	Impedance	Return Loss	verdict
Head	<b>48</b> .4 Ω -5.0j Ω	-25.5dB	<b>47.1</b> Ω <b>-4.2</b> j Ω	-25.4dB	Complied
Body	<b>45.3</b> Ω <b>-4.3</b> j Ω	-23.5dB	<b>46</b> .8 Ω <b>-3</b> .4j Ω	-23.6dB	Complied

Remark: According to KDB 865664 D01,instead of the typical annual calibration recommended by measurement standards, longer calibration intervals of up to three years may be considered when it is demonstrated that the SAR target, impedance and return loss of a dipole have remain stable according to the following requirements:

- 1) The most recent return-loss result, measured at least annually, deviates by less than 20% from the previous measurement and meeting the required 20 dB minimum return-loss requirement.
- 2) The most recent measurement of the real and imaginary parts of the impedance, measured at least annually, deviates by less than 5  $\Omega$  from the previous measurement.

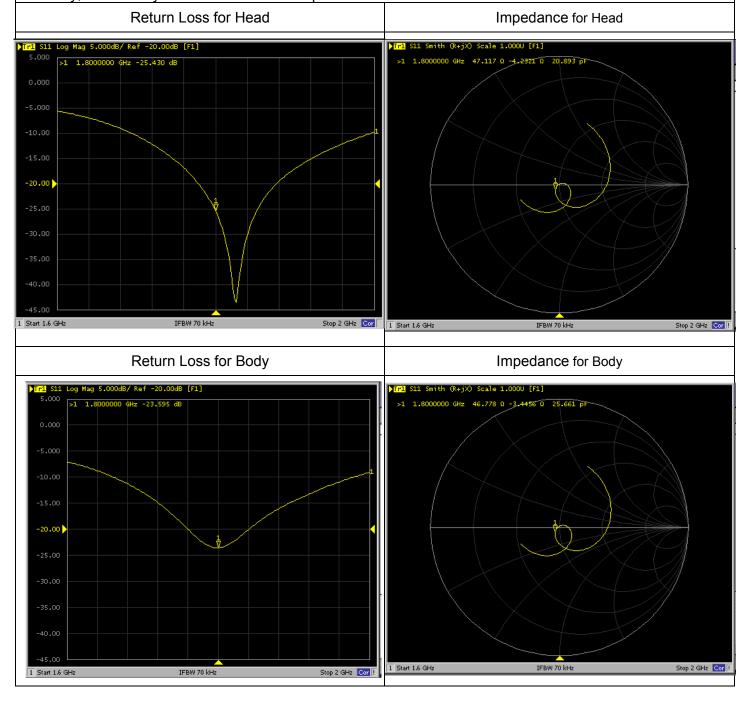

## Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

SGS-SZ (Auden)

Accreditation No.: SCS 108

Certificate No: D1900V2-5d028\_Nov13

## CALIBRATION CERTIFICATE

Object D1900V2 - SN: 5d028

Calibration procedure(s) QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

Calibration date: November 27, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	US37292783	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01828)	Oct-14
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-13 (No. 217-01736)	Apr-14
Type-N mismatch combination	SN: 5047.3 / 06327	04-Apr-13 (No. 217-01739)	Apr-14
Reference Probe ES3DV3	SN: 3205	28-Dec-12 (No. ES3-3205_Dec12)	Dec-13
DAE4	SN: 601	25-Apr-13 (No. DAE4-601_Apr13)	Apr-14
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-15
	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

Calibrated by:

Jeton Kastrati Laboratory Technician

Approved by:

Katja Pokovic Technical Manager

Issued: November 27, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D1900V2-5d028\_Nov13

## Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S wiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

### Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

## Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D1900V2-5d028\_Nov13 Page 2 of 8

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

## **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.39 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.2 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.9 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.33 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.4 W/kg ± 16.5 % (k=2)

## **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.4 ± 6 %	1.51 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	****	

## SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.1 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	40.6 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.39 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.6 W/kg ± 16.5 % (k=2)

Page 3 of 8

Certificate No: D1900V2-5d028\_Nov13

## **Appendix**

## Antenna Parameters with Head TSL

Impedance, transformed to feed point	$50.8 \Omega + 6.8 j\Omega$	
Return Loss	- 23.4 dB	

## Antenna Parameters with Body TSL

Impedance, transformed to feed point	$46.6 \Omega + 6.8 jΩ$	
Return Loss	- 22.1 dB	

## General Antenna Parameters and Design

Electrical Delay (one direction)	1.201 ns
The state of the s	

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG	
Manufactured on	December 17, 2002	

Certificate No: D1900V2-5d028\_Nov13

## **DASY5 Validation Report for Head TSL**

Date: 27.11.2013

Test Laboratory: SPEAG, Zurich, Switzerland

## DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d028

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz;  $\sigma = 1.39 \text{ S/m}$ ;  $\varepsilon_r = 39.8$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.98, 4.98, 4.98); Calibrated: 28.12.2012;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 25.04.2013

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

## Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 97.112 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 18.6 W/kg


SAR(1 g) = 10.2 W/kg; SAR(10 g) = 5.33 W/kg

Maximum value of SAR (measured) = 12.5 W/kg

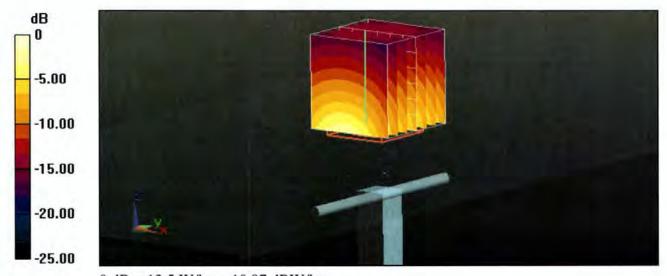

0 dB = 12.5 W/kg = 10.97 dBW/kg

## Impedance Measurement Plot for Head TSL

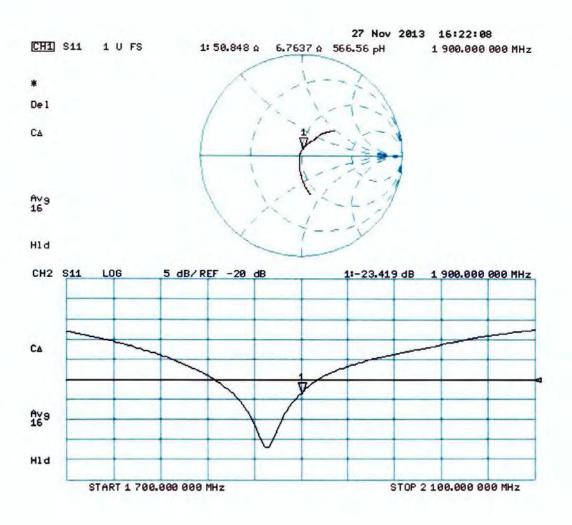

## **DASY5 Validation Report for Body TSL**

Date: 27.11.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d028

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz;  $\sigma = 1.51 \text{ S/m}$ ;  $\varepsilon_r = 53.4$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.6, 4.6, 4.6); Calibrated: 28.12.2012;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 25.04.2013

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

## Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.784 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 17.3 W/kg


SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.39 W/kg

Maximum value of SAR (measured) = 12.6 W/kg

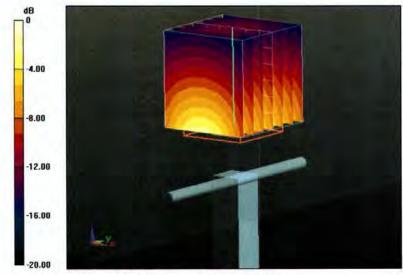

0 dB = 12.6 W/kg = 11.00 dBW/kg

## Impedance Measurement Plot for Body TSL

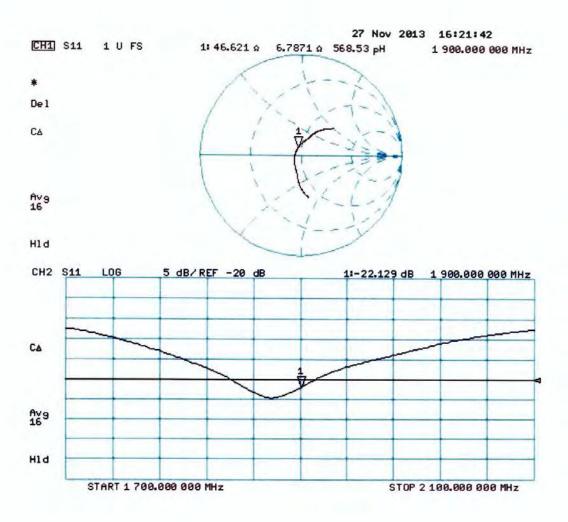


# SGS-CSTC Standards Technical Services Co., Ltd. Shenzhen Branch

Dipole Calibration for Impedance and Return-loss							
Model NO.:	D1900V2	Serial NO.:	5d082	Measurement Date:	2015-11-25		
	Target Value:		Target Value: Measured Value:		Measured Value:		
Liquid Type	Impedance	Return Loss	Impedance	Return Loss	verdict		
Head	50.8Ω+6.8jΩ	-23.4dB	50.3Ω+7.3jΩ	-23.3dB	Complied		
Body	46.6Ω+6.8jΩ	-22.1dB	46.3Ω+6.6jΩ	-22.9dB	Complied		

Remark: According to KDB 865664 D01,instead of the typical annual calibration recommended by measurement standards, longer calibration intervals of up to three years may be considered when it is demonstrated that the SAR target, impedance and return loss of a dipole have remain stable according to the following requirements:

- 1) The most recent return-loss result, measured at least annually, deviates by less than 20% from the previous measurement and meeting the required 20 dB minimum return-loss requirement.
- 2) The most recent measurement of the real and imaginary parts of the impedance, measured at least annually, deviates by less than 5  $\Omega$  from the previous measurement.

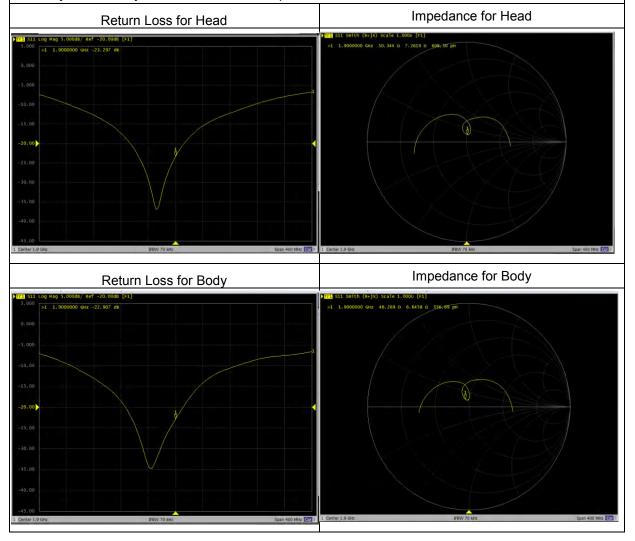

## Calibration Laboratory of Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage C Servizio svizzero di taratura **Swiss Calibration Service** 

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

SGS-SZ (Auden)

Certificate No: D2450V2-733\_Nov13

Accreditation No.: SCS 108

## **ALIBRATION CERTIFICATE**

D2450V2 - SN: 733 Object

QA CAL-05.v9 Calibration procedure(s)

Calibration procedure for dipole validation kits above 700 MHz

Calibration date: November 26, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	US37292783	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01828)	Oct-14
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-13 (No. 217-01736)	Apr-14
Type-N mismatch combination	SN: 5047.3 / 06327	04-Apr-13 (No. 217-01739)	Apr-14
Reference Probe ES3DV3	SN: 3205	28-Dec-12 (No. ES3-3205_Dec12)	Dec-13
DAE4	SN: 601	25-Apr-13 (No. DAE4-601_Apr13)	Apr-14
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-15
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14
	Name	Function	Signature
Calibrated by:	Claudio Leubler	Laboratory Technician	

Calibrated by:

Katja Pokovic Technical Manager Approved by:

Issued: November 26, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D2450V2-733\_Nov13

Page 1 of 8

## Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

## Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

## **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, $dy$ , $dz = 5 mm$	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.7 ± 6 %	1.84 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.2 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.4 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.10 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.3 W/kg ± 16.5 % (k=2)

## **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.1 ± 6 %	2.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	1.450	

## SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.6 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	49.4 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.81 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.0 W/kg ± 16.5 % (k=2)

Page 3 of 8 Certificate No: D2450V2-733\_Nov13

## **Appendix**

## **Antenna Parameters with Head TSL**

Impedance, transformed to feed point	$54.2 \Omega + 2.5 j\Omega$	
Return Loss	- 26.6 dB	

## Antenna Parameters with Body TSL

Impedance, transformed to feed point	$51.0 \Omega + 4.2 j\Omega$	
Return Loss	- 27.5 dB	

## **General Antenna Parameters and Design**

·	
Electrical Delay (one direction)	1.149 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	May 07, 2003

Certificate No: D2450V2-733\_Nov13 Page 4 of 8