





## ANNEX B – RELEVANT PAGES FROM CALIBRATION REPORTS

DAE4 Sn:546

<div style="text-align: center;">   </div> <p style="text-align: center;">In Collaboration with <b>TTL s p e e g</b> CALIBRATION LABORATORY</p> <p style="text-align: center;">中国认可 国际互认 校准 CALIBRATION CNAS L6570</p> <p>ADD: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62596313-2312 Fax: +86-10-62596313-2304 E-mail: cal@ttsl.com.cn http://www.ttsl.com.cn</p> <p>Client: <b>SRTC</b> Certificate No: <b>Z18-60400</b></p> <div style="border: 1px solid black; padding: 5px;"> <p style="text-align: center;"><b>CALIBRATION CERTIFICATE</b></p> <p>Object: DAE4 - SN: 546</p> <p>Calibration Procedure(s): FF-Z11-002-01 Calibration Procedure for the Data Acquisition Electronics (DAEx)</p> <p>Calibration date: October 15, 2018</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature(23±3)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date(Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Process Calibrator 793</td> <td>1971018</td> <td>20-Jun-19 (CTTL, No.J18XG5034)</td> <td>June-19</td> </tr> </tbody> </table> <p>Calibrated by: Yu Zengying SAR Test Engineer</p> <p>Reviewed by: Lin Han SAR Test Engineer</p> <p>Approved by: Qi Dianyan SAR Project Leader</p> <p style="text-align: right;">Issued: October 17, 2018</p> <p style="font-size: small;">This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> </div> <p style="text-align: center; font-size: x-small;">Certificate No: Z18-60400 Page 1 of 3</p>	Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration	Process Calibrator 793	1971018	20-Jun-19 (CTTL, No.J18XG5034)	June-19	<div style="text-align: center;">  </div> <p style="text-align: center;">In Collaboration with <b>TTL s p e e g</b> CALIBRATION LABORATORY</p> <p style="text-align: center;">中国认可 国际互认 校准 CALIBRATION CNAS L6570</p> <p>ADD: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62596313-2312 Fax: +86-10-62596313-2304 E-mail: cal@ttsl.com.cn http://www.ttsl.com.cn</p> <p><b>Glossary:</b> DAE: data acquisition electronics Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system.</p> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li><b>DC Voltage Measurement:</b> Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.</li> <li><b>Connector angle:</b> The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.</li> <li>The report provide only calibration results for DAE, it does not contain other performance test results.</li> </ul> <p style="text-align: center; font-size: x-small;">Certificate No: Z18-60400 Page 2 of 3</p>
Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration						
Process Calibrator 793	1971018	20-Jun-19 (CTTL, No.J18XG5034)	June-19						



In Collaboration with  
**TTL s p e e g**  
CALIBRATION LABORATORY

中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L6570

ADD: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62596313-2312 Fax: +86-10-62596313-2304  
E-mail: cal@ttsl.com.cn http://www.ttsl.com.cn

**DC Voltage Measurement**  
ADC Converter Resolution nominal  
High Range: 1LSB = 5.1μV, full range = -100...+300 mV  
Low Range: 1LSB = 819V, full range = -1...+3mV  
DASY measurement parameter: Auto GARD 1 time, 3 sec, Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	405.306 ± 0.15% (k=2)	404.259 ± 0.15% (k=2)	404.180 ± 0.15% (k=2)
Low Range	3.98993 ± 0.7% (k=2)	3.95978 ± 0.7% (k=2)	3.98021 ± 0.7% (k=2)

**Connector Angle**

Connector Angle to be used in DASY system	238° ± 1°
---	-----------

Certificate No: Z.8-60400 Page 3 of 3

ES3DV3 Sn:3127



Client: SRTC Certificate No: Z18-60398

**CALIBRATION CERTIFICATE**

Object: ES3DV3 - SN:3127

Calibration Procedure(s): FF-Z11-004-01  
Calibration Procedures for Dosimetric E-field Probes

Calibration date: November 02, 2018

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature(23±3)°C and humidity<70%.

Calibration Equipment used (M&E critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by Certificate No.)	Scheduled Calibration
Power Meter	NRP2 101919	20-Jun-18 (CTTL No.J18X05032)	Jun-19
Power sensor	NRP-Z91 101547	20-Jun-18 (CTTL No.J18X05032)	Jun-19
Power sensor	NRP-Z91 101548	20-Jun-18 (CTTL No.J18X05032)	Jun-19
Reference10dBAttenuator	18N50W-10dB	09-Feb-18(CTTL No.J18X01133)	Feb-20
Reference20dBAttenuator	18N50W-20dB	09-Feb-18(CTTL No.J18X01133)	Feb-20
Reference Probe EX3DV4	SN 3846	25-Jan-18(GPEAG No.EK3-3846_Jan18)	Jan-19
DAE4	SN 777	15-Dec-17(GPEAG No.DAE4-777_Dec17)	Dec-18
Secondary Standards	ID #	Cal Date(Calibrated by Certificate No.)	Scheduled Calibration
SignalGeneratorMG3700A	6201052605	21-Jun-18 (CTTL No.J18X05033)	Jun-19
NetworkAnalyzer E5071C	M746110673	14-Jan-18 (CTTL No.J18X00561)	Jan-19

Calibrated by: Yu Zongying SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyuan SAR Project Leader

Issued: November 04, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z18-60398 Page 1 of 11



**Glossary:**

TS: tissue simulating liquid

NORM<sub>x,y,z</sub>: sensitivity in free space

ComF: sensitivity in TSL / NORM<sub>x,y,z</sub>

DCP: diode compression point

CF: crest factor (1/Mod<sub>cycle</sub>) of the RF signal

A, E, C, D: modulation dependent linearization parameters

φ: rotation around probe axis

Polarization θ: θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i

θ=0 is normal to probe axis

Connector Angle: information used in DASY system to align probe sensor K to the root coordinate system

**Calibration is Performed According to the following standards:**

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2016
- KDB 865654, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Methods Applied and Interpretation of Parameters:**

- NORM<sub>x,y,z</sub>: Assessed for E-field polarization θ=0 (5000MHz in TEM-cell; f>1800MHz: waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e. the uncertainties of NORM<sub>x,y,z</sub> does not affect the  $k^2$ -field uncertainty inside TSL (see below ComF).
- NORM(f);  $y,z = NORM_{x,y,z}$ : frequency response (see Frequency Response Chart). This linearization is implemented in DASYV4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ComF.
- DCP<sub>x,y,z</sub>: DCP are numerical linearization parameters assessed using the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A<sub>x,y,z</sub>, B<sub>x,y,z</sub>, C<sub>x,y,z</sub>, V<sub>PK</sub>, Z<sub>0</sub>, M, C: are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VB is the maximum calibration range expressed in RMS voltage across the diode.
- ComF and Boundary Effect Parameters Assessed in flat phantom using E-field (or Temperature Transfer Standard for 500MHz) and inside waveguide using analytical field distributions based on power measurements for f>600MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASYV4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> ComF whereas the uncertainty corresponds to that given for ComF. A frequency dependent ComF is used in DASY version 4.4 and higher which allows extending the validity from 50MHz to 100MHz.
- Spherical isotropy (SD observation from isotropy):  $k^2$  field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: the angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

Certificate No: Z18-60398 Page 2 of 11

Probe ES3DV3

SN: 3127

Calibrated: November 02, 2018

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: Z18-60398

Page 3 of 11



Address: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-42304633-2312 Fax: +86-10-42304633-2504  
E-mail: cnt@china.ttl.com.cn Http://www.chinatit.com

**DASY/EASY – Parameters of Probe: ES3DV3 - SN: 3127**

**Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm( $\mu V/(V/m)^2$ ) <sup>A</sup>	1.27	1.26	1.21	$\pm 10.0\%$
DCP(mV) <sup>B</sup>	103.3	104.4	105.0	

**Modulation Calibration Parameters**

UID	Communication System Name	A dB	B dB- $\mu V$	C	D dB	VR mV	Unc <sup>C</sup> (k=2)
0	CW	X 0.0	0.0	1.0	0.00	285.6	$\pm 2.2\%$
		Y 0.0	0.0	1.0		287.9	
		Z 0.0	0.0	1.0		282.9	

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X, Y, Z do not affect the E<sup>2</sup> field uncertainty inside TSL (see Page 5 and Page 6).  
<sup>B</sup> Numerical linearization parameter; uncertainty not required.  
<sup>C</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



Address: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-42304633-2312 Fax: +86-10-42304633-2504  
E-mail: cnt@china.ttl.com.cn Http://www.chinatit.com

**DASY/EASY – Parameters of Probe: ES3DV3 - SN: 3127**

**Calibration Parameter Determined in Head Tissue Simulating Media**

f [MHz] <sup>E</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>G</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>H</sup>	Depth <sup>I</sup> (mm)	Unc. (k=2)
750	41.9	0.99	6.34	6.34	6.34	0.40	1.35	$\pm 12.1\%$
835	41.5	0.90	6.18	6.18	6.18	0.35	1.58	$\pm 12.1\%$
1810	40.0	1.40	5.07	5.07	5.07	0.68	1.24	$\pm 12.1\%$
2000	40.0	1.40	4.96	4.96	4.96	0.70	1.20	$\pm 12.1\%$
2300	39.6	1.67	4.79	4.79	4.79	0.90	1.08	$\pm 12.1\%$
2450	39.2	1.80	4.66	4.66	4.66	0.90	1.08	$\pm 12.1\%$
2600	39.0	1.96	4.40	4.40	4.40	0.80	1.21	$\pm 12.1\%$

<sup>E</sup> Frequency validity above 300 MHz of  $\pm 100$  MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to  $\pm 50$  MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is  $\pm 10, 25, 40, 50$  and  $70$  MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to  $\pm 10$  MHz.  
<sup>F</sup> At frequency below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm 10\%$  if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm 5\%$ . The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.  
<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than  $\pm 1\%$  for frequencies below 3 GHz and below  $\pm 2\%$  for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



Address: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-42304633-2312 Fax: +86-10-42304633-2504  
E-mail: cnt@china.ttl.com.cn Http://www.chinatit.com

**DASY/EASY – Parameters of Probe: ES3DV3 - SN: 3127**

**Calibration Parameter Determined in Body Tissue Simulating Media**


f [MHz] <sup>E</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>G</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>H</sup>	Depth <sup>I</sup> (mm)	Unc. (k=2)
750	55.5	0.96	6.33	6.33	6.33	0.40	1.40	$\pm 12.1\%$
835	55.2	0.87	6.13	6.13	6.13	0.37	1.62	$\pm 12.1\%$
1810	53.3	1.52	4.78	4.78	4.78	0.65	1.27	$\pm 12.1\%$
2000	53.3	1.52	4.80	4.80	4.80	0.67	1.27	$\pm 12.1\%$
2300	52.9	1.81	4.46	4.46	4.46	0.90	1.16	$\pm 12.1\%$
2450	52.7	1.95	4.31	4.31	4.31	0.78	1.28	$\pm 12.1\%$
2600	52.6	2.16	4.14	4.14	4.14	0.90	1.10	$\pm 12.1\%$

<sup>E</sup> Frequency validity above 300 MHz of  $\pm 100$  MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to  $\pm 50$  MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is  $\pm 10, 25, 40, 50$  and  $70$  MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to  $\pm 10$  MHz.  
<sup>F</sup> At frequency below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm 10\%$  if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm 5\%$ . The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.  
<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than  $\pm 1\%$  for frequencies below 3 GHz and below  $\pm 2\%$  for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



Address: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-42304633-2312 Fax: +86-10-42304633-2504  
E-mail: cnt@china.ttl.com.cn Http://www.chinatit.com

**Frequency Response of E-Field (TEM-Cell: If110 EXX, Waveguide: R22)**

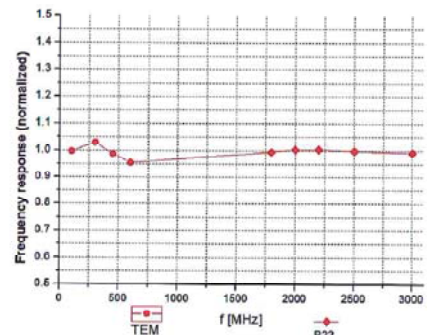


Uncertainty of Frequency Response of E-field:  $\pm 7.4\%$  (k=2)





In Collaboration with  
TTL Speaq  
CALIBRATION LABORATORY  
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2312 Fax: +86-10-62304633-2304  
E-mail: csl@ttspeaq.com.cn http://www.ttspeaq.com

Receiving Pattern ( $\Phi$ ),  $\theta=0^\circ$

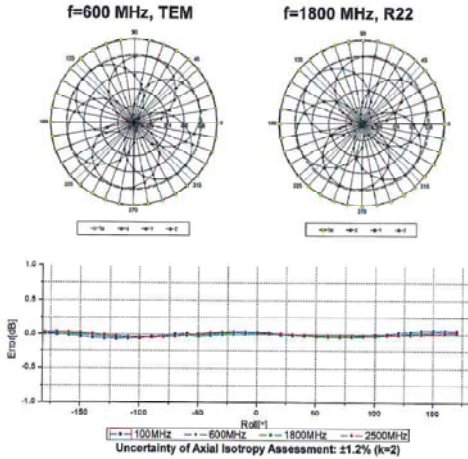


In Collaboration with  
TTL Speaq  
CALIBRATION LABORATORY  
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2312 Fax: +86-10-62304633-2304  
E-mail: csl@ttspeaq.com.cn http://www.ttspeaq.com

Dynamic Range f(SAR<sub>head</sub>)  
(TEM cell, f = 900 MHz)

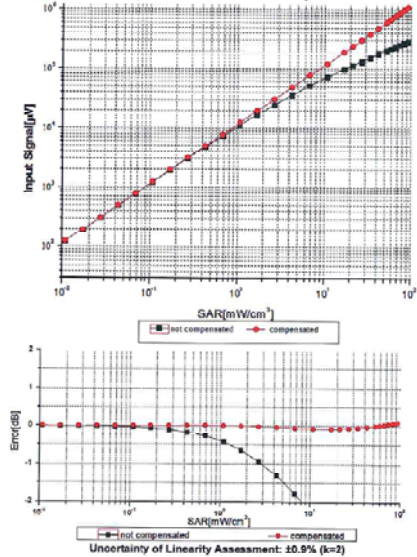


In Collaboration with  
TTL Speaq  
CALIBRATION LABORATORY  
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2312 Fax: +86-10-62304633-2304  
E-mail: csl@ttspeaq.com.cn http://www.ttspeaq.com

Conversion Factor Assessment

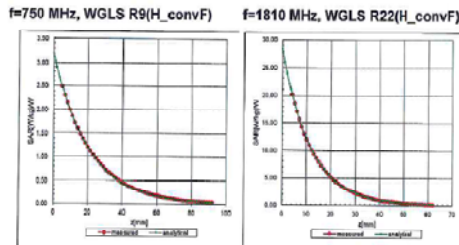

Deviation from Isotropy in Liquid

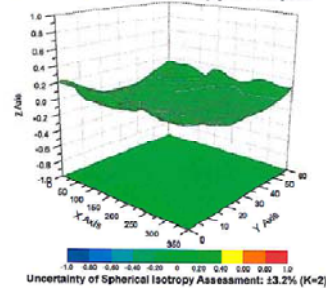

In Collaboration with  
TTL Speaq  
CALIBRATION LABORATORY  
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2318 Fax: +86-10-62304633-2309  
E-mail: csl@ttspeaq.com.cn http://www.ttspeaq.com

Appendix: Modulation Calibration Parameters

UID	Communication System Name	PAR	A dB	B dB $\mu$ V	C	VR mV	Unc <sup>±</sup> (k=2)
0	CW	0.00	X	0.0	0.0	1.0	282.3
			Y	0.0	0.0	1.0	280.9
			Z	0.0	0.0	1.0	275.1
10012	IEEE 802.11b WIFI 2.4 GHz (DSSS, 1 Mbps)	1.87	X	2.77	68.02	18.46	143.0
			Y	2.75	68.05	18.52	145.0
			Z	2.71	67.79	18.25	142.3
10100	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	5.67	X	6.13	66.4	18.97	141.9
			Y	6.15	66.49	19.06	144.2
			Z	6.09	66.32	18.90	140.9
10108	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	5.80	X	6.09	66.24	19.07	139.5
			Y	6.10	66.33	19.15	141.5
			Z	6.05	66.19	19.05	138.0
10154	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	5.75	X	5.81	65.85	18.93	136.1
			Y	5.82	65.92	19.01	137.8
			Z	5.79	65.89	18.97	134.7
10169	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	5.73	X	4.84	65.92	19.20	130.8
			Y	4.82	65.98	19.27	131.3
			Z	4.80	66.00	19.29	129.1
10175	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	5.72	X	4.88	66.14	19.40	131.6
			Y	4.83	66.08	19.33	130.9
			Z	4.79	66.02	19.29	129.3
10297	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	5.81	X	6.19	66.61	19.42	141.9
			Y	6.13	66.43	19.26	140.7
			Z	6.14	66.52	19.33	139.6



DAE4 Sn:720

In Collaboration with  
**TTL s p e e g**  
CALIBRATION LABORATORY

中国认可  
国际互认  
校准  
CNAS L6579

Address: No.51 Xuyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62306633-2512 Fax: +86-10-62306633-2504  
E-mail: csl@chinaeet.com http://www.chinaeet.com

Client: SRTC Certificate No: Z18-60399

**CALIBRATION CERTIFICATE**

Object: DAE4 - SN: 720

Calibration Procedure(s): FF-Z11-002-01  
Calibration Procedure for the Data Acquisition Electronics (DAEx)

Calibration date: October 15, 2018

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(23±3)°C and humidity<70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Process Calibrator 753	1971018	20-Jun-18 (CTTL, No.J18X05034)	June-19

Calibrated by:	Name	Function	Signature
	Yu Zongying	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyuan	SAR Project Leader	

Issued: October 17, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

In Collaboration with  
**TTL s p e e g**  
CALIBRATION LABORATORY

中国认可  
国际互认  
校准  
CNAS L6579

Address: No.51 Xuyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62306633-2512 Fax: +86-10-62306633-2504  
E-mail: csl@chinaeet.com http://www.chinaeet.com

Client: SRTC Certificate No: Z18-60399

**Glossary:**

DAE: data acquisition electronics  
Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system.

**Methods Applied and Interpretation of Parameters:**

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.

In Collaboration with  
**TTL s p e e g**  
CALIBRATION LABORATORY

中国认可  
国际互认  
校准  
CNAS L6579

Address: No.51 Xuyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62306633-2512 Fax: +86-10-62306633-2504  
E-mail: csl@chinaeet.com http://www.chinaeet.com

**DC Voltage Measurement**

A/D - Converter Resolution nominal  
High Range: 1LSB = 6.1µV, full range = -100...+300 mV  
Low Range: 1LSB = 61nV, full range = -1...+30mV  
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	403.343 ± 0.15% (k=2)	404.773 ± 0.15% (k=2)	403.208 ± 0.15% (k=2)
Low Range	3.95574 ± 0.7% (k=2)	3.95589 ± 0.7% (k=2)	3.95585 ± 0.7% (k=2)

**Connector Angle**

Connector Angle to be used in DASY system	Value
Connector Angle to be used in DASY system	25° ± 1°

EX3DV4 Sn:3708 (1/7)

Calibration Laboratory of Schmid & Partner Engineering AG  
Zugstrasse 43, 8004 Zurich, Switzerland

Schweizerischer Kollaborations Service suisse d'Etalonnage Service svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0106

Client: SRTC (Auden) Certificate No: EX3-3708\_Oct18

**CALIBRATION CERTIFICATE**

Object: EX3DV4 - SN:3708

Calibration procedure(s): QA CAL-01-v8, QA CAL-12-v8, QA CAL-14-v4, QA CAL-23-v6, QA CAL-25-v8  
Calibration procedure for dosimetric E-field probes

Calibration date: October 22, 2018

This calibration certificate documents the traceability to national standards, which include the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the stated laboratory facility, environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID	Call Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 184779	08-Apr-18 (No. 217-0887920879)	Apr-19
Power sensor NRP-231	SN: 183244	08-Apr-18 (No. 217-08879)	Apr-19
Power sensor NRP-231	SN: 183345	08-Apr-18 (No. 217-08873)	Apr-19
Reference 30 dB Attenuator	SN: 88377 (25b)	08-Apr-18 (No. 217-08883)	Apr-19
Reference Probe E587W2	SN: 2615	20-Dec-17 (No. 028-19015-06e17)	Dec-18
OMG	SN: 660	20-Dec-17 (No. 0484-660-06e17)	Dec-18

Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4418B	SN: 0841220274	06-Apr-18 (in house check Jun-18)	In house check Jun-20
Power sensor E4412A	SN: M74189327	06-Apr-18 (in house check Jun-18)	In house check Jun-20
Power sensor E4412A	SN: M5111219	06-Apr-18 (in house check Jun-18)	In house check Jun-20
RF generator HP 8546C	SN: 163646301700	03-Aug-09 (in house check Jun-18)	In house check Jun-20
Network Analyser F8358A	SN: U841080477	31-Mar-14 (in house check Oct-18)	In house check Oct-19

Calibrated by: Gerdin Louche Laboratory Technician

Approved by: Kjetil Phalick Technical Manager

Issued: October 23, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX3-3708\_Oct18 Page 1 of 39

Calibration Laboratory of Schmid & Partner Engineering AG  
Zugstrasse 43, 8004 Zurich, Switzerland

Schweizerischer Kollaborations Service suisse d'Etalonnage Service svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client: SRTC (Auden) Certificate No: EX3-3708\_Oct18

**Glossary:**

TSL: Issue simulating liquid  
sensitivity in free space  
sensitivity in TSL / NORM<sub>M,y,z</sub>  
DCP: diode compression point  
CF: crest factor (10duty\_cycle) of the RF signal  
A, B, C, D: modulation dependent linearization parameters  
Polarization  $\phi$ :  $\phi$  rotation around probe axis  
Polarization  $\theta$ :  $\theta$  rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e.,  $\theta = 0$  is normal to probe axis  
Connector Angle: information used in DASY system to align probe sensor X to the robot coordinate system

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2019
- KDB 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Methods Applied and Interpretation of Parameters:**

- NORM<sub>M,y,z</sub>: Assessed for E-field polarization  $\theta = 0$  (if  $\pm 900$  MHz in TEM-cell,  $f > 1800$  MHz: R22 wireguide). NORM<sub>M,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>M,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM<sub>M,y,z</sub> = NORM<sub>M,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>y,z</sub>: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required), DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A<sub>x,y,z</sub>, B<sub>x,y,z</sub>, C<sub>x,y,z</sub>, D<sub>x,y,z</sub>, VR<sub>x,y,z</sub>: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f < 800$  MHz) and inside neoprene using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>M,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 90$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom required by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORM (no uncertainty required).

Certificate No: EX3-3708\_Oct18 Page 2 of 39

EX3DV4 - SN:3708 October 22, 2018

**Probe EX3DV4**

**SN:3708**

Manufactured: July 21, 2009  
Calibrated: October 22, 2018

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

Certificate No: EX3-3708\_Oct18 Page 3 of 39

EX3DV4 - SN:3708 October 22, 2018

**DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708**

**Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (km2)
Norm (µV/m) <sup>2</sup>	0.20	0.35	0.42	± 10.1 %
DCP (mV)	95.4	103.6	100.4	

**Modulation Calibration Parameters**

URD	Communication System Name	A	B	C	D	VR	Unc <sup>a</sup> (km2)
C	CW	X	0.0	0.0	1.0	0.00	134.7 ± 8.6 %
		Y	0.0	0.0	1.0	0.00	130.8 ± 8.6 %
		Z	0.0	0.0	1.0	0.00	146.5 ± 8.6 %

Note: For details on URD parameters see Appendix.

**Sensor Model Parameters**

CF	C2	a	T1	T2	T3	T4	T5	T6
ms.V <sup>-1</sup>	ms.V <sup>-1</sup>	ms.V <sup>-1</sup>	ms.V <sup>-1</sup>	ms.V <sup>-1</sup>	ms.V <sup>-1</sup>	ms.V <sup>-1</sup>	ms.V <sup>-1</sup>	ms.V <sup>-1</sup>
X	33.84	270.1	40.07	9.383	1.302	0.102	0.006	0.762
Y	42.04	291.1	34.06	13.47	0.801	0.112	1.758	0.196
Z	38.84	282.2	35.97	11.65	0.630	0.031	0.000	0.009

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>a</sup> The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 1 and 6).  
<sup>b</sup> Numerical linearization parameter, uncertainty not required.  
<sup>c</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: EX3-3708\_Oct18 Page 4 of 39

EX3DV4 Sn:3708 (2/7)

EX3DV4- SN:3708

October 22, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>1</sup>	Relative Permittivity <sup>2</sup>	Conductivity (S/m) <sup>2</sup>	CorrF X	CorrF Y	CorrF Z	Alpha <sup>3</sup>	Depth (mm)	Unc (k=2)
450	43.5	0.87	9.79	9.79	9.79	0.54	1.20	± 13.3 %
750	41.9	0.89	9.59	9.59	9.59	0.54	0.80	± 12.0 %
835	41.5	0.90	9.16	9.16	9.16	0.51	0.82	± 12.0 %
1450	40.5	1.20	8.50	8.50	8.50	0.33	0.80	± 12.0 %
1750	40.1	1.37	8.20	8.20	8.20	0.28	0.94	± 12.0 %
1900	40.0	1.40	7.89	7.89	7.89	0.35	0.85	± 12.0 %
2000	40.0	1.40	7.86	7.86	7.86	0.34	0.80	± 12.0 %
2300	39.5	1.67	7.51	7.51	7.51	0.29	0.86	± 12.0 %
2480	39.2	1.80	7.13	7.13	7.13	0.38	0.86	± 12.0 %
2600	39.0	1.96	7.01	7.01	7.01	0.36	0.87	± 12.0 %
5200	35.0	4.66	5.46	5.46	5.46	0.40	1.80	± 13.1 %
5300	35.0	4.78	5.25	5.25	5.25	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.84	4.84	4.84	0.40	1.80	± 13.1 %
5800	30.3	5.27	5.04	5.04	5.04	0.40	1.80	± 13.1 %

<sup>1</sup> Frequency validity above 300 MHz of a 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to a 10 MHz. The uncertainty is the RSS of the CorrF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 20, 40, 50 and 70 MHz for CorrF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 3 GHz frequency validity can be extended to a 1% MHz.  
<sup>2</sup> At frequencies below 3 GHz, the validity of tissue parameters (μ and σ) can be related to a 10% liquid compensation formula is applied to measured S11 values. At frequencies above 3 GHz, the validity of tissue parameters (μ and σ) is restricted to ± 3%. The uncertainty is the RSS of the CorrF uncertainty for indicated target tissue parameters.  
<sup>3</sup> AlphaDepth was determined during calibration. SRTCAC warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe diameter from the boundary.

Certificate No: EX3-3708\_Oct18

Page 5 of 39

EX3DV4- SN:3708

October 22, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>1</sup>	Relative Permittivity <sup>2</sup>	Conductivity (S/m) <sup>2</sup>	CorrF X	CorrF Y	CorrF Z	Alpha <sup>3</sup>	Depth (mm)	Unc (k=2)
450	56.7	0.94	10.35	10.35	10.35	0.68	1.20	± 13.3 %
750	55.5	0.96	9.51	9.51	9.51	0.50	0.85	± 12.0 %
835	55.2	0.97	9.33	9.33	9.33	0.47	0.84	± 12.0 %
1450	54.0	1.30	7.84	7.84	7.84	0.38	0.80	± 12.0 %
1750	53.4	1.49	7.69	7.69	7.69	0.37	0.85	± 12.0 %
1900	53.3	1.52	7.56	7.56	7.56	0.42	0.84	± 12.0 %
2000	53.3	1.52	7.53	7.53	7.53	0.41	0.85	± 12.0 %
2300	52.9	1.81	7.34	7.34	7.34	0.39	0.86	± 12.0 %
2480	52.7	1.95	7.19	7.19	7.19	0.33	0.85	± 12.0 %
2600	52.5	2.16	7.14	7.14	7.14	0.32	0.85	± 12.0 %
5200	49.0	5.30	4.53	4.53	4.53	0.50	1.90	± 13.1 %
5300	48.9	5.42	4.41	4.41	4.41	0.50	1.90	± 13.1 %
5600	48.8	5.77	3.99	3.99	3.99	0.50	1.90	± 13.1 %
5800	48.2	6.00	4.21	4.21	4.21	0.50	1.90	± 13.1 %

<sup>1</sup> Frequency validity above 300 MHz of a 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to a 10 MHz. The uncertainty is the RSS of the CorrF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 20, 40, 50 and 70 MHz for CorrF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 3 GHz frequency validity can be extended to a 1% MHz.  
<sup>2</sup> At frequencies below 3 GHz, the validity of tissue parameters (μ and σ) can be related to a 10% liquid compensation formula is applied to measured S11 values. At frequencies above 3 GHz, the validity of tissue parameters (μ and σ) is restricted to ± 3%. The uncertainty is the RSS of the CorrF uncertainty for indicated target tissue parameters.  
<sup>3</sup> AlphaDepth was determined during calibration. SRTCAC warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe diameter from the boundary.


Certificate No: EX3-3708\_Oct18

Page 6 of 39

EX3DV4- SN:3708

October 22, 2018

Frequency Response of E-Field  
(TEM-Cell:IH110 EXX, Waveguide: R22)

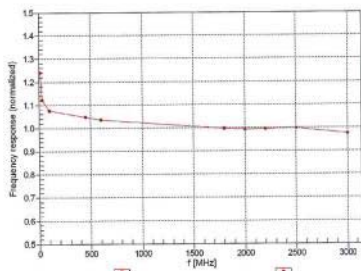

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)



Certificate No: EX3-3708\_Oct18

Page 7 of 39

EX3DV4- SN:3708

October 22, 2018

Receiving Pattern (φ), θ = 0°

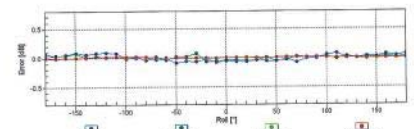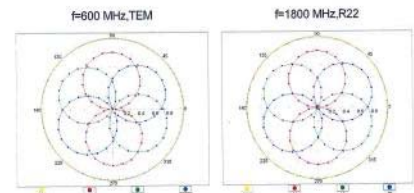

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: EX3-3708\_Oct18



Page 9 of 39

EX3DV4 Sn:3708 (3/7)

EX3DV4-SN3708

October 22, 2018

**Dynamic Range f(SAR<sub>head</sub>)**  
(TEM cell, f<sub>max</sub>=1900 MHz)

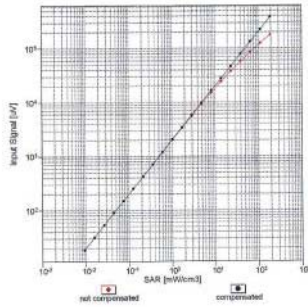

Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Certificate No: EX3-3708\_Out18

Page 9 of 38


EX3DV4-SN3708

October 22, 2018

**Conversion Factor Assessment**

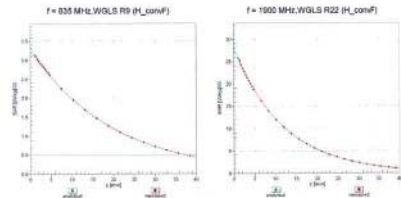

**Deviation from Isotropy in Liquid**  
Error (ϕ, θ), f = 900 MHz

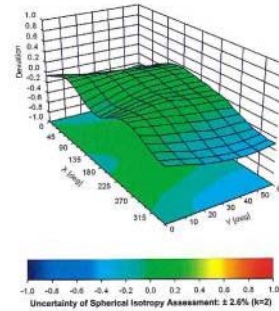

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: EX3-3708\_Out18

Page 10 of 38

EX3DV4-SN3708

October 22, 2018

**DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708**

**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	0.5
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Certificate No: EX3-3708\_Out18

Page 11 of 38



EX3DV4 Sn:3708 (4/7)

EX3DV4- SN:3708 October 22, 2018

Appendix: Modulation Calibration Parameters

Mod. Communication System Name	A dB	B dB $\mu$ V	C	D dB	VR mV	Max Ume (dBm)
0 CW	0.00	0.00	1.00	0.00	134.7	$\pm 3.5\%$
10010-CAA SAR Validation (Square, 100ms, 10ms)	2.38	85.10	8.80	10.00	20.0	$\pm 0.8\%$
10011-CAB UHF5-FDD (WCDMA)	1.99	86.70	18.45	15.00	50.0	$\pm 0.6\%$
10012-CAB IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	1.01	85.94	14.96	0.41	150.0	$\pm 0.6\%$
10013-CAB IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 6 Mbps)	1.17	84.69	15.71	15.00	50.0	$\pm 0.6\%$
10021-DAC GSM-FDD (TDMA, GMSK)	0.01	75.83	15.85	9.38	50.0	$\pm 0.6\%$
10023-DAC GPRS-FDD (TDMA, GMSK, TN 0)	0.00	100.32	23.48	50.0	50.0	$\pm 0.6\%$
10024-DAC GPRS-FDD (TDMA, GMSK, TN 0-1)	0.00	100.43	23.68	50.0	50.0	$\pm 0.6\%$
10025-DAC EDGE-FDD (TDMA, BPSK, TN 0)	0.00	100.46	23.85	50.0	50.0	$\pm 0.6\%$
10026-DAC EDGE-FDD (TDMA, BPSK, TN 0-1)	0.00	100.48	23.98	50.0	50.0	$\pm 0.6\%$
10027-DAC GPRS-FDD (TDMA, GMSK, TN 0-1-2)	0.00	100.50	24.02	50.0	50.0	$\pm 0.6\%$
10028-DAC GPRS-FDD (TDMA, GMSK, TN 0-1-3-3)	0.00	100.52	24.08	50.0	50.0	$\pm 0.6\%$
10029-DAC EDGE-FDD (TDMA, BPSK, TN 0-1-2)	0.00	100.55	24.15	50.0	50.0	$\pm 0.6\%$
10030-CAA IEEE 802.15.1 Bluetooth (QPSK, DH1)	1.56	87.01	10.18	0.30	70.0	$\pm 0.6\%$
10031-CAA IEEE 802.15.1 Bluetooth (QPSK, DH3)	1.00	100.48	23.10	1.88	100.0	$\pm 0.6\%$

Certificate No: EX3-3708\_Out8 Page 12 of 39

EX3DV4- SN:3708 October 22, 2018

10061-CAB IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	1.38	84.82	23.28	110.0	110.0	$\pm 0.6\%$
10062-CAC IEEE 802.11ah WFI 5 GHz (OFDM, 6 Mbps)	4.35	85.56	16.46	0.49	100.0	$\pm 0.6\%$
10063-CAC IEEE 802.11ah WFI 5 GHz (OFDM, 9 Mbps)	4.55	85.88	16.50	100.0	100.0	$\pm 0.6\%$
10064-CAC IEEE 802.11ah WFI 5 GHz (OFDM, 12 Mbps)	4.38	85.68	16.35	0.72	100.0	$\pm 0.6\%$
10065-CAC IEEE 802.11ah WFI 5 GHz (OFDM, 18 Mbps)	4.62	87.17	16.77	1.21	100.0	$\pm 0.6\%$
10066-CAC IEEE 802.11ah WFI 5 GHz (OFDM, 24 Mbps)	4.69	86.94	16.62	1.48	100.0	$\pm 0.6\%$
10067-CAC IEEE 802.11ah WFI 5 GHz (OFDM, 36 Mbps)	4.81	87.08	17.46	2.04	100.0	$\pm 0.6\%$
10068-CAC IEEE 802.11ah WFI 5 GHz (OFDM, 48 Mbps)	4.92	87.20	17.58	2.55	100.0	$\pm 0.6\%$
10069-CAC IEEE 802.11ah WFI 5 GHz (OFDM, 54 Mbps)	4.92	87.07	17.82	2.87	100.0	$\pm 0.6\%$
10071-CAB IEEE 802.11g WFI 2.4 GHz (DSSS/OFDM, 9 Mbps)	1.01	85.94	14.96	1.89	100.0	$\pm 0.6\%$
10072-CAB IEEE 802.11g WFI 2.4 GHz (DSSS/OFDM, 12 Mbps)	1.17	84.69	15.71	2.30	100.0	$\pm 0.6\%$
10073-CAB IEEE 802.11g WFI 2.4 GHz (DSSS/OFDM, 18 Mbps)	1.38	84.82	23.28	2.83	100.0	$\pm 0.6\%$
10074-CAB IEEE 802.11g WFI 2.4 GHz (DSSS/OFDM, 24 Mbps)	1.56	87.01	10.18	3.30	100.0	$\pm 0.6\%$
10075-CAB IEEE 802.11g WFI 2.4 GHz (DSSS/OFDM, 36 Mbps)	1.81	87.33	16.28	3.82	90.0	$\pm 0.6\%$
10076-CAB IEEE 802.11g WFI 2.4 GHz (DSSS/OFDM, 48 Mbps)	2.07	87.71	16.53	4.10	80.0	$\pm 0.6\%$
10077-CAB IEEE 802.11g WFI 2.4 GHz (DSSS/OFDM, 54 Mbps)	2.30	87.58	16.34	4.30	70.0	$\pm 0.6\%$

Certificate No: EX3-3708\_Out8 Page 14 of 39

EX3DV4- SN:3708 October 22, 2018

10112-CAG LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	2.71	87.18	19.88	0.00	150.0	$\pm 0.6\%$
10113-CAG LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	2.97	88.02	19.17	0.00	150.0	$\pm 0.6\%$
10114-CAC LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	2.49	87.28	18.38	0.00	150.0	$\pm 0.6\%$
10115-CAC IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK)	4.85	87.01	15.53	0.00	150.0	$\pm 0.6\%$
10116-CAC IEEE 802.11n (HT Greenfield, 81 Mbps, 64-QAM)	5.09	87.58	16.16	0.00	150.0	$\pm 0.6\%$
10117-CAC IEEE 802.11n (HT Greenfield, 130 Mbps, 64-QAM)	5.23	87.39	16.50	0.00	150.0	$\pm 0.6\%$
10118-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	3.38	86.86	18.23	0.00	150.0	$\pm 0.6\%$
10119-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	2.49	87.28	18.38	0.00	150.0	$\pm 0.6\%$
10120-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	3.38	86.86	18.23	0.00	150.0	$\pm 0.6\%$
10121-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	2.49	87.28	18.38	0.00	150.0	$\pm 0.6\%$
10122-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	3.38	86.86	18.23	0.00	150.0	$\pm 0.6\%$
10123-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	2.49	87.28	18.38	0.00	150.0	$\pm 0.6\%$
10124-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	3.38	86.86	18.23	0.00	150.0	$\pm 0.6\%$
10125-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	2.49	87.28	18.38	0.00	150.0	$\pm 0.6\%$
10126-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	3.38	86.86	18.23	0.00	150.0	$\pm 0.6\%$
10127-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	2.49	87.28	18.38	0.00	150.0	$\pm 0.6\%$
10128-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	3.38	86.86	18.23	0.00	150.0	$\pm 0.6\%$
10129-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	2.49	87.28	18.38	0.00	150.0	$\pm 0.6\%$
10130-CAG LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	3.38	86.86	18.23	0.00	150.0	$\pm 0.6\%$

Certificate No: EX3-3708\_Out8 Page 16 of 39

EX3DV4- SN:3708 October 22, 2018

10131-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	3.04	77.28	22.08	3.01	150.0	$\pm 0.6\%$
10132-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	2.15	76.05	22.54	3.01	150.0	$\pm 0.6\%$
10133-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	3.04	77.28	22.08	3.01	150.0	$\pm 0.6\%$
10134-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	2.15	76.05	22.54	3.01	150.0	$\pm 0.6\%$
10135-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	3.04	77.28	22.08	3.01	150.0	$\pm 0.6\%$
10136-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	2.15	76.05	22.54	3.01	150.0	$\pm 0.6\%$
10137-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	3.04	77.28	22.08	3.01	150.0	$\pm 0.6\%$
10138-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	2.15	76.05	22.54	3.01	150.0	$\pm 0.6\%$
10139-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	3.04	77.28	22.08	3.01	150.0	$\pm 0.6\%$
10140-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	2.15	76.05	22.54	3.01	150.0	$\pm 0.6\%$
10141-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	3.04	77.28	22.08	3.01	150.0	$\pm 0.6\%$
10142-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	2.15	76.05	22.54	3.01	150.0	$\pm 0.6\%$
10143-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	3.04	77.28	22.08	3.01	150.0	$\pm 0.6\%$
10144-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	2.15	76.05	22.54	3.01	150.0	$\pm 0.6\%$
10145-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	3.04	77.28	22.08	3.01	150.0	$\pm 0.6\%$
10146-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	2.15	76.05	22.54	3.01	150.0	$\pm 0.6\%$
10147-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	3.04	77.28	22.08	3.01	150.0	$\pm 0.6\%$
10148-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	2.15	76.05	22.54	3.01	150.0	$\pm 0.6\%$
10149-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	3.04	77.28	22.08	3.01	150.0	$\pm 0.6\%$
10150-CAG LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	2.15	76.05	22.54	3.01	150.0	$\pm 0.6\%$

Certificate No: EX3-3708\_Out8 Page 18 of 39

EX3DV4 Sn:3708 (5/7)

EX3DV4-SN3708		October 22, 2018	
10223-CAZ	IEEE 802.11n (HT Mixed, 80 MHz, 16-QAM)	X	5.08 67.07 16.58 0.00 150.0 ±0.6%
		Y	5.23 67.44 16.54 150.0
		Z	5.15 67.02 16.29 150.0
10224-CAZ	IEEE 802.11n (HT Mixed, 150 MHz, 64-QAM)	X	4.84 67.01 16.40 0.00 150.0 ±0.6%
		Y	4.98 67.37 16.42 150.0
		Z	4.90 66.88 16.11 150.0
10225-CAB	UMTS-FDD (HS-PA+)	X	2.44 65.81 16.68 0.00 150.0 ±0.6%
		Y	2.73 65.77 15.43 150.0
		Z	2.56 65.53 14.48 150.0
10226-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	9.80 67.52 24.37 0.02 65.0 ±0.6%
		Y	11.18 108.28 31.14 65.0
		Z	8.85 66.88 25.48 65.0
10227-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	8.31 65.60 23.99 0.02 65.0 ±0.6%
		Y	25.63 154.20 28.94 65.0
		Z	8.57 67.04 24.32 65.0
10228-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	6.85 67.47 26.82 0.00 65.0 ±0.6%
		Y	11.49 67.98 30.08 65.0
		Z	6.33 66.07 26.42 65.0
10229-CAZ	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	8.39 66.81 24.42 0.02 65.0 ±0.6%
		Y	27.65 106.98 30.33 65.0
		Z	8.38 67.87 25.02 65.0
10230-CAZ	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	X	7.76 64.41 23.10 0.02 65.0 ±0.6%
		Y	22.43 101.87 28.20 65.0
		Z	8.02 65.84 23.27 65.0
10231-CAZ	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	6.41 66.23 28.29 0.00 65.0 ±0.6%
		Y	10.71 66.21 29.23 65.0
		Z	6.06 65.16 28.01 65.0
10232-CAF	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	8.37 66.60 24.42 0.02 65.0 ±0.6%
		Y	27.65 106.94 30.32 65.0
		Z	8.35 67.55 25.01 65.0
10233-CAF	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	X	7.75 64.54 23.12 0.02 65.0 ±0.6%
		Y	22.38 101.83 28.21 65.0
		Z	8.05 65.81 23.85 65.0
10234-CAF	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	6.12 65.15 25.79 0.00 65.0 ±0.6%
		Y	10.08 64.88 28.87 65.0
		Z	6.05 64.38 24.68 65.0
10235-CAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	8.39 66.63 24.42 0.02 65.0 ±0.6%
		Y	27.68 107.02 30.34 65.0
		Z	8.35 67.57 25.02 65.0
10236-CAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	X	7.71 64.48 23.12 0.02 65.0 ±0.6%
		Y	22.71 103.14 28.26 65.0
		Z	8.11 65.03 23.90 65.0
10237-CAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	6.42 66.27 28.30 0.02 65.0 ±0.6%
		Y	10.73 66.29 29.26 65.0
		Z	6.06 65.19 28.02 65.0
10238-CAF	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	8.38 66.87 24.43 0.02 65.0 ±0.6%
		Y	26.94 106.92 30.31 65.0
		Z	8.33 67.52 25.00 65.0

Certificate No: EX3-3708\_Oct18

Page 20 of 39

EX3DV4-SN3708		October 22, 2018	
10245-CAF	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	5.52 76.10 20.55 3.98 65.0 ±0.6%
		Y	8.54 78.25 21.42 65.0
		Z	5.28 75.07 20.52 65.0
10255-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	2.40 63.21 19.47 3.98 65.0 ±0.6%
		Y	3.51 67.97 12.86 65.0
		Z	3.12 66.29 13.20 65.0
10257-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	X	2.44 65.83 19.21 3.98 65.0 ±0.6%
		Y	3.41 66.94 13.18 65.0
		Z	2.56 65.76 11.23 65.0
10258-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	1.90 63.35 19.82 3.98 65.0 ±0.6%
		Y	3.32 69.86 14.27 65.0
		Z	2.71 67.24 13.62 65.0
10259-CAZ	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	4.04 70.43 19.24 3.98 65.0 ±0.6%
		Y	5.28 74.31 18.23 65.0
		Z	4.48 72.23 17.26 65.0
10260-CAZ	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	X	4.07 70.51 19.13 3.98 65.0 ±0.6%
		Y	5.78 73.97 18.48 65.0
		Z	4.55 71.99 17.28 65.0
10261-CAZ	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	4.80 70.90 19.89 3.98 65.0 ±0.6%
		Y	6.07 80.88 21.37 65.0
		Z	5.30 74.50 19.86 65.0
10262-CAF	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	3.90 76.46 20.76 65.0 ±0.6%
		Y	5.30 74.50 19.86 65.0
		Z	3.52 72.30 18.94 65.0
10264-CAF	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	4.81 71.41 17.89 3.98 65.0 ±0.6%
		Y	5.53 73.09 19.33 65.0
		Z	3.52 72.30 18.94 65.0
10265-CAF	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	4.99 71.77 18.88 3.98 65.0 ±0.6%
		Y	7.20 81.83 22.43 65.0
		Z	5.93 78.98 21.13 65.0
10266-CAF	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	X	4.99 71.77 18.88 3.98 65.0 ±0.6%
		Y	6.78 73.73 19.79 65.0
		Z	5.21 72.50 19.12 65.0
10269-CAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	6.42 73.17 19.92 3.98 65.0 ±0.6%
		Y	8.19 74.91 20.65 65.0
		Z	5.72 73.47 20.01 65.0
10269-CAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	5.78 73.50 20.41 3.98 65.0 ±0.6%
		Y	6.05 76.98 20.55 65.0
		Z	5.07 72.68 19.68 65.0
10269-CAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	X	5.80 71.79 19.55 3.98 65.0 ±0.6%
		Y	8.09 73.51 20.23 65.0
		Z	5.09 72.51 19.12 65.0
10270-CAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	6.37 73.31 20.11 65.0 ±0.6%
		Y	8.09 73.16 19.61 65.0
		Z	5.72 74.15 19.92 3.98 65.0 ±0.6%
		Y	6.58 75.97 20.51 65.0
		Z	6.01 74.38 19.89 65.0

Certificate No: EX3-3708\_Oct18

Page 22 of 39

EX3DV4-SN3708		October 22, 2018	
10303-AAA	IEEE 802.16e WIMAX (3.1-15, 5ms, 10MHz, 64QAM, PUSC)	X	4.86 67.04 16.30 4.96 50.0 ±0.6%
		Y	4.63 66.01 17.92 50.0
		Z	4.77 65.64 17.36 50.0
10304-AAA	IEEE 802.16e WIMAX (20-18, 4ms, 10MHz, 64QAM, PUSC)	X	4.60 66.87 17.42 4.17 50.0 ±0.6%
		Y	4.64 65.92 17.42 50.0
		Z	4.57 65.48 17.05 50.0
10305-AAA	IEEE 802.16e WIMAX (3.1-15, 10ms, 10MHz, 64QAM, PUSC, 15 symbols)	X	4.90 71.08 19.94 0.02 30.0 ±0.6%
		Y	4.91 68.82 19.76 30.0
		Z	4.92 69.06 19.46 30.0
10306-AAA	IEEE 802.16e WIMAX (20-18, 10ms, 10MHz, 64QAM, PUSC, 18 symbols)	X	4.85 68.79 19.42 0.02 30.0 ±0.6%
		Y	4.69 67.30 19.20 30.0
		Z	4.71 67.32 18.88 30.0
10307-AAA	IEEE 802.16e WIMAX (20-18, 10ms, 10MHz, QPSK, PUSC, 18 symbols)	X	4.82 69.04 19.35 0.02 30.0 ±0.6%
		Y	4.60 67.51 19.18 30.0
		Z	4.62 67.50 18.94 30.0
10308-AAA	IEEE 802.16e WIMAX (20-18, 10ms, 10MHz, 16QAM, PUSC)	X	4.84 69.40 19.59 0.02 30.0 ±0.6%
		Y	4.62 67.78 19.38 30.0
		Z	4.62 67.77 19.11 30.0
10309-AAA	IEEE 802.16e WIMAX (20-18, 10ms, 10MHz, 16QAM, AMC, 3x3, 18 symbols)	X	4.90 68.85 19.51 0.02 35.0 ±0.6%
		Y	4.75 67.44 19.31 35.0
		Z	4.74 67.44 19.59 35.0
10310-AAA	IEEE 802.16e WIMAX (20-18, 10ms, 10MHz, QPSK, AMC, 2x3, 18 symbols)	X	4.87 68.98 19.40 0.02 35.0 ±0.6%
		Y	4.65 67.42 19.21 35.0
		Z	4.65 67.43 18.99 35.0
10311-AAD	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	2.77 66.48 16.08 0.00 150.0 ±0.6%
		Y	3.14 70.90 16.79 150.0
		Z	2.75 67.28 15.39 150.0
10313-AAA	iDEN 1.3	X	2.37 67.25 12.88 0.99 70.0 ±0.6%
		Y	3.64 72.65 15.49 70.0
		Z	2.67 66.89 14.27 70.0
10314-AAA	iDEN 1.9	X	3.93 74.44 18.42 10.00 30.0 ±0.6%
		Y	5.14 82.13 17.83 30.0
		Z	4.16 76.04 18.35 30.0
10315-AAB	IEEE 802.11n WiFi 2.4 GHz (5555, 1 Mbps, 64q, duty cycle)	X	0.92 63.63 14.83 0.17 150.0 ±0.6%
		Y	1.08 64.20 15.74 150.0
		Z	0.97 62.77 14.10 150.0
10316-AAB	IEEE 802.11n WiFi 2.4 GHz (ERP-COFDM, 6 Mbps, 64q, duty cycle)	X	4.25 66.50 16.29 0.17 150.0 ±0.6%
		Y	4.42 66.80 16.29 150.0
		Z	4.38 66.39 15.84 150.0
10317-AAC	IEEE 802.11n WiFi 5 GHz (OFDM, 6 Mbps, 64q, duty cycle)	X	4.25 66.52 16.20 0.17 150.0 ±0.6%
		Y	4.45 66.89 16.29 150.0
		Z	4.30 66.30 15.94 150.0
10400-AAD	IEEE 802.11ac WiFi (20MHz, 64-QAM, 390c, duty cycle)	X	4.50 66.79 16.22 0.00 150.0 ±0.6%
		Y	4.54 67.23 16.32 150.0
		Z	4.43 66.57 15.93 150.0
10401-AAD	IEEE 802.11ac WiFi (40MHz, 64-QAM, 390c, duty cycle)	X	4.86 68.55 16.27 0.00 150.0 ±0.6%
		Y	5.78 87.55 16.33 150.0
		Z	5.12 66.71 16.08 150.0

Certificate No: EX3-3708\_Oct18

Page 24 of 39

EX3DV4-SN3708		October 22, 2018	
10427-AAB	IEEE 802.11n (HT Greenfield, 150 Mbps, 64-QAM)	X	5.02 67.00 16.51 0.00 150.0 ±0.6%
		Y	6.19 67.39 16.49 150.0
		Z	5.11 66.94 16.20 150.0
10430-AAD	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1)	X	4.36 67.53 16.68 0.00 150.0 ±0.6%
		Y	4.48 73.15 19.04 150.0
		Z	4.10 71.38 17.84 150.0
10431-AAD	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1)	X	3.79 67.15 15.98 0.00 150.0 ±0.6%
		Y	4.07 67.63 16.28 150.0
		Z	3.95 66.98 15.74 150.0
10432-AAD	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1)	X	4.13 66.99 16.21 0.00 150.0 ±0.6%
		Y	4.37 67.41 16.36 150.0
		Z	4.28 66.79 15.92 150.0
10433-AAC	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1)	X	4.39 66.91 16.34 0.00 150.0 ±0.6%
		Y	4.63 67.93 16.42 150.0
		Z	4.51 66.77 16.04 150.0
10434-AAA	W-CDMA (BS Test Model 1, 84 DPCCH)	X	4.42 74.13 18.28 0.00 150.0 ±0.6%
		Y	4.78 74.54 18.12 150.0
		Z	4.17 72.08 17.69 150.0
10435-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, 15, Subframe=3,5,7,9)	X	9.40 89.31 20.93 3.23 80.0 ±0.6%
		Y	100.00 117.05 27.59 80.0
		Z	11.68 92.88 22.28 80.0
10447-AAD	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1, Clipping 44%)	X	2.96 66.90 14.33 0.00 150.0 ±0.6%
		Y	3.37 67.76 14.49 150.0
		Z	3.15 65.53 14.35 150.0
10448-AAD	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1, Clipping 44%)	X	3.66 66.90 14.33 0.00 150.0 ±0.6%
		Y	3.93 67.43 14.16 150.0
		Z	3.78 66.66 14.00 150.0
10449-AAC	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1, Clipping 44%)	X	3.97 66.81 14.10 0.00 150.0 ±0.6%
		Y	4.20 67.26 14.26 150.0
		Z	4.08 66.81 14.01 150.0
10450-AAC	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)	X	4.19 66.69 14.18 0.00 150.0 ±0.6%
		Y	4.40 67.14 14.02 150.0
		Z	4.28 66.34 13.89 150.0
10451-AAA	W-CDMA (BS Test Model 1, 84 DPCCH, Clipping 44%)		



EX3DV4 Sn:3708 (6/7)

EX3DV4-SN3708		October 22, 2018	
10427-AAB	IEEE 802.11n (HT Greenfield, 150 Mbps, 84-QAM)	X	5.02 67.70 16.51 0.00 150.0 ± 0.8 %
		Y	5.19 67.39 16.48 150.0
		Z	5.11 66.84 16.29 150.0
10430-AAD	LTE-FDD (FDDMA, 5 MHz, E-TM 3.1)	X	4.38 73.73 18.86 0.00 150.0 ± 0.8 %
		Y	4.48 73.15 18.04 150.0
		Z	4.70 73.36 17.94 150.0
10431-AAD	LTE-FDD (FDDMA, 10 MHz, E-TM 3.1)	X	3.79 67.15 15.96 0.00 150.0 ± 0.8 %
		Y	4.07 67.63 16.28 150.0
		Z	3.92 66.88 16.74 150.0
10432-AAD	LTE-FDD (FDDMA, 15 MHz, E-TM 3.1)	X	4.13 68.99 16.23 0.00 150.0 ± 0.8 %
		Y	4.37 67.41 16.38 150.0
		Z	4.25 66.79 16.20 150.0
10433-AAC	LTE-FDD (FDDMA, 20 MHz, E-TM 3.1)	X	4.39 66.91 16.34 0.00 150.0 ± 0.8 %
		Y	4.60 67.33 16.42 150.0
		Z	4.50 66.77 16.24 150.0
10434-AAA	WCDMA (BS Test Model 1, 84 DPCCH)	X	4.42 74.13 18.28 0.00 150.0 ± 0.8 %
		Y	4.78 74.54 18.12 150.0
		Z	4.17 72.09 17.89 150.0
10435-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	9.40 69.31 20.51 3.23 80.0 ± 0.8 %
		Y	100.00 117.06 27.58 80.0
		Z	11.08 62.88 22.38 80.0
10447-AAD	LTE-FDD (FDDMA, 5 MHz, E-TM 3.1, Clipping 44%)	X	2.96 66.50 14.33 0.00 150.0 ± 0.8 %
		Y	3.37 67.75 14.49 150.0
		Z	3.10 66.53 14.25 150.0
10448-AAD	LTE-FDD (FDDMA, 10 MHz, E-TM 3.1, Clipping 44%)	X	3.66 66.95 14.83 0.00 150.0 ± 0.8 %
		Y	3.93 67.43 14.16 150.0
		Z	3.70 66.68 14.85 150.0
10449-AAC	LTE-FDD (FDDMA, 15 MHz, E-TM 3.1, Clipping 44%)	X	3.97 66.81 14.10 0.00 150.0 ± 0.8 %
		Y	4.20 67.26 14.24 150.0
		Z	4.08 66.61 14.81 150.0
10450-AAD	LTE-FDD (FDDMA, 20 MHz, E-TM 3.1, Clipping 44%)	X	4.19 66.68 14.16 0.00 150.0 ± 0.8 %
		Y	4.48 67.13 14.25 150.0
		Z	4.29 66.54 14.89 150.0
10451-AAA	WCDMA (BS Test Model 1, 84 DPCCH, Clipping 44%)	X	2.70 62.69 13.23 0.00 150.0 ± 0.8 %
		Y	3.22 67.79 14.95 150.0
		Z	2.98 66.32 13.88 150.0
10456-AAB	IEEE 802.11ac WiFi (160MHz, 84-QAM, 80ps duty cycle)	X	5.06 67.79 16.82 0.00 150.0 ± 0.8 %
		Y	6.10 68.03 16.69 150.0
		Z	5.05 67.70 16.49 150.0
10457-AAA	UMTS-FDD (3G-HSPA)	X	3.37 65.33 15.53 0.00 150.0 ± 0.8 %
		Y	3.72 65.64 16.01 150.0
		Z	3.64 65.12 15.61 150.0
10458-AAA	CDMA2000 (1xEV-DO, Rev. B, 2, 3.1MHz)	X	3.31 69.88 15.53 0.00 150.0 ± 0.8 %
		Y	4.24 73.24 16.12 150.0
		Z	3.30 70.45 15.45 150.0
10459-AAA	CDMA2000 (1xEV-DO, Rev. B, 3, 3.1MHz)	X	5.26 71.27 16.49 0.00 150.0 ± 0.8 %
		Y	5.12 69.87 16.56 150.0
		Z	4.91 69.06 17.99 150.0

Certificate No: EX3-3708\_Oct18

Page 26 of 38

EX3DV4-SN3708		October 22, 2018	
10477-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	0.86 69.00 7.77 3.23 80.0 ± 0.8 %
		Y	0.86 69.00 7.77 80.0
		Z	0.85 69.75 8.59 80.0
10478-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	0.86 69.00 7.79 3.23 80.0 ± 0.8 %
		Y	0.86 69.00 8.05 80.0
		Z	0.80 69.00 7.59 80.0
10479-AAA	LTE-TDD (SC-FDMA, 80% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	46.10 108.19 27.60 3.23 80.0 ± 0.8 %
		Y	10.72 96.20 28.05 80.0
		Z	6.80 84.81 21.76 80.0
10480-AAA	LTE-TDD (SC-FDMA, 90% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.04 68.21 13.43 3.23 80.0 ± 0.8 %
		Y	3.14 79.40 17.60 80.0
		Z	3.04 68.21 13.43 80.0
10481-AAA	LTE-TDD (SC-FDMA, 90% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	2.10 65.01 11.27 3.23 80.0 ± 0.8 %
		Y	4.29 72.85 14.93 80.0
		Z	2.98 68.84 13.89 80.0
10482-AAB	LTE-TDD (SC-FDMA, 90% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	1.17 61.31 8.26 2.23 80.0 ± 0.8 %
		Y	2.03 70.92 15.29 80.0
		Z	1.70 64.90 12.42 80.0
10483-AAB	LTE-TDD (SC-FDMA, 90% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	1.68 60.67 8.66 2.23 80.0 ± 0.8 %
		Y	3.07 68.75 13.78 80.0
		Z	2.34 65.92 12.29 80.0
10484-AAB	LTE-TDD (SC-FDMA, 90% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.49 60.41 8.72 2.23 80.0 ± 0.8 %
		Y	2.87 67.74 13.34 80.0
		Z	2.23 64.87 11.98 80.0
10485-AAC	LTE-TDD (SC-FDMA, 90% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	2.12 68.28 14.58 2.23 80.0 ± 0.8 %
		Y	3.39 74.14 16.00 80.0
		Z	2.30 68.58 13.26 80.0
10489-AAB	LTE-TDD (SC-FDMA, 90% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	1.68 60.67 8.66 2.23 80.0 ± 0.8 %
		Y	2.97 68.66 15.17 80.0
		Z	2.31 63.39 13.27 80.0
10487-AAB	LTE-TDD (SC-FDMA, 90% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.86 62.92 11.27 2.23 80.0 ± 0.8 %
		Y	2.84 68.97 14.83 80.0
		Z	2.33 68.12 13.13 80.0
10488-AAB	LTE-TDD (SC-FDMA, 90% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	2.93 71.00 17.45 2.23 80.0 ± 0.8 %
		Y	3.58 73.22 18.66 80.0
		Z	2.30 68.54 13.26 80.0
10489-AAC	LTE-TDD (SC-FDMA, 90% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	2.60 67.87 12.87 2.23 80.0 ± 0.8 %
		Y	3.42 69.49 17.05 80.0
		Z	2.89 67.24 14.84 80.0
10490-AAB	LTE-TDD (SC-FDMA, 90% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	2.97 67.51 10.80 2.23 80.0 ± 0.8 %
		Y	5.60 69.30 17.97 80.0
		Z	3.07 67.17 13.82 80.0
10491-AAC	LTE-TDD (SC-FDMA, 90% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.19 69.71 17.30 2.23 80.0 ± 0.8 %
		Y	3.74 71.43 18.14 80.0
		Z	3.00 68.92 16.86 80.0
10492-AAB	LTE-TDD (SC-FDMA, 90% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.30 67.35 16.40 2.23 80.0 ± 0.8 %
		Y	3.73 69.40 17.08 80.0
		Z	3.40 68.98 16.20 80.0

Certificate No: EX3-3708\_Oct18

Page 28 of 39

EX3DV4-SN3708		October 22, 2018	
10508-AAC	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.41 67.37 16.58 2.23 80.0 ± 0.8 %
		Y	3.62 66.99 17.16 80.0
		Z	3.52 67.03 16.70 80.0
10509-AAB	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.76 69.64 17.37 2.23 80.0 ± 0.8 %
		Y	4.38 71.43 18.03 80.0
		Z	3.37 69.14 18.84 80.0
10510-AAD	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.80 69.28 16.80 2.23 80.0 ± 0.8 %
		Y	4.21 69.49 17.24 80.0
		Z	3.51 67.13 18.03 80.0
10511-AAB	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.87 67.13 16.77 2.23 80.0 ± 0.8 %
		Y	4.26 66.26 17.16 80.0
		Z	3.89 66.89 16.51 80.0
10512-AAB	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.83 70.87 17.64 2.23 80.0 ± 0.8 %
		Y	4.26 66.26 17.16 80.0
		Z	3.79 67.26 18.57 80.0
10513-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	4.37 72.98 18.50 80.0 ± 0.8 %
		Y	3.81 70.11 17.16 80.0
		Z	3.69 69.38 16.85 80.0
10514-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	4.10 68.72 17.33 80.0 ± 0.8 %
		Y	4.12 68.32 17.25 80.0
		Z	3.84 66.87 16.51 80.0
10515-AAC	IEEE 802.11ac WiFi (2 GHz, DSSS, 5 MHz, 80ps duty cycle)	X	0.81 63.02 14.44 0.00 150.0 ± 0.8 %
		Y	0.86 64.09 15.32 150.0
		Z	0.87 64.17 15.38 150.0
10516-AAA	IEEE 802.11ac WiFi (2 GHz, DSSS, 5 MHz, 80ps duty cycle)	X	0.90 77.81 30.96 150.0 ± 0.8 %
		Y	0.82 64.17 15.38 150.0
		Z	0.82 64.17 15.38 150.0
10517-AAA	IEEE 802.11ac WiFi (2 GHz, DSSS, 11 MHz, 80ps duty cycle)	X	0.69 65.32 13.85 0.00 150.0 ± 0.8 %
		Y	0.63 65.10 13.38 150.0
		Z	0.69 65.32 13.85 150.0
10518-AAB	IEEE 802.11ac WiFi (5 GHz, OFDM, 9 MHz, 80ps duty cycle)	X	4.19 66.67 16.18 0.00 150.0 ± 0.8 %
		Y	4.40 67.06 16.28 150.0
		Z	4.30 66.49 16.98 150.0
10519-AAB	IEEE 802.11ac WiFi (5 GHz, OFDM, 12 MHz, 80ps duty cycle)	X	4.33 66.84 16.27 0.00 150.0 ± 0.8 %
		Y	4.56 67.23 16.37 150.0
		Z	4.45 66.68 16.99 150.0
10520-AAB	IEEE 802.11ac WiFi (5 GHz, OFDM, 18 MHz, 80ps duty cycle)	X	4.19 66.76 16.18 0.00 150.0 ± 0.8 %
		Y	4.42 67.19 16.30 150.0
		Z	4.30 66.60 16.89 150.0
10521-AAB	IEEE 802.11ac WiFi (5 GHz, OFDM, 24 MHz, 80ps duty cycle)	X	4.12 66.71 16.18 0.00 150.0 ± 0.8 %
		Y	4.35 67.13 16.29 150.0
		Z	4.23 66.57 16.96 150.0
10522-AAA	IEEE 802.11ac WiFi (5 GHz, OFDM, 36 MHz, 80ps duty cycle)	X	4.17 66.84 16.25 0.00 150.0 ± 0.8 %
		Y	4.41 67.31 16.36 150.0
		Z	4.28 66.70 16.97 150.0

Certificate No: EX3-3708\_Oct18

Page 30 of 39

EX3DV4-SN3708		October 22, 2018	
10541-AAB	IEEE 802.11ac WiFi (80MHz, MCS7, 80ps duty cycle)	X	4.79 66.10 16.07 0.00 150.0 ± 0.8 %
		Y	4.88 66.69 16.11 150.0
		Z	4.87 66.05 15.76 150.0
10542-AAB	IEEE 802.11ac WiFi (80MHz, MCS8, 80ps duty cycle)	X	4.85 66.23 16.10 0.00 150.0 ± 0.8 %
		Y	5.13 66.67 16.15 150.0
		Z	5.03 66.16 15.84 150.0
10543-AAB	IEEE 802.11ac WiFi (80MHz, MCS9, 80ps duty cycle)	X	5.05 66.42 16.28 0.00 150.0 ± 0.8 %
		Y	5.19 66.68 16.19 150.0
		Z	5.10 66.20 15.89 150.0
10544-AAB	IEEE 802.11ac WiFi (80MHz, MCS10, 80ps duty cycle)	X	5.14 66.17 16.00 0.00 150.0 ± 0.8 %
		Y	5.33 66.70 16.08 150.0
		Z	5.26 66.20 15.77 150.0
10545-AAB	IEEE 802.11ac WiFi (80MHz, MCS11, 80ps duty cycle)	X	5.40 66.40 16.32 0.00 150.0 ± 0.8 %
		Y	5.49 67.26 16.21 150.0
		Z	5.41 66.82 15.94 150.0
10546-AAB	IEEE 802.11ac WiFi (80MHz, MCS12, 80ps duty cycle)	X	5.21 66.30 16.09 0.00 150.0 ± 0.8 %
		Y	5.39 66.84 16.12 150.0
		Z	5.27 66.33 15.81 150.0
10547-AAB	IEEE 802.11ac WiFi (80MHz, MCS13, 80ps duty cycle)	X	5.35 66.64 16.25 0.00 150.0 ± 0.8 %
		Y	5.43 66.89 16.14 150.0
		Z	5.36 66.36 15.86 150.0
10548-AAB	IEEE 802.11ac WiFi (80MHz, MCS14, 80ps duty cycle)	X	5.50 67.27 16.54 0.00 150.0 ± 0.8 %
		Y	5.58 67.53 16.43 150.0
		Z	5.51 67.08 16.13 150.0
10550-AAB	IEEE 802.11ac WiFi (80MHz, MCS16, 80ps duty cycle)	X	5.35 66.79 16.34 0.00 150.0 ± 0.8 %
		Y	5.40 66.91 16.17 150.0
		Z	5.32 66.47 15.85 150.0
10551-AAB	IEEE 802.11ac WiFi (80MHz, MCS17, 80ps duty cycle)	X	5.19 66.22 16.03 0.00 150.0 ± 0.8 %
		Y	5.

EX3DV4 Sn:3708 (7/7)

EX3DV4-SN3708		October 22, 2018	
10807-AAB	IEEE 802.11ac WFI (20MHz, MCS6, 90pc duty cycle)	X	4.30 85.88 16.10 0.46 130.0 ± 9.6 %
		Y	4.30 86.24 16.15 130.0
		Z	4.40 85.92 15.89 130.0
10808-AAB	IEEE 802.11ac WFI (20MHz, MCS1, 90pc duty cycle)	X	4.43 86.20 16.24 0.46 130.0 ± 9.6 %
		Y	4.66 86.30 16.30 130.0
		Z	4.34 86.06 15.65 130.0
10809-AAB	IEEE 802.11ac WFI (20MHz, MCS2, 90pc duty cycle)	X	4.33 86.00 16.03 0.46 130.0 ± 9.6 %
		Y	4.54 86.42 16.12 130.0
		Z	4.41 86.97 15.76 130.0
10810-AAB	IEEE 802.11ac WFI (20MHz, MCS3, 90pc duty cycle)	X	4.38 86.21 16.23 0.46 130.0 ± 9.6 %
		Y	4.60 86.00 16.30 130.0
		Z	4.49 86.05 15.53 130.0
10811-AAB	IEEE 802.11ac WFI (20MHz, MCS4, 90pc duty cycle)	X	4.29 85.97 16.05 0.46 130.0 ± 9.6 %
		Y	4.51 86.39 16.13 130.0
		Z	4.40 86.84 16.12 130.0
10812-AAB	IEEE 802.11ac WFI (20MHz, MCS5, 90pc duty cycle)	X	4.36 86.08 16.04 0.46 130.0 ± 9.6 %
		Y	4.51 86.92 16.17 130.0
		Z	4.30 86.98 15.80 130.0
10813-AAB	IEEE 802.11ac WFI (20MHz, MCS6, 90pc duty cycle)	X	4.27 85.86 15.86 0.46 130.0 ± 9.6 %
		Y	4.50 86.34 16.02 130.0
		Z	4.39 85.79 15.65 130.0
10814-AAB	IEEE 802.11ac WFI (20MHz, MCS7, 90pc duty cycle)	X	4.25 86.17 16.21 0.46 130.0 ± 9.6 %
		Y	4.47 86.62 16.30 130.0
		Z	4.36 86.03 15.92 130.0
10815-AAB	IEEE 802.11ac WFI (20MHz, MCS8, 90pc duty cycle)	X	4.27 85.75 15.76 0.46 130.0 ± 9.6 %
		Y	4.60 86.18 15.88 130.0
		Z	4.39 86.65 15.52 130.0
10816-AAB	IEEE 802.11ac WFI (40MHz, MCS0, 90pc duty cycle)	X	4.98 86.20 16.34 0.46 130.0 ± 9.6 %
		Y	5.12 86.54 16.26 130.0
		Z	5.06 86.10 16.02 130.0
10817-AAB	IEEE 802.11ac WFI (40MHz, MCS1, 90pc duty cycle)	X	5.02 86.34 16.39 0.46 130.0 ± 9.6 %
		Y	5.17 86.69 16.34 130.0
		Z	5.10 86.06 16.07 130.0
10818-AAB	IEEE 802.11ac WFI (40MHz, MCS2, 90pc duty cycle)	X	4.91 86.30 16.40 0.46 130.0 ± 9.6 %
		Y	5.08 86.77 16.40 130.0
		Z	5.09 86.31 16.11 130.0
10819-AAB	IEEE 802.11ac WFI (40MHz, MCS3, 90pc duty cycle)	X	4.93 86.33 16.32 0.46 130.0 ± 9.6 %
		Y	5.08 86.82 16.20 130.0
		Z	5.01 86.09 16.30 130.0
10820-AAB	IEEE 802.11ac WFI (40MHz, MCS4, 90pc duty cycle)	X	5.02 86.21 16.21 0.46 130.0 ± 9.6 %
		Y	5.16 86.55 16.28 130.0
		Z	5.09 86.11 15.99 130.0
10821-AAB	IEEE 802.11ac WFI (40MHz, MCS5, 90pc duty cycle)	X	5.01 86.30 16.00 0.46 130.0 ± 9.6 %
		Y	5.18 86.72 16.48 130.0
		Z	5.10 86.27 16.20 130.0
10822-AAB	IEEE 802.11ac WFI (40MHz, MCS6, 90pc duty cycle)	X	5.01 86.42 16.33 0.46 130.0 ± 9.6 %
		Y	5.18 86.82 16.52 130.0
		Z	5.09 86.37 16.24 130.0

Certificate No: EX3-3708\_Oct18

Page 36 of 38

EX3DV4-SN3708		October 22, 2018	
10839-AAC	IEEE 802.11ac WFI (160MHz, MCS3, 90pc duty cycle)	X	5.86 96.76 18.30 0.46 130.0 ± 9.2 %
		Y	5.86 97.16 18.45 130.0
		Z	5.60 96.12 18.20 130.0
10840-AAC	IEEE 802.11ac WFI (160MHz, MCS4, 90pc duty cycle)	X	5.79 96.55 18.33 0.46 130.0 ± 9.6 %
		Y	5.85 97.13 18.36 130.0
		Z	5.65 96.72 16.13 130.0
10841-AAC	IEEE 802.11ac WFI (160MHz, MCS5, 90pc duty cycle)	X	5.87 96.80 18.21 0.46 130.0 ± 9.6 %
		Y	6.01 97.20 18.36 130.0
		Z	5.98 96.74 16.15 130.0
10842-AAC	IEEE 802.11ac WFI (160MHz, MCS6, 90pc duty cycle)	X	5.94 96.92 18.72 0.46 130.0 ± 9.6 %
		Y	6.06 97.38 18.68 130.0
		Z	5.89 96.95 16.45 130.0
10843-AAC	IEEE 802.11ac WFI (160MHz, MCS7, 90pc duty cycle)	X	5.78 96.59 18.43 0.46 130.0 ± 9.6 %
		Y	5.89 97.02 18.39 130.0
		Z	5.83 96.65 16.18 130.0
10844-AAC	IEEE 802.11ac WFI (160MHz, MCS8, 90pc duty cycle)	X	5.83 96.71 18.22 0.46 130.0 ± 9.6 %
		Y	5.98 97.32 18.36 130.0
		Z	5.91 96.89 16.31 130.0
10845-AAC	IEEE 802.11ac WFI (160MHz, MCS9, 90pc duty cycle)	X	6.10 97.41 19.33 0.46 130.0 ± 9.6 %
		Y	6.07 97.25 18.48 130.0
		Z	6.04 96.85 16.31 130.0
10846-AAC	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL_SchInterleave=2)	X	9.04 82.83 31.00 9.30 60.0 ± 9.6 %
		Y	18.22 106.00 35.45 60.0
		Z	10.43 96.01 32.33 60.0
10847-AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL_SchInterleave=2)	X	8.54 81.27 30.60 9.30 60.0 ± 9.6 %
		Y	13.54 103.45 34.79 60.0
		Z	8.34 84.22 31.85 60.0
10848-AAC	CDMA2000 (1X Advantedge)	X	3.32 82.90 6.03 0.00 150.0 ± 9.6 %
		Y	5.66 83.51 5.94 150.0
		Z	3.44 80.36 7.17 150.0
10850-AAC	LTE-TDD (OFDMA, 5 MHz, E-TM 3.1, CQIreq 44)	X	3.20 86.29 15.67 2.23 60.0 ± 9.6 %
		Y	3.96 87.36 16.44 60.0
		Z	3.26 82.84 15.69 60.0
10853-AAC	LTE-TDD (OFDMA, 10 MHz, E-TM 3.1, CQIreq 44)	X	3.78 85.70 16.24 2.23 60.0 ± 9.6 %
		Y	4.03 86.83 16.60 60.0
		Z	3.81 85.57 16.54 60.0
10854-AAC	LTE-TDD (OFDMA, 15 MHz, E-TM 3.1, CQIreq 44)	X	3.81 85.39 16.33 2.23 60.0 ± 9.6 %
		Y	4.06 86.15 16.62 60.0
		Z	3.89 85.26 16.10 60.0
10855-AAC	LTE-TDD (OFDMA, 20 MHz, E-TM 3.1, CQIreq 44)	X	3.88 85.27 16.38 2.23 60.0 ± 9.6 %
		Y	4.13 86.58 16.65 60.0
		Z	3.85 85.32 16.15 60.0
10858-AAC	Pulse Waveform (200Hz, 10%)	X	3.85 89.00 12.97 10.00 90.0 ± 9.6 %
		Y	7.30 77.55 16.50 60.0
		Z	4.32 76.24 16.00 60.0
10859-AAC	Pulse Waveform (200Hz, 20%)	X	2.83 88.91 10.74 6.99 60.0 ± 9.6 %
		Y	30.89 53.57 15.50 60.0
		Z	2.16 81.85 16.51 60.0

Certificate No: EX3-3708\_Oct18

Page 38 of 39



750V3 Sn:1101 (1/2)

In Collaboration with  
**TTL** **SPEAG**  
CALIBRATION LABORATORY

中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L6570

Address: No. 31 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-42204633-2079 Fax: +86-10-42204633-2304  
E-mail: cti@chinaul.com http://www.chinaul.cn

Client: **SRTC** Certificate No: **Z17-97134**

### CALIBRATION CERTIFICATE

Object: D750V3 - SN: 1101

Calibration Procedure(s): FF-Z11-003-01  
Calibration Procedures for dipole validation kits

Calibration date: September 13, 2017

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(S). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(2±3)°C and humidity<70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date/(Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRV-D	102198	02-Mar-17 (CTTL No.J17X01254)	Mar-18
Power sensor NRV-Z5	100596	02-Mar-17 (CTTL No.J17X01254)	Mar-18
Reference Probe EX3DV4	SN 7433	28-Sep-16(SPEAG.No EX3-7433_Sep16)	Sep-17
DAE4	SN 1331	19-Jan-17(CTTL_SPEAG.No.Z17-97015)	Jan-18

Secondary Standards	ID #	Cal Date/(Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-17 (CTTL No.J17X00286)	Jan-18
Network Analyzer ES071C	MY46111013	13-Jan-17 (CTTL No.J17X00285)	Jan-18

Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Yu Zongying	SAR Test Engineer	
Approved by:	Qi Dianyuan	SAR Project Leader	

Issued: September 16, 2017  
This calibration certificate shall not be reproduced except in full without written approval of the laboratory

In Collaboration with  
**TTL** **SPEAG**  
CALIBRATION LABORATORY

中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L6570

Address: No. 31 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-42204633-2079 Fax: +86-10-42204633-2304  
E-mail: cti@chinaul.com http://www.chinaul.cn

Glossary:  
TSL Issue simulating liquid  
ConvF sensitivity in TSL / NORMx,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- KDB955664, SAR Measurement Requirements for 100 MHz to 6 GHz

**Additional Documentation:**

- DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power: No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

In Collaboration with  
**TTL** **SPEAG**  
CALIBRATION LABORATORY

中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L6570

Address: No. 31 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-42204633-2079 Fax: +86-10-42204633-2304  
E-mail: cti@chinaul.com http://www.chinaul.cn

**Measurement Conditions**  
DASY system configuration, as far as not given on page 1

DASY Version	DASY92	52.10.0.1448
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz ± 1 MHz	

**Head TSL parameters**  
The following parameters and calculations were applied:

Temperature	Permittivity	Conductivity	
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.5 ± 6 %	0.88 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.05 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	8.26 mW / g ± 18.8 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.34 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	5.39 mW / g ± 18.7 % (k=2)

**Body TSL parameters**  
The following parameters and calculations were applied:

Temperature	Permittivity	Conductivity	
Nominal Body TSL parameters	22.0 °C	55.5	0.96 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.4 ± 6 %	0.95 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	---	---

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.15 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	8.69 mW / g ± 18.8 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.42 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	5.73 mW / g ± 18.7 % (k=2)

In Collaboration with  
**TTL** **SPEAG**  
CALIBRATION LABORATORY

中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L6570

Address: No. 31 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-42204633-2079 Fax: +86-10-42204633-2304  
E-mail: cti@chinaul.com http://www.chinaul.cn

**Appendix (Additional assessments outside the scope of CNAS L6570)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	53.90 ± 0.24jΩ
Return Loss	-28.4dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	52.00 ± 2.22jΩ
Return Loss	-30.8dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.136 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------