








ANNEX B – RELEVANT PAGES FROM CALIBRATION REPORTS

DAE4 Sn:546

<div style="text-align: center;">   </div> <p style="text-align: center;">In Collaboration with TTL Calibration Laboratory 中国认可 国家互认 校准 CNAS L5570</p> <p>Client: SRTC Certificate No: Z18-60400</p> <div style="border: 1px solid black; padding: 5px;"> <p>CALIBRATION CERTIFICATE</p> <p>Object: DAE4 - SN: 546</p> <p>Calibration Procedure(s): FF-Z11-002-01 Calibration Procedure for the Data Acquisition Electronics (DAE)</p> <p>Calibration date: October 15, 2018</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature(23±3)°C and humidity<70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date/Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Process Calibrator 753</td> <td>1971018</td> <td>20-Jun-18 (CTTL, No.J18X02034)</td> <td>June-19</td> </tr> </tbody> </table> <p>Calibrated by: Yu Zengying BAR Test Engineer </p> <p>Reviewed by: Lin Han BAR Test Engineer </p> <p>Approved by: Qi Dianyuan BAR Project Leader </p> <p style="text-align: right;">Issued: October 17, 2018</p> <p><small>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</small></p> </div> <p style="text-align: center;">Certificate No: Z18-60400 Page 1 of 3</p>	Primary Standards	ID #	Cal Date/Calibrated by, Certificate No.)	Scheduled Calibration	Process Calibrator 753	1971018	20-Jun-18 (CTTL, No.J18X02034)	June-19	<div style="text-align: center;">  </div> <p style="text-align: center;">In Collaboration with TTL Calibration Laboratory 中国认可 国家互认 校准 CNAS L5570</p> <p>Address: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62204633-2312 Fax: +86-10-62204633-2304 E-mail: cti@ttl.com.cn Http://www.ttl.com.cn</p> <p>Glossary: DAE: data acquisition electronics Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system.</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range. Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required. The report provides only calibration results for DAE, it does not contain other performance test results. <p style="text-align: center;">Certificate No: Z18-60400 Page 2 of 3</p>
Primary Standards	ID #	Cal Date/Calibrated by, Certificate No.)	Scheduled Calibration						
Process Calibrator 753	1971018	20-Jun-18 (CTTL, No.J18X02034)	June-19						



In Collaboration with
TTL Calibration Laboratory
中国认可
国家互认
校准
CNAS L5570

Address: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62204633-2312 Fax: +86-10-62204633-2304
E-mail: cti@ttl.com.cn Http://www.ttl.com.cn

DC Voltage Measurement
A/D - Converter Resolution nominal
High Range: 1LSB = 5.1µV, full range = -100...+200 mV
Low Range: 1LSB = 81µV, full range = -1...+3mV
DASY measurement parameters: Auto Zero Time: 2 sec, Measuring time: 2 sec

Calibration Factors	X	Y	Z
High Range	405.306 ± 0.12% (k=2)	404.059 ± 0.15% (k=2)	404.180 ± 0.15% (k=2)
Low Range	3.98893 ± 0.7% (k=2)	3.95978 ± 0.7% (k=2)	3.98021 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system	258° ± 1°
-------------------------------------------	-----------

Certificate No: Z: 8-60400 Page 1 of 3

ES3DV3 Sn:3127



In Collaboration with
CALIBRATION LABORATORY
Address: No.51 Xuyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42316633-2312 Fax: +86-10-42316633-2304
E-mail: cal@ttsl.com.cn http://www.ttsl.com.cn



中国合格评定
国家认可
校准
CALIBRATION
CNAS L6570

Client: SRTC Certificate No: Z18-60398

CALIBRATION CERTIFICATE

Object: ES3DV3 - SN3127

Calibration Procedure(s): FF-Z11-004-01
Calibration Procedures for Dosimetric E-field Probes

Calibration date: November 02, 2018

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature(22±0.1)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	101919	20-Jun-18 (CTTL No.J18X05032)	Jun-19
Power sensor NRP-Z31	101547	20-Jun-18 (CTTL No.J18X05032)	Jun-19
Power sensor NRP-Z31	101548	20-Jun-18 (CTTL No.J18X05032)	Jun-19
Reference10dBAttenuator	18N50W-10dB	09-Feb-18(CTTL No.J18X01133)	Feb-20
Reference20dBAttenuator	18N50W-20dB	09-Feb-18(CTTL No.J18X01133)	Feb-20
Reference Probe EX3DV4	SN 3846	25-Jan-18(SPEAG No.EX3-3846_Jan18)	Jan-19
DAE4	SN 777	15-Dec-17(SPEAG No.DAE4-777_Dec17)	Dec-18

Secondary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
SignalGeneratorMG3700A	6201052605	21-Jun-18 (CTTL No.J18X05033)	Jun-19
Network Analyzer E5071C	MY46110673	14-Jan-18 (CTTL No.J18X00581)	Jan-19

Calibrated by: Yu Zongying SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyuan SAR Project Leader

Issued: November 04, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z18-60398

Page 1 of 11



In Collaboration with
CALIBRATION LABORATORY
Address: No.51 Xuyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42316633-2312 Fax: +86-10-42316633-2304
E-mail: cal@ttsl.com.cn http://www.ttsl.com.cn

Glossary:

TSL: tissue simulating liquid

NCRM_{x,y,z}: sensitivity in free space

ComF: sensitivity in TSL / NORM_{x,y,z}

DCP: diode compression point

CF: local factor (1/disk_offset) of the RF signal

A, E, C, D: modulation dependent linearization parameters

Polarization θ : θ rotation around probe axis

Polarization ϕ : ϕ rotation around an axis that is in the plane normal to probe axis (at measurement center), i

$\theta=0$ is normal to probe axis

Connector Angle: information used in DASY system to align probe sensor K to the root coordinate system

Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

b) IEC 62205-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 3 GHz)", July 2018

c) IEC 62208-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2018

d) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}: Assessed for E-field polarization $\theta=0$ (500MHz in TEM-cell; F>1800MHz: waveguide) NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not effect the E-field uncertainty inside TSL (see below ComF).
- NORM_(θ , ϕ , ψ) = NORM_{x,y,z} frequency response (see Frequency Response Chart). This function is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ComF.
- DCP_{x,y,z}: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A_k, B_k, C_k, D_k, V_k, X_k, Y_k, Z_k, A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ComF and Boundary Effect Parameters Assessed in flat phantom using E-field (or Temperature Transfer Standard for 600MHz) and inside waveguide using analytical field distributions based on power measurements for F<300MHz. The semi-ellipsoids are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} ComF whereas the uncertainty corresponds to that given for ComF. A frequency dependent ComF is used in DASY version 4.4 and higher which allows extending the validity from 50MHz to 100MHz.
- Spherical isotropy (SD deviation from isotropy): in a field of low gradients realized using a fix phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORM (no uncertainty required).

Certificate No: Z18-60398

Page 2 of 11

Probe ES3DV3

SN: 3127

Calibrated: November 02, 2018

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system)

Certificate No: Z18-60398

Page 3 of 11



In Collaboration with
TTL Calibration Laboratory
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-6230633-2512 Fax: +86-10-6230633-2504
E-mail: ent@ttest.com.cn Http://www.ttest.com.cn

DASY/EASY – Parameters of Probe: ES3DV3 - SN: 3127

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm($\mu\text{V}/\text{Vim}^2$) ^A	1.27	1.28	1.21	$\pm 10.0\%$
DCP(mV) ^B	103.3	104.4	105.0	

Modulation Calibration Parameters

UID	Communication System Name	A dB	B dB/ μV	C	D dB	VR mV	Unc ^C (k=2)
0	CW	X 0.0	0.0	1.0	0.00	285.6	$\pm 2.2\%$
		Y 0.0	0.0	1.0		287.9	
		Z 0.0	0.0	1.0		282.9	

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X, Y, Z do not affect the E² field uncertainty inside TSL (see Page 5 and Page 6).
^B Numerical linearization parameter; uncertainty not required.
^C Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



In Collaboration with
TTL Calibration Laboratory
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-6230633-2512 Fax: +86-10-6230633-2504
E-mail: ent@ttest.com.cn Http://www.ttest.com.cn

DASY/EASY – Parameters of Probe: ES3DV3 - SN: 3127

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] ^B	Relative Permittivity ^C	Conductivity (S/m) ^D	ConvF X	ConvF Y	ConvF Z	Alpha ^E	Depth ^F (mm)	Unc ^G (k=2)
750	41.9	0.89	6.34	6.34	6.34	0.40	1.35	$\pm 12.1\%$
835	41.5	0.90	6.18	6.18	6.18	0.35	1.58	$\pm 12.1\%$
1810	40.0	1.40	5.07	5.07	5.07	0.66	1.24	$\pm 12.1\%$
2000	40.0	1.40	4.95	4.95	4.95	0.70	1.20	$\pm 12.1\%$
2300	39.5	1.57	4.79	4.79	4.79	0.80	1.08	$\pm 12.1\%$
2450	39.2	1.80	4.65	4.65	4.65	0.90	1.08	$\pm 12.1\%$
2600	39.0	1.95	4.40	4.40	4.40	0.80	1.21	$\pm 12.1\%$

^B Frequency validity above 300 MHz of $\pm 100\text{MHz}$ only applies for DASY v4.4 and higher (Page 2), else it is restricted to $\pm 50\text{MHz}$. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is $\pm 10, 25, 40, 50$ and 70MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to $\pm 110\text{MHz}$.

^C At frequency below 3 GHz, the validity of tissue parameters (c and d) can be relaxed to $\pm 10\%$ if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and d) is restricted to $\pm 5\%$. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^E Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than $\pm 1\%$ for frequencies below 3 GHz and below $\pm 2\%$ for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



In Collaboration with
TTL Calibration Laboratory
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-6230633-2512 Fax: +86-10-6230633-2504
E-mail: ent@ttest.com.cn Http://www.ttest.com.cn

DASY/EASY – Parameters of Probe: ES3DV3 - SN: 3127

Calibration Parameter Determined in Body Tissue Simulating Media

f [MHz] ^B	Relative Permittivity ^C	Conductivity (S/m) ^D	ConvF X	ConvF Y	ConvF Z	Alpha ^E	Depth ^F (mm)	Unc ^G (k=2)
750	55.5	0.96	6.33	6.33	6.33	0.40	1.40	$\pm 12.1\%$
835	55.2	0.97	6.13	6.13	6.13	0.37	1.62	$\pm 12.1\%$
1810	53.3	1.52	4.78	4.76	4.76	0.65	1.27	$\pm 12.1\%$
2000	53.3	1.52	4.80	4.80	4.80	0.67	1.27	$\pm 12.1\%$
2300	52.9	1.81	4.48	4.46	4.46	0.90	1.16	$\pm 12.1\%$
2450	52.7	1.95	4.31	4.31	4.31	0.76	1.28	$\pm 12.1\%$
2600	52.5	2.10	4.14	4.14	4.14	0.90	1.10	$\pm 12.1\%$

^B Frequency validity above 300 MHz of $\pm 100\text{MHz}$ only applies for DASY v4.4 and higher (Page 2), else it is restricted to $\pm 50\text{MHz}$. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is $\pm 10, 25, 40, 50$ and 70MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to $\pm 110\text{MHz}$.


^C At frequency below 3 GHz, the validity of tissue parameters (c and d) can be relaxed to $\pm 10\%$ if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and d) is restricted to $\pm 5\%$. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^E Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than $\pm 1\%$ for frequencies below 3 GHz and below $\pm 2\%$ for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



In Collaboration with
TTL Calibration Laboratory
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-6230633-2512 Fax: +86-10-6230633-2504
E-mail: ent@ttest.com.cn Http://www.ttest.com.cn

Frequency Response of E-Field (TEM-Cell: if110 EXX, Waveguide: R22)

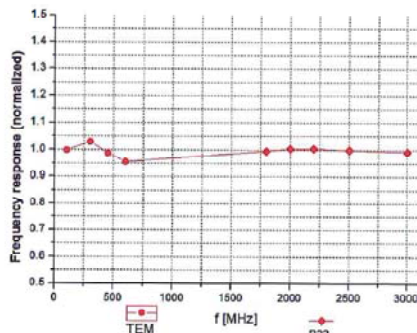


Uncertainty of Frequency Response of E-field: $\pm 7.4\%$ (k=2)



In Collaboration with
TTL Calibration Laboratory
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62194631-2312 Fax: +86-10-62194631-2304
E-mail: csl@china.ttl.com.cn <http://www.china.ttl.com>

Receiving Pattern (Φ), $\theta=0^\circ$

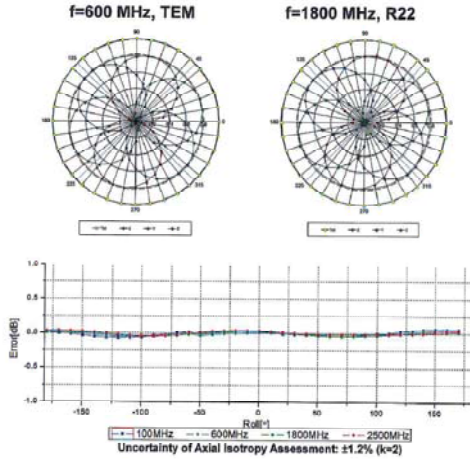


Certificate No: Z18-60398 Page 8 of 11



In Collaboration with
TTL Calibration Laboratory
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62194631-2312 Fax: +86-10-62194631-2304
E-mail: csl@china.ttl.com.cn <http://www.china.ttl.com>

Dynamic Range f(SAR_{head})
(TEM cell, f = 900 MHz)

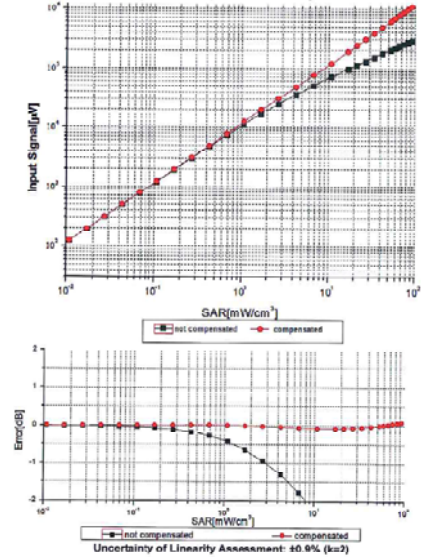


Certificate No: Z18-60398 Page 9 of 11




In Collaboration with
TTL Calibration Laboratory
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62194631-2312 Fax: +86-10-62194631-2304
E-mail: csl@china.ttl.com.cn <http://www.china.ttl.com>

Conversion Factor Assessment

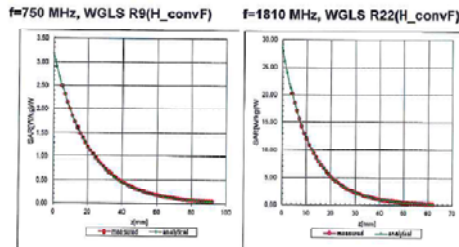

Deviation from Isotropy in Liquid

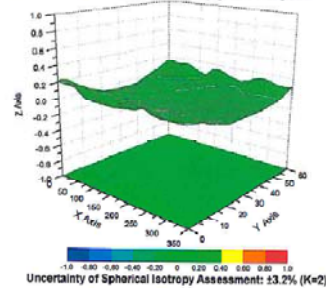

Certificate No: Z18-60398 Page 10 of 11



In Collaboration with
TTL Calibration Laboratory
Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62194631-2312 Fax: +86-10-62194631-2309
E-mail: csl@china.ttl.com.cn <http://www.china.ttl.com>

Appendix: Modulation Calibration Parameters

UID	Communication System Name	PAR	A dB	B dB μ V	C	VR mV	Unc ² (k=2)
0	CW	0.00	X	0.0	0.0	1.0	282.3
			Y	0.0	0.0	1.0	280.9
			Z	0.0	0.0	1.0	275.1
10012	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	1.87	X	2.77	68.02	18.46	143.0
			Y	2.75	68.05	18.52	145.0
			Z	2.71	67.79	18.25	142.3
10100	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	5.67	X	6.13	66.4	18.97	141.9
			Y	6.15	66.49	19.06	144.2
			Z	6.09	66.32	18.90	140.9
10108	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	5.80	X	6.09	66.24	19.07	139.5
			Y	6.10	66.33	19.15	141.5
			Z	6.05	66.19	19.05	138.0
10154	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	5.75	X	5.81	65.85	18.93	136.1
			Y	5.82	65.92	19.01	137.8
			Z	5.79	65.89	18.97	134.7
10169	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	5.73	X	4.84	65.92	19.20	130.8
			Y	4.82	65.98	19.27	131.3
			Z	4.80	66.00	19.29	129.1
10175	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	5.72	X	4.88	66.14	19.40	131.6
			Y	4.83	66.08	19.33	130.9
			Z	4.79	66.02	19.29	129.3
10297	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	5.81	X	6.19	66.61	19.42	141.9
			Y	6.13	66.43	19.26	140.7
			Z	6.14	66.52	19.33	139.6

Certificate No: Z17-97142 Page 12 of 12

DAE4 Sn:720

In Collaboration with
TTL S P E A G
CALIBRATION LABORATORY

中国认可
国际互认
校准
CNAS L6570

Address: No.31 Xuyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62394633-2512 Fax: +86-10-62394633-2504
E-mail: csl@chinafl.com Http://www.chinafl.com

Client: SRTC Certificate No: Z18-60399

CALIBRATION CERTIFICATE

Object: DAE4 - SN: 720

Calibration Procedure(s): FF-Z11-002-01
Calibration Procedure for the Data Acquisition Electronics (DAEx)

Calibration date: October 15, 2018

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(23±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Process Calibrator 753	1971018	20-Jun-18 (CTTL, No.J18X05034)	June-19

Calibrated by: Yu Zongying SAR Test Engineer
Reviewed by: Lin Hao SAR Test Engineer
Approved by: Qi Dianyuan SAR Project Leader

Signature: [Signatures]

Issued: October 17, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z18-60399

Page 1 of 3

In Collaboration with
TTL S P E A G
CALIBRATION LABORATORY

中国认可
国际互认
校准
CNAS L6570

Address: No.31 Xuyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62394633-2512 Fax: +86-10-62394633-2504
E-mail: csl@chinafl.com Http://www.chinafl.com

Glossary:
DAE: data acquisition electronics
Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters:

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.

Certificate No: Z18-60399

Page 2 of 3

In Collaboration with
TTL S P E A G
CALIBRATION LABORATORY

中国认可
国际互认
校准
CNAS L6570

Address: No.31 Xuyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62394633-2512 Fax: +86-10-62394633-2504
E-mail: csl@chinafl.com Http://www.chinafl.com

DC Voltage Measurement
A/D - Converter Resolution constant
High Range: 1LSB = 6.1µV, full range = -100...+300 mV
Low Range: 1LSB = 61µV, full range = -1...+3mV
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	403.543 ± 0.15% (k=2)	404.773 ± 0.15% (k=2)	403.205 ± 0.15% (k=2)
Low Range	3.95574 ± 0.7% (k=2)	3.95559 ± 0.7% (k=2)	3.95585 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system	29° ± 1°
-------------------------------------------	----------

Certificate No: Z18-60399

Page 3 of 3

EX3DV4 Sn:3708 (1/7)

Calibration Laboratory of Schmid & Partner Engineering AG
Zughohestrasse 43, 8034 Zurich, Switzerland
Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates
Client: SRTC (Auden)
Certificate No: EX3-3708_Oct18



CALIBRATION CERTIFICATE

Object: EX3DV4 - SN:3708
Calibration procedure(s): QA CAL-01-v9, QA CAL-12-v9, QA CAL-14-v4, QA CAL-23-V5, QA CAL-25-V6
Calibration procedure for dosimetric E-field probes
Calibration date: October 22, 2018

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.
All calibrations have been conducted in the closed laboratory facility, environment temperature (22 ± 0.2°C) and humidity = 70%.

Calibration Equipment used (MUTC critical for calibration)

Primary Standards	ID	Cal Data (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-18 (No. 217-208720282)	Apr-18
Power sensor NRP-231	SN: 103244	06-Apr-18 (No. 217-20872)	Apr-18
Reference 50 Ω Attenuator	SN: 59377 (270)	06-Apr-18 (No. 217-20883)	Apr-18
Reference Probe ERK3V1	SN: 3013	30-Dec-17 (No. 203-3013_Cert17)	Dec-18
DASA	SN: 680	21-Dec-17 (No. 204-4905_Cert17)	Dec-18

Secondary Standards	ID	Check Data (in house)	Scheduled Check
Power meter U4418B	SN: 1081202074	06-Apr-18 (in house check Jun-18)	In house check Jun-20
Power sensor E4413A	SN: M14189307	06-Apr-18 (in house check Jun-18)	In house check Jun-20
Power sensor E4413A	SN: 20110270	06-Apr-18 (in house check Jun-18)	In house check Jun-20
HP generator HP 8548C	SN: 10590005100	06-Apr-18 (in house check Jun-18)	In house check Jun-20
Network Analyser F5550A	SN: 1054100077	31-Mar-14 (in house check Oct-16)	In house check Oct-19

Calibrated by: Gualdo LAMAR, Laboratory Technician
Approved by: Kjetil FRIBO, Technical Manager
Issued: October 23, 2018
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of Schmid & Partner Engineering AG
Zughohestrasse 43, 8034 Zurich, Switzerland
Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates
Accreditation No.: SCS 0108



Glossary:
TSL: Issue simulating liquid sensitivity in base space
NORM_{x,y,z}: sensitivity in TSL, NORM_{x,y,z} disc compression point
CompF: crest factor (1/√duty_cycle) of the RF signal
DCP: modulation dependent linearization parameters
A, B, C, D: rotation around probe axis
Polarization α: rotation around probe axis that is in the plane normal to probe axis (at measurement center), i.e. α = 0 is normal to probe axis
Connector Angle: information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:
a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from head-and-body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
d) ICB 855654, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:
• NORM_{x,y,z}: Assessed for E-field polarization S = 0 (f ≤ 300 MHz in TEM-cell; f = 300 MHz: R12 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E-field uncertainty inside TSL (see below CompF).
• NORM_{x,y,z} = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions lower than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of CompF.
• DCP_{x,y,z}: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
• PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
• A_{x,y,z}, B_{x,y,z}, C_{x,y,z}, D_{x,y,z}, VR_{x,y,z}, A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the disc.
• CompF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 300 MHz) and inside waveguide using analytical field distributions based on power measurements for f = 300 MHz. The same values are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy data to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * CompF whereby the uncertainty corresponds to that given for CompF. A frequency dependent CompF is used in DASY version 4.4 and higher which allows extending the validity from 40 MHz to ± 100 MHz.
• Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
• Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
• Connector Angle: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

EX3DV4 - SN:3708 October 22, 2018

Probe EX3DV4
SN:3708

Manufactured: July 21, 2009
Calibrated: October 22, 2018

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

EX3DV4 - SN:3708 October 22, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc. (k=2)
Norm. $\sqrt{U_{rms}^2}$ [V/m]	0.20	0.35	0.42	± 10.1 %
DCP [mV]	95.4	103.6	100.4	

Modulation Calibration Parameters

UD	Communication System Name	A	B	C	D	VR	Unc. (k=2)
0	CW	X: 0.0	0.0	1.0	0.00	134.7	± 3.5 %
		Y: 0.0	0.0	1.0	0.00	130.8	
		Z: 0.0	0.0	1.0	0.00	146.8	

Note: For details on UD parameters see Appendix.

Sensor Model Parameters

	C1	C2	σ	T1	T2	T3	T4	T5	T6
	dB	dB	V ²	ms/V ²	ms/V ²	ms	V ²	V ²	V ²
X	33.84	270.1	40.07	9.383	1.302	0.022	0.006	0.762	1.008
Y	40.04	291.1	34.06	15.47	0.801	0.012	1.758	0.156	1.005
Z	36.34	262.2	35.97	11.65	0.890	0.001	0.000	0.909	1.008

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

¹ The uncertainties of Norm. X,Y,Z do not affect the E-field uncertainty inside TSL, (see Pages 2 and 6).
² Numerical linearization parameter; uncertainty not required.
³ Uncertainty is determined using the rms. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4 Sn:3708 (2/7)

EX3DV4-SN3708

October 22, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz)	Relative Permittivity ^a	Conductivity (S/m) ^b	ConvF X	ConvF Y	ConvF Z	Alpha ^c	Depth (mm)	Unc (k=2)
450	43.5	0.87	9.79	9.79	9.79	0.14	1.20	± 13.3 %
750	41.8	0.89	9.59	9.59	9.59	0.54	0.80	± 12.0 %
835	41.5	0.90	9.16	9.16	9.16	0.51	0.82	± 12.0 %
1450	40.5	1.20	8.50	8.50	8.50	0.33	0.80	± 12.0 %
1750	40.1	1.37	8.20	8.20	8.20	0.28	0.84	± 12.0 %
1900	40.0	1.40	7.89	7.89	7.89	0.35	0.85	± 12.0 %
2000	40.0	1.40	7.86	7.86	7.86	0.34	0.80	± 12.0 %
2300	39.5	1.87	7.51	7.51	7.51	0.29	0.86	± 12.0 %
2450	39.2	1.80	7.13	7.13	7.13	0.38	0.86	± 12.0 %
2600	38.0	1.96	7.01	7.01	7.01	0.38	0.87	± 12.0 %
5200	35.0	4.68	5.48	5.48	5.48	0.40	1.80	± 13.1 %
5300	35.9	4.78	5.25	5.25	5.25	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.84	4.84	4.84	0.40	1.80	± 13.1 %
5800	35.3	5.27	5.04	5.04	5.04	0.40	1.80	± 13.1 %

^a Frequency validity above 300 MHz of a 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 10 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is a 10, 20, 40, 50 and 70 MHz for ConvF assessments at 30, 60, 120, 150 and 230 MHz respectively. Above 5 GHz frequency validity can be extended to a 100 MHz.
^b At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured S11 values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.
^c Alpha (α) is determined during calibration. SRTAC warrants that the repeatability deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX3-3708_Oct18

Page 5 of 39

EX3DV4-SN3708

October 22, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz)	Relative Permittivity ^a	Conductivity (S/m) ^b	ConvF X	ConvF Y	ConvF Z	Alpha ^c	Depth (mm)	Unc (k=2)
450	56.7	0.94	10.35	10.35	10.35	0.08	1.20	± 13.3 %
750	55.5	0.96	9.51	9.51	9.51	0.50	0.85	± 12.0 %
835	55.2	0.97	9.33	9.33	9.33	0.47	0.84	± 12.0 %
1450	54.0	1.30	7.84	7.84	7.84	0.38	0.80	± 12.0 %
1750	53.4	1.49	7.69	7.69	7.69	0.37	0.85	± 12.0 %
1900	53.3	1.52	7.56	7.56	7.56	0.42	0.84	± 12.0 %
2000	53.3	1.52	7.53	7.53	7.53	0.41	0.85	± 12.0 %
2300	52.9	1.81	7.34	7.34	7.34	0.39	0.88	± 12.0 %
2450	52.7	1.95	7.19	7.19	7.19	0.32	0.95	± 12.0 %
2600	52.5	2.16	7.14	7.14	7.14	0.32	0.95	± 12.0 %
5200	48.0	5.30	4.53	4.53	4.53	0.50	1.90	± 13.1 %
5300	48.9	5.42	4.41	4.41	4.41	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.99	3.99	3.99	0.50	1.90	± 13.1 %
5800	48.2	6.00	4.21	4.21	4.21	0.50	1.90	± 13.1 %

^a Frequency validity above 300 MHz of a 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 10 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is a 10, 20, 40, 50 and 70 MHz for ConvF assessments at 30, 60, 120, 150 and 230 MHz respectively. Above 5 GHz frequency validity can be extended to a 100 MHz.
^b At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured S11 values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.
^c Alpha (α) is determined during calibration. SRTAC warrants that the repeatability deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


Certificate No: EX3-3708_Oct18

Page 6 of 39

EX3DV4-SN3708

October 22, 2018

Frequency Response of E-Field
(TEM-Cell:1H110 EXX, Waveguide: R22)

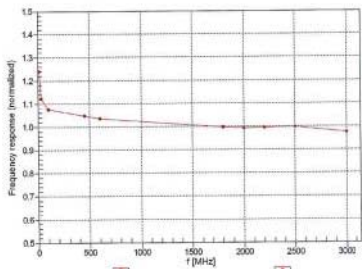

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)



Certificate No: EX3-3708_Oct18

Page 7 of 39

EX3DV4-SN3708

October 22, 2018

Receiving Pattern (ϕ), θ = 0°

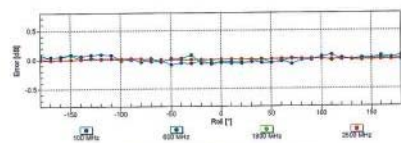
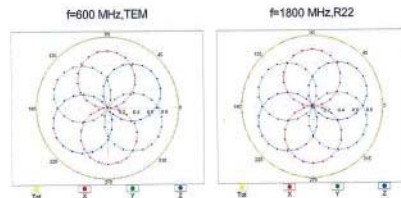


Uncertainty of Axial isotropy Assessment: ± 0.5% (k=2)

Certificate No: EX3-3708_Oct18

Page 8 of 39

EX3DV4 Sn:3708 (3/7)

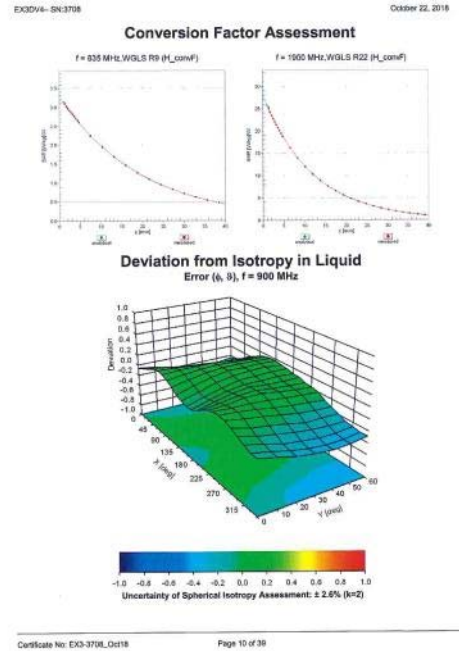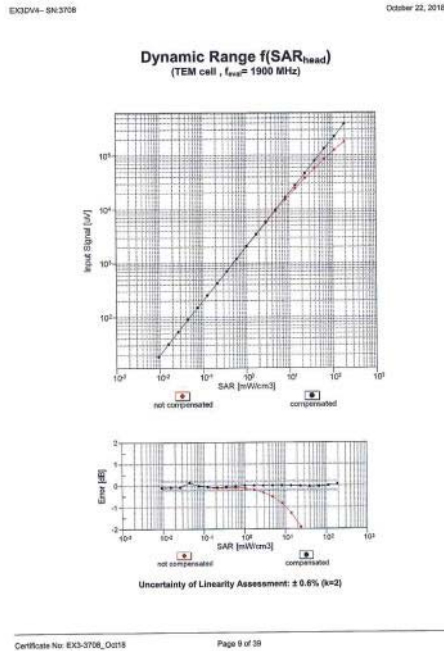

EX3DV4-SN3708 October 22, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708

Other Probe Parameters	
Sensor Arrangement	Triangular
Connector Angle (°)	0.5
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4 Sn:3708 (7/7)

EX3DV4- SN:3708		October 22, 2018	
1007- AAB	IEEE 802.11ac WFI (20MHz, MCS0, 30pps duty cycle)	X	4.30 68.88 16.10 0.46 130.0 ±9.6%
		Y	4.50 69.24 16.15 130.0
		Z	4.40 69.22 16.20 130.0
1008- AAB	IEEE 802.11ac WFI (20MHz, MCS1, 30pps duty cycle)	X	4.43 69.20 16.24 0.46 130.0 ±9.6%
		Y	4.65 69.50 16.30 130.0
		Z	4.54 69.56 16.35 130.0
1009- AAB	IEEE 802.11ac WFI (20MHz, MCS2, 30pps duty cycle)	X	4.33 69.20 16.03 0.46 130.0 ±9.6%
		Y	4.54 69.42 16.12 130.0
		Z	4.45 69.37 16.10 130.0
1010- AAB	IEEE 802.11ac WFI (20MHz, MCS3, 30pps duty cycle)	X	4.38 69.08 16.23 0.46 130.0 ±9.6%
		Y	4.60 69.00 16.30 130.0
		Z	4.48 69.05 16.25 130.0
1011- AAB	IEEE 802.11ac WFI (20MHz, MCS4, 30pps duty cycle)	X	4.39 69.07 16.25 0.46 130.0 ±9.6%
		Y	4.51 69.39 16.13 130.0
		Z	4.40 69.34 16.17 130.0
1012- AAB	IEEE 802.11ac WFI (20MHz, MCS5, 30pps duty cycle)	X	4.35 69.08 16.18 0.46 130.0 ±9.6%
		Y	4.51 69.50 16.17 130.0
		Z	4.39 69.58 16.50 130.0
1013- AAB	IEEE 802.11ac WFI (20MHz, MCS6, 30pps duty cycle)	X	4.27 69.09 16.09 0.46 130.0 ±9.6%
		Y	4.50 69.34 16.02 130.0
		Z	4.39 69.39 16.05 130.0
1014- AAB	IEEE 802.11ac WFI (20MHz, MCS7, 30pps duty cycle)	X	4.26 69.17 16.21 0.46 130.0 ±9.6%
		Y	4.47 69.29 16.30 130.0
		Z	4.36 69.23 16.30 130.0
1015- AAB	IEEE 802.11ac WFI (20MHz, MCS8, 30pps duty cycle)	X	4.27 69.16 16.16 0.46 130.0 ±9.6%
		Y	4.50 69.18 16.66 130.0
		Z	4.39 69.85 16.52 130.0
1016- AAB	IEEE 802.11ac WFI (40MHz, MCS0, 30pps duty cycle)	X	4.96 69.20 16.34 0.46 130.0 ±9.6%
		Y	5.12 69.50 16.39 130.0
		Z	5.10 69.38 16.07 130.0
1017- AAB	IEEE 802.11ac WFI (40MHz, MCS1, 30pps duty cycle)	X	5.02 69.34 16.39 0.46 130.0 ±9.6%
		Y	5.17 69.39 16.34 130.0
		Z	5.10 69.38 16.07 130.0
1018- AAB	IEEE 802.11ac WFI (40MHz, MCS2, 30pps duty cycle)	X	4.91 69.35 16.40 0.46 130.0 ±9.6%
		Y	5.08 69.77 16.40 130.0
		Z	5.00 69.31 16.11 130.0
1019- AAB	IEEE 802.11ac WFI (40MHz, MCS3, 30pps duty cycle)	X	4.96 69.33 16.32 0.46 130.0 ±9.6%
		Y	5.08 69.52 16.20 130.0
		Z	5.01 69.09 16.30 130.0
1020- AAB	IEEE 802.11ac WFI (40MHz, MCS4, 30pps duty cycle)	X	5.03 69.21 16.31 0.46 130.0 ±9.6%
		Y	5.18 69.53 16.25 130.0
		Z	5.09 69.11 16.09 130.0
1021- AAB	IEEE 802.11ac WFI (40MHz, MCS5, 30pps duty cycle)	X	5.01 69.30 16.50 0.46 130.0 ±9.6%
		Y	5.18 69.72 16.48 130.0
		Z	5.10 69.37 16.20 130.0
1022- AAB	IEEE 802.11ac WFI (40MHz, MCS6, 30pps duty cycle)	X	5.01 69.42 16.50 0.46 130.0 ±9.6%
		Y	5.18 69.83 16.52 130.0
		Z	5.09 69.37 16.24 130.0

Certificate No: EX3-3708_Out16

Page 36 of 38

EX3DV4- SN:3708		October 22, 2018	
1023- AAC	IEEE 802.11ac WFI (80MHz, MCS0, 30pps duty cycle)	X	5.68 69.76 16.50 0.46 130.0 ±9.6%
		Y	5.98 67.16 16.45 130.0
		Z	5.90 69.26 16.52 130.0
1024- AAC	IEEE 802.11ac WFI (80MHz, MCS4, 30pps duty cycle)	X	5.70 69.53 16.33 0.46 130.0 ±9.6%
		Y	5.88 67.13 16.50 130.0
		Z	5.88 69.72 16.13 130.0
10241- AAC	IEEE 802.11ac WFI (80MHz, MCS5, 30pps duty cycle)	X	5.97 69.06 16.51 0.46 130.0 ±9.6%
		Y	6.01 67.08 16.50 130.0
		Z	5.98 69.74 16.16 130.0
10242- AAC	IEEE 802.11ac WFI (80MHz, MCS6, 30pps duty cycle)	X	5.94 69.92 16.72 0.46 130.0 ±9.6%
		Y	6.08 67.38 16.68 130.0
		Z	5.98 69.88 16.48 130.0
10243- AAC	IEEE 802.11ac WFI (80MHz, MCS7, 30pps duty cycle)	X	5.76 69.59 16.43 0.46 130.0 ±9.6%
		Y	5.89 67.02 16.50 130.0
		Z	5.83 69.05 16.18 130.0
10244- AAC	IEEE 802.11ac WFI (80MHz, MCS8, 30pps duty cycle)	X	5.83 69.71 16.52 0.46 130.0 ±9.6%
		Y	5.98 67.32 16.50 130.0
		Z	5.97 69.89 16.31 130.0
10246- AAC	IEEE 802.11ac WFI (160MHz, MCS0, 30pps duty cycle)	X	6.16 67.41 16.53 0.46 130.0 ±9.6%
		Y	6.27 67.25 16.48 130.0
		Z	6.04 69.05 16.31 130.0
10246- AAF	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL, Subframe=2,7)	X	9.04 92.83 31.00 0.30 130.0 ±9.6%
		Y	16.22 106.00 36.65 60.0
		Z	10.43 96.01 32.33 60.0
10247- AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL, Subframe=2,7)	X	9.34 91.27 30.00 0.30 130.0 ±9.6%
		Y	13.94 103.46 34.79 60.0
		Z	9.34 94.22 31.85 60.0
10248- AAA	CDMA2000 (1X Adaptive)	X	0.32 90.00 5.00 0.00 130.0 ±9.6%
		Y	0.59 93.51 9.94 160.0
		Z	0.44 90.36 7.17 130.0
10252- AAD	LTE-TDD (OFDMA, 3 MHz, E-TM 3.1, Clipping 44%)	X	3.20 69.29 16.87 2.23 60.0 ±9.6%
		Y	3.96 67.38 16.44 60.0
		Z	3.26 69.84 16.56 60.0
10253- AAD	LTE-TDD (OFDMA, 10 MHz, E-TM 3.1, Clipping 44%)	X	3.78 69.70 16.24 2.23 60.0 ±9.6%
		Y	4.08 66.63 16.60 60.0
		Z	3.87 68.57 16.54 60.0
10254- AAD	LTE-TDD (OFDMA, 13 MHz, E-TM 3.1, Clipping 44%)	X	3.81 69.38 16.33 2.23 60.0 ±9.6%
		Y	4.08 66.15 16.62 60.0
		Z	3.89 68.38 16.50 60.0
10255- AAD	LTE-TDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)	X	3.89 69.27 16.38 2.23 60.0 ±9.6%
		Y	4.12 68.58 16.65 60.0
		Z	3.96 69.32 16.15 60.0
10265- AAA	Pulse Waveform (200Hz, 10%)	X	3.95 69.00 12.97 10.00 50.0 ±9.6%
		Y	7.30 77.05 16.50 50.0
		Z	3.92 76.95 16.50 50.0
10269- AAA	Pulse Waveform (200Hz, 20%)	X	3.90 68.91 13.74 6.69 50.0 ±9.6%
		Y	6.69 83.57 16.50 50.0
		Z	3.84 81.85 16.51 50.0

Certificate No: EX3-3708_Out16

Page 36 of 39

750V3 Sn:1101 (1/2)

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

中国认可
国际互认
校准
CNAS 18070

Client: **SRTC** Certificate No: **Z17-97134**

CALIBRATION CERTIFICATE

Object: D750V3 - SN: 1101

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: September 13, 2017

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(23±1)°C and humidity<70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRV0	102196	02-Mar-17 (CTTL, No.J17X01254)	Mar-18
Power sensor NRV-Z5	100596	02-Mar-17 (CTTL, No.J17X01254)	Mar-18
Reference Probe EX3DV4	SN 7433	26-Sep-16(SPEAG, No EX3-7433_Sep16)	Sep-17
DAEA	SN 1331	19-Jan-17(CTTL-SPEAG, No Z17-97015)	Jan-18

Secondary Standards	ID #	Cal Date(Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-17 (CTTL, No.J17X00286)	Jan-18
Network Analyzer ES071C	MY46111013	13-Jan-17 (CTTL, No.J17X00285)	Jan-18

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Yu Zongying SAR Test Engineer

Approved by: Qi Dianyuan SAR Project Leader

Issued: September 16, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: Z17-97134 Page 1 of 8

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Address: No. 51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2304
E-mail: csl@china-test.com http://www.china-test.cn

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- KDB85664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z17-97134 Page 2 of 8

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Address: No. 51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2304
E-mail: csl@china-test.com http://www.china-test.cn

Measurement Conditions

DASY system configuration, as far as not given on page 1

DASY Version	DASY52	52.10.0.1448
Extrapolation	Advanced Extrapolation	
Phantom	Triaxial Flat Phantom S-1C	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied

Temperature	Permittivity	Conductivity	
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.5 ± 6 %	0.88 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.05 mW/g
SAR for nominal Head TSL parameters	normalized to 1W	8.26 mW/g ± 18.8 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.34 mW/g
SAR for nominal Head TSL parameters	normalized to 1W	5.39 mW/g ± 18.7 % (k=2)

Body TSL parameters

The following parameters and calculations were applied

Temperature	Permittivity	Conductivity	
Nominal Body TSL parameters	22.0 °C	55.5	0.96 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.4 ± 6 %	0.95 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.15 mW/g
SAR for nominal Body TSL parameters	normalized to 1W	8.69 mW/g ± 18.8 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.42 mW/g
SAR for nominal Body TSL parameters	normalized to 1W	5.73 mW/g ± 18.7 % (k=2)

Certificate No: Z17-97134 Page 3 of 8

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Address: No. 51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2304
E-mail: csl@china-test.com http://www.china-test.cn

Appendix (Additional assessments outside the scope of CNAS 18070)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.00 ± 0.24jΩ
Return Loss	-28.4dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	52.00 ± 0.22jΩ
Return Loss	-30.9dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.136 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z17-97134 Page 4 of 8