

---

## APPENDIX B EUT TEST POSITION PHOTOS

---

### Liquid depth $\geq 15\text{cm}$

Phantom: SAM (30deg probe tilt) with CRP v5.0\_20150321; Type: QD000P40CD; Serial: TP:1874



**Handheld Mode:**

**Handheld Back Setup Photo(0mm)**




**Handheld Front Setup Photo(0mm)**



**Handheld Left Setup Photo(0mm)**



**Handheld Right Setup Photo(0mm)**

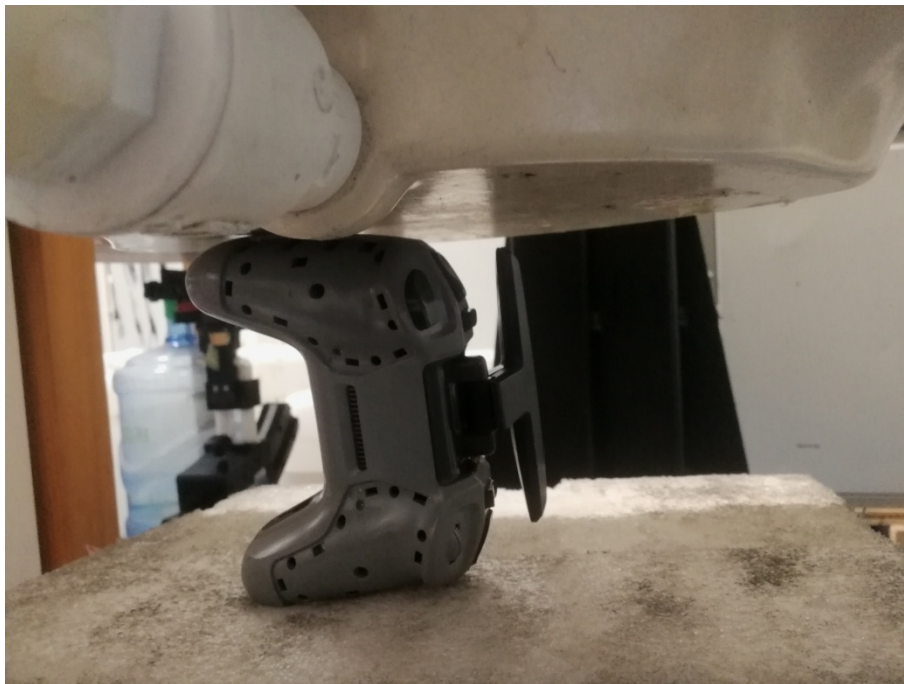

**Handheld Top Setup Photo(0mm)**




**Handheld Bottom Setup Photo(0mm)**




**Close to Body Mode:**


**Close to Body Back Setup Photo (10mm)**

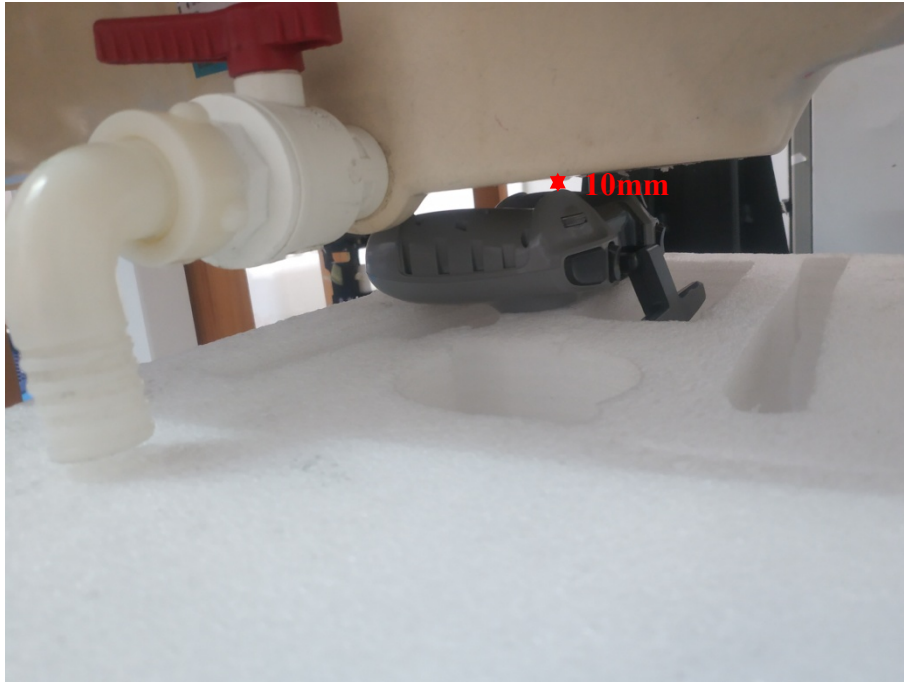


**Close to Body Front Setup Photo (10mm)**

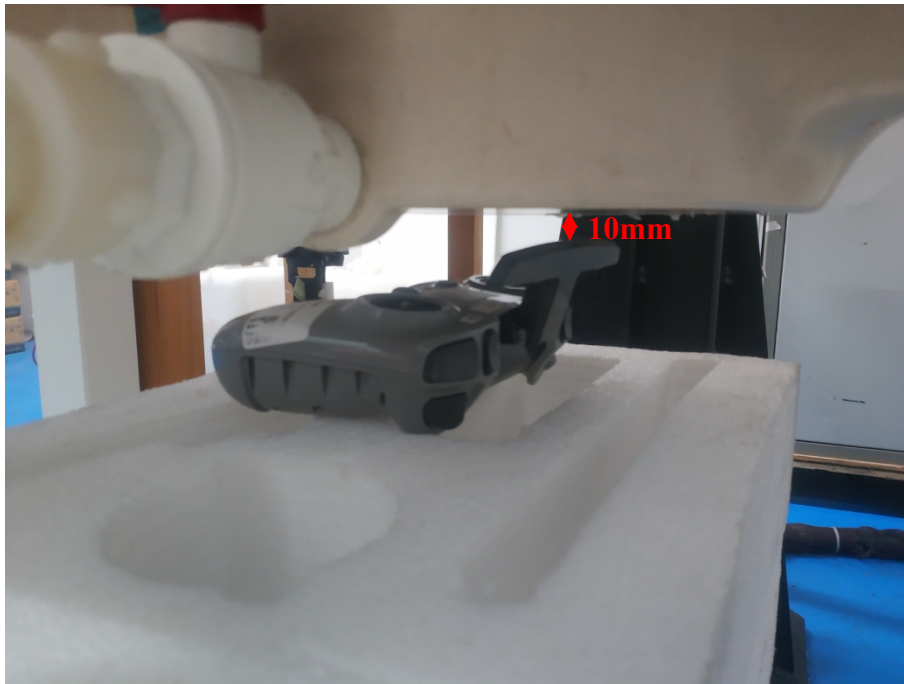


**Close to Body Left Setup Photo (10mm)**

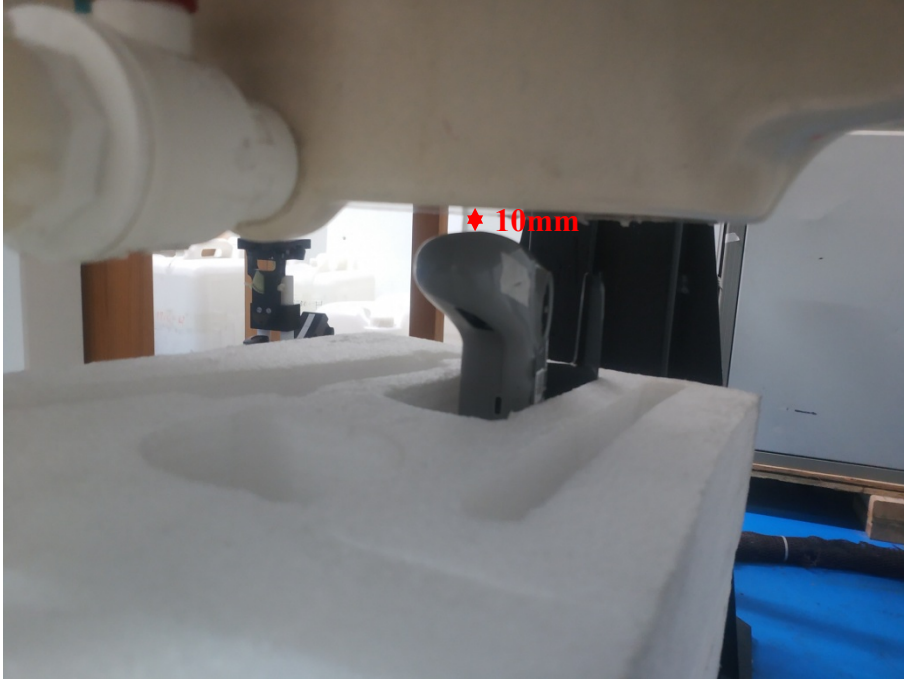

**Close to Body Right Setup Photo (10mm)**

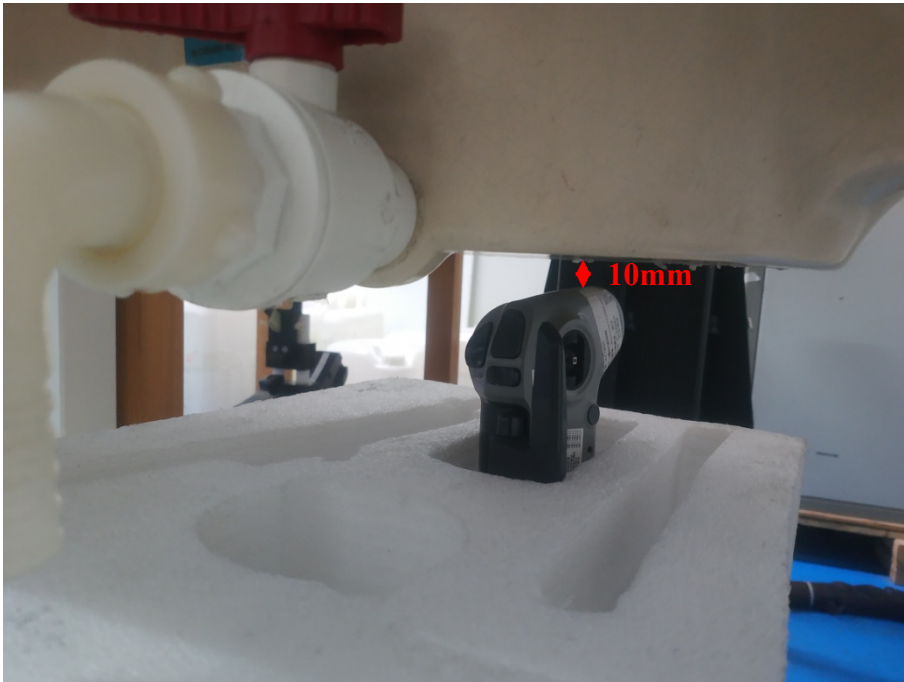

**Close to Body Top Setup Photo (10mm)**

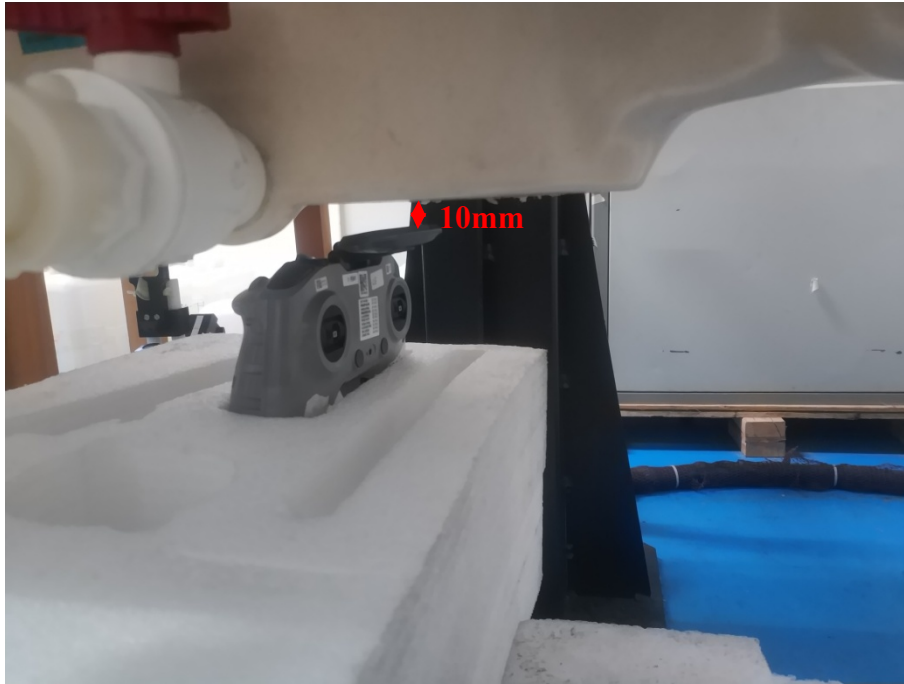

**Close to Body Bottom Setup Photo (10mm)**

