

# SAR EVALUATION REPORT

<b>Test Report No.</b>	<b>W158R-D006</b>		
<b>Applicant</b>	<b>Bluebird Inc.</b> <b>(Dogok-dong, SEI Tower 13,14)39, Eonjuro30-gil, Gangnam-gu, Seoul, South Korea</b>		
<b>Model Name</b>	<b>MT280</b>		
<b>DUT Type</b>	<b>Mobile Payment Terminal</b>		
<b>Application Type</b>	<b>Certification</b>		
<b>FCC ID</b>	<b>SS4MT280</b>		
<b>Date of Report</b>	<b>Aug 31, 2015</b>		
<b>Date of Test</b>	<b>Aug 17, 2015 ~ Aug 28, 2015</b>		
<b>Test Laboratory</b>	<b>ONETECH</b> <b>301-14 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862, Korea</b>		
<b>Procedures</b>	<b>KDB 865664</b> <b>IEEE 1528-2003</b> <b>ANSI/IEEE C95.1, C95.3</b> <b>FCC CFR §2.1093</b> <b>RSS-102 Issue 4</b>		
<b>Max SAR(1g)</b>	<b>1.657 W/kg</b>		
<b>Test Opinion</b>	<b>Satisfied to FCC requirements</b>		
<b>Report Author</b>	<b>Jungwook Kim</b>	 _____	<b>Aug 31, 2015</b>
<b>Test Engineer</b>	<b>Youngyong Kim</b>	 _____	<b>Aug 31, 2015</b>

This report details the results of the testing carried out on one sample, the results contained in this test report do not relate to other samples of the same product. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report.

This report may only be reproduced and distribute in full. If the product in this report is used in any configuration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards. Any mention of ONETECH Corp. or testing done by ONETECH Corp. In connection with distribution or use of the product described in this report must be approved by ONETECH Corp. in writing.

# TABLE OF CONTENTS

1. DUT INFORMATION .....	3
2. INTRODUCTION .....	4
3. SAR MEASUREMENT SETUP .....	5
4. MEASUREMENT UNCERTAINTY .....	9
5. ANSI/IEEE C95.1-2005 RF EXPOSURE LIMIT .....	11
6. SYSTEM AND LIQUID VERIFICATION .....	12
7. SAR MEASUREMENT PROCEDURES .....	16
8. TEST EQUIPMENT LIST .....	18
9. RF CONDUCTED POWER .....	20
10. SAR TEST RESULTS .....	24
ANNEX A. SYSTEM VERIFICATION PLOTS .....	25
ANNEX B. SAR TEST PLOTS .....	28
ANNEX C. PHOTOGRAPHS .....	47
ANNEX D. ANTENNA INFORMATION .....	59
ANNEX E. PROBE AND DIPOLE CALIBRATION CERTIFICATES .....	62

## 1. DUT INFORMATION

DUT Description	Mobile Payment Terminal
Model Name	MT280
Serial Number	Identical Prototype
Mode of Operation	GSM 850, GSM 1900, WLAN, Bluetooth
TX Frequency Range	824.2 MHz ~ 848.8 MHz (GSM 850) 1 850.2 MHz ~ 1 909.8 MHz (GSM 1900) 2 412 MHz ~ 2 462 MHz (802.11 b/g/n_HT20) 2 402 MHz ~ 2 480 MHz (Bluetooth)
Maximum Average Conducted Power	GSM 850 : 33.01 dBm (ch 251) GSM 1900 : 29.85 dBm (ch 661) 802.11b : 14.24 dBm (ch 11) Bluetooth : 7.03 dBm (ch 78)
Summary of peak SAR (10g)	<b>GSM 850 : 1.657 W/kg</b> GSM 1900 : 1.574 W/kg 802.11b : 0.510 W/kg
Antenna Type & Gain	WWAN Antenna Type : PiFA WLAN Antenna Type : PCB Antenna 824 MHz : -4.19 dBi / 849 MHz : -3.10 dBi 1 850 MHz : 2.57 dBi / 1 880 MHz : 2.64 dBi / 1 910 MHz : 1.73 dBi 2 410 MHz : -1.90 dBi / 2 440 MHz : -1.04 dBi / 2 460 MHz : -1.13 dBi
Antenna Operation	1 Antenna Transmit
USED AC/DC ADAPTER	DC 7.4 V

## 2. INTRODUCTION

The FCC and Industry Canada have adopted the guidelines for evaluating the environmental effects of radio frequency (RF) radiation in ET Docket 93-62 on Aug. 6, 1996 and Health Canada Safety Code 6 to protect the public and workers from the potential hazards of RF emissions due to FCC-regulated portable devices.

The safety limits used for the environmental evaluation measurements are based on the criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate (SAR) in IEEE/ANSI C95.1-1992 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz and Health Canada RF Exposure Guidelines Safety Code 6. The measurement procedure described in IEEE/ANSI C95.3-2002 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields - RF and Microwave is used for guidance in measuring the Specific Absorption Rate (SAR) due to the RF radiation exposure from the Equipment Under Test (EUT). These criteria for SAR evaluation are similar to those recommended by the International Committee for Non-Ionizing Radiation Protection (ICNIRP) in Biological Effects and Exposure Criteria for Radiofrequency Electromagnetic Fields," Report No. Vol 74. SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards.

### 2.1 SAR Definition

Specific Absorption Rate is defined as the time derivative (rate) of the incremental energy (dU) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dV) of a given density ( $\rho$ ).

$$SAR = \frac{d}{dt} \left( \frac{dW}{dm} \right) = \frac{d}{dt} \left( \frac{dW}{\rho dV} \right)$$

SAR is expressed in units of watts per kilogram (W/kg). SAR can be related to the electric field at a point by


$$SAR = \frac{\sigma |E|^2}{\rho}$$

where:


- $\sigma$  = conductivity of the tissue (S/m)
- $\rho$  = mass density of the tissue (kg/m<sup>3</sup>)
- E = rms electric field strength (V/m)

### 3. SAR MEASUREMENT SETUP


- A standard high precision 6-axis robot with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- An isotropic Field probe optimized and calibrated for the targeted measurement.
- Data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing,
- AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- A computer running WinXP or Win7 and the DASY5 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.

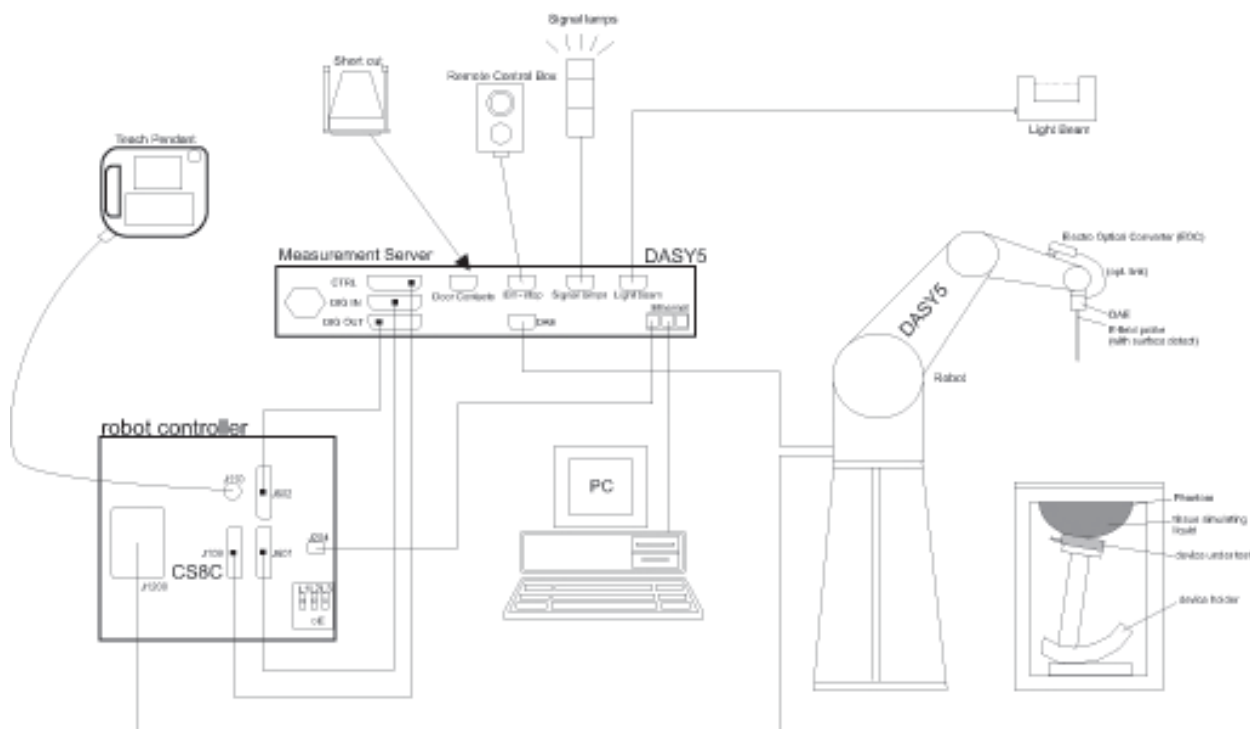


### 3.1 Dasy 5 system

DASY52 SAR	
	<p>DASY52 SAR is a cost-effective package for demonstration of compliance of mobile phones with specific absorption rate (SAR) limits. The fastest and most accurate scanner on the market, it is fully compatible with all worldwide standards for transmitters operating at the ear or near the body (&lt;200 mm from the skin).</p>
<p><b>Components</b> (typical configuration)</p>	<ul style="list-style-type: none"> <li>1 <b>TX90XL</b> Stäubli Robot and Controller CS8c incl. Cabinet</li> <li>1 <b>EOCx</b> Electro Optical Converter (mounted on robot arm)</li> <li>1 Robot Stand for TX90XL</li> <li>1 Robot Arm Extension and Adaptors</li> <li>1 Robot Remote Control</li> <li>1 <b>LB5</b> Light Beam Switch for Probe Tooling (incl. LB Adaptor)</li> <li>1 Light Beam Mounting Plate</li> <li>1 DASY5 Measurement Server</li> <li>1 PC Intel Core 2 Dual / 3.16 GHz (or higher) incl. Color-Monitor 23" - 4 GB RAM, 220 GB HD (or larger) / Win7</li> <li>1 <b>SAM Twin</b> Phantom V5.0 incl. Support DASY5</li> <li>1 <b>MD4HHTV5</b> Mounting Device for Hand-Held Transmitters</li> <li>1 <b>DAEx</b> Data Acquisition Electronics</li> <li>1 <b>ES3DVx</b> SAR Probe (incl. ConvF for HSL at 900 and 1750 MHz)</li> </ul>


### 3.2 E-Field Probe (EX3DV4)

EX3DV4 Smallest Isotropic E-Field Probe for Dosimetric Measurements (Preliminary Specifications)	
	<p>Symmetrical design with triangular core Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., DGBE)</p>
<b>Calibration</b>	ISO/IEC 17025 <a href="#">calibration service</a> available.
<b>Frequency</b>	10 MHz to > 6 GHz Linearity: ± 0.2 dB (30 MHz to 6 GHz)
<b>Directivity</b>	± 0.3 dB in TSL (rotation around probe axis) ± 0.5 dB in TSL (rotation normal to probe axis)
<b>Dynamic Range</b>	10 µW/g to > 100 mW/g Linearity: ± 0.2 dB (noise: typically < 1 µW/g)
<b>Dimensions</b>	Overall length: 337 mm (Tip: 20 mm) Tip diameter: 2.5 mm (Body: 12 mm) Typical distance from probe tip to dipole centers: 1 mm
<b>Application</b>	High precision dosimetric measurements in any exposure scenario (e.g., very strong gradient fields); the only probe that enables compliance testing for frequencies up to 6 GHz with precision of better 30%.

### 3.3 E-Field Probe(ES3DV3)

<b>ES3DV3</b> <b>Isotropic E-Field Probe for Dosimetric Measurements</b>	
	Symmetrical design with triangular core Interleaved sensors Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., DGBE)
<b>Calibration</b>	ISO/IEC 17025 <a href="#">calibration service</a> available.
<b>Frequency</b>	10 MHz to 4 GHz; Linearity: $\pm 0.2$ dB (30 MHz to 4 GHz)
<b>Directivity</b>	$\pm 0.2$ dB in TSL (rotation around probe axis) $\pm 0.3$ dB in TSL (rotation normal to probe axis)
<b>Dynamic Range</b>	5 $\mu$ W/g to > 100 mW/g; Linearity: $\pm 0.2$ dB
<b>Dimensions</b>	Overall length: 337 mm (Tip: 20 mm) Tip diameter: 3.9 mm (Body: 12 mm) Distance from probe tip to dipole centers: 2.0 mm
<b>Application</b>	General dosimetry up to 4 GHz Dosimetry in strong gradient fields Compliance tests of mobile phones
<b>Compatibility</b>	DASY3, DASY4, DASY52 SAR and higher, EASY4/MRI

### 3.4 ELI Phantom

<b>ELI</b>	
	Phantom for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30 MHz to 6 GHz. ELI is fully compatible with the IEC 62209-2 standard and all known tissue simulating liquids. ELI has been optimized regarding its performance and can be integrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points. The phantom is compatible with all SPEAG dosimetric probes and dipoles.  ELI V5.0 has the same shell geometry and is manufactured from the same material as ELI4, but has reinforced top structure.
<b>Material</b>	Vinylester, glass fiber reinforced (VE-GF)
<b>Liquid Compatibility</b>	Compatible with all SPEAG tissue simulating liquids (incl. DGBE type)
<b>Shell Thickness</b>	2.0 $\pm$ 0.2 mm (bottom plate)
<b>Dimensions</b>	Major axis: 600 mm Minor axis: 400 mm
<b>Filling Volume</b>	approx. 30 liters
<b>Wooden Support</b>	SPEAG standard phantom table

### 3.5 Twin SAM Phantom

Twin SAM	
	<p>The shell corresponds to the specifications of the Specific Anthropomorphic Mannequin (SAM) phantom defined in IEEE 1528 and IEC 62209-1. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents evaporation of the liquid. Reference markings on the phantom allow the complete setup of all predefined phantom positions and measurement grids by teaching three points with the robot.</p> <p>Twin SAM V5.0 has the same shell geometry and is manufactured from the same material as Twin SAM V4.0, but has reinforced top structure.</p>
<b>Material</b>	Vinylester, glass fiber reinforced (VE-GF)
<b>Liquid Compatibility</b>	Compatible with all SPEAG tissue simulating liquids (incl. DGBE type)
<b>Shell Thickness</b>	2 ± 0.2 mm (6 ± 0.2 mm at ear point)
<b>Dimensions (incl. Wooden Support)</b>	Length: 1000 mm Width: 500 mm Height: adjustable feet
<b>Filling Volume</b>	approx. 25 liters
<b>Wooden Support</b>	SPEAG standard phantom table
<b>Accessories</b>	<a href="#">Mounting Device and Adaptors</a>

### 3.6 Mounting Device

 <p>Mounting Device for Hand-Held Transmitters</p>	<p><b>MD4HHTV5 - Mounting Device for Hand-Held Transmitters</b></p> <p>In combination with the Twin SAM V5.0/V5.0c or ELI Phantoms, the Mounting Device for Hand-Held Transmitters enables rotation of the mounted transmitter device to specified spherical coordinates. At the heads, the rotation axis is at the ear opening. Transmitter devices can be easily and accurately positioned according to IEC 62209-1, IEEE 1528, FCC, or other specifications. The device holder can be locked for positioning at different phantom sections (left head, right head, flat).</p> <p><b>Material:</b> Polyoxymethylene (POM)</p>
---	---



## 4. MEASUREMENT UNCERTAINTY

### Uncertainty of SAR equipment for measurement Body 0.3 GHz to 3 GHz

No.		Error Description	Uncertainty Value (1 g) (%)	Uncertainty Value (10 g) (%)	Probe Dist.	Div.	C <sub>1</sub> (1 g)	C <sub>1</sub> (10 g)	U <sub>i</sub> (g) (1 g)	U <sub>i</sub> (g) (10 g)	V <sub>i</sub> or V <sub>eff</sub>
1	U(PR <sub>cal</sub> )	Probe Calibration	6.30	6.30	N	1.00	1.00	1.00	6.30	6.30	∞
2	U(PR <sub>is</sub> )	Isotropy	1.87	1.87	R	√3	1.00	1.00	1.08	1.08	∞
3	U(L)	Linearity	0.60	0.60	R	√3	1.00	1.00	0.35	0.35	∞
4	U(PR <sub>mr</sub> )	Probe modulation response	2.40	2.40	R	√3	1.00	1.00	1.39	1.39	∞
6	U(DL)	Detection Limits	1.00	1.00	R	√3	1.00	1.00	0.58	0.58	∞
5	U(BE)	Boundary effect	1.00	1.00	R	√3	1.00	1.00	0.58	0.58	∞
7	U(RE)	Readout Electronics	0.30	0.30	N	1.00	1.00	1.00	0.30	0.30	∞
8	U(T <sub>rr</sub> )	Response Time	0.80	0.80	R	√3	1.00	1.00	0.46	0.46	∞
9	U(T <sub>rr</sub> )	Integration Time	2.60	2.60	R	√3	1.00	1.00	1.50	1.50	∞
10	U(A <sub>amb</sub> )	RF ambient conditions–noise	3.00	3.00	R	√3	1.00	1.00	1.73	1.73	∞
11	U(A <sub>amb</sub> )	RF ambient conditions–reflections	3.00	3.00	R	√3	1.00	1.00	1.73	1.73	∞
12	U(PR <sub>rm</sub> )	Probe positioner mech. Restrictions	0.40	0.40	R	√3	1.00	1.00	0.23	0.23	∞
13	U(PR <sub>rp</sub> )	Probe positioning with respect to phantom	2.90	2.90	R	√3	1.00	1.00	1.67	1.67	∞
14	U(PP <sub>pr</sub> )	Post-processing(for max. SAR evaluation)	2.00	2.00	R	√3	1.00	1.00	1.15	1.15	∞
15	U(DL)	Device Holder Uncertainty	3.60	3.60	N	1.00	1.00	1.00	3.60	3.60	5.00
16	U(PO <sub>st</sub> )	Test sample positioning	8.32	6.37	N	1.00	1.00	1.00	8.32	6.37	9.00
17	U(PS)	Power scaling	0.00	0.00	R	√3	1.00	1.00	0.00	0.00	∞
18	U(PD)	Drift of output power(measured SAR drift)	5.00	5.00	R	√3	1.00	1.00	2.89	2.89	∞
19	U(PL)	Phantom Uncertainty	6.10	6.10	R	√3	1.00	1.00	3.52	3.52	∞
20	U(CS <sub>alg</sub> )	Algorithm for correcting SAR for deviations in permittivity and conductivity	1.90	1.90	N	1.00	1.00	0.84	1.90	1.60	∞
21	U(LC <sub>me</sub> )	Liquid Conductivity (meas.)	1.53	1.53	N	1.00	0.78	0.71	1.19	1.09	5.00
22	U(LP <sub>me</sub> )	Liquid Permittivity (meas.)	3.07	3.07	N	1.00	0.23	0.26	0.71	0.80	5.00
23	U(LC <sub>tr</sub> )	Liquid conductivity(temperature uncertainty)	4.16	4.16	R	√3	0.78	0.71	1.87	1.71	∞
24	U(LP <sub>tr</sub> )	Liquid permittivity(temperature uncertainty)	0.84	0.84	R	√3	0.23	0.26	0.11	0.13	∞
		<b>U<sub>c</sub>(sar) Combined standard uncertainty (%)</b>							<b>12.97</b>	<b>11.74</b>	<b>50</b>
		<b>Extended uncertainty U(%)</b>							<b>25.94</b>	<b>23.48</b>	

### Uncertainty of SAR equipment for measurement Body 3 GHz to 6 GHz

No.		Error Description	Uncertainty Value (1 g) (%)	Uncertainty Value (10 g) (%)	Probe Dist.	Div.	C <sub>1</sub> (1 g)	C <sub>1</sub> (10 g)	U <sub>i</sub> (g) (1 g)	U <sub>i</sub> (g) (10 g)	V <sub>i</sub> or V <sub>eff</sub>
1	U(PR <sub>c</sub> )	Probe Calibration	6.30	6.30	N	1.00	1.00	1.00	6.30	6.30	∞
2	U(PR <sub>i</sub> )	Isotropy	1.87	1.87	R	√3	1.00	1.00	1.08	1.08	∞
3	U(L)	Linearity	0.60	0.60	R	√3	1.00	1.00	0.35	0.35	∞
4	U(PR <sub>mr</sub> )	Probe modulation response	2.40	2.40	R	√3	1.00	1.00	1.39	1.39	∞
6	U(DL)	Detection Limits	1.00	1.00	R	√3	1.00	1.00	0.58	0.58	∞
5	U(BE)	Boundary effect	2.00	2.00	R	√3	1.00	1.00	1.15	1.15	∞
7	U(RE)	Readout Electronics	0.30	0.30	N	1.00	1.00	1.00	0.30	0.30	∞
8	U(T <sub>rr</sub> )	Response Time	0.80	0.80	R	√3	1.00	1.00	0.46	0.46	∞
9	U(T <sub>rr</sub> )	Integration Time	2.60	2.60	R	√3	1.00	1.00	1.50	1.50	∞
10	U(A <sub>amb</sub> )	RF ambient conditions–noise	3.00	3.00	R	√3	1.00	1.00	1.73	1.73	∞
11	U(A <sub>amb</sub> )	RF ambient conditions–reflections	3.00	3.00	R	√3	1.00	1.00	1.73	1.73	∞
12	U(PR <sub>rr</sub> )	Probe positioner mech. Restrictions	0.80	0.80	R	√3	1.00	1.00	0.46	0.46	∞
13	U(PR <sub>rr</sub> )	Probe positioning with respect to phantom	6.70	6.70	R	√3	1.00	1.00	3.87	3.87	∞
14	U(PP <sub>max</sub> )	Post-processing(for max. SAR evaluation)	4.00	4.00	R	√3	1.00	1.00	2.31	2.31	∞
15	U(DU)	Device Holder Uncertainty	3.60	3.60	N	1.00	1.00	1.00	3.60	3.60	5.00
16	U(PO <sub>err</sub> )	Test sample positioning	7.76	6.03	N	1.00	1.00	1.00	7.76	6.03	9.00
17	U(PS)	Power scaling	0.00	0.00	R	√3	1.00	1.00	0.00	0.00	∞
18	U(PD)	Drift of output power(measured SAR drift)	5.00	5.00	R	√3	1.00	1.00	2.89	2.89	∞
19	U(PL)	Phantom Uncertainty	6.60	6.60	R	√3	1.00	1.00	3.81	3.81	∞
20	U(CS <sub>avg</sub> )	Algorithm for correcting SAR for deviations in permittivity and conductivity	1.90	1.90	N	1.00	1.00	0.84	1.90	1.60	∞
21	U(EC <sub>sp</sub> )	Liquid Conductivity (meas.)	1.50	1.50	N	1.00	0.78	0.71	1.17	1.07	5.00
22	U(LP <sub>sp</sub> )	Liquid Permittivity (meas.)	2.23	2.23	N	1.00	0.23	0.26	0.51	0.58	5.00
23	U(EC <sub>temp</sub> )	Liquid conductivity(temperature uncertainty)	2.12	2.12	R	√3	0.78	0.71	0.95	0.87	∞
24	U(LP <sub>temp</sub> )	Liquid permittivity(temperature uncertainty)	0.40	0.40	R	√3	0.23	0.26	0.05	0.06	∞
		<b>U<sub>c</sub>(sar) Combined standard uncertainty (%)</b>							<b>13.26</b>	<b>12.27</b>	<b>71</b>
		<b>Extended uncertainty U(%)</b>							<b>26.52</b>	<b>24.54</b>	

## 5. ANSI/IEEE C95.1-2005 RF EXPOSURE LIMIT

In order for users to be aware of the body-worn operating requirements for meeting RF exposure compliance, operating instructions and cautions statements are included in the user's manual.

### 5.1 Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

### 5.2 Controlled Environment

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

**Human Exposure Limits**

	UNCONTROLLED ENVIRONMENT General Population (W/kg) or (mW/g)	CONTROLLED ENVIROMENT Professional Population (W/kg) or (mW/g)
SPATIAL PEAK SAR <sup>1</sup> Brain	1.60	8.00
SPATIAL AVERAGE SAR <sup>2</sup> Whole Body	0.08	0.40
SPATIAL PEAK SAR <sup>3</sup> Hands, Feet, Ankles, Wrists	4.00	20.00


<sup>1</sup> The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

<sup>2</sup> The Spatial Average value of the SAR averaged over the whole body.

<sup>3</sup> The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

## 6. SYSTEM AND LIQUID VERIFICATION

### 6.1 System Verification setup

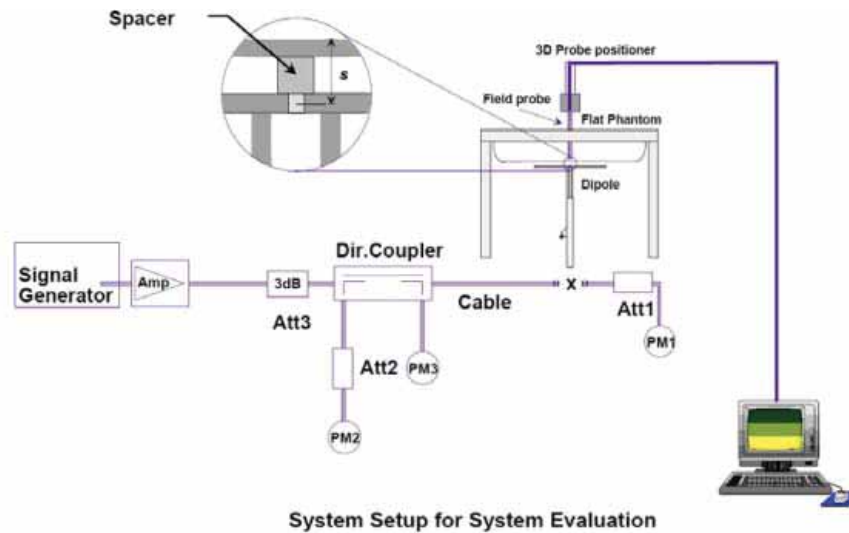

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave that comes from a signal generator. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

1. Signal Generator
2. Amplifier
3. Directional Coupler
4. Power Meter
5. Calibrated Dipole

The output power on dipole port must be calibrated to 30 dBm (1000 mW) before dipole is connected.

**Numerical reference SAR values (W/kg) for reference dipole and flat phantom**

1	2	3	4	5	6
Frequency MHz	Phantom shell thickness mm	1 g SAR W/kg	10 g SAR W/kg	Local SAR at surface (above feedpoint) W/kg	Local SAR at surface (y = 2 cm offset from feedpoint) W/kg
300	6.3	3.02	2.04	4.40	2.10
300	2.0	2.85	1.94	4.14	2.00
450	6.3	4.92	3.28	7.20	3.20
450	2.0	4.58	3.05	6.75	2.98
750	2.0	8.49	5.55	12.6	4.59
835	2.0	9.56	6.22	14.1	4.90
900	2.0	10.9	6.99	16.4	5.40
1 450	2.0	29.0	16.0	50.2	6.50
1 800	2.0	36.4	20.1	69.5	6.80
1 900	2.0	39.7	20.5	72.1	6.60
1 950	2.0	40.5	20.9	72.7	6.60
2 000	2.0	41.1	21.1	74.6	6.50
2 450	2.0	52.4	24.0	104	7.70
2 585	2.0	55.9	24.4	119	7.90
2 600	2.0	55.3	24.6	113	8.29
3 000	2.0	63.8	25.7	140	9.50
3 500	2.0	67.1	25.0	169	12.1
3 700	2.0	67.4	24.2	178	12.7
5 000	2.0	77.9	22.1	305	15.1
5 200	2.0	76.5	21.6	310	15.9
5 500	2.0	83.3	23.4	349	18.1
5 800	2.0	78.0	21.9	341	20.3

### 6.2 Liquid Validation

The dielectric parameters were checked prior to assessment using the DAK dielectric probe kit. The dielectric parameters measured are reported in each correspondent section.

### 6.3 Recommended Tissue Dielectric Parameters

The head and body tissue dielectric parameters recommended by KDB865664 have been incorporated in the following table.

Target Frequency (MHz)	Head		Body	
	$\epsilon_r$	$\sigma$ (S/m)	$\epsilon_r$	$\sigma$ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800 – 2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00

( $\epsilon_r$  = relative permittivity,  $\sigma$  = conductivity and  $\rho = 1000 \text{ kg/m}^3$ )

## 6.4 Liquid Confirmation Results

### 6.4.1 System Verification

Frequency (MHz)	Tissue Type	Liquid Temp.(°C)	Parameter	Target Value	Measured Value	Deviation	Limit (%)	Date
835	Body	21.9	Permittivity	55.20	54.40	-1.45%	± 5	08/17/2015
			Conductivity	0.97	0.96	-1.19%	± 5	
1 950	Body	21.7	Permittivity	53.32	54.75	2.68%	± 5	08/18/2015
			Conductivity	1.51	1.58	4.54%	± 5	
2 450	Body	21.4	Permittivity	52.70	53.45	1.43%	± 5	08/28/2015
			Conductivity	1.95	1.95	-0.25%	± 5	

## 6.5 System Verification Results

Freq. (MHz)	Tissue Type	Amb. Temp (°C)	Liquid Temp (°C)	Input Power (mW)	Dipole S/N	Probe S/N	Measured SAR 10g	1W Normalized SAR 10g	1W Target SAR 10g	Deviation	Date
835	Body	22.3	21.9	250	4d172	3171	1.56	6.24	6.30	-0.95%	08/17/2015
1 950	Body	22.0	21.7	250	1156	3171	5.26	21.0	20.6	2.14%	08/18/2015
2 450	Body	21.7	21.4	250	923	3716	6.02	24.1	23.7	1.60%	08/28/2015

## 7. SAR MEASUREMENT PROCEDURES

### Step 1: Power Reference Measurement

The Power Reference Measurement and Power Drift Measurements are for monitoring the power drift of the device under test in the batch process. The Minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. The minimum distance of probe sensors to surface is 2 mm. This distance cannot be smaller than the Distance of sensor calibration points to probe tip as defined in the probe properties.

### Step 2: Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values, before doing a fine measurement around the hot spot. The sophisticated interpolation routines implemented in DASYS software can find the maximum locations even in relatively coarse grids. When an Area Scan has measured all reachable points, it computes the field maximal found in the scanned area, within a range of the global maximum. The range (in dB) is specified in the standards for compliance testing.

For example, a 2 dB range is required in IEEE Standard 1528 and IEC 62209 standards, whereby 3 dB is a requirement when compliance is assessed in accordance with the ARIB standard (Japan). If only one Zoom Scan follows the Area Scan, then only the absolute maximum will be taken as reference. For cases where multiple maximums are detected, the number of Zoom Scans has to be increased accordingly.

### Step 3: Zoom Scan

Zoom Scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The Zoom Scan measures 5x5x7 points within a cube whose base faces are centered on the maxima found in a preceding area scan job within the same procedure. When the measurement is done, the Zoom Scan evaluates the averaged SAR for 1 g and 10 g and displays these values next to the job's label.

### Step 4: Power drift measurement

The Power Drift Measurement measures the field at the same location as the most recent power reference measurement within the same procedure, and with the same settings. The Power Drift Measurement gives the field difference in dB from the reading conducted within the last Power Reference Measurement. This allows a user to monitor the power drift of the device under test within a batch process. The measurement procedure is the same as Step 1.



### Step 5: Z-Scan

The Z Scan measures points along a vertical straight line. The line runs along the Z-axis of a one dimensional grid. In order to get a reasonable extrapolation, the extrapolated distance should not be larger than the step size in Z-direction.

\* Z Scan Report on Liquid Measure the height ANNEX C. Liquid Depth photo to replace

		$\leq 3$ GHz	$> 3$ GHz
Maximum distance from closest measurement point (geometric center of probe sensors) to phantom surface		$5 \pm 1$ mm	$\frac{1}{2} \cdot \delta \cdot \ln(2) \pm 0.5$ mm
Maximum probe angle from probe axis to phantom surface normal at the measurement location		$30^\circ \pm 1^\circ$	$20^\circ \pm 1^\circ$
Maximum area scan spatial resolution: $\Delta x_{Area}, \Delta y_{Area}$		$\leq 2$ GHz: $\leq 15$ mm 2 – 3 GHz: $\leq 12$ mm	3 – 4 GHz: $\leq 12$ mm 4 – 6 GHz: $\leq 10$ mm
		When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be $\leq$ the corresponding x or y dimension of the test device with at least one measurement point on the test device.	
Maximum zoom scan spatial resolution: $\Delta x_{Zoom}, \Delta y_{Zoom}$		$\leq 2$ GHz: $\leq 8$ mm 2 – 3 GHz: $\leq 5$ mm*	3 – 4 GHz: $\leq 5$ mm* 4 – 6 GHz: $\leq 4$ mm*
Maximum zoom scan spatial resolution, normal to phantom surface	uniform grid: $\Delta z_{Zoom}(n)$	$\leq 5$ mm	3 – 4 GHz: $\leq 4$ mm 4 – 5 GHz: $\leq 3$ mm 5 – 6 GHz: $\leq 2$ mm
	graded grid	$\Delta z_{Zoom}(1)$ : between 1 <sup>st</sup> two points closest to phantom surface	$\leq 4$ mm
		$\Delta z_{Zoom}(n>1)$ : between subsequent points	$\leq 1.5 \cdot \Delta z_{Zoom}(n-1)$
Minimum zoom scan volume	x, y, z	$\geq 30$ mm	3 – 4 GHz: $\geq 28$ mm 4 – 5 GHz: $\geq 25$ mm 5 – 6 GHz: $\geq 22$ mm
<p>Note: <math>\delta</math> is the penetration depth of a plane-wave at normal incidence to the tissue medium; see draft standard IEEE P1528-2011 for details.</p> <p>* When zoom scan is required and the <i>reported</i> SAR from the area scan based <i>1-g SAR estimation</i> procedures of KDB 447498 is <math>\leq 1.4</math> W/kg, <math>\leq 8</math> mm, <math>\leq 7</math> mm and <math>\leq 5</math> mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.</p>			

## 8. TEST EQUIPMENT LIST

Manufacturer	Model	Serial No.	CaL.Due	Used
STAUBLI	RX90XL	F07/56X0A1/A/01	N/A	V
STAUBLI	CS8C Speag TX90XL	F07/56X0A1/C/01	N/A	V
SPEAG	SE UMS 011 AA	1019	N/A	V
STAUBLI	RX90BL	F01/5J92A1/A/01	N/A	
STAUBLI	CS7MBsp RX90BL	F01/5J92A1/C/01	N/A	
SPEAG	SE UMS 001 BC	1164	N/A	
STAUBLI	SP1	D 211 421 02	N/A	V
STAUBLI	Manual Control III Operator	D 221 340 01	N/A	V
Di-Soric	LB5	80	N/A	
Di-Soric	LB2	270	N/A	
SPEAG	Twin Phantom	TP-1069	N/A	V
SPEAG	Twin Phantom	TP-1086	N/A	
SPEAG	Twin Phantom	TP-1112	N/A	
SPEAG	Twin Phantom	TP-1155	N/A	
SPEAG	ELI4 Phantom	S 000 T01 DA	N/A	V
SPEAG	Triple Phantom	QD 000 P51 CA	N/A	
SPEAG	Mounting Device	N/A	N/A	
SPEAG	Mounting Device	SM LH1 001 AC	N/A	V
Agilent	85033E	N/A	N/A	V
SPEAG	DAE4	444	11/11/2015	V
SPEAG	DAE3	383	03/18/2015	
SPEAG	EX3DV4	3666	05/25/2016	
SPEAG	ES3DV3	3171	07/20/2016	V
SPEAG	EX3DV4	3716	11/17/2015	V
SPEAG	D2450V2	923	11/12/2015	V
SPEAG	D5GHzV2	1094	12/15/2015	
SPEAG	D835V2	4d172	07/08/2016	V
SPEAG	D1750V2	1122	07/08/2016	
SPEAG	D1950V3	1156	07/08/2016	V
SPEAG	DAK-3.5	1140	11/10/2015	V
HP	8665B	3744A01333	10/09/2015	V
EMPOWER	BBS3Q7ELU-2001	1009D/C0105	10/09/2015	V
VARIAN	VZC6961K11212	6673	10/09/2015	
HP	778D	12679	10/07/2015	V
Agilent	772D	2839A01119	10/07/2015	V
Agilent	E4419B	MY41291366	10/07/2015	V
HP	437B	3125U25121	04/28/2016	V
HP	8481H	3318A18722	10/12/2015	V
HP	8481H	3318A17600	10/12/2015	V
HP	8481A	1550A14928	10/12/2015	
WAAINWRIGHT	WLJS1500-6EF	1	10/07/2015	
WAAINWRIGHT	WLJS3000-6EF	1	10/07/2015	
WAAINWRIGHT	WLJS6000-7EF	1	10/12/2015	V
Agilent	E8357A	US41070399	10/09/2015	V

EMC-003 (Rev.2)

Rohde-Schwarz	FSP	100017	10/08/2015	V
LKM Electronic Gmbh	DTM3000-spezial	3247	10/10/2015	V
CAS	TE-201	14011777-2	10/09/2015	V
CAS	TE-201	14011777-1	10/10/2015	
Bird	50-6A-MFN-30	14100882-1	10/12/2015	
Bird	50-6A-MFN-30	14100882-2	10/12/2015	V
ANRITSU	MT8820A	6200270787	08/20/2015	
Agilent	E5515C	GB41450265	03/09/2016	V
Agilent	E5515C	GB44350208	03/09/2016	

## 9. RF CONDUCTED POWER

### 9.1 GSM Conducted output power (Burst-Average)

Mode	Freq. (MHz)	CH	GPRS Conducted Power (dBm)				Tolerance (dBm)
			1TX	2TX	3TX	4TX	
GSM 850	824.2	128	32.28	30.75	28.36	27.93	33.0 -1/+0.5
	836.6	190	32.42	30.97	29.51	28.21	33.0 -1/+0.5
	848.8	251	<b>33.01</b>	31.32	29.97	28.46	33.0 -1/+0.5
GSM 1900	824.2	128	29.82	28.44	27.12	25.73	30.0 -1/+0.5
	836.6	190	<b>29.85</b>	28.51	27.25	25.88	30.0 -1/+0.5
	848.8	251	29.77	28.31	27.03	25.57	30.0 -1/+0.5

Mode	Freq. (MHz)	CH	EGPRS Conducted Power (dBm)				Tolerance (dBm)
			1TX	2TX	3TX	4TX	
GSM 850	824.2	128	32.22	30.58	28.19	27.88	33.0 -1/+0.5
	836.6	190	32.37	30.63	29.45	28.03	33.0 -1/+0.5
	848.8	251	32.96	31.02	29.65	28.32	33.0 -1/+0.5
GSM 1900	824.2	128	29.77	28.36	26.96	25.55	30.0 -1/+0.5
	836.6	190	29.81	28.42	27.05	25.71	30.0 -1/+0.5
	848.8	251	29.73	28.29	26.88	25.43	30.0 -1/+0.5

### 9.2 GSM Conducted output power (Frame-Average)

Mode	Freq. (MHz)	CH	GPRS Conducted Power (dBm)			
			1TX	2TX	3TX	4TX
GSM 850	824.2	128	23.25	24.73	26.49	24.92
	836.6	190	23.39	24.95	26.71	25.20
	848.8	251	23.98	25.3	27.06	25.45
GSM 1900	824.2	128	20.79	22.42	24.18	22.72
	836.6	190	20.82	22.49	24.25	22.87
	848.8	251	20.74	22.29	24.05	22.56

Mode	Freq. (MHz)	CH	EGPRS Conducted Power (dBm)			
			1TX	2TX	3TX	4TX
GSM 850	824.2	128	23.19	24.56	26.32	24.87
	836.6	190	23.34	24.61	26.37	25.02
	848.8	251	23.93	25	26.76	25.31
GSM 1900	824.2	128	20.74	22.34	24.10	22.54
	836.6	190	20.78	22.4	24.16	22.70
	848.8	251	20.70	22.27	24.03	22.42

### 9.3 802.11b

Mode	Freq. (MHz)	CH	Conducted Power (dBm)				Tolerance (dBm)
			Data Rate (Mbps)				
			1	2	5.5	11	
802.11b	2 412	1	13.59	13.55	13.71	13.49	14.0 ± 2 (Band edge -4)
	2 437	6	13.94	13.85	13.97	13.73	
	2 462	11	14.20	14.17	14.24	14.01	

### 9.4 802.11g

Mode	Freq. (MHz)	CH	Conducted Power (dBm)								Tolerance (dBm)
			Data Rate (Mbps)								
			6	9	12	18	24	36	48	54	
802.11g	2 412	1	8.79	8.72	8.34	8.28	8.01	7.74	7.48	7.40	9.0 ± 2 (Band edge -4)
	2 437	6	8.96	8.87	8.75	8.55	8.38	8.11	7.75	7.52	
	2 462	11	9.32	9.21	9.11	8.70	8.66	8.29	8.03	7.93	

### 9.5 802.11n HT20

Mode	Freq. (MHz)	CH	Conducted Power (dBm)								Tolerance (dBm)
			Data Rate (Mbps)								
			6.5	13	19.5	26	39	52	58.5	65	
802.11n HT20	2 412	1	8.57	8.43	8.27	8.05	7.74	7.30	7.12	7.14	9.0 ± 2 (Band edge -4)
	2 437	6	8.75	8.56	8.36	8.22	7.92	7.49	7.59	7.46	
	2 462	11	9.10	8.89	8.71	8.59	8.23	7.96	7.96	7.88	

Justification for reduced test configurations for WIFI channels per KDB Publication 248227 D01v01r02 and October 2012/April 2013 FCC/TCB Meeting Notes:

- For 2.4 GHz, highest average RF output power channel for the lowest data rate for IEEE 802.11b were selected for SAR evaluation. Other IEEE 802.11 modes (including 802.11g/n) were not investigated since the average output powers over all channels and data rates were not more than 0.25 dB higher than the tested channel in the lowest data rate of IEEE 802.11b mode.
- For 5 GHz, highest average RF output power channel for the lowest data rate for IEEE 802.11a were selected for SAR evaluation. Other IEEE 802.11 modes (including 802.11n 20 MHz and 40 MHz) were not investigated since the average output powers over all channels and data rates were not more than 0.25 dB higher than the tested channel in the lowest data rate of IEEE 802.11a mode.
- When the maximum extrapolated peak SAR of the zoom scan for the maximum output channel is <math><1.6\text{ W/kg}</math> and the reported 1g averaged SAR is <math><0.8\text{ W/kg}</math>, SAR testing on other channels is not required. Otherwise, the other default (or corresponding required) test channels were additionally tested using the lowest data rate.
- The bolded data rate and channel above were tested for SAR.

## 9.6 Bluetooth

### BDR

Mode	Freq. (MHz)	CH	DH1	DH3	DH5	Tolerance (dBm)
BDR (1M)	2402	0	-0.63	2.30	3.14	7.0 ± 1
	2441	39	2.65	5.54	6.38	
	2480	78	3.31	6.23	<b>7.03</b>	

### EDR

Mode	Freq. (MHz)	CH	DH1	DH3	DH5	Tolerance (dBm)
EDR (2M)	2402	0	-3.30	-0.77	-0.09	3.0 ± 1
	2441	39	-0.52	2.00	2.66	
	2480	78	0.10	2.63	<b>3.25</b>	
EDR (3M)	2402	0	-3.30	-0.77	-0.11	
	2441	39	-0.53	1.97	2.62	
	2480	78	-0.10	2.61	<b>3.23</b>	

## 10.SAR TEST RESULTS

### < GSM 850 Body SAR >

Mode	Position	Freq. (MHz)	CH	Conducted Power (dBm)	Max Allowed Power (dBm)	Scaling Factor	Measured 10g SAR (W/kg)	Reported SAR (W/kg)
GPRS	Back	824.2	128	32.28	33.00	1.18	1.290	1.523
		836.6	190	32.42	33.00	1.14	1.450	<b>1.657</b>
		848.8	251	33.01	33.00	1.00	1.590	1.586
	Front	836.6	190	32.42	33.00	1.14	0.608	0.695
	Bottom	836.6	190	32.42	33.00	1.14	1.190	1.360
	Left	836.6	190	32.42	33.00	1.14	0.966	1.104
	Right	836.6	190	32.42	33.00	1.14	1.340	1.531

### < GSM 1900 Body SAR >

Mode	Position	Freq. (MHz)	CH	Conducted Power (dBm)	Max Allowed Power (dBm)	Scaling Factor	Measured 10g SAR (W/kg)	Reported SAR (W/kg)
GPRS	Bottom	1 850.2	512	29.82	30.00	1.04	1.510	<b>1.574</b>
		1 880.0	661	29.85	30.00	1.04	1.510	1.563
		1 909.8	810	29.77	30.00	1.05	1.460	1.539
	Front	1 880.0	661	29.85	30.00	1.04	0.641	0.664
	Back	1 880.0	661	29.85	30.00	1.04	0.739	0.765
	Left	1 880.0	661	29.85	30.00	1.04	1.420	1.470
	Right	1 880.0	661	29.85	30.00	1.04	0.244	0.253

### < 802.11b Body SAR >

Mode	Position	Freq. (MHz)	CH	Conducted Power (dBm)	Max Allowed Power (dBm)	Scaling Factor	Measured 10g SAR (W/kg)	Reported SAR (W/kg)
802.11b	Right	2 412	1	13.71	14.50	1.20	0.311	0.373
		2 437	6	14.02	14.50	1.12	0.422	0.471
		2 462	11	14.28	14.50	1.05	0.485	<b>0.510</b>
	Front	2 437	6	14.02	14.50	1.12	0.012	0.013
	Back	2 437	6	14.02	14.50	1.12	0.013	0.015



## ANNEX A. SYSTEM VERIFICATION PLOTS

< 835 MHz Body / Date : Aug 17, 2015 >

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d172

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.958 \text{ mho/m}$ ;  $\epsilon_r = 54.4$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(5.97, 5.97, 5.97); Calibrated: 2015-07-21

- Sensor-Surface: 3mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn444; Calibrated: 2014-11-12

- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069

- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

835MHz SPC/Area Scan (71x101x1): Measurement grid:  $dx=12\text{mm}$ ,  $dy=12\text{mm}$

Maximum value of SAR = 2.72 mW/g


835MHz SPC/Zoom Scan (7x7x7)/Cube 0: Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 53.4 V/m; Power Drift = -0.012 dB

Peak SAR (extrapolated) = 3.4 W/kg

SAR(1 g) = 2.34 mW/g; SAR(10 g) = 1.56 mW/g

Maximum value of SAR (measured) = 2.74 mW/g

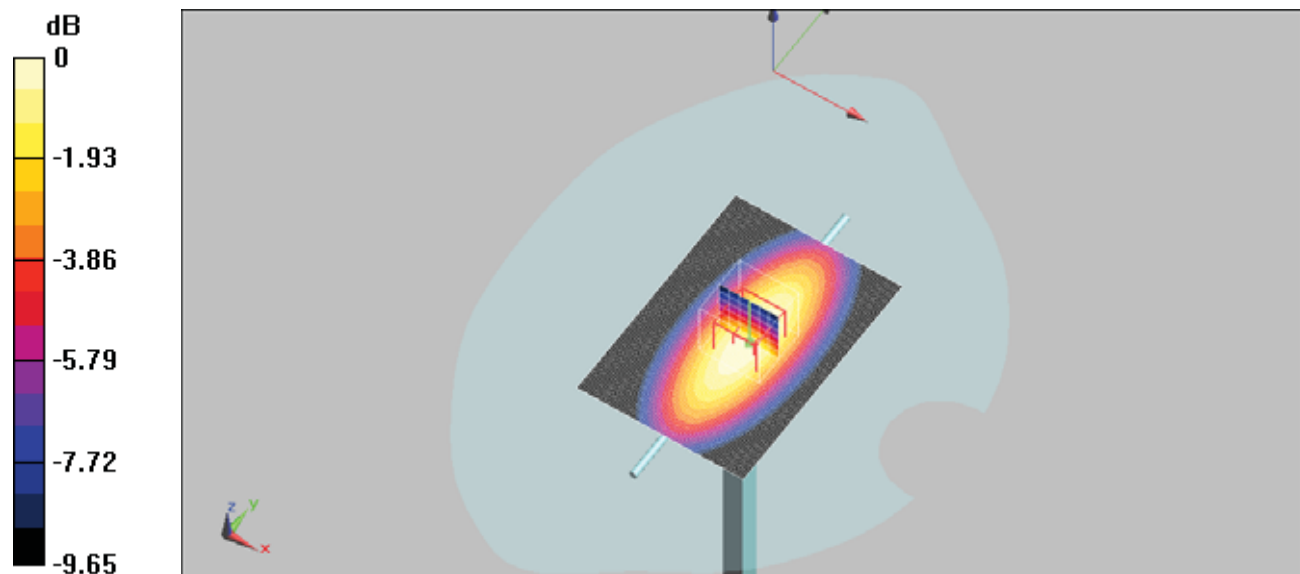

0 dB = 2.74mW/g

< 1 950 MHz Body / Date : Aug 18, 2015 >

DUT: Dipole 1950 MHz; Type: D1950V3; Serial: D1950V3 - SN:1156

Communication System: CW; Frequency: 1950 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 1950$  MHz;  $\sigma = 1.58$  mho/m;  $\epsilon_r = 54.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

**DASY5 Configuration:**

- Probe: ES3DV3 - SN3171; ConvF(4.84, 4.84, 4.84); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

1 950MHz SPC/Area Scan (71x101x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR = 13 mW/g


1 950MHz SPC/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 88.6 V/m; Power Drift = -0.116 dB

Peak SAR (extrapolated) = 17.8 W/kg

SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.26 mW/g

Maximum value of SAR (measured) = 12.7 mW/g

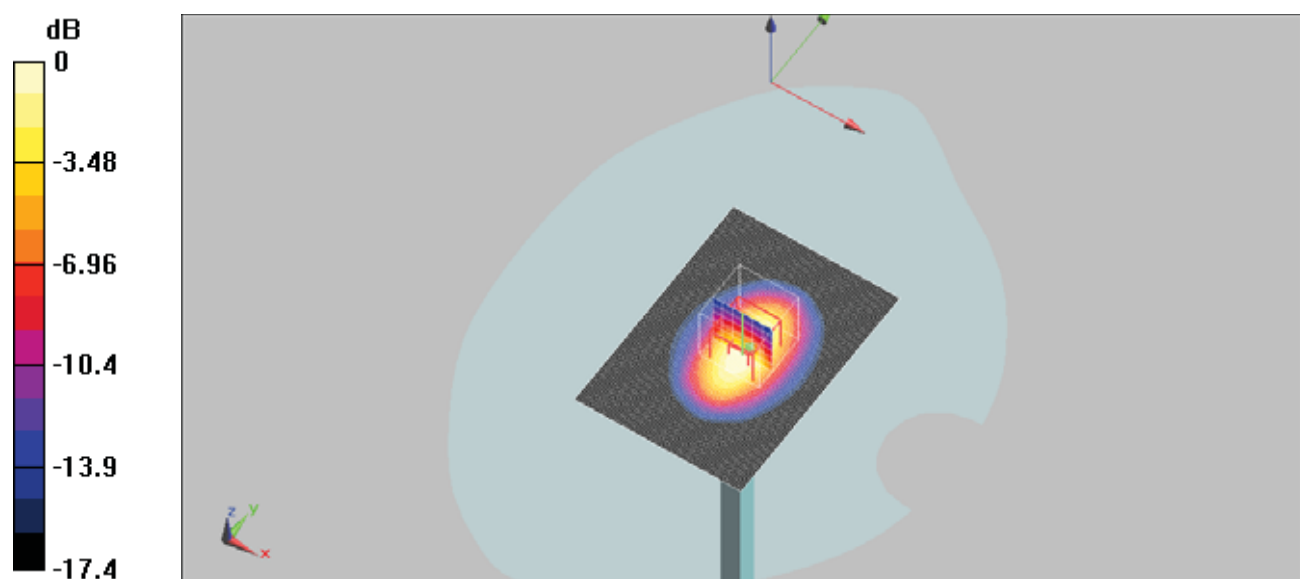

0 dB = 12.7mW/g

< 2 450 MHz Body / Date : Aug 28, 2015 >

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:923

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.95$  mho/m;  $\epsilon_r = 53.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

**DASY5 Configuration:**

- Probe: EX3DV4 - SN3716; ConvF(7.13, 7.13, 7.13); Calibrated: 2014-11-18
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1030
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

2450MHz SPC/Area Scan (71x101x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR = 19.5 mW/g


2450MHz SPC/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 99.6 V/m; Power Drift = 0.117 dB

Peak SAR (extrapolated) = 25.8 W/kg

SAR(1 g) = 12.8 mW/g; SAR(10 g) = 6.02 mW/g

Maximum value of SAR (measured) = 19.4 mW/g

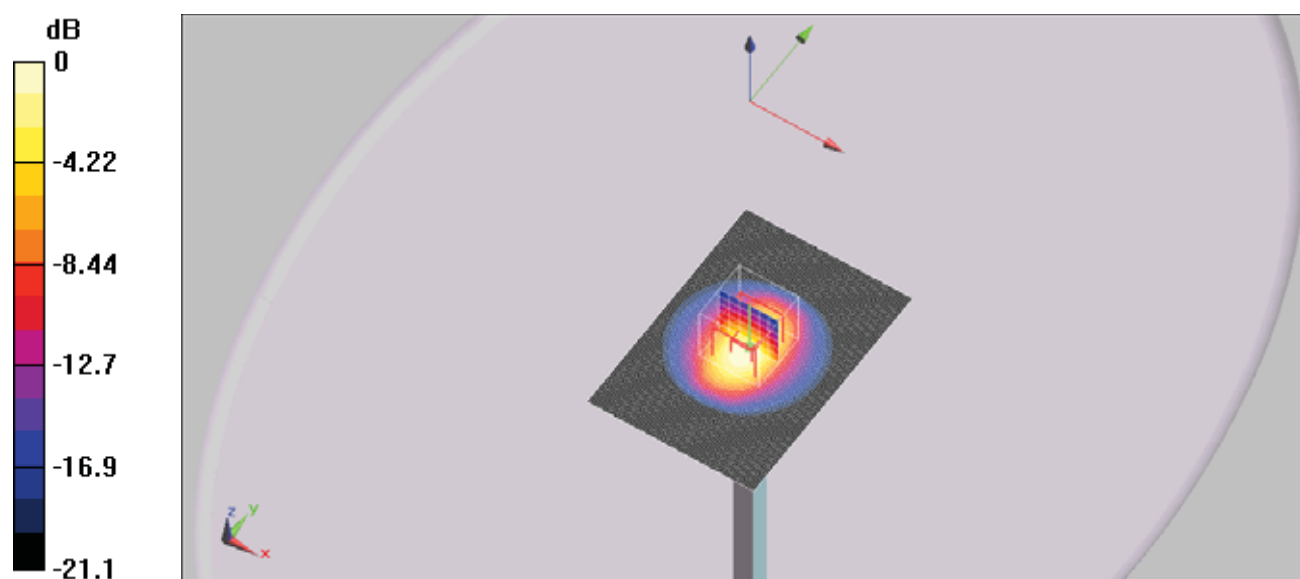

**0 dB = 19.4mW/g**

## ANNEX B. SAR TEST PLOTS

< GMS 850 CH128 824.2 MHz Back Body / Date : Aug 17, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: GSM 850; Frequency: 824.2 MHz; Duty Cycle: 1:8.3

Medium parameters used:  $f = 824.2$  MHz;  $\sigma = 0.947$  mho/m;  $\epsilon_r = 54.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(5.97, 5.97, 5.97); Calibrated: 2015-07-21

- Sensor-Surface: 3mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn444; Calibrated: 2014-11-12

- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069

- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 850\_ch128\_824.2 MHz\_Back/Area Scan (71x81x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR = 4.28 mW/g


GSM 850\_ch128\_824.2 MHz\_Back/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 45.1 V/m; Power Drift = -0.219 dB

Peak SAR (extrapolated) = 8.76 W/kg

SAR(1 g) = 2.98 mW/g; SAR(10 g) = 1.29 mW/g

Maximum value of SAR (measured) = 4 mW/g

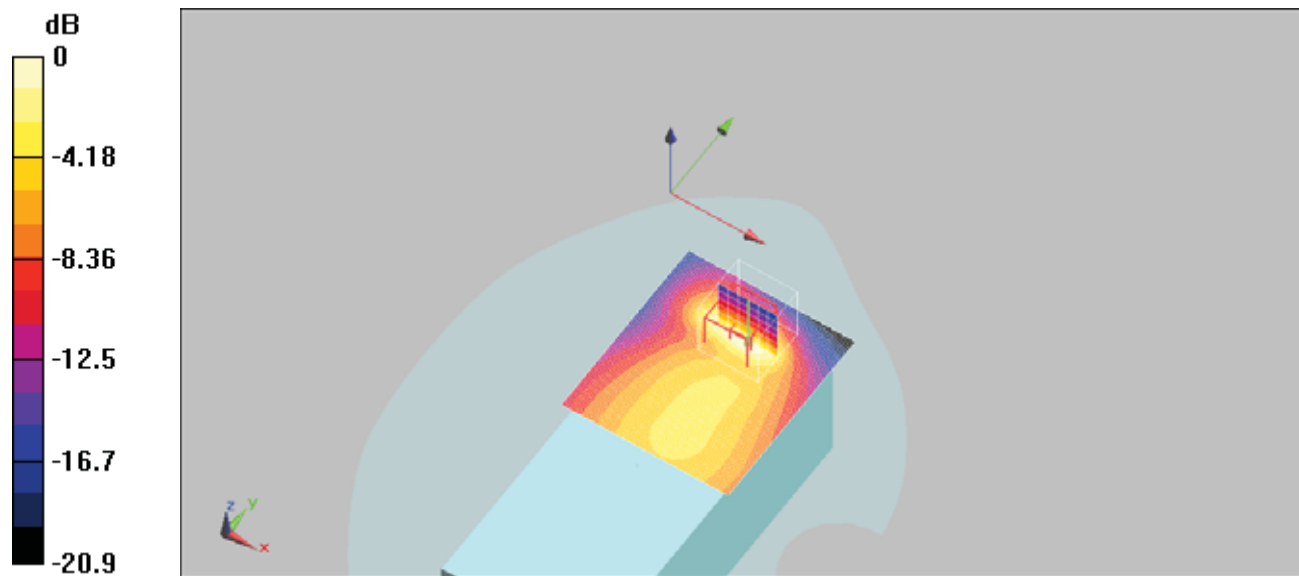

0 dB = 4mW/g

\* note : Found the maximum hot spot from edge SAR because of antenna position of the bottom, so performed partial scan.

< GSM 850 CH190 836.6 MHz Back Body / Date : Aug 17, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: GSM 850; Frequency: 836.6 MHz; Duty Cycle: 1:8.3  
 Medium parameters used :  $f = 836.6 \text{ MHz}$ ;  $\sigma = 0.96 \text{ mho/m}$ ;  $\epsilon_r = 54.4$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(5.97, 5.97, 5.97); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 850\_ch190\_836.6 MHz\_Back/Area Scan (71x81x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR = 4.75 mW/g


GSM 850\_ch190\_836.6 MHz\_Back/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 44.3 V/m; Power Drift = -0.055 dB

Peak SAR (extrapolated) = 9.93 W/kg

SAR(1 g) = 3.39 mW/g; SAR(10 g) = 1.45 mW/g

Maximum value of SAR (measured) = 4.76 mW/g

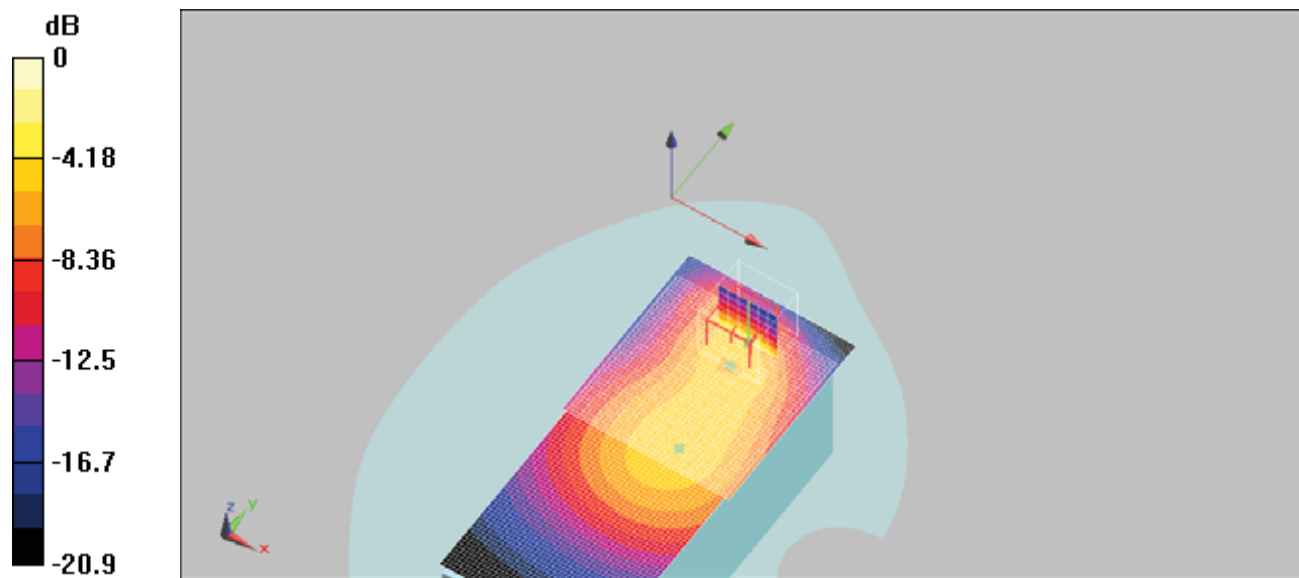

0 dB = 4.76mW/g

< GSM 850 CH251 848.8 MHz Back Body / Date : Aug 17, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: GSM 850; Frequency: 848.8 MHz; Duty Cycle: 1:8.3

Medium parameters used :  $f = 848.8 \text{ MHz}$ ;  $\sigma = 0.975 \text{ mho/m}$ ;  $\epsilon_r = 54.3$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(5.97, 5.97, 5.97); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 850\_ch251\_848.8 MHz\_Back/Area Scan (71x81x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR = 5.06 mW/g


GSM 850\_ch251\_848.8 MHz\_Back/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 45.7 V/m; Power Drift = -0.052 dB

Peak SAR (extrapolated) = 11 W/kg

SAR(1 g) = 3.76 mW/g; SAR(10 g) = 1.59 mW/g

Maximum value of SAR (measured) = 5.29 mW/g

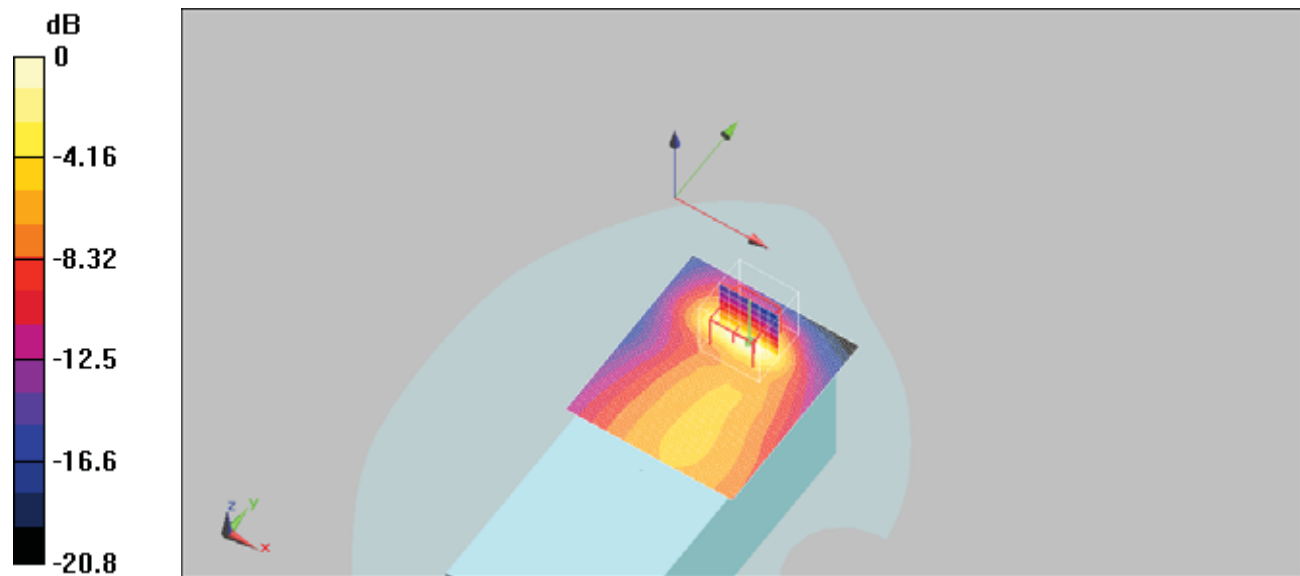

0 dB = 5.29mW/g

\* note : Found the maximum hot spot from edge SAR because of antenna position of the bottom, so performed partial scan.

< GSM 850 CH190 836.6 MHz Front Body / Date : Aug 17, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: GSM 850; Frequency: 836.6 MHz; Duty Cycle: 1:8.3  
 Medium parameters used :  $f = 836.6$  MHz;  $\sigma = 0.96$  mho/m;  $\epsilon_r = 54.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(5.97, 5.97, 5.97); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 850\_ch190\_836.6 MHz\_Front/Area Scan (71x81x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR = 1.11 mW/g


GSM 850\_ch190\_836.6 MHz\_Front/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 34.5 V/m; Power Drift = 0.010 dB

Peak SAR (extrapolated) = 1.56 W/kg

SAR(1 g) = 0.940 mW/g; SAR(10 g) = 0.608 mW/g

Maximum value of SAR (measured) = 1.12 mW/g

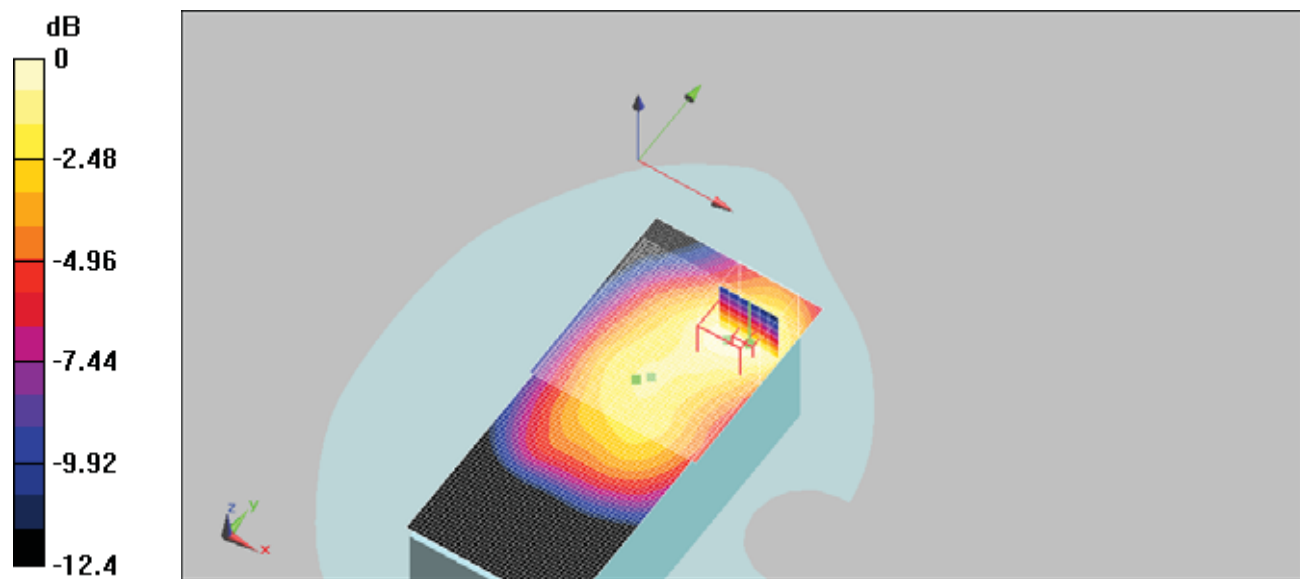

0 dB = 1.12mW/g

< GSM 850 CH190 836.6 MHz Bottom Body / Date : Aug 17, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified


Communication System: GSM 850; Frequency: 836.6 MHz; Duty Cycle: 1:8.3  
 Medium parameters used :  $f = 836.6 \text{ MHz}$ ;  $\sigma = 0.96 \text{ mho/m}$ ;  $\epsilon_r = 54.4$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(5.97, 5.97, 5.97); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 850\_ch190\_836.6 MHz\_Bottom/Area Scan (81x51x1): Measurement grid:  $dx=12\text{mm}$ ,  $dy=12\text{mm}$   
 Maximum value of SAR = 4.6 mW/g

GSM 850\_ch190\_836.6 MHz\_Bottom/Zoom Scan (7x7x7)/Cube 0: Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 63.4 V/m; Power Drift = -0.040 dB  
 Peak SAR (extrapolated) = 17.5 W/kg  
 SAR(1 g) = 3.29 mW/g; SAR(10 g) = 1.19 mW/g  
 Maximum value of SAR (measured) = 4.92 mW/g

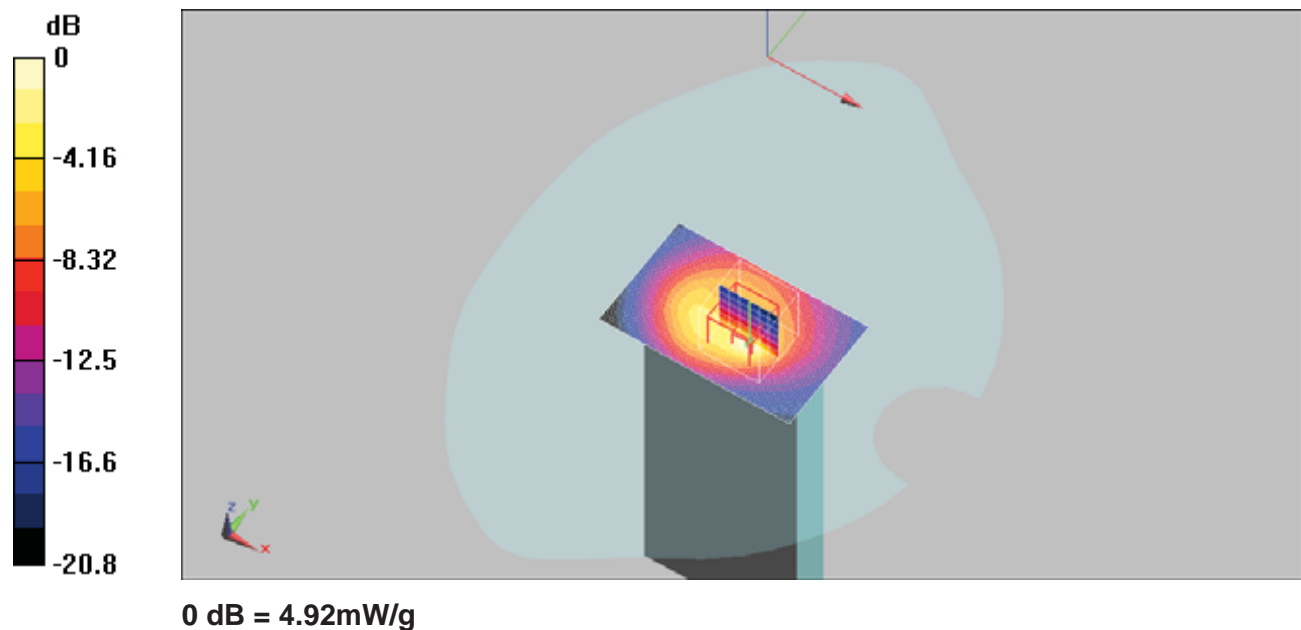



< GSM 850 CH190 836.6 MHz Left Body / Date : Aug 17, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: GSM 850; Frequency: 836.6 MHz; Duty Cycle: 1:8.3  
 Medium parameters used :  $f = 836.6$  MHz;  $\sigma = 0.96$  mho/m;  $\epsilon_r = 54.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(5.97, 5.97, 5.97); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 850\_ch190\_836.6 MHz\_Left/Area Scan (71x151x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR = 1.68 mW/g


GSM 850\_ch190\_836.6 MHz\_Left/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 42.9 V/m; Power Drift = 0.141 dB

Peak SAR (extrapolated) = 2.33 W/kg

SAR(1 g) = 1.5 mW/g; SAR(10 g) = 0.966 mW/g

Maximum value of SAR (measured) = 1.77 mW/g

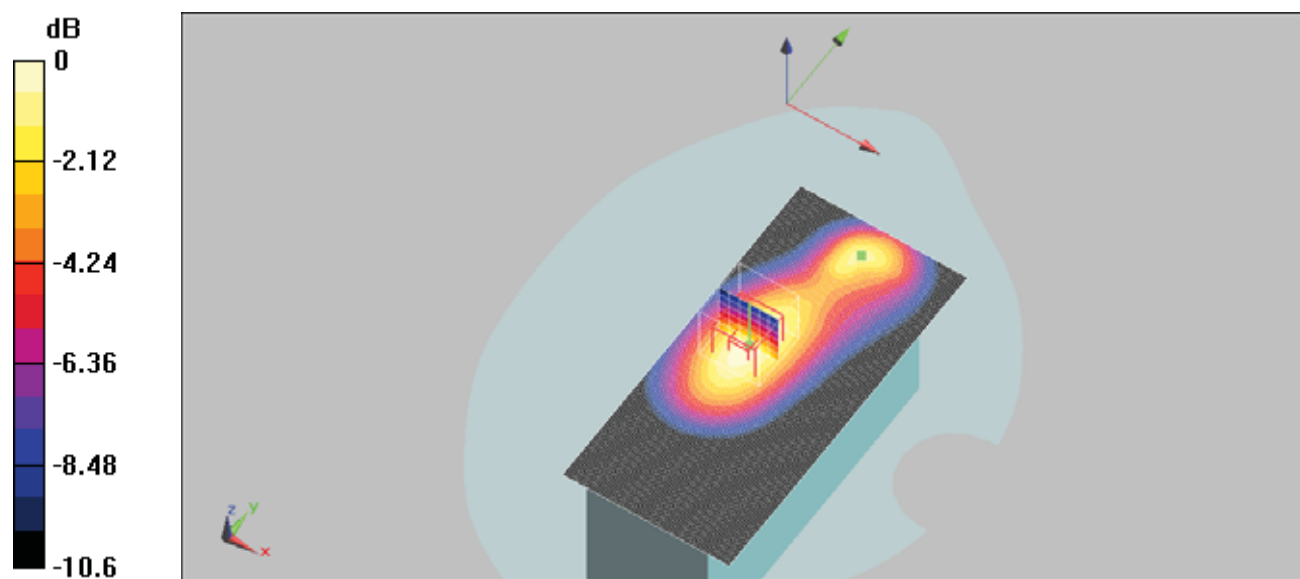

0 dB = 1.77mW/g

**< GSM 850 CH190 836.6 MHz Right Body / Date : Aug 17, 2015 >**

**DUT: MT280; Type: Sample; Serial: Not Specified**

**Communication System: GSM 850; Frequency: 836.6 MHz; Duty Cycle: 1:8.3**  
**Medium parameters used : f = 836.6 MHz;  $\sigma$  = 0.96 mho/m;  $\epsilon_r$  = 54.4;  $\rho$  = 1000 kg/m<sup>3</sup>**  
**Phantom section: Flat Section**

**DASY5 Configuration:**

- Probe: ES3DV3 - SN3171; ConvF(5.97, 5.97, 5.97); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

**GSM 850\_ch190\_836.6 MHz\_Right/Area Scan (71x151x1): Measurement grid: dx=12mm, dy=12mm**

**Maximum value of SAR = 2.27 mW/g**


**GSM 850\_ch190\_836.6 MHz\_Right/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm**

**Reference Value = 48.8 V/m; Power Drift = -0.049 dB**

**Peak SAR (extrapolated) = 2.78 W/kg**

**SAR(1 g) = 1.97 mW/g; SAR(10 g) = 1.34 mW/g**

**Maximum value of SAR (measured) = 2.28 mW/g**

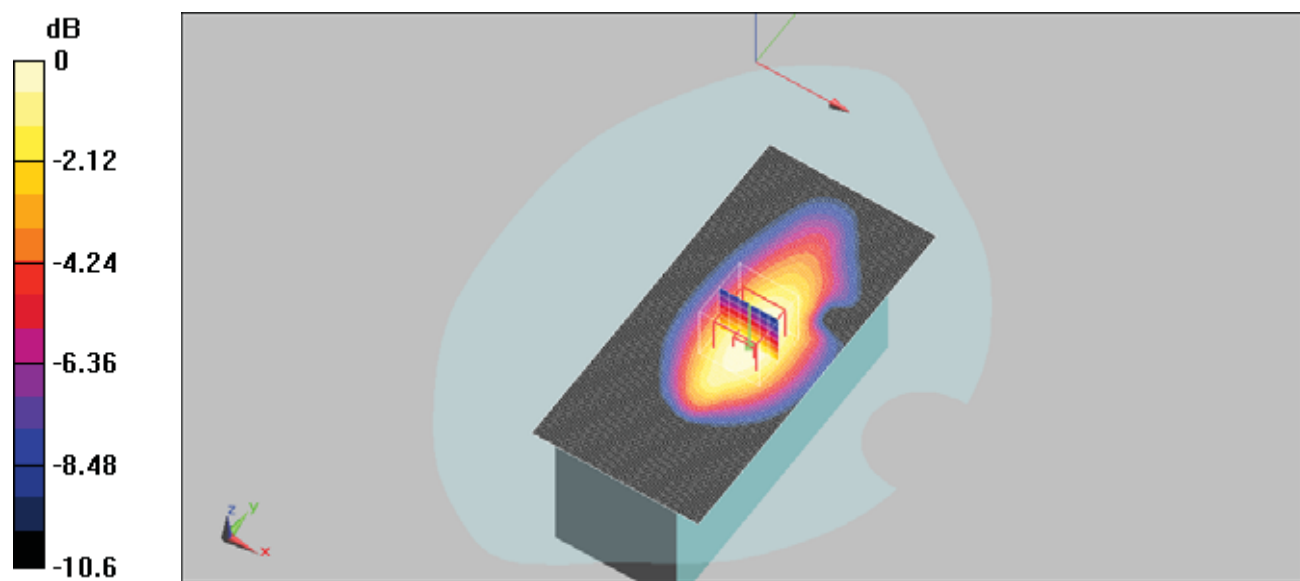

**0 dB = 2.28mW/g**

< GSM 1900 CH512 1 850.2 MHz Bottom Body / Date : Aug 18, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: GSM 1900; Frequency: 1850.2 MHz; Duty Cycle: 1:8.3  
 Medium parameters used :  $f = 1850.2 \text{ MHz}$ ;  $\sigma = 1.46 \text{ mho/m}$ ;  $\epsilon_r = 55.1$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(4.84, 4.84, 4.84); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 1900\_ch512\_1 850.2 MHz\_Bottom/Area Scan (81x51x1): Measurement grid:  $dx=12\text{mm}$ ,  $dy=12\text{mm}$

Maximum value of SAR = 5.16 mW/g


GSM 1900\_ch512\_1 850.2 MHz\_Bottom/Zoom Scan (7x7x7)/Cube 0: Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 52.8 V/m; Power Drift = -0.047 dB

Peak SAR (extrapolated) = 7.88 W/kg

SAR(1 g) = 3.43 mW/g; SAR(10 g) = 1.51 mW/g

Maximum value of SAR (measured) = 4.9 mW/g

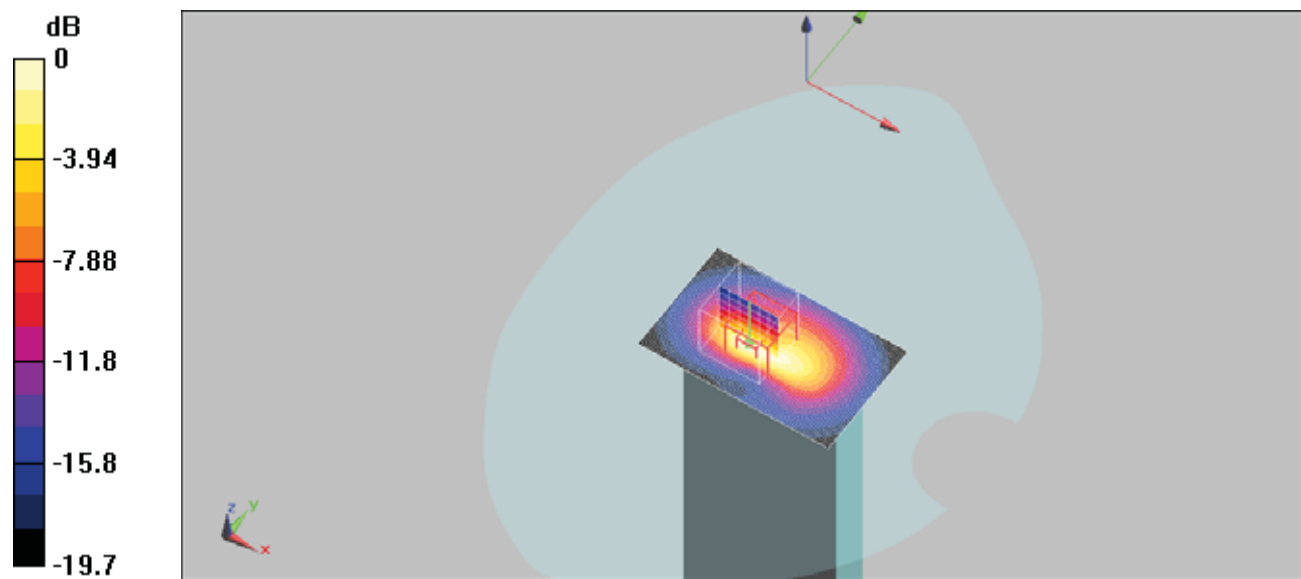

0 dB = 4.9mW/g

< GSM 1900 CH661 1 880.0 MHz Bottom Body / Date : Aug 18, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified


Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3  
 Medium parameters used:  $f = 1880 \text{ MHz}$ ;  $\sigma = 1.5 \text{ mho/m}$ ;  $\epsilon_r = 55$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(4.84, 4.84, 4.84); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 1900\_ch661\_1 880.0 MHz\_Bottom/Area Scan (81x51x1): Measurement grid:  $dx=12\text{mm}$ ,  $dy=12\text{mm}$   
 Maximum value of SAR = 5.23 mW/g

GSM 1900\_ch661\_1 880.0 MHz\_Bottom/Zoom Scan (7x7x7)/Cube 0: Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 54.6 V/m; Power Drift = 0.022 dB  
 Peak SAR (extrapolated) = 8.49 W/kg  
 SAR(1 g) = 3.58 mW/g; SAR(10 g) = 1.51 mW/g  
 Maximum value of SAR (measured) = 5.2 mW/g

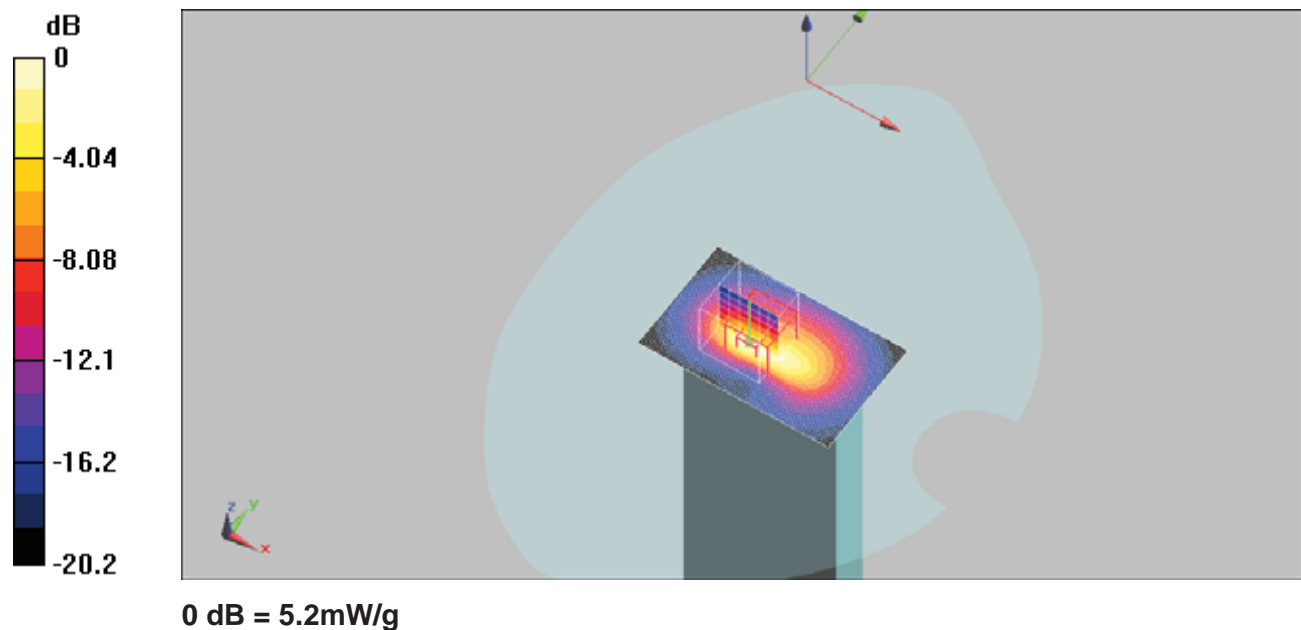

< GSM 1900 CH810 1 909.8 MHz Bottom Body / Date : Aug 18, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: GSM 1900; Frequency: 1909.8 MHz; Duty Cycle: 1:8.3  
 Medium parameters used:  $f = 1909.8 \text{ MHz}$ ;  $\sigma = 1.54 \text{ mho/m}$ ;  $\epsilon_r = 54.9$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(4.84, 4.84, 4.84); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 1900\_ch810\_1 909.8 MHz\_Bottom/Area Scan (81x51x1): Measurement grid:  $dx=12\text{mm}$ ,  $dy=12\text{mm}$

Maximum value of SAR = 5.06 mW/g


GSM 1900\_ch810\_1 909.8 MHz\_Bottom/Zoom Scan (7x7x7)/Cube 0: Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 48.4 V/m; Power Drift = -0.031 dB

Peak SAR (extrapolated) = 7.77 W/kg

SAR(1 g) = 3.36 mW/g; SAR(10 g) = 1.46 mW/g

Maximum value of SAR (measured) = 4.69 mW/g

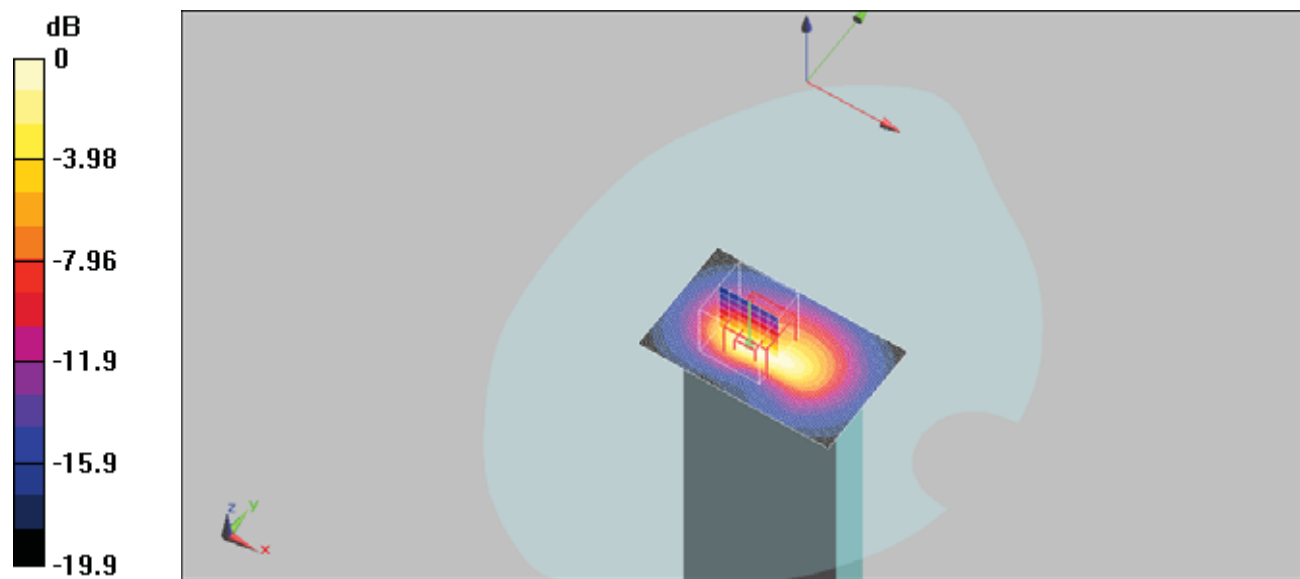

0 dB = 4.69mW/g

< GSM 1900 CH661 1 880.0 MHz Front Body / Date : Aug 18, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3  
 Medium parameters used:  $f = 1880 \text{ MHz}$ ;  $\sigma = 1.5 \text{ mho/m}$ ;  $\epsilon_r = 55$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(4.84, 4.84, 4.84); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 1900\_ch661\_1 880.0 MHz\_Front/Area Scan (71x81x1): Measurement grid:  $dx=12\text{mm}$ ,  $dy=12\text{mm}$

Maximum value of SAR = 1.43 mW/g


GSM 1900\_ch661\_1 880.0 MHz\_Front/Zoom Scan (7x7x7)/Cube 0: Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 26.1 V/m; Power Drift = 0.018 dB

Peak SAR (extrapolated) = 2.03 W/kg

SAR(1 g) = 1.13 mW/g; SAR(10 g) = 0.641 mW/g

Maximum value of SAR (measured) = 1.4 mW/g

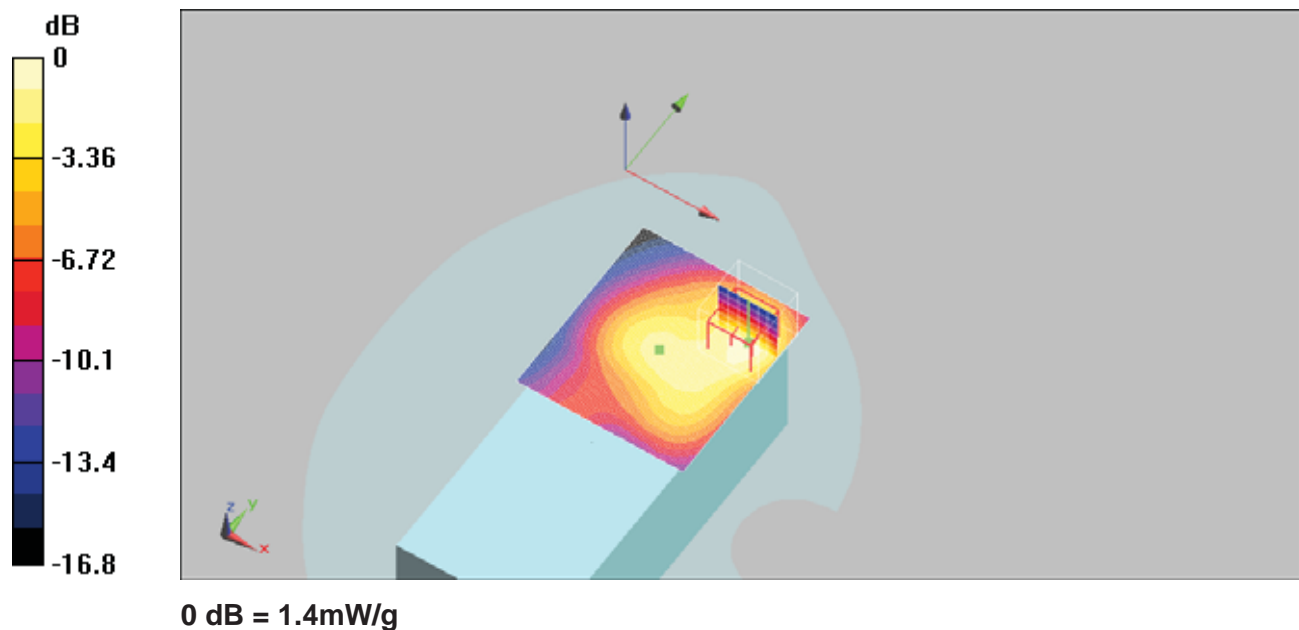

\* note : Found the maximum hot spot from edge SAR because of antenna position of the bottom, so performed partial scan.

< GSM 1900 CH661 1 880.0 MHz Back Body / Date : Aug 18, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3  
 Medium parameters used:  $f = 1880$  MHz;  $\sigma = 1.5$  mho/m;  $\epsilon_r = 55$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(4.84, 4.84, 4.84); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 1900\_ch661\_1 880.0 MHz\_Back/Area Scan (71x81x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR = 1.82 mW/g


GSM 1900\_ch661\_1 880.0 MHz\_Back/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 30.6 V/m; Power Drift = 0.169 dB

Peak SAR (extrapolated) = 2.98 W/kg

SAR(1 g) = 1.46 mW/g; SAR(10 g) = 0.739 mW/g

Maximum value of SAR (measured) = 1.93 mW/g

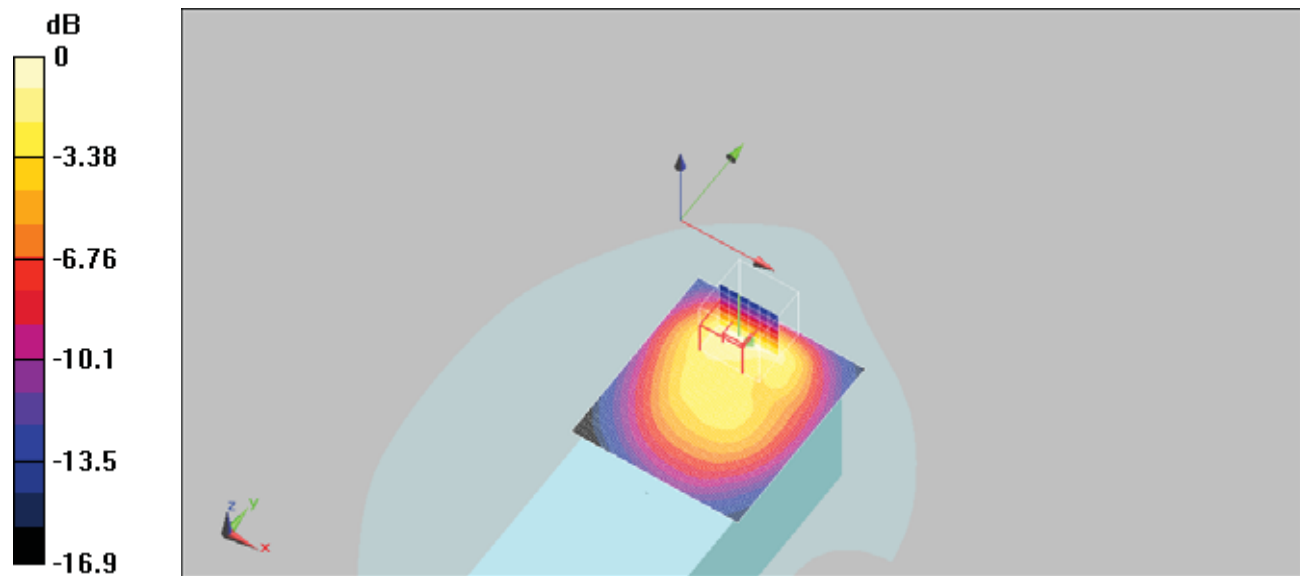

0 dB = 1.93mW/g

\* note : Found the maximum hot spot from edge SAR because of antenna position of the bottom, so performed partial scan.

< GSM 1900 CH661 1 880.0 MHz Left Body / Date : Aug 18, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3  
 Medium parameters used:  $f = 1880 \text{ MHz}$ ;  $\sigma = 1.5 \text{ mho/m}$ ;  $\epsilon_r = 55$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(4.84, 4.84, 4.84); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 1900\_ch661\_1 880.0 MHz\_Left/Area Scan (71x151x1): Measurement grid:  $dx=12\text{mm}$ ,  $dy=12\text{mm}$

Maximum value of SAR = 4.24 mW/g


GSM 1900\_ch661\_1 880.0 MHz\_Left/Zoom Scan (7x7x7)/Cube 0: Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 39.2 V/m; Power Drift = 0.158 dB

Peak SAR (extrapolated) = 6.54 W/kg

SAR(1 g) = 3.09 mW/g; SAR(10 g) = 1.42 mW/g

Maximum value of SAR (measured) = 4.18 mW/g

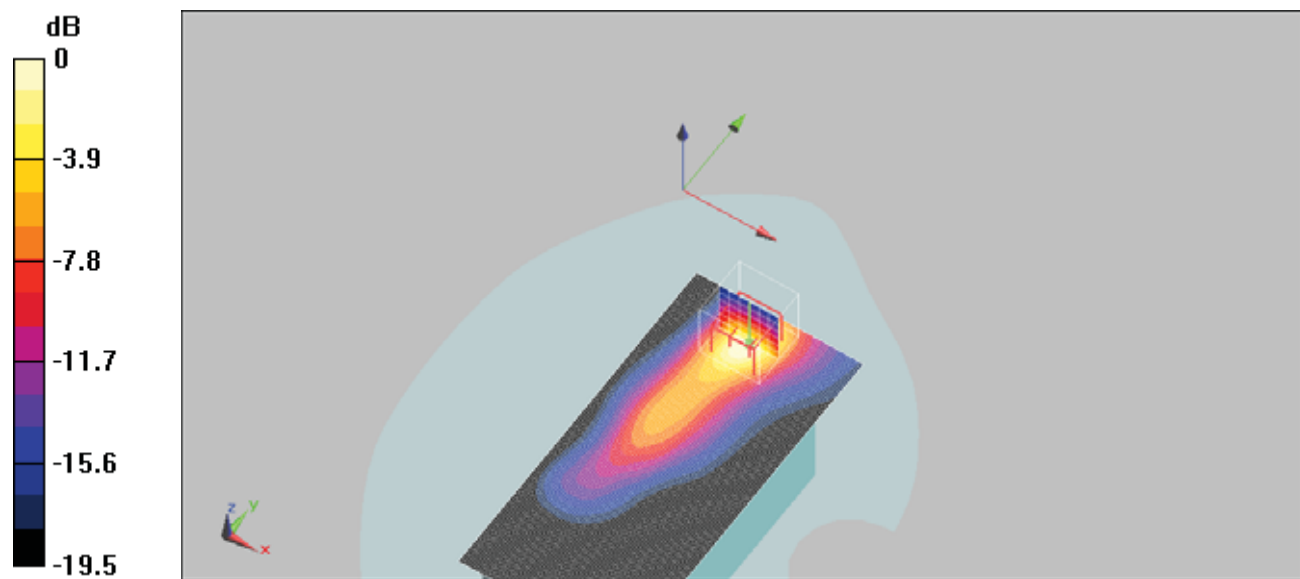

0 dB = 4.18mW/g



< GSM 1900 CH661 1 880.0 MHz Right Body / Date : Aug 18, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified


Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3  
 Medium parameters used:  $f = 1880$  MHz;  $\sigma = 1.5$  mho/m;  $\epsilon_r = 55$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3171; ConvF(4.84, 4.84, 4.84); Calibrated: 2015-07-21
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: SAM with CRP(right side)\_2015\_01\_20; Type: SAM; Serial: 1069
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

GSM 1900\_ch661\_1 880.0 MHz\_Right/Area Scan (71x151x1): Measurement grid: dx=12mm, dy=12mm  
 Maximum value of SAR = 0.475 mW/g

GSM 1900\_ch661\_1 880.0 MHz\_Right/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm  
 Reference Value = 18.1 V/m; Power Drift = -0.00704 dB  
 Peak SAR (extrapolated) = 0.625 W/kg  
 SAR(1 g) = 0.394 mW/g; SAR(10 g) = 0.244 mW/g  
 Maximum value of SAR (measured) = 0.467 mW/g

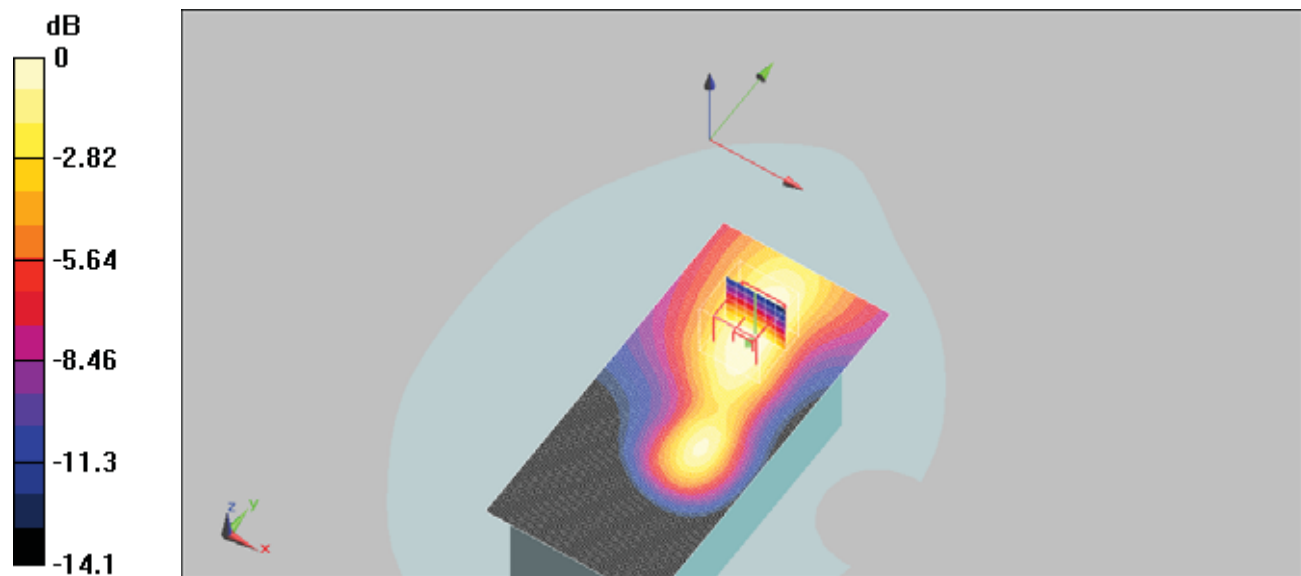

0 dB = 0.467mW/g

< 802.11b CH1 2 412 MHz 5.5 Mbps Right Body / Date : Aug 28, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified


Communication System: 802.11 b/g/n; Frequency: 2412 MHz;Duty Cycle: 1:1  
 Medium parameters used :  $f = 2412$  MHz;  $\sigma = 1.9$  mho/m;  $\epsilon_r = 53.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Phantom section: Flat Section

**DASY5 Configuration:**

- Probe: EX3DV4 - SN3716; ConvF(7.13, 7.13, 7.13); Calibrated: 2014-11-18
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1030
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

802.11b ch1\_2 412 MHz\_5.5 Mbps\_Right/Area Scan (71x151x1): Measurement grid: dx=12mm, dy=12mm  
 Maximum value of SAR = 1.81 mW/g

802.11b ch1\_2 412 MHz\_5.5 Mbps\_Right/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm  
 Reference Value = 15.3 V/m; Power Drift = -0.174 dB  
 Peak SAR (extrapolated) = 2.01 W/kg  
 SAR(1 g) = 0.836 mW/g; SAR(10 g) = 0.311 mW/g  
 Maximum value of SAR (measured) = 1.43 mW/g

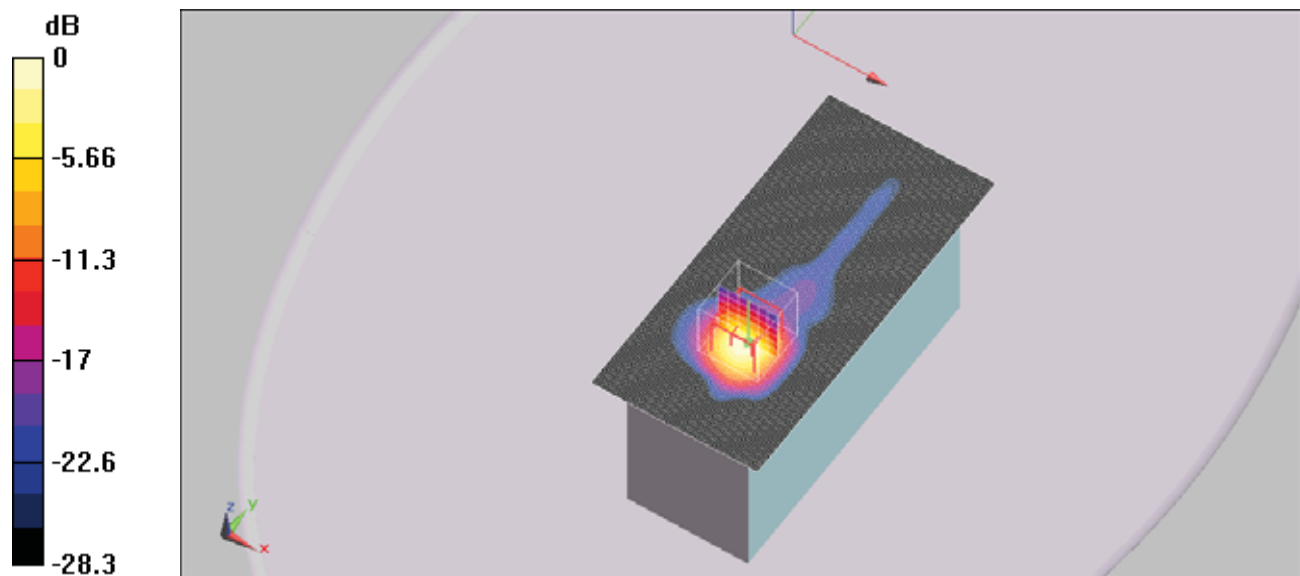

0 dB = 1.43mW/g

< 802.11b CH6 2 437 MHz 5.5 Mbps Right Body / Date : Aug 28, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: 802.11 b/g/n; Frequency: 2437 MHz;Duty Cycle: 1:1  
 Medium parameters used :  $f = 2437 \text{ MHz}$ ;  $\sigma = 1.93 \text{ mho/m}$ ;  $\epsilon_r = 53.5$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

**DASY5 Configuration:**

- Probe: EX3DV4 - SN3716; ConvF(7.13, 7.13, 7.13); Calibrated: 2014-11-18
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1030
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

802.11b ch6\_2 437 MHz\_5.5 Mbps\_Right/Area Scan (71x151x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR = 2.26 mW/g


802.11b ch6\_2 437 MHz\_5.5 Mbps\_Right/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 21.3 V/m; Power Drift = 0.221 dB

Peak SAR (extrapolated) = 2.74 W/kg

SAR(1 g) = 1.14 mW/g; SAR(10 g) = 0.422 mW/g

Maximum value of SAR (measured) = 1.94 mW/g

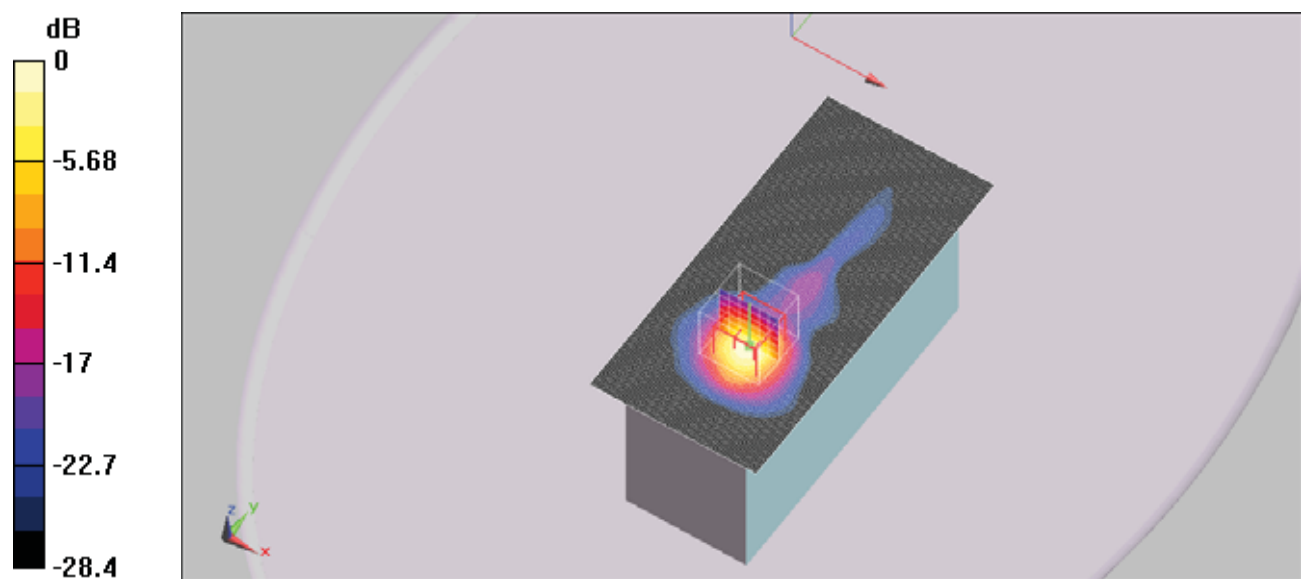

0 dB = 1.94mW/g

< 802.11b CH11 2 462 MHz 5.5 Mbps Right Body / Date : Aug 28, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: 802.11 b/g/n; Frequency: 2462 MHz; Duty Cycle: 1:1  
 Medium parameters used :  $f = 2462 \text{ MHz}$ ;  $\sigma = 1.96 \text{ mho/m}$ ;  $\epsilon_r = 53.4$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

**DASY5 Configuration:**

- Probe: EX3DV4 - SN3716; ConvF(7.13, 7.13, 7.13); Calibrated: 2014-11-18
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1030
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

802.11b ch11\_2 462 MHz\_5.5 Mbps\_Right/Area Scan (71x151x1): Measurement grid:  
 $dx=12\text{mm}$ ,  $dy=12\text{mm}$

Maximum value of SAR = 2.68 mW/g


802.11b ch11\_2 462 MHz\_5.5 Mbps\_Right/Zoom Scan (7x7x7)/Cube 0: Measurement grid:  
 $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 21.7 V/m; Power Drift = -0.114 dB

Peak SAR (extrapolated) = 3.24 W/kg

SAR(1 g) = 1.32 mW/g; SAR(10 g) = 0.485 mW/g

Maximum value of SAR (measured) = 2.29 mW/g

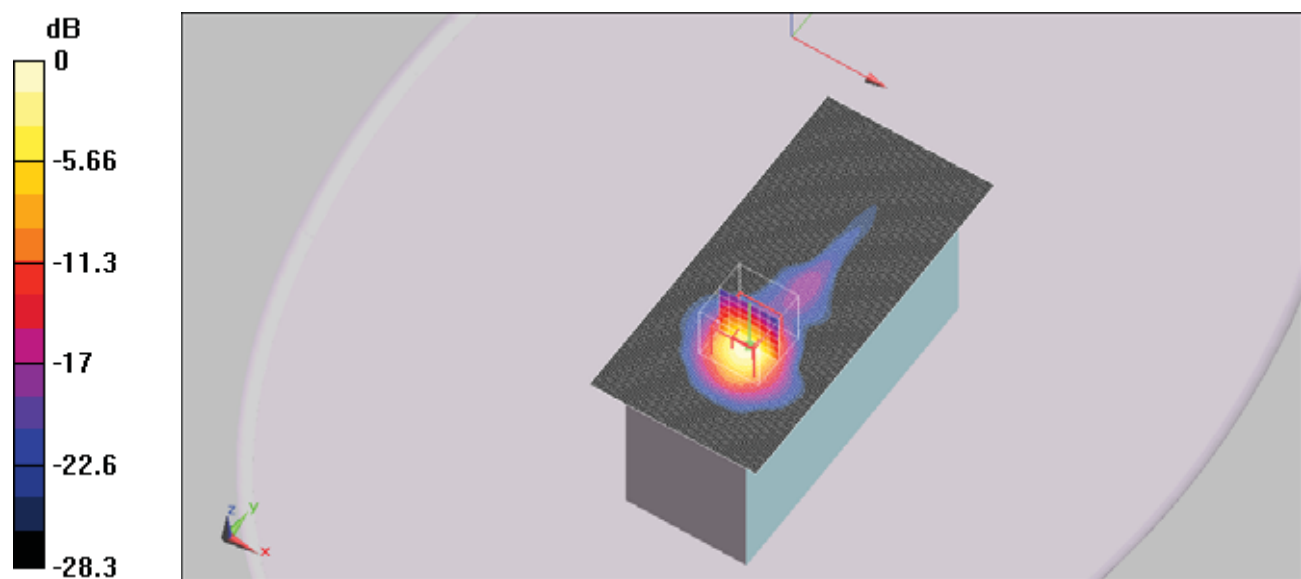

0 dB = 2.29mW/g

< 802.11b CH6 2 437 MHz 5.5 Mbps Front Body / Date : Aug 28, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: 802.11 b/g/n; Frequency: 2437 MHz; Duty Cycle: 1:1  
 Medium parameters used :  $f = 2437 \text{ MHz}$ ;  $\sigma = 1.93 \text{ mho/m}$ ;  $\epsilon_r = 53.5$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

**DASY5 Configuration:**

- Probe: EX3DV4 - SN3716; ConvF(7.13, 7.13, 7.13); Calibrated: 2014-11-18
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1030
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

802.11b ch6\_2 437 MHz\_5.5 Mbps\_Front/Area Scan (101x171x1): Measurement grid:  
 $dx=12\text{mm}$ ,  $dy=12\text{mm}$

Maximum value of SAR = 0.040 mW/g


802.11b ch6\_2 437 MHz\_5.5 Mbps\_Front/Zoom Scan (7x7x7)/Cube 0: Measurement grid:  
 $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 4.1 V/m; Power Drift = 0.065 dB

Peak SAR (extrapolated) = 0.047 W/kg

SAR(1 g) = 0.023 mW/g; SAR(10 g) = 0.012 mW/g

Maximum value of SAR (measured) = 0.035 mW/g

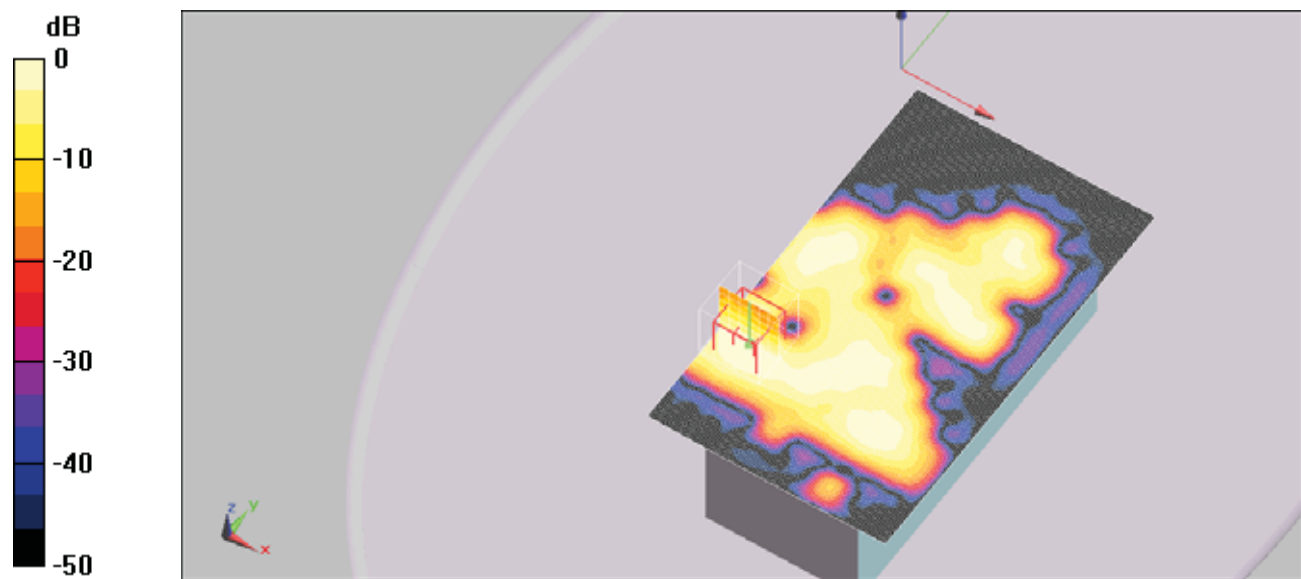

0 dB = 0.035mW/g

< 802.11b CH6 2 437 MHz 5.5 Mbps Back Body / Date : Aug 28, 2015 >

DUT: MT280; Type: Sample; Serial: Not Specified

Communication System: 802.11 b/g/n; Frequency: 2437 MHz; Duty Cycle: 1:1  
 Medium parameters used :  $f = 2437 \text{ MHz}$ ;  $\sigma = 1.93 \text{ mho/m}$ ;  $\epsilon_r = 53.5$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3716; ConvF(7.13, 7.13, 7.13); Calibrated: 2014-11-18
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn444; Calibrated: 2014-11-12
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1030
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

802.11b ch6\_2 437 MHz\_5.5 Mbps\_Back/Area Scan (101x171x1): Measurement grid:  
 $dx=12\text{mm}$ ,  $dy=12\text{mm}$

Maximum value of SAR = 0.030 mW/g


802.11b ch6\_2 437 MHz\_5.5 Mbps\_Back/Zoom Scan (7x7x7)/Cube 0: Measurement grid:  
 $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 3.56 V/m; Power Drift = 0.213 dB

Peak SAR (extrapolated) = 0.040 W/kg

SAR(1 g) = 0.023 mW/g; SAR(10 g) = 0.013 mW/g


Maximum value of SAR (measured) = 0.031 mW/g

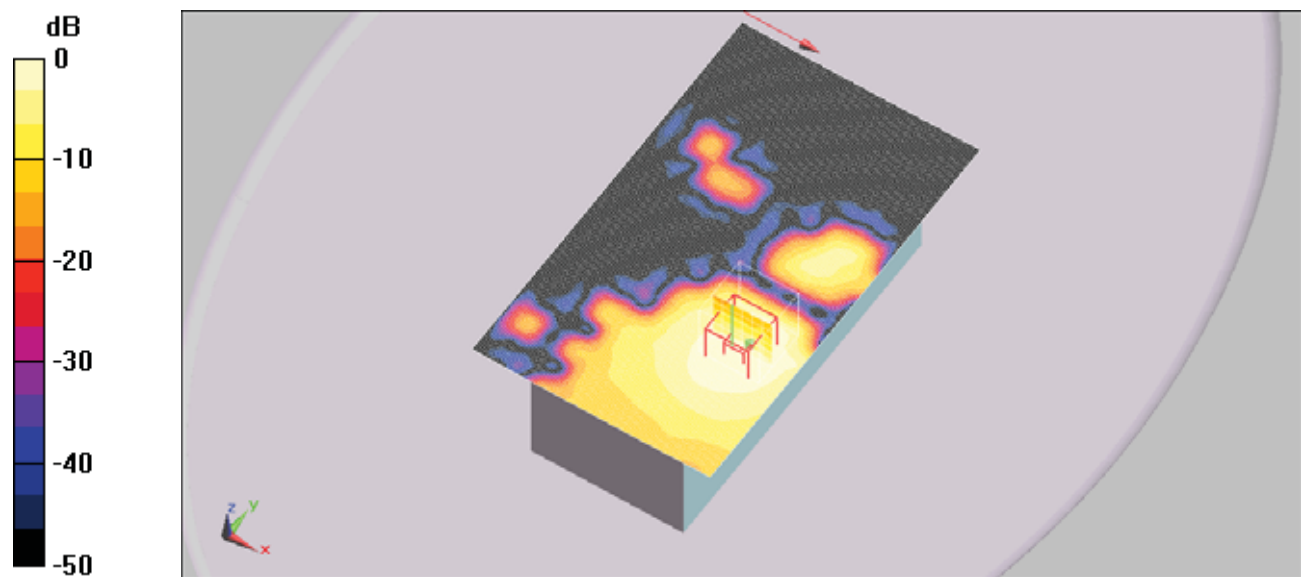

0 dB = 0.031mW/g

## ANNEX C. PHOTOGRAPHS

### < System Verification >

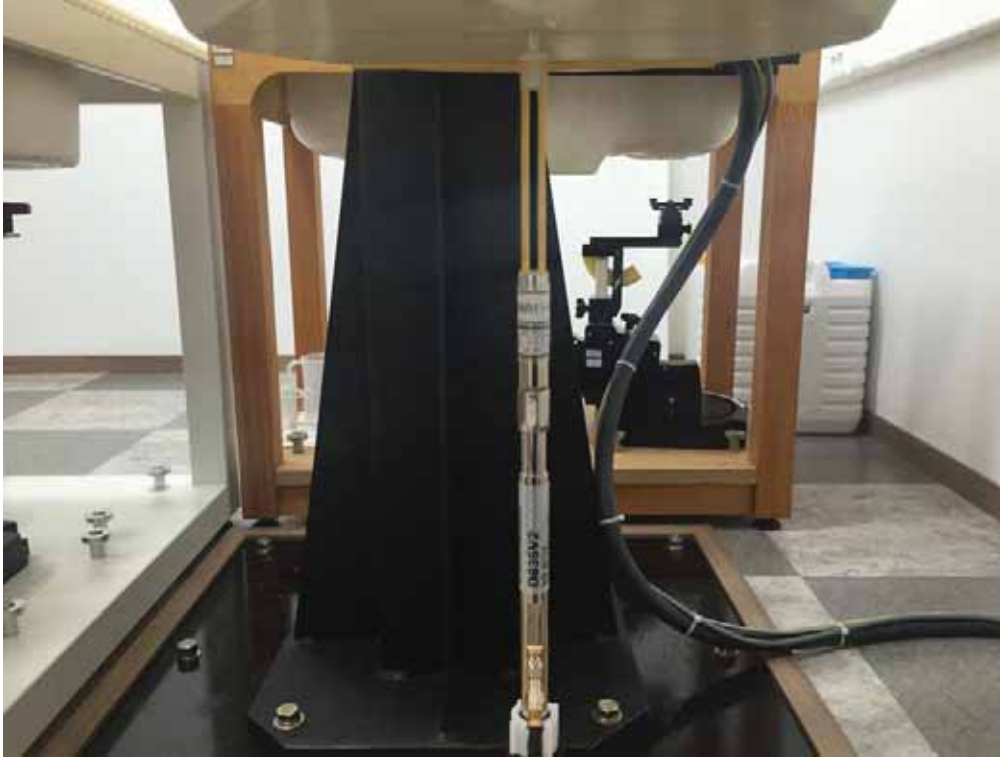

< 835 MHz >



< 1 950 MHz >



< 2 450 MHz >



< Test position >



Front view (Front of DUT)



Side view (Front of DUT)



Front view (Back of DUT)



Side view (Back of DUT)




Front view (Bottom of DUT)



Side view (Bottom of DUT)



Front view (Left of DUT)

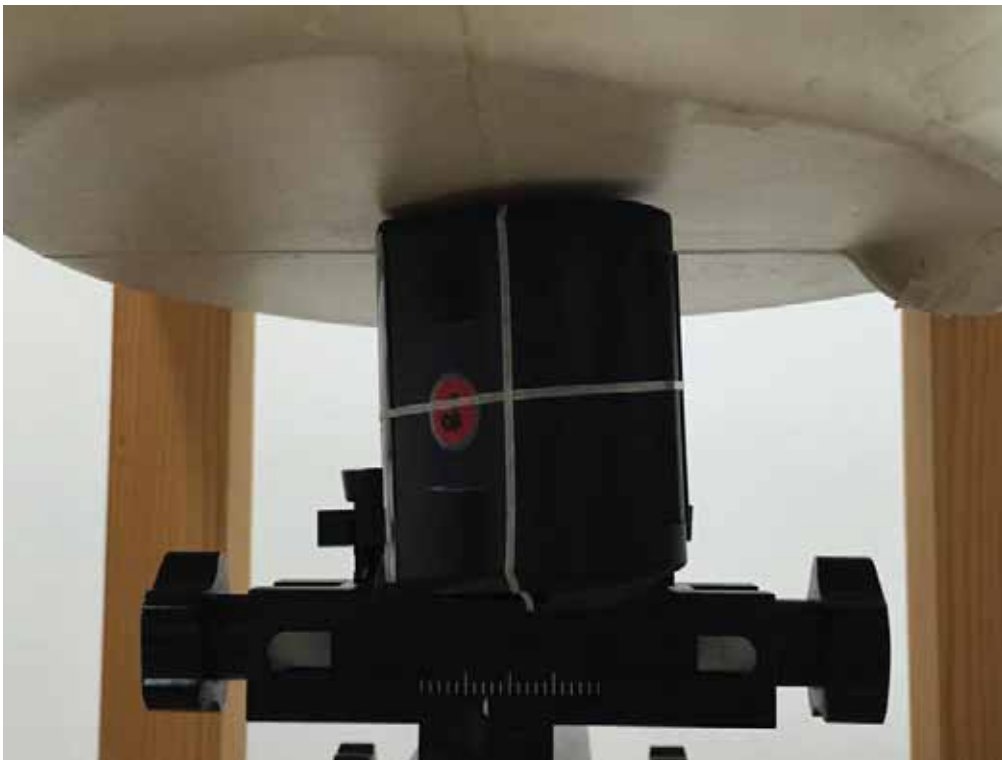

Side view (Left of DUT)



Front view (Right of DUT)



Side view (Right of DUT)


< Liquid Depth >



< 835 MHz >



< 1 950 MHz >

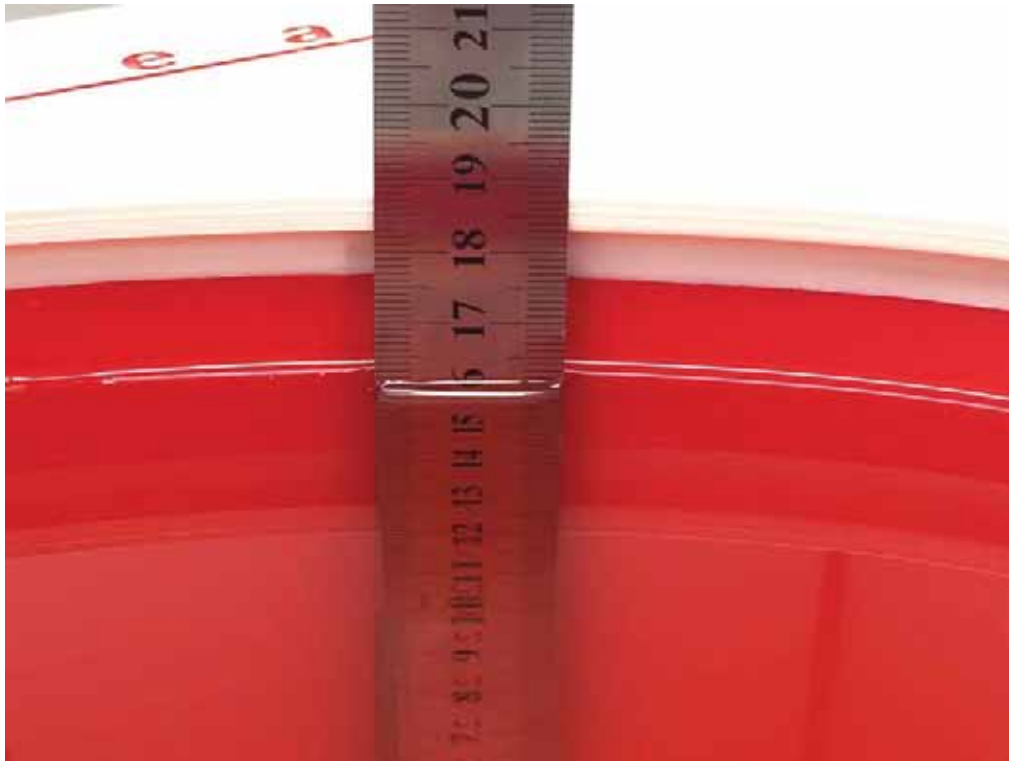

< 2 450 MHz >

< DUT Photograph >



< Front >



< Back >





< Top >



< Bottom >




< Left >



< Right >


## ANNEX D. ANTENNA INFORMATION

### < Antenna location >

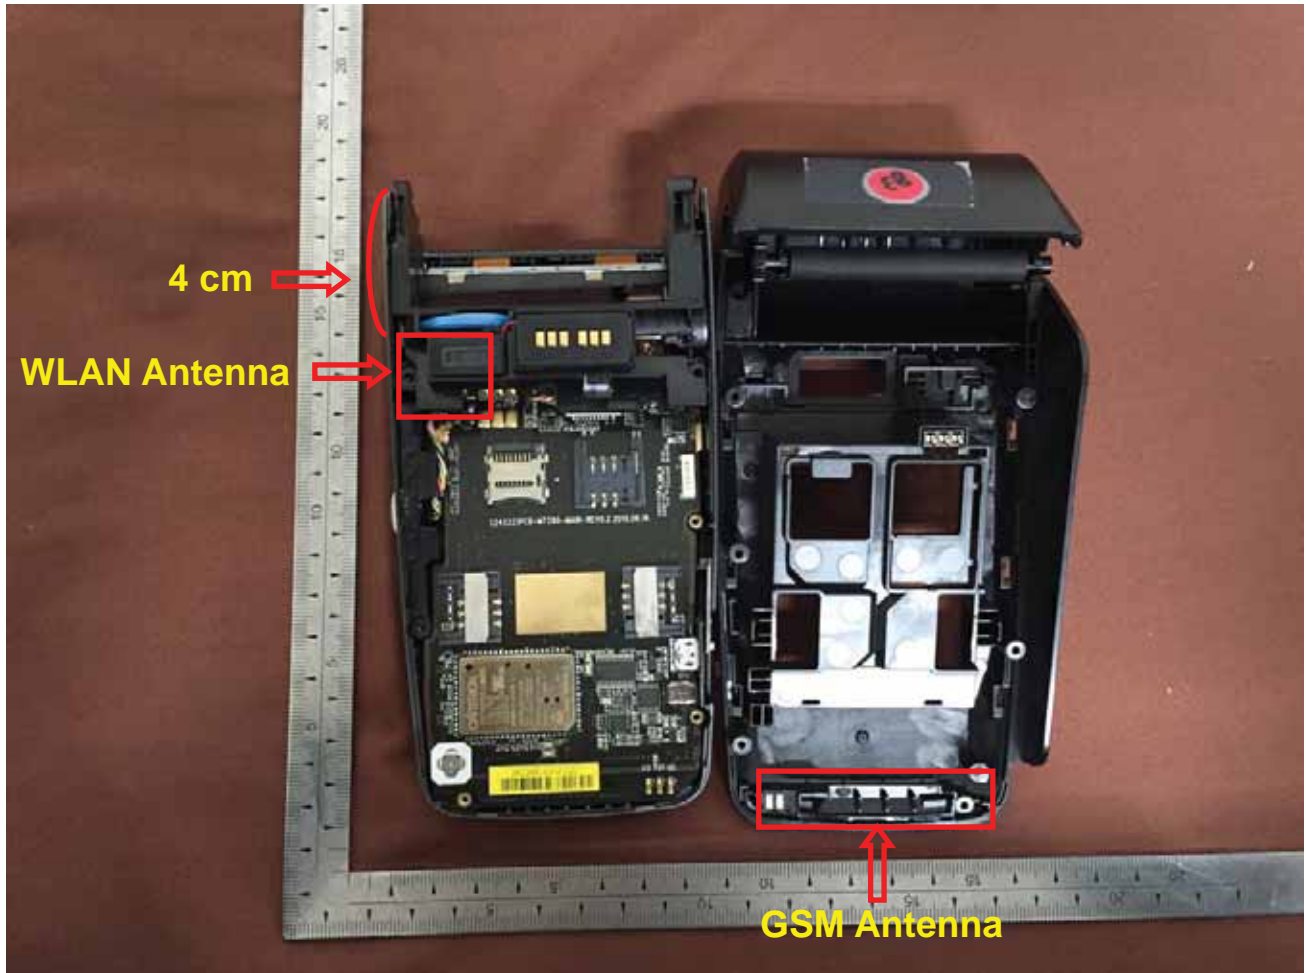

< Antenna Data Sheet >

1. WWAN Antenna Data Sheet

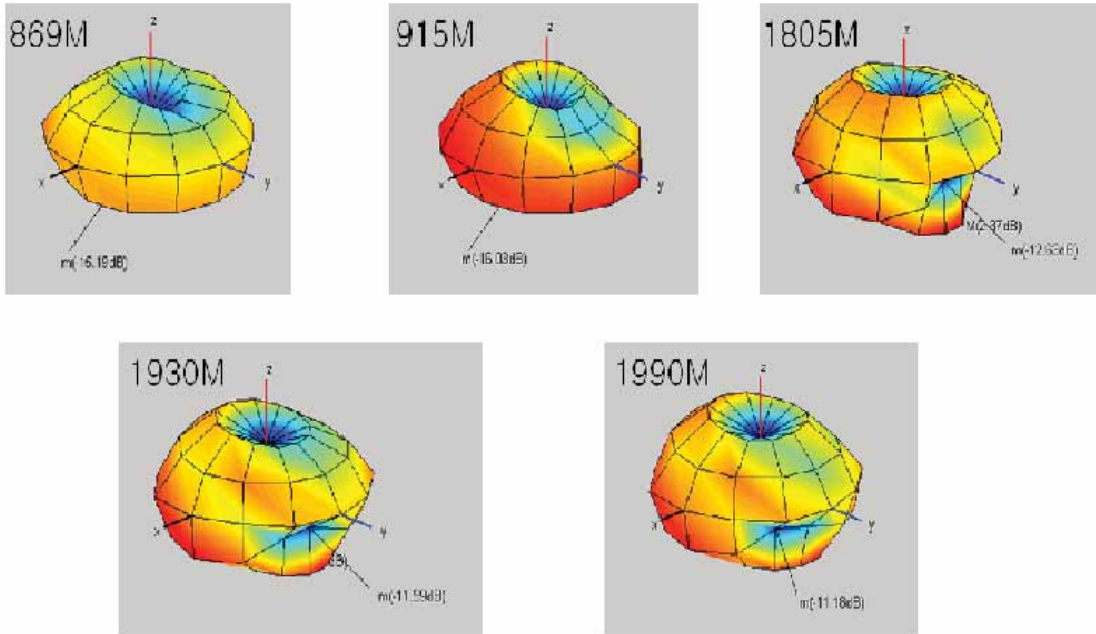


< 3D Pattern >

	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19
Frequency [MHz]	824	849	869	880	894	915	925	960	1710	1785	1805	1850	1880	1910	1930	1980	1990	2110	2170
Efficiency [dB]	-7.86	-6.25	-5.46	-5.02	-4.60	-4.47	-3.86	-3.57	-4.77	-2.54	-2.39	-2.39	-2.14	-2.72	-2.81	-2.24	-2.23	-4.84	-4.72
Efficiency [%]	16.37	23.70	28.45	31.48	34.66	35.74	41.12	43.92	33.34	55.74	57.69	57.70	61.04	53.40	52.40	59.76	59.87	32.84	33.72
TRG [dB]	-7.86	-6.25	-5.46	-5.02	-4.60	-4.47	-3.86	-3.57	-4.77	-2.54	-2.39	-2.39	-2.14	-2.72	-2.81	-2.24	-2.23	-4.84	-4.72
TRG <sub>max</sub> [dBi]	-9.75	-7.99	-7.00	-6.53	-6.04	-5.47	-5.33	-4.97	-7.74	-5.13	-4.96	-4.93	-4.76	-5.55	-5.78	-5.44	-5.59	-7.80	-7.71
Gain <sub>max</sub> [dBi]	-6.23	-3.69	-3.28	-3.03	-2.45	-1.70	-1.53	-1.31	-1.01	1.74	1.92	1.37	1.16	0.21	-0.22	-0.53	-0.64	-2.80	-2.24
Gain <sub>min</sub> [dBi]	-30.67	-28.08	-31.24	-32.36	-38.06	-26.07	-25.24	-24.45	-31.17	-19.92	-23.69	-29.13	-40.20	-23.46	-23.60	-27.43	-28.95	-24.91	-25.99
TRG <sub>min</sub> [dBi]	-12.39	-11.07	-10.70	-10.34	-10.09	-11.35	-9.28	-9.19	-7.82	-6.02	-5.89	-5.92	-5.59	-5.93	-5.85	-5.06	-4.91	-7.89	-7.75
Gain <sub>min</sub> [dBi]	-8.16	-6.17	-5.76	-5.59	-4.91	-5.62	-3.48	-3.54	-2.32	0.65	1.07	0.86	0.73	-0.19	0.20	1.28	1.40	-3.46	-2.92
Gain <sub>avg</sub> [dBi]	-33.24	-20.98	-24.01	-25.32	-23.06	-26.67	-27.10	-31.34	-19.17	-24.03	-25.61	-25.05	-34.61	-29.33	-28.57	-28.89	-26.17	-23.48	-25.29
UHRG [dB]	-11.94	-9.96	-9.22	-9.01	-8.86	-8.87	-8.28	-7.69	-8.06	-6.58	-6.57	-6.36	-6.15	-6.87	-7.08	-6.61	-6.53	-7.66	-7.44
UHRG/TRG [%]	39.12	42.61	42.02	39.92	37.55	36.33	36.10	38.75	46.87	39.47	38.22	40.03	39.80	38.53	37.37	36.50	37.14	52.19	53.50
H-Plane	-8.49	-5.80	-5.12	-4.90	-4.63	-4.09	-3.88	-3.26	-7.94	-5.73	-5.27	-5.12	-5.57	-6.45	-6.52	-6.25	-6.50	-8.88	-8.70
E1-Plane, AVG [dB]	-10.62	-9.23	-8.03	-7.43	-6.87	-6.26	-6.10	-5.68	-7.77	-5.32	-5.40	-5.26	-5.48	-6.81	-7.12	-7.33	-7.61	-11.02	-12.07
E2-Plane, AVG [dB]	-10.39	-8.45	-7.60	-7.11	-6.59	-5.96	-5.79	-5.73	-6.47	-4.34	-4.07	-4.23	-3.91	-4.54	-4.79	-4.20	-4.19	-6.38	-6.10
Peak Gain [dBi]	-4.19	-3.10	-2.29	-1.37	-0.50	-0.22	0.60	0.71	-0.87	2.37	2.73	2.57	2.64	1.73	1.42	1.97	1.98	-2.04	-1.55
Directivity [dB]	3.67	3.15	3.17	3.65	4.10	4.25	4.46	4.28	3.90	4.91	5.11	4.96	4.79	4.45	4.23	4.20	4.21	2.79	3.17
Minimum Gain [dBi]	-15.87	-14.15	-15.20	-17.22	-17.98	-16.04	-13.25	-15.54	-17.10	-12.63	-14.75	-13.89	-12.50	-12.60	-11.60	-10.60	-11.19	-11.29	-11.67

< Antenna Gain >

2. WLAN Antenna Data Sheet

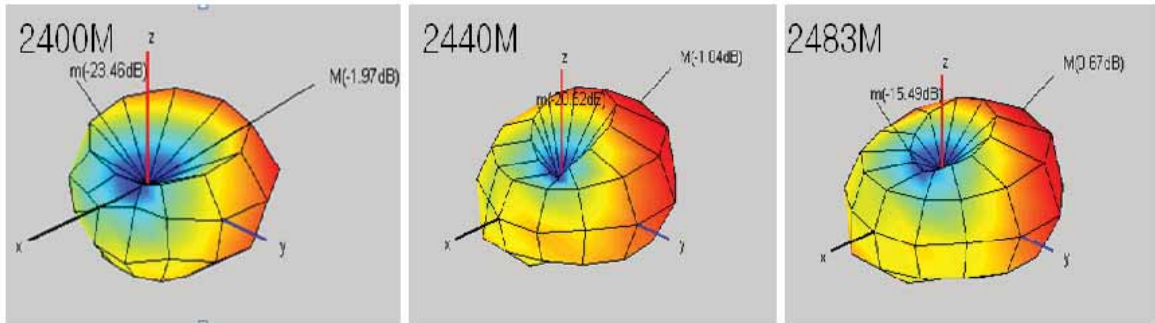

< 3D Pattern >

	1	2	3	4	5	6	7	8	9
<b>Frequency [MHz]</b>	2400	2410	2420	2430	2440	2450	2460	2470	2483
<b>Efficiency [dB]</b>	-7.85	-7.65	-7.32	-6.83	-6.58	-6.73	-6.32	-5.96	-5.59
<b>Efficiency [%]</b>	16.41	17.18	18.54	20.73	21.95	21.23	23.33	25.33	27.57
<b>TRG [dB]</b>	-7.85	-7.65	-7.32	-6.83	-6.58	-6.73	-6.32	-5.96	-5.59
<b>TRG<sub>0</sub> [dB]</b>	-8.91	-8.63	-8.27	-7.77	-7.50	-7.72	-7.26	-6.93	-6.58
<b>Gain<sub>0 Peak</sub> [dBi]</b>	-2.16	-1.92	-1.61	-1.21	-1.08	-1.48	-1.18	-0.98	-0.76
<b>Gain<sub>0 Min</sub> [dBi]</b>	-27.16	-27.89	-28.94	-29.91	-30.77	-31.25	-30.89	-30.73	-29.23
<b>TRG<sub>0</sub> [dB]</b>	-14.48	-14.59	-14.37	-13.94	-13.79	-13.64	-13.44	-12.95	-12.54
<b>Gain<sub>0 Peak</sub> [dBi]</b>	-7.53	-7.83	-7.85	-7.67	-7.81	-8.01	-7.99	-7.42	-6.78
<b>Gain<sub>0 Min</sub> [dBi]</b>	-30.61	-30.31	-32.03	-34.82	-35.29	-33.73	-27.43	-24.26	-25.67
<b>UHRG [dB]</b>	-9.98	-9.83	-9.55	-9.13	-8.95	-9.17	-8.83	-8.53	-8.23
<b>UHRG/TRG [%]</b>	61.20	60.54	59.82	58.99	58.06	57.05	56.16	55.35	54.53
<b>H-Plane</b>	-8.10	-7.78	-7.39	-6.84	-6.51	-6.66	-6.15	-5.79	-5.38
<b>E1-Plane, AVG [dB]</b>	-7.84	-7.57	-7.23	-6.75	-6.50	-6.76	-6.34	-6.08	-5.80
<b>E2-Plane, AVG [dB]</b>	-11.80	-11.51	-11.13	-10.62	-10.34	-10.56	-10.13	-9.85	-9.54
<b>Peak Gain [dBi]</b>	-1.97	-1.90	-1.58	-1.18	-1.04	-1.44	-1.13	-0.91	-0.67
<b>Directivity [dB]</b>	5.88	5.75	5.73	5.66	5.54	5.29	5.19	5.05	4.93
<b>Minimum Gain [dBi]</b>	-23.47	-23.53	-22.46	-21.77	-20.63	-19.42	-17.72	-16.43	-15.49

< Antenna Gain >

## ANNEX E. PROBE AND DIPOLE CALIBRATION CERTIFICATES

### < E-Field Probe : ES3DV3 – SN 3171 >

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SA5)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Onetech (Dymstec)**

Certificate No: **ES3-3171\_Jul15**

#### CALIBRATION CERTIFICATE

Object: **ES3DV3 - SN:3171**

Calibration procedure(s): **QA CAL-01.v9, QA CAL-23.v5, QA CAL-25.v6  
Calibration procedure for dosimetric E-field probes.**

Calibration date: **July 21, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GD41293874	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41488087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Attenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02129)	Mar-16
Reference 20 dB Attenuator	SN: S6277 (20x)	01-Apr-15 (No. 217-02132)	Mar-16
Reference 30 dB Attenuator	SN: S5129 (30b)	01-Apr-15 (No. 217-02133)	Mar-16
Reference Probe ES3DV2	SN: 3013	30 Dec-14 (No. ES3-3013 Dec14)	Dec-15
DAE4	SN: 660	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

	Name	Function	Signature
Calibrated by:	Jeton Kasrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: July 23, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\varphi$	$\varphi$ rotation around probe axis
Polarization $\theta$	$\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Methods Applied and Interpretation of Parameters:**

- **NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1600$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- **NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- **DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- **PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- **A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- **ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- **Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- **Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- **Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

ES3DV3 – SN:3171

July 21, 2015

# Probe ES3DV3

## SN:3171

Manufactured: January 23, 2008  
Calibrated: July 21, 2015

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)



ES3DV3- SN:3171

July 21, 2015

### DASY/EASY - Parameters of Probe: ES3DV3 - SN:3171

#### Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup>	1.06	1.20	1.19	$\pm 10.1 \%$
DCP (mV) <sup>B</sup>	105.3	96.5	102.7	

#### Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc <sup>E</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	190.3	$\pm 3.8 \%$
		Y	0.0	0.0	1.0		201.5	
		Z	0.0	0.0	1.0		202.8	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ES3DV3- SN:3171

July 21, 2015

### DASY/EASY - Parameters of Probe: ES3DV3 - SN:3171

#### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>c</sup>	Relative Permittivity <sup>f</sup>	Conductivity (S/m) <sup>f</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth <sup>g</sup> (mm)	Unc (k=2)
835	41.5	0.90	6.29	6.29	6.29	0.55	1.37	± 12.0 %
1750	40.1	1.37	5.24	5.24	5.24	0.72	1.22	± 12.0 %
1950	40.0	1.40	4.91	4.91	4.91	0.48	1.46	± 12.0 %

<sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>f</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>g</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ES3DV3- SN:3171

July 21, 2015

### DASY/EASY - Parameters of Probe: ES3DV3 - SN:3171

#### Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>c</sup>	Relative Permittivity <sup>f</sup>	Conductivity (S/m) <sup>f</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth <sup>g</sup> (mm)	Unc (k=2)
835	55.2	0.97	5.97	5.97	5.97	0.80	1.14	± 12.0 %
1750	53.4	1.49	4.87	4.87	4.87	0.39	1.82	± 12.0 %
1950	53.3	1.52	4.84	4.84	4.84	0.57	1.46	± 12.0 %

<sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


<sup>f</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>g</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ES3DV3- SN:3171

July 21, 2015

### Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

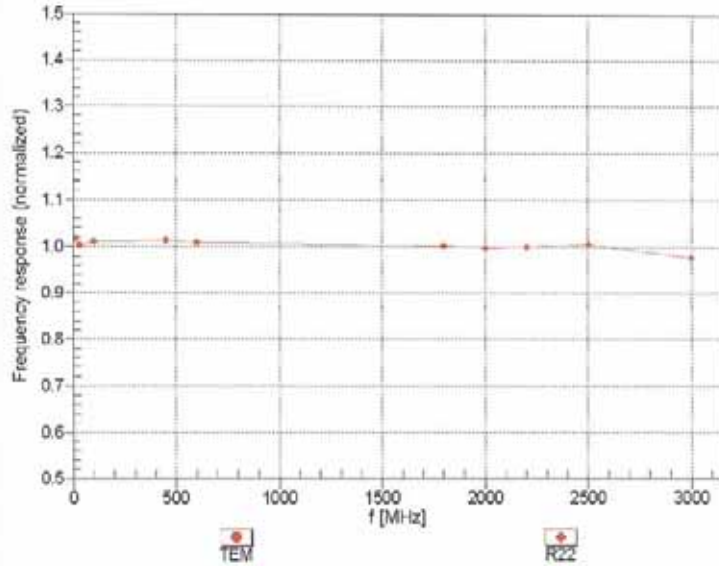

Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)



ES3DV3- SN:3171

July 21, 2015

Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$

f=600 MHz,TEM

f=1800 MHz,R22

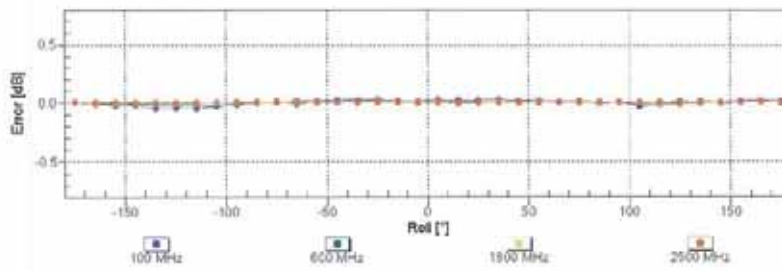
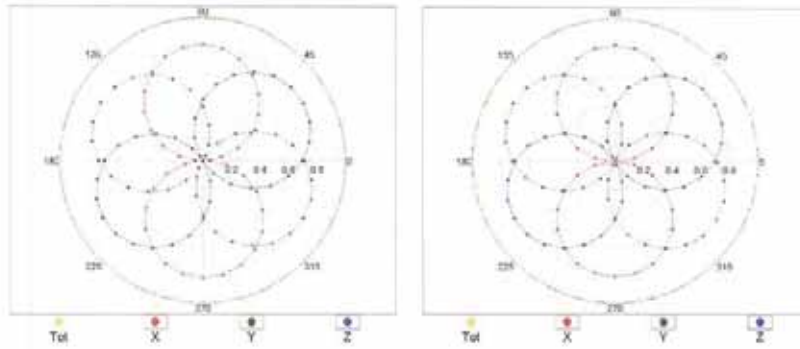


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)

ES3DV3-SN:3171

July 21, 2015

**Dynamic Range f(SAR<sub>head</sub>)**  
 (TEM cell, f<sub>eval</sub>= 1900 MHz)

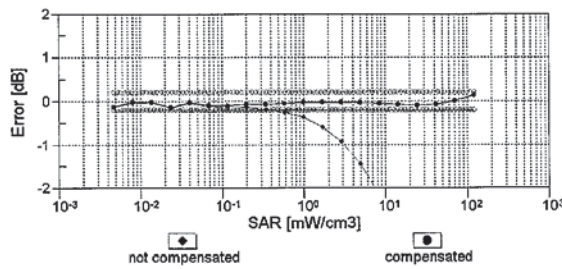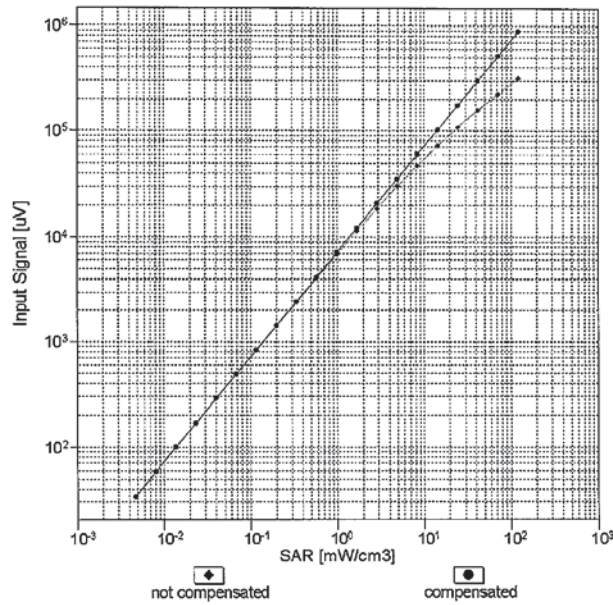


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


ES3DV3-5N:3171

July 21, 2015

### Conversion Factor Assessment

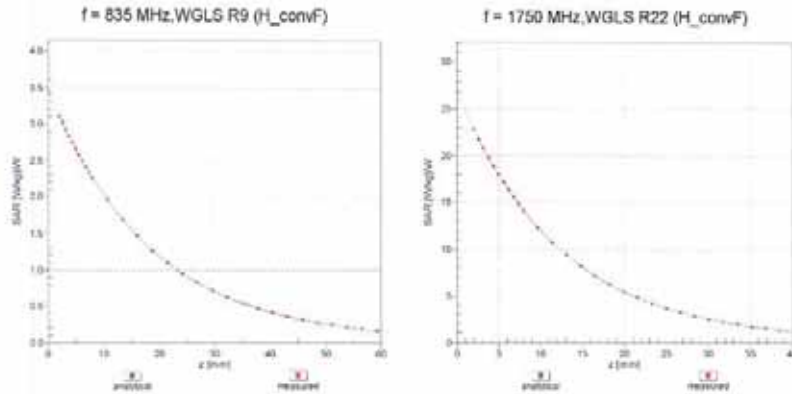

### Deviation from Isotropy in Liquid Error ( $\phi, \theta$ ), $f = 900 \text{ MHz}$

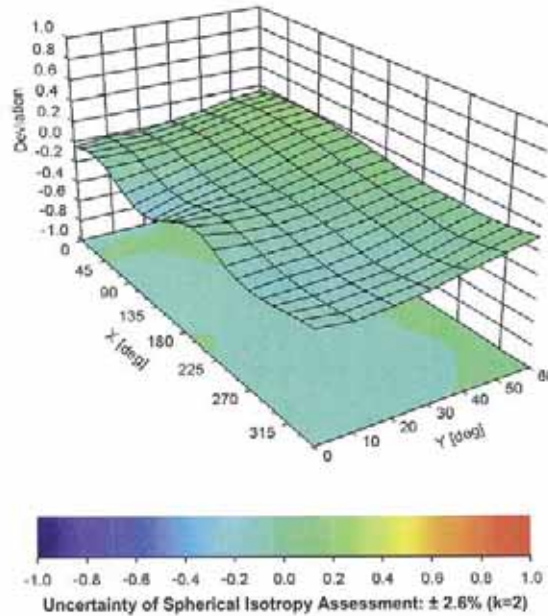

ES3DV3- SN:3171

July 21, 2015

**DASY/EASY - Parameters of Probe: ES3DV3 - SN:3171**

**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	105.2
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

Certificate No: ES3-3171\_Jul15

Page 11 of 11



< Probe : EX3DV4 – SN 3716 >

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **One-Tech (Dymstec)**

Certificate No: **EX3-3716\_Nov14**

**CALIBRATION CERTIFICATE**

Object: **EX3DV4 - SN:3716**

Calibration procedure(s): **QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6  
Calibration procedure for dosimetric E-field probes**

Calibration date: **November 18, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E44198B	GB41293874	03-Apr-14 (No. 217-01911)	Apr-15
Power sensor E4412A	MY41498087	03-Apr-14 (No. 217-01911)	Apr-15
Reference 3 dB Attenuator	SN: S5054 (3c)	03-Apr-14 (No. 217-01915)	Apr-15
Reference 20 dB Attenuator	SN: S5277 (20x)	03-Apr-14 (No. 217-01919)	Apr-15
Reference 30 dB Attenuator	SN: S5129 (30b)	03-Apr-14 (No. 217-01920)	Apr-15
Reference Probe ES3DV2	SN: 3013	30-Dec-13 (No. ES3-3013_Dec13)	Dec-14
DAE4	SN: 860	13-Dec-13 (No. DAE4-860_Dec13)	Dec-14
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

Calibrated by:	Name <b>Claudio Leubler</b>	Function <b>Laboratory Technician</b>	Signature 
Approved by:	Name <b>Katja Pokovic</b>	Technical Manager	

Issued: November 18, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
S Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: SCS 108

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

**Glossary:**

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\phi$	$\phi$ rotation around probe axis
Polarization $\theta$	$\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

**Methods Applied and Interpretation of Parameters:**

- **NORM<sub>x,y,z</sub>:** Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- **NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- **DCP<sub>x,y,z</sub>:** DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- **PAR:** PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- **A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>:** A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- **ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- **Spherical Isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- **Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- **Connector Angle:** The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

EX3DV4 – SN:3716

November 18, 2014

# Probe EX3DV4

## SN:3716

Manufactured: August 14, 2009  
Calibrated: November 18, 2014

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

---

Certificate No: EX3-3716\_Nov14

Page 3 of 11

EX3DV4- SN:3716

November 18, 2014

### DASY/EASY - Parameters of Probe: EX3DV4 - SN:3716

#### Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>a</sup>	0.48	0.54	0.48	$\pm 10.1 \%$
DCP (mV) <sup>b</sup>	97.9	98.9	97.7	

#### Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc <sup>c</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	137.7	$\pm 2.5 \%$
		Y	0.0	0.0	1.0		134.9	
		Z	0.0	0.0	1.0		135.3	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>a</sup> The uncertainties of Norm: X, Y, Z do not affect the E<sup>2</sup>-field uncertainty inside TSI. (see Pages 5 and 6).

<sup>b</sup> Numerical linearization parameter: uncertainty not required.

<sup>c</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:3716

November 18, 2014

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3716

### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>E</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>H</sup> (mm)	Unct. (k=2)
2450	39.2	1.80	6.94	6.94	6.94	0.54	0.70	± 12.0 %
5200	36.0	4.66	4.97	4.97	4.97	0.35	1.80	± 13.1 %
5300	35.9	4.76	4.74	4.74	4.74	0.35	1.80	± 13.1 %
5500	35.6	4.96	4.56	4.56	4.56	0.35	1.80	± 13.1 %
5600	35.5	5.07	4.30	4.30	4.30	0.35	1.80	± 13.1 %
5800	35.3	5.27	4.29	4.29	4.29	0.40	1.80	± 13.1 %

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>E</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3716

November 18, 2014

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3716

### Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>c</sup>	Relative Permittivity <sup>e</sup>	Conductivity (S/m) <sup>f</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth (mm) <sup>h</sup>	Unct. (k=2)
2450	52.7	1.95	7.13	7.13	7.13	0.76	0.58	± 12.0 %
5200	49.0	5.30	4.41	4.41	4.41	0.45	1.90	± 13.1 %
5300	48.9	5.42	4.22	4.22	4.22	0.45	1.90	± 13.1 %
5500	48.6	5.65	3.89	3.89	3.89	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.85	3.85	3.85	0.50	1.90	± 13.1 %
5800	48.2	6.00	4.03	4.03	4.03	0.50	1.90	± 13.1 %

<sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


<sup>e</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>h</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3716

November 18, 2014

### Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

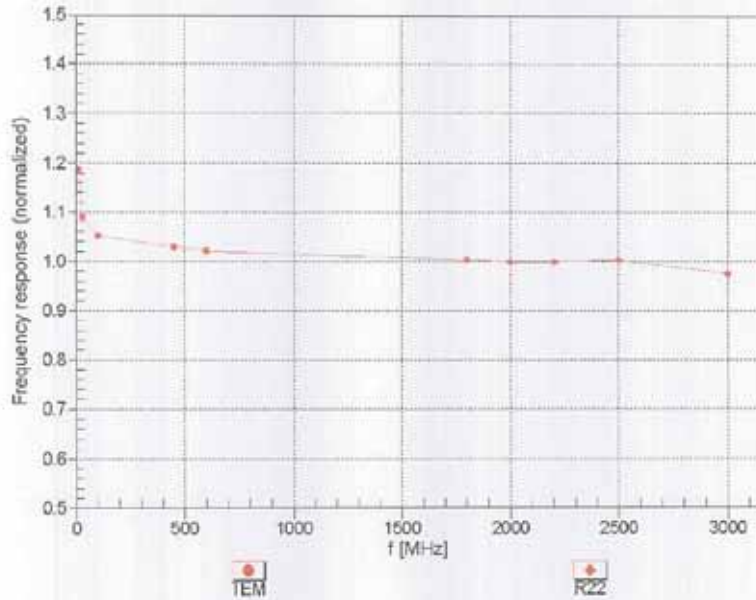

Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)



EX3DV4- SN:3716

November 18, 2014

Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$

f=600 MHz,TEM

f=1800 MHz,R22

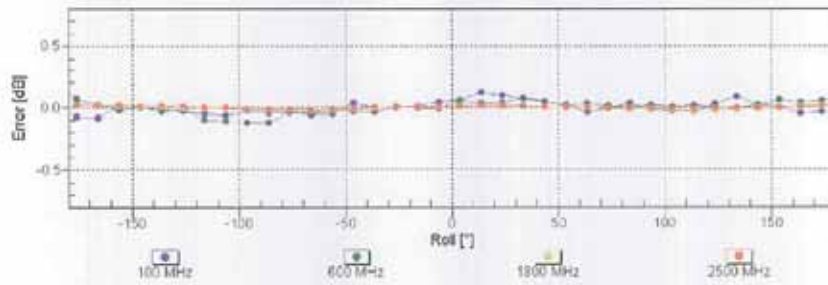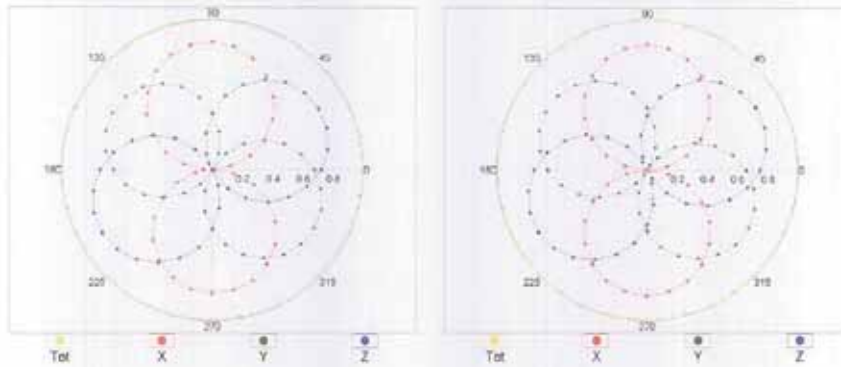



Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)



EX3DV4-SN:3716

November 18, 2014

**Dynamic Range f(SAR<sub>head</sub>)**  
 (TEM cell, f<sub>eval</sub>= 1900 MHz)

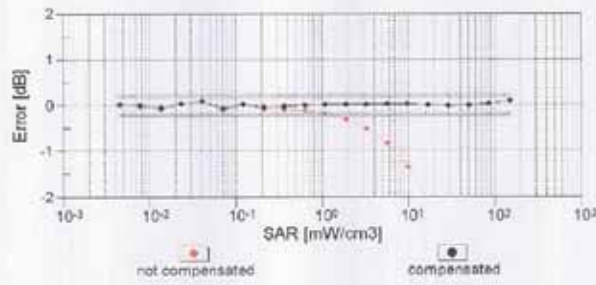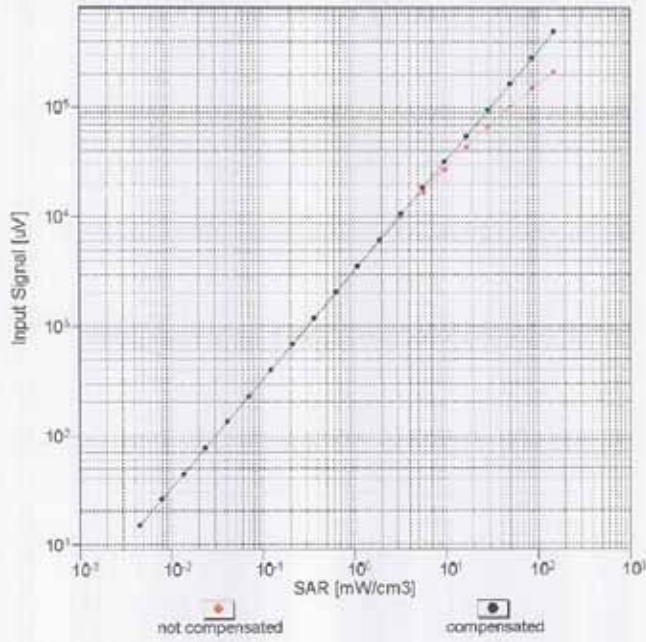


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


EX3DV4-SN:3716

November 18, 2014

### Conversion Factor Assessment

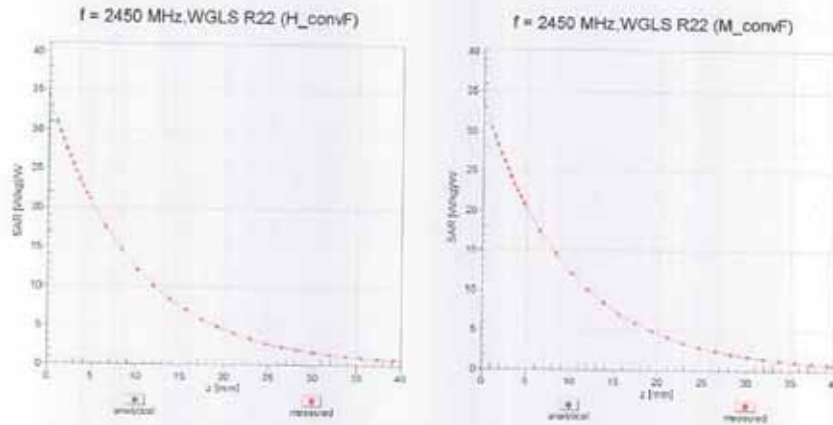

### Deviation from Isotropy in Liquid Error ( $\phi, \theta$ ), f = 900 MHz

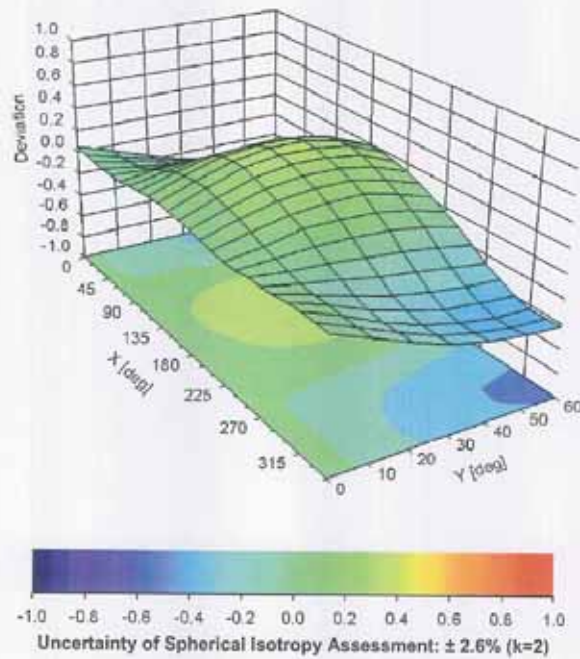

EX3DV4- SN:3716

November 18, 2014

### DASY/EASY - Parameters of Probe: EX3DV4 - SN:3716

#### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-76.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

< Dipole Antenna : D835V2 – SN 4d172 >

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client **One-Tech (Dymstec)**

Certificate No: **D835V2-4d172\_Jul14**

**CALIBRATION CERTIFICATE**

Object: **D835V2 - SN: 4d172**

Calibration procedure(s): **QA CAL-05.v9  
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **July 10, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	US37292783	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	MY41082317	09-Oct-13 (No. 217-01828)	Oct-14
Reference 20 dB Attenuator	SN: 5058 (20k)	03-Apr-14 (No. 217-01918)	Apr-15
Type-N mismatch combination	SN: 5047.2 / 06327	03-Apr-14 (No. 217-01921)	Apr-15
Reference Probe ES30V3	SN: 3205	30-Dec-13 (No. ES3-3205_Dec13)	Dec-14
DAE4	SN: 601	30-Apr-14 (No. DAE4-601_Apr14)	Apr-15

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator P&S SMT-06	100005	04-Aug-09 (in house check Oct-13)	In house check: Oct-16
Network Analyzer HP 8753E	US37390585-54206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

Calibrated by:	Name: <b>Michael Weber</b>	Function: <b>Laboratory Technician</b>	Signature:
Approved by:	Name: <b>Katja Pokovic</b>	Function: <b>Technical Manager</b>	Signature:

Issued: July 11, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D835V2-4d172\_Jul14

Page 1 of 8

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- d) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.1 ± 6 %	0.94 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.39 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.23 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.55 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.03 W/kg ± 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.8 ± 6 %	1.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.50 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.58 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.63 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.30 W/kg ± 16.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	52.6 Ω - 2.0 jΩ
Return Loss	- 29.9 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	47.8 Ω - 4.3 jΩ
Return Loss	- 26.1 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.393 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	November 11, 2013

**DASY5 Validation Report for Head TSL**

Date: 10.07.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d172**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0,94 \text{ S/m}$ ;  $\epsilon_r = 41.1$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.22, 6.22, 6.22); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 56.39 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 3.59 W/kg


SAR(1 g) = 2.39 W/kg; SAR(10 g) = 1.55 W/kg

Maximum value of SAR (measured) = 2.81 W/kg

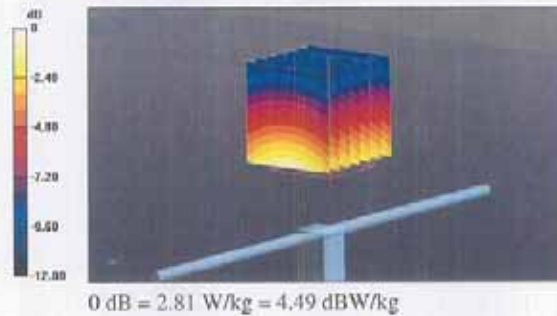



Impedance Measurement Plot for Head TSL

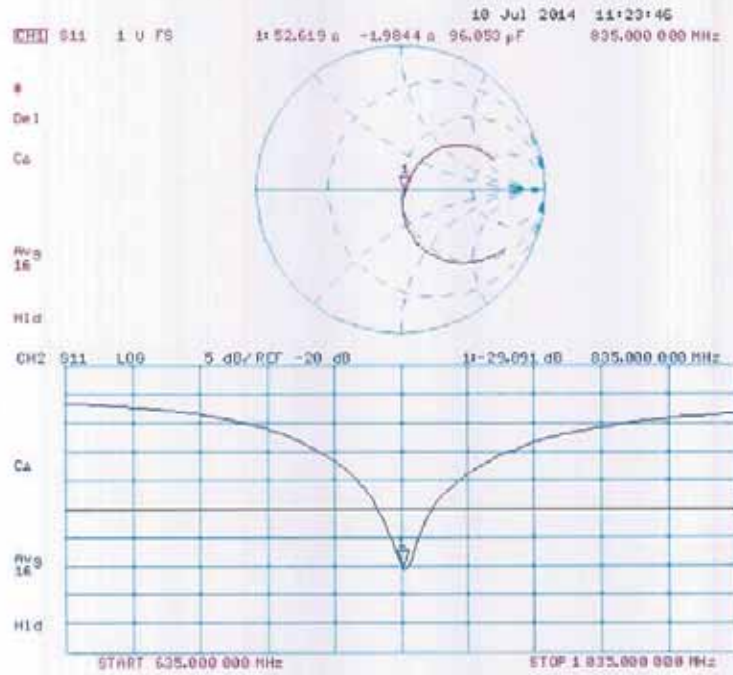

**DASY5 Validation Report for Body TSL**

Date: 09.07.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d172**


Communication System: UID 0 - CW; Frequency: 835 MHz  
 Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 1.02 \text{ S/m}$ ;  $\epsilon_r = 53.8$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

**DASY52 Configuration:**


- Probe: ES3DV3 - SN3205; ConvF(6.09, 6.09, 6.09); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)


**Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**

Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 55.24 V/m; Power Drift = -0.01 dB  
 Peak SAR (extrapolated) = 3.71 W/kg  
**SAR(1 g) = 2.5 W/kg; SAR(10 g) = 1.63 W/kg**  
 Maximum value of SAR (measured) = 2.92 W/kg

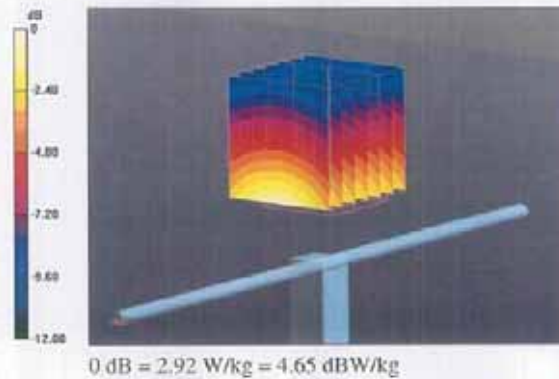

Impedance Measurement Plot for Body TSL

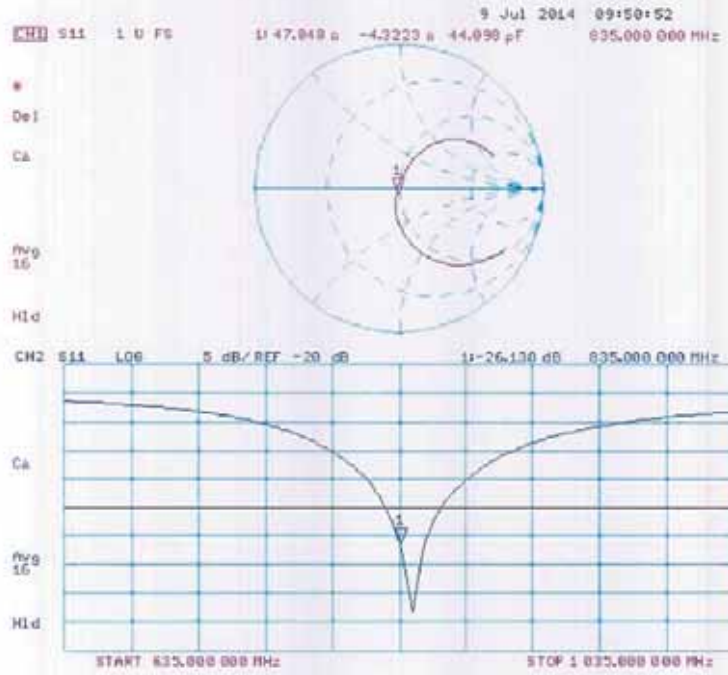

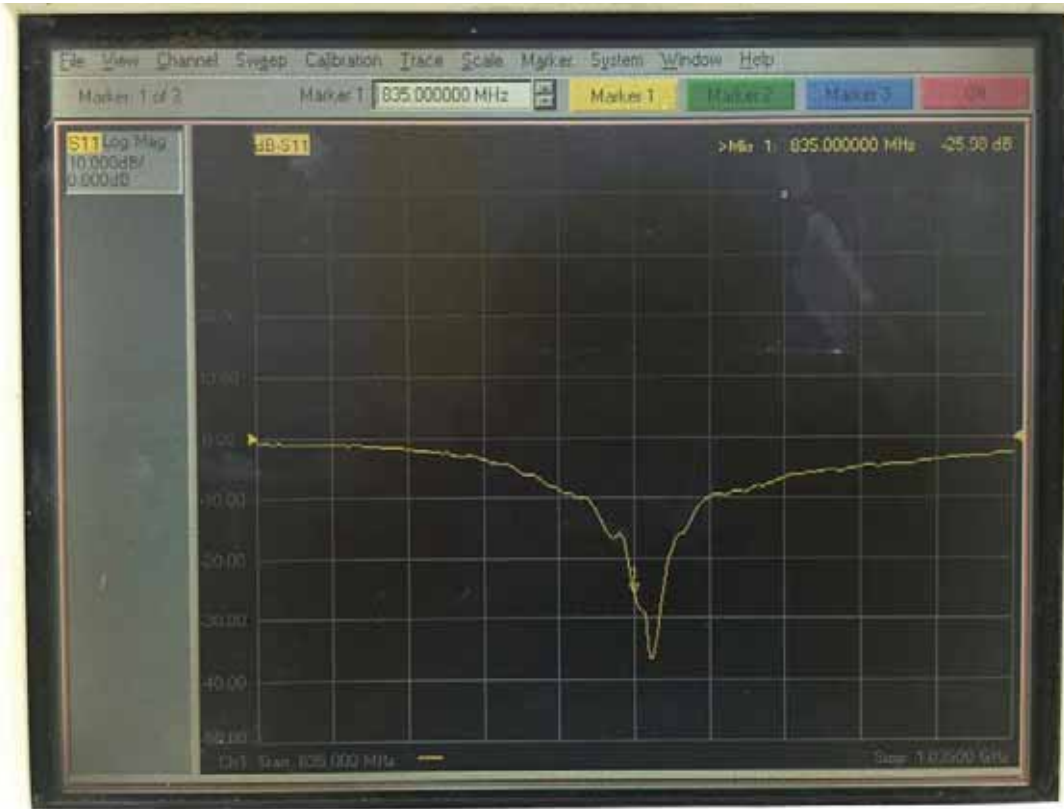

\* Justification for Extended SAR Dipole Calibrations

Instead of the typical annual calibration recommended by measurement standards, longer calibration intervals of up to three years may be considered when it is demonstrated that the SAR target, Impedance and return loss of a dipole have remain stable according to the following requirements.

KDB865664 requirements

- a) return loss : < -20 dB, within 20 % of previous measurement
- b) impedance: within 5 Ω from previous measurement.

Dipole Antenna	Head/Body	Date of Measurement	Freq. (MHz)	Return loss (dB)
D835V2 S/N-4d172	Body	July.10.2014	835	-26.1
			835	-25.9

< Dipole Antenna : D1950V3 – SN 1156 >

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client **One-Tech (Dymstec)**

Certificate No: D1950V3-1156\_Jul14

CALIBRATION CERTIFICATE																																															
Object	D1950V3 - SN: 1156																																														
Calibration procedure(s)	QA CAL-05.v9 Calibration procedure for dipole validation kits above 700 MHz																																														
Calibration date:	July 11, 2014																																														
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter EPM-442A</td> <td>GB37480704</td> <td>09-Oct-13 (No. 217-01827)</td> <td>Oct-14</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>US37292763</td> <td>09-Oct-13 (No. 217-01827)</td> <td>Oct-14</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>MY41092317</td> <td>09-Oct-13 (No. 217-01828)</td> <td>Oct-14</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: 5058 (20k)</td> <td>03-Apr-14 (No. 217-01918)</td> <td>Apr-15</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 5047.2 / 06327</td> <td>03-Apr-14 (No. 217-01921)</td> <td>Apr-15</td> </tr> <tr> <td>Reference Probe ES3DV3</td> <td>SN: 3205</td> <td>30-Dec-13 (No. ES3-3205_Dec13)</td> <td>Dec-14</td> </tr> <tr> <td>DAE4</td> <td>SN: 601</td> <td>30-Apr-14 (No. DAE4-601_Apr14)</td> <td>Apr-15</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>RF generator R&amp;S SMT-06</td> <td>100005</td> <td>04-Aug-99 (in house check Oct-13)</td> <td>In house check: Oct-16</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>US37390585 S4206</td> <td>18-Oct-01 (in house check Oct-13)</td> <td>In house check: Oct-14</td> </tr> </tbody> </table>				Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14	Power sensor HP 8481A	US37292763	09-Oct-13 (No. 217-01827)	Oct-14	Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01828)	Oct-14	Reference 20 dB Attenuator	SN: 5058 (20k)	03-Apr-14 (No. 217-01918)	Apr-15	Type-N mismatch combination	SN: 5047.2 / 06327	03-Apr-14 (No. 217-01921)	Apr-15	Reference Probe ES3DV3	SN: 3205	30-Dec-13 (No. ES3-3205_Dec13)	Dec-14	DAE4	SN: 601	30-Apr-14 (No. DAE4-601_Apr14)	Apr-15	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16	Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																																												
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14																																												
Power sensor HP 8481A	US37292763	09-Oct-13 (No. 217-01827)	Oct-14																																												
Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01828)	Oct-14																																												
Reference 20 dB Attenuator	SN: 5058 (20k)	03-Apr-14 (No. 217-01918)	Apr-15																																												
Type-N mismatch combination	SN: 5047.2 / 06327	03-Apr-14 (No. 217-01921)	Apr-15																																												
Reference Probe ES3DV3	SN: 3205	30-Dec-13 (No. ES3-3205_Dec13)	Dec-14																																												
DAE4	SN: 601	30-Apr-14 (No. DAE4-601_Apr14)	Apr-15																																												
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																																												
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16																																												
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14																																												
Calibrated by:	Name Michael Weber	Function Laboratory Technician	Signature 																																												
Approved by:	Name Katja Pokovic	Function Technical Manager	Signature 																																												
			Issued: July 14, 2014																																												
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																																															

Certificate No: D1950V3-1156\_Jul14

Page 1 of 8

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- d) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1950 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.3 ± 6 %	1.43 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.5 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	41.3 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.44 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.5 W/kg ± 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.3 ± 6 %	1.56 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.97 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	39.1 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.20 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.6 W/kg ± 16.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	49.1 $\Omega$ - 1.3 j $\Omega$
Return Loss	- 36.2 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	45.5 $\Omega$ - 1.5 j $\Omega$
Return Loss	- 26.1 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.198 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	September 23, 2009



**DASY5 Validation Report for Head TSL**

Date: 11.07.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1950 MHz; Type: D1950V3; Serial: D1950V3 - SN: 1156**

Communication System: UID 0 - CW; Frequency: 1950 MHz

Medium parameters used:  $f = 1950$  MHz;  $\sigma = 1.43$  S/m;  $\epsilon_r = 39.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

**DASY52 Configuration:**

- Probe: ES3DV3 - SN3205; ConvF(4.92, 4.92, 4.92); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 100.3 V/m; Power Drift = 0.01 dB


Peak SAR (extrapolated) = 19.1 W/kg

**SAR(1 g) = 10.5 W/kg; SAR(10 g) = 5.44 W/kg**

Maximum value of SAR (measured) = 13.4 W/kg

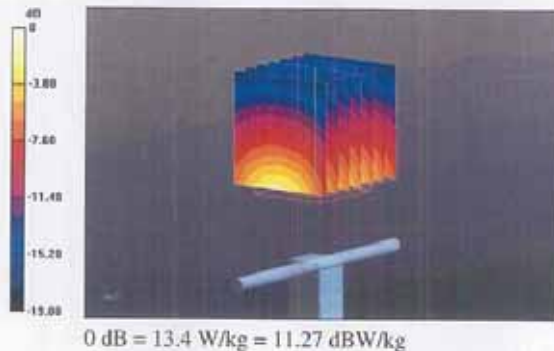

Impedance Measurement Plot for Head TSL

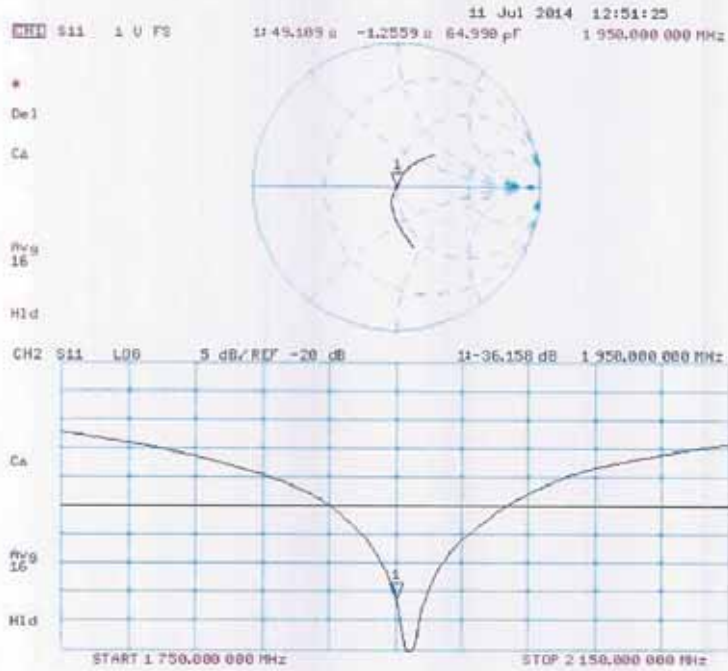

**DASY5 Validation Report for Body TSL**

Date: 11.07.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1950 MHz; Type: D1950V3; Serial: D1950V3 - SN: 1156**


Communication System: UID 0 - CW; Frequency: 1950 MHz  
 Medium parameters used;  $f = 1950 \text{ MHz}$ ;  $\sigma = 1.56 \text{ S/m}$ ;  $\epsilon_r = 52.3$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

**DASY52 Configuration:**


- Probe: ES3DV3 - SN3205; ConvF(4.78, 4.78, 4.78); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)


**Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**

Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 94.21 V/m; Power Drift = 0.01 dB  
 Peak SAR (extrapolated) = 17.6 W/kg  
**SAR(1 g) = 9.97 W/kg; SAR(10 g) = 5.2 W/kg**  
 Maximum value of SAR (measured) = 12.7 W/kg

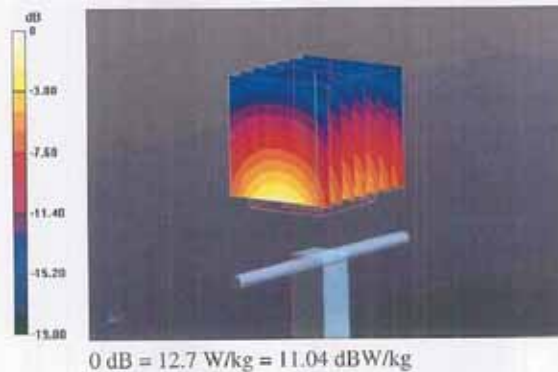

Impedance Measurement Plot for Body TSL

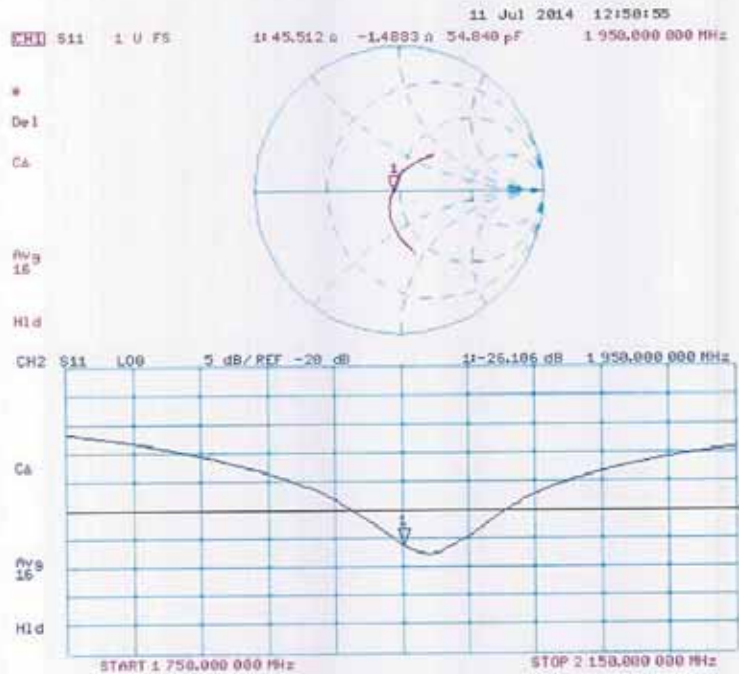

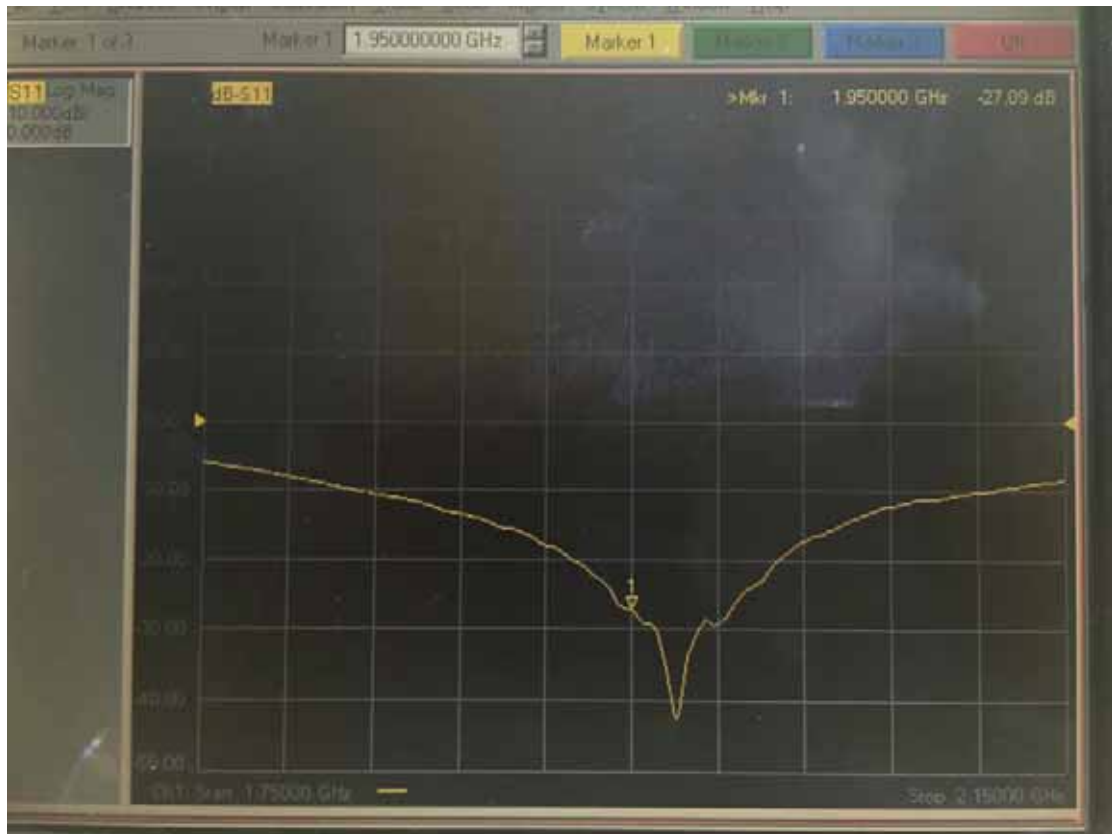

\* Justification for Extended SAR Dipole Calibrations

Instead of the typical annual calibration recommended by measurement standards, longer calibration intervals of up to three years may be considered when it is demonstrated that the SAR target, Impedance and return loss of a dipole have remain stable according to the following requirements.

KDB865664 requirements

- a) return loss : < -20 dB, within 20 % of previous measurement
- b) impedance: within 5 Ω from previous measurement.

Dipole Antenna	Head/Body	Date of Measurement	Freq. (MHz)	Return loss (dB)
D1950V3 S/N-1156	Body	July.11.2014	1 950	-26.1
			1 950	-27.0

< Dipole Antenna : D2450V2 – SN 923 >

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland

S Schweizerischer Kalibrierdienst  
S Service suisse d'étalonnage  
C Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)      Accreditation No.: **SCS 108**  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Client **One-Tech (Dymstec)**

Certificate No: **D2450V2-923\_Nov13**

CALIBRATION CERTIFICATE

Object:	D2450V2 - SN: 923
Calibration procedure(s):	QA CAL-05.v9 Calibration procedure for dipole validation kits above 700 MHz
Calibration date:	November 13, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	US37292783	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01829)	Oct-14
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-13 (No. 217-01738)	Apr-14
Type-N mismatch combination	SN: 5047.3 / 06327	04-Apr-13 (No. 217-01739)	Apr-14
Reference Probe ES3DV3	SN: 3205	28-Dec-12 (No. ES3-3205_Dec12)	Dec-13
DAE4	SN: 601	25-Apr-13 (No. DAE4-601_Apr13)	Apr-14

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-15
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

	Name	Function	Signature
Calibrated by:	Israe El-Nasouq	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: November 13, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D2450V2-923\_Nov13

Page 1 of 8

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- d) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.B.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.7 ± 6 %	1.84 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.2 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.4 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.12 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.4 W/kg ± 16.5 % (k=2)

### Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.1 ± 6 %	2.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.9 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	50.6 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.98 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.7 W/kg ± 16.5 % (k=2)



**Appendix**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	53.8 Ω + 0.4 jΩ
Return Loss	- 26.8 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	49.8 Ω + 1.9 jΩ
Return Loss	- 34.1 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.159 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	September 26, 2013

**DASY5 Validation Report for Head TSL**

Date: 13.11.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 923**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.84$  S/m;  $\epsilon_r = 39.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.52, 4.52, 4.52); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 98.97 V/m; Power Drift = 0.07 dB


Peak SAR (extrapolated) = 27.5 W/kg

**SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.12 W/kg**

Maximum value of SAR (measured) = 16.8 W/kg

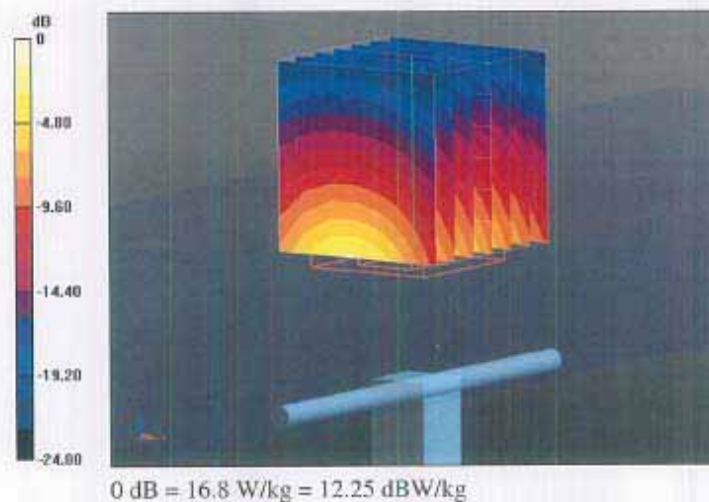

Impedance Measurement Plot for Head TSL

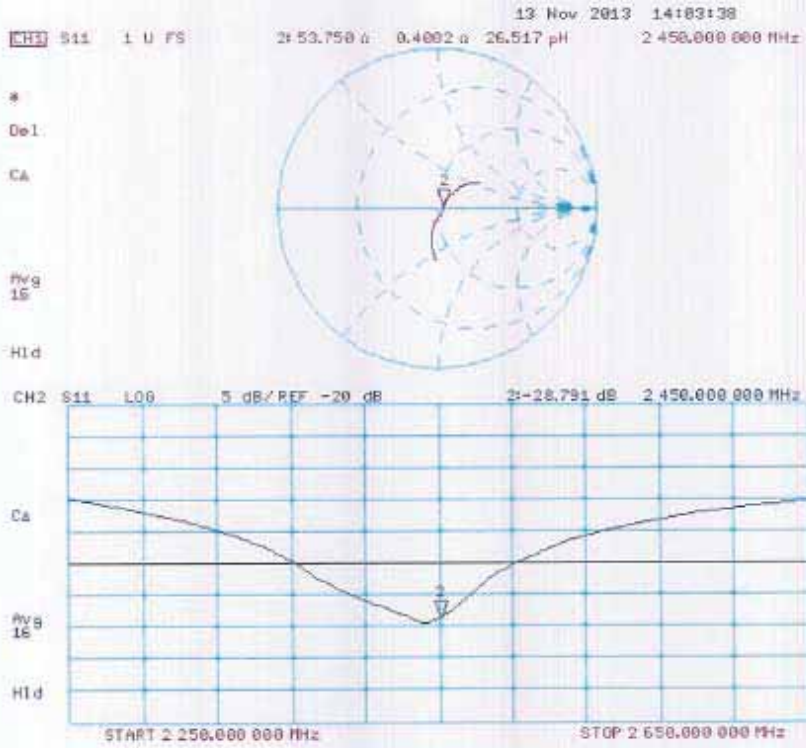

**DASY5 Validation Report for Body TSL**

Date: 13.11.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 923**


Communication System: UID 0 - CW; Frequency: 2450 MHz  
 Medium parameters used:  $f = 2450$  MHz;  $\sigma = 2.02$  S/m;  $\epsilon_r = 52.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Phantom section: Flat Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY52 Configuration:**

- Probe: ES3DV3 - SN3205; ConvF(4.42, 4.42, 4.42); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)


**Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm  
 Reference Value = 94.525 V/m; Power Drift = -0.09 dB  
 Peak SAR (extrapolated) = 27.0 W/kg  
**SAR(1 g) = 12.9 W/kg; SAR(10 g) = 5.98 W/kg**  
 Maximum value of SAR (measured) = 17.0 W/kg

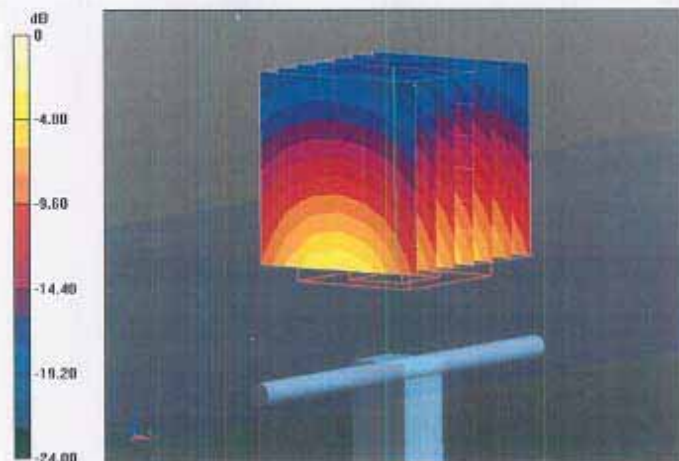

0 dB = 17.0 W/kg = 12.30 dBW/kg

Impedance Measurement Plot for Body TSL

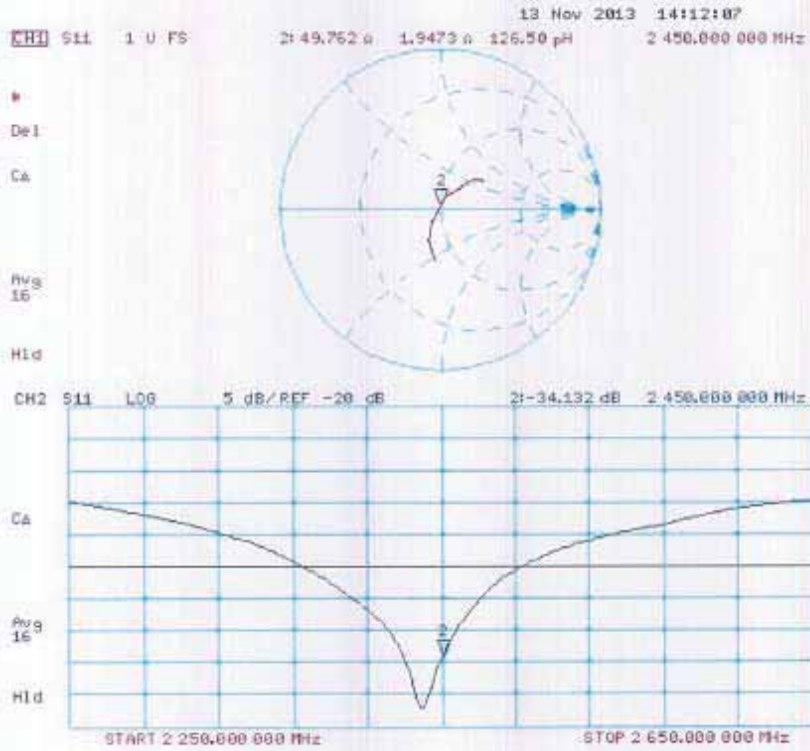

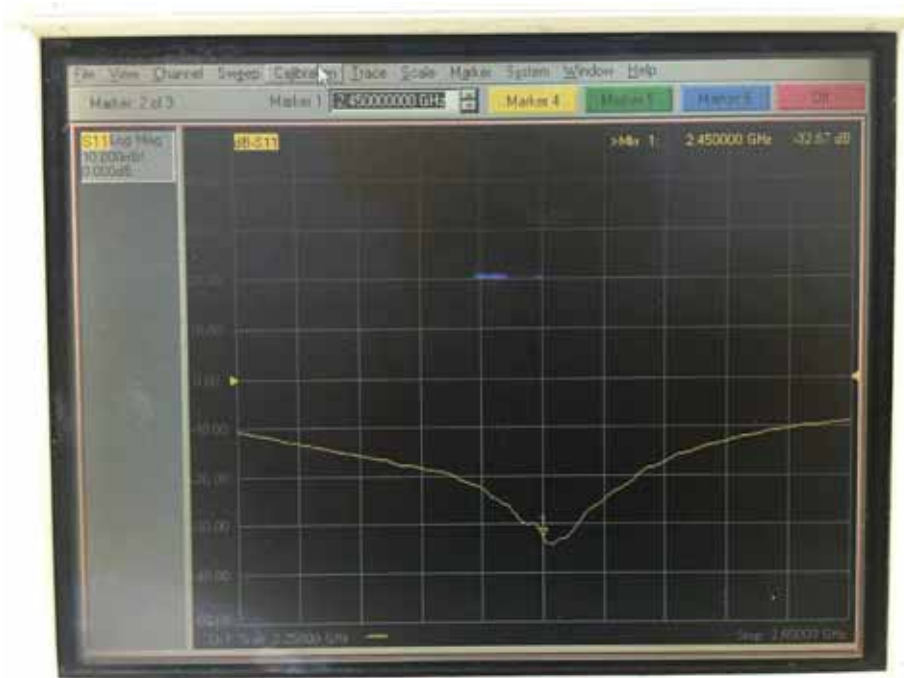

\* Justification for Extended SAR Dipole Calibrations

Instead of the typical annual calibration recommended by measurement standards, longer calibration intervals of up to three years may be considered when it is demonstrated that the SAR target, Impedance and return loss of a dipole have remain stable according to the following requirements.

KDB865664 requirements

- c) return loss : < -20 dB, within 20 % of previous measurement
- d) impedance: within 5 Ω from previous measurement.

Dipole Antenna	Head/Body	Date of Measurement	Freq. (MHz)	Return loss (dB)
D2450V2 S/N-923	Body	Mar.20.2014	2 450	-34.1
			2 450	-32.6

< Dielectric Probe : DAK-3.5 SN 1140 >

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8904 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client **One-Tech (Dymstec)**

Certificate No: **OCP-DAK3.5-1140\_Nov14**

**CALIBRATION CERTIFICATE**

Object: **DAK-3.5 - SN: 1140**

Calibration procedure(s): **QA CAL-33.v2  
Calibration of dielectric parameter probes**

Calibration date: **November 11, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
OCP DAK-3.5 (weighted)	SN: 1203	7-Oct-14 (OCP-DAK3.5-1203_Oct14)	Oct-15
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Rohde & Schwarz ZVA50	T0170	10-Jun-14 (in house check Jun-14)	Jun-15
Digital Thermometer DTM3000	2148	04-Apr-14 (DTM-2148_Apr14)	Apr-15
Methanol 99.9% Type 34860	SZBC143SV	19-Aug-14 (bottle opened, check Aug-14)	Apr-15
Head Liquid, HSL U12	121204-1	15-Apr-14 (in house check Apr-14)	Apr-15
0.1 mol/L NaCl solution Type 35275	SZBA2560	15-Apr-14 (in house check Apr-14)	Apr-15
0.05 mol/L NaCl solution	120427-1	15-Apr-14 (in house check Apr-14)	Apr-15
Head Gel, SL AGH U07 AA	120423	15-Apr-14 (in house check Apr-14)	Apr-15
Solid Substrate	AK9	15-Apr-14 (in house check Apr-14)	Apr-15

	Name	Function	Signature
Calibrated by:	Ferenc Muranyi	External Expert	
Approved by:	Katja Pokovic	Technical Manager	

Issued: November 11, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**References**

- [1] IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- [2] IEC 62209 – 1, "Specific Absorption Rate (SAR) in the frequency range of 300 MHz to 3 GHz – Measurement Procedure, Part 1: Hand-held mobile wireless communication devices", February 2005
- [3] IEC 62209-2 Ed.1, "Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices – Human models, Instrumentation, and Procedures Part 2: Procedure to determine the specific absorption rate (SAR) for mobile wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- [4] A. P. Gregory and R. N. Clarke, "NPL Report MAT 23", January 2012  
Tables of the Complex Permittivity of Dielectric Reference Liquids at Frequencies up to 5 GHz
- [5] Agilent 85070E Dielectric Probe Kit, Technical Overview, document 5989-0222EN, October 2006
- [6] A. Toropainen et al, "Method for accurate measurement of complex permittivity of tissue equivalent liquids", Electronics Letters 36 (1) 2000 pp32-34
- [7] J. Hilland, "Simple sensor system for measuring the dielectric properties of saline solutions", Meas. Sci. Technol. 8 pp901–910 (1997)
- [8] K. Nörtemann, J. Hilland and U. Kaatze, "Dielectric Properties of Aqueous NaCl Solutions at Microwave Frequencies", J. Phys. Chem. A 101 pp6864-6869 (1997)
- [9] R. Buchner, G. T. Hefter and Peter M. May, "Dielectric Relaxation of Aqueous NaCl Solutions", J. Phys. Chem. A 103 (1) (1999)

**Description of the dielectric probe**

Dielectric probes are used to measure the dielectric parameters of tissue simulating media in a wide frequency range. The complex permittivity  $\epsilon_r = (\epsilon'/\epsilon_0) - j(\epsilon''/\epsilon_0)$  is determined from the S parameters measured with a vector network analyzer (VNA) with software specific to the probe type. The parameters of interest e.g. in standards [1, 2, 3] and for other applications are presented are calculated as follows:

(Relative) permittivity  $\epsilon'$  (real part of  $\epsilon_r = (\epsilon'/\epsilon_0) - j(\epsilon''/\epsilon_0)$  where  $\epsilon_0 = 8.854 \text{ pF/m}$  is the permittivity in free space)

Conductivity  $\sigma = 2 \pi f \epsilon'' \epsilon_0$ ,

Loss Tangent =  $(\epsilon''/\epsilon')$

The OCP (open ended coaxial) is a cut off section of 50 Ohm transmission line, similar to the system described in [1, 2, 3, 5], used for contact measurement. The material is measured either by touching the probe to the surface of a solid/gelly or by immersing it into a liquid media. The electromagnetic fields at the probe end fringe into the material to be measured, and its parameters are determined from the change of the  $S_{11}$  parameters. With larger diameter of the dielectrics, the probe can be used down to lower frequencies.

The flange surrounding the active area shapes the near field similar to a semi-infinite geometry and is inserted fully into the measured lossy liquid.



The probe is connected with a phase and amplitude stable cable to a VNA which is then calibrated with Open, Short and a Liquid with well-known parameters. All parts in the setup influencing the amplitude and phase of the signal are important and shall remain stable.

**Handling of the item**

Before usage, the active probe area has to be cleaned from any material residuals potentially contaminating the reference standards. The metal and dielectric surface must be protected to keep the precision of the critical mechanical dimensions. The connector and cable quality are critical; any movements between calibration and measurement shall be avoided. The temperature must be stable and must not differ from the material temperature.

**Methods Applied and Interpretation of Parameters**

The calibration of the dielectric probe system is done in the steps described below for the desired frequency range and calibration package (SAR/MRI liquids, Semi-solid/solid material). Because the standard calibration in step 3 is critical for the results in steps 4 to 8, the sequence 3 to 8 is repeated 3 times. As a result, the result from these 3 sets is represented.

1. Configuration and mechanical / optical status.
2. Measurement resolution is 5 MHz from 10 to 300 MHz, 50 MHz from 300 to 6000 MHz and 250 MHz from 6 to 20 GHz.
3. Standard calibration uses Air / Short / Liquid. 1 liter liquid quantity is used to reduce the influence the reflections. The liquid type is selected depending on the lowest frequency and probe diameter:  
 DAK-1.2, DAK-3.5, Agilent OCP: de-ionized water (approx. 22 °C)  
 DAK-12: saline solution with static conductivity 1 S/m (approx. 22 °C)  
 NPL OCP: pure ethanol (approx. 22 °C)
4. The cable used in the setup stays in a fixed position, i.e. the probe is fixed and measuring from the top in an angle of typ. 20° from the vertical axis. For DAK and Agilent probes, the refresh function (air standard) is used previous to the individual measurements in order to compensate for possible deviations from cable movements. After insertion of the probe into a liquid, the possible air bubbles are removed from the active surface.
5. Measurement of multiple shorts if not already available from the calibration in the previous step (NPL). Evaluation of the deviation from the previous calibration short with graphical representation of the complex quantities and magnitude over the frequency range. The specific probe short will be used if provided. This assessment shows ability to define a short circuit at the end of the probe for the VNA calibration in the setup which is essential at high frequencies and depends on the probe surface quality.
6. Measurement of validation liquids in a quantity of 1 liter at well defined temperature. Evaluation of the deviations from the target. The targets base on traceable data from reference sources. The deviation of the measurement is graphically presented for permittivity and conductivity (for lossy liquids) or loss tangent (for low losses at low frequencies).
7. Measurement of lossy liquids in a quantity of 1 liter at well defined temperature. Head tissue simulating liquid or saline solution with 0.5 S/m static conductivity are representative. The target data base on traceable data from reference sources or from multiple measurements with precision reference probes or different evaluations such as transmission line or slotted line methods. Evaluation of the deviation from the target and graphical representation for permittivity and conductivity over the frequency range
8. Semi-solid / solid material calibration:  
 Measurements of an elastic lossy broadband semi-solid gel with parameters close to the head tissue target. Measurements of a planar very low loss solid microwave-substrate. The average of 4 measurements of the same sample at different location is shown as a single result. The deviation of the permittivity and conductivity from the reference data is evaluated.  
 Measurements of a planar very low loss solid microwave-substrate. The average of 4 measurements of the same sample at different location is shown as a single result. The relative deviation of the permittivity and the absolute deviation of the loss tangent is evaluated.  
 The targets base on multiple measurements (on the same material batch at identical temperature) on convex and planar surfaces with precision reference OCP.

- The measurement on semi-solid / solid materials is sensitive to the quality and planarity of the probe contact area, such as air gaps due to imperfect probes (resulting lower permittivity values).
9. Table for the probe uncertainty: The uncertainty of the probe depending on probe type, size, material parameter range and frequency is given in a table. It represents the best measurement capability of the specific probe but does not include the material (deviation from the target values).
  10. Appendix with detailed results of all measurements with the uncertainties for the specific measurement. In addition to the probe uncertainty (see above), it includes the uncertainty of the reference material used for the measurement. A set of results from independent calibrations represents the capability of the setup and the lossy materials used, including the precision of the measured material and the influence of temperature deviations. Temperature and operator influence was minimized and gives a good indication of the achievable repeatability of a measurement.
  11. Summary assessment of the measured deviations and detailed comments if not typical for the probe type.

**Dielectric probe identification and configuration data**

Item description

Probe type	OCP Open-ended coaxial probe
Probe name	SPEAG Dielectric Assessment Kit DAK-3.5
Type No	SM DAK 040 CA
Serial No	1140
Description	Open-ended coaxial probe with flange Flange diameter: 19.0 mm Dielectric diameter: 3.5 mm Material: stainless steel
Connector 1	PC 3.5 pos.
Software version	DAK Measurement Solver 1.12.356.11 Calibration Type: Air / short / water (set to measured water temp.) Probe type: "DAK3.5" (software setting)
Further settings	VNA bandwidth setting: 50 Hz

Accessories

Cable	Huber & Suhner Sucoflex 404, SN: 1695, length 1 m, PC3.5 neg. – PC3.5 neg.
Short	DAK-3.5 shorting block, type SM DAK 200 BA Contact area covered with cleaned Cu stripe

Additional items used during measurements

Adapter 1	PC3.5 pos. – PC2.4 (VNA side)
Adapter 2	PC3.5 pos. – PC3.5 neg. (probe side)

**Notes**

- Before the calibration, the connectors of the probe and cable were inspected and cleaned.
- Probe visual inspection: according to requirements
- Short inspection: according to the requirements

**Probe Uncertainty**

The following tables provide material and frequency specific uncertainties (k=2) for the dielectric probe. The values in the tables represent the measurement capability for the probe when measuring a material in the indicated parameter range. They include all uncertainties of

- probe system
- possible systematic errors due to the design
- calibration
- temperature differences during the calibration and measurements, as described,
- VNA noise

Apart from the material used for the calibration (de-ionized water), material uncertainties of the reference materials used during the measurement in Appendix A are not included in these tables.

DAK-3.5				
Permittivity range		Frequency range	(sigma / LT range)	Unc. (k=2)
1 – 15		10 MHz - 20 MHz		---
		20 MHz - 200 MHz		---
		200 MHz - 3 GHz	LT < 0.1	2.4%
		3 GHz - 6 GHz	LT < 0.1	2.0%
		6 GHz - 20 GHz	LT < 0.1	2.1%
10 – 40		10 MHz - 20 MHz		---
		20 MHz - 200 MHz		---
		200 MHz - 3 GHz	sigma : 1 – 10 S/m	1.9%
		3 GHz - 6 GHz	sigma : 1 – 10 S/m	2.3%
		6 GHz - 20 GHz	sigma > 10 S/m	3.5%
35 – 100		10 MHz - 20 MHz		---
		20 MHz - 200 MHz		---
		200 MHz - 3 GHz	sigma : 1 – 10 S/m	1.8%
		3 GHz - 6 GHz	sigma : 1 – 10 S/m	1.9%
		6 GHz - 20 GHz	sigma > 10 S/m	2.4%
Conductivity range (S/m)				
		Frequency range	(epsilon / LT range)	Unc. (k=2)
1 – 10		10 MHz - 20 MHz		---
		20 MHz - 200 MHz		---
		200 MHz - 3 GHz	eps : 35 - 100	2.7%
		3 GHz - 6 GHz	eps : 35 - 100	3.0%
		6 GHz - 20 GHz	eps : 10 - 40	3.0%
Loss tangent range				
		Frequency range	(epsilon / LT range)	Unc. (k=2)
< 0.1		10 MHz - 20 MHz		---
		20 MHz - 200 MHz		---
		200 MHz - 3 GHz	eps : 1 - 15	0.03
		3 GHz - 6 GHz	eps : 1 - 15	0.03
		6 GHz - 20 GHz	eps : 1 - 15	0.03

**Calibration Results**

Uncertainty limits ( $k=2$ ) for the material measurements in the figures of Appendix A are represented with red dashed lines. These uncertainties contain - in addition to probe uncertainty - the uncertainty of the material target parameter determination.

The measurements show the results obtained from independent calibrations for the same material. The differences between the individual measurement curves give therefore an indication for the obtainable repeatability and shall lie within the uncertainties stated in the tables.

*Materials for DAK-3.5 calibration:*

*Appendix A with curves for Methanol, HSL, and 0.05 mol/L NaCl solution (200 MHz - 6 GHz, optional 20 GHz), HS gel and low loss solid substrate are optional.*

**Appendix A: Detailed Results**

**A.1 Probe appearance and calibration sequence**

**A.1.1 Appearance**

The OCP appearance is fully according to the expectations:

- the flange surface is intact

**A.1.2 Calibration sequence**

The following sequence was repeated 3 times in the low frequency range from 200 – 300 MHz in 5 MHz steps and in the high frequency range from 300 to 6000 MHz in 50 MHz steps, and from 6 GHz to 20 GHz in 250 MHz steps.

- Air
- Short 1 short, then immediate verification with a second short (with eventual repetition)
- Water De-ionized water, temperature measured and set in the software (for DAK-12 0.1 mol/L saline solution, temperature measured and set in the software)
- Methanol Pure methanol, temperature measured and set in the software
- Liquids Measurement of further liquids (e.g. Head tissue simulating liquid and 0.05 mol/l saline)
- Cleaning Probe washed with water and isopropanol at the end of the sequence.
- Shorts 4 additional separate short measurements to determine the deviation from the original
- Refresh Refresh with Air
- Solid 4 separate solid low loss planar substrate measurements to determine one average (optional)
- Semisolid 4 separate head gel measurements on fresh intact surface to determine one average (optional)
- Cleaning Probe washed with water and isopropanol at the end of the sequence

Evaluation of the additional shorts from the calibrated (ideal) short point at the left edge of the Smith Chart, represented as magnitude over the frequency range (fig. 2.1.x) and in polar representation (fig. 2.2.x).

Evaluation of the Liquid measurements and representation of the permittivity and conductivity deviation from their reference data at the measurement temperature. The results of each of the 3 calibrations is shown in the appendix for each material (fig. 3ff) in black, red, blue. The red dashed line shows the uncertainty of the reference material parameter determination.

Evaluation of the Semisolid measurements (optional) by representing the 3 average deviations (each resulting from the 4 separate measurements per set), equivalent to the liquid measurement. Representation of the permittivity and conductivity deviation from their reference data at the nominal temperature.

Evaluation of the Solid measurements (optional) by representing the 3 average deviations (each resulting from the 4 separate measurements per set), equivalent to the liquid measurement. Representation of the permittivity deviation from their reference data and the loss tangent at the nominal temperature.

**A.2 Short residual magnitudes**

After each of the 3 calibrations with a single short (as per the DAK software), 4 additional separate, short measurements were performed after the liquid measurements and evaluated from the S11 data. The residuals in the graphs represent the deviation from the ideal short point on the polar representation on the VNA screen.

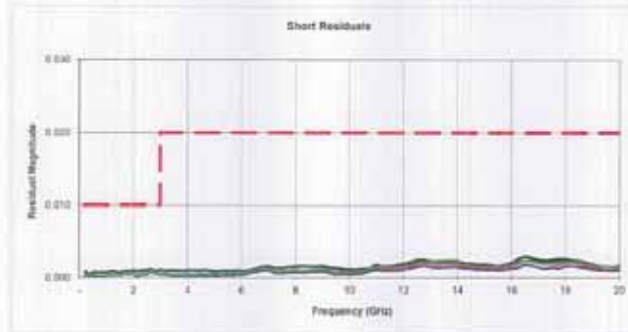


Fig. 2.1a Magnitude of the residual of the shorts, 200 MHz – 20 GHz, after calibration a)

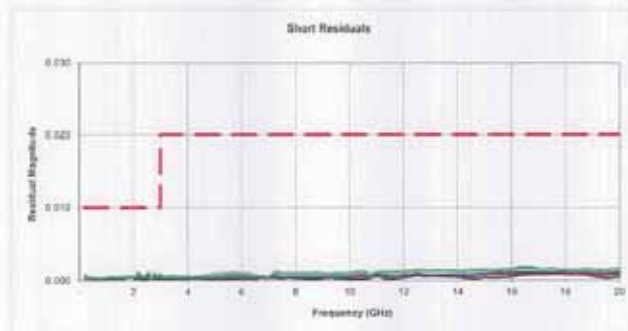


Fig. 2.1b Magnitude of the residual of the shorts, 200 MHz – 20 GHz, after calibration b)

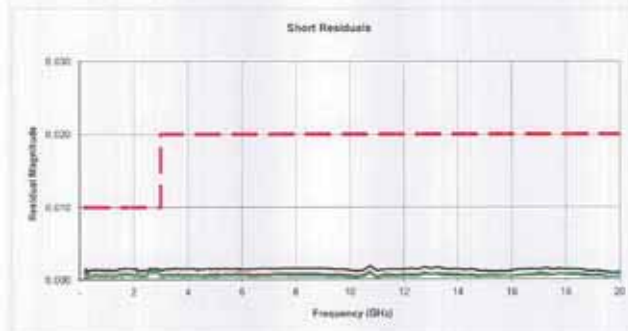


Fig. 2.1c Magnitude of the residual of the shorts, 200 MHz – 20 GHz, after calibration c)

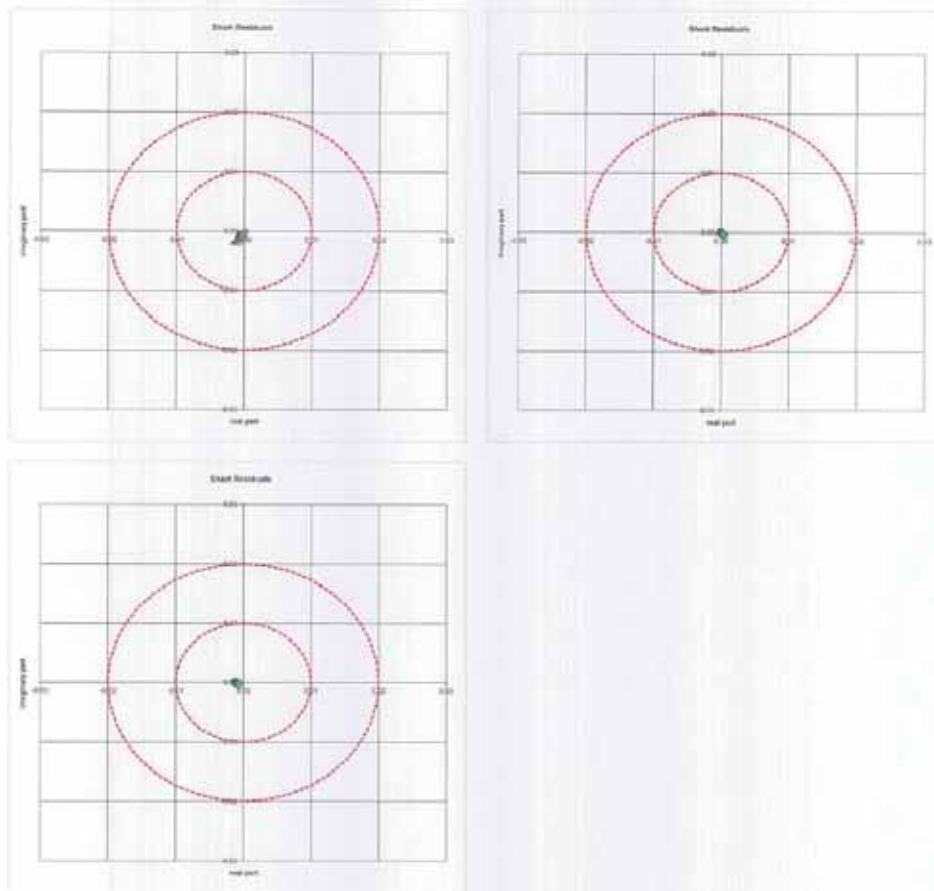


Fig. 2.2a-c Complex representation of the residuals of the shorts, 200 MHz - 20 GHz, after calibrations a)-b) in the top and c) in the bottom

All shorts have good quality. Some minor deviations might be visible from contact quality (left - right).

**A.3 Methanol**

Methanol (99.9% pure) was measured at a temperature of 22 +/- 2 °C. The liquid temperature was stabilized within 0.05 °C of the desired temperature. Deviations are presented relative to the nominal material parameters at this temperature, calculated from NPL data for this temperature.

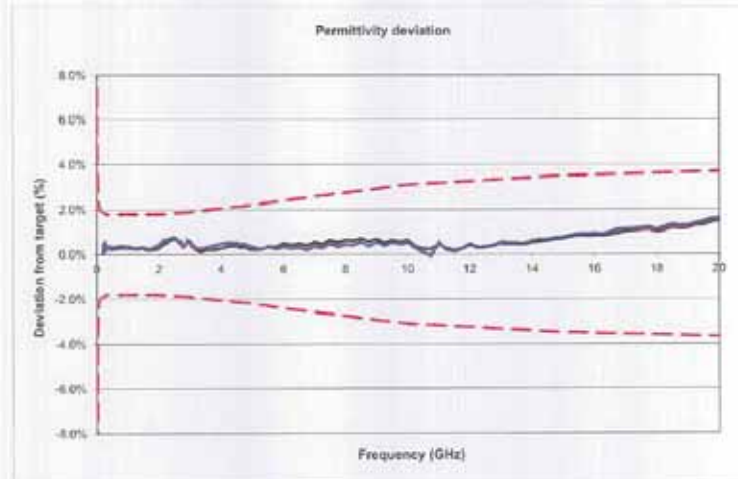


Fig. 3.1 Methanol permittivity deviation from target, 200 MHz – 20 GHz

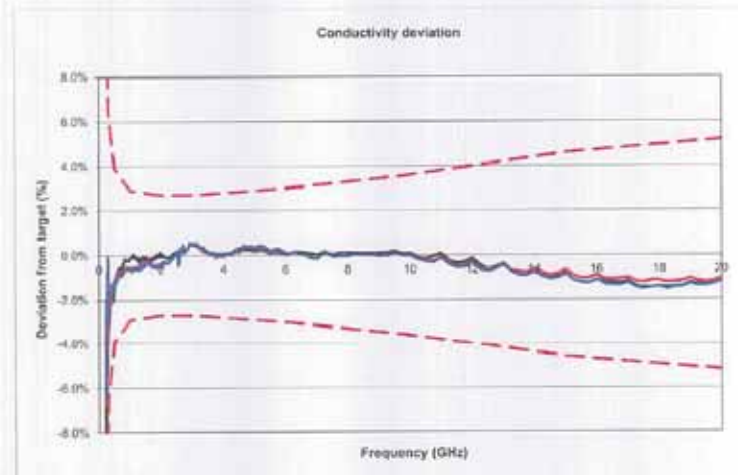


Fig. 3.2 Methanol conductivity deviation from target, 200 MHz – 20 GHz  
Conductivity error can be high at low frequencies due to the low absolute conductivity values



**A.4 Head Tissue**

Broadband head simulating liquid was measured at a temperature of 22 +/- 2 °C. The liquid temperature was stabilized within 0,05 °C of the desired temperature. Deviations are presented relative to the reference data for this material. Those parameters have been evaluated from multiple measurements on the used bath with precision reference OCP and further methods.

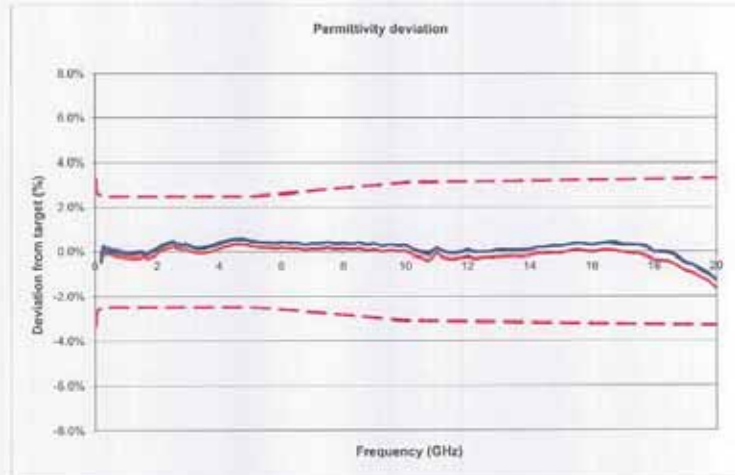


Fig. 4.1 HSL permittivity deviation from target, 200 MHz – 20 GHz

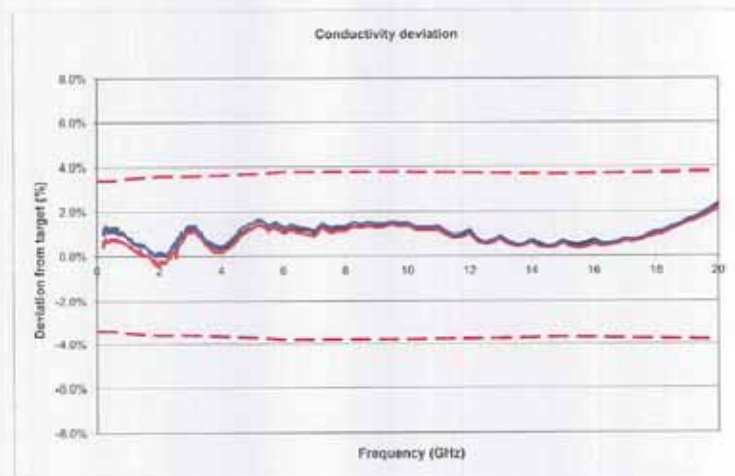


Fig. 4.2 HSL conductivity deviation from target, 200 MHz – 20 GHz

**A.5 0.05 mol/L NaCl solution**

0.05 mol/L NaCl / water solution has a static conductivity of 0.5 S/m, similar to MRI HCL (High Conductivity Liquid). It was measured at a temperature of 22 +/- 2 °C. The liquid temperature was stabilized within 0.05 °C of the desired temperature. Deviations are presented relative to the reference data for this material. These parameters have been derived from the theoretical model according to [7], matched to the measurements from reference probes and other sources. A quantity of 1 liter was used for the measurement.

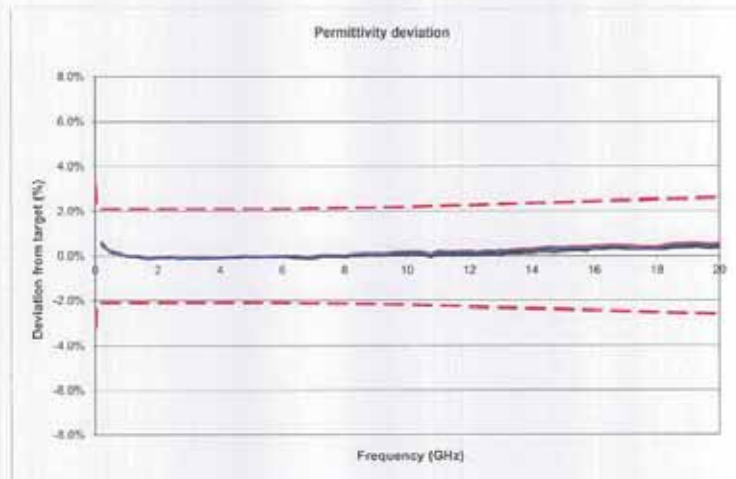


Fig. 5.1 0.05 mol/L solution permittivity deviation from target, 200 MHz – 20 GHz



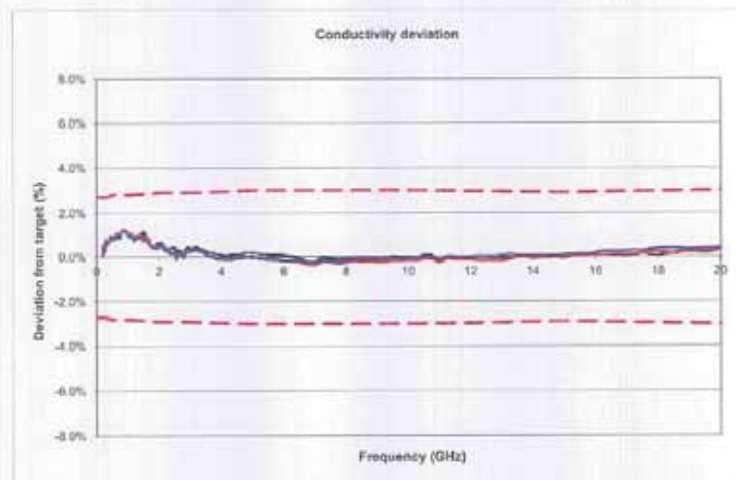


Fig. 5.2 0.05 mol/L solution conductivity deviation from target, 200 MHz – 20 GHz


**Appendix B: Nominal parameters of reference materials used for calibration**

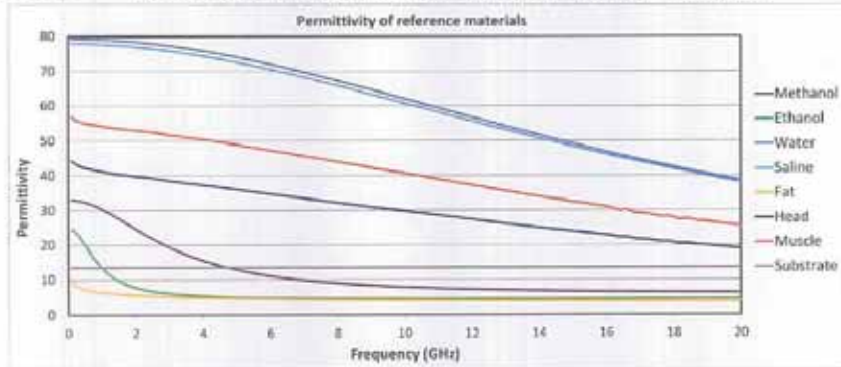

**Fig. B.1** Permittivity of reference materials

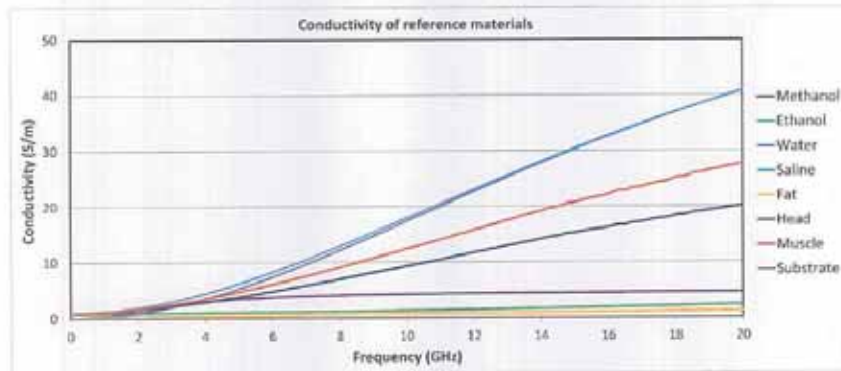

**Fig. B.2** Conductivity of reference materials

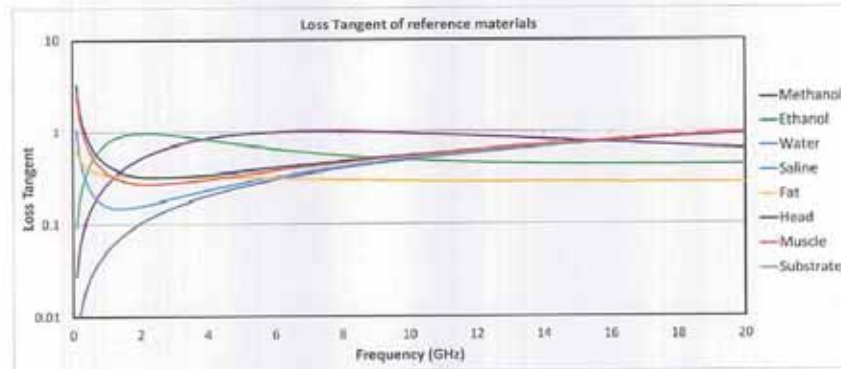

**Fig. B.3** Loss tangent of reference materials