



EX3DV4 – SN:3932

September 16, 2013

Probe EX3DV4

SN:3932

Manufactured: July 24, 2013
Calibrated: September 16, 2013

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)



EX3DV4- SN:3932

September 16, 2013

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3932

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.52	0.55	0.46	$\pm 10.1 \%$
DCP (mV) ^B	102.3	102.8	101.8	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	167.8	$\pm 3.0 \%$
		Y	0.0	0.0	1.0		179.9	
		Z	0.0	0.0	1.0		157.1	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



DASY/EASY - Parameters of Probe: EX3DV4 - SN:3932

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
750	41.9	0.89	10.36	10.36	10.36	0.20	1.35	± 12.0 %
835	41.5	0.90	9.89	9.89	9.89	0.29	1.02	± 12.0 %
900	41.5	0.97	9.67	9.67	9.67	0.21	1.33	± 12.0 %
1750	40.1	1.37	8.47	8.47	8.47	0.33	0.89	± 12.0 %
1900	40.0	1.40	8.21	8.21	8.21	0.12	1.47	± 12.0 %
2100	39.8	1.49	8.31	8.31	8.31	0.80	0.50	± 12.0 %
2300	39.5	1.67	7.75	7.75	7.75	0.43	0.70	± 12.0 %
2450	39.2	1.80	7.40	7.40	7.40	0.36	0.81	± 12.0 %
2600	39.0	1.96	7.16	7.16	7.16	0.44	0.78	± 12.0 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.



DASY/EASY - Parameters of Probe: EX3DV4 - SN:3932

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
750	55.5	0.96	9.92	9.92	9.92	0.21	1.47	± 12.0 %
835	55.2	0.97	9.92	9.92	9.92	0.30	1.12	± 12.0 %
900	55.0	1.05	9.67	9.67	9.67	0.51	0.79	± 12.0 %
1750	53.4	1.49	8.14	8.14	8.14	0.56	0.73	± 12.0 %
1900	53.3	1.52	7.80	7.80	7.80	0.42	0.80	± 12.0 %
2100	53.2	1.62	8.12	8.12	8.12	0.29	1.01	± 12.0 %
2300	52.9	1.81	7.57	7.57	7.57	0.59	0.68	± 12.0 %
2450	52.7	1.95	7.34	7.34	7.34	0.80	0.50	± 12.0 %
2600	52.5	2.16	7.08	7.08	7.08	0.80	0.50	± 12.0 %
5200	49.0	5.30	4.69	4.69	4.69	0.45	1.90	± 13.1 %
5300	48.9	5.42	4.48	4.48	4.48	0.45	1.90	± 13.1 %
5500	48.6	5.65	4.15	4.15	4.15	0.50	1.90	± 13.1 %
5600	48.5	5.77	4.07	4.07	4.07	0.45	1.90	± 13.1 %
5800	48.2	6.00	4.19	4.19	4.19	0.55	1.90	± 13.1 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.



EX3DV4- SN:3932

September 16, 2013

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

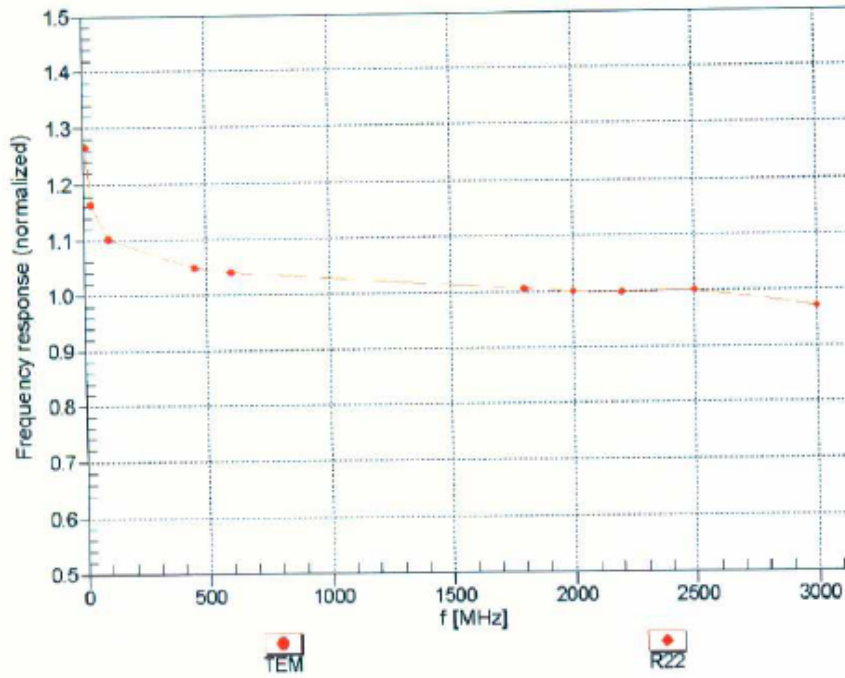


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

EX3DV4-SN:3932



September 16, 2013

Receiving Pattern (ϕ), $\theta = 0^\circ$

f=600 MHz,TEM

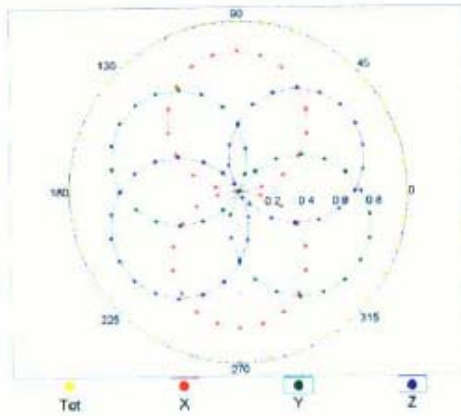

f=1800 MHz,R22

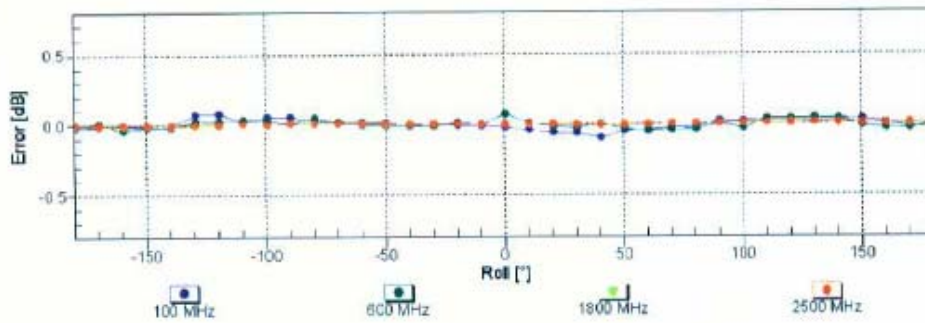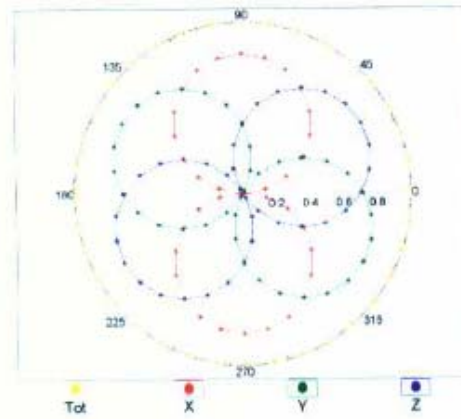



Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)



EX3DV4- SN:3932

September 16, 2013

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f = 900 \text{ MHz}$)

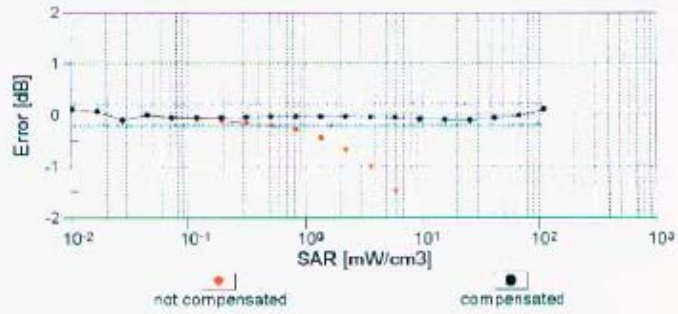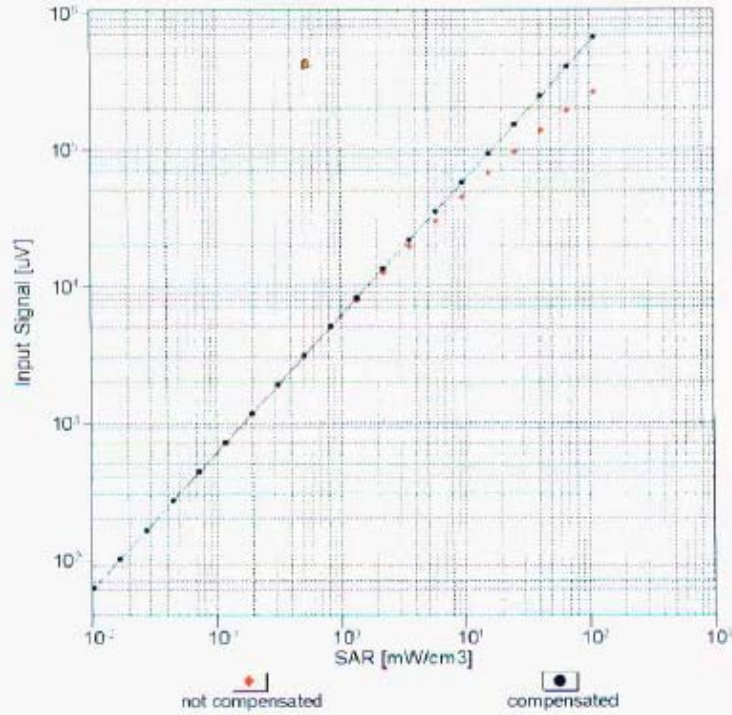


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)



EX3DV4- SN:3932

September 16, 2013

Conversion Factor Assessment

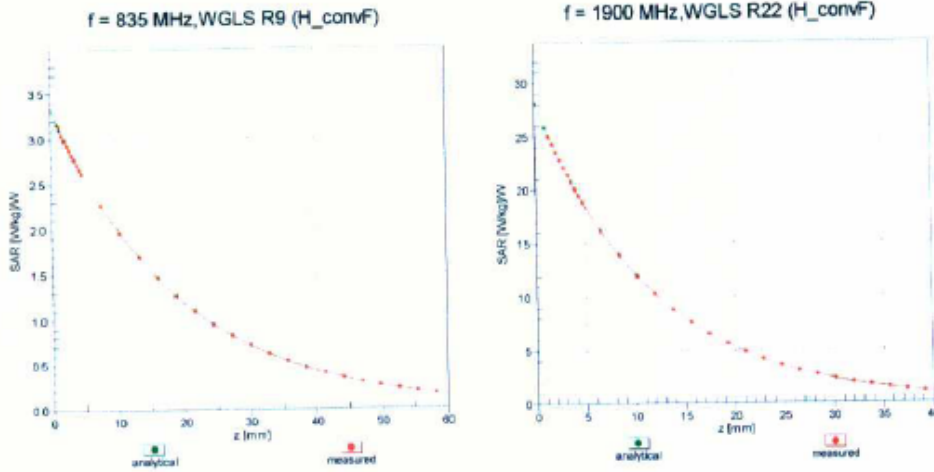

Deviation from Isotropy in Liquid Error (ϕ, θ), f = 900 MHz

