

RF Exposure Lab

802 N. Twin Oaks Valley Road, Suite 105 • San Marcos, CA 92069 • U.S.A.

TEL (760) 471-2100 • FAX (760) 471-2121

<http://www.rfexposurelab.com>

CERTIFICATE OF COMPLIANCE SAR EVALUATION

DeLorme
2 DeLorme Drive
Yarmouth, ME 04096

Dates of Test: February 25-26, 2015
Test Report Number: SAR.20150208
Revision B

| | |
|------------------------------|--|
| FCC ID: | Q639603N & T7V1315 |
| IC Certificate: | 4629A-9603N & 216Q-1315 |
| Model(s): | INRCH25 |
| Test Sample: | Engineering Unit Same as Production |
| Serial No.: | 300434060775980 |
| Equipment Type: | Location Transceiver |
| Classification: | Portable Transmitter Next to Body |
| TX Frequency Range: | 1616 MHz – 1616.333 MHz; 1625.666 – 1625.9999 MHz; 2402 – 2480 MHz |
| Frequency Tolerance: | ± 2.5 ppm |
| Maximum RF Output: | 1621 MHz – 31.7 dBm Conducted |
| Signal Modulation: | TDMA/FDMA, GFSK |
| Antenna Type: | Stub |
| Application Type: | Certification |
| FCC Rule Parts: | Part 25 |
| KDB Test Methodology: | KDB 447498 D01 v05 |
| Industry Canada: | RSS-102 Issue 5 Draft, Safety Code 6 |
| Max. Stand Alone SAR Value: | 1.36 W/kg |
| Max. Simultaneous SAR Value: | 1.54 W/kg |
| Separation Distance: | 0 mm |

This wireless mobile and/or portable device has been shown to be compliant for localized specific absorption rate (SAR) for uncontrolled environment/general exposure limits specified in ANSI/IEEE Std. C95.1-1992 and had been tested in accordance with the measurement procedures specified in IEEE 1528-2013 and IEC 62209-2:2010 (See test report).

I attest to the accuracy of the data. All measurements were performed by myself or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

RF Exposure Lab, LLC certifies that no party to this application has been denied FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 853(a).



Jay M. Moulton
Vice President



Testing Cert. # 2387.01

Table of Contents

| | | |
|-----|---|----|
| 1. | Introduction | 3 |
| | SAR Definition [5]..... | 4 |
| 2. | SAR Measurement Setup..... | 5 |
| | Robotic System..... | 5 |
| | System Hardware..... | 5 |
| | System Electronics..... | 6 |
| | Probe Measurement System..... | 6 |
| 3. | Probe and Dipole Calibration..... | 14 |
| 4. | Phantom & Simulating Tissue Specifications..... | 15 |
| | Head & Body Simulating Mixture Characterization | 15 |
| 5. | ANSI/IEEE C95.1 – 1999 RF Exposure Limits [2]..... | 16 |
| | Uncontrolled Environment | 16 |
| | Controlled Environment..... | 16 |
| 6. | Measurement Uncertainty | 17 |
| 7. | System Validation..... | 18 |
| | Tissue Verification..... | 18 |
| | Test System Verification..... | 18 |
| 8. | SAR Test Data Summary | 19 |
| | Procedures Used To Establish Test Signal | 19 |
| | Device Test Condition | 19 |
| | SAR Data Summary – 1620 MHz Body..... | 22 |
| | SAR Data Summary – Simultaneous Evaluation | 23 |
| 9. | Test Equipment List..... | 24 |
| 10. | Conclusion | 25 |
| 11. | References..... | 26 |
| | Appendix A – System Validation Plots and Data | 27 |
| | Appendix B – SAR Test Data Plots | 30 |
| | Appendix C – SAR Test Setup Photos | 32 |
| | Appendix D – Probe Calibration Data Sheets..... | 38 |
| | Appendix E – Dipole Calibration Data Sheets | 50 |
| | Appendix F – Phantom Calibration Data Sheets | 60 |

1. Introduction

This measurement report shows compliance of the DeLorme Model INRCH25 FCC ID: Q639603N & T7V1315 with FCC Part 2, 1093, ET Docket 93-62 Rules for mobile and portable devices and IC Certificate: 4629A-9603N & 216Q-1315 with RSS102 Issue 5 Draft & Safety Code 6. The FCC have adopted the guidelines for evaluating the environmental effects of radio frequency radiation in ET Docket 93-62 on August 6, 1996 to protect the public and workers from the potential hazards of RF emissions due to FCC regulated portable devices. [1], [6]

The test results recorded herein are based on a single type test of DeLorme Model INRCH25 and therefore apply only to the tested sample.

The test procedures, as described in ANSI C95.1 – 1999 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz [2], ANSI C95.3 – 2002 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields [3], FCC OET Bulletin 65 Supp. C – 2001 [4], IEEE Std.1528 – 2003 Recommended Practice [5], and Industry Canada Safety Code 6 Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz were employed.

The following table indicates all the wireless technologies operating in the INRCH25 wireless Location Transceiver. The table also shows the tolerance for the power level for each mode.

| Band | Technology | 3GPP Nominal Power dBm | Setpoint Nominal Power dBm | Tolerance dBm | Lower Tolerance dBm | Upper Tolerance dBm |
|-----------|------------|------------------------|----------------------------|---------------|---------------------|---------------------|
| 1620 MHz | TDMA/FDMA | N/A | N/A | N/A | N/A | 31.7 |
| 2402-2480 | GFSK | N/A | N/A | N/A | N/A | 10.2 |

SAR Definition [5]

Specific Absorption Rate is defined as the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dV) of a given density (ρ).

$$SAR = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dV} \right)$$

SAR is expressed in units of watts per kilogram (W/kg). SAR can be related to the electric field at a point by

$$SAR = \frac{\sigma |E|^2}{\rho}$$

where:

σ = conductivity of the tissue (S/m)

ρ = mass density of the tissue (kg/m³)

E = rms electric field strength (V/m)

2. SAR Measurement Setup

Robotic System

These measurements are performed using the DASY52 automated dosimetric assessment system. The DASY52 is made by Schmid & Partner Engineering AG (SPEAG) in Zurich, Switzerland and consists of high precision robotics system (Staubli), robot controller, Intel Core2 computer, near-field probe, probe alignment sensor, and the generic twin phantom containing the brain equivalent material. The robot is a six-axis industrial robot performing precise movements to position the probe to the location (points) of maximum electromagnetic field (EMF) (see Fig. 2.1).

System Hardware

A cell controller system contains the power supply, robot controller teach pendant (Joystick), and a remote control used to drive the robot motors. The PC consists of the HP Intel Core2 computer with Windows XP system and SAR Measurement Software DASY52, A/D interface card, monitor, mouse, and keyboard. The Staubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit that performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. is connected to the Electro-optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC plug-in card.

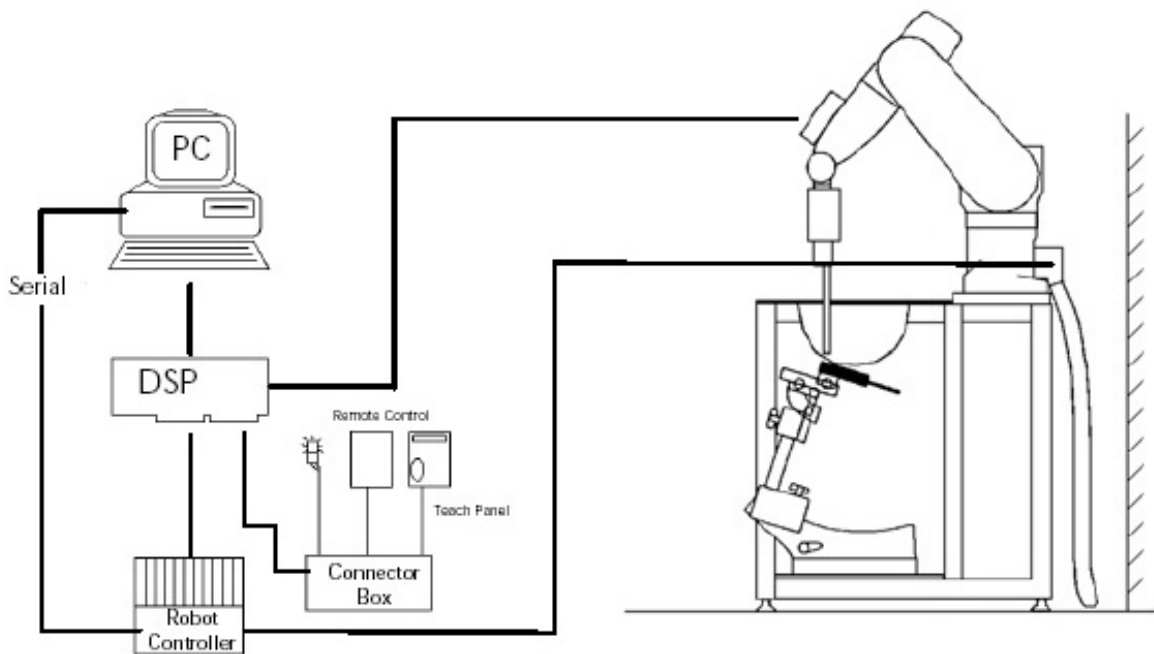


Figure 2.1 SAR Measurement System Setup

System Electronics

The DAE4 consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer. The system is described in detail in.

Probe Measurement System

The SAR measurements were conducted with the dosimetric probe EX3DV4, designed in the classical triangular configuration (see Fig. 2.2) and optimized for dosimetric evaluation. The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multi fiber line ending at the front of the probe tip. (see Fig. 2.3) It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY52 software reads the reflection during a software approach and looks for the maximum using a 2nd order fitting. The approach is stopped at reaching the maximum.



DAE System

Probe Specifications

Calibration: In air from 10 MHz to 6.0 GHz
In brain and muscle simulating tissue at Frequencies of 450 MHz, 835 MHz, 1750 MHz, 1900 MHz, 2450 MHz, 2600 MHz, 3500 MHz, 5200 MHz, 5300 MHz, 5600 MHz, 5800 MHz

Frequency: 10 MHz to 6 GHz

Linearity: ± 0.2 dB (30 MHz to 6 GHz)

Dynamic: 10 mW/kg to 100 W/kg

Range: Linearity: ± 0.2 dB

Dimensions: Overall length: 330 mm

Tip length: 20 mm

Body diameter: 12 mm

Tip diameter: 2.5 mm

Distance from probe tip to sensor center: 1 mm

Application: SAR Dosimetry Testing
Compliance tests of wireless device




Figure 2.2 Triangular Probe Configurations



Figure 2.3 Probe Thick-Film Technique

Probe Calibration Process

Dosimetric Assessment Procedure

Each probe is calibrated according to a dosimetric assessment procedure described in with accuracy better than +/- 10%. The spherical isotropy was evaluated with the procedure described in and found to be better than +/-0.25dB. The sensitivity parameters (Norm X, Norm Y, Norm Z), the diode compression parameter (DCP) and the conversion factor (Conv F) of the probe is tested.

Free Space Assessment

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies below 1 GHz, and in a waveguide above 1GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity at the proper orientation with the field. The probe is then rotated 360 degrees until the three channels show the maximum reading. The power density readings equates to 1 mW/cm².

Temperature Assessment *

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium, correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor based temperature probe is used in conjunction with the E-field probe

$$SAR = C \frac{\Delta T}{\Delta t}$$

$$SAR = \frac{|E|^2 \cdot \sigma}{\rho}$$

where:

where:

Δt = exposure time (30 seconds),

σ = simulated tissue conductivity,

C = heat capacity of tissue (brain or muscle),

ρ = Tissue density (1.25 g/cm³ for brain tissue)

ΔT = temperature increase due to RF exposure.

SAR is proportional to $\Delta T / \Delta t$, the initial rate of tissue heating, before thermal diffusion takes place.

Now it's possible to quantify the electric field in the simulated tissue by equating the thermally derived SAR to the E- field;



Figure 2.4 E-Field and Temperature Measurements at 900MHz



Figure 2.5 E-Field and Temperature Measurements at 1800MHz

Data Extrapolation

The DASY52 software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given like below;

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with V_i = compensated signal of channel i (i=x,y,z)
 U_i = input signal of channel i (i=x,y,z)
 cf = crest factor of exciting field (DASY parameter)
 dcp_i = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes: $E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$

with V_i = compensated signal of channel i (i = x,y,z)
 $Norm_i$ = sensor sensitivity of channel i (i = x,y,z)
 $\mu V/(V/m)^2$ for E-field probes
 $ConvF$ = sensitivity of enhancement in solution
 E_i = electric field strength of channel i in V/m

The RSS value of the field components gives the total field strength (Hermetian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with SAR = local specific absorption rate in W/g
 E_{tot} = total field strength in V/m
 σ = conductivity in [mho/m] or [Siemens/m]
 ρ = equivalent tissue density in g/cm³

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{free} = \frac{E_{tot}^2}{3770}$$

with P_{pwe} = equivalent power density of a plane wave in W/cm²
 E_{tot} = total electric field strength in V/m

Scanning procedure

- The DASY installation includes predefined files with recommended procedures for measurements and system check. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.
- The „reference“ and „drift“ measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. +/- 5 %.
- The highest integrated SAR value is the main concern in compliance test applications. These values can mostly be found at the inner surface of the phantom and cannot be measured directly due to the sensor offset in the probe. To extrapolate the surface values, the measurement distances to the surface must be known accurately. A distance error of 0.5mm could produce SAR errors of 6% at 1800 MHz. Using predefined locations for measurements is not accurate enough. Any shift of the phantom (e.g., slight deformations after filling it with liquid) would produce high uncertainties. For an automatic and accurate detection of the phantom surface, the DASY5 system uses the mechanical surface detection. The detection is always at touch, but the probe will move backward from the surface the indicated distance before starting the measurement.
- The „area scan“ measures the SAR above the DUT or verification dipole on a parallel plane to the surface. It is used to locate the approximate location of the peak SAR with 2D spline interpolation. The robot performs a stepped movement along one grid axis while the local electrical field strength is measured by the probe. The probe is touching the surface of the SAM during acquisition of measurement values. The scan uses different grid spacings for different frequency measurements. Standard grid spacing for head measurements in frequency ranges ≤ 2 GHz is 15 mm in x - and y- dimension. For higher frequencies a finer resolution is needed, thus for the grid spacing is reduced according the following table:

| Area scan grid spacing for different frequency ranges | |
|---|--------------|
| Frequency range | Grid spacing |
| ≤ 2 GHz | ≤ 15 mm |
| 2 – 4 GHz | ≤ 12 mm |
| 4 – 6 GHz | ≤ 10 mm |

Grid spacing and orientation have no influence on the SAR result. For special applications where the standard scan method does not find the peak SAR within the grid, e.g. mobile phones with flip cover, the grid can be adapted in orientation. Results of this coarse scan are shown in annex B.

- A „zoom scan“ measures the field in a volume around the 2D peak SAR value acquired in the previous „coarse“ scan. It uses a fine meshed grid where the robot moves the probe in steps along all the 3 axis (x,y and z-axis) starting at the bottom of the Phantom. The grid spacing for the cube measurement is varied according to the measured frequency range, the dimensions are given in the following table:

| Zoom scan grid spacing and volume for different frequency ranges | | | |
|---|----------------------------|-------------------------|--------------------------|
| Frequency range | Grid spacing for x, y axis | Grid spacing for z axis | Minimum zoom scan volume |
| ≤ 2 GHz | ≤ 8 mm | ≤ 5 mm | ≥ 30 mm |
| 2 – 3 GHz | ≤ 5 mm | ≤ 5 mm | ≥ 28 mm |
| 3 – 4 GHz | ≤ 5 mm | ≤ 4 mm | ≥ 28 mm |
| 4 – 5 GHz | ≤ 4 mm | ≤ 3 mm | ≥ 25 mm |
| 5 – 6 GHz | ≤ 4 mm | ≤ 2 mm | ≥ 22 mm |

DASY is also able to perform repeated zoom scans if more than 1 peak is found during area scan. In this document, the evaluated peak 1g and 10g averaged SAR values are shown in the 2D-graphics in annex B. Test results relevant for the specified standard (see section 3) are shown in table form in section 7.

Spatial Peak SAR Evaluation

The spatial peak SAR - value for 1 and 10 g is evaluated after the Cube measurements have been done. The basis of the evaluation are the SAR values measured at the points of the fine cube grid consisting of all points in the three directions x, y and z. The algorithm that finds the maximal averaged volume is separated into three different stages.

- The data between the dipole center of the probe and the surface of the phantom are extrapolated. This data cannot be measured since the center of the dipole is 1 to 2.7 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is about 1 mm (see probe calibration sheet). The extrapolated data from a cube measurement can be visualized by selecting 'Graph Evaluated'.
- The maximum interpolated value is searched with a straight-forward algorithm. Around this maximum the SAR - values averaged over the spatial volumes (1g or 10 g) are computed using the 3d-spline interpolation algorithm. If the volume cannot be evaluated (i.e., if a part of the grid was cut off by the boundary of the measurement area) the evaluation will be started on the corners of the bottom plane of the cube.
- All neighbouring volumes are evaluated until no neighbouring volume with a higher average value is found.

Extrapolation

The extrapolation is based on a least square algorithm [W. Gander, Computermathematik, p.168-180]. Through the points in the first 3 cm along the z-axis, polynomials of order four are calculated. These polynomials are then used to evaluate the points between the surface and the probe tip. The points, calculated from the surface, have a distance of 1 mm from each other.

Interpolation

The interpolation of the points is done with a 3d-Spline. The 3d-Spline is composed of three one-dimensional splines with the "Not a knot"-condition [W. Gander, Computermathematik, p.141-150] (x, y and z -direction) [Numerical Recipes in C, Second Edition, p.123ff].

Volume Averaging

At First the size of the cube is calculated. Then the volume is integrated with the trapezoidal algorithm. 8000 points (20x20x20) are interpolated to calculate the average.

Advanced Extrapolation

DASY uses the advanced extrapolation option which is able to compensate boundary effects on E-field probes.

SAM PHANTOM

The SAM Twin Phantom V4.0 is constructed of a fiberglass shell integrated in a wooden table. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90% of all users. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. (see Fig. 2.6)

Phantom Specification

Phantom: SAM Twin Phantom (V4.0)
Shell Material: Vivac Composite
Thickness: 2.0 ± 0.2 mm

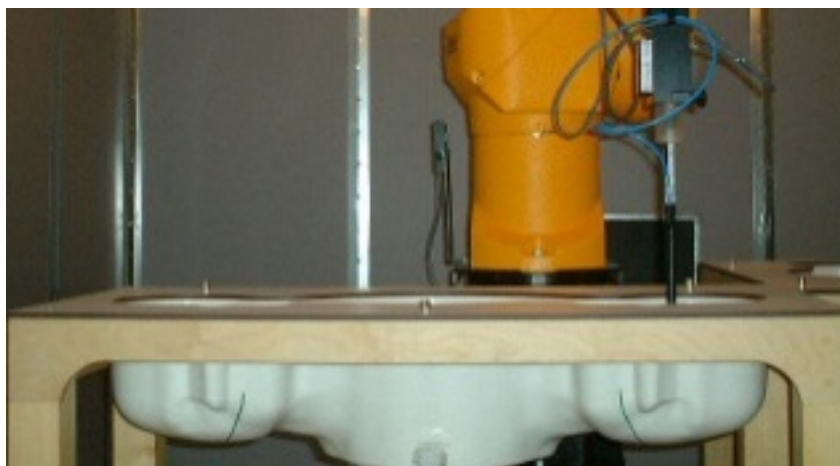


Figure 2.6 SAM Twin Phantom

Device Holder for Transmitters

In combination with the SAM Twin Phantom V4.0 the Mounting Device (see Fig. 2.7), enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation point is the ear opening. The devices can be easily, accurately, and repeatedly positioned according to the FCC, CENELEC, IEC and IEEE specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).



Figure 2.7 Mounting Device

Note: A simulating human hand is not used due to the complex anatomical and geometrical structure of the hand that may produce infinite number of configurations. To produce the worst-case condition (the hand absorbs antenna output power), the hand is omitted during the tests.

3. Probe and Dipole Calibration

See Appendix D and E.

4. Phantom & Simulating Tissue Specifications

Head & Body Simulating Mixture Characterization

The head and body mixtures consist of the material based on the table listed below. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the desired tissue. Body tissue parameters that have not been specified in IEEE1528-2013 are derived from the issue dielectric parameters computed from the 4-Cole-Cole equations.

Table 4.1 Typical Composition of Ingredients for Tissue

| Ingredients | | Simulating Tissue |
|---------------------|--------|-------------------|
| | | 1640 MHz Body |
| Mixing Percentage | | |
| Water | | 54.47 |
| Sugar | | 0.00 |
| Salt | | 0.33 |
| HEC | | 0.00 |
| Bactericide | | 0.00 |
| DGBE | | 45.22 |
| Dielectric Constant | Target | 53.72 |
| Conductivity (S/m) | Target | 1.42 |

5. ANSI/IEEE C95.1 – 1999 RF Exposure Limits [2]

Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

Controlled Environment

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

Table 5.1 Human Exposure Limits

| | UNCONTROLLED ENVIRONMENT General Population (W/kg) or (mW/g) | CONTROLLED ENVIRONMENT Professional Population (W/kg) or (mW/g) |
|--|--|---|
| SPATIAL PEAK SAR ¹ Brain | 1.60 | 8.00 |
| SPATIAL AVERAGE SAR ² Whole Body | 0.08 | 0.40 |
| SPATIAL PEAK SAR ³ Hands, Feet, Ankles, Wrists | 4.00 | 20.00 |

¹ The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

² The Spatial Average value of the SAR averaged over the whole body.

³ The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

6. Measurement Uncertainty

Exposure Assessment Measurement Uncertainty

| Relative DASYS Uncertainty Budget for SAR Tests | | | | | | | | |
|---|-------------------|--------------------------|---------|-------|-------|----------------------|------------|----------------------|
| According to IEC62209-2/2010 (30 MHz - 6 GHz range) | | | | | | | | |
| Error Description | Uncertainty Value | Probability Distribution | Divisor | c_i | c_i | Standard Uncertainty | | v_i^2 or v_{eff} |
| | | | | (1g) | (10g) | ± %, (1g) | ± %, (10g) | |
| Measurement System | | | | | | | | |
| Probe calibration | ± 6.6% | Normal | 1 | 1 | 1 | ± 6.6% | ± 6.6% | ∞ |
| Axial isotropy | ± 4.7% | Rectangular | √3 | 0.7 | 0.7 | ± 1.9% | ± 1.9% | ∞ |
| Hemispherical isotropy | ± 9.6% | Rectangular | √3 | 0.7 | 0.7 | ± 3.9% | ± 3.9% | ∞ |
| Boundary effects | ± 2.0% | Rectangular | √3 | 1 | 1 | ± 1.2% | ± 1.2% | ∞ |
| Probe linearity | ± 4.7% | Rectangular | √3 | 1 | 1 | ± 2.7% | ± 2.7% | ∞ |
| System detection limits | ± 1.0% | Rectangular | √3 | 1 | 1 | ± 0.6% | ± 0.6% | ∞ |
| Modulation response | ± 2.4% | Rectangular | √3 | 1 | 1 | ± 1.4% | ± 1.4% | ∞ |
| Readout electronics | ± 0.3% | Normal | 1 | 1 | 1 | ± 0.3% | ± 0.3% | ∞ |
| Response time | ± 0.8% | Rectangular | √3 | 1 | 1 | ± 0.5% | ± 0.5% | ∞ |
| Integration time | ± 2.6% | Rectangular | √3 | 1 | 1 | ± 1.5% | ± 1.5% | ∞ |
| RF ambient noise | ± 3.0% | Rectangular | √3 | 1 | 1 | ± 1.7% | ± 1.7% | ∞ |
| RF ambient reflections | ± 3.0% | Rectangular | √3 | 1 | 1 | ± 1.7% | ± 1.7% | ∞ |
| Probe positioner | ± 0.8% | Rectangular | √3 | 1 | 1 | ± 0.5% | ± 0.5% | ∞ |
| Probe positioning | ± 6.7% | Rectangular | √3 | 1 | 1 | ± 3.9% | ± 3.9% | ∞ |
| Post-processing | ± 4.0% | Rectangular | √3 | 1 | 1 | ± 2.3% | ± 2.3% | ∞ |
| Test Sample Related | | | | | | | | |
| Device positioning | ± 2.9% | Normal | 1 | 1 | 1 | ± 2.9% | ± 2.9% | 145 |
| Device holder uncertainty | ± 3.6% | Normal | 1 | 1 | 1 | ± 3.6% | ± 3.6% | 5 |
| Power drift | ± 5.0% | Rectangular | √3 | 1 | 1 | ± 2.9% | ± 2.9% | ∞ |
| Phantom and Setup | | | | | | | | |
| Phantom uncertainty | ± 7.9% | Rectangular | √3 | 1 | 1 | ± 4.6% | ± 4.6% | ∞ |
| SAR algorithm correction | ± 1.9% | Normal | 1 | 1 | 0.84 | ± 1.9% | ± 1.9% | ∞ |
| Liquid conductivity (meas.) | ± 5.0% | Rectangular | √3 | 0.78 | 0.71 | ± 0.1% | ± 0.1% | ∞ |
| Liquid permittivity (meas.) | ± 5.0% | Rectangular | √3 | 0.26 | 0.26 | ± 0.1% | ± 0.1% | ∞ |
| Temp. Unc. – Conductivity | ± 3.4% | Rectangular | √3 | 0.78 | 0.71 | ± 1.5% | ± 1.5% | ∞ |
| Temp. Unc. – Permittivity | ± 0.4% | Rectangular | √3 | 0.23 | 0.26 | ± 0.1% | ± 0.1% | ∞ |
| Combined Uncertainty | | | | | | ± 12.4% | ± 12.3% | 330 |
| Expanded Std. Uncertainty | | | | | | ± 24.8% | ± 24.6% | |

Worst case uncertainty budget for DASYS assessed according to IEC62209-2/2010 standard. The budget is valid for the frequency range 30 MHz – 6 GHz and represents a worst-case analysis. For specific tests and configurations, the uncertainty could be considerable smaller.

7. System Validation

Tissue Verification

Table 7.1 Measured Tissue Parameters

| | | | |
|---------------------------------|------|---------------|----------|
| | | 1640 MHz Body | |
| Date(s) | | Feb. 25, 2015 | |
| Liquid Temperature (°C) | 20.0 | Target | Measured |
| Dielectric Constant: ϵ | | 53.72 | 53.65 |
| Conductivity: σ | | 1.42 | 1.43 |

See Appendix A for data printout.

Test System Verification

Prior to assessment, the system is verified to the $\pm 10\%$ of the specifications at the test frequency by using the system kit. Power is extrapolated to 1 watt. (Graphic Plots Attached)

Table 7.2 System Dipole Validation Target & Measured

| | Test Frequency | Targeted SAR _{1g} (W/kg) | Measure SAR _{1g} (W/kg) | Tissue Used for Verification | Deviation Target and Fast SAR to SAR (%) | Plot Number |
|-------------|----------------|-----------------------------------|----------------------------------|------------------------------|--|-------------|
| 25-Feb-2015 | 1640 MHz | 32.82 | 33.50 | Body | + 2.07 | 1 |

See Appendix A for data plots.

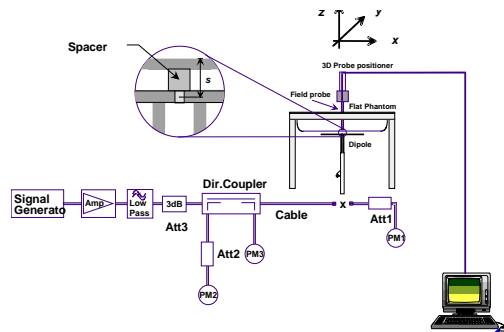


Figure 7.1 Dipole Validation Test Setup

8. SAR Test Data Summary

See Measurement Result Data Pages

See Appendix B for SAR Test Data Plots.
See Appendix C for SAR Test Setup Photos.

Procedures Used To Establish Test Signal

The device was placed into simulated transmit mode using the manufacturer's test codes. Such test signals offer a consistent means for testing SAR and are recommended for evaluating SAR. When test modes are not available or inappropriate for testing a device, the actual transmission is activated through a base station simulator or similar equipment. See data pages for actual procedure used in measurement.

Device Test Condition

In order to verify that the device was tested at full power, conducted output power measurements were performed before and after each SAR measurement to confirm the output power unless otherwise noted. If a conducted power deviation of more than 5% occurred, the test was repeated. The power drift of each test is measured at the start of the test and again at the end of the test. The drift percentage is calculated by the formula $((\text{end}/\text{start})-1)*100$ and rounded to three decimal places. The drift percentage is calculated into the resultant SAR value on the data sheet for each test.

The total frequency band of the device was 10 MHz. Per KDB 447498 D01 v05r02 section 4.1 6) on page 8, there is only one channel required to be tested.

$$N_c = \text{Round} \{ [100(f_{\text{high}} - f_{\text{low}})/f_c]^{0.5} \times (f_c/100)^{0.2} \} = \text{Round} \{ [100(1626 - 1616)/1621]^{0.5} \times (1621/100)^{0.2} \} = 1$$

The testing was conducted on the Back, Front, Left Side and Right Side of the device. The transmitter is controlled by the firmware to limit the duty cycle. The TDMA signal has a maximum duty cycle of 10%. All measurements were conducted with the transmitter at the TDMA duty cycle for the SAR tests as this was the maximum value achievable.

Bluetooth operation was not evaluated as the power level of the BT transmitter was lower than the excluded limit per KDB 447498 D01 v05r02. The Bluetooth transmitter does simultaneously transmit with the 1621 MHz transmitter. The simultaneous transmit is evaluated on page 23.

| 1621 MHz | | |
|----------|---------|-------|
| Freq | Channel | Power |
| 1616 | 1 | 30.36 |
| 1625 | 2 | 30.33 |

Conduct Power Measurements

Figure 8.1 Test Reduction Table

| Band | Side | Required Channel | Tested/Reduced |
|----------|------------|------------------|----------------|
| 1620 MHz | Back | 1 – 1616.2 MHz | Tested |
| | | 2 – 1625.8 MHz | Tested |
| | Left Side | 1 – 1616.2 MHz | Tested |
| | | 2 – 1625.8 MHz | Tested |
| | Right Side | 1 – 1616.2 MHz | Tested |
| | | 2 – 1625.8 MHz | Tested |
| | Front | 1 – 1616.2 MHz | Tested |
| | | 2 – 1625.8 MHz | Tested |


SAR Data Summary – 1620 MHz Body

MEASUREMENT RESULTS

| Gap | Plot | Position | Frequency | | Modulation | End Power (dBm) | Measured SAR (W/kg) | Reported SAR (W/kg) |
|------|------|------------|-----------|----|------------|--------------------|---------------------|---------------------|
| | | | MHz | Ch | | | | |
| 0 mm | ---- | Back | 1616 | 1 | BPSK | 30.36 | 0.351 | 0.38 |
| | ---- | Front | 1616 | 1 | BPSK | 30.36 | 1.26 | 1.36 |
| | ---- | Left Side | 1616 | 1 | BPSK | 30.36 | 0.639 | 0.69 |
| | ---- | Right Side | 1616 | 1 | BPSK | 30.36 | 0.0859 | 0.09 |
| | ---- | Back | 1625 | 2 | BPSK | 30.33 | 0.519 | 0.57 |
| | ---- | Front | 1625 | 2 | BPSK | 30.33 | 1.21 | 1.32 |
| | ---- | Left Side | 1625 | 2 | BPSK | 30.33 | 0.607 | 0.66 |
| | ---- | Right Side | 1625 | 2 | BPSK | 30.33 | 0.0935 | 0.10 |

Body
1.6 W/kg (mW/g)
 averaged over 1 gram

- 1. Battery is fully charged for all tests.
 Power Measured Conducted ERP EIRP
- 2. SAR Measurement
 Phantom Configuration Left Head Eli4 Right Head
 SAR Configuration Head Body
- 3. Test Signal Call Mode Test Code Base Station Simulator
- 4. Test Configuration With Belt Clip Without Belt Clip N/A
- 5. Tissue Depth is at least 15.0 cm



Jay M. Moulton
 Vice President

SAR Data Summary – Simultaneous Evaluation

| MEASUREMENT RESULTS - BT | | | | | | | | |
|---|-----|------------|-----------|-----|------------|------------------|------------------|-----------|
| Frequency | | Modulation | Frequency | | Modulation | SAR ₁ | SAR ₂ | SAR Total |
| MHz | Ch. | | MHz | Ch. | | | | |
| 1616 | 1 | BPSK | 2440 | 39 | GFSK | 1.36 | 0.18 | 1.54 |
| Body 1.6 W/kg (mW/g) averaged over 1 gram | | | | | | | | |

The sum of the two transmitters is less than the limit; therefore, the simultaneous transmission meets the requirements of KDB447498 D01 v05r02 section 4.3.2 page 11.

The BT was calculated as it was excluded from stand-alone SAR. The calculation formula was from KDB 447498 D01 v05r02 section 4.3.2 2) on page 13. The closest distance a user can get to the BT antenna is 12 mm.

$[(\text{max. power of channel, mW})/(\text{minimum test separation distance, mm})] \cdot [\sqrt{f_{(\text{GHz})}/x}] \text{ W/kg: } x=7.5$

$(10.5 \text{ mW}/12 \text{ mm}) \cdot (\sqrt{2.48/7.5}) = 0.18 \text{ W/kg}$

9. Test Equipment List

Table 9.1 Equipment Specifications

| Type | Calibration Due Date | Calibration Done Date | Serial Number |
|---|----------------------|-----------------------|-----------------|
| Staubli Robot TX60L | N/A | N/A | F07/55M6A1/A/01 |
| Measurement Controller CS8c | N/A | N/A | 1012 |
| ELI4 Flat Phantom | N/A | N/A | 1065 |
| Device Holder | N/A | N/A | N/A |
| Data Acquisition Electronics 4 | 04/10/2015 | 04/10/2014 | 1217 |
| SPEAG E-Field Probe EX3DV4 | 01/23/2016 | 01/23/2015 | 3833 |
| Apriel Validation Dipole ALS-D-1640-S-2 | 01/16/2016 | 01/16/2013 | 207-00101 |
| Speag Validation Dipole D2450V2 | 12/04/2015 | 12/04/2012 | 829 |
| Agilent N1911A Power Meter | 03/24/2015 | 03/24/2014 | GB45100254 |
| Advantest R3261A Spectrum Analyzer | 03/24/2015 | 03/24/2014 | 31720068 |
| Agilent (HP) 8350B Signal Generator | 03/24/2015 | 03/24/2014 | 2749A10226 |
| Agilent (HP) 83525A RF Plug-In | 03/24/2015 | 03/24/2014 | 2647A01172 |
| Agilent (HP) 8753C Vector Network Analyzer | 03/25/2015 | 03/25/2014 | 3135A01724 |
| Agilent (HP) 85047A S-Parameter Test Set | 03/25/2015 | 03/25/2014 | 2904A00595 |
| Agilent (HP) 8960 Base Station Sim. | 10/18/2016 | 10/18/2014 | MY48360364 |
| Anritsu MT8820C | 07/29/2015 | 07/29/2014 | 6201176199 |
| Agilent 778D Dual Directional Coupler | N/A | N/A | MY48220184 |
| MiniCircuits BW-N20W5+ Fixed 20 dB Attenuator | N/A | N/A | N/A |
| MiniCircuits SPL-10.7+ Low Pass Filter | N/A | N/A | R8979513746 |
| Apriel Dielectric Probe Assembly | N/A | N/A | 0011 |
| Body Equivalent Matter (1640 MHz) | N/A | N/A | N/A |
| Body Equivalent Matter (2450 MHz) | N/A | N/A | N/A |

10. Conclusion

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the FCC/IC. These measurements are taken to simulate the RF effects exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The tested device complies with the requirements in respect to all parameters subject to the test. The test results and statements relate only to the item(s) tested.

Please note that the absorption and distribution of electromagnetic energy in the body is a very complex phenomena that depends on the mass, shape, and size of the body; the orientation of the body with respect to the field vectors; and, the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because innumerable factors may interact to determine the specific biological outcome of an exposure to electromagnetic fields, any protection guide shall consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables. [3]

11. References

- [1] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radio Frequency Radiation, August 1996
- [2] ANSI/IEEE C95.1 – 1992, American National Standard Safety Levels with respect to Human Exposure to Radio Frequency Electromagnetic Fields, 300kHz to 100GHz, New York: IEEE, 1992.
- [3] ANSI/IEEE C95.3 – 1992, IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields – RF and Microwave, New York: IEEE, 1992.
- [4] International Electrotechnical Commission, IEC 62209-2 (Edition 1.0), Human Exposure to radio frequency fields from hand-held and body mounted wireless communication devices – Human models, instrumentation, and procedures – Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz), March 2010.
- [5] IEEE Standard 1528 – 2013, IEEE Recommended Practice for Determining the Peak-Spatial Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communication Devices: Measurement Techniques, June 2013.
- [6] Industry Canada, RSS – 102 Issue 5 Draft, Radio Frequency Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands), March 2014.
- [7] Health Canada, Safety Code 6, Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz, 2009.

Appendix A – System Validation Plots and Data

```
*****
Test Result for UIM Dielectric Parameter
Wed 25/Feb/2015
Freq  Frequency(GHz)
FCC_eH Limits for Head Epsilon
FCC_sH Limits for Head Sigma
FCC_eB Limits for Body Epsilon
FCC_sB Limits for Body Sigma
Test_e Epsilon of UIM
Test_s Sigma of UIM
*****
Freq          FCC_eB FCC_sB Test_e Test_s
1.6100        53.80  1.40  53.73  1.40
1.6162        53.781 1.406 53.711 1.406*
1.6200        53.77  1.41  53.70  1.41
1.6258        53.758 1.41  53.683 1.416*
1.6300        53.75  1.41  53.67  1.42
1.6400        53.72  1.42  53.65  1.43
1.6500        53.69  1.43  53.62  1.44
1.6600        53.67  1.43  53.60  1.45
1.6700        53.64  1.44  53.56  1.46
```

* value interpolated

RF Exposure Lab

Plot 1

DUT: ALS-D-1640-S-2; Type: Dipole; Serial: 207-00101

Communication System: CW; Frequency: 1640 MHz; Duty Cycle: 1:1
Medium: MSL1640; Medium parameters used: $f = 1640 \text{ MHz}$; $\sigma = 1.43 \text{ S/m}$; $\epsilon_r = 53.65$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section


Test Date: Date: 2/25/2015; Ambient Temp: 23 °C; Tissue Temp: 21 °C


Probe: EX3DV4 - SN3833; ConvF(7.64, 7.64, 7.64); Calibrated: 1/23/2015;
Sensor-Surface: 2mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1217; Calibrated: 4/10/2014
Phantom: ELI v4.0; Type: QDOVA001BB; Serial: 1065
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Procedure Notes:

1640 MHz/Verification/Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (measured) = 5.33 W/kg

1640 MHz/Verification/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm
Reference Value = 31.227 V/m; Power Drift = -0.01 dB
Peak SAR (extrapolated) = 6.89 W/kg
SAR(1 g) = 3.35 W/kg; SAR(10 g) = 1.93 W/kg
Maximum value of SAR (measured) = 5.49 W/kg

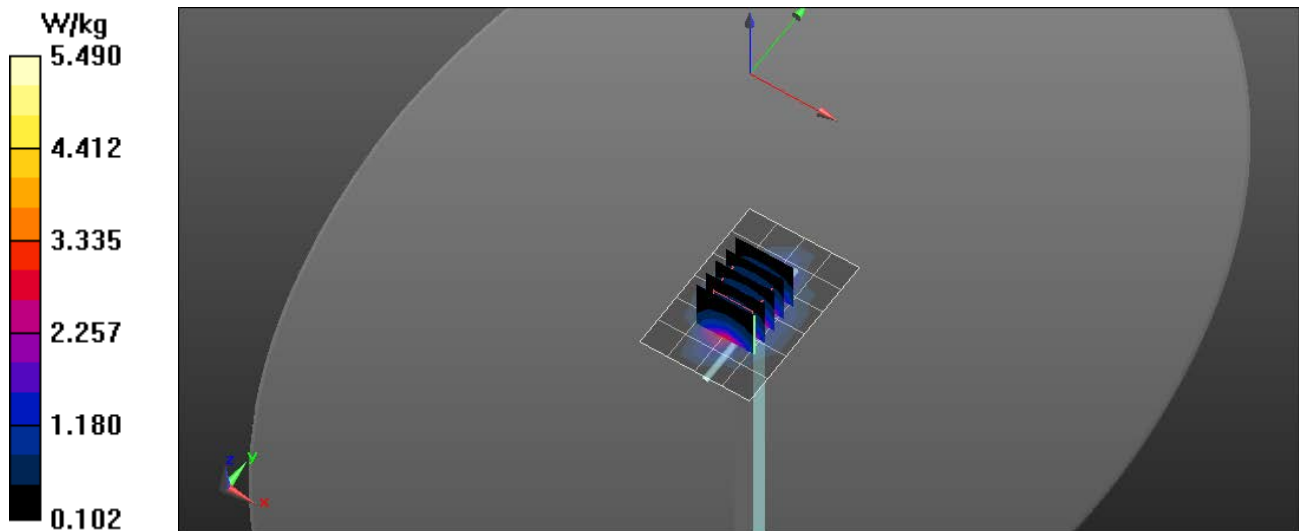

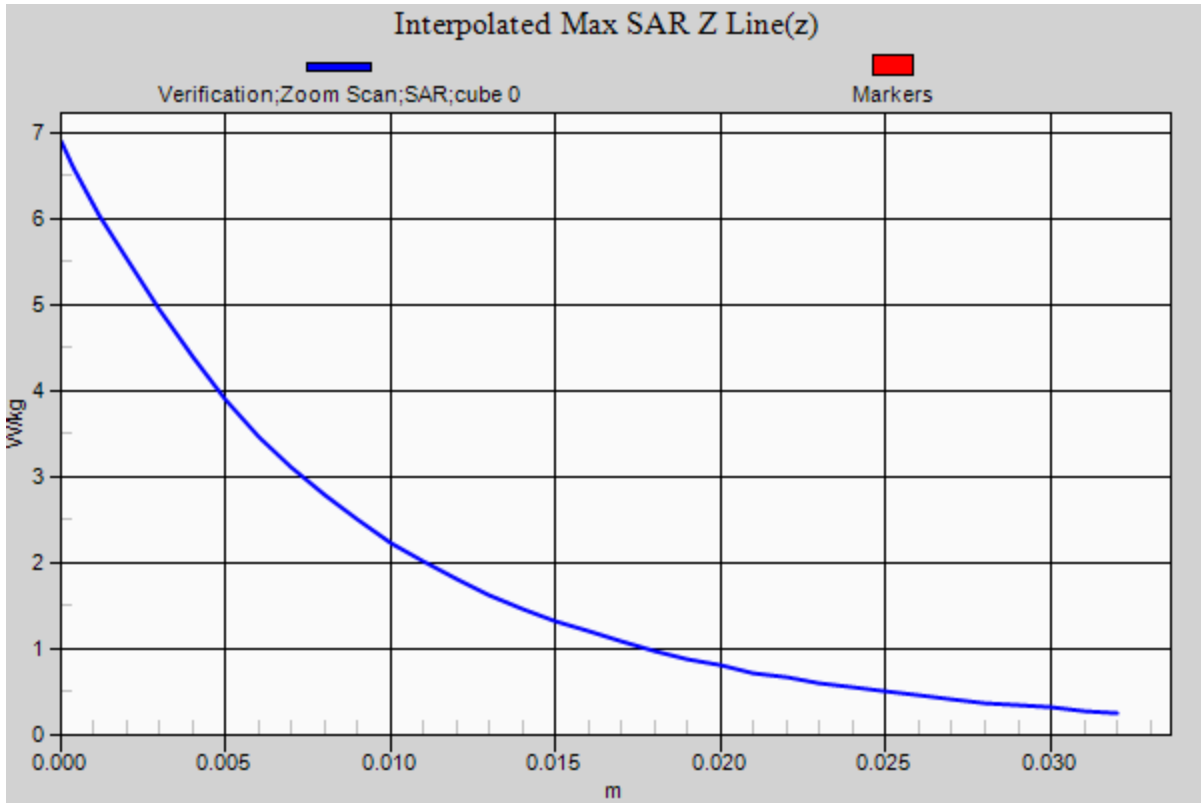

Appendix B – SAR Test Data Plots

RF Exposure Lab

Plot 1

DUT: INRCH25; Type: Satellite Tracker; Serial: 300434060775980

Communication System: DECT (TDD, TDMA/FDM, GFSK) (0); Frequency: 1616.2 MHz; Duty Cycle: 1:9.8696
Medium: MSL1640; Medium parameters used (interpolated): $f = 1616.2$ MHz; $\sigma = 1.406$ S/m; $\epsilon_r = 53.711$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

Test Date: Date: 2/25/2015; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 - SN3833; ConvF(7.64, 7.64, 7.64); Calibrated: 1/23/2015;
Sensor-Surface: 2mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1217; Calibrated: 4/10/2014
Phantom: ELI v4.0; Type: QDOVA001BB; Serial: 1065
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Procedure Notes:

1640 MHz Body/Front Low/Area Scan (7x13x1): Measurement grid: dx=15mm, dy=15mm

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 2.15 W/kg

1640 MHz Body/Front Low/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 4.323 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 2.81 W/kg

SAR(1 g) = 1.26 W/kg; SAR(10 g) = 0.741 W/kg

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 2.09 W/kg

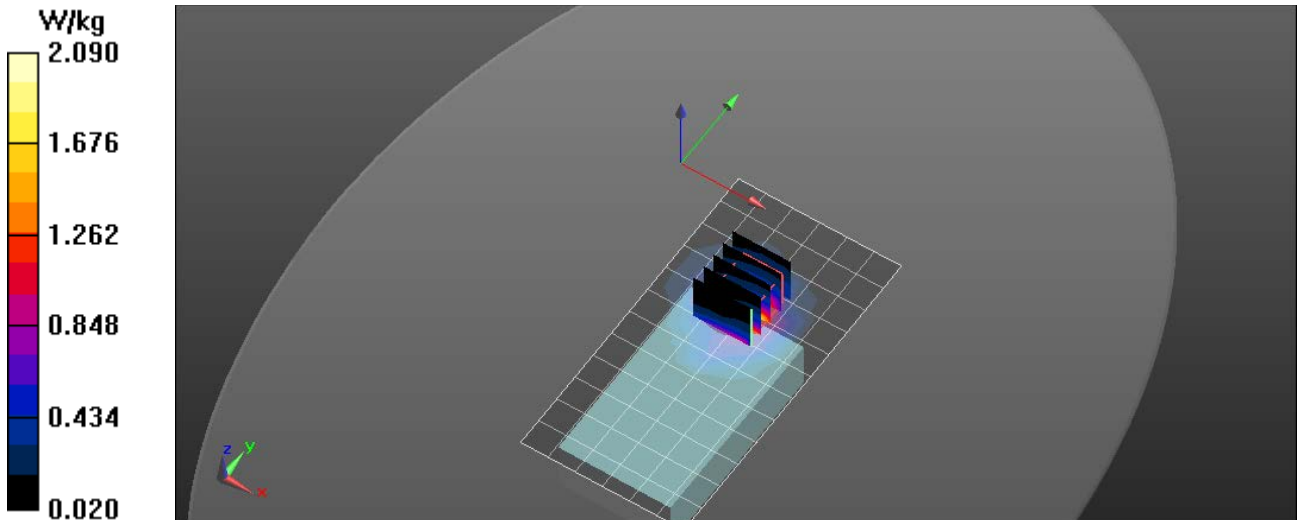

Appendix C – SAR Test Setup Photos



Test Position Back 0 mm Gap



Test Position Front 0 mm Gap



Test Position Left Side 0 mm Gap



Test Position Right Side 0 mm Gap



Front of Device



Back of Device

Appendix D – Probe Calibration Data Sheets



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **RF Exposure Lab**

Certificate No: **EX3-3833_Jan15**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3833**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,
QA CAL-25.v6
Calibration procedure for dosimetric E-field probes**

Calibration date: **January 23, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID | Cal Date (Certificate No.) | Scheduled Calibration |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B | GB41293874 | 03-Apr-14 (No. 217-01911) | Apr-15 |
| Power sensor E4412A | MY41498087 | 03-Apr-14 (No. 217-01911) | Apr-15 |
| Reference 3 dB Attenuator | SN: S5054 (3c) | 03-Apr-14 (No. 217-01915) | Apr-15 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 03-Apr-14 (No. 217-01919) | Apr-15 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 03-Apr-14 (No. 217-01920) | Apr-15 |
| Reference Probe ES3DV2 | SN: 3013 | 30-Dec-14 (No. ES3-3013_Dec14) | Dec-15 |
| DAE4 | SN: 660 | 14-Jan-15 (No. DAE4-660_Jan15) | Jan-16 |
| Secondary Standards | ID | Check Date (in house) | Scheduled Check |
| RF generator HP 8648C | US3642U01700 | 4-Aug-99 (in house check Apr-13) | In house check: Apr-16 |
| Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (in house check Oct-14) | In house check: Oct-15 |

| | | | |
|----------------|--------------------------------|--|---------------|
| Calibrated by: | Name Cluadio Leubler | Function Laboratory Technician | Signature |
| Approved by: | Name Katja Pokovic | Function Technical Manager | Signature |

Issued: January 26, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

| | |
|--------------------------|---|
| TSL | tissue simulating liquid |
| NORM _{x,y,z} | sensitivity in free space |
| ConvF | sensitivity in TSL / NORM _{x,y,z} |
| DCP | diode compression point |
| CF | crest factor (1/duty_cycle) of the RF signal |
| A, B, C, D | modulation dependent linearization parameters |
| Polarization φ | φ rotation around probe axis |
| Polarization ϑ | ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis |
| Connector Angle | information used in DASY system to align probe sensor X to the robot coordinate system |

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E^2 -field uncertainty inside TSL (see below *ConvF*).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * *frequency_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * *ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

Probe EX3DV4

SN:3833

Manufactured: November 7, 2011
Calibrated: January 23, 2015

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3833

Basic Calibration Parameters

| | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|---|----------|----------|----------|--------------|
| Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A | 0.47 | 0.49 | 0.35 | $\pm 10.1\%$ |
| DCP (mV) ^B | 101.8 | 100.3 | 103.5 | |

Modulation Calibration Parameters

| UID | Communication System Name | | A dB | B dB $\sqrt{\mu\text{V}}$ | C | D dB | VR mV | Unc ^E (k=2) |
|-----|---------------------------|---|---------|------------------------------|-----|---------|----------|---------------------------|
| 0 | CW | X | 0.0 | 0.0 | 1.0 | 0.00 | 131.5 | $\pm 3.5\%$ |
| | | Y | 0.0 | 0.0 | 1.0 | | 133.2 | |
| | | Z | 0.0 | 0.0 | 1.0 | | 131.7 | |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3833

Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) ^C | Relative Permittivity ^F | Conductivity (S/m) ^F | ConvF X | ConvF Y | ConvF Z | Alpha ^G | Depth ^G (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 150 | 52.3 | 0.76 | 11.02 | 11.02 | 11.02 | 0.00 | 1.00 | ± 13.3 % |
| 220 | 49.0 | 0.81 | 10.50 | 10.50 | 10.50 | 0.00 | 1.00 | ± 13.3 % |
| 300 | 45.3 | 0.87 | 10.41 | 10.41 | 10.41 | 0.10 | 1.25 | ± 13.3 % |
| 450 | 43.5 | 0.87 | 9.34 | 9.34 | 9.34 | 0.16 | 1.40 | ± 13.3 % |
| 600 | 42.7 | 0.88 | 9.41 | 9.41 | 9.41 | 0.10 | 1.10 | ± 13.3 % |
| 750 | 41.9 | 0.89 | 8.98 | 8.98 | 8.98 | 0.35 | 0.98 | ± 12.0 % |
| 900 | 41.5 | 0.97 | 8.51 | 8.51 | 8.51 | 0.34 | 0.99 | ± 12.0 % |
| 1640 | 40.3 | 1.29 | 7.50 | 7.50 | 7.50 | 0.23 | 1.08 | ± 12.0 % |
| 1750 | 40.1 | 1.37 | 7.42 | 7.42 | 7.42 | 0.49 | 0.70 | ± 12.0 % |
| 1900 | 40.0 | 1.40 | 7.29 | 7.29 | 7.29 | 0.57 | 0.62 | ± 12.0 % |
| 2450 | 39.2 | 1.80 | 6.58 | 6.58 | 6.58 | 0.41 | 0.76 | ± 12.0 % |
| 5200 | 36.0 | 4.66 | 4.62 | 4.62 | 4.62 | 0.35 | 1.80 | ± 13.1 % |
| 5300 | 35.9 | 4.76 | 4.44 | 4.44 | 4.44 | 0.35 | 1.80 | ± 13.1 % |
| 5500 | 35.6 | 4.96 | 4.18 | 4.18 | 4.18 | 0.40 | 1.80 | ± 13.1 % |
| 5600 | 35.5 | 5.07 | 4.03 | 4.03 | 4.03 | 0.40 | 1.80 | ± 13.1 % |
| 5800 | 35.3 | 5.27 | 4.12 | 4.12 | 4.12 | 0.40 | 1.80 | ± 13.1 % |

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3833

Calibration Parameter Determined in Body Tissue Simulating Media

| f (MHz) ^C | Relative Permittivity ^F | Conductivity (S/m) ^F | ConvF X | ConvF Y | ConvF Z | Alpha ^G | Depth ^G (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 150 | 61.9 | 0.80 | 11.21 | 11.21 | 11.21 | 0.00 | 1.00 | ± 13.3 % |
| 220 | 60.2 | 0.86 | 10.20 | 10.20 | 10.20 | 0.00 | 1.00 | ± 13.3 % |
| 300 | 58.2 | 0.92 | 10.29 | 10.29 | 10.29 | 0.06 | 1.15 | ± 13.3 % |
| 450 | 56.7 | 0.94 | 10.02 | 10.02 | 10.02 | 0.08 | 1.12 | ± 13.3 % |
| 600 | 56.1 | 0.95 | 9.37 | 9.37 | 9.37 | 0.10 | 1.10 | ± 13.3 % |
| 750 | 55.5 | 0.96 | 8.75 | 8.75 | 8.75 | 0.24 | 1.32 | ± 12.0 % |
| 900 | 55.0 | 1.05 | 8.51 | 8.51 | 8.51 | 0.41 | 0.88 | ± 12.0 % |
| 1640 | 53.8 | 1.40 | 7.64 | 7.64 | 7.64 | 0.31 | 0.95 | ± 12.0 % |
| 1750 | 53.4 | 1.49 | 7.18 | 7.18 | 7.18 | 0.34 | 0.93 | ± 12.0 % |
| 1900 | 53.3 | 1.52 | 7.04 | 7.04 | 7.04 | 0.60 | 0.67 | ± 12.0 % |
| 2450 | 52.7 | 1.95 | 6.69 | 6.69 | 6.69 | 0.80 | 0.57 | ± 12.0 % |
| 5200 | 49.0 | 5.30 | 3.92 | 3.92 | 3.92 | 0.45 | 1.90 | ± 13.1 % |
| 5300 | 48.9 | 5.42 | 3.81 | 3.81 | 3.81 | 0.45 | 1.90 | ± 13.1 % |
| 5500 | 48.6 | 5.65 | 3.52 | 3.52 | 3.52 | 0.50 | 1.90 | ± 13.1 % |
| 5600 | 48.5 | 5.77 | 3.47 | 3.47 | 3.47 | 0.50 | 1.90 | ± 13.1 % |
| 5800 | 48.2 | 6.00 | 3.57 | 3.57 | 3.57 | 0.50 | 1.90 | ± 13.1 % |


^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)


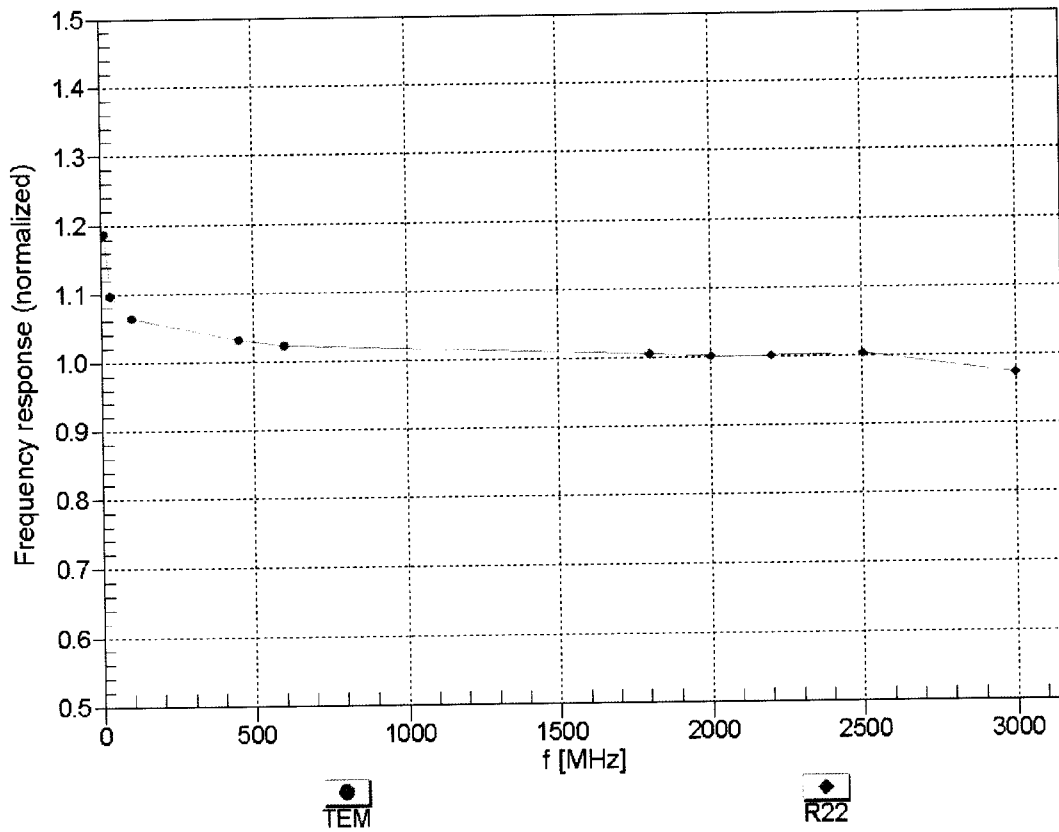


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

Receiving Pattern (ϕ), $\vartheta = 0^\circ$



f=600 MHz, TEM

f=1800 MHz, R22

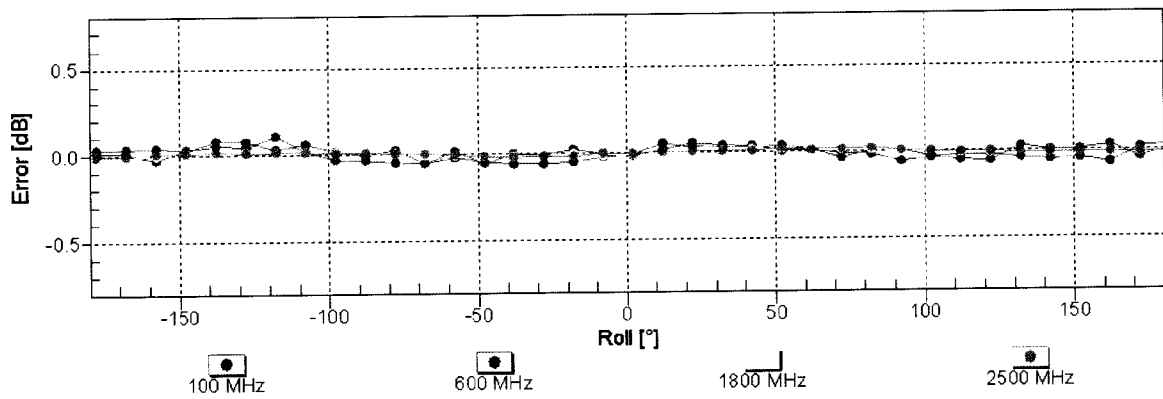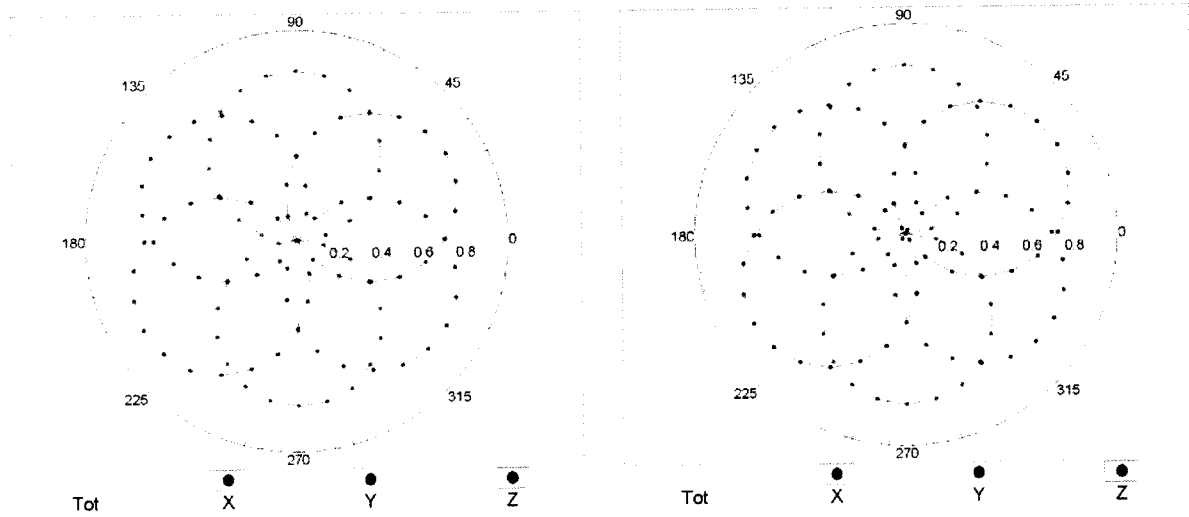


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

Dynamic Range $f(SAR_{head})$ (TEM cell , $f_{eval}= 1900$ MHz)

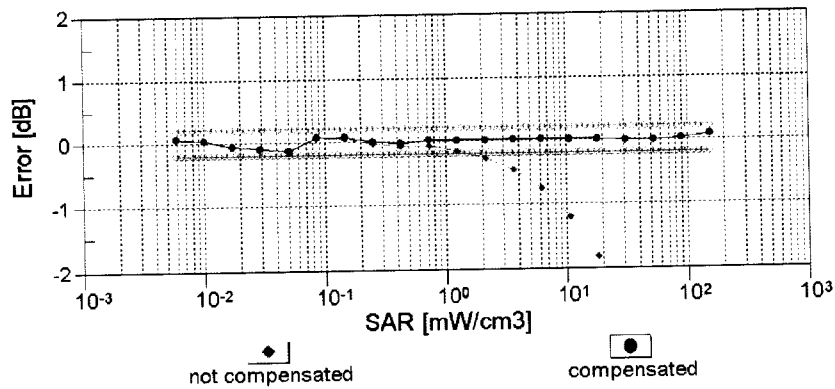
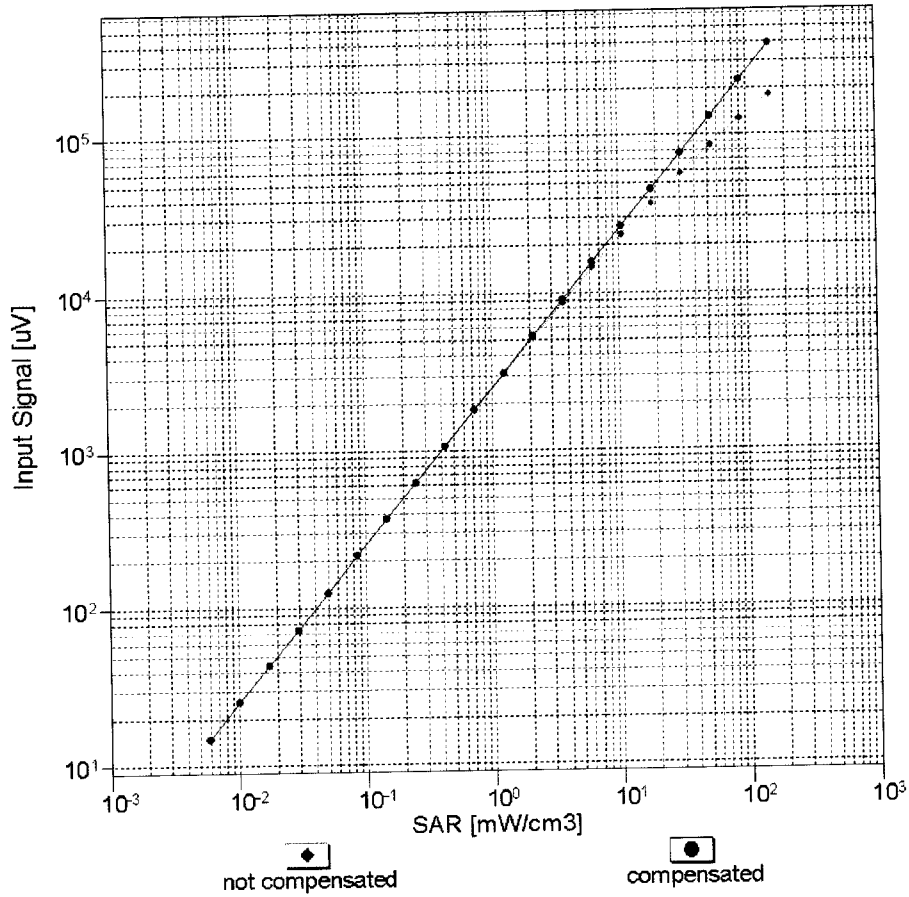


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Conversion Factor Assessment

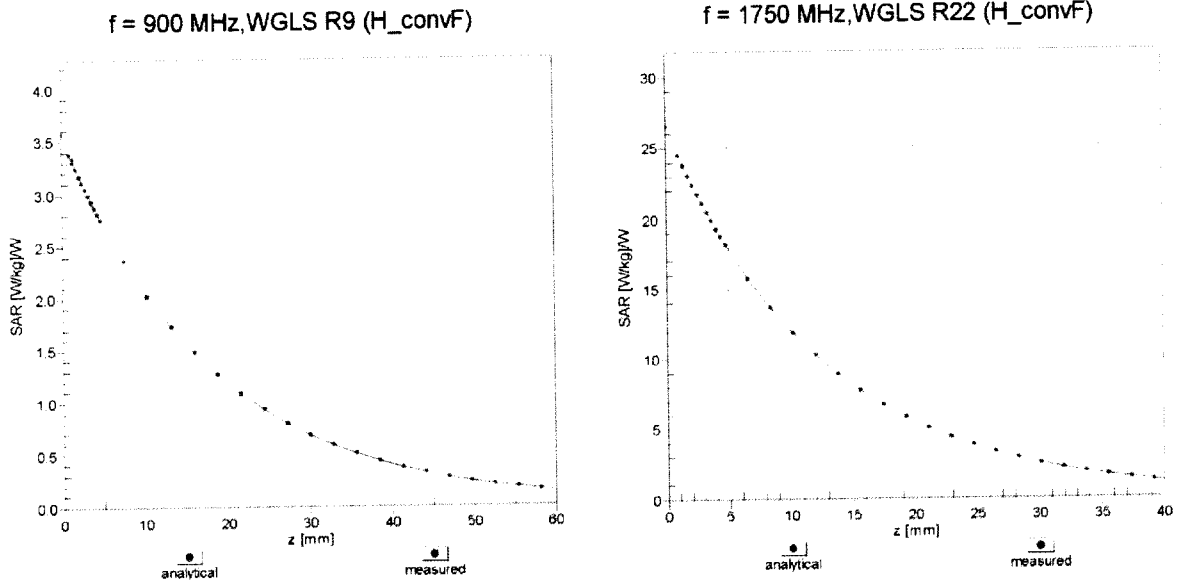

Deviation from Isotropy in Liquid Error (ϕ, ϑ), f = 900 MHz

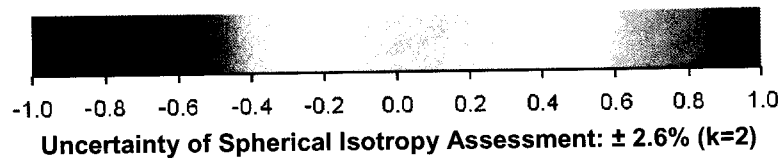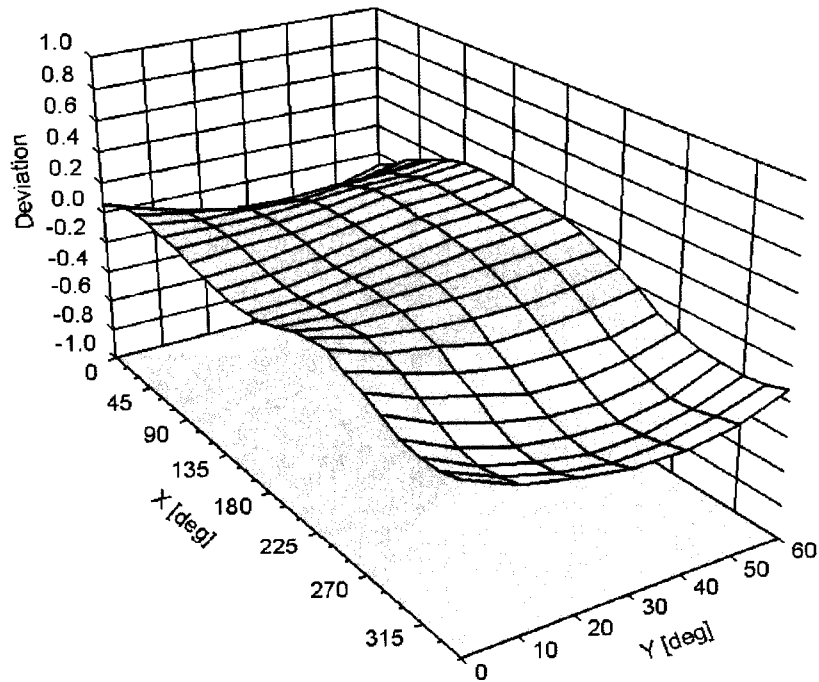

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3833**Other Probe Parameters**

| | |
|---|------------|
| Sensor Arrangement | Triangular |
| Connector Angle (°) | 12.2 |
| Mechanical Surface Detection Mode | enabled |
| Optical Surface Detection Mode | disabled |
| Probe Overall Length | 337 mm |
| Probe Body Diameter | 10 mm |
| Tip Length | 9 mm |
| Tip Diameter | 2.5 mm |
| Probe Tip to Sensor X Calibration Point | 1 mm |
| Probe Tip to Sensor Y Calibration Point | 1 mm |
| Probe Tip to Sensor Z Calibration Point | 1 mm |
| Recommended Measurement Distance from Surface | 1.4 mm |

Appendix E – Dipole Calibration Data Sheets

NCL CALIBRATION LABORATORIES

Calibration File No: DC-1474

Project Number: RFEL-5706

C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Validation Dipole

Manufacturer: APREL Laboratories

Part number: ALS-D-1640-S-2

Frequency: 1640 MHz

Serial No: 207-00101

Customer: RFEL

Head and Body Calibration

Calibrated: 16th January 2013
Released on: 17th January 2013

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By:



Art Brennan, Quality Manager

NCL CALIBRATION LABORATORIES

303 Terry Fox Drive, Suite 102
Kanata, Ontario
CANADA K2K 3J1

Division of APREL
TEL: (613) 435-8300
FAX: (613) 435-8306

NCL Calibration Laboratories

Division of APREL Laboratories.

Conditions

Dipole 207-00101 was a re-calibration..

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this subject has been accurately conducted and that all information contained within the results pages have been reviewed for accuracy.



Art Brennan, Quality Manager



Dan Brooks, Test Engineer

Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions

Length: 80.4 mm
Height: 45.7 mm


Electrical Calibration

| Test | Result Head | Result Body |
|-----------|-------------|-------------|
| S11 R/L | -27.230 dB | -21.566 dB |
| SWR | 1.092 U | 1.182 U |
| Impedance | 50.157 Ω | 46.306 Ω |

This page has been reviewed for content and attested to by signature within this document.


System Validation Results Head

| Frequency | 1 Gram | 10 Gram | Peak |
|------------------|---------------|----------------|-------------|
| 1640 MHz | 34.244 | 18.425 | 38.8 |

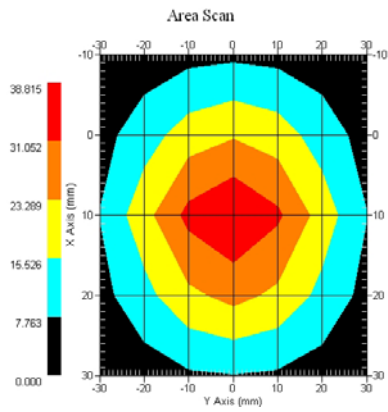

System Validation Results Body

| Frequency | 1 Gram | 10 Gram | Peak |
|------------------|---------------|----------------|-------------|
| 1640 MHz | 32.82 | 17.78 | 38.02 |

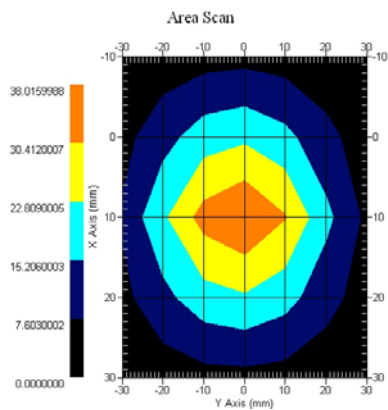

Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole 207-00101. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-020 130 MHz to 26 GHz E-Field Probe Serial Number 212.

References

SSI-TP-018-ALSAS Dipole Calibration Procedure

SSI-TP-016 Tissue Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

Conditions

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C

Temperature of the Tissue: 20 °C +/- 0.5°C

Dipole Calibration Results

Mechanical Verification

| APREL Length | APREL Height | Measured Length | Measured Height |
|---------------------|---------------------|------------------------|------------------------|
| 80.4 mm | 45.7 mm | 80.4 mm | 45.6 mm |

Tissue Validation

| Tissue 450MHz | Measured Head | Measured Body |
|---|----------------------|----------------------|
| Dielectric constant, ϵ_r | 38.5 | 52.03 |
| Conductivity, σ [S/m] | 1.25 | 1.39 |

Dipole Calibration uncertainty

The calibration uncertainty for the dipole is made up of various parameters presented below.

| | |
|--------------------------|---------------------------|
| Mechanical | 1% |
| Positioning Error | 1.22% |
| Electrical | 1.7% |
| Tissue | 2.2% |
| Dipole Validation | 2.2% |
| TOTAL | 8.32% (16.64% K=2) |


Electrical Calibration

| Test | Result Head | Result Body |
|-----------|-----------------|-----------------|
| S11 R/L | -27.230 dB | -21.566 dB |
| SWR | 1.092 U | 1.182 U |
| Impedance | 50.157 Ω | 46.306 Ω |


The Following Graphs are the results as displayed on the Vector Network Analyzer.

S11 Parameter Return Loss

HEAD

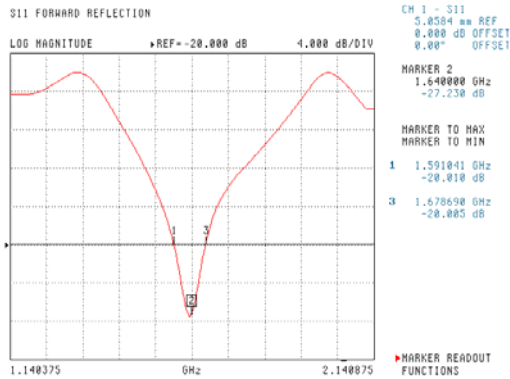


BODY

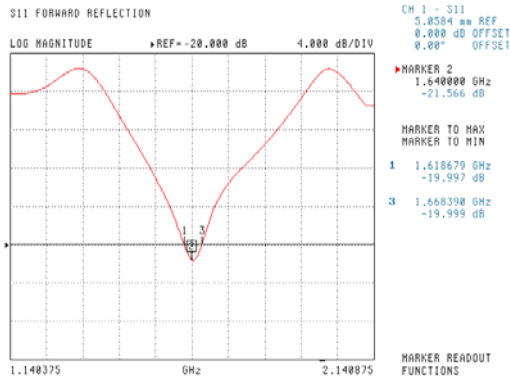


SWR


HEAD

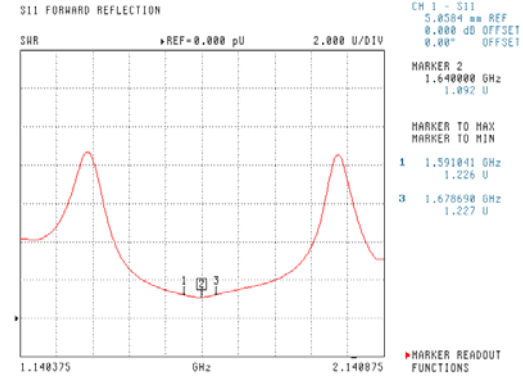


BODY

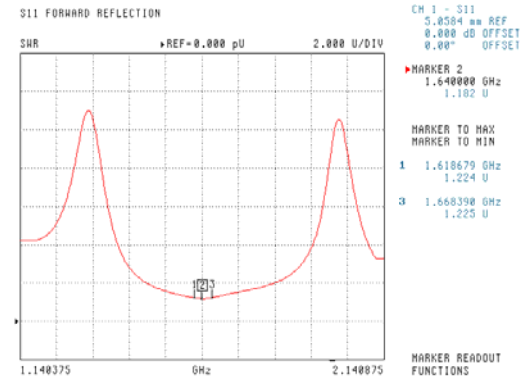

Smith Chart Dipole Impedance HEAD

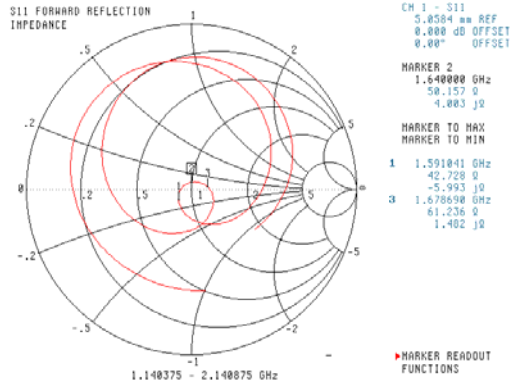

BODY

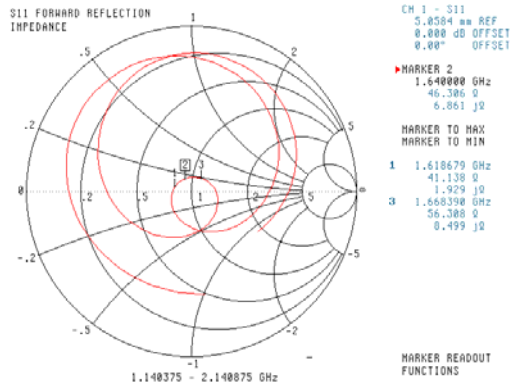

NCL Calibration Laboratories

Division of APREL Laboratories.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2012.

Extended Calibration

Usage of SAR dipoles calibrated less than 2 years ago but more than 1 year ago were confirmed in maintaining return loss (< -20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r03.

| ALS-D-1640-S-2 SN: 207-00101 - Head | | | | | | |
|-------------------------------------|------------------|------------|------------------------|----------------|-----------------------------------|----------------|
| Date of Measurement | Return Loss (dB) | $\Delta\%$ | Impedance (Ω) | $\Delta\Omega$ | Impedance Imaginary ($j\Omega$) | $\Delta\Omega$ |
| 1/16/2013 | -27.23 | | 50.16 | | 4.003 | |
| 1/17/2014 | -26.57 | -2.4 | 49.67 | -0.49 | 3.986 | -0.017 |
| 1/16/2015 | -26.94 | -1.1 | 49.86 | -0.3 | 4.058 | 0.055 |

| ALS-D-1640-S-2 SN: 207-00101 - Body | | | | | | |
|-------------------------------------|------------------|------------|------------------------|----------------|-----------------------------------|----------------|
| Date of Measurement | Return Loss (dB) | $\Delta\%$ | Impedance (Ω) | $\Delta\Omega$ | Impedance Imaginary ($j\Omega$) | $\Delta\Omega$ |
| 1/16/2013 | -21.57 | | 46.31 | | 6.861 | |
| 1/17/2014 | -22.35 | 3.6 | 46.97 | 0.66 | 7.053 | 0.192 |
| 1/16/2015 | -22.06 | 2.3 | 45.87 | -0.44 | 6.952 | 0.091 |

Appendix F – Phantom Calibration Data Sheets

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Certificate of Conformity / First Article Inspection

| | |
|--------------|---|
| Item | Oval Flat Phantom ELI 4.0 |
| Type No | QD OVA 001 B |
| Series No | 1003 and higher |
| Manufacturer | Untersee Composites Knebelstrasse 8 CH-8268 Mannenbach, Switzerland |

Tests

Complete tests were made on the prototype units QD OVA 001 AA 1001, QD OVA 001 AB 1002, pre-series units QD OVA 001 BA 1003-1005 as well as on the series units QD OVA 001 BB, 1006 ff.

| Test | Requirement | Details | Units tested |
|----------------------|---|---|--------------------------------------|
| Material thickness | Compliant with the standard requirements | Bottom plate: 2.0mm +/- 0.2mm | all |
| Material parameters | Dielectric parameters for required frequencies | < 6 GHz: Rel. permittivity = 4 +/-1, Loss tangent ≤ 0.05 | Material sample |
| Material resistivity | The material has been tested to be compatible with the liquids defined in the standards if handled and cleaned according to the instructions. | DGBE based simulating liquids. Observe Technical Note for material compatibility. | Equivalent phantoms, Material sample |
| Shape | Thickness of bottom material, Internal dimensions, Sagging compatible with standards from minimum frequency | Bottom elliptical 600 x 400 mm Depth 190 mm, Shape is within tolerance for filling height up to 155 mm, Eventual sagging is reduced or eliminated by support via DUT | Prototypes, Sample testing |

Standards

- [1] CENELEC EN 50361-2001, « Basic standard for the measurement of the Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz – 3 GHz) », July 2001
- [2] IEEE 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques, December 2003
- [3] IEC 62209 – 1, "Specific Absorption Rate (SAR) in the frequency range of 300 MHz to 3 GHz – Measurement Procedure, Part 1: Hand-held mobile wireless communication devices", February 2005
- [4] IEC 62209 – 2, Draft, "Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices – Human models, Instrumentation and Procedures – Part 2: Procedure to determine the Specific Absorption Rate (SAR) in the head and body for 30 MHz to 6 GHz Handheld and Body-Mounted Devices used in close proximity to the Body.", February 2005
- [5] OET Bulletin 65, Supplement C, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields", Edition January 2001

Based on the tests above, we certify that this item is in compliance with the standards [1] to [5] if operated according to the specific requirements and considering the thickness. The dimensions are fully compliant with [4] from 30 MHz to 6 GHz. For the other standards, the minimum lower frequency limit is limited due to the dimensional requirements ([1]: 450 MHz, [2]: 300 MHz, [3]: 800 MHz, [5]: 375 MHz) and possibly further by the dimensions of the DUT.

Date 28.4.2008 Signature / Stamp

s p e a g
 Schmid & Partner Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com; http://www.speag.com