

Test report No. : 29CE0014-HO-01-C-R1  
Page : 54 of 89  
Issued date : January 26, 2009  
FCC ID : T87SS25BGXXT  
Revised date : January 19, 2009

---

### APPENDIX 3 : Test instruments

---

**UL Japan, Inc.**  
**Head Office EMC Lab.**  
4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN  
Telephone : +81 596 24 8116  
Facsimile : +81 596 24 8124

## 1. Equipment used

| Control No. | Name of Equipment                | Manufacture                   | Model number            | Serial number | Calibration |                         |
|-------------|----------------------------------|-------------------------------|-------------------------|---------------|-------------|-------------------------|
|             |                                  |                               |                         |               | Last Cal    | due date                |
| MPM-01      | Power Meter                      | Agilent                       | E4417A                  | 3008A01671    | 2008/02/06  | 2009/02/28              |
| MPSE-01     | Power Sensor                     | Agilent                       | E9300B                  | US40010300    | 2008/02/04  | 2009/02/28              |
| MPSE-03     | Power sensor                     | Agilent                       | E9327A                  | US40440576    | 2008/02/09  | 2009/02/28              |
| MAT-15      | Attenuator(30dB)                 | Agilent                       | 8498A                   | 100023        | 2008/02/21  | 2009/02/28              |
| MSG-10      | Signal Genelator                 | Agilent                       | N5181A                  | MY47421098    | 2008/06/16  | 2009/06/30              |
| MRFA-08     | Pre Amplifier                    | TSJ                           | TCBP0206                | -             | 2008/03/19  | 2009/03/30              |
| MHDC-12     | Dual Directional Coupler         | Hewlett Packard               | 772D                    | 2839A0016     | -           | -                       |
| MOS-12      | Thermo-Hygrometer                | Custom                        | CTH-180                 | -             | 2008/01/10  | 2009/01/31              |
| MPM-08      | Power Meter                      | Anritsu                       | ML2495A                 | 6K00003338    | 2008/09/24  | 2009/09/30              |
| MPSE-11     | Power sensor                     | Anritsu                       | MA2411B                 | 011737        | 2008/09/24  | 2009/09/30              |
| MAT-25      | Attenuator(10dB)(above 1G Hz)    | Agilent                       | 8493C                   | 71642         | 2008/06/25  | 2009/06/30              |
| MNA-01      | Network Analyzer                 | Agilent                       | E8358A                  | US41080381    | 2006/02/10  | 2009/02/28              |
| MNCK-01     | Type N Calibration Kit           | Agilent                       | 85032F                  | MY41495257    | 2006/02/08  | 2009/02/28              |
| MPB-03      | Dosimetric E-Field Probe         | Schmid&Partner Engineering AG | EX3DV3                  | 3507          | 2008/01/25  | 2009/01/31              |
| MDAE-01     | Data Acquisition Electronics     | Schmid&Partner Engineering AG | DAE3 V1                 | 509           | 2008/07/10  | 2009/07/31              |
| MSTW-16     | SAR/HAC measurement System       | Schmid&Partner Engineering AG | DASY4                   | I021834       | N/A         | N/A                     |
| MDA-07      | 2450MHz System Validation Dipole | Schmid&Partner Engineering AG | D2450V2                 | 713           | 2008/09/08  | 2010/09/30              |
| MPF-02      | 2mm Flat phantom ERI4.0          | Schmid&Partner Engineering AG | 2mm Flat phantom ERI4.0 | 1045          | -           | -                       |
| MDPK-01     | Dielectric probe kit             | Agilent                       | 85070D                  | -             | -           | -                       |
| MOS-05      | Thermo-Hygrometer                | Custom                        | CTH-190                 | 810201        | 2008/04/03  | 2009/04/30              |
| MOS-10      | Digital thermometer              | HANNA                         | Checktemp-2             | -             | 2007/03/23  | 2009/03/31              |
| -           | Head 2450MHz                     | -                             | -                       | -             | Daily check | Target value $\pm$ 5%   |
| -           | Muscle 2450MHz                   | -                             | -                       | -             | Daily check | Target value $\pm$ 5%   |
| -           | SAR room                         | -                             | -                       | -             | Daily check | Ambient Noise<0.012W/kg |

## UL Japan, Inc.

### Head Office EMC Lab.

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

## 2. Dosimetry assessment setup

These measurements were performed with the automated near-field scanning system DASY4 from Schmid & Partner Engineering AG (SPEAG). The system is based on a high precision robot (working range greater than 0.9 m), which positions the probes with a positional repeatability of better than +/- 0.02 mm. Special E- and H-field probes have been developed for measurements close to material discontinuity, the sensors of which are directly loaded with a Schottky diode and connected via highly resistive lines to the data acquisition unit. The SAR measurements were conducted with the dosimetry probe ET3DV6, SN: 1700 (manufactured by SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe has been calibrated according to the procedure described in [2] with accuracy of better than +/-10%. The spherical isotropy was evaluated with the procedure described in [3] and found to be better than +/-0.25 dB. The phantom used was the SAM Twin Phantom as described in FCC supplement C, IEEE P1528 and CENELEC EN50361.

---

**UL Japan, Inc.**


**Head Office EMC Lab.**

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

### 3. Configuration and peripherals

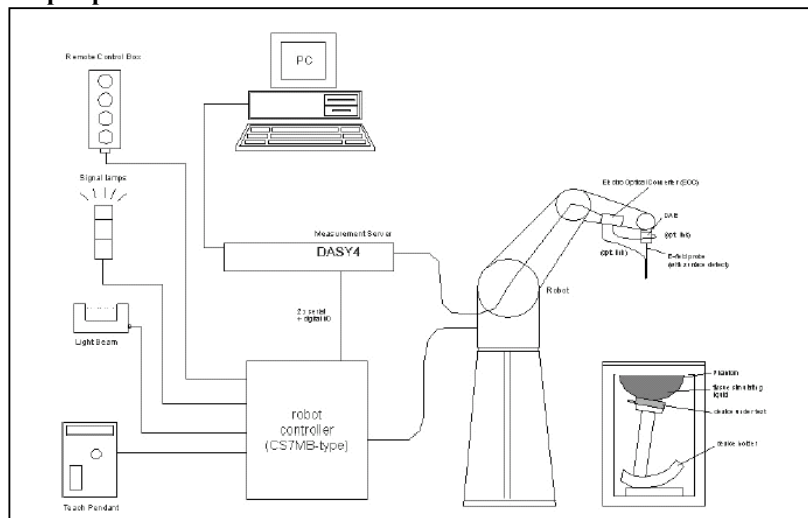

The DASY4 system for performing compliance tests consist of the following items:

1. A standard high precision 6-axis robot (Stäubli RX family) with controller and software.  
An arm extension for accommodating the data acquisition electronics (DAE).
2. A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
3. A data acquisition electronic (DAE), which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
4. The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection.  
The EOC is connected to the measurement server.
5. The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
6. A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
7. A computer operating Windows XP.
8. DASY4 software.
9. Remote control with teaches pendant and additional circuitry for robot safety such as warning lamps, etc.
10. The 2mm Flat phantom ERI4.0 enabling testing left-hand and right-hand usage.
11. The device holder for handheld mobile phones.
12. Tissue simulating liquid mixed according to the given recipes.
13. Validation dipole kits allowing to validate the proper functioning of the system.

---

#### UL Japan, Inc.

##### Head Office EMC Lab.

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

#### 4. System components

##### EX3DV3 Probe Specification

**Construction:**

Symmetrical design with triangular core  
Built-in shielding against static charges  
PEEK enclosure material (resistant to organic solvents, e.g., glycol ether)

**Calibration:**

Basic Broad Band calibration in air : 10-3000 MHz

**Conversion Factors (Head and Body):**

900 MHz, 1640MHz, 1810MHz, 2000MHz, 2450MHz,  
5.2GHz, 5.5GHz and 5.8GHz (Head and Body)

**Frequency:**

10 MHz to > 6GHz; Linearity: +/-0.2 dB (30 MHz to 3 GHz)

**Directivity:**

+/-0.3 dB in HSL (rotation around probe axis)  
+/-0.5 dB in tissue material (rotation normal probe axis)

**Dynamic Range:**

10uW/g to > 100 mW/g; Linearity: +/-0.2 dB (noise: typically < 1uW/g)

**Dimensions:**

Overall length: 330 mm (Tip: 20 mm)  
Tip diameter: 2.5mm (Body: 12 mm)  
Typical distance from probe tip to dipole centers: 1 mm

**Application:**

High precision dosimetric measurement in any exposure scenario  
(e.g., very strong gradient fields). Only probe which enables compliance  
testing for frequencies up to 6GHz with precision of better 30%.



**EX3DV3 E-field Probe**

---

**UL Japan, Inc.**

**Head Office EMC Lab.**

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

## 2mm Flat phantom ERI4.0

### Description

Phantom for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30 MHz to 6 GHz. ELI4 is fully compatible with the latest draft of the standard IEC 62209 Part II and all known tissue simulating liquids. ELI4 has been optimized regarding its performance and can be integrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points. The phantom is supported by software version DASY4.5 and higher and is compatible with all SPEAG dosimetric probes and dipoles.

### Shell Thickness

2.0 ± 0.2 mm (sagging: <1%)

### Filling Volume

approx. 30 liters

### Dimensions

Major ellipse axis: 600 mm

Minor axis: 400 mm

### Compatibilities

- Standard: IEC 62209 Part II (Draft 0.9 and higher)
- Software release: DASY 4.5 or higher
- SPEAG standard phantom table
- all SPEAG dosimetric probes and dipoles

### Device Holder

For this measurement, the urethane foam was used as device holder.

---

## UL Japan, Inc.

### Head Office EMC Lab.

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

## 5. Test system specifications

### Robot RX60L

|                      |   |   |
|----------------------|---|---|
| Number of Axes       | : | 6   |
| Payload              | : | 1.6 kg                                    |
| Reach                | : | 800mm                                     |
| Repeatability        | : | +/-0.025mm                                |
| Control Unit         | : | CS7M                                      |
| Programming Language | : | V+  |
| Manufacture          | : | Stäubli Unimation Corp. Robot Model: RX60 |

### DASY4 Measurement server

|             |   |  |
|-------------|---|--|
| Features    | : | 166MHz low power Pentium MMX 32MB chipdisk and 64MB RAM<br>Serial link to DAE (with watchdog supervision)<br>16 Bit A/D converter for surface detection system<br>Two serial links to robot (one for real-time communication which is supervised by watchdog)<br>Ethernet link to PC (with watchdog supervision)<br>Emergency stop relay for robot safety chain<br>Two expansion slots for future applications |
| Manufacture | : | Schimid & Partner Engineering AG   |

### Data Acquisition Electronic (DAE)

|                      |   |   |
|----------------------|---|---|
| Features             | : | Signal amplifier, multiplexer, A/D converter and control logic<br>Serial optical link for communication with DASY4 embedded system (fully remote controlled)<br>2 step probe touch detector for mechanical surface detection and emergency robot stop (not in -R version) |
| Measurement Range    | : | 1 $\mu$ V to > 200 mV (16 bit resolution and two range settings: 4mV, 400mV)  |
| Input Offset voltage | : | < 1 $\mu$ V (with auto zero)  |
| Input Resistance     | : | 200 M $\Omega$  |
| Battery Power        | : | > 10 h of operation (with two 9 V battery)  |
| Dimension            | : | 60 x 60 x 68 mm   |
| Manufacture          | : | Schimid & Partner Engineering AG  |

### Software

|                      |   |                                   |
|----------------------|---|-----------------------------------|
| Item                 | : | Dosimetric Assesment System DASY4 |
| Type No.             | : | SD 000 401A, SD 000 402A          |
| Software version No. | : | 4.6                               |
| Manufacture / Origin | : | Schimid & Partner Engineering AG  |

### E-Field Probe

|              |   |   |
|--------------|---|---|
| Model        | : | EX3DV3                                  |
| Serial No.   | : | 3507                                    |
| Construction | : | Symmetrical design with triangular core |
| Frequency    | : | 10 MHz to 6 GHz                         |
| Linearity    | : | +/-0.2 dB (30 MHz to 3 GHz)             |
| Manufacture  | : | Schimid & Partner Engineering AG        |

### Phantom

|                 |   |   |
|-----------------|---|---|
| Type            | : | 2mm   |
| Shell Thickness | : | 2.0 $\pm$ 0.2 mm (sagging: <1%)               |
| Filling Volume  | : | approx. 30 liters                             |
| Dimensions      | : | Major ellipse axis: 600 mm Minor axis: 400 mm |
| Manufacture     | : | Schimid & Partner Engineering AG              |

---

## UL Japan, Inc.

### Head Office EMC Lab.

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

**6. Simulated Tissues Composition of 2450MHz**

| Ingredient | MIXTURE(%)   |                |
|------------|--------------|----------------|
|            | Head 2450MHz | Muscle 2450MHz |
| Water      | 45.0         | 69.83          |
| DGMBE      | 55.0         | 30.2           |

Note:DGMBE(Diethylenglycol-monobuthyl ether)

**7. Validation Measurement**

**Simulated tissue liquid parameter**

**7-a Simulated Tissue Liquid Parameter confirmation**

The dielectric parameters were checked prior to assessment using the HP85070D dielectric probe kit. The dielectric parameters measurement are reported in each correspondent section.

**7-b Head 2450 MHz**

Type of liquid : **Head 2450 MHz**  
Ambient temperature (deg.c.) : **24.5 (Dec-17)**  
Relative Humidity (%) : **32(Dec-17)**  
Liquid depth (cm) : **15.0**

| DIELECTRIC PARAMETERS MEASUREMENT RESULTS |           |                     |       |                                    |                |          |               |           |
|---|-----------|---------------------|-------|------------------------------------|----------------|----------|---------------|-----------|
| Date                                      | Frequency | Liquid Temp [deg.c] |       | Parameters                         | Target Value*1 | Measured | Deviation [%] | Limit [%] |
|   |           | Before              | After |                                    |                |          |               |           |
| 17-Dec                                    | 2450      | 24.2                | 24.2  | Relative Permittivity $\epsilon_r$ | 39.2           | 37.5     | -4.3          | +/-5      |
|   |           |                     |       | Conductivity $\sigma$ [mho/m]      | 1.80           | 1.87     | 3.9           | +/-5      |

\*1 The target values is a parameter defined in FCC OET 65.

| DIELECTRIC PARAMETERS MEASUREMENT RESULTS |           |                     |       |                                    |                |          |               |           |
|---|-----------|---------------------|-------|------------------------------------|----------------|----------|---------------|-----------|
| Date                                      | Frequency | Liquid Temp [deg.c] |       | Parameters                         | Target Value*2 | Measured | Deviation [%] | Limit [%] |
|   |           | Before              | After |                                    |                |          |               |           |
| 17-Dec                                    | 2450      | 24.2                | 24.2  | Relative Permittivity $\epsilon_r$ | 39.8           | 37.5     | -5.8          | +/-10     |
|   |           |                     |       | Conductivity $\sigma$ [mho/m]      | 1.80           | 1.87     | 3.9           | +/-10     |

\*2 The target value is the calibrated dipole Head TSL parameters. (D2450V2 SN:713)



**7-c Muscle 2450 MHz**

Type of liquid : **Muscle 2450 MHz**  
 Ambient temperature (deg.c.) : **24.5 (Dec-17)**  
 Relative Humidity (%) : **32(Dec-17)**  
 Liquid depth (cm) : **15.0**

| DIELECTRIC PARAMETERS MEASUREMENT RESULTS |           |                     |       |                                    |                |          |               |           |
|---|-----------|---------------------|-------|------------------------------------|----------------|----------|---------------|-----------|
| Date                                      | Frequency | Liquid Temp [deg.c] |       | Parameters                         | Target Value*1 | Measured | Deviation [%] | Limit [%] |
|   |           | Before              | After |                                    |                |          |               |           |
| 17-Dec                                    | 2450      | 24.0                | 24.0  | Relative Permittivity $\epsilon_r$ | 52.7           | 50.1     | -4.9          | +/-5      |
|   |           |                     |       | Conductivity $\sigma$ [mho/m]      | 1.95           | 1.98     | 1.5           | +/-5      |

\*1 The target values is a parameter defined in FCC OET 65.

### 8. System validation data

Prior to the assessment, the system validation kit was used to test whether the system was operating within its specifications of +/-10%. The validation results are in the table below. Please refer to APPENDIX3.

#### System validation of 2450MHz

Type of liquid : HEAD 2450MHz  
Frequency : 2450MHz  
Ambient temperature (deg.c.) : 24.5 (Dec-17)  
Relative Humidity (%) : 32(Dec-17)  
Dipole : D2450V2 SN:713  
Power : 250mW



| SYSTEM PERFORMANCE CHECK |                       |       |                                    |          |                               |          |  |          |               |           |
|--------------------------|-----------------------|-------|------------------------------------|----------|-------------------------------|----------|--|----------|---------------|-----------|
| Date                     | Liquid (HEAD 2450MHz) |       |                                    |          |                               |          | System dipole validation target & measured |          |               |           |
|                          | Liquid Temp [deg.c.]  |       | Relative Permittivity $\epsilon_r$ |          | Conductivity $\sigma$ [mho/m] |          | SAR 1g [W/kg]                              |          | Deviation [%] | Limit [%] |
|                          | Before                | After | Target                             | Measured | Target                        | Measured | Target*1                                   | Measured |               |           |
| 17-Dec                   | 24.1                  | 24.1  | 39.2                               | 37.5     | 1.80                          | 1.87     | 13.1                                       | 13.7     | 4.6           | +/-10     |

\*1 The target values is a 1g SAR value defined in IEEE Standard 1528.

| SYSTEM PERFORMANCE CHECK |                       |       |                                    |          |                               |          |  |          |               |           |
|--------------------------|-----------------------|-------|------------------------------------|----------|-------------------------------|----------|--|----------|---------------|-----------|
| Date                     | Liquid (HEAD 2450MHz) |       |                                    |          |                               |          | System dipole validation target & measured |          |               |           |
|                          | Liquid Temp [deg.c.]  |       | Relative Permittivity $\epsilon_r$ |          | Conductivity $\sigma$ [mho/m] |          | SAR 1g [W/kg]                              |          | Deviation [%] | Limit [%] |
|                          | Before                | After | Target                             | Measured | Target                        | Measured | Target*2                                   | Measured |               |           |
| 17-Dec                   | 24.1                  | 24.1  | 39.8                               | 37.5     | 1.80                          | 1.87     | 12.7                                       | 13.7     | 7.9           | +/-10     |

\*2 The target value is a manufacturer calibrated dipole 1g SAR value. (D2450V2 SN:713)

Note: Please refer to Attachment for the result representation in plot format

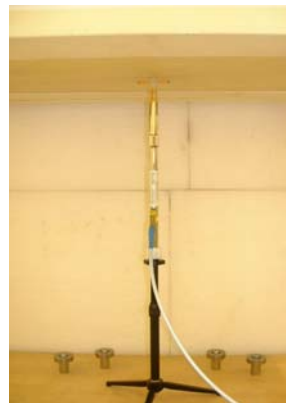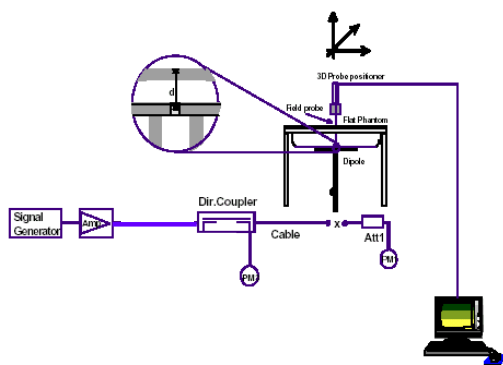

2450MHz System performance check setup

### Test system for the system performance check setup diagram

**UL Japan, Inc.**  
**Head Office EMC Lab.**  
4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN  
Telephone : +81 596 24 8116  
Facsimile : +81 596 24 8124

## 9. Validation uncertainty

The uncertainty budget has been determined for the DASY4 measurement system according to the SPEAG documents[6][7] and is given in the following Table.

| Error Description                    | Uncertainty value $\pm$ % | Probability distribution | divisor    | (ci) 1g | Standard Uncertainty (1g)      | vi or veff |
|--------------------------------------|---------------------------|--------------------------|------------|---------|--------------------------------|------------|
| <b>Measurement System</b>            |                           |                          |            |         |                                |            |
| Probe calibration                    | $\pm 6.8$                 | Normal                   | 1          | 1       | $\pm 6.8$                      | $\infty$   |
| Axial isotropy of the probe          | $\pm 4.7$                 | Rectangular              | $\sqrt{3}$ | 1       | $\pm 2.7$                      | $\infty$   |
| Spherical isotropy of the probe      | $\pm 9.6$                 | Rectangular              | 0          | 0       | 0                              | $\infty$   |
| Boundary effects                     | $\pm 2.0$                 | Rectangular              | $\sqrt{3}$ | 1       | $\pm 1.2$                      | $\infty$   |
| Probe linearity                      | $\pm 4.7$                 | Rectangular              | $\sqrt{3}$ | 1       | $\pm 2.7$                      | $\infty$   |
| Detection limit                      | $\pm 1.0$                 | Rectangular              | $\sqrt{3}$ | 1       | $\pm 0.6$                      | $\infty$   |
| Readout electronics                  | $\pm 0.3$                 | Normal                   | 1          | 1       | $\pm 0.3$                      | $\infty$   |
| Response time                        | 0                         | Rectangular              | $\sqrt{3}$ | 1       | 0                              | $\infty$   |
| Integration time                     | 0                         | Rectangular              | $\sqrt{3}$ | 1       | 0                              | $\infty$   |
| RF ambient Noise                     | $\pm 3.0$                 | Rectangular              | $\sqrt{3}$ | 1       | $\pm 1.7$                      | $\infty$   |
| RF ambient Reflections               | $\pm 3.0$                 | Rectangular              | $\sqrt{3}$ | 1       | $\pm 1.7$                      | $\infty$   |
| Probe Positioner                     | $\pm 0.8$                 | Rectangular              | $\sqrt{3}$ | 1       | $\pm 0.5$                      | $\infty$   |
| Probe positioning                    | $\pm 9.9$                 | Rectangular              | 1          | 1       | $\pm 5.7$                      | $\infty$   |
| Algorithms for Max.SAR Eval.         | $\pm 4.0$                 | Rectangular              | $\sqrt{3}$ | 1       | $\pm 2.3$                      | $\infty$   |
| <b>Dipole</b>                        |                           |                          |            |         |                                |            |
| Dipole Axis to Liquid Distance       | $\pm 2.0$                 | Rectangular              | $\sqrt{3}$ | 1       | $\pm 1.2$                      | $\infty$   |
| Input power and SAR drift meas.      | $\pm 4.7$                 | Rectangular              | $\sqrt{3}$ | 1       | $\pm 2.7$                      | $\infty$   |
| <b>Phantom and Setup</b>             |                           |                          |            |         |                                |            |
| Phantom uncertainty                  | $\pm 4.0$                 | Rectangular              | $\sqrt{3}$ | 1       | $\pm 2.3$                      | $\infty$   |
| Liquid conductivity (target)         | $\pm 5.0$                 | Rectangular              | $\sqrt{3}$ | 0.64    | $\pm 1.8$                      | $\infty$   |
| Liquid conductivity (meas.)          | $\pm 5.0$                 | Rectangular              | 1          | 0.64    | $\pm 3.2$                      | $\infty$   |
| Liquid permittivity (target)         | $\pm 5.0$                 | Rectangular              | $\sqrt{3}$ | 0.6     | $\pm 1.7$                      | $\infty$   |
| Liquid permittivity (meas.)          | $\pm 5.0$                 | Rectangular              | 1          | 0.6     | $\pm 3.0$                      | $\infty$   |
| <b>Combined Standard Uncertainty</b> |                           |                          |            |         | <b><math>\pm 12.079</math></b> |            |
| <b>Expanded Uncertainty (k=2)</b>    |                           |                          |            |         | <b><math>\pm 24.2</math></b>   |            |

**UL Japan, Inc.**

**Head Office EMC Lab.**

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

## 10. Validation Measurement data

### System Validation / Dipole 2450 MHz / Forward Conducted Power : 250mW

#### Dipole 2450MHz; Type: D2450V2; Serial: 713

Communication System: CW; Frequency:2450 MHz; Crest factor: 1

Medium: HSL2450 Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.87$  mho/m;  $\epsilon_r = 37.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3507; ConvF(7.99, 7.99, 7.99); Calibrated: 2008/01/25

- Sensor-Surface: 2mm (Mechanical Surface Detection)

- Phantom: Flat Phantom ELI4.0

- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

**Area Scan (61x61x1):** Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 22.7 mW/g

**Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 107.5 V/m; Power Drift = -0.001 dB

Peak SAR (extrapolated) = 30.0 W/kg


**SAR(1 g) = 13.7 mW/g; SAR(10 g) = 6.19 mW/g**

Maximum value of SAR (measured) = 21.3 mW/g

Test Date = 12/17/08

Ambient Temperature = 24.5 degree.c

Liquid Temperature = Before 24.1 degree.C , After 24.1 degree.C

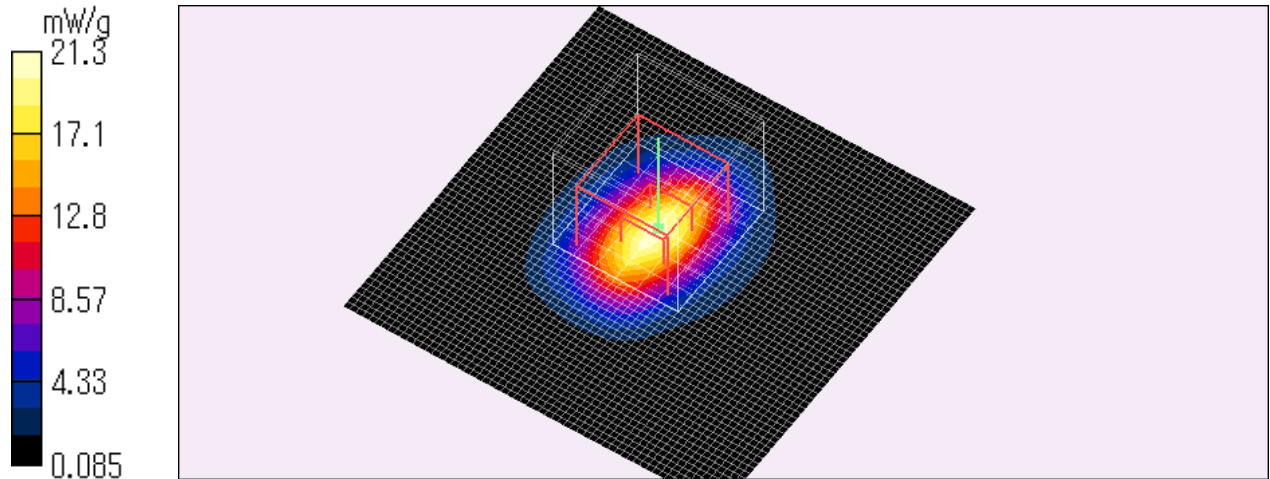

**UL Japan, Inc.**

**Head Office EMC Lab.**

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

11. System Validation Dipole (D2450V2,S/N: 713)

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client **UL Japan (MTT)**

Certificate No: **D2450V2-713\_Sep08**

**CALIBRATION CERTIFICATE**

Object **D2450V2 - SN: 713**

Calibration procedure(s) **QA CAL-05.v7  
Calibration procedure for dipole validation kits**

Calibration date: **September 08, 2008**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)     | Scheduled Calibration |
|-----------------------------|--------------------|--------------------------------|-----------------------|
| Power meter EPM-442A        | GB37480704         | 04-Oct-07 (No. 217-00736)      | Oct-08                |
| Power sensor HP 8481A       | US37292783         | 04-Oct-07 (No. 217-00736)      | Oct-08                |
| Reference 20 dB Attenuator  | SN: S5086 (20g)    | 01-Jul-08 (No. 217-00864)      | Jul-09                |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 01-Jul-08 (No. 217-00867)      | Jul-09                |
| Reference Probe ES3DV2      | SN: 3025           | 28-Apr-08 (No. ES3-3025_Apr08) | Apr-09                |
| DAE4                        | SN: 601            | 14-Mar-08 (No. DAE4-601_Mar08) | Mar-09                |

| Secondary Standards       | ID #             | Check Date (in house)             | Scheduled Check        |
|---------------------------|------------------|-----------------------------------|------------------------|
| Power sensor HP 8481A     | MY41092317       | 18-Oct-02 (in house check Oct-07) | In house check: Oct-09 |
| RF generator R&S SMT-06   | 100005           | 4-Aug-99 (in house check Oct-07)  | In house check: Oct-09 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-07) | In house check: Oct-08 |

|                | Name           | Function              | Signature |
|----------------|----------------|-----------------------|-----------|
| Calibrated by: | Jeton Kastrati | Laboratory Technician |           |
| Approved by:   | Katja Pokovic  | Technical Manager     |           |

Issued: September 9, 2008

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**UL Japan, Inc.**  
**Head Office EMC Lab.**  
4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN  
Telephone : +81 596 24 8116  
Facsimile : +81 596 24 8124



**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- d) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

**UL Japan, Inc.**

**Head Office EMC Lab.**

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

|                              |                           |             |
|------------------------------|---------------------------|-------------|
| DASY Version                 | DASY5                     | V5.0        |
| Extrapolation                | Advanced Extrapolation    |             |
| Phantom                      | Modular Flat Phantom V5.0 |             |
| Distance Dipole Center - TSL | 10 mm                     | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm         |             |
| Frequency                    | 2450 MHz ± 1 MHz          |             |

**Head TSL parameters**

The following parameters and calculations were applied.

|                                  | Temperature     | Permittivity | Conductivity     |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters      | 22.0 °C         | 39.2         | 1.80 mho/m       |
| Measured Head TSL parameters     | (22.0 ± 0.2) °C | 39.8 ± 6 %   | 1.80 mho/m ± 6 % |
| Head TSL temperature during test | (22.0 ± 0.2) °C | ----         | ----             |

**SAR result with Head TSL**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                                  |
|---|--------------------|----------------------------------|
| SAR measured  | 250 mW input power | 12.7 mW / g                      |
| SAR normalized  | normalized to 1W   | 50.8 mW / g                      |
| SAR for nominal Head TSL parameters <sup>1</sup>      | normalized to 1W   | <b>51.2 mW /g ± 17.0 % (k=2)</b> |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                                  |
|---|--------------------|----------------------------------|
| SAR measured  | 250 mW input power | 5.91 mW / g                      |
| SAR normalized  | normalized to 1W   | 23.6 mW / g                      |
| SAR for nominal Head TSL parameters <sup>1</sup>        | normalized to 1W   | <b>23.8 mW /g ± 16.5 % (k=2)</b> |

<sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

**UL Japan, Inc.**

**Head Office EMC Lab.**

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

**Body TSL parameters**

The following parameters and calculations were applied.

|                                  | Temperature     | Permittivity | Conductivity     |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters      | 22.0 °C         | 52.7         | 1.95 mho/m       |
| Measured Body TSL parameters     | (22.0 ± 0.2) °C | 50.7 ± 6 %   | 1.97 mho/m ± 6 % |
| Body TSL temperature during test | (22.5 ± 0.2) °C | ---          | ---              |

**SAR result with Body TSL**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                                   |
|---|--------------------|-----------------------------------|
| SAR measured  | 250 mW input power | 12.1 mW / g                       |
| SAR normalized  | normalized to 1W   | 48.4 mW / g                       |
| SAR for nominal Body TSL parameters <sup>2</sup>      | normalized to 1W   | <b>47.1 mW / g ± 17.0 % (k=2)</b> |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                                   |
|---|--------------------|-----------------------------------|
| SAR measured  | 250 mW input power | 5.68 mW / g                       |
| SAR normalized  | normalized to 1W   | 22.7 mW / g                       |
| SAR for nominal Body TSL parameters <sup>2</sup>        | normalized to 1W   | <b>22.3 mW / g ± 16.5 % (k=2)</b> |

<sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

**UL Japan, Inc.**

**Head Office EMC Lab.**

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124



## Appendix

### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 51.8 $\Omega$ + 1.6 j $\Omega$ |
| Return Loss                          | - 32.7 dB                      |

### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 48.2 $\Omega$ + 3.5 j $\Omega$ |
| Return Loss                          | - 28.1 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.159 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.  
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |               |
|-----------------|---------------|
| Manufactured by | SPEAG         |
| Manufactured on | July 05, 2002 |

---

**UL Japan, Inc.**

**Head Office EMC Lab.**

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

**DASY5 Validation Report for Head TSL**

Date/Time: 08.09.2008 12:47:07

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN713**

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U10 BB

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.8$  mho/m;  $\epsilon_r = 39.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC)

DASY5 Configuration:

- Probe: ES3DV2 - SN3025; ConvF(4.4, 4.4, 4.4); Calibrated: 28.04.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 14.03.2008
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY5, V5.0 Build 119; SEMCAD X Version 13.2 Build 87


**Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.8 V/m; Power Drift = 0.012 dB

Peak SAR (extrapolated) = 26.7 W/kg

**SAR(1 g) = 12.7 mW/g; SAR(10 g) = 5.91 mW/g**

Maximum value of SAR (measured) = 15.3 mW/g

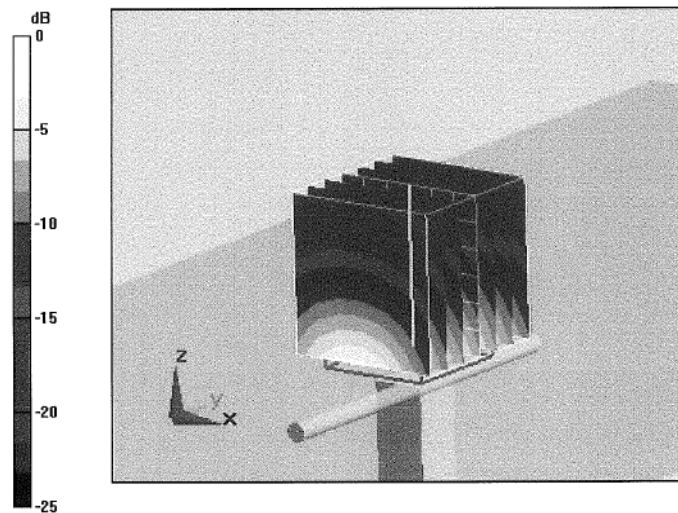

0 dB = 15.3mW/g

**UL Japan, Inc.**


**Head Office EMC Lab.**

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

**Impedance Measurement Plot for Head TSL**

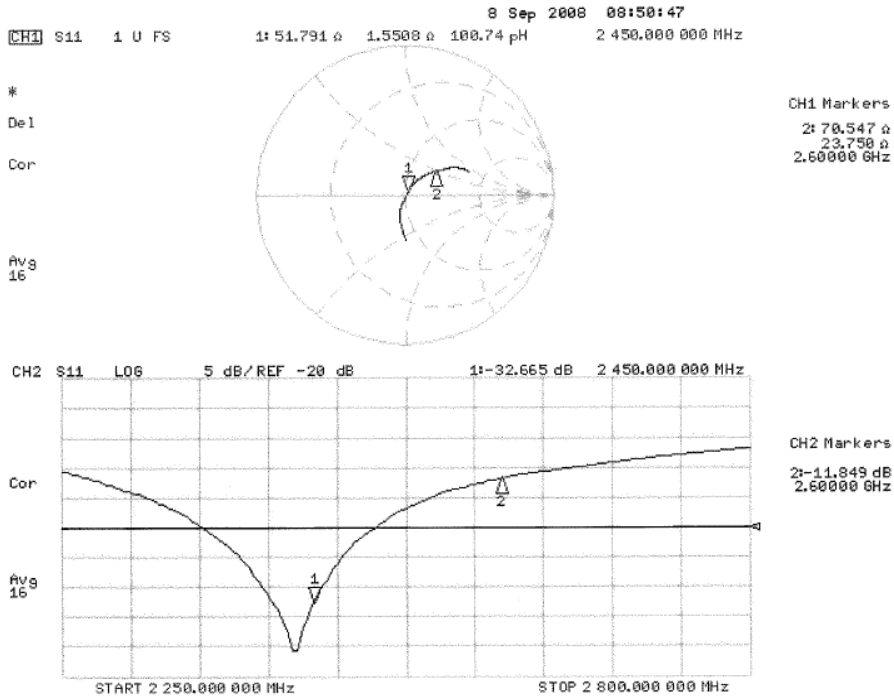

**DASY5 Validation Report for Body TSL**

Date/Time: 08.09.2008 15:47:52

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:713**

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U10 BB

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.96$  mho/m;  $\epsilon_r = 50.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC)

DASY5 Configuration:

- Probe: ES3DV2 - SN3025; ConvF(4.07, 4.07, 4.07); Calibrated: 28.04.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 14.03.2008
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY5, V5.0 Build 119; SEMCAD X Version 13.2 Build 87


**Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 90.5 V/m; Power Drift = 0.00036 dB

Peak SAR (extrapolated) = 24 W/kg

**SAR(1 g) = 12.1 mW/g; SAR(10 g) = 5.68 mW/g**

Maximum value of SAR (measured) = 15.1 mW/g

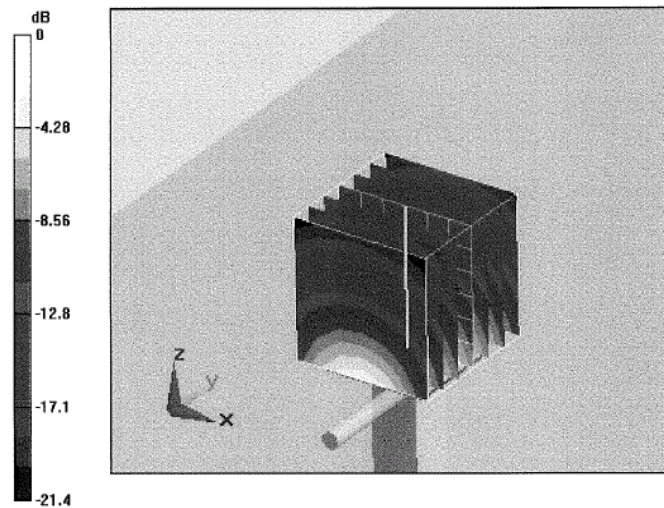

0 dB = 15.1mW/g

**UL Japan, Inc.**

**Head Office EMC Lab.**

4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 JAPAN

Telephone : +81 596 24 8116

Facsimile : +81 596 24 8124

**Impedance Measurement Plot for Body TSL**

