



# RF EXPOSURE LAB, LLC

2867 Progress Place, Suite 4D • Escondido, CA 92029 • U.S.A.  
TEL (760) 737-3131 • FAX (760) 737-9131  
<http://www.rfexposurelab.com>

## CERTIFICATE OF COMPLIANCE SAR EVALUATION

Cmotech Co., Ltd.  
8F Yongsan Bldg. 14-14  
Yido-Dong, Youngdunpo-Gu  
Seoul, South Korea 150-871

Dates of Test: September 21-22, 2009  
Test Report Number: SAR.20090902

FCC ID:	TARCMU-301
Model(s):	U-301, CMU-301, CMU-301S
Test Sample:	Engineering Unit Same as Production
Serial No.:	91
Equipment Type:	Wireless Modem
Classification:	Portable Transmitter Next to Body
TX Frequency Range:	824.7 – 848.31 MHz, 1851.25 – 1908.75 MHz, 2501 – 2685 MHz
Frequency Tolerance:	± 25 ppm
Maximum RF Output:	835 MHz – 23.91 dBm, 1900 MHz – 23.95 dBm, 2600 MHz – 23.89 dBm Conducted
Signal Modulation:	QPSK,16QAM
Antenna Type (Length):	Internal
Application Type:	Certification
FCC Rule Parts:	Part 22, 24, 27

This wireless mobile and/or portable device has been shown to be compliant for localized specific absorption rate (SAR) for uncontrolled environment/general exposure limits specified in ANSI/IEEE Std. C95.1-1999 and had been tested in accordance with the measurement procedures specified in IEEE 1528-2003, OET Bulletin 65 Supp. C, RSS-102 and Safety Code 6 (See test report).

I attest to the accuracy of the data. All measurements were performed by myself or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

RF Exposure Lab, LLC certifies that no party to this application has been denied FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 853(a).

Jay M. Moulton  
Vice President



Certificate # 2387.01

## Table of Contents

1. Introduction .....	3
SAR Definition [5].....	3
2. SAR Measurement Setup .....	4
Robotic System.....	4
System Hardware .....	4
System Description .....	4
E-Field Probe .....	5
3. Robot Specifications .....	7
4. Probe and Dipole Calibration .....	8
5. Phantom & Simulating Tissue Specifications.....	9
SAM Phantom.....	9
Brain & Muscle Simulating Mixture Characterization .....	9
Device Holder .....	9
6. Definition of Reference Points.....	10
Ear Reference Point.....	10
Device Reference Points .....	10
7. Test Configuration Positions .....	11
Positioning for Cheek/Touch [5].....	11
Positioning for Ear / 15° Tilt [5].....	12
Body Worn Configurations .....	13
8. ANSI/IEEE C95.1 – 1999 RF Exposure Limits [2].....	14
Uncontrolled Environment.....	14
Controlled Environment .....	14
9. Measurement Uncertainty.....	15
10. System Validation .....	16
Tissue Verification.....	16
Test System Verification .....	16
11. SAR Test Data Summary.....	17
Procedures Used To Establish Test Signal.....	17
Device Test Condition .....	17
12. FCC Measurement Procedures – March 2008 .....	18
12.1 Procedures Used to Establish RF Signal for SAR.....	18
12.2 SAR Measurement Conditions .....	18
SAR Data Summary – 835 MHz Body – EvDo .....	23
SAR Data Summary – 1900 MHz Body – EvDo .....	24
SAR Data Summary – 2600 MHz Body – WiMax QPSK ½ 5 MHz.....	25
SAR Data Summary – 2600 MHz Body – WiMax QPSK ½ 10 MHz.....	26
13. Test Equipment List .....	27
14. Conclusion .....	28
15. References.....	29
Appendix A – System Validation Plots and Data .....	30
Appendix B – SAR Test Data Plots.....	41
Appendix C – SAR Test Setup Photos .....	128
Appendix D – Probe Calibration Data Sheets.....	133
Appendix E – Dipole Calibration Data Sheets .....	164
Appendix F – Phantom Calibration Data Sheets .....	198

## 1. Introduction

This measurement report shows compliance of the Cmotech Co., Ltd. Model U301, CMU-301 and CMU-301S Family FCC ID: TARCMU-301 with FCC Part 2, 1093, ET Docket 93-62 Rules for mobile and portable devices. The FCC have adopted the guidelines for evaluating the environmental effects of radio frequency radiation in ET Docket 93-62 on August 6, 1996 to protect the public and workers from the potential hazards of RF emissions due to FCC regulated portable devices. [1], [6]

The test procedures, as described in ANSI C95.1 – 1999 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz [2], ANSI C95.3 – 2002 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields [3], FCC OET Bulletin 65 Supp. C – 2001 [4], IEEE Std.1528 – 2003 Recommended Practice [5], and Industry Canada Safety Code 6 Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz were employed.

For USB dongle transmitters, the device is required to be tested on all four sides of the modem. Two of the orientations (1 horizontal side and 1 vertical side) must be conducted installed in a laptop. The remaining two sides may be conducted at the end of 12" high quality USB extender cable.

### SAR Definition [5]

Specific Absorption Rate is defined as the time derivative (rate) of the incremental energy ( $dW$ ) absorbed by (dissipated in) an incremental mass ( $dm$ ) contained in a volume element ( $dV$ ) of a given density ( $\rho$ ).

$$SAR = \frac{d}{dt} \left( \frac{dW}{dm} \right) = \frac{d}{dt} \left( \frac{dW}{\rho dV} \right)$$

SAR is expressed in units of watts per kilogram (W/kg). SAR can be related to the electric field at a point by

$$SAR = \frac{\sigma |E|^2}{\rho}$$

where:

$\sigma$  = conductivity of the tissue (S/m)

$\rho$  = mass density of the tissue (kg/m<sup>3</sup>)

$E$  = rms electric field strength (V/m)

## 2. SAR Measurement Setup

### Robotic System

The measurements are conducted utilizing the ALSAS-10-U automated dosimetric assessment system. The ALSAS-10-U is designed and manufactured by Aprel Laboratories in Nepean, Ontario, Canada. The system utilizes a Robcomm 3 robot manufactured by ThermoCRS located in Michigan USA.

### System Hardware

The system consists of a six axis articulated arm, controller for precise probe positioning (0.05 mm repeatability), a power supply, a teach pendent for teaching area scans, near field probe, an IBM Pentium 4™ 2.66 GHz PC with Windows XP Pro™, and custom software developed to enable communications between the robot controller software and the host operating system.

An amplifier is located on the articulated arm, which is isolated from the custom designed end effector and robot arm. The end effector provides the mechanical touch detection functionality and probe connection interface. The amplifier is functionally validated within the manufacturer's site and calibrated at NCL Calibration Laboratories. A Data Acquisition Card (DAC) is used to collect the signal as detected by the isotropic e-field probe. The DAC manufacturer calibrates the DAC to NIST standards. A formal validation is executed using all mechanical and electronic components to prove conformity of the measurement platform as a whole.

### System Description

The ALSAS-10-U has been designed to measure devices within the compliance environment to meet all recognized standards. The system also conforms to standards, which are currently being developed by the scientific and manufacturing community.

The course scan resolution is defined by the operator and reflects the requirements of the standard to which the device is being tested. Precise measurements are made within the predefined course scan area and the values are logged.

The user predefines the sample rate for which the measurements are made so as to ensure that the full duty-cycle of a pulse modulation device is covered during the sample. The following algorithm is an example of the function used by the system for linearization of the output for the probe.

$$V_i = U_i + U_i^2 \bullet \frac{cf}{dcpi}$$



The Aprel E-Field probe is evaluated to establish the diode compression point.

A complex algorithm is then used to calculate the values within the measured points down to a resolution of 1mm. The data from this process is then used to provide the co-ordinates from which the cube scan is created for the determination of the 1 g and 10 g averages.

Cube scan averaging consists of a number of complex algorithms, which are used to calculate the one, and ten gram averages. The basis for the cube scan process is centered on the location where the maximum measured SAR value was found. When a secondary peak value is found which is within 60% of the initial peak value, the system will report this back to the operator who can then assess the need for further analysis of both the peak values prior to the one and ten-gram cube scan averaging process. The algorithm consists of 3D cubic Spline, and Lagrange extrapolation to the surface, which form the matrix for calculating the measurement output for the one and ten gram average values. The resolution for the physical scan integral is user defined with a final calculated resolution down to 1mm.

In-depth analysis for the differential of the physical scanning resolution for the cube scan analysis has been carried out, to identify the optimum setting for the probe positioning steps, and this has been determined at 8mm increments on the X, & Y planes. The reduction of the physical step increment increased the time taken for analysis but did not provide a better uncertainty or return on measured values.

The final output from the system provides data for the area scan measurements, physical and splined (1mm resolution) cube scan with physical and calculated values (1mm resolution).

The overall uncertainty for the methodology and algorithms the ALSAS-10-U used during the SAR calculation was evaluated using the data from IEEE 1528 f3 algorithm:

$$f_3(x, y, z) = A \frac{a^2}{\frac{a^2}{4} + x'^2 + y'^2} \left( e^{-\frac{2z}{a}} + \frac{a^2}{2(a + 2z)^2} \right)$$

The probe used during the measurement process has been assessed to provide values for diode compression. These values are calculated during the probe calibration exercise and are used in the mathematical calculations for the assessment of SAR.

## E-Field Probe

The E-field probe used by RF Exposure Lab, LLC, has been fully calibrated and assessed for isotropic, and boundary effect. The probe utilizes a triangular sensor arrangement as detailed in the diagram below right.



The SAR is assessed with the probe which moves at a default height of 5mm from the center of the diode, which is mounted to the sensor, to the phantom surface (Z height). The diagram above right shows how the center of the sensor is defined with the location of the diode placed at the center of the dipole. The 5mm default in the Z axis is the optimum height for assessing SAR where the boundary effect is at its least, with the probe located closest to the phantom surface (boundary).

The manufacturer specified precision of the robot is  $\pm 0.05$  mm and the precision of the APREL bottom detection device is  $\pm 0.1$  mm. These precisions are calibrated and tested in the manufacturing process of the bottom detection device. A constant distance is maintained because the surface of the phantom is dynamically detected for each point. The surface detection algorithm corrects the position of the robot so that the probe rests on the surface of the phantom. The probe is then moved to the measurement location 2.44 mm above the phantom surface resulting in the probe center location to be at 4.0 mm above the phantom surface. Therefore, the probe sensor will be at 4.0 mm above the phantom surface  $\pm 0.1$  mm for each SAR location for frequencies below 3 GHz. The probe is moved to the measurement location 1.44 mm above the phantom surface resulting in the probe center location to be at 2.0 mm above the phantom surface. Therefore, the probe sensor will be at 2.0 mm above the phantom surface  $\pm 0.1$  mm for each SAR location for frequencies above 3 GHz.

The probe boundary effect compensation cannot be disabled in the ALSAS-10U testing system. The probe tip will always be at least half a probe tip diameter from the phantom surface. For frequencies up to 3 GHz, the probe diameter is 5 mm. With the sensor offset set at 1.54 mm (default setting), the sensor to phantom gap will be 4.0 mm which is greater than half the probe tip diameter. For frequencies greater than 3 GHz, the probe diameter is 3 mm. With the sensor offset set at 0.56 mm (default setting), the sensor to phantom gap will be 3.0 mm which is greater than half the probe tip diameter.

The separation of the first 2 measurement points in the zoom scan is specified in the test setup software. For frequencies below 3 GHz, the user must specify a zoom scan resolution of less than 6 mm in the z-axis to have the first two measurements within 1 cm of the surface. The z-axis is set to 4 mm as shown on each of the data sheets in Appendix B. For frequencies above 3 GHz, the user must specify a zoom scan resolution of less than 3 mm in the z-axis to have the first two measurements within 5 mm of the surface. The z-axis is set to 2 mm as shown on each of the data sheets in Appendix B.

The zoom scan volume for devices  $\leq 3$  GHz with a cube scan of 5x5x8 yields a volume of  $32 \times 32 \times 28 \text{ mm}^3$ . For devices  $> 3$  GHz and  $< 4.5$  GHz, the cube scan of 9x9x9 yields a volume of  $32 \times 32 \times 24 \text{ mm}^3$ . For devices  $\geq 4.5$  GHz, the cube scan of 7x7x12 yields a volume of  $24 \times 24 \times 22 \text{ mm}^3$ .

### 3. Robot Specifications

#### Specifications

Positioner:	ThermoCRS, Robot Model: Robocomm 3
Repeatability:	0.05 mm
No. of axis:	6

#### Data Acquisition Card (DAC) System

#### Cell Controller

Processor:	Pentium 4™
Clock Speed:	2.66 GHz
Operating System:	Windows XP Pro™

#### Data Converter

Features:	Signal Amplifier, End Effector, DAC
Software:	ALSAS 10-U Software

#### E-Field Probe

Model:	Various See Probe Calibration Sheet
Serial Number:	Various See Probe Calibration Sheet
Construction:	Triangular Core Touch Detection System
Frequency:	10MHz to 6GHz

#### Phantom

Phantom:	Uniphantom, Right Phantom, Left Phantom
----------	---



## 4. Probe and Dipole Calibration

See Appendix D and E.

## 5. Phantom & Simulating Tissue Specifications

### SAM Phantom



The Aprel system utilizes three separate phantoms. Each phantom for SAR assessment testing is a low loss dielectric shell, with shape and dimensions derived from the anthropomorphic data of the 90<sup>th</sup> percentile adult male head dimensions as tabulated by the US Army. The SAM phantom shell is bisected along the mid sagittal plane into right and left halves. The perimeter sidewalls of each phantom half is extended to allow filling with liquid to a depth of 15 cm that is sufficient to minimize reflections from the upper surface [5]. The Uni-Phantom is used to conduct body measurements and head to face measurements. The depth of the phantom allows for 15 cm of tissue material to be filled within the phantom. See photos in Appendix C.

### Brain & Muscle Simulating Mixture Characterization

The brain and muscle mixtures consist of the material based on the table listed below. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the desired tissue. Body tissue parameters that have not been specified in P1528 are derived from the issue dielectric parameters computed from the 4-Cole-Cole equations.

**Table 5.1 Typical Composition of Ingredients for Tissue**

Ingredients	Simulating Tissue		
	835 MHz Muscle	1900 MHz Muscle	2600 MHz Muscle
Mixing Percentage			
Water	52.40	69.91	69.83
Sugar	45.00	0.00	0.00
Salt	1.40	0.13	0.00
HEC	1.00	0.00	0.00
Bactericide	0.10	0.00	0.00
DGBE	0.00	29.96	30.17
Dielectric Constant	Target	55.20	53.30
Conductivity (S/m)	Target	0.97	1.52
			2.16

### Device Holder




In combination with the SAM phantom, the mounting device enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation point is the ear opening. The devices can easily, accurately, and repeatably be positioned according to the FCC specifications. The device holder can be locked at different phantom locations (left head, right head, and uni-phantom).

## 6. Definition of Reference Points

### Ear Reference Point

Figure 6.2 shows the front, back and side views of the SAM Phantom. The point "M" is the reference point for the center of the mouth, "LE" is the left ear reference point (ERP), and "RE" is the right ERP. The ERPs are 15mm posterior to the entrance to the ear canal (EEC) along the B-M line (Back-Mouth), as shown in Figure 6.1. The plane passing through the two ear canals and M is defined as the Reference Plane. The line N-F (Neck-Front) is perpendicular to the reference plane and passing through the RE (or LE) is called the Reference Pivoting Line (see Figure 6.1). Line B-M is perpendicular to the N-F line. Both N-F and B-M lines are marked on the external phantom shell to facilitate handset positioning [5].

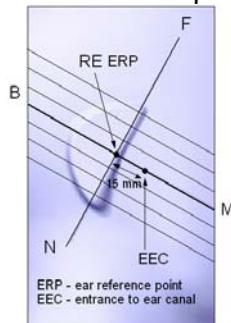


**Figure 6.1 Close-up side view of ERP's**



**Figure 6.2 Front, back and side view of SAM**

### Device Reference Points

Two imaginary lines on the device need to be established: the vertical centerline and the horizontal line. The test device is placed in a normal operating position with the "test device reference point" located along the "vertical centerline" on the front of the device aligned to the "ear reference point" (See Fig. 6.3). The "test device reference point" is then located at the same level as the center of the ear reference point. The test device is positioned so that the "vertical centerline" is bisecting the front surface of the device at its top and bottom edges, positioning the "ear reference point" on the outer surface of both the left and right head phantoms on the ear reference point [5].

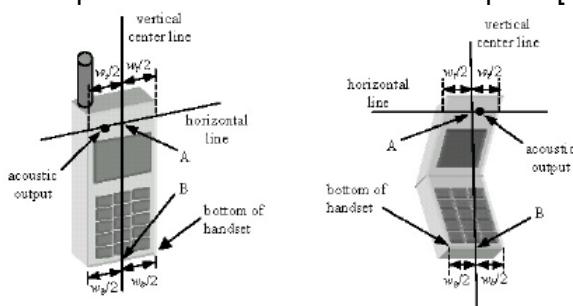


**Figure 6.3 Handset Vertical Center & Horizontal Line Reference Points**

## 7. Test Configuration Positions


### Positioning for Cheek/Touch [5]

1. Position the device close to the surface of the phantom such that point A is on the (virtual) extension of the line passing through points RE and LE on the phantom (see Figure 7.1), such that the plane defined by the vertical center line and the horizontal line of the device is approximately parallel to the sagittal plane of the phantom.

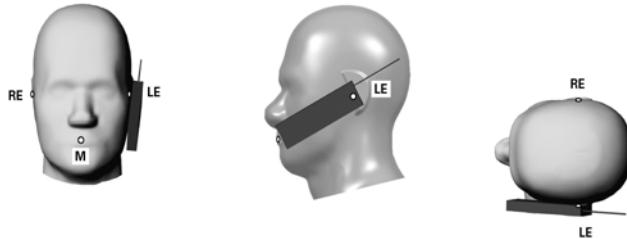

**Figure 7.1 Front, Side and Top View of Cheek/Touch Position**

2. Translate the device towards the phantom along the line passing through RE and LE until the device touches the ear.
3. While maintaining the device in this plane, rotate it around the LE-RE line until the vertical centerline is in the plane normal to MB-NF including the line MB (called the reference plane).
4. Rotate the device around the vertical centerline until the device (horizontal line) is symmetrical with respect to the line NF.
5. While maintaining the vertical centerline in the reference plane, keeping point A on the line passing through RE and LE and maintaining the device contact with the ear, rotate the device about the line NF until any point on the device is in contact with a phantom point below the ear (cheek). See Figure 7.2.




**Figure 7.2 Side view w/ relevant markings**

## Positioning for Ear / 15° Tilt [5]

With the test device aligned in the Cheek/Touch Position":

1. While maintaining the orientation of the device, retracted the device parallel to the reference plane far enough to enable a rotation of the device by 15 degrees.
2. Rotate the device around the horizontal line by 15 degrees.
3. While maintaining the orientation of the device, move the device parallel to the reference plane until any part of the device touches the head. (In this position, point A is located on the line RE-LE). The tilted position is obtained when the contact is on the pinna. If the contact is at any location other than the pinna, the angle of the device shall be reduced. The tilted position is obtained when any part of the device is in contact with the ear as well as a second part of the device is in contact with the head (see Figure 7.3).

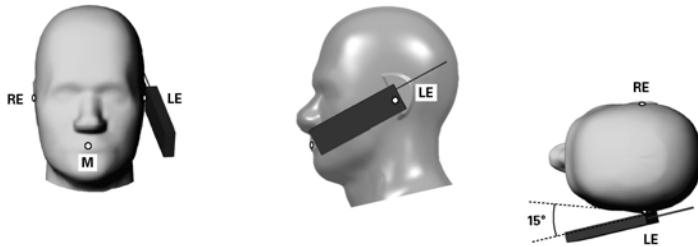

**Figure 7.3 Front, Side and Top View of Ear/15° Tilt Position**

## Body Worn Configurations

Body-worn operating configurations are tested with the accessories attached to the device and positioned against a flat phantom in a normal use configuration. A device with a headset output is tested with a headset connected to the device. Body dielectric parameters are used.

Accessories for Body-worn operation configurations are divided into two categories: those that do not contain metallic components and those that do contain metallic components. When multiple accessories that do not contain metallic components are supplied with the device, the device is tested with only the accessory that dictates the closest spacing to the body. Then, when multiple accessories that contain metallic components are supplied with the device, the device is tested with each accessory that contains a unique metallic component. If multiple accessories share an identical metallic component (i.e. the same metallic belt-clip used with different holsters with no other metallic components) only the accessory that dictates the closest spacing to the body is tested.

Body-worn accessories may not always be supplied or available as options for some devices intended to be authorized for body-worn use. In this case, a test configuration where a separation distance between the back of the device and the flat phantom is used. All test position spacings are documented.

Transmitters that are designed to operate in front of a person's face, as in push-to-talk configurations, are tested for SAR compliance with the front of the device positioned to face the flat phantom. For devices that are carried next to the body such as a shoulder, waist or chest-worn transmitters, SAR compliance is tested with the accessory(ies), including headsets and microphones, attached to the device and positioned against a flat phantom in a normal use configuration.

In all cases SAR measurements are performed to investigate the worst-case positioning. Worst-case positioning is then documented and used to perform Body SAR testing.

In order for users to be aware of the body-worn operating requirements for meeting RF exposure compliance, operating instructions and cautions statements are included in the user's manual.

## 8. ANSI/IEEE C95.1 – 1999 RF Exposure Limits [2]

### Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

### Controlled Environment

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

**Table 8.1 Human Exposure Limits**

	UNCONTROLLED ENVIRONMENT General Population (W/kg) or (mW/g)	CONTROLLED ENVIRONMENT Professional Population (W/kg) or (mW/g)
SPATIAL PEAK SAR <sup>1</sup> Brain	1.60	8.00
SPATIAL AVERAGE SAR <sup>2</sup> Whole Body	0.08	0.40
SPATIAL PEAK SAR <sup>3</sup> Hands, Feet, Ankles, Wrists	4.00	20.00

<sup>1</sup> The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

<sup>2</sup> The Spatial Average value of the SAR averaged over the whole body.

<sup>3</sup> The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

## 9. Measurement Uncertainty

### Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	$c_i^1 (1-g)$	$c_i^1 (10-g)$	Standard Uncertainty (1-g) %	Standard Uncertainty (10-g) %
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	•3	$(1-cp)^{1/2}$	$(1-cp)^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	•3	•cp	•cp	4.4	4.4
Boundary Effect	1.0	rectangular	•3	1	1	0.6	0.6
Linearity	4.7	rectangular	•3	1	1	2.7	2.7
Detection Limit	1.0	rectangular	•3	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	•3	1	1	0.5	0.5
Integration Time	1.7	rectangular	•3	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	•3	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	•3	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	•3	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	•3	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	7.1	rectangular	•3	1	1	4.1	4.1
Phantom and Setup							
Phantom Uncertainty (shape & thickness tolerance)	3.4	rectangular	•3	1	1	2.0	2.0
Liquid Conductivity (target)	5.0	rectangular	•3	0.7	0.5	2.0	1.4
Liquid Conductivity (meas.)	2.1	normal	1	0.7	0.5	1.4	1.0
Liquid Permittivity (target)	5.0	rectangular	•3	0.6	0.5	1.7	1.4
Liquid Permittivity (meas.)	0.1	normal	1	0.6	0.5	0.1	0.0
Combined Uncertainty		RSS				10.2	10.0
Combined Uncertainty (coverage factor=2)		Normal (k=2)				20.4	20.0

## 10. System Validation

### Tissue Verification

**Table 10.1 Measured Tissue Parameters**

		835 MHz Body		1900 MHz Body		2590 MHz Body	
Date(s)		Sep. 21, 2009		Sep. 21, 2009		Aug. 30, 2009	
Liquid Temperature (°C)	20.0	Target	Measured	Target	Measured	Target	Measured
Dielectric Constant: $\epsilon$	55.20	55.25	53.30	53.10	52.52	52.48	
Conductivity: $\sigma$	0.97	0.99	1.52	1.53	2.15	2.13	

See Appendix A for data printout.


### Test System Verification

Prior to assessment, the system is verified to the  $\pm 10\%$  of the specifications at the test frequency by using the system kit. Power is extrapolated to 1 watt. (Graphic Plots Attached)

**Table 10.2 System Dipole Validation Target & Measured**

	Test Frequency	Targeted SAR <sub>1g</sub> (W/kg)	Measure SAR <sub>1g</sub> (W/kg)	Deviation (%)
21-Sep-2009	835 MHz	9.75	9.51	- 2.46
21-Sep-2009	1900 MHz	40.99	39.99	- 2.44
22-Sep-2009	2600 MHz	54.26	54.40	+ 0.26

See Appendix A for data plots.

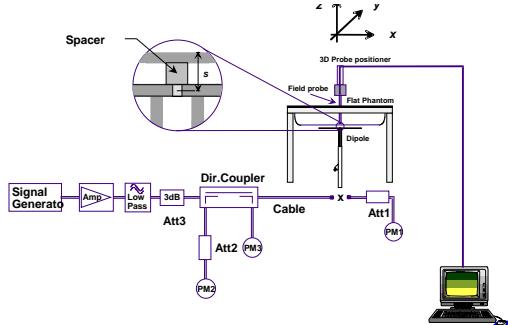
**Figure 10.1 Dipole Validation Test Setup**

## 11. SAR Test Data Summary

### See Measurement Result Data Pages

See Appendix B for SAR Test Data Plots.

See Appendix C for SAR Test Setup Photos.

### Procedures Used To Establish Test Signal

The device was placed into simulated transmit mode using the manufacturer's test codes. Such test signals offer a consistent means for testing SAR and are recommended for evaluating SAR. When test modes are not available or inappropriate for testing a device, the actual transmission is activated through a base station simulator or similar equipment. See data pages for actual procedure used in measurement.

### Device Test Condition

In order to verify that the device was tested at full power, conducted output power measurements were performed before and after each SAR measurement to confirm the output power unless otherwise noted. If a conducted power deviation of more than 5% occurred, the test was repeated.

The testing was conducted on all side sides of the modem. The bottom back side testing was conducted with the modem installed in a side USB port on a Dell Latitude 910 Laptop. The right side testing was conducted with the modem installed in a rear USB port on a Toshiba Satellite 2400 Laptop. All other positions were conducted with the modem installed on a 12 inch USB extension cable. The extension cable was installed in a side USB port on a Dell Latitude 910 Laptop. The gap was measured to be 5 mm from the phantom at the USB connector end of the body for the top and bottom, and 5 mm from the phantom for the left, right and tip sides of the device.

The 1xRTT testing was conducted in RC3 with the device configured using TDSO/SO32 with FCH transmitting at full rate. The power control was set to "All Bits Up." Multiple code channels were not tested due to the conducted power measured was less than  $\frac{1}{4}$  dB higher than with FCH only.

The Rev. 0 and Rev. A Subtype 0/1 testing was conducted with the Reverse Data Channel rate of 153.6 kbps. The Forward Traffic Channel data rate is set to the 2-slot version of 307.2 kbps with the ACK Channel transmitting in all slots. The power control was set to "All Bits Up." Other rates were not tested due to the conducted power measured was less than  $\frac{1}{4}$  dB higher than 153.6 kbps.

The Rev. A Subtype 2 testing was conducted with the Reverse Data Channel payload size of 4096 bits and Termination Target of 16 slots. The Forward Traffic Channel data rate is set to the 2-slot version of 307.2 kbps with the ACK Channel transmitting in all slots. The power control was set to "All Bits Up." Other rates were not tested due to the conducted power measured was less than  $\frac{1}{4}$  dB higher than 4096 bits.

The testing was conducted on the middle channel first. If the SAR value was 3 dB or more below the limit, the remaining two channels were not tested.

## 12. FCC Measurement Procedures – March 2008

Power measurements were performed using a base station simulator under average power.

### 12.1 Procedures Used to Establish RF Signal for SAR

The device was placed into a simulated call using a base station simulator in a screen room. Such test signals offer a consistent means for testing SAR and recommended for evaluating SAR. The SAR measurement software calculates a reference point at the start and end of the test to check for power drifts. If conducted power deviations of more than 5% occurred, the tests were repeated.

### 12.2 SAR Measurement Conditions

#### 12.2.1 Output Power Verification Ev-Do

Maximum output power is verified on the High, Middle, and Low channels according to the procedures in section 3.1.2.3.4 of 3GPP2 C.S0033-0/TIA-866 for Rev. 0 and section 4.3.4 of 3GPP2 C.S0033-1 for Rev. A. For Rev. A, maximum output power for both Subtype 0/1 and Subtype 2 Physical Layer configurations should be measured. The device operating configurations under TAP/ETAP shall be documented in the test report; including power control, code channel and RF channel output power levels. The measurement results should be tabulated in the SAR report with any measurement difficulties and equipment limitations clearly identified.

#### 12.2.2 Body SAR Measurements

SAR is measured using FTAP/RTAP and FETAP/RETAP respectively for Rev. 0 and Rev. A devices. The AT is tested with a Reverse Data Channel rate of 153.6 kbps in Subtype 0/1 Physical Layer configurations; and a Reverse Data Channel payload size of 4096 bits and Termination Target of 16 slots in Subtype 2 Physical Layer configurations. Both FTAP and FETAP are configured with a Forward Traffic Channel data rate corresponding to the 2-slot version of 307.2 kbps with the ACK Channel transmitting in all slots. AT power control should be in All Bits Up conditions for TAP/ETAP modes.

Body SAR is measured using Subtype 0/1 Physical Layer configurations for Rev. 0. SAR for Subtype 2 Physical Layer configurations is not required for Rev. A when the maximum average output of each RF channel is less than that measured in Subtype 0/1 Physical Layer configurations. Otherwise, SAR is measured on the maximum output channel for Rev. A using the exposure configurations that results in the highest SAR for that RF channel in Rev. 0.

#### 1x RTT Support

For Ev-Do devices that also support 1x RTT voice and/or data operations, SAR is not required for 1x RTT when the maximum average output of each channel is less than  $\frac{1}{4}$  dB higher than that measured in Subtype 0/1 Physical Layer configurations for Rev. 0. Otherwise, the 'Body SAR Measurements' procedures in the 'CDMA-2000 1x Handsets' section should be applied.

Due to the higher conducted power numbers in 1xRTT (+ 1 dB higher than Rev.0) the SAR measurements were conducted with the device transmitting in 1xRTT.

### 12.2.3 Output Power Verification 1x RTT

Maximum output power is verified on the High, Middle, and Low channels according to procedures in section 4.4.5.2 of 3 GPP2 C.S0011/TIA-98-E. Results for at least steps 3, 4 and 10 of the power measurement procedures should be tabulated in the SAR report. Steps 3 and 4 should be measured using SO55 with power control bits in "All Up" condition. TDSO / SO32 may be used instead of SO55 for step 4. Step 10 should be measured using TDSO / SO32 with power control bits in the "Bits Hold" condition (i.e. alternative Up/Down Bits). All power measurements defined in C.S0011/TIA-98-E that are inapplicable to the DUT or cannot be measured due to technical or equipment limitations should be clearly identified in the test report.

#### 1xRTT Power Measurements

IS-2000	Channel	SO2 [dBm]	SO2 [dBm]	SO2 [dBm]	SO55 [dBm]	SO55 [dBm]	SO9 [dBm]	SO9 [dBm]	SO55 [dBm]	TDSO SO32 FCH Only [dBm]	TDSO SO32 FCH+SCH [dBm]
	F-RC	RC1	RC3	RC4	RC1	RC3	RC2	RC5	RC2	RC3	RC3
Band	Vocoder Rate	Full	Full	Full	Full	Full	Full	Full	Full	Full	Full
	1013	23.81	23.82	23.76	23.86	23.86	23.86	23.86	23.79	23.88	23.91
Cellular	384	23.80	23.86	23.82	23.80	23.82	23.75	23.82	23.76	23.84	23.86
	777	23.56	23.69	23.64	23.56	23.62	23.54	23.59	23.58	23.69	23.67
PCS	25	23.66	23.75	23.79	23.69	23.85	23.68	23.79	23.79	23.83	23.80
	600	23.79	23.90	23.93	23.85	23.95	23.83	23.95	23.90	23.92	23.93
	1175	23.75	23.86	23.86	23.76	23.90	23.79	23.87	23.84	23.90	23.89

#### EvDo Rev 0 Power Measurements

1x EvDo Rev. 0 [dBm] - FTAP rate = 2 Slot Version 307.2 kbps							
		RTAP Rate	9.6 kbps	19.2 kbps	38.4 kbps	76.8 kbps	153.6 kbps
Band	Channel						
Cellular	1013	22.85	22.97	22.91	22.96	22.98	
	384	22.86	22.91	22.86	22.86	22.95	
	777	22.67	22.68	22.65	22.62	22.70	
PCS	25	22.76	22.61	22.73	22.68	22.76	
	600	22.80	22.79	22.79	22.80	22.86	
	1175	22.76	22.76	22.75	22.74	22.81	

#### EvDo Rev A Power Measurements

1x EvDo Rev. A Type 2 [dBm] - FETAP rate = 2 Slot Version 307.2 kbps													
	RETAP Payload	128 bits	256 bits	512 bits	768 bits	1024 bits	1536 bits	2048 bits	3072 bits	4096 bits	6144 bits	8192 bits	12288 bits
Band	Channel												
Cellular	1013	22.98	22.98	23.02	22.88	23.02	23.05	23.09	22.98	23.08	23.06	23.05	22.96
	384	23.06	23.02	22.95	22.99	23.08	23.01	23.05	22.86	22.92	22.79	22.97	22.94
	777	22.78	22.74	22.74	22.74	22.77	22.87	22.86	22.78	22.81	22.75	22.79	22.75
PCS	25	22.86	22.87	22.86	22.87	22.89	22.91	22.89	22.89	22.95	22.92	22.86	22.89
	600	22.94	23.01	23.03	22.98	22.94	22.94	23.02	22.99	22.98	22.95	23.03	23.01
	1175	22.96	22.94	22.97	22.93	22.90	22.96	22.85	22.90	22.86	22.86	22.86	22.86

Power Control was set in "All Bits Up" for all measurements.

### 12.2.4 WiMax System Description

The device is a 2.5 GHz WiMax transceiver in a USB dongle configuration using Beceem chipset which supports 1xTx and 2xRx for this device. Only one antenna is used for both transmitting and receiving while the other antenna is strictly used for RX diversity. Its uplink is capable of both 10 MHz and 5 MHz bandwidths. The uplink sub-frame is triggered by an Allocation Start Time contained in the information of UL-MAP. This information specifies the starting times of the Uplink and Downlink frames. In any UL sub-frame, the duty factor ranging and bandwidth information is used to ensure optimal system operation. In normal device transmission, the device will transmit control signaling at the first 3 uplink symbols and then use the rest of the uplink symbols for data traffic bursts in the uplink sub-frame. Since the first 3 symbols are also used for ranging detection purposes and are shared among other device users, its transmitting power is much smaller than the data burst symbol power. During the testing modes, the first 3 symbols have no power output and the data traffic bursts are always running at the maximum output power level. In the real usage, the data burst power will be adjusted according to the signal strength of the communication. In this way, by using the test mode arrangement, we are transmitting at a worst case RF level during the data portion Symbols 4 to 18.

The data burst zone can operate in one of two modes:

#### PUSC

For the 10 MHz bandwidth, it has 35 sub-channels structured from 1024 subcarriers; 184 are used as spare/safeguard subcarriers, leaving 840 available for transmission. From this, 560 subcarriers for data transmission with 280 subcarriers intended for pilot use. For the 5 MHz bandwidth, it contains 17 sub-channels using 512 subcarriers; 104 subcarriers are spare/safeguard subcarriers, 272 for data transmission, and 136 for pilot.

#### AMC

For the 10 MHz bandwidth, it has 48 sub-channels structured from 1024 subcarriers; 160 are used as spare/safeguard subcarriers, leaving 864 available for transmission. From this, 768 subcarriers for data transmission with 96 subcarriers intended for pilot use. For the 5 MHz bandwidth, it contains 24 sub-channels using 512 subcarriers; 80 subcarriers as spare/safeguard subcarriers, 384 for data transmission, and 48 for pilot.

The signal generator (MXG VSG) produces a downlink DL burst every 5 milliseconds which simulates the transmission of a base-station operating under normal mode. This DL burst instructs the mobile station MS to transmit for 15 symbols in the UL data zone. This UL transmission is repeated every 5 milliseconds. The TX power of the mobile station is set to maximum power. The MXG VSG and MS use the same frequency. The MXG VSG power is much lower than the MS Tx power (~80 dB lower) and does not affect the SAR readings.

The MXG VSG is loaded with a BS downlink signal which contains the 29:18 information. The MS synchronizes to the signal from the MXG VSG in frequency and time. It then demodulates two maps contained in the MXG VSG DL frame. The first map (DL map) specifies the number of DL symbols (29). The second map (UL map) specifies the number of UL symbols (18). The UL map also tells the MS to transmit a burst which occupies all data symbols and all sub-channels. No control channel transmissions are requested by the MXG VSG. Measurements

are taken in this configuration with the MS transmitting using the 29:18 ratio, but since there is not energy in the control symbols, the effective power is only across 15 symbols.

As mentioned above the DL:UL frame is specified in the DL and UL maps respectively. There is no ranging present when there is data traffic. The other types of control traffic are HARQ ACK/NACK, CQICH (CINR reporting) and bandwidth BW requests. BW requests are piggy-backed onto the data symbols when traffic is present. Since the BW requests are shared across the Control Symbols (traffic versus non-traffic modes), the control traffic that is relevant to the SAR calculation is CQICH and HARQ ACK/NACK. The maximum power for this control traffic is 32.9 mW (5/35 of 230.1 mW) for 10 MHz and 72.03 mw (5/17 of 244.91 mW) for 5 MHz.

In the test mode, the UL operates in PUSC or AMC with all data sub-channels (All 35 sub-channels for 10 MHz) occupied with data. During normal operation, the MS will transmit on all sub-channels when the maximum UL throughput is required. It is possible for the MS to transmit with fewer sub-channels. The sub-channels consist of tones that are distributed over the entire signal BW and a jump every three symbols so that the spectral density and hence SAR for the fractional sub-channel case will be similar to the full sub-channel case that is tested. (Note: In the WiMax standard, a sub-channel consists of tones that are spread across the occupied bandwidth. After every three symbols, the tones that make up the sub-channel switch to a new set of frequencies spread across the band. This “jumping” is called sub-channel rotation and helps to give the sub-channel frequency diversity.)

Equipment Used for network side:

Agilent N5182A MXG Vector Network Generator with the below options:  
N7615B-3FP : WiMax – Connect to N5182A Signal Generator  
N7615B-EFP : Basic 802.16 OFDMA  
N7615B-QFP : Advanced 802.16 OFDMA

Software is loaded into the MXG VSG that products an output signal that looks like a 29:18 WiMax frame, the EUT detects the “network” and begins to transmit based on the commands from the MXG VSG signal and the measurements are taken on the EUT.

The testing was done using a common 29:18 ratio as this is the maximum achievable ratio for the product. The 29 indicates the number of downlink (from the base station) symbols, and the 18 indicates the number of uplink (transmitted from the MS) symbols. Inside the uplink, 15 symbols are used for data, and three of the symbols are used for sending control information to the network. During the testing, the control symbols contained no information, so did not contribute to the total energy transmitted. To compensate for the maximum energy which may be present in the 3 control symbols, the following scheme is used for the scaling factor:

Maximum output power of 5 MHz is 23.89 dBm = 244.91 mW

The maximum power in 5 MHz control traffic is 72.03 mW (5/17 of 244.91 mW)

**Scaled factor for 5 MHz Bandwidth =**

$$(72.03 \text{ mW} \times 3 + 15 \times 244.91 \text{ mW}) / (15 \times 244.91 \text{ mW}) = 1.059$$

Maximum output power of 10 MHz is 23.62 dBm = 230.1 mW

The maximum power in 10 MHz control traffic is 32.9 mW (5/35 of 230.1 mW)

**Scaled factor for 10 MHz Bandwidth =**

$$(32.9 \text{ mW} \times 3 + 15 \times 230.1 \text{ mW}) / (15 \times 230.1 \text{ mW}) = 1.029$$

### 12.2.5 WiMax Conducted Power Measurements

Bandwidth	Frequency (MHz)	QPSK		16QAM	
		Coding Rate 1/2 (dBm)	Coding Rate 3/4 (dBm)	Coding Rate 1/2 (dBm)	Coding Rate 3/4 (dBm)
5 MHz	2498.5	23.89	23.79	23.86	23.84
	2593.0	23.06	22.72	23.45	23.29
	2687.5	22.74	22.69	22.81	22.68
10 MHz	2501.0	23.52	23.54	23.62	23.53
	2593.0	23.12	23.02	23.01	22.98
	2685.0	22.69	22.60	22.70	22.51

Transmitter conducted output power was measured by channel power with RBW, VBW=100 kHz, RMS detector on TX burst time (1.56 ms) only using the gate function of the Spectrum Analyzer.

#### Linearity Response Check

Output Power	dBm	11	14	17	20	23
	mW	12.5	25	50	100	200
5 MHz Single Point SAR (W/kg)	0.15	0.31	0.61	1.33	2.72	
10 MHz Single Point SAR (W/kg)	0.09	0.19	0.40	1.03	2.11	

#### Worst Case (Each modulation and Coding Rate)

Bandwidth	Modulation Type	Power Drift	SAR Value (W/kg)
5 MHz	QPSK 1/2	3.014%	1.106
	QPSK 3/4	3.317%	1.035
	16QAM 1/2	1.642%	0.953
	16QAM 3/4	2.304%	0.866

## SAR Data Summary – 835 MHz Body – EvDo

MEASUREMENT RESULTS									
Gap	Side	Frequency		Mode	Begin/End Power		Reverse Channel	Forward Channel	SAR (W/kg)
		MHz	Ch.		(dBm)	(dBm)			
5 mm	Top	836.60	384	1xRTT	23.84	23.83	RC3	TDSO/SO32 FCH Only	0.76
	Bottom	836.60	384	1xRTT	23.82	23.80	RC3	TDSO/SO32 FCH Only	0.68
	Right Side	836.60	384	1xRTT	23.83	23.81	RC3	TDSO/SO32 FCH Only	0.34
	Left Side	836.60	384	1xRTT	23.81	23.79	RC3	TDSO/SO32 FCH Only	0.61
	Tip	836.60	384	1xRTT	23.84	23.82	RC3	TDSO/SO32 FCH Only	0.13

**Muscle**  
**1.6 W/kg (mW/g)**  
averaged over 1 gram

1. Battery is fully charged for all tests.

Power Measured

Conducted

ERP

EIRP

2. SAR Measurement

Phantom Configuration  
SAR Configuration

Left Head  
Head

Uniphantom  
Body

Right Head

3. Test Signal Call Mode

Test Code

Base Station Simulator

4. Test Configuration

With Belt Clip

Without Belt Clip

N/A



Jay M. Moulton  
Vice President

Note: When the mid channel is 3 dB or more below the limit the low and high channel are not required to be tested.

## SAR Data Summary – 1900 MHz Body – EvDo

### MEASUREMENT RESULTS

Gap	Side	Frequency		Mode	Begin/End Power		Reverse Channel	Forward Channel	SAR (W/kg)
		MHz	Ch.		(dBm)	(dBm)			
5 mm	Top	1851.25	25	1xRTT	23.82	23.81	RC3	TDSO/SO32 FCH Only	1.21
		1880.00	600		23.92	23.90	RC3	TDSO/SO32 FCH Only	1.44
		1908.75	1175		23.90	23.89	RC3	TDSO/SO32 FCH Only	1.29
	Top Lower	1880.00	600		23.91	23.89	RC3	TDSO/SO32 FCH Only	0.67
	Bottom	1851.25	25	1xRTT	23.82	23.80	RC3	TDSO/SO32 FCH Only	1.35
		1880.00	600		23.91	23.89	RC3	TDSO/SO32 FCH Only	1.44
		1908.75	1175		23.89	23.87	RC3	TDSO/SO32 FCH Only	1.50
	Bottom Lower	1908.75	1175		23.89	23.88	RC3	TDSO/SO32 FCH Only	0.73
	Right Side	1880.00	600	1xRTT	23.92	23.90	RC3	TDSO/SO32 FCH Only	0.58
	Left Side	1851.25	25	1xRTT	23.81	23.80	RC3	TDSO/SO32 FCH Only	1.08
		1880.00	600		23.90	23.88	RC3	TDSO/SO32 FCH Only	1.29
		1908.75	1175		23.89	23.89	RC3	TDSO/SO32 FCH Only	1.24
	Left Lower	1880.00	600		23.91	23.90	RC3	TDSO/SO32 FCH Only	0.66
	Tip	1880.00	600	1xRTT	23.92	23.90	RC3	TDSO/SO32 FCH Only	0.59

**Muscle**  
**1.6 W/kg (mW/g)**  
averaged over 1 gram

1. Battery is fully charged for all tests.

Power Measured

Conducted

ERP

EIRP

2. SAR Measurement

Phantom Configuration  
SAR Configuration

Left Head  
Head

Uniphantom  
Body

Right Head

3. Test Signal Call Mode

Test Code

Base Station Simulator

4. Test Configuration

With Belt Clip

Without Belt Clip

N/A



Jay M. Moulton  
Vice President

Note: When the mid channel is 3 dB or more below the limit the low and high channel are not required to be tested.

**SAR Data Summary – 2600 MHz Body – WiMax QPSK ½ 5 MHz**
**MEASUREMENT RESULTS**

Gap	Side	Frequency		Modulation	Begin/End Power		SAR (W/kg)	Scaling Factor	Calculated SAR
		MHz	Ch.		(dBm)	(dBm)			
5 mm	Top	2498.5	Low	QPSK ½	23.89	23.88	0.68	1.059	0.72
		2593.0	Mid		23.06	23.04	0.83	1.059	0.88
		2687.5	High		22.74	22.73	0.80	1.059	0.85
	Top Lower	2593.0	Mid	QPSK ½	23.05	23.04	0.57	1.059	0.60
	Bottom	2593.0	Mid		23.06	23.04	0.78	1.059	0.83
	Bottom Lower	2593.0	Mid		23.05	23.03	0.54	1.059	0.57
	Right Side	2593.0	Mid	QPSK ½	23.04	23.02	0.56	1.059	0.59
	Left Side	2498.5	Low		23.88	23.88	0.90	1.059	0.95
		2593.0	Mid		23.05	23.05	1.11	1.059	1.18
		2687.5	High		22.73	22.71	1.06	1.059	1.12
	Left Lower	2593.0	Mid	QPSK ½	23.06	23.05	0.65	1.059	0.69
	Tip	2593.0	Mid		23.05	23.05	0.63	1.059	0.67

**Muscle**  
**1.6 W/kg (mW/g)**  
averaged over 1 gram

1. Battery is fully charged for all tests.

Power Measured

Conducted

ERP

EIRP

2. SAR Measurement

Phantom Configuration  
SAR Configuration

Left Head  
Head

Uniphantom  
Body

Right Head

3. Test Signal Call Mode

Test Code

Base Station Simulator

4. Test Configuration

With Belt Clip

Without Belt Clip

N/A



Jay M. Moulton  
Vice President

Note: When the measured mid channel is 3 dB or more below the limit the low and high channel are not required to be tested.

**SAR Data Summary – 2600 MHz Body – WiMax QPSK ½ 10 MHz**

MEASUREMENT RESULTS									
Gap	Side	Frequency		Modulation	Begin/End Power		SAR (W/kg)	Scaling Factor	Calculated SAR
		MHz	Ch.		(dBm)	(dBm)			
5 mm	Top	2593.0	Mid	QPSK ½	23.12	23.11	0.65	1.029	0.67
	Bottom	2593.0	Mid	QPSK ½	23.11	23.10	0.68	1.029	0.70
	Right Side	2593.0	Mid	QPSK ½	23.12	23.10	0.52	1.029	0.54
	Left Side	2593.0	Mid	QPSK ½	23.11	23.11	0.80	1.029	0.82
	Left Lower	2593.0	Mid		23.11	23.10	0.60	1.029	0.62
	Tip	2593.0	Mid	QPSK ½	23.12	23.12	0.58	1.029	0.60

**Muscle**  
**1.6 W/kg (mW/g)**  
averaged over 1 gram

1. Battery is fully charged for all tests.

Power Measured

Conducted

ERP

EIRP

2. SAR Measurement

Phantom Configuration  
SAR Configuration

Left Head  
Head

Uniphantom  
Body

Right Head

3. Test Signal Call Mode

Test Code

Base Station Simulator

4. Test Configuration

With Belt Clip

Without Belt Clip

N/A



Jay M. Moulton  
Vice President

Note: When the mid channel is 3 dB or more below the limit the low and high channel are not required to be tested.

## 13. Test Equipment List

**Table 13.1 Equipment Specifications**

Type	Calibration Due Date	Serial Number
ThermoCRS Robot	N/A	RAF0338198
ThermoCRS Controller	N/A	RCF0338224
ThermoCRS Teach Pendant (Joystick)	N/A	STP0334405
IBM Computer, 2.66 MHz P4	N/A	8189D8U KCPR08N
Aprel E-Field Probe ALS-E020	11/03/2009	RFE-215
Aprel E-Field Probe ALS-E030	07/15/2009	E030-001
Aprel Dummy Probe	N/A	023
Aprel Left Phantom	N/A	RFE-267
Aprel Right Phantom	N/A	RFE-268
Aprel UniPhantom	N/A	RFE-273
Aprel Validation Dipole ALS-D-450-S-2	06/01/2009	RFE-362
Aprel Validation Dipole ALS-D-835-S-2	02/22/2010	RFE-274
Aprel Validation Dipole ALS-D-1900-S-2	02/21/2010	RFE-277
Aprel Validation Dipole ALS-D-2450-S-2	02/20/2010	RFE-278
Aprel Validation Dipole RFE-D-2600-S-2	02/23/2010	RFE-121
Agilent (HP) 437B Power Meter	12/01/2009	3125U08837
Agilent (HP) 8481B Power Sensor	12/02/2009	3318A05384
Advantest R3261A Spectrum Analyzer	12/02/2009	31720068
Agilent (HP) 8350B Signal Generator	12/01/2009	2749A10226
Agilent (HP) 83525A RF Plug-In	12/01/2009	2647A01172
Agilent (HP) 8753C Vector Network Analyzer	12/01/2009	3135A01724
Agilent (HP) 85047A S-Parameter Test Set	12/01/2009	2904A00595
Agilent (HP) E55125C Base Station Sim.	10/30/2010	MY48360364
Agilent (HP) N5182A MXG VSG	08/31/2011	MY47070302
Aprel Dielectric Probe Assembly	N/A	0011
Brain Equivalent Matter (450 MHz)	N/A	N/A
Brain Equivalent Matter (835 MHz)	N/A	N/A
Brain Equivalent Matter (1900 MHz)	N/A	N/A
Brain Equivalent Matter (2450 MHz)	N/A	N/A
Muscle Equivalent Matter (450 MHz)	N/A	N/A
Muscle Equivalent Matter (835 MHz)	N/A	N/A
Muscle Equivalent Matter (1900 MHz)	N/A	N/A
Muscle Equivalent Matter (2450 MHz)	N/A	N/A
Muscle Equivalent Matter (5200 MHz)	N/A	N/A
Muscle Equivalent Matter (5800 MHz)	N/A	N/A

## 14. Conclusion

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the FCC. These measurements are taken to simulate the RF effects exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The tested device complies with the requirements in respect to all parameters subject to the test. The test results and statements relate only to the item(s) tested.

Please note that the absorption and distribution of electromagnetic energy in the body is a very complex phenomena that depends on the mass, shape, and size of the body; the orientation of the body with respect to the field vectors; and, the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because innumerable factors may interact to determine the specific biological outcome of an exposure to electromagnetic fields, any protection guide shall consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables. [3]

## 15. References

- [1] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radio Frequency Radiation, August 1996
- [2] ANSI/IEEE C95.1 – 1999, American National Standard Safety Levels with respect to Human Exposure to Radio Frequency Electromagnetic Fields, 300kHz to 100GHz, New York: IEEE, 1992.
- [3] ANSI/IEEE C95.3 – 2002, IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields – RF and Microwave, New York: IEEE, 1992.
- [4] Federal Communications Commission, OET Bulletin 65 (Edition 97-01), Supplement C (Edition 01-01), Evaluating Compliance with FCC Guidelines for Human Exposure to Radio Frequency Electromagnetic Fields, July 2001.
- [5] IEEE Standard 1528 – 2003, IEEE Recommended Practice for Determining the Peak-Spatial Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communication Devices: Measurement Techniques, October 2003.
- [6] Industry Canada, RSS – 102e, Radio Frequency Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands), November 2005.
- [7] Industry Canada, Safety Code 6, Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz, 1999.

## Appendix A – System Validation Plots and Data

```
*****
Test Result for UIM Dielectric Parameter
Mon 21/Sep/2009 08:07:31
Freq Frequency(GHz)
FCC_eH      FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon
FCC_sH      FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma
FCC_eB      FCC Limits for Body Epsilon
FCC_sB      FCC Limits for Body Sigma
Test_e      Epsilon of UIM
Test_s      Sigma of UIM
*****
Freq      FCC_eB      FCC_sB      Test_e      Test_s
0.8050    55.32      0.97      55.38      0.96
0.8150    55.28      0.97      55.35      0.96
0.8250    55.24      0.97      55.33      0.97
0.8350    55.20      0.97      55.25      0.99
0.8450    55.17      0.98      55.20      1.01
0.8550    55.14      0.99      55.16      1.01
0.8650    55.11      1.01      55.12      1.02
```

```
*****
Test Result for UIM Dielectric Parameter
Mon 21/Sep/2009 11:47:36
Freq Frequency(GHz)
FCC_eH      FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon
FCC_sH      FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma
FCC_eB      FCC Limits for Body Epsilon
FCC_sB      FCC Limits for Body Sigma
Test_e      Epsilon of UIM
Test_s      Sigma of UIM
*****
Freq      FCC_eB      FCC_sB      Test_e      Test_s
1.8700    53.30      1.52      52.92      1.57
1.8800    53.30      1.52      53.01      1.56
1.8900    53.30      1.52      53.06      1.54
1.9000    53.30      1.52      53.10      1.53
1.9100    53.30      1.52      53.19      1.51
1.9200    53.30      1.52      53.24      1.49
1.9300    53.30      1.52      53.28      1.47
```

\*\*\*\*\*

Test Result for UIM Dielectric Parameter

Tue 22/Sep/2009 08:12:51

Freq Frequency(GHz)

FCC\_eH FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon

FCC\_sH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma

FCC\_eB FCC Limits for Body Epsilon

FCC\_sB FCC Limits for Body Sigma

Test\_e Epsilon of UIM

Test\_s Sigma of UIM

\*\*\*\*\*

Freq	FCC_eB	FCC_sB	Test_e	Test_s
2.5600	52.56	2.11	52.55	2.08
2.5700	52.55	2.12	52.53	2.10
2.5800	52.53	2.13	52.51	2.11
<b>2.5900</b>	<b>52.52</b>	<b>2.15</b>	<b>52.48</b>	<b>2.13</b>
2.6000	52.51	2.16	52.46	2.14
2.6100	52.50	2.18	52.44	2.16
2.6200	52.48	2.19	52.41	2.18

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 08:14:19 AM  
End Time : 21-Sep-2009 08:29:26 AM  
Scanning Time : 907 secs

## Product Data

Device Name : Validation  
Serial No. : 835  
Type : Dipole  
Model : ALS-D-835-S-2  
Frequency : 835.00 MHz  
Max. Transmit Pwr : 0.1 W  
Drift Time : 0 min(s)  
Length : 161 mm  
Width : 3.6 mm  
Depth : 89.8 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 1.038 W/kg  
Power Drift-Finish: 1.045 W/kg  
Power Drift (%) : 0.605

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 835  
Frequency : 835.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 49.00 RH%  
Epsilon : 55.25 F/m  
Sigma : 0.99 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 835.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 6.3  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 25.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 9:21:48 AM  
 Area Scan : 5x7x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


**Other Data**

DUT Position : Touch  
 Separation : 15 mm  
 Channel : Low

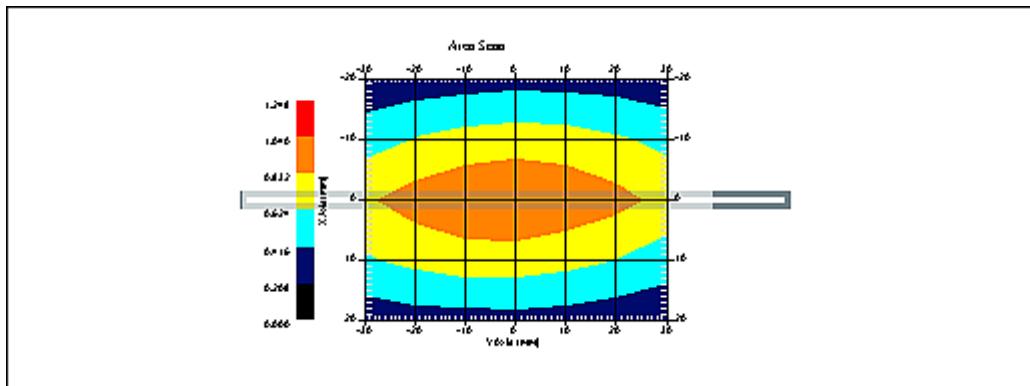

1 gram SAR value : 0.951 W/kg  
 10 gram SAR value : 0.603 W/kg  
 Area Scan Peak SAR : 1.042 W/kg  
 Zoom Scan Peak SAR : 1.461 W/kg

**SAR-Z Axis**  
at Hotspot x:0.21 y:-0.14

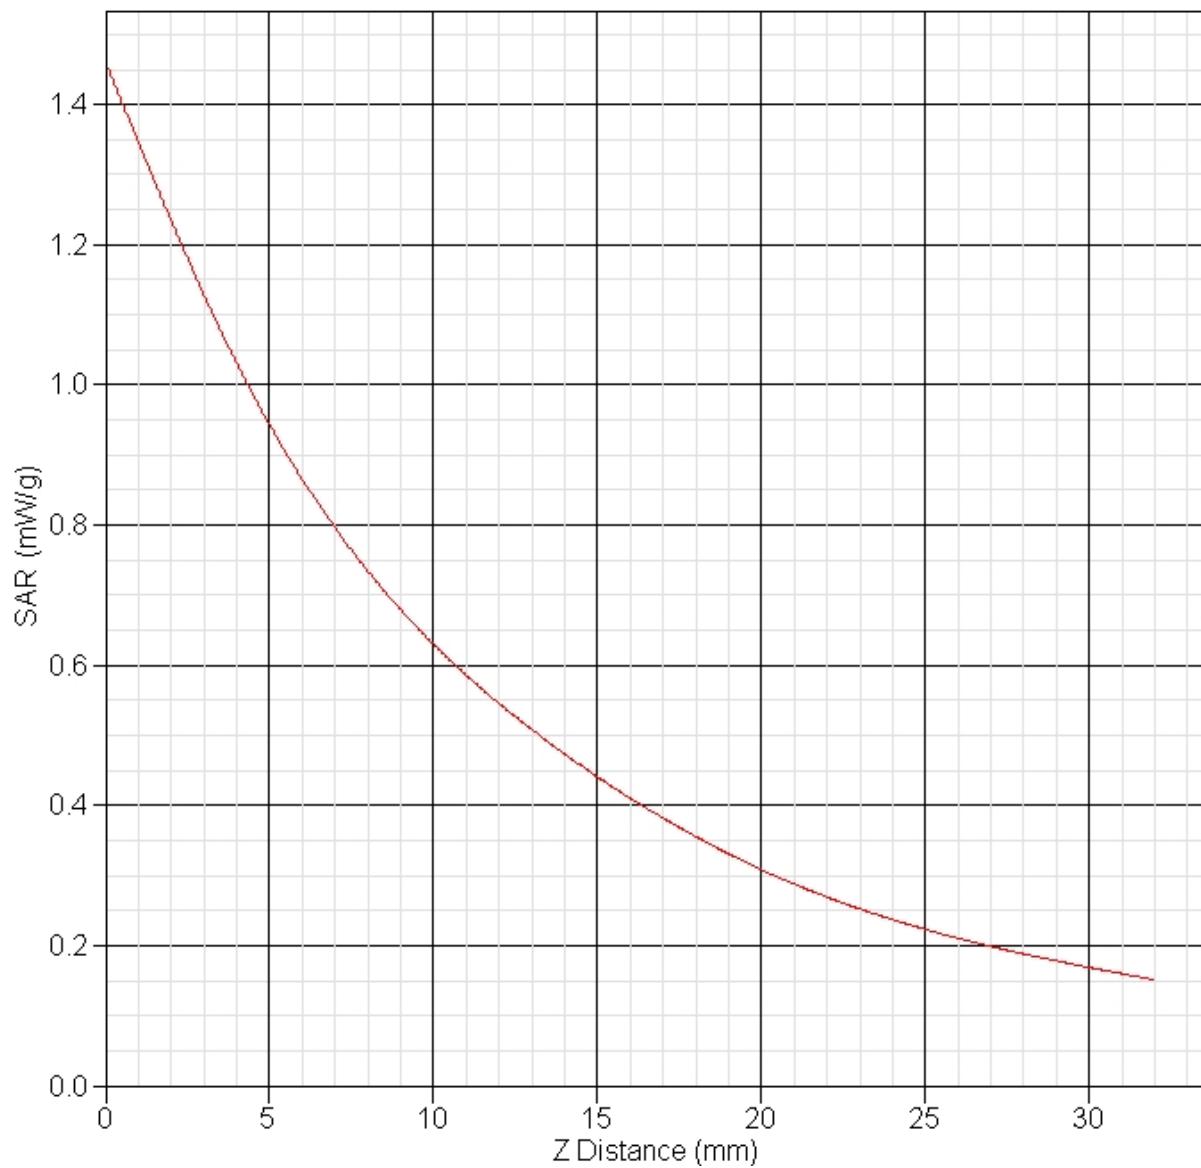

**SAR Test Report**

By Operator : Jay  
Measurement Date : 18-Sep-2009  
Starting Time : 18-Sep-2009 12:27:44 PM  
End Time : 18-Sep-2009 12:40:46 PM  
Scanning Time : 782 secs

## Product Data

Device Name : Validation  
Serial No. : 1900  
Type : Dipole  
Model : ALS-D-1900-S-2  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.1 W  
Drift Time : 0 min(s)  
Length : 68 mm  
Width : 3.6 mm  
Depth : 39.5 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 4.383 W/kg  
Power Drift-Finish: 4.402 W/kg  
Power Drift (%) : 0.434

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 18-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 49.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

## Measurement Data

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 20.00 °C  
Ambient Temp. : 23.00 °C  
Set-up Date : 18-Sep-2009  
Set-up Time : 8:03:12 AM  
Area Scan : 5x5x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


## Other Data

DUT Position : Touch  
Separation : 10 mm  
Channel : Mid

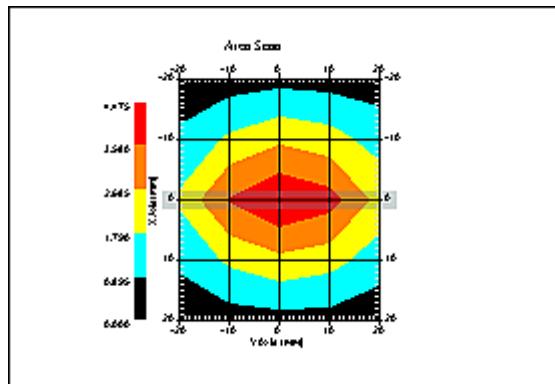

1 gram SAR value : 3.999 W/kg  
10 gram SAR value : 1.958 W/kg  
Area Scan Peak SAR : 4.396 W/kg  
Zoom Scan Peak SAR : 7.129 W/kg

**SAR-Z Axis**  
at Hotspot x:0.25 y:-0.18

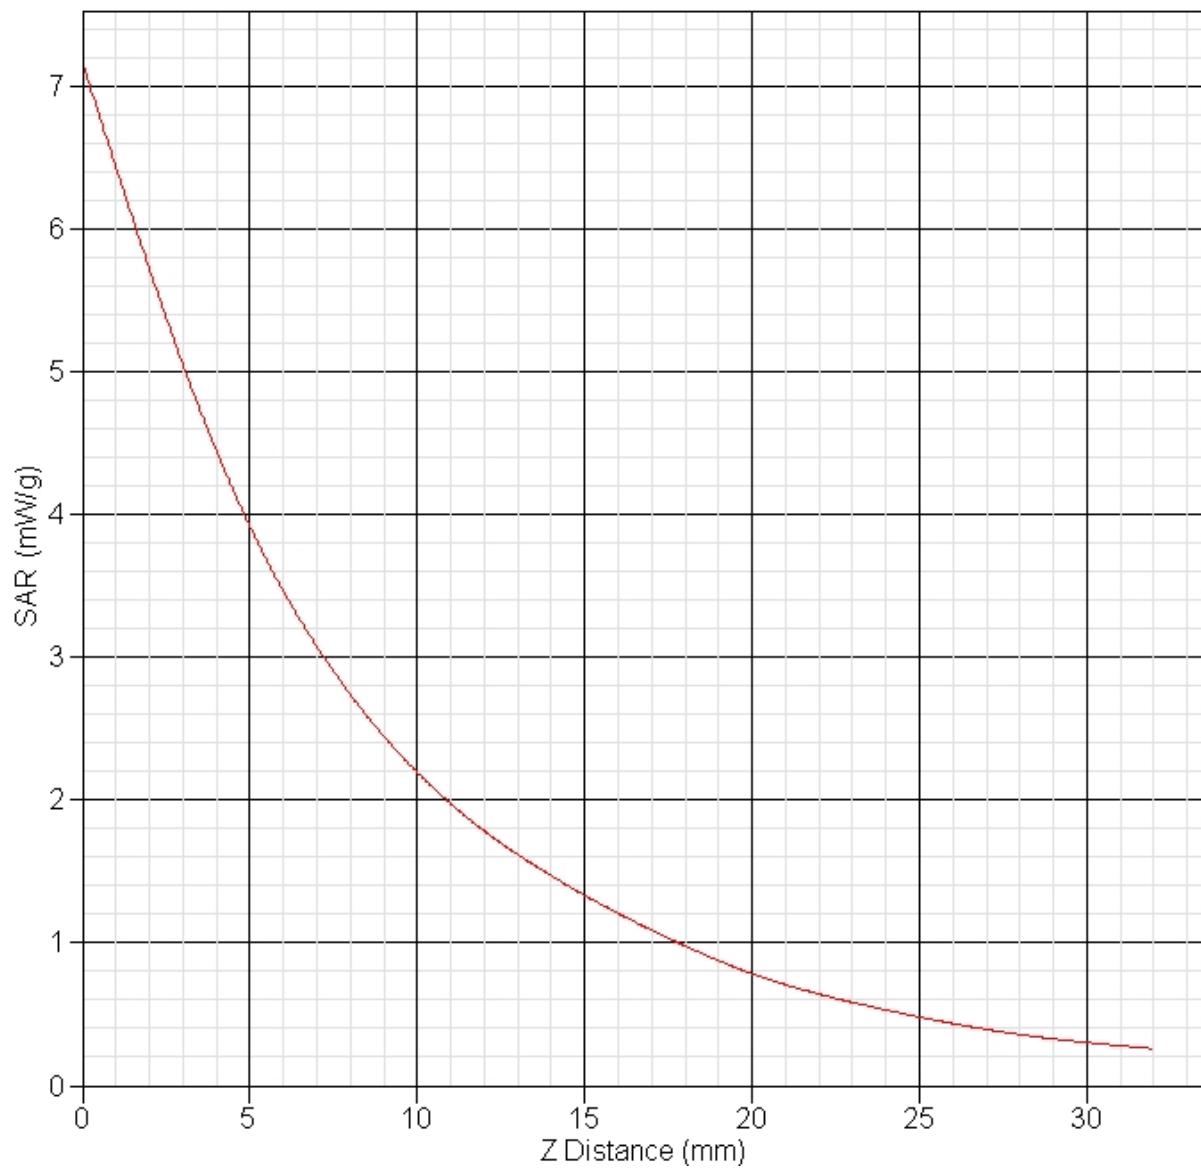

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 08:22:56 AM  
End Time : 22-Sep-2009 08:36:02 AM  
Scanning Time : 786 secs

## Product Data

Device Name : Validation  
Serial No. : 2600  
Type : Dipole  
Model : RFE-D-2600-S-2  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.1 W  
Drift Time : 0 min(s)  
Length : 49.5 mm  
Width : 3.6 mm  
Depth : 30.0 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 6.381 W/kg  
Power Drift-Finish: 6.404 W/kg  
Power Drift (%) : 0.355

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

## Measurement Data

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 20.00 °C  
Ambient Temp. : 23.00 °C  
Set-up Date : 22-Sep-2009  
Set-up Time : 7:40:13 AM  
Area Scan : 5x5x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


## Other Data

DUT Position : Touch  
Separation : 10 mm  
Channel : Mid

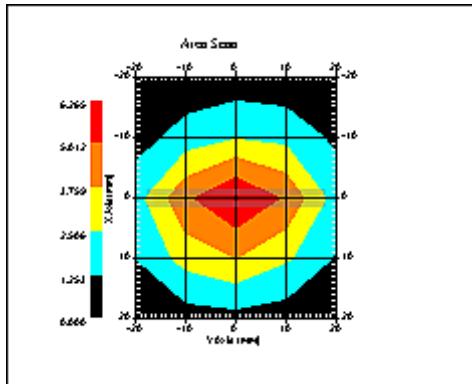

1 gram SAR value : 5.440 W/kg  
10 gram SAR value : 2.476 W/kg  
Area Scan Peak SAR : 6.265 W/kg  
Zoom Scan Peak SAR : 11.190 W/kg

**SAR-Z Axis**  
at Hotspot x:0.24 y:-0.18

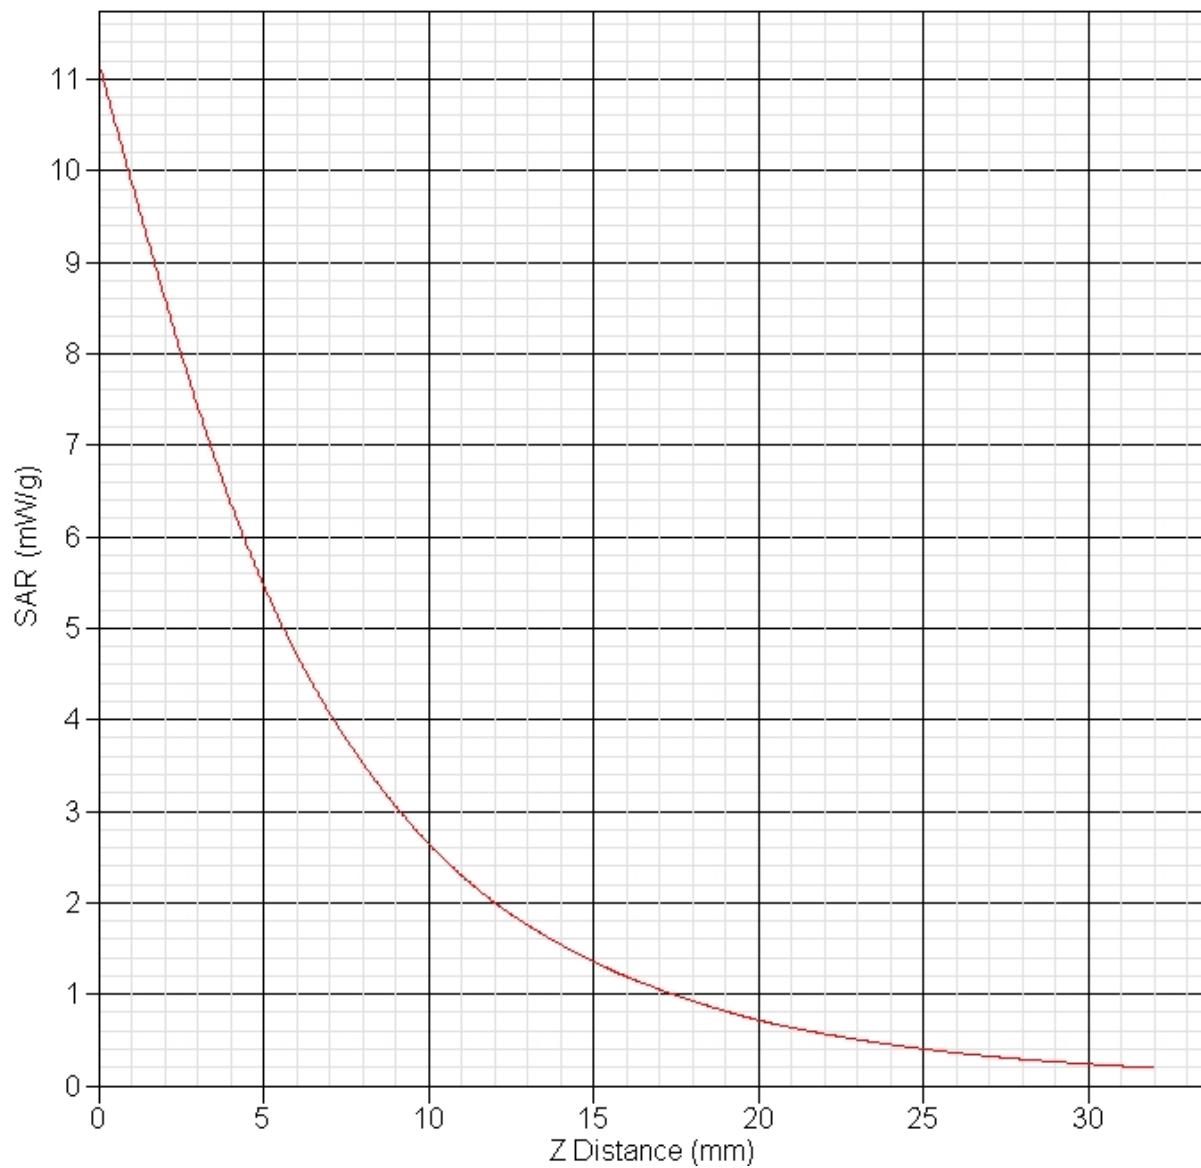

## Appendix B – SAR Test Data Plots

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 12:23:18 PM  
End Time : 22-Sep-2009 12:37:52 PM  
Scanning Time : 874 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\frac{1}{2}$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable - Worst Case Condition Data  
Power Drift-Start : 1.184 W/kg  
Power Drift-Finish: 1.220 W/kg  
Power Drift (%) : 3.014

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable - Worst Case Condition Data  
 Separation : 5 mm  
 Channel : Mid

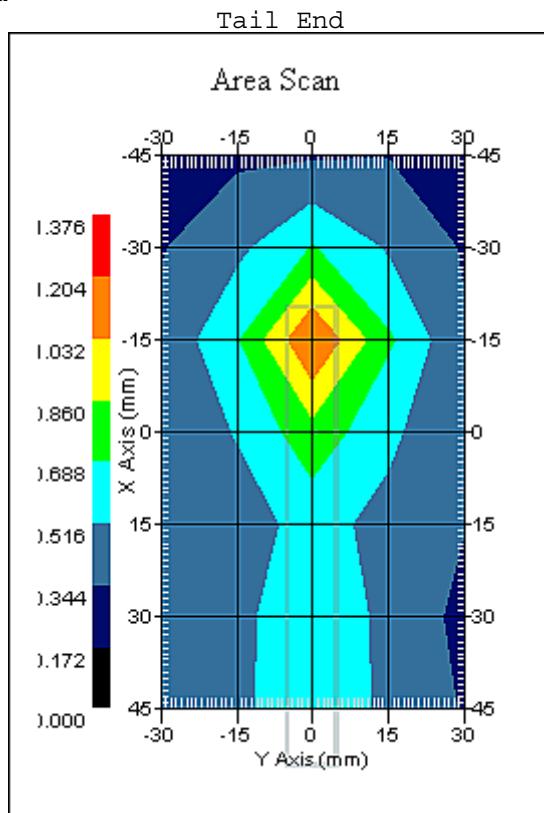

1 gram SAR value : 1.106 W/kg  
 10 gram SAR value : 0.724 W/kg  
 Area Scan Peak SAR : 1.207 W/kg  
 Zoom Scan Peak SAR : 1.661 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 05:07:13 PM  
End Time : 22-Sep-2009 05:21:54 PM  
Scanning Time : 881 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK ¾ 5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable - Worst Case Condition Data  
Power Drift-Start : 1.135 W/kg  
Power Drift-Finish: 1.173 W/kg  
Power Drift (%) : 3.317

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable - Worst Case Condition Data  
 Separation : 5 mm  
 Channel : Mid

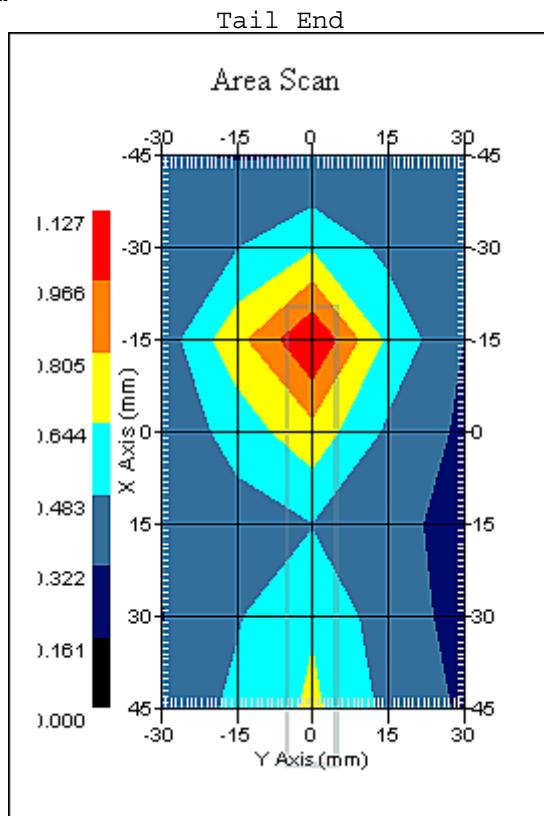

1 gram SAR value : 1.035 W/kg  
 10 gram SAR value : 0.672 W/kg  
 Area Scan Peak SAR : 1.125 W/kg  
 Zoom Scan Peak SAR : 1.611 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 05:30:05 PM  
End Time : 22-Sep-2009 05:44:46 PM  
Scanning Time : 881 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 16QAM  $\frac{1}{2}$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable - Worst Case Condition Data  
Power Drift-Start : 1.028 W/kg  
Power Drift-Finish: 1.045 W/kg  
Power Drift (%) : 1.642

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable - Worst Case Condition Data  
 Separation : 5 mm  
 Channel : Mid

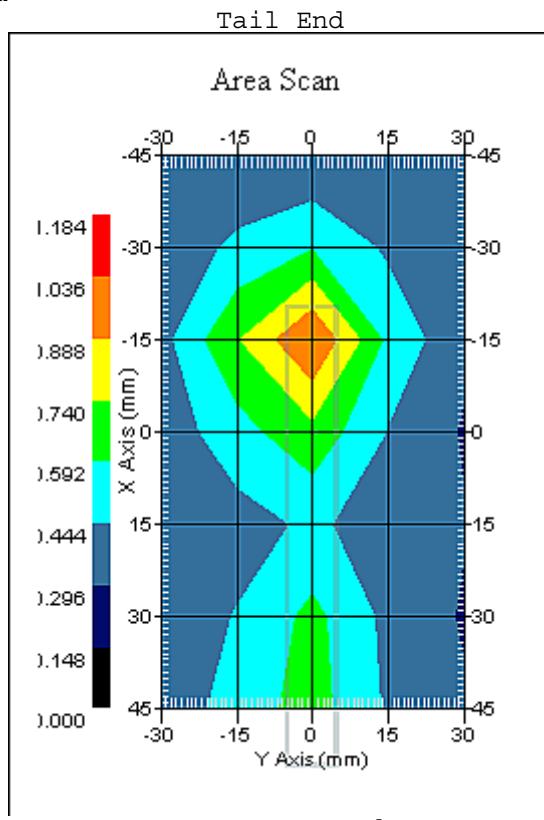

1 gram SAR value : 0.953 W/kg  
 10 gram SAR value : 0.636 W/kg  
 Area Scan Peak SAR : 1.039 W/kg  
 Zoom Scan Peak SAR : 1.461 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 05:45:46 PM  
End Time : 22-Sep-2009 06:00:31 PM  
Scanning Time : 885 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 16QAM ¾ 5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable - Worst Case Condition Data  
Power Drift-Start : 1.015 W/kg  
Power Drift-Finish: 1.038 W/kg  
Power Drift (%) : 2.304

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable - Worst Case Condition Data  
 Separation : 5 mm  
 Channel : Mid

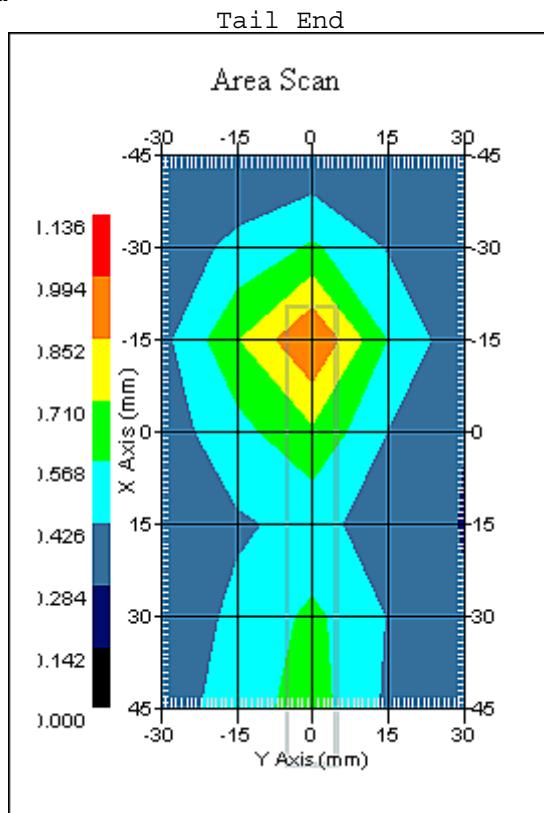

1 gram SAR value : 0.866 W/kg  
 10 gram SAR value : 0.583 W/kg  
 Area Scan Peak SAR : 0.997 W/kg  
 Zoom Scan Peak SAR : 1.341 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 10:39:51 AM  
End Time : 21-Sep-2009 10:54:45 AM  
Scanning Time : 894 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 835.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Top On Cable  
Power Drift-Start : 0.755 W/kg  
Power Drift-Finish: 0.730 W/kg  
Power Drift (%) : -3.312

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 835  
Frequency : 835.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 40.00 RH%  
Epsilon : 55.25 F/m  
Sigma : 0.99 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 835.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 6.3  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 10:38:48 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


**Other Data**

DUT Position : Top On Cable  
 Separation : 5 mm  
 Channel : Mid

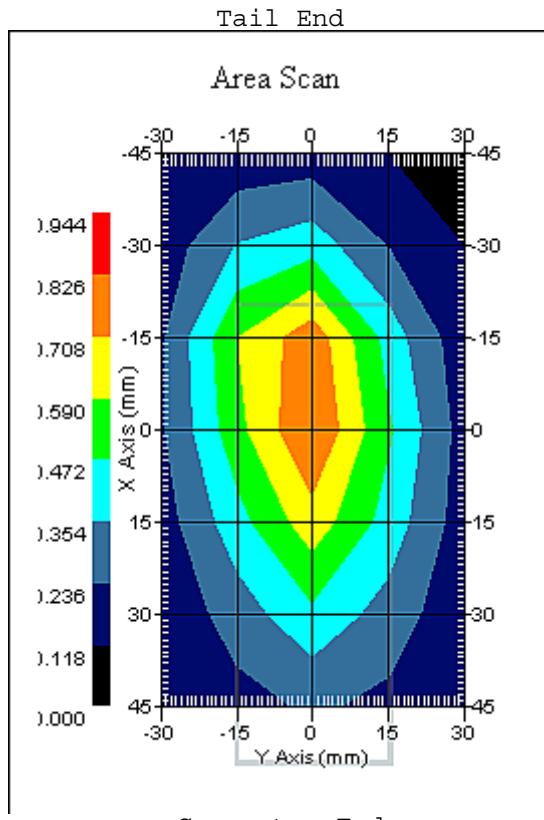

1 gram SAR value : 0.762 W/kg  
 10 gram SAR value : 0.521 W/kg  
 Area Scan Peak SAR : 0.827 W/kg  
 Zoom Scan Peak SAR : 1.081 W/kg

**SAR-Z Axis**  
at Hotspot x:7.12 y:-0.10

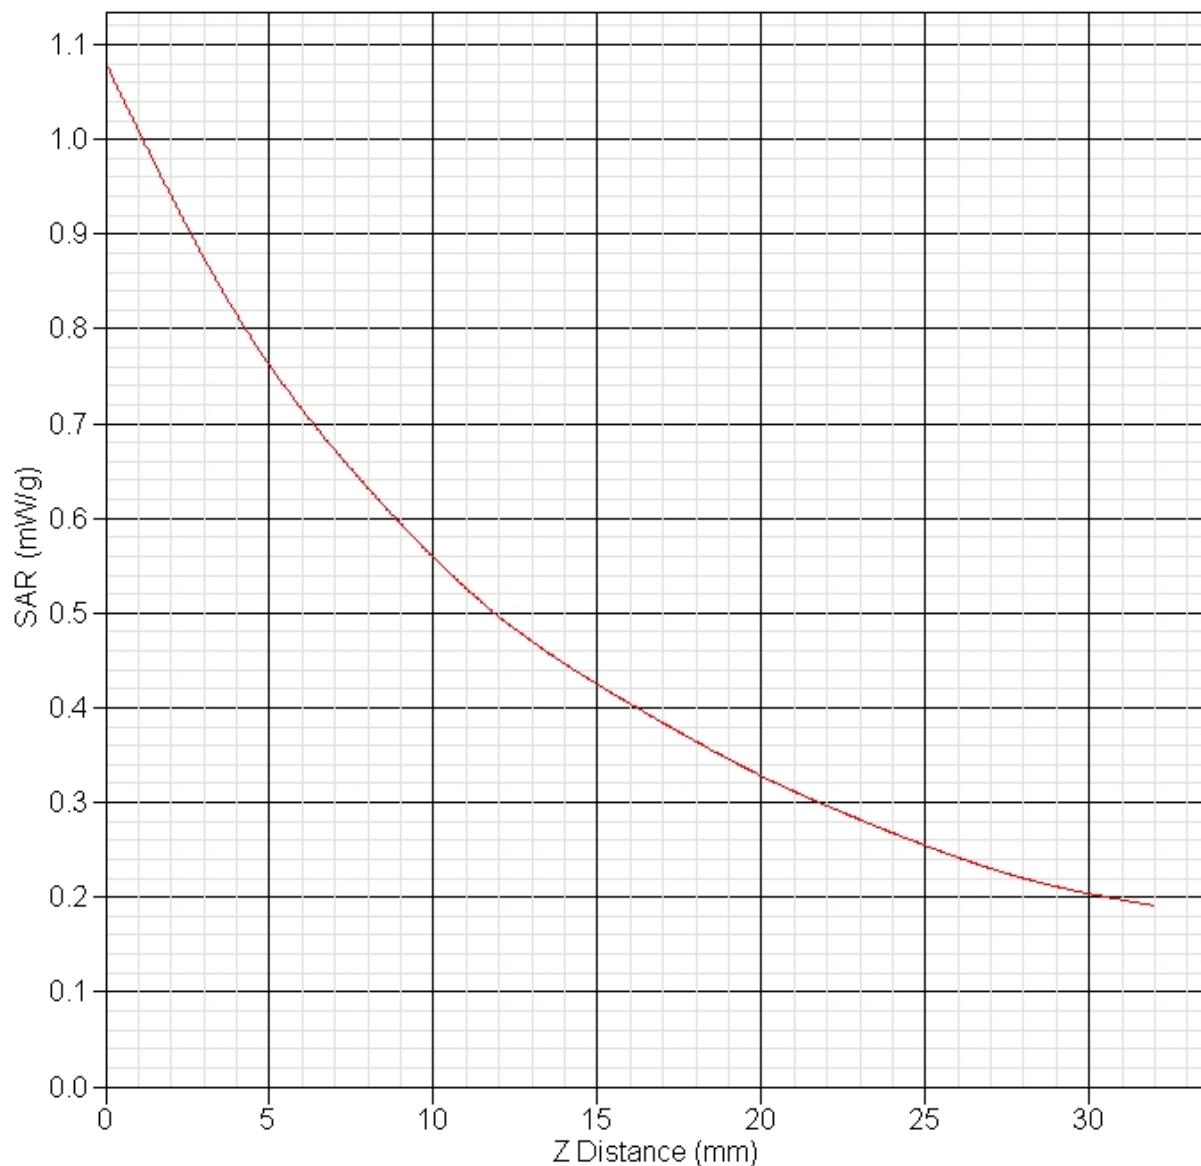

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 10:57:46 AM  
End Time : 21-Sep-2009 11:12:19 AM  
Scanning Time : 873 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 835.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Bottom Installed In Dell 910  
Power Drift-Start : 0.622 W/kg  
Power Drift-Finish: 0.631 W/kg  
Power Drift (%) : 1.479

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 835  
Frequency : 835.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 40.00 RH%  
Epsilon : 55.25 F/m  
Sigma : 0.99 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 835.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 6.3  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/(V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 10:38:48 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Bottom Installed In Dell 910  
 Separation : 5 mm  
 Channel : Mid

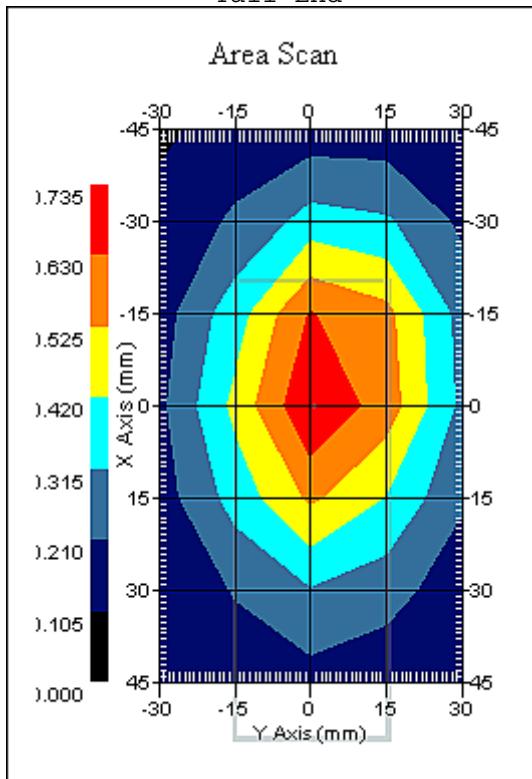**Tail End**

**Connector End**

1 gram SAR value : 0.677 W/kg  
 10 gram SAR value : 0.483 W/kg  
 Area Scan Peak SAR : 0.735 W/kg  
 Zoom Scan Peak SAR : 0.890 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 11:16:38 AM  
End Time : 21-Sep-2009 11:31:18 AM  
Scanning Time : 880 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 835.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Right Side Installed In Toshiba 2400  
Power Drift-Start : 0.323 W/kg  
Power Drift-Finish: 0.337 W/kg  
Power Drift (%) : 4.285

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 835  
Frequency : 835.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 40.00 RH%  
Epsilon : 55.25 F/m  
Sigma : 0.99 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 835.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 6.3  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 10:38:48 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Right Side Installed In Toshiba 2400  
 Separation : 5 mm  
 Channel : Mid

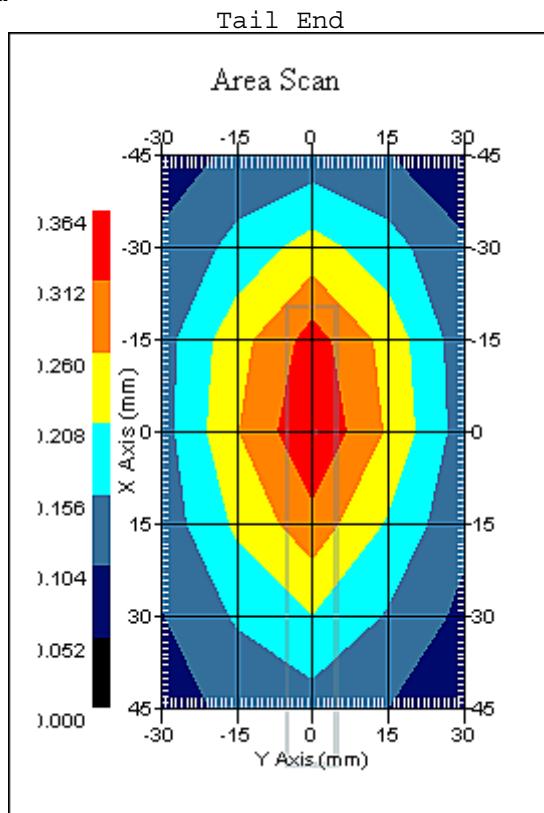

1 gram SAR value : 0.342 W/kg  
 10 gram SAR value : 0.247 W/kg  
 Area Scan Peak SAR : 0.362 W/kg  
 Zoom Scan Peak SAR : 0.470 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 11:33:50 AM  
End Time : 21-Sep-2009 11:48:34 AM  
Scanning Time : 884 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 835.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable  
Power Drift-Start : 0.619 W/kg  
Power Drift-Finish: 0.618 W/kg  
Power Drift (%) : -0.190

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 835  
Frequency : 835.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 40.00 RH%  
Epsilon : 55.25 F/m  
Sigma : 0.99 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 835.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 6.3  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 10:38:48 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable  
 Separation : 5 mm  
 Channel : Mid

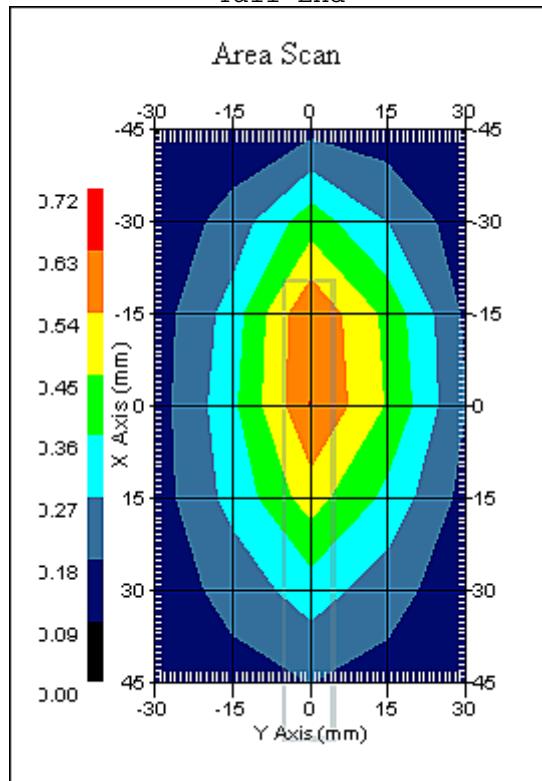**Tail End**

**Connector End**

1 gram SAR value : 0.609 W/kg  
 10 gram SAR value : 0.410 W/kg  
 Area Scan Peak SAR : 0.631 W/kg  
 Zoom Scan Peak SAR : 0.900 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 11:54:22 AM  
End Time : 21-Sep-2009 12:07:04 PM  
Scanning Time : 762 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 835.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 12 mm  
Width : 32 mm  
Depth : 90 mm  
Antenna Type : Internal  
Orientation : Tip On Cable  
Power Drift-Start : 0.133 W/kg  
Power Drift-Finish: 0.133 W/kg  
Power Drift (%) : -0.206

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 835  
Frequency : 835.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 40.00 RH%  
Epsilon : 55.25 F/m  
Sigma : 0.99 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 835.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 6.3  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 10:38:48 AM  
 Area Scan : 5x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Tip On Cable  
 Separation : 5 mm  
 Channel : Mid

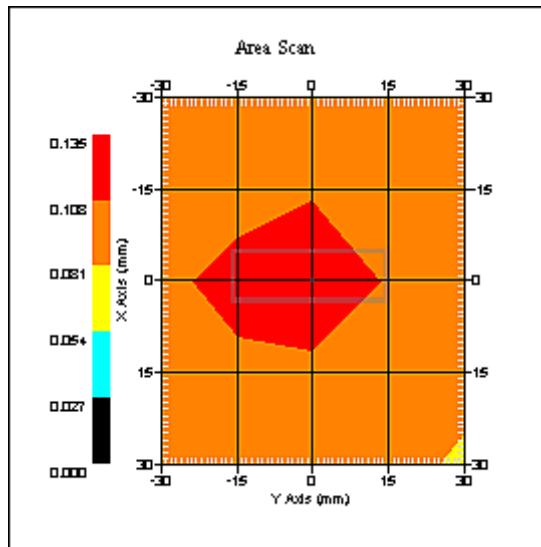

1 gram SAR value : 0.129 W/kg  
 10 gram SAR value : 0.096 W/kg  
 Area Scan Peak SAR : 0.133 W/kg  
 Zoom Scan Peak SAR : 0.190 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 01:24:57 PM  
End Time : 21-Sep-2009 01:39:37 PM  
Scanning Time : 880 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Top On Cable  
Power Drift-Start : 1.189 W/kg  
Power Drift-Finish: 1.194 W/kg  
Power Drift (%) : 0.441

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Top On Cable  
 Separation : 5 mm  
 Channel : Low

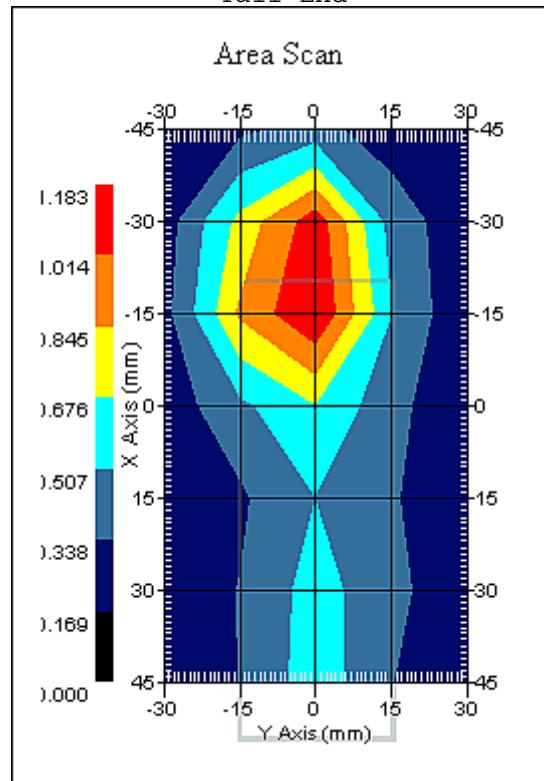**Tail End**


1 gram SAR value : 1.213 W/kg  
 10 gram SAR value : 0.720 W/kg  
 Area Scan Peak SAR : 1.180 W/kg  
 Zoom Scan Peak SAR : 2.051 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 01:06:36 PM  
End Time : 21-Sep-2009 01:21:35 PM  
Scanning Time : 899 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Top On Cable  
Power Drift-Start : 1.493 W/kg  
Power Drift-Finish: 1.494 W/kg  
Power Drift (%) : 0.058

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Top On Cable  
 Separation : 5 mm  
 Channel : Mid

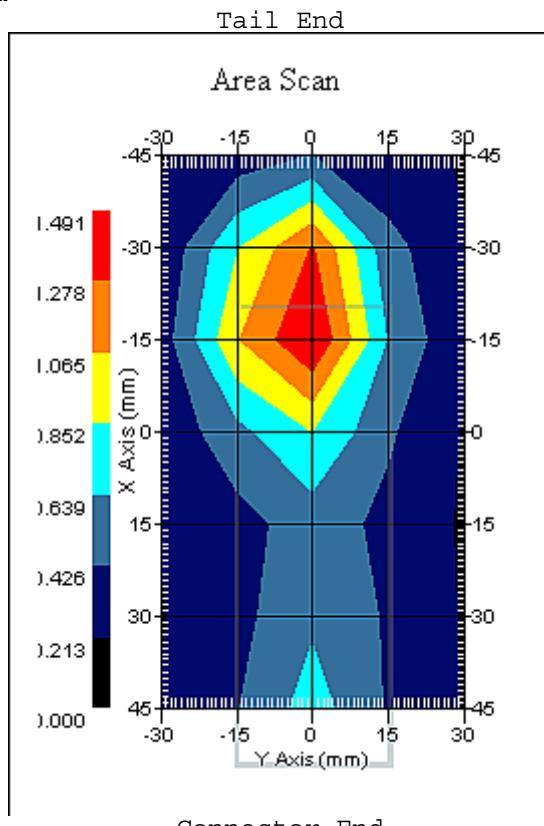

1 gram SAR value : 1.444 W/kg  
 10 gram SAR value : 0.847 W/kg  
 Area Scan Peak SAR : 1.489 W/kg  
 Zoom Scan Peak SAR : 2.442 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 01:40:42 PM  
End Time : 21-Sep-2009 01:55:14 PM  
Scanning Time : 872 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Top On Cable  
Power Drift-Start : 1.416 W/kg  
Power Drift-Finish: 1.402 W/kg  
Power Drift (%) : -0.965

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Top On Cable  
 Separation : 5 mm  
 Channel : High

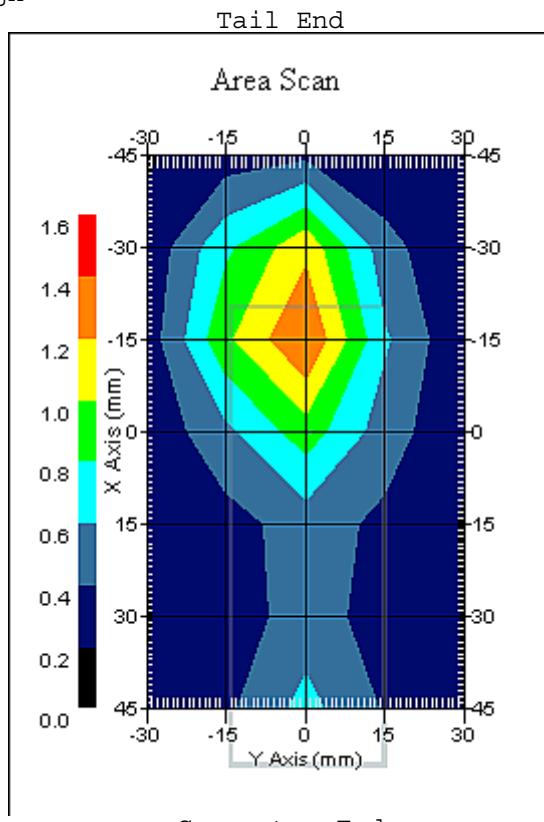

1 gram SAR value : 1.288 W/kg  
 10 gram SAR value : 0.760 W/kg  
 Area Scan Peak SAR : 1.402 W/kg  
 Zoom Scan Peak SAR : 2.171 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 01:57:47 PM  
End Time : 21-Sep-2009 02:12:29 PM  
Scanning Time : 882 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Top On Cable  
Power Drift-Start : 0.596 W/kg  
Power Drift-Finish: 0.593 W/kg  
Power Drift (%) : -0.612

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Top On Cable  
 Separation : 5 mm  
 Channel : Mid

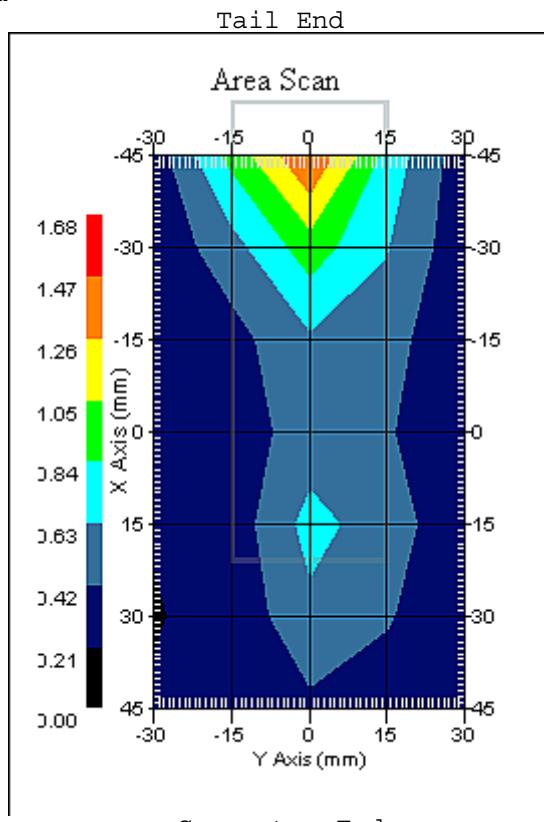

1 gram SAR value : 0.674 W/kg  
 10 gram SAR value : 0.448 W/kg  
 Area Scan Peak SAR : 1.473 W/kg  
 Zoom Scan Peak SAR : 0.990 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 02:37:32 PM  
End Time : 21-Sep-2009 02:52:11 PM  
Scanning Time : 879 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Bottom Installed In Dell 910  
Power Drift-Start : 1.379 W/kg  
Power Drift-Finish: 1.352 W/kg  
Power Drift (%) : -1.986

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Bottom Installed In Dell 910  
 Separation : 5 mm  
 Channel : Low

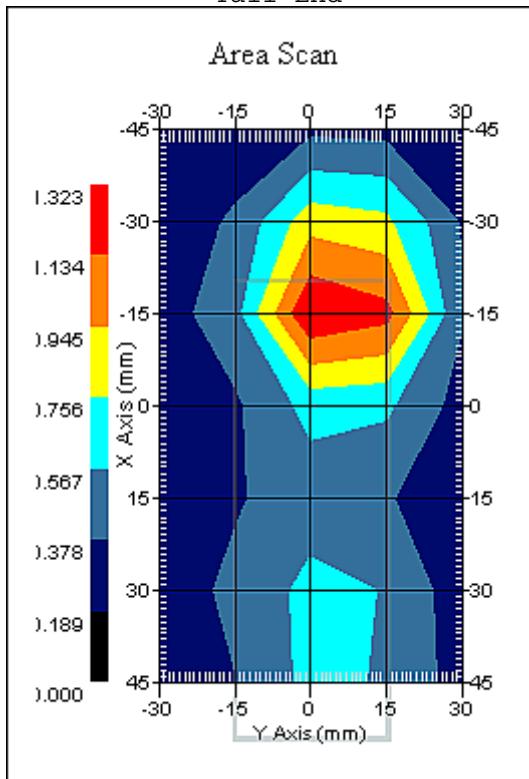**Tail End**

**Connector End**

1 gram SAR value : 1.346 W/kg  
 10 gram SAR value : 0.791 W/kg  
 Area Scan Peak SAR : 1.322 W/kg  
 Zoom Scan Peak SAR : 2.232 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 02:18:25 PM  
End Time : 21-Sep-2009 02:33:05 PM  
Scanning Time : 880 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Bottom Installed In Dell910  
Power Drift-Start : 1.479 W/kg  
Power Drift-Finish: 1.487 W/kg  
Power Drift (%) : 0.560

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Bottom Installed In Dell910  
 Separation : 5 mm  
 Channel : Mid

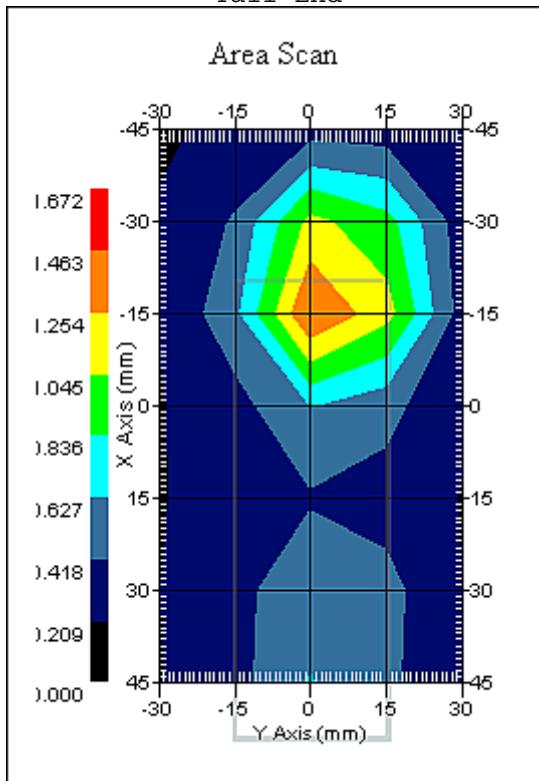**Tail End**

**Connector End**

1 gram SAR value : 1.440 W/kg  
 10 gram SAR value : 0.800 W/kg  
 Area Scan Peak SAR : 1.464 W/kg  
 Zoom Scan Peak SAR : 2.532 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 03:00:01 PM  
End Time : 21-Sep-2009 03:14:34 PM  
Scanning Time : 873 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Bottom Installed In Dell 910  
Power Drift-Start : 1.537 W/kg  
Power Drift-Finish: 1.520 W/kg  
Power Drift (%) : -1.108

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


**Other Data**

DUT Position : Bottom Installed In Dell 910  
 Separation : 5 mm  
 Channel : High

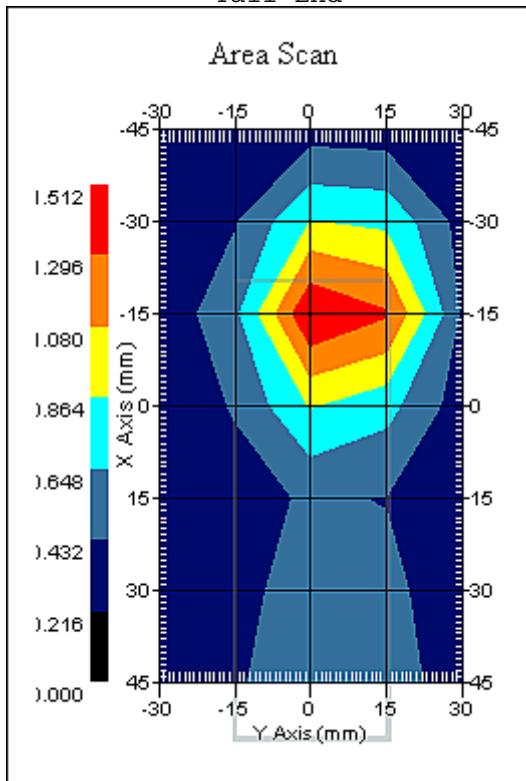**Tail End**

**Connector End**

1 gram SAR value : 1.497 W/kg  
 10 gram SAR value : 0.873 W/kg  
 Area Scan Peak SAR : 1.510 W/kg  
 Zoom Scan Peak SAR : 2.502 W/kg

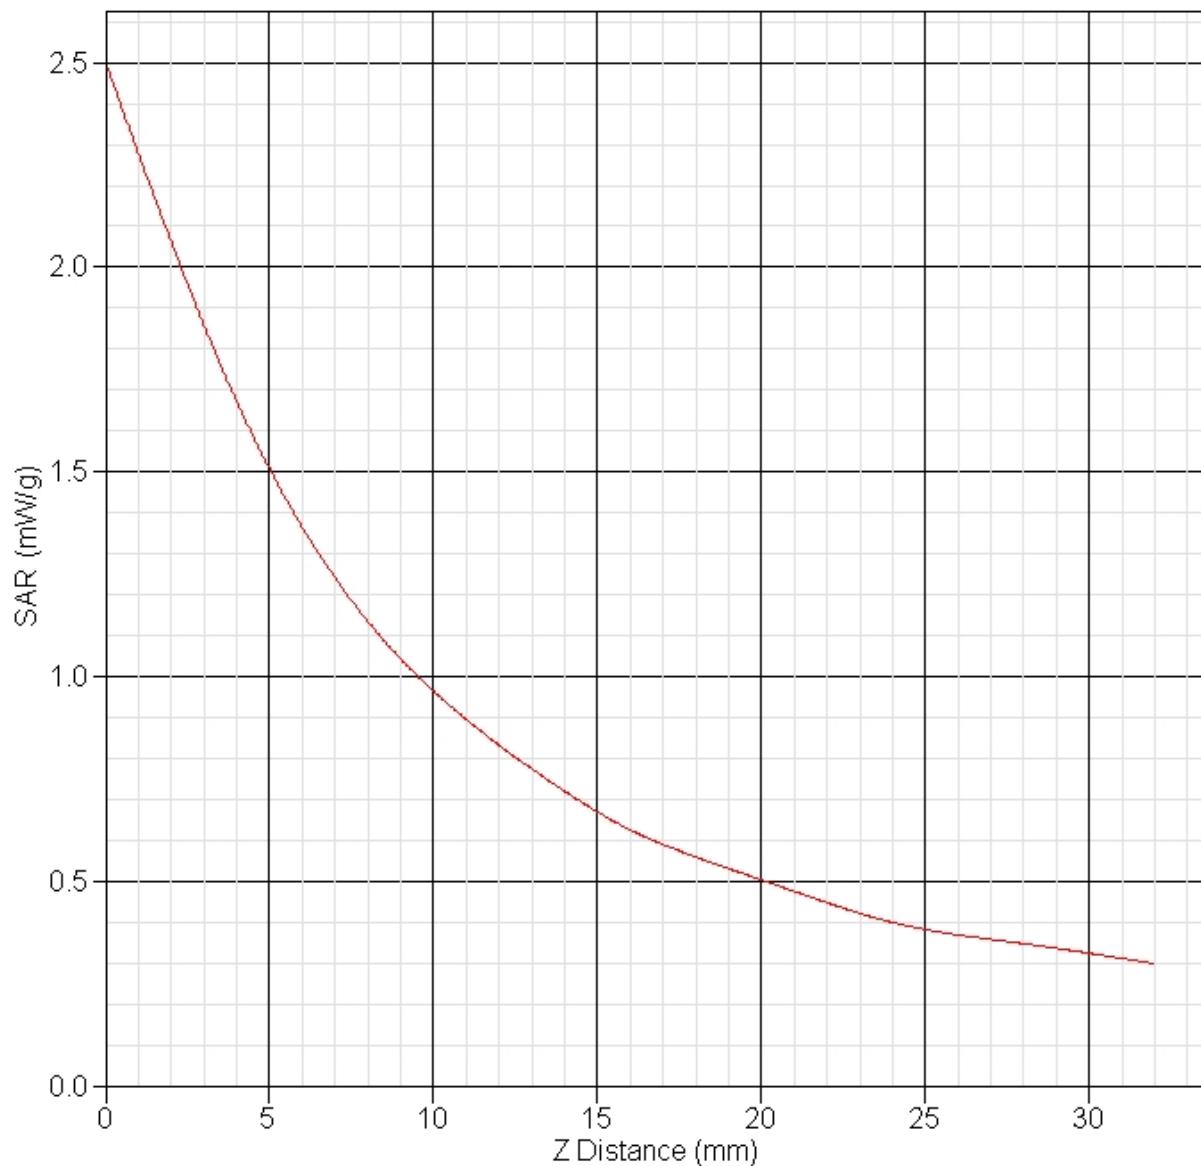**SAR-Z Axis**  
at Hotspot x:0.07 y:7.86



**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 03:18:12 PM  
End Time : 21-Sep-2009 03:32:46 PM  
Scanning Time : 874 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Bottom Installed In Dell 910  
Power Drift-Start : 0.476 W/kg  
Power Drift-Finish: 0.475 W/kg  
Power Drift (%) : -0.163

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Bottom Installed In Dell 910  
 Separation : 5 mm  
 Channel : High

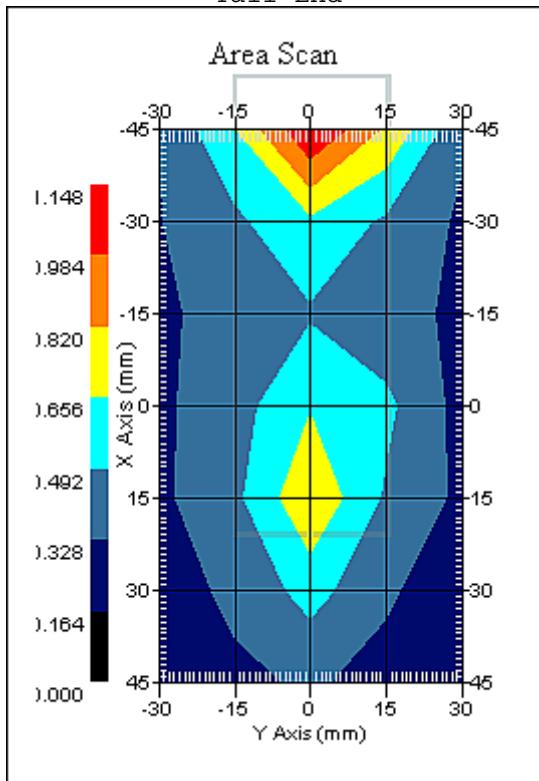**Tail End**

**Connector End**

1 gram SAR value : 0.725 W/kg  
 10 gram SAR value : 0.519 W/kg  
 Area Scan Peak SAR : 1.147 W/kg  
 Zoom Scan Peak SAR : 1.030 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 03:41:02 PM  
End Time : 21-Sep-2009 04:03:48 PM  
Scanning Time : 1366 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Right Side Installed In Toshiba 2400  
Power Drift-Start : 0.530 W/kg  
Power Drift-Finish: 0.543 W/kg  
Power Drift (%) : 2.373

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Right Side Installed In Toshiba 2400  
 Separation : 5 mm  
 Channel : Mid

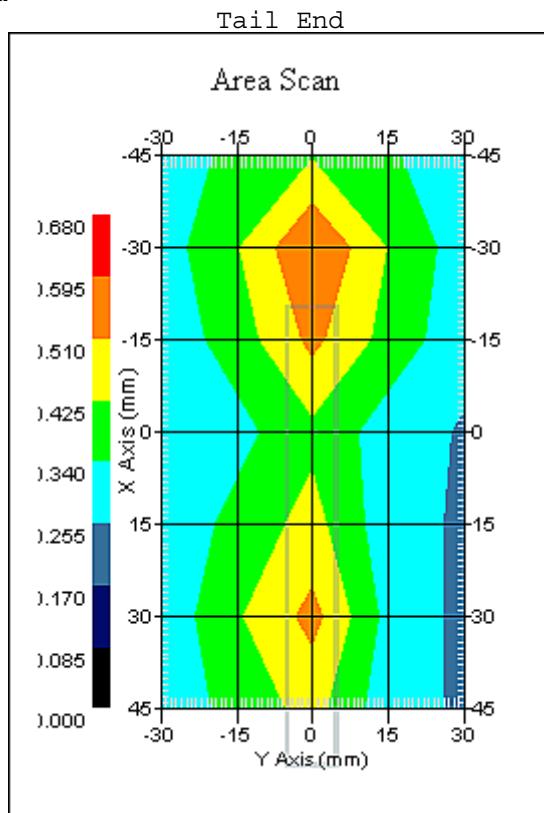

1 gram SAR value : 0.575 W/kg  
 10 gram SAR value : 0.414 W/kg  
 Area Scan Peak SAR : 0.596 W/kg  
 Zoom Scan Peak SAR : 0.810 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 05:16:34 PM  
End Time : 21-Sep-2009 05:31:18 PM  
Scanning Time : 884 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable  
Power Drift-Start : 1.261 W/kg  
Power Drift-Finish: 1.230 W/kg  
Power Drift (%) : -2.458

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable  
 Separation : 5 mm  
 Channel : Low

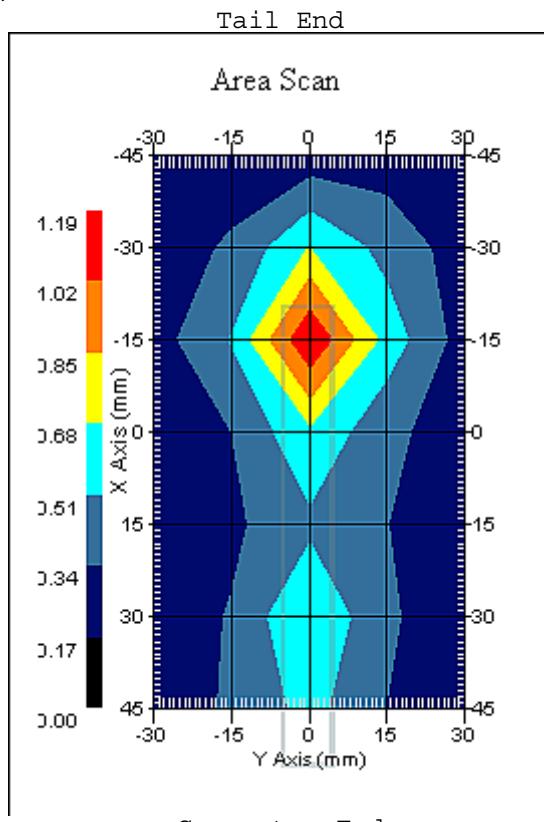

1 gram SAR value : 1.077 W/kg  
 10 gram SAR value : 0.655 W/kg  
 Area Scan Peak SAR : 1.187 W/kg  
 Zoom Scan Peak SAR : 1.801 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 04:47:21 PM  
End Time : 21-Sep-2009 05:02:05 PM  
Scanning Time : 884 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable  
Power Drift-Start : 1.520 W/kg  
Power Drift-Finish: 1.490 W/kg  
Power Drift (%) : -1.947

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable  
 Separation : 5 mm  
 Channel : Mid

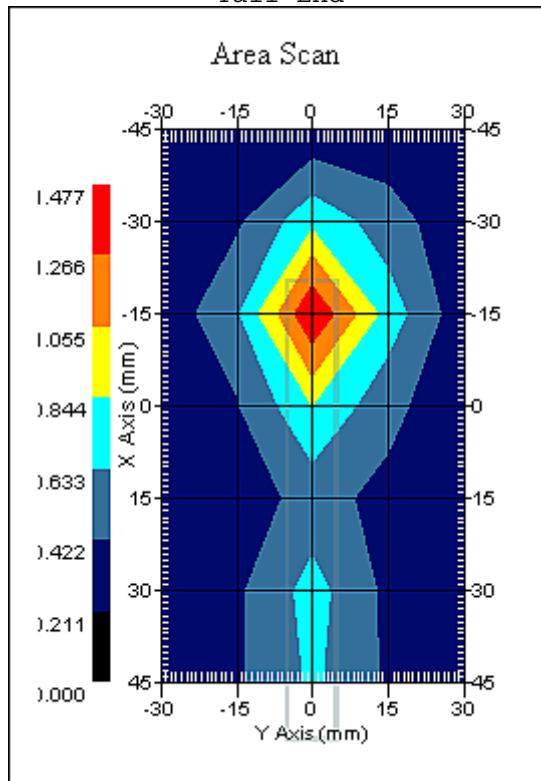**Tail End**

**Connector End**

1 gram SAR value : 1.291 W/kg  
 10 gram SAR value : 0.769 W/kg  
 Area Scan Peak SAR : 1.476 W/kg  
 Zoom Scan Peak SAR : 2.131 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 05:32:08 PM  
End Time : 21-Sep-2009 05:46:49 PM  
Scanning Time : 881 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable  
Power Drift-Start : 1.445 W/kg  
Power Drift-Finish: 1.432 W/kg  
Power Drift (%) : -0.879

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/(V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable  
 Separation : 5 mm  
 Channel : High

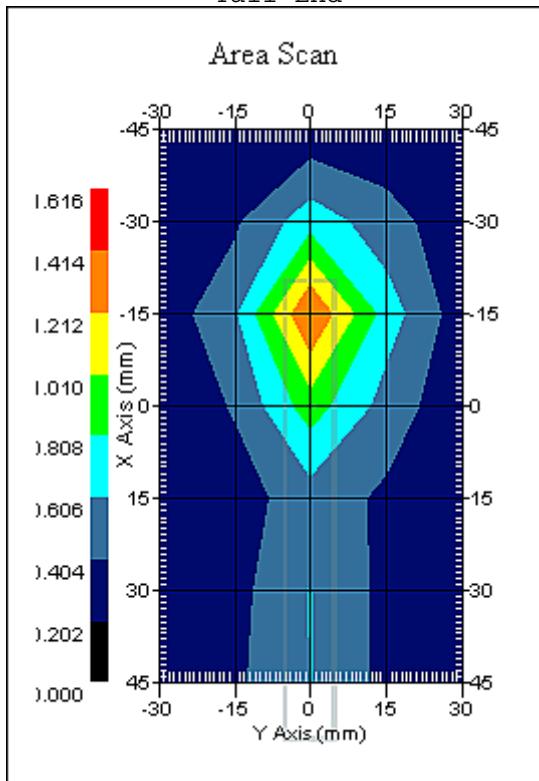**Tail End**

**Connector End**

1 gram SAR value : 1.243 W/kg  
 10 gram SAR value : 0.744 W/kg  
 Area Scan Peak SAR : 1.415 W/kg  
 Zoom Scan Peak SAR : 2.071 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 05:48:12 PM  
End Time : 21-Sep-2009 06:02:49 PM  
Scanning Time : 877 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable  
Power Drift-Start : 0.683 W/kg  
Power Drift-Finish: 0.690 W/kg  
Power Drift (%) : 1.021

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable  
 Separation : 5 mm  
 Channel : Mid

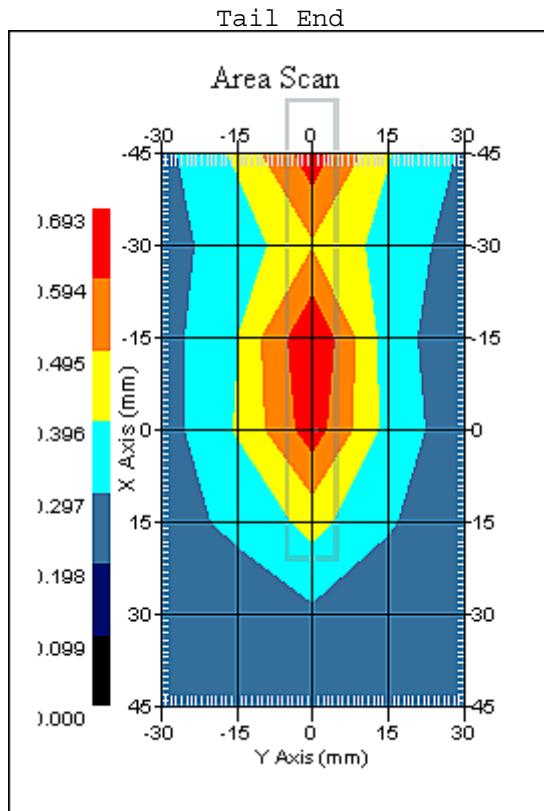

1 gram SAR value : 0.660 W/kg  
 10 gram SAR value : 0.459 W/kg  
 Area Scan Peak SAR : 0.692 W/kg  
 Zoom Scan Peak SAR : 1.030 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 21-Sep-2009  
Starting Time : 21-Sep-2009 12:46:33 PM  
End Time : 21-Sep-2009 12:59:11 PM  
Scanning Time : 758 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : 1xRTT  
Model : U301  
Frequency : 1900.00 MHz  
Max. Transmit Pwr : 0.25 W  
Drift Time : 0 min(s)  
Length : 12 mm  
Width : 32 mm  
Depth : 90 mm  
Antenna Type : Internal  
Orientation : Tip On Cable  
Power Drift-Start : 0.677 W/kg  
Power Drift-Finish: 0.674 W/kg  
Power Drift (%) : -0.543

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 1900  
Frequency : 1900.00 MHz  
Last Calib. Date : 21-Sep-2009  
Temperature : 23.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 44.00 RH%  
Epsilon : 53.10 F/m  
Sigma : 1.53 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 21-Sep-2009  
 Set-up Time : 12:46:06 PM  
 Area Scan : 5x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Tip On Cable  
 Separation : 5 mm  
 Channel : Mid

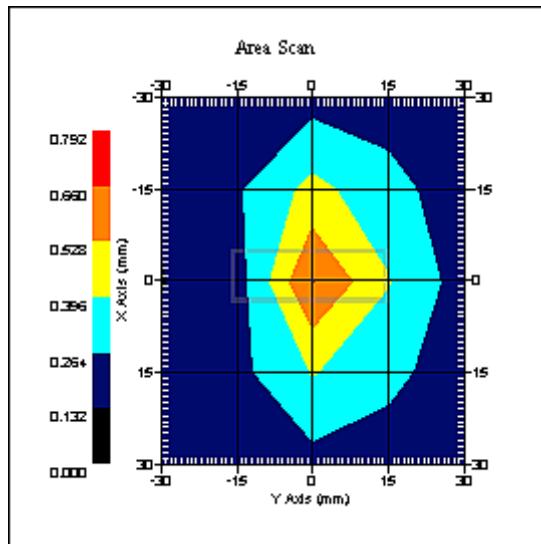

1 gram SAR value : 0.585 W/kg  
 10 gram SAR value : 0.361 W/kg  
 Area Scan Peak SAR : 0.662 W/kg  
 Zoom Scan Peak SAR : 0.970 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 10:30:26 AM  
End Time : 22-Sep-2009 10:45:14 AM  
Scanning Time : 888 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\frac{1}{2}$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Top On Cable  
Power Drift-Start : 0.648 W/kg  
Power Drift-Finish: 0.652 W/kg  
Power Drift (%) : 0.577

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Top On Cable  
 Separation : 5 mm  
 Channel : Low

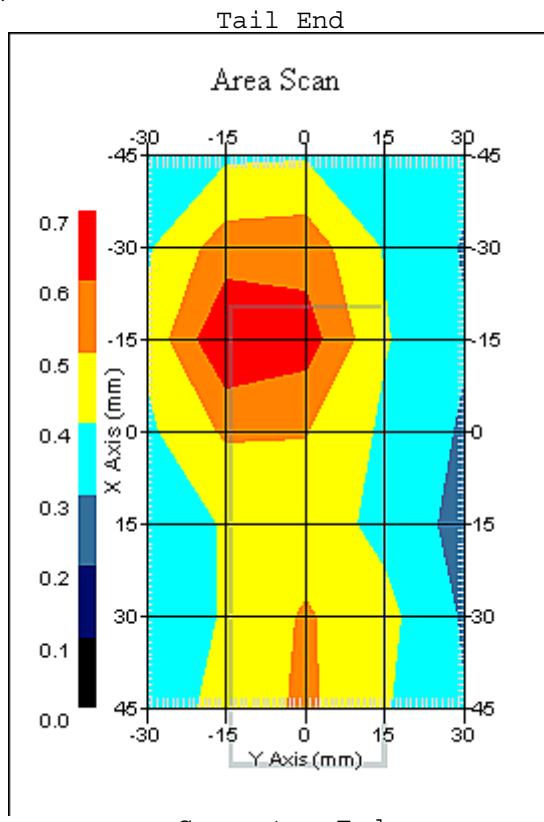

1 gram SAR value : 0.683 W/kg  
 10 gram SAR value : 0.506 W/kg  
 Area Scan Peak SAR : 0.697 W/kg  
 Zoom Scan Peak SAR : 0.940 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 10:14:35 AM  
End Time : 22-Sep-2009 10:29:15 AM  
Scanning Time : 880 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Top On Cable  
Power Drift-Start : 0.774 W/kg  
Power Drift-Finish: 0.795 W/kg  
Power Drift (%) : 2.742

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Top On Cable  
 Separation : 5 mm  
 Channel : Mid

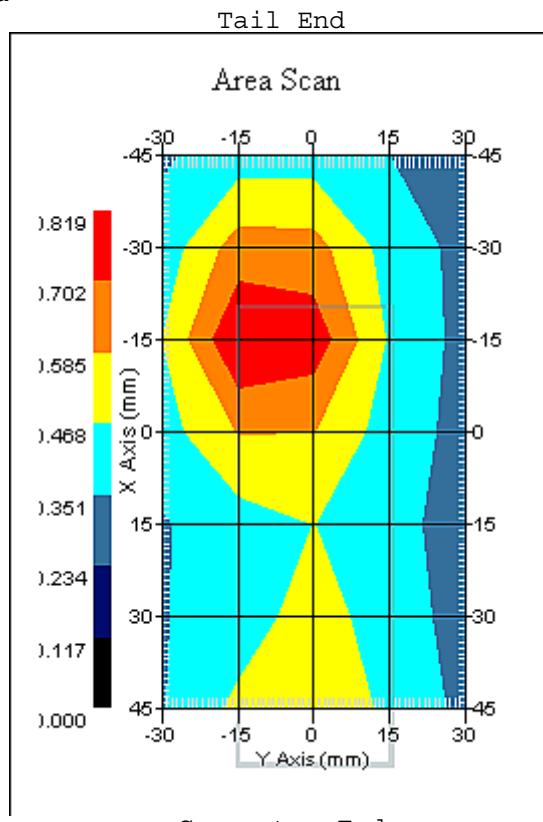

1 gram SAR value : 0.833 W/kg  
 10 gram SAR value : 0.577 W/kg  
 Area Scan Peak SAR : 0.818 W/kg  
 Zoom Scan Peak SAR : 1.231 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 10:45:55 AM  
End Time : 22-Sep-2009 11:00:40 AM  
Scanning Time : 885 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Top On Cable  
Power Drift-Start : 0.789 W/kg  
Power Drift-Finish: 0.804 W/kg  
Power Drift (%) : 1.983

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Top On Cable  
 Separation : 5 mm  
 Channel : High

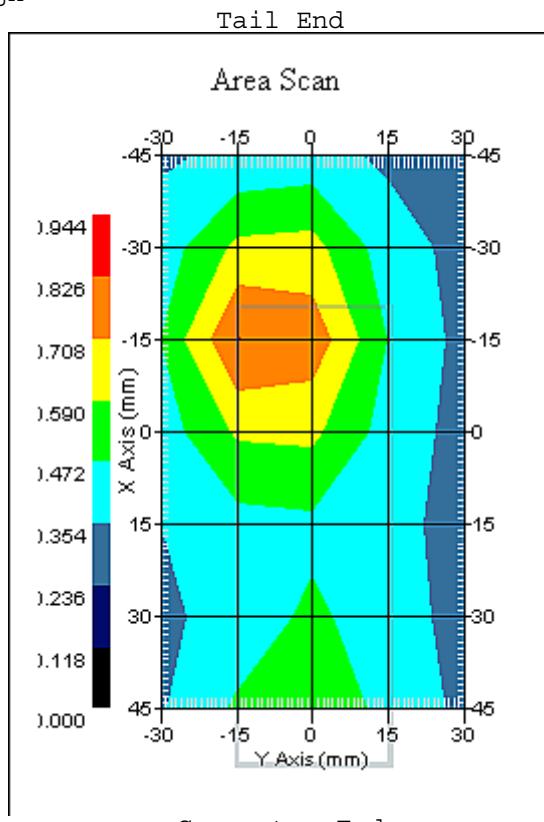

1 gram SAR value : 0.796 W/kg  
 10 gram SAR value : 0.562 W/kg  
 Area Scan Peak SAR : 0.829 W/kg  
 Zoom Scan Peak SAR : 1.181 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 11:03:33 AM  
End Time : 22-Sep-2009 11:18:16 AM  
Scanning Time : 883 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Top On Cable  
Power Drift-Start : 0.502 W/kg  
Power Drift-Finish: 0.478 W/kg  
Power Drift (%) : -4.782

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Top On Cable  
 Separation : 5 mm  
 Channel : Mid

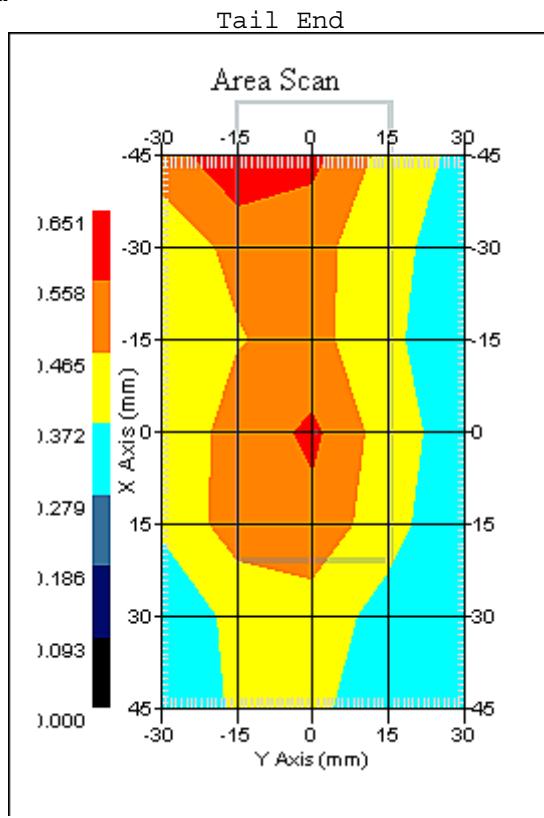

1 gram SAR value : 0.565 W/kg  
 10 gram SAR value : 0.464 W/kg  
 Area Scan Peak SAR : 0.648 W/kg  
 Zoom Scan Peak SAR : 0.660 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 11:21:57 AM  
End Time : 22-Sep-2009 11:36:37 AM  
Scanning Time : 880 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Bottom Installed In Dell 910  
Power Drift-Start : 0.811 W/kg  
Power Drift-Finish: 0.828 W/kg  
Power Drift (%) : 2.114

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data


Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m  
Probe Data  
Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Bottom Installed In Dell 910  
 Separation : 5 mm  
 Channel : Mid

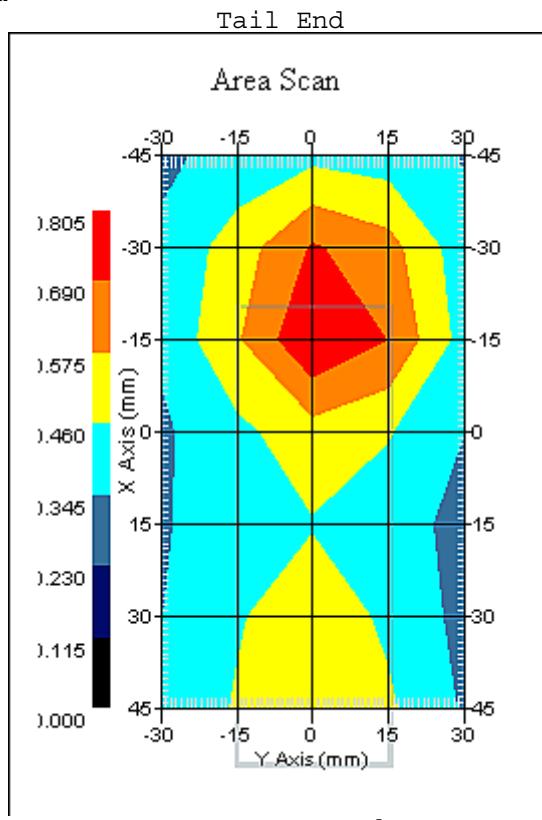

1 gram SAR value : 0.784 W/kg  
 10 gram SAR value : 0.559 W/kg  
 Area Scan Peak SAR : 0.805 W/kg  
 Zoom Scan Peak SAR : 1.111 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 11:37:49 AM  
End Time : 22-Sep-2009 11:52:24 AM  
Scanning Time : 875 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Bottom Installed In Dell 910  
Power Drift-Start : 0.507 W/kg  
Power Drift-Finish: 0.490 W/kg  
Power Drift (%) : -3.359

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/(V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Bottom Installed In Dell 910  
 Separation : 5 mm  
 Channel : Mid

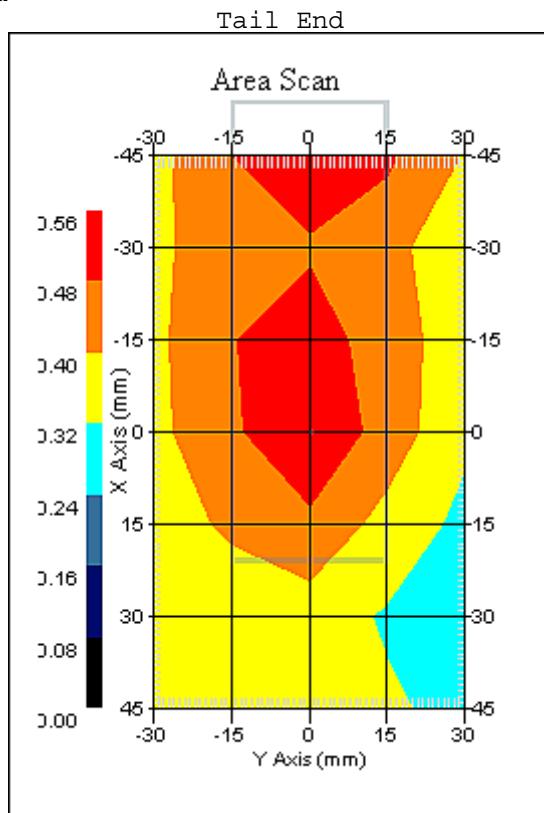

1 gram SAR value : 0.535 W/kg  
 10 gram SAR value : 0.449 W/kg  
 Area Scan Peak SAR : 0.559 W/kg  
 Zoom Scan Peak SAR : 0.660 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 11:57:02 AM  
End Time : 22-Sep-2009 12:19:38 PM  
Scanning Time : 1356 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\frac{1}{2}$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Right Side Installed In Toshiba 2400  
Power Drift-Start : 0.501 W/kg  
Power Drift-Finish: 0.492 W/kg  
Power Drift (%) : -1.796

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Right Side Installed In Toshiba 2400  
 Separation : 5 mm  
 Channel : Mid

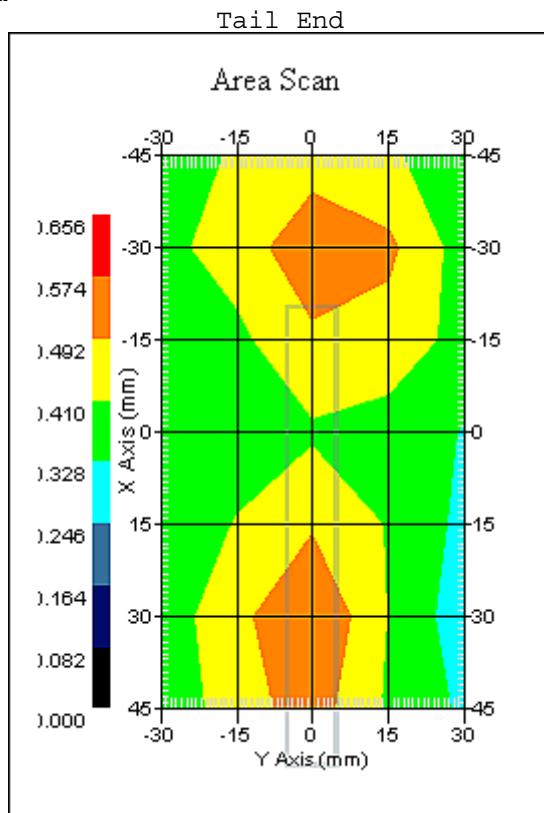

1 gram SAR value : 0.563 W/kg  
 10 gram SAR value : 0.448 W/kg  
 Area Scan Peak SAR : 0.575 W/kg  
 Zoom Scan Peak SAR : 0.740 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 12:38:55 PM  
End Time : 22-Sep-2009 12:53:21 PM  
Scanning Time : 866 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable  
Power Drift-Start : 0.977 W/kg  
Power Drift-Finish: 1.007 W/kg  
Power Drift (%) : 3.015

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable  
 Separation : 5 mm  
 Channel : Low

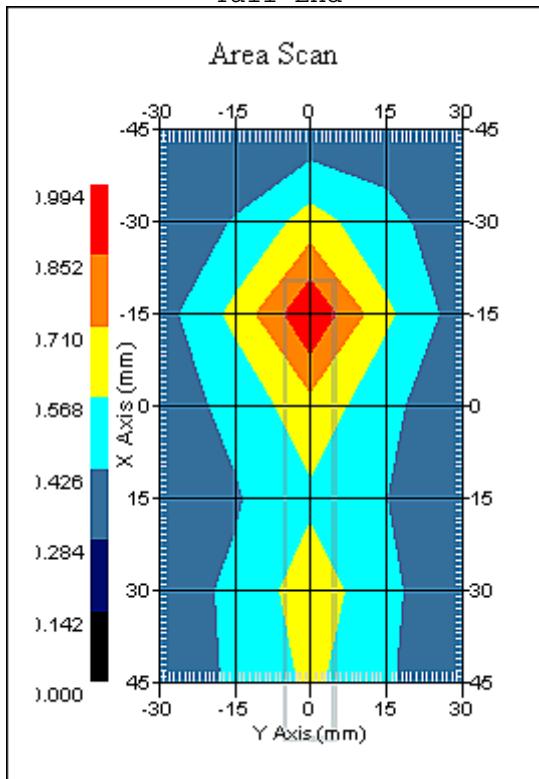**Tail End**

**Connector End**

1 gram SAR value : 0.902 W/kg  
 10 gram SAR value : 0.622 W/kg  
 Area Scan Peak SAR : 0.993 W/kg  
 Zoom Scan Peak SAR : 1.331 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 12:23:18 PM  
End Time : 22-Sep-2009 12:37:52 PM  
Scanning Time : 874 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\frac{1}{2}$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable  
Power Drift-Start : 1.184 W/kg  
Power Drift-Finish: 1.220 W/kg  
Power Drift (%) : 3.014

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


**Other Data**

DUT Position : Left Side On Cable  
 Separation : 5 mm  
 Channel : Mid

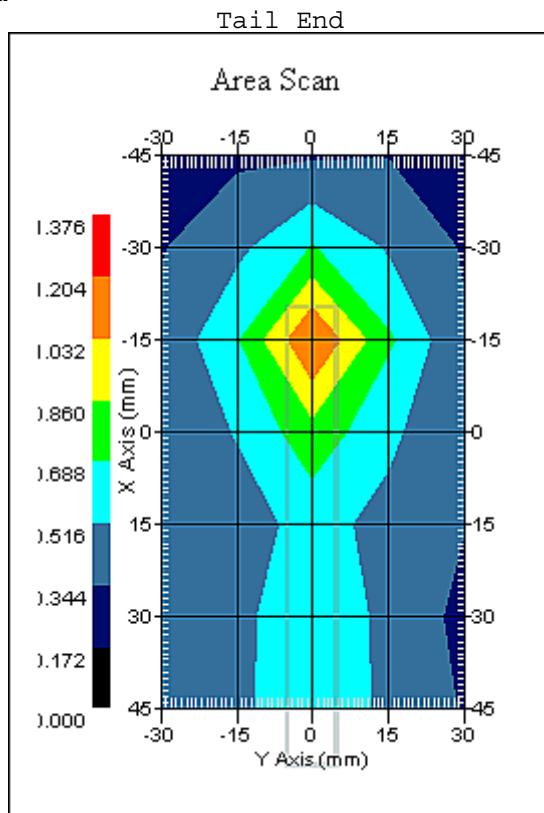

1 gram SAR value : 1.106 W/kg  
 10 gram SAR value : 0.724 W/kg  
 Area Scan Peak SAR : 1.207 W/kg  
 Zoom Scan Peak SAR : 1.661 W/kg

**SAR-Z Axis**  
at Hotspot x:0.04 y:-0.16

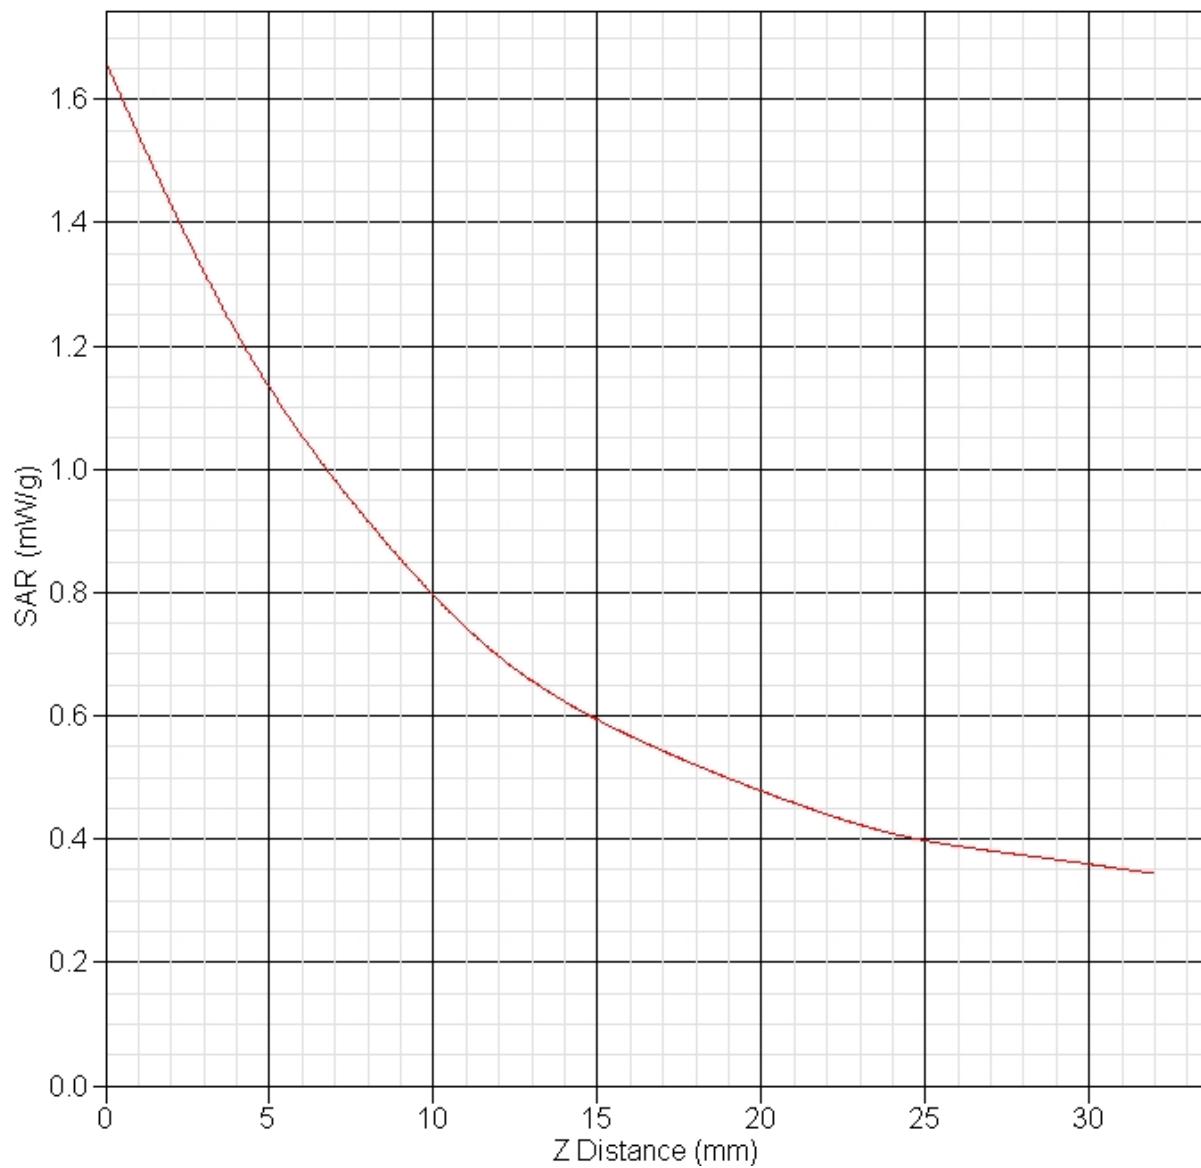

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 12:54:53 PM  
End Time : 22-Sep-2009 01:09:28 PM  
Scanning Time : 875 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable  
Power Drift-Start : 1.172 W/kg  
Power Drift-Finish: 1.168 W/kg  
Power Drift (%) : -0.416

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable  
 Separation : 5 mm  
 Channel : High

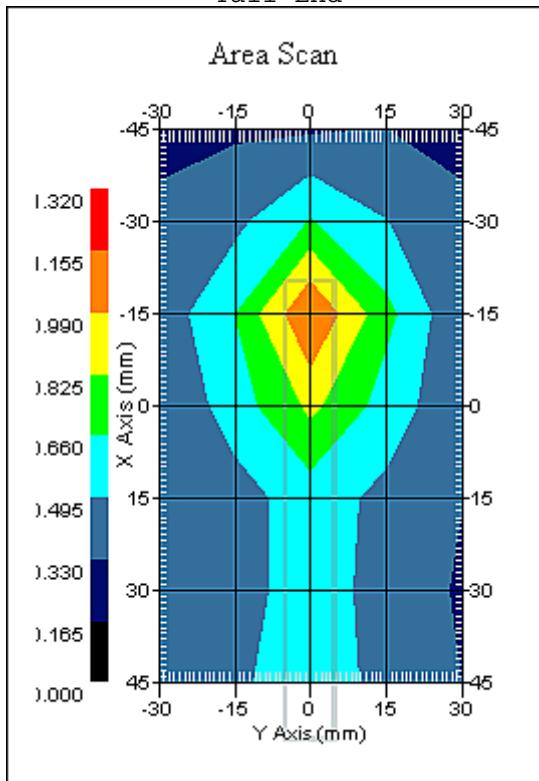**Tail End**

**Connector End**

1 gram SAR value : 1.060 W/kg  
 10 gram SAR value : 0.706 W/kg  
 Area Scan Peak SAR : 1.158 W/kg  
 Zoom Scan Peak SAR : 1.611 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 01:11:24 PM  
End Time : 22-Sep-2009 01:26:15 PM  
Scanning Time : 891 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable  
Power Drift-Start : 0.629 W/kg  
Power Drift-Finish: 0.602 W/kg  
Power Drift (%) : -4.282

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/(V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable  
 Separation : 5 mm  
 Channel : Mid

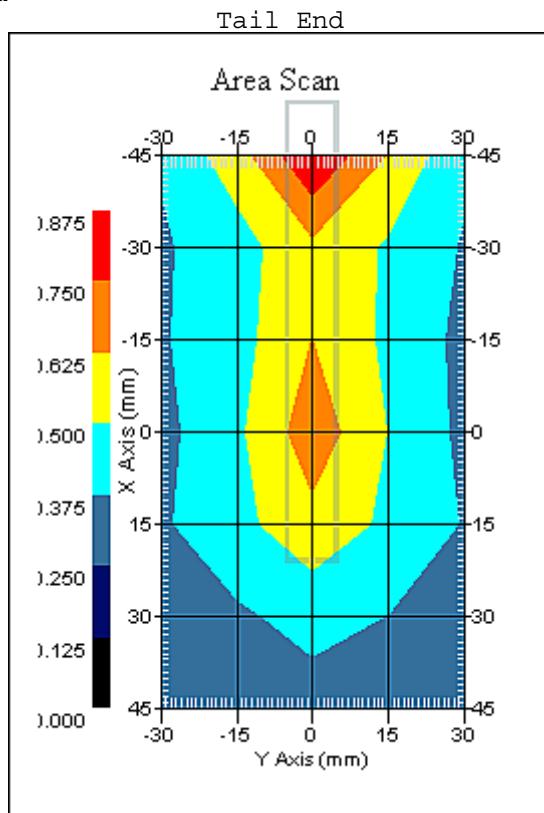

1 gram SAR value : 0.654 W/kg  
 10 gram SAR value : 0.512 W/kg  
 Area Scan Peak SAR : 0.874 W/kg  
 Zoom Scan Peak SAR : 0.840 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 01:30:03 PM  
End Time : 22-Sep-2009 01:42:45 PM  
Scanning Time : 762 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  5 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 12 mm  
Width : 32 mm  
Depth : 90 mm  
Antenna Type : Internal  
Orientation : Tip On Cable  
Power Drift-Start : 0.692 W/kg  
Power Drift-Finish: 0.680 W/kg  
Power Drift (%) : -1.836

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 5x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Tip On Cable  
 Separation : 5 mm  
 Channel : Mid

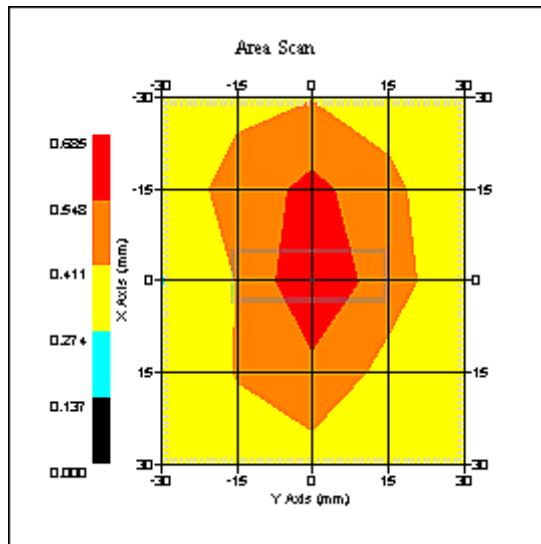

1 gram SAR value : 0.628 W/kg  
 10 gram SAR value : 0.466 W/kg  
 Area Scan Peak SAR : 0.685 W/kg  
 Zoom Scan Peak SAR : 0.870 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 03:19:42 PM  
End Time : 22-Sep-2009 03:34:31 PM  
Scanning Time : 889 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  10 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Top On Cable  
Power Drift-Start : 0.583 W/kg  
Power Drift-Finish: 0.610 W/kg  
Power Drift (%) : 4.633

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Top On Cable  
 Separation : 5 mm  
 Channel : Mid

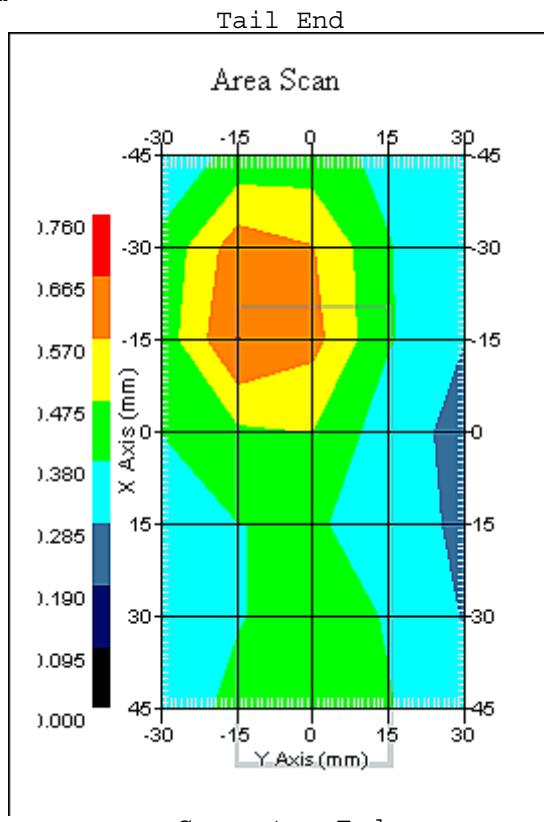

1 gram SAR value : 0.650 W/kg  
 10 gram SAR value : 0.492 W/kg  
 Area Scan Peak SAR : 0.668 W/kg  
 Zoom Scan Peak SAR : 0.880 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 03:36:08 PM  
End Time : 22-Sep-2009 03:50:49 PM  
Scanning Time : 881 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  10 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 32 mm  
Depth : 12 mm  
Antenna Type : Internal  
Orientation : Bottom Installed In Dell 910  
Power Drift-Start : 0.694 W/kg  
Power Drift-Finish: 0.712 W/kg  
Power Drift (%) : 2.663

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Bottom Installed In Dell 910  
 Separation : 5 mm  
 Channel : Mid

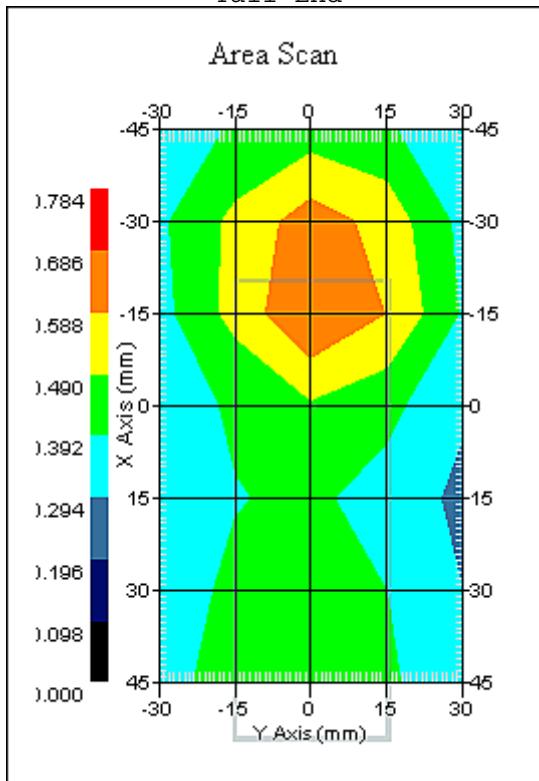**Tail End**

**Connector End**

1 gram SAR value : 0.681 W/kg  
 10 gram SAR value : 0.510 W/kg  
 Area Scan Peak SAR : 0.687 W/kg  
 Zoom Scan Peak SAR : 0.970 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 03:52:45 PM  
End Time : 22-Sep-2009 04:15:21 PM  
Scanning Time : 1356 secs

**Product Data**

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  10 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Right Side Installed In Toshiba 2400  
Power Drift-Start : 0.408 W/kg  
Power Drift-Finish: 0.396 W/kg  
Power Drift (%) : -2.949

**Phantom Data**

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

**Tissue Data**

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

**Probe Data**


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Right Side Installed In Toshiba 2400  
 Separation : 5 mm  
 Channel : Mid

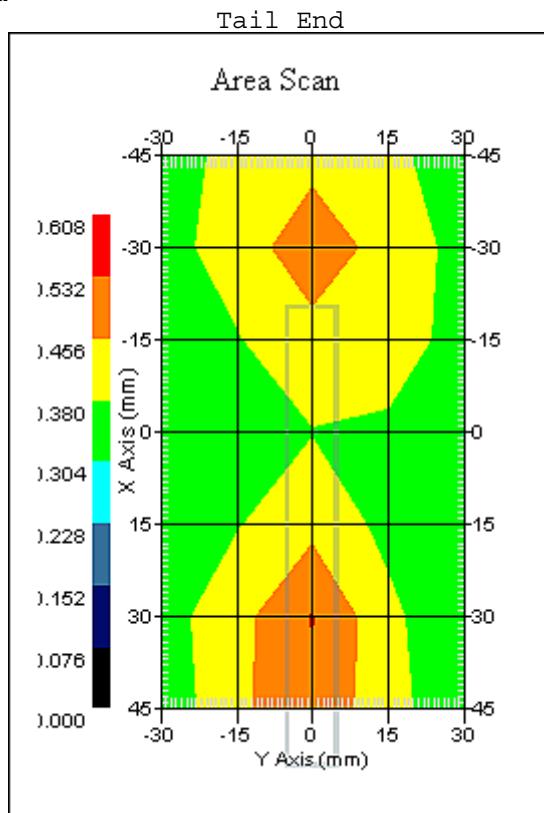

1 gram SAR value : 0.524 W/kg  
 10 gram SAR value : 0.428 W/kg  
 Area Scan Peak SAR : 0.535 W/kg  
 Zoom Scan Peak SAR : 0.660 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 04:18:50 PM  
End Time : 22-Sep-2009 04:33:28 PM  
Scanning Time : 878 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  10 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable  
Power Drift-Start : 0.865 W/kg  
Power Drift-Finish: 0.889 W/kg  
Power Drift (%) : 2.773

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


**Other Data**

DUT Position : Left Side On Cable  
 Separation : 5 mm  
 Channel : Mid

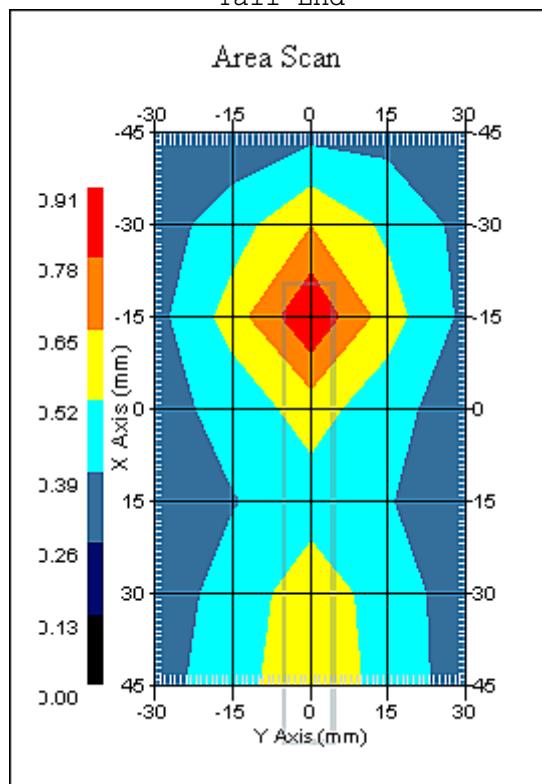**Tail End**

**Connector End**

1 gram SAR value : 0.796 W/kg  
 10 gram SAR value : 0.558 W/kg  
 Area Scan Peak SAR : 0.907 W/kg  
 Zoom Scan Peak SAR : 1.221 W/kg

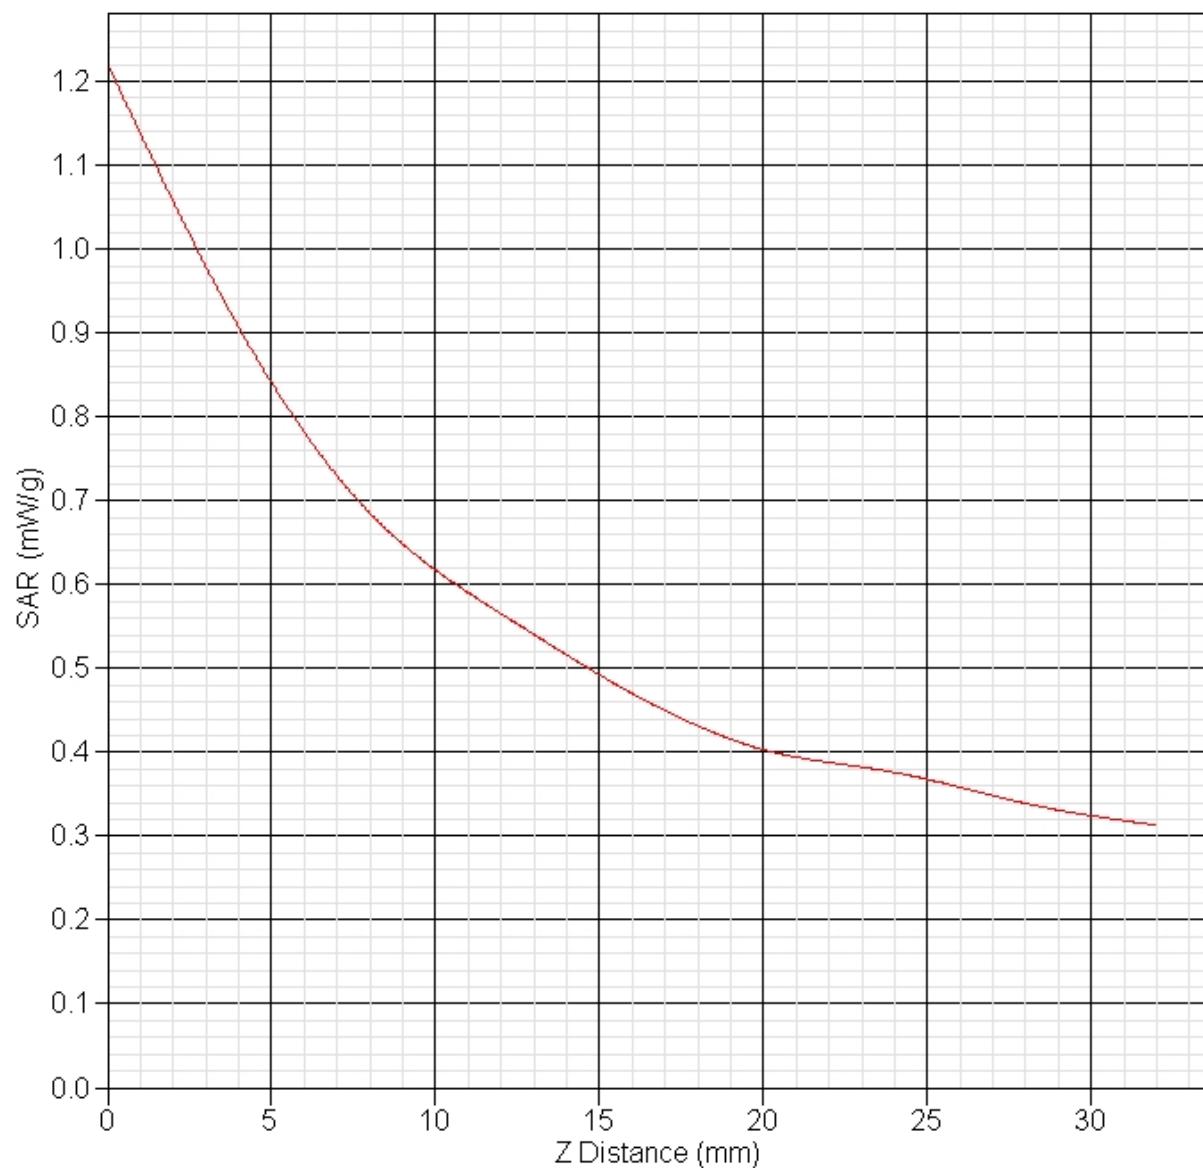**SAR-Z Axis**  
at Hotspot x:0.04 y:-0.14



**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 04:36:58 PM  
End Time : 22-Sep-2009 04:51:35 PM  
Scanning Time : 877 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  10 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 90 mm  
Width : 12 mm  
Depth : 32 mm  
Antenna Type : Internal  
Orientation : Left Side On Cable  
Power Drift-Start : 0.533 W/kg  
Power Drift-Finish: 0.529 W/kg  
Power Drift (%) : -0.758

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 7x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Left Side On Cable  
 Separation : 5 mm  
 Channel : Mid

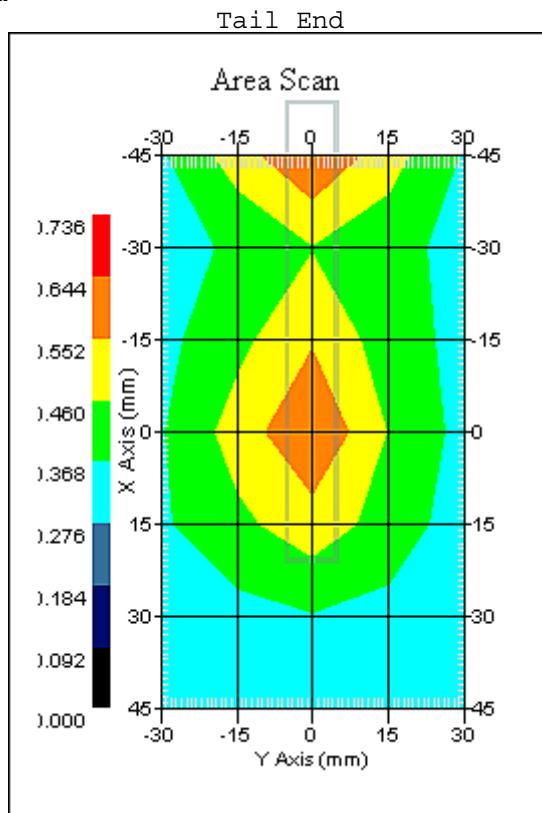

1 gram SAR value : 0.597 W/kg  
 10 gram SAR value : 0.479 W/kg  
 Area Scan Peak SAR : 0.646 W/kg  
 Zoom Scan Peak SAR : 0.780 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 22-Sep-2009  
Starting Time : 22-Sep-2009 04:53:46 PM  
End Time : 22-Sep-2009 05:06:32 PM  
Scanning Time : 766 secs

## Product Data

Device Name : Cmotech  
Serial No. : 91  
Mode : QPSK  $\times$  10 MHz  
Model : U301  
Frequency : 2600.00 MHz  
Max. Transmit Pwr : 0.2 W  
Drift Time : 0 min(s)  
Length : 12 mm  
Width : 32 mm  
Depth : 90 mm  
Antenna Type : Internal  
Orientation : Tip On Cable  
Power Drift-Start : 0.634 W/kg  
Power Drift-Finish: 0.636 W/kg  
Power Drift (%) : 0.302

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 2590  
Frequency : 2590.00 MHz  
Last Calib. Date : 22-Sep-2009  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 52.48 F/m  
Sigma : 2.13 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe 215 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 215  
Last Calib. Date : 03-Nov-2008  
Frequency : 2600.00 MHz  
Duty Cycle Factor: 3.24  
Conversion Factor: 5  
Probe Sensitivity: 1.20 1.20 1.20  $\mu$ V/ (V/m)<sup>2</sup>  
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 3.24  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 22-Sep-2009  
 Set-up Time : 9:24:08 AM  
 Area Scan : 5x5x1 : Measurement x=15mm, y=15mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

**Other Data**

DUT Position : Tip On Cable  
 Separation : 5 mm  
 Channel : Mid

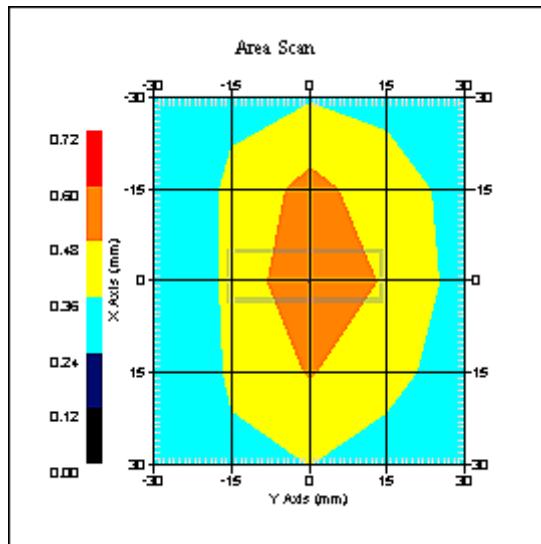

1 gram SAR value : 0.576 W/kg  
 10 gram SAR value : 0.430 W/kg  
 Area Scan Peak SAR : 0.602 W/kg  
 Zoom Scan Peak SAR : 0.790 W/kg

## Appendix D – Probe Calibration Data Sheets

# NCL CALIBRATION LABORATORIES

Calibration File No.: CP-926

Client.: RFEL

## C E R T I F I C A T E   O F   C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 835 MHz

BODY Calibration

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 215

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: RFEL-00150-CAL-5367

Calibrated: 3<sup>rd</sup> November 2008  
Released on: 3<sup>rd</sup> November 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary  
This calibration has been conducted in line with the SCC ISO-IEC 17025 Scope of Accreditation

Accredited Laboratory Number 48

Released By: \_\_\_\_\_

**NCL** CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## **NCL Calibration Laboratories**

---

Division of APREL Laboratories.

### **Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 215.

### **References**

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
IEEE 1309 "IEEE Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9 KHz to 40 GHz" 2005  
SSI-TP-011 Tissue Calibration Procedure  
IEC 62209 "Human exposure to radio frequency fields from handheld and body-mounted wireless communication devices –Human models, instrumentation and procedures Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for handheld devices used in close proximity of the ear (frequency range of 200MHz to 3GHz)"

### **Conditions**

Probe 215 was a re-calibration.


**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

**We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.**



---

Stuart Nicol



---

Jesse Hones

## Calibration Results Summary

<b>Probe Type:</b>	E-Field Probe E-020
<b>Serial Number:</b>	215
<b>Frequency:</b>	835 MHz
<b>Sensor Offset:</b>	1.56 mm
<b>Sensor Length:</b>	2.5 mm
<b>Tip Enclosure:</b>	Ertalyte*
<b>Tip Diameter:</b>	<5 mm
<b>Tip Length:</b>	60 mm
<b>Total Length:</b>	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

### Sensitivity in Air

<b>Channel X:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Y:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Z:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Diode Compression Point:</b>	95 mV

**Sensitivity in Body Tissue Measured****Frequency:** 835 MHz**Epsilon:** 55.2 (+/-5%) **Sigma:** 0.96 S/m (+/-5%)**ConvF****Channel X:** 6.3**Channel Y:** 6.3**Channel Z:** 6.3

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


**Boundary Effect:**



Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

**Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


## Receiving Pattern 835 MHz (Air)

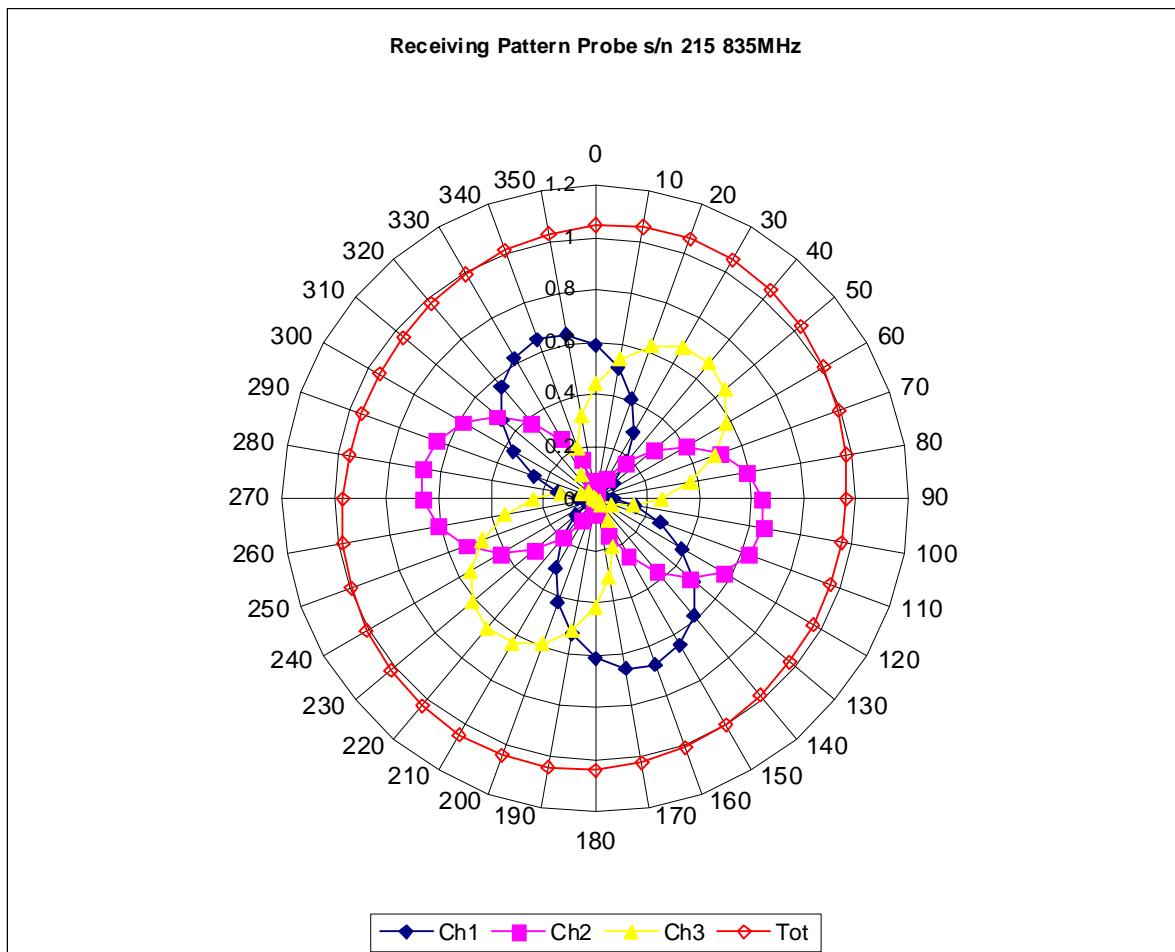

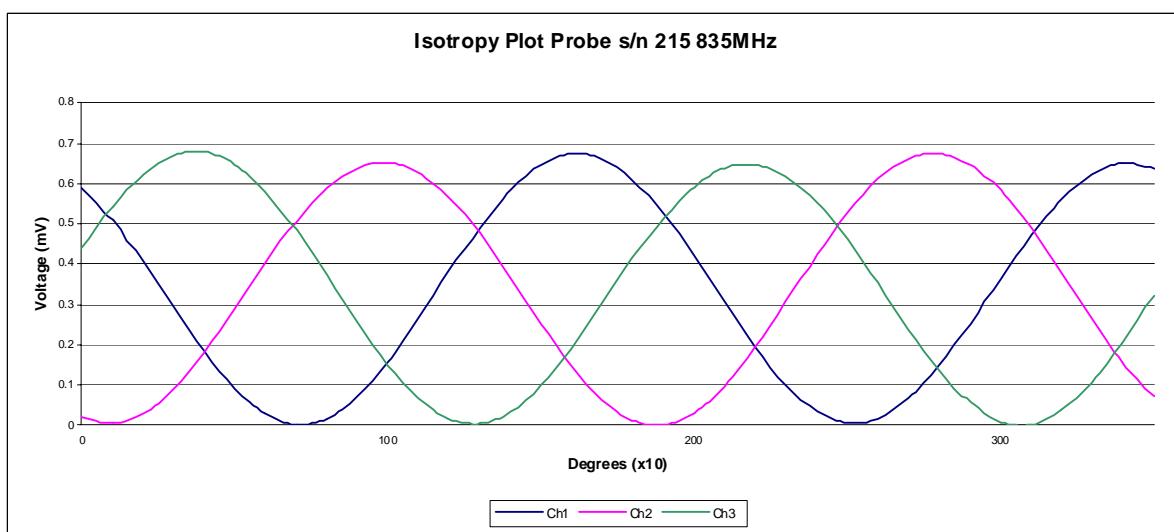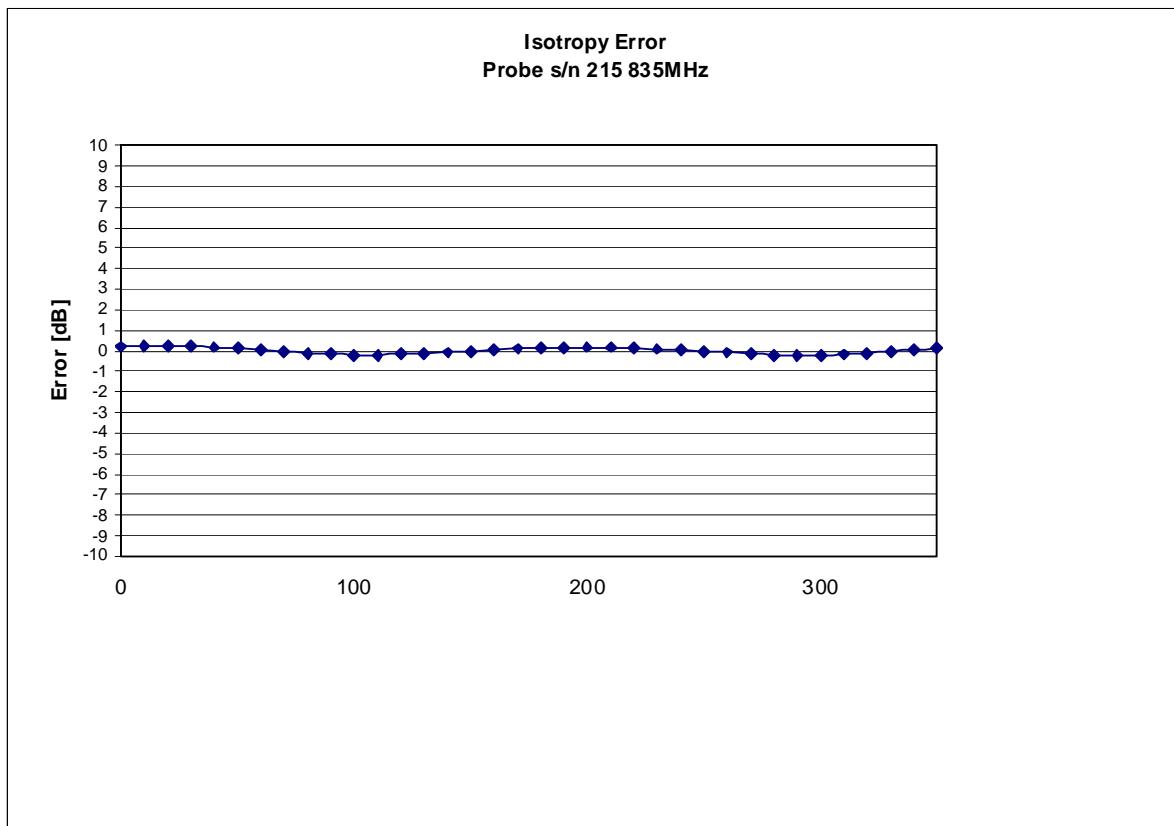**Isotropy Error 835 MHz (Air)****Isotropicity Tissue:**


0.10 dB

## Dynamic Range

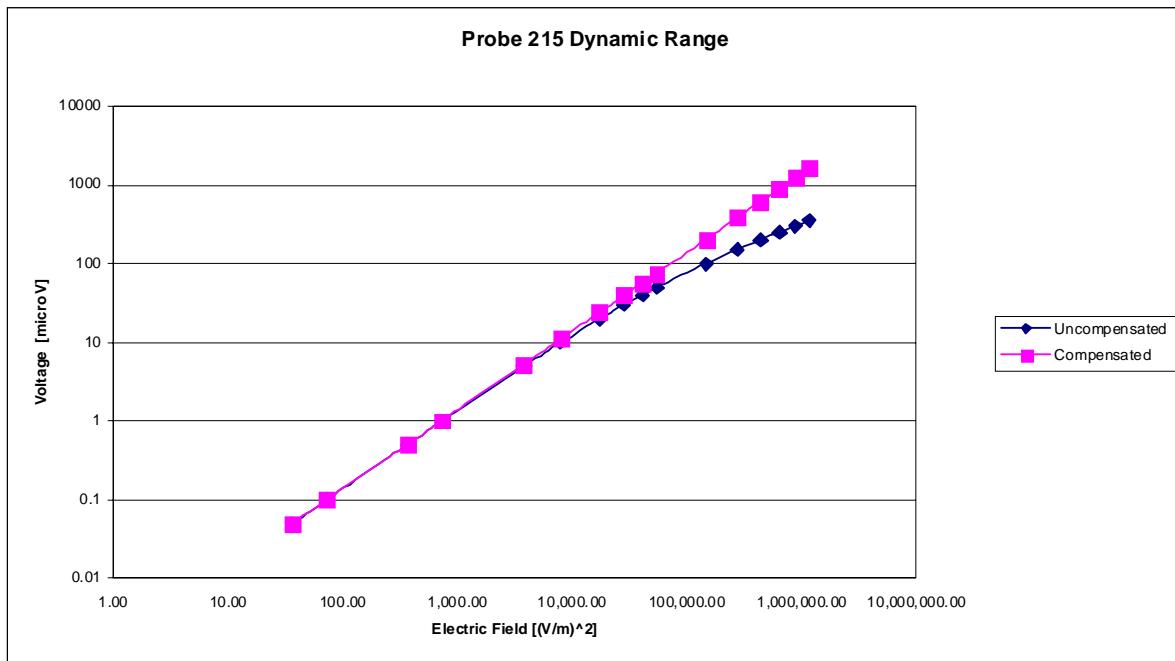

## Video Bandwidth

**Probe Frequency Characteristics**

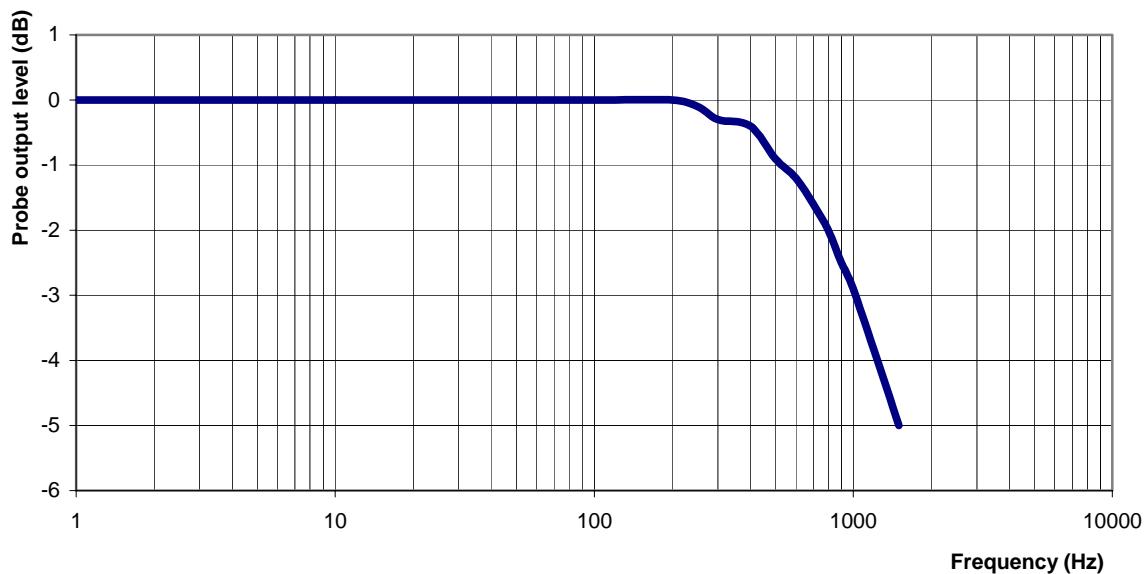

**Video Bandwidth at 500 Hz** 1 dB  
**Video Bandwidth at 1.02 KHz:** 3 dB

## **Conversion Factor Uncertainty Assessment Measured**

### **Sensitivity in Body Tissue**

**Frequency:** 835 MHz

**Epsilon:** 55.2 (+/-5%) **Sigma:** 0.96 S/m (+/-5%)

#### **ConvF**

**Channel X:** 6.3 7%(K=2)

**Channel Y:** 6.3 7%(K=2)

**Channel Z:** 6.3 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

#### **Boundary Effect:**

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

# NCL CALIBRATION LABORATORIES

Calibration File No.: CP-933

Client.: RFEL

## C E R T I F I C A T E   O F   C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 1900 MHz

BODY Calibration

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 215

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: RFEL-00150-CAL-5367

Calibrated: 3<sup>rd</sup> November 2008  
Released on: 3<sup>rd</sup> November 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary  
This calibration has been conducted in line with the SCC ISO-IEC 17025 Scope of Accreditation

Accredited Laboratory Number 48

Released By: \_\_\_\_\_

**NCL** CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## **NCL Calibration Laboratories**

---

Division of APREL Laboratories.

### **Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 215.

### **References**


SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
IEEE 1309 "IEEE Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9 KHz to 40 GHz" 2005  
SSI-TP-011 Tissue Calibration Procedure  
IEC 62209 "Human exposure to radio frequency fields from handheld and body-mounted wireless communication devices –Human models, instrumentation and procedures Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for handheld devices used in close proximity of the ear (frequency range of 200MHz to 3GHz)"

### **Conditions**

Probe 215 was a re-calibration.


**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

**We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.**



---

Stuart Nicol



---

Jesse Hones

## Calibration Results Summary

<b>Probe Type:</b>	E-Field Probe E-020
<b>Serial Number:</b>	215
<b>Frequency:</b>	1900 MHz
<b>Sensor Offset:</b>	1.56 mm
<b>Sensor Length:</b>	2.5 mm
<b>Tip Enclosure:</b>	Ertalyte*
<b>Tip Diameter:</b>	<5 mm
<b>Tip Length:</b>	60 mm
<b>Total Length:</b>	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

### Sensitivity in Air

<b>Channel X:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Y:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Z:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Diode Compression Point:</b>	95 mV

## **Sensitivity in Body Tissue Measured**

**Frequency:** 1900 MHz

**Epsilon:** 54.2 (+/-5%) **Sigma:** 1.57 S/m (+/-5%)

### **ConvF**

**Channel X:** 5.0

**Channel Y:** 5.0

**Channel Z:** 5.0

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


### **Boundary Effect:**



Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

### **Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


## Receiving Pattern 1900 MHz (Air)

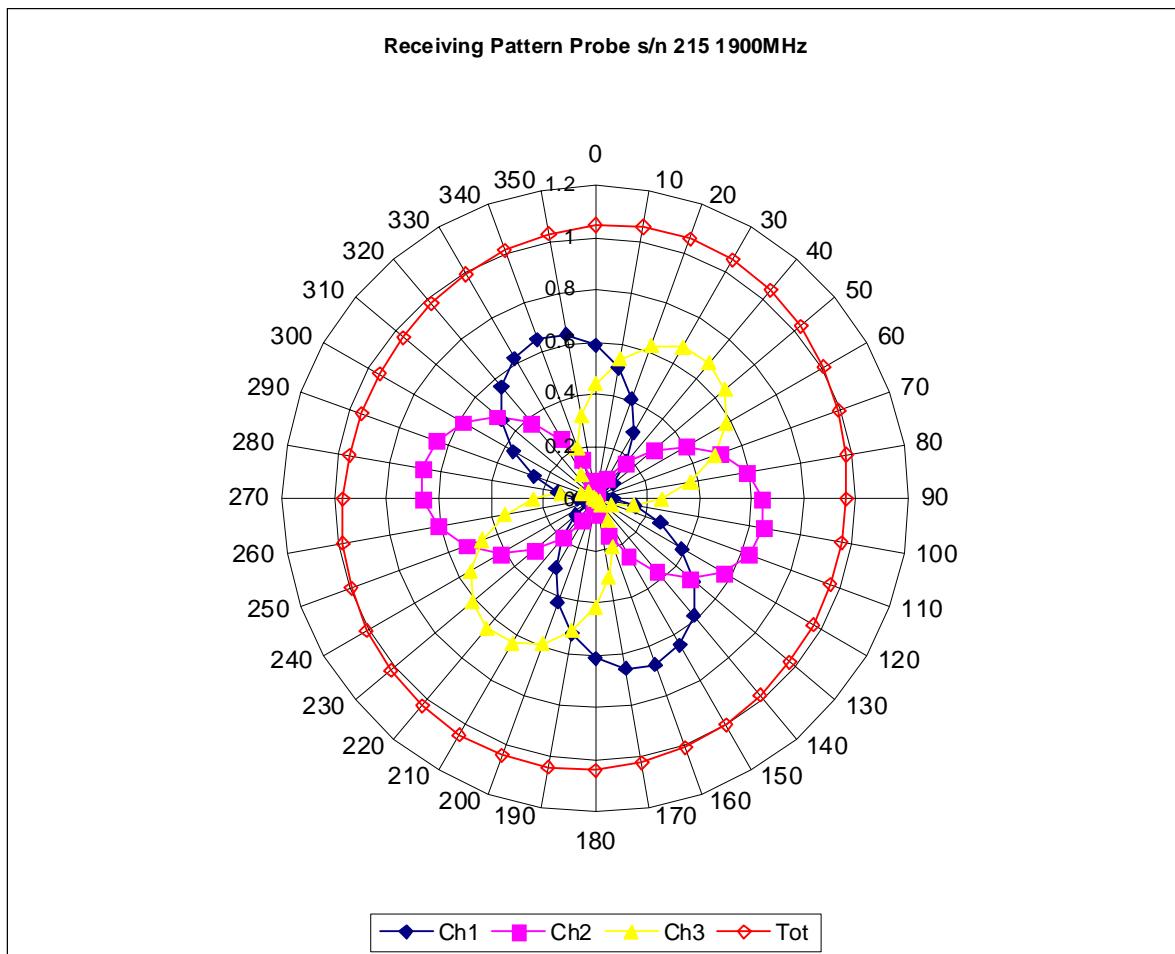

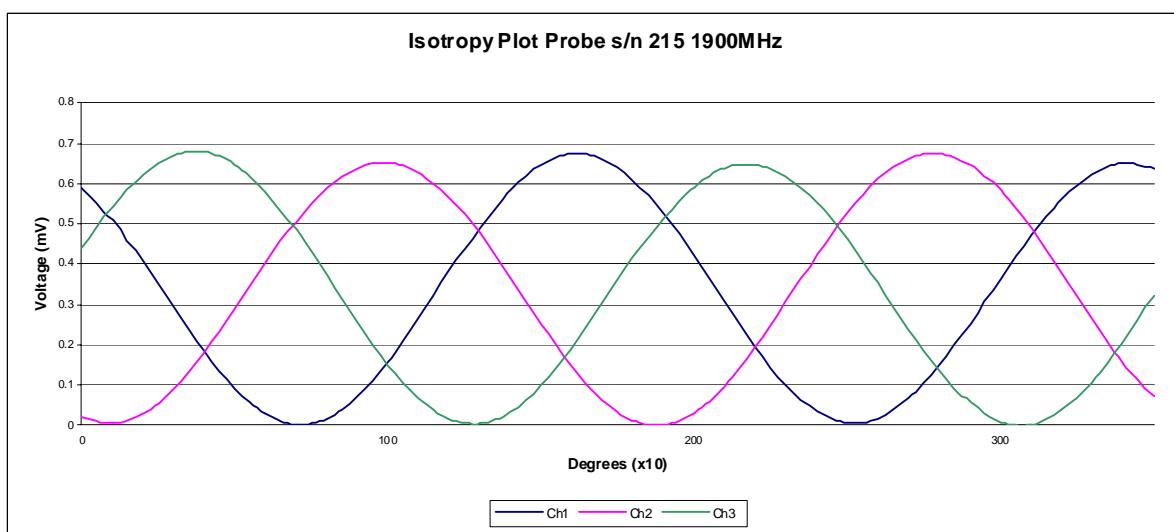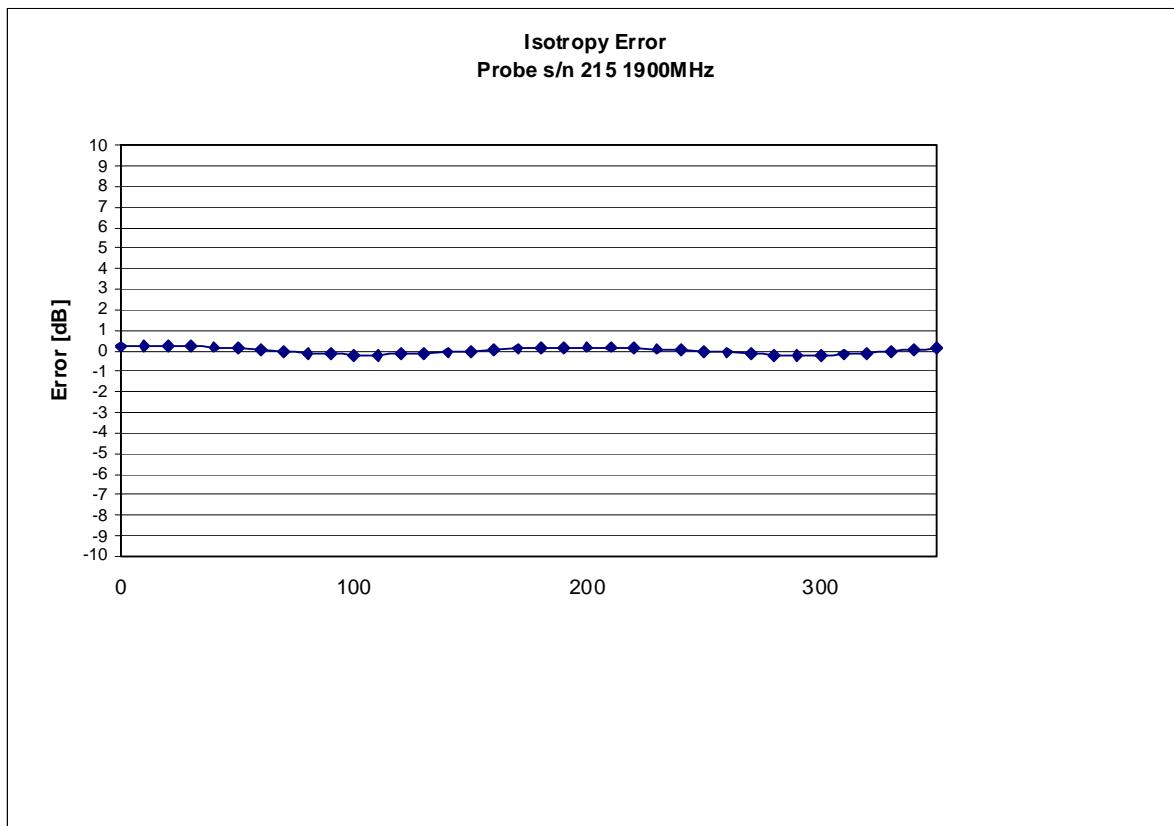**Isotropy Error 1900 MHz (Air)****Isotropicity Tissue:**


0.10 dB

## Dynamic Range

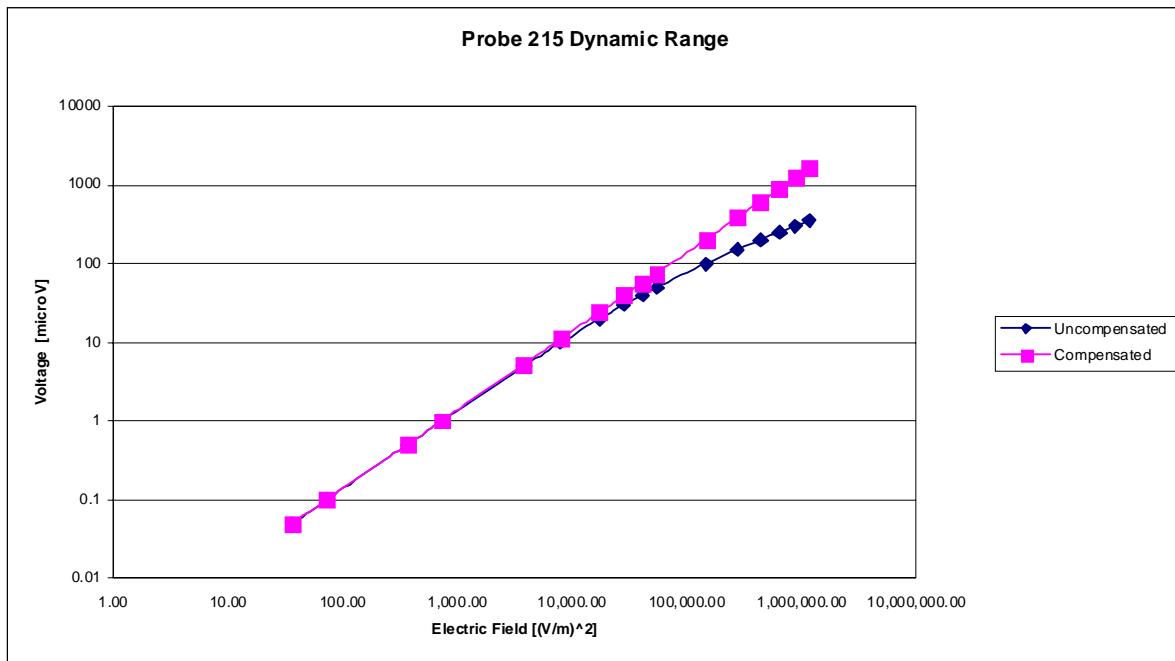

## Video Bandwidth

**Probe Frequency Characteristics**

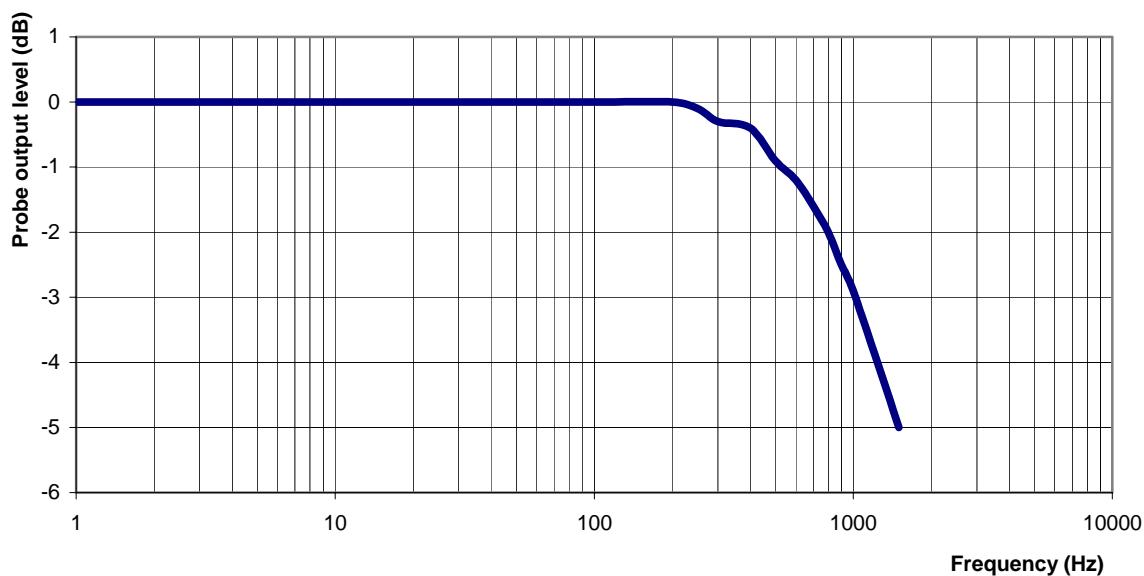

**Video Bandwidth at 500 Hz** 1 dB  
**Video Bandwidth at 1.02 KHz:** 3 dB

## **Conversion Factor Uncertainty Assessment Measured**

### **Sensitivity in Body Tissue**

**Frequency:** 1900 MHz

**Epsilon:** 54.2 (+/-5%) **Sigma:** 1.57 S/m (+/-5%)

**ConvF**

**Channel X:** 5.0 7%(K=2)

**Channel Y:** 5.0 7%(K=2)

**Channel Z:** 5.0 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

### **Boundary Effect:**

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

# NCL CALIBRATION LABORATORIES

Calibration File No.: CP-936

Client.: RFEL

## C E R T I F I C A T E   O F   C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 2600 MHz

BODY Calibration

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 215

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: RFEL-00150-CAL-5367

Calibrated: 3<sup>rd</sup> November 2008  
Released on: 3<sup>rd</sup> November 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary  
This calibration has been conducted in line with the SCC ISO-IEC 17025 Scope of Accreditation

Accredited Laboratory Number 48

Released By: \_\_\_\_\_

**NCL** CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## **NCL Calibration Laboratories**

---

Division of APREL Laboratories.

### **Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 215.

### **References**


SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
IEEE 1309 "IEEE Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9 KHz to 40 GHz" 2005  
SSI-TP-011 Tissue Calibration Procedure  
IEC 62209 "Human exposure to radio frequency fields from handheld and body-mounted wireless communication devices –Human models, instrumentation and procedures Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for handheld devices used in close proximity of the ear (frequency range of 200MHz to 3GHz)"

### **Conditions**

Probe 215 was a re-calibration.


**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

**We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.**



---

Stuart Nicol



---

Jesse Hones

## Calibration Results Summary

<b>Probe Type:</b>	E-Field Probe E-020
<b>Serial Number:</b>	215
<b>Frequency:</b>	2600 MHz
<b>Sensor Offset:</b>	1.56 mm
<b>Sensor Length:</b>	2.5 mm
<b>Tip Enclosure:</b>	Ertalyte*
<b>Tip Diameter:</b>	<5 mm
<b>Tip Length:</b>	60 mm
<b>Total Length:</b>	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

### Sensitivity in Air

<b>Channel X:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Y:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Z:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Diode Compression Point:</b>	95 mV

## **Sensitivity in Body Tissue Measured**

**Frequency:** 2600 MHz

**Epsilon:** 51.53 (+/-5%) **Sigma:** 2.24 S/m (+/-5%)

### **ConvF**

**Channel X:** 5.0

**Channel Y:** 5.0

**Channel Z:** 5.0

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


### **Boundary Effect:**



Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

### **Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


## Receiving Pattern 2600 MHz (Air)

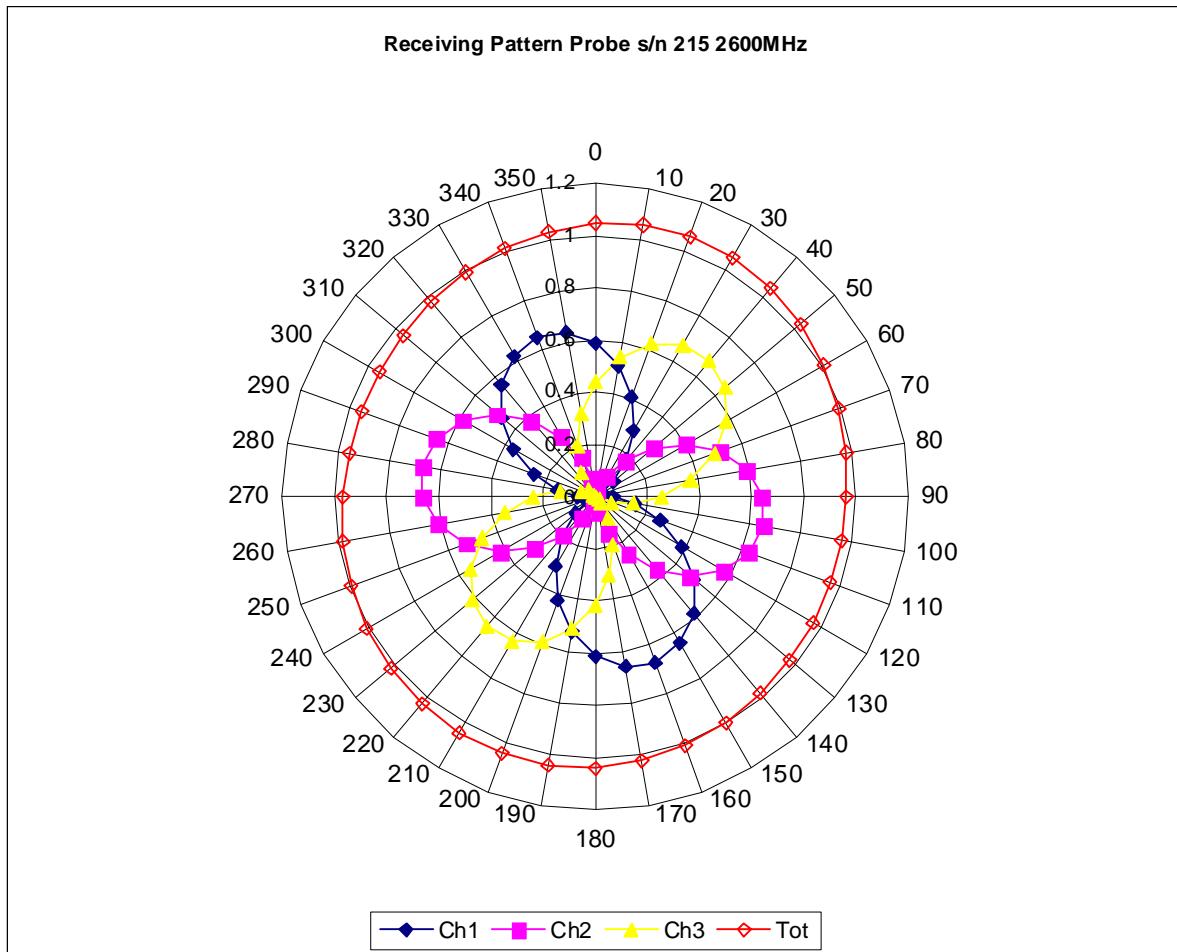

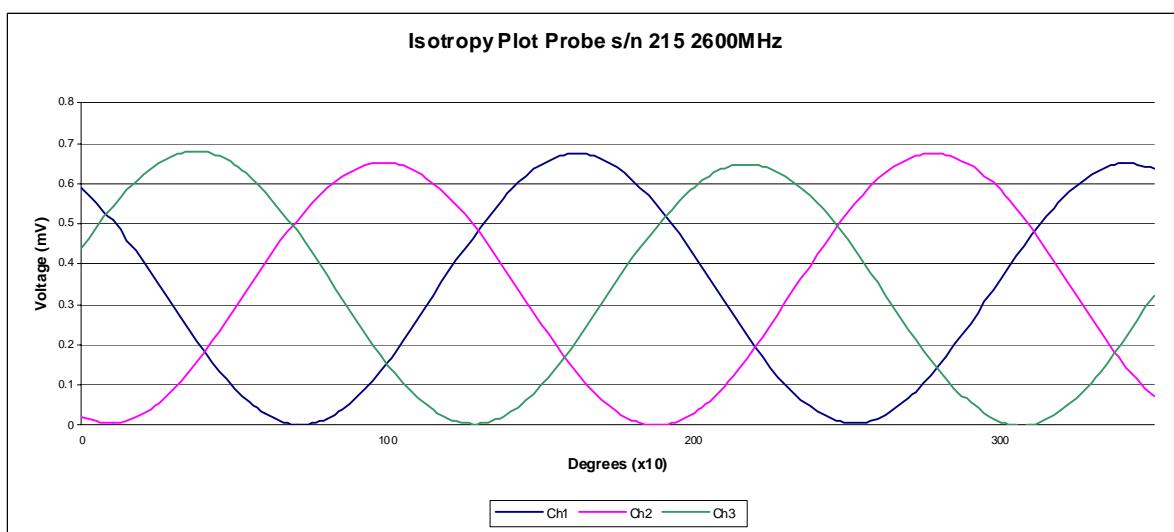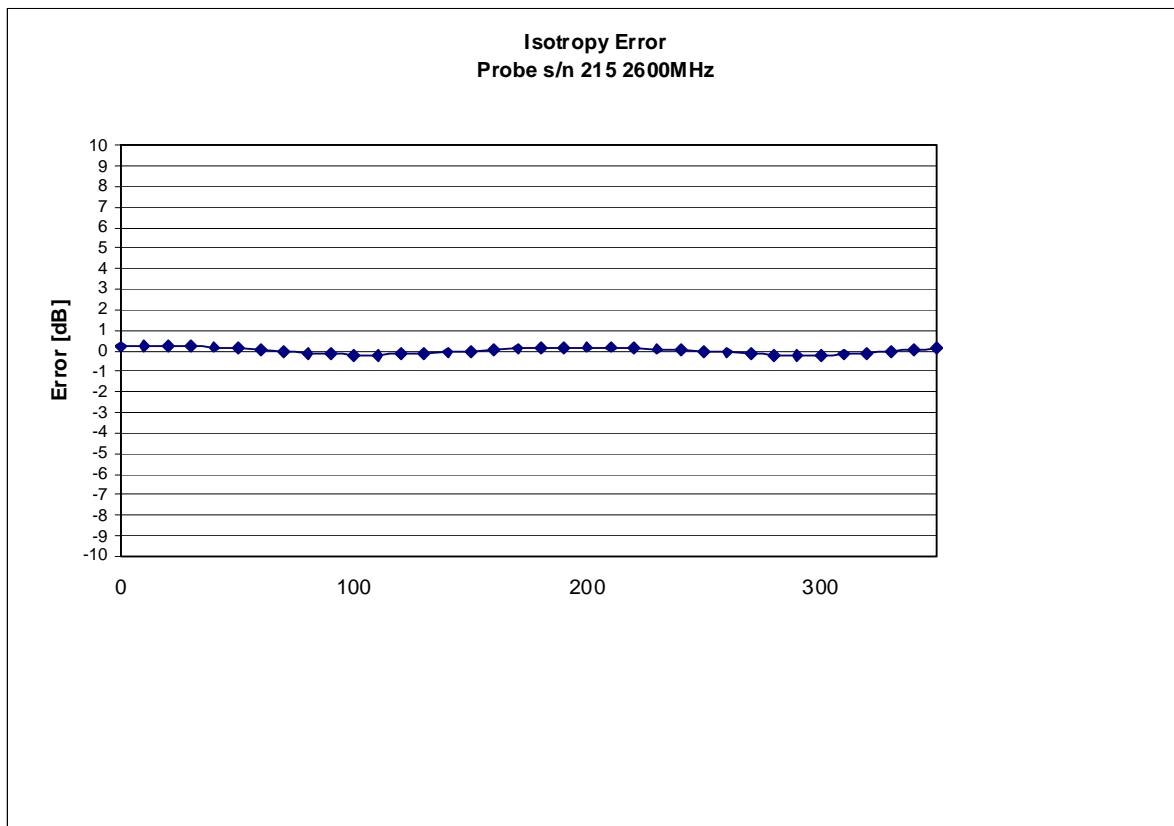**Isotropy Error 2600 MHz (Air)****Isotropicity Tissue:**


0.10 dB

## Dynamic Range

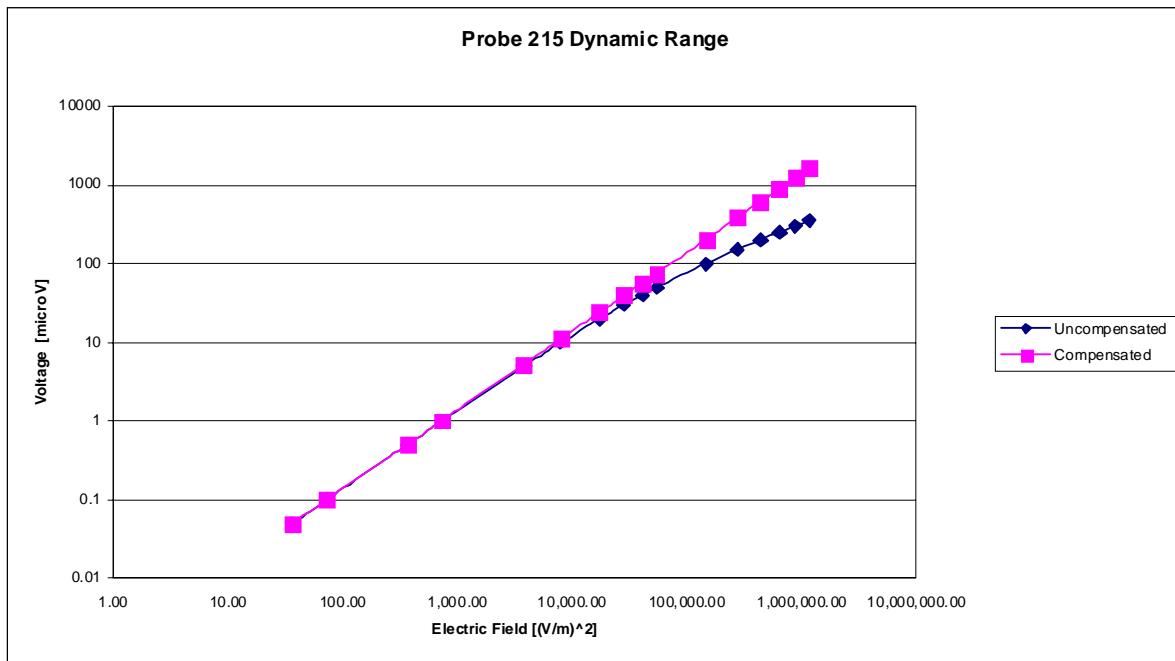

## Video Bandwidth

**Probe Frequency Characteristics**

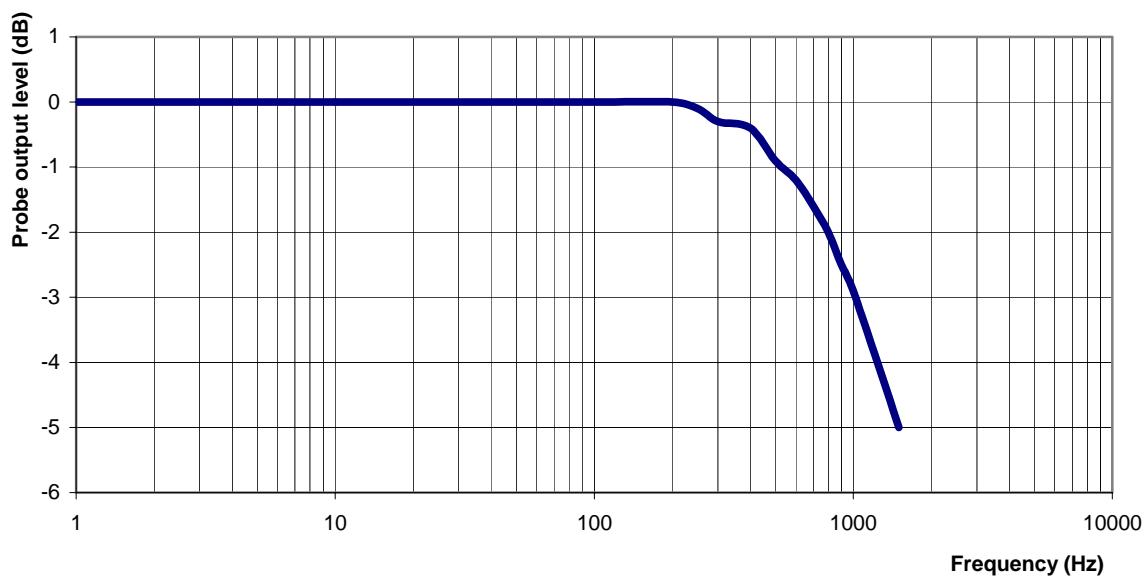

**Video Bandwidth at 500 Hz** 1 dB  
**Video Bandwidth at 1.02 KHz:** 3 dB

## **Conversion Factor Uncertainty Assessment Measured**

### **Sensitivity in Body Tissue**

**Frequency:** 2600 MHz

**Epsilon:** 51.53 (+/-5%) **Sigma:** 2.24 S/m (+/-5%)

**ConvF**

**Channel X:** 5.0 7%(K=2)

**Channel Y:** 5.0 7%(K=2)

**Channel Z:** 5.0 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

### **Boundary Effect:**

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

## Appendix E – Dipole Calibration Data Sheets

## RF Exposure Lab, LLC

Calibration File No: CAL.20080203

### C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated at RF Exposure Lab, LLC by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

#### Validation Dipole

Manufacturer: APREL Laboratories

Part Number: ALS-D-835-S-2

Frequency: 835 MHz

Serial No: RFE-274

Manufactured: 20 February 2004

Calibrated: 22 February 2008

Calibrated By: Signature on File  
Jay Moulton – Technical Manager

Approved By: Signature on File  
Tamara Moulton – Quality Manager

Measurement Uncertainty:

Repeatability:	2.3%
Tissue Uncertainty:	3.2%
Network Analyzer:	2.5%



**RF EXPOSURE LAB, LLC**

2867 Progress Place, Suite 4D  
Escondido, CA 92029

Tel: (760) 737-3131  
FAX: (760) 737-9131

## Calibration Results Summary

The following results relate to the Calibrated Dipole and should be used as a quick reference for the user.

### Mechanical Dimensions

**Length:** 161.8 mm  
**Height:** 91.1 mm

### Electrical Specifications

#### Head

**SWR:** 1.1182 U  
**Return Loss:** -27.508 dB  
**Impedance:** 49.648  $\Omega$

### System Validation Results

Frequency	1 Gram	10 Gram
835 MHz	9.500	6.000

#### Body

**SWR:** 1.1533 U  
**Return Loss:** -23.596 dB  
**Impedance:** 51.395  $\Omega$

### System Validation Results

Frequency	1 Gram	10 Gram
835 MHz	9.750	6.240

## Head Measurement Conditions

The measurements were performed in the Uni-Phantom filled with head simulating liquid of the following electrical parameters at 835 MHz:

Relative Dielectricity	41.48	± 5%
Conductivity	0.92 mho/m	± 5%

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 6.0 at 835 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW ± 3%. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.


Ambient Temperature of the Laboratory:	24 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	40%

## SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm<sup>3</sup> (1 g) of tissue: 9.500 mW/g ± 19.0% (k=2)<sup>1</sup>

Averaged over 10 cm<sup>3</sup> (10 g) of tissue: 6.000 mW/g ± 18.5% (k=2)<sup>1</sup>

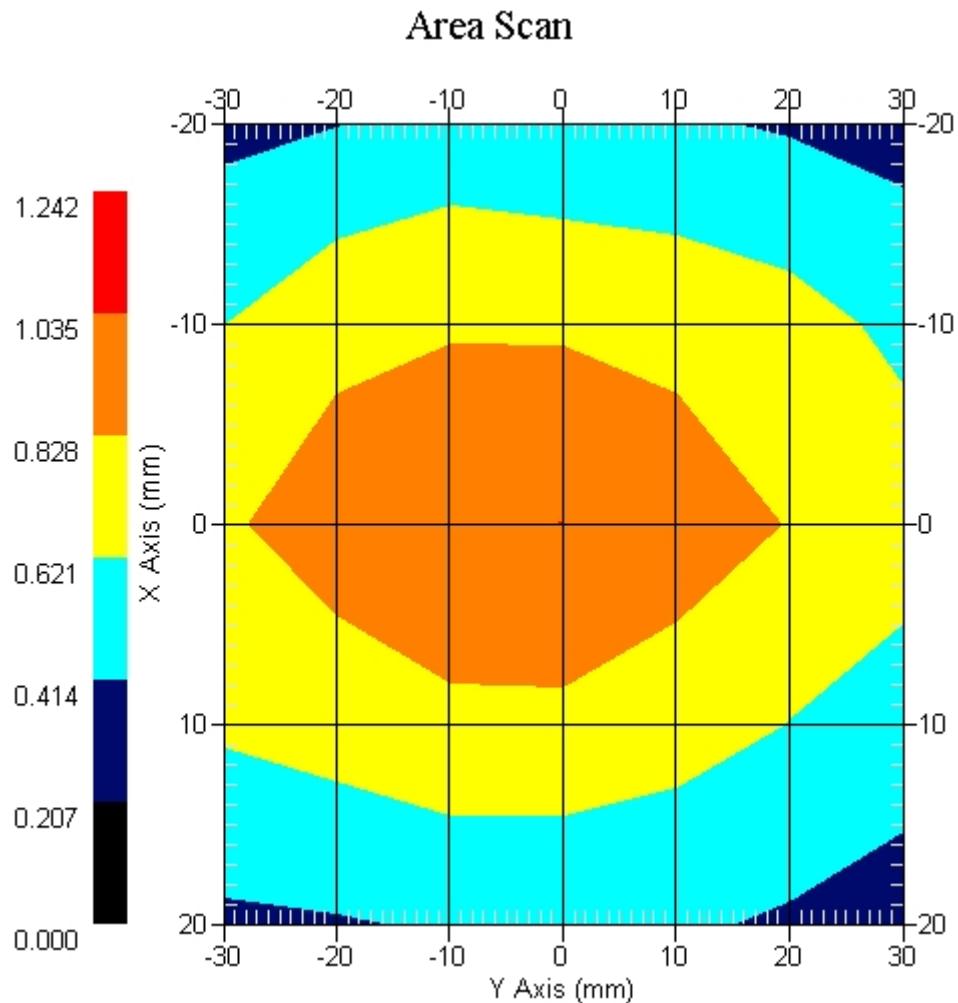

1 gram SAR value : 0.950 W/kg

10 gram SAR value : 0.600 W/kg

Area Scan Peak SAR : 1.037 W/kg

Zoom Scan Peak SAR : 1.541 W/kg

<sup>1</sup> validation uncertainty


## Dipole Impedance and Return Loss



The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.

Test	Result
S11 R/L	-27.508 dB
SWR	1.1182 U
Impedance	49.648 $\Omega$

The following graphs are the results as displayed on the Vector Network Analyzer.

### S11 Parameter Return Loss

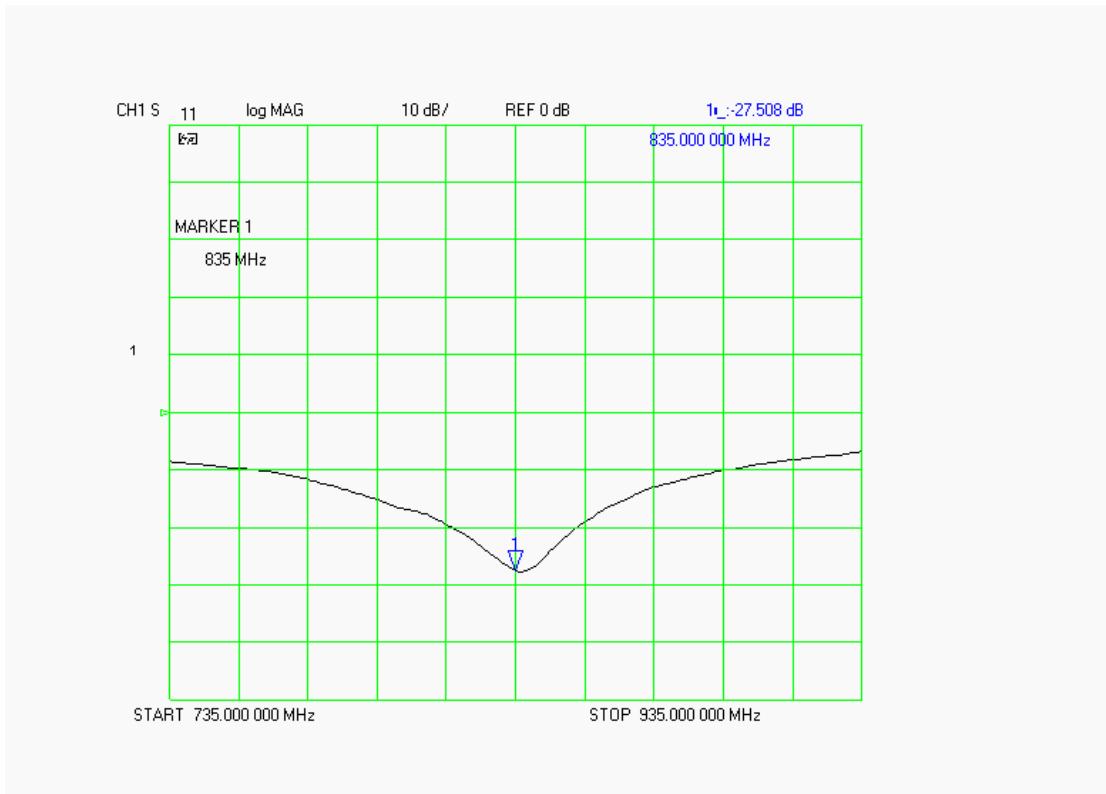

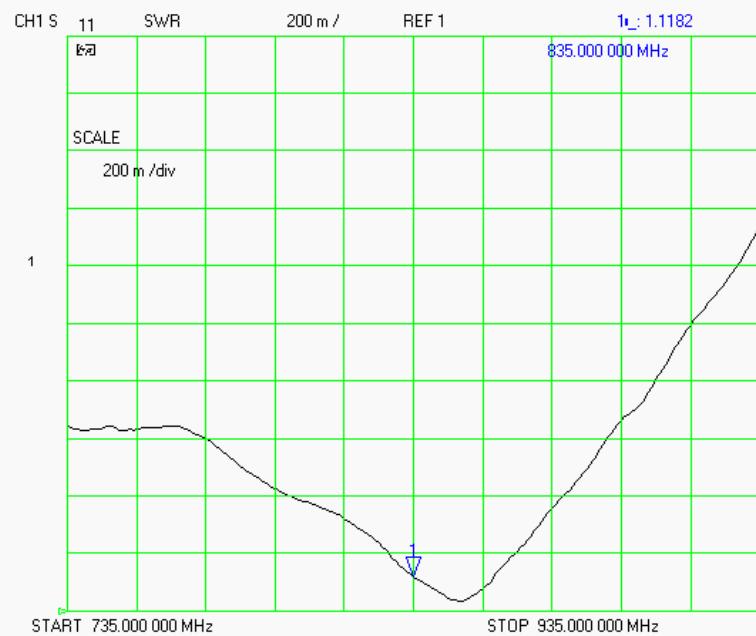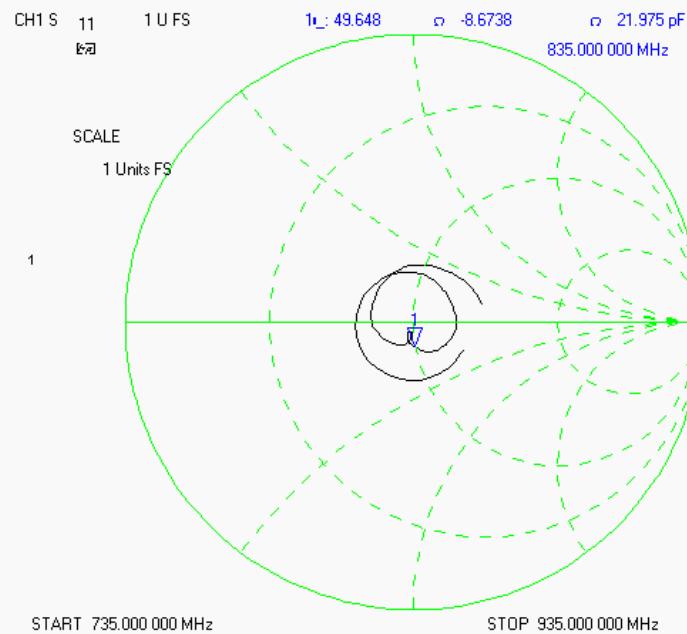**SWR**

**Smith Chart Dipole Impedance**


## Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 835 MHz:

Relative Dielectricity	55.20	± 5%
Conductivity	0.96 mho/m	± 5%

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 6.1 at 835 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW ± 3%. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

Ambient Temperature of the Laboratory:	24 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	40%


## SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm<sup>3</sup> (1 g) of tissue: 9.750 mW/g ± 19.1% (k=2)<sup>1</sup>

Averaged over 10 cm<sup>3</sup> (10 g) of tissue: 6.240 mW/g ± 18.6% (k=2)<sup>1</sup>

**Area Scan**

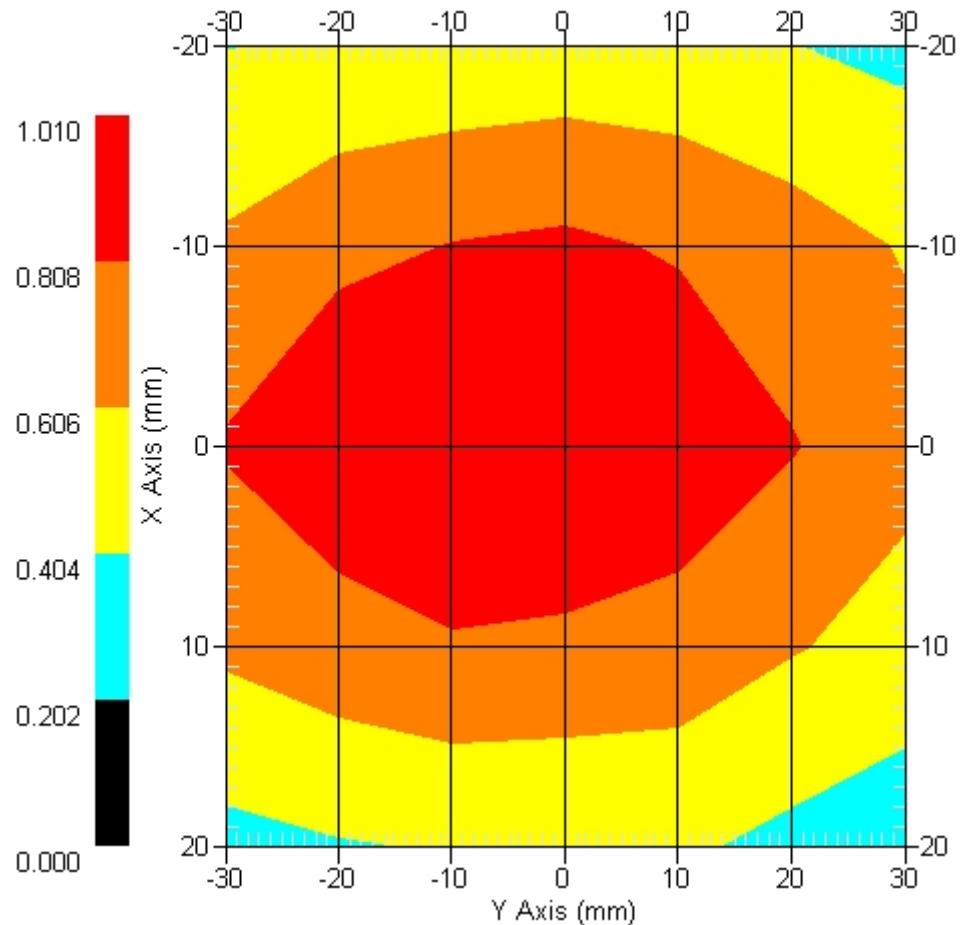

1 gram SAR value : 0.975 W/kg

10 gram SAR value : 0.624 W/kg

Area Scan Peak SAR : 1.009 W/kg

Zoom Scan Peak SAR : 1.571 W/kg

<sup>1</sup> validation uncertainty


## Dipole Impedance and Return Loss



The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.

Test	Result
S11 R/L	-23.596 dB
SWR	1.1533 U
Impedance	51.395 $\Omega$

The following graphs are the results as displayed on the Vector Network Analyzer.

### S11 Parameter Return Loss

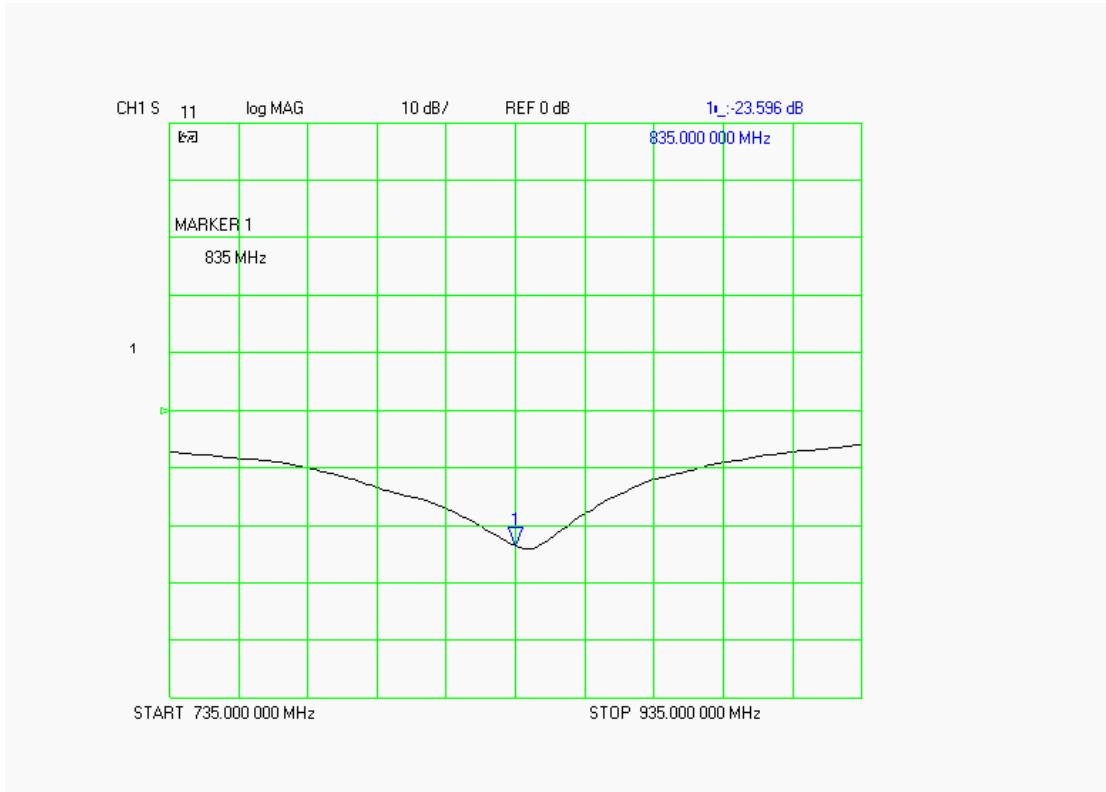

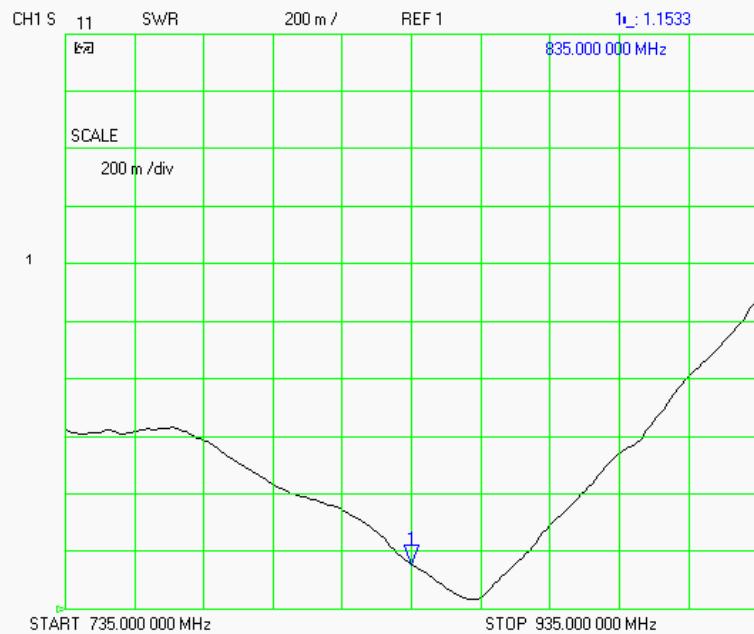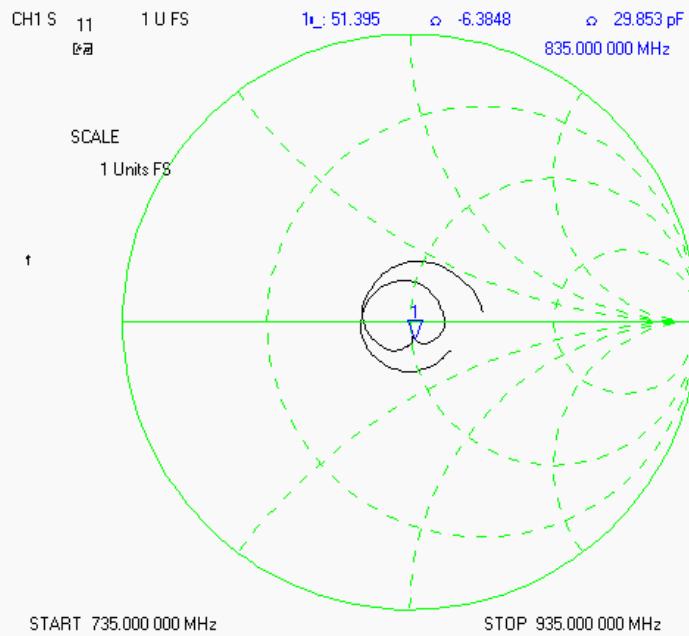**SWR**

**Smith Chart Dipole Impedance**


## Test Equipment List

The test equipment used during Dipole Calibration, manufacturer, model number and, current calibration status are listed and located on the RF Exposure Lab, LLC system computer C:\Test Equipment\Calibration Equipment\Instrument List February 2008.

## RF Exposure Lab, LLC

Calibration File No: CAL.20080202

### C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated at RF Exposure Lab, LLC by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

#### Validation Dipole

Manufacturer: APREL Laboratories

Part Number: ALS-D-1900-S-2

Frequency: 1.9 GHz

Serial No: RFE-277

Manufactured: 20 February 2004

Calibrated: 21 February 2008

Calibrated By: Signature on File  
Jay Moulton – Technical Manager

Approved By: Signature on File  
Tamara Moulton – Quality Manager

Measurement Uncertainty:

Repeatability:	2.3%
Tissue Uncertainty:	3.2%
Network Analyzer:	2.5%



**RF EXPOSURE LAB, LLC**

2867 Progress Place, Suite 4D  
Escondido, CA 92029

Tel: (760) 737-3131  
FAX: (760) 737-9131

## Calibration Results Summary

The following results relate to the Calibrated Dipole and should be used as a quick reference for the user.

### Mechanical Dimensions

**Length:** 68.0 mm  
**Height:** 37.5 mm

### Electrical Specifications

#### Head

**SWR:** 1.0793 U  
**Return Loss:** -38.514 dB  
**Impedance:** 49.063 Ω

### System Validation Results

Frequency	1 Gram	10 Gram
1.9 GHz	39.380	20.270

#### Body

**SWR:** 1.1006 U  
**Return Loss:** -41.682 dB  
**Impedance:** 53.580 Ω

### System Validation Results

Frequency	1 Gram	10 Gram
1.9 GHz	40.990	21.090

## Head Measurement Conditions

The measurements were performed in the Uni-Phantom filled with head simulating liquid of the following electrical parameters at 1900 MHz:

Relative Dielectricity	39.97	± 5%
Conductivity	1.41 mho/m	± 5%

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 4.65 at 1900 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW ± 3%. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

Ambient Temperature of the Laboratory:	23 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	40%


## SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm<sup>3</sup> (1 g) of tissue: 39.380 mW/g ± 19.2% (k=2)<sup>1</sup>

Averaged over 10 cm<sup>3</sup> (10 g) of tissue: 20.270 mW/g ± 18.8% (k=2)<sup>1</sup>

**Area Scan**

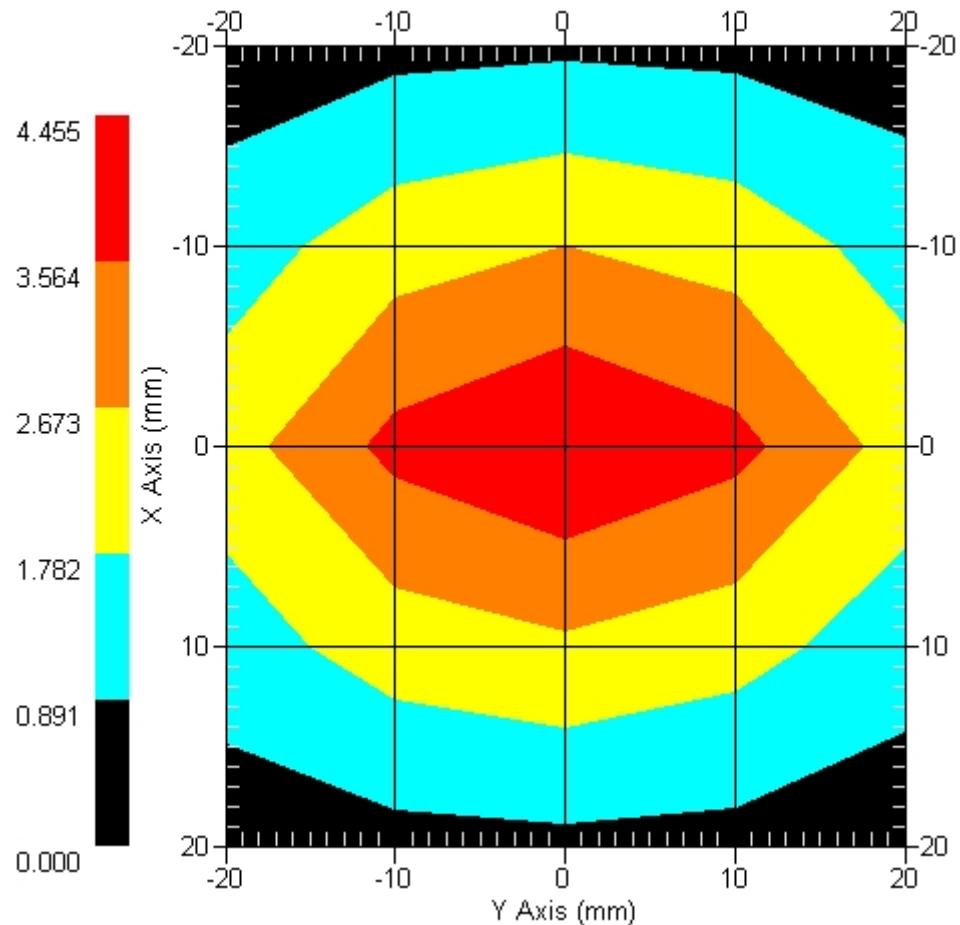

1 gram SAR value : 3.938 W/kg

10 gram SAR value : 2.027 W/kg

Area Scan Peak SAR : 4.455 W/kg

Zoom Scan Peak SAR : 7.246 W/kg

<sup>1</sup> validation uncertainty


## Dipole Impedance and Return Loss

The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.


Test	Result
S11 R/L	-38.514 dB
SWR	1.0793 U
Impedance	49.063 Ω

The following graphs are the results as displayed on the Vector Network Analyzer.


### S11 Parameter Return Loss

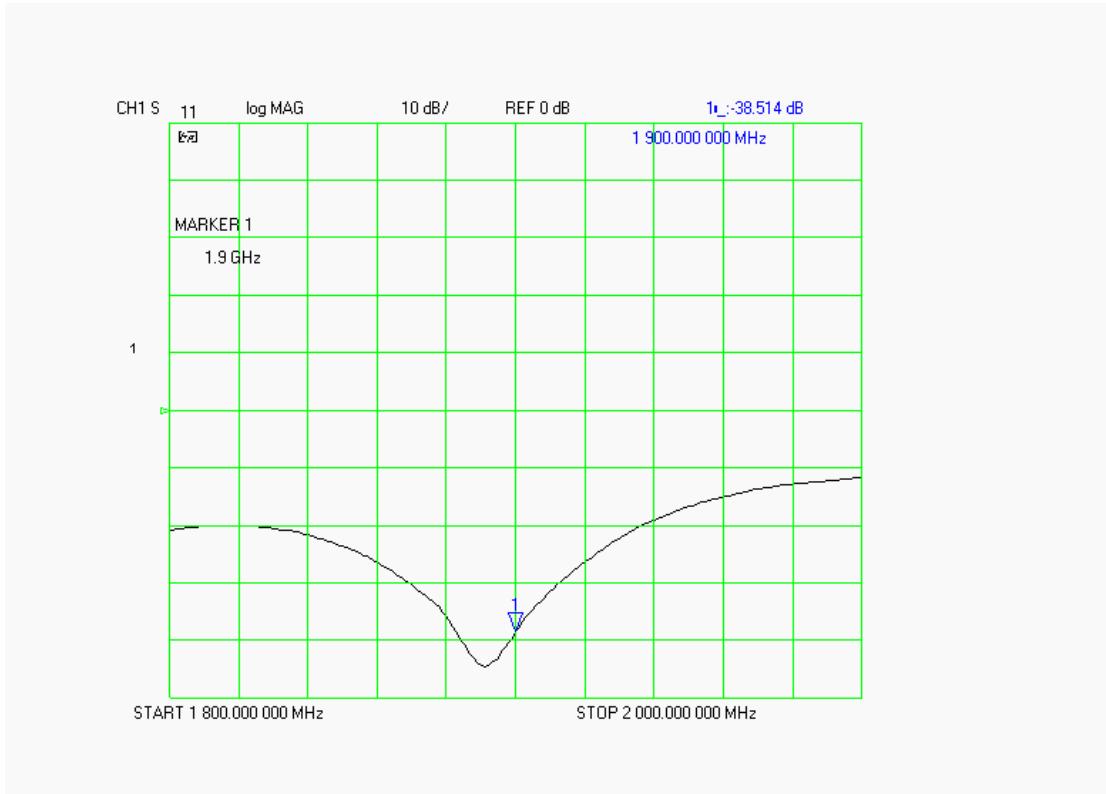

**SWR**

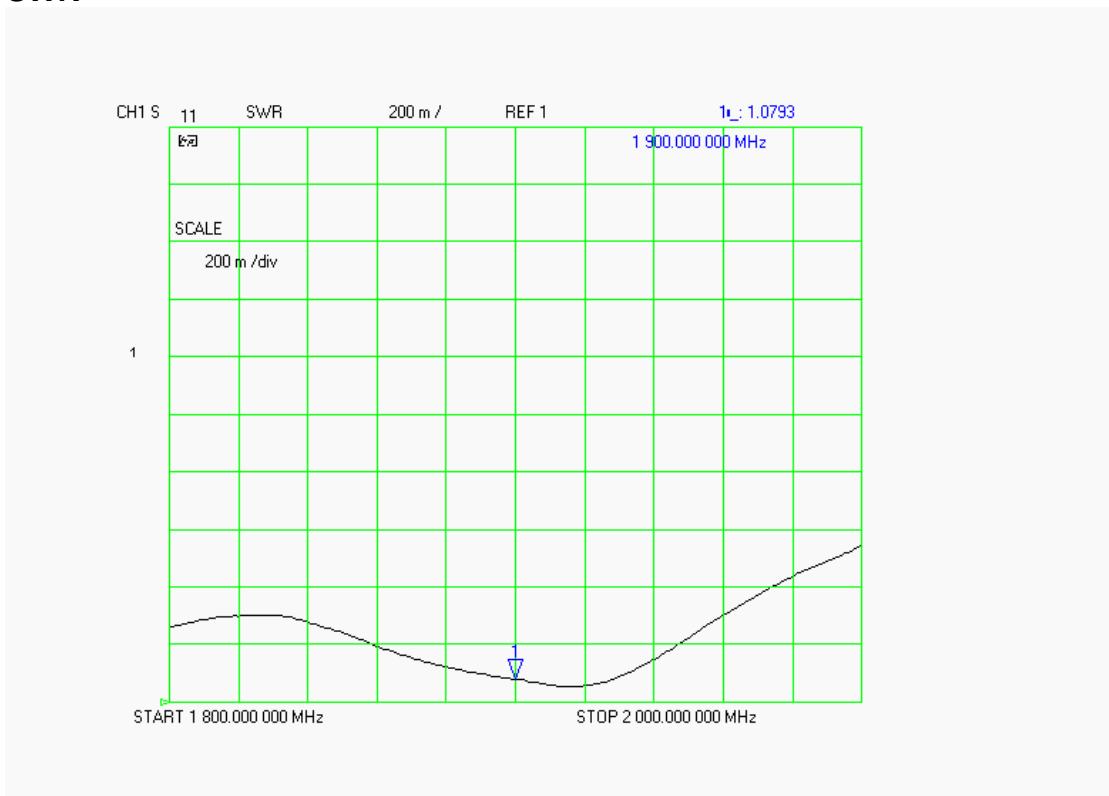

## Smith Chart Dipole Impedance

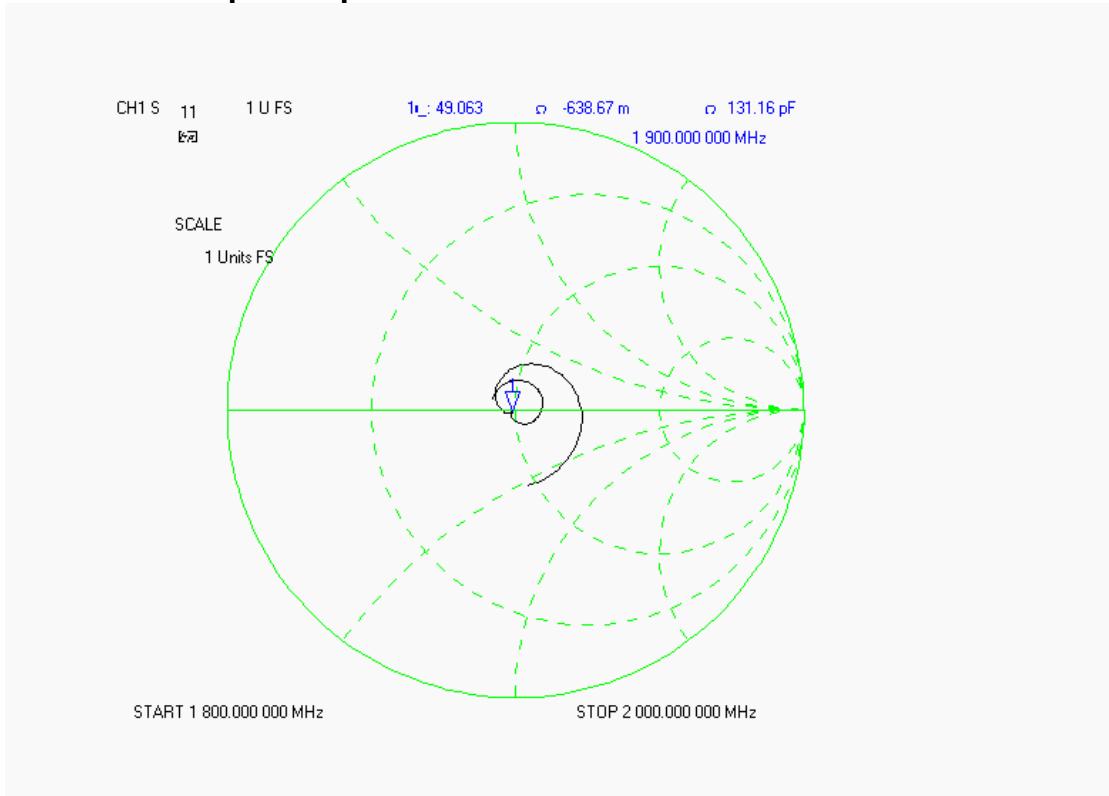

## Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 1900 MHz:

Relative Dielectricity	53.27	± 5%
Conductivity	1.50 mho/m	± 5%

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 4.85 at 1900 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW ± 3%. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

Ambient Temperature of the Laboratory:	23 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	40%


## SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm<sup>3</sup> (1 g) of tissue: 40.990 mW/g ± 18.9% (k=2)<sup>1</sup>

Averaged over 10 cm<sup>3</sup> (10 g) of tissue: 21.090 mW/g ± 18.5% (k=2)<sup>1</sup>

**Area Scan**

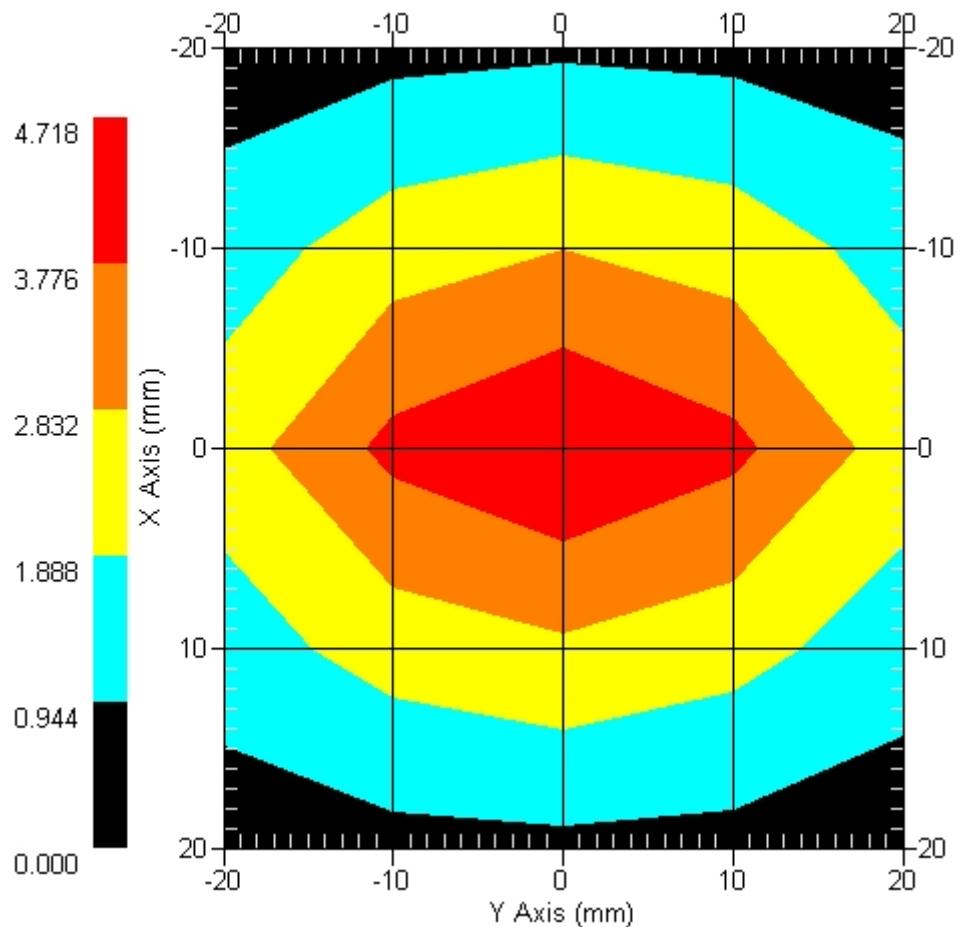

1 gram SAR value : 4.099 W/kg

10 gram SAR value : 2.109 W/kg

Area Scan Peak SAR : 4.718 W/kg

Zoom Scan Peak SAR : 7.606 W/kg

<sup>1</sup> validation uncertainty


## Dipole Impedance and Return Loss

The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.


Test	Result
S11 R/L	-41.682 dB
SWR	1.1006 U
Impedance	53.580 $\Omega$

The following graphs are the results as displayed on the Vector Network Analyzer.


### S11 Parameter Return Loss

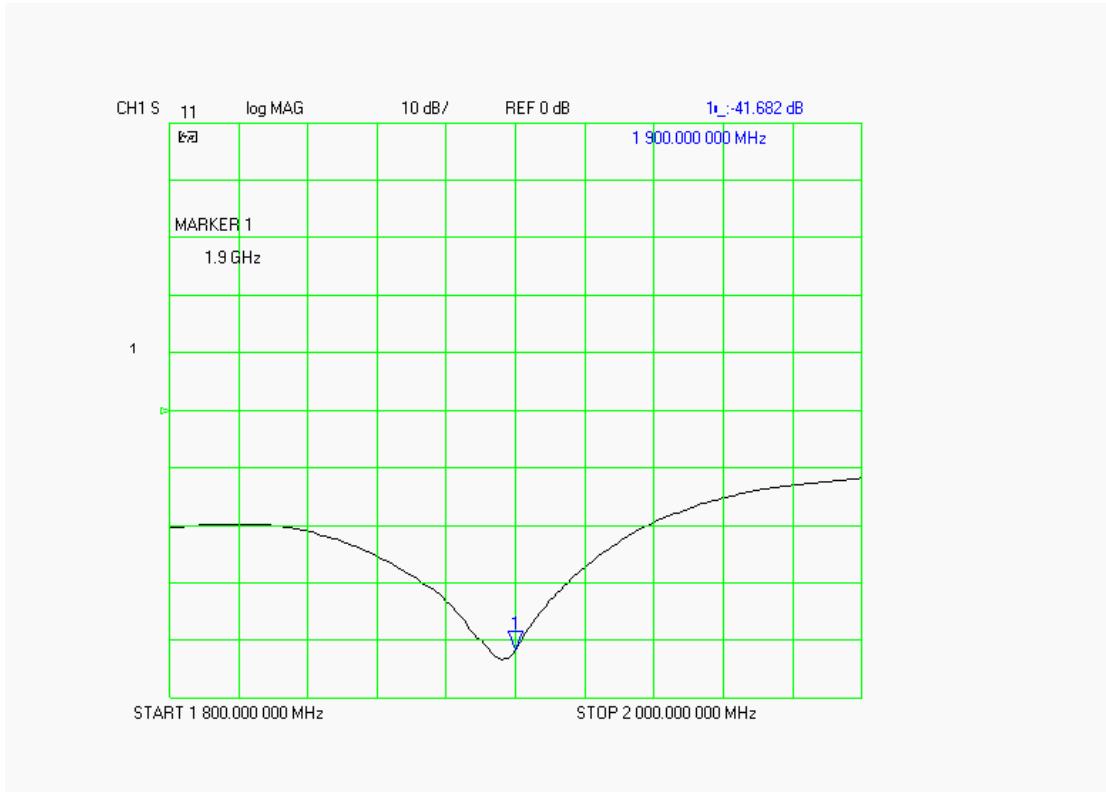

SWR

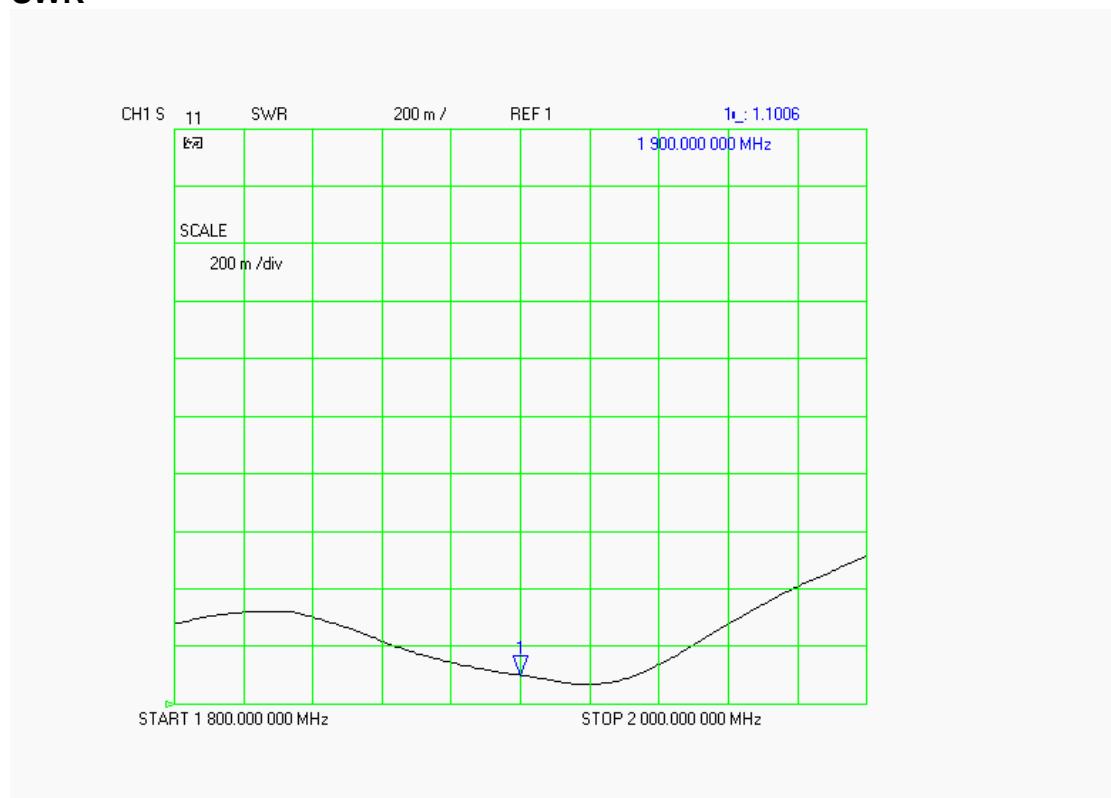

## Smith Chart Dipole Impedance

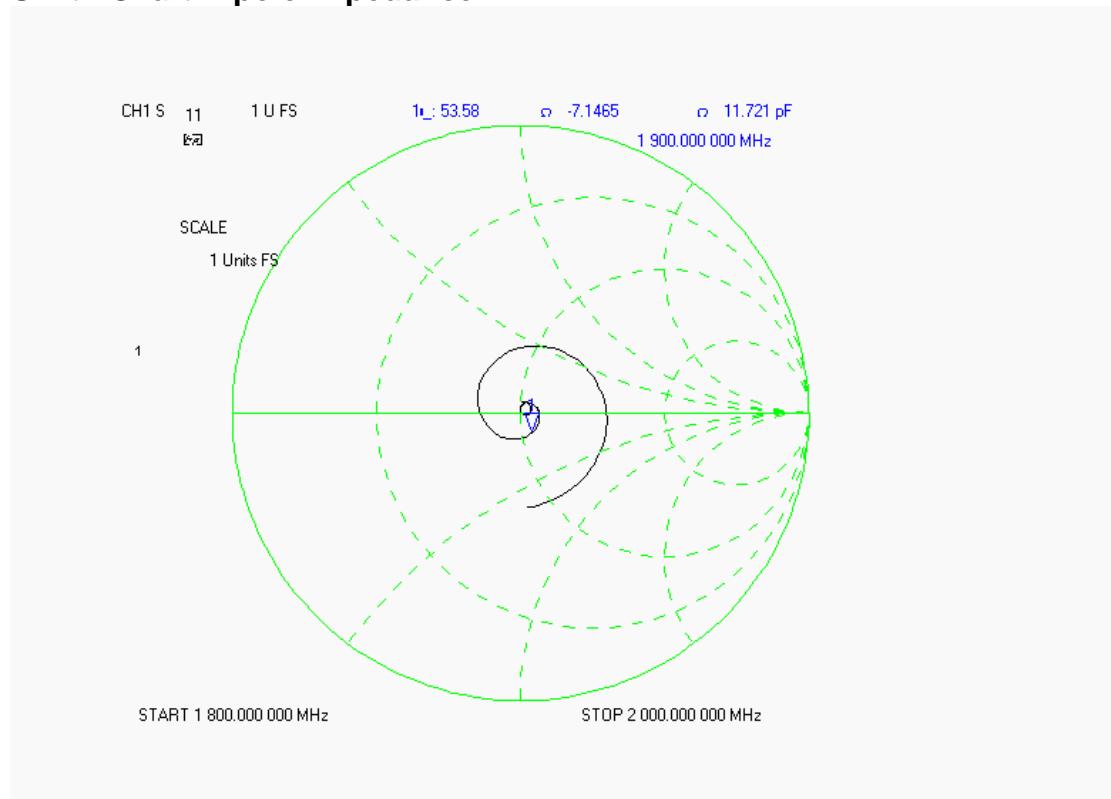

## Test Equipment List

The test equipment used during Dipole Calibration, manufacturer, model number and, current calibration status are listed and located on the RF Exposure Lab, LLC system computer C:\Test Equipment\Calibration Equipment\Instrument List February 2008.

## RF Exposure Lab, LLC

Calibration File No: CAL.20080204

### C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated at RF Exposure Lab, LLC by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

#### Validation Dipole

Manufacturer: APREL Laboratories

Part Number: RFE-D-2600-S-2

Frequency: 2.6 GHz

Serial No: RFE-121

Manufactured: 21 February 2008

Calibrated: 23 February 2008

Calibrated By:

Signature on File  
Jay Moulton – Technical Manager

Approved By:

Signature on File  
Tamara Moulton – Quality Manager

Measurement Uncertainty:

Repeatability:	2.3%
Tissue Uncertainty:	3.2%
Network Analyzer:	2.5%



**RF EXPOSURE LAB, LLC**

2867 Progress Place, Suite 4D  
Escondido, CA 92029

Tel: (760) 737-3131  
FAX: (760) 737-9131

## Calibration Results Summary

The following results relate to the Calibrated Dipole and should be used as a quick reference for the user.

### Mechanical Dimensions

**Length:** 49.5 mm  
**Height:** 30.0 mm

### Electrical Specifications

#### Head

**SWR:** 1.2642 U  
**Return Loss:** -27.293 dB  
**Impedance:** 47.576 Ω

### System Validation Results

Frequency	1 Gram	10 Gram
2.60 GHz	53.240	24.140

#### Body

**SWR:** 1.2697 U  
**Return Loss:** -28.239 dB  
**Impedance:** 48.523 Ω

### System Validation Results

Frequency	1 Gram	10 Gram
2.60 GHz	54.260	24.590

## Head Measurement Conditions

The measurements were performed in the Uni-Phantom filled with head simulating liquid of the following electrical parameters at 2600 MHz:

Relative Dielectricity	39.04	± 5%
Conductivity	1.97 mho/m	± 5%

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 3.37 at 2600 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW ± 3%. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

Ambient Temperature of the Laboratory:	24 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	41%


## SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm<sup>3</sup> (1 g) of tissue: 53.240 mW/g ± 19.7% (k=2)<sup>1</sup>

Averaged over 10 cm<sup>3</sup> (10 g) of tissue: 24.140 mW/g ± 19.4% (k=2)<sup>1</sup>

**Area Scan**

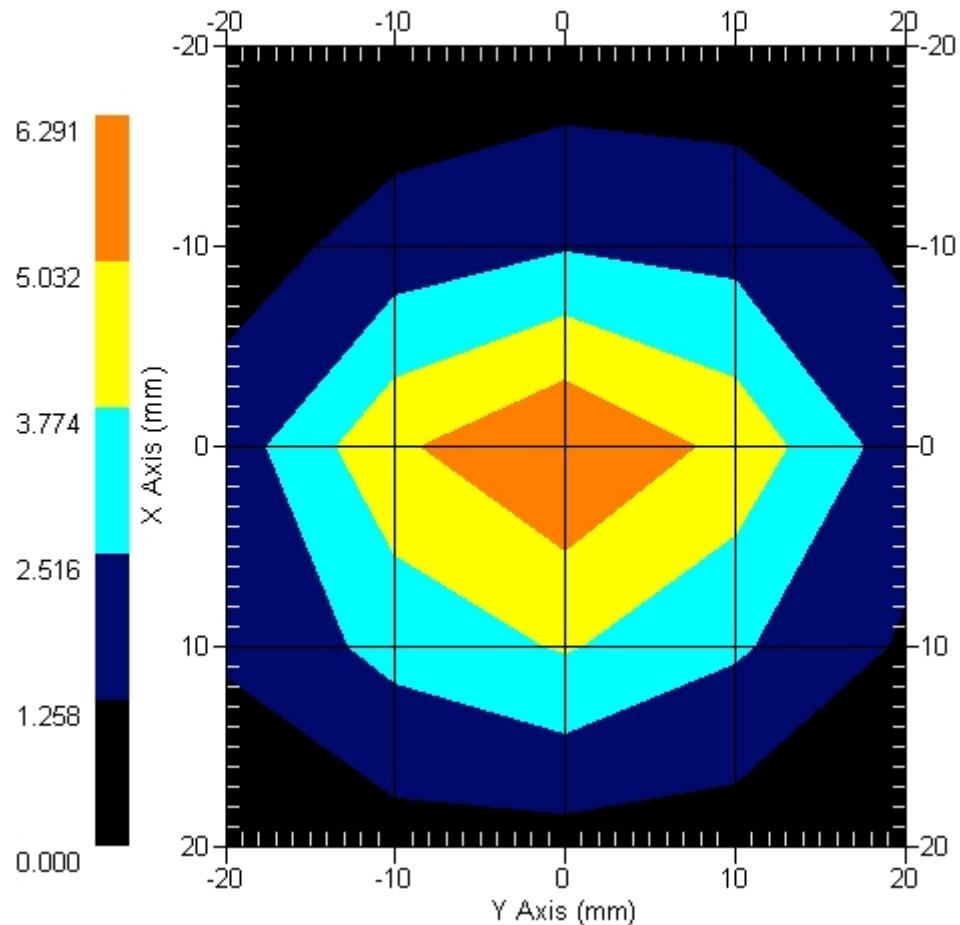

1 gram SAR value : 5.324 W/kg

10 gram SAR value : 2.414 W/kg

Area Scan Peak SAR : 6.291 W/kg

Zoom Scan Peak SAR : 11.090 W/kg

<sup>1</sup> validation uncertainty


## Dipole Impedance and Return Loss

The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.


Test	Result
S11 R/L	-27.293 dB
SWR	1.2642 U
Impedance	47.576 Ω

The following graphs are the results as displayed on the Vector Network Analyzer.


### S11 Parameter Return Loss

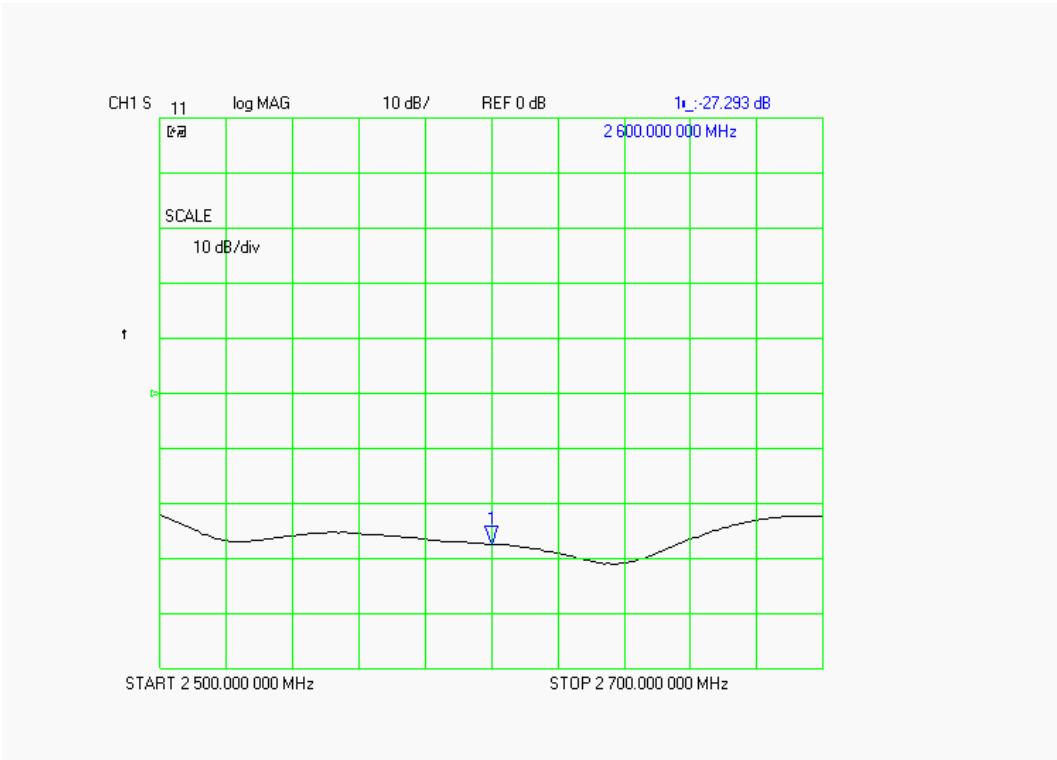

SWR

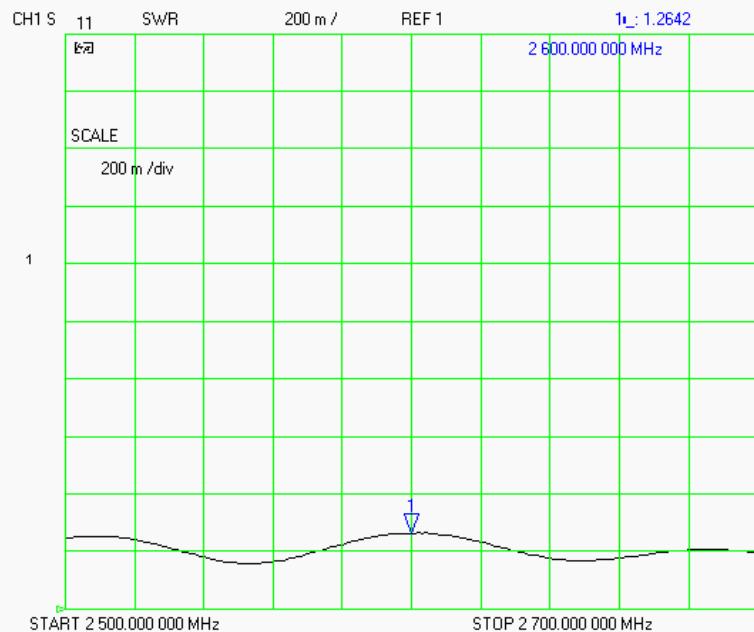

## Smith Chart Dipole Impedance

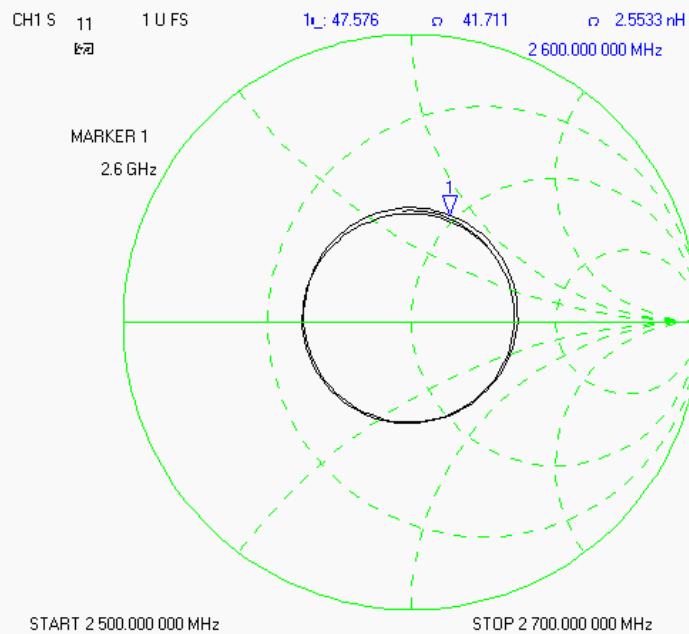

## Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 2600 MHz:

Relative Dielectricity	52.51	± 5%
Conductivity	2.14 mho/m	± 5%

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 3.6 at 2600 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW ± 3%. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

Ambient Temperature of the Laboratory:	24 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	41%


## SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm<sup>3</sup> (1 g) of tissue: 54.260 mW/g ± 18.8% (k=2)<sup>1</sup>

Averaged over 10 cm<sup>3</sup> (10 g) of tissue: 24.590 mW/g ± 18.4% (k=2)<sup>1</sup>

**Area Scan**

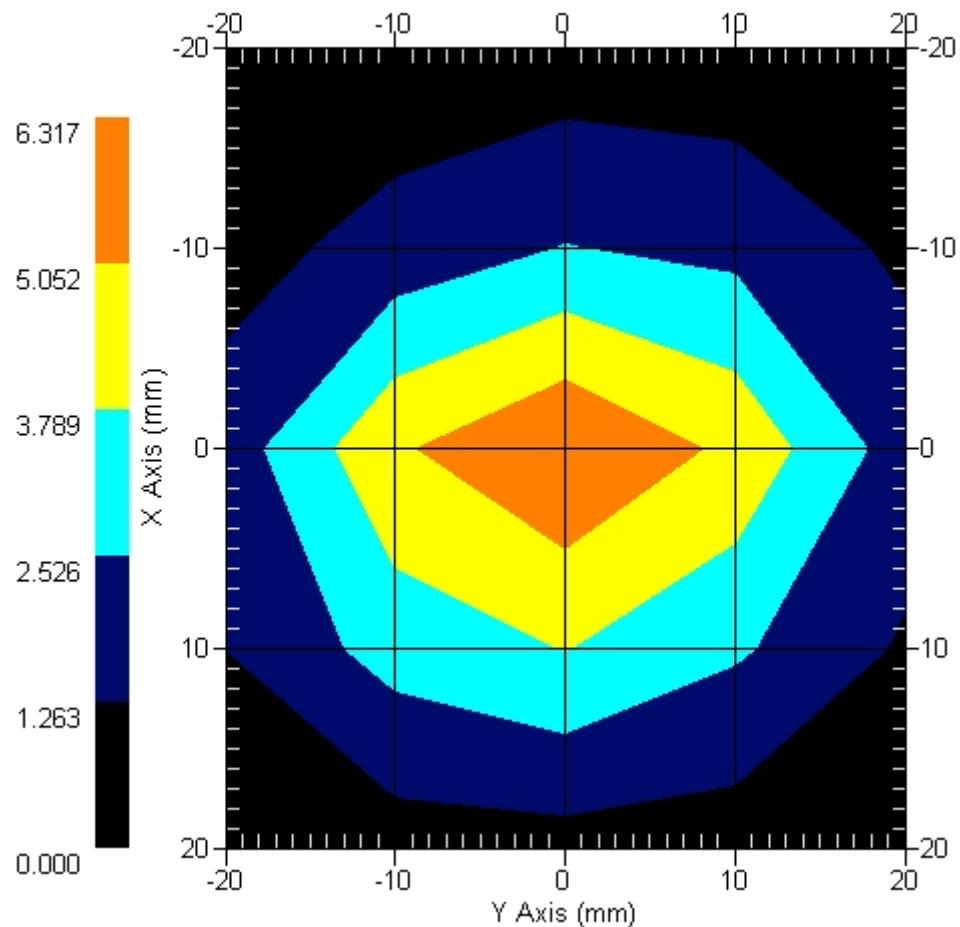

1 gram SAR value : 5.426 W/kg

10 gram SAR value : 2.459 W/kg

Area Scan Peak SAR : 6.317 W/kg

Zoom Scan Peak SAR : 11.590 W/kg

<sup>1</sup> validation uncertainty


## Dipole Impedance and Return Loss



The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.

Test	Result
S11 R/L	-28.239 dB
SWR	1.2697 U
Impedance	48.523 Ω

The following graphs are the results as displayed on the Vector Network Analyzer.

### S11 Parameter Return Loss

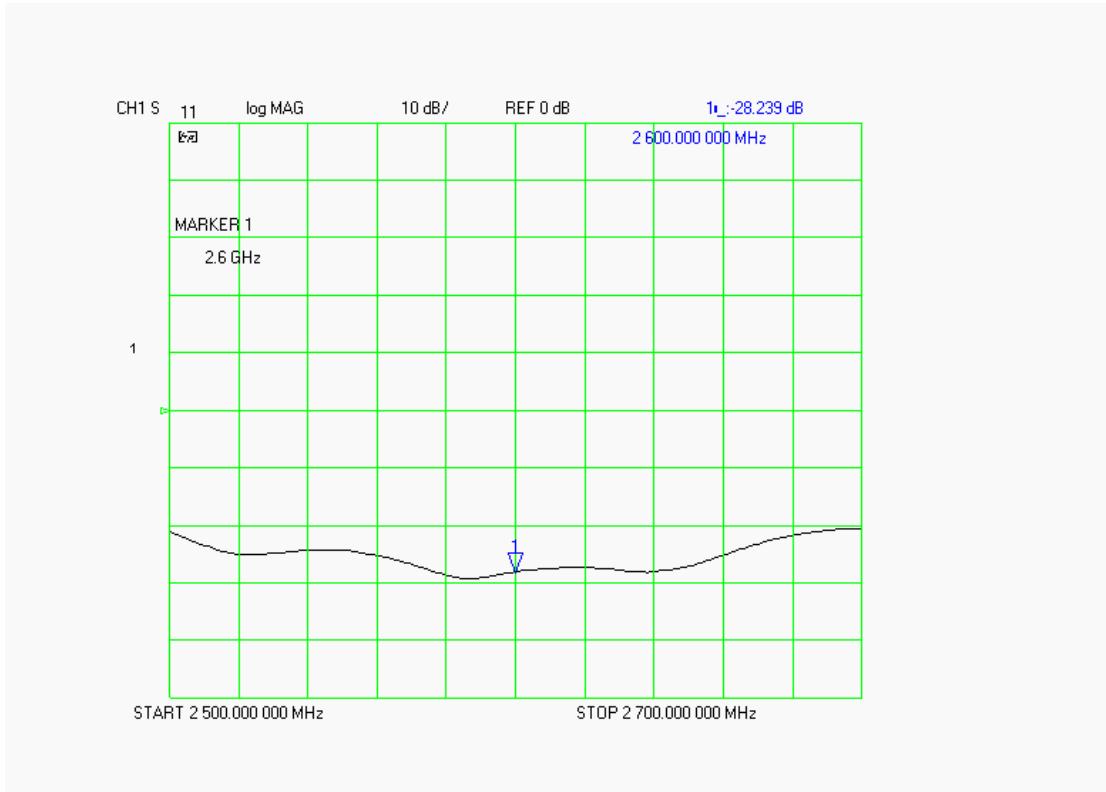

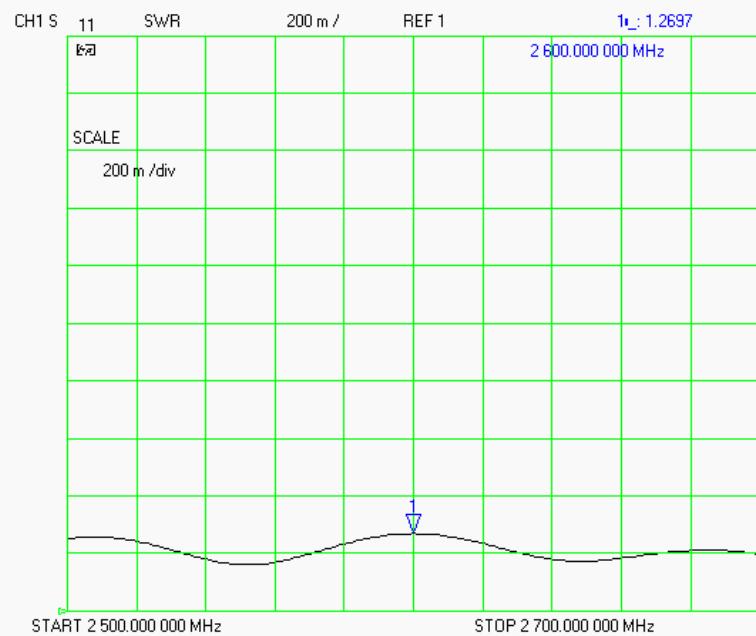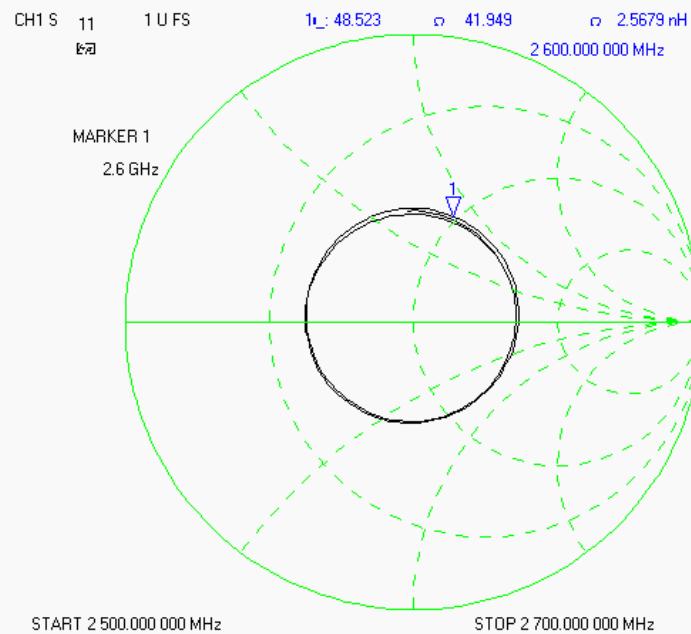**SWR**

**Smith Chart Dipole Impedance**


## Test Equipment List

The test equipment used during Dipole Calibration, manufacturer, model number and, current calibration status are listed and located on the RF Exposure Lab, LLC system computer C:\Test Equipment\Calibration Equipment\Instrument List February 2008.

## Appendix F – Phantom Calibration Data Sheets

## NCL CALIBRATION LABORATORIES

Calibration File No.: RFE-273

### CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to National Standards.

Thickness of the UniPhantom is 2 mm  $\pm$  10%  
Pinna thickness is 6 mm  $\pm$  10%

Resolution: 0.01 mm      Calibrated to: 0.0 mm  
Stability: OK      Accuracy: < 0.1 mm

Calibrated By:

Karen K.      Feb 17/04

### **NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161