



TEST REPORT

Product Name	150Mbps Mini Wireless N USB Adapter
Model	TL-WN723N
FCC ID	TE7WN723NV2
IC	8853A-WN723NV2
Client	TP-LINK TECHNOLOGIES CO., LTD.

TA Technology (Shanghai) Co., Ltd.

Report No.: RZA1112-2131SAR01R1

Page 2 of 64

GENERAL SUMMARY

Product	150Mbps Mini Wireless N USB Adapter	Model	TL-WN723N
Name		Woder	TE-WIN723IN
FCC ID	TE7WN723NV2	IC	8853A-WN723NV2
Report No.	RZA1112-2131SAR01R1		
Client	TP-LINK TECHNOLOGIES CO., LTD.		
Manufacturer	TP-LINK TECHNOLOGIES CO., LTD.		
Reference Standard(s)	 IFEE Std C95.1, 1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz. SUPPLEMENT C Edition 01-01 to OET BULLETIN 65 Edition 97-01 June 2001 including DA 02-1438, published June 2002: Evaluating Compliance with FCC Guidelines for Human Exposure to Radio frequency Electromagnetic Fields Additional Information for Evaluation Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radio frequency Emissions. RSS-102 Issue 4 March 2010: Radio Frequency (RF) Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands) KDB 248227 D01 SAR meas for 802 11 a b g v01r02: SAR Measurement Procedures for 802.11a/b/g Transmitters. KDB 447498 D02 SAR Procedures for Dongle Xmtr v02: SAR Measurement Procedures for USB Dongle Transmitters. 		
Conclusion	This portable wireless equipment has been measured in all cases requested by the relevant standards. Test results in Chapter 7 of this test report are below limits specified in the relevant standards. General Judgment: Pass (Stamp) Date of issue: February 29 th , 2012		
Comment	The test result only responds to the measured sample.		

¥þ itite Revised by Approved by Performed by_ SAR Engineer SAR Manager Director

TA Technology (Sh	anghai) Co.,	Ltd.
Test R	eport	

Page 3 of 64

TABLE OF CONTENT

1. General Information	5
1.1. Notes of the Test Report	5
1.2. Testing Laboratory	5
1.3. Applicant Information	6
1.4. Manufacturer Information	6
1.5. Information of EUT	
1.6. The Maximum SAR _{1g} Values	
1.7. Test Date	8
2. SAR Measurements System Configuration	9
2.1. SAR Measurement Set-up	9
2.2. DASY4 E-field Probe System	. 10
2.2.1. EX3DV4 Probe Specification	. 10
2.2.2. E-field Probe Calibration	. 11
2.3. Other Test Equipment	
2.3.1. Device Holder for Transmitters	
2.3.2. Phantom	
2.4. Scanning Procedure	
2.5. Data Storage and Evaluation	
2.5.1. Data Storage	
2.5.2. Data Evaluation by SEMCAD	. 14
3. Laboratory Environment	. 16
4. Tissue-equivalent Liquid	. 17
4.1. Tissue-equivalent Liquid Ingredients	
4.2. Tissue-equivalent Liquid Properties	
5. Systerm Check	. 18
5.1. Description of System Check	. 18
5.2. System Check Results	. 19
6. Operational Conditions during Test	. 20
6.1. General Description of Test Procedures	. 20
6.2. Test Positions	. 21
6.3. Picture of Host Product	. 22
7. Test Results	. 23
7.1. Conducted Power Results	. 23
7.2. SAR Test Results	. 24
7.2.1. WIFI (802.11b/g/n)	. 24
8. Measurement Uncertainty	. 25
9. Main Test Instruments	. 27
ANNEX A: Test Layout	. 28
ANNEX B: System Check Results	
ANNEX C: Graph Results	

Report No.: RZA1112-2131SAR01R1	Page 4 of 64
ANNEX D: Probe Calibration Certificate	
ANNEX E: D2450V2 Dipole Calibration Certificate	

ANNEX F: DAE4 Calibration Certificate	. 57
ANNEX G: The EUT Appearances and Test Configuration	. 62

1. General Information

1.1. Notes of the Test Report

TA Technology (Shanghai) Co., Ltd. guarantees the reliability of the data presented in this test report, which is the results of measurements and tests performed for the items under test on the date and under the conditions stated in this test report and is based on the knowledge and technical facilities available at TA Technology (Shanghai) Co., Ltd. at the time of execution of the test.

TA Technology (Shanghai) Co., Ltd. is liable to the client for the maintenance by its personnel of the confidentiality of all information related to the items under test and the results of the test. This report only refers to the item that has undergone the test.

This report standalone dose not constitute or imply by its own an approval of the product by the certification Bodies or competent Authorities. This report cannot be used partially or in full for publicity and/or promotional purposes without previous written approval of **TA Technology (Shanghai) Co., Ltd.** and the Accreditation Bodies, if it applies.

If the electrical report is inconsistent with the printed one, it should be subject to the latter.

1.2. Testing Laboratory

Company:	TA Technology (Shanghai) Co., Ltd.
Address:	No.145, Jintang Rd, Tangzhen Industry Park, Pudong Shanghai, China
City:	Shanghai
Post code:	201201
Country:	P. R. China
Contact:	Yang Weizhong
Telephone:	+86-021-50791141/2/3
Fax:	+86-021-50791141/2/3-8000
Website:	http://www.ta-shanghai.com
E-mail:	yangweizhong@ta-shanghai.com

Report No.: RZA1112-2131SAR01R1

1.3. Applicant Information

Company:	TP-LINK TECHNOLOGIES CO., LTD.	
Address:	Building 24 (floors 1,3,4,5) and 28 (floors1-4)	Central Science and Technology
	Park, Shennan Rd, Nanshan, Shenzhen, China	
City:	Shenzhen	
Postal Code:	518057	
Country:	P.R.China	
Contact:	LiQian	
Telephone:	755-26525554	
Fax:	755-26508930	

1.4. Manufacturer Information

Company:	TP-LINK TECHNOLOGIES CO., LTD.	
Address:	Building 24 (floors 1,3,4,5) and 28 (floors1-4) Park, Shennan Rd, Nanshan, Shenzhen, China	Central Science and Technology
City:	Shenzhen	
Postal Code:	518057	
Country:	P.R.China	
Telephone:	755-26525554	
Fax:	755-26508930	

1.5. Information of EUT

General Information

Device Type:	Portable Device			
Exposure Category:	Uncontrolled Environment / General Population			
State of Sample:	Prototype Unit			
Product Name:	150Mbps Mini Wireless N US	B Adapter		
SN:	1	1		
Hardware Version:	2.0			
Software Version:	1			
Antenna Type:	Internal Antenna			
Device Operating Configurations:				
Supporting Mode(s):	802.11b; (tested) 802.11g; (tested) 802.11n HT20; (tested) 802.11n HT40; (tested)			
	Mode	Tx (MHz)		
Operating Frequency Range(s):	802.11b/g/n HT20	2412 ~ 2462MHz		
	802.11n HT40	2422 ~ 2452MHz		
Test Channel: (Low - Middle - High)	1-6-11 (802.11b/g/n HT20) 3-6-9 (802.11n HT40)			
Used Host Products:	IBM T61			

Report No.: RZA1112-2131SAR01R1

Equipment Under Test (EUT) is 150Mbps Mini Wireless N USB Adapter. During SAR test of the EUT, it was connected to a portable computer. The EUT has a WIFI antenna that can be used for Tx/Rx. SAR is tested for 802.11b/g/n in this report.

The sample under test was selected by the Client.

Components list please refer to documents of the manufacturer.

1.6. The Maximum SAR_{1g} Values

Body Worn Configuration

Mode	Channel	Position	Separation distance	SAR _{1g} (W/kg)
802.11b	Low/1	Back Side	5mm	0.298
802.11g	Low/1	Back Side	5mm	0.524
802.11n HT20	Low/1	Back Side	5mm	0.541
802.11n HT40	Middle/6	Back Side	5mm	0.469

1.7. Test Date

The test is performed on February 1, 2012.

2. SAR Measurements System Configuration

2.1. SAR Measurement Set-up

The DASY4 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Stäubli RX family) with controller and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e. an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronic (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- A unit to operate the optical surface detector which is connected to the EOC.
- The Electro-Optical Coupler (EOC) performs the conversion from the optical into a digital electric signal of the DAE. The EOC is connected to the DASY4 measurement server.
- The DASY4 measurement server, which performs all real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operation. A computer operating Windows 2003
- DASY4 software and SEMCAD data evaluation software.
- Remote control with teach panel and additional circuitry for robot safety such as warning lamps, etc.
- The generic twin phantom enabling the testing of left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- System validation dipoles allowing to validate the proper functioning of the system.

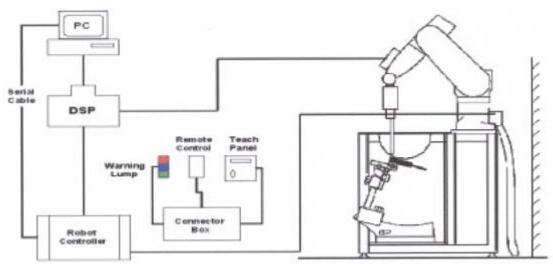


Figure 1 SAR Lab Test Measurement Set-up

2.2. DASY4 E-field Probe System

The SAR measurements were conducted with the dosimetric probe EX3DV4 (manufactured by SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation.

2.2.1. EX3DV4 Probe Specification

- Construction Symmetrical design with triangular core Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., DGBE)
- Calibration ISO/IEC 17025 calibration service available
- Frequency 10 MHz to > 6 GHz Linearity: ± 0.2 dB (30 MHz to 6 GHz)

Directivity ± 0.3 dB in HSL (rotation around probe axis) ± 0.5 dB in tissue material (rotation normal to probe axis)

- Dynamic Range 10μ W/g to > 100 mW/g Linearity:
 - \pm 0.2dB (noise: typically < 1 μ W/g)
- Dimensions Overall length: 330 mm (Tip: 20 mm) Tip diameter: 2.5 mm (Body: 12 mm) Typical distance from probe tip to dipole centers: 1 mm
- Application High precision dosimetric measurements in any exposure scenario (e.g., very strong gradient fields). Only probe which enables compliance testing for frequencies up to 6 GHz with precision of better 30%.



Figure 2.EX3DV4 E-field Probe



Figure 3. EX3DV4 E-field probe

Report No.: RZA1112-2131SAR01R1

2.2.2. E-field Probe Calibration

Each probe is calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy was evaluated and found to be better than \pm 0.25dB. The sensitivity parameters (NormX, NormY, NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested.

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies bellow 1 GHz, and in a wave guide above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$\mathbf{SAR} = \mathbf{C} \frac{\Delta \mathbf{T}}{\Delta \mathbf{t}}$$

Where: Δt = Exposure time (30 seconds), C = Heat capacity of tissue (brain or muscle), ΔT = Temperature increase due to RF exposure. Or

$$\mathbf{SAR} = \frac{|\mathbf{E}|^2 \sigma}{\rho}$$

Where:

 σ = Simulated tissue conductivity,

 ρ = Tissue density (kg/m3).

2.3. Other Test Equipment

2.3.1. Device Holder for Transmitters

The DASY device holder is designed to cope with the die rent positions given in the standard.

It has two scales for device rotation (with respect to the body axis) and device inclination (with respect to the line between the ear reference points). The rotation centers for both scales is the ear reference point (ERP). Thus the device needs no repositioning when changing the angles. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the inference of the clamp on the test results could thus be lowered.



Figure 4 Device Holder

2.3.2. Phantom

The Generic Twin Phantom is constructed of a fiberglass shell integrated in a wooden Figure. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90% of all users. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot.

Shell Thickness2±0.1 mmFilling VolumeApprox. 20 litersDimensions810 x 1000 x 500 mm (H x L x W)AailableSpecial



Figure 5 Generic Twin Phantom

2.4. Scanning Procedure

The DASY4 installation includes predefined files with recommended procedures for measurements and validation. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.

- The "reference" and "drift" measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. ± 5 %.
- The "surface check" measurement tests the optical surface detection system of the DASY4 system by repeatedly detecting the surface with the optical and mechanical surface detector and comparing the results. The output gives the detecting heights of both systems, the difference between the two systems and the standard deviation of the detection repeatability. Air bubbles or refraction in the liquid due to separation of the sugar-water mixture gives poor repeatability (above ± 0.1mm). To prevent wrong results tests are only executed when the liquid is free of air bubbles. The difference between the optical surface detection and the actual surface depends on the probe and is specified with each probe. (It does not depend on the surface reflectivity or the probe angle to the surface within ± 30°.)
- Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values before running a detailed measurement around the hot spot.Before starting the area scan a grid

Report No.: RZA1112-2131SAR01R1

spacing of 10 mm x 10 mm is set. During the scan the distance of the probe to the phantom remains unchanged.

After finishing area scan, the field maxima within a range of 2 dB will be ascertained.

Zoom Scan

Zoom Scans are used to estimate the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The default Zoom Scan is done by 7x7x7 points within a cube whose base is centered around the maxima found in the preceding area scan.

• Spatial Peak Detection

The procedure for spatial peak SAR evaluation has been implemented and can determine values of masses of 1g and 10g, as well as for user-specific masses. The DASY4 system allows evaluations that combine measured data and robot positions, such as:

- maximum search
- extrapolation
- boundary correction
- peak search for averaged SAR

During a maximum search, global and local maxima searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard's method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation. Extrapolation routines require at least 10 measurement points in 3-D space. They are used in the Zoom Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the modified Quadratic Shepard's method for extrapolation. For a grid using 7x7x7 measurement points with 5mm resolution amounting to 343 measurement points, the uncertainty of the extrapolation routines is less than 1% for 1g and 10g cubes.

• A Z-axis scan measures the total SAR value at the x-and y-position of the maximum SAR value found during the cube 7x7x7 scan. The probe is moved away in z-direction from the bottom of the SAM phantom in 5mm steps.

2.5. Data Storage and Evaluation

2.5.1. Data Storage

The DASY4 software stores the acquired data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension ".DA4". The software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of incorrect parameter settings. For example, if a measurement has been performed with a wrong crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be re-evaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type ([V/m], [A/m], [°C], [mW/g], [mW/cm²], [dBrel], etc.). Some of these units are not available in certain situations or show meaningless results, e.g., a SAR output in a lossless media will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

2.5.2. Data Evaluation by SEMCAD

The SEMCAD software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters:	•	Normi, a _{i0} , a _{i1} , a _{i2}
	- Conversion factor	ConvF _i
	- Diode compression point	Dcpi
Device parameters:	- Frequency	f
•	- Crest factor	cf
Media parameters:	- Conductivity	

- Density

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY4 components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics.

Report No.: RZA1112-2131SAR01R1

If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot c f / d c p_i$$

With	V_i = compensated signal of channel i	(i = x, y, z)
	\boldsymbol{U}_i = input signal of channel i	(i = x, y, z)
	<i>cf</i> = crest factor of exciting field	(DASY parameter)
	<i>dcp</i> _i = diode compression point	(DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes:		$E_i = (V_i / Norm_i \cdot ConvF)^{1/2}$						
H-field p	probes:	$H_i = (V_i)^{1/2} \cdot (a_{i0} + a_{i1}f + a_{i2}f^2) / f$						
With	Vi	= compensated signal of channel i	(i = x, y, z)					
	Norm _i	= sensor sensitivity of channel i [mV/(V/m) ²] for E-field Probes	(i = x, y, z)					
	ConvF	= sensitivity enhancement in solution						
	a _{ij}	= sensor sensitivity factors for H-field probes						
	f	= carrier frequency [GHz]						

- E_i = electric field strength of channel i in V/m
- H_i = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = (E_x^2 + E_y^2 + E_z^2)^{1/2}$$

The primary field data are used to calculate the derived field units.

$$SAR = (E_{tot})^2 \cdot \sigma / (\rho \cdot 1000)$$

with **SAR** = local specific absorption rate in mW/g

- **E**_{tot} = total field strength in V/m
 - = conductivity in [mho/m] or [Siemens/m]
 - = equivalent tissue density in g/cm³

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid. The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = E_{tot}^2 / 3770$$
 or $P_{pwe} = H_{tot}^2 \cdot 37.7$

with P_{pwe} = equivalent power density of a plane wave in mW/cm²

 E_{tot} = total electric field strength in V/m

 H_{tot} = total magnetic field strength in A/m

3. Laboratory Environment

Table 1: The Requirements of the Ambient Conditions

•					
Temperature	Min. = 20°C, Max. = 25 °C				
Relative humidity	Min. = 30%, Max. = 70%				
Ground system resistance	< 0.5 Ω				
Ambient noise is checked and found very low and in compliance with requirement of standards.					
Reflection of surrounding objects is minimized and in compliance with requirement of standards.					

4. Tissue-equivalent Liquid

4.1. Tissue-equivalent Liquid Ingredients

The liquid is consisted of water, salt, Glycol. The liquid has previously been proven to be suited for worst-case. The table 2 shows the detail solution. It's satisfying the latest tissue dielectric parameters requirements proposed by the OET 65.

Table 2: Composition of the Body Tissue Equivalent Matter

MIXTURE%	FREQUENCY(Body) 2450MHz			
Water	73.2			
Glycol	26.7			
Salt	0.1			
Dielectric Parameters Target Value	f=2450MHz ε=52.70 σ=1.95			

4.2. Tissue-equivalent Liquid Properties

Table 3: Dielectric Performance of Body Tissue Simulating Liquid

Frequency	Description	Dielectric Par	Temp	
Frequency			σ(s/m)	°C
	Target value	52.72	1.94	,
2437MHz	±5% window	50.08 — 55.36	1.84 — 2.04	1
(Middle)	Measurement value	52.0	1.05	21.9
	2012-2-1	52.0	1.95	21.9
	Target value	52.75	1.91	,
2412MHz	±5% window	50.11 — 55.39	1.81 — 2.00	1
(Low)	Measurement value	52.1	1 02	21.9
	2012-2-1	JZ. I	1.92	21.9

5. Systerm Check

5.1. Description of System Check

The manufacturer calibrates the probes annually. Dielectric parameters of the tissue simulates were measured every day using the dielectric probe kit and the network analyzer. A system check measurement was made following the determination of the dielectric parameters of the simulates, using the dipole validation kit. A power level of 250 mW was supplied to the dipole antenna, which was placed under the flat section of the twin SAM phantom. The system check results (dielectric parameters and SAR values) are given in the table 4.

TA Technology (Shanghai) Co., Ltd. Test Report

System check results have to be equal or near the values determined during dipole calibration with the relevant liquids and test system (±10 %).

System check is performed regularly on all frequency bands where tests are performed with the DASY4 system.

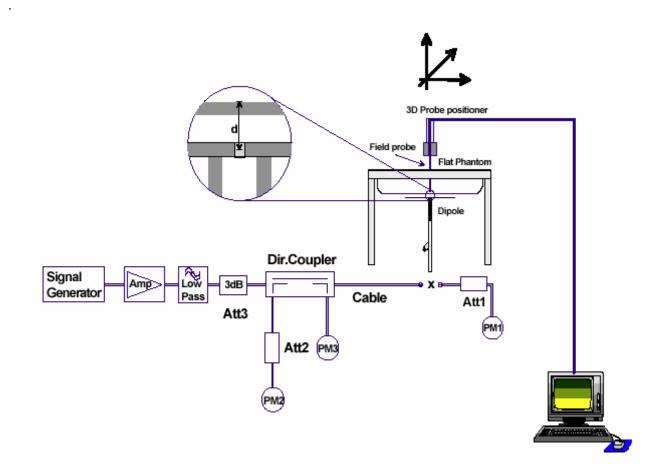


Figure 6 System Check Set-up

Page 19 of 64

5.2. System Check Results

Table 4: System Check in Body Tissue Simulating Liquid

Frequency	Test Date	Dielectric Parameters		Temp	250mW Measured SAR _{1g}	1W Normalized SAR _{1g}	1W Target SAR _{1g} (±10 % deviation)	
		٤r	σ(s/m)	(°C)				
2450MHz	2012-2-1	51.97	1.97	21.9	14.01	56.04	51.70 (46.53~56.87)	
Note: 1. The graph results see ANNEX B.								
2. Target Values used derive from the calibration certificate								

6. Operational Conditions during Test

6.1. General Description of Test Procedures

For the 802.11b/g SAR body tests, a communication link is set up with the test mode software for WIFI mode test. The Absolute Radio Frequency Channel Number (ARFCN) is allocated to 1, 6 and 11 respectively in the case of 2450 MHz. During the test, at the each test frequency channel, the EUT is operated at the RF continuous emission mode. Each channel should be tested at the lowest data rate in each mode. Testing at higher data rates is not required when the maximum average output power is less than 0.25dB higher than those measured at the lowest data rate.

802.11b/g operating modes are tested independently according to the service requirements in each frequency band. 802.11b/g modes are tested on channels 1,6 and 11; however, if output power reduction is necessary for channels 1 and /or 11 to meet restricted band requirements the highest output channels closest to each of these channels must be tested instead.

SAR is not required for 802.11g channels when the maximum average output power is less than 0.25dB higher than that measured on the corresponding 802.11b channels. When the maximum average output channel in each frequency band is not included in the "default test channels", the maximum channel should be tested instead of an adjacent "default test channels", these are referred to as the "required test channels" and are illustrated in Table 5.

			Turbo Channel	"Default Test Channels"				
Mode	GHz	Channel		15.247				
			Gilailliei	802.11b	802.11g	UNII		
	2.412	1#		\checkmark	*			
802.11b/g	2.437	6	6	\checkmark	*			
	2.462	11 [#]		\checkmark	*			

Table 5: "Default Test Channels"

Note: [#]=when output power is reduced for channel 1 and /or 11to meet restricted band requirements the highest out put channels closet to each of these channels should be tested.

√= "default test channels"

* =possible 802.11g channels with maximum average output 0.25dB>=the "default test channels"

6.2. Test Positions

The measurements were performed in combination with a host product (IBM T61). IBM T61 laptop has horizontal USB slot, and vertical USB slot.

A test distance of 5mm or less, according to KDB 447498 D02, should be considered for the orientation that can satisfy such requirements.

For each channel, the EUT is tested at the following 4 test positions:

- Test Position 1: The EUT is connected to the portable computer with horizontal USB slot. The back side of the EUT towards to the bottom of the flat phantom. The distance from back side of the EUT to the bottom of the flat phantom is 5mm. (ANNEX G Picture 5)
- Test Position 2: The EUT is connected to the portable computer through a 19 cm USB cable. The front side of the EUT towards the bottom of the flat phantom. The distance from front side of the EUT to the bottom of the flat phantom is 5mm. (ANNEX G Picture 6)
- Test Position 3: The EUT is connected to the portable computer through a 19 cm USB cable. The left side of the EUT towards the bottom of the flat phantom. The distance from left side of the EUT to the bottom of the flat phantom is 5mm. (ANNEX G Picture 7)
- Test Position 4: The EUT is connected to the portable computer with vertical USB slot. The right side of the EUT towards the bottom of the flat phantom. The distance from right side of the EUT to the bottom of the flat phantom is 5mm. (ANNEX G Picture 8)

Report No.: RZA1112-2131SAR01R1

6.3. Picture of Host Product


During the test, IBM T61 was used as an assistant to help to setup communication. (See Picture 1)



Picture 1-a: IBM T61 Close



Picture 1-b: IBM T61 Open

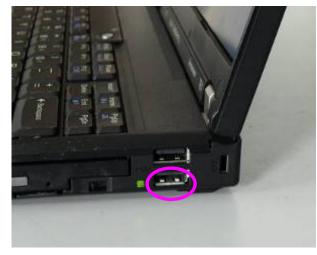

Picture 1-c: IBM T61 with horizontal USB slot



Picture 1-d: IBM T61 with Vertical USB slot



Picture 1-e: a 19 cm USB cable Picture 1: Computer as a test assistant

7. Test Results

7.1. Conducted Power Results

Table 6: Conducted Power Measurement Results

		,	Average Power(dBm)					
Mode	Data rate	2412MHz	2437MHz	2462 MHz				
		(Ch1)	(Ch6)	(Ch11)				
	1 Mbp	13.38	13.32	12.85				
000 11h	2 Mbps	13.46	13.29	12.51				
802.11b	5.5 Mbps	13.52	13.27	12.53				
	11 Mbps	13.42	13.21	12.54				
	6 Mbps	17.52	16.26	15.75				
	9 Mbps	17.06	16.12	15.81				
	12 Mbps	15.56	14.65	14.33				
900 11 a	18 Mbps	14.85	14.02	13.49				
802.11g	24 Mbps	13.64	12.92	12.43				
	36 Mbps	13.09	12.35	11.95				
	48 Mbps	12.29	11.43	11.02				
	54 Mbps	11.15	10.42	9.98				
	MCS0	16.95	16.32	15.93				
	MCS1	15.65	15.11	14.74				
	MCS2	15.58	15.15	14.78				
802.11n HT20	MCS3	15.27	14.57	14.41				
002.THTHT20	MCS4	12.81	12.28	12.02				
	MCS5	12.24	11.78	11.53				
	MCS6	11.32	10.75	10.56				
	MCS7	9.61	9.05	8.79				
		/	Average Power(dBm)				
Mode	Date rata	2422MHz	2437MHz	2452 MHz				
		(Ch3)	(Ch6)	(Ch9)				
	MCS0	16.15	16.25	15.95				
	MCS1	14.82	14.91	14.71				
	MCS2	14.87	14.81	14.57				
802.11n HT40	MCS3	14.46	14.42	14.31				
002.11111140	MCS4	12.15	12.07	11.89				
	MCS5	11.62	11.56	11.34				
	MCS6	10.71	10.54	10.46				
	MCS7	8.96	8.81	8.68				
Note: SAR is not re	equired for 802.	11g/n channels whe	en the maximum ave	rage output power				
is less than 0.25	dB higher than	that measured on t	he corresponding 80	2.11b channels.				

7.2. SAR Test Results

7.2.1. WIFI (802.11b/g/n)

Table 7: SAR Values [WIFI (802.11b/g/n)]

	_ 、	10 g Average	1g Average	Power Drift					
Limit of SA	AR	2.0 W/kg	1.6 W/kg	± 0.21 dB	Quenh				
Test Case Of	Body	Measurement	Result (W/kg)	Deuxer Drift	Graph Results				
Different Test Position	Channel	10 g Average 1 g Average		Power Drift (dB)					
	Test Positio	on of 802.11b With	IBM T61 (Distance	e 5mm)					
Test Position 1	Low/1	0.136	0.298	-0.077	Figure 8				
Test Position 2	Low/1	0.119	0.252	-0.030	Figure 9				
Test Position 3	Low/1	0.096	0.204	-0.060	Figure 10				
Test Position 4	Low/1	0.110	0.239	-0.012	Figure 11				
Worst	case positio	n of 802.11b with 8	302.11g (IBM T61, I	Distance 5mm)					
Test Position 1	Low/1	0.234	0.524	-0.070	Figure 12				
Worst cas	se position o	of 802.11b with 802	.11n/HT20 (IBM T6	1, Distance 5m	nm)				
Test Position 1	Low/1	0.257	0.541	-0.043	Figure 13				
Worst cas	se position o	of 802.11b with 802	.11n/HT40 (IBM T6	1, Distance 5m	ım)				
Test Position 1	Middle/6	0.227	0.469	-0.022	Figure 14				
Note: 1.The value w	ith blue color	is the maximum SA	R Value of each tes	st band.					
2. The SAR test shall be performed at the high, middle and low frequency channels of each									
operating mode. If the SAR measured at the channel with the maximum conducted power									
for each te	st configuration	on is at least 3.0 dB	(< 0.8W/kg) lower t	han the SAR lir	nit, testing at				
the other tw	vo channels i	s optional.							

Page 25 of 64

8. Measurement Uncertainty

No.	source	Туре	Uncertainty Value (%)	Probability Distribution	k	Ci	Standard ncertainty $u'_i(\%)$	Degree of freedom V _{eff} or v _i			
1	System repetivity	А	0.5	Ν	1	1	0.5	9			
	Measurement system										
2	-probe calibration	В	5.9	Ν	1	1	5.9	∞			
3	-axial isotropy of the probe	В	4.7	R	$\sqrt{3}$	$\sqrt{0.5}$	1.9	∞			
4	- Hemispherical isotropy of the probe	В	9.4	R	$\sqrt{3}$	$\sqrt{0.5}$	3.9	×			
6	-boundary effect	В	1.9	R	$\sqrt{3}$	1	1.1	∞			
7	-probe linearity	В	4.7	R	$\sqrt{3}$	1	2.7	∞			
8	- System detection limits	В	1.0	R	$\sqrt{3}$	1	0.6	∞			
9	-readout Electronics	В	1.0	Ν	1	1	1.0	∞			
10	-response time	В	0	R	$\sqrt{3}$	1	0	∞			
11	-integration time	В	4.32	R	$\sqrt{3}$	1	2.5	8			
12	-noise	В	0	R	$\sqrt{3}$	1	0	∞			
13	-RF Ambient Conditions	В	3	R	$\sqrt{3}$	1	1.73	∞			
14	-Probe Positioner Mechanical Tolerance	В	0.4	R	$\sqrt{3}$	1	0.2	∞			
15	-Probe Positioning with respect to Phantom Shell	В	2.9	R	$\sqrt{3}$	1	1.7	∞			
16	-Extrapolation, interpolation and Integration Algorithms for Max. SAR Evaluation	В	3.9	R	$\sqrt{3}$	1	2.3	∞			
		Tes	st sample Relate	ed							
17	-Test Sample Positioning	А	2.9	Ν	1	1	4.92	71			
18	-Device Holder Uncertainty	А	4.1	Ν	1	1	4.1	5			
19	-Output Power Variation - SAR drift measurement	В	5.0	R	$\sqrt{3}$	1	2.9	∞			
		Ph	ysical paramete	er				Γ			
20	-phantom	В	4.0	R	$\sqrt{3}$	1	2.3	∞			

Report No.: RZA1112-2131SAR01R1

Page 26 of 64

21	-liquid conductivity (deviation from target)	В	5.0	R	$\sqrt{3}$	0.64	1.8	8
22	-liquid conductivity (measurement uncertainty)	В	2.5	Ν	1	0.64	1.6	9
23	-liquid permittivity (deviation from target)	В	5.0	R	$\sqrt{3}$	0.6	1.7	8
24	-liquid permittivity (measurement uncertainty)	В	2.5	Ν	1	0.6	1.5	9
Combined standard uncertainty		$u_{c}' = \sqrt{\sum_{i=1}^{21} c_{i}^{2} u_{i}^{2}}$					12.12	
Expanded uncertainty (confidence interval of 95 %)		$u_e = 2u_c$		N k=2		24.24		


9. Main Test Instruments

Table 8: List of Main Instruments


No.	Name	Туре	Serial Number	Calibration Date	Valid Period
01	Network analyzer	Agilent 8753E	US37390326	September 12, 2011	One year
02	Dielectric Probe Kit	Agilent 85070E	US44020115	No Calibration Rec	quested
03	Power meter	Agilent E4417A	GB41291714	March 12, 2011	One year
04	Power sensor	Agilent N8481H	MY50350004	September 25, 2011	One year
05	Power sensor	E9327A	US40441622	September 24, 2011	One year
06	Signal Generator	HP 8341B	2730A00804	September 12, 2011	One year
07	Amplifier	IXA-020	0401	No Calibration Requested	
08	E-field Probe	EX3DV4	3816	October 3, 2011	One year
09	DAE	DAE4	871	November 22, 2011	One year
10	Validation Kit 2450MHz	D2450V2	786	August 29, 2011	One year
11	Temperature Probe	JM222	AA1009129	March 16, 2011	One year
12	Hygrothermograph	HTC-1	TASH121602	June 21, 2011	One year
13	Dual directional coupler	777D	50146	August 21, 2011	One year

*****END OF REPORT BODY*****

ANNEX A: Test Layout

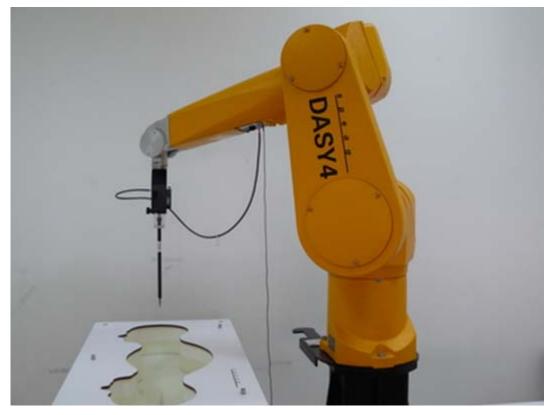

Picture 2: Specific Absorption Rate Test Layout

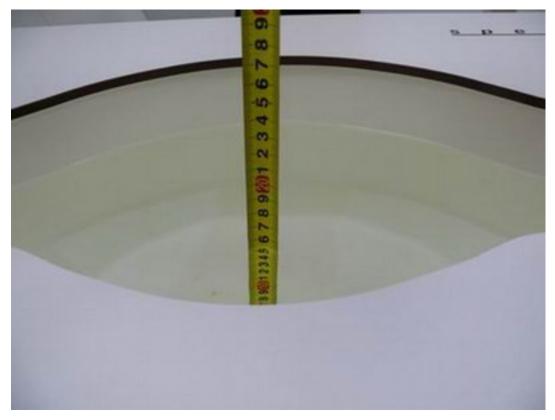

Picture 3: Liquid depth in the flat Phantom (2450 MHz, 15.3cm depth)

ANNEX B: System Check Results

System Performance Check at 2450 MHz Body TSL

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 786

Date/Time: 2/1/2012 10:15:36 AM

Communication System: CW; Frequency: 2450 MHz;Duty Cycle: 1:1

Medium parameters used: f = 2450 MHz; σ = 1.97 mho/m; ϵ_r = 51.97; ρ = 1000 kg/m³

Ambient Temperature: 22.3 °C Liquid Temperature: 21.9 °C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3816; ConvF(7.19, 7.19, 7.19) Calibrated: 10/3/2011;

Electronics: DAE4 Sn871; Calibrated: 11/22/2011

Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246


Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

d=10mm, Pin=250mW/Area Scan (61x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 21.5 mW/g

d=10mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 71.0 V/m; Power Drift = 0.011 dB

Peak SAR (extrapolated) = 28.2 W/kg



Maximum value of SAR (measured) = 19.82 mW/g

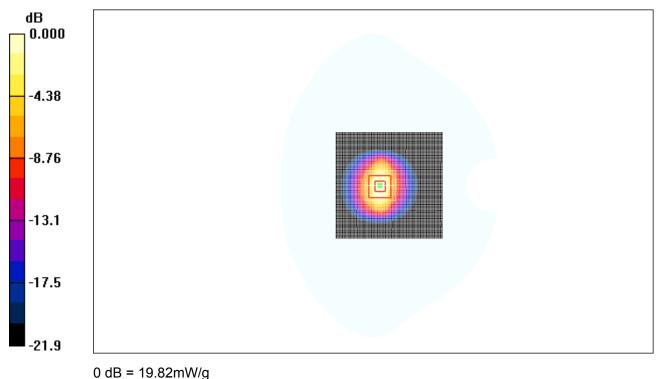


Figure 7 System Performance Check 2450MHz 250mW

ANNEX C: Graph Results


802.11b with IBM T61 Test Position 1 Low

Date/Time: 2/1/2012 11:47:33 AM Communication System: 802.11b; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium parameters used: f = 2412 MHz; σ = 1.92 mho/m; ϵ_r = 52.1; ρ = 1000 kg/m³ Ambient Temperature:22.3 °C Liquid Temperature: 21.5 °C Phantom section: Flat Section DASY4 Configuration: Probe: EX3DV4 - SN3816; ConvF(7.19, 7.19, 7.19) Calibrated: 10/3/2011; Electronics: DAE4 Sn871; Calibrated: 11/22/2011 Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246 Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Test Position 1 Low/Area Scan (31x61x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.391 mW/g

Test Position 1 Low/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 13.3 V/m; Power Drift = -0.077 dB Peak SAR (extrapolated) = 0.718 W/kg SAR(1 g) = 0.298 mW/g; SAR(10 g) = 0.136 mW/g

Maximum value of SAR (measured) = 0.340 mW/g

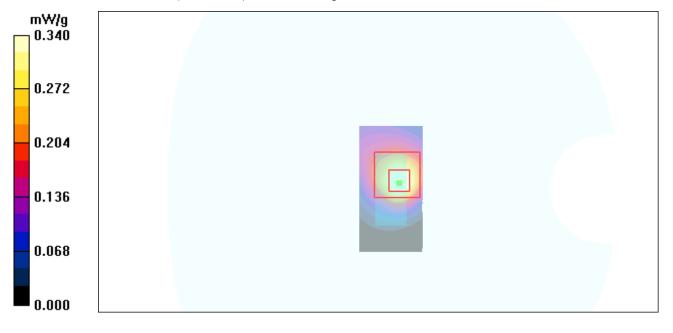



Report No.: RZA1112-2131SAR01R1

Page 31 of 64


802.11b with IBM T61 Test Position 2 Low

Date/Time: 2/1/2012 12:36:54 PM Communication System: 802.11b; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium parameters used: f = 2412 MHz; σ = 1.92 mho/m; ϵ_r = 52.1; ρ = 1000 kg/m³ Ambient Temperature:22.3 °C Liquid Temperature: 21.5 °C Phantom section: Flat Section DASY4 Configuration: Probe: EX3DV4 - SN3816; ConvF(7.19, 7.19, 7.19) Calibrated: 10/3/2011; Electronics: DAE4 Sn871; Calibrated: 11/22/2011 Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246 Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Test Position 2 Low/Area Scan (31x61x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.336 mW/g

Test Position 2 Low/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 13.8 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 0.591 W/kg SAR(1 g) = 0.252 mW/g; SAR(10 g) = 0.119 mW/g

Maximum value of SAR (measured) = 0.277 mW/g

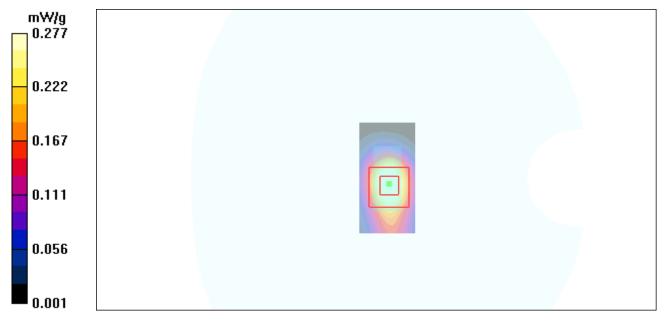



Report No.: RZA1112-2131SAR01R1

Page 32 of 64

802.11b with IBM T61 Test Position 3 Low

Date/Time: 2/1/2012 12:57:28 PM Communication System: 802.11b; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium parameters used: f = 2412 MHz; σ = 1.92 mho/m; ϵ_r = 52.1; ρ = 1000 kg/m³ Ambient Temperature:22.3 °C Liquid Temperature: 21.5 °C Phantom section: Flat Section DASY4 Configuration: Probe: EX3DV4 - SN3816; ConvF(7.19, 7.19, 7.19) Calibrated: 10/3/2011; Electronics: DAE4 Sn871; Calibrated: 11/22/2011 Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246 Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Test Position 3 Low/Area Scan (31x61x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.241 mW/g

Test Position 3 Low/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 11.0 V/m; Power Drift = -0.060 dB Peak SAR (extrapolated) = 0.474 W/kg SAR(1 g) = 0.204 mW/g; SAR(10 g) = 0.096 mW/g

Maximum value of SAR (measured) = 0.223 mW/g

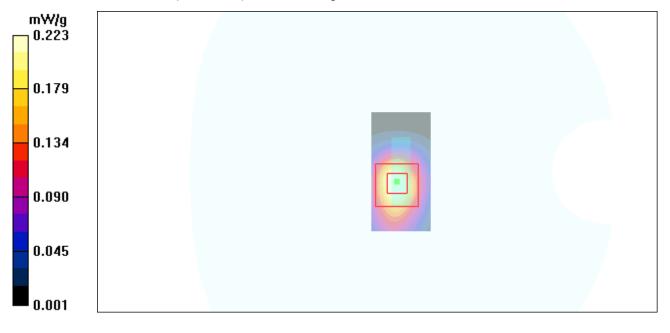


Figure 10 802.11b with IBM T61 Test Position 3 Channel 1

Report No.: RZA1112-2131SAR01R1

Page 33 of 64


802.11b with IBM T61 Test Position 4 Low

Date/Time: 2/1/2012 1:18:09 PM Communication System: 802.11b; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium parameters used: f = 2412 MHz; σ = 1.92 mho/m; ϵ_r = 52.1; ρ = 1000 kg/m³ Ambient Temperature:22.3 °C Liquid Temperature: 21.5 °C Phantom section: Flat Section DASY4 Configuration: Probe: EX3DV4 - SN3816; ConvF(7.19, 7.19, 7.19) Calibrated: 10/3/2011; Electronics: DAE4 Sn871; Calibrated: 11/22/2011 Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246 Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Test Position 4 Low/Area Scan (31x61x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.275 mW/g

Test Position 4 Low/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 11.8 V/m; Power Drift = -0.012 dB Peak SAR (extrapolated) = 0.585 W/kg SAR(1 g) = 0.239 mW/g; SAR(10 g) = 0.110 mW/g

Maximum value of SAR (measured) = 0.267 mW/g

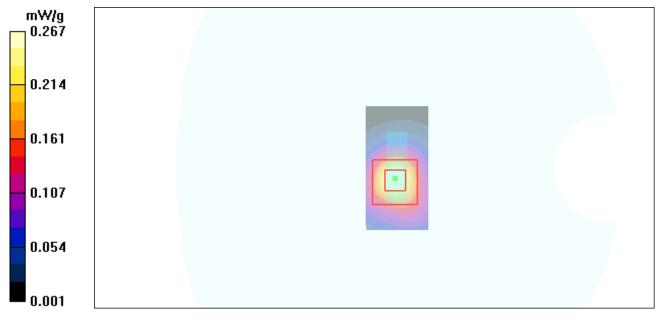



Report No.: RZA1112-2131SAR01R1

Page 34 of 64


802.11g with IBM T61 Test Position 1 Low

Date/Time: 2/1/2012 4:26:08 PM Communication System: 802.11g; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium parameters used: f = 2412 MHz; σ = 1.92 mho/m; ϵ_r = 52.1; ρ = 1000 kg/m³ Ambient Temperature:22.3 °C Liquid Temperature: 21.5 °C Phantom section: Flat Section DASY4 Configuration: Probe: EX3DV4 - SN3816; ConvF(7.19, 7.19, 7.19) Calibrated: 10/3/2011; Electronics: DAE4 Sn871; Calibrated: 11/22/2011 Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246 Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Test Position 1 Low/Area Scan (31x61x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.654 mW/g

Test Position 1 Low/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 16.7 V/m; Power Drift = -0.070 dB Peak SAR (extrapolated) = 1.26 W/kg SAR(1 g) = 0.524 mW/g; SAR(10 g) = 0.234 mW/g

Maximum value of SAR (measured) = 0.577 mW/g

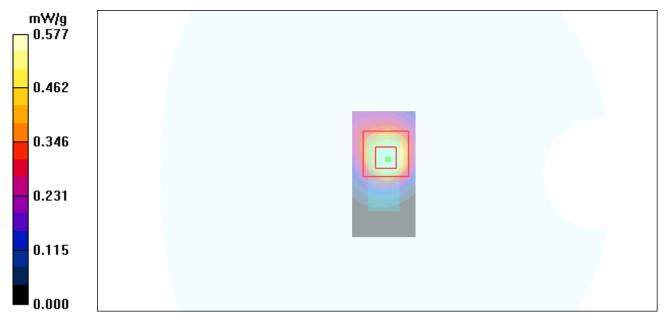



Report No.: RZA1112-2131SAR01R1

Page 35 of 64


802.11n/HT20 with IBM T61 Test Position 1 Low

Date/Time: 2/1/2012 4:43:43 PM Communication System: 802.11n; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium parameters used: f = 2412 MHz; $\sigma = 1.92$ mho/m; $\epsilon_r = 52.1$; $\rho = 1000$ kg/m³ Ambient Temperature:22.3 °C Liquid Temperature: 21.5 °C Phantom section: Flat Section DASY4 Configuration: Probe: EX3DV4 - SN3816; ConvF(7.19, 7.19, 7.19) Calibrated: 10/3/2011; Electronics: DAE4 Sn871; Calibrated: 11/22/2011 Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246 Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Test Position 1 Low/Area Scan (31x61x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.643 mW/g

Test Position 1 Low/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 16.1 V/m; Power Drift = -0.043 dB Peak SAR (extrapolated) = 1.30 W/kg

SAR(1 g) = 0.541 mW/g; SAR(10 g) = 0.257 mW/g Maximum value of SAR (measured) = 0.593 mW/g

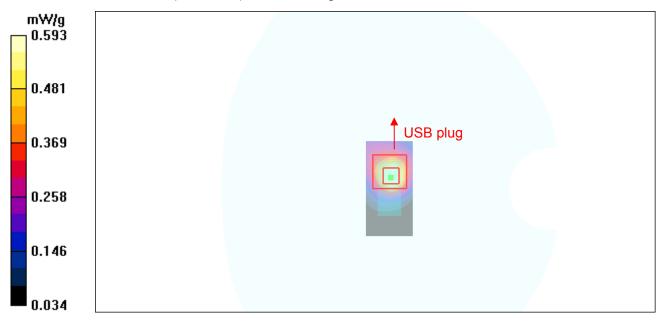

Report No.: RZA1112-2131SAR01R1

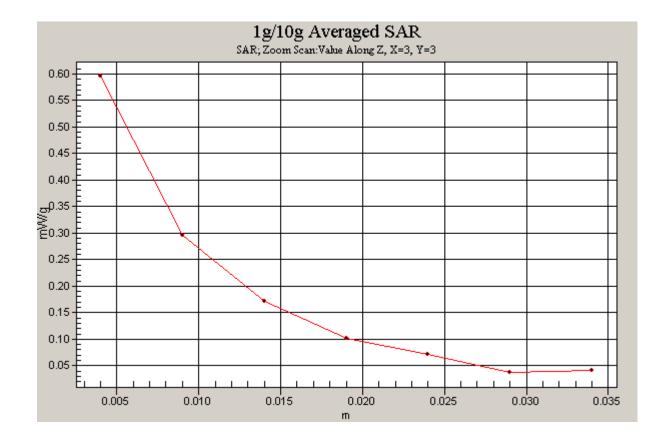


Figure 13 802.11n/HT20 with IBM T61 Test Position 1 Channel 1


Report No.: RZA1112-2131SAR01R1

802.11n/HT40 with IBM T61 Test Position 1 Middle

Date/Time: 2/1/2012 5:05:22 PM Communication System: 802.11n; Frequency: 2437 MHz;Duty Cycle: 1:1 Medium parameters used (interpolated): f = 2437 MHz; σ = 1.95 mho/m; ϵ_r = 52; ρ = 1000 kg/m³ Ambient Temperature:22.3 °C Liquid Temperature: 21.5 °C Phantom section: Flat Section DASY4 Configuration: Probe: EX3DV4 - SN3816; ConvF(7.19, 7.19, 7.19) Calibrated: 10/3/2011; Electronics: DAE4 Sn871; Calibrated: 11/22/2011 Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246 Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Test Position 1 Middle/Area Scan (31x61x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.562 mW/g

Test Position 1 Middle/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 15.2 V/m; Power Drift = -0.022 dB Peak SAR (extrapolated) = 1.09 W/kg SAR(1 g) = 0.469 mW/g; SAR(10 g) = 0.227 mW/g Maximum value of SAR (measured) = 0.514 mW/g

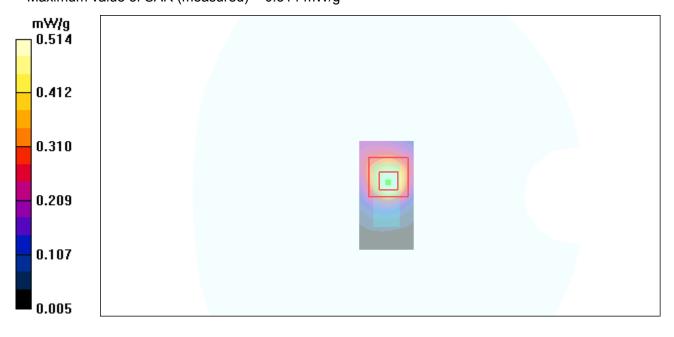



Report No.: RZA1112-2131SAR01R1

ANNEX D: Probe Calibration Certificate

Engineering AG eughausstrasse 43, 8004 Zur	ich, Switzerland	RACIMENA (C. C. Z. Z. S.	Servizio svizzero di taratura Swiss Calibration Service
ccredited by the Swiss Accredit			to.: SCS 108
he Swiss Accreditation Servi Iultilateral Agreement for the	이 이 사람이 있는 것이 집에서 가운 집안이 없다.		
lient TMC Shangha	d (Auden)	Certificate No:	EX3-3816_Oct11
CALIBRATION	CERTIFICATI		
N 999	Part Caller State American		
Object	EX3DV4 - SN:38	16	
Calibration procedure(s)	QA CAL-01 VA	A CAL-12 V7. OA CAL-23 V4. OA	CAL 25 V4
	Calibration proce	dure for dosimetric E-field probes	
	要用於自然的影響的認識的影響		BAR AND
Calibration date:	October 3 2044		BRANTING COLORIDATION AND
	PARAMAR AND AND AND	CLUM CONTRACTOR NEWSFILM CONTRACTOR OF THE CONTRACTOR OF CON	0.636.6476.4699.00895815492722231
The measurements and the unc		robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C a	
The measurements and the unc	ucted in the closed laborator	robability are given on the following pages and ry facility: environment temperature (22 ± 3) °C ϵ	
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi	ucted in the closed laborator BTE critical for calibration)	ry facility: environment temperature (22 ± 3)°C a	and humidity < 70%.
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards	ucted in the closed laborator 8'TE onlocal for calibration)	ry facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.)	and humidity < 70%.
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi	ucted in the closed laborator BTE critical for calibration)	ry facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372)	and humidity < 70%. Scheduled Calibration Apr-12
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198	ucted in the closed laborator 8TE critical for calibration) ID GB41293874	ry facility: environment temperature (22 ± 3)*C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372)	and humidity < 70%. Scheduled Calibration Apr-12 Apr-12
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44199 Power sensor E4412A	ID GB41293874 MY41496087	ry facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372)	Scheduled Calibration Apr-12 Apr-12 Apr-12
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power standards Power sensor E44198 Reference 3 dB Attenuator	ID GB41293874 MY41496087 SN: S5054 (3c)	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01372)	Scheduled Calibration Apr-12 Apr-12 Apr-12 Apr-12 Apr-12
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 20 dB Attenuator	ID GB41293874 MY41496087 SN: S5054 (3c) SN: S5066 (20b)	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367)	Scheduled Calibration Apr-12 Apr-12 Apr-12
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator	ID GB41293874 MY41496087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b)	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367)	Scheduled Calibration Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ID GB41293874 MY41496087 SN: 55066 (20b) SN: 55129 (30b) SN: 3013 SN: 654	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01370) 29-Dec-10 (No. ES3-3013_Dec10)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-11
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	ID GB41293874 MY41496087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01370) 29-Dec-10 (No. ES3-3013_Dec10)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-11
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	Ucted in the closed laborator STE critical for calibration) ID GB41293874 MY41496087 SN: S5054 (3c) SN: S5066 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: 3013 SN: 654 ID US3642U01700	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01370) 29-Dec-10 (No. ES3-3013_Dec10) 3-May-11 (No. DAE4-654_May11)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	Ucted in the closed laborator BTE critical for calibration) ID GB41293874 MY41496087 SN: 55066 (20b) SN: 55129 (30b) SN: 55129 (30b) SN: 3013 SN: 654 ID	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01370) 29-Dec-10 (No. ES3-3013_Dec10) 3-May-11 (No. DAE4-654_May11) Check Date (in house)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Scheduled Check
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E44198 Power sensor E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ucted in the closed laborator BTE critical for calibration) ID GB41293874 MY41496087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID US3642U01700 US37390585	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367) 29-Dec-10 (No. ES3-3013_Dec10) 3-May-11 (No. DAE4-654_May11) Check Date (in house) 4-Aug-99 (in house check Oct-09) 18-Oct-01 (in house check Oct-09)	Scheduled Calibration Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-11 Mey-12 Scheduled Check In house check: Oct-11 In house check: Oct-11
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 9 robe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	Ucted in the closed laborator STE critical for calibration) ID GB41293874 MY41496087 SN: S5054 (3c) SN: S5066 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: 3013 SN: 654 ID US3642U01700	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01370) 29-Dec-10 (No. ES3-3013_Dec10) 3-May-11 (No. DAE4-654_May11) Check Date (in house) 4-Aug-99 (in house check Oct-09)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-11 May-12 Scheduled Check In house check: Oct-11
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 9648C Network Analyzer HP 8753E Calibrated by:	ucted in the closed laborator aTE critical for calibration) ID GB41293874 MY41496087 SN: S5054 (3c) SN: S5066 (20b) SN: S5066 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: 3013 SN: 654 ID US3642U01700 US37390585 Name Jeiger Kastrali	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367) 29-Dec-10 (No. ES3-3013_Dec10) 3-May-11 (No. DAE4-854_May11) Check Date (in house) 4-Aug-99 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) 3-May-11 (No. Technicien	Scheduled Calibration Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-11 Mey-12 Scheduled Check In house check: Oct-11 In house check: Oct-11
The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E Calibrated by:	ucted in the closed laborator BTE critical for calibration) ID GB41293874 MY41496087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: 3013 SN: 654 ID US3642U01700 US37390585 Name	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01370) 29-Dec-10 (No. ES3-3013_Dec10) 3-May-11 (No. DAE4-654_May11) Check Date (in house) 4-Aug-99 (in house check Oct-09) 18-Oct-01 (in house check Oct-10) Function	Scheduled Calibration Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-11 Mey-12 Scheduled Check In house check: Oct-11 In house check: Oct-11
All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ucted in the closed laborator aTE critical for calibration) ID GB41293874 MY41496087 SN: S5054 (3c) SN: S5066 (20b) SN: S5066 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: 3013 SN: 654 ID US3642U01700 US37390585 Name Jeiger Kastrali	Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367) 29-Dec-10 (No. ES3-3013_Dec10) 3-May-11 (No. DAE4-854_May11) Check Date (in house) 4-Aug-99 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) 3-May-11 (No. Technicien	Scheduled Calibration Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-11 Mey-12 Scheduled Check In house check: Oct-11 In house check: Oct-11

Certificate No: EX3-3616_Oct11

Report No.: RZA1112-2131SAR01R1

Page 39 of 64

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étaionnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

s

C

S

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the algoratories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y.z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization ϕ	φ rotation around probe axis
Polarization 3	9 rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- Techniques", December 2003 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z, VRx,y,z: A, B, C are numerical linearization parameters assessed based on the data of
 power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the
 maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom
 exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: EX3-3816_Oct11

Report No.: RZA1112-2131SAR01R1

EX3DV4 - SN:3816

October 3, 2011

Probe EX3DV4

SN:3816

Manufactured: Calibrated: September 2, 2011 October 3, 2011

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: EX3-3816_Oct11

Page 3 of 11

Page 40 of 64

EX3DV4- SN:3816

October 3, 2011

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3816

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^4$	0.48	0.56	0.61	± 10.1 %
DCP (mV) ⁸	99.8	102.2	102.1	

Modulation Calibration Parameters

UID	Communication System Name	PAR		A dB	B dB	C dB	VR mV	Unc ^E (k=2)
10000	CW	0.00	X	0.00	0.00	1.00	111.3	±2.7 %
			Y	0.00	0.00	1.00	127.3	
		1	Z	0.00	0.00	1.00	127.7	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

⁴ The uncertainties of NormX,Y,Z do not affect the E³-field uncertainty inside TSL (see Pages 5 and 6). ⁹ Numerical linearization parameter: uncertainty not required. ⁶ Uncertainty is detarmined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4-SN:3816

October 3, 2011

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3816

Parameter D	etermined in	Head Tis	sue Simu	lating Me	edia	
Relative Permittivity	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)
43.5	0.87	9.97	9.97	9.97	0.11	1.00
	Relative Permittivity	Relative Conductivity Permittivity (S/m)	Relative Permittivity (S/m) ConvF X	Relative Conductivity Permittivity (S/m) ConvF X ConvF Y	Relative Permittivity (S/m) ConvF X ConvF Y ConvF Z	Permittivity (S/m) ConvF X ConvF Y ConvF Z Alpha

f(MHz) ^c	Relative Permittivity	Conductivity (S/m)	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
450	43.5	0.87	9.97	9.97	9.97	0.11	1.00	± 13.4 %
750	41.9	0.89	9.47	9.47	9.47	0.62	0.78	± 12.0 %
835	41.5	0.90	9.22	9.22	9.22	0.76	0.66	± 12.0 %
1450	40.5	1.20	8.58	8.58	8.58	0.65	0.77	± 12.0 %
1750	40.1	1.37	8.23	8.23	8.23	0.80	0.58	± 12.0 %
1900	40.0	1.40	7.90	7.90	7.90	0.80	0.57	± 12.0 %
2450	39.2	1.80	7.17	7.17	7.17	0.66	0.64	± 12.0 %
2600	39.0	1.96	7.06	7.06	7.06	0.64	0.67	± 12.0 %

^c Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.
^c At frequencies below 3 GHz, the validity of tissue parameters (s and o) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (s and o) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Page 5 of 11

EX3DV4-SN:3816

October 3, 2011

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3816

Calibration Parameter Determined in Body Tissue Simulating Med
--


f (MHz) ^c	Relative Permittivity F	Conductivity (S/m)	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
450	56.7	0.94	10.83	10.83	10.83	0.02	1.00	± 13.4 %
750	55.5	0.96	9.50	9.50	9.50	0.80	0.70	± 12.0 %
835	55.2	0.97	9.38	9.38	9.38	0.68	0.69	± 12.0 %
1750	53.4	1.49	7.80	7.80	7.80	0.80	0.65	± 12.0 %
1900	53.3	1.52	7.51	7.51	7.51	0.80	0.65	± 12.0 %
2450	52.7	1.95	7.19	7.19	7.19	0.80	0.60	± 12.0 %
2600	52.5	2.16	7.14	7.14	7.14	0.80	0.59	± 12.0 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. ^P At frequencies below 3 GHz, the validity of tissue parameters (*z* and *σ*) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (*z* and *σ*) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

EX3DV4-SN:3816

October 3, 2011

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

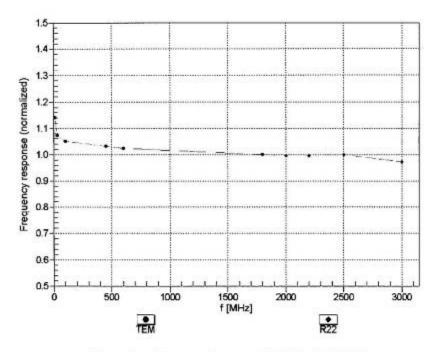





Page 7 of 11

EX3DV4- SN:3816

October 3, 2011

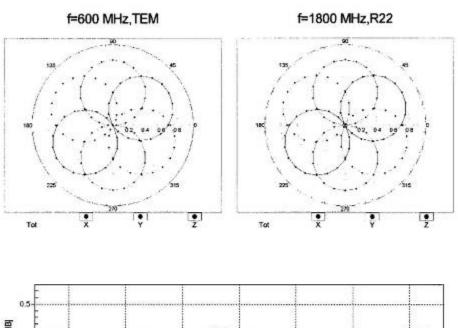

Receiving Pattern (\$), 9 = 0°

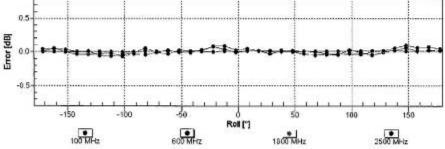

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Page 8 of 11


Report No.: RZA1112-2131SAR01R1

Page 46 of 64

EX3DV4-SN:3816


October 3, 2011

Dynamic Range f(SAR_{head}) (TEM cell , f = 900 MHz)

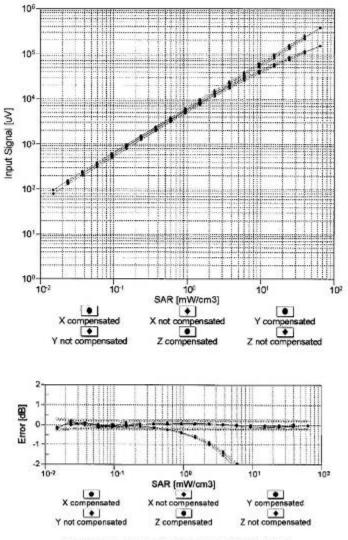

Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: EX3-3816_Oct11

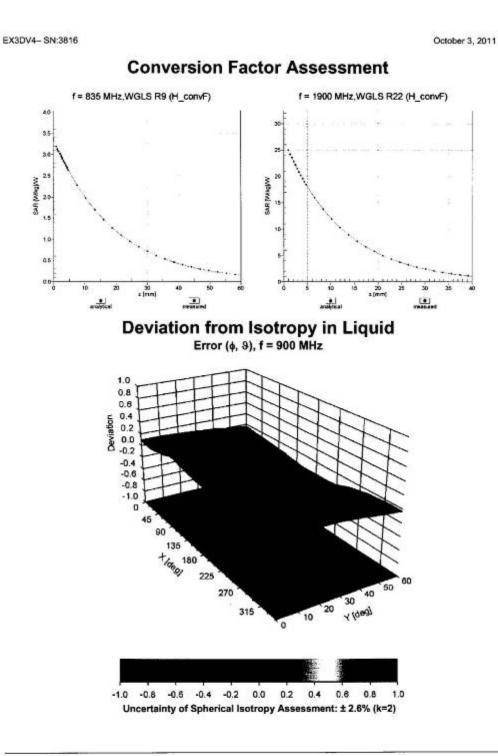

Certificate No: EX3-3816_Oct11

Page 10 of 11

EX3DV4- SN:3816

October 3, 2011

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3816

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 ៣៣
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

Report No.: RZA1112-2131SAR01R1

Page 49 of 64

ANNEX E: D2450V2 Dipole Calibration Certificate

Schmid & Partner Engineering AG eughausstrasse 43, 8004 Zuric	ry of	ILAC MRA (C V Z)	S Schweizerischer Kalibrierdiens Service suisse d'étalonnage Servizio svizzero di taratura S swiss Calibration Service
Accredited by the Swiss Accredit The Swiss Accreditation Servic Multilateral Agreement for the r	e is one of the signatorie	es to the EA	ion No.: SCS 108
CALIBRATION (ACCOUNTS OF A CONTRACTOR OF A CONT	No: D2450V2-786_Aug11
	D2450V2 - SN: 7		
Calibration procedure(s)	QA CAL-05.v8 Calibration proce	dure for dipole validation kits a	bove 700 MHz
Calibration date:	August 29, 2011		
		*	
The measurements and the unce	ertainties with confidence p	ional standards, which realize the physical robability are given on the following pages ry facility: environment temperature (22 ± 3	and are part of the certificate.
The measurements and the unce All calibrations have been condu	ertainties with confidence p	robability are given on the following pages	and are part of the certificate.
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards	ertainties with confidence p cted in the closed laborato TE critical for calibration)	robability are given on the following pages ry facility: environment temperature (22 ± 3 Cal Date (Certificate No.)	and are part of the certificate.
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A	ertainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704	robability are given on the following pages ny facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 06-Oct-10 (No. 217-01266)	and are part of the certificate.)*C and humidity < 70%. Scheduled Calibration Oct-11
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	ertainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783	robability are given on the following pages ny facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 06-Oct-10 (No. 217-01266) 06-Oct-10 (No. 217-01266)	and are part of the certificate.)*C and humidity < 70%. Scheduled Calibration Oct-11 Oct-11
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	ertainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704	robability are given on the following pages ry facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 06-Oct-10 (No. 217-01266) 06-Oct-10 (No. 217-01266) 29-Mar-11 (No. 217-01367)	and are part of the certificate.)*C and humidity < 70%. Scheduled Calibration Oct-11 Oct-11 Apr-12
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination	ertainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: S5086 (20b)	robability are given on the following pages ny facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 06-Oct-10 (No. 217-01266) 06-Oct-10 (No. 217-01266)	and are part of the certificate.)*C and humidity < 70%. Scheduled Calibration Oct-11 Oct-11
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: S5086 (20b) SN: 5047.2 / 06327	robability are given on the following pages ry facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 06-Oct-10 (No. 217-01266) 06-Oct-10 (No. 217-01266) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01371)	and are part of the certificate.)*C and humidity < 70%. Scheduled Calibration Oct-11 Oct-11 Apr-12 Apr-12 -
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: S5086 (20b) SN: S5086 (20b) SN: S5086 (20b) SN: S507.2 / 06327 SN: 3205 SN: 601	robability are given on the following pages ry facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 06-Oct-10 (No. 217-01266) 06-Oct-10 (No. 217-01266) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01371) 29-Apr-11 (No. ES3-3205_Apr11) 04-Jul-11 (No. DAE4-601_Jul11)	and are part of the certificate.)*C and humidity < 70%. Scheduled Calibration Oct-11 Oct-11 Apr-12 Apr-12 Apr-12 Jul-12
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: S5086 (20b) SN: 5047.2 / 06327 SN: 3205 SN: 601	robability are given on the following pages ry facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 06-Oct-10 (No. 217-01266) 06-Oct-10 (No. 217-01266) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01371) 29-Apr-11 (No. ES3-3205_Apr11) 04-Jul-11 (No. DAE4-601_Jul11) Check Date (in house)	and are part of the certificate.)*C and humidity < 70%. Scheduled Calibration Oct-11 Oct-11 Apr-12 Apr-12 Apr-12 Jul-12 Scheduled Check
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: S5086 (20b) SN: S5086 (20b) SN: S5086 (20b) SN: S507.2 / 06327 SN: 3205 SN: 601	robability are given on the following pages ry facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 06-Oct-10 (No. 217-01266) 06-Oct-10 (No. 217-01266) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01371) 29-Apr-11 (No. ES3-3205_Apr11) 04-Jul-11 (No. DAE4-601_Jul11)	and are part of the certificate.)*C and humidity < 70%. Scheduled Calibration Oct-11 Oct-11 Apr-12 Apr-12 Apr-12 Jul-12
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: S5086 (20b) SN: 5047.2 / 06327 SN: 3205 SN: 601 = ID # MY41092317	robability are given on the following pages ry facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 06-Oct-10 (No. 217-01266) 06-Oct-10 (No. 217-01266) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01371) 29-Apr-11 (No. ES3-3205_Apr11) 04-Jul-11 (No. DAE4-601_Jul11) Check Date (in house) 18-Oct-02 (in house check Oct-09)	and are part of the certificate.)*C and humidity < 70%. Scheduled Calibration Oct-11 Oct-11 Apr-12 Apr-12 Apr-12 Jul-12 Scheduled Check In house check: Oct-11
The measurements and the unce	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 55086 (20b) SN: 55047.2 / 06327 SN: 3205 SN: 601 = ID # MY41092317 100005	Cal Date (Certificate No.) 06-Oct-10 (No. 217-01266) 06-Oct-10 (No. 217-01266) 06-Oct-10 (No. 217-01266) 08-Oct-10 (No. 217-01266) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01371) 29-Apr-11 (No. 217-01371) 29-Apr-11 (No. 253-3205_Apr11) 04-Jul-11 (No. DAE4-601_Jul11) Check Date (in house) 18-Oct-02 (in house check Oct-09) 04-Aug-99 (in house check Oct-09) 18-Oct-01 (in house check Oct-10)	and are part of the certificate.)*C and humidity < 70%. Scheduled Calibration Oct-11 Oct-11 Oct-11 Apr-12 Apr-12 Jul-12 Scheduled Check In house check: Oct-11 In house check: Oct-11 In house check: Oct-11
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 55086 (20b) SN: 55047.2 / 06327 SN: 3205 SN: 601 ID # ID # MY41092317 100005 US37390585 S4206	robability are given on the following pages ry facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 06-Oct-10 (No. 217-01266) 06-Oct-10 (No. 217-01266) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01371) 29-Apr-11 (No. ES3-3205_Apr11) 04-Jul-11 (No. DAE4-601_Jul11) Check Date (in house) 18-Oct-02 (in house check Oct-09) 04-Aug-99 (in house check Oct-09)	and are part of the certificate.)*C and humidity < 70%. Scheduled Calibration Oct-11 Oct-11 Apr-12 Apr-12 Apr-12 Jul-12 Scheduled Check In house check: Oct-11 In house check: Oct-11

Certificate No: D2450V2-786_Aug11

Page 1 of 8

Report No.: RZA1112-2131SAR01R1

Page 50 of 64

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



SHISS CRUBRATO

s

С

s

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D2450V2-786_Aug11

Report No.: RZA1112-2131SAR01R1

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.4 ± 6 %	1.85 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.7 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	53.8 mW /g ± 17.0 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured	condition 250 mW input power	6.41 mW / g

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mhơ/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.8 ± 6 %	2.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.2 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	51.7 mW / g ± 17.0 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR averaged over 10 cm ³ (10 g) of Body TSL SAR measured	condition 250 mW input power	6.10 mW / g

Certificate No: D2450V2-786_Aug11

Report No.: RZA1112-2131SAR01R1

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	55.0 Ω + 2.4 jΩ		
Return Loss	- 25.5 dB		

Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.4 Ω + 3.5 jΩ		
Return Loss	- 29.0 dB		

General Antenna Parameters and Design

Electrical Delay (one direction)	1.154 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG		
Manufactured on	May 06, 2005		

Page 4 of 8

Report No.: RZA1112-2131SAR01R1


Page 53 of 64

DASY5 Validation Report for Head TSL Date: 29.08.2011 Test Laboratory: SPEAG, Zurich, Switzerland DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 786 Communication System: CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz; σ = 1.85 mho/m; ε_r = 38.4; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY52 Configuration: Probe: ES3DV3 - SN3205; ConvF(4.45, 4.45, 4.45); Calibrated: 29.04.2011 Sensor-Surface: 3mm (Mechanical Surface Detection) Electronics: DAE4 Sn601; Calibrated: 04.07.2011 Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 101.5 V/m; Power Drift = 0.06 dB Peak SAR (extrapolated) = 28.303 W/kg SAR(1 g) = 13.7 mW/g; SAR(10 g) = 6.41 mW/g Maximum value of SAR (measured) = 17.561 mW/g




0 dB = 17.560 mW/g

Certificate No: D2450V2-786_Aug11

Page 5 of 8


Report No.: RZA1112-2131SAR01R1

Page 54 of 64

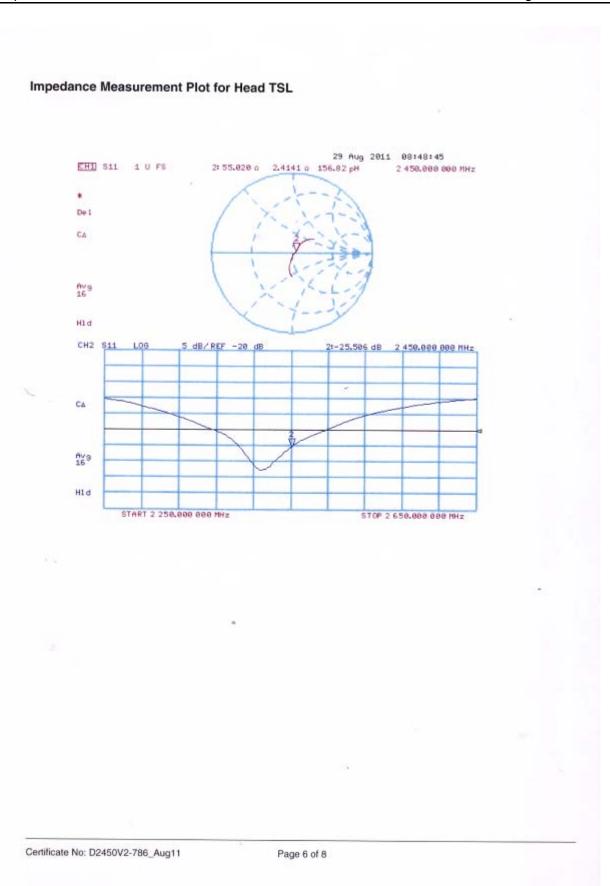


Report No.: RZA1112-2131SAR01R1

Page 55 of 64

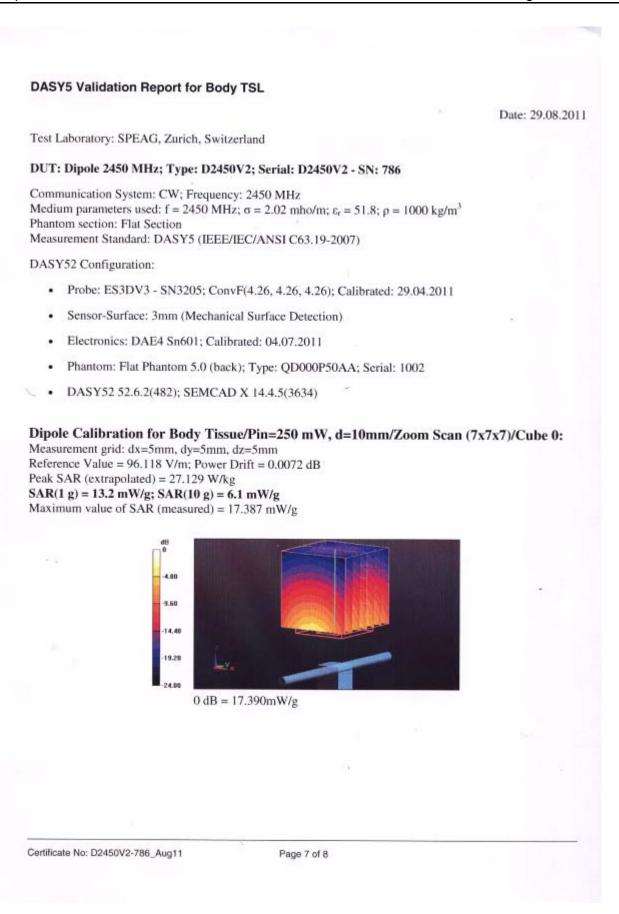

Report No.: RZA1112-2131SAR01R1

Page 56 of 64

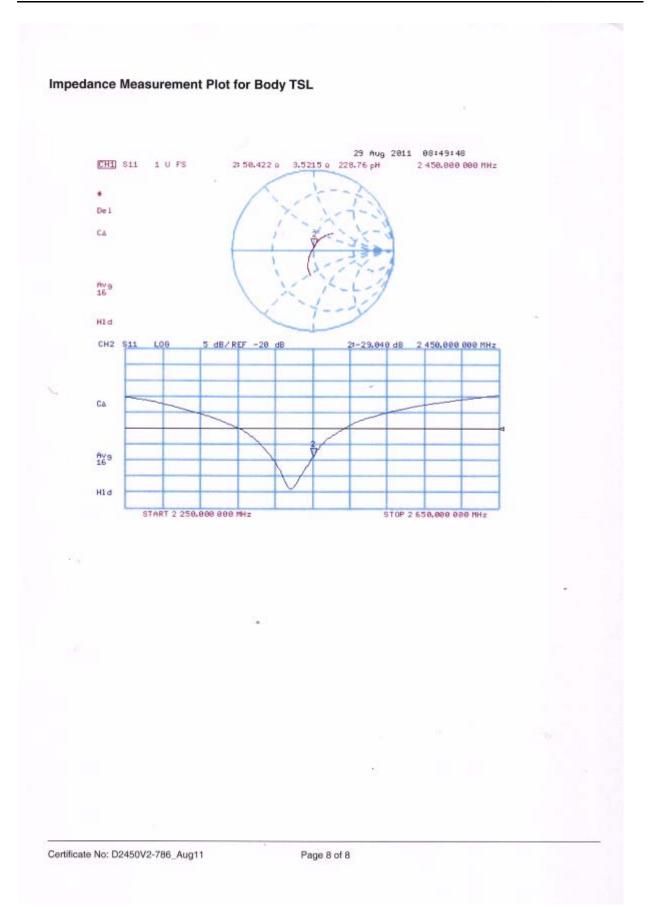

Report No.: RZA1112-2131SAR01R1

Page 57 of 64

ANNEX F: DAE4 Calibration Certificate

Calibration Laboratory Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurict	-	BC MRA	WISS Z BRAT	 S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service
Accredited by the Swiss Accredita The Swiss Accreditation Service Multilateral Agreement for the re	is one of the signatories		Accreditat	tion No.: SCS 108
Client TA SH (Audei			Certificate	• No: DAE4-871_Nov11
CALIBRATION C	 =:11 =(07 411=			
Object	DAE4 - SD 000 D	04 BJ - SN: 871		
Calibration procedure(s)	QA CAL-06.v23 Calibration proces	dure for the data ac	quisition e	lectronics (DAE)
Calibration date:	November 22, 20	n e sage		
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Keithley Multimeter Type 2001	ted in the closed laboratory		perature (22 ±	
Secondary Standards	ID #	Check Date (in house)		Scheduled Check
Calibrator Box V1.1	SE UMS 006 AB 1004	08-Jun-11 (in house che	ck)	In house check: Jun-12
Calibrated by:	• Andrea Cunti	Function Technician		Signature
Approved by:	Fin Bomholt	R&D Direct	×	i.v. Claur
This calibration certificate shall no	t be reproduced except in	full without written approva	I of the laborat	Issued: November 22, 2011 tory.

Certificate No: DAE4-871_Nov11

Report No.: RZA1112-2131SAR01R1

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates



SWISS CP Z Z Prisert

S

С

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Glossary

DAE Connector angle data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle*: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - *Input resistance:* Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - *Power consumption:* Typical value for information. Supply currents in various operating modes.

Report No.: RZA1112-2131SAR01R1

DC Voltage Measurement

A/D - Converter Resolution nominal

 High Range:
 1LSB =
 6.1μ V
 full range =
 -100...+300 mV

 Low Range:
 1LSB =
 61nV
 full range =
 -1.....+3mV

 DASY measurement parameters:
 Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	404.749 ± 0.1% (k=2)	404.733 ± 0.1% (k=2)	405.174 ± 0.1% (k=2)
Low Range	3.98175 ± 0.7% (k=2)	3.93601 ± 0.7% (k=2)	3.96830 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system	90.0 ° ± 1 °

Appendix

1. DC Voltage Linearity

High Range		Reading (µV)	Difference (µV)	Error (%)
Channel X	+ Input	199991.9	-0.91	-0.00
Channel X	+ Input	20000.28	0.48	0.00
Channel X	- Input	-19998.51	0.59	-0.00
Channel Y	+ Input	200003.0	1.24	0.00
Channel Y	+ Input	19999.67	0.17	0.00
Channel Y	- Input	-20000.04	-0.34	0.00
Channel Z	+ Input	200010.1	-0.11	-0.00
Channel Z	+ Input	19999.33	-0.07	-0.00
Channel Z	- Input	-20001.45	-0.85	0.00

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2000.0	0.05	0.00
Channel X + Input	199.81	-0.09	-0.04
Channel X - Input	-199.63	0.37	-0.19
Channel Y + Input	1999.9	-0.22	-0.01
Channel Y + Input	198.81	-1.19	-0.59
Channel Y - Input	-201.62	-1.72	0.86
Channel Z + Input	2000.4	0.48	0.02
Channel Z + Input	199.30	-0.70	-0.35
Channel Z - Input	-200.86	-1.06	0.53

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	14.43	13.13
	- 200 *	-12.22	-13.72
Channel Y	200	-10.07	-9.78
	- 200	9.61	8.66
Channel Z	200	-0.56	-0.83
	- 200	-0.01	0.11

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Υ (μV)	Channel Ζ (μV)
Channel X	200	-	3.08	0.09
Channel Y	200	3.19	-	4.59
Channel Z	200	0.90	-0.06	-

Certificate No: DAE4-871_Nov11

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15920	15519
Channel Y	16179	17567
Channel Z	15791	15270

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	0.03	-1.16	2.66	0.46
Channel Y	-0.63	-3.22	0.29	0.46
Channel Z	-0.87	-2.03	0.28	0.46

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)


Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9


ANNEX G: The EUT Appearances and Test Configuration



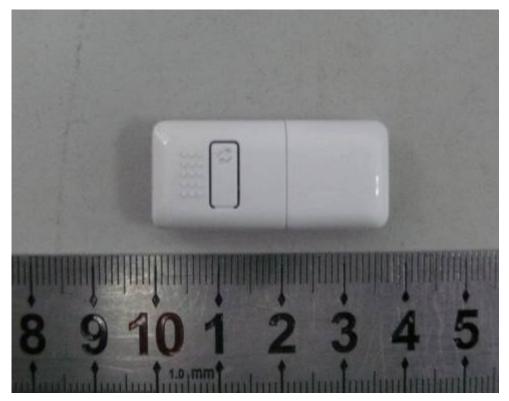


Picture 4: Constituents of EUT


Report No.: RZA1112-2131SAR01R1

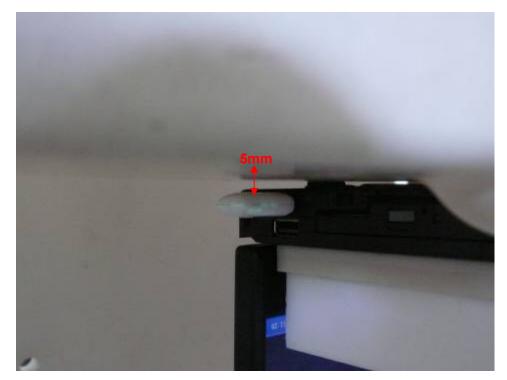

Picture 5: Test position 1

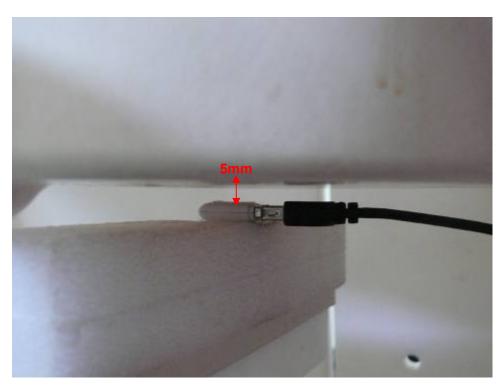

Picture 6: Test position 2

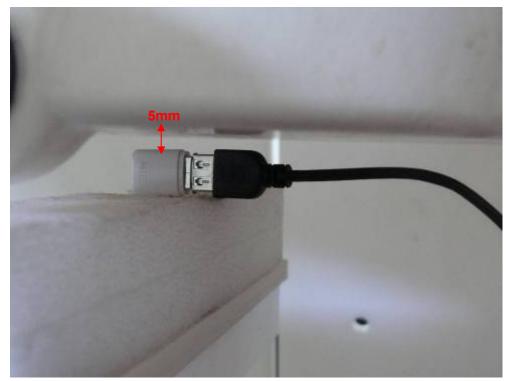

Picture 7: Test Position 3



Picture 8: Test Position 4