

APPENDIX**11. Photographs of Test Setup**

Fig.1 Photograph of the SAR measurement system

Photograph of the tissue simulant fluid liquid depth (Body)

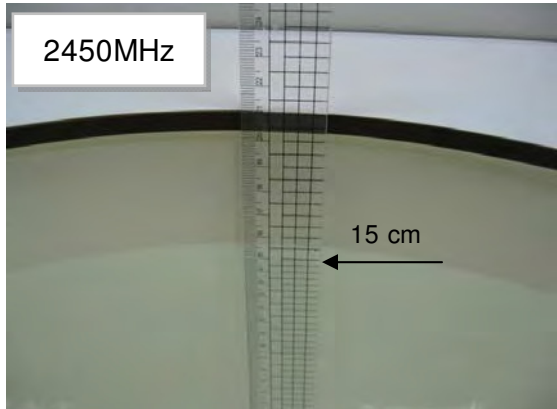


Fig.2.1

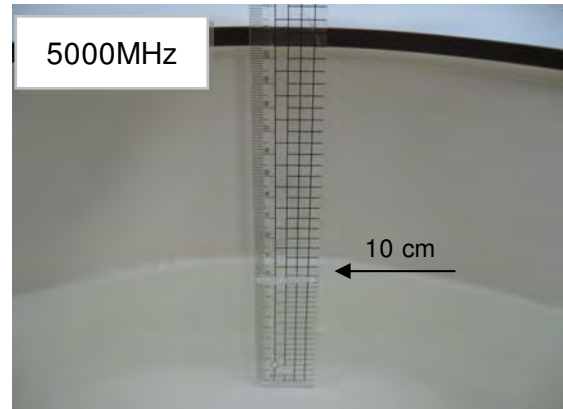


Fig.2.2

Body - distance between flat phantom and EUT is 0 mm

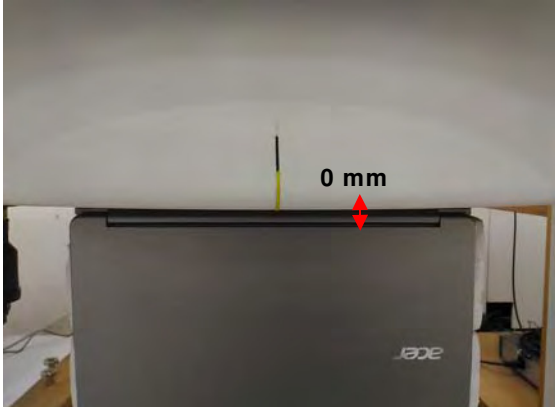


Fig.3 EUT Back side to flat phantom (Laptop mode)

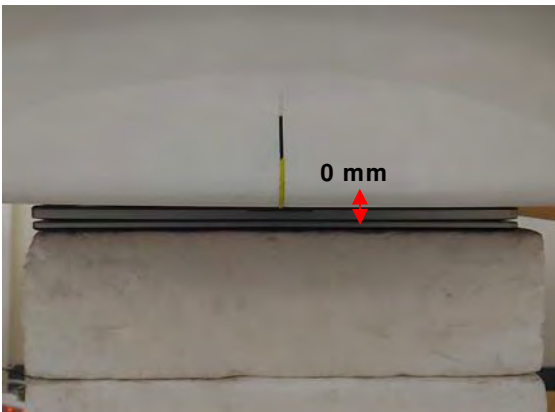


Fig.4 EUT Back side to flat phantom (tablet mode)

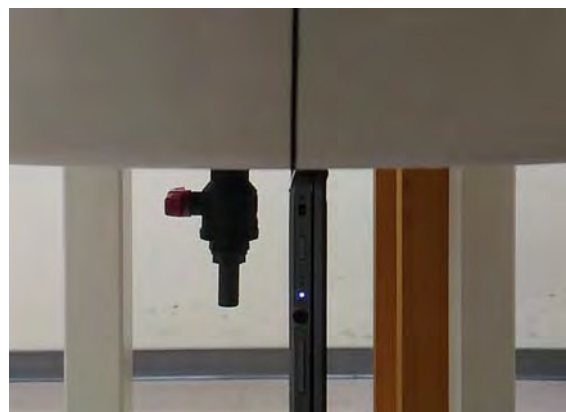
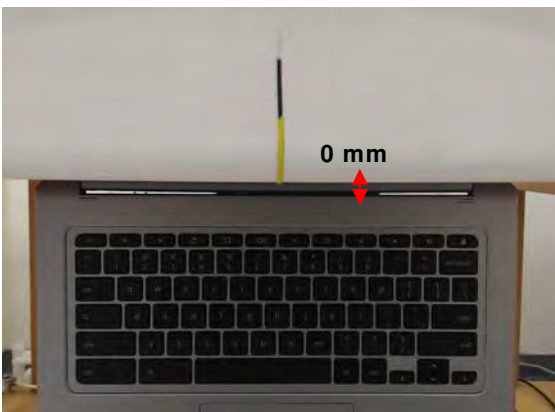


Fig.5 EUT Bottom side to flat phantom (table mode)

12. Photographs of the EUT



Fig.6 Front view of EUT



Fig.7 Back view of EUT

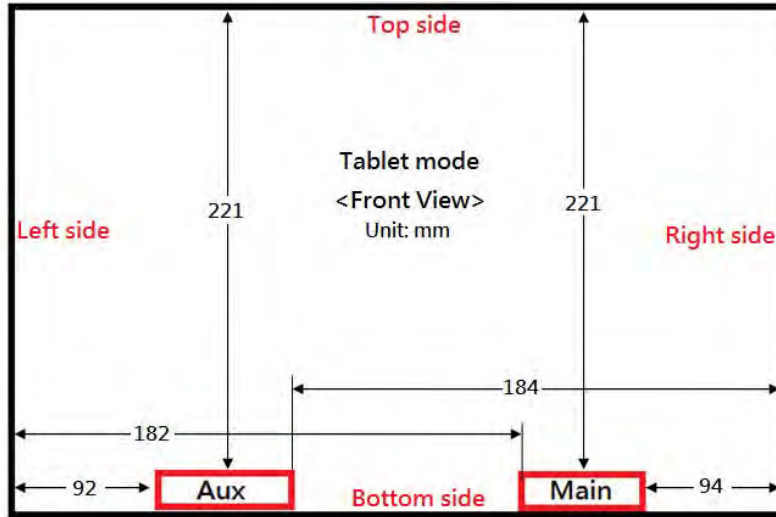


Fig.8 Antenna location of EUT (Tablet mode)

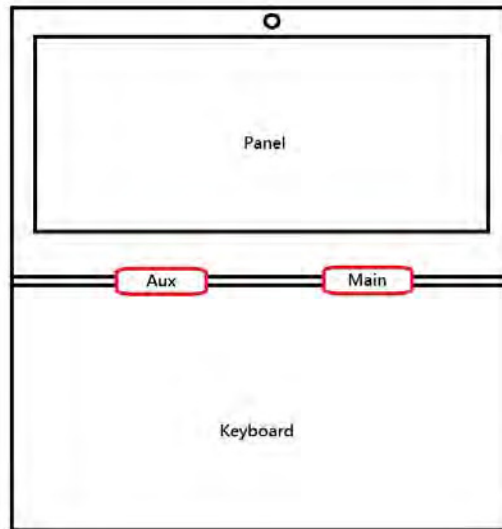


Fig.9 Antenna location of EUT (Laptop mode)

- End of Report -