



## APPENDIX

### 11. Photographs of Test Setup

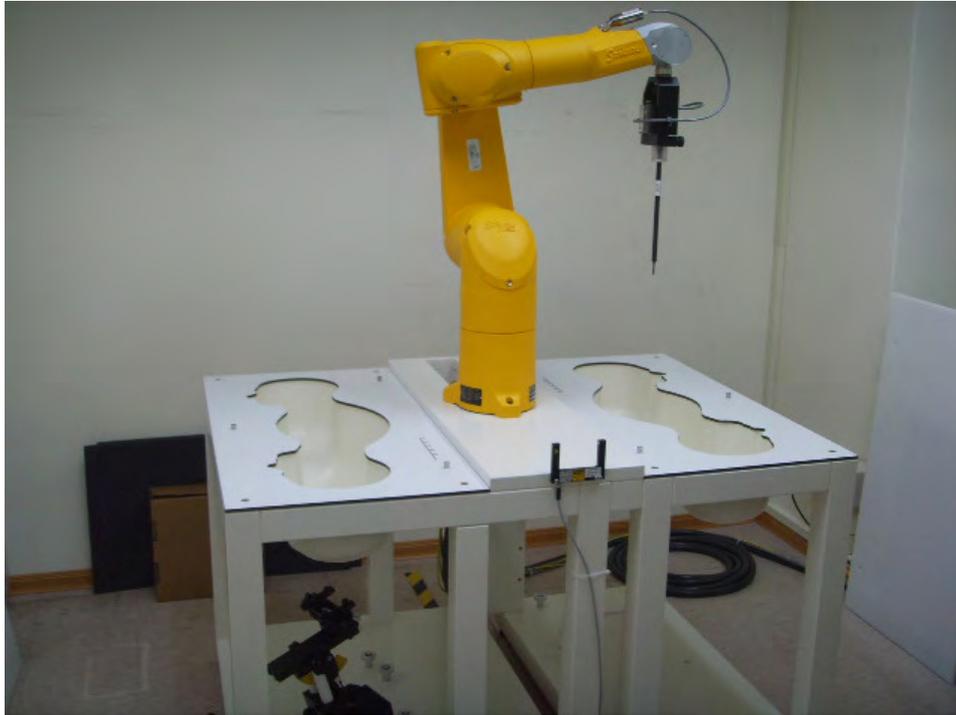

**Fig.1 Photograph of the SAR measurement system**

### Photograph of the Tissue Simulant Fluid Liquid Depth

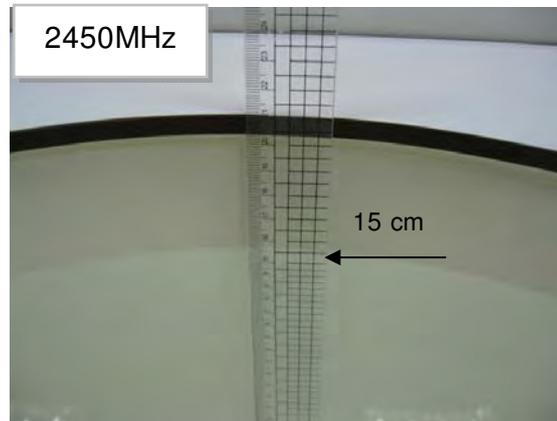

**Fig.2**


**Body - distance between flat phantom and EUT is 0 mm**



**Fig.3 EUT Top side to flat phantom**



**Fig.4 EUT Back side to flat phantom**

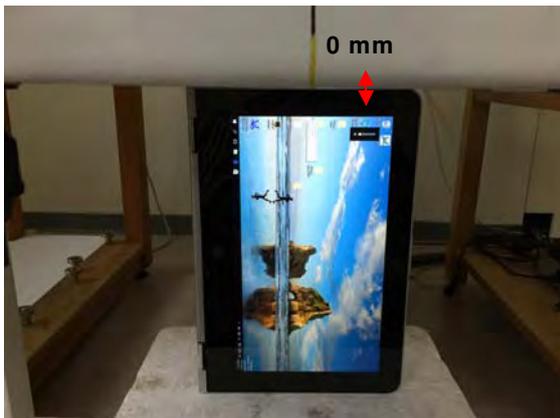

**Fig.5 EUT Left side to flat phantom**

## 12. Photographs of the EUT




**Fig.6 Front view of EUT**



**Fig.7 Back view of EUT**



**Fig.8 Tablet mode of EUT(Front view)**

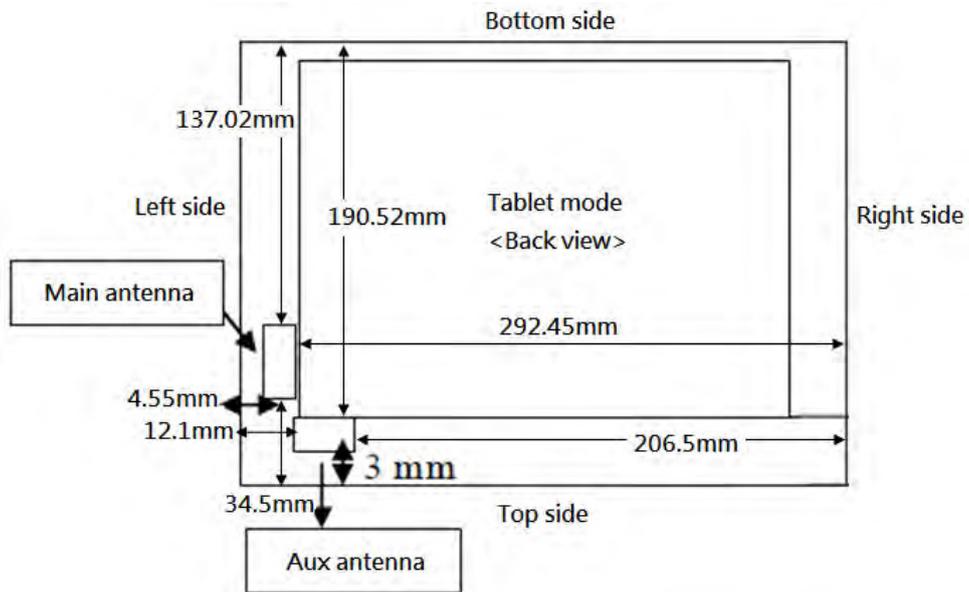

**Fig.9 Antenna position of EUT (Back view of tablet mode)**

- End of Report -