



Rear view of DRYVIEW 5950 Laser Imaging System  
Showing label placement

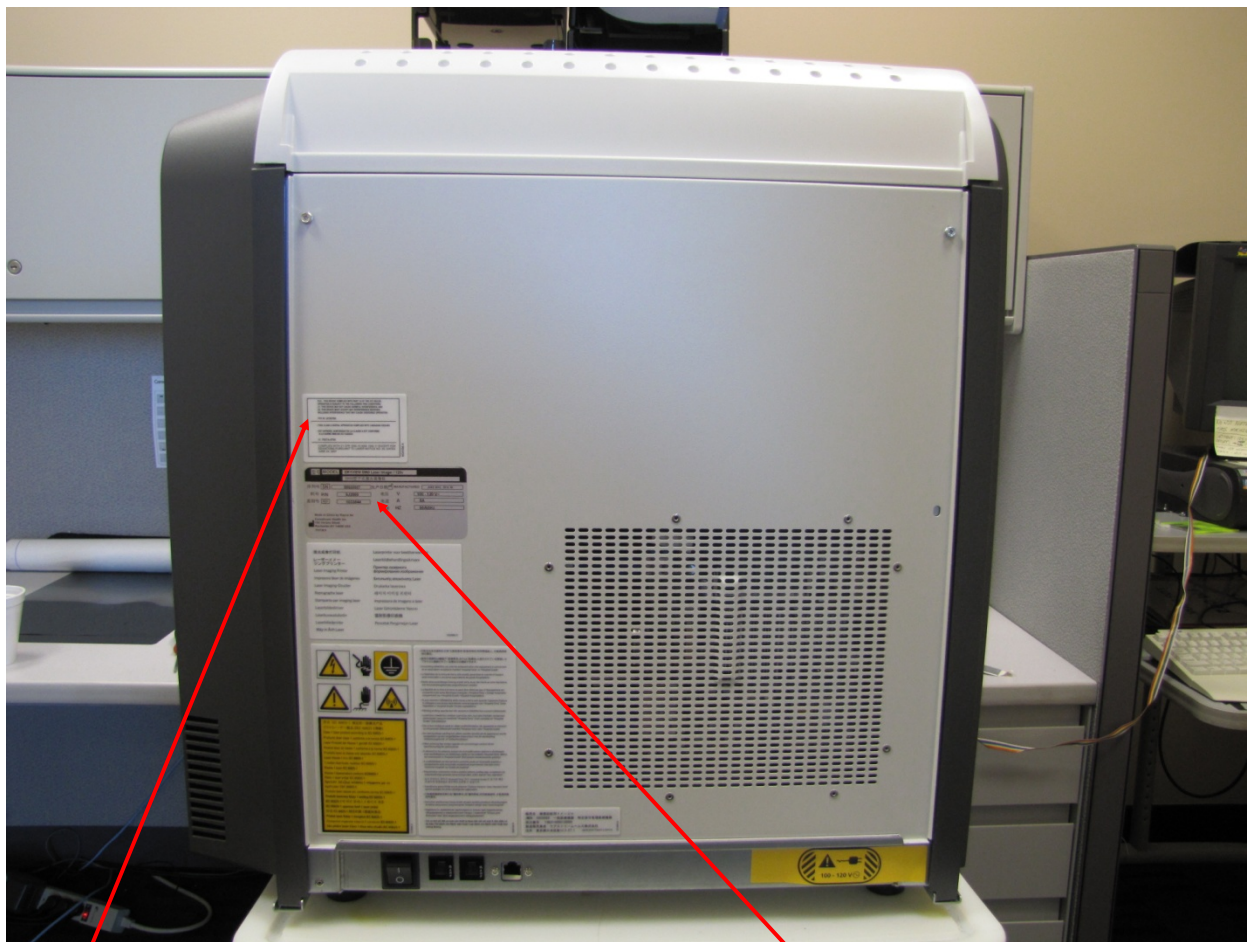

Placement of label with label statement  
FCC ID and IC ID. See page 2 for close-  
up of this label

Placement of label with Model Number &  
company name. See page 3 for close-  
up of this label

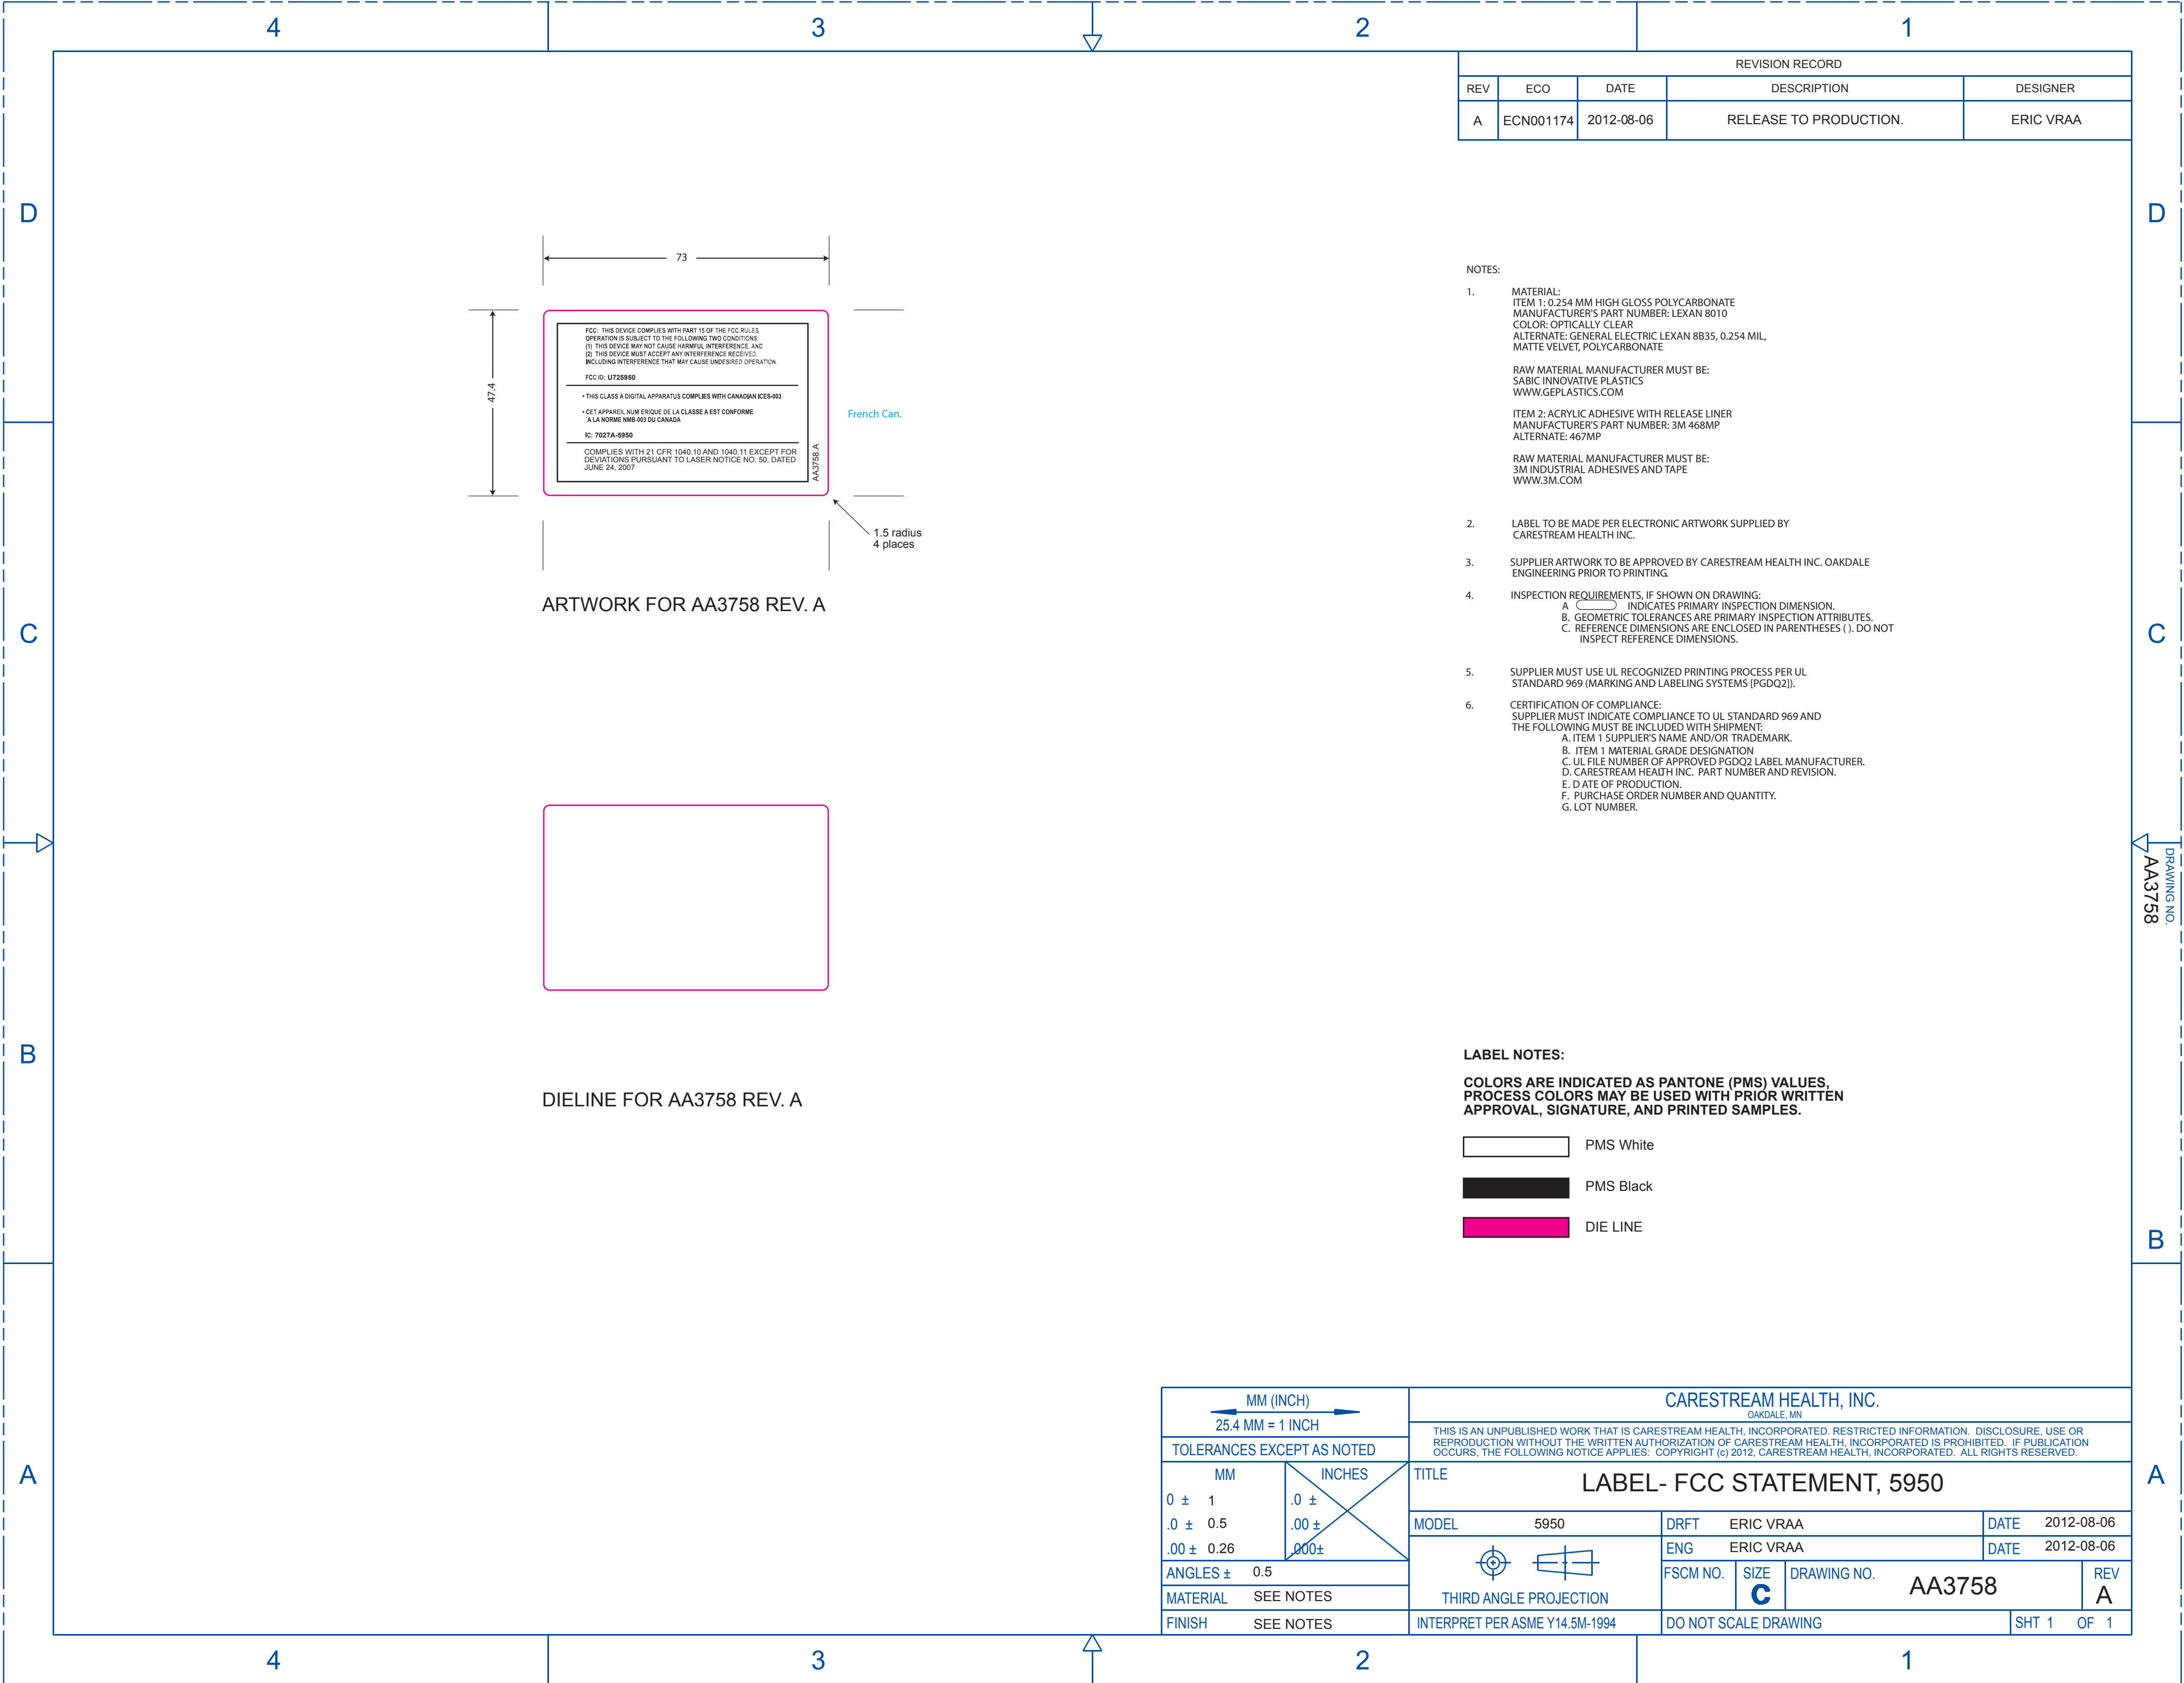

型号 MODEL

DRYVIEW 5950 Laser Imaging System

5950 型干式激光成像仪

序列号 SN

59130050

生产日期  MANUFACTURED Month-yyyy / yymmdd

料号 P/N

9J2001

电压

V

200 - 240 ~

类别号 REF

1033869

B

电流

A

4


频率


Hz

50/60

锐珂（上海）医疗器材有限公司  
上海市浦东新区金桥出口加工区川桥路1510号  
第四、七幢通用厂房 邮编201206

Made in China by Rayco for

 Carestream Health, Inc.  
150 Verona Street  
Rochester, NY 14608  
7F3118.P



沪食药监械（准）字 **2012** 第 1240342 号 （更）  
企业标准号：YZB/沪5120-24A 2012

UL60601-1

