


PACKAGING SPECIFICATION

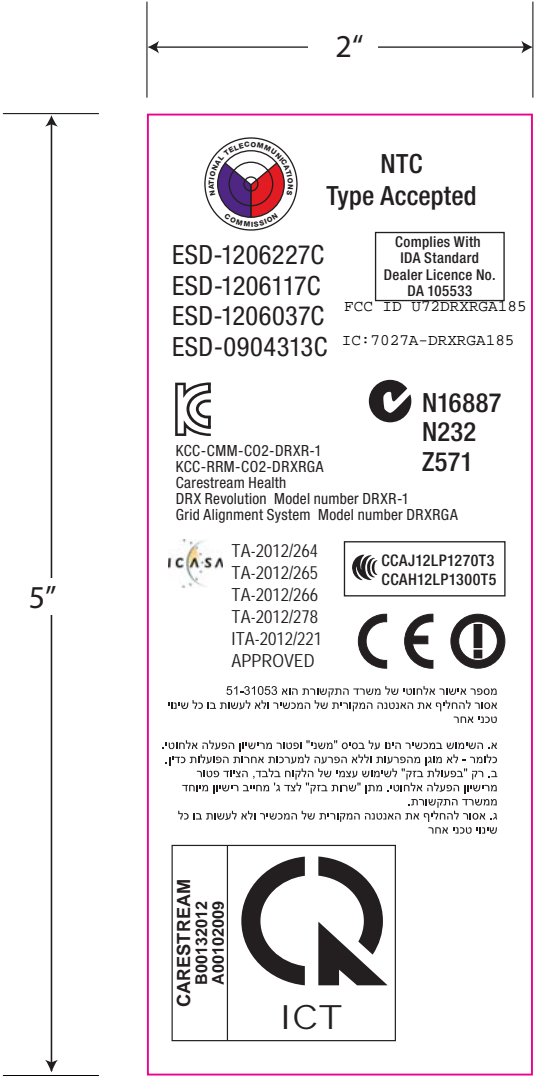

- NOTES:
- 1. MATERIAL: 3M 7815 WITH A 1 MIL CLEAR GLOSS POLYESTER OVERLAMINATE
 - 2. TRIM SIZE: 5" x 2"
 - 3. PRINTING TO BE 4 COLOR PROCESS
 - 4. SHALL SATISFY THE DURABILITY REQUIREMENTS OF UL60601-1

ALL DIMENSIONS IN INCHES, LINEAR TOLERANCES: +/- 0.063. ANGULAR TOLERANCE: +/- 0°. THE FOLLOWING MUST BE ADHERED TO, AS THEY APPLY ON DATE OF MANUFACTURE: ALL CORRUGATED MATERIALS SHALL MEET EKSP-1265 INCLUDING PRINT SUPPLEMENTS AND KAD-X1003; ALL CARTONS MUST SHOW PART NUMBER AND BOX MAKER CERTIFICATE ON BOTTOM OUTSIDE FLAP. ALL PACKAGING MATERIALS SHALL MEET EKSP-0038, PERTAINING TO HEAVY METAL RESTRICTIONS; ALL FOAM MATERIALS SHALL MEET EKSP-1594, PERTAINING TO THE KOREAN DISCHARGE MARK. NO OZONE DEPLETING SUBSTANCES PERMITTED. ALL FOAM ASSEMBLIES TO BE SECURELY BONDED USING COLD GLUE OR EQUIVALENT. NO LOOSENING OR BREAKDOWN OF CELLULAR STRUCTURE PERMITTED. BOND SEPARATION SHOULD RESULT FROM FAILURE OF BONDED MATERIALS ONLY, NOT BONDING AGENT. ALL WOOD COMPONENTS MUST COMPLY WITH ISPM 15, REGARDING PROPER "BUG FREE" TREATMENT AND LABELING. REFER TO BOM FOR MATERIAL SPECIFICATIONS. CARESTREAM HEALTH PACKAGING ENGINEER APPROVAL REQUIRED FOR ANY MATERIAL SUBSTITUTIONS.

NO.		AA4539		REV
SHEET:		1 OF 1		D
REV	CHG. NO. DATE REL	DESCRIPTION		DR BY APPS.
A	2012/09/20	PRODUCTION RELEASE		BATZ
B	2012/11/15	ADDED KCC AND NCC SYMBOLS		BATZ
C	2012/11/20	REVISED KCC SERIAL NUMBER		BATZ
D	2013/06/18	REVISED KCC SERIAL NUMBER		BATZ
CARESTREAM HEALTH, INC. ROCHESTER, NEW YORK				
DRAFTER: D BATZ		ENGINEER: D BATZ	DATE 2012/09/20	
ORIG CHG NUMBER			RELEASED 2012/09/20	
FIRST USED ON DRX-REVOLUTION				
NAME LABEL, WIRELESS CERT <small>AA4539 REV. D</small>				
UNITS: ENGLISH			DWG SIZE A4	
NO. AA4539			REV	
SHEET: 1 OF 1			D	