

4

3


2

1

NOTES

- 1.  DENOTES FIELD TO BE FILLED IN WITH SERIAL NUMBER OR REVISION PER 900-8.5.2.0
- 2. ALL REGULATORY MARKINGS TO BE 6mm OR GREATER. ALL TEXT MUST BE 1mm OR GREATER.
- 3. BARCODE TO CONTAIN SERIAL NUMBER AND BE IN 2-D DATA MATRIX FORMAT
- 4. BARCODE TO BE CENTERED ON LABEL
- 5. PARTS AND COMPONENTS ON THIS DRAWING SHALL BE COMPLIANT WITH ROHS2 DIRECTIVE 2011/65/EU, REACH REGULATION NO.1907/2006 (SEE 900-8.3.2.4 - ENVIRONMENTAL COMPLIANCE REQUIREMENTS GUIDELINES),
- 6. SUPPLIER SHALL BE FULLY COMPLIANT WITH 900-8.4.1.1 - SUPPLIER QUALITY GUIDELINES AND RELATED PROCEDURES UNLESS APPROVED BY CIMS IN WRITING
- 7. PARTS AND COMPONENTS ON THIS DRAWING SHALL BE COMPLIANT TO 900-8.5.1.1 - GENERAL COSMETIC ACCEPTANCE CRITERIA AND INSPECTION REQUIREMENTS, AND 900-8.5.2.0 - IDENTIFICATION AND TRACEABILITY
- 8. DRAWING NOT TO SCALE

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	1	INITIAL DESIGN	1/14/2019	EG
	2	CHANGE DESIGN	2/25/2019	EG

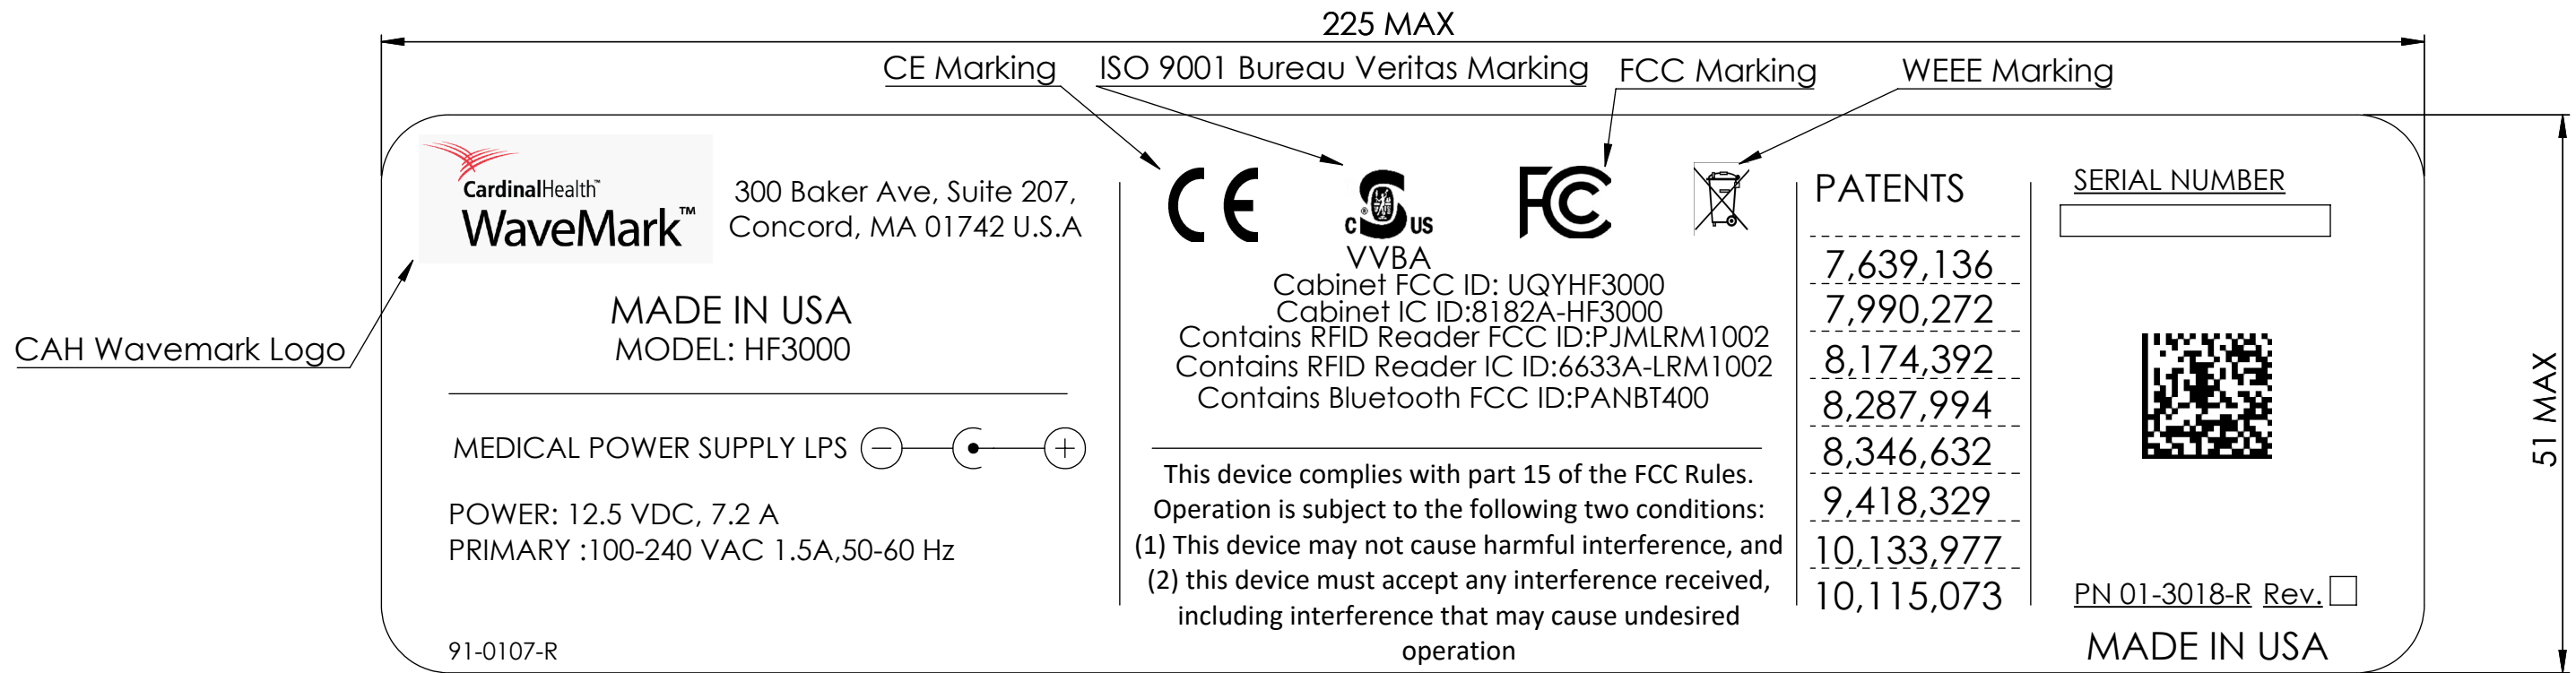

UNLESS OTHERWISE SPECIFIED	PROPRIETARY NOTICE THE INFORMATION CONTAINED IN THIS DRAWING IS THE PROPERTY OF CARDINAL HEALTH INC AND IS CONFIDENTIAL AND PROPRIETARY TO THE COMPANY. IT IS NOT TO BE COPIED OR REPRODUCED IN WHOLE OR IN PART UNLESS AUTHORIZED BY CARDINAL HEALTH INC.	
ALL DIMENSIONS ARE IN MILLIMETERS ALL DIMENSIONS APPLY AFTER FINISH	DO NOT SCALE DRAWING	
STANDARD TOLERANCES X. = ±0.5 X.X = ±0.25 X.XX = ±0.13 CONCENTRICITY .13 TIR	PROJECTION 	
MATERIAL:	APPROVALS	DATE
FINISH:	DRAWN Eli Greenwald	1/14/2019
	CHECKED	
	ENGINEER	

**CardinalHealth**  
300 BAKER AVE, CONCORD, MA 01742

TITLE: Label,Regulatory, HF3000

SIZE B	DOC NO. 91-0107-R	REV 2
SCALE 1:1	SHEET 1 OF 1	

4

3

2

1

D

REV SHEET 1

DOC NO.

C

B

A