

Test Set-up Photos for Draeger Medical job 30862280.004



Figure 1 – Prescans for emissions

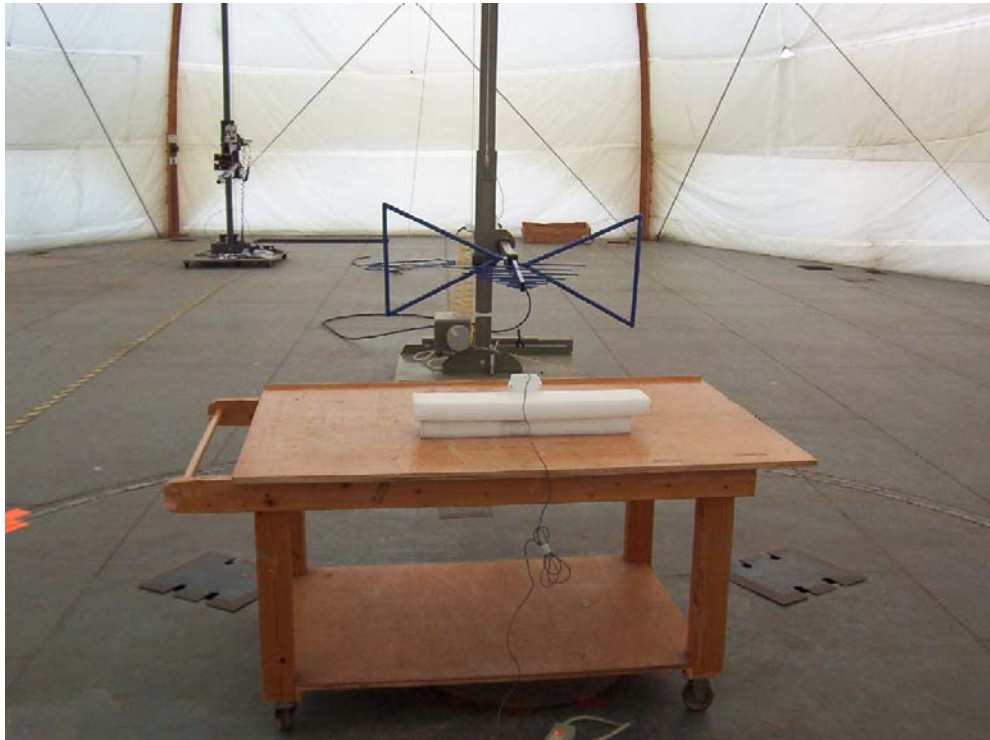


Figure 2 – Finals at OATS



Figure 3 – Conducted Emissions



Figure 4 – Conducted Measurements

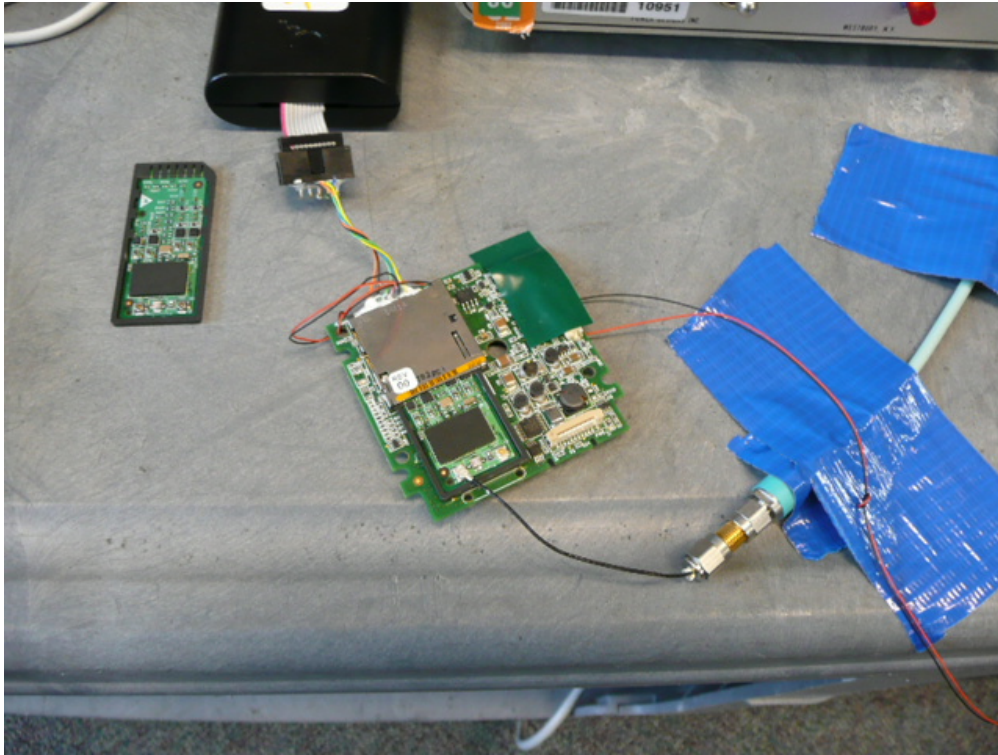


Figure 5 – Conducted Measurements Close up

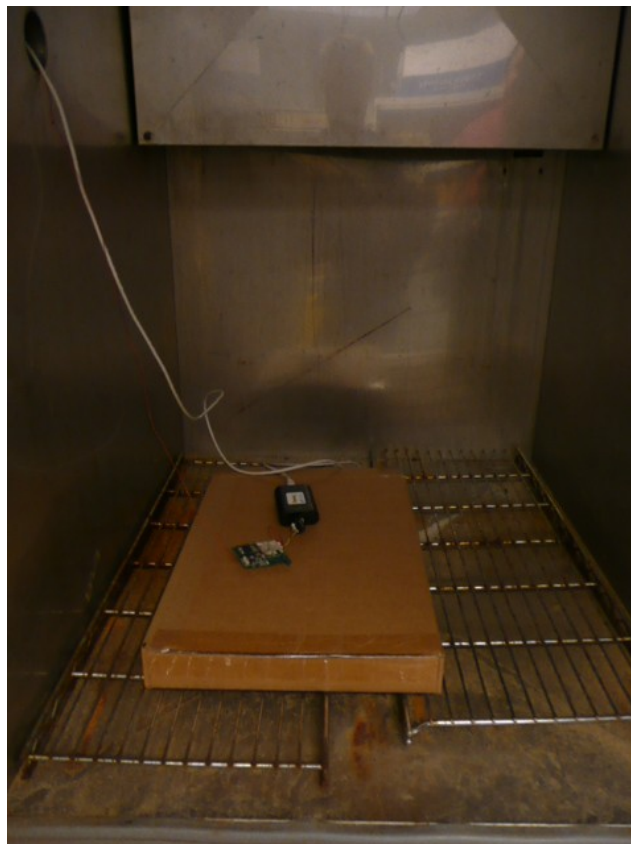


Figure 6 – Temperature Stability