

SystemCheck_750MHz

D750V3-SN:1099

Communication System: D700; Frequency: 750.0

Medium: HSL. Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 43.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7577; ConvF(9.78, 9.78, 9.78); Calibrated: 2021/11/23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2022/04/12
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1233; Section: Flat
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--
- MAIA: Area Scan: N/A; Zoom Scan: N/A


Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.22 W/kg; SAR (10g) = 1.48 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.17 W/kg; SAR (10g) = 1.46 W/kg;

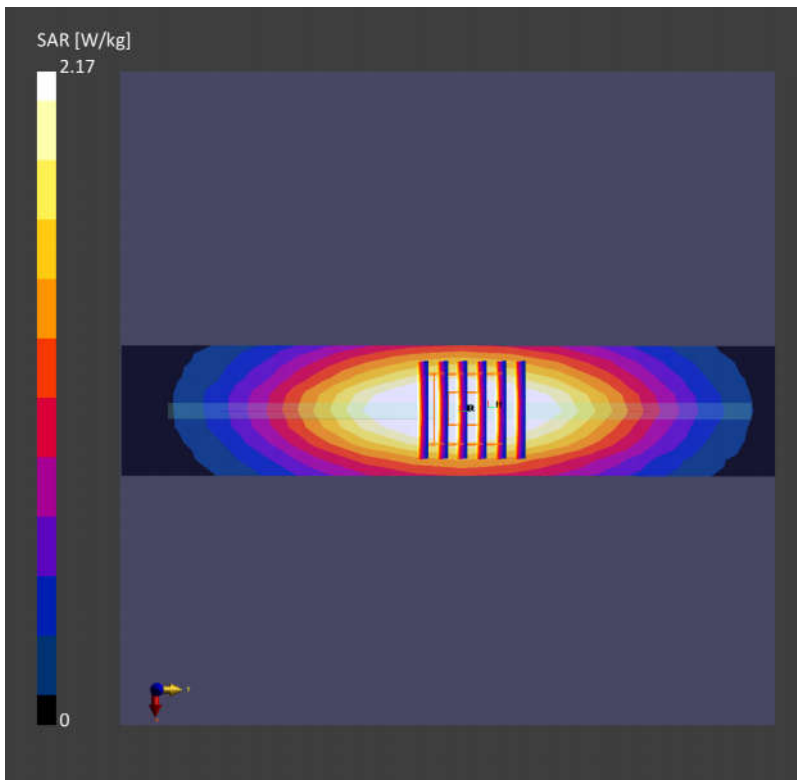

SystemCheck_2600MHz

D2600V2-SN:1070

Communication System: D2600; Frequency: 2600.0

Medium: HSL. Medium parameters used: $f = 2600.0$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7577; ConvF(7.68, 7.68, 7.68); Calibrated: 2021/11/23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2022/04/12
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1233; Section: Flat
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--
- MAIA: Area Scan: N/A; Zoom Scan: N/A

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 13.6 W/kg; SAR (10g) = 6.14 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 13.4 W/kg; SAR (10g) = 6.11 W/kg;

