

System Check_Head_750MHz

DUT: D750V3-SN:1087

Communication System: ; Frequency: 750.0

Medium: HSL. Medium parameters used: $f= 750.0$ MHz; $\sigma= 0.924$ S/m; $\epsilon_r = 42.1$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(10.86, 10.86, 10.86); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.408 W/kg; SAR (10g) = 0.273 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.02 dB

SAR (1g) = 0.409 W/kg; SAR (10g) = 0.273 W/kg;

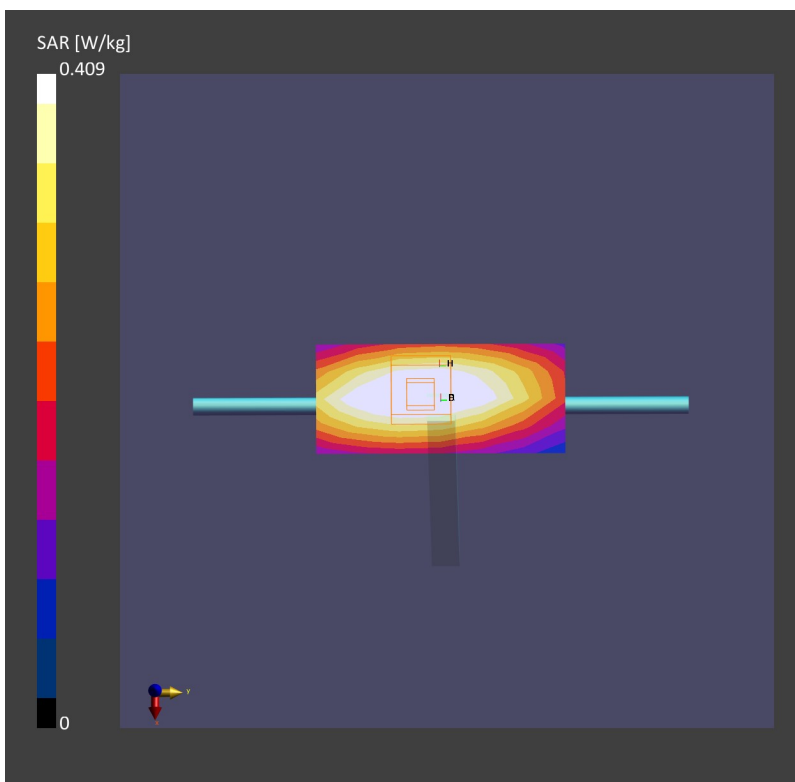

System Check_Head_835MHz

DUT: D835V2-SN:4d162

Communication System: ; Frequency: 835.0

Medium: HSL. Medium parameters used: $f= 835.0$ MHz; $\sigma= 0.911$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(10.57,10.57, 10.57); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.433 W/kg; SAR (10g) = 0.284 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.03 dB

SAR (1g) = 0.455 W/kg; SAR (10g) = 0.293 W/kg;

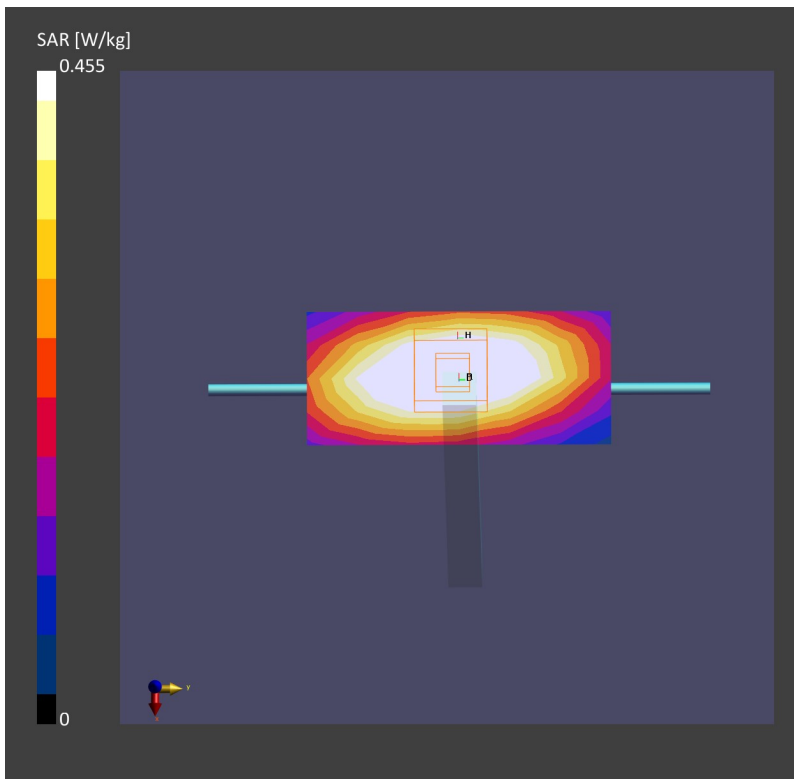

System Check_Head_1750MHz

DUT: D1750V2-SN:1090

Communication System: ; Frequency: 1750.0

Medium: HSL. Medium parameters used: $f= 1750.0$ MHz; $\sigma= 1.34$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.22, 9.22, 9.22); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.73 W/kg; SAR (10g) = 0.896 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.01 dB

SAR (1g) = 1.76 W/kg; SAR (10g) = 0.923 W/kg;

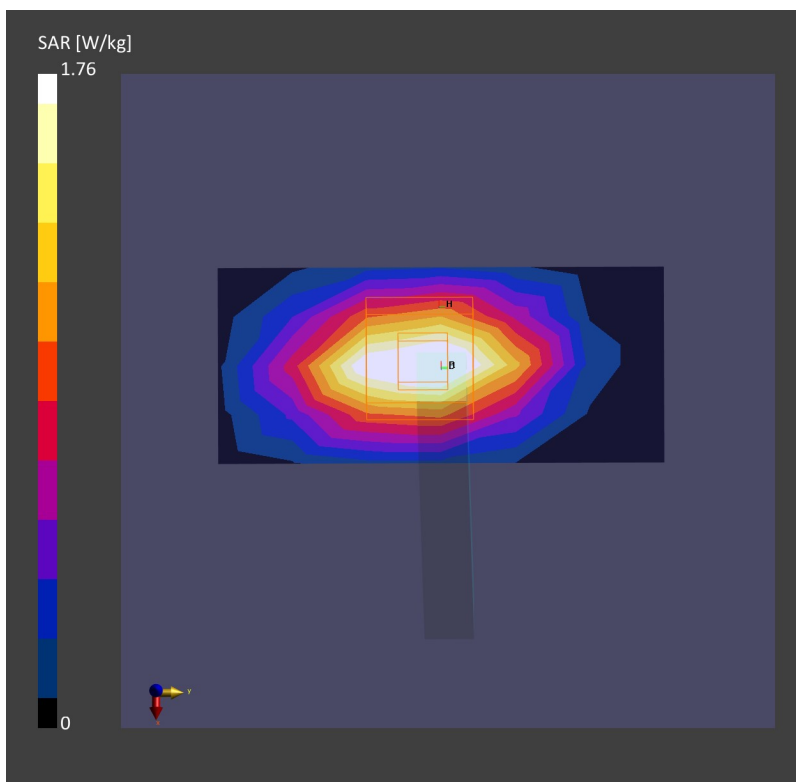

System Check_Head_1900MHz

DUT: D1900V2-SN:5d182

Communication System: ; Frequency: 1900.0

Medium: HSL. Medium parameters used: $f= 1900.0$ MHz; $\sigma= 1.40$ S/m; $\epsilon_r = 41.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.8, 8.8, 8.8); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.971 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.06 dB

SAR (1g) = 1.92 W/kg; SAR (10g) = 0.995 W/kg;

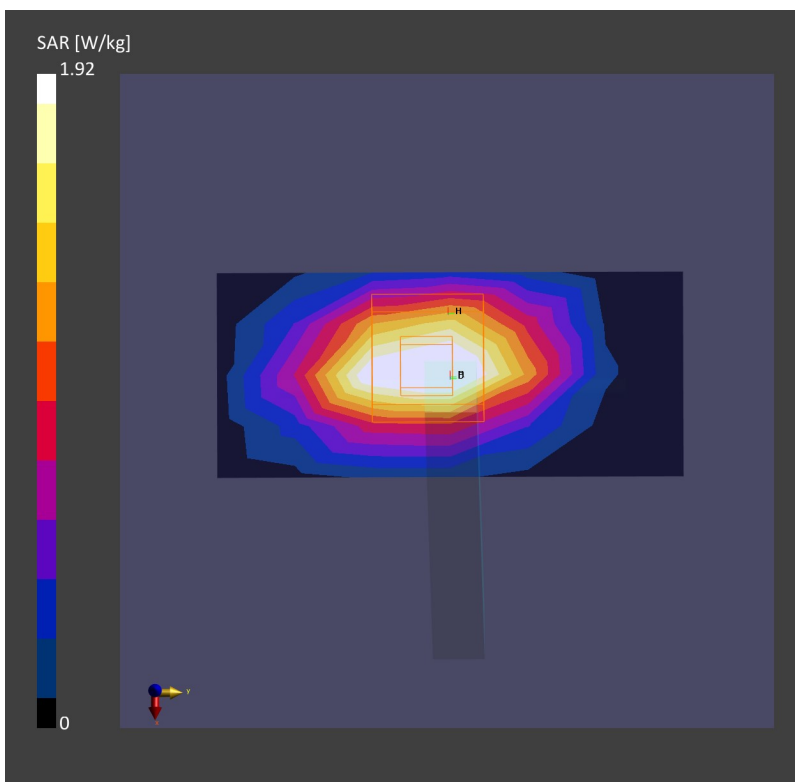

System Check_Head_2450MHz

DUT: D2450V2-SN:1040

Communication System: ; Frequency: 2450.0

Medium: HSL. Medium parameters used: $f= 2450.0$ MHz; $\sigma= 1.81$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.29, 8.29, 8.29); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.49 W/kg; SAR (10g) = 1.15 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = -0.06 dB

SAR (1g) = 2.62 W/kg; SAR (10g) = 1.25 W/kg;

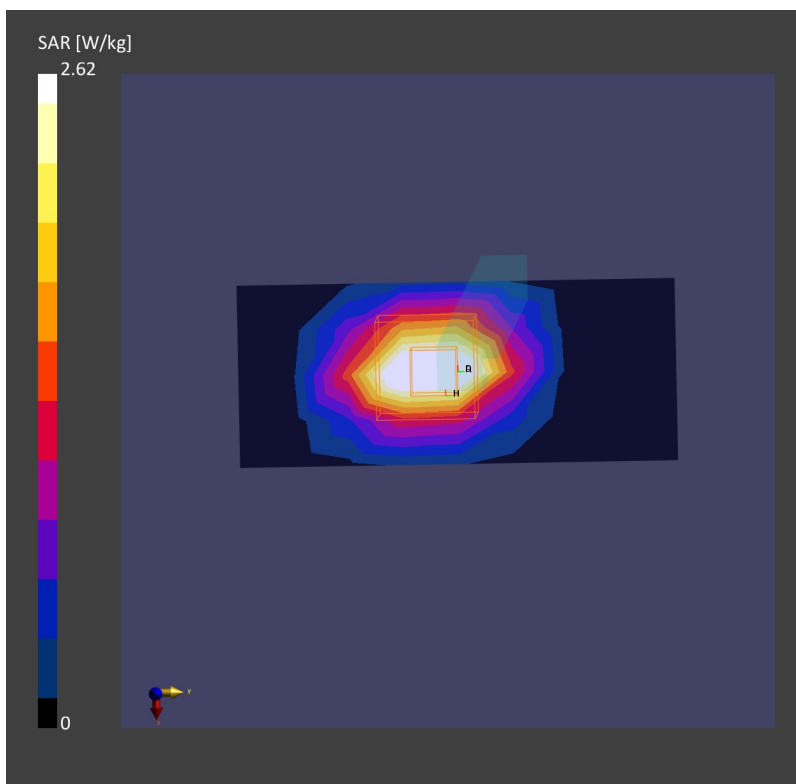

System Check_Head_2600MHz

DUT: D2600V2-SN:1061

Communication System: ; Frequency: 2600.0

Medium: HSL. Medium parameters used: $f= 2600.0$ MHz; $\sigma= 2.03$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.02, 8.02, 8.02); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.58 W/kg; SAR (10g) = 1.18 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = -0.07 dB

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.21 W/kg;

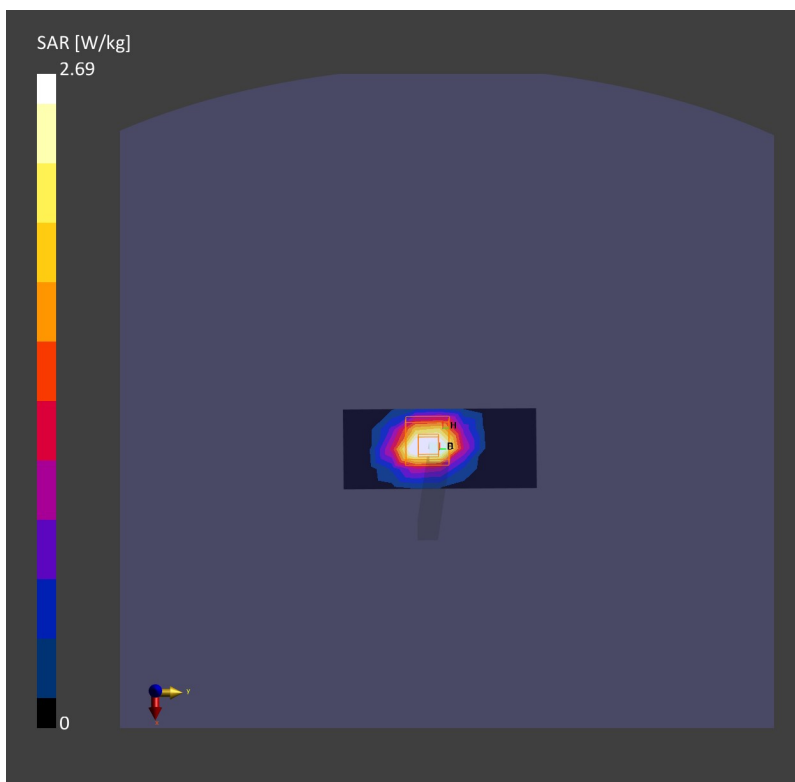

System Check_Head_2600MHz

DUT: D2600V2-SN:1061

Communication System: ; Frequency: 2600.0

Medium: HSL. Medium parameters used: $f= 2600.0$ MHz; $\sigma= 1.93$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.02, 8.02, 8.02); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.58 W/kg; SAR (10g) = 1.15 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = -0.05 dB

SAR (1g) = 2.71 W/kg; SAR (10g) = 1.23 W/kg;

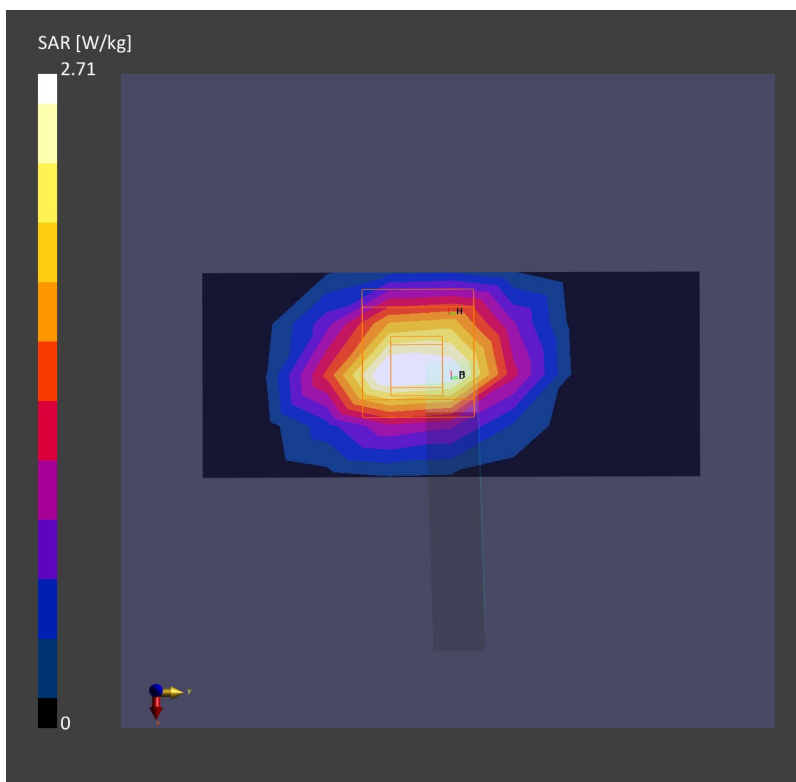

System Check_Head_3500MHz

DUT: D3500V2-SN:1037

Communication System: ; Frequency: 3500.0

Medium: HSL. Medium parameters used: $f= 3500.0$ MHz; $\sigma= 2.78$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.55, 7.55, 7.55); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.13 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.32 W/kg; SAR (10g) = 1.28 W/kg;

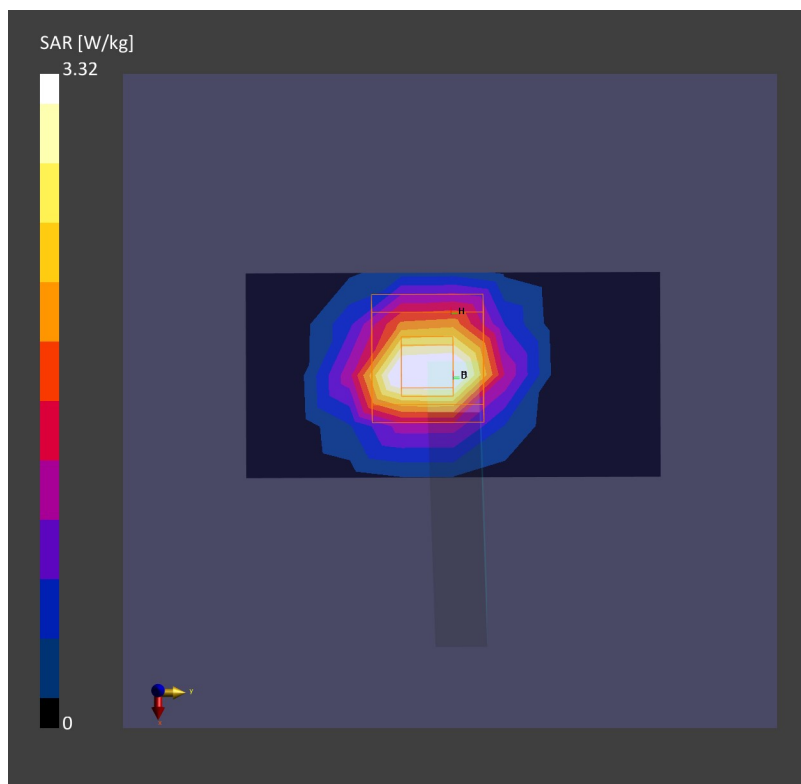

System Check_Head_3700MHz

DUT: D3700V2-SN:1008

Communication System: ; Frequency: 3700.0

Medium: HSL. Medium parameters used: $f= 3700.0$ MHz; $\sigma= 3.14$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.5, 7.5, 7.5); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.10 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.06 dB

SAR (1g) = 3.41 W/kg; SAR (10g) = 1.18 W/kg;

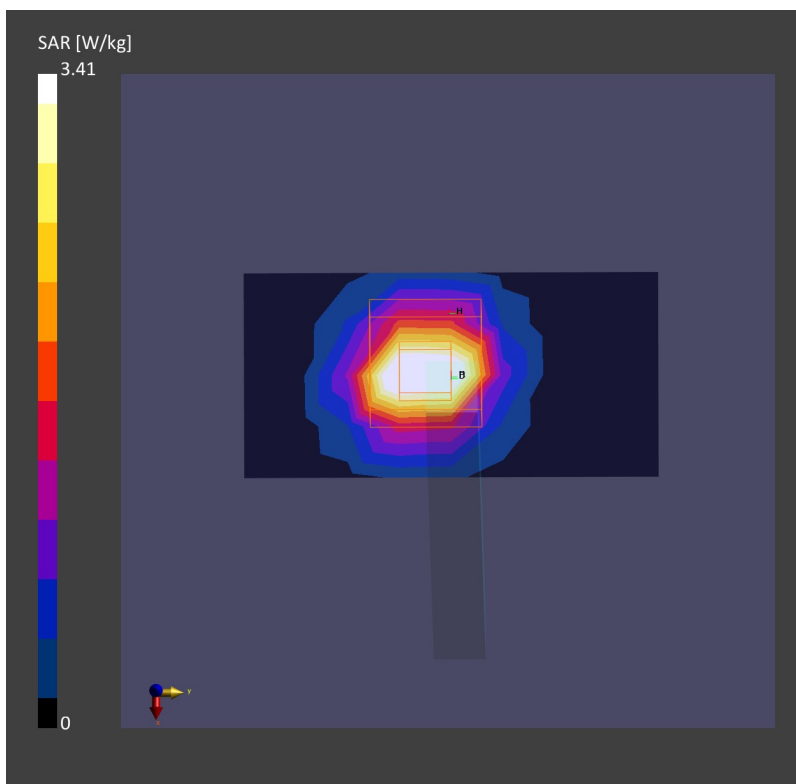

System Check_Head_3900MHz

DUT: D3900V2-SN:1048

Communication System: ; Frequency: 3900.0

Medium: HSL. Medium parameters used: $f= 3900.0$ MHz; $\sigma= 3.31$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.2, 7.2, 7.2); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.33 W/kg; SAR (10g) = 1.08 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.04 dB

SAR (1g) = 3.51 W/kg; SAR (10g) = 1.22 W/kg;

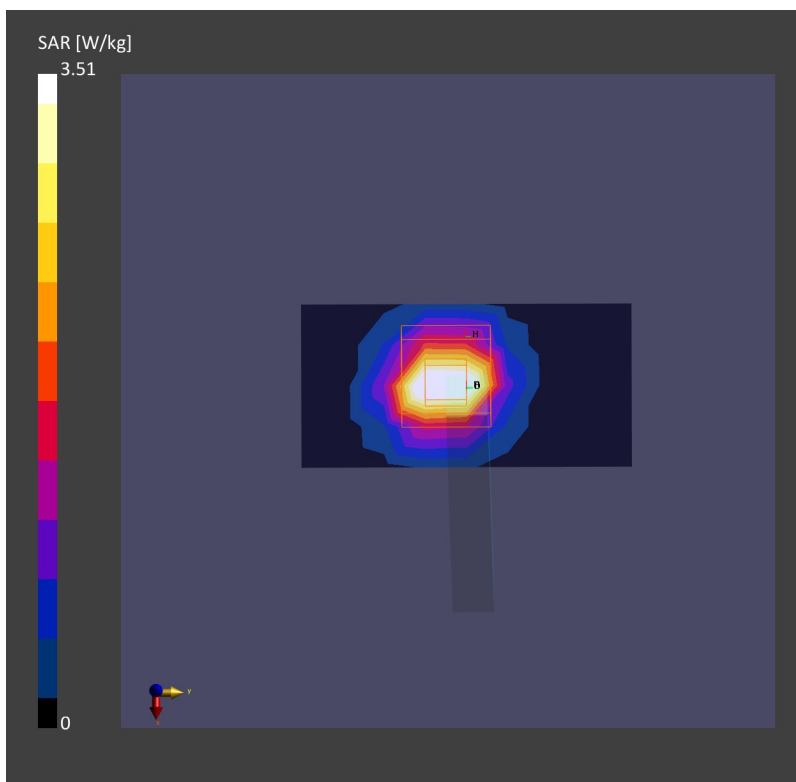

System Check_Head_5250MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5250.0

Medium: HSL. Medium parameters used: $f= 5250.0$ MHz; $\sigma= 4.55$ S/m; $\epsilon_r = 36.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.07, 6.07, 6.07); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.78 W/kg; SAR (10g) = 1.08 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.05 dB

SAR (1g) = 3.82 W/kg; SAR (10g) = 1.18 W/kg;

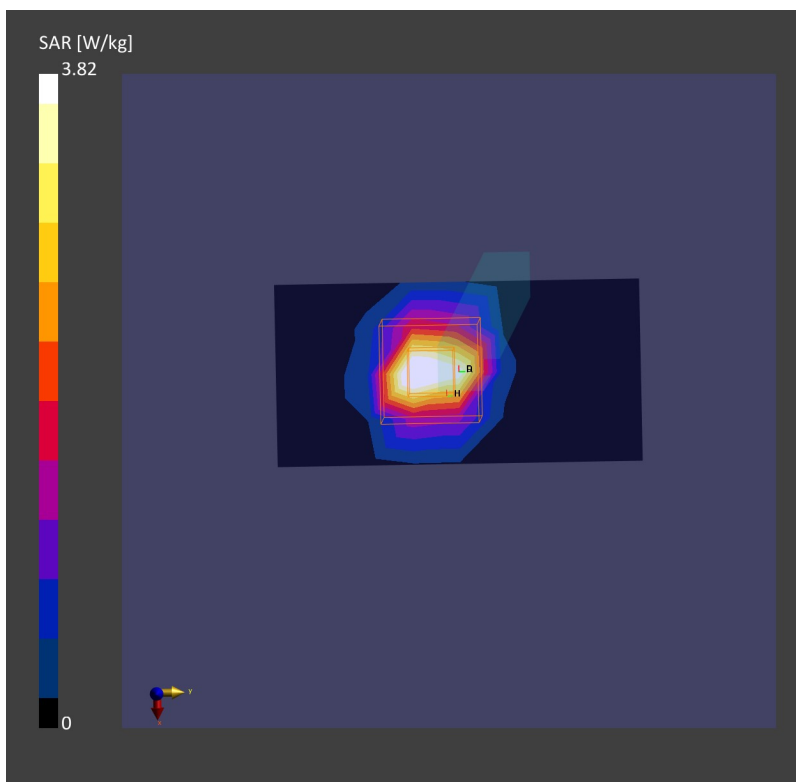

System Check_Head_5600MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5600.0

Medium: HSL. Medium parameters used: $f= 5600.0$ MHz; $\sigma= 4.93$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.3, 5.3, 5.3); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.93 W/kg; SAR (10g) = 1.03 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 4.06 W/kg; SAR (10g) = 1.16 W/kg;

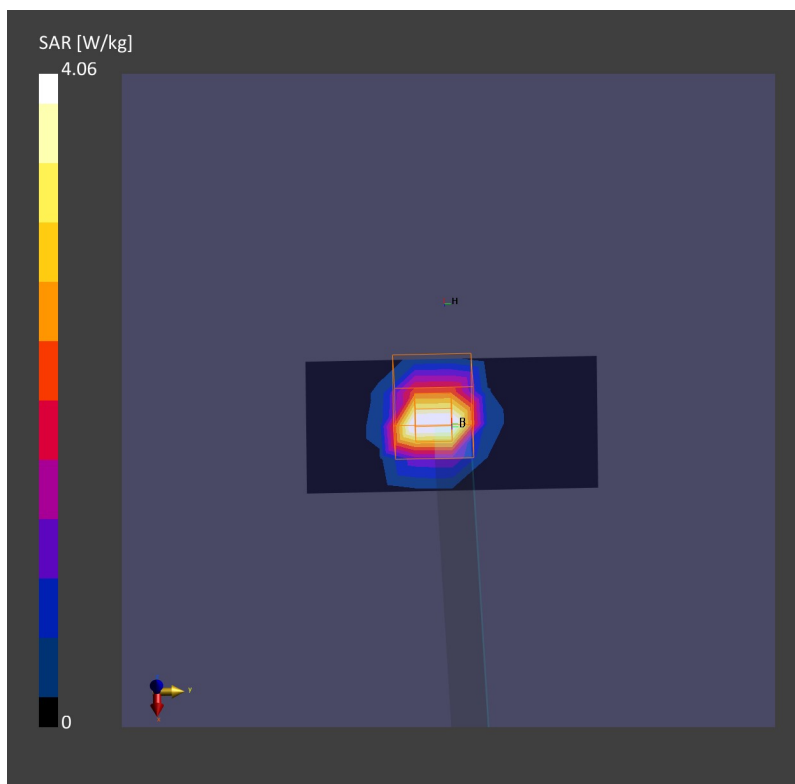

System Check_Head_5750MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5750.0

Medium: HSL. Medium parameters used: $f= 5750.0$ MHz; $\sigma= 5.10$ S/m; $\epsilon_r = 35.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.49, 5.49, 5.49); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.16 W/kg; SAR (10g) = 1.02 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 3.69 W/kg; SAR (10g) = 1.05 W/kg;

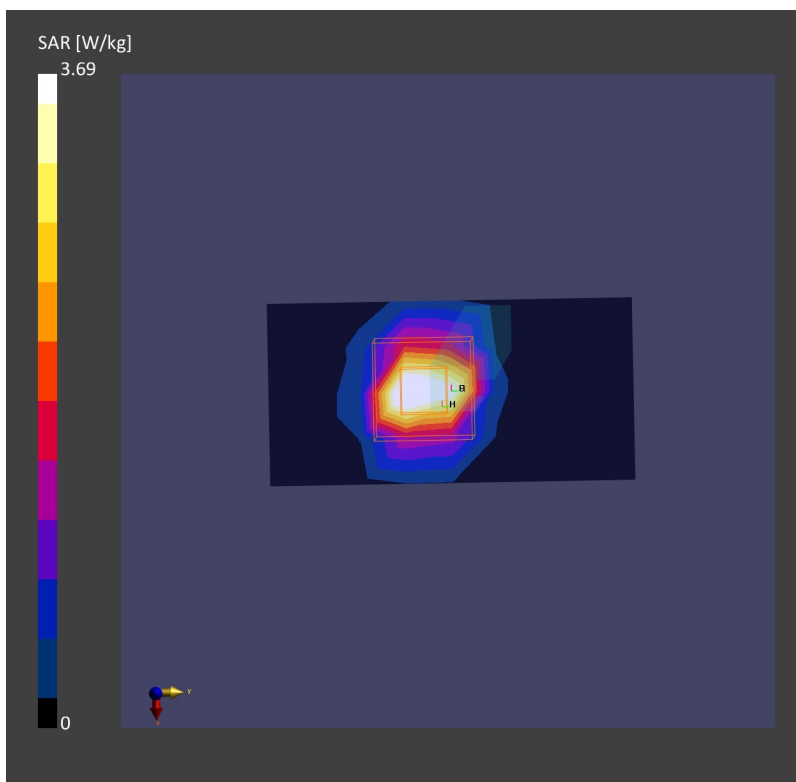

System Check_Head_13MHz

DUT: CLA-13-1020

Communication System: ; Frequency: 13.0

Medium: HSL. Medium parameters used: $f= 13.0$ MHz; $\sigma= 0.757$ S/m; $\epsilon_r = 53.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(19.14, 19.14, 19.14); Calibrated: 2022-04-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2021-12-01
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.136 W/kg; SAR (10g) = 0.112 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.02 dB

SAR (1g) = 0.133 W/kg; SAR (10g) = 0.084 W/kg;

