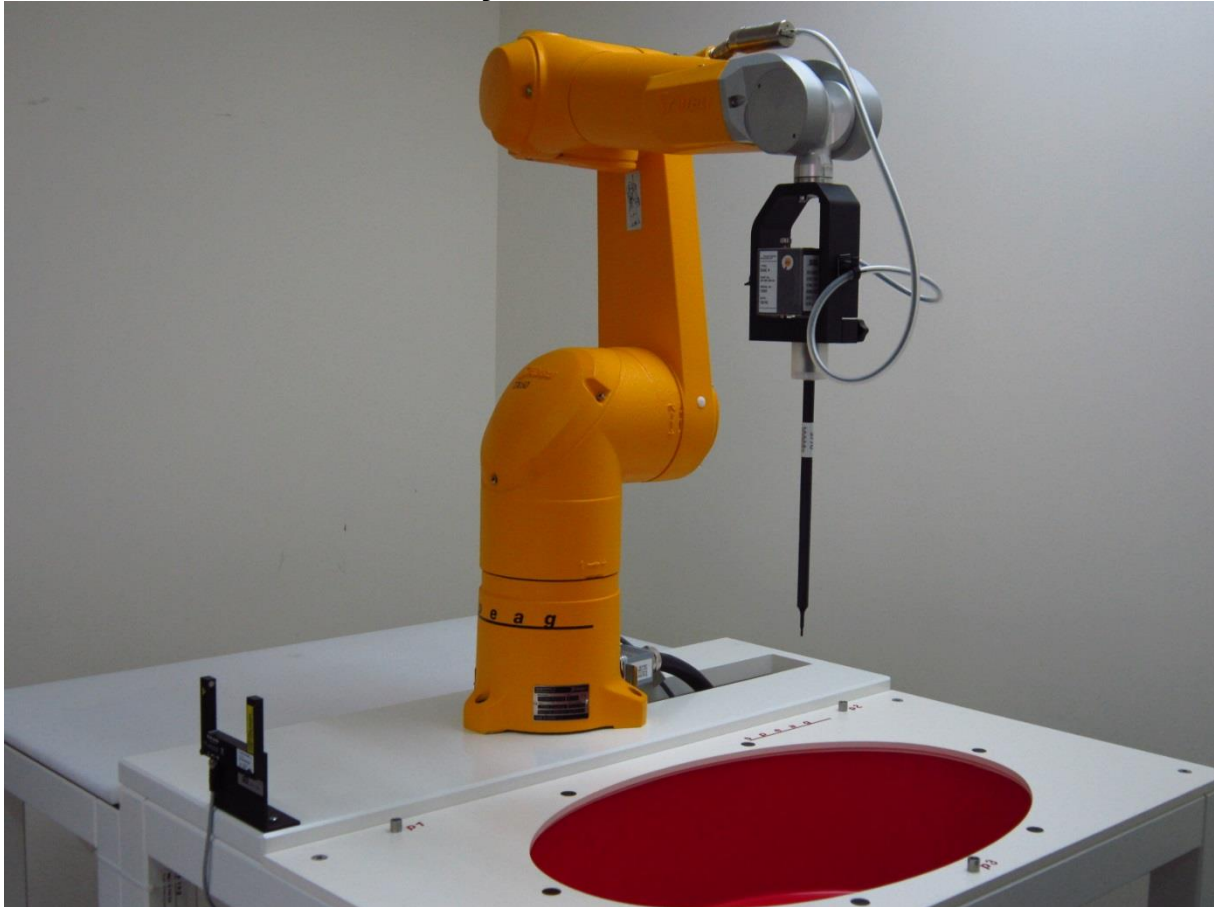


Appendix D

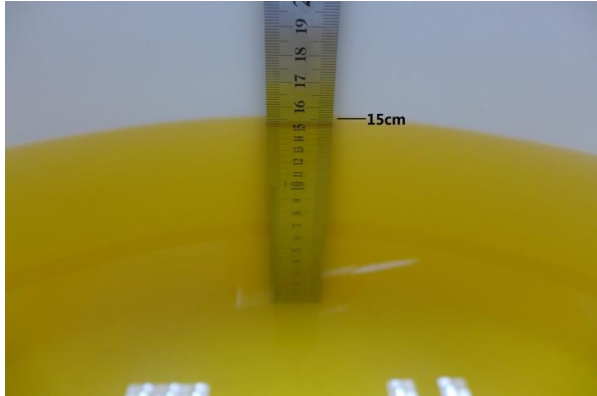
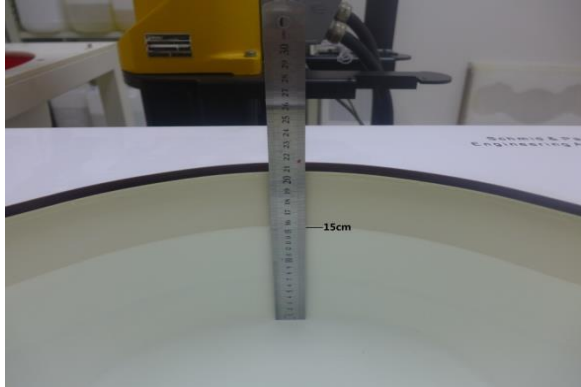
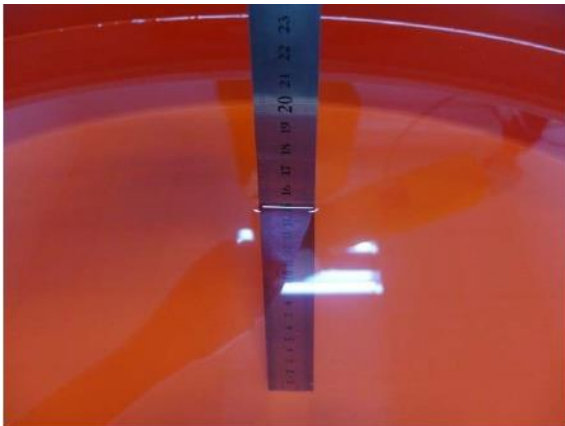
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid


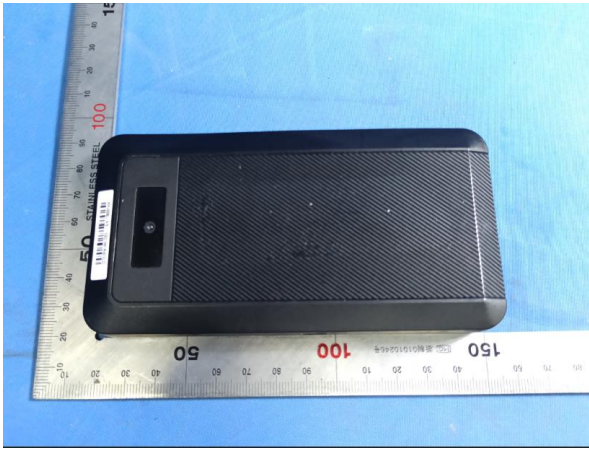


<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Head 1900</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 2450</p>	
	

3. Photographs of EUT test position

<p>Photo 4: Front side 0mm</p>	<p>Photo 5: Back side 0mm</p>
	
<p>Photo 6: Left side 0mm</p>	<p>Photo 7: Right side 0mm</p>
	
<p>Photo 8: Top side 0mm</p>	<p>Photo 9: Bottom side 0mm</p>
	

<p>Photo 10: Front side 10mm</p>	<p>Photo 11: Back side 10mm</p>
	
<p>Photo 12: Left side 10mm</p>	<p>Photo 13: Right side 10mm</p>
	
<p>Photo 14: Top side 10mm</p>	<p>Photo 15: Bottom side 10mm</p>
	

4. EUT Constructional Details

<p align="center">Photo 16: Front View</p>	<p align="center">Photo 17: Back View</p>
	
<p align="center">Photo 18: Left View</p>	<p align="center">Photo 19: Right View</p>
	
<p align="center">Photo 20: Top View</p>	<p align="center">Photo 21: Bottom View</p>
