

Appendix D

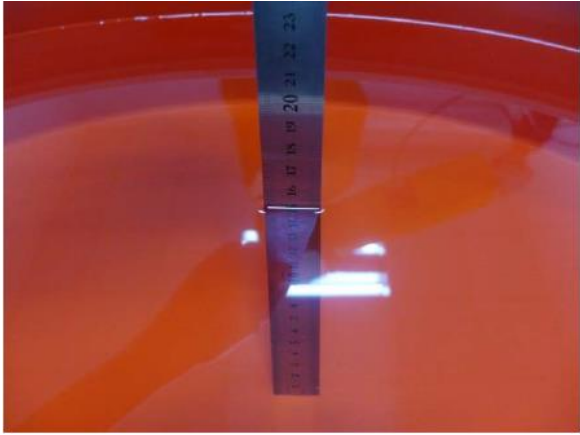

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

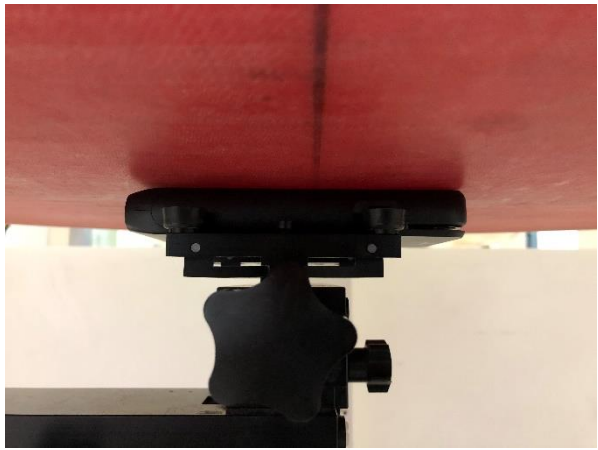
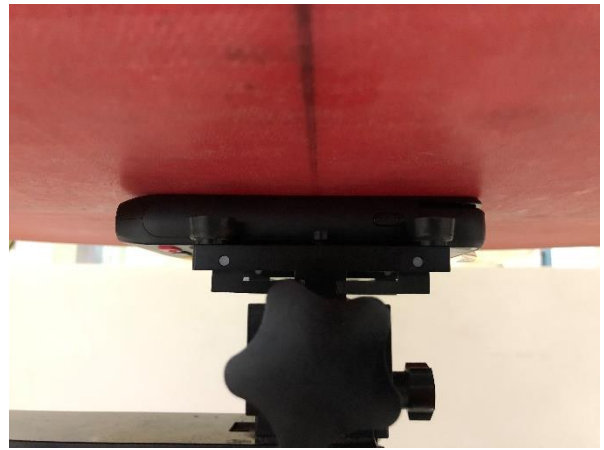




1. SAR measurement System

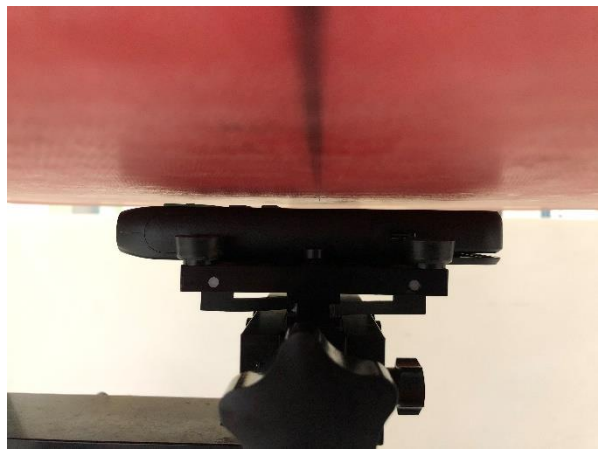






2. Photographs of Tissue Simulate Liquid





Photo 1: Tissue Simulant Liquid for Head 2450	Photo 2: Tissue Simulant Liquid for Head 5GHz
 A photograph showing a red liquid in a container. A ruler is placed vertically in the liquid, showing a scale from 16 to 25. The liquid is a uniform red color.	 A close-up photograph of a ruler in red liquid. The ruler shows a scale from 17 to 20. A white label with the red text 'P3' is visible in the background.

3. Photographs of EUT test position

<p>Photo 3: Front side 0mm</p>	<p>Photo 4: Back side 0mm</p>
	
<p>Photo 5: Left side 0mm</p>	<p>Photo 6: Right side 0mm</p>
	
<p>Photo 7: Top side 0mm</p>	<p>Photo 8: Bottom side 0mm</p>
	

<p>Photo 9: Front side 10mm</p>	<p>Photo 10: Back side 10mm</p>
	
<p>Photo 11: Left side 10mm</p>	<p>Photo 12: Right side 10mm</p>
	
<p>Photo 13: Top side 10mm</p>	<p>Photo 14: Bottom side 10mm</p>
	

4. EUT Constructional Details

<p align="center">Photo 15: Front View</p>	<p align="center">Photo 16: Back View</p>
	
<p align="center">Photo 17: Left View</p>	<p align="center">Photo 18: Right View</p>
	
<p align="center">Photo 19: Top View</p>	<p align="center">Photo 20: Bottom View</p>
