

Appendix C for KSCR2207001162AT

Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date
	<input type="checkbox"/>	1	D750V3	1188	2022/03/29
	<input checked="" type="checkbox"/>	2	D835V2	4d114	2022/03/31
	<input type="checkbox"/>	3	D900V2	1d079	2022/06/07
	<input checked="" type="checkbox"/>	4	D1800V2	2d170	2022/03/31
	<input checked="" type="checkbox"/>	5	D1900V2	5d136	2022/06/07
	<input type="checkbox"/>	6	D2000V2	1041	2022/06/06
	<input type="checkbox"/>	7	D2300V2	1096	2022/03/31
	<input checked="" type="checkbox"/>	8	D2450V2	817	2022/04/01
	<input checked="" type="checkbox"/>	9	D2600V2	1158	2022/03/31
	<input checked="" type="checkbox"/>	10	D5GHzV2	1095	2022/06/01
DAE	<input checked="" type="checkbox"/>	11	DAE4	1245	2022/05/30
Probe	<input checked="" type="checkbox"/>	12	EX3DV4	7346	2022/03/30



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
 No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300 t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1 Dipole

1.1 CLA150 - SN 4025

<p>Calibration Laboratory of Schmid & Partner Engineering AG Zughausstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: SGS-CN (Auden) Certificate No: CLA150-4025_Apr21</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: CLA150 - SN: 4025</p> <p>Calibration procedure(s): QA CAL-15.v9 Calibration Procedure for SAR Validation Sources below 700 MHz</p> <p>Calibration date: April 26, 2021</p> <p>This calibration certificate documents the traceability to national standards, which involve the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 2)°C and humidity < 70%.</p> <p>Calibration Equipment used (MATE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN: 1047/6</td> <td>09-Apr-21 (No. 217-0320103202)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103044</td> <td>09-Apr-21 (No. 217-03201)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103045</td> <td>09-Apr-21 (No. 217-03202)</td> <td>Apr-22</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: CC262 (20)</td> <td>09-Apr-21 (No. 217-03344)</td> <td>Apr-22</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 31092 / 0027</td> <td>09-Apr-21 (No. 217-03344)</td> <td>Apr-22</td> </tr> <tr> <td>Reference Probe CCKN/4</td> <td>SN: 3877</td> <td>30-Dec-20 (No. D3X3877_Dec20)</td> <td>Dec-21</td> </tr> <tr> <td>E1A/4</td> <td>SN: 664</td> <td>26-Jun-20 (No. D464/664_Jun20)</td> <td>Jun-21</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter E4413B</td> <td>SN: GB91203874</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check Jun-21</td> </tr> <tr> <td>Power sensor E4413A</td> <td>SN: M41498057</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check Jun-22</td> </tr> <tr> <td>Power sensor E4413A</td> <td>SN: 000100210</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check Jun-22</td> </tr> <tr> <td>RF generator HP 8542C</td> <td>SN: US3404101710</td> <td>04-Aug-19 (in house check Jun-20)</td> <td>In house check Jun-22</td> </tr> <tr> <td>Network Analyzer Agilent E8363A</td> <td>SN: US41080477</td> <td>31-Mar-14 (in house check Oct-20)</td> <td>In house check Oct-21</td> </tr> </tbody> </table> <p>Calibrated by: Jeffrey Katzman (Signature) Function: Laboratory Technician</p> <p>Approved by: Katja Pokovic (Signature) Function: Technical Manager</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued: April 26, 2021</p> <p>Certificate No: CLA150-4025_Apr21 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NRP	SN: 1047/6	09-Apr-21 (No. 217-0320103202)	Apr-22	Power sensor NRP-Z91	SN: 103044	09-Apr-21 (No. 217-03201)	Apr-22	Power sensor NRP-Z91	SN: 103045	09-Apr-21 (No. 217-03202)	Apr-22	Reference 20 dB Attenuator	SN: CC262 (20)	09-Apr-21 (No. 217-03344)	Apr-22	Type-N mismatch combination	SN: 31092 / 0027	09-Apr-21 (No. 217-03344)	Apr-22	Reference Probe CCKN/4	SN: 3877	30-Dec-20 (No. D3X3877_Dec20)	Dec-21	E1A/4	SN: 664	26-Jun-20 (No. D464/664_Jun20)	Jun-21	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Power meter E4413B	SN: GB91203874	09-Apr-16 (in house check Jun-20)	In house check Jun-21	Power sensor E4413A	SN: M41498057	09-Apr-16 (in house check Jun-20)	In house check Jun-22	Power sensor E4413A	SN: 000100210	09-Apr-16 (in house check Jun-20)	In house check Jun-22	RF generator HP 8542C	SN: US3404101710	04-Aug-19 (in house check Jun-20)	In house check Jun-22	Network Analyzer Agilent E8363A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check Oct-21	<p>Calibration Laboratory of Schmid & Partner Engineering AG Zughausstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Accreditation No: SCS 0108</p> <p>Glossary:</p> <p>TSL: liquid simulating liquid</p> <p>CorvF: sensitivity in TSL / NORM x,y,z</p> <p>N/A: not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <ol style="list-style-type: none"> IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013 IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016 IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010 KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz" <p>Additional Documentation:</p> <ol style="list-style-type: none"> DASY4/5 System Handbook <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The source is mounted in a touch configuration below the center marking of the flat phantom. Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p>The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: CLA150-4025_Apr21 Page 2 of 6</p>				
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																																																										
Power meter NRP	SN: 1047/6	09-Apr-21 (No. 217-0320103202)	Apr-22																																																										
Power sensor NRP-Z91	SN: 103044	09-Apr-21 (No. 217-03201)	Apr-22																																																										
Power sensor NRP-Z91	SN: 103045	09-Apr-21 (No. 217-03202)	Apr-22																																																										
Reference 20 dB Attenuator	SN: CC262 (20)	09-Apr-21 (No. 217-03344)	Apr-22																																																										
Type-N mismatch combination	SN: 31092 / 0027	09-Apr-21 (No. 217-03344)	Apr-22																																																										
Reference Probe CCKN/4	SN: 3877	30-Dec-20 (No. D3X3877_Dec20)	Dec-21																																																										
E1A/4	SN: 664	26-Jun-20 (No. D464/664_Jun20)	Jun-21																																																										
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																																																										
Power meter E4413B	SN: GB91203874	09-Apr-16 (in house check Jun-20)	In house check Jun-21																																																										
Power sensor E4413A	SN: M41498057	09-Apr-16 (in house check Jun-20)	In house check Jun-22																																																										
Power sensor E4413A	SN: 000100210	09-Apr-16 (in house check Jun-20)	In house check Jun-22																																																										
RF generator HP 8542C	SN: US3404101710	04-Aug-19 (in house check Jun-20)	In house check Jun-22																																																										
Network Analyzer Agilent E8363A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check Oct-21																																																										
<p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASYs</th> <th>V32.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>EL14 Flat Phantom</td> <td>Shell thickness: 2 ± 0.2 mm</td> </tr> <tr> <td>EUT Positioning</td> <td>Touch Position</td> <td></td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy = 4.0 mm, dz = 1.4 mm</td> <td>Graded Ratio = 1.4 (Z direction)</td> </tr> <tr> <td>Frequency</td> <td>150 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p>Head TSL parameters The following parameters and calculations were applied.</p> <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>52.3</td> <td>0.75 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>51.1 ± 6 %</td> <td>0.75 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>< 0.5 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p>SAR result with Head TSL</p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>1 W input power</td> <td>3.90 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>3.88 W/kg ± 18.4 % (k=2)</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>SAR averaged over 10 cm³ (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>1 W input power</td> <td>2.60 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>2.59 W/kg ± 18.0 % (k=2)</td> </tr> </tbody> </table> <p>Certificate No: CLA150-4025_Apr21 Page 3 of 6</p>	DASY Version	DASYs	V32.10.4	Extrapolation	Advanced Extrapolation		Phantom	EL14 Flat Phantom	Shell thickness: 2 ± 0.2 mm	EUT Positioning	Touch Position		Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)	Frequency	150 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	52.3	0.75 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	51.1 ± 6 %	0.75 mho/m ± 6 %	Head TSL temperature change during test	< 0.5 °C	---	---	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	1 W input power	3.90 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	3.88 W/kg ± 18.4 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	1 W input power	2.60 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	2.59 W/kg ± 18.0 % (k=2)	<p>Appendix (Additional assessments outside the scope of SCS 0108)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <thead> <tr> <th>Impedance, transformed to feed point</th> <th>47.8 Ω ± 1.5 Ω</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-31.4 dB</td> </tr> </tbody> </table> <p>Additional EUT Data</p> <table border="1"> <thead> <tr> <th>Manufactured by</th> <th>SPEAG</th> </tr> </thead> <tbody> <tr> <td></td> <td></td> </tr> </tbody> </table> <p>Certificate No: CLA150-4025_Apr21 Page 4 of 6</p>	Impedance, transformed to feed point	47.8 Ω ± 1.5 Ω	Return Loss	-31.4 dB	Manufactured by	SPEAG		
DASY Version	DASYs	V32.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	EL14 Flat Phantom	Shell thickness: 2 ± 0.2 mm																																																											
EUT Positioning	Touch Position																																																												
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)																																																											
Frequency	150 MHz ± 1 MHz																																																												
	Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.0 °C	52.3	0.75 mho/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	51.1 ± 6 %	0.75 mho/m ± 6 %																																																										
Head TSL temperature change during test	< 0.5 °C	---	---																																																										
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																												
SAR measured	1 W input power	3.90 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	3.88 W/kg ± 18.4 % (k=2)																																																											
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																												
SAR measured	1 W input power	2.60 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	2.59 W/kg ± 18.0 % (k=2)																																																											
Impedance, transformed to feed point	47.8 Ω ± 1.5 Ω																																																												
Return Loss	-31.4 dB																																																												
Manufactured by	SPEAG																																																												



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

DASY5 Validation Report for Head TSL

Date: 26.04.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4025

Communication System: UTD 0 - CW; Frequency: 150 MHz
Medium parameters used: $f = 150 \text{ MHz}$; $\sigma = 0.76 \text{ S/m}$; $\epsilon_0 = 51.1$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(12.51, 12.51, 12.51) @ 150 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Snt54; Calibrated: 26.06.2020
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP.1003
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan, dist=1.4mm (8x10x8) Cube @ Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 85.93 W/m; Power Drift = -0.02 dB
Peak SAR (extrapolated) = 7.36 W/kg
SAR(1 g) = 3.90 W/kg; SAR(10 g) = 2.60 W/kg
Smallest distance from peaks to all points 3 dB below: Larger than measurement grid (> 30mm)
Ratio of SAR at M2 to SAR at M1 = 80.4%
Maximum value of SAR (measured) = 5.48 W/kg

0 dB = 5.48 W/kg = 7.39 dBW/kg

Certificate No: CLA150-4025_Apr21 Page 6 of 6

Certificate No: CLA150-4025_Apr21 Page 6 of 6

1.2 D450V3 - SN 1103

Calibration Laboratory of Schmid & Partner Engineering AG
Ziegelhausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client: **SGS-CN (Aude)** Certificate No: **D450V3-1103_Apr21**

CALIBRATION CERTIFICATE

Object: **D450V3 - SN: 1103**

Calibration procedure(s): **QA CAL-15_v9**
Calibration Procedure for SAR Validation Sources below 700 MHz

Calibration date: **April 21, 2021**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closest laboratory facility: environment temperature (22 ± 0)°C and humidity < 70%.

Calibration Equipment used (M&T critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NP#	SN: 104778	09-Apr-21 (No: 217-03201/03202)	Apr-22
Power sensor NP#-291	SN: 103244	09-Apr-21 (No: 217-03201)	Apr-22
Power sensor NP#-291	SN: 103245	09-Apr-21 (No: 217-03202)	Apr-22
Reference 20 dB Attenuator	SN: C2352 (200)	09-Apr-21 (No: 217-03343)	Apr-22
Type-N mismatch combinator	SN: 310952 / 06327	09-Apr-21 (No: 217-03344)	Apr-22
Reference Probe EPC004	SN: 3877	30-Dec-20 (No: EX3-3877_Dec20)	Dec-21
DAEA	SN: 654	26-Jan-20 (No: DAE4-654_Jan20)	Jan-21

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4414B	SN: GB41290274	06-Apr-16 (In house check Jun-20)	In house check Jun-22
Power sensor E4412A	SN: MY41496067	06-Apr-16 (In house check Jun-20)	In house check Jun-22
Power sensor E4413A	SN: 000116218	06-Apr-16 (In house check Jun-20)	In house check Jun-22
HP generator HP 8644C	SN: L25349/01700	06-Apr-16 (In house check Jun-20)	In house check Jun-22
Network Analyzer Agilent E8363A	SN: U841980477	31-Mar-14 (In house check Oct-20)	In house check Oct-21

Calibrated by: **Chao Liu** (Function: Laboratory Technician)

Approved by: **Kello Polovic** (Function: Technical Manager)

Issued: April 23, 2021

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D450V3-1103_Apr21 Page 1 of 6

Calibration Laboratory of Schmid & Partner Engineering AG
Ziegelhausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Glossary:

TSL: Issue simulating liquid
ConvF: sensitivity in TSL / NORM x,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 656564, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D450V3-1103_Apr21 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

Measurement Conditions
DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELH Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters
The following parameters and calculations were applied:

Nominal Head TSL parameters	Temperature: 22.0 °C	Permittivity: 43.5	Conductivity: 0.57 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	43.1 ± 6 %	0.57 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.55 W/kg ± 18.1 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	0.757 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.06 W/kg ± 17.6 % (k=2)

Certificate No: D450V3-1103_Apr21 Page 3 of 6

DASY5 Validation Report for Head TSL

Date: 21.04.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1103


Communication System: UID 0 - CW; Frequency: 450 MHz
Medium parameters used: f = 450 MHz; o = 0.87 S/m; ε_r = 43.1; ρ = 1000 kg/m³
Phantom section: Flat Section
Measurement Standard: DASY5 (IEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.64, 10.64) @ 450 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sa654; Calibrated: 26.06.2020
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP.1003
- DASY52.52.10.4(1527); SEMCAD X 14.6.14(7483)

Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 39.18 W/m; Power Drift = -0.08 dB
Peak SAR (extrapolated) = 1.76 W/kg
SAR(1g) = 1.14 W/kg; SAR(10g) = 0.767 W/kg
Smallest distance from peaks to all points 3 dB below: Larger than measurement grid
Ratio of SAR at M2 to SAR at M1 = 64.9%
Maximum value of SAR (measured) = 1.53 W/kg

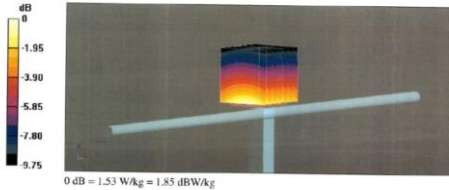

Certificate No: D450V3-1103_Apr21 Page 5 of 6

Appendix (Additional assessments outside the scope of SCS 0106)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	57.1 Ω - 2.8 jΩ
Return Loss	-23.0 dB

General Antenna Parameters and Design


Electrical Delay (one direction)	1.346 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is set according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: D450V3-1103_Apr21 Page 4 of 6

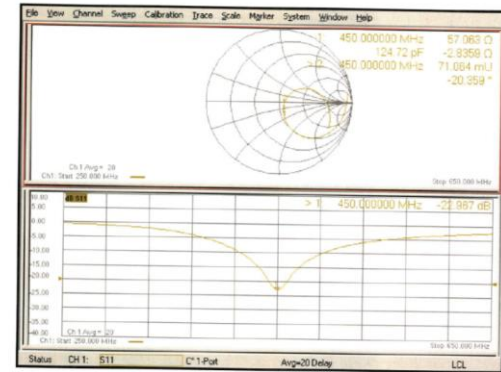

Certificate No: D450V3-1103_Apr21 Page 6 of 6







Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.3 D750V3 - SN 1188

 		 																							
Client: SGS-CN Certificate No: Z22-60103		Glossary: TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx.yz N/A: not applicable or not measured																							
CALIBRATION CERTIFICATE Object: D750V3 - SN: 1188 Calibration Procedure(s): FF-Z11-003-01 Calibration date: March 29, 2022		Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.		Additional Documentation: c) DASy4/5 System Handbook																							
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity<70%.		Methods Applied and Interpretation of Parameters: <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. 																							
Calibration Equipment used (M&TE critical for calibration)		The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.																							
<table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>108277</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX30V4</td> <td>SN 7307</td> <td>26-May-21(SPEAG.No.EX3-7307_May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22(CTTL-SPEAG.No.Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table>		Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	108277	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX30V4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23	Issued: April 3, 2022 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																						
Power Meter NRP2	108277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																						
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																						
Reference Probe EX30V4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22																						
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23																						
Certificate No: Z22-60103 Page 1 of 6		Certificate No: Z22-60103 Page 2 of 6																							
Measurement Conditions DASy system configuration, as far as not given on page 1.		Appendix (Additional assessments outside the scope of CNAS L0570)																							
<table border="1"> <thead> <tr> <th>DASy Version</th> <th>DASyV2</th> <th>V52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>750 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table>		DASy Version	DASyV2	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	750 MHz ± 1 MHz		Antenna Parameters with Head TSL <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>53.60 - 1.13jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-28.7dB</td> </tr> </table>		Impedance, transformed to feed point	53.60 - 1.13jΩ	Return Loss	-28.7dB
DASy Version	DASyV2	V52.10.4																							
Extrapolation	Advanced Extrapolation																								
Phantom	Triple Flat Phantom 5.1C																								
Distance Dipole Center - TSL	15 mm	with Spacer																							
Zoom Scan Resolution	dx, dy, dz = 5 mm																								
Frequency	750 MHz ± 1 MHz																								
Impedance, transformed to feed point	53.60 - 1.13jΩ																								
Return Loss	-28.7dB																								
Head TSL parameters The following parameters and calculations were applied.		General Antenna Parameters and Design <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>0.947 ns</td> </tr> </table>		Electrical Delay (one direction)	0.947 ns																				
Electrical Delay (one direction)	0.947 ns																								
<table border="1"> <thead> <tr> <th>Nominal Head TSL parameters</th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td></td> <td>22.0 °C</td> <td>42.0</td> <td>0.90 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>41.4 ± 6 %</td> <td>0.89 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table>		Nominal Head TSL parameters	Temperature	Permittivity	Conductivity		22.0 °C	42.0	0.90 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---	After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.							
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																						
	22.0 °C	42.0	0.90 mho/m																						
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %																						
Head TSL temperature change during test	<1.0 °C	---	---																						
SAR result with Head TSL <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm² (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.07 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>8.27 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm² (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.37 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>5.48 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table>		SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		SAR measured	250 mW input power	2.07 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		SAR measured	250 mW input power	1.37 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)	Additional EUT Data <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table>		Manufactured by	SPEAG		
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition																								
SAR measured	250 mW input power	2.07 W/kg																							
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)																							
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition																								
SAR measured	250 mW input power	1.37 W/kg																							
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)																							
Manufactured by	SPEAG																								
Certificate No: Z22-60103 Page 3 of 6		Certificate No: Z22-60103 Page 4 of 6																							



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
 No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300 t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

In Collaboration with
TTL Speaq
CALIBRATION LABORATORY

CAICT


Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4204633-2079 Fax: +86-10-4204633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.com

DASY5 Validation Report for Head TSL Date: 2022-03-29

Test Laboratory: CTTL, Beijing, China
DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1188
Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.888 \text{ S/m}$; $\epsilon_r = 41.36$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Right Section
Measurement Standard: DASY5 (IEEE/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(10.31, 10.31, 10.31) @ 750 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 S11556; Calibrated: 2022-01-12
- Phantom: MFP_V5.IC (204mg probe fill); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 55.06 V/m; Power Drift = 0.00 dB
Peak SAR (extrapolated) = 3.07 W/kg
SAR(1 g) = 2.07 W/kg; SAR(10 g) = 1.37 W/kg
Smallest distance from peaks to all points 3 dB below = 18.9 mm
Ratio of SAR at M2 to SAR at M1 = 67.1%
Maximum value of SAR (measured) = 2.74 W/kg

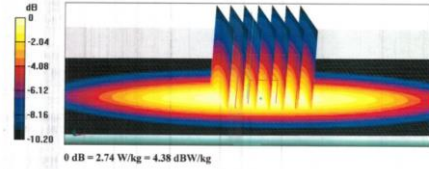

0 dB = 2.74 W/kg = 4.38 dBW/kg


Certificate No: Z22-60103 Page 5 of 6

In Collaboration with
TTL Speaq
CALIBRATION LABORATORY

CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4204633-2079 Fax: +86-10-4204633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.com

Impedance Measurement Plot for Head TSL

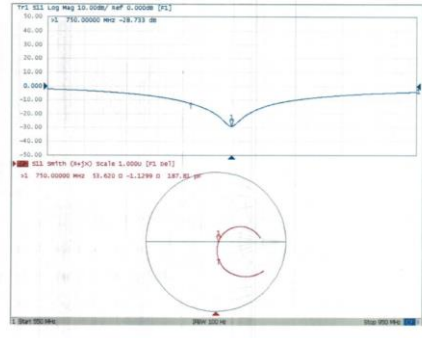

Certificate No: Z22-60103 Page 6 of 6

1.4 D835V2 - SN 4d114

In Collaboration with
TTL Speaq
CALIBRATION LABORATORY

CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4204633-2512 Fax: +86-10-4204633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.com

Client: **SGS-CN** Certificate No: **Z22-60104**

CALIBRATION CERTIFICATE

Object: D835V2 - SN: 4d114

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: March 31, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity < 70%.

Calibration Equipment used (M&E critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22
Power sensor NRPBS	104291	24-Sep-21 (CTTL, No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG, No. EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG, No. Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No.J22X00409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X00406)	Jan-23

Calibrated by: Zhao Jing, SAR Test Engineer, Signature: [Signature]

Reviewed by: Lin Hao, SAR Test Engineer, Signature: [Signature]

Approved by: Qi Diyuan, SAR Project Leader, Signature: [Signature]

Issued: April 8, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60104 Page 1 of 6

In Collaboration with
TTL Speaq
CALIBRATION LABORATORY

CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4204633-2079 Fax: +86-10-4204633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.com

Glossary:

- TSL: tissue simulating liquid
- ConvF: sensitivity in TSL / NORMx.yz
- N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528: "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/S System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60104 Page 2 of 6













Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed on the leaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

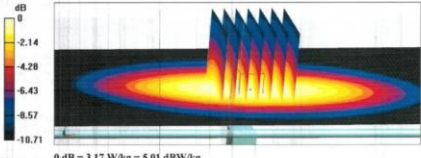t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com
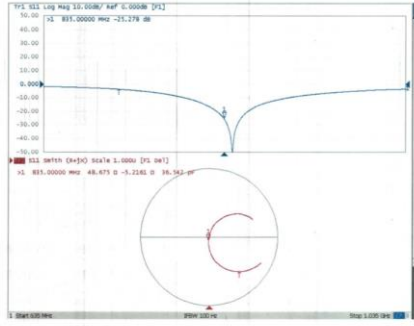
<p style="text-align: center;">   </p> <p style="font-size: small;"> In Collaboration with TTL Calibration Laboratory Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatit.com </p> <p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY52</td> <td>V52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td colspan="2">Advanced Extrapolation</td> </tr> <tr> <td>Phantom</td> <td colspan="2">Triple Flat Phantom 5.1C</td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td colspan="2">dx, dy, dz = 5 mm</td> </tr> <tr> <td>Frequency</td> <td colspan="2">835 MHz ± 1 MHz</td> </tr> </table> <p>Head TSL parameters The following parameters and calculations were applied.</p> <table border="1"> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>41.5</td> <td>0.90 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>41.0 ± 6 %</td> <td>0.91 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><+1.0 °C</td> <td>---</td> <td>---</td> </tr> </table> <p>SAR result with Head TSL</p> <table border="1"> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.37 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>9.40 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm³ (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.54 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>6.12 W/kg ± 18.7 % (k=2)</td> </tr> </table> <p style="text-align: right;">Certificate No: Z22-60104 Page 3 of 6</p>	DASY Version	DASY52	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	835 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 6 %	0.91 mho/m ± 6 %	Head TSL temperature change during test	<+1.0 °C	---	---	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	2.37 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	9.40 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	1.54 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	6.12 W/kg ± 18.7 % (k=2)	<p style="text-align: center;">   </p> <p style="font-size: small;"> In Collaboration with TTL Calibration Laboratory Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatit.com </p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>48.70-5.22jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-25.3dB</td> </tr> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>1.307 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> <p style="text-align: right;">Certificate No: Z22-60104 Page 4 of 6</p>	Impedance, transformed to feed point	48.70-5.22jΩ	Return Loss	-25.3dB	Electrical Delay (one direction)	1.307 ns	Manufactured by	SPEAG
DASY Version	DASY52	V52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple Flat Phantom 5.1C																																																												
Distance Dipole Center - TSL	15 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																												
Frequency	835 MHz ± 1 MHz																																																												
	Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 6 %	0.91 mho/m ± 6 %																																																										
Head TSL temperature change during test	<+1.0 °C	---	---																																																										
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	2.37 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	9.40 W/kg ± 18.8 % (k=2)																																																											
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	1.54 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	6.12 W/kg ± 18.7 % (k=2)																																																											
Impedance, transformed to feed point	48.70-5.22jΩ																																																												
Return Loss	-25.3dB																																																												
Electrical Delay (one direction)	1.307 ns																																																												
Manufactured by	SPEAG																																																												
<p style="text-align: center;">   </p> <p style="font-size: small;"> In Collaboration with TTL Calibration Laboratory Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatit.com </p> <p>DASY5 Validation Report for Head TSL Test Laboratory: CTTI, Beijing, China Date: 2022-03-31 DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d114 Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium parameters used: f = 835 MHz; σ = 0.907 S/m; ε_r = 40.98; ρ = 1000 kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:</p> <ul style="list-style-type: none"> Probe: EX3DV4 - SN7307; ConvF(10.13, 10.13, 10.13) @ 835 MHz; Calibrated: 2021-05-26 Sensor-Surface: 1.4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1556; Calibrated: 2022-01-12 Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 DASY52.10.4(1535); SEMCAD X 14.6.14(7501) <p>Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 57.88 V/m; Power Drift = 0.04 dB Peak SAR (extrapolated) = 3.56 W/kg SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.54 W/kg Smallest distance from peaks to all points 3 dB below = 15.8 mm Ratio of SAR at M2 to SAR at M1 = 66.2% Maximum value of SAR (measured) = 3.17 W/kg</p>  <p style="text-align: center;">0 dB = 3.17 W/kg = 5.01 dBW/kg</p> <p style="text-align: right;">Certificate No: Z22-60104 Page 5 of 6</p>	<p style="text-align: center;">   </p> <p style="font-size: small;"> In Collaboration with TTL Calibration Laboratory Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatit.com </p> <p>Impedance Measurement Plot for Head TSL</p>  <p style="text-align: right;">Certificate No: Z22-60104 Page 6 of 6</p>																																																												







Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留园创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.5 D900V2 - SN 1d079

 <p>Client: SGS-CN Certificate No: Z22-60184</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: D900V2 - SN: 1d079</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: June 7, 2022</p> <p>The calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CITL No. J21X06326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRPBS</td> <td>104291</td> <td>24-Sep-21 (CITL No. J21X06326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX32V4</td> <td>SN 7464</td> <td>26-Jan-22 (SPEAG/NO. EX3-7464, Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22 (CITL-SPEAG/NO. Z22-40007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>MV49071430</td> <td>13-Jan-22 (CITL No. J22X00406)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MV48110673</td> <td>14-Jan-22 (CITL No. J22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> <p>Calibrated by: Zhao Jing SAR Test Engineer</p> <p>Reviewed by: Lin Hao SAR Test Engineer</p> <p>Approved by: Qi Dianguan SAR Project Leader</p> <p>Issued: June 13, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: Z22-60184 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CITL No. J21X06326)	Sep-22	Power sensor NRPBS	104291	24-Sep-21 (CITL No. J21X06326)	Sep-22	Reference Probe EX32V4	SN 7464	26-Jan-22 (SPEAG/NO. EX3-7464, Jan22)	Jan-23	DAE4	SN 1556	12-Jan-22 (CITL-SPEAG/NO. Z22-40007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MV49071430	13-Jan-22 (CITL No. J22X00406)	Jan-23	Network Analyzer E5071C	MV48110673	14-Jan-22 (CITL No. J22X00406)	Jan-23	 <p>Glossary:</p> <p>TSL: tissue simulating liquid</p> <p>Con/F: sensitivity in TSL / NORMx,y,z</p> <p>N/A: not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020</p> <p>b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Additional Documentation:</p> <p>c) DASy4/5 System Handbook</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor $k=2$, which for a normal distribution Corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z22-60184 Page 2 of 6</p>												
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																										
Power Meter NRP2	106277	24-Sep-21 (CITL No. J21X06326)	Sep-22																																										
Power sensor NRPBS	104291	24-Sep-21 (CITL No. J21X06326)	Sep-22																																										
Reference Probe EX32V4	SN 7464	26-Jan-22 (SPEAG/NO. EX3-7464, Jan22)	Jan-23																																										
DAE4	SN 1556	12-Jan-22 (CITL-SPEAG/NO. Z22-40007)	Jan-23																																										
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																										
Signal Generator E4438C	MV49071430	13-Jan-22 (CITL No. J22X00406)	Jan-23																																										
Network Analyzer E5071C	MV48110673	14-Jan-22 (CITL No. J22X00406)	Jan-23																																										
 <p>Measurement Conditions</p> <p>DASY system configuration, as far as not given on page 1.</p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASy/52</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advised Extrapolation</td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom S.1C</td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> </tr> <tr> <td>Frequency</td> <td>900 MHz ± 1 MHz</td> </tr> </tbody> </table> <p>Head TSL parameters</p> <p>The following parameters and calculations were applied:</p> <table border="1"> <thead> <tr> <th>Nominal Head TSL parameters</th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Measured Head TSL parameters</td> <td>22.0 °C</td> <td>41.5</td> <td>0.97 mho/m</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p>SAR result with Head TSL</p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm² (1 g) of Head TSL</th> <th>Condition</th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> </tr> <tr> <td>SAR averaged over 10 cm² (10 g) of Head TSL</td> <th>Condition</th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> </tr> </tbody> </table> <p>Certificate No: Z22-60184 Page 3 of 6</p>	DASY Version	DASy/52	Extrapolation	Advised Extrapolation	Phantom	Triple Flat Phantom S.1C	Distance Dipole Center - TSL	15 mm with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm	Frequency	900 MHz ± 1 MHz	Nominal Head TSL parameters	Temperature	Permittivity	Conductivity	Measured Head TSL parameters	22.0 °C	41.5	0.97 mho/m	Head TSL temperature change during test	<1.0 °C	---	---	SAR averaged over 1 cm ² (1 g) of Head TSL	Condition	SAR measured	250 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	SAR measured	250 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	 <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <thead> <tr> <th>Impedance, transformed to feed point</th> <th>48.10 - 6.49jΩ</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-23.3 dB</td> </tr> </tbody> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <thead> <tr> <th>Electrical Delay (one direction)</th> <th>1.312 ns</th> </tr> </thead> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <thead> <tr> <th>Manufactured by</th> <th>SPEAG</th> </tr> </thead> </table> <p>Certificate No: Z22-60184 Page 4 of 6</p>	Impedance, transformed to feed point	48.10 - 6.49jΩ	Return Loss	-23.3 dB	Electrical Delay (one direction)	1.312 ns	Manufactured by	SPEAG
DASY Version	DASy/52																																												
Extrapolation	Advised Extrapolation																																												
Phantom	Triple Flat Phantom S.1C																																												
Distance Dipole Center - TSL	15 mm with Spacer																																												
Zoom Scan Resolution	dx, dy, dz = 5 mm																																												
Frequency	900 MHz ± 1 MHz																																												
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																																										
Measured Head TSL parameters	22.0 °C	41.5	0.97 mho/m																																										
Head TSL temperature change during test	<1.0 °C	---	---																																										
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition																																												
SAR measured	250 mW input power																																												
SAR for nominal Head TSL parameters	normalized to 1W																																												
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition																																												
SAR measured	250 mW input power																																												
SAR for nominal Head TSL parameters	normalized to 1W																																												
Impedance, transformed to feed point	48.10 - 6.49jΩ																																												
Return Loss	-23.3 dB																																												
Electrical Delay (one direction)	1.312 ns																																												
Manufactured by	SPEAG																																												



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4230663-2117
 Email: cti@china.ttl.com http://www.china.ttl.com

DASY5 Validation Report for Head TSL Date: 2022-06-07

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN: 14079

Communication System: UTD 0, CW; Frequency: 900 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 900 \text{ MHz}$; $\sigma = 0.98 \text{ S/m}$; $\epsilon = 42.05$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(9.72, 9.72, 9.72) @ 900 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1 Ann (Mechanical Surface Detection)
- Electronics: DA4E Sot1556; Calibrated: 2022-01-12
- Phantom: MFP_V5.1C (2ddeg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52.52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube @ Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 59.81 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 4.20 W/kg

SAR1 (g) = 2.76 W/kg; SAR10 (g) = 1.78 W/kg

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 65.8%

Maximum value of SAR (measured) = 3.71 W/kg

0 dB = 3.71 W/kg = 5.69 dBW/kg

Certificate No: Z22-40184 Page 1 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4230663-2117
 Email: cti@china.ttl.com http://www.china.ttl.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-40184 Page 6 of 6

1.6 D1800V2 - SN 2d170

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY, **ILAC-MRA**, **CNAS** 中国认可 国家互认 校准实验室 CNAS L670, and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4230663-2117 Fax: +86-10-4230663-2204
 E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60105**

CALIBRATION CERTIFICATE

Object: **D1800V2 - SN: 2d170**

Calibration Procedure(s): **FF-Z11-003-01**
 Calibration Procedures for dipole validation kits

Calibration date: **March 31, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&E critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104281	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EK3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY46110873	14-Jan-22 (CTTL No.J22X00409)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer

Reviewed by: **Lin Hao** SAR Test Engineer

Approved by: **Qi Dianyan** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60105 Page 1 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4230663-2079 Fax: +86-10-4230663-2204
 E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:

- TSL: tissue simulating liquid
- ConvF: sensitivity in TSL / NORMx.y.z
- N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60105 Page 2 of 6





Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com
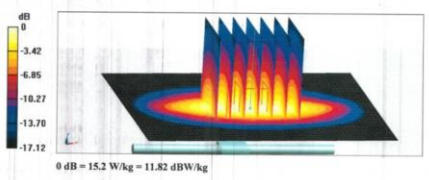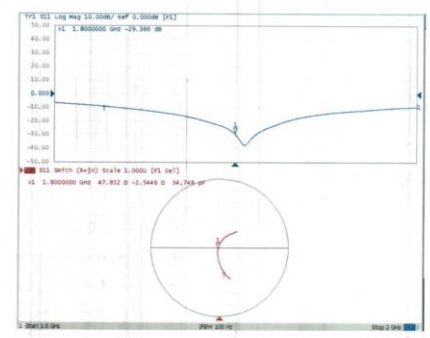
<p>In Collaboration with TTL Speag CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p> <p>Measurement Conditions DASY system configuration, as far as not given on page 1</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY52</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>1800 MHz ± 1 MHz</td> <td></td> </tr> </table> <p>Head TSL parameters The following parameters and calculations were applied:</p> <table border="1"> <tr> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>40.0</td> <td>1.40 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>40.6 ± 6 %</td> <td>1.41 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>+1.0 °C</td> <td>---</td> <td>---</td> </tr> </table> <p>SAR result with Head TSL</p> <table border="1"> <tr> <td>SAR averaged over 1 cm³ (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>9.73 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>38.9 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.11 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>20.4 W/kg ± 18.7 % (k=2)</td> </tr> </table> <p>Certificate No: Z22-60105 Page 3 of 6</p>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	1800 MHz ± 1 MHz		Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	40.6 ± 6 %	1.41 mho/m ± 6 %	Head TSL temperature change during test	+1.0 °C	---	---	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	9.73 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	38.9 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	5.11 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	20.4 W/kg ± 18.7 % (k=2)	<p>In Collaboration with TTL Speag CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>47.90 - 2.54jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-29.4dB</td> </tr> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>1.118 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> <p>Certificate No: Z22-60105 Page 4 of 6</p>	Impedance, transformed to feed point	47.90 - 2.54jΩ	Return Loss	-29.4dB	Electrical Delay (one direction)	1.118 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																										
Extrapolation	Advanced Extrapolation																																																											
Phantom	Triple Flat Phantom 5.1C																																																											
Distance Dipole Center - TSL	10 mm	with Spacer																																																										
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																											
Frequency	1800 MHz ± 1 MHz																																																											
Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m																																																									
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.6 ± 6 %	1.41 mho/m ± 6 %																																																									
Head TSL temperature change during test	+1.0 °C	---	---																																																									
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																											
SAR measured	250 mW input power	9.73 W/kg																																																										
SAR for nominal Head TSL parameters	normalized to 1W	38.9 W/kg ± 18.8 % (k=2)																																																										
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																											
SAR measured	250 mW input power	5.11 W/kg																																																										
SAR for nominal Head TSL parameters	normalized to 1W	20.4 W/kg ± 18.7 % (k=2)																																																										
Impedance, transformed to feed point	47.90 - 2.54jΩ																																																											
Return Loss	-29.4dB																																																											
Electrical Delay (one direction)	1.118 ns																																																											
Manufactured by	SPEAG																																																											
<p>In Collaboration with TTL Speag CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p> <p>DASY5 Validation Report for Head TSL Test Laboratory: TTL, Beijing, China Date: 2022-03-31 DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN; 2d170 Communication System: UID 0, CW; Frequency: 1800 MHz; Duty Cycle: 1:1 Medium parameters used: f = 1800 MHz; σ = 1.411 S/m; ε = 40.62; ρ = 1000 kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:</p> <ul style="list-style-type: none"> Probe: EX3DV4 - SN7307; ConvF(8.34, 8.34, 8.34) @ 1800 MHz; Calibrated: 2021-05-26 Sense-Surface: 1.4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1556; Calibrated: 2022-01-12 Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) <p>Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 98.14 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 18.2 W/kg SAR(1 g) = 9.73 W/kg; SAR(10 g) = 5.11 W/kg Smallest distance from peaks to all points 3 dB below = 10 mm Ratio of SAR at M2 to SAR at M1 = 54% Maximum value of SAR (measured) = 15.2 W/kg</p>  <p>0 dB = 15.2 W/kg = 11.82 dBW/kg</p> <p>Certificate No: Z22-60105 Page 5 of 6</p>	<p>In Collaboration with TTL Speag CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p> <p>Impedance Measurement Plot for Head TSL</p>  <p>Certificate No: Z22-60105 Page 6 of 6</p>																																																											



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.7 D1900V2 - SN 5d136

<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191 Tel: +86-10-4208633-2117 E-mail: cti@china.ttl.com</p>	<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4208633-2117 E-mail: cti@china.ttl.com</p>																					
<p>Client: SGS-CN Certificate No: Z22-60185</p>																						
<p>CALIBRATION CERTIFICATE</p>																						
<p>Object: D1900V2 - SN: 5d136</p>																						
<p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p>																						
<p>Calibration date: June 7, 2022</p>																						
<p>The calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p>																						
<p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.</p>																						
<p>Calibration Equipment used (M&TE critical for calibration)</p>																						
<table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP6S</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EKSDV4</td> <td>SN 7464</td> <td>26-Jan-22(SPEAG No.E33-71464_Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAE4</td> <td>SN 1656</td> <td>12-Jan-22(CTTL-SPEAG No.222-60007)</td> <td>Jan-23</td> </tr> </tbody> </table>			Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP6S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EKSDV4	SN 7464	26-Jan-22(SPEAG No.E33-71464_Jan22)	Jan-23	DAE4	SN 1656	12-Jan-22(CTTL-SPEAG No.222-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																			
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																			
Power sensor NRP6S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																			
Reference Probe EKSDV4	SN 7464	26-Jan-22(SPEAG No.E33-71464_Jan22)	Jan-23																			
DAE4	SN 1656	12-Jan-22(CTTL-SPEAG No.222-60007)	Jan-23																			
<table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4383C</td> <td>MY46071430</td> <td>13-Jan-22 (CTTL No. J22X00406)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CTTL No. J22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table>			Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4383C	MY46071430	13-Jan-22 (CTTL No. J22X00406)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																			
Signal Generator E4383C	MY46071430	13-Jan-22 (CTTL No. J22X00406)	Jan-23																			
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23																			
<table border="1"> <thead> <tr> <th>Calibrated by:</th> <th>Name</th> <th>Function</th> <th>Signature</th> </tr> </thead> <tbody> <tr> <td>Reviewed by:</td> <td>Lin Hao</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Approved by:</td> <td>Qi Dianyuan</td> <td>SAR Project Leader</td> <td></td> </tr> </tbody> </table>			Calibrated by:	Name	Function	Signature	Reviewed by:	Lin Hao	SAR Test Engineer		Approved by:	Qi Dianyuan	SAR Project Leader									
Calibrated by:	Name	Function	Signature																			
Reviewed by:	Lin Hao	SAR Test Engineer																				
Approved by:	Qi Dianyuan	SAR Project Leader																				
<p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p>																						
<p>Certificate No: Z22-60185 Page 1 of 6</p>																						

<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4208633-2117 E-mail: cti@china.ttl.com</p>	
<p>Glossary:</p> <p>TSL: Issue simulating liquid ConW: sensitivity in TSL / NORM x,y,z N/A: not applicable or not measured</p>	
<p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865964, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p>	
<p>Additional Documentation:</p> <p>c) DASY4/8 System Handbook</p>	
<p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the fat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. 	
<p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p>	
<p>Certificate No: Z22-60185 Page 2 of 6</p>	

<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4208633-2117 E-mail: cti@china.ttl.com</p>																			
<p>Measurement Conditions</p> <p>DASY system configuration, as far as not given on page 1</p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY92</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 9 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>1900 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table>		DASY Version	DASY92	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 9 mm		Frequency	1900 MHz ± 1 MHz	
DASY Version	DASY92	52.10.4																	
Extrapolation	Advanced Extrapolation																		
Phantom	Triple Flat Phantom 5.1C																		
Distance Dipole Center - TSL	10 mm	with Spacer																	
Zoom Scan Resolution	dx, dy, dz = 9 mm																		
Frequency	1900 MHz ± 1 MHz																		
<p>Head TSL parameters</p> <p>The following parameters and calculations were applied:</p> <table border="1"> <thead> <tr> <th>Parameter</th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>40.0</td> <td>1.40 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.9 ± 6 %</td> <td>1.39 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table>		Parameter	Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.9 ± 6 %	1.39 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---		
Parameter	Temperature	Permittivity	Conductivity																
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m																
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.9 ± 6 %	1.39 mho/m ± 6 %																
Head TSL temperature change during test	<1.0 °C	---	---																
<p>SAR result with Head TSL</p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm² (10 g) of Head TSL</th> <th>Condition</th> <th>Result</th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>9.55 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>40.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm² (10 g) of Head TSL</td> <th>Condition</th> <th>Result</th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.18 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>20.8 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table>		SAR averaged over 1 cm ² (10 g) of Head TSL	Condition	Result	SAR measured	250 mW input power	9.55 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	Result	SAR measured	250 mW input power	5.18 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (k=2)
SAR averaged over 1 cm ² (10 g) of Head TSL	Condition	Result																	
SAR measured	250 mW input power	9.55 W/kg																	
SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 18.8 % (k=2)																	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	Result																	
SAR measured	250 mW input power	5.18 W/kg																	
SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (k=2)																	
<p>Certificate No: Z22-60185 Page 3 of 6</p>																			

<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4208633-2117 E-mail: cti@china.ttl.com</p>							
<p>Appendix (Additional assessments outside the scope of CNAS L0570)</p>							
<p>Antenna Parameters with Head TSL</p> <table border="1"> <thead> <tr> <th>Parameter</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td>51.2Ω ± 7.5Ω(j)</td> </tr> <tr> <td>Return Loss</td> <td>-22.4dB</td> </tr> </tbody> </table>		Parameter	Value	Impedance, transformed to feed point	51.2Ω ± 7.5Ω(j)	Return Loss	-22.4dB
Parameter	Value						
Impedance, transformed to feed point	51.2Ω ± 7.5Ω(j)						
Return Loss	-22.4dB						
<p>General Antenna Parameters and Design</p> <table border="1"> <thead> <tr> <th>Parameter</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>1.109 ns</td> </tr> </tbody> </table>		Parameter	Value	Electrical Delay (one direction)	1.109 ns		
Parameter	Value						
Electrical Delay (one direction)	1.109 ns						
<p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is oriented short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p>							
<p>Additional EUT Data</p> <table border="1"> <thead> <tr> <th>Parameter</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table>		Parameter	Value	Manufactured by	SPEAG		
Parameter	Value						
Manufactured by	SPEAG						
<p>Certificate No: Z22-60185 Page 4 of 6</p>							



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com


In Collaboration with **TTL Speag** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanRoad, Haidian District, Beijing, 100191, China
Tel: +86-10-6258663-2117 E-mail: cti@china.ttl.com http://www.caict.ac.cn

DASY5 Validation Report for Head TSL Date: 2022-06-07
Test Laboratory: CTTL, Beijing, China
DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 54126
Communication System: UTD 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 1900$ MHz; $\alpha = 1.385$ S/m; $\epsilon = 39.85$; $\rho = 1000$ kg/m³
Phantom section: Right Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7464; Conv.F(R, L, 8, 18, 8, 18) @ 1900 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Ser1556; Calibrated: 2022-01-12
- Phantom: MFR VS.1C (20kg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52.10.4(1535); SEMCAD X.18.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 99.99 V/m; Power Drift = 0.04 dB
Peak SAR (extrapolated) = 18.6 W/kg
SAR(1g) = 9.95 W/kg; SAR(10g) = 5.18 W/kg
Smallest distance from peaks to all points: 3 dB below = 9.2 mm
Ratio of SAR at M2 to SAR at M1 = 54.1%
Maximum value of SAR (measured) = 15.6 W/kg

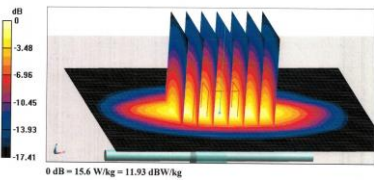


Certificate No: Z22-60185 Page 3 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanRoad, Haidian District, Beijing, 100191, China
Tel: +86-10-6258663-2117 E-mail: cti@china.ttl.com http://www.caict.ac.cn

Impedance Measurement Plot for Head TSL

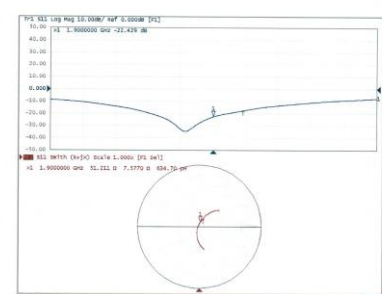

Certificate No: Z22-60185 Page 4 of 6

1.8 D2000V2 - SN 1041

In Collaboration with **TTL Speag** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanRoad, Haidian District, Beijing, 100191, China
Tel: +86-10-6258663-2117 E-mail: cti@china.ttl.com http://www.caict.ac.cn

Client: **SGS-CN** Certificate No: **Z22-60186**

CALIBRATION CERTIFICATE

Object: D2000V2 - SN: 1041

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: June 8, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (S). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (23±3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	110277	24-Sep-21 (CTTL No.Z21X08208)	Sep-22
Power sensor NRPBS	104291	24-Sep-21 (CTTL No.Z21X08208)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG No EX3-7464-Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.Z22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.Z22X00406)	Jan-23

Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Diaryuan	SAR Project Leader	

Issued: June 13, 2022
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60186 Page 1 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanRoad, Haidian District, Beijing, 100191, China
Tel: +86-10-6258663-2117 E-mail: cti@china.ttl.com http://www.caict.ac.cn

Glossary:

TSL: Issue simulating liquid
ConvF: sensitivity in TSL / NGRMx.yz
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedures for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-Held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 855964, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/S System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60186 Page 2 of 6





Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed on separate leaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com
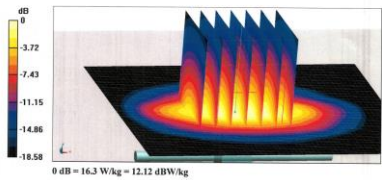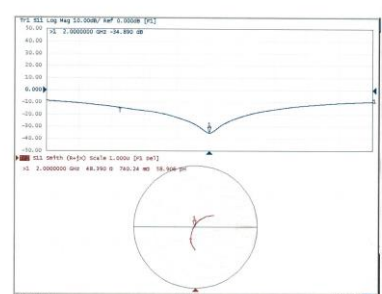
<p>In Collaboration with TTL S p e a g CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6236832-2117 E-mail: ott@china.com http://www.caict.ac.cn</p> <p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p> <table border="1"> <tr><td>DASY Version</td><td>DASY52</td><td>52.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr> <tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr> <tr><td>Frequency</td><td>2000 MHz ± 1 MHz</td><td></td></tr> </table> <p>Head TSL parameters The following parameters and calculations were applied:</p> <table border="1"> <tr><th>Nominal Head TSL parameters</th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr> <tr><td></td><td>22.0 °C</td><td>40.0</td><td>1.40 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22 ± 0.2) °C</td><td>40.2 ± 6 %</td><td>1.39 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td><±1.0 °C</td><td>---</td><td>---</td></tr> </table> <p>SAR result with Head TSL</p> <table border="1"> <tr><th>SAR averaged over 1 cm³ (1 g) of Head TSL</th><th>Condition</th><th></th></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>10.4 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>41.8 W/kg ± 18.8 % (n=2)</td></tr> <tr><th>SAR averaged over 10 cm³ (10 g) of Head TSL</th><th>Condition</th><th></th></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>5.30 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>21.3 W/kg ± 18.7 % (n=2)</td></tr> </table> <p>Certificate No: Z22-60186 Page 3 of 6</p>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2000 MHz ± 1 MHz		Nominal Head TSL parameters	Temperature	Permittivity	Conductivity		22.0 °C	40.0	1.40 mho/m	Measured Head TSL parameters	(22 ± 0.2) °C	40.2 ± 6 %	1.39 mho/m ± 6 %	Head TSL temperature change during test	<±1.0 °C	---	---	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	10.4 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 18.8 % (n=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	5.30 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 18.7 % (n=2)	<p>In Collaboration with TTL S p e a g CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6236832-2117 E-mail: ott@china.com http://www.caict.ac.cn</p> <p>Appendix (Additional assessments outside the scope of CNAS L6070)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <tr><td>Impedance, transformed to feed point</td><td>48.4 ± 0.74 Ω</td></tr> <tr><td>Return Loss</td><td>-34.8 dB</td></tr> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <tr><td>Electrical Delay (one direction)</td><td>1.088 ns</td></tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <tr><td>Manufactured by</td><td>SPEAG</td></tr> </table> <p>Certificate No: Z22-60186 Page 4 of 6</p>	Impedance, transformed to feed point	48.4 ± 0.74 Ω	Return Loss	-34.8 dB	Electrical Delay (one direction)	1.088 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple Flat Phantom 5.1C																																																												
Distance Dipole Center - TSL	10 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																												
Frequency	2000 MHz ± 1 MHz																																																												
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																																																										
	22.0 °C	40.0	1.40 mho/m																																																										
Measured Head TSL parameters	(22 ± 0.2) °C	40.2 ± 6 %	1.39 mho/m ± 6 %																																																										
Head TSL temperature change during test	<±1.0 °C	---	---																																																										
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	10.4 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 18.8 % (n=2)																																																											
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	5.30 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 18.7 % (n=2)																																																											
Impedance, transformed to feed point	48.4 ± 0.74 Ω																																																												
Return Loss	-34.8 dB																																																												
Electrical Delay (one direction)	1.088 ns																																																												
Manufactured by	SPEAG																																																												
<p>In Collaboration with TTL S p e a g CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6236832-2117 E-mail: ott@china.com http://www.caict.ac.cn</p> <p>DASY5 Validation Report for Head TSL Date: 2022-06-06 Test Laboratory: TTL, Beijing, China DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1041 Communication System: UTD 0, CW; Frequency: 2000 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2000 MHz; σ = 1.392 S/m; ε = 40.21; ρ = 1000 kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:</p> <ul style="list-style-type: none"> Probe: EX3DV4 - SN7464; ConvF(8.2, 8.2, 8.2) @ 2000 MHz; Calibrated: 2022-01-26 Sensor-Surface: 1.4mm (Mechanical Surface Detection) Electronics: DA64 Sn1556; Calibrated: 2022-01-12 Phantom: MFP_V5.1C (20kg probe 01); Type: QD 000 P51 Cx; Serial: 1062 DASY52.10.4(S35); SEMCAD X (4.6.14.7501) <p>Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 103.4 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 19.6 W/kg SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg Smallest distance from peaks to all points 3 dB below = 9.1 mm Ratio of SAR at M2 to SAR at M1 = 53.6% Maximum value of SAR (measured) = 16.3 W/kg</p>  <p>Certificate No: Z22-60186 Page 5 of 6</p>	<p>In Collaboration with TTL S p e a g CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6236832-2117 E-mail: ott@china.com http://www.caict.ac.cn</p> <p>Impedance Measurement Plot for Head TSL</p>  <p>Certificate No: Z22-60186 Page 6 of 6</p>																																																												














Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.9 D2300V2 - SN 1096

 		 																					
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-62366433-2512 Fax: +86-10-62366433-2504 E-mail: cti@chinaast.com http://www.chinaast.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62366433-2079 Fax: +86-10-62366433-2504 E-mail: cti@chinaast.com http://www.chinaast.com																					
Client: SGS-CN Certificate No: Z22-60106																							
CALIBRATION CERTIFICATE																							
Object: D2300V2 - SN: 1096																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: March 31, 2022																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity < 70%.																							
Calibration Equipment used (M&TE critical for calibration)																							
<table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL No.J21X08328)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X08328)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21 (SPEAG.No.EX3-7307_May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22 (CTTL-SPEAG.No.Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table>				Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08328)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG.No.EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG.No.Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08328)	Sep-22																				
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22																				
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG.No.EX3-7307_May21)	May-22																				
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG.No.Z22-60007)	Jan-23																				
<table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>MY46071430</td> <td>13-Jan-22 (CTTL No.J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyser E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CTTL No.J22X00409)</td> <td>Jan-23</td> </tr> </tbody> </table>				Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY46071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23	Network Analyser E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Signal Generator E4438C	MY46071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23																				
Network Analyser E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23																				
Calibrated by: Zhao Jing SAR Test Engineer		Signature: 																					
Reviewed by: Lin Hao SAR Test Engineer		Signature: 																					
Approved by: Qi Dianyu SAR Project Leader		Signature: 																					
Issued: April 6, 2022 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							
Certificate No: Z22-60106 Page 1 of 6		Certificate No: Z22-60106 Page 2 of 6																					
																							
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62366433-2079 Fax: +86-10-62366433-2504 E-mail: cti@chinaast.com http://www.chinaast.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62366433-2079 Fax: +86-10-62366433-2504 E-mail: cti@chinaast.com http://www.chinaast.com																					
Measurement Conditions DASY system configuration, as far as not given on page 1																							
<table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY52</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm with Spacer</td> <td></td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2300 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table>				DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm with Spacer		Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2300 MHz ± 1 MHz			
DASY Version	DASY52	52.10.4																					
Extrapolation	Advanced Extrapolation																						
Phantom	Triple Flat Phantom 5.1C																						
Distance Dipole Center - TSL	10 mm with Spacer																						
Zoom Scan Resolution	dx, dy, dz = 5 mm																						
Frequency	2300 MHz ± 1 MHz																						
Head TSL parameters The following parameters and calculations were applied.																							
<table border="1"> <thead> <tr> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.5</td> <td>1.67 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.8 ± 6 %</td> <td>1.70 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>< 1.0 °C</td> <td>—</td> <td>—</td> </tr> </tbody> </table>				Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.70 mho/m ± 6 %	Head TSL temperature change during test	< 1.0 °C	—	—					
Temperature	Permittivity	Conductivity																					
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m																				
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.70 mho/m ± 6 %																				
Head TSL temperature change during test	< 1.0 °C	—	—																				
SAR result with Head TSL																							
<table border="1"> <thead> <tr> <th>SAR averaged over 1 cm² (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>12.4 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>49.2 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm² (10 g) of Head TSL</td> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.88 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>23.4 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table>				SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		SAR measured	250 mW input power	12.4 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		SAR measured	250 mW input power	5.88 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)		
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition																						
SAR measured	250 mW input power	12.4 W/kg																					
SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (k=2)																					
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition																						
SAR measured	250 mW input power	5.88 W/kg																					
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)																					
Certificate No: Z22-60106 Page 3 of 6		Certificate No: Z22-60106 Page 4 of 6																					
																							
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62366433-2079 Fax: +86-10-62366433-2504 E-mail: cti@chinaast.com http://www.chinaast.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62366433-2079 Fax: +86-10-62366433-2504 E-mail: cti@chinaast.com http://www.chinaast.com																					
Appendix (Additional assessments outside the scope of CNAS L0570)																							
Antenna Parameters with Head TSL																							
<table border="1"> <thead> <tr> <th>Impedance, transformed to feed point</th> <th>49.20 - 4.56jΩ</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-26.5dB</td> </tr> </tbody> </table>				Impedance, transformed to feed point	49.20 - 4.56jΩ	Return Loss	-26.5dB																
Impedance, transformed to feed point	49.20 - 4.56jΩ																						
Return Loss	-26.5dB																						
General Antenna Parameters and Design																							
<table border="1"> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>1.083 ns</td> </tr> </tbody> </table>				Electrical Delay (one direction)	1.083 ns																		
Electrical Delay (one direction)	1.083 ns																						
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.																							
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.																							
Additional EUT Data																							
<table border="1"> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table>				Manufactured by	SPEAG																		
Manufactured by	SPEAG																						



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2084
E-mail: cti@china.ttl.com http://www.china.ttl.com

DASY5 Validation Report for Head TSL Date: 2022-03-31
Test Laboratory: CTTL, Beijing, China
DUT: Dipole 2300 MHz; Type: D2300V2; Serial: D2300V2 - SN: 1096
Communication System: UID 0, CW; Frequency: 2300 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2300$ MHz; $\sigma = 1.702$ S/m; $\epsilon = 39.77$; $\rho = 1000$ kg/m³
Phantom section: Right Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(R.01, 8.01, 8.01) @ 2300 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA64 Sml1556; Calibrated: 2022-01-13
- Phantom: MFP_V5.1C (2ldag probe kit); Type: QD 000 P51 Cx; Serial: 1062
- DASY5 52.10.4(1535); SEMCAD X 14.6,14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 102.7 V/m; Power Drift = 0.00 dB
Peak SAR (extrapolated) = 24.8 W/kg
SAR(1 g) = 12.4 W/kg; SAR(10 g) = 5.88 W/kg
Smallest distance from peaks to all points 3 dB below = 9 mm
Ratio of SAR at M2 to SAR at M1 = 50.4%
Maximum value of SAR (measured) = 20.3 W/kg

Certificate No: Z22-60106 Page 1 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2084
E-mail: cti@china.ttl.com http://www.china.ttl.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60106 Page 6 of 6

1.10 D2450V2 - SN 817

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT** **CNAS** 中国认可 国家认证 校准 CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2084
E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60107**

CALIBRATION CERTIFICATE

Object: **D2450V2 - SN: 817**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **April 1, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No. J22X00408)	Jan-23
Network Analyzer E5071C	MY48110873	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer
Reviewed by: **Lin Hao** SAR Test Engineer
Approved by: **Qi Dianyan** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60107 Page 1 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2084
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:

- TSL: tissue simulating liquid
- ConvF: sensitivity in TSL / NORMx.y.z
- N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528: "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/S System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60107 Page 2 of 6













Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed on the back, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

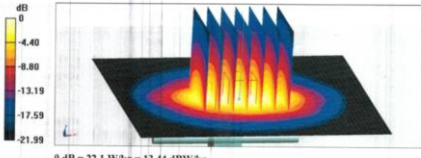t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

<p style="text-align: center;">   </p> <p style="font-size: small;"> In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn </p> <p>Measurement Conditions DASYS system configuration, as far as not given on page 1.</p> <table border="1"> <tr> <td>DASYS Version</td> <td>DASYS2</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 6 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2450 MHz ± 1 Mhz</td> <td></td> </tr> </table> <p>Head TSL parameters The following parameters and calculations were applied.</p> <table border="1"> <tr> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.2</td> <td>1.80 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.5 ± 6 %</td> <td>1.79 mho/m ± 8 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>---</td> <td>---</td> </tr> </table> <p>SAR result with Head TSL</p> <table border="1"> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>13.2 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>53.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm³ (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>6.15 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>24.7 W/kg ± 18.7 % (k=2)</td> </tr> </table>	DASYS Version	DASYS2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 6 mm		Frequency	2450 MHz ± 1 Mhz		Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 8 %	Head TSL temperature change during test	<1.0 °C	---	---	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	13.2 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	53.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	6.15 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)	<p style="text-align: center;">   </p> <p style="font-size: small;"> In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn </p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>52.10-3.20jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-28.5dB</td> </tr> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>1.066 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table>	Impedance, transformed to feed point	52.10-3.20jΩ	Return Loss	-28.5dB	Electrical Delay (one direction)	1.066 ns	Manufactured by	SPEAG
DASYS Version	DASYS2	52.10.4																																																										
Extrapolation	Advanced Extrapolation																																																											
Phantom	Triple Flat Phantom 5.1C																																																											
Distance Dipole Center - TSL	10 mm	with Spacer																																																										
Zoom Scan Resolution	dx, dy, dz = 6 mm																																																											
Frequency	2450 MHz ± 1 Mhz																																																											
Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m																																																									
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 8 %																																																									
Head TSL temperature change during test	<1.0 °C	---	---																																																									
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																											
SAR measured	250 mW input power	13.2 W/kg																																																										
SAR for nominal Head TSL parameters	normalized to 1W	53.0 W/kg ± 18.8 % (k=2)																																																										
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																											
SAR measured	250 mW input power	6.15 W/kg																																																										
SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)																																																										
Impedance, transformed to feed point	52.10-3.20jΩ																																																											
Return Loss	-28.5dB																																																											
Electrical Delay (one direction)	1.066 ns																																																											
Manufactured by	SPEAG																																																											
<p>Certificate No: Z22-60107 Page 3 of 6</p> <p style="text-align: center;">   </p> <p style="font-size: small;"> In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn </p> <p>DASYS Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China. Date: 2022-04-01 DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817 Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz; σ = 1.79 S/m; ε = 39.52; ρ = 1000 kg/m³ Phantom section: Right Section Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007) DASYS Configuration:</p> <ul style="list-style-type: none"> Probe: EX3DV4 - SN7307; ConvF(7.75, 7.75, 7.75) @ 2450 MHz; Calibrated: 2021-05-26 Sensor-Surface: 1.4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1556; Calibrated: 2022-01-12 Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 DASYS2 52.10.4(1535); SEMCAD X 14.6.14(7501) <p>Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 104.6 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 27.0 W/kg SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.15 W/kg Smallest distance from peaks to all points 3 dB below = 8.9 mm Ratio of SAR at M2 to SAR at M1 = -49.2% Maximum value of SAR (measured) = 22.1 W/kg</p>  <p>0 dB = 22.1 W/kg = 13.44 dBW/kg</p>	<p>Certificate No: Z22-60107 Page 4 of 6</p> <p style="text-align: center;">   </p> <p style="font-size: small;"> In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn </p> <p>Impedance Measurement Plot for Head TSL</p> 																																																											
<p>Certificate No: Z22-60107 Page 5 of 6</p>	<p>Certificate No: Z22-60107 Page 6 of 6</p>																																																											














Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300 t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.11 D2600V2 - SN 1158

 		 																					
Client: SGS-CN Certificate No: Z22-60108																							
CALIBRATION CERTIFICATE																							
Object: D2600V2 - SN: 1158																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: March 31, 2022																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.																							
Calibration Equipment used (M&TE critical for calibration)																							
<table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21(SPEAG.No.EX3-7307_May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22(CTTL-SPEAG.No.Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table>				Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Reference Probe EX3DV4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22																				
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23																				
<table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>MY48071438</td> <td>13-Jan-22 (CTTL No.J22X03049)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY48110673</td> <td>14-Jan-22 (CTTL No.J22X03049)</td> <td>Jan-23</td> </tr> </tbody> </table>				Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY48071438	13-Jan-22 (CTTL No.J22X03049)	Jan-23	Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X03049)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Signal Generator E4438C	MY48071438	13-Jan-22 (CTTL No.J22X03049)	Jan-23																				
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X03049)	Jan-23																				
Calibrated by: Zhao Jing SAR Test Engineer 																							
Reviewed by: Lin Hao SAR Test Engineer 																							
Approved by: Qi Dianyuan SAR Project Leader 																							
Issued: April 6, 2022 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							
Certificate No: Z22-60108		Page 1 of 6																					
 		 																					
Measurement Conditions DASY system configuration, as far as not given on page 1.																							
<table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY52</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2650 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table>				DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2650 MHz ± 1 MHz			
DASY Version	DASY52	52.10.4																					
Extrapolation	Advanced Extrapolation																						
Phantom	Triple Flat Phantom 5.1C																						
Distance Dipole Center - TSL	10 mm	with Spacer																					
Zoom Scan Resolution	dx, dy, dz = 5 mm																						
Frequency	2650 MHz ± 1 MHz																						
Head TSL parameters The following parameters and calculations were applied.																							
<table border="1"> <thead> <tr> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.0</td> <td>1.96 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>38.7 ± 6 %</td> <td>1.96 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table>				Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.96 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---					
Temperature	Permittivity	Conductivity																					
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m																				
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.96 mho/m ± 6 %																				
Head TSL temperature change during test	<1.0 °C	---	---																				
SAR result with Head TSL																							
<table border="1"> <thead> <tr> <th>SAR averaged over 1 cm² (1 g) of Head TSL</th> <th>Condition</th> <th>13.7 W/kg</th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td></td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>54.8 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm² (10 g) of Head TSL</td> <th>Condition</th> <th>6.12 W/kg</th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td></td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>24.5 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table>				SAR averaged over 1 cm ² (1 g) of Head TSL	Condition	13.7 W/kg	SAR measured	250 mW input power		SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	6.12 W/kg	SAR measured	250 mW input power		SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)		
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition	13.7 W/kg																					
SAR measured	250 mW input power																						
SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)																					
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	6.12 W/kg																					
SAR measured	250 mW input power																						
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)																					
Certificate No: Z22-60108		Page 3 of 6																					
Appendix (Additional assessments outside the scope of CNAS L0570)																							
Antenna Parameters with Head TSL																							
<table border="1"> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td>49.90 - 6.49jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-23.8dB</td> </tr> </tbody> </table>				Impedance, transformed to feed point	49.90 - 6.49jΩ	Return Loss	-23.8dB																
Impedance, transformed to feed point	49.90 - 6.49jΩ																						
Return Loss	-23.8dB																						
General Antenna Parameters and Design																							
<table border="1"> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>1.053 ns</td> </tr> </tbody> </table>				Electrical Delay (one direction)	1.053 ns																		
Electrical Delay (one direction)	1.053 ns																						
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.																							
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.																							
Additional EUT Data																							
<table border="1"> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table>				Manufactured by	SPEAG																		
Manufactured by	SPEAG																						
Certificate No: Z22-60108		Page 4 of 6																					



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
 No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300 t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT


Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-82304633-2079 Fax: +86-10-82304633-2504
 E-mail: cti@ttspeag.com http://www.ttspeag.com

DASY5 Validation Report for Head TSL Date: 2022-03-31

Test Laboratory: CTTL, Beijing, China
DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1158
 Communication System: UID 0, CW; Frequency: 2600 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.955$ S/m; $\epsilon_s = 38.68$; $\rho = 1000$ kg/m³
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(7.5, 7.5) @ 2600 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MEP_V5.1C (2Dtag probe kit); Type: QD 000 P51 Cx; Serial: 1062
- DASY5 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 103.3 V/m; Power Drift = 0.04 dB
 Peak SAR (extrapolated) = 29.0 W/kg
SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.12 W/kg
 Smallest distance from peaks to all points 3 dB below = 8.9 mm
 Ratio of SAR at M2 to SAR at M1 = 47.5%
 Maximum value of SAR (measured) = 23.4 W/kg

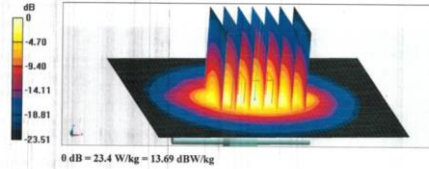

0 dB = 23.4 W/kg = 13.69 dBW/kg


Certificate No: Z22-60108 Page 5 of 6

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-82304633-2079 Fax: +86-10-82304633-2504
 E-mail: cti@ttspeag.com http://www.ttspeag.com

Impedance Measurement Plot for Head TSL

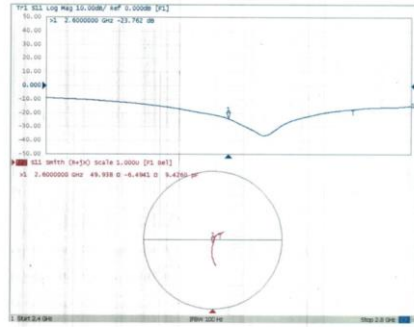

Certificate No: Z22-60108 Page 6 of 6

1.12 D5GHzV2 - SN 1095

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-82304633-2079 Fax: +86-10-82304633-2504
 E-mail: cti@ttspeag.com http://www.ttspeag.com

Client: **SGS-CN** Certificate No: **Z22-60187**

CALIBRATION CERTIFICATE

Object: **D5GHzV2 - SN: 1095**

Calibration Procedure(s): **FF-Z11-003-01**
 Calibration Procedures for dipole validation kits

Calibration date: **June 1, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X06326)	Step-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X06326)	Step-22
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG.No.EX3-7464_Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer

Reviewed by: **Lin Hao** SAR Test Engineer

Approved by: **Qi Diqian** SAR Project Leader

Issued: June 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60187 Page 1 of 10

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-82304633-2079 Fax: +86-10-82304633-2504
 E-mail: cti@ttspeag.com http://www.ttspeag.com

Glossary:

TSL: Issue simulating liquid sensitivity in TSL / NORM.y,z

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure for the Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- ICB 865964, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transferred from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60187 Page 2 of 10



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

In Collaboration with **SPQ** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62321117
E-mail: utsg@chinaet.com.cn http://www.caict.ac.cn

Measurement Conditions
DASY system configuration, as far as not given on page 1.

DASY Version	DASYV2	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5200 MHz ± 1 MHz 5300 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5200MHz
The following parameters and calculations were applied.

Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.62 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5200MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	7.79 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	77.6 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.22 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)

Certificate No: Z22-60187 Page 3 of 10

In Collaboration with **SPQ** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62321117
E-mail: utsg@chinaet.com.cn http://www.caict.ac.cn

Head TSL parameters at 5300MHz
The following parameters and calculations were applied.

Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5300MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.94 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	79.1 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.27 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg ± 24.2 % (k=2)

Head TSL parameters at 5500MHz
The following parameters and calculations were applied.

Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.94 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5500MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.26 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	82.5 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.34 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg ± 24.2 % (k=2)

Certificate No: Z22-60187 Page 4 of 10

In Collaboration with **SPQ** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62321117
E-mail: utsg@chinaet.com.cn http://www.caict.ac.cn

Head TSL parameters at 5600MHz
The following parameters and calculations were applied.

Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.05 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5600MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.12 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	80.8 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.9 W/kg ± 24.2 % (k=2)

Head TSL parameters at 5800MHz
The following parameters and calculations were applied.

Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.25 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5800MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.71 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	76.7 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.16 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.5 W/kg ± 24.2 % (k=2)

Certificate No: Z22-60187 Page 5 of 10

In Collaboration with **SPQ** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62321117
E-mail: utsg@chinaet.com.cn http://www.caict.ac.cn

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL at 5200MHz

Impedance, transformed to feed point	48.1D-8.03jΩ
Return Loss	-23.6dB

Antenna Parameters with Head TSL at 5300MHz

Impedance, transformed to feed point	47.8D-2.42jΩ
Return Loss	-28.5dB

Antenna Parameters with Head TSL at 5500MHz

Impedance, transformed to feed point	50.3D-4.29jΩ
Return Loss	-27.4dB

Antenna Parameters with Head TSL at 5600MHz

Impedance, transformed to feed point	54.5D-4.80jΩ
Return Loss	-24.6dB

Antenna Parameters with Head TSL at 5800MHz

Impedance, transformed to feed point	51.5D-5.61jΩ
Return Loss	-24.9dB

Certificate No: Z22-60187 Page 6 of 10

Compliance Certification Services (Kunshan) Inc. Inspection & Testing Services

中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

程智电子科技有限公司 (昆山) 有限公司
检验检测专用章
Inspection & Testing Services
Compliance Certification Services (Kunshan) Inc.

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

<div data-bbox="271 358 710 448"> <p>In Collaboration with TTL CALIBRATION LABORATORY CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62920117 E-mail: ott@china.ttl.com http://www.caict.ac.cn</p> </div> <div data-bbox="271 448 710 492"> <p>General Antenna Parameters and Design</p> <p>Electrical Delay (one direction): 1.101 na</p> </div> <div data-bbox="271 492 710 593"> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> </div> <div data-bbox="271 593 710 649"> <p>Additional EUT Data</p> <p>Manufactured by: SPEAG</p> </div> <div data-bbox="271 940 710 985"> <p>Certificate No: Z22-60187 Page 7 of 10</p> </div>	<div data-bbox="877 358 1316 448"> <p>In Collaboration with TTL CALIBRATION LABORATORY CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62920117 E-mail: ott@china.ttl.com http://www.caict.ac.cn</p> </div> <div data-bbox="877 448 1316 470"> <p>DASY5 Validation Report for Head STL</p> <p>Test Laboratory: GTTL, Beijing, China Date: 2022-06-01</p> </div> <div data-bbox="877 470 1316 716"> <p>DUT: Dipole 5GHz; Type: DSGHzV2; Serial: DSGHzV2 - SN: 1095</p> <p>Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1 Medium parameters used: f = 5200 MHz; $\sigma = 4.62$ S/m; $\epsilon_r = 35.39$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5300 MHz; $\sigma = 4.73$ S/m; $\epsilon_r = 35.19$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5500 MHz; $\sigma = 4.939$ S/m; $\epsilon_r = 34.83$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5600 MHz; $\sigma = 5.051$ S/m; $\epsilon_r = 34.69$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5800 MHz; $\sigma = 5.247$ S/m; $\epsilon_r = 34.42$; $\rho = 1000$ kg/m³ Phantom section: Right Section Measurement standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:</p> <ul style="list-style-type: none"> Probe: EX3DV4 - SN7484; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5, 5, 5) @ 5800 MHz; Calibrated: 2022-01-26 Sensor-Surface: 1.4mm (Mechanical Surface Detection) Electronics: DA64 Sn1558; Calibrated: 2022-01-12 Phantom: MFP_V5-1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) </div> <div data-bbox="877 716 1316 940"> <p>Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 60.80 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 29.8 W/kg SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.22 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 66.8% Maximum value of SAR (measured) = 18.3 W/kg</p> <p>Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 31.5 W/kg SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65.5% Maximum value of SAR (measured) = 19.0 W/kg</p> </div> <div data-bbox="877 940 1316 985"> <p>Certificate No: Z22-60187 Page 8 of 10</p> </div>
<div data-bbox="271 1030 710 1120"> <p>In Collaboration with TTL CALIBRATION LABORATORY CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62920117 E-mail: ott@china.ttl.com http://www.caict.ac.cn</p> </div> <div data-bbox="271 1120 710 1220"> <p>Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.82 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 34.7 W/kg SAR(1 g) = 8.29 W/kg; SAR(10 g) = 2.34 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 63.9% Maximum value of SAR (measured) = 20.2 W/kg</p> </div> <div data-bbox="271 1220 710 1332"> <p>Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 35.2 W/kg SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.3 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 62.5% Maximum value of SAR (measured) = 19.1 W/kg</p> </div> <div data-bbox="271 1332 710 1444"> <p>Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 62.13 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 34.8 W/kg SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 61.6% Maximum value of SAR (measured) = 18.7 W/kg</p> </div> <div data-bbox="271 1444 710 1624"> </div> <div data-bbox="271 1624 710 1668"> <p>Certificate No: Z22-60187 Page 9 of 10</p> </div>	<div data-bbox="877 1030 1316 1120"> <p>In Collaboration with TTL CALIBRATION LABORATORY CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62920117 E-mail: ott@china.ttl.com http://www.caict.ac.cn</p> </div> <div data-bbox="877 1120 1316 1142"> <p>Impedance Measurement Plot for Head STL</p> </div> <div data-bbox="877 1142 1316 1456"> </div> <div data-bbox="877 1456 1316 1668"> <p>Certificate No: Z22-60187 Page 10 of 10</p> </div>



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

2 DAE4 - SN 1245

<p style="text-align: center;">s p e a g</p> <p style="text-align: center;">IMPORTANT NOTICE</p> <p>USAGE OF THE DAE4</p> <p>The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:</p> <p>Battery Exchange: The battery cover of the DAE4 unit is fixed using a screw, over tightening the screw may cause the threads inside the DAE to wear out.</p> <p>Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an anti-static bag. This anti-static bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.</p> <p>E-Stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.</p> <p>Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough professional handling caused the defect.</p> <p>DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file.</p> <p>Important Note: Warning and calibration is void if the DAE unit is disassembled partly or fully by the Customer.</p> <p>Important Note: Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure.</p> <p>Important Note: To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.</p> <p style="font-size: small;">TH_EH190306AE DAE4.docx 07.03.2019</p>	<p style="text-align: center;">Calibration Laboratory of Schmid & Partner Engineering AG</p> <p style="text-align: center; font-size: small;">Zeughausstrasse 43, 8004 Zurich, Switzerland</p> <p style="text-align: center; font-size: x-small;">Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p style="text-align: center; font-size: x-small;">Client: SGS-CN (Audem) Certificate No: DAE4-1245_May22</p> <p style="text-align: center;">CALIBRATION CERTIFICATE</p> <p>Client: DAE4 - SD 000 D04 BM - SN: 1245</p> <p>Calibration procedure(s): QA CAL-06.v30 Calibration procedure for the data acquisition electronics (DAE)</p> <p>Calibration date: May 30, 2022</p> <p style="font-size: x-small;">This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p style="font-size: x-small;">All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.</p> <p style="font-size: x-small;">Calibration Equipment used (MATE critical for calibration)</p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Kelvin Multimeter Type 2001</td> <td>SN: 0810276</td> <td>31-Aug-21 (No.31366)</td> <td>Aug-22</td> </tr> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> <tr> <td>Auto DMC Calibration Unit</td> <td>SE LMS 000 AA 1001</td> <td>24-Jan-22 (in house check)</td> <td>In house check: Jan-23</td> </tr> <tr> <td>Calibrator Box V2.1</td> <td>SE LMS 000 AA 1002</td> <td>24-Jan-22 (in house check)</td> <td>In house check: Jan-23</td> </tr> </table> <p>Calibrated by: Dominique Steffen (Name) / Laboratory Technician (Function) / <i>[Signature]</i> (Signature)</p> <p>Approved by: Steen Kullen (Name) / Technical Manager (Function) / <i>[Signature]</i> (Signature)</p> <p style="font-size: x-small;">This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued: May 30, 2022</p> <p style="font-size: x-small;">Certificate No: DAE4-1245_May22 Page 1 of 5</p>	Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Kelvin Multimeter Type 2001	SN: 0810276	31-Aug-21 (No.31366)	Aug-22	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Auto DMC Calibration Unit	SE LMS 000 AA 1001	24-Jan-22 (in house check)	In house check: Jan-23	Calibrator Box V2.1	SE LMS 000 AA 1002	24-Jan-22 (in house check)	In house check: Jan-23
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																		
Kelvin Multimeter Type 2001	SN: 0810276	31-Aug-21 (No.31366)	Aug-22																		
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																		
Auto DMC Calibration Unit	SE LMS 000 AA 1001	24-Jan-22 (in house check)	In house check: Jan-23																		
Calibrator Box V2.1	SE LMS 000 AA 1002	24-Jan-22 (in house check)	In house check: Jan-23																		
<p style="text-align: center;">Calibration Laboratory of Schmid & Partner Engineering AG</p> <p style="text-align: center; font-size: small;">Zeughausstrasse 43, 8004 Zurich, Switzerland</p> <p style="text-align: center; font-size: x-small;">Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p style="text-align: center; font-size: x-small;">Accreditation No.: SCS 0108</p> <p>Glossary</p> <p>DAE: data acquisition electronics</p> <p>Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system.</p> <p>Methods Applied and Interpretation of Parameters</p> <ul style="list-style-type: none"> DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range. Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required. The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty. <ul style="list-style-type: none"> DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement. Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement. Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage. AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage. Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements. Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance. Input resistance: Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement. Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated. Power consumption: Typical value for information. Supply currents in various operating modes. <p style="font-size: x-small;">Certificate No: DAE4-1245_May22 Page 2 of 5</p>	<p>DC Voltage Measurement</p> <p style="font-size: x-small;">AD - Converter Resolution nominal: 6.1µV, full range = -100...+300 mV High Range: 1LSB = 6.1µV, full range = -100...+300 mV Low Range: 1LSB = 61nV, full range = -1...+30mV DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec</p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <thead> <tr> <th>Calibration Factors</th> <th>X</th> <th>Y</th> <th>Z</th> </tr> </thead> <tbody> <tr> <td>High Range</td> <td>405.265 ± 0.02% (k=2)</td> <td>403.974 ± 0.02% (k=2)</td> <td>406.092 ± 0.02% (k=2)</td> </tr> <tr> <td>Low Range</td> <td>3.99534 ± 1.50% (k=2)</td> <td>3.99508 ± 1.50% (k=2)</td> <td>4.01015 ± 1.50% (k=2)</td> </tr> </tbody> </table> <p>Connector Angle</p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <tr> <td>Connector Angle to be used in DASY system</td> <td>30.0° ± 1°</td> </tr> </table> <p style="font-size: x-small;">Certificate No: DAE4-1245_May22 Page 3 of 5</p>	Calibration Factors	X	Y	Z	High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)	Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)	Connector Angle to be used in DASY system	30.0° ± 1°						
Calibration Factors	X	Y	Z																		
High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)																		
Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)																		
Connector Angle to be used in DASY system	30.0° ± 1°																				



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300 t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

Appendix (Additional assessments outside the scope of SCS0108)			
1. DC Voltage Linearity			
High Range			
Channel X + Input	19994.45	1.82	0.00
Channel X + Input	20004.58	2.22	0.01
Channel X - Input	-20000.14	1.12	-0.01
Channel Y + Input	19994.72	1.98	0.00
Channel Y + Input	20001.22	-1.00	-0.00
Channel Y - Input	-20003.05	-1.07	0.01
Channel Z + Input	19992.64	0.19	0.00
Channel Z + Input	20003.09	0.88	0.00
Channel Z - Input	-20001.73	-0.27	0.00
Low Range			
Channel X + Input	201.91	0.41	0.20
Channel X + Input	202.54	0.65	0.32
Channel X - Input	-197.86	0.07	-0.04
Channel Y + Input	202.05	0.58	0.03
Channel Y + Input	201.27	-0.57	-0.28
Channel Y - Input	-198.29	-0.05	0.00
Channel Z + Input	200.29	0.08	0.00
Channel Z + Input	200.09	-1.53	-0.78
Channel Z - Input	-199.85	-1.57	0.79
2. Common mode sensitivity			
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec			
Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)	
Channel X	200	-3.87	-7.69
	-200	9.12	7.79
Channel Y	200	-8.68	-8.28
	-200	8.52	6.36
Channel Z	200	-5.36	-5.80
	-200	3.58	3.08
3. Channel separation			
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec			
Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	4.07
Channel Y	200	9.36	-
Channel Z	200	10.11	7.14
Certificate No: DAE4-1245_Mar22 Page 4 of 5			

4. AD-Converter Values with inputs shorted				
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec				
	High Range (LSB)	Low Range (LSB)		
Channel X	15984	17040		
Channel Y	16562	16788		
Channel Z	16035	15958		
5. Input Offset Measurement				
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec				
Input 10MΩ				
	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	1.00	-0.15	1.93	0.45
Channel Y	-0.18	-1.28	0.94	0.45
Channel Z	-0.58	-2.61	0.58	0.60
6. Input Offset Current				
Nominal input circuitry offset current on all channels: <25nA				
7. Input Resistance (Typical values for information)				
	Zeroing (MΩ)	Measuring (MΩ)		
Channel X	200	200		
Channel Y	200	200		
Channel Z	200	200		
8. Low Battery Alarm Voltage (Typical values for information)				
	Alarm Level (VDC)			
Supply (+ Vec)		+7.9		
Supply (- Vec)		-7.8		
9. Power Consumption (Typical values for information)				
	Switched off (mA)	Stand by (mA)	Transmitting (mA)	
Supply (+ Vec)	<0.01	<6	<14	
Supply (- Vec)	<0.01	<6	<6	

3 EX3DV4 - SN 7346

<p>Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 6, 804 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: Auden Certificate No: EX3-7346_Mar22</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: EX3DV4 - SN 7346</p> <p>Calibration procedure(s): QA CAL-01 v8 QA CAL-14 v6 QA CAL-23 v5 QA CAL-25 V7 Calibration is performed for dosimetric E-field probes</p> <p>Calibration date: March 30, 2022</p> <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 75%.</p> <p>Calibration Equipment used (MTEC critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power source HPF</td> <td>SN: 98178</td> <td>08-Apr-21 (No. 211-021020)</td> <td>Apr-22</td> </tr> <tr> <td>Power source NRP-291</td> <td>SN: 153245</td> <td>09-Apr-21 (No. 211-021091)</td> <td>Apr-22</td> </tr> <tr> <td>Power source NRP-291</td> <td>SN: 153245</td> <td>09-Apr-21 (No. 211-021091)</td> <td>Apr-22</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: C22052 (20)</td> <td>09-Apr-21 (No. 211-021043)</td> <td>Apr-22</td> </tr> <tr> <td>DAE4</td> <td>SN: 660</td> <td>13-Oct-21 (No. 21A-0486_045(21))</td> <td>Oct-22</td> </tr> <tr> <td>Reference Probe ES3012</td> <td>SN: 3013</td> <td>27-Dec-21 (No. ES3-3013_045(21))</td> <td>Dec-22</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power source E4138</td> <td>SN: G18129874</td> <td>08-Apr-21 (in house check Jun-20)</td> <td>In house check Jun-22</td> </tr> <tr> <td>Power source E4413A</td> <td>SN: M71149808</td> <td>08-Apr-21 (in house check Jun-20)</td> <td>In house check Jun-22</td> </tr> <tr> <td>Power source E4413A</td> <td>SN: 020112102</td> <td>08-Apr-21 (in house check Jun-20)</td> <td>In house check Jun-22</td> </tr> <tr> <td>RF generator HP 8640C</td> <td>SN: US342411700</td> <td>04-Aug-19 (in house check Jun-20)</td> <td>In house check Jun-22</td> </tr> <tr> <td>Network Analyzer E8303A</td> <td>SN: US4106047</td> <td>31-Mar-14 (in house check Oct-20)</td> <td>In house check Oct-22</td> </tr> </tbody> </table> <p>Calibrated by: Ivan Kattler (Laboratory Technician) Signature: <i>[Signature]</i></p> <p>Approved by: Ivan Kuhn (Quality Manager) Signature: <i>[Signature]</i></p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued March 31, 2022</p> <p>Certificate No: EX3-7346_Mar22 Page 1 of 24</p>	Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration	Power source HPF	SN: 98178	08-Apr-21 (No. 211-021020)	Apr-22	Power source NRP-291	SN: 153245	09-Apr-21 (No. 211-021091)	Apr-22	Power source NRP-291	SN: 153245	09-Apr-21 (No. 211-021091)	Apr-22	Reference 20 dB Attenuator	SN: C22052 (20)	09-Apr-21 (No. 211-021043)	Apr-22	DAE4	SN: 660	13-Oct-21 (No. 21A-0486_045(21))	Oct-22	Reference Probe ES3012	SN: 3013	27-Dec-21 (No. ES3-3013_045(21))	Dec-22	Secondary Standards	ID	Check Date (in house)	Scheduled Check	Power source E4138	SN: G18129874	08-Apr-21 (in house check Jun-20)	In house check Jun-22	Power source E4413A	SN: M71149808	08-Apr-21 (in house check Jun-20)	In house check Jun-22	Power source E4413A	SN: 020112102	08-Apr-21 (in house check Jun-20)	In house check Jun-22	RF generator HP 8640C	SN: US342411700	04-Aug-19 (in house check Jun-20)	In house check Jun-22	Network Analyzer E8303A	SN: US4106047	31-Mar-14 (in house check Oct-20)	In house check Oct-22	<p>Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 6, 804 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Accreditation No.: SCS 0108</p> <p>Glossary:</p> <p>TSL: Issue simulating input sensitivity in free space</p> <p>NORM_{x,y,z}: sensitivity in TSL / NORM_{x,y,z}</p> <p>ConF: crest factor (15μs, cycle) of the RF signal</p> <p>DCP: diode compression point</p> <p>A, B, C, D: modulation dependent linearization parameters</p> <p>Polarization φ: φ rotation around probe axis</p> <p>Polarization θ: θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., θ = 0 is normal to probe axis</p> <p>Connector Angle: information used in DASY system to align probe sensor X to the robot coordinate system</p> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1208: Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1208: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz), October 2020</p> <p>b) KOB 865664: "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> NORM_{x,y,z}: Assessed for E-field polarization θ = 0 if it is 800 MHz in TEM-coil; f = 1600 MHz: R22 waveguide; NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} do not affect the E-field uncertainty inside TSL (see below ConF). NORM_{x,y,z} < 1: Frequency response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConF. DCP_φ < 1: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media. PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics. A, B, C, D: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. 10% is the maximum calibration range expressed in RMS voltage across the diode. ConF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f < 800 MHz) and wide waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConF whereby the uncertainty corresponds to that given for ConF. A frequency dependent ConF is used in DASY version 4.4 and higher which allows extending the validity from 1.50 MHz to 100 MHz. Spherical Isotropy (3D deviation from isotropy): In a field of low gradients realized using a flat phantom exposed by a patch antenna. Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (or probe axis). No tolerance required. Connector Angle: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required). <p>Certificate No: EX3-7346_Mar22 Page 2 of 24</p>
Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration																																																		
Power source HPF	SN: 98178	08-Apr-21 (No. 211-021020)	Apr-22																																																		
Power source NRP-291	SN: 153245	09-Apr-21 (No. 211-021091)	Apr-22																																																		
Power source NRP-291	SN: 153245	09-Apr-21 (No. 211-021091)	Apr-22																																																		
Reference 20 dB Attenuator	SN: C22052 (20)	09-Apr-21 (No. 211-021043)	Apr-22																																																		
DAE4	SN: 660	13-Oct-21 (No. 21A-0486_045(21))	Oct-22																																																		
Reference Probe ES3012	SN: 3013	27-Dec-21 (No. ES3-3013_045(21))	Dec-22																																																		
Secondary Standards	ID	Check Date (in house)	Scheduled Check																																																		
Power source E4138	SN: G18129874	08-Apr-21 (in house check Jun-20)	In house check Jun-22																																																		
Power source E4413A	SN: M71149808	08-Apr-21 (in house check Jun-20)	In house check Jun-22																																																		
Power source E4413A	SN: 020112102	08-Apr-21 (in house check Jun-20)	In house check Jun-22																																																		
RF generator HP 8640C	SN: US342411700	04-Aug-19 (in house check Jun-20)	In house check Jun-22																																																		
Network Analyzer E8303A	SN: US4106047	31-Mar-14 (in house check Oct-20)	In house check Oct-22																																																		



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

EX3DV4 - SN:7346 March 30, 2022

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $\mu\text{V}/\text{mV}^2$	0.46	0.47	0.61	$\pm 10.1\%$
DGP (mV) ²	101.4	106.0	106.9	

Calibration Results for Modulation Response

UID	Communication System Name	A dB	B dB	C dB	D dB	VR mV	Max dev.	Max Unc (%)
0	CW	X: 0.00, Y: 0.00, Z: 0.00	0.00	0.00	0.00	143.5	$\pm 3.0\%$	$\pm 4.1\%$
10353-AAA	Pulse Waveform (200Hz, 10%)	X: 3.33, Y: 68.90, Z: 4.03	11.66	10.00	66.0	60.0	$\pm 3.5\%$	$\pm 9.6\%$
10353-AAA	Pulse Waveform (200Hz, 20%)	X: 1.63, Y: 61.25, Z: 3.00	6.76	6.99	80.0	80.0	$\pm 2.4\%$	$\pm 9.6\%$
10354-AAA	Pulse Waveform (200Hz, 40%)	X: 7.41, Y: 79.85, Z: 2.93	12.51	3.98	95.0	95.0	$\pm 2.7\%$	$\pm 9.6\%$
10355-AAA	Pulse Waveform (200Hz, 60%)	X: 0.18, Y: 136.38, Z: 1.56	0.01	99.0	120.0	120.0	$\pm 1.7\%$	$\pm 9.6\%$
10387-AAA	QPSK Waveform, 1 MHz	X: 1.47, Y: 64.88, Z: 1.47	13.82	1.00	150.0	150.0	$\pm 4.2\%$	$\pm 9.6\%$
10388-AAA	QPSK Waveform, 10 MHz	X: 0.45, Y: 61.88, Z: 1.51	11.05	0.00	150.0	150.0	$\pm 1.1\%$	$\pm 9.6\%$
10396-AAA	64-QAM Waveform, 100 kHz	X: 2.63, Y: 66.51, Z: 1.74	18.25	3.01	150.0	150.0	$\pm 1.0\%$	$\pm 9.6\%$
10396-AAA	64-QAM Waveform, 40 MHz	X: 1.70, Y: 64.72, Z: 1.38	15.99	0.00	150.0	150.0	$\pm 2.0\%$	$\pm 9.6\%$
10414-AAA	WLAN CCDF, 64-QAM, 40MHz	X: 4.71, Y: 65.35, Z: 1.38	15.27	0.00	150.0	150.0	$\pm 3.8\%$	$\pm 9.6\%$

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

* The uncertainties of Norm X, Y, Z do not affect the E-field uncertainty mode TSI, see Pages 1 and 6.
* Numerical transition parameter, uncertainty not required.
* Uncertainty is determined using the error deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: EX3-7346_Mar22 Page 3 of 24

EX3DV4 - SN:7346 March 30, 2022

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346

Sensor Model Parameters

	C1	C2	a	T1	T2	T3	T4	T5	T6
	°	°	V ⁻¹	ms V ⁻¹	ms V ⁻¹	ms	V ⁻¹	V ⁻¹	V ⁻¹
X	39.3	291.80	35.10	5.63	0.03	5.66	1.42	0.12	1.01
Y	37.1	270.84	34.12	8.29	0.00	5.01	1.82	0.05	1.01
Z	9.7	69.14	33.27	4.96	0.00	4.94	0.61	0.00	1.00

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-166.1
Mechanical Surface Detection Mode	enabled
Cylindrical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Note: Measurement distance from surface can be increased to 3-4 mm for an Area Scan job.

Certificate No: EX3-7346_Mar22 Page 4 of 24

EX3DV4 - SN:7346 March 30, 2022

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz)	Relative Permittivity ¹	Conductivity (S/m) ²	ConvF X	ConvF Y	ConvF Z	Alpha ³	Depth ⁴ (mm)	Unc (k=2)
750	41.8	0.89	10.56	10.56	10.56	0.55	0.85	$\pm 12.0\%$
835	41.5	0.90	10.12	10.12	10.12	0.42	0.96	$\pm 12.0\%$
900	41.5	0.97	10.10	10.10	10.10	0.53	0.80	$\pm 12.0\%$
1426	40.5	1.20	9.26	9.26	9.26	0.50	0.80	$\pm 12.0\%$
1750	40.1	1.37	8.83	8.83	8.83	0.34	0.86	$\pm 12.0\%$
1900	40.0	1.40	8.48	8.48	8.48	0.35	0.86	$\pm 12.0\%$
2000	40.0	1.40	8.35	8.35	8.35	0.34	0.86	$\pm 12.0\%$
2300	39.5	1.67	7.86	7.86	7.86	0.39	0.90	$\pm 12.0\%$
2450	39.2	1.80	7.63	7.63	7.63	0.41	0.90	$\pm 12.0\%$
2600	39.0	1.96	7.33	7.33	7.33	0.44	0.90	$\pm 12.0\%$
3300	38.2	2.71	7.15	7.15	7.15	0.30	1.35	$\pm 13.1\%$
3350	37.8	2.81	7.14	7.14	7.14	0.30	1.35	$\pm 13.1\%$
3700	37.7	3.12	6.65	6.65	6.65	0.30	1.35	$\pm 13.1\%$
3900	37.5	3.32	6.71	6.71	6.71	0.40	1.60	$\pm 13.1\%$
4100	37.2	3.53	6.58	6.58	6.58	0.40	1.60	$\pm 13.1\%$
4200	37.1	3.63	6.30	6.30	6.30	0.40	1.70	$\pm 13.1\%$
4400	36.9	3.84	6.24	6.24	6.24	0.40	1.70	$\pm 13.1\%$
4600	36.7	4.04	6.11	6.11	6.11	0.40	1.70	$\pm 13.1\%$
4800	36.4	4.25	6.08	6.08	6.08	0.40	1.80	$\pm 13.1\%$
4900	36.3	4.40	5.84	5.84	5.84	0.40	1.80	$\pm 13.1\%$
5200	36.0	4.66	5.25	5.25	5.25	0.40	1.80	$\pm 13.1\%$
5300	35.9	4.76	5.12	5.12	5.12	0.40	1.80	$\pm 13.1\%$
5500	35.6	4.98	4.85	4.85	4.85	0.40	1.80	$\pm 13.1\%$
5600	35.5	5.07	4.70	4.70	4.70	0.40	1.80	$\pm 13.1\%$
5800	35.3	5.27	4.75	4.75	4.75	0.40	1.80	$\pm 13.1\%$

¹ Frequency validly above 300 MHz at a 100 MHz only applies for DASY/EASY v4 and higher (see Page 2), else it is restricted to a 50 MHz. The uncertainty is the RSS of ConfF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validly below 300 MHz is 10, 25, 40, 50 and 70 MHz for ConfF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConfF assessed at 8 MHz to 8 MHz, and ConfF assessed at 13 MHz to 13 MHz. Above 12 GHz frequency validly can be extended to a 110 MHz.
² At frequencies below 3 GHz, the validity of tissue parameters (i) and (ii) can be related to a 10% liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (i) and (ii) is restricted to a 3%. The uncertainty in the RSS of the ConfF conductivity for indicated target tissue parameters.
³ Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than 1% for frequencies below 3 GHz and below 3% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.
⁴ Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than 1% for frequencies below 3 GHz and below 3% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX3-7346_Mar22 Page 5 of 24

EX3DV4 - SN:7346 March 30, 2022

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz)	Relative Permittivity ¹	Conductivity (S/m) ²	ConvF X	ConvF Y	ConvF Z	Alpha ³	Depth ⁴ (mm)	Unc (k=2)
6500	34.5	6.07	5.30	5.30	5.30	0.20	2.50	$\pm 19.6\%$

¹ Frequency validly above 600 MHz is a 700 MHz. The uncertainty is the RSS of the ConfF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.
² At frequencies 6-10 GHz, the validity of tissue parameters (i) and (ii) can be related to a 10% liquid compensation formula is applied to measured SAR values. The uncertainty in the RSS of the ConfF uncertainty for indicated target tissue parameters.
³ Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than 1% for frequencies below 3 GHz, below 3% for frequencies between 3-6 GHz, and below 3% for frequencies between 6-10 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX3-7346_Mar22 Page 6 of 24



Compliance Certification Services (Kunshan) Inc.
EMC Laboratory

Test Report Form Version: Rev01


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: C.N.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

Member of the SGS Group (SGS SA)

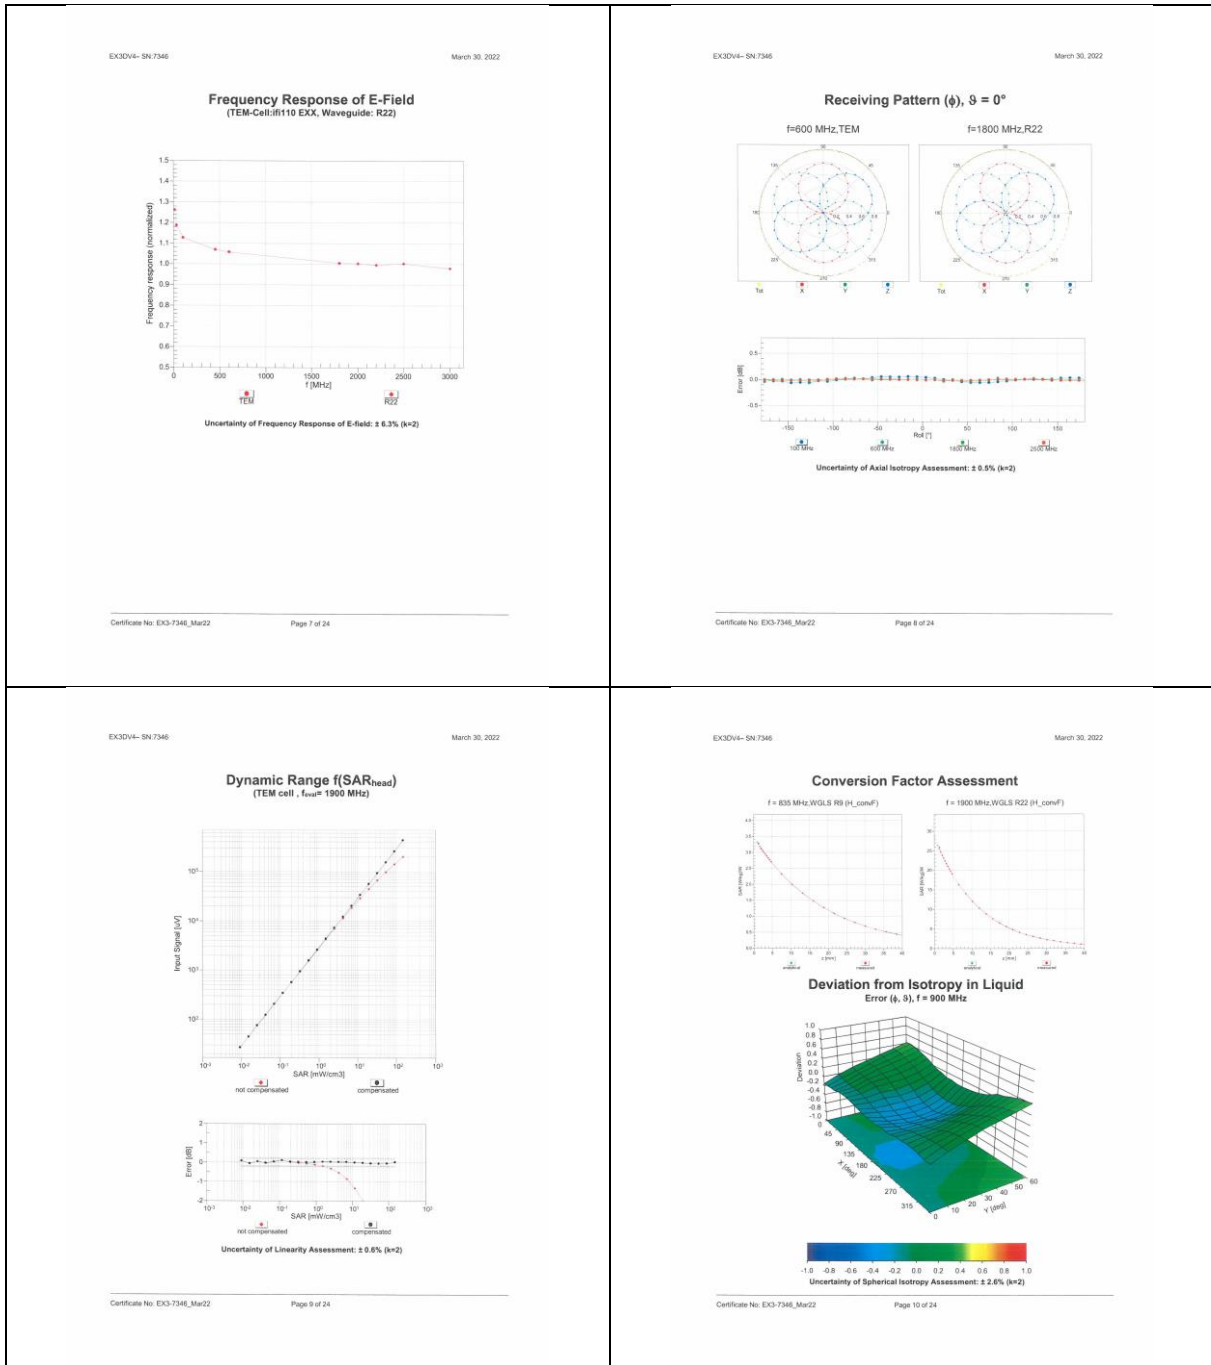

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
 No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



Compliance Certification Services (Kunshan) Inc.

UID	Rev	Communication System Name	Group	PAR (dB)	Unit
		CA	CA	0.00	+1.7%
10010	CAA	SAR Validation (Square, 10mm, 10mm)	Test	10.00	+0.5%
10011	CAB	UMTS-FDD (WCDMA)	WCDMA	2.81	+0.5%
10012	CAB	IEEE 802.11a WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	1.87	+0.5%
10013	CAB	IEEE 802.11a WFI 2.4 GHz (DSSS-OFDM, 6 Mbps)	WLAN	9.46	+0.5%
10014	DAC	EDGE-FDD (TDMA, GSMK, TN-0)	GSM	9.39	+0.5%
10015	DAC	EDGE-FDD (TDMA, GSMK, TN-0-1)	GSM	6.56	+0.5%
10016	DAC	EDGE-FDD (TDMA, GSMK, TN-0-1)	GSM	12.62	+0.5%
10017	DAC	EDGE-FDD (TDMA, GSMK, TN-0-1)	GSM	9.55	+0.5%
10018	CAA	IEEE 802.15.1 Bluetooth (FSK, D1)	Bluetooth	4.88	+0.5%
10019	CAA	IEEE 802.15.1 Bluetooth (FSK, D1)	Bluetooth	3.55	+0.5%
10020	DAC	EDGE-FDD (TDMA, GSMK, TN-0-1)	GSM	7.78	+0.5%
10021	CAA	IEEE 802.15.1 Bluetooth (FSK, D1)	Bluetooth	5.30	+0.5%
10022	CAA	IEEE 802.15.1 Bluetooth (FSK, D1)	Bluetooth	1.16	+0.5%
10023	CAA	IEEE 802.15.1 Bluetooth (FH-QPSK, D1)	Bluetooth	7.74	+0.5%
10024	CAA	IEEE 802.15.1 Bluetooth (FH-QPSK, D1)	Bluetooth	4.53	+0.5%
10025	CAA	IEEE 802.15.1 Bluetooth (FH-QPSK, D1)	Bluetooth	3.83	+0.5%
10026	CAA	IEEE 802.15.1 Bluetooth (FH-QPSK, D1)	Bluetooth	8.01	+0.5%
10027	CAA	IEEE 802.15.1 Bluetooth (FH-QPSK, D1)	Bluetooth	4.77	+0.5%
10028	CAA	IEEE 802.15.1 Bluetooth (FH-QPSK, D1)	Bluetooth	4.10	+0.5%
10029	CAB	CDMA2000 1X (RTT, RC1)	CDMA2000	4.57	+0.5%
10030	CAB	IS-54 IS-136 FDD (TDMA/FD, FH, DQPSK, HalfRate)	AMPS	7.78	+0.5%
10031	CAA	IS-54 IS-136 FDD (TDMA/FD, FH, DQPSK, FullRate)	AMPS	8.00	+0.5%
10032	CAB	DECT (DCT, TDMA/FD, GFSK, FullRate, 24)	DECT	13.80	+0.5%
10033	CAA	DECT (DCT, TDMA/FD, GFSK, Double Slot, 12)	DECT	10.79	+0.5%
10034	CAA	UMTS-TDD (TD-SCDMA, 3.1M) (3.1M)	TD-SCDMA	11.01	+0.5%
10035	DAC	EDGE-FDD (TDMA, GSMK, TN-0-1-2-3)	GSM	6.52	+0.5%
10036	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 2 Mbps)	WLAN	2.12	+0.5%
10037	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	2.83	+0.5%
10038	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	3.80	+0.5%
10039	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	8.68	+0.5%
10040	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	8.83	+0.5%
10041	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	9.09	+0.5%
10042	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	9.00	+0.5%
10043	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	9.38	+0.5%
10044	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	10.12	+0.5%
10045	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	10.24	+0.5%
10046	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	10.56	+0.5%
10047	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	9.83	+0.5%
10048	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	9.82	+0.5%
10049	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	9.84	+0.5%
10050	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	10.20	+0.5%
10051	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	10.77	+0.5%
10052	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	10.94	+0.5%
10053	CAB	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps)	WLAN	11.00	+0.5%
10054	CAB	CDMA2000 1X (RTT, RC1)	CDMA2000	4.77	+0.5%
10055	CAB	IS-54 IS-136 FDD (TDMA/FD, FH, DQPSK, FullRate)	AMPS	4.77	+0.5%
10056	DAC	EDGE-FDD (TDMA, GSMK, TN-0-1)	GSM	6.56	+0.5%
10057	CAB	UMTS-FDD (WCDMA)	WCDMA	3.98	+0.5%
10058	CAB	UMTS-FDD (HSPA, Subset2)	WCDMA	3.98	+0.5%
10059	DAC	EDGE-FDD (TDMA, GSMK, TN-0-1)	GSM	9.55	+0.5%

Certificate No: EK3-7346_Mar22

Page 12 of 24

UID	Rev	Communication System Name	Group	PAR (dB)	Unit
10100	CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	LTE-FDD	5.67	+0.5%
10101	CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	LTE-FDD	6.40	+0.5%
10102	CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	LTE-FDD	6.60	+0.5%
10103	CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	LTE-TDD	9.29	+0.5%
10104	CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	LTE-TDD	9.87	+0.5%
10105	CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	LTE-TDD	10.01	+0.5%
10106	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	LTE-FDD	5.80	+0.5%
10107	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	LTE-FDD	6.43	+0.5%
10108	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	LTE-FDD	6.63	+0.5%
10109	CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	LTE-FDD	5.76	+0.5%
10110	CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	LTE-FDD	6.44	+0.5%
10111	CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	LTE-FDD	6.59	+0.5%
10112	CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	LTE-FDD	6.62	+0.5%
10113	CAD	IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK)	WLAN	8.10	+0.5%
10114	CAD	IEEE 802.11n (HT Mixed, 6.75 Mbps, BPSK)	WLAN	8.46	+0.5%
10115	CAD	IEEE 802.11n (HT Mixed, 13.5 Mbps, 64-QAM)	WLAN	8.55	+0.5%
10116	CAD	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	WLAN	8.67	+0.5%
10117	CAD	IEEE 802.11n (HT Mixed, 6.75 Mbps, 64-QAM)	WLAN	8.89	+0.5%
10118	CAD	IEEE 802.11n (HT Mixed, 13.5 Mbps, 64-QAM)	WLAN	8.13	+0.5%
10119	CAD	IEEE 802.11n (HT Mixed, 13.5 Mbps, 64-QAM)	WLAN	8.49	+0.5%
10120	CAD	IEEE 802.11n (HT Mixed, 13.5 Mbps, 64-QAM)	WLAN	8.55	+0.5%
10121	CAD	IEEE 802.11n (HT Mixed, 13.5 Mbps, 64-QAM)	WLAN	8.73	+0.5%
10122	CAD	IEEE 802.11n (HT Mixed, 13.5 Mbps, 64-QAM)	WLAN	8.85	+0.5%
10123	CAD	IEEE 802.11n (HT Mixed, 13.5 Mbps, 64-QAM)	WLAN	6.65	+0.5%
10124	CAD	IEEE 802.11n (HT Mixed, 13.5 Mbps, 64-QAM)	WLAN	5.76	+0.5%
10125	CAD	IEEE 802.11n (HT Mixed, 13.5 Mbps, 64-QAM)	WLAN	6.41	+0.5%
10126	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	LTE-FDD	6.67	+0.5%
10127	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.72	+0.5%
10128	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.73	+0.5%
10129	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.81	+0.5%
10130	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.80	+0.5%
10131	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.82	+0.5%
10132	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.83	+0.5%
10133	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.84	+0.5%
10134	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.85	+0.5%
10135	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.86	+0.5%
10136	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.87	+0.5%
10137	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.88	+0.5%
10138	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.89	+0.5%
10139	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.90	+0.5%
10140	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.91	+0.5%
10141	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.92	+0.5%
10142	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.93	+0.5%
10143	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.94	+0.5%
10144	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.95	+0.5%
10145	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.96	+0.5%
10146	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.97	+0.5%
10147	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.98	+0.5%
10148	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.99	+0.5%
10149	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.00	+0.5%
10150	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.01	+0.5%
10151	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.02	+0.5%
10152	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.03	+0.5%
10153	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.04	+0.5%
10154	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.05	+0.5%
10155	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.06	+0.5%
10156	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.07	+0.5%
10157	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.08	+0.5%
10158	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.09	+0.5%
10159	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.10	+0.5%
10160	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.11	+0.5%
10161	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.12	+0.5%
10162	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.13	+0.5%
10163	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.14	+0.5%
10164	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.15	+0.5%
10165	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.16	+0.5%
10166	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.17	+0.5%
10167	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.18	+0.5%
10168	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.19	+0.5%
10169	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.20	+0.5%
10170	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.21	+0.5%
10171	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.22	+0.5%
10172	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.23	+0.5%
10173	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.24	+0.5%
10174	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.25	+0.5%
10175	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.26	+0.5%
10176	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.27	+0.5%
10177	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.28	+0.5%
10178	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.29	+0.5%
10179	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.30	+0.5%
10180	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.31	+0.5%
10181	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	7.32	+0.5%

Certificate No: EK3-7346_Mar22

Page 12 of 24

UID	Rev	Communication System Name	Group	PAR (dB)	Unit
10182	CAE	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	LTE-FDD	6.52	+0.5%
10183	AAE	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	LTE-FDD	6.50	+0.5%
10184	CAB	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	LTE-FDD	5.73	+0.5%
10185	CAB	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	LTE-FDD	6.51	+0.5%
10186	AAE	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	LTE-FDD	6.50	+0.5%
10187	CAF	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	LTE-FDD	5.73	+0.5%
10188	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	LTE-FDD	6.52	+0.5%
10189	CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.50	+0.5%
10190	CAD	IEEE 802.11n (HT Greenfield, 13.5 Mbps, 64-QAM)	WLAN	6.09	+0.5%
10191	CAD	IEEE 802.11n (HT Greenfield, 13.5 Mbps, 64-QAM)	WLAN	8.21	+0.5%
10192	CAD	IEEE 802.11n (HT Greenfield, 13.5 Mbps, 64-QAM)			



Compliance Certification Services (Kunshan) Inc.

EX3044-SN 7346		March 30, 2022	
10414	AAA WLAN CCDF 64 QAM 40MHz	Generic	8.54
10415	AAA IEEE 802.11n WFI 2.4 GHz (IEEE 802.11n, 900cc)	WLAN	1.54
10416	AAA IEEE 802.11g WFI 2.4 GHz (ERP-OFDM, 6 Mbps, 900cc)	WLAN	8.23
10417	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 6 Mbps, 900cc)	WLAN	8.23
10418	AAA IEEE 802.11g WFI 2.4 GHz (SSSS-OFDM, 6 Mbps, 900cc Long)	WLAN	8.14
10419	AAA IEEE 802.11g WFI 2.4 GHz (SSSS-OFDM, 8 Mbps, 900cc Short)	WLAN	8.19
10420	AAAC IEEE 802.11n HT Greenfield, 7.2 Mbps, 64-QAM	WLAN	8.32
10421	AAAC IEEE 802.11n HT Greenfield, 4.3 Mbps, 16-QAM	WLAN	8.47
10422	AAAC IEEE 802.11n HT Greenfield, 11 Mbps, 64-QAM	WLAN	8.40
10423	AAAC IEEE 802.11n HT Greenfield, 30 Mbps, 16-QAM	WLAN	8.45
10424	AAAC IEEE 802.11n HT Greenfield, 10 Mbps, 64-QAM	WLAN	8.41
10425	AAAC IEEE 802.11n HT Greenfield, 10 Mbps, 64-QAM	WLAN	8.41
10426	AAAC IEEE 802.11n HT Greenfield, 30 Mbps, 16-QAM	WLAN	8.45
10427	AAAC IEEE 802.11n HT Greenfield, 10 Mbps, 64-QAM	WLAN	8.41
10428	AAAD LTE-FDD (OFDMA, 5 MHz, E-TR 1.1)	LTE-FDD	8.28
10429	AAAD LTE-FDD (OFDMA, 10 MHz, E-TR 1.1)	LTE-FDD	8.36
10430	AAAC LTE-FDD (OFDMA, 10 MHz, E-TR 1.1, Clipping 44%)	LTE-FDD	8.34
10431	AAAC LTE-FDD (OFDMA, 20 MHz, E-TR 1.1, Clipping 44%)	LTE-FDD	8.34
10432	AAA W-CDMA (BS Test Model 1, 64 QPSK, Clipping 44%)	WCDMA	8.60
10433	AAAF LTE-TDD (SC-FDMA, 1.8 RB, 20 MHz, QPSK, UL, Sub)	LTE-TDD	7.82
10434	AAAD LTE-FDD (OFDMA, 1.8 RB, 20 MHz, QPSK, UL, Sub)	LTE-FDD	7.96
10435	AAAD LTE-FDD (OFDMA, 1.8 RB, 20 MHz, QPSK, UL, Sub)	LTE-FDD	7.93
10436	AAAC LTE-FDD (OFDMA, 1.8 RB, 20 MHz, QPSK, UL, Sub)	LTE-FDD	7.91
10437	AAAC LTE-FDD (OFDMA, 1.8 RB, 20 MHz, QPSK, UL, Sub)	LTE-FDD	7.89
10438	AAA W-CDMA (BS Test Model 1, 64 QPSK, Clipping 44%)	WCDMA	7.99
10439	AAAD Validation (SISO, Tone, 1mg)	Test	10.00
10440	AAAC IEEE 802.11ac WFI 160MHz, 64-QAM, 900cc	WLAN	8.63
10441	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10442	AAA COMAR200 (14E-DO, Rev. 8, 3 cameras)	CEMARA200	8.53
10443	AAAC COMAR200 (14E-DO, Rev. 8, 3 cameras)	CEMARA200	8.25
10444	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10445	AAA WMTS-FDD (IS-97A)	WCDMA	8.62
10446	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10447	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10448	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10449	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10450	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10451	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10452	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10453	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10454	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10455	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10456	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10457	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10458	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10459	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10460	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10461	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10462	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10463	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10464	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10465	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10466	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10467	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10468	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10469	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10470	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10471	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10472	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10473	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10474	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10475	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10476	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10477	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10478	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10479	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10480	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10481	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10482	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10483	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10484	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10485	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10486	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10487	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10488	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10489	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10490	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10491	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10492	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10493	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10494	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10495	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10496	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10497	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10498	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10499	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62
10500	AAAD WMTS-FDD (IS-97A)	WCDMA	8.62

EX3044-SN 7346		March 30, 2022	
10499	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.31
10500	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.54
10501	AAAE LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	7.74
10502	AAAE LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.41
10503	AAAE LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.59
10504	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	7.74
10505	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.31
10506	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.54
10507	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.31
10508	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.54
10509	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.31
10510	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.54
10511	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.31
10512	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.54
10513	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.31
10514	AAAF LTE-TDD (SC-FDMA, 50% RB, 18 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.54
10515	AAA IEEE 802.11n WFI 2.4 GHz (IEEE 802.11n, 900cc)	WLAN	1.54
10516	AAA IEEE 802.11n WFI 2.4 GHz (IEEE 802.11n, 900cc)	WLAN	1.54
10517	AAA IEEE 802.11n WFI 2.4 GHz (IEEE 802.11n, 900cc)	WLAN	1.54
10518	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 6 Mbps, 900cc)	WLAN	8.23
10519	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 12 Mbps, 900cc)	WLAN	8.39
10520	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 18 Mbps, 900cc)	WLAN	8.45
10521	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 24 Mbps, 900cc)	WLAN	8.51
10522	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 30 Mbps, 900cc)	WLAN	8.57
10523	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 36 Mbps, 900cc)	WLAN	8.63
10524	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 42 Mbps, 900cc)	WLAN	8.69
10525	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 48 Mbps, 900cc)	WLAN	8.75
10526	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 54 Mbps, 900cc)	WLAN	8.81
10527	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 60 Mbps, 900cc)	WLAN	8.87
10528	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 66 Mbps, 900cc)	WLAN	8.93
10529	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 72 Mbps, 900cc)	WLAN	8.99
10530	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 78 Mbps, 900cc)	WLAN	9.05
10531	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 84 Mbps, 900cc)	WLAN	9.11
10532	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 90 Mbps, 900cc)	WLAN	9.17
10533	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 96 Mbps, 900cc)	WLAN	9.23
10534	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 102 Mbps, 900cc)	WLAN	9.29
10535	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 108 Mbps, 900cc)	WLAN	9.35
10536	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 114 Mbps, 900cc)	WLAN	9.41
10537	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 120 Mbps, 900cc)	WLAN	9.47
10538	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 126 Mbps, 900cc)	WLAN	9.53
10539	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 132 Mbps, 900cc)	WLAN	9.59
10540	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 138 Mbps, 900cc)	WLAN	9.65
10541	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 144 Mbps, 900cc)	WLAN	9.71
10542	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 150 Mbps, 900cc)	WLAN	9.77
10543	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 156 Mbps, 900cc)	WLAN	9.83
10544	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 162 Mbps, 900cc)	WLAN	9.89
10545	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 168 Mbps, 900cc)	WLAN	9.95
10546	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 174 Mbps, 900cc)	WLAN	10.01
10547	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 180 Mbps, 900cc)	WLAN	10.07
10548	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 186 Mbps, 900cc)	WLAN	10.13
10549	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 192 Mbps, 900cc)	WLAN	10.19
10550	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 198 Mbps, 900cc)	WLAN	10.25
10551	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 204 Mbps, 900cc)	WLAN	10.31
10552	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 210 Mbps, 900cc)	WLAN	10.37
10553	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 216 Mbps, 900cc)	WLAN	10.43
10554	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 222 Mbps, 900cc)	WLAN	10.49
10555	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 228 Mbps, 900cc)	WLAN	10.55
10556	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 234 Mbps, 900cc)	WLAN	10.61
10557	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 240 Mbps, 900cc)	WLAN	10.67
10558	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 246 Mbps, 900cc)	WLAN	10.73
10559	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 252 Mbps, 900cc)	WLAN	10.79
10560	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 258 Mbps, 900cc)	WLAN	10.85
10561	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 264 Mbps, 900cc)	WLAN	10.91
10562	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 270 Mbps, 900cc)	WLAN	10.97
10563	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 276 Mbps, 900cc)	WLAN	11.03
10564	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 282 Mbps, 900cc)	WLAN	11.09
10565	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 288 Mbps, 900cc)	WLAN	11.15
10566	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 294 Mbps, 900cc)	WLAN	11.21
10567	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 300 Mbps, 900cc)	WLAN	11.27
10568	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 306 Mbps, 900cc)	WLAN	11.33
10569	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 312 Mbps, 900cc)	WLAN	11.39
10570	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 318 Mbps, 900cc)	WLAN	11.45
10571	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 324 Mbps, 900cc)	WLAN	11.51
10572	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 330 Mbps, 900cc)	WLAN	11.57
10573	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 336 Mbps, 900cc)	WLAN	11.63
10574	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 342 Mbps, 900cc)	WLAN	11.69
10575	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 348 Mbps, 900cc)	WLAN	11.75
10576	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 354 Mbps, 900cc)	WLAN	11.81
10577	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 360 Mbps, 900cc)	WLAN	11.87
10578	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 366 Mbps, 900cc)	WLAN	11.93
10579	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 372 Mbps, 900cc)	WLAN	11.99
10580	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 378 Mbps, 900cc)	WLAN	12.05
10581	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 384 Mbps, 900cc)	WLAN	12.11
10582	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 390 Mbps, 900cc)	WLAN	12.17
10583	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 396 Mbps, 900cc)	WLAN	12.23
10584	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 402 Mbps, 900cc)	WLAN	12.29
10585	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 408 Mbps, 900cc)	WLAN	12.35
10586	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 414 Mbps, 900cc)	WLAN	12.41
10587	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 420 Mbps, 900cc)	WLAN	12.47
10588	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 426 Mbps, 900cc)	WLAN	12.53
10589	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 432 Mbps, 900cc)	WLAN	12.59
10590	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 438 Mbps, 900cc)	WLAN	12.65
10591	AAAC IEEE 802.11n WFI 5 GHz (OFDM, 444 Mbps, 900cc)	WLAN	12.71
10592			

EX30V4-- SN 7346		March 30, 2022	
10985	AAA	SG NR DL_CPF-QPCW TM 3.1, 40 MHz, 64-QAM, 30 kHz	SG NR FR1 TDD 9.54 ± 0.8 %
10986	AAA	SG NR DL_CPF-QPCW TM 3.1, 50 MHz, 64-QAM, 30 kHz	SG NR FR1 TDD 9.50 ± 0.8 %
10987	AAA	SG NR DL_CPF-QPCW TM 3.1, 60 MHz, 64-QAM, 30 kHz	SG NR FR1 TDD 9.53 ± 0.8 %
10988	AAA	SG NR DL_CPF-QPCW TM 3.1, 70 MHz, 64-QAM, 30 kHz	SG NR FR1 TDD 9.58 ± 0.8 %
10989	AAA	SG NR DL_CPF-QPCW TM 3.1, 80 MHz, 64-QAM, 30 kHz	SG NR FR1 TDD 9.51 ± 0.8 %
10990	AAA	SG NR DL_CPF-QPCW TM 3.1, 90 MHz, 64-QAM, 30 kHz	SG NR FR1 TDD 9.52 ± 0.8 %

¹ Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the full value.

Certificate No: EX3-7346_Mar22 Page 24 of 24



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com