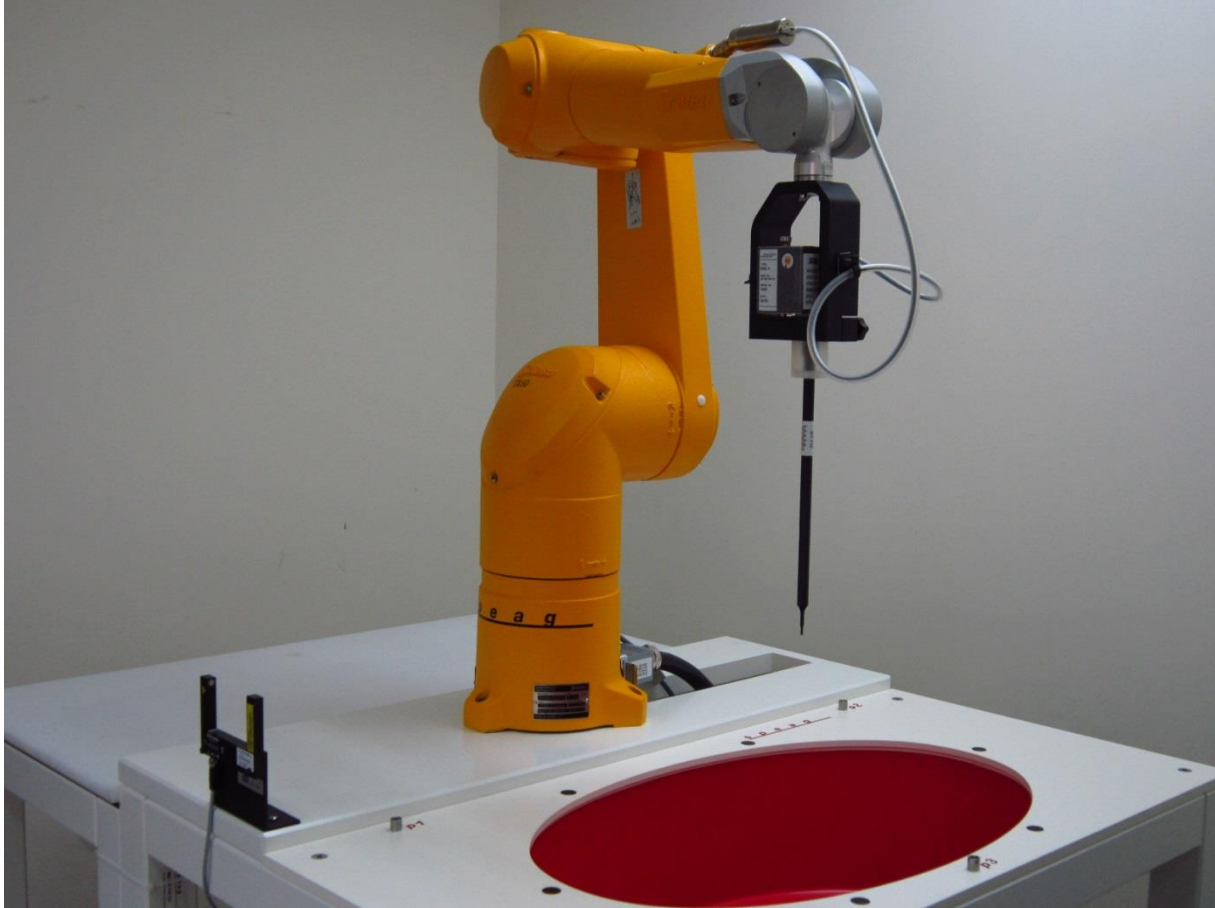


Appendix D







Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details


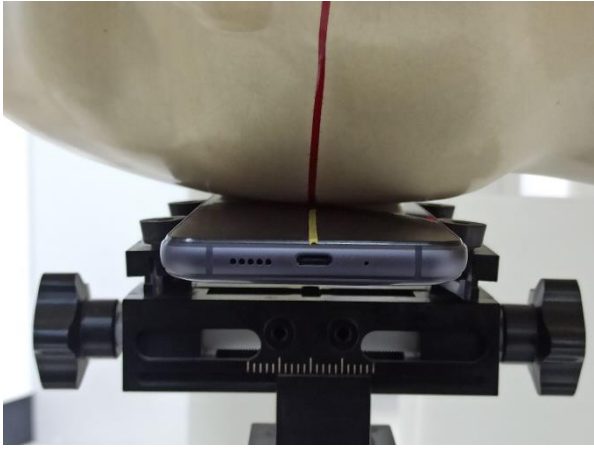

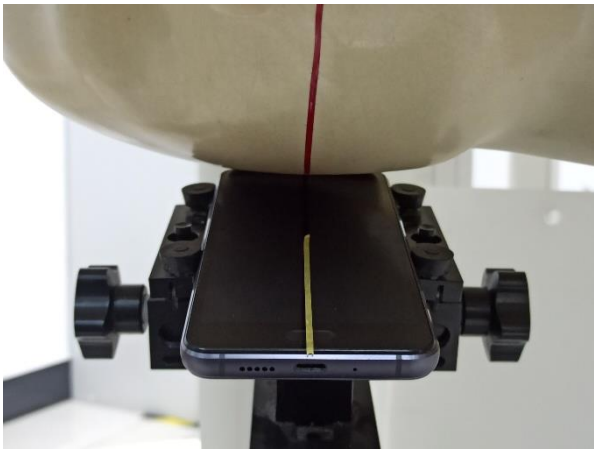


1. SAR measurement System



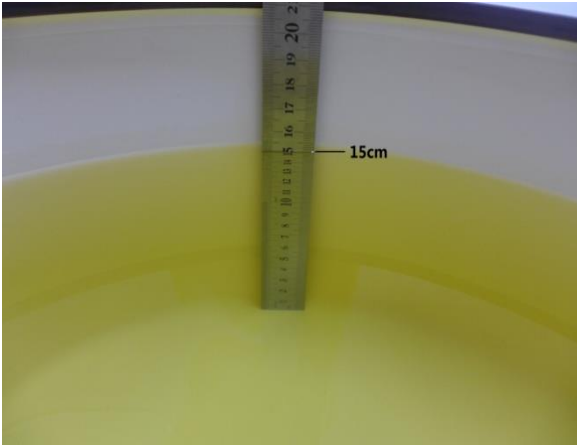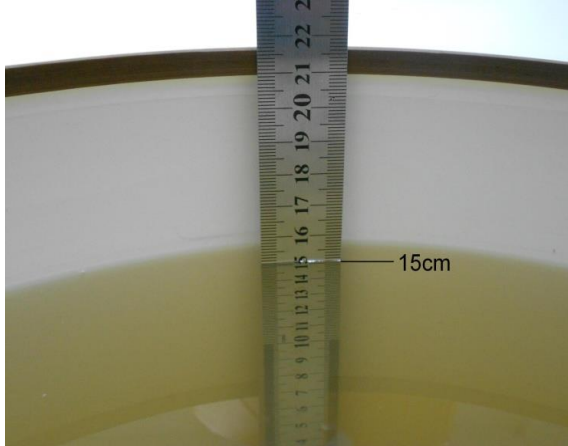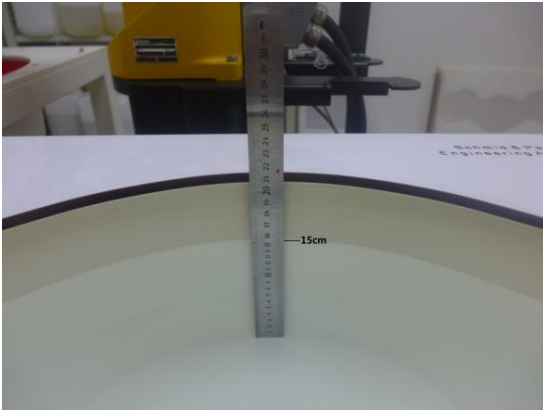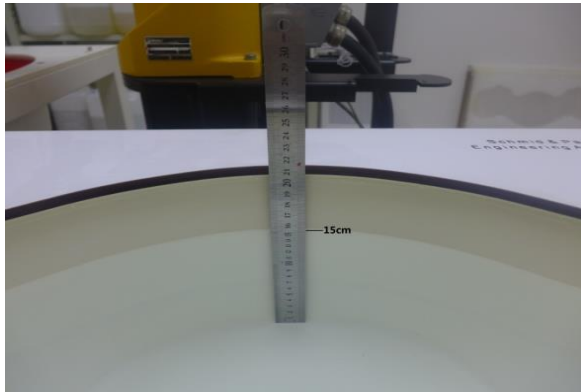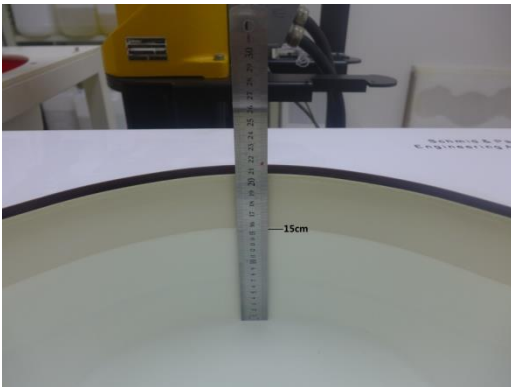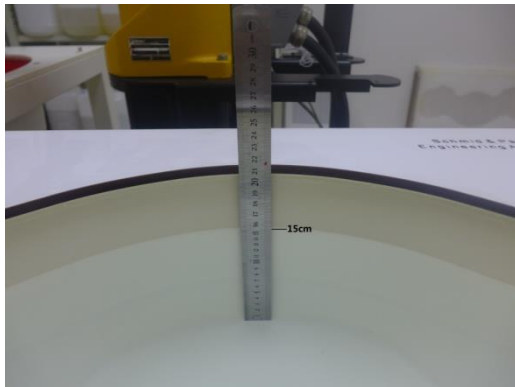



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Head 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1800</p>	<p>Photo 4: Tissue Simulant Liquid for Head 1900</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Head 5GHz</p>
	

3. Photographs of EUT test position

<p>Photo 7: Left cheek 0mm</p>	<p>Photo 8: Right cheek 0mm</p>
	
<p>Photo 9: Left tilted</p>	<p>Photo 10: Right tilted</p>
	
<p>Photo 11: Front side 10mm</p>	<p>Photo 12: Back side 10mm</p>
	

<p>Photo 13: Left side 10mm</p>	<p>Photo 14: Right side 10mm</p>
	
<p>Photo 15: Top side 10mm</p>	<p>Photo 16: Bottom side 10mm</p>
	

4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.