



NVLAP LAB CODE 200707-0



# SAR EVALUATION REPORT

For

## PAX Technology Limited

Room 2416, 24/F., Sun Hung Kai Centre, 30 Harbour Road,

Wanchai Hong Kong, 518057 CHN

**FCC ID: V5PS90**

<b>Report Type:</b> Original Report	<b>Product Type:</b> Mobile Payment Terminal
<b>Test Engineer:</b> Eric Zhang	<i>Eric Zhang</i>
<b>Report No.:</b> RSZ09022501-SAR	
<b>Report Date:</b> 2009-04-07	
<b>Reviewed By:</b> William Chen EMC Engineer	<i>William . Chan .</i>
<b>Prepared By:</b> Bay Area Compliance Laboratories Corporation (Shenzhen) 6/F, the 3 <sup>rd</sup> Phase of WanLi Industrial Building, Shi Hua Road, Fu Tian Free Trade Zone, Shen Zhen, Guangdong, P.R. of China Tel: +86-755-33320018 Fax: +86-755-33320008	

**Note:** This test report is prepared for the customer shown above and for the device described herein. It may not be duplicated or used in part without prior written consent from Bay Area Compliance Laboratories Corp. (Shenzhen). This report **must not** be used by the customer to claim product certification, approval, or endorsement by NVLAP\*, NIST, or any agency of the Federal Government.

\* This report may contain data that are not covered by the NVLAP accreditation and are marked with an asterisk “\*”.

### Summary of Test Results

<b>Rule Part(s):</b>	CFR 47 §2.1093
<b>Test Procedure(s):</b>	FCC OET Bulletin 65C IEEE 1528-2003
<b>Device Type:</b>	Portable device
<b>Exposure Category</b>	Population/Uncontrolled
<b>Modulation:</b>	GMSK
<b>TX Frequency Range:</b>	824-849 MHz (Cellular Band) 1850-1910 MHz (PCS Band)
<b>Maximum Conducted Power Tested:</b>	32.66 dBm (Cellular Band) 29.77 dBm(PCS Band)
<b>Antenna Type(s):</b>	Internal Antenna
<b>Body-Worn Accessories:</b>	Headset
<b>Face-Head Accessories:</b>	None
<b>Max. SAR Level(s) Measured:</b>	0.384 W/Kg 1g Body Tissue (Cellular Band) 0.345 W/Kg 1g Body Tissue (PCS Band)

This wireless device has been shown to be capable of compliance for localized specific absorption rate (SAR) for General Population/Uncontrolled Exposure limits specified in ANSI/IEEE Standards and has been tested in accordance with the measurement procedures specified in FCC OET 65 Supplement C and IEEE 1528-2003.

**The results and statements contained in this report pertain only to the device(s) evaluated.**



**EUT Photo**

## TABLE OF CONTENTS

<b>REFERENCE, STANDARDS, AND GUIDELINES .....</b>	<b>4</b>
SAR LIMITS .....	5
<b>EUT DESCRIPTION .....</b>	<b>6</b>
TECHNICAL SPECIFICATION .....	6
EUT PHOTO .....	6
<b>FACILITIES AND ACCREDITATION .....</b>	<b>7</b>
<b>DESCRIPTION OF TEST SYSTEM .....</b>	<b>8</b>
<b>EQUIPMENT LIST AND CALIBRATION .....</b>	<b>15</b>
EQUIPMENTS LIST & CALIBRATION INFO .....	15
<b>SAR MEASUREMENT SYSTEM VERIFICATION .....</b>	<b>16</b>
LIQUID VERIFICATION .....	16
SYSTEM ACCURACY VERIFICATION .....	19
<b>EUT TEST STRATEGY AND METHODOLOGY .....</b>	<b>20</b>
TEST POSITIONS FOR DEVICE OPERATING NEXT TO A PERSON’S EAR .....	20
CHEEK/TOUCH POSITION .....	21
EAR/TILT POSITION .....	21
TEST POSITIONS FOR BODY-WORN AND OTHER CONFIGURATIONS .....	22
SAR EVALUATION PROCEDURE .....	23
<b>SAR MEASUREMENT RESULTS .....</b>	<b>24</b>
SAR TEST DATA .....	24
<b>APPENDIX A – MEASUREMENT UNCERTAINTY .....</b>	<b>25</b>
<b>APPENDIX B – PROBE CALIBRATION CERTIFICATES .....</b>	<b>26</b>
<b>APPENDIX C – DIPOLE CALIBRATION CERTIFICATES .....</b>	<b>66</b>
<b>APPENDIX D – SAR SYSTEM VALIDATION DATA .....</b>	<b>86</b>
<b>APPENDIX E – EUT SCAN RESULTS.....</b>	<b>90</b>
<b>APPENDIX F – CONDUCTED OUTPUT POWER MEASUREMENT .....</b>	<b>102</b>
PROVISION APPLICABLE.....	102
TEST PROCEDURE .....	102
TEST EQUIPMENT LIST AND DETAILS.....	102
TEST RESULTS .....	102
<b>APPENDIX G – EUT TEST POSITION PHOTOS .....</b>	<b>103</b>
BODY-WORN SETUP PHOTO .....	103
<b>APPENDIX H – EUT PHOTOS.....</b>	<b>104</b>
EUT - TOP VIEW .....	104
EUT - BOTTOM VIEW .....	104
<b>APPENDIX I - INFORMATIVE REFERENCES.....</b>	<b>106</b>

---

## REFERENCE, STANDARDS, AND GUIDELINES

---

### **FCC:**

The Report and Order requires routine SAR evaluation prior to equipment authorization of portable transmitter devices, including portable telephones. For consumer products, the applicable limit is 1.6 mW/g as recommended by the ANSI/IEEE standard C95.1-1992 [6] for an uncontrolled environment (Paragraph 65). According to the Supplement C of OET Bulletin 65 "Evaluating Compliance with FCC Guide-lines for Human Exposure to Radio frequency Electromagnetic Fields", released on Jun 29, 2001 by the FCC, the device should be evaluated at maximum output power (radiated from the antenna) under "worst-case" conditions for normal or intended use, incorporating normal antenna operating positions, device peak performance frequencies and positions for maximum RF energy coupling.

This report describes the methodology and results of experiments performed on wireless data terminal. The objective was to determine if there is RF radiation and if radiation is found, what is the extent of radiation with respect to safety limits. SAR (Specific Absorption Rate) is the measure of RF exposure determined by the amount of RF energy absorbed by human body (or its parts) – to determine how the RF energy couples to the body or head which is a primary health concern for body worn devices. The limit below which the exposure to RF is considered safe by regulatory bodies in North America is 1.6 mW/g average over 1 gram of tissue mass.

### **CE:**

The order requires routine SAR evaluation prior to equipment authorization of portable transmitter devices, including portable telephones. For consumer products, the applicable limit is 2 mW/g as recommended by the EN50360 for an uncontrolled environment. According to the Standard, the device should be evaluated at maximum output power (radiated from the antenna) under "worst-case" conditions for normal or intended use, incorporating normal antenna operating positions, device peak performance frequencies and positions for maximum RF energy coupling.

This report describes the methodology and results of experiments performed on wireless data terminal. The objective was to determine if there is RF radiation and if radiation is found, what is the extent of radiation with respect to safety limits. SAR (Specific Absorption Rate) is the measure of RF exposure determined by the amount of RF energy absorbed by human body (or its parts) – to determine how the RF energy couples to the body or head which is a primary health concern for body worn devices. The limit below which the exposure to RF is considered safe by regulatory bodies in Europe is 2 mW/g average over 10 gram of tissue mass.

The test configurations were laid out on a specially designed test fixture to ensure the reproducibility of measurements. Each configuration was scanned for SAR. Analysis of each scan was carried out to characterize the above effects in the device.

**SAR Limits**

## FCC Limit (1g Tissue)

EXPOSURE LIMITS	SAR (W/kg)	
	(General Population / Uncontrolled Exposure Environment)	(Occupational / Controlled Exposure Environment)
Spatial Average (averaged over the whole body)	0.08	0.4
Spatial Peak (averaged over any 1 g of tissue)	1.60	8.0
Spatial Peak (hands/wrists/feet/ankles averaged over 10 g)	4.0	20.0

## CE Limit (10g Tissue)

EXPOSURE LIMITS	SAR (W/kg)	
	(General Population / Uncontrolled Exposure Environment)	(Occupational / Controlled Exposure Environment)
Spatial Average (averaged over the whole body)	0.08	0.4
Spatial Peak (averaged over any 1 g of tissue)	2.0	10
Spatial Peak (hands/wrists/feet/ankles averaged over 10 g)	4.0	20.0

Population/Uncontrolled Environments are defined as locations where there is the exposure of individual who have no knowledge or control of their exposure.

Occupational/Controlled Environments are defined as locations where there is exposure that may be incurred by people who are aware of the potential for exposure (i.e. as a result of employment or occupation).

## EUT DESCRIPTION

This Bay Area Compliance Laboratories Corp. test report has been prepared on behalf of PAX Technology Limited and their product, model: S90, FCC ID: V5PS90 or the EUT (Equipment Under Test) as referred to in the rest of this report.

### Technical Specification

Item	Content
Modulation	GMSK
Frequency Band	Cellular Band: 824-849 MHz 869-894 MHz PCS Band: 1850-1910 MHz 1930-1990 MHz
Dimensions (L*W*H)	200mm(L)× 90mm(W)×60mm(H)
Weight	495 g
Power Source	7.4 Vdc/1800mAh Rechargeable Battery
Normal Operation	Body-worn

### EUT Photo



*Model: S90  
Please refer to Appendix H*

---

## FACILITIES AND ACCREDITATION

---

The test site used by Bay Area Compliance Laboratories Corp. (Shenzhen) to collect data is located at

6/F, the 3rd Phase of WanLi Industrial Building,  
Shi Hua Road, Fu Tian Free Trade Zone,  
ShenZhen, Guangdong, P.R. of China

Additionally, Bay Area Compliance Laboratories Corp. (Shenzhen) is a National Institute of Standards and Technology (NIST) accredited laboratory, under the National Voluntary Laboratory Accredited Program (Lab Code 200707-0).



NVLAP LAB CODE 200707-0

The current scope of accreditations can be found at  
<http://ts.nist.gov/Standards/scopes/2007070.htm>

## DESCRIPTION OF TEST SYSTEM

---

These measurements were performed with ALSAS 10 Universal Integrated SAR Measurement system from APREL Laboratories.



### ALSAS-10U System Description

**ALSAS-10-U** is fully compliant with the technical and scientific requirements of IEEE 1528, IEC 62209, CENELEC, ARIB, ACA, and the Federal Communications Commission. The system comprises of a six axes articulated robot which utilizes a dedicated controller. ALSAS-10U uses the latest methodologies. And FDTD modeling to provide a platform which is repeatable with minimum uncertainty.

### Applications

Predefined measurement procedures compliant with the guidelines of CENELEC, IEEE, IEC, FCC, etc are utilized during the assessment for the device. Automatic detection for all SAR maxima are embedded within the core architecture for the system, ensuring that peak locations used for centering the zoom scan are within a 1mm resolution and a 0.05mm repeatable position. System operation range currently available up-to 6 GHz in simulated tissue.

### Area Scans

Area scans are defined prior to the measurement process being executed with a user defined variable spacing between each measurement point (integral) allowing low uncertainty measurements to be conducted. Scans defined for FCC applications utilize a 10mm<sup>2</sup> step integral, with 1mm interpolation used to locate the peak SAR area used for zoom scan assessments. Where the system identifies multiple SAR peaks (which are within 25% of peak value) the system will provide the user with the option of assessing each peak location individually for zoom scan averaging.

### Zoom Scan (Cube Scan Averaging)

The averaging zoom scan volume utilized in the ALSAS-10U software is in the shape of a cube and the side dimension of a 1 g or 10 g mass is dependent on the density of the liquid representing the simulated tissue. A density of 1000 kg/m<sup>3</sup> is used to represent the head and body tissue density and not the phantom liquid density, in order to be consistent with the definition of the liquid dielectric properties, i.e. the side length of the 1 g cube is 10mm, with the side length of the 10 g cube 21,5mm.



When the cube intersects with the surface of the phantom, it is oriented so that 3 vertices touch the surface of the shell or the center of a face is tangent to the surface. The face of the cube closest to the surface is modified in order to conform to the tangent surface.

The zoom scan integer steps can be user defined so as to reduce uncertainty, but normal practice for typical test applications (including FCC) utilize a physical step of 5x5x8 (8mmx8mmx5mm) providing a volume of 32mm in the X & Y axis, and 35mm in the Z axis.

### ALSAS-10U Interpolation and Extrapolation Uncertainty


The overall uncertainty for the methodology and algorithms the used during the SAR calculation was evaluated using the data from IEEE 1528 based on the example f3 algorithm:

$$f_3(x, y, z) = A \frac{a^2}{\frac{a^2}{4} + x'^2 + y'^2} \cdot \left( e^{-\frac{2z}{a}} + \frac{a^2}{2(a + 2z)^2} \right)$$

### Isotropic E-Field Probe

The isotropic E-Field probe has been fully calibrated and assessed for isotropicity, and boundary effect within a controlled environment. Depending on the frequency for which the probe is calibrated the method utilized for calibration will change.

The E-Field probe utilizes a triangular sensor arrangement as detailed in the diagram below:

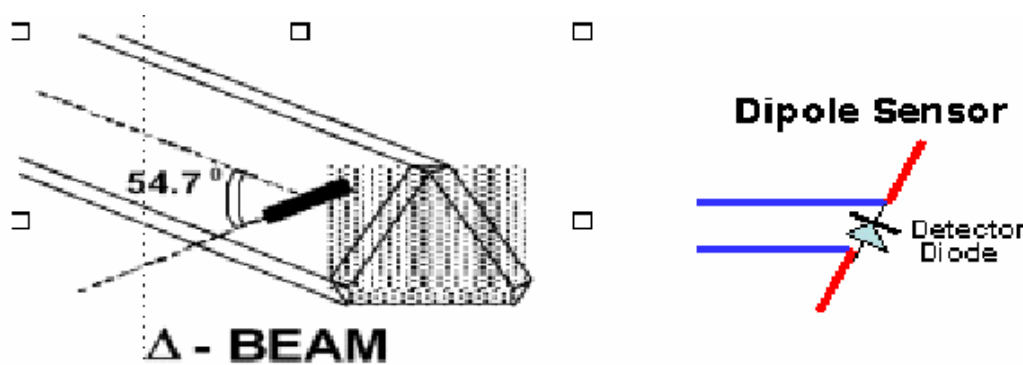

SAR is assessed with a calibrated probe which moves at a default height of 5mm from the center of the diode, which is mounted to the sensor, to the phantom surface (in the Z Axis). The 5mm offset height has been selected so as to minimize any resultant boundary effect due to the probe being in close proximity to the phantom surface.

The following algorithm is an example of the function used by the system for linearization of the output from the probe when measuring complex modulation schemes.

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

## Isotropic E-Field Probe Specification

<b>Calibration in Air</b>	Frequency Dependent Below 2 GHz Calibration in air performed in a TEM Cell Above 2 GHz Calibration in air performed in waveguide
<b>Sensitivity</b>	0.70 $\mu\text{V}/(\text{V}/\text{m})^2$ to 0.85 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Dynamic Range</b>	0.0005 W/kg to 100 W/kg
<b>Isotropic Response</b>	Better than 0.2 dB
<b>Diode Compression Point (DCP)</b>	Calibration for Specific Frequency
<b>Probe Tip Radius</b>	< 5 mm
<b>Sensor Offset</b>	1.56 (+/- 0.02 mm)
<b>Probe Length</b>	290 mm
<b>Video Bandwidth</b>	@ 500 Hz: 1 dB @ 1.02 kHz: 3 dB
<b>Boundary Effect</b>	Less than 2% for distance greater than 2.4 mm
<b>Spatial Resolution</b>	Diameter less than 5 mm Compliant with Standards

## Boundary Detection Unit and Probe Mounting Device

ALSAS-10U incorporates a boundary detection unit with a sensitivity of 0.05mm for detecting all types of surfaces. The robust design allows for detection during probe tilt (probe normalize) exercises, and utilizes a second stage emergency stop. The signal electronics are fed directly into the robot controller for high accuracy surface detection in lateral and axial detection modes (X, Y, & Z).

The probe is mounted directly onto the Boundary Detection unit for accurate tooling and displacement calculations controlled by the robot kinematics. The probe is connect to an isolated probe interconnect where the output stage of the probe is fed directly into the amplifier stage of the Daq-Paq.

## Daq-Paq (Analog to Digital Electronics)

ALSAS-10U incorporates a fully calibrated Daq-Paq (analog to digital conversion system) which has a 4 channel input stage, sent via a 2 stage auto-set amplifier module. The input signal is amplified accordingly so as to offer a dynamic range from 5 $\mu\text{V}$  to 800mV. Integration of the fields measured is carried out at board level utilizing a Co-Processor which then sends the measured fields down into the main computational module in digitized form via an RS232 communications port. Probe linearity and duty cycle compensation is carried out within the main Daq-Paq module.

<b>ADC</b>	12 Bit
<b>Amplifier Range</b>	20 mV to 200 mV and 150 mV to 800 mV
<b>Field Integration</b>	Local Co-Processor utilizing proprietary integration algorithms
<b>Number of Input Channels</b>	4 in total 3 dedicated and 1 spare
<b>Communication</b>	Packet data via RS232

## Axis Articulated Robot

ALSAS-10U utilizes a six axis articulated robot, which is controlled using a Pentium based real-time movement controller. The movement kinematics engine utilizes proprietary (Thermo CRS) interpolation and extrapolation algorithms, which allow full freedom of movement for each of the six joints within the working envelope. Utilization of joint 6 allows for full probe rotation with a tolerance better than 0.05mm around the central axis.



<b>Robot/Controller Manufacturer</b>	Thermo CRS
<b>Number of Axis</b>	Six independently controlled axis
<b>Positioning Repeatability</b>	0.05 mm
<b>Controller Type</b>	Single phase Pentium based C500C
<b>Robot Reach</b>	710 mm
<b>Communication</b>	RS232 and LAN compatible

## ALSAS Universal Workstation

ALSAS Universal workstation allows for repeatability and fast adaptability. It allows users to do calibration, testing and measurements using different types of phantoms with one set up, which significantly speeds up the measurement process.

### Universal Device Positioner

The universal device positioner allows complete freedom of movement of the EUT. Developed to hold a EUT in a free-space scenario any additional loading attributable to the material used in the construction of the positioner has been eliminated. Repeatability has been enhanced through the linear scales which form the design used to indicate positioning for any given test scenario in all major axes. A 15° tilt indicator is included for the of aid cheek to tilt movements for head SAR analysis. Overall uncertainty for measurements have been reduced due to the design of the Universal device positioner, which allows positioning of a device in as near to a free-space scenario as possible, and by providing the means for complete repeatability.




### Phantom Types

The ALSAS-10U allows the integration of multiple phantom types. SAM Phantoms fully compliant with IEEE 1528, Universal Phantom, and Universal Flat.

### APREL SAM Phantoms

The SAM phantoms developed using the IEEE SAM CAD file. They are fully compliant with the requirements for both IEEE 1528 and FCC Supplement C. Both the left and right SAM phantoms are interchangeable, transparent and include the IEEE 1528 grid with visible NF and MB lines.

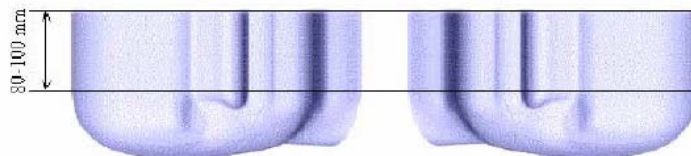

### APREL Laboratories Universal Phantom

The Universal Phantom is used on the ALSAS-10U as a system validation phantom. The Universal Phantom has been fully validated both experimentally from 800MHz to 6GHz and numerically using XFDTD numerical software.

The shell thickness is 2mm overall, with a 4mm spacer located at the NF/MB intersection providing an overall thickness of 6mm in line with the requirements of IEEE-1528.

The design allows for fast and accurate measurements, of handsets, by allowing the conservative SAR to be evaluated at on frequency for both left and right head experiments in one measurement.



### Tissue Dielectric Parameters for Head and Body Phantoms

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in P1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in a human head. Other head and body tissue parameters that have not been specified in P1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equations described in Reference [12] and extrapolated according to the head parameters specified in P1528.

Ingredients (% by weight)	Frequency (MHz)									
	450		835		915		1900		2450	
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body
Water	38.56	51.16	41.45	52.4	41.05	56.0	54.9	40.4	62.7	73.2
Salt (Nacl)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.5	0.5	0.04
Sugar	56.32	46.78	56.0	45.0	56.5	41.76	0.0	58.0	0.0	0.0
HEC	0.98	0.52	1.0	1.0	1.0	1.21	0.0	1.0	0.0	0.0
Bactericide	0.19	0.05	0.1	0.1	0.1	0.27	0.0	0.1	0.0	0.0
Triton x-100	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	36.8	0.0
DGBE	0.0	0.0	0.0	0.0	0.0	0.0	44.92	0.0	0.0	26.7
Dielectric Constant	43.42	58.0	42.54	56.1	42.0	56.8	39.9	54.0	39.8	52.5
Conductivity (s/m)	0.85	0.83	0.91	0.95	1.0	1.07	1.42	1.45	1.88	1.78

### IEEE SCC-34/SC-2 P1528 Recommended Tissue Dielectric Parameters

Frequency (MHz)	Head Tissue		Body Tissue	
	$\epsilon_r$	$\sigma$ (S/m)	$\epsilon_r$	$\sigma$ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800-2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00


## EQUIPMENT LIST AND CALIBRATION

### Equipments List & Calibration Info

Equipment	Model	Calibration Due Date	S/N:
CRS F3 robot	ALS-F3	N/A	RAF0805352
CRS F3 Software	ALS-F3-SW	N/A	N/A
CRS C500C controller	ALS-C500	N/A	RCF0805379
Probe mounting device & Boundary Detection Sensor System	ALS-PMDPS-3	N/A	120-00270
Universal Work Station	ALS-UWS	N/A	100-00157
Data Acquisition Package	ALS-DAQ-PAQ-3	N/A	110-00212
Miniature E-Field Probe	ALS-E-020	2009-08-01	273
Dipole, 835MHz	ALS-D-835-S-2	2009-08-01	180-00558
Dipole,1900MHz	ALS-D-1900-S-2	2009-08-01	210-00710
Dipole Spacer	ALS-DS-U	N/A	250-00907
R&S, universal Radio Communication Tester	CMU200	2008-06-21	1100.0008.02
Device holder/Positioner	ALS-H-E-SET-2	N/A	170-00510
Left ear SAM phantom	ALS-P-SAM-L	N/A	130-00311
Right ear SAM phantom	ALS-P-SAM-R	N/A	140-00359
UniPhantom	ALS-P-UP-1	N/A	150-00413
Simulated Tissue 835 MHz Head	ALS-T-835-1-H	Each Time	270-01002
Simulated Tissue 835 MHz Body	ALS-T-835-1-B	Each Time	270-02101
Simulated Tissue 1900 MHz Head	ALS-T-1900-1-H	Each Time	295-01103
Simulated Tissue 1900 MHz Body	ALS-T-1900-1-B	Each Time	295-02102
Signal Generator	HP8341B	2009-11-06	2624A00116
Power Amplifier	5S1G4	N/A	71377
Spectrum Analyzer	FSEM30	2009-05-08	849720/019

## SAR MEASUREMENT SYSTEM VERIFICATION

### Liquid Verification

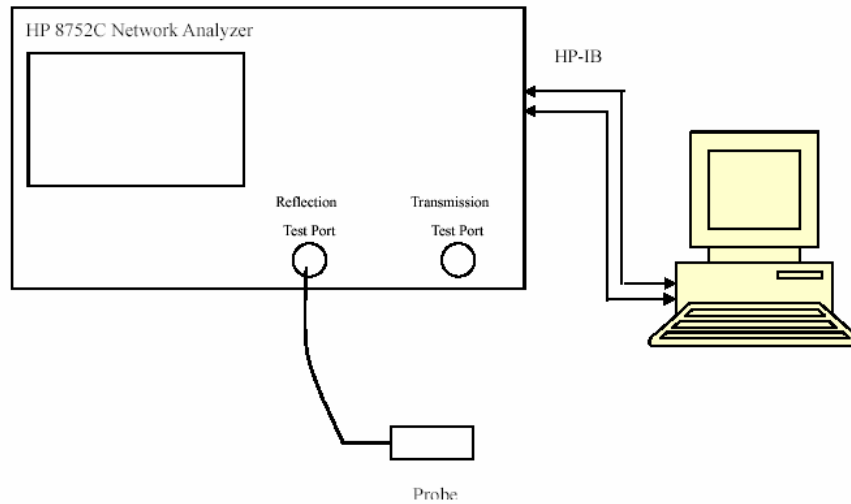

Liquid Verification Setup Block Diagram

### Liquid Verification Results

Frequency (MHz)	Liquid Type	Liquid Parameter		Result
		$\epsilon_r$	$\sigma$ (S/m)	
850	Head	41.60	0.94	In Tolerance
850	Body	53.77	0.99	In Tolerance
1900	Head	39.30	1.43	In Tolerance
1900	Body	53.45	1.50	In Tolerance

Please refer to the following tables.




850 MHz Head				850 MHz Body		
Frequency	e'	e''		Frequency	e'	e''
824000000	41.559471	19.286859		824000000	53.848536	21.046323
824900000	41.626348	19.255343		824900000	53.836878	21.061756
825800000	41.574921	18.749347		825800000	53.912873	21.012184
826700000	41.495317	18.769255		826700000	53.866372	21.084608
827600000	41.524503	19.572751		827600000	53.877533	21.086146
828500000	41.453219	19.691251		828500000	53.871826	21.071617
829400000	41.474825	19.555821		829400000	53.877225	21.102917
830300000	41.540509	19.645248		830300000	53.871114	21.071928
831200000	41.528031	19.439698		831200000	53.889893	21.109305
832100000	41.529694	18.625416		832100000	53.890904	21.097009
833000000	41.451107	18.859946		833000000	53.813935	21.114849
833900000	41.505843	19.748819		833900000	53.815945	21.136105
834800000	41.548821	19.990147		834800000	53.837467	21.150323
835700000	41.577195	19.928789		835700000	53.831505	21.119378
836600000	41.562617	20.000158		836600000	53.825562	21.088466
837500000	41.565365	19.635072		837500000	53.847083	21.102551
838400000	41.551863	18.826912		838400000	53.777799	21.138862
839300000	41.518373	19.182774		839300000	53.844231	21.125409
840200000	41.545771	20.321049		840200000	53.819974	21.134238
841100000	41.625198	20.278847		841100000	53.808977	21.149140
842000000	41.644704	20.208828		842000000	53.822442	21.111184
842900000	41.611098	19.964607		842900000	53.782588	21.136709
843800000	41.567551	19.334881		843800000	53.770196	21.102855
844700000	41.492495	18.737412		844700000	53.752283	21.098440
845600000	41.595294	19.849752		845600000	53.780704	21.071480
846500000	41.716167	20.359021		846500000	53.735288	21.066359
847400000	41.761452	20.362395		847400000	53.759404	21.057366
848300000	41.748065	20.406468		848300000	53.754931	21.015368
849200000	41.701477	20.356443		849200000	53.815223	21.074627
850100000	41.603102	19.852319		850100000	53.773529	21.079109
851000000	41.530275	18.995781		851000000	53.719508	21.050097
851900000	41.640412	19.799573		851900000	53.811076	20.988771
852800000	41.785317	19.918771		852800000	53.758841	21.008161
853700000	41.820011	20.020379		853700000	53.775759	20.980049
854600000	41.833948	19.752405		854600000	53.774788	20.991163
855500000	41.755612	20.411683		855500000	53.743539	21.008146
856400000	41.701542	20.095651		856400000	53.768792	20.944475
857300000	41.565348	19.274689		857300000	53.782708	20.966214
858200000	41.626269	19.932137		858200000	53.704827	20.973672
859100000	41.904471	20.173105		859100000	53.706962	20.934978
860000000	41.931189	20.211592		860000000	53.756966	20.894565
860900000	41.874312	19.770067		860900000	53.710082	20.869027
861800000	41.810654	19.615594		861800000	53.679795	20.858803
862700000	41.611673	19.940681		862700000	53.782839	20.916826
863600000	41.590152	19.470003		863600000	53.695937	20.841984
864500000	41.800318	19.776664		864500000	53.743292	20.781077
865400000	41.881244	20.312102		865400000	53.721500	20.821493
866300000	41.032187	19.433891		866300000	53.734735	20.784253
867200000	41.967076	20.189665		867200000	53.688203	20.758977
868100000	40.895861	19.992624		868100000	53.689825	20.747634
869000000	40.794425	19.572079		869000000	53.659863	20.737600

1900 MHz Head				1900 MHz Body		
Frequency	e'	e''		Frequency	e'	e''
185000000	39.515658	13.572314		185000000	53.610099	13.990623
185120000	39.515289	13.565529		185120000	53.571643	13.969518
185240000	39.534231	13.531715		185240000	53.591382	14.016414
185360000	39.519764	13.545747		185360000	53.601427	13.984232
185480000	39.502872	13.546224		185480000	53.541049	13.942952
185600000	39.497180	13.506712		185600000	53.474739	13.866918
185720000	39.500860	13.530467		185720000	53.455789	13.802804
185840000	39.474062	13.510156		185840000	53.509401	13.862545
185960000	39.494788	13.508248		185960000	53.535671	13.892453
186080000	39.438101	13.497654		186080000	53.515867	13.927822
186200000	39.453150	13.496261		186200000	53.516868	13.925835
186320000	39.447747	13.471730		186320000	53.517987	13.879928
186440000	39.432646	13.489195		186440000	53.509250	13.971032
186560000	39.444456	13.501814		186560000	53.467224	13.906060
186680000	39.430990	13.512279		186680000	53.472851	13.932776
186800000	39.430980	13.496352		186800000	53.486695	13.944676
186920000	39.406545	13.498728		186920000	53.520130	13.989808
187040000	39.396632	13.509950		187040000	53.477556	13.984009
187160000	39.393963	13.489747		187160000	53.506378	14.004006
187280000	39.410400	13.490464		187280000	53.505101	14.015174
187400000	39.409164	13.520195		187400000	53.487669	14.048473
187520000	39.396773	13.470258		187520000	53.471347	14.055113
187640000	39.394553	13.512516		187640000	53.490980	14.068930
187760000	39.388998	13.521024		187760000	53.482507	14.072093
187880000	39.370037	13.508110		187880000	53.474685	14.012444
188000000	39.362834	13.475894		188000000	53.471632	14.025257
188120000	39.356824	13.478749		188120000	53.494337	14.058128
188240000	39.359419	13.500034		188240000	53.479498	14.03061
188360000	39.326293	13.469313		188360000	53.482734	13.979059
188480000	39.373110	13.513351		188480000	53.480697	14.016541
188600000	39.376419	13.507375		188600000	53.488158	14.001264
188720000	39.357561	13.494509		188720000	53.465653	14.028468
188840000	39.340179	13.507513		188840000	53.455706	14.124422
188960000	39.319444	13.486927		188960000	53.497573	14.154019
189080000	39.311965	13.496670		189080000	53.474272	14.152728
189200000	39.314546	13.494114		189200000	53.487210	14.146963
189320000	39.301156	13.489781		189320000	53.397435	13.995489
189440000	39.311254	13.494353		189440000	53.444571	14.041923
189560000	39.296686	13.511587		189560000	53.448325	14.026514
189680000	39.268058	13.534731		189680000	53.441965	14.086315
189800000	39.280711	13.519834		189800000	53.444669	14.101031
189920000	39.281002	13.560333		189920000	53.461806	14.138903
190040000	39.295196	13.538512		190040000	53.454226	14.236515
190160000	39.331695	13.579749		190160000	53.500872	14.298093
190280000	39.314727	13.583670		190280000	53.460710	14.353000
190400000	39.325468	13.593681		190400000	53.502438	14.338487
190520000	39.325825	13.568739		190520000	53.502035	14.341576
190640000	39.303602	13.629451		190640000	53.531387	14.360696
190760000	39.323946	13.645180		190760000	53.487790	14.411610
190880000	39.327462	13.671673		190880000	53.511743	14.421008
191000000	39.321504	13.650727		191000000	53.503154	14.384005

### System Accuracy Verification

Prior to the assessment, the system validation kit was used to test whether the system was operating within its specifications of  $\pm 10\%$ . The validation results are tabulated below. And also the corresponding SAR plot is attached as well in the SAR plots files.

### System Verification Setup Block Diagram

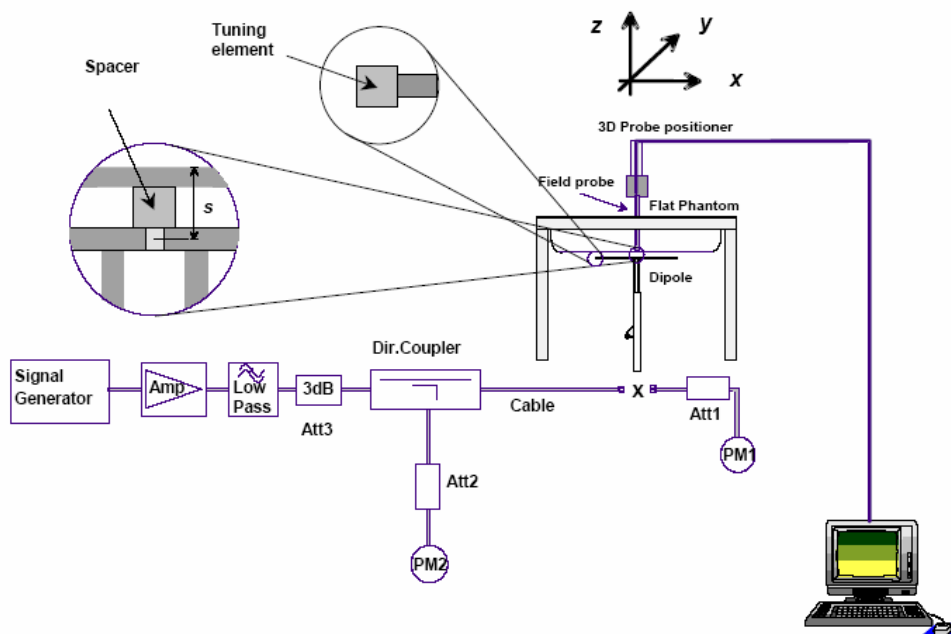

### System Accuracy Check Results

Frequency (MHz)	1 g SAR (W/Kg)	10 g SAR (W/Kg)	Result
835	9.651	6.042	In Tolerance
1900	40.328	20.137	In Tolerance

\* Note: All SAR values are normalized to 1 Watt forward power.

### IEEE P1528 recommended reference value for Head Tissue


Frequency (MHz)	1 g SAR (W/Kg)	10 g SAR (W/Kg)	Local SAR at surface (above feed point)	Local SAR at surface ( $v=2\text{cm}$ offset from feed point)
300	3.0	2.0	4.4	2.1
450	4.9	3.3	7.2	3.2
835	9.5	6.2	14.1	4.9
900	10.8	6.9	16.4	5.4
1450	29.0	16.0	50.2	6.5
1800	38.1	19.8	69.5	6.8
1900	39.7	20.5	72.1	6.6
2000	41.1	21.1	74.6	6.5
2450	52.4	24.0	104.2	7.7
3000	63.8	25.7	140.2	9.5

## EUT TEST STRATEGY AND METHODOLOGY

### Test Positions for Device Operating Next to a Person’s Ear

This category includes most wireless handsets with fixed, retractable or internal antennas located toward the top half of the device, with or without a foldout, sliding or similar keypad cover. The handset should have its earpiece located within the upper ¼ of the device, either along the centerline or off-centered, as perceived by its users. This type of handset should be positioned in a normal operating position with the “test device reference point” located along the “vertical centerline” on the front of the device aligned to the “ear reference point”. The “test device reference point” should be located at the same level as the center of the earpiece region. The “vertical centerline” should bisect the front surface of the handset at its top and bottom edges. A “ear reference point” is located on the outer surface of the head phantom on each ear spacer. It is located 1.5 cm above the center of the ear canal entrance in the “phantom reference plane” defined by the three lines joining the center of each “ear reference point” (left and right) and the tip of the mouth.

A handset should be initially positioned with the earpiece region pressed against the ear spacer of a head phantom. For the SCC-34/SC-2 head phantom, the device should be positioned parallel to the “N-F” line defined along the base of the ear spacer that contains the “ear reference point”. For interim head phantoms, the device should be positioned parallel to the cheek for maximum RF energy coupling. The “test device reference point” is aligned to the “ear reference point” on the head phantom and the “vertical centerline” is aligned to the “phantom reference plane”. This is called the “initial ear position”. While maintaining these three alignments, the body of the handset is gradually adjusted to each of the following positions for evaluating SAR:

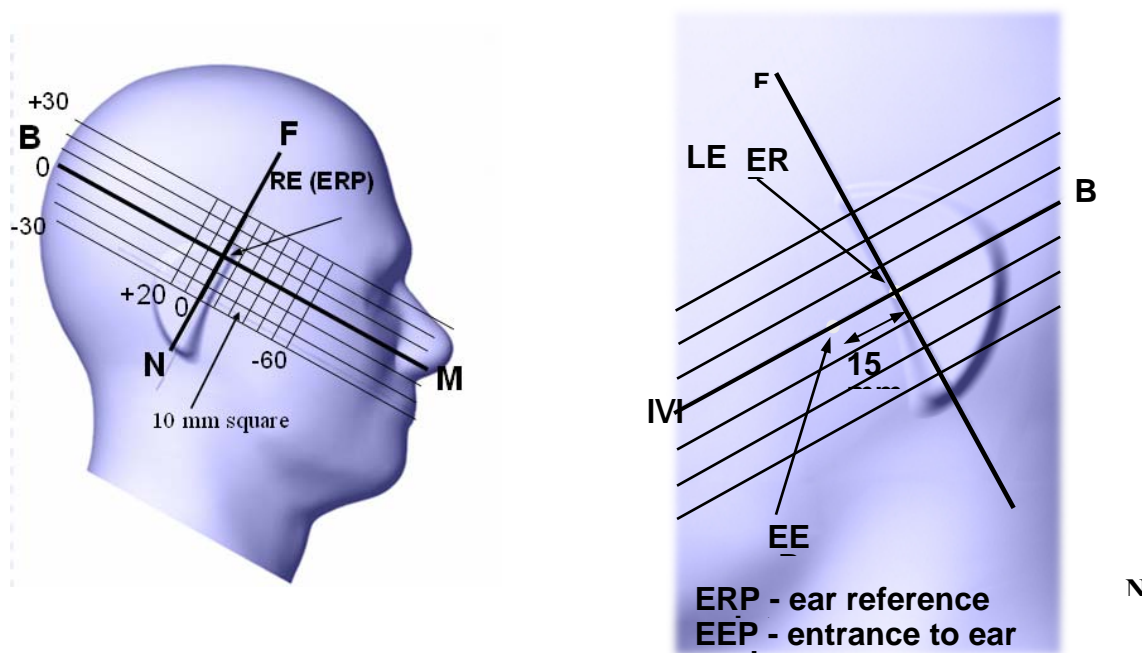

## Cheek/Touch Position


The device is brought toward the mouth of the head phantom by pivoting against the “ear reference point” or along the “N-F” line for the SCC-34/SC-2 head phantom.

This test position is established:

- When any point on the display, keypad or mouthpiece portions of the handset is in contact with the phantom.
- (or) When any portion of a foldout, sliding or similar keypad cover opened to its intended self-adjusting normal use position is in contact with the cheek or mouth of the phantom.

For existing head phantoms – when the handset loses contact with the phantom at the pivoting point, rotation should continue until the device touches the cheek of the phantom or breaks its last contact from the ear spacer.

### Check /Touch Position

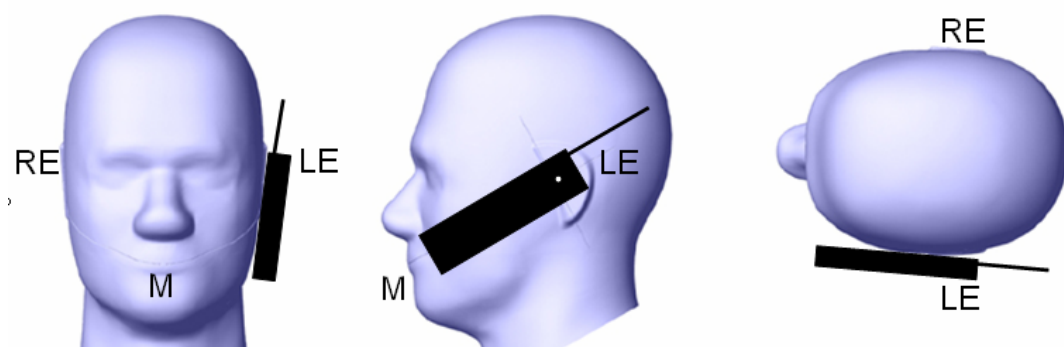

## Ear/Tilt Position


With the handset aligned in the “Cheek/Touch Position”:

1) If the earpiece of the handset is not in full contact with the phantom’s ear spacer (in the “Cheek/Touch position”) and the peak SAR location for the “Cheek/Touch” position is located at the ear spacer region or corresponds to the earpiece region of the handset, the device should be returned to the “initial ear position” by rotating it away from the mouth until the earpiece is in full contact with the ear spacer.

2) (otherwise) The handset should be moved (translated) away from the cheek perpendicular to the line passes through both “ear reference points” (note: one of these ear reference points may not physically exist on a split head model) for approximate 2-3 cm. While it is in this position, the device handset is tilted away from the mouth with respect to the “test device reference point” until the inside angle between the vertical centerline on the front surface of the phone and the horizontal line passing through the ear reference point is by 15 80°. After the tilt, it is then moved (translated) back toward the head perpendicular to the line passes through both “ear reference points” until the device touches the phantom or the ear spacer. If the antenna touches the head first, the positioning process should be repeated with a tilt angle less than 15° so that the device and its antenna would touch the phantom simultaneously. This test position may require a device holder or positioner to achieve the translation and tilting with acceptable positioning repeatability.

If a device is also designed to transmit with its keypad cover closed for operating in the head position, such positions should also be considered in the SAR evaluation. The device should be tested on the left and right side of the head phantom in the “Cheek/Touch” and “Ear/Tilt” positions. When applicable, each configuration should be tested with the antenna in its fully extended and fully retracted positions. These test configurations should be tested at the high, middle and low frequency channels of each operating mode; for example, AMPS, CDMA, and TDMA. If the SAR measured at the middle channel for each test configuration (left, right, Cheek/Touch, Tile/Ear, extended and retracted) is at least 2.0 dB lower than the SAR limit, testing at the high and low channels is optional for such test configuration(s). If the transmission band of the test device is less than 10 MHz, testing at the high and low frequency channels is optional.

### Ear /Tilt 15° Position

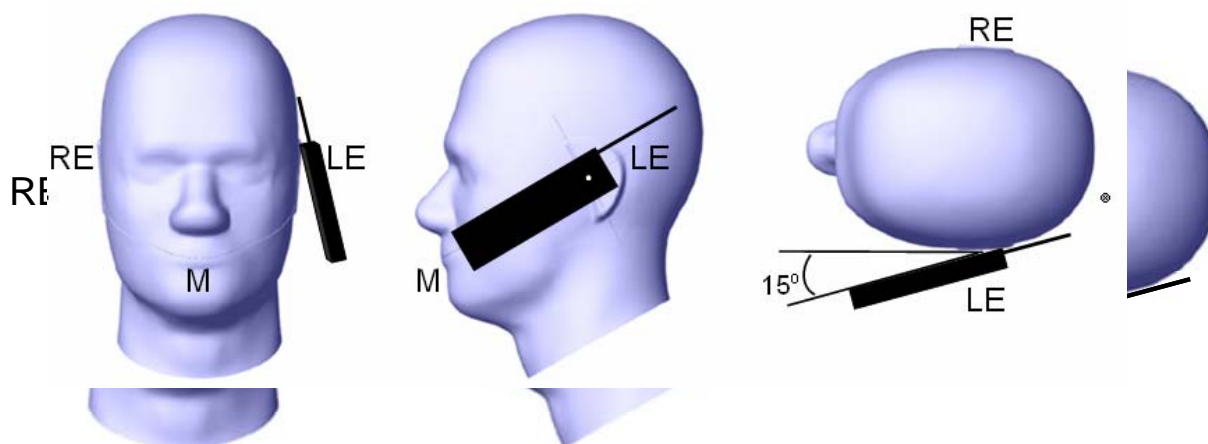

### **Test positions for body-worn and other configurations**

Body-worn operating configurations should be tested with the belt-clips and holsters attached to the device and positioned against a flat phantom in normal use configurations. Devices with a headset output should be tested with a headset connected to the device. When multiple accessories that do not contain metallic components are supplied with the device, the device may be tested with only the accessory that dictates the closest spacing to the body. When multiple accessories that contain metallic components are supplied with the device, the device must be tested with each accessory that contains a unique metallic component. If multiple accessories share an identical metallic component (e.g., the same metallic belt-clip used with different holsters with no other metallic components), only the accessory that dictates the closest spacing to the body must be tested.

Body-worn accessories may not always be supplied or available as options for some devices that are intended to be authorized for body-worn use. A separation distance of 1.5 cm between the back of the device and a flat phantom is recommended for testing body-worn SAR compliance under such circumstances. Other separation distances may be used, but they should not exceed 2.5 cm. In these cases, the device may use body-worn accessories that provide a separation distance greater than that tested for the device provided however that the accessory contains no metallic components.

## SAR Evaluation Procedure

The evaluation was performed with the following procedure:

**Step 1:** Measurement of the SAR value at a fixed location above the ear point or central position was used as a reference value for assessing the power drop. The SAR at this point is measured at the start of the test and then again at the end of the testing.

**Step 2:** The SAR distribution at the exposed side of the head was measured at a distance of 4 mm from the inner surface of the shell. The area covered the entire dimension of the head or EUT and the horizontal grid spacing was 15 mm x 15 mm. Based on these data, the area of the maximum absorption was determined by spline interpolation. The first Area Scan covers the entire dimension of the EUT to ensure that the hotspot was correctly identified.

**Step 3:** Around this point, a volume of 30 mm x 30 mm x 21 mm was assessed by measuring 5 x 5 x 7 points. On the basis of this data set, the spatial peak SAR value was evaluated under the following procedure:

- 1) The data at the surface were extrapolated, since the center of the dipoles is 1.2 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is 1.3 mm. The extrapolation was based on a least square algorithm. A polynomial of the fourth order was calculated through the points in z-axes. This polynomial was then used to evaluate the points between the surface and the probe tip.
- 2) The maximum interpolated value was searched with a straightforward algorithm. Around this maximum the SAR values averaged over the spatial volumes (1 g or 10 g) were computed by the 3D-Spline interpolation algorithm. The 3D-Spline is composed of three one dimensional splines with the "Not a knot"-condition (in x, y and z-directions). The volume was integrated with the trapezoidal-algorithm. One thousand points (10 x 10 x 10) were interpolated to calculate the averages.

All neighboring volumes were evaluated until no neighboring volume with a higher average value was found.

**Step 4:** Re-measurement of the SAR value at the same location as in Step 1. If the value changed by more than 5%, the evaluation was repeated.

## SAR MEASUREMENT RESULTS

This page summarizes the results of the performed dosimetric evaluation. The plots with the corresponding SAR distributions, which reveal information about the location of the maximum SAR with respect to the device, could be found in Appendix E.

### SAR Test Data

#### Environmental Conditions

<b>Temperature:</b>	21° C
<b>Relative Humidity:</b>	54%
<b>ATM Pressure:</b>	1010 mbar

\* Testing was performed by Eric Zhang on 2009-03-12.

#### Cellular Band:

EUT Position	Frequency (MHz)	Test mode	Test Type	Liquid Type	Phantom	Accessories	1 g SAR Value (W/Kg)	1 g SAR Limit (W/Kg)	Ref. Plot #
Body-Worn Back	836.6	GPRS	Body	Body	Flat	-	0.263	1.6	1
Body-Worn Back	824.2	GPRS	Body	Body	Flat	-	0.352	1.6	2
Body-Worn Back	848.8	GPRS	Body	Body	Flat	-	0.370	1.6	3
Body-Worn Back	836.6	GSM	Body	Body	Flat	-	0.366	1.6	4
Body-Worn Back	824.2	GSM	Body	Body	Flat	-	0.346	1.6	5
Body-Worn Back	848.8	GSM	Body	Body	Flat	-	0.384	1.6	6

#### PCS Band:

EUT Position	Frequency (MHz)	Test mode	Test Type	Liquid Type	Phantom	Accessories	1 g SAR Value (W/Kg)	1 g SAR Limit (W/Kg)	Ref. Plot #
Body-Worn Back	1880.0	GPRS	Body	Body	Flat	-	0.345	1.6	7
Body-Worn Back	1850.2	GPRS	Body	Body	Flat	-	0.204	1.6	8
Body-Worn Back	1909.8	GPRS	Body	Body	Flat	-	0.301	1.6	9
Body-Worn Back	1880.0	GSM	Body	Body	Flat	-	0.322	1.6	10
Body-Worn Back	1850.2	GSM	Body	Body	Flat	-	0.188	1.6	11
Body-Worn Back	1909.8	GSM	Body	Body	Flat	-	0.304	1.6	12



## APPENDIX A – MEASUREMENT UNCERTAINTY

The uncertainty budget has been determined for the measurement system and is given in the following Table.

### Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	$c_i^1$ (1-g)	$c_i^1$ (10-g)	Standard Uncertainty (1-g) %	Standard Uncertainty (10-g) %
<b>Measurement System</b>							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)^{1/2}$	$(\frac{1-cp}{2})^1$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
<b>Restriction</b>							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	3.2	rectangular	$\sqrt{3}$	1	1	1.8	1.8
<b>Phantom and Setup</b>							
Phantom Uncertainty(shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity(target)	5.0	rectangular	$\sqrt{3}$	0.7	0.5	2.0	1.4
Liquid Conductivity(meas.)	0.0	normal	1	0.7	0.5	0.0	0.0
Liquid Permittivity(target)	5.0	rectangular	$\sqrt{3}$	0.6	0.5	1.7	1.4
Liquid Permittivity(meas.)	0.0	normal	1	0.6	0.5	0.0	0.0
Combined Uncertainty		RSS				9.4	9.2
Combined Uncertainty (coverage factor=2)		Normal(k=2)				18.8	18.5

## APPENDIX B – PROBE CALIBRATION CERTIFICATES

---

### NCL CALIBRATION LABORATORIES

Calibration File No.: CP-871

Client.: BACL

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 835 MHz

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 273

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: BACB-ALSAS10U-5323

Calibrated: 1<sup>st</sup> August 2008

Released on: 1<sup>st</sup> September 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E8

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

**NCL Calibration Laboratories**Division of APREL Laboratories.

---

**Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 273.

**References**


SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices; Experimental Techniques"  
SSI-TP-011 Tissue Calibration Procedure

**Conditions**

Probe 273 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

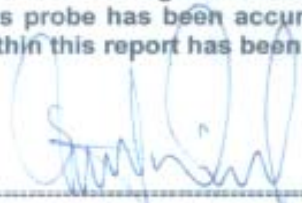

---

Stuart Nicol



---

Jesse Hones

---

Page 2 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Calibration Results Summary**

<b>Probe Type:</b>	E-Field Probe E-020
<b>Serial Number:</b>	273
<b>Frequency:</b>	835 MHz
<b>Sensor Offset:</b>	1.56 mm
<b>Sensor Length:</b>	2.5 mm
<b>Tip Enclosure:</b>	Ertalyte*
<b>Tip Diameter:</b>	<5 mm
<b>Tip Length:</b>	60 mm
<b>Total Length:</b>	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

**Sensitivity in Air**

<b>Channel X:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Y:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Z:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Diode Compression Point:</b>	95 mV

Page 3 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**Division of APREL Laboratories.

---

**Sensitivity in Head Tissue Measured**

**Frequency:** 835 MHz

**Epsilon:** 41.24 (+/-5%)      **Sigma:** 0.87 S/m (+/-5%)

**ConvF****Channel X:** 6.5**Channel Y:** 6.5**Channel Z:** 6.5

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

**Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

**Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

---

Page 4 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.



**Receiving Pattern 835 MHz (Air)**



**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Isotropy Error 835 MHz (Air)**

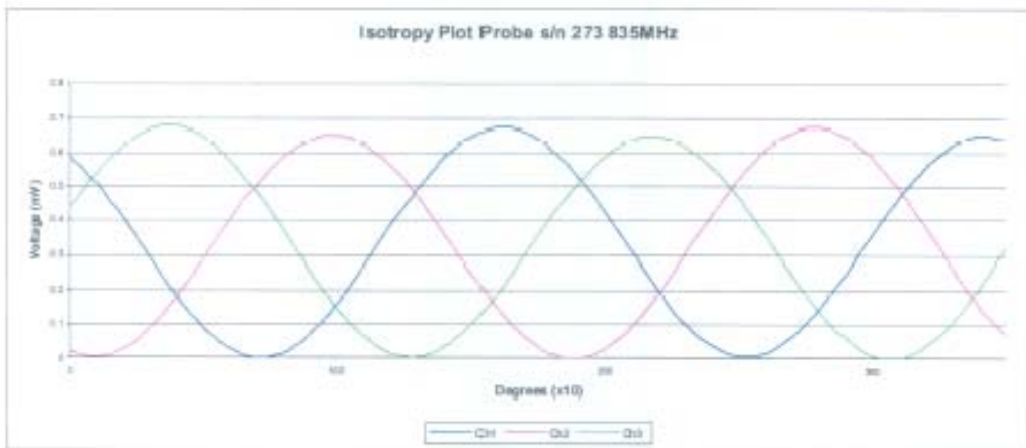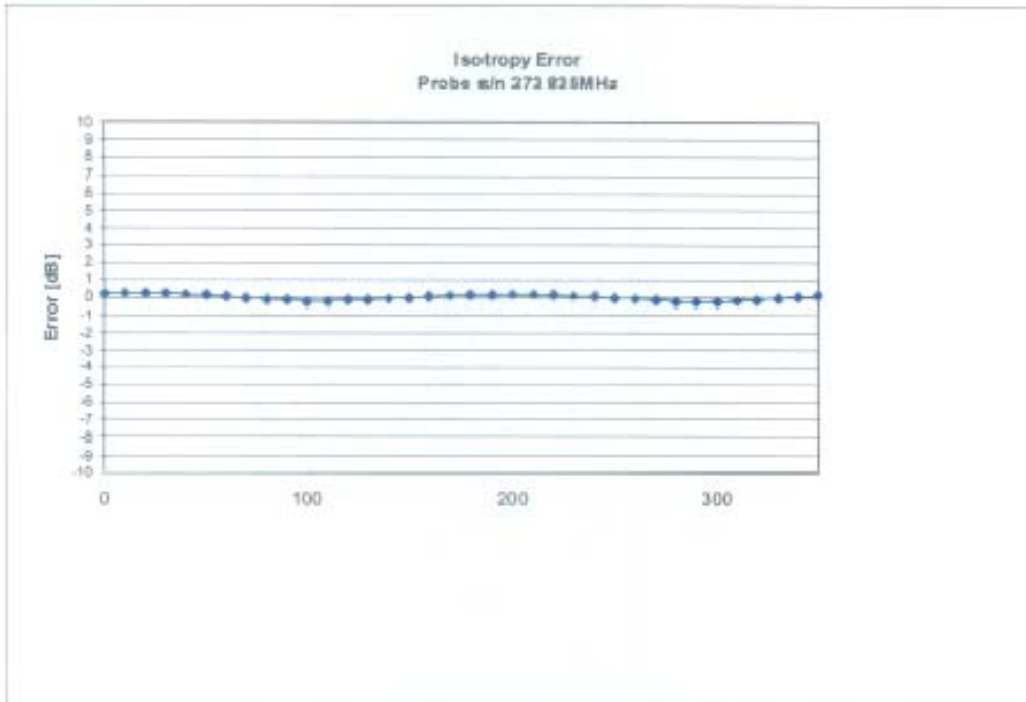

**Isotropy Tissue:**

**0.10 dB**

Page 6 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Dynamic Range**






**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Video Bandwidth**

**Probe Frequency Characteristics**

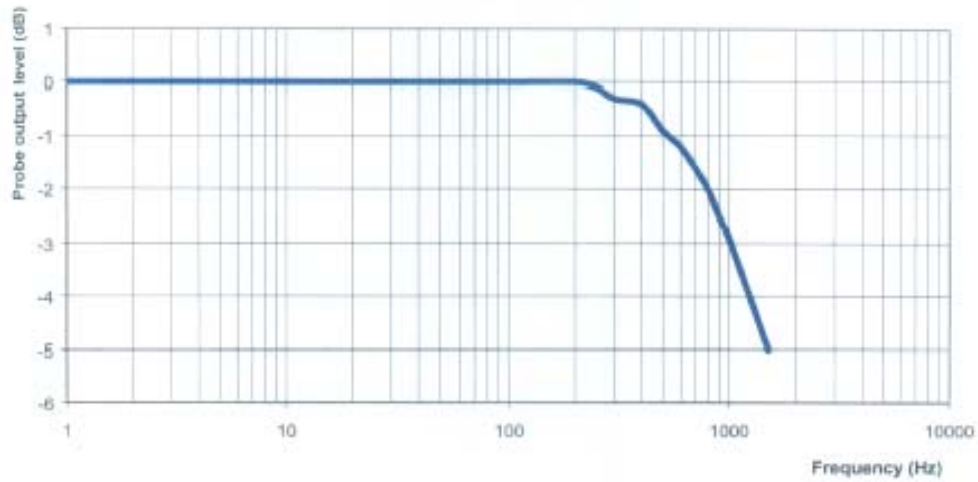

**Video Bandwidth at 500 Hz**            1 dB  
**Video Bandwidth at 1.02 KHz:**        3 dB

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Conversion Factor Uncertainty Assessment**

**Frequency:** 835MHz  
**Epsilon:** 41.24 (+/-5%)      **Sigma:** 0.87 S/m (+/-5%)

**ConvF**

**Channel X:** 6.5      7%(K=2)  
**Channel Y:** 6.5      7%(K=2)  
**Channel Z:** 6.5      7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

**Boundary Effect:**

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

---

Page 9 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

---

Division of APREL Laboratories.

**Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

---

Page 10 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL CALIBRATION LABORATORIES**

Calibration File No.: CP-872

Client.: BACL

**CERTIFICATE OF CALIBRATION**

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 835 MHz

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 273

Calibration in Body Tissue

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: BACL-ALSAS10U-5323

Calibrated: 1<sup>st</sup> September 2008

Released on: 1<sup>st</sup> September 2008

This Calibration Certificate is incomplete unless accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E8

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 273.

**References**

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
SSI-TP-011 Tissue Calibration Procedure

**Conditions**

Probe 273 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

  
-----  
Stuart Nicol  
-----  
Jesse Hones

---

Page 2 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Calibration Results Summary**

<b>Probe Type:</b>	E-Field Probe E-020
<b>Serial Number:</b>	273
<b>Frequency:</b>	835 MHz
<b>Sensor Offset:</b>	1.56 mm
<b>Sensor Length:</b>	2.5 mm
<b>Tip Enclosure:</b>	Ertalyte*
<b>Tip Diameter:</b>	<5 mm
<b>Tip Length:</b>	60 mm
<b>Total Length:</b>	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

**Sensitivity in Air**

<b>Channel X:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Y:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Z:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Diode Compression Point:</b>	95 mV

Page 3 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**Division of APREL Laboratories.

---

**Sensitivity in Body Tissue Measured****Frequency:** 835 MHz**Epsilon:** 56.16 (+/-5%)**Sigma:** 0.99 S/m (+/-10%)**ConvF****Channel X:** 6.7**Channel Y:** 6.7**Channel Z:** 6.7

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

**Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

**Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


---

Page 4 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**  
Division of APREL Laboratories.

**Receiving Pattern 835 MHz (Air)**


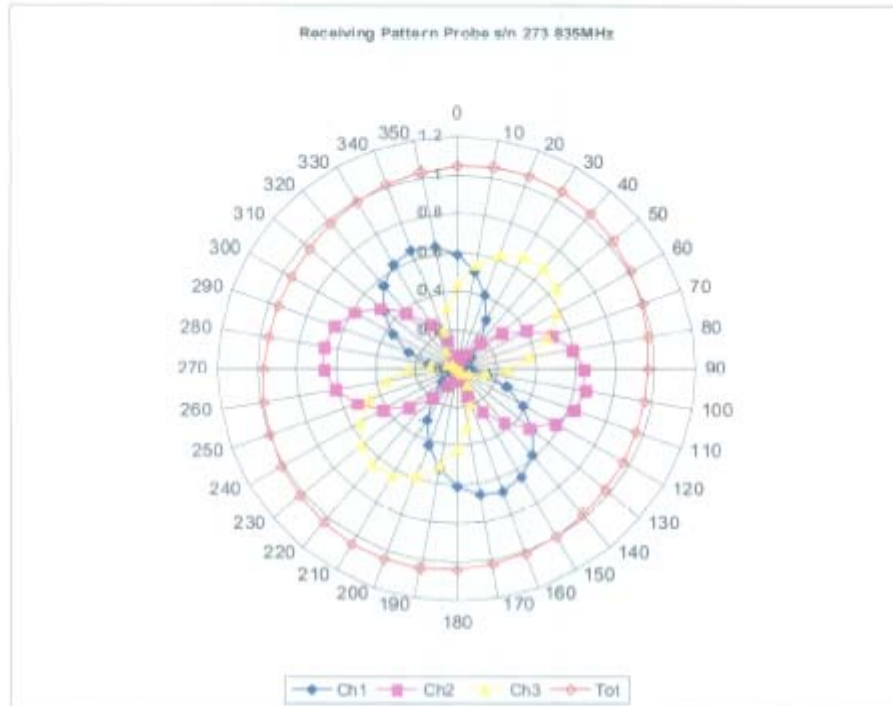


Page 5 of 10  
This page has been reviewed for content and attested to on Page 2 of this document.



**NCL Calibration Laboratories**  
Division of APREL Laboratories.

**Isotropy Error 835 MHz (Air)**

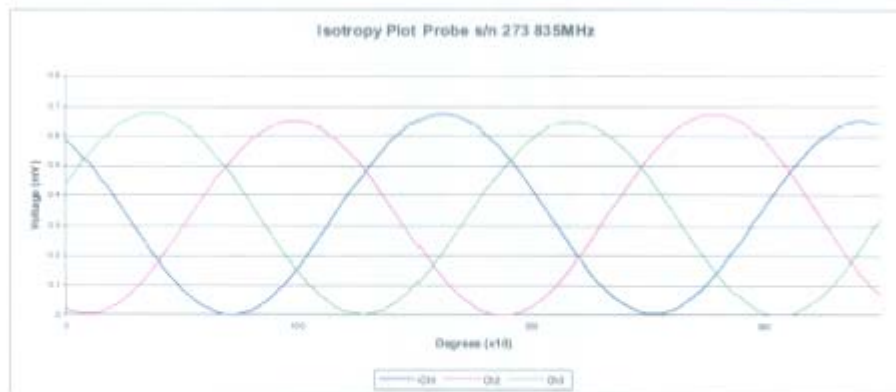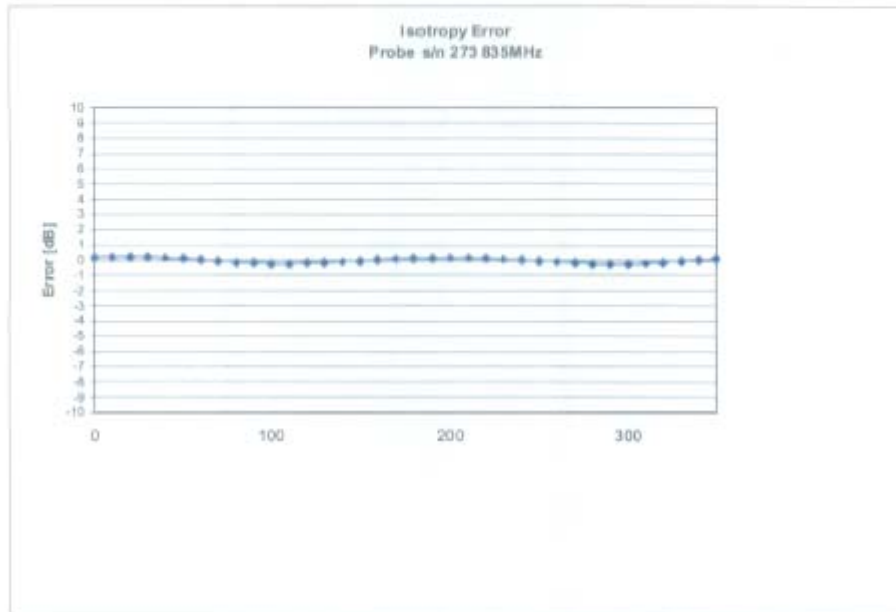

**Isotropy in Tissue: 0.10 dB**

Page 6 of 10  
This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories

Division of APREL Laboratories.

Dynamic Range




Page 7 of 10  
This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Video Bandwidth**

Probe Frequency Characteristics

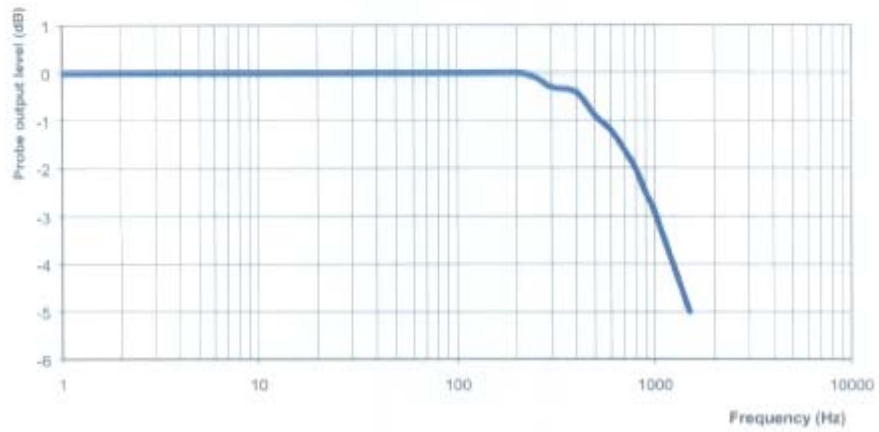

Video Bandwidth at 500 Hz            1 dB  
Video Bandwidth at 1.02 KHz:        3 dB

Page 8 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Conversion Factor Uncertainty Assessment**

**Frequency:** 835MHz  
**Epsilon:** 56.16 (+/-5%)      **Sigma:** 0.99 S/m (+/-10%)

**ConvF**

**Channel X:** 6.7      7%(K=2)

**Channel Y:** 6.7      7%(K=2)

**Channel Z:** 6.7      7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

**Boundary Effect:**

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

---

Page 9 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

---

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

---

Page 10 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL CALIBRATION LABORATORIES**

Calibration File No.: CP-877

Client.: BACL

**CERTIFICATE OF CALIBRATION**

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 1900 MHz

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 273

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: BACB-ALSAS10U-5323

Calibrated: 1<sup>st</sup> August 2008

Released on: 1<sup>st</sup> September 2008

This Calibration Certificate is incomplete unless accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E9

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 273.

**References**

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
SSI-TP-011 Tissue Calibration Procedure


**Conditions**

Probe 273 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C

**Temperature of the Tissue:** 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

  
-----  
Stuart Nicol  
-----  
Jesse Hones

---

Page 2 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Calibration Results Summary**

<b>Probe Type:</b>	E-Field Probe E-020
<b>Serial Number:</b>	273
<b>Frequency:</b>	1900 MHz
<b>Sensor Offset:</b>	1.56 mm
<b>Sensor Length:</b>	2.5 mm
<b>Tip Enclosure:</b>	Ertalyte*
<b>Tip Diameter:</b>	<5 mm
<b>Tip Length:</b>	60 mm
<b>Total Length:</b>	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

**Sensitivity in Air**

<b>Channel X:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Y:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Z:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Diode Compression Point:</b>	95 mV

Page 3 of 10

This page has been reviewed for content and attested to on Page 2 of this document.



---

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Sensitivity in Head Tissue Measured****Frequency:** 1900 MHz**Epsilon:** 38.50 (+/-5%)      **Sigma:** 1.40 S/m (+/-5%)**ConvF****Channel X:** 5.25**Channel Y:** 5.25**Channel Z:** 5.25

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

**Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

**Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

---

Page 4 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories



**Receiving Pattern 1900 MHz (Air)**



**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Isotropy Error 1900 MHz (Air)**

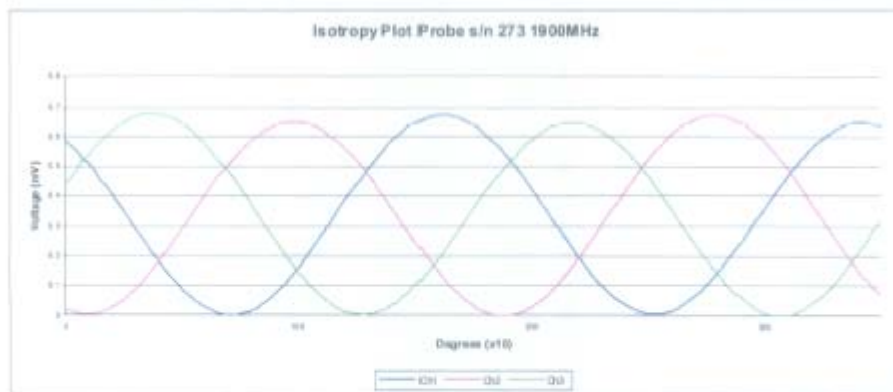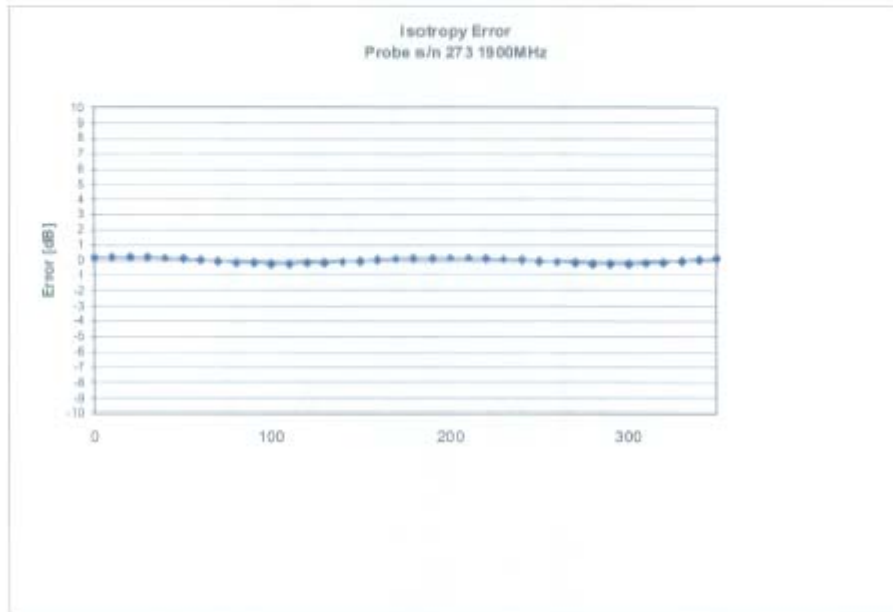

**Isotropicity in Tissue:**

**0.10 dB**

Page 6 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Dynamic Range**




**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Video Bandwidth**

Probe Frequency Characteristics

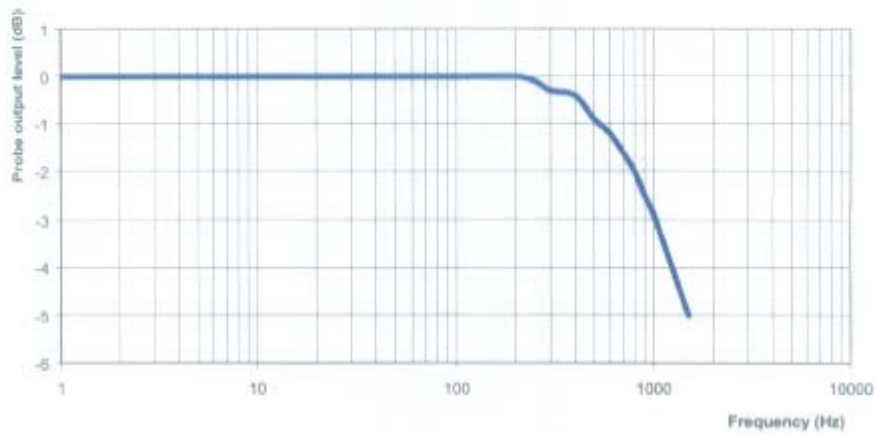

Video Bandwidth at 500 Hz            1 dB  
Video Bandwidth at 1.02 KHz:       3 dB

Page 8 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

11/2/17

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Conversion Factor Uncertainty Assessment**

<b>Frequency:</b>		1900MHz	
<b>Epsilon:</b>	38.50 (+/-5%)	<b>Sigma:</b>	1.40 S/m (+/-5%)
<b>ConvF</b>			
<b>Channel X:</b>	5.25		7%(K=2)
<b>Channel Y:</b>	5.25		7%(K=2)
<b>Channel Z:</b>	5.25		7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

**Boundary Effect:**

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

---

Page 9 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

---

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

---

Page 10 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

## NCL CALIBRATION LABORATORIES

Calibration File No.: CP-278

Client.: BACL

# CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 1900 MHz

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 273

Calibration in Body Tissue

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: BACB-ALSAS10U-5323

Calibrated: 1<sup>st</sup> August 2008

Released on: 1<sup>st</sup> September 2008

This Calibration Certificate is incomplete unless accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_



### **NCL** CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E8

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161



**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 273.

**References**

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
SSI-TP-011 Tissue Calibration Procedure

**Conditions**

Probe 273 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

  
-----  
**Stuart Nicol**

  
-----  
**Jesse Hones**

Page 2 of 10  
This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Calibration Results Summary**

<b>Probe Type:</b>	E-Field Probe E-020
<b>Serial Number:</b>	273
<b>Frequency:</b>	1900 MHz
<b>Sensor Offset:</b>	1.56 mm
<b>Sensor Length:</b>	2.5 mm
<b>Tip Enclosure:</b>	Ertalyte*
<b>Tip Diameter:</b>	<5 mm
<b>Tip Length:</b>	60 mm
<b>Total Length:</b>	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

**Sensitivity in Air**

<b>Channel X:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Y:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Z:</b>	1.2 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Diode Compression Point:</b>	95 mV

---

Page 3 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**Division of APREL Laboratories.

---

**Sensitivity in Body Tissue Measured****Frequency:** 1900 MHz**Epsilon:** 53.05 (+/-5%)      **Sigma:** 1.58 S/m (+/-5%)**ConvF****Channel X:** 5.15**Channel Y:** 5.15**Channel Z:** 5.15

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

**Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

**Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

---


Page 4 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.



**Receiving Pattern 1900 MHz (Air)**

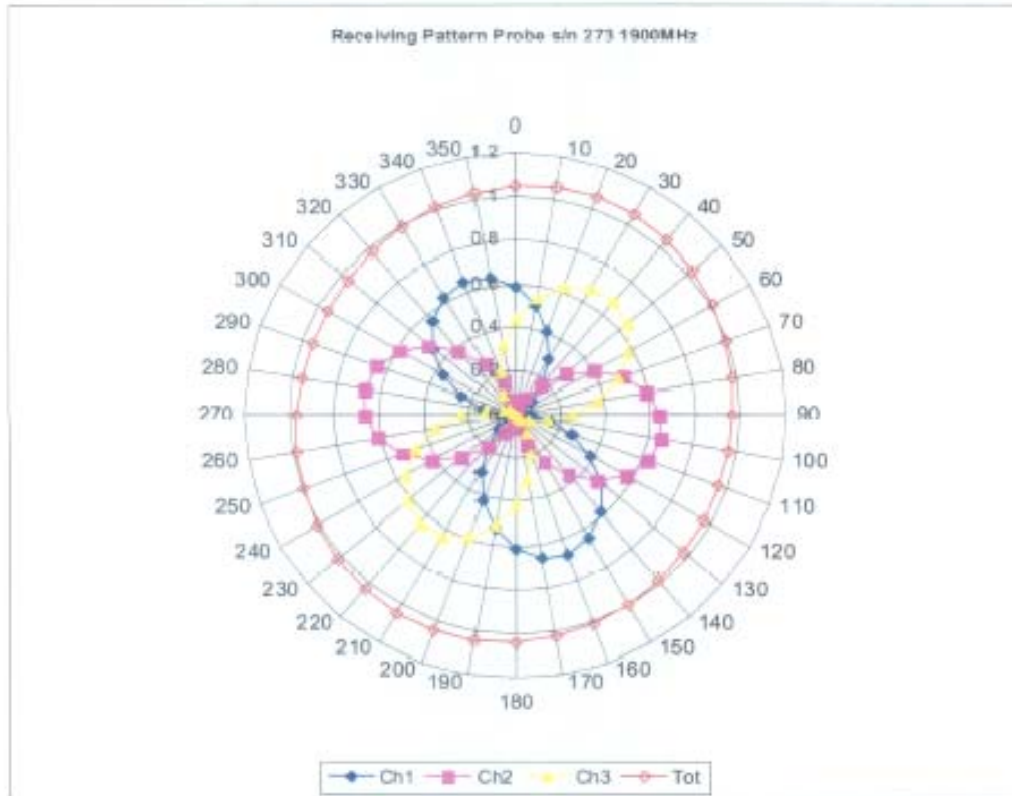

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Isotropy Error 1900 MHz (Air)**

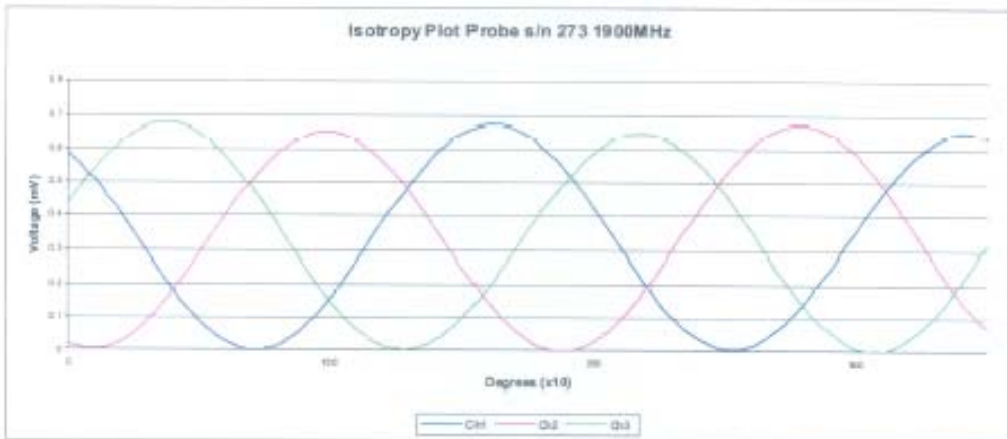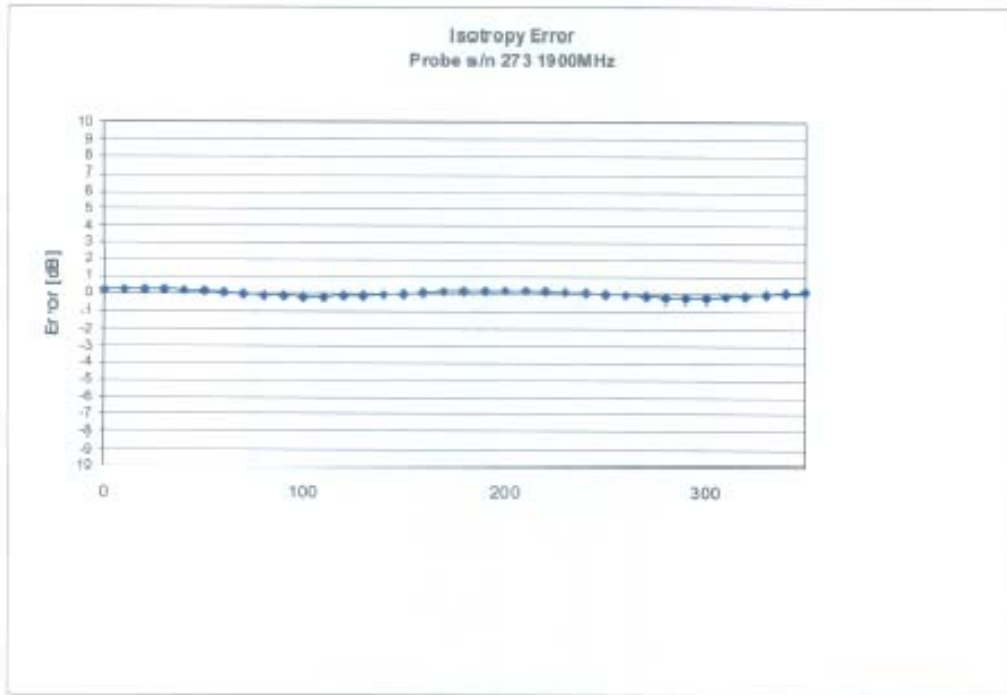

**Isotropicity in Tissue:**

**0.10 dB**

Page 6 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories,

**Dynamic Range**




**NCL Calibration Laboratories**

Division of APREL Laboratories,

---

**Video Bandwidth**

**Probe Frequency Characteristics**

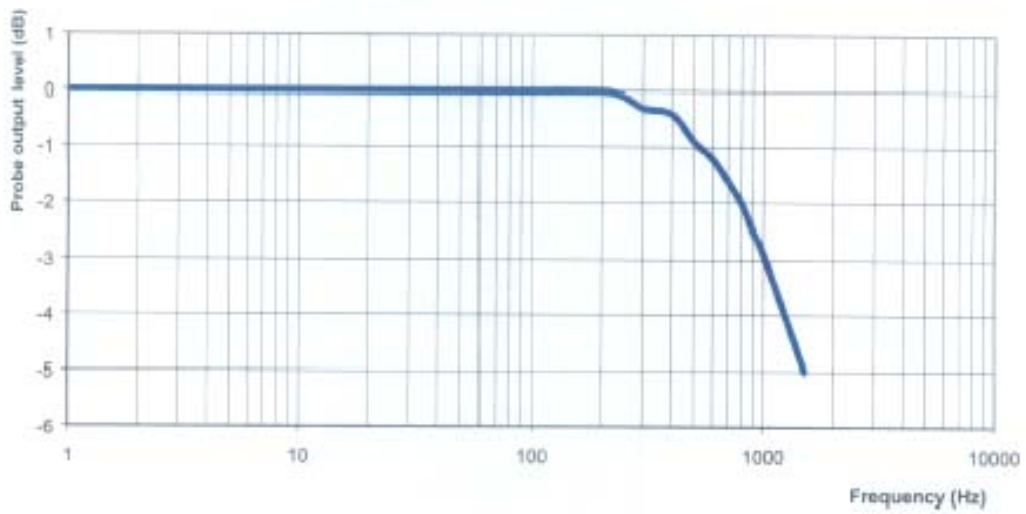

**Video Bandwidth at 500 Hz**            1 dB  
**Video Bandwidth at 1.02 KHz:**        3 dB

**NCL Calibration Laboratories**Division of APREL Laboratories.

---

**Conversion Factor Uncertainty Assessment**

<b>Frequency:</b>		1900MHz	
<b>Epsilon:</b>	53.05 (+/-5%)	<b>Sigma:</b>	1.58 S/m (+/-5%)
<b>ConvF</b>			
<b>Channel X:</b>	5.15		7%(K=2)
<b>Channel Y:</b>	5.15		7%(K=2)
<b>Channel Z:</b>	5.15		7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .

**Boundary Effect:**

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

---

Page 9 of 10

This page has been reviewed for content and attested to on Page 2 of this document.



**NCL Calibration Laboratories**

---

Division of APREL Laboratories.

**Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

---

Page 10 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

---

## APPENDIX C – DIPOLE CALIBRATION CERTIFICATES

---

### NCL CALIBRATION LABORATORIES

Calibration File No: DC-917  
Project Number: BACL-ALSAS10U-5323

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Validation Dipole

Manufacturer: APREL Laboratories

Part number: ALS-D-835-S-2

Frequency: 835 MHz

Serial No: 180-00558

Customer: Bay Area Compliance Laboratory

Calibrated: 1<sup>st</sup> September 2008

Released on: 1<sup>st</sup> September 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL** CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4162

**NCL Calibration Laboratories**

Division of APREL Laboratories.

---

**Conditions**

Dipole 180-00558 was new and taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C

**Temperature of the Tissue:** 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



-----  
**Stuart Nicol**



-----  
**C. Teodorian**

This page has been reviewed for content and attested to by signature within this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Calibration Results Summary**

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

**Mechanical Dimensions**


**Length:** 162.2 mm  
**Height:** 89.4 mm

**Electrical Specification**

**SWR:** 1.018 U  
**Return Loss:** -41.371 dB  
**Impedance:** 51.739 Ω

**System Validation Results**

Frequency	1 Gram	10 Gram	Peak
835 MHz	9.49	6.1	14.21

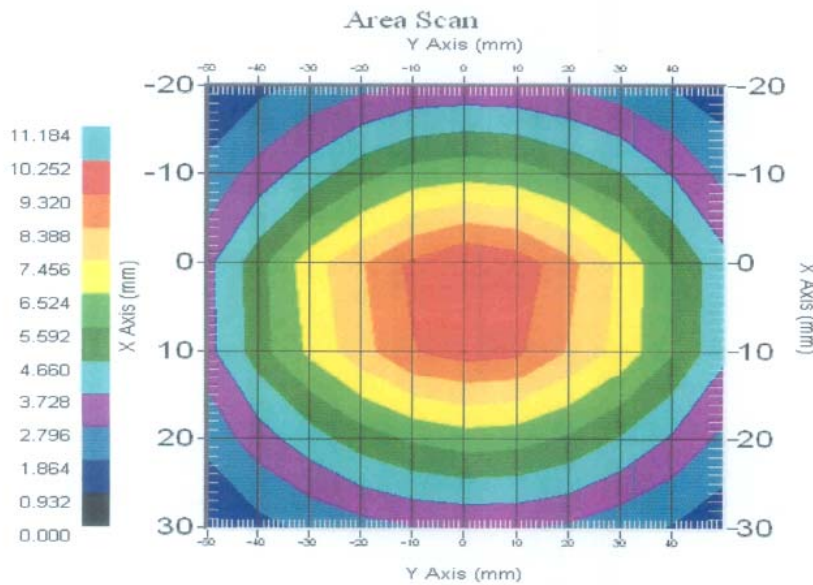

This page has been reviewed for content and attested to by signature within this document.

## **NCL Calibration Laboratories**

Division of APREL Laboratories.

### **Introduction**

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole 180-00558. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-020 130 MHz to 26 GHz E-Field Probe Serial Number 212.

### **References**

SSI-TP-018-ALSAS Dipole Calibration Procedure  
SSI-TP-016 Tissue Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

### **Conditions**

Dipole 180-00558 was new taken from stock.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 20 °C +/- 0.5°C

This page has been reviewed for content and attested to by signature within this document.

4

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Dipole Calibration Results****Mechanical Verification**

APREL Length	APREL Height	Measured Length	Measured Height
161.0 mm	89.8 mm	162.2 mm	89.4 mm

**Tissue Validation**

Head Tissue 835MHz	Measured
Dielectric constant, $\epsilon_r$	41.12
Conductivity, $\sigma$ [S/m]	0.92

This page has been reviewed for content and attested to by signature within this document.

5

**NCL Calibration Laboratories**


Division of APREL Laboratories.

**Electrical Calibration**

Test	Result
S11 RL	-41.371 dB
SWR	1.018 U
Impedance	51.739 Ω

The Following Graphs are the results as displayed on the Vector Network Analyzer.

**S11 Parameter Return Loss**

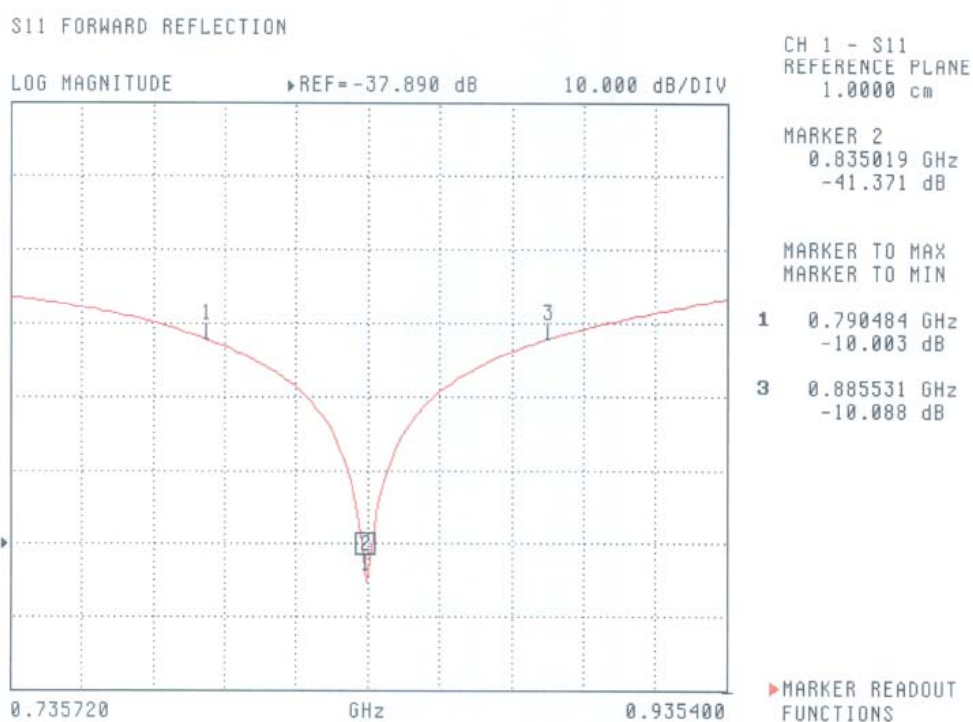

This page has been reviewed for content and attested to by signature within this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**SWR**

S11 FORWARD REFLECTION

SWR REF=500.000 mU 1.000 U/DIV



CH 1 - S11  
REFERENCE PLANE  
1.0000 cm

MARKER 2  
0.835019 GHz  
1.018 U

MARKER TO MAX  
MARKER TO MIN

1 0.790484 GHz  
1.925 U

3 0.885531 GHz  
1.911 U

MARKER READOUT  
FUNCTIONS

This page has been reviewed for content and attested to by signature within this document.


7



**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Smith Chart Dipole Impedance**

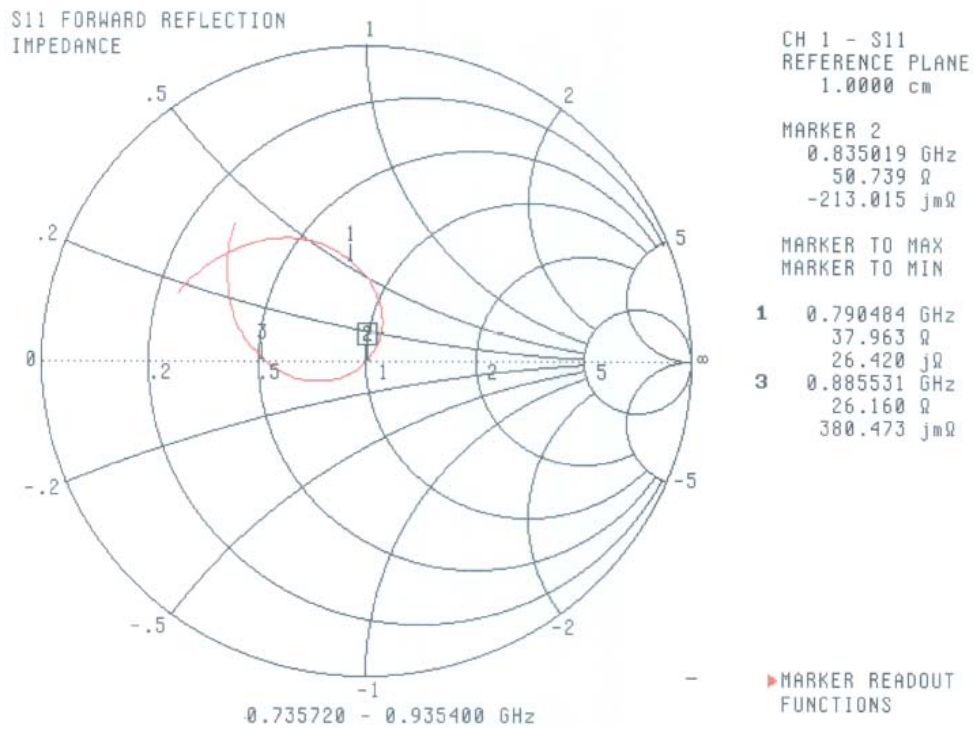


This page has been reviewed for content and attested to by signature within this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**System Validation Results Using the Electrically Calibrated Dipole**

Head Tissue Frequency	1 Gram	10 Gram	Peak Above Feed Point
835 MHz	9.49	6.1	14.21

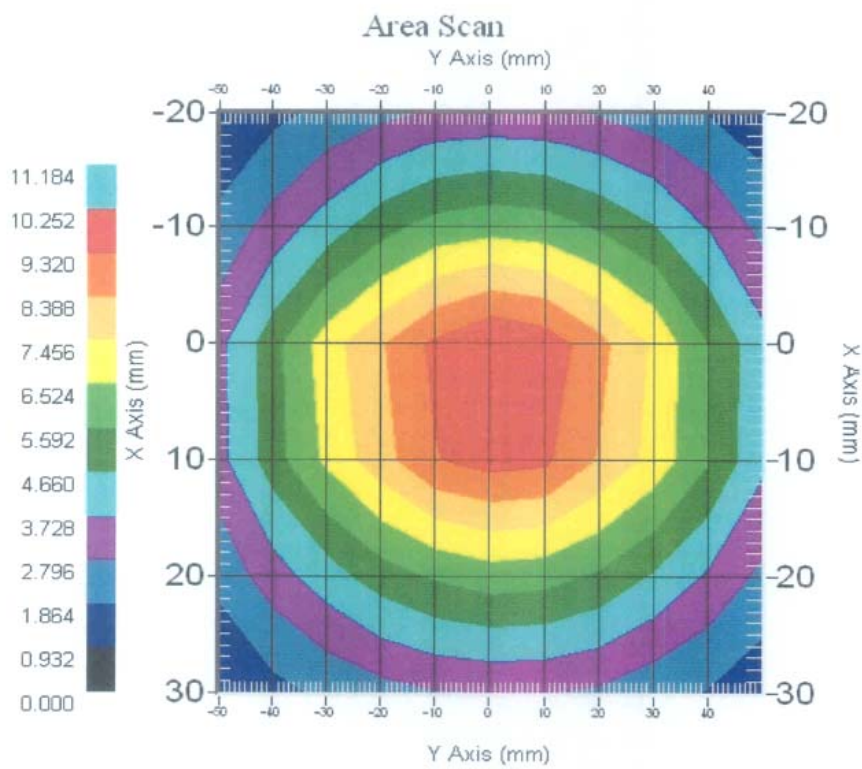

This page has been reviewed for content and attested to by signature within this document.

**NCL Calibration Laboratories**

---

Division of APREL Laboratories.

**Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List 2008.

This page has been reviewed for content and attested to by signature within this document.

10

**NCL CALIBRATION LABORATORIES**

Calibration File No: DC-920  
Project Number: BACL-ALSAS10U-5323

**CERTIFICATE OF CALIBRATION**

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Validation Dipole

Manufacturer: APREL Laboratories  
Part number: ALS-D-1900-S-2  
Frequency: 1900 MHz  
Serial No: 210-00710

Customer: Bay Area Compliance Laboratory

Calibrated: 1<sup>st</sup> September 2008  
Released on: 1<sup>st</sup> September 2008

This Calibration Certificate is incomplete unless accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4162

**NCL Calibration Laboratories**


Division of APREL Laboratories.

**Conditions**

Dipole 210-00710 was new and taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol



C. Teodorian

This page has been reviewed for content and attested to by signature within this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Calibration Results Summary**

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

**Mechanical Dimensions**


**Length:** 67.1 mm  
**Height:** 38.9 mm

**Electrical Specification**

**SWR:** 1.059 U  
**Return Loss:** -30.831 dB  
**Impedance:** 50.914  $\Omega$

**System Validation Results**

Frequency	1 Gram	10 Gram	Peak
1900 MHz	38.7	20.5	69.7

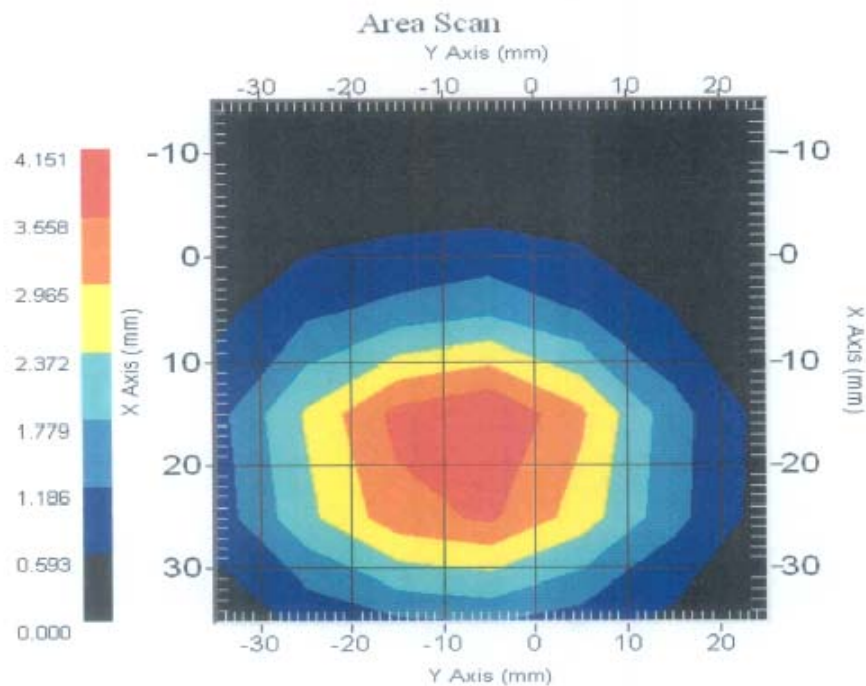

This page has been reviewed for content and attested to by signature within this document.

## **NCL Calibration Laboratories**

Division of APREL Laboratories.

## **Introduction**

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole 210-00710. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-020 130 MHz to 26 GHz E-Field Probe Serial Number 212.

## **References**

SSI-TP-018-ALSAS Dipole Calibration Procedure  
SSI-TP-016 Tissue Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

## **Conditions**

Dipole 210-00710 was new taken from stock.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 20 °C +/- 0.5°C

This page has been reviewed for content and attested to by signature within this document.

4

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Dipole Calibration Results****Mechanical Verification**

APREL Length	APREL Height	Measured Length	Measured Height
68.0 mm	39.5 mm	67.1mm	38.9 mm

**Tissue Validation**

Head Tissue 1900 MHz	Measured
Dielectric constant, $\epsilon_r$	40.03
Conductivity, $\sigma$ [S/m]	1.38

This page has been reviewed for content and attested to by signature within this document.

5



**NCL Calibration Laboratories**


Division of APREL Laboratories.

**Electrical Calibration**

Test	Result
S11 R/L	-30.831 dB
SWR	1.059 U
Impedance	50.914 Ω

The Following Graphs are the results as displayed on the Vector Network Analyzer.

**S11 Parameter Return Loss**

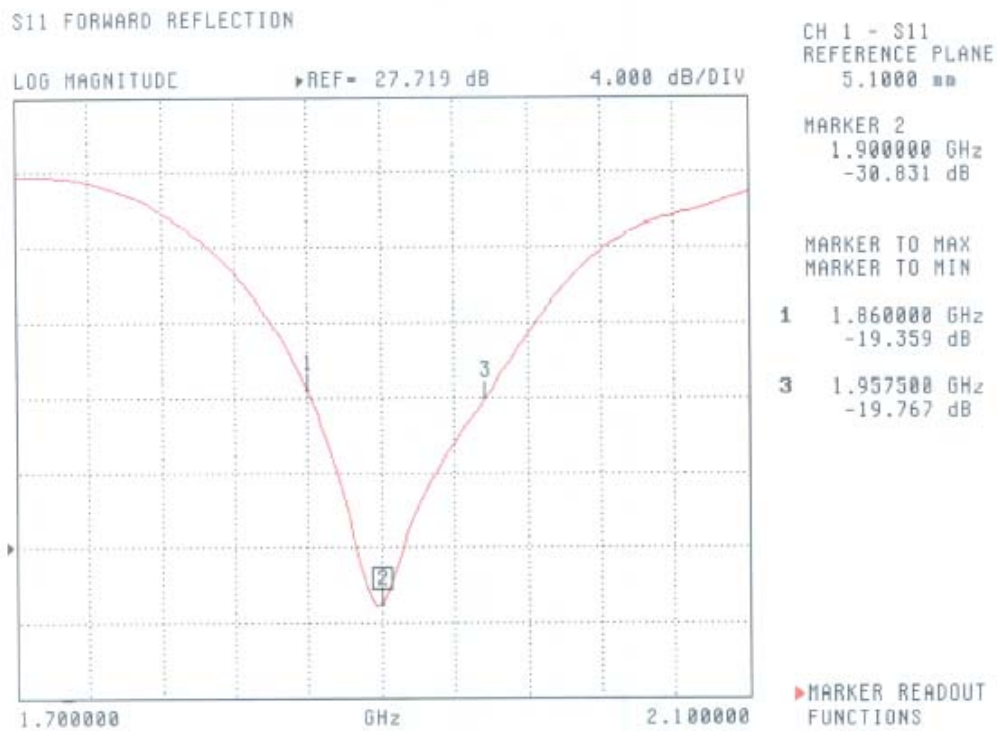

This page has been reviewed for content and attested to by signature within this document.


**NCL Calibration Laboratories**

Division of APREL Laboratories.

**SWR**

S11 FORWARD REFLECTION

SWR REF=449.865  $\mu$ U 900.000  $\mu$ U/DIV

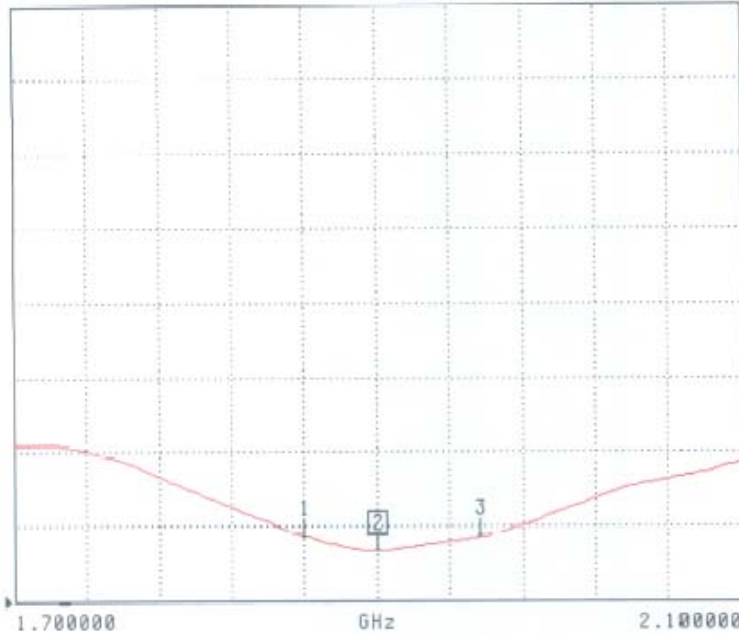

CH 1 - S11  
REFERENCE PLANE  
5.1000 mm

MARKER 2  
1.900000 GHz  
1.059 U

MARKER TO MAX  
MARKER TO MIN

**1** 1.860000 GHz  
1.241 U

**3** 1.957500 GHz  
1.229 U

▶ MARKER READOUT  
FUNCTIONS


This page has been reviewed for content and attested to by signature within this document.

7

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**Smith Chart Dipole Impedance**

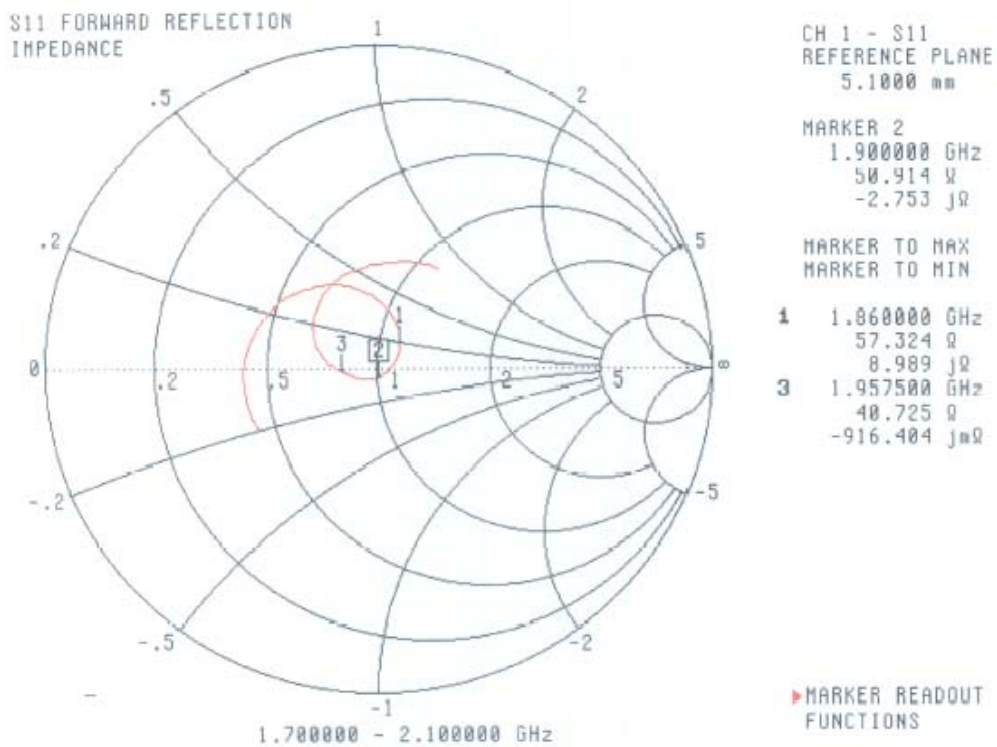


This page has been reviewed for content and attested to by signature within this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

**System Validation Results Using the Electrically Calibrated Dipole**

Head Tissue Frequency	1 Gram	10 Gram	Peak Above Feed Point
1900 MHz	38.7	20.5	69.7

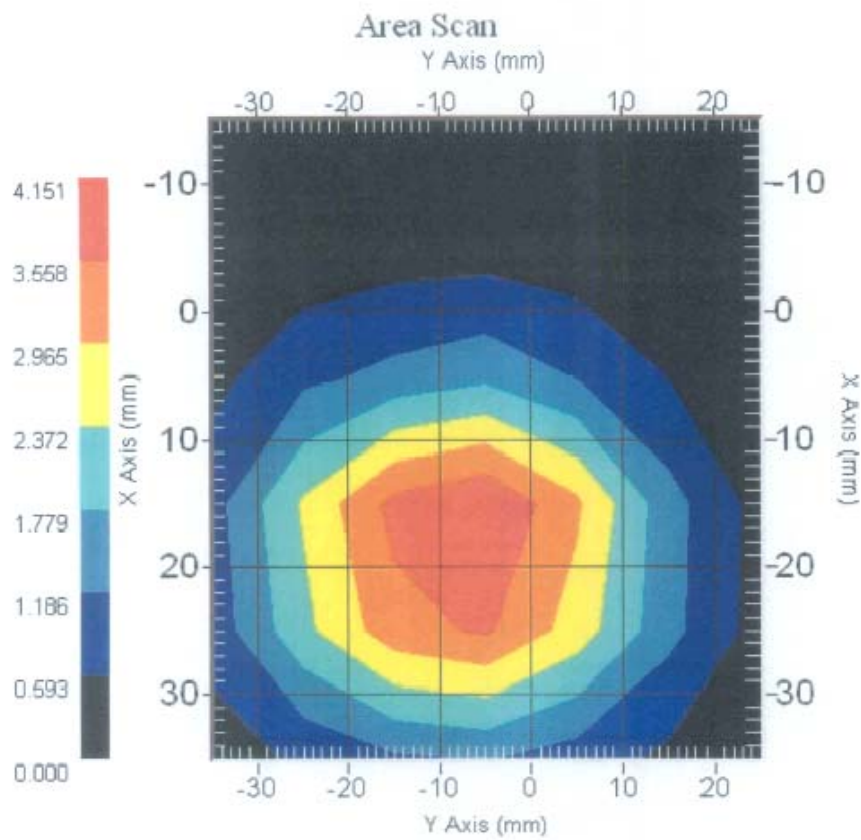

This page has been reviewed for content and attested to by signature within this document.

**NCL Calibration Laboratories**

Division of APREL Laboratories.

---

**Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List 2007.

This page has been reviewed for content and attested to by signature within this document.

10

---

**APPENDIX D – SAR SYSTEM VALIDATION DATA**

---

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****System Performance Check 835 MHz Head Liquid****Dipole 835 MHz; Type: ALS-D-835-S-2; S/N: 180-00558****Product Data**

Device Name : Dipole 835 MHz  
Serial No. : 180-00558  
Type : Dipole  
Model : ALS-D-835-S-2  
Frequency : 835.00 MHz  
Max. Transmit Power : 1 W  
Drift Time : 3 min(s)  
Power Drift-Start : 10.066 W/kg  
Power Drift-Finish : 9.926 W/kg  
Power Drift (%) : -1.391

**Phantom Data**

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Default  
Phantom Data

**Tissue Data**

Type : HEAD  
Serial No. : 270-01002  
Frequency : 835.00 MHz  
Last Calib. Date : 15-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 20.00 °C  
Humidity : 50.00 RH%  
Epsilon : 41.50 F/m  
Sigma : 0.90 S/m  
Density : 1000.00 kg/cu. m


**Probe Data**

Name : E-Field  
Model : E-020  
Type : E-Field Triangle  
Serial No. : 273  
Last Calib. Date : 08-Jan-2008  
Frequency : 835.00 MHz  
Duty Cycle Factor : 1  
Conversion Factor : 6.5  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 21.00 °C  
Ambient Temp. : 21.00 °C  
Area Scan : 7x9x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

1 gram SAR value : 9.651 W/kg  
10 gram SAR value : 6.042 W/kg  
Area Scan Peak SAR : 10.936 W/kg  
Zoom Scan Peak SAR : 15.013 W/kg

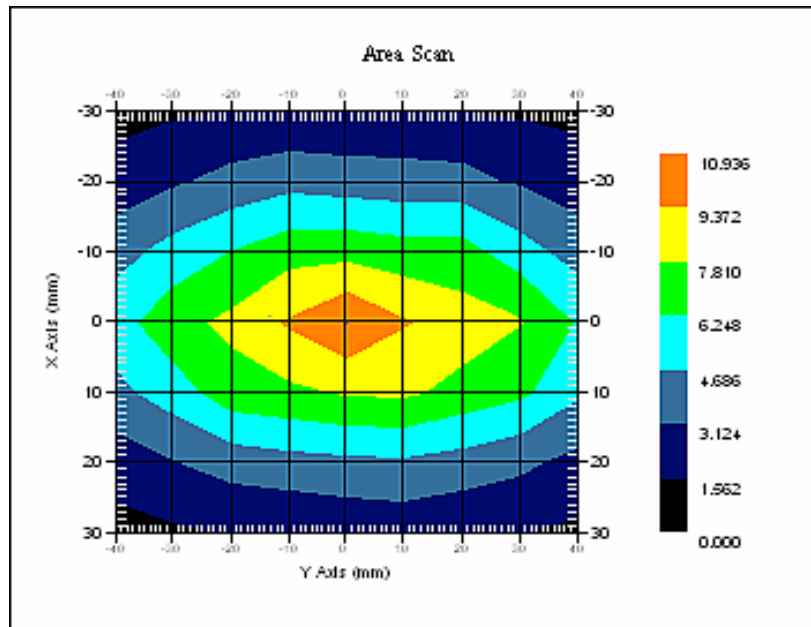

### 835 MHz System Validation

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****System Performance Check 1900 MHz Head Liquid****Dipole 1900 MHz; Type: ALS-D-1900-S-2; S/N: 210-00710**

## Product Data

Device Name : Dipole 1900MHz  
Serial No. : 210-00710  
Type : Dipole  
Model : ALS-D-1900-S-2  
Frequency : 1900.00 MHz  
Max. Transmit Power : 1 W  
Drift Time : 3 min(s)  
Power Drift-Start : 43.370 W/kg  
Power Drift-Finish : 41.609 W/kg  
Power Drift (%) : -4.059

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Default

## Tissue Data

Type : HEAD  
Serial No. : 295-01103  
Frequency : 1900.00 MHz  
Last Calib. Date : 16-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 20.00 °C  
Humidity : 56.00 RH%  
Epsilon : 40.00 F/m  
Sigma : 1.40 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : E-Field  
Model : E-020  
Type : E-Field Triangle  
Serial No. : 273  
Last Calib. Date : 01-Aug-2008  
Frequency : 1900.00 MHz  
Duty Cycle Factor : 1  
Conversion Factor : 5.25  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

## Measurement Data

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 20.00 °C  
Ambient Temp. : 20.00 °C  
Area Scan : 7x9x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm



1 gram SAR value : 40.328 W/kg  
 10 gram SAR value : 20.137 W/kg  
 Area Scan Peak SAR : 44.786 W/kg  
 Zoom Scan Peak SAR : 75.567 W/kg

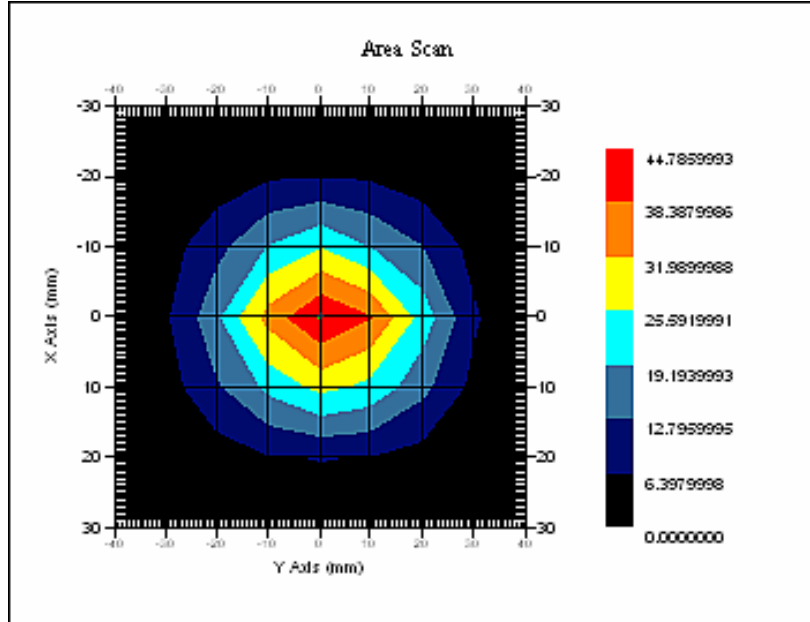

**1900 MHz System Validation**

## APPENDIX E – EUT SCAN RESULTS

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)**

**Body- worn Back Touching the Flat Phantom (835 MHz Middle Channel)**

### Measurement Data

Test mode :GPRS  
 Crest Factor : 8  
 Scan Type : Complete  
 Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

### Tissue Data


Type : BODY  
 Frequency : 835.00 MHz  
 Epsilon : 55.20 F/m  
 Sigma : 0.97 S/m  
 Density : 1000.00 kg/cu. m

### Probe Data

Serial No. : 273  
 Frequency : 835.00 MHz  
 Duty Cycle Factor : 8  
 Conversion Factor : 6.7  
 Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
 Compression Point : 95.00 mV  
 Offset : 1.56 mm

1 gram SAR value : 0.263 W/kg  
 10 gram SAR value : 0.186 W/kg  
 Area Scan Peak SAR : 0.283 W/kg  
 Zoom Scan Peak SAR : 0.570 W/kg

**Plot 1#**

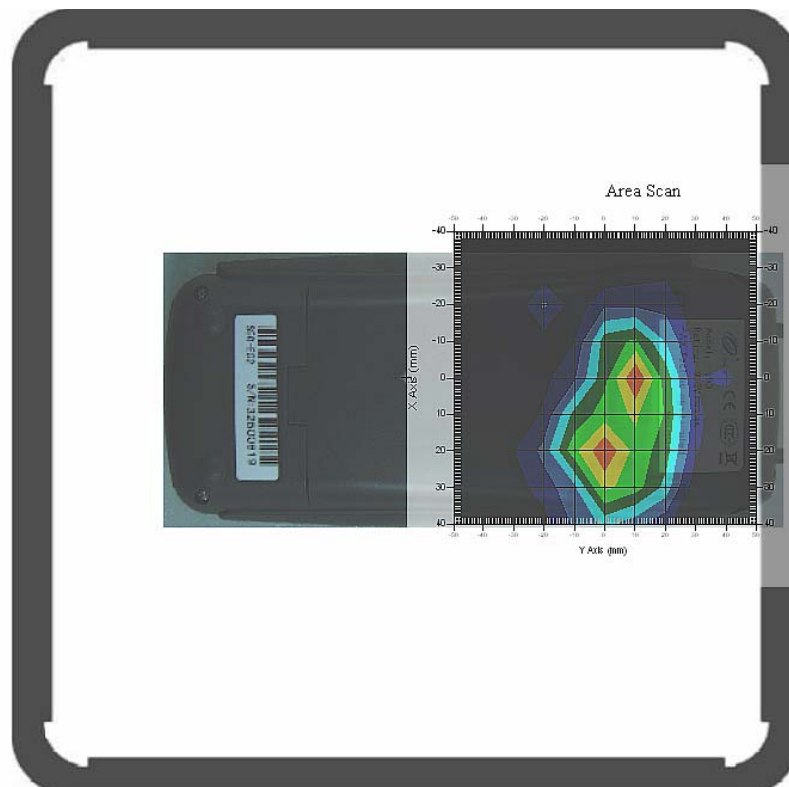

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****Body- worn Back Touching the Flat Phantom (835 MHz Low Channel)**

## Measurement Data

Test mode :GPRS  
Crest Factor : 8  
Scan Type : Complete  
Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


## Tissue Data

Type : BODY  
Frequency : 835.00 MHz  
Epsilon : 55.20 F/m  
Sigma : 0.97 S/m  
Density : 1000.00 kg/cu. m

## Probe Data

Serial No. : 273  
Frequency : 835.00 MHz  
Duty Cycle Factor : 8  
Conversion Factor : 6.7  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

1 gram SAR value : 0.352 W/kg  
10 gram SAR value : 0.265 W/kg  
Area Scan Peak SAR : 0.480 W/kg  
Zoom Scan Peak SAR : 0.560 W/kg

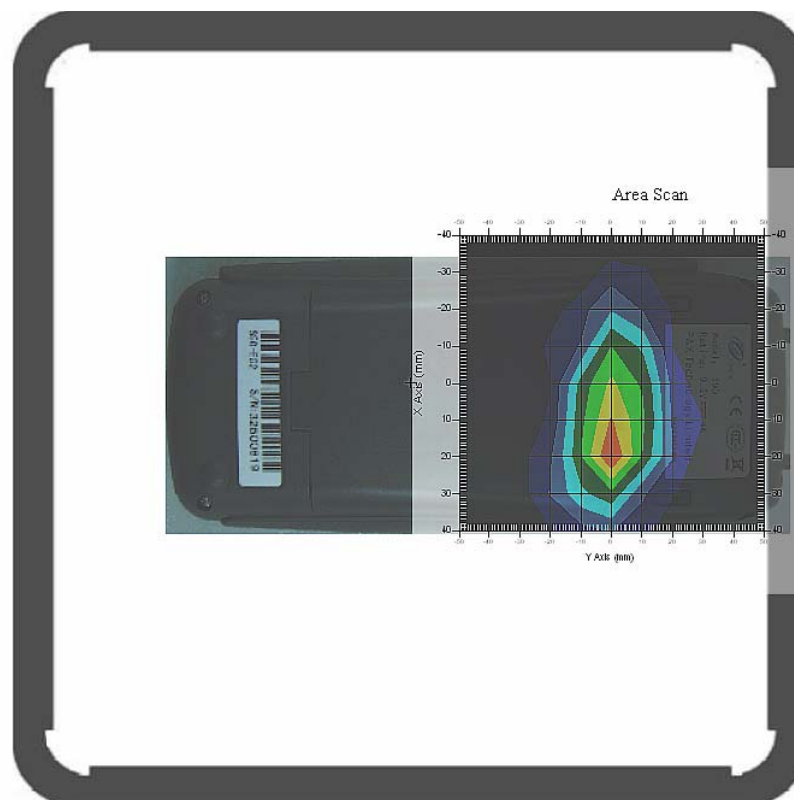**Plot 2#**

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****Body- worn Back Touching the Flat Phantom (835 MHz High Channel)**

## Measurement Data

Test mode :GPRS  
Crest Factor : 8  
Scan Type : Complete  
Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


## Tissue Data

Type : BODY  
Frequency : 835.00 MHz  
Epsilon : 55.20 F/m  
Sigma : 0.97 S/m  
Density : 1000.00 kg/cu. m

## Probe Data

Serial No. : 273  
Frequency : 835.00 MHz  
Duty Cycle Factor : 8  
Conversion Factor : 6.7  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

1 gram SAR value : 0.370 W/kg  
10 gram SAR value : 0.272 W/kg  
Area Scan Peak SAR : 0.488 W/kg  
Zoom Scan Peak SAR : 0.930 W/kg

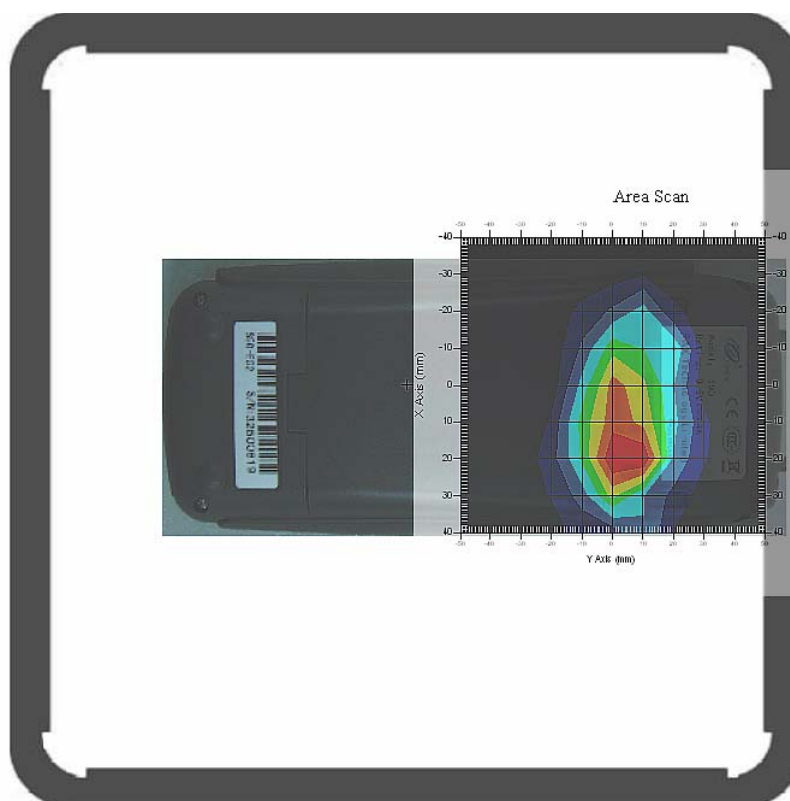**Plot 3#**

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****Body- worn Back (835 MHz Middle Channel)**

## Measurement Data

Test mode : GSM  
Crest Factor : 8  
Scan Type : Complete  
Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


## Tissue Data

Type : BODY  
Frequency : 835.00 MHz  
Epsilon : 55.20 F/m  
Sigma : 0.97 S/m  
Density : 1000.00 kg/cu. m

## Probe Data

Serial No. : 273  
Frequency : 835.00 MHz  
Duty Cycle Factor : 8  
Conversion Factor : 6.7  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

1 gram SAR value : 0.366 W/kg  
10 gram SAR value : 0.244 W/kg  
Area Scan Peak SAR : 0.465 W/kg  
Zoom Scan Peak SAR : 0.750 W/kg

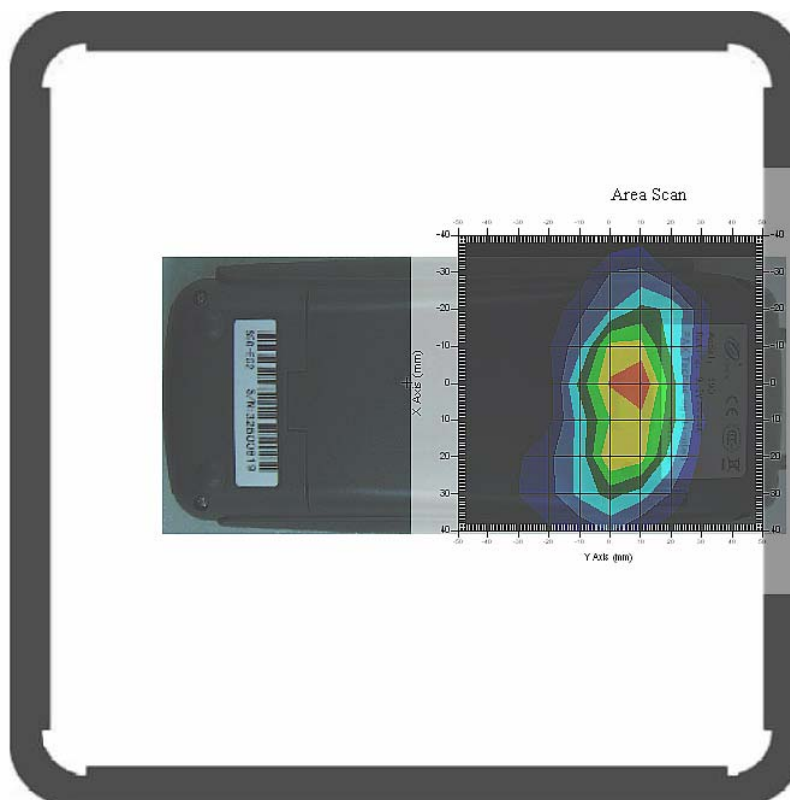**Plot 4#**

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****Body- worn Back Touching the Flat Phantom (835 MHz Low Channel)**

## Measurement Data

Test mode : GSM  
Crest Factor : 8  
Scan Type : Complete  
Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


## Tissue Data

Type : BODY  
Frequency : 835.00 MHz  
Epsilon : 55.20 F/m  
Sigma : 0.97 S/m  
Density : 1000.00 kg/cu. m

## Probe Data

Serial No. : 273  
Frequency : 835.00 MHz  
Duty Cycle Factor : 8  
Conversion Factor : 6.7  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

1 gram SAR value : 0.346 W/kg  
10 gram SAR value : 0.283 W/kg  
Area Scan Peak SAR : 0.542 W/kg  
Zoom Scan Peak SAR : 0.861 W/kg

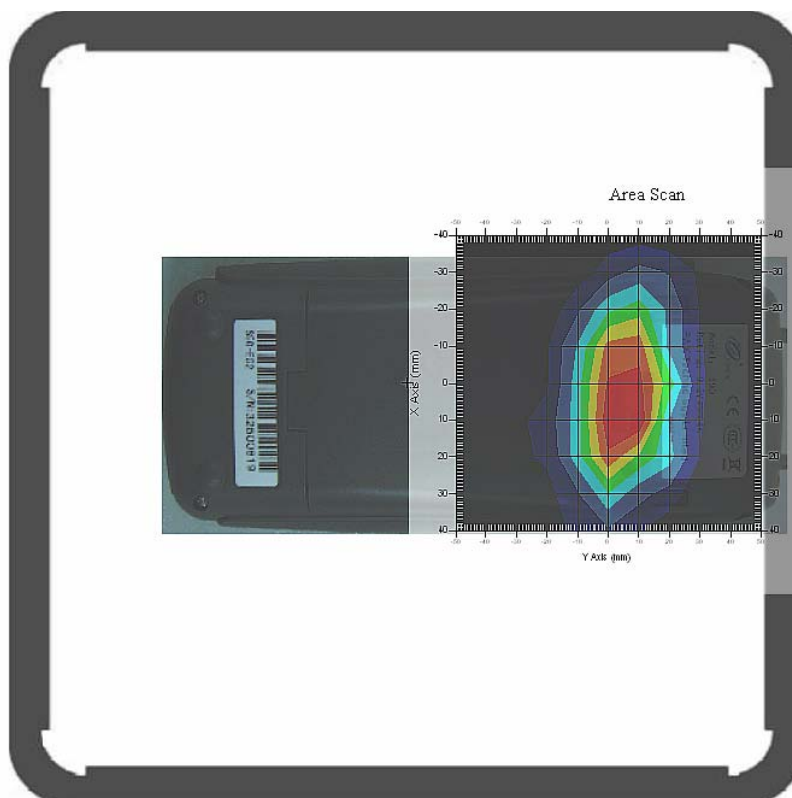**Plot 5#**

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****Body- worn Back Touching the Flat Phantom (835 MHz High Channel)**

## Measurement Data

Test mode : GSM  
Crest Factor : 8  
Scan Type : Complete  
Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


## Tissue Data

Type : BODY  
Frequency : 835.00 MHz  
Epsilon : 55.20 F/m  
Sigma : 0.97 S/m  
Density : 1000.00 kg/cu. m

## Probe Data

Serial No. : 273  
Frequency : 835.00 MHz  
Duty Cycle Factor : 8  
Conversion Factor : 6.7  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

1 gram SAR value : 0.384 W/kg  
10 gram SAR value : 0.295 W/kg  
Area Scan Peak SAR : 0.614 W/kg  
Zoom Scan Peak SAR : 0.890 W/kg

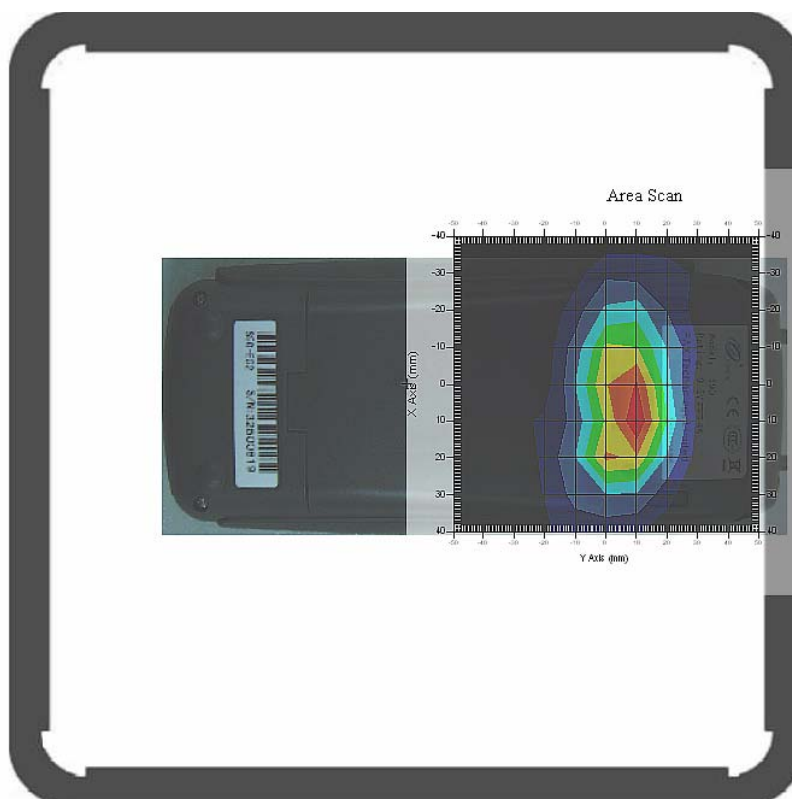**Plot 6#**

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****Body- worn Back Touching the Flat Phantom (1900 MHz Middle Channel)**

## Measurement Data

Test mode :GPRS  
Crest Factor : 8  
Scan Type : Complete  
Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


## Tissue Data

Type : BODY  
Frequency : 1900.00 MHz  
Epsilon : 53.30 F/m  
Sigma : 1.52 S/m  
Density : 1000.00 kg/cu. m

## Probe Data

Serial No. : 273  
Frequency : 1900.00 MHz  
Duty Cycle Factor : 8  
Conversion Factor : 5.15  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

1 gram SAR value : 0.345 W/kg  
10 gram SAR value : 0.171 W/kg  
Area Scan Peak SAR : 0.395 W/kg  
Zoom Scan Peak SAR : 0.810 W/kg

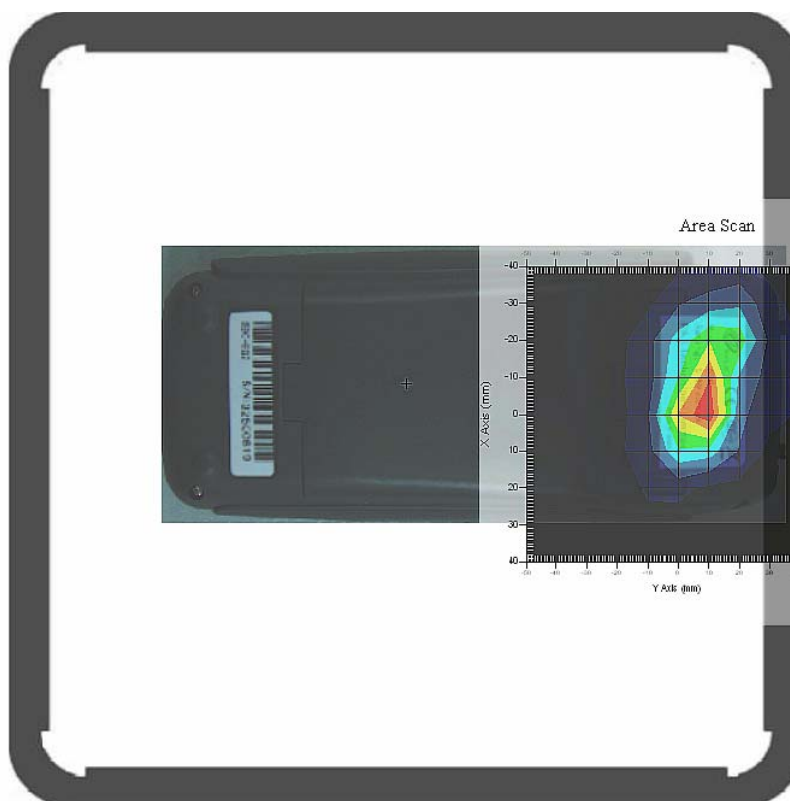**Plot 7#**



**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****Body- worn Back Touching the Flat Phantom (1900 MHz Low Channel)**

## Measurement Data

Test mode :GPRS  
Crest Factor : 8  
Scan Type : Complete  
Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


## Tissue Data

Type : BODY  
Frequency : 1900.00 MHz  
Epsilon : 53.30 F/m  
Sigma : 1.52 S/m  
Density : 1000.00 kg/cu. m

## Probe Data

Serial No. : 273  
Frequency : 1900.00 MHz  
Duty Cycle Factor : 8  
Conversion Factor : 5.15  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

1 gram SAR value : 0.204 W/kg  
10 gram SAR value : 0.155 W/kg  
Area Scan Peak SAR : 0.322 W/kg  
Zoom Scan Peak SAR : 0.670 W/kg

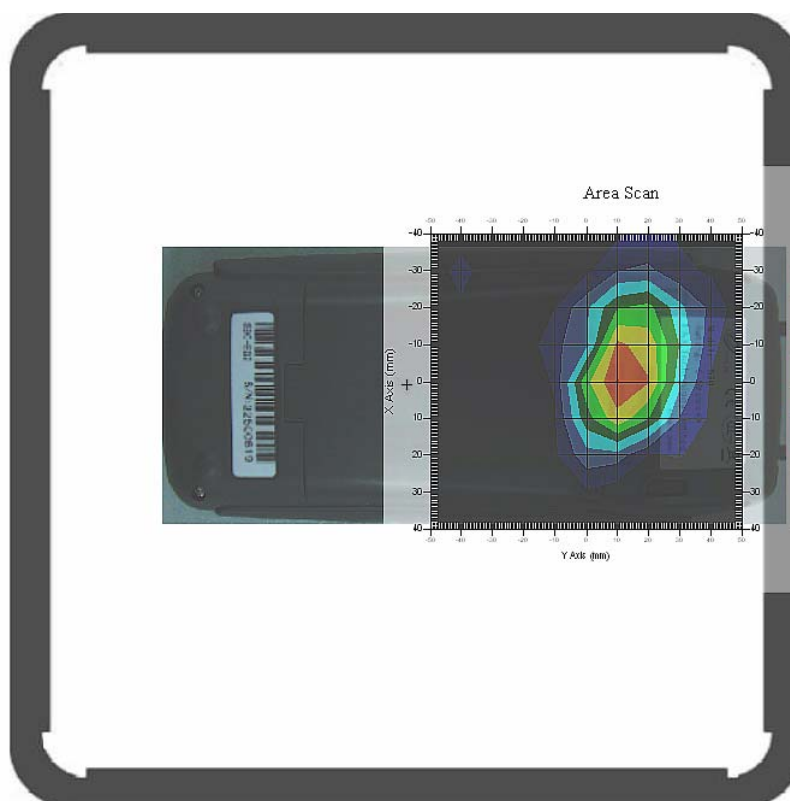**Plot 8#**

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****Body- worn Back Touching the Flat Phantom (1900 MHz High Channel)**

## Measurement Data

Test mode : GPRS  
Crest Factor : 8  
Scan Type : Complete  
Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


## Tissue Data

Type : BODY  
Frequency : 1900.00 MHz  
Epsilon : 53.30 F/m  
Sigma : 1.52 S/m  
Density : 1000.00 kg/cu. m

## Probe Data

Serial No. : 273  
Frequency : 1900.00 MHz  
Duty Cycle Factor : 8  
Conversion Factor : 5.15  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

1 gram SAR value : 0.301 W/kg  
10 gram SAR value : 0.175 W/kg  
Area Scan Peak SAR : 0.349 W/kg  
Zoom Scan Peak SAR : 0.765 W/kg

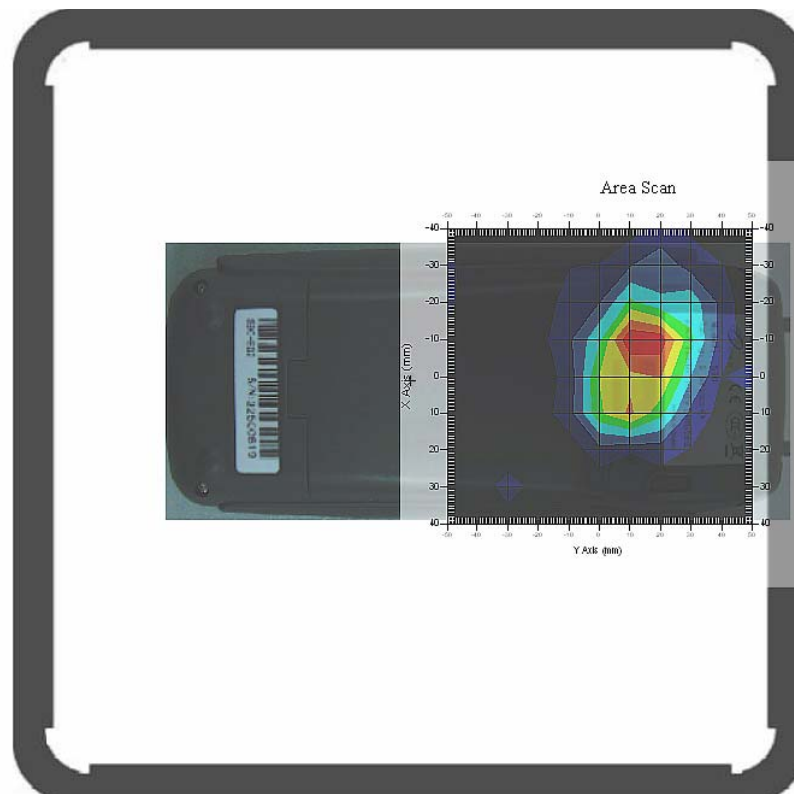**Plot 9#**

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****Body- worn Back Touching the Flat Phantom (1900 MHz Middle Channel)**

## Measurement Data

Test mode : GSM  
Crest Factor : 8  
Scan Type : Complete  
Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


## Tissue Data

Type : BODY  
Frequency : 1900.00 MHz  
Epsilon : 53.30 F/m  
Sigma : 1.52 S/m  
Density : 1000.00 kg/cu. m

## Probe Data

Serial No. : 273  
Frequency : 1900.00 MHz  
Duty Cycle Factor : 8  
Conversion Factor : 5.15  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

1 gram SAR value : 0.322 W/kg  
10 gram SAR value : 0.180 W/kg  
Area Scan Peak SAR : 0.430 W/kg  
Zoom Scan Peak SAR : 0.670 W/kg

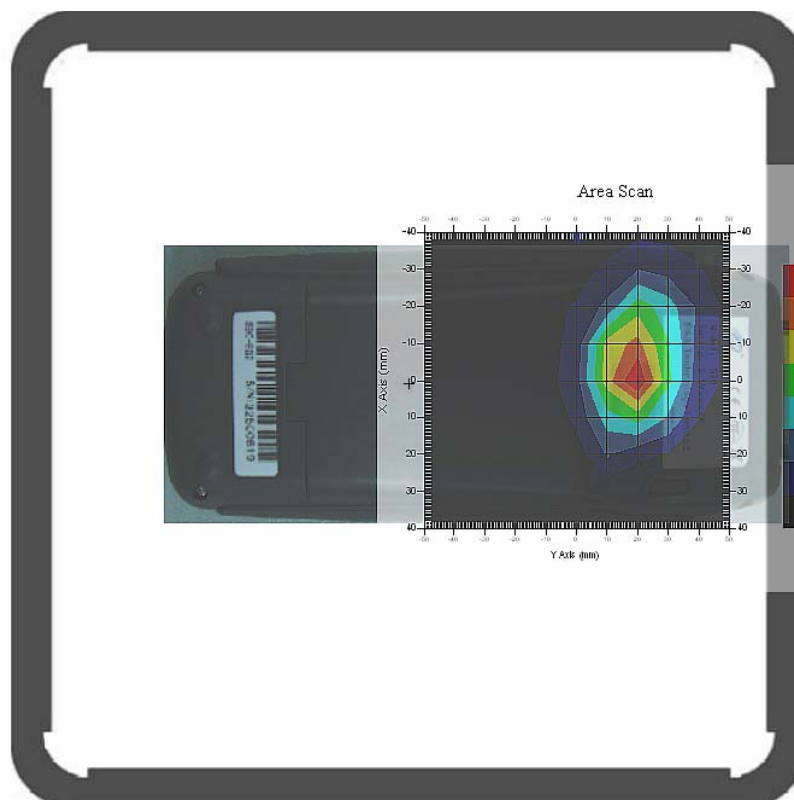**Plot 10#**

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****Body- worn Back Touching the Flat Phantom (1900 MHz Low Channel)**

## Measurement Data

Test mode : GSM  
Crest Factor : 8  
Scan Type : Complete  
Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


## Tissue Data

Type : BODY  
Frequency : 1900.00 MHz  
Epsilon : 53.30 F/m  
Sigma : 1.52 S/m  
Density : 1000.00 kg/cu. m

## Probe Data

Serial No. : 273  
Frequency : 1900.00 MHz  
Duty Cycle Factor : 8  
Conversion Factor : 5.15  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

1 gram SAR value : 0.188 W/kg  
10 gram SAR value : 0.097 W/kg  
Area Scan Peak SAR : 0.291 W/kg  
Zoom Scan Peak SAR : 0.440 W/kg

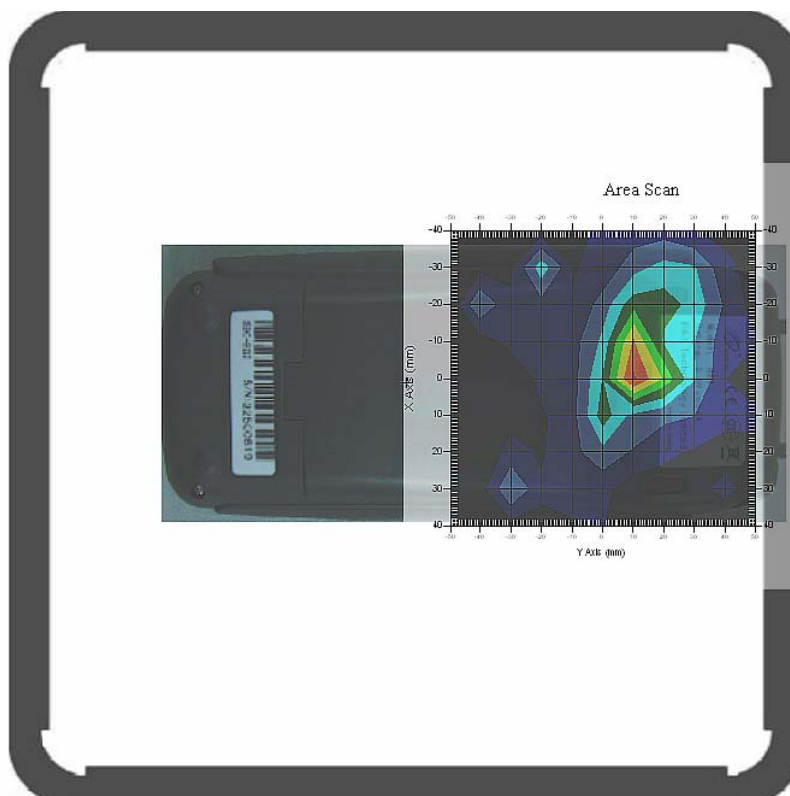**Plot 11#**

**Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)****Body- worn Back (1900 MHz High Channel)**

## Measurement Data

Test mode : GSM  
Crest Factor : 8  
Scan Type : Complete  
Area Scan : 9x11x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm


## Tissue Data

Type : BODY  
Frequency : 1900.00 MHz  
Epsilon : 53.30 F/m  
Sigma : 1.52 S/m  
Density : 1000.00 kg/cu. m

## Probe Data

Serial No. : 273  
Frequency : 1900.00 MHz  
Duty Cycle Factor : 8  
Conversion Factor : 5.15  
Probe Sensitivity : 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
Compression Point : 95.00 mV  
Offset : 1.56 mm

1 gram SAR value : 0.304 W/kg  
10 gram SAR value : 0.187 W/kg  
Area Scan Peak SAR : 0.327 W/kg  
Zoom Scan Peak SAR : 0.560 W/kg

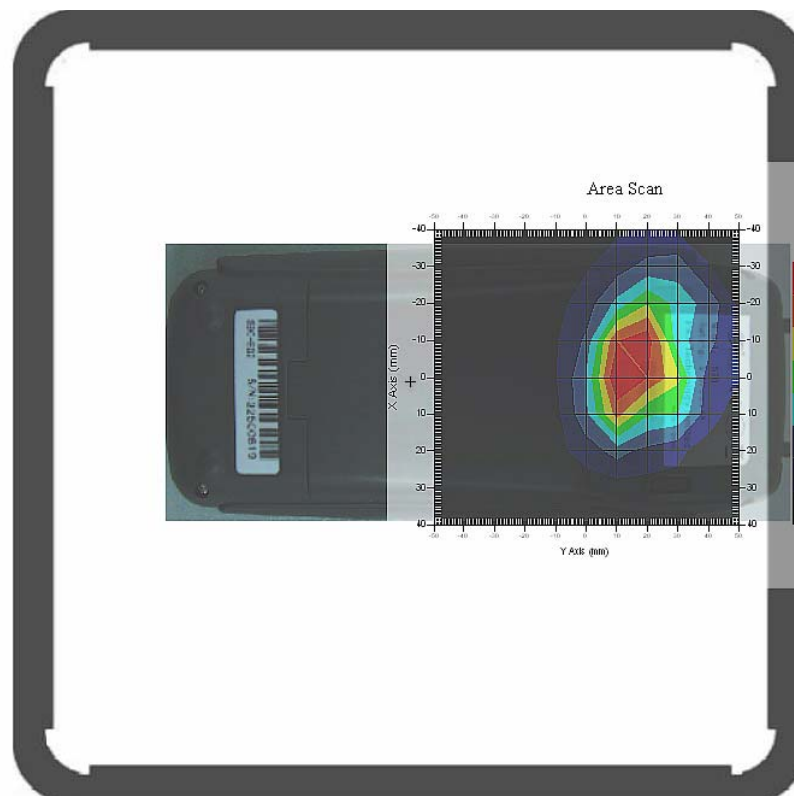**Plot 12#**


## APPENDIX F – CONDUCTED OUTPUT POWER MEASUREMENT

### Provision Applicable

The measured peak output power should be greater and within 5% than EMI measurement.

### Test Procedure

The RF output of the transmitter was connected to the input of the spectrum analyzer through sufficient attenuation.

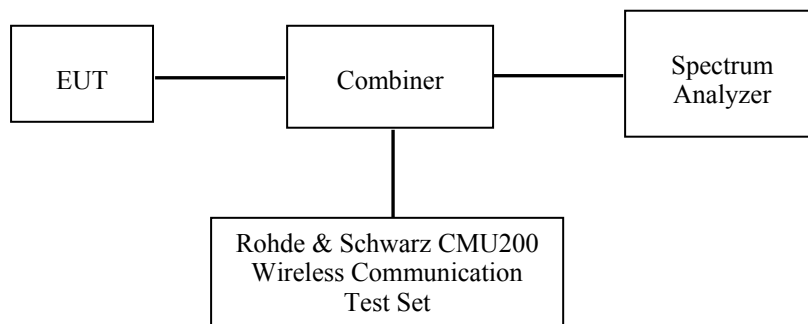

### Test Equipment List and Details

Manufacturer	Equipment Description	Model No.	Serial No.	Calibration Date
Rohde & Schwarz	Communication Tester	CMU200	1100.0008.02	2008-06-21
Rohde & Schwarz	Spectrum Analyzer	FSEM30	849720/019	2008-05-09

### Test Results

Band	Frequency (MHz)	Conducted Output Power			
		GPRS (dBm)	GSM (dBm)	GPRS (Watt)	GSM (Watt)
Cellular	824.2	32.36	32.45	1.722	1.758
	836.6	32.51	32.66	1.782	1.845
	848.8	32.62	32.52	1.828	1.786
PCS	1850.2	29.77	29.45	0.948	0.881
	1880.0	29.65	29.69	0.923	0.931
	1909.8	29.05	29.17	0.804	0.826

---

## APPENDIX G – EUT TEST POSITION PHOTOS

---

**Body-worn Setup Photo**  
(Back touching the flat phantom)



## APPENDIX H – EUT PHOTOS

**EUT - Top View**



**EUT - Bottom View**





**EUT- Battery off View**



## APPENDIX I - INFORMATIVE REFERENCES

---

- [1] Federal Communications Commission, \Report and order: Guidelines for evaluating the environmental effects of radiofrequency radiation", Tech. Rep. FCC 96-326, FCC, Washington, D.C. 20554, 1996.
- [2] David L. Means Kwok Chan, Robert F. Cleveland, \Evaluating compliance with FCC guidelines for human exposure to radiofrequency electromagnetic fields", Tech. Rep., Federal Communication Commission, Office of Engineering & Technology, Washington, DC, 1997.
- [3] Thomas Schmid, Oliver Egger, and Niels Kuster, \Automated E-field scanning system for dosimetric assessments", IEEE Transactions on Microwave Theory and Techniques, vol. 44, pp. 105-113, Jan. 1996.
- [4] Niels Kuster, Ralph Kastle, and Thomas Schmid, \Dosimetric evaluation of mobile communications equipment with known precision", IEEE Transactions on Communications, vol. E80-B, no. 5, pp. 645-652, May 1997.
- [5] CENELEC, \Considerations for evaluating of human exposure to electromagnetic fields (EMFs) from mobile telecommunication equipment (MTE) in the frequency range 30MHz - 6GHz", Tech. Rep., CENELEC, European Committee for Electrotechnical Standardization, Brussels, 1997.
- [6] ANSI, ANSI/IEEE C95.1-1992: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz, The Institute of Electrical and Electronics Engineers, Inc., New York, NY 10017, 1992.
- [7] Katja Pokovic, Thomas Schmid, and Niels Kuster, \Robust setup for precise calibration of E-field probes in tissue simulating liquids at mobile communications frequencies", in ICECOM '97, Dubrovnik, October 15-17, 1997, pp. 120-24.
- [8] Katja Pokovic, Thomas Schmid, and Niels Kuster, \E-field probe with improved isotropy in brain simulating liquids", in Proceedings of the ELMAR, Zadar, Croatia, 23-25 June, 1996, pp. 172-175.
- [9] Volker Hombach, Klaus Meier, Michael Burkhardt, Eberhard Kuhn, and Niels Kuster, \The dependence of EM energy absorption upon human head modeling at 900 MHz", IEEE Transactions on Microwave Theory and Techniques, vol. 44, no. 10, pp. 1865-1873, Oct. 1996.
- [10] Klaus Meier, Ralf Kastle, Volker Hombach, Roger Tay, and Niels Kuster, \The dependence of EM energy absorption upon human head modeling at 1800 MHz", IEEE Transactions on Microwave Theory and Techniques, Oct. 1997, in press.
- [11] W. Gander, Computermathematik, Birkhaeuser, Basel, 1992.
- [12] W. H. Press, S. A. Teukolsky, W. T. Vetterling, and B. P. Flannery, Numerical Recipes in C, The Art of Scientific Computing, Second Edition, Cambridge University Press, 1992. Dosimetric Evaluation of Sample device, month 1998 9
- [13] NIS81 NAMAS, \The treatment of uncertainty in EMC measurement", Tech. Rep., NAMAS Executive, National Physical Laboratory, Teddington, Middlesex, England, 1994.
- [14] Barry N. Taylor and Christ E. Kuyatt, \Guidelines for evaluating and expressing the uncertainty of NIST measurement results", Tech. Rep., National Institute of Standards and Technology, 1994. Dosimetric Evaluation of Sample device, month 1998 10.

\*\*\*\*\* END OF REPORT \*\*\*\*\*