



Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

Exhibit 12 Appendix C: HAC RF Data Plot

CELL – BC0

CDMA 835 BC-0 Channel 1013

Date: 07/23/2012

Communication System: CDMA_Tri_BC0&10, Frequency: 824.7 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2282 Probe: H3DV6 - SN6123, ConvF(1, 1, 1), Calibrated: 2/17/2012

Sensor-Surface: (Fix Surface),

Electronics: DAE4 Sn675, Calibrated: 5/23/2012

Measurement SW: DASY4, V4.7 Build 80

Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 °C ± 1 deg C, Liquid T = 22.0 °C ± 1 deg C

CELL_1013/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 70.5 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 87.0 V/m; Power Drift = 0.048 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
67.3 M4	71.8 M4	69.7 M4
Grid 4	Grid 5	Grid 6
64.9 M4	70.5 M4	68.8 M4
Grid 7	Grid 8	Grid 9
60.0 M4	65.0 M4	63.1 M4

CELL_1013/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.143 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.102 A/m; Power Drift = 0.036 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.181 M4	0.143 M4	0.092 M4
Grid 4	Grid 5	Grid 6
0.161 M4	0.122 M4	0.086 M4
Grid 7	Grid 8	Grid 9
0.164 M4	0.123 M4	0.086 M4



Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

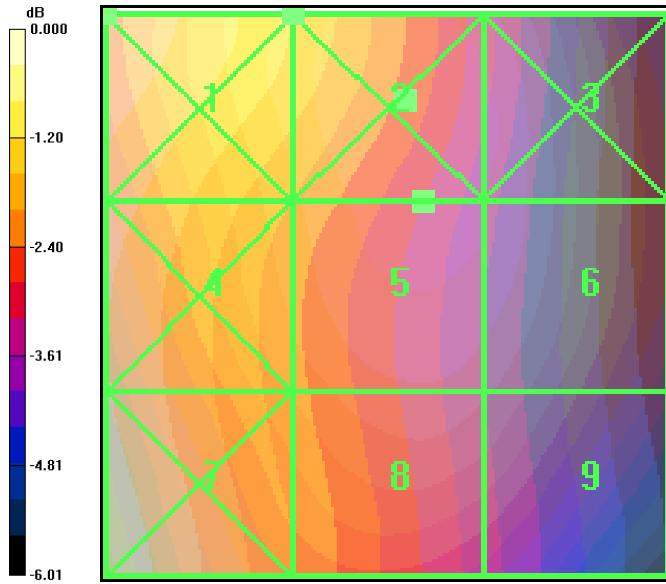

0 dB = 71.8V/m

CDMA 835 BC-0 Channel 384

Date: 07/23/2012

Communication System: CDMA_Tri_BC0&10, Frequency: 836.52 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2282 Probe: H3DV6 - SN6123, ConvF(1, 1, 1), Calibrated: 2/17/2012
 Sensor-Surface: (Fix Surface),
 Electronics: DAE4 Sn675, Calibrated: 5/23/2012
 Measurement SW: DASY4, V4.7 Build 80
 Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 °C ± 1 deg C, Liquid T = 22.0 °C ± 1 deg C

CELL_384/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 67.1 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 83.0 V/m; Power Drift = 0.101 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 58.7 M4	Grid 2 67.5 M4	Grid 3 66.7 M4
Grid 4 59.2 M4	Grid 5 67.1 M4	Grid 6 66.7 M4
Grid 7 58.4 M4	Grid 8 64.7 M4	Grid 9 64.5 M4

CELL_384/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.142 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.096 A/m; Power Drift = -0.165 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.176 M4	Grid 2 0.142 M4	Grid 3 0.089 M4
Grid 4 0.151 M4	Grid 5 0.114 M4	Grid 6 0.076 M4
Grid 7 0.157 M4	Grid 8 0.117 M4	Grid 9 0.077 M4



Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

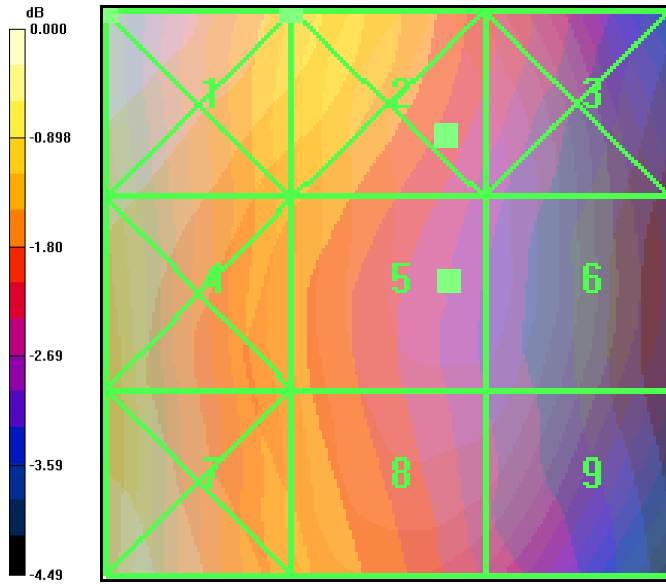

0 dB = 67.5V/m

CDMA 835 BC-0 Channel 777

Date: 07/23/2012

Communication System: CDMA_Tri_BC0&10, Frequency: 848.31 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2282 Probe: H3DV6 - SN6123, ConvF(1, 1, 1), Calibrated: 2/17/2012
 Sensor-Surface: (Fix Surface),
 Electronics: DAE4 Sn675, Calibrated: 5/23/2012
 Measurement SW: DASY4, V4.7 Build 80
 Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 °C ± 1 deg C, Liquid T = 22.0 °C ± 1 deg C

CELL_777/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 60.2 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 75.0 V/m; Power Drift = -0.145 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
55.2 M4	61.2 M4	59.7 M4
Grid 4	Grid 5	Grid 6
54.4 M4	60.2 M4	59.0 M4
Grid 7	Grid 8	Grid 9
51.6 M4	56.1 M4	55.2 M4

CELL_777/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.133 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.095 A/m; Power Drift = 0.011 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.156 M4	0.131 M4	0.083 M4
Grid 4	Grid 5	Grid 6
0.131 M4	0.108 M4	0.073 M4
Grid 7	Grid 8	Grid 9
0.133 M4	0.099 M4	0.069 M4




Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

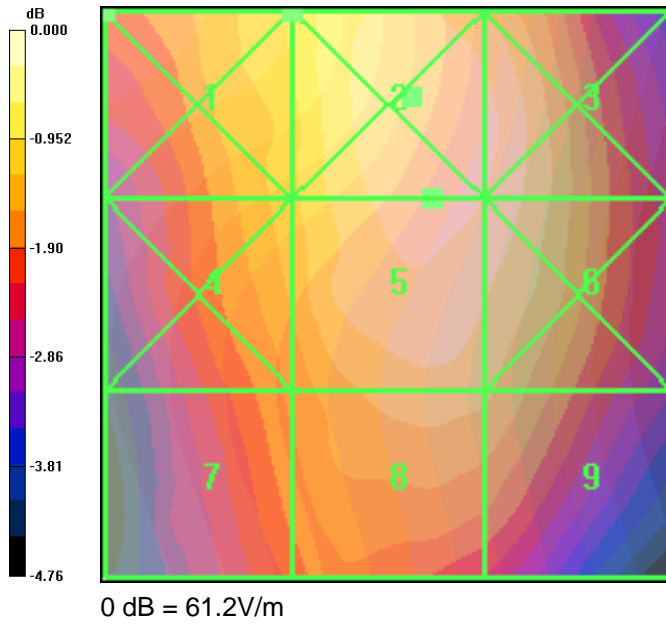



Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

CDMA 835 Channel 1013 (360) E roll

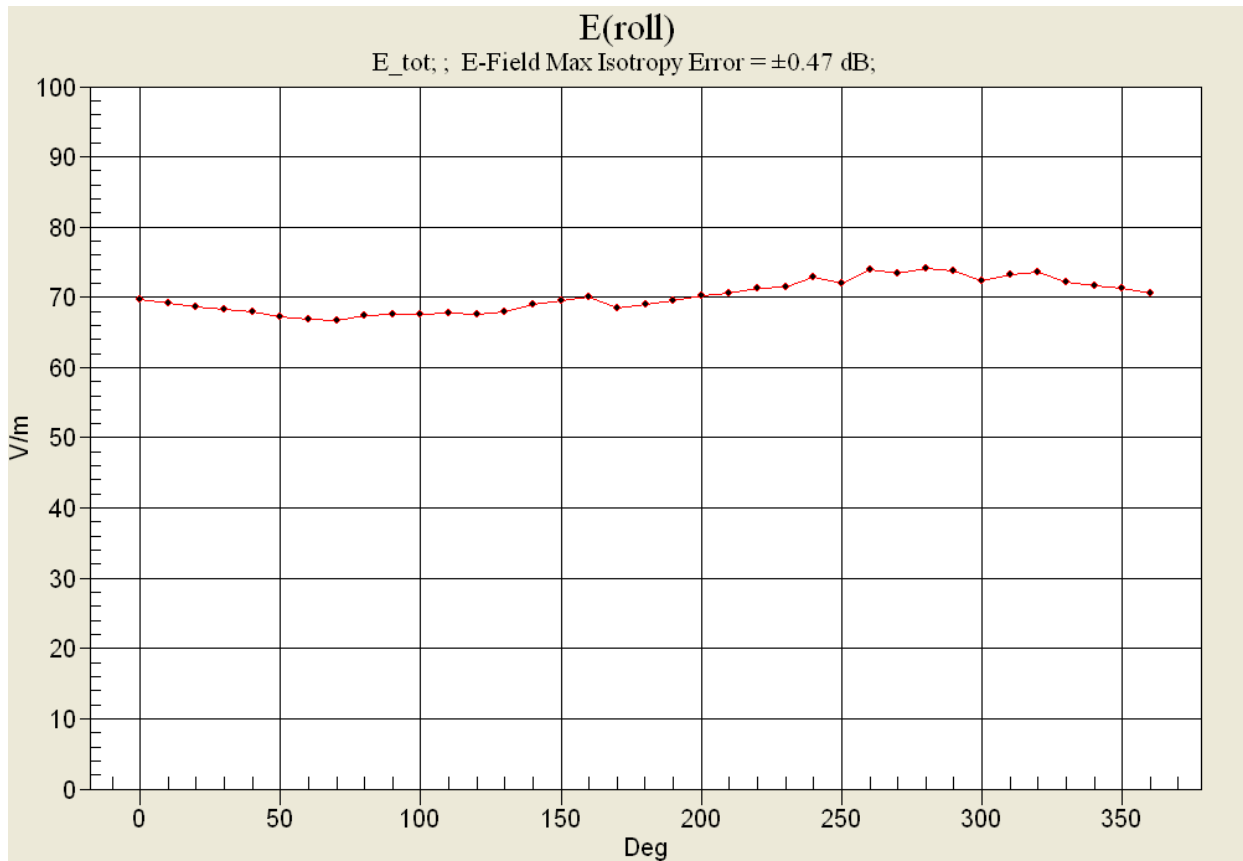

Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

AWS

CDMA 1700 Channel 25

Date: 07/23/2012

Communication System: CDMA_Tri_BC0&10, Frequency: 1711.25 MHz, Duty Cycle: 1:1

Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2282 Probe: H3DV6 - SN6123, ConvF(1, 1, 1), Calibrated: 2/17/2012

Sensor-Surface: (Fix Surface),

Electronics: DAE4 Sn527, Calibrated: 7/30/2012

Measurement SW: DASY4, V4.7 Build 80

Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 +/- 1 deg C, Liquid T = 22.0 +/- 1 deg C

AWS_25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 36.3 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 31.0 V/m; Power Drift = -0.191 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
40.7 M4	43.8 M4	41.5 M4
Grid 4	Grid 5	Grid 6
29.2 M4	34.4 M4	34.4 M4
Grid 7	Grid 8	Grid 9
36.3 M4	34.5 M4	30.1 M4

AWS_25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.106 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.125 A/m; Power Drift = -0.036 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.116 M4	0.100 M4	0.089 M4
Grid 4	Grid 5	Grid 6
0.102 M4	0.106 M4	0.097 M4
Grid 7	Grid 8	Grid 9
0.109 M4	0.105 M4	0.096 M4



Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

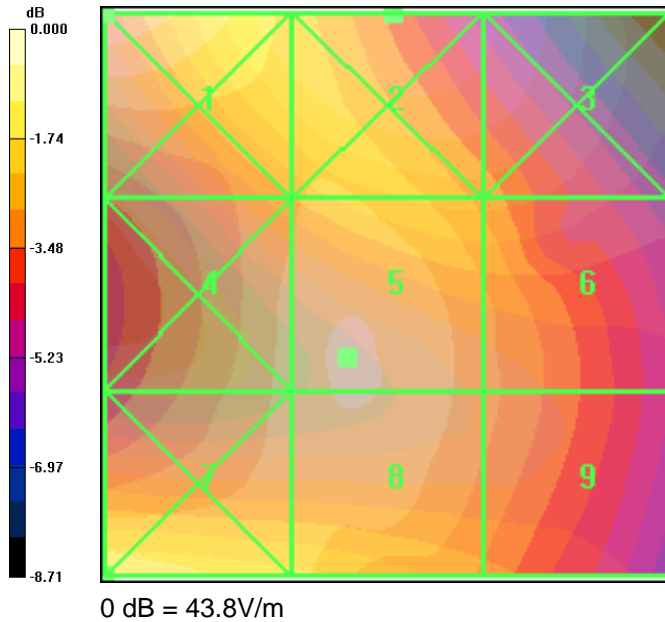

CDMA 1700 Channel 450

Date: 07/23/2012

Communication System: CDMA_Tri_BC0&10, Frequency: 1732.5 MHz, Duty Cycle: 1:1

Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2282 Probe: H3DV6 - SN6123, ConvF(1, 1, 1), Calibrated: 2/17/2012

Sensor-Surface: (Fix Surface),

Electronics: DAE4 Sn527, Calibrated: 7/30/2012

Measurement SW: DASY4, V4.7 Build 80

Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 +/- 1 deg C, Liquid T = 22.0 +/- 1 deg C

AWS_450/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 34.2 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 28.3 V/m; Power Drift = -0.007 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
38.9 M4	40.7 M4	38.8 M4
Grid 4	Grid 5	Grid 6
27.5 M4	30.6 M4	30.2 M4
Grid 7	Grid 8	Grid 9
34.2 M4	34.1 M4	29.1 M4

AWS_450/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.089 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.108 A/m; Power Drift = 0.030 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.097 M4	0.086 M4	0.080 M4
Grid 4	Grid 5	Grid 6
0.085 M4	0.089 M4	0.086 M4
Grid 7	Grid 8	Grid 9
0.088 M4	0.088 M4	0.086 M4



Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

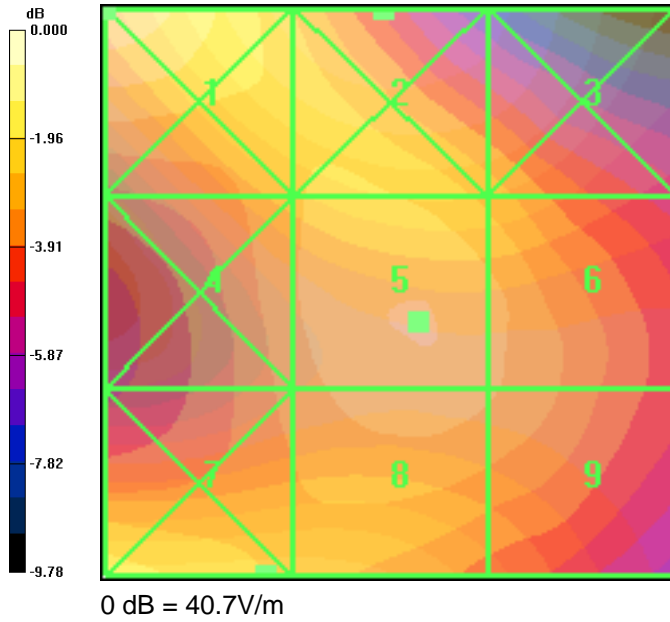

Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

CDMA 1700 Channel 875

Date: 07/23/2012

Communication System: CDMA_Tri_BC0&10, Frequency: 1753.75 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2282 Probe: H3DV6 - SN6123, ConvF(1, 1, 1), Calibrated: 2/17/2012

Sensor-Surface: (Fix Surface),

Electronics: DAE4 Sn527, Calibrated: 7/30/2012

Measurement SW: DASY4, V4.7 Build 80

Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 +/- 1 deg C, Liquid T = 22.0 +/- 1 deg C

AWS_875/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 29.6 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 25.9 V/m; Power Drift = -0.120 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 37.3 M4	Grid 2 38.3 M4	Grid 3 34.2 M4
Grid 4 26.9 M4	Grid 5 28.2 M4	Grid 6 26.3 M4
Grid 7 29.6 M4	Grid 8 29.6 M4	Grid 9 26.8 M4

AWS_875/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.090 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.110 A/m; Power Drift = -0.151 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.118 M4	Grid 2 0.089 M4	Grid 3 0.076 M4
Grid 4 0.086 M4	Grid 5 0.090 M4	Grid 6 0.085 M4
Grid 7 0.095 M4	Grid 8 0.089 M4	Grid 9 0.084 M4




Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

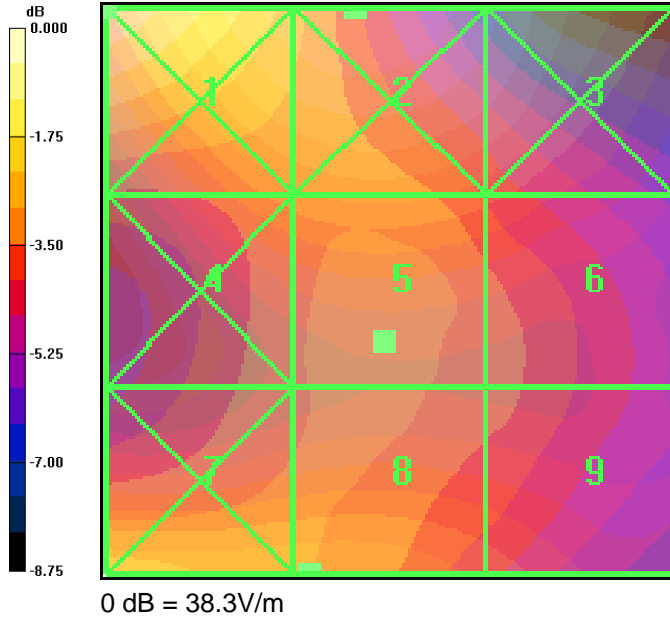



Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

CDMA 1700 Channel 25 (360) E roll

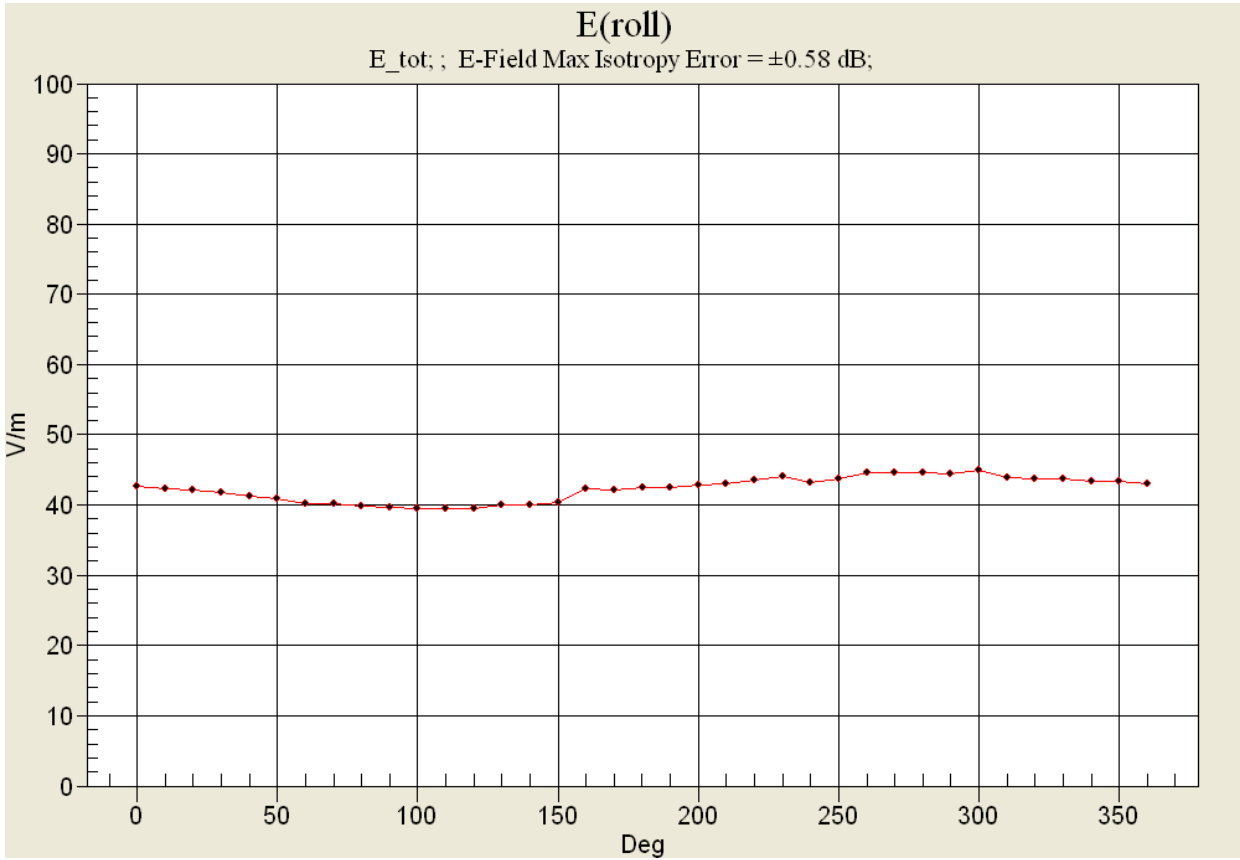

Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

PCS

CDMA 1900 Channel 25

Date: 07/23/2012

Communication System: CDMA_Tri_BC0&10, Frequency: 1850 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2282 Probe: H3DV6 - SN6123, ConvF(1, 1, 1), Calibrated: 2/17/2012

Sensor-Surface: (Fix Surface),

Electronics: DAE4 Sn675, Calibrated: 5/23/2012

Measurement SW: DASY4, V4.7 Build 80

Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 +/- 1 deg C, Liquid T = 22.0 +/- 1 deg C

PCS_25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 30.1 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 22.6 V/m; Power Drift = -0.142 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 35.0 M4	Grid 2 36.7 M4	Grid 3 34.0 M4
Grid 4 23.3 M4	Grid 5 25.1 M4	Grid 6 24.8 M4
Grid 7 28.9 M4	Grid 8 30.1 M4	Grid 9 29.2 M4

PCS_25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.099 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.123 A/m; Power Drift = -0.136 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.104 M4	Grid 2 0.095 M4	Grid 3 0.086 M4
Grid 4 0.096 M4	Grid 5 0.099 M4	Grid 6 0.092 M4
Grid 7 0.107 M4	Grid 8 0.099 M4	Grid 9 0.090 M4



Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

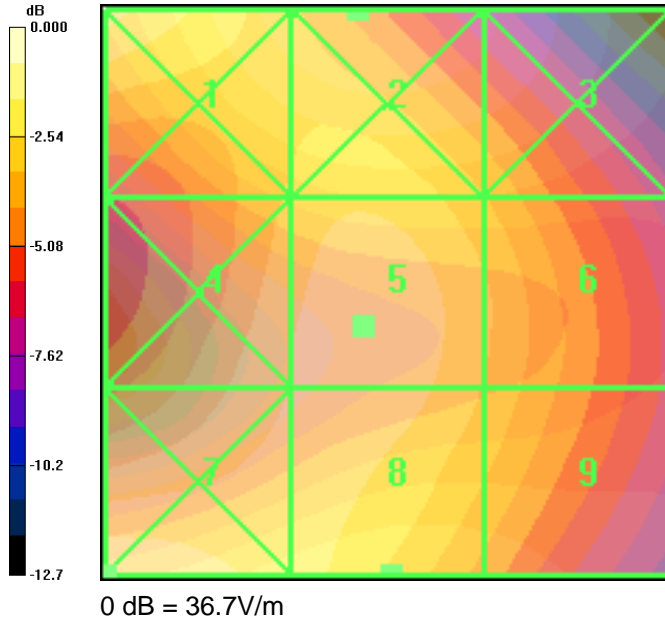

CDMA 1900 Channel 600

Date: 07/23/2012

Communication System: CDMA_Tri_BC0&10, Frequency: 1880 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2282 Probe: H3DV6 - SN6123, ConvF(1, 1, 1), Calibrated: 2/17/2012

Sensor-Surface: (Fix Surface),

Electronics: DAE4 Sn675, Calibrated: 5/23/2012

Measurement SW: DASY4, V4.7 Build 80

Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 +/- 1 deg C, Liquid T = 22.0 +/- 1 deg C

PCS_600/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 34.8 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 22.2 V/m; Power Drift = -0.020 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
35.1 M4	37.0 M4	34.2 M4
Grid 4	Grid 5	Grid 6
18.9 M4	21.2 M4	20.1 M4
Grid 7	Grid 8	Grid 9
33.1 M4	34.8 M4	32.2 M4

PCS_600/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.109 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.139 A/m; Power Drift = -0.115 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.098 M4	0.108 M4	0.103 M4
Grid 4	Grid 5	Grid 6
0.098 M4	0.109 M4	0.105 M4
Grid 7	Grid 8	Grid 9
0.103 M4	0.102 M4	0.099 M4



Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

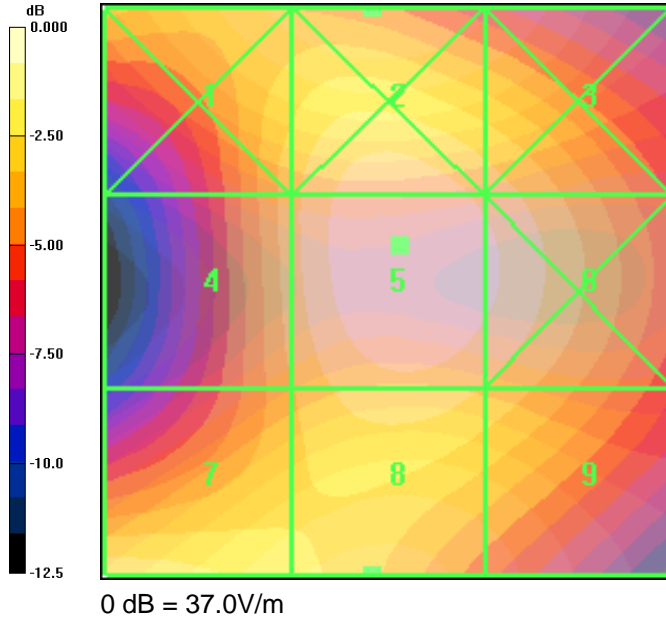

Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

CDMA 1900 Channel 1175

Date: 07/23/2012

Communication System: CDMA_Tri_BC0&10, Frequency: 1910 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2282 Probe: H3DV6 - SN6123, ConvF(1, 1, 1), Calibrated: 2/17/2012

Sensor-Surface: (Fix Surface),

Electronics: DAE4 Sn675, Calibrated: 5/23/2012

Measurement SW: DASY4, V4.7 Build 80

Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 +/- 1 deg C, Liquid T = 22.0 +/- 1 deg C

PCS_1175/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 20.5 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 16.7 V/m; Power Drift = 0.099 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
24.6 M4	26.9 M4	25.5 M4
Grid 4	Grid 5	Grid 6
15.5 M4	18.1 M4	18.0 M4
Grid 7	Grid 8	Grid 9
20.5 M4	20.5 M4	17.6 M4

PCS_1175/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.072 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.090 A/m; Power Drift = -0.126 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.073 M4	0.070 M4	0.064 M4
Grid 4	Grid 5	Grid 6
0.066 M4	0.072 M4	0.068 M4
Grid 7	Grid 8	Grid 9
0.066 M4	0.071 M4	0.067 M4



Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

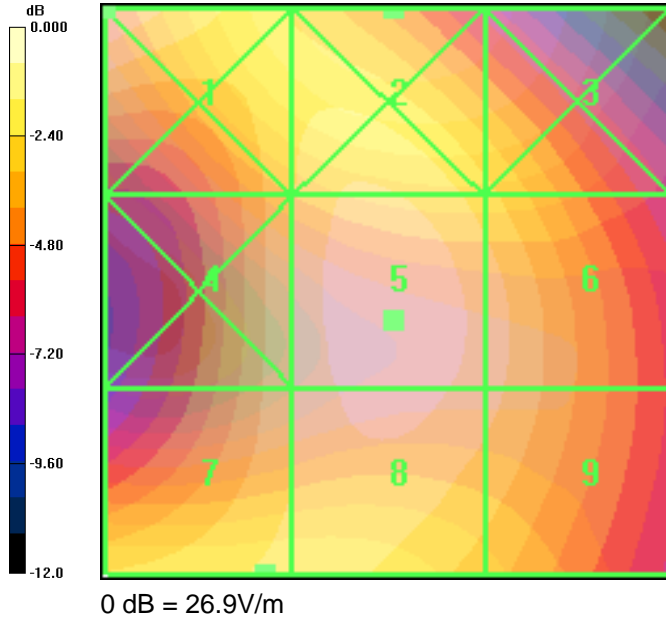



Applicant:	Kyocera
FCC ID:	V65C5171
Report #:	CT- C5171-20RFC-0712-R0

CDMA 1900 Channel 600 (360) E roll

