

The Testcenter facility 'Dosimetric Test Lab' within IMST GmbH is accredited by the German National 'Deutsche Akkreditierungsstelle GmbH (DAkkS)' for testing according to the scope as listed in the accreditation certificate: D-PL-12139-01-01.

Annex to Report

Dosimetric Assessment of the Portable Device Kyocera F42 (FCC ID: V65OASY1)

According to the FCC Requirements

November 24, 2011

IMST GmbH
Carl-Friedrich-Gauß-Str. 2
D-47475 Kamp-Lintfort

Customer
KYOCERA Corporation
2-1-1 Kagahara, Tsuzuki-ku,
224-8502 Yokohama-shi
Japan

The test results only relate to the items tested. This report shall not be reproduced except in full without the written approval of the testing laboratory.

1 Subject of Investigation



Fig. 1: Pictures of the device under test.

9.5 Pictures of the Device under Test

Figure 16 - 18 show the device under test and the used accessories.



Fig. 16: Front and side view of the Kyocera F42.



Fig. 17: Back and side view of the Kyocera F42.



Fig. 18: Pictures of the used headset under test.

9.6 Test positions for the Device under Test

Figure 19 - 24 show the test positions for the SAR measurements for the Kyocera F42.



Fig. 19: Cheek position, left side.



Fig. 20: Tilted position, left side.



Fig. 21: Cheek position, right side.



Fig. 22: Tilted position, right side.

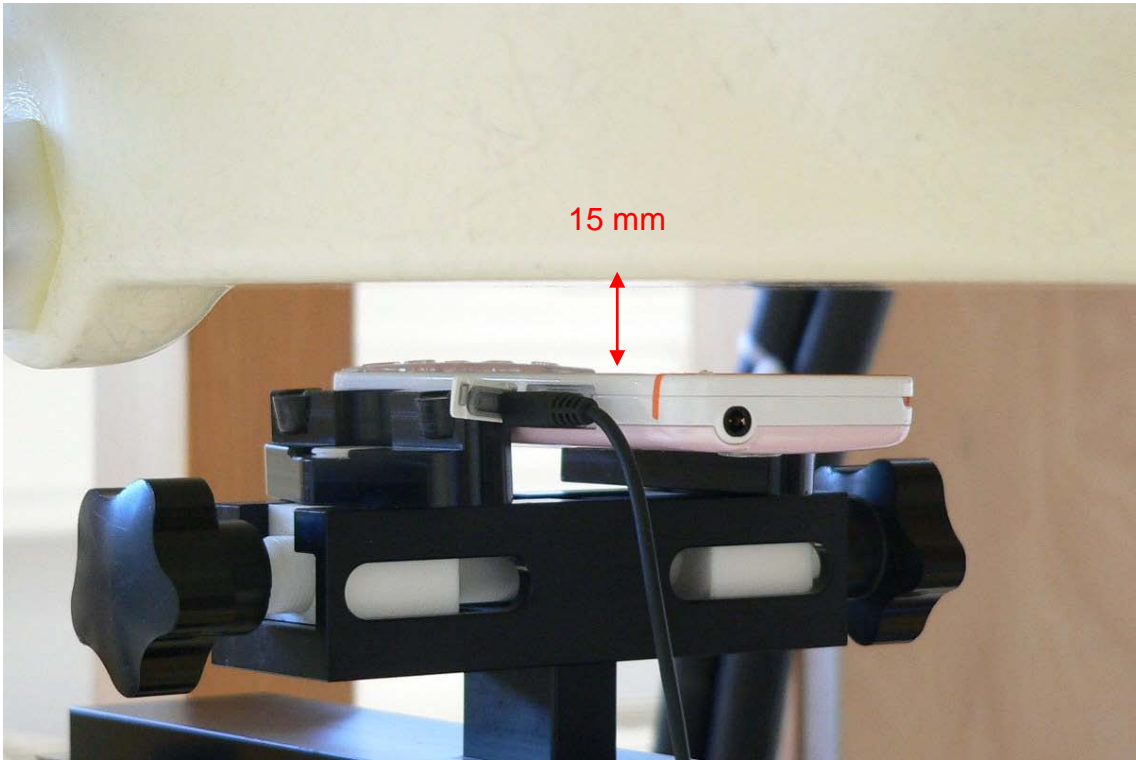


Fig. 23: Body worn configuration, position 1, display towards the phantom, headset attached, 15 mm distance



Fig. 24: Body worn configuration, position 2, display towards the ground, headset attached, 15 mm distance.