

SAR TEST REPORT

for

Texas Instruments Incorporated

TI-Nspire Navigator Access Point

Model No.: TINAVAP2

FCC ID : V7R-TINAVAP2

Prepared for : Texas Instruments Incorporated
12500 TI Boulevard Dallas, TX 75243-4136 USA

Prepared By : Audix Technology (Shenzhen) Co., Ltd.
No. 6, Ke Feng Rd., 52 Block,
Shenzhen Science & Industrial Park,
Nantou, Shenzhen, Guangdong, China

Tel: (0755) 26639496

Fax: (0755) 26632877

Report Number : ACS-SF11010
Date of Test : Dec.16, 2011~Feb.10, 2012
Date of Report : Feb.10, 2012

TABLE OF CONTENTS

Description	Page
Test Report Verification.....	3
1. GENERAL INFORMATION.....	4
1.1. Description of Device (EUT).....	4
1.2. The Maximum SAR Level.....	5
1.3. The Maximum Conducted Power Level.....	5
2. OPERATIONAL CONDITIONS.....	6
2.1. General description of test procedures.....	6
2.2. Block Diagram of connection between EUT and simulators.....	7
2.3. Test Equipment.....	7
2.4. Laboratory Environment.....	7
2.5. Measurement Uncertainty.....	7
3. TEST POSITION	9
3.1. Test Setup of EUT	9
4. SPECIFIC ABSORPTION RATE (SAR)	10
4.1. Specific Absorption Rate SAR Introduction.....	10
4.2. Specific Absorption Rate SAR Definition.....	10
5. SAR MEASUREMENTS SYSTEM CONFIGURATION.....	11
5.1. SAR Measurement Set-up.....	11
5.2. SAM Twin Phantom.....	12
5.3. ES3DV3 Isotropic E-Field Probe for Dosimetric Measurements.....	13
5.4. Device Holder for SAM Twin Phantom.....	14
5.5. E-field Probe Calibration.....	15
5.6. Scanning procedure.....	16
6. DATA STORAGE AND EVALUATION.....	18
6.1. Data Storage.....	18
6.2. Data Evaluation by SEMCAD.....	18
7. TISSUE SIMULATING LIQUIDS.....	20
8. SYSTEM CHECK.....	21
9. TEST RESULTS.....	22
9.1. Table 10.1 System Check for Body Tissue simulating liquid.....	22
9.2. Table 10.2 Dielectric Performance for Body Tissue simulating liquid.....	22
10. TEST RESULTS.....	23
10.1. Conducted Output Average Power (WIFI).....	23
10.2. Conducted Output Peak Power (WIFI).....	23
10.3. The SAR Test Results.....	24
10.4. System Check Results.....	25
10.5. Graph Results.....	27
11. DIPOLE CALIBRATION CERTIFICATE	47
12. E-FIELD PROBES DIPOLE CALIBRATION CERTIFICATE	56
13. DAE CALIBRATION CERTIFICATE:	67
14. PHOTOGRAPHS OF TEST	73
15. PHOTOS OF THE EUT	75

SAR TEST REPORT

Applicant : Texas Instruments Incorporated
 Manufacturer : Inventec Appliances(Pudong) Corporation
 EUT Description : TI-Nspire Navigator Access Point
 FCC ID : V7R-TINAVAP2
 (A) Model NO. : TINAVAP2
 (B) SERIAL NO. : N/A
 (C) POWER SUPPLY : DC 5V (Via Laptop)
 (D) TEST VOLTAGE : DC 5V

Measurement Standard Used:

OET 65 Supplement C
 IEEE Std C95.1-1999
 IEEE Std C95.3-2002
 IEEE 1528-2003
 47 CFR Part 2(2.1093)
 KDB 447498 D01 Mobile Portable RF Exposure v04
 KDB 248227 D01 SAR Measure for 802.11 a b g v01r02

The device described above is tested by Audix Technology (Shenzhen) Co., Ltd. to determine the maximum emission levels emanating from the device and the severe levels of the device can endure and its performance criterion. The test results are contained in this test report and Audix Technology (Shenzhen) Co., Ltd. is assumed full responsibility for the accuracy and completeness of test. This report contains data that are not covered by the NVLAP accreditation. Also, this report shows that the EUT is technically compliant with the OET 65 Supplement C, IEEE Std C95.1-1999, IEEE Std C95.3-2002, IEEE 1528-2003, 47 CFR Part 2(2.1093), This report applies to above tested sample only. This report shall not be reproduced in part without written approval of Audix Technology (Shenzhen) Co., Ltd.

Date of Test : Dec.16, 2011~Feb.10, 2012 Report of date: Feb.10, 2012

Prepared by : Sala Yang / Sala Yang / Supervisor
 Reviewer by : Sunny Lu / Sunny Lu / Supervisor



Approved & Authorized Signer : Ken Lu / Manager

1. GENERAL INFORMATION

1.1. Description of Device (EUT)

Description	: TI-Nspire Navigator Access Point
Model Number	: TINAVAP2
FCC ID	: V7R-TINAVAP2
Applicant	: Texas Instruments Incorporated 12500 TI Boulevard Dallas, TX 75243-4136 USA
Manufacturer	: Inventec Appliances(Pudong) Corporation No. 789 Pu Xing Road, Shanghai, PRC
Operation frequency	: IEEE 802.11b: 2412 MHz—2462 MHz IEEE 802.11g: 2412 MHz—2462 MHz IEEE802.11n HT20: 2412MHz—2462MHz
Modulation	: IEEE 802.11b: DSSS(CCK,DQPSK,DBPSK) IEEE 802.11g: OFDM(64QAM, 16QAM, QPSK, BPSK) IEEE 802.11n HT20: OFDM (64QAM, 16QAM, QPSK,BPSK)
Transfer Rate	802.11b: 11/5.5/2/1 Mbps 802.11g: 54/48/36/24/18/12/9/6 Mbps 802.11n: (1 data stream) 6.5/13/19.5/26/39/52/58.5/65 Mbps
Maximum Output Power	: 802.11b data rates, 13dBm max 802.11g data rates, 16dBm max 802.11n data rates, 13dBm max
Antenna Type	: Etched Antenna for TX and RX (3.4dBi peak) Etched Antenna for RX diversity (3.2dBi peak)
Antenna Gain	: 3.4 dBi
Adapter	: Manufacturer: HuntKey, M/N: HKA00905015-2C
I/O Ports	: Micro B High Speed USB (2.0) port
Data Cable	: 12" and 60" Micro B to Standard A USB cable
Date of Test	: Dec.16, 2011~Feb.10, 2012
Date of Receipt	: Dec.16, 2011
Sample Type	: Prototype production

1.2. The Maximum SAR Level

Test Position		Channel	Results		Limit	
			1g SAR Average	10g SAR Average	1g SAR (1.6W/Kg)	10g SAR (2.0W/Kg)
11b	Top	CH6	0.449	0.191	PASS	
11g	Front	CH1	0.995	0.497	PASS	
11n HT20	Front	CH6	0.477	0.245	PASS	

1.3.The Maximum Conducted Power Level

Test Mode	Max Average Power (dBm)
11b	11.88
11g	15.21
11n HT20	11.93

2. OPERATIONAL CONDITIONS

2.1. General description of test procedures

For the 802.11b/g SAR body tests, a communication link is set up with the test mode software for WIFI mode test. The Absolute Radiofrequency Channel Number (ARFCN) is allocated to 1,6 and 11 respectively in the case of 2450 MHz. During the test, at the each test frequency channel, the EUT is operated at the RF continuous emission mode. Each channel should be tested at the lowest data rate. Testing at higher data rates is not required when the maximum average output power is less than 0.25dB higher than those measured at the lowest data rate.

802.11b/g operating modes are tested independently according to the service requirements in each frequency band. 802.11b/g modes are tested on channels 1,6,11; however, if output power reduction is necessary for channels 1 and/or 11 to meet restricted band requirements the highest output channels closest to each of these channels must be tested instead.

SAR is not required for 802.11g channels when the maximum average output power is less than 0.25dB higher than that measured on the corresponding 802.11b channels. When the maximum average output channel in each frequency band is not included in the “default test channels”, the maximum channel should be tested instead of an adjacent “default test channels”, these are referred to as the “required test channels” and are illustrated in table 1.

Then The Absolute Radiofrequency Channel Number (ARFCN) is firstly allocated to 2437 respectively in the case of 802.11b/g.

Mode	GHz	CH	Turbo Channel	“Default Test Channels”	
				15.247	
				802.11b	802.11g
802.11b/g	2.412	1 [#]		√	*
	2.437	6	6	√	*
	2.462	11 [#]		√	*

Table 1

Note: [#]= when output power is reduced for channel 1 and/or 11 to meet restricted band requirements the highest out put channels closet to each of these channels should be tested.


√= ” default test channels”

* = possible 802.11g channels with maximum average output 0.25dB>=the “default test channels”

2.2. Tested Supporting System Details

No.	Description	ACS No.	Manufacturer	Model	Serial Number	Approved type
1	Notebook	Test PC R	DELL	D430	PP09S	<input checked="" type="checkbox"/> FCC DoC

2.3. Block Diagram of connection between EUT and simulators

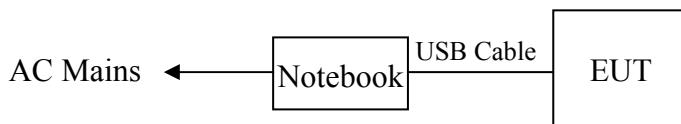

(EUT: TI-Nspire Navigator Access Point)

2.4. Test Equipment

Item	Equipment	Manufacturer	Model No.	S/N	Last Cal Date	Cal. Interval
1.	SAR Test System	Speag	DASY5 TX60L SAR	N/A	June.4,11	1 Year
2.	Wireless Communication Test Set	Agilent	E5515C	GB44300243	May.08, 11	1Year
3.	Power Meter	Anritsu	ML2487A	6K00002472	May.08, 11	1 Year
4.	Power Sensor	Anritsu	MA2491A	032516	May.08, 11	1 Year
5.	Signal Generator	Marconi	2031B	119606/058	May.08, 11	1 Year
6.	Amplifier	Milmega	AS0206-50	1036253	NCR	N/A
7.	Dipole Antenna	Speag	D900V2	1d088	Mar.23,11	1 Year
8.	Dipole Antenna	Speag	D1800V2	2d186	Mar.22,11	1 Year
9.	Dipole Antenna	Speag	D2000V2	1055	Mar.24,11	1 Year
10.	Dipole Antenna	Speag	D2450V2	862	Mar.22,11	1 Year
11.	Dipole Antenna	Speag	D5GHzV2	1102	Mar.14,11	1 Year
12.	Attenuator	Agilent	8491A 3dB	MY39262001	May.08, 11	1 Year
13.	Attenuator	Agilent	8491A 10dB	MY39264375	May.08, 11	1 Year
14.	DAE	Speag	DAE4	899	Mar.18,11	1 Year
15.	E-Field Probe	Speag	ES3DV3	3139	Mar.23,11	1 Year
16.	E-Field Probe	Speag	EX3DV4	3767	Mar.21,11	1Year

2.5. Laboratory Environment

Temperature	Min:20°C ,Max.25°C
Relative humidity	Min. = 30%, Max. = 70%
Note: Ambient noise is checked and found very low and in compliance with requirement of standards.	

2.6. Measurement Uncertainty

Test Item	Uncertainty
Uncertainty for SAR test	1g: 21.14
	10g: 20.64
Uncertainty for test site temperature and humidity	0.6°C
	3%

Source	Type	Uncertainty Value (%)	Probability Distribution	K	C1(1g)	C1(10g)	Standard uncertainty y ul(%)1g	Standard uncertainty y ul(%)10g	Degree of freedom Veff or Vi
Measurement system repetivity	A	0.5	N	1		1	0.5	0.5	9
Probe calibration	B	5.9	N	1	1	1	5.9	5.9	∞
Isotropy	B	4.7	R	√3	1	1	2.7	2.7	∞
Linearity	B	4.7	R	√3	1	1	2.7	2.7	∞
Probe modulation response	B	0	R	√3	1	1	0	0	∞
Detection limits	B	1.0	R	√3	1	1	0.6	0.6	∞
Boundary effect	B	1.9	R	√3	1	1	1.1	1.1	∞
Readout electronics	B	1.0	N	1	1	1	1.0	1.0	∞
Response time	B	0	R	√3	1	1	0	0	∞
Integration time	B	4.32	R	√3	1	1	2.5	2.5	∞
RF ambient conditions – noise	B	0	R	√3	1	1	0	0	∞
RF ambient conditions – reflections	B	3	R	√3	1	1	1.73	1.73	∞
Probe positioner mech. restrictions	B	0.4	R	√3	1	1	0.2	0.2	∞
Probe positioning with respect to phantom shell	B	2.9	R	√3	1	1	1.7	1.7	∞
Post-processing	B	0	R	√3	1	1	0	0	∞
Test sample related									
Device holder uncertainty	A	2.94	N	1	1	1	2.94	2.94	M-1
Test sample positioning	A	4.1	N	1	1	1	4.1	4.1	M-1
Power scaling	B	5.0	R	√3	1	1	2.9	2.9	∞
Drift of output power (measured SAR drift)	B	5.0	R	√3	1	1	2.9	2.9	∞
Phantom and set-up									
Phantom uncertainty (shape and thickness tolerances)	B	4.0	R	√3	1	1	2.3	2.1	∞
Algorithm for correcting SAR for deviations in permittivity and conductivity	B	1.9	N	1	1	0,84	1,9	1,6	∞
Liquid conductivity (meas.)	A	0.55	N	1	0.78	0.71	0.24	0.21	M-1
Liquid permittivity (meas.)	A	0.19	N	1	0.23	0.26	0.09	0.06	M
Liquid permittivity – temperature uncertainty	A	5.0	R	√3	0,78	0,71	1.4	1.1	∞
Liquid conductivity – temperature uncertainty	A	5.0	R	√3	0.23	0,26	1.2	0.8	∞
Combined standard uncertainty	$u_c = \sqrt{\sum_{i=1}^{23} c_i^2 u_i^2}$						10.57	10.32	
Expanded uncertainty (95 % conf. interval)	$u_e = 2u_c$		N		K=2		21.14	20.64	

3. TEST POSITION

3.1. Test Setup of EUT

Due to the display or overall diagonal dimension $30\text{ cm} > 20\text{ cm}$, according to KDB447498 D01 Mobile Portable RF Exposure v04 SAR is tested for back and edge with most conservative exposure conditions, the EUT is tested at the following test positions.

- (1) Test Position Back Side: The Back Side of the EUT towards and directed tightly to touch the flat phantom.
 - (2) Test Position Top Side: The Top Side of the EUT towards and directed tightly to touch the flat phantom.
 - (3) Test Position Right Side: The Right Side of the EUT towards and directed tightly to touch the flat phantom.
 - (4) Test Position Front Side: The Front Side of the EUT towards and directed tightly to touch the flat phantom.
 - (5) Test Position Bottom Side: The SAR is not required.
(Because the distance is more than 2.5 cm between antenna and Bottom side)
 - (6) Test Position Left Side: The SAR is not required.
(Because the distance is more than 2.5 cm between antenna and Left side)
- The 5/6 positions are not the most conservative antenna - to - user distance at edge mode. According to KDB 447498 4) ii) (2) –SAR is required only the edge with the most conservative exposure conditions, No SAR)

4. SPECIFIC ABSORPTION RATE (SAR)

4.1. Specific Absorption Rate SAR Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

4.2. Specific Absorption Rate SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density (ρ). The equation description is as below:

$$\mathbf{SAR} = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per Kilogram (W/Kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$\mathbf{SAR} = C \frac{\delta T}{\delta t}$$

where C is the specific heat capacity, δT the temperature rise and δt is the exposure duration, or related to the electrical field in the tissue by

$$\mathbf{SAR} = \frac{\sigma |E|^2}{\rho}$$

where σ is the conductivity of the tissue, ρ is the mass density of the tissue and E is the rms electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.

5. SAR MEASUREMENTS SYSTEM CONFIGURATION

5.1. SAR Measurement Set-up

DASY5 system for performing compliance tests consists of the following items:

- (1) A standard high precision 6-axis robot (Stäubli RX family) with controller and software. An arm extension for accommodating the data acquisition electronics (DAE).
- (2) A dosimetric probe, i.e. an isotropic E-field probe optimized and calibrated for usage. It issues simulating liquid. The probe is equipped with an optical surface detector system.
- (3) A data acquisition electronic (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- (4) A unit to operate the optical surface detector which is connected to the EOC.
- (5) The Electro-Optical Coupler (EOC) performs the conversion from the optical into a digital electric signal of the DAE. The EOC is connected to the DASY5 measurement server.
- (6) The DASY5 measurement server, which performs all real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operation. A computer operating Windows 2003.
- (7) DASY5 software and SEMCAD data evaluation software.
- (8) Remote control with teach panel and additional circuitry for robot safety such as warning lamps, etc.
- (9) The generic twin phantom enabling the testing of left-hand and right-hand usage.
- (10) The device holder for handheld mobile phones.
- (11) Tissue simulating liquid mixed according to the given recipes.
- (12) System validation dipoles allowing to validate the proper functioning of the system.

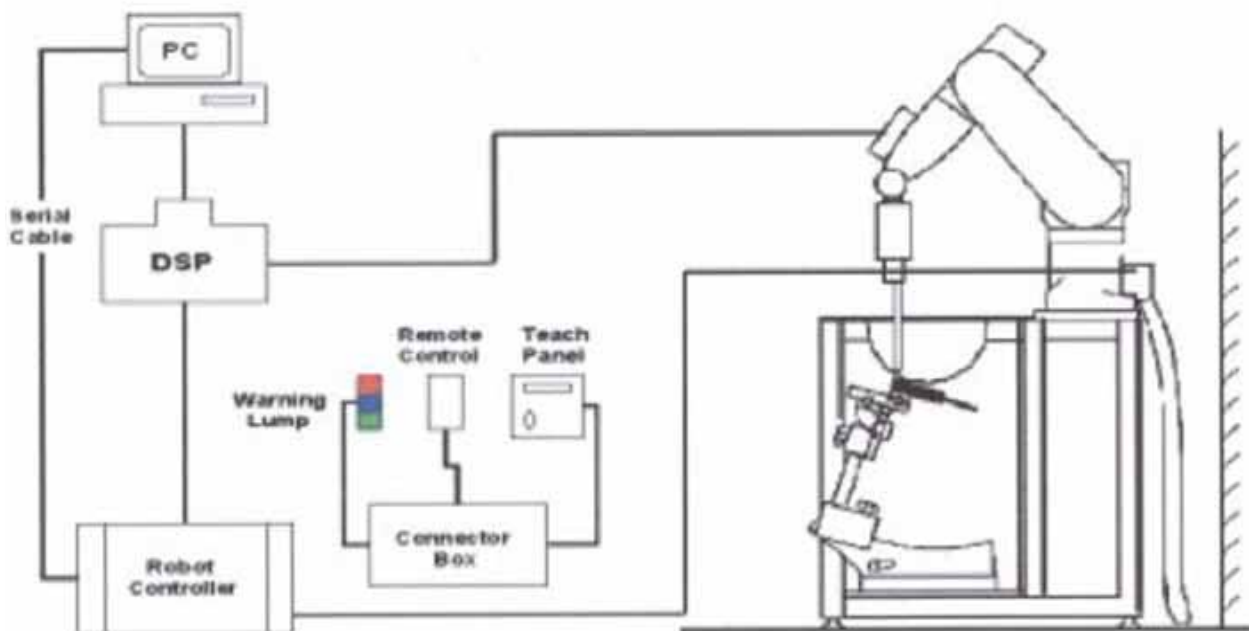


Figure 6.1 SAR Lab Test Measurement Set-up

5.2.SAM Twin Phantom

Phantom for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30 MHz to 6 GHz. ELI is fully compatible with the IEC 62209-2 standard and all known tissue simulating liquids. ELI has been optimized regarding its performance and can be integrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points. The phantom is compatible with all SPEAG dosimetric probes and dipoles.



Material	Vinylester, glass fiber reinforced (VE-GF)
Liquid Compatibility	Compatible with all SPEAG tissue simulating liquids (incl. DGBE type)
Shell Thickness	2.0 ± 0.2 mm (bottom plate)
Dimensions	Major axis: 600 mm Minor axis: 400 mm
Filling Volume	approx. 30 liters
Wooden Support	SPEAG standard phantom table

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections.

Figure 6.2 Top View of Twin Phantom

A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters.

On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

The phantom can be used with the following tissue simulating liquids:

*Water-sugar based liquid

*Glycol based liquids

5.3.ES3DV3 Isotropic E-Field Probe for Dosimetric Measurements

Symmetrical design with triangular core
 Interleaved sensors
 Built-in shielding against static charges
 PEEK enclosure material (resistant to organic solvents, e.g., DGBE)



Calibration	ISO/IEC 17025 calibration service available.
Frequency	10MHz to 4GHz Linearity:0.2dB (30MHz to 4GHz)
Directivity	±0.2dB in HSL (rotation around probe axis) ±0.3dB in tissue material (rotation normal to probe axis)
Dynamic Range	5uW/g to > 100 mW/g; Linearity: 0.2dB
Dimensions	Overall length: 337 mm (Tip:20 mm) Tip diameter: 3.9mm (Body:12mm) Distance from probe tip to dipole centers: 2.0mm
Application	General dosimetry up to 4 GHz Dosimetry in strong gradient fields Compliance tests of mobile phones
Compatibility	DASY3, DASY4, DASY52 SAR and higher, EASY4/MRI

5.4. Device Holder for SAM Twin Phantom

The SAR in the Phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source in 5 mm distance, a positioning uncertainty of $\pm 0.5\text{mm}$ would produce a SAR uncertainty of $\pm 20\%$. An accurate device position is therefore crucial for accurate and repeatable measurement. The position in which the devices must be measured, are defined by the standards.

The DASY5 device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation centers for both scales is the ear reference point (EPR).

Thus the device needs no repositioning when changing the angles.

The DASY5 device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity $\epsilon_r=3$ and loss tangent $\delta=0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.

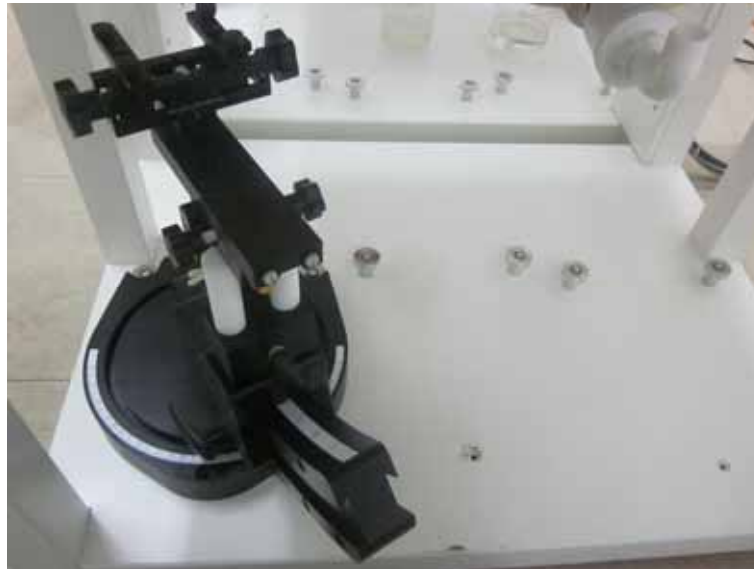


Figure 6.4 Device Holder

5.5.E-field Probe Calibration

Each probe is calibrated according to a dosimetric assessment procedure with accuracy better than $\pm 10\%$. The spherical isotropy was evaluated and found to be better than $\pm 0.25\text{dB}$. The sensitivity parameters (NormX, NormY, NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested.

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies below 1 GHz, and in a wave guide above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$\text{SAR} = C * (\Delta T / \Delta t)$$

Where: Δt = Exposure time (30 seconds),

C = Heat capacity of tissue (brain or muscle),

ΔT = Temperature increase due to RF exposure.

Or

$$\text{SAR} = (E^2 * \sigma) / \rho$$

Where:

σ = Simulated tissue conductivity,

ρ = Tissue density (kg/m^3).

5.6. Scanning procedure

The DASY5 installation includes predefined files with recommended procedures for measurements and validation. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.

The "reference" and "drift" measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. $\pm 5\%$.

The "surface check" measurement tests the optical surface detection system of the DASY5 system by repeatedly detecting the surface with the optical and mechanical surface detector and comparing the results. The output gives the detecting heights of both systems, the difference between the two systems and the standard deviation of the detection repeatability. Air bubbles or refraction in the liquid due to separation of the sugar-water mixture gives poor repeatability (above $\pm 0.1\text{mm}$). To prevent wrong results tests are only executed when the liquid is free of air bubbles.

The difference between the optical surface detection and the actual surface depends on the Probe and is specified with each probe. (It does not depend on the surface reflectivity or the probe angle to the surface within $\pm 30^\circ$.)

Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values before running a detailed measurement around the hot spot. Before starting the area scan a grid spacing of 15 mm x 15 mm is set. During the scan the distance of the probe to the phantom remains unchanged.

After finishing area scan, the field maxima within a range of 2 dB will be ascertained.

Zoom Scan

Zoom Scans are used to estimate the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The default Zoom Scan is done by 7x7x7 points within a cube whose base is centered around the maxima found in the preceding area scan.

Spatial Peak Detection

The procedure for spatial peak SAR evaluation has been implemented and can determine values of masses of 1g and 10g, as well as for user-specific masses. The DASY5 system allows evaluations that combine measured data and robot positions, such as:

- maximum search
- extrapolation
- boundary correction
- peak search for averaged SAR

During a maximum search, global and local maxima searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard's method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation. Extrapolation routines require at least 10 measurement points in 3-D space. They are used in the Zoom Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the modified Quadratic Shepard's method for extrapolation. For a grid using 7x7x7 measurement points with 5mm resolution amounting to 343 measurement points, the uncertainty of the extrapolation routines is less than 1% for 1g and 10g cubes.

A Z-axis scan measures the total SAR value at the x-and y-position of the maximum SAR value found during the cube 7x7x7 scan. The probe is moved away in z-direction from the bottom of the SAM phantom in 5mm steps.

6. DATA STORAGE AND EVALUATION

6.1. Data Storage

The DASY5 software stores the acquired data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension ".DA4". The software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of incorrect parameter settings. For example, if a measurement has been performed with a wrong crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be re-evaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type ([V/m], [A/m], [°C], [mW/g], [mW/cm²], [dBrel], etc.). Some of these units are not available in certain situations or show meaningless results, e.g., a SAR output in a lossless media will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

6.2. Data Evaluation by SEMCAD

The SEMCAD software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters: - Sensitivity Normi, ai0, ai1, ai2
 - Conversion factor ConvFi
 - Diode compression point Dcpi

Device parameters: - Frequency f
 - Crest factor cf

Media parameters: - Conductivity
 - Density

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY5 components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics.

If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot c f / d c p i$$

With V_i = compensated signal of channel i (i = x, y, z)
 U_i = input signal of channel i (i = x, y, z)
 cf = crest factor of exciting field (DASY parameter)
 $dcpi$ = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes: $E_i = (V_i / Norm_i \cdot ConvF)^{1/2}$

H-field probes: $H_i = (V_i)^{1/2} \cdot (ai_0 + ai_1 f + ai_2 f^2) / f$

With V_i = compensated signal of channel i (i = x, y, z)
 $Norm_i$ = sensor sensitivity of channel i (i = x, y, z)
 $ConvF$ = sensitivity enhancement in solution
 ai_j = sensor sensitivity factors for H-field probes
 f = carrier frequency [GHz]
 E_i = electric field strength of channel i in V/m
 H_i = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = (E_x^2 + E_y^2 + E_z^2)^{1/2}$$

The primary field data are used to calculate the derived field units.

$$SAR = (E_{tot}^2 \cdot \rho) / (\sigma \cdot 1000)$$

with

SAR = local specific absorption rate in mW/g

E_{tot} = total field strength in V/m

ρ = conductivity in [mho/m] or [Siemens/m]

σ = equivalent tissue density in g/cm³

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid. The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = E_{tot}^2 / 3770 \quad \text{or} \quad P_{pwe} = H_{tot}^2 \cdot 37.7$$

with P_{pwe} = equivalent power density of a plane wave in mW/cm²

E_{tot} = total electric field strength in V/m

H_{tot} = total magnetic field strength in A/m

7. TISSUE SIMULATING LIQUIDS

For the measurement of the field distribution inside the SAM phantom with DASY5, the phantom must be filled with around 25 liters of homogeneous tissue simulating liquid. The liquid height from the ear reference point (ERP) of the phantom to the liquid top surface is (head SAR) or from the flat phantom to the liquid top surface (body SAR) is 15.2cm.

The liquid is consisted of water, sugar, salt, Glycol monobutyl, Preventol and Cellulose. The liquid has previously been proven to be suited for worst-case. The Table 8 shows the detail solution.

The following ingredients for tissue simulating liquid are used:

Water: deionized water, resistivity $\geq 16M \Omega$ - as basis for the liquid

Sugar: refined sugar in crystals, as available in food shops-to reduce relative permittivity

Salt: pure NaCl-to increase conductivity

Cellulose: Hydroxyethyl-cellulose medium viscosity(75-125mPa.s, 2% in water, 20°C), CAS#54290-to increase viscosity and to keep sugar in solution.

Preservative: Preventol D-7 Bayer

Deithlenglycol-monobutyl ether (DGMBE), Fluka Chemie GmbH, CAS#112-34-5-to reduce relative permittivity.

Table 6.1 gives the recipes for one liter of head and body tissue simulating liquid for frequency band 2450 MHz.

Ingredient	MSL 2450MHz
Water	698.3 ml
DGMBE	301.7 ml
Total Amount	1 L
Dielectric Parameters at 22°C	F=2450MHz $\epsilon = 52.5 \pm 5\%$ $\sigma = 2.00 \pm 10\% \text{ S/m}$

Table 8.1 Ingredient for Tissue Simulating Liquid


The dielectric parameters of the liquids were verified prior to the SAR evaluation using an Agilent 85070E Dielectric Probe Kit and an Agilent Network Analyzer.

8. SYSTEM CHECK

The manufacturer calibrates the probes annually. Dielectric parameters of the tissue simulates were measured every day using the dielectric probe kit and the network analyzer. A system check measurement was made following the determination of the dielectric parameters of the simulates, using the dipole validation kit. A power level of 250 mW was supplied to the dipole antenna, which was placed under the flat section of the twin SAM phantom. The system check results (dielectric parameters and SAR values) are given in the Table 6.

System check results have to be equal or near the values determined during dipole calibration with the relevant liquids and test system ($\pm 10\%$).

System check is performed regularly on all frequency bands where tests are performed with the DASY5 system.

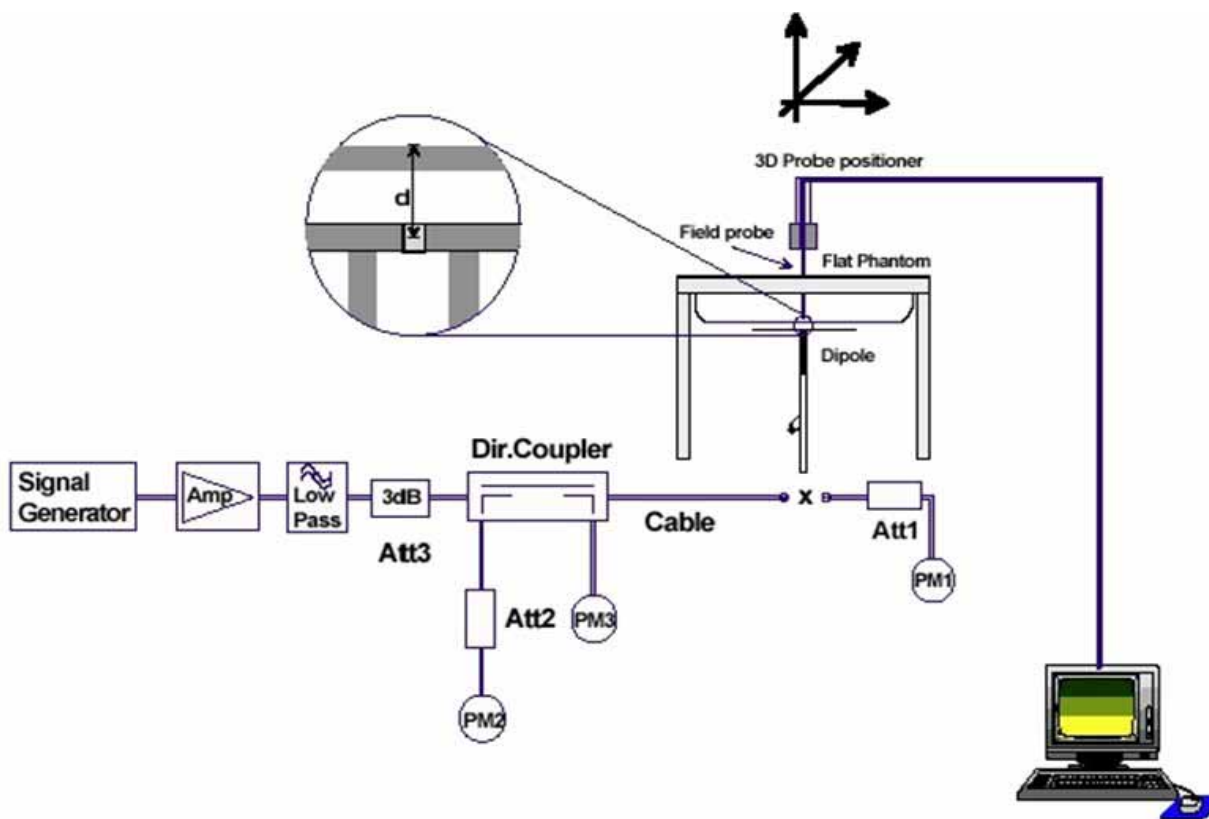

System Check Set-up

9. TEST RESULTS

9.1. Table 10.1 System Check for Body Tissue simulating liquid

Frequency	Description	SAR(W/kg)		Temp
		1g	10g	°C
2450MHz	Recommended value ±10% window	12.8 11.7 — 14.3	5.97 5.37 — 6.57	/
	Measurement value 2011-12-16	13.62	6.37	22.3
	Measurement value 2012-02-10	13.65	6.44	22.2

Note: Recommended Values used derive from the calibration certificate and 250 mW is used as feeding power to the calibrated dipole.

9.2. Table 10.2 Dielectric Performance for Body Tissue simulating liquid

Frequency	Description	Dielectric Parameters		Temp
		ϵ_r	σ (s/m)	°C
	Target value ±5% window	52.7 50.07-55.34	1.95 1.85-2.05	/
2410MHz	Measurement value 2011-12-16	50.861	1.968	21.3
	Measurement value 2012-02-10	50.739	2.013	21.2
2450MHz	Measurement value 2011-12-16	52.330	1.970	21.3
2460MHz	Measurement value 2011-12-16	50.622	2.048	21.3



Figure 10.2: Liquid depth in the Flat Phantom (2450MHz, 15.2 depth)

10. TEST RESULTS

10.1. Conducted Output Average Power (WIFI)

Test Mode	Channel	Frequency (MHz)	Max Average Power	
			Before Test (dBm)	After Test (dBm)
11b	CH1	2412	11.68	11.88
	CH6	2437	11.23	11.19
	CH11	2462	11.45	11.49
11g	CH1	2412	15.23	15.21
	CH6	2437	15.05	15.07
	CH11	2462	14.85	14.78
11n HT20	CH1	2412	11.92	11.93
	CH6	2437	11.50	11.52
	CH11	2462	11.72	11.70

10.2. Conducted Output Peak Power (WIFI)

802.11b

Rate/ Channel	CH1	CH6	CH11
1Mbps	12.98	13.23	13.51
2Mbps	12.90	13.06	13.50
5.5Mbps	12.88	13.14	13.47
11Mbps	12.93	13.19	13.36

802.11g

Rate/ Channel	CH1	CH6	CH11
6Mbps	22.76	22.93	23.23
9Mbps	22.28	22.36	22.69
12 Mbps	22.72	22.91	23.17
18 Mbps	22.39	22.59	22.79
24 Mbps	22.68	22.79	23.17
36 Mbps	22.54	22.77	22.81
48 Mbps	22.26	22.19	22.78
54 Mbps	22.03	22.33	22.39

802.11n HT20

Rate/ Channel	CH1	CH6	CH11
MCS0	20.23	20.46	20.80
MCS1	20.17	20.33	20.19
MCS2	19.89	20.43	20.45
MCS3	19.84	20.03	20.28
MCS4	20.03	20.37	20.36
MCS5	19.85	20.06	20.11
MCS6	20.21	20.08	20.18
MCS7	19.65	20.03	20.14

10.3. The SAR Test Results

Test Position		Channel	Results		Power Drift ±0.2	Limit	
			1g SAR Average	10g SAR Average		1g SAR (1.6W/Kg)	10g SAR (2.0W/Kg)
11b	Front	CH6	0.427	0.218	-0.12	PASS	
	Back	Ch6	0.381	0.198	0.14	PASS	
	Right	CH6	0.325	0.139	0.18	PASS	
	Top	CH6	0.449	0.191	-0.07	PASS	
11g	Front	CH1	0.995	0.497	0.10	PASS	
		CH6	0.939	0.461	0.05	PASS	
		CH11	0.761	0.359	0.06	PASS	
	Back	CH6	0.783	0.404	-0.16	PASS	
	Right	CH6	0.644	0.274	0.17	PASS	
	Top	CH1	0.991	0.422	-0.07	PASS	
		CH6	0.851	0.360	-0.02	PASS	
CH11		0.614	0.262	-0.14	PASS		
Top-2	CH1	0.707	0.329	0.18	PASS		
11n HT20	Front	CH6	0.477	0.245	0.12	PASS	
	Back	CH6	0.398	0.209	-0.16	PASS	
	Right	CH6	0.218	0.093	0.18	PASS	
	Top	CH6	0.405	0.123	0.17	PASS	

Note: 1. The SAR test shall be performed at the high, middle and low frequency channels of each operating mode. If the SAR measured at mid-band channel for each test configuration is at least 3.0 dB lower than the SAR limit, testing at the high and low channels is optional.

10.4. System Check Results

Date: 12/16/2011 Time: 09:13:37 AM

DUT: Dipole 2450 MHz; Serial: D2450V2 S/N: 3139

Communication System: CW; Communication System Band: D2450 (2450.0 MHz);

Frequency: 2450 MHz; Communication System PAR: 0 dB; Crest factor: 1

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.97$ mho/m; $\epsilon_r = 52.33$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: SAM1; Type: SAM; Serial: TP-1543
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=xx mW, dist=3.0mm (ES-Probe)/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 17.500 mW/g


System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=xx mW, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.979 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 28.640 W/kg

SAR(1 g) = 13.62mW/g; SAR(10 g) = 6.37 mW/g

Maximum value of SAR (measured) = 15.737 mW/g

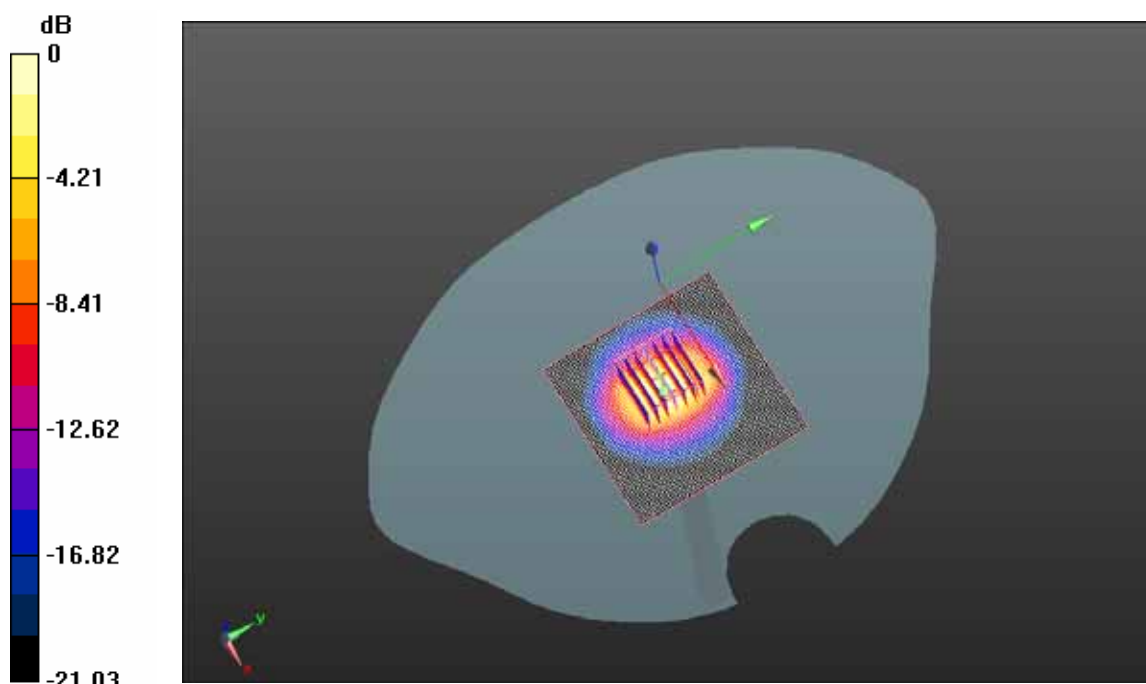

0 dB = 15.740mW/g

Date: 10/02/2011 Time: 13:40:50

DUT: Dipole 2450 MHz; Serial: D2450V2 S/N: 3139

Communication System: CW; Communication System Band: D2450 (2450.0 MHz);

Frequency: 2450 MHz; Communication System PAR: 0 dB; Crest factor: 1

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.95$ mho/m; $\epsilon_r = 52.32$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: SAM1; Type: SAM; Serial: TP-1543
- Measurement SW: DASYS2, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=xx mW, dist=3.0mm (ES-Probe)/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 17.500 mW/g


System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=xx mW, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.979 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 28.640 W/kg

SAR(1 g) = 13.65mW/g; SAR(10 g) = 6.44 mW/g

Maximum value of SAR (measured) = 15.742 mW/g

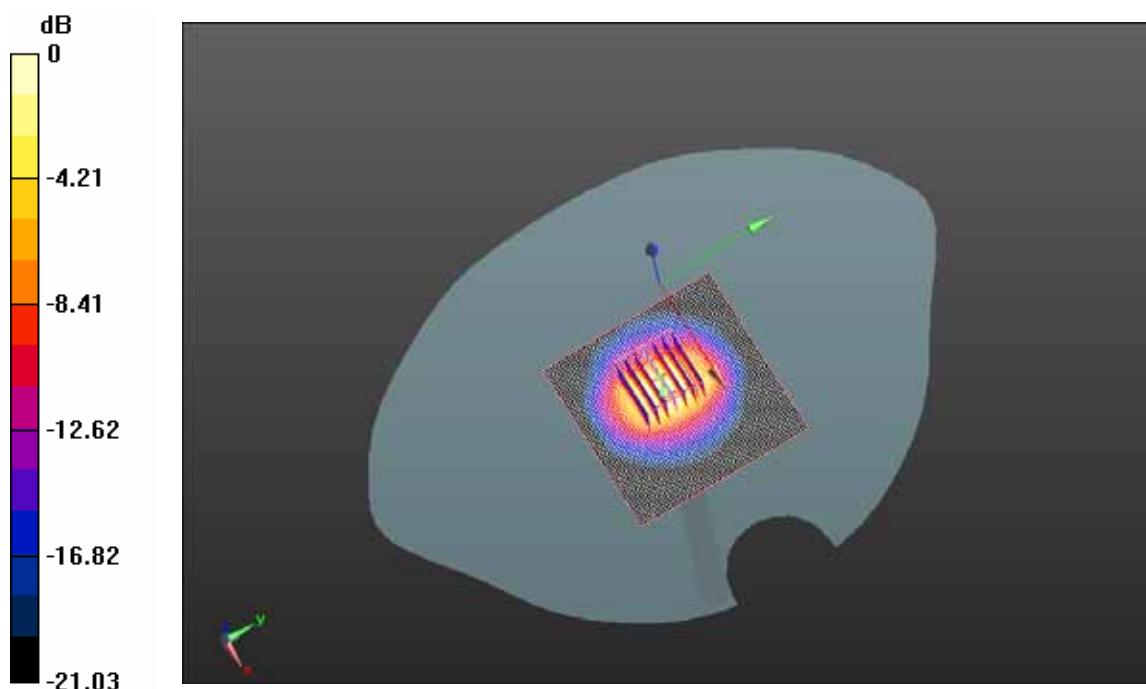

0 dB = 15.740mW/g

10.5. Graph Results

Front 11b CH6

Date/Time: 12/16/2011 09:40:58

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section ; Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Front/Area Scan (161x101x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.519 mW/g


Configuration/Front/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 11.751 V/m; Power Drift = -0.12 dB

Peak SAR (extrapolated) = 0.973 W/kg

SAR(1 g) = 0.427 mW/g; SAR(10 g) = 0.218 mW/g

Maximum value of SAR (measured) = 0.486 mW/g

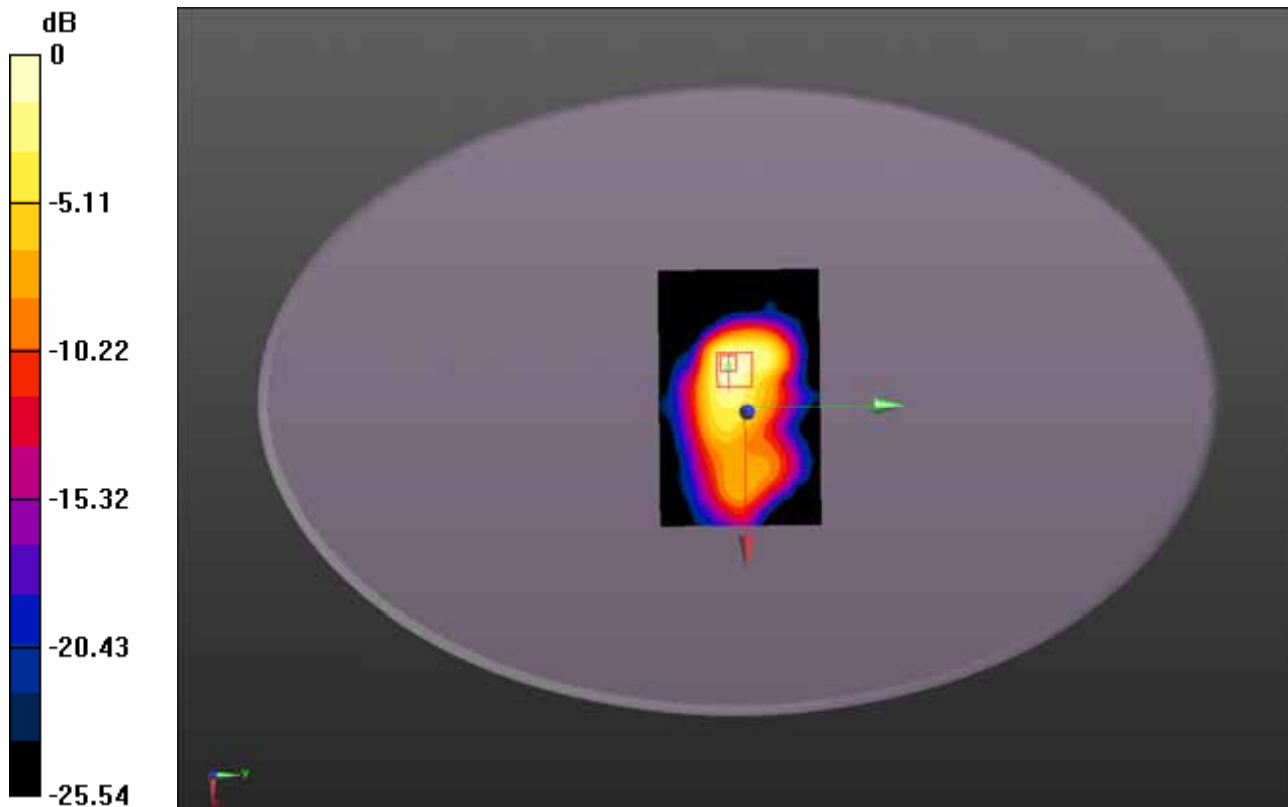

0 dB = 0.490mW/g

Back 11b CH6

Date/Time: 16/12/2011 10:14:25

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASYS2, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Back/Area Scan (161x101x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.430 mW/g


Configuration/Back/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 14.512 V/m; Power Drift = 0.14 dB

Peak SAR (extrapolated) = 0.775 W/kg

SAR(1 g) = 0.381 mW/g; SAR(10 g) = 0.198 mW/g

Maximum value of SAR (measured) = 0.429 mW/g

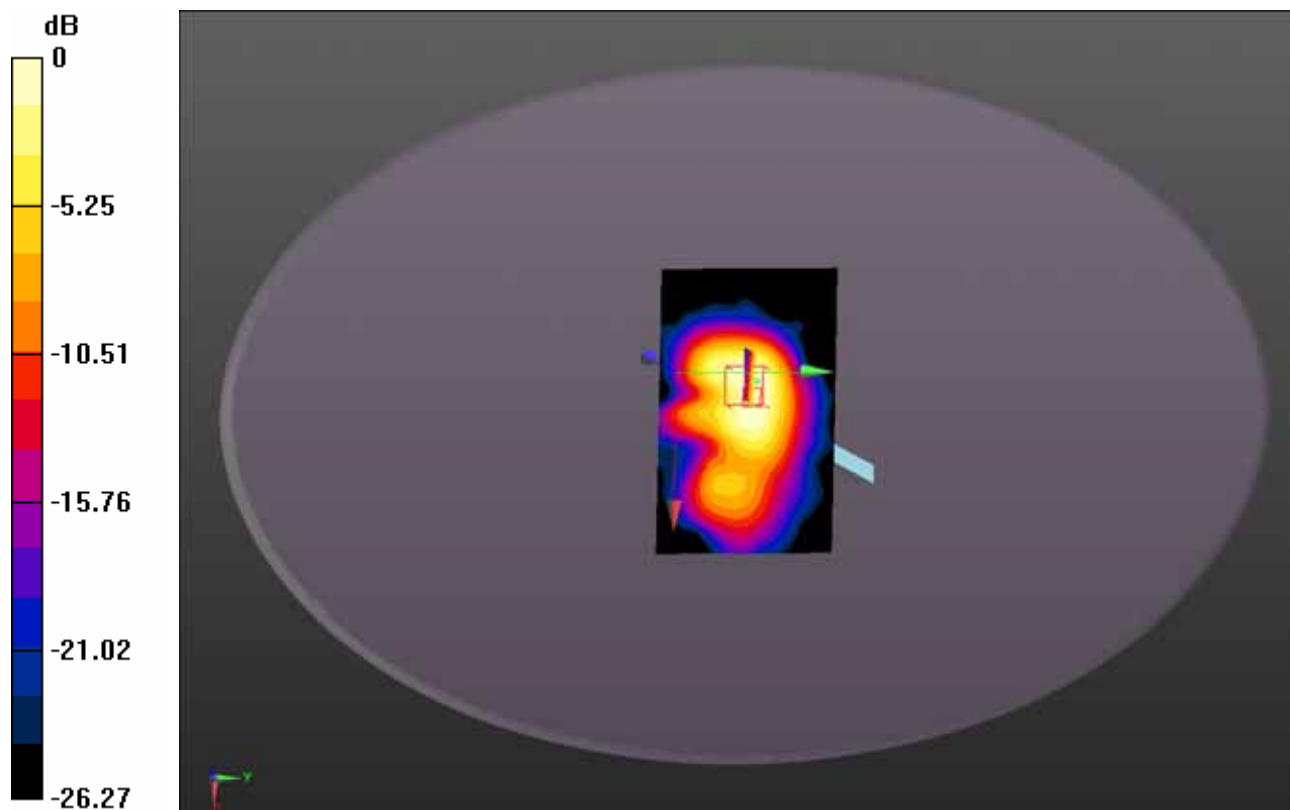

0 dB = 0.430mW/g

Right 11b CH6

Date/Time: 16/12/2011 10:35:37

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/ Right /Area Scan (121x71x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.390 mW/g


Configuration/ Right /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 10.696 V/m; Power Drift = 0.18 dB

Peak SAR (extrapolated) = 0.703 W/kg

SAR(1 g) = 0.325 mW/g; SAR(10 g) = 0.139 mW/g

Maximum value of SAR (measured) = 0.376 mW/g

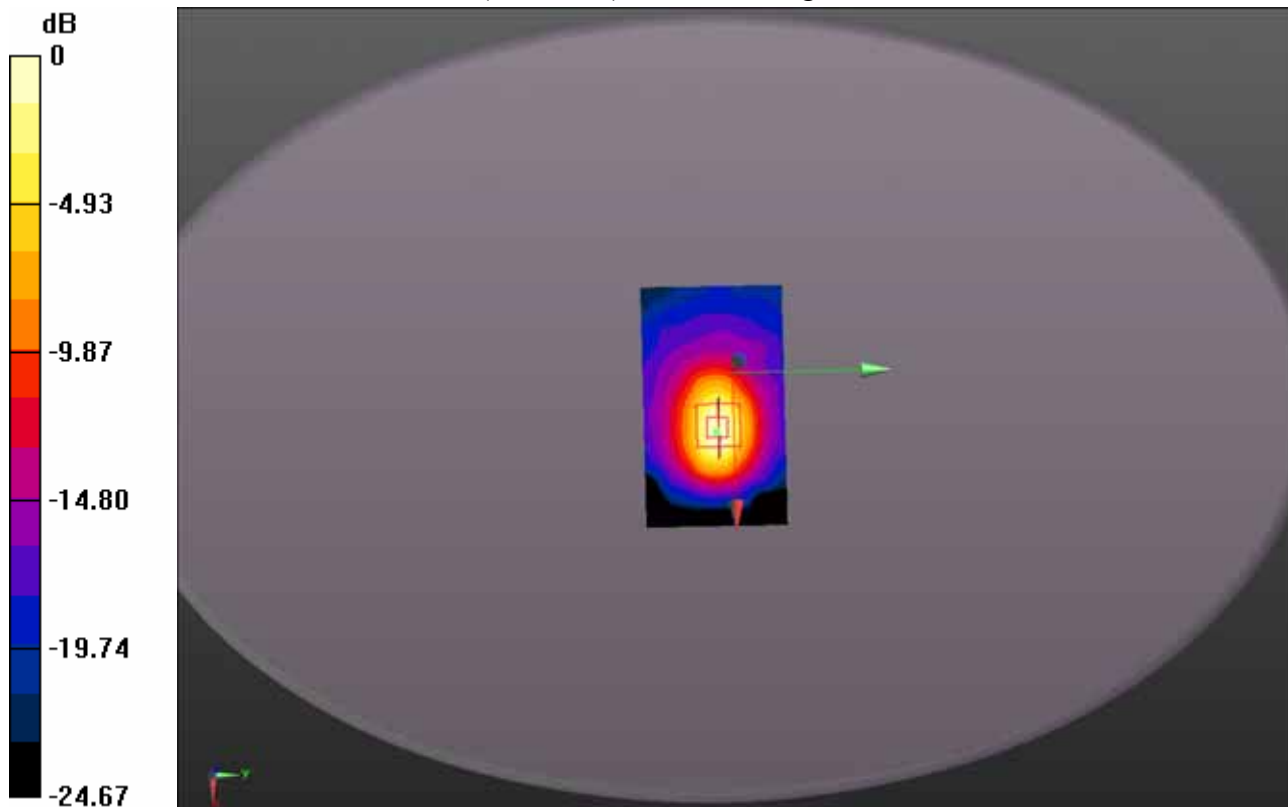

0 dB = 0.380mW/g

Top 11b CH6

Date/Time: 16/12/2011 11:04:52

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Top/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.513 mW/g


Configuration/Top/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 9.063 V/m; Power Drift = -0.07 dB


Peak SAR (extrapolated) = 1.056 W/kg

SAR(1 g) = 0.449 mW/g; SAR(10 g) = 0.191 mW/g

Maximum value of SAR (measured) = 0.516 mW/g

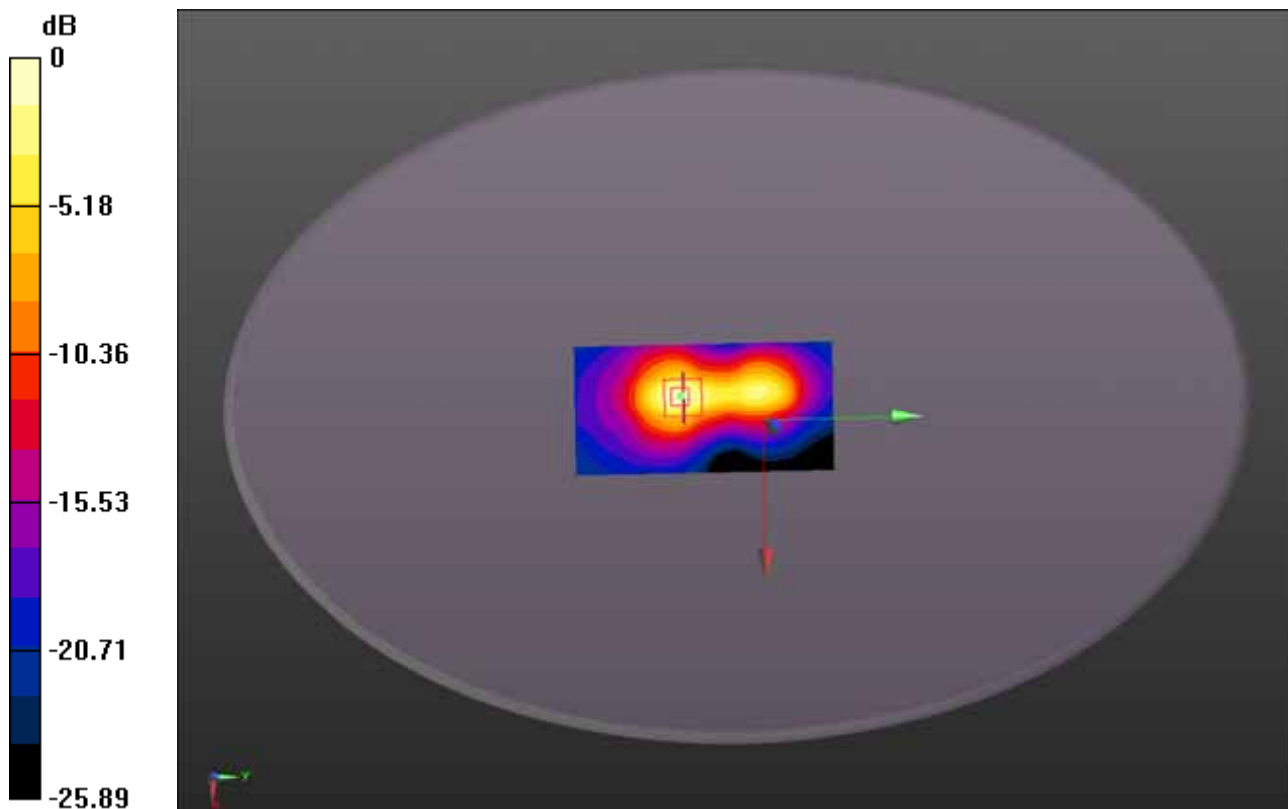

0 dB = 0.520mW/g

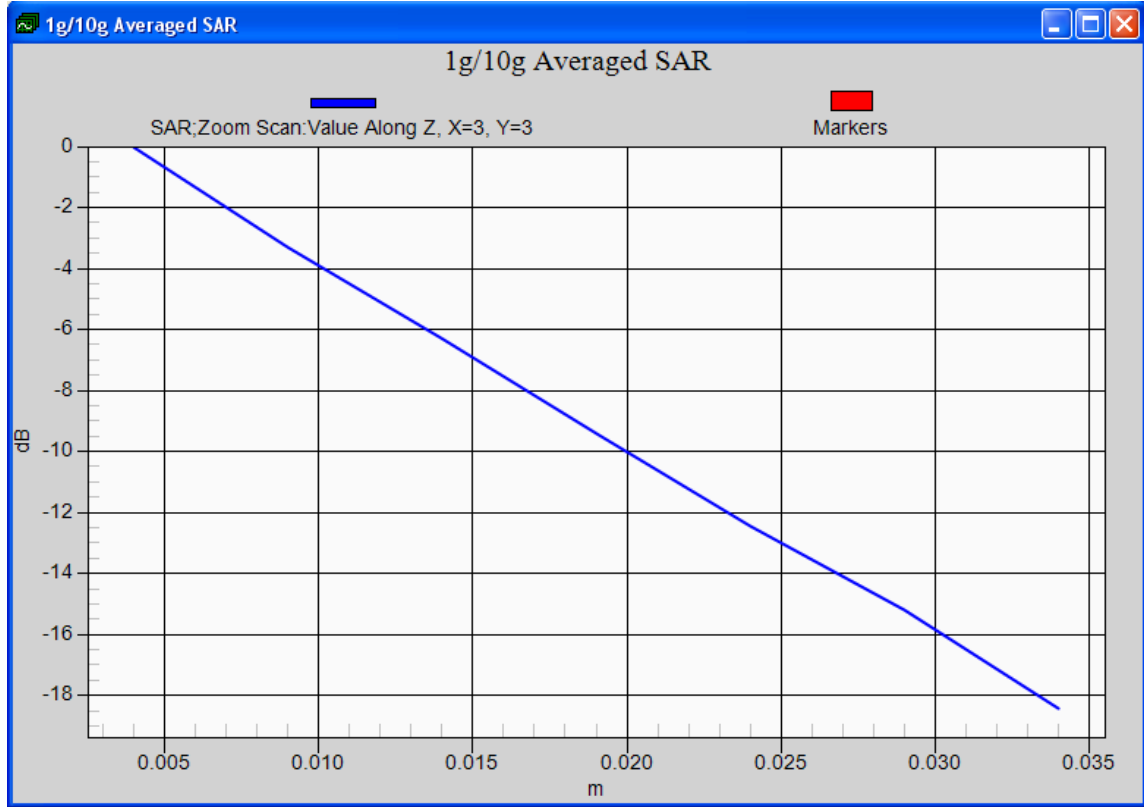

Front 11g CH1

Date/Time: 16/12/2011 11:36:19

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2412 MHz; Medium parameters used (interpolated): $f = 2412$ MHz; $\sigma = 1.968$ mho/m; $\epsilon_r = 50.861$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASYS2, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Front/Area Scan (161x101x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 1.171 mW/g


Configuration/Front/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 16.303 V/m; Power Drift = 0.10 dB


Peak SAR (extrapolated) = 2.416 W/kg

SAR(1 g) = 0.995 mW/g; SAR(10 g) = 0.497 mW/g

Maximum value of SAR (measured) = 1.044 mW/g

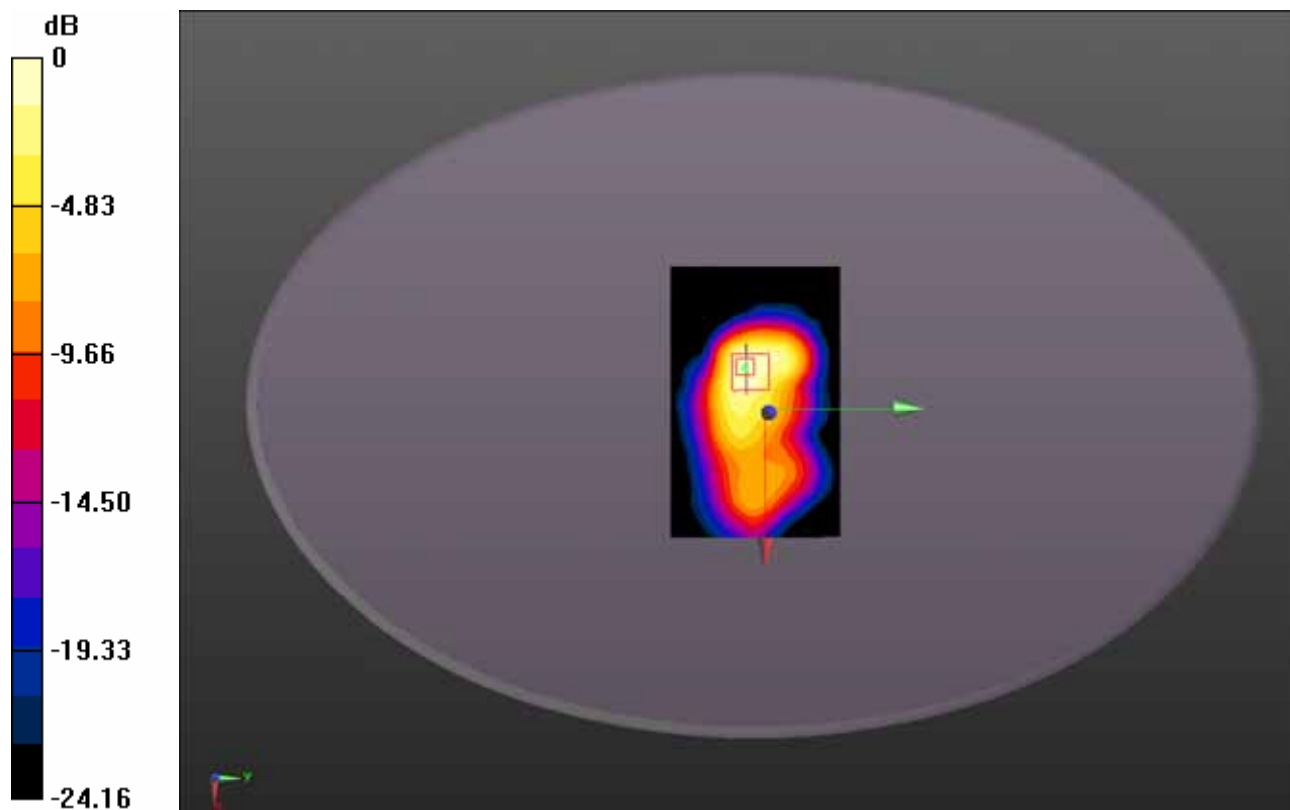

0 dB = 1.040mW/g

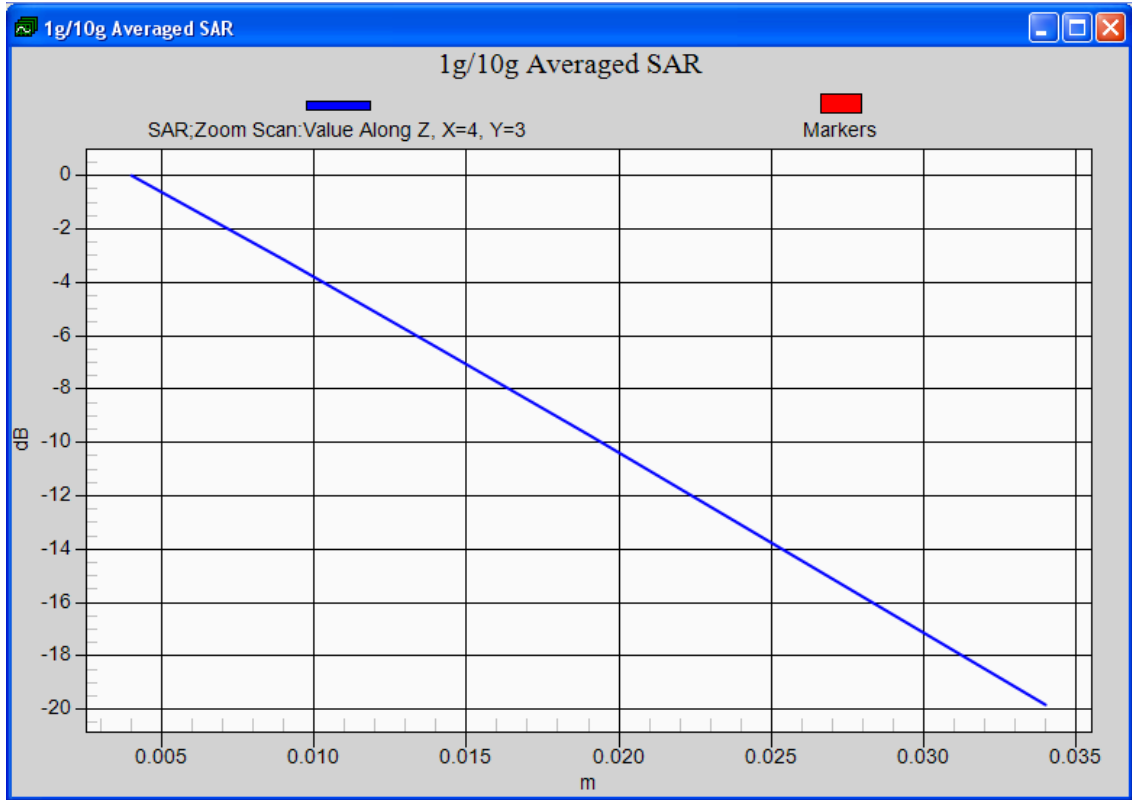

Front 11g CH6

Date/Time: 16/12/2011 12:08:25

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Front/Area Scan (161x101x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 1.160 mW/g


Configuration/Front/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 16.599 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 2.217 W/kg

SAR(1 g) = 0.939 mW/g; SAR(10 g) = 0.461 mW/g

Maximum value of SAR (measured) = 1.017 mW/g

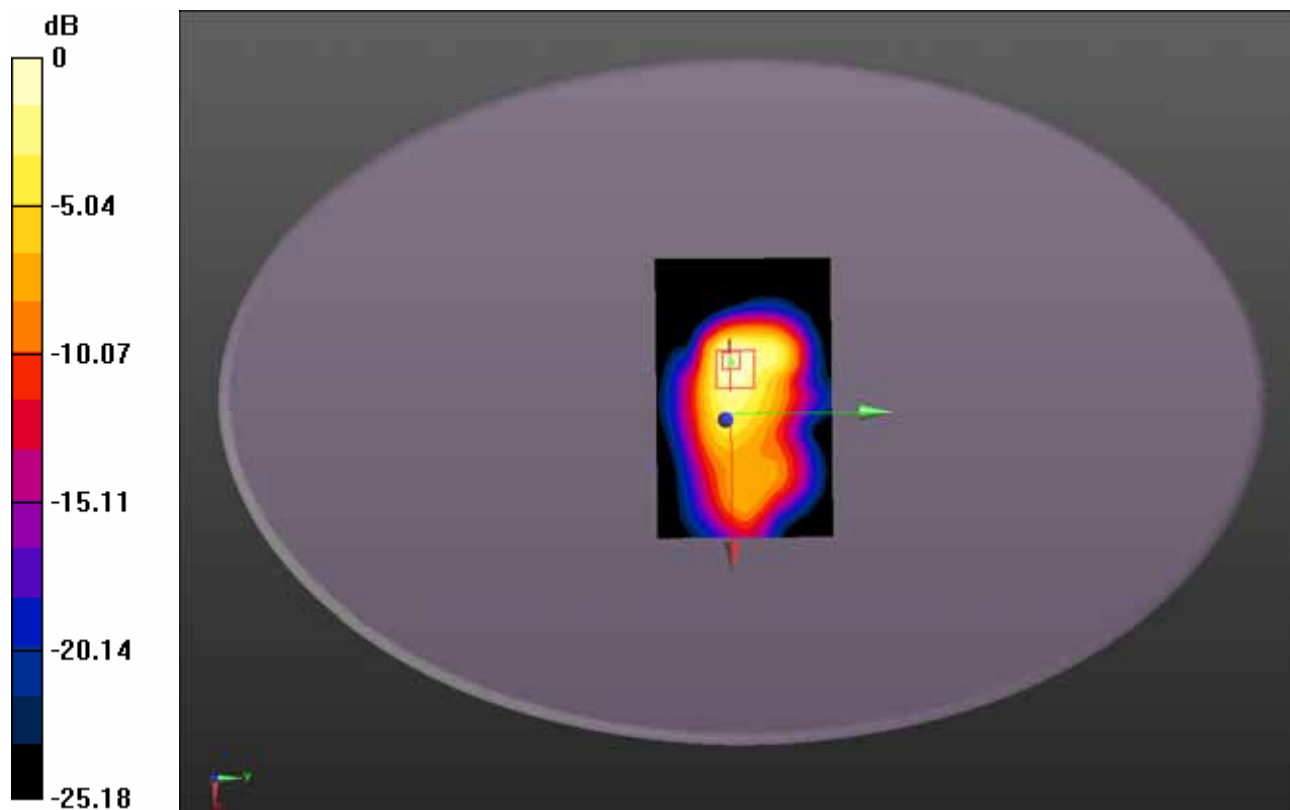

0 dB = 1.020mW/g

Front 11g CH11

Date/Time: 16/12/2011 12:37:39

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2462 MHz; Medium parameters used (interpolated): $f = 2462$ MHz; $\sigma = 2.048$ mho/m; $\epsilon_r = 50.622$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Front/Area Scan (161x101x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.922 mW/g


Configuration/Front/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 14.658 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 1.877 W/kg

SAR(1 g) = 0.761 mW/g; SAR(10 g) = 0.359 mW/g

Maximum value of SAR (measured) = 0.831 mW/g

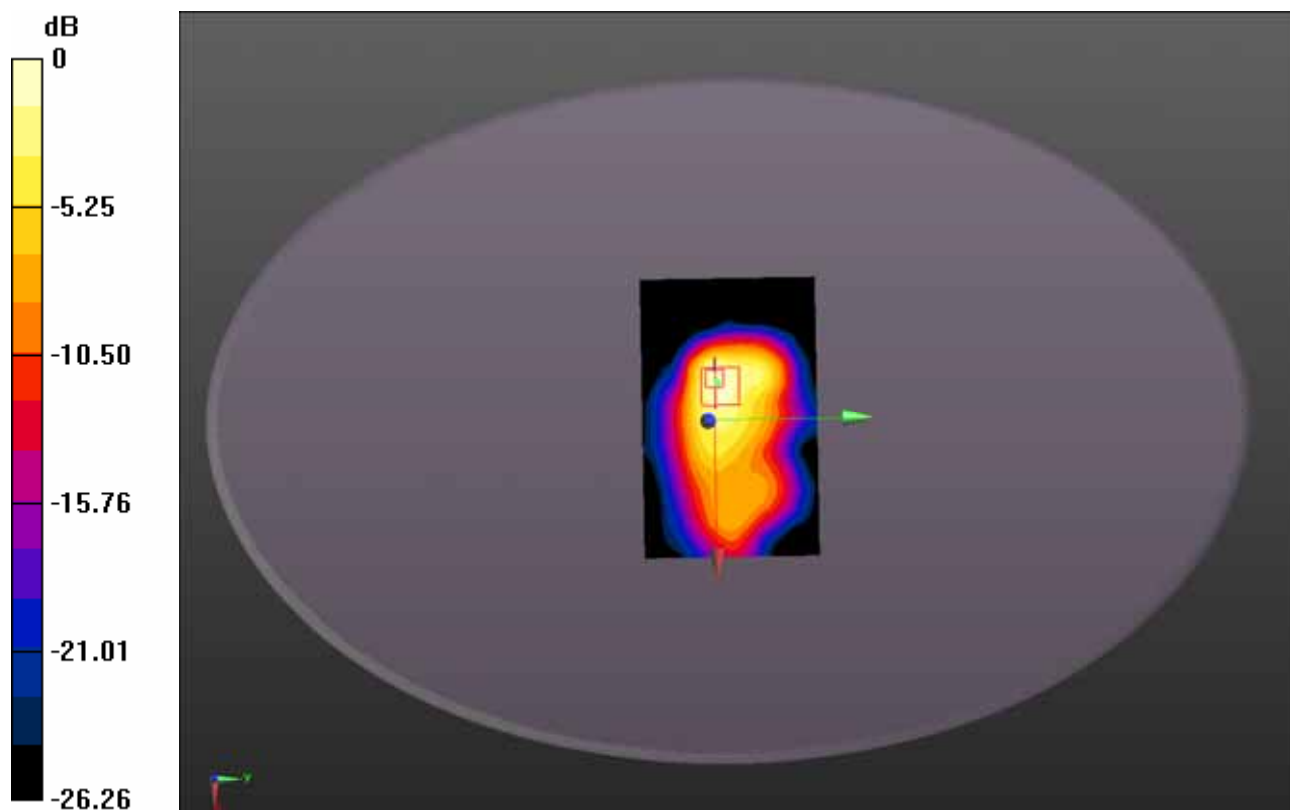

0 dB = 0.830mW/g

Back 11g CH6

Date/Time: 16/12/2011 12:37:39

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Back/Area Scan (181x121x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.994 mW/g


Configuration/Back/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 22.098 V/m; Power Drift = -0.16 dB

Peak SAR (extrapolated) = 1.808 W/kg

SAR(1 g) = 0.783 mW/g; SAR(10 g) = 0.404 mW/g

Maximum value of SAR (measured) = 1.011 mW/g

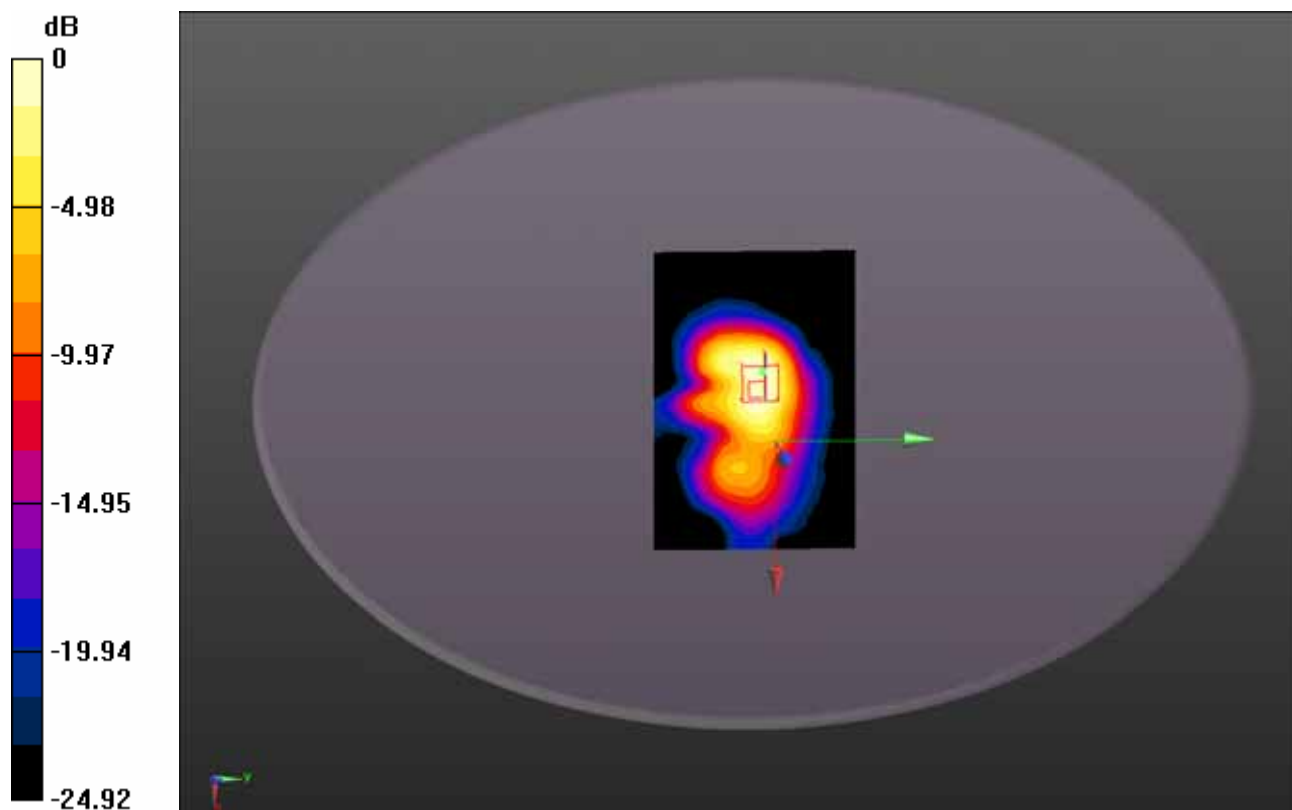

0 dB = 1.010mW/g

Right 11g CH6

Date/Time: 16/12/2011 13:05:45

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/ Right /Area Scan (121x71x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.813 mW/g


Configuration/ Right /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 14.649 V/m; Power Drift = 0.17 dB

Peak SAR (extrapolated) = 1.711 W/kg

SAR(1 g) = 0.644 mW/g; SAR(10 g) = 0.274 mW/g

Maximum value of SAR (measured) = 0.766 mW/g

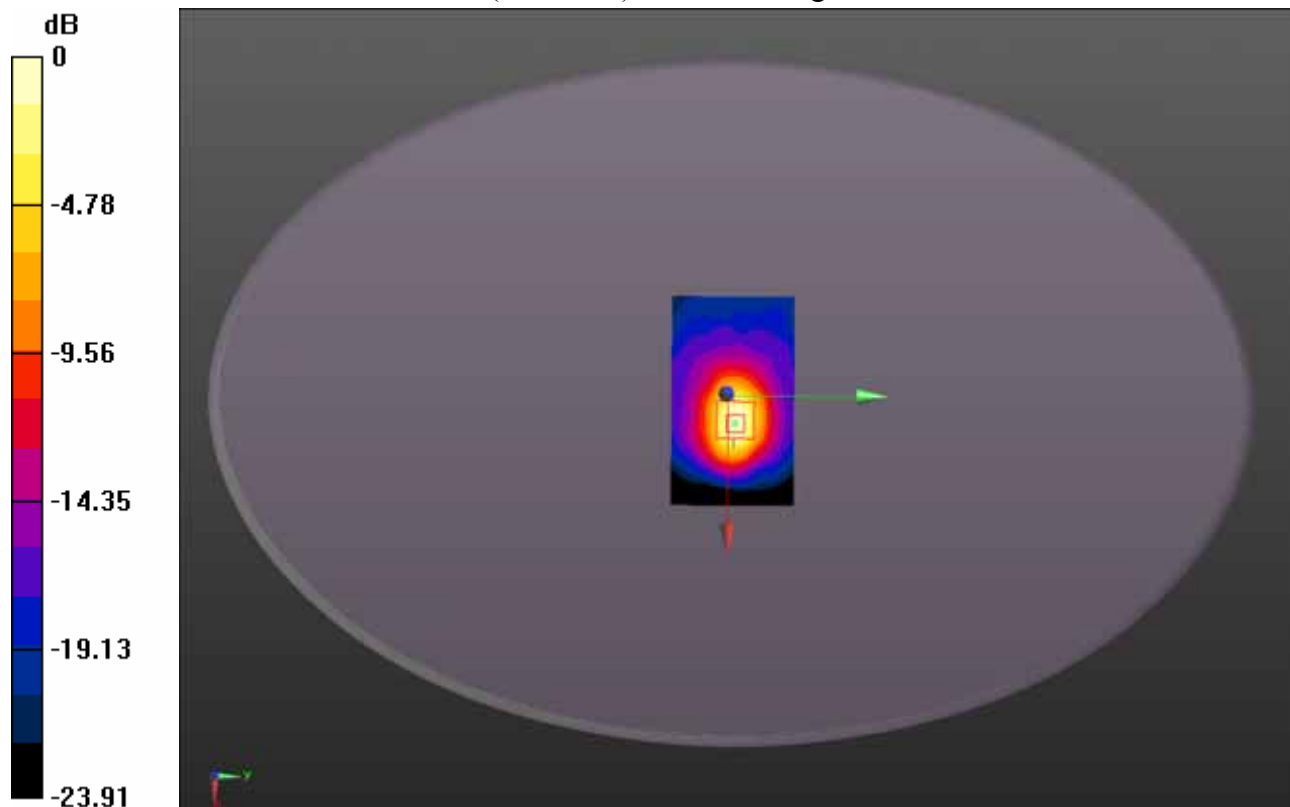

0 dB = 0.770mW/g

Top 11g CH1

Date/Time: 16/12/2011 13:36:05

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2412 MHz; Medium parameters used (interpolated): $f = 2412$ MHz; $\sigma = 1.968$ mho/m; $\epsilon_r = 50.861$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Top/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 1.177 mW/g


Configuration/Top/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 13.539 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 2.302 W/kg

SAR(1 g) = 0.991 mW/g; SAR(10 g) = 0.422 mW/g

Maximum value of SAR (measured) = 1.153 mW/g

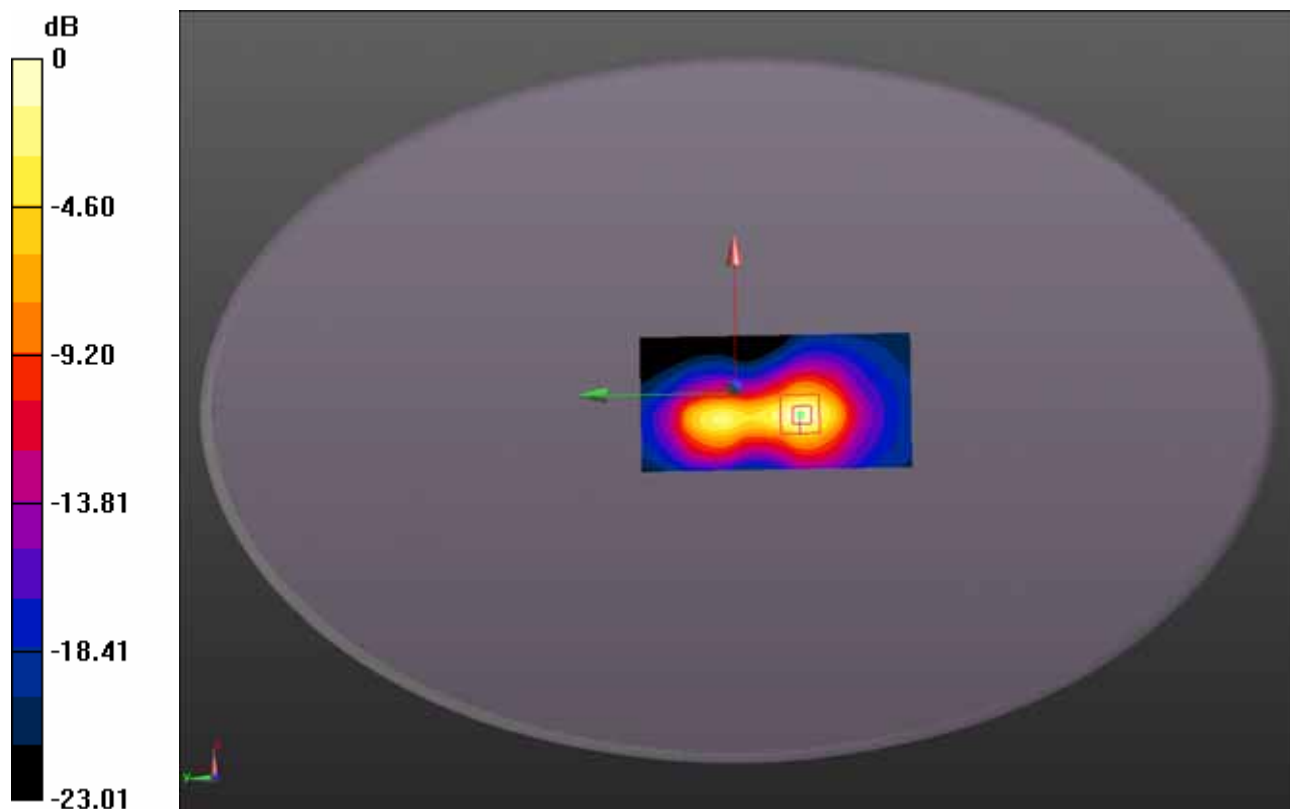

0 dB = 1.150mW/g

Top-2 11g CH1

Date/Time: 10/02/2012 14:05:15

DUT: TI-Nspire Navigator Access Point

M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2412MHz

Medium parameters used (interpolated): $f = 2412$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³ ; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: xxxx
- Measurement SW: DASY52, Version 52.8 (0); SEMCAD X Version 14.6.4 (4989)

Configuration/Top_Hot Post-2/Area Scan (41x41x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.683 mW/g

Configuration/ Top_Hot Post-2/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 15.802 V/m; Power Drift = 0.18 dB

Peak SAR (extrapolated) = 1.4870

SAR(1 g) = 0.707 mW/g; SAR(10 g) = 0.329 mW/g

Maximum value of SAR (measured) = 0.842 mW/g

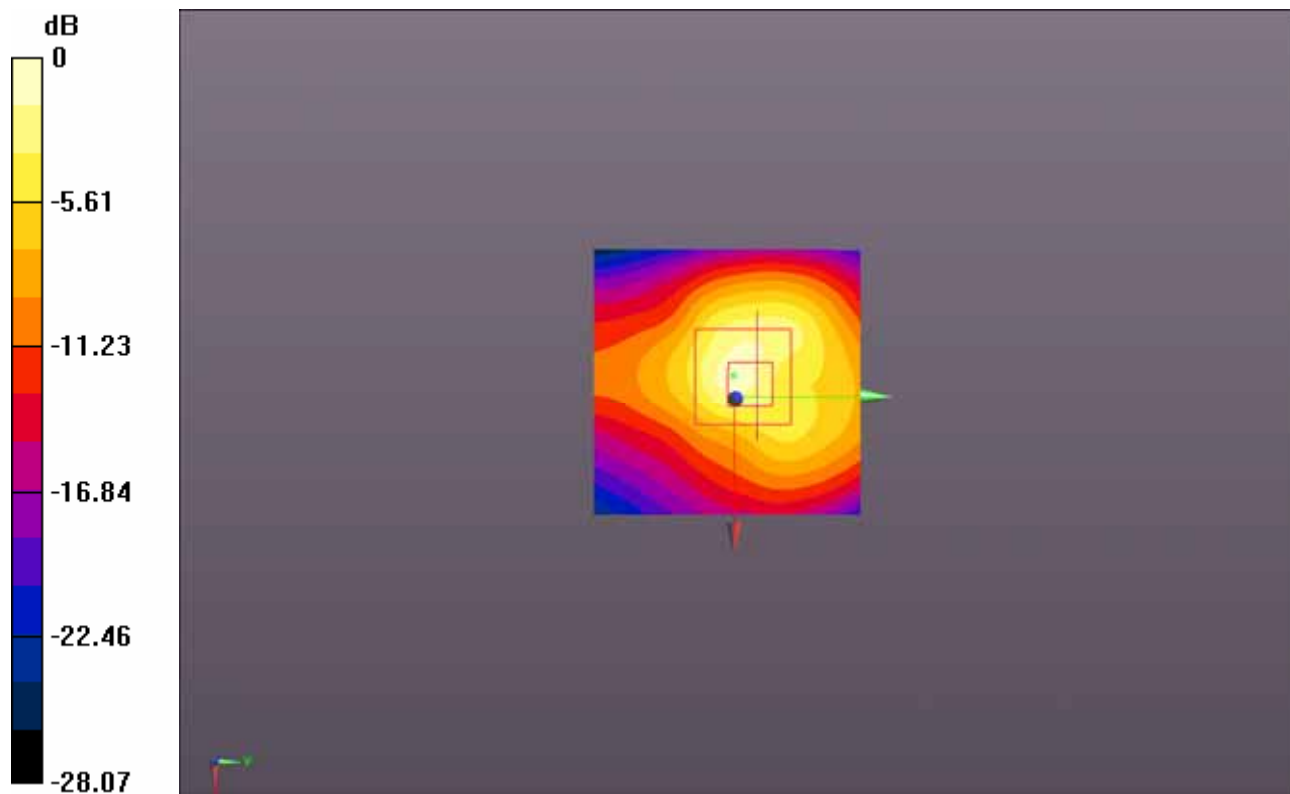

0 dB = 0.840mW/g = -1.51 dB mW/g

Top 11g CH6

Date/Time: 16/12/2011 14:07:13

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASYS2, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Top/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.971 mW/g


Configuration/Top/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 12.157 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 2.094 W/kg

SAR(1 g) = 0.851 mW/g; SAR(10 g) = 0.360 mW/g

Maximum value of SAR (measured) = 0.973 mW/g

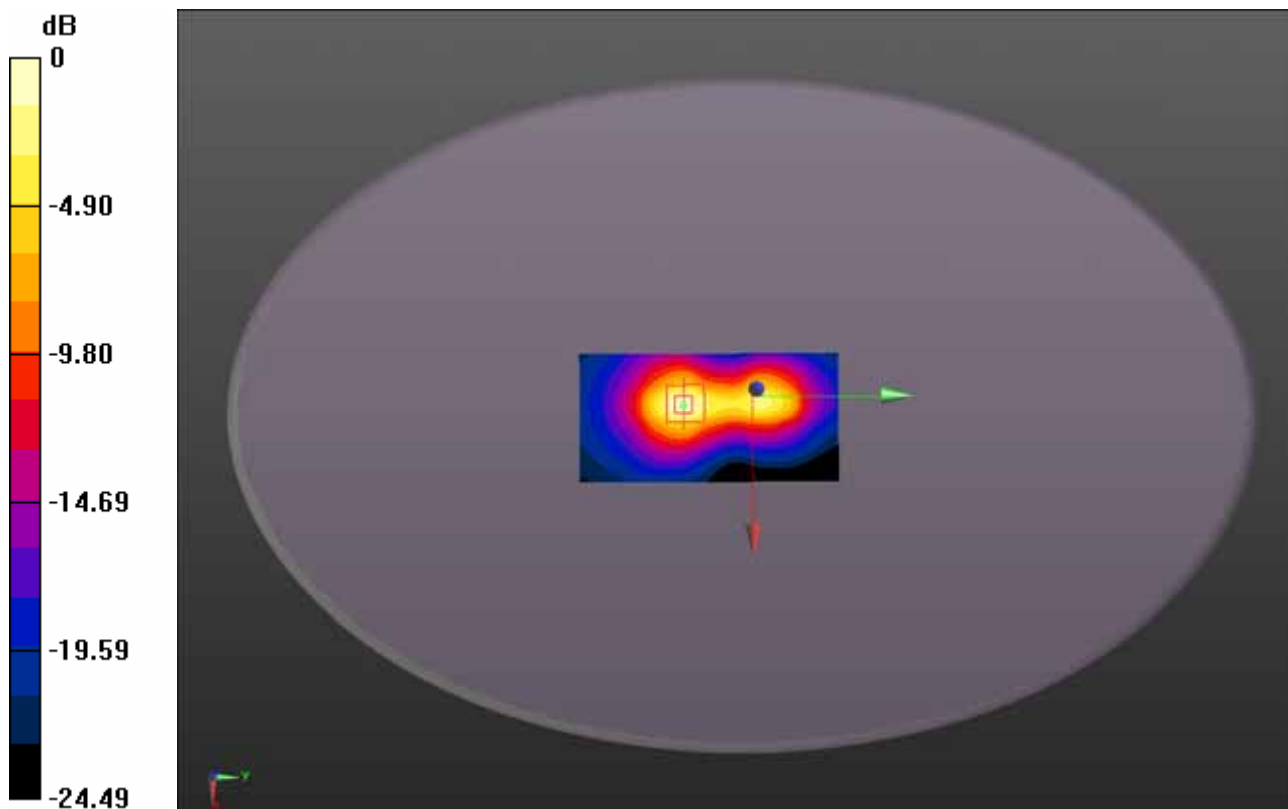

0 dB = 0.970mW/g

Top 11g CH11

Date/Time: 16/12/2011 14:37:48

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2462 MHz; Medium parameters used (interpolated): $f = 2462$ MHz; $\sigma = 2.048$ mho/m; $\epsilon_r = 50.622$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Top/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.671 mW/g


Configuration/Top/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 12.398 V/m; Power Drift = -0.14 dB

Peak SAR (extrapolated) = 1.438 W/kg

SAR(1 g) = 0.614 mW/g; SAR(10 g) = 0.262 mW/g

Maximum value of SAR (measured) = 0.711 mW/g

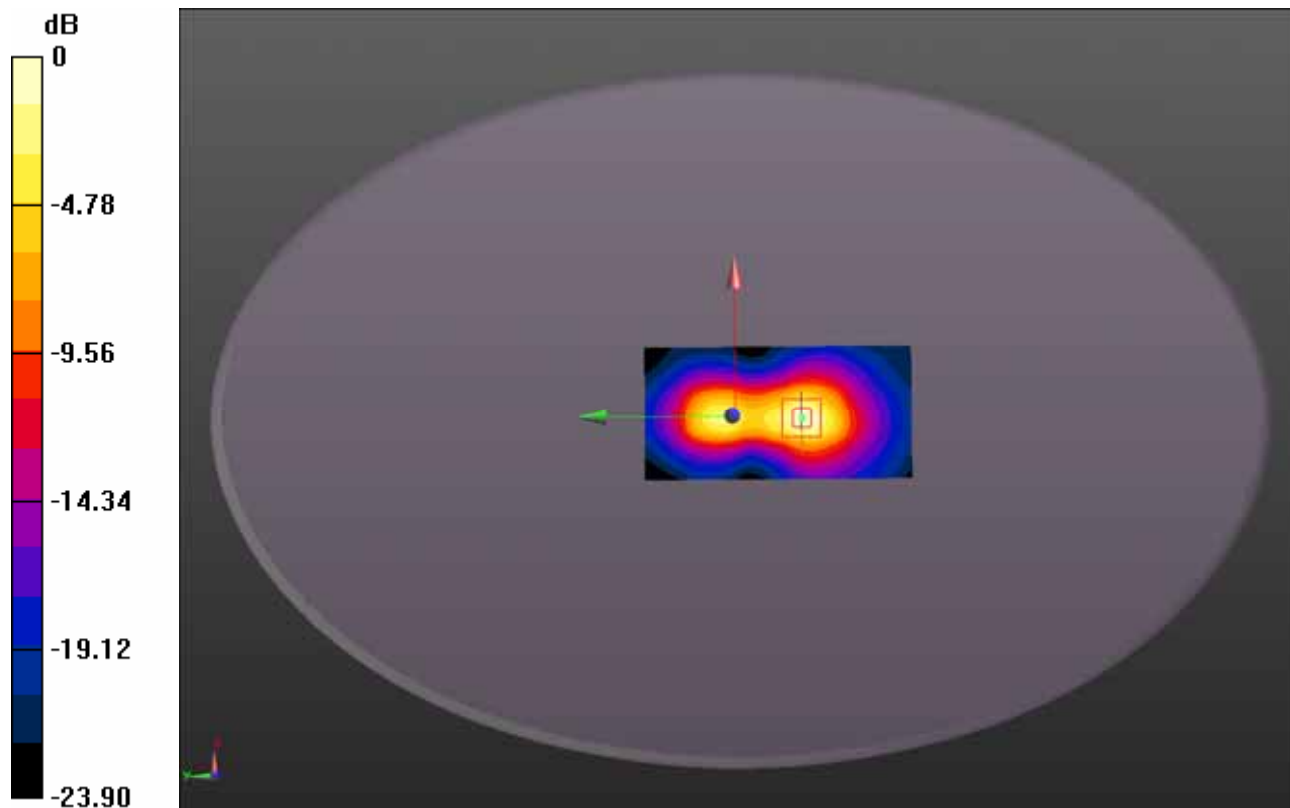

0 dB = 0.710mW/g

Front 11nHT20 CH6

Date/Time: 16/12/2011 15:08:33

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Front/Area Scan (161x101x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.601 mW/g


Configuration/Front/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 12.044 V/m; Power Drift = 0.12 dB


Peak SAR (extrapolated) = 1.092 W/kg

SAR(1 g) = 0.477 mW/g; SAR(10 g) = 0.245 mW/g

Maximum value of SAR (measured) = 0.572 mW/g

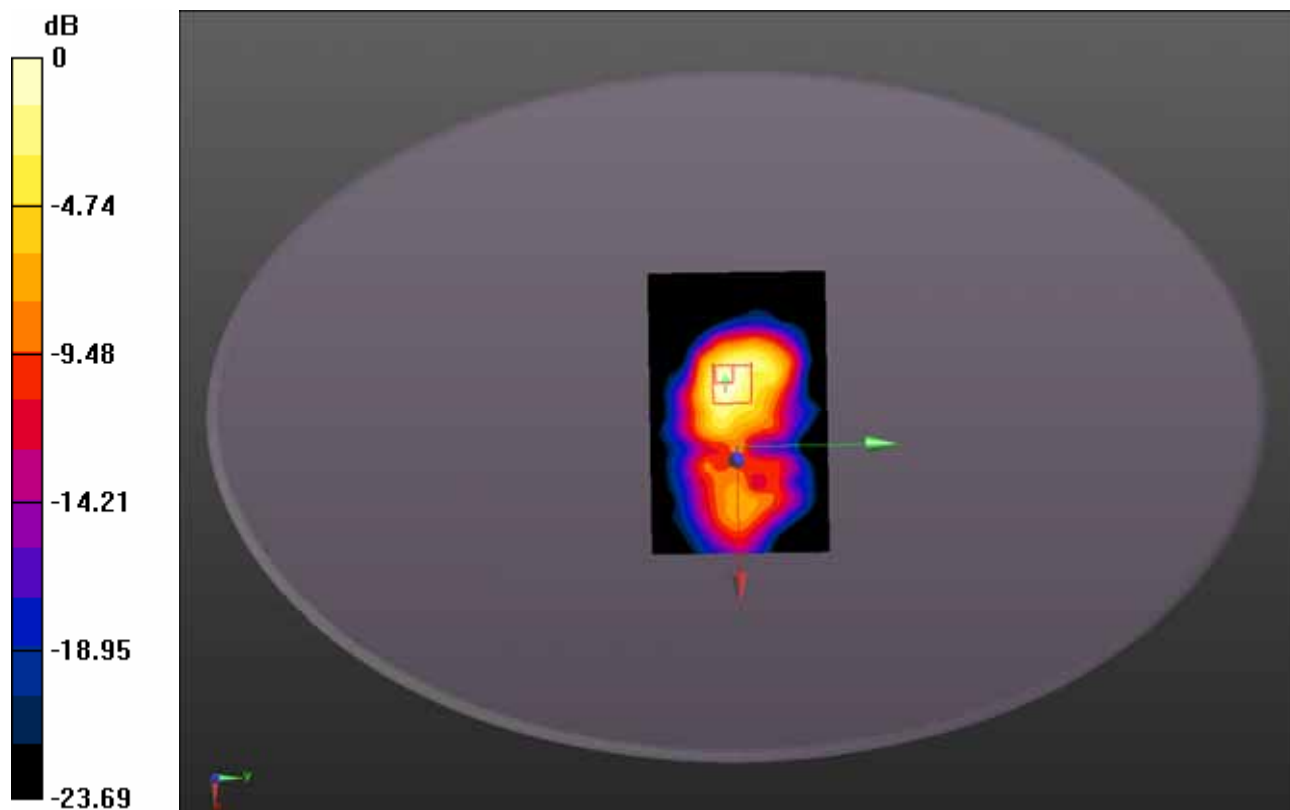

0 dB = 0.570mW/g

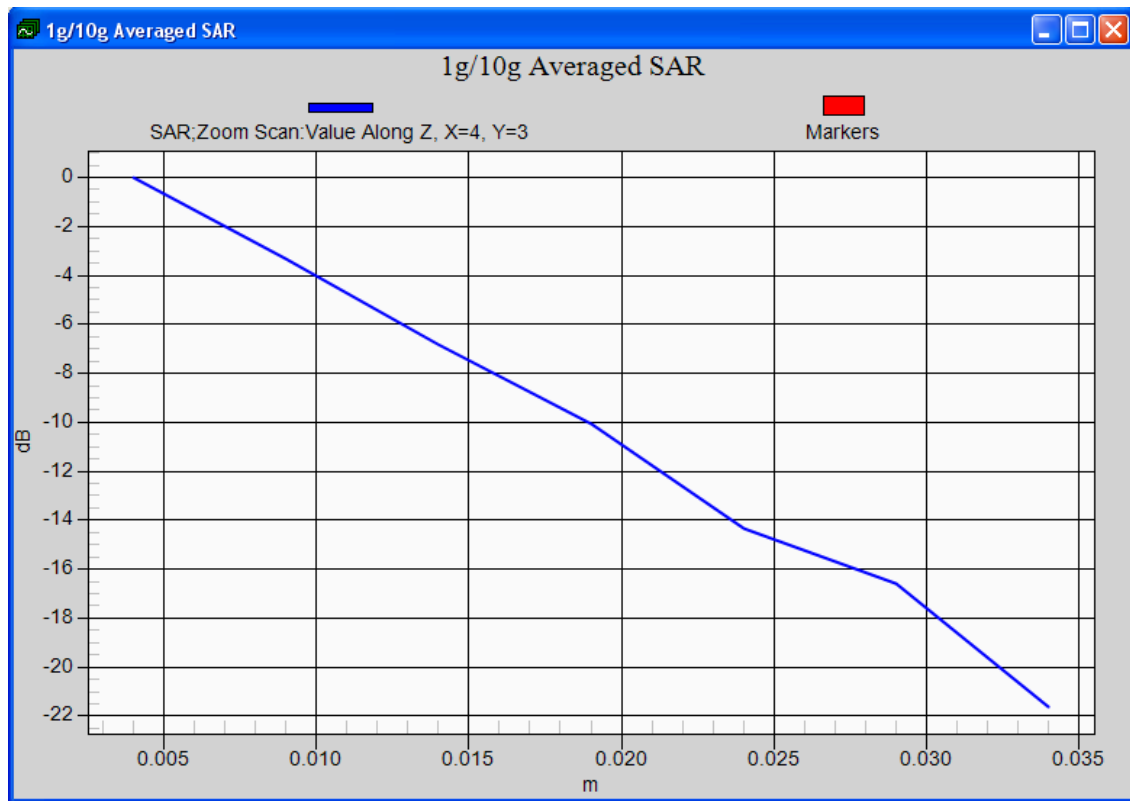

Back 11nHT20 CH6

Date/Time: 16/12/2011 15:40:09

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: xxxx
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Back/Area Scan (161x101x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.434 mW/g


Configuration/Back/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 14.749 V/m; Power Drift = -0.16 dB

Peak SAR (extrapolated) = 0.824 W/kg

SAR(1 g) = 0.398 mW/g; SAR(10 g) = 0.209 mW/g

Maximum value of SAR (measured) = 0.439 mW/g

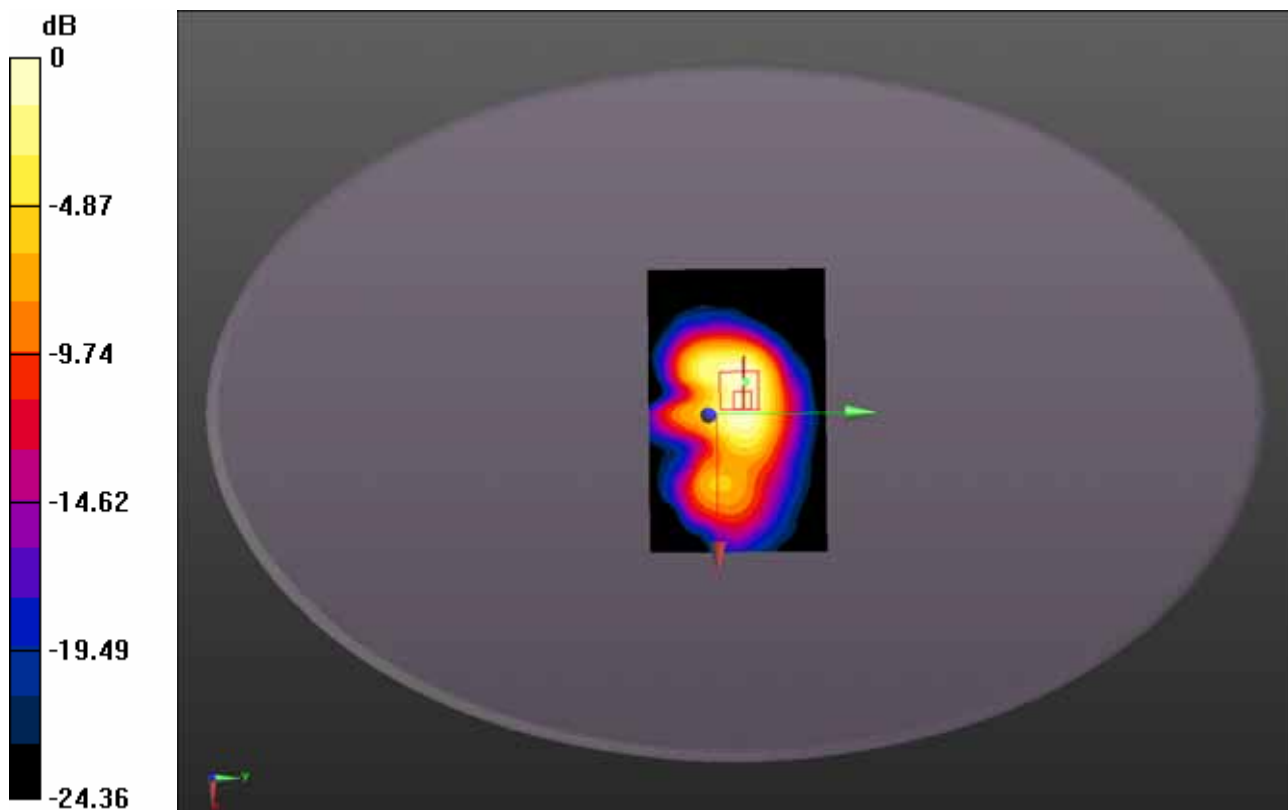

0 dB = 0.440mW/g

Right 11nHT20 CH6

Date/Time: 16/12/2011 16:09:27

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/ Right /Area Scan (121x71x1): Measurement grid:

dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.305 mW/g

Configuration/Right/Zoom Scan (7x7x7)/Cube 0: Measurement grid:


dx=5mm, dy=5mm, dz=5mm

Reference Value = 9.967 V/m; Power Drift = 0.18 dB

Peak SAR (extrapolated) = 0.640 W/kg

SAR(1 g) = 0.218 mW/g; SAR(10 g) = 0.093 mW/g

Maximum value of SAR (measured) = 0.319 mW/g

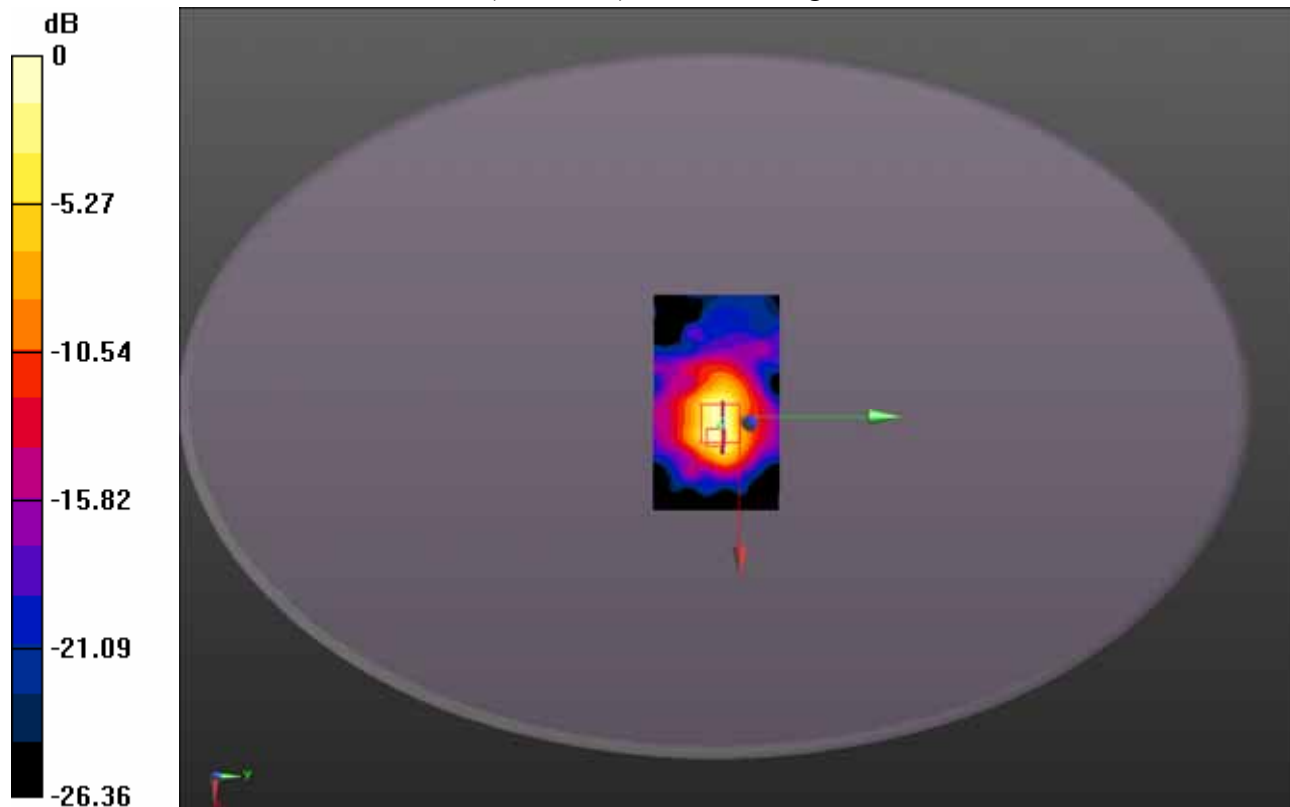

0 dB = 0.320mW/g

Top 11nHT20 CH6

Date/Time: 16/12/2011 16:40:36

DUT: TI-Nspire Navigator Access Point M/N: TINAVAP2

Communication System: IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps); Frequency: 2437 MHz; Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.013$ mho/m; $\epsilon_r = 50.739$; $\rho = 1000$ kg/m³; PAR= 0 dB; Crest factor=1; Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3139; ConvF(4, 4, 4); Calibrated: 23/03/2011
- Electronics: DAE4 Sn899; Calibrated: 18/03/2011
- Phantom: ELI 4.0; Type: QDOVA001BA;
- Measurement SW: DASY52, Version 52.6 (2); SEMCAD X Version 14.4.5 (3634)

Configuration/Top/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.220 mW/g


Configuration/Top/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 4.200 V/m; Power Drift = 0.17 dB

Peak SAR (extrapolated) = 1.971 W/kg

SAR(1 g) = 0.405 mW/g; SAR(10 g) = 0.123 mW/g

Maximum value of SAR (measured) = 0.459 mW/g

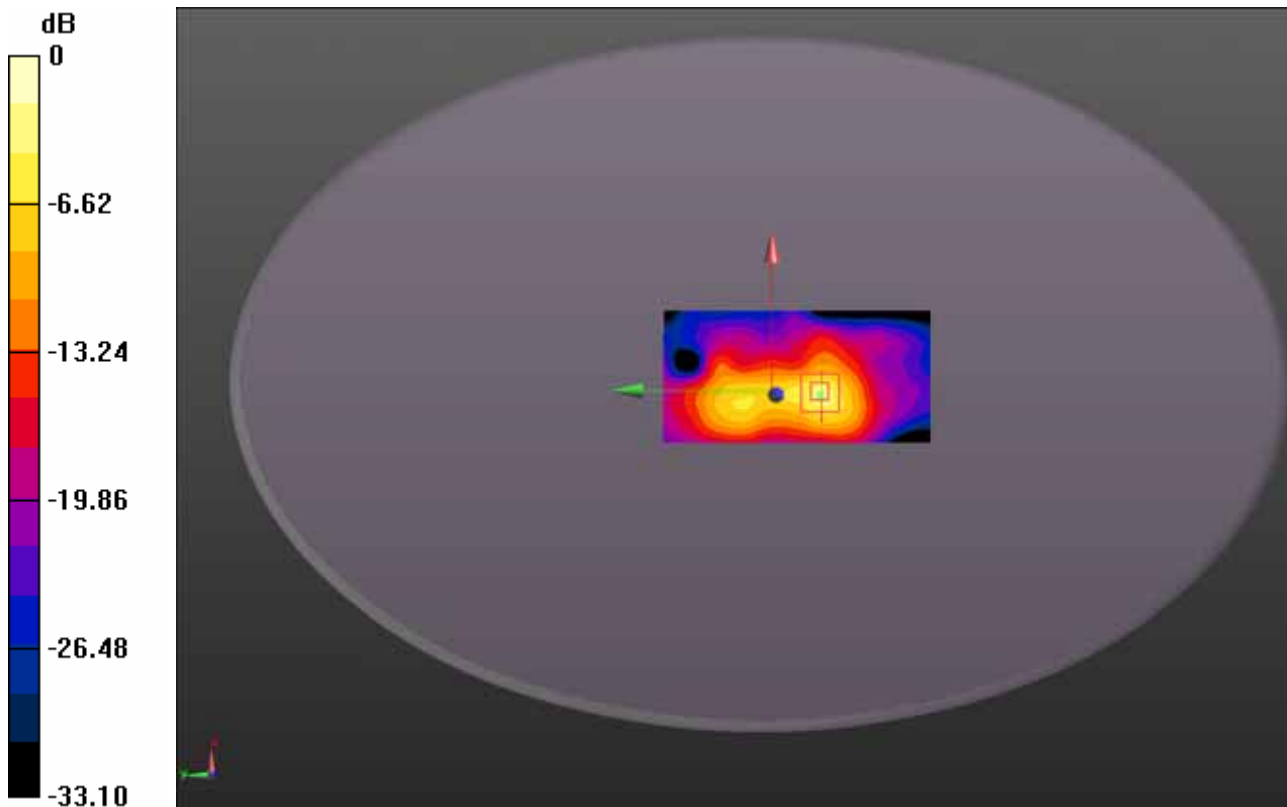

0 dB = 0.460mW/g

11. DIPOLE CALIBRATION CERTIFICATE

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.72 mho/m ± 6 %
Head TSL temperature during test	(21.3 ± 0.2) °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.1 mW / g
SAR normalized	normalized to 1W	52.4 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	53.3 mW /g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.12 mW / g
SAR normalized	normalized to 1W	24.5 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.6 mW /g ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.5 ± 6 %	1.92 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.8 mW / g
SAR normalized	normalized to 1W	51.2 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	51.3 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.86 mW / g
SAR normalized	normalized to 1W	23.4 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	23.4 mW / g ± 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.6 Ω + 3.6 j Ω
Return Loss	- 25.0 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.3 Ω + 4.9 j Ω
Return Loss	- 26.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.160 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	April 23, 2010

DASY5 Validation Report for Head TSL

Date/Time: 22.03.2011 14:07:14

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:862

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used: $f = 2450 \text{ MHz}$; $\sigma = 1.72 \text{ mho/m}$; $\epsilon_r = 38.8$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY52, V52.6.2 Build (424)
- Postprocessing SW: SEMCAD X, V14.4.4 Build (2829)


Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.7 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 26.808 W/kg

SAR(1 g) = 13.1 mW/g; SAR(10 g) = 6.12 mW/g

Maximum value of SAR (measured) = 16.641 mW/g

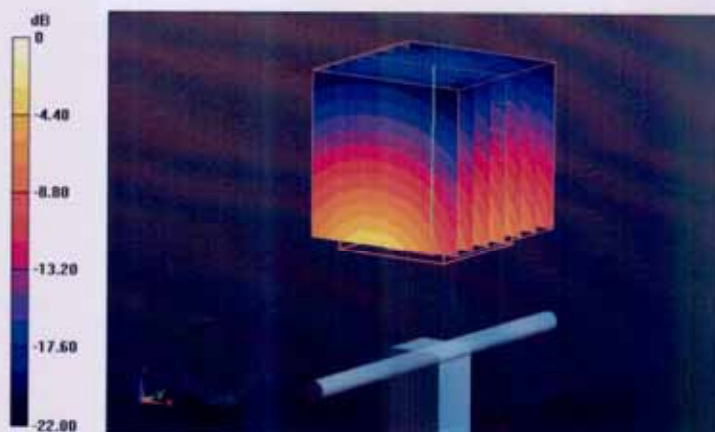


0 dB = 16.640mW/g

Impedance Measurement Plot for Head TSL


22 Mar 2011 10:23:53
 CH1 S11 1 U FS \Re 54.645 Ω 3.6445 Ω 236.75 pF 2 450.000 000 MHz

De l
 CA
 Avg
 16
 †

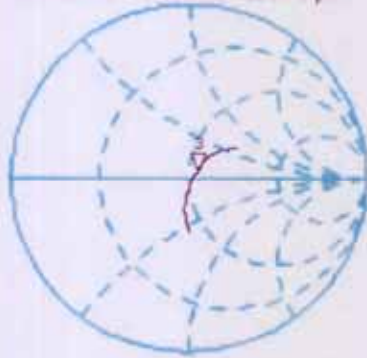

CH2 S11 LOG 5 dB/REF -20 dB \Re -24.974 dB 2 450.000 000 MHz

CA
 Avg
 16
 †

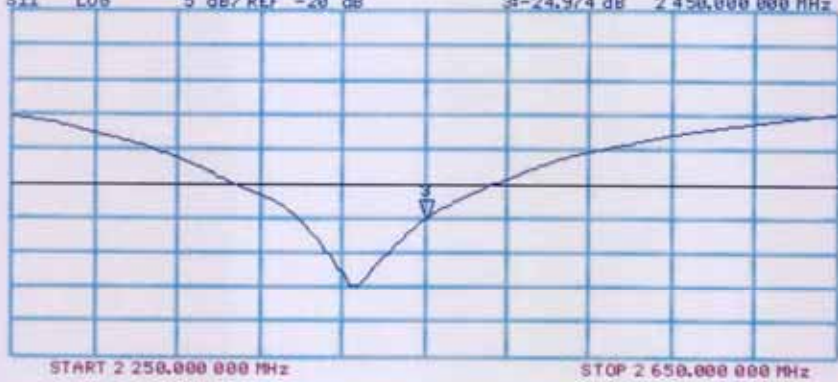

DASY5 Validation Report for Body TSL

Date/Time: 21.03.2011 14:22:38

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:862

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U12 BB

Medium parameters used: $f = 2450 \text{ MHz}$; $\sigma = 1.92 \text{ mho/m}$; $\epsilon_r = 51.5$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.31, 4.31, 4.31); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY52, V52.6.2 Build (424)
- Postprocessing SW: SEMCAD X, V14.4.4 Build (2829)


Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.402 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 27.156 W/kg


SAR(1 g) = 12.8 mW/g; SAR(10 g) = 5.86 mW/g

Maximum value of SAR (measured) = 16.826 mW/g

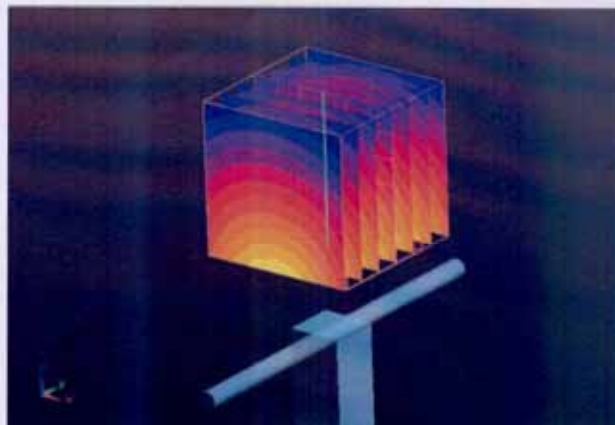

0 dB = 16.830mW/g

Impedance Measurement Plot for Body TSL

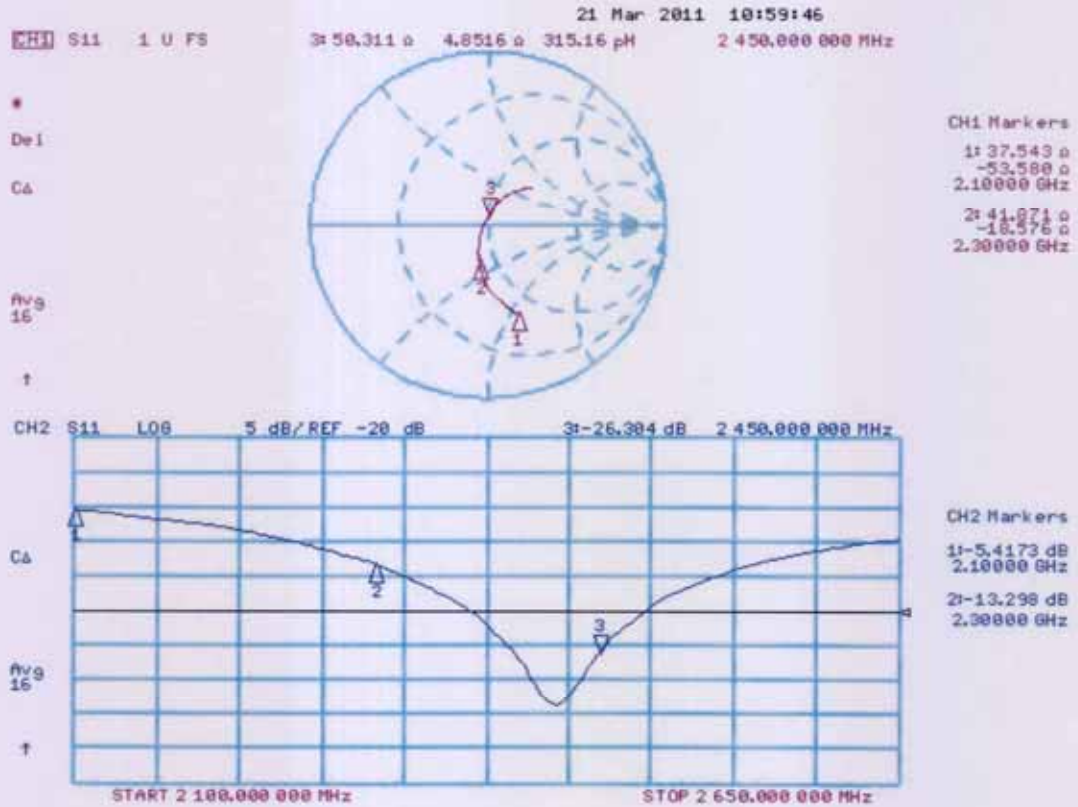

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Audix (Auden)**

Certificate No: **D2450V2-862_Mar11**

CALIBRATION CERTIFICATE

Object: **D2450V2 - SN: 862**

Calibration procedure(s): **QA CAL-05.v8
Calibration procedure for dipole validation kits**

Calibration date: **March 22, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37292783	06-Oct-10 (No. 217-01266)	Oct-11
Reference 20 dB Attenuator	SN: 5086 (20g)	30-Mar-10 (No. 217-01158)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe ES3DV3	SN: 3205	30-Apr-10 (No. ES3-3205_Apr10)	Apr-11
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

Calibrated by:	Name	Function	Signature
	Dimce Iliev	Laboratory Technician	
Approved by:	Name	Function	Signature
	Katja Pokovic	Technical Manager	

Issued: March 23, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

12. E-FIELD PROBES DIPOLE CALIBRATION CERTIFICATE

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Audix (Auden)**

Certificate No: **ES3-3139_Mar11**

CALIBRATION CERTIFICATE

Object **ES3DV3 - SN:3139**

Calibration procedure(s) **QA CAL-01.v7, QA CAL-23.v4, QA CAL-25.v3
Calibration procedure for dosimetric E-field probes**



Calibration date: **March 23, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	01-Apr-10 (No. 217-01136)	Apr-11
Power sensor E4412A	MY41495277	01-Apr-10 (No. 217-01136)	Apr-11
Power sensor E4412A	MY41498087	01-Apr-10 (No. 217-01136)	Apr-11
Reference 3 dB Attenuator	SN: S5054 (3c)	30-Mar-10 (No. 217-01159)	Mar-11
Reference 20 dB Attenuator	SN: S5086 (20b)	30-Mar-10 (No. 217-01161)	Mar-11
Reference 30 dB Attenuator	SN: S5129 (30b)	30-Mar-10 (No. 217-01160)	Mar-11
Reference Probe ES3DV2	SN: 3013	29-Dec-10 (No. ES3-3013_Dec10)	Dec-11
DAE4	SN: 654	23-Apr-10 (No. DAE4-654_Apr10)	Apr-11
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

	Name	Function	Signature
Calibrated by:	Claudio Leubler	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
			Issued: March 25, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization Θ	Θ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- **NORM_{x,y,z}:** Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- **NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- **DCP_{x,y,z}:** DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- **PAR:** PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- **A_{x,y,z}; B_{x,y,z}; C_{x,y,z}** are numerical linearization parameters in dB assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media.
- **VR:** VR is the validity range of the calibration related to the average diode voltage or DAE voltage in mV.
- **ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- **Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- **Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

ES3DV3 – SN:3139

March 23, 2011

Probe ES3DV3

SN:3139

Manufactured: February 12, 2007
Calibrated: March 23, 2011

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

ES3DV3-- SN:3139

March 23, 2011

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3139

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu V/(V/m)^2$) ^A	1.31	1.35	1.38	± 10.1 %
DCP (mV) ^B	104.0	99.4	101.7	

Modulation Calibration Parameters

UID	Communication System Name	PAR		A dB	B dB	C dB	VR mV	Unc ^C (k=2)
10000	CW	0.00	X	0.00	0.00	1.00	119.4	±2.5 %
			Y	0.00	0.00	1.00	114.8	
			Z	0.00	0.00	1.00	121.6	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^C Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ES3DV3- SN:3139

March 23, 2011

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3139

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
835	41.5	0.90	5.87	5.87	5.87	0.99	1.09	± 12.0 %
900	41.5	0.97	5.79	5.79	5.79	0.99	1.10	± 12.0 %
1810	40.0	1.40	4.94	4.94	4.94	0.99	1.13	± 12.0 %
2000	40.0	1.40	4.85	4.85	4.85	0.99	1.11	± 12.0 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

ES3DV3- SN:3139

March 23, 2011

DASY/EASY - Parameters of Probe: ES3DV3- SN:3139

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
835	55.2	0.97	5.83	5.83	5.83	0.99	1.17	± 12.0 %
900	55.0	1.05	5.76	5.76	5.76	0.99	1.15	± 12.0 %
1810	53.3	1.52	4.61	4.61	4.61	0.93	1.23	± 12.0 %
2000	53.3	1.52	4.45	4.45	4.45	0.80	1.28	± 12.0 %
2450	52.7	1.95	4.00	4.00	4.00	0.99	1.04	± 12.0 %


^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

ES3DV3-- SN:3139

March 23, 2011

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

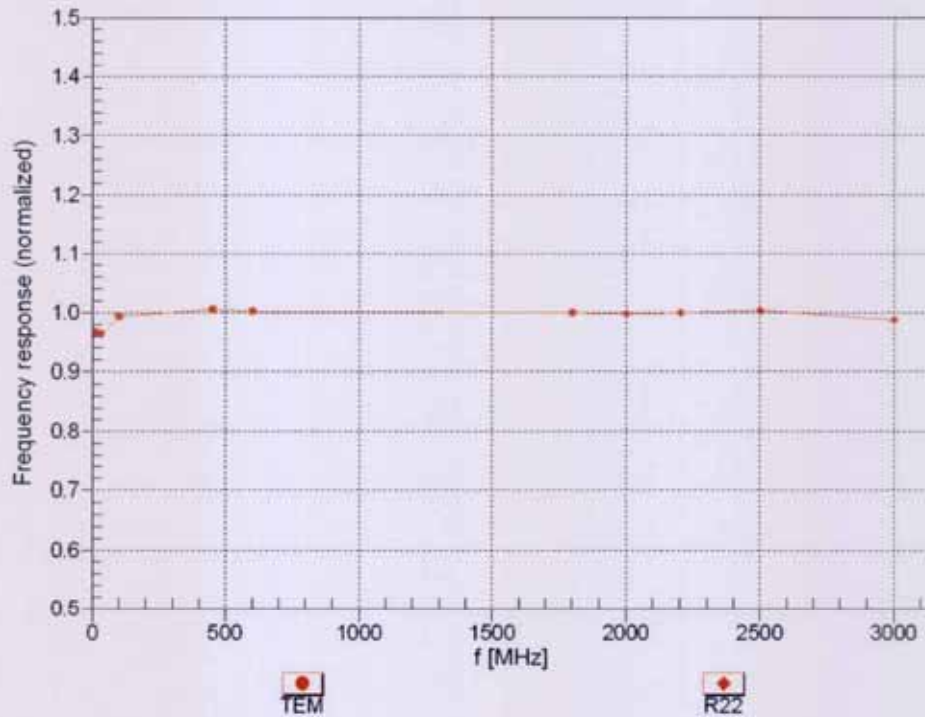


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

ES3DV3-SN:3139



March 23, 2011

Receiving Pattern (ϕ), $\theta = 0^\circ$

f=600 MHz, TEM

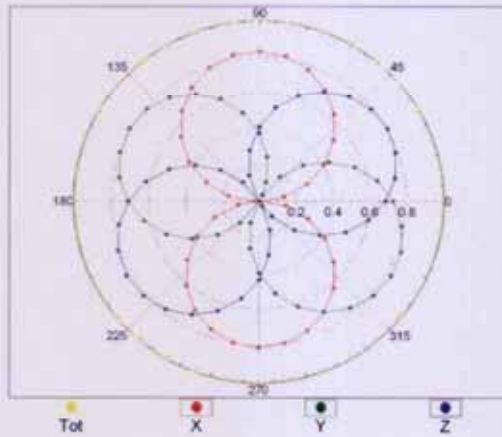

f=1800 MHz, R22

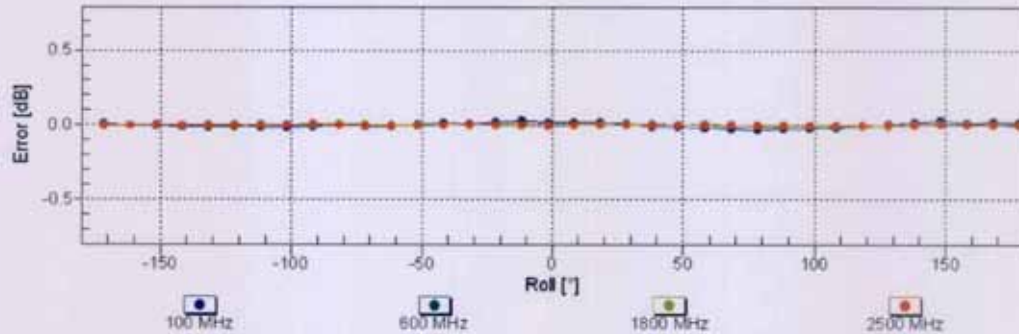
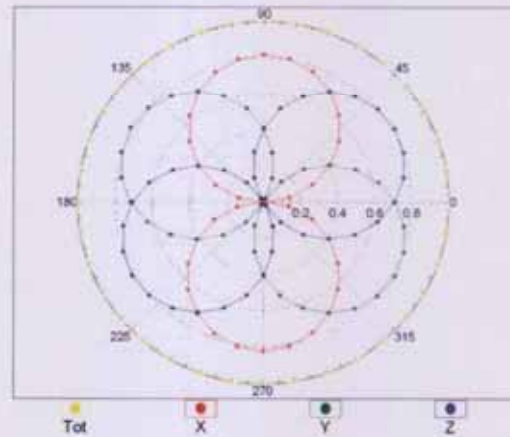


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

ES3DV3- SN:3139

March 23, 2011

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell , $f = 900 \text{ MHz}$)

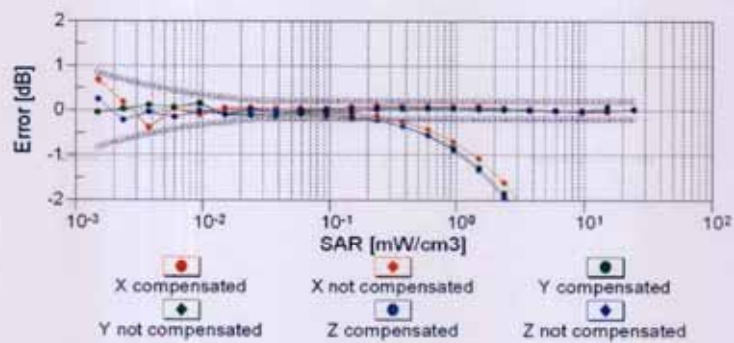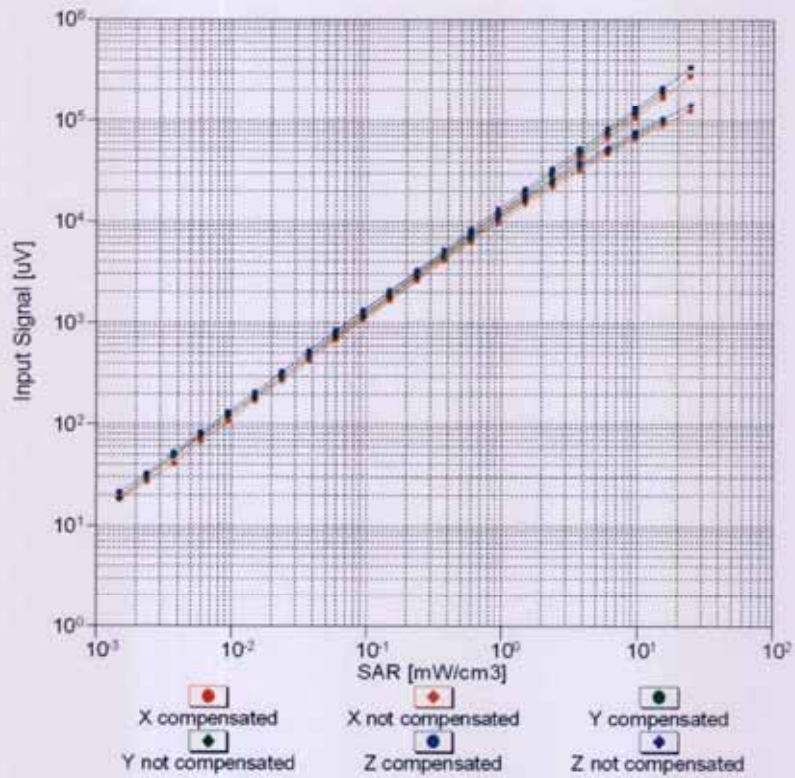


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)


ES3DV3- SN:3139

March 23, 2011

Conversion Factor Assessment

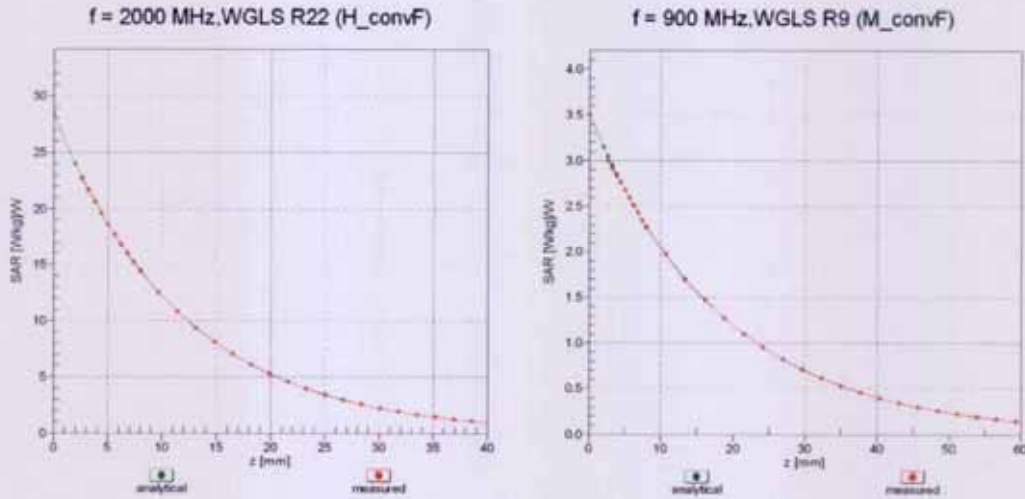

Deviation from Isotropy in Liquid Error (ϕ, θ), f = 900 MHz

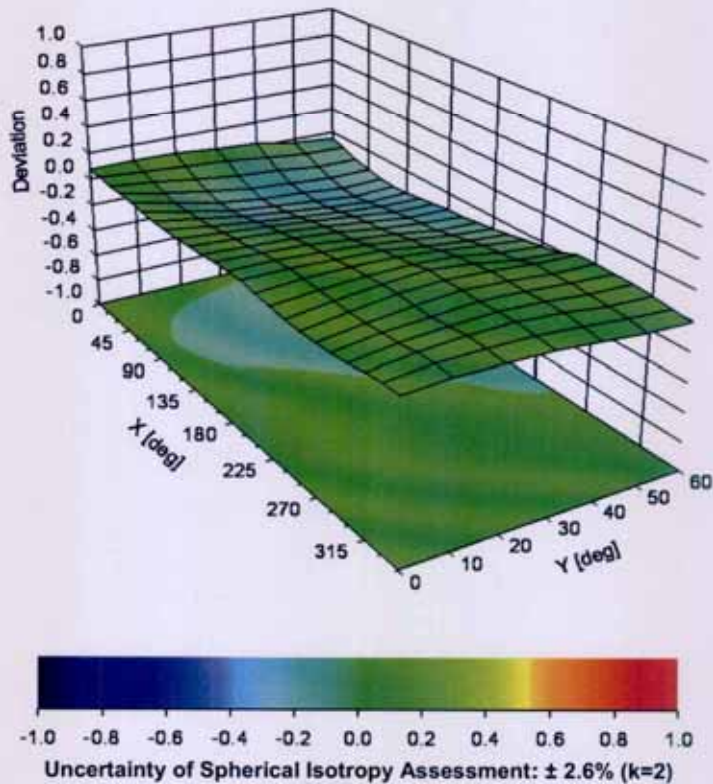

ES3DV3- SN:3139

March 23, 2011

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3139**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

13. DAE CALIBRATION CERTIFICATE:

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 44 245 9700, Fax +41 44 245 9779
info@speag.com, http://www.speag.com

IMPORTANT NOTICE

USAGE OF THE DAE 4

The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:

Battery Exchange: The battery cover of the DAE4 unit is closed using a screw, over tightening the screw may cause the threads inside the DAE to wear out.

Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an antistatic bag. This antistatic bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.

E-Stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.

Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect.

DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file.

Important Note:

Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer.

Important Note:

Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure.

Important Note:

To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.

Schmid & Partner Engineering

TN_BR040315AD DAE4.doc

11.12.2009

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Audix (Auden)**

Certificate No: **DAE4-899_Mar11**

CALIBRATION CERTIFICATE

Object **DAE4 - SD 000 D04 BJ - SN: 899**

Calibration procedure(s) **QA CAL-06.v22
Calibration procedure for the data acquisition electronics (DAE)**



Calibration date: **March 18, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	28-Sep-10 (No:10376)	Sep-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Calibrator Box V1.1	SE UMS 006 AB 1004	07-Jun-10 (in house check)	In house check: Jun-11

Calibrated by:	Name	Function	Signature
	Dominique Steffen	Technician	
Approved by:	Fin Bomholt	R&D Director	

Issued: March 18, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary

DAE data acquisition electronics
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - **DC Voltage Measurement Linearity:** Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - **Common mode sensitivity:** Influence of a positive or negative common mode voltage on the differential measurement.
 - **Channel separation:** Influence of a voltage on the neighbor channels not subject to an input voltage.
 - **AD Converter Values with inputs shorted:** Values on the internal AD converter corresponding to zero input voltage
 - **Input Offset Measurement:** Output voltage and statistical results over a large number of zero voltage measurements.
 - **Input Offset Current:** Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - **Input resistance:** Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - **Low Battery Alarm Voltage:** Typical value for information. Below this voltage, a battery alarm signal is generated.
 - **Power consumption:** Typical value for information. Supply currents in various operating modes.

DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1μV , full range = -100...+300 mV

Low Range: 1LSB = 61nV , full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	402.471 ± 0.1% (k=2)	403.052 ± 0.1% (k=2)	403.039 ± 0.1% (k=2)
Low Range	3.98081 ± 0.7% (k=2)	3.95588 ± 0.7% (k=2)	3.98377 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system	348.5 ° ± 1 °
---	---------------

Appendix

1. DC Voltage Linearity

High Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	200005.3	-3.18	-0.00
Channel X + Input	19999.58	0.28	0.00
Channel X - Input	-19998.40	1.80	-0.01
Channel Y + Input	199993.2	-4.06	-0.00
Channel Y + Input	20000.38	0.08	0.00
Channel Y - Input	-20001.20	-0.80	0.00
Channel Z + Input	199994.6	-1.77	-0.00
Channel Z + Input	19998.79	-1.71	-0.01
Channel Z - Input	-20001.20	-1.00	0.00

Low Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	2000.3	0.36	0.02
Channel X + Input	199.90	-0.10	-0.05
Channel X - Input	-200.05	-0.05	0.03
Channel Y + Input	2000.6	0.40	0.02
Channel Y + Input	198.61	-1.29	-0.65
Channel Y - Input	-200.62	-0.62	0.31
Channel Z + Input	2000.2	0.07	0.00
Channel Z + Input	198.61	-1.29	-0.65
Channel Z - Input	-200.71	-0.81	0.41

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	8.14	7.31
	- 200	-6.04	-7.82
Channel Y	200	12.77	13.21
	- 200	-14.98	-14.77
Channel Z	200	-7.28	-7.24
	- 200	5.94	5.68

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	4.08	-0.12
Channel Y	200	3.16	-	5.26
Channel Z	200	1.92	-0.07	-

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16020	17047
Channel Y	15654	13539
Channel Z	15817	15639

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	-0.25	-1.34	1.03	0.47
Channel Y	-0.29	-0.95	0.53	0.36
Channel Z	-0.68	-1.67	0.05	0.36

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9