

## EMC TEST REPORT

(FULL COMPLIANCE)

**Report Number:** 102675709BOX-001  
**Project Number:** G102675709

**Report Issue Date:** 11/21/2016

**Model(s) Tested:** WHITESTAR Signature Pro System  
NGP680301 Containing Japan MIC and  
US FCC compliant  
Bluetooth Radio- 0100-3070 PCBA,  
GU Interface, BT2.0

**Model(s) Partially Tested:** None

**Model(s) Not Tested but declared equivalent by the client:** None

**Standards:** CFR47 FCC Part 15 Subpart C (15.247): 08/2016  
RSS-247 Issue 1: 05/2015

Tested by:  
Intertek Testing Services NA, Inc.  
70 Codman Hill Road  
Boxborough, MA 01719  
USA

Client:  
Abbott Medical Optics, Inc.  
1700 E Saint Andrew PI Mail Station SA-2M  
Santa Ana, CA 92705  
USA

Report prepared by Naga Suryadevara



Naga Suryadevara/EMC Engineer

Report reviewed by



Michael F. Murphy / Technical Team Leader

*This report is for the exclusive use of Intertek's Client and is provided pursuant to the agreement between Intertek and its Client. Intertek's responsibility and liability are limited to the terms and conditions of the agreement. Intertek assumes no liability to any party, other than to the Client in accordance with the agreement, for any loss, expense or damage occasioned by the use of this report. Only the Client is authorized to permit copying or distribution of this report and then only in its entirety. Any use of the Intertek name or one of its marks for the sale or advertisement of the tested material, product or service must first be approved in writing by Intertek. The observations and test results in this report are relevant only to the sample tested. This report by itself does not imply that the material, product, or service is or has ever been under an Intertek certification program.*

## Table of Contents

<b>1</b>	<b><i>Introduction and Conclusion</i></b> .....	<b>3</b>
<b>2</b>	<b><i>Test Summary</i></b> .....	<b>3</b>
<b>3</b>	<b><i>Client Information</i></b> .....	<b>5</b>
<b>4</b>	<b><i>Description of Equipment Under Test and Variant Models</i></b> .....	<b>5</b>
<b>5</b>	<b><i>System Setup and Method</i></b> .....	<b>7</b>
<b>6</b>	<b><i>Output Power and Human RF Exposure</i></b> .....	<b>8</b>
<b>7</b>	<b><i>20 dB and Occupied (99%) Bandwidth</i></b> .....	<b>20</b>
<b>8</b>	<b><i>Channel Separation</i></b> .....	<b>28</b>
<b>9</b>	<b><i>Number of Hopping Channels</i></b> .....	<b>31</b>
<b>10</b>	<b><i>Average Channel Occupancy Time</i></b> .....	<b>34</b>
<b>11</b>	<b><i>Out of Band and Band Edge Conducted Emissions</i></b> .....	<b>38</b>
<b>12</b>	<b><i>Transmitter Spurious Emissions</i></b> .....	<b>56</b>
<b>13</b>	<b><i>Receiver Spurious Emissions</i></b> .....	<b>63</b>
<b>14</b>	<b><i>Revision History</i></b> .....	<b>69</b>

## 1 Introduction and Conclusion

The tests indicated in section 2.0 were performed on the product constructed as described in section 4.0. The remaining test sections are the verbatim text from the actual data sheets used during the investigation. These test sections include the test name, the specified test Method, a list of the actual Test Equipment Used, documentation Photos, Results and raw Data. No additions, deviations, or exclusions have been made from the standard(s) unless specifically noted.

Based on the results of our investigation, we have concluded the product tested **complies** with the requirements of the standard(s) indicated. The results obtained in this test report pertain only to the item(s) tested. Intertek does not make any claims of compliance for samples or variants which were not tested.

## 2 Test Summary

Section	Test full name	Result
3	Client Information	
4	Description of Equipment Under Test and Variant Models	
5	System Setup and Method	
6	Output Power and Human RF Exposure (CFR47 FCC Part 15 Subpart C (15.247): 08/2016 RSS-247 Issue 1: 05/2015 RSS-102 Issue 5: 03/2015)	Pass
7	Occupied (99%) and 20 dB Bandwidth (CFR47 FCC Part 15 Subpart C (15.247): 08/2016 RSS-247 Issue 1: 05/2015)	Pass
8	Channel Separation (CFR47 FCC Part 15 Subpart C (15.247): 08/2016 RSS-247 Issue 1: 05/2015)	Pass
9	Number of Hopping Channels (CFR47 FCC Part 15 Subpart C (15.247): 08/2016 RSS-247 Issue 1: 05/2015)	Pass
10	Average Channel Occupancy Time (CFR47 FCC Part 15 Subpart C (15.247): 08/2016 RSS-247 Issue 1: 05/2015)	Pass
11	Out of Band Conducted Emissions (CFR47 FCC Part 15 Subpart C (15.247): 08/2016 RSS-247 Issue 1: 05/2015)	Pass
12	Out of Band Radiated Spurious Emissions (CFR47 FCC Part 15 Subpart C (15.247): 08/2016 RSS-247 Issue 1: 05/2015)	Pass
13	Transmitter Spurious Emissions (CFR47 FCC Part 15 Subpart C (15.247): 08/2016 RSS-247 Issue 1: 05/2015)	Pass

14	Radiated Emissions from Digital parts and Receiver (CFR47 FCC Part 15 (15.109): 08/2016 ICES 003: 01/2016 and updated 06/2016)	Pass
--	AC Mains Conducted Emissions	NA <sup>(1)</sup>
15	Revision History	

(1) Not Applicable. The EUT does not have any direct connection to public power network. In normal use, EUT is installed inside the host unit and it is DC powered internally.

### 3 Client Information

This EUT was tested at the request of:

**Client:** Abbott Medical Optics, Inc.  
1700 E Saint Andrew PI Mail Station SA-2M  
Santa Ana, CA 92705  
USA

**Contact:** Fred Lee  
**Telephone:** (714) 247-8578  
**Email:** Fred.Lee@amo.abbott.com

### 4 Description of Equipment Under Test and Variant Models

**Manufacturer:** Abbott Medical Optics, Inc.  
1700 E Saint Andrew PI Mail Station SA-2M  
Santa Ana, CA 92705  
USA

Equipment Under Test			
Description	Manufacturer	Model Number	Serial Number
WHITESTAR Signature Pro System NGP680301 Containing Japan MIC and US FCC compliant Bluetooth Radio- 0100-3070 PCBA, GU Interface, BT2.0	Abbott Medical Optics, Inc.	0100-3070 revA	131121003

Receive Date:	08/22/2016
Received Condition:	Good
Type:	Production

Description of Equipment Under Test (provided by client)
The WHITESTAR Signature Advanced Control Pedal & Remote Control system consists of the Advanced Control Pedal (1RF module for a Foot Pedal control mounted in main system) and Remote Control Master 2.0 (2RF module for remote control of Monitor mounted in main system), Advanced Control Pedal Slave (3 RF module for a Foot Pedal control mounted outside of main system) and Remote Control Slave 2.0 (4RF module for remote control of Monitor mounted outside of main system).
The <sup>1</sup> RF module for a Foot Pedal control mounted in main system and <sup>3</sup> RF module for a Foot Pedal control mounted outside of main system consists two National Semiconductor's LMX98XX series Bluetooth radios ICs (transceivers), operating in the 2.4 GHz frequency band. Only one transmitter can report the data to the host at any given time. This radio subsystem is used to communicate the footpedal control signal to the WHITESTAR Signature™ system for use in cataract surgery.
The <sup>2</sup> RF module for remote control of Monitor mounted in main system and 4RF module for remote control of Monitor mounted outside of main system consists one National Semiconductor's LMX98XX series Bluetooth radios ICs (transceivers), operating in the 2.4 GHz frequency band. This radio subsystem is used to communicate the monitor control signal to the WHITESTAR Signature™ system for use in cataract surgery.
This report covers the <sup>2</sup> RF module for remote control of Monitor mounted in main system and the 1RF

module for a Foot Pedal control mounted in main system is covered in separate report #3184783MPK-001A.

<sup>3</sup>RF module for a Foot Pedal control mounted outside of main system and 4RF module for remote control of Monitor mounted outside of main system are already FCC and Industry Canada certified.

Equipment Under Test Power Configuration			
Rated Voltage	Rated Current	Rated Frequency	Number of Phases
5V/12V	100mA/100mA	N/A	N/A

#### Operating modes of the EUT:

No.	Descriptions of EUT Exercising
1	Transmit mode with Frequency hopping enabled.
2	Transmit mode with Frequency hopping disabled.
3	Receive mode

#### Software used by the EUT:

No.	Descriptions of EUT Exercising
1	Tera Term Version 4.82

Radio/Receiver Characteristics	
<b>Frequency Band(s)</b>	2402 – 2480 MHz
<b>Modulation Type(s)</b>	GFSK (FHSS)
<b>Maximum Output Power</b>	-11.73 dBm
<b>Test Channels</b>	Low Channel – 2402 MHz Mid Channel – 2441 MHz High Channel – 2480 MHz
<b>Occupied Bandwidth</b>	980 kHz
<b>Frequency Hopper: Number of Hopping Channels</b>	79
<b>Frequency Hopper: Channel Occupancy Time</b>	0.366 seconds
<b>Frequency Hopper: Max interval between two instances of use of the same channel</b>	N/A
<b>MIMO Information (# of Transmit and Receive antenna ports)</b>	1
<b>Equipment Type</b>	Standalone
<b>ETSI LBT/Adaptivity</b>	N/A
<b>ETSI Adaptivity Type</b>	N/A
<b>ETSI Temperature Category (I, II, III)</b>	N/A
<b>ETSI Receiver Category (1, 2, 3)</b>	N/A
<b>Antenna Type and Gain</b>	On-Board Antenna 2.2 dBi

**Variant Models:**

The following variant models were not tested as part of this evaluation, but have been identified by the manufacturer as being electrically identical models, depopulated models, or with reasonable similarity to the model(s) tested. Intertek does not make any claims of compliance for samples or variants which were not tested.

None

## 5 System Setup and Method


Cables					
ID	Description	Length (m)	Shielding	Ferrites	Termination
1	USB to Serial Cable	1	None	None	Laptop

Support Equipment			
Description	Manufacturer	Model Number	Serial Number
Laptop	HP	EliteBook 840	53G537057N

### 5.1 Method:

Configuration as required by FCC CFR47 Part 15 Subpart C (15.247): 08/2016, RSS-247 Issue 1: 05/2015 RSS-102 Issue 5: 03/2015 and ANSI C63.1: 2013.

### 5.2 EUT Block Diagram:

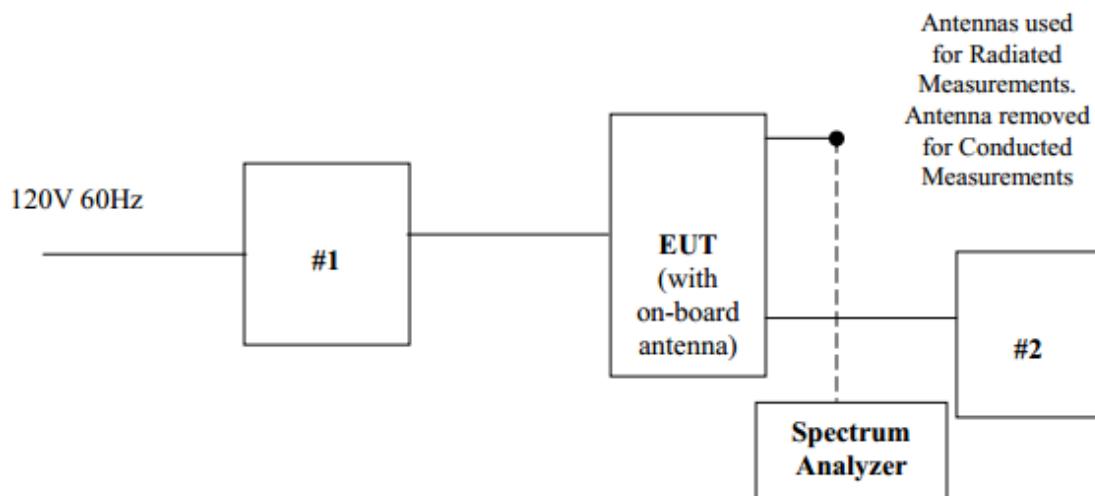

**S** = Shielded  
**U** = Unshielded

**F** = With Ferrite  
**m** = Length in Meters

## 6 Output Power and Human RF Exposure

### 6.1 Method

Tests are performed in accordance with FCC Part 15 Subpart C (15.247), RSS 247 and RSS 102.

**TEST SITE:** EMC Lab – Intertek Lake Forest CA

**The EMC Lab** has one Semi-anechoic Chamber and one Shielded Chamber. AC Mains Power is available at 120, 230, and 277 Single Phase; 208, 380, and 440 3-Phase. Large reference ground-planes are installed in the general lab area to facilitate EMC work not requiring a shielded environment.

### 6.2 Test Equipment Used:

Asset	Description	Manufacturer	Model	Serial	Cal Date	Cal Due
001001'	Barometer/Humidity Control	Omega	iBTHX-W	0440775	04/22/2016	04/22/2017
000690'	Spectrum Analyzer, 9 KHz - 40 GHz	Rohde & Schwarz	FSP40	100027	01/11/2016	01/11/2017
CBLHF20 12-5M-1'	5m 9kHz-40GHz Coaxial Cable - SET 1	Huber & Suhner	SF102	252676001	02/09/2016	02/09/2017

### Software Utilized:

Name	Manufacturer	Version
None		


### 6.3 Results:


The sample tested was found to Comply. For systems operating in the 2400-2483.5 MHz band employing at least 75 hopping channels, the maximum peak output power is 1 watt (30 dBm), for all other systems 0.125 W (21 dBm).

The GUI board has 79 hopping channels.


Frequency	Data Rate	Output Power in dBm	Output Power in mW	Limit
2402	DH5	-11.79	0.06622165037	1 W
2402	DH3	-12.43	0.057147863667	1 W
2402	DH1	-11.73	0.067142885293	1 W
2441	DH5	-13.87	0.041020410299	1 W
2441	DH3	-13.58	0.043853069777	1 W
2441	DH1	-13.61	0.043551187369	1 W
2480	DH5	-13.18	0.048083934845	1 W
2480	DH3	-13.11	0.048865235934	1 W
2480	DH1	-13.02	0.049888448746	1 W

Note: The EUT's antenna has less than 6 dBi gain.

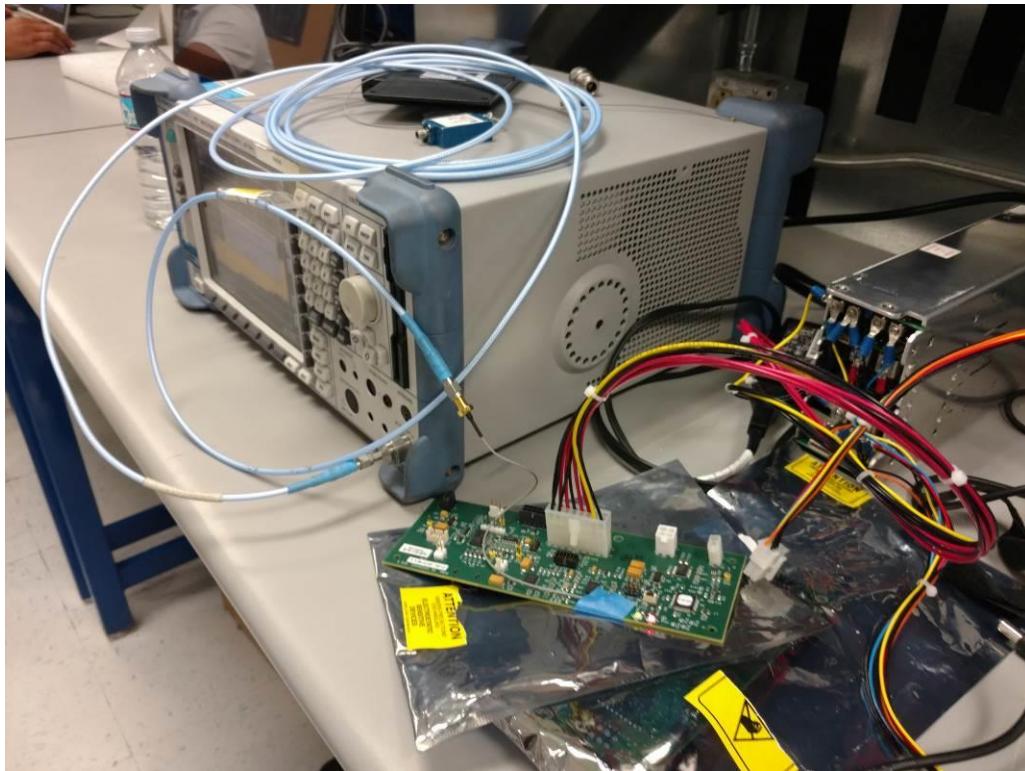
**6.4 Setup Photographs:**

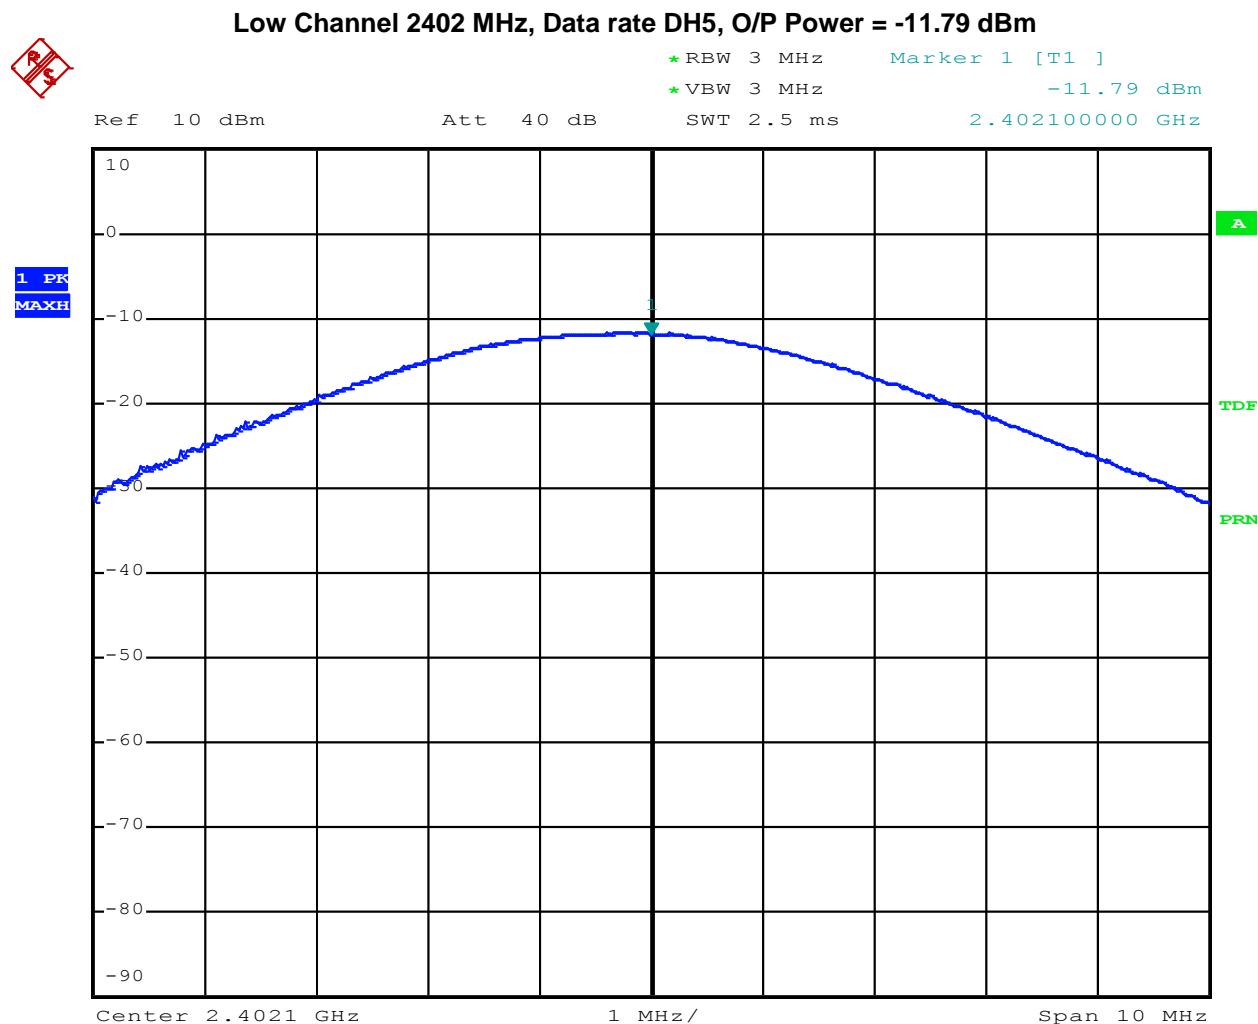**6.5 Plots/Data:**


## Low Channel 2402 MHz, Data rate DH3, O/P Power = -12.43 dBm

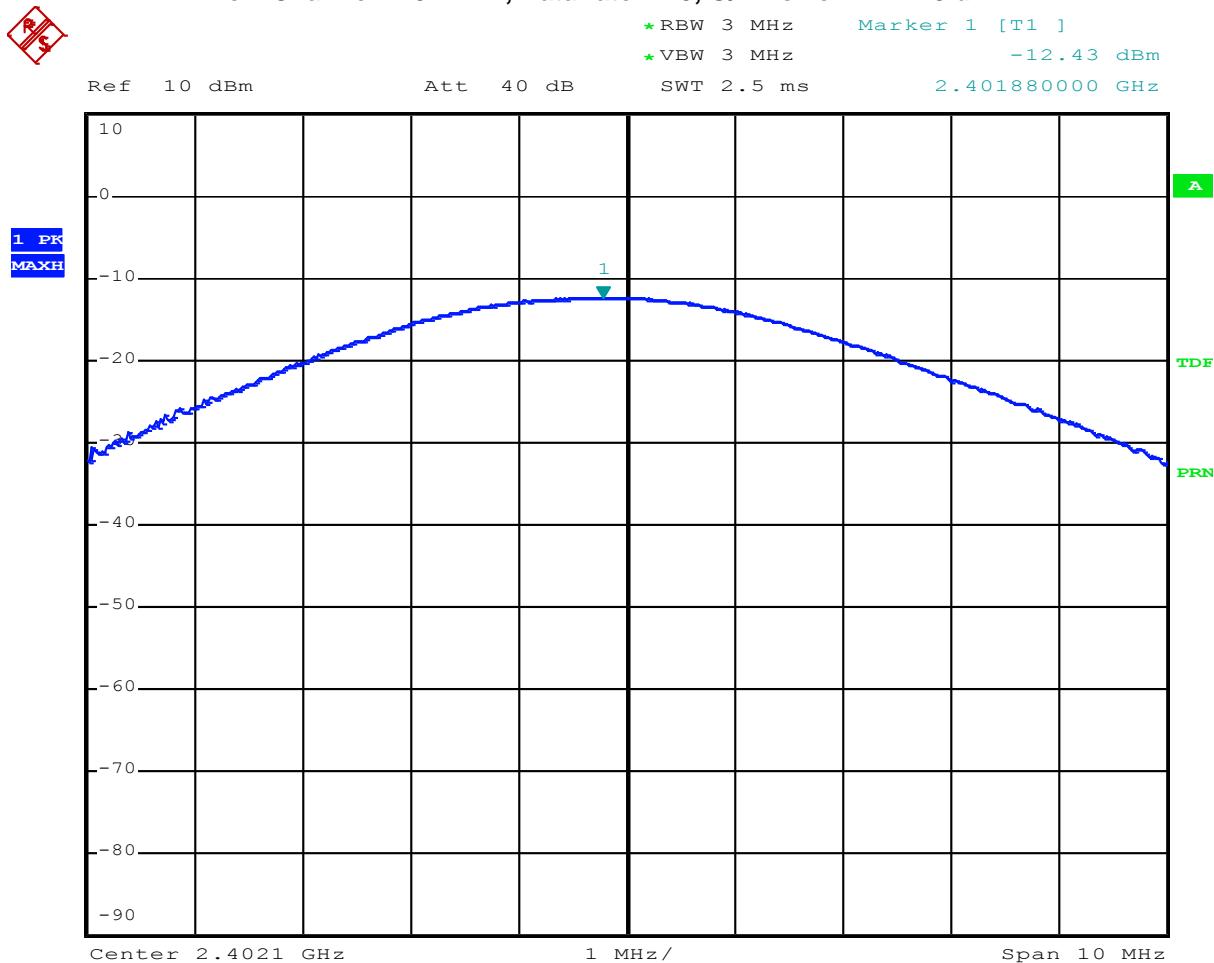


## Low Channel 2402 MHz, Data rate DH1, O/P Power = -11.73 dBm

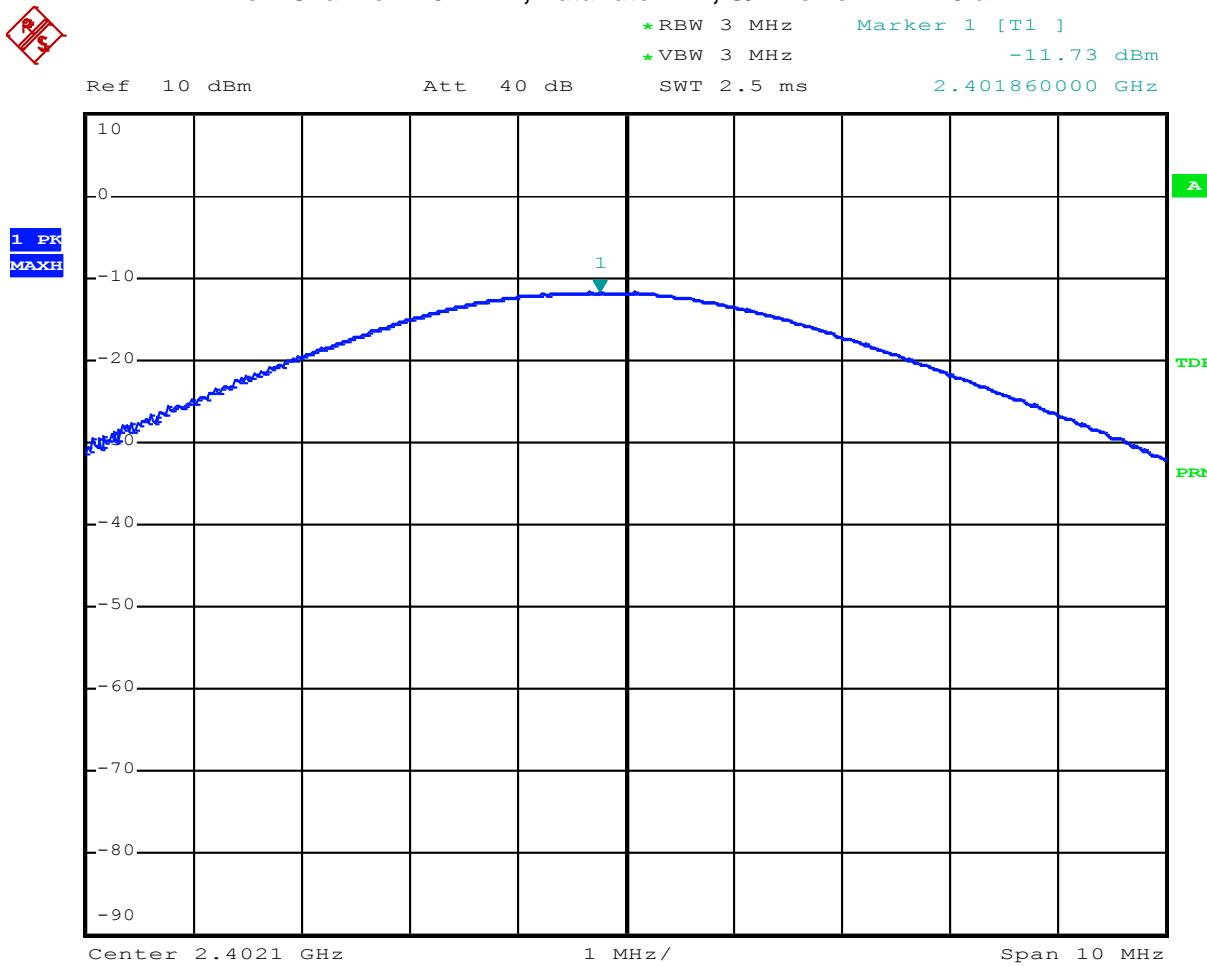


## Mid Channel 2441 MHz, Data rate DH5, O/P Power = -13.87 dBm

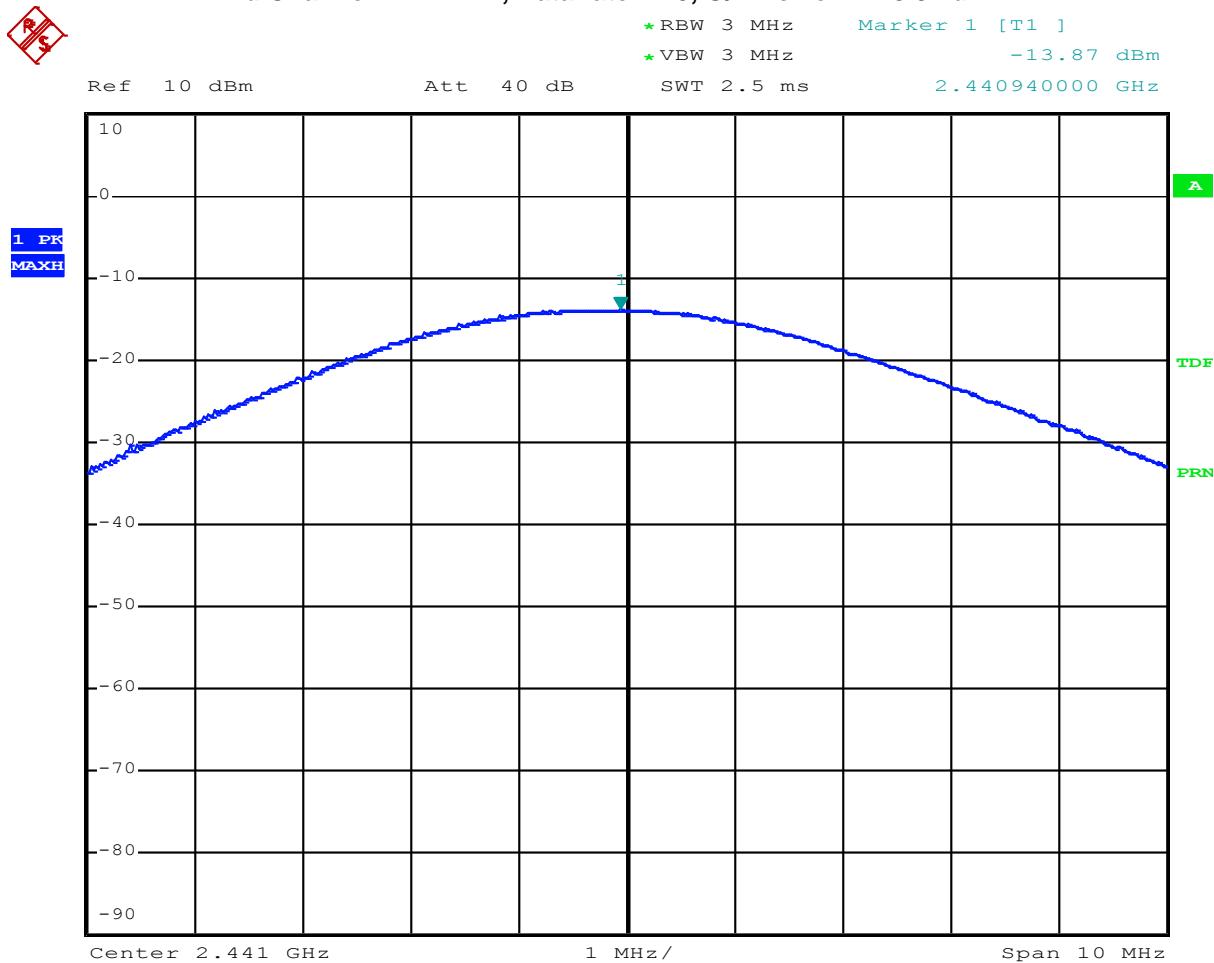


## Mid Channel 2441 MHz, Data rate DH3, O/P Power = -13.58 dBm

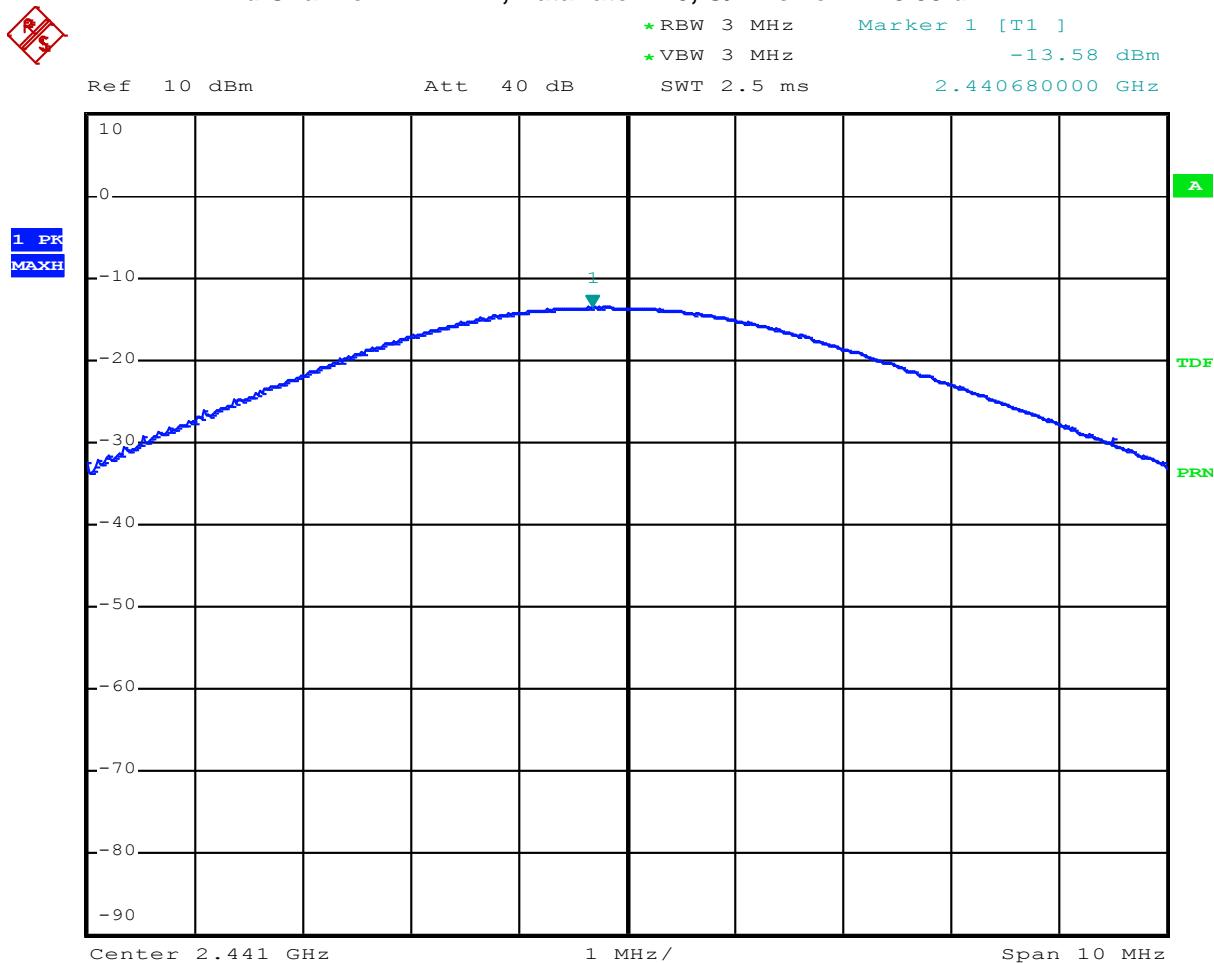


## Mid Channel 2441 MHz, Data rate DH1, O/P Power = -13.61 dBm

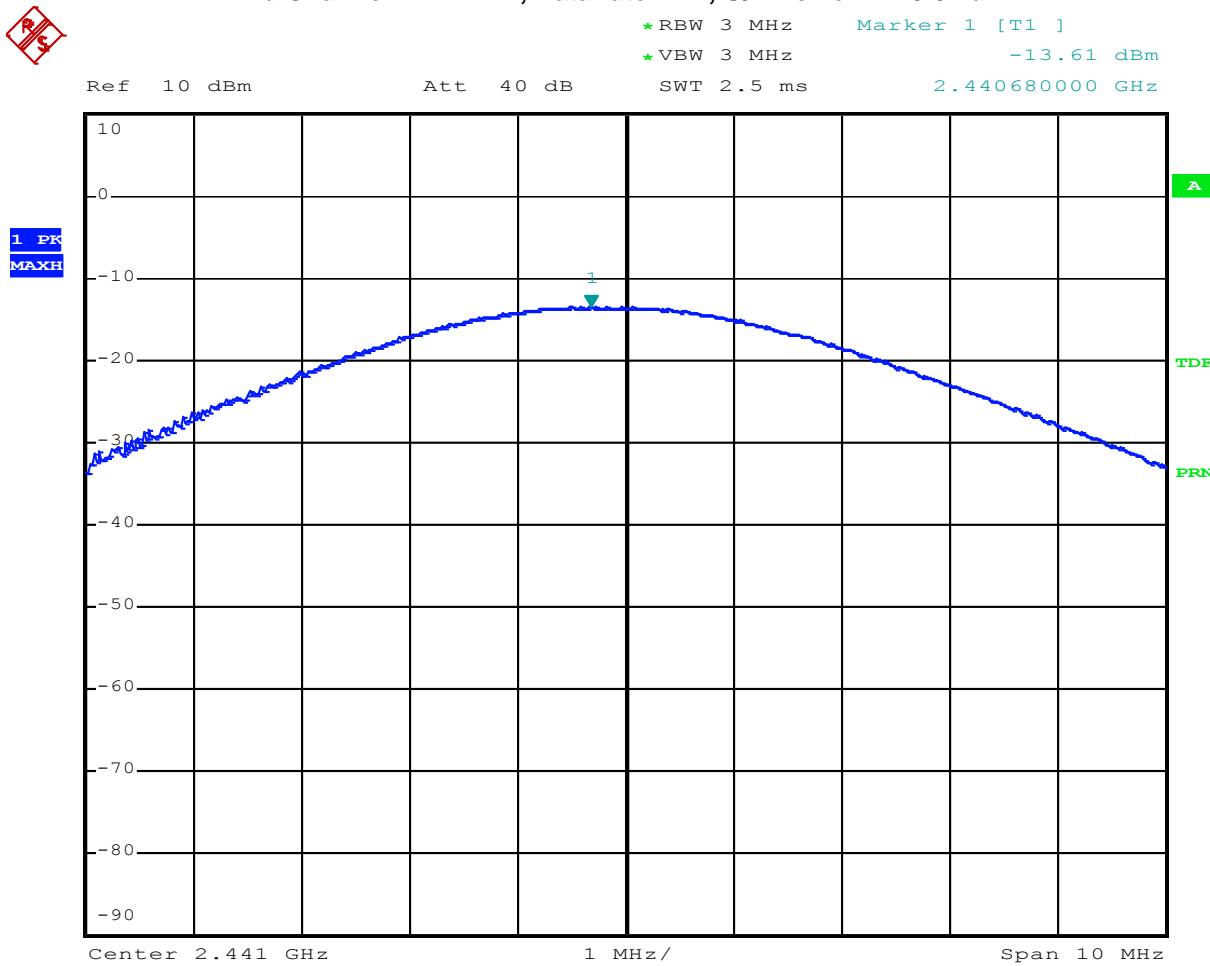


## High Channel 2480 MHz, Data rate DH5, O/P Power = -13.18 dBm

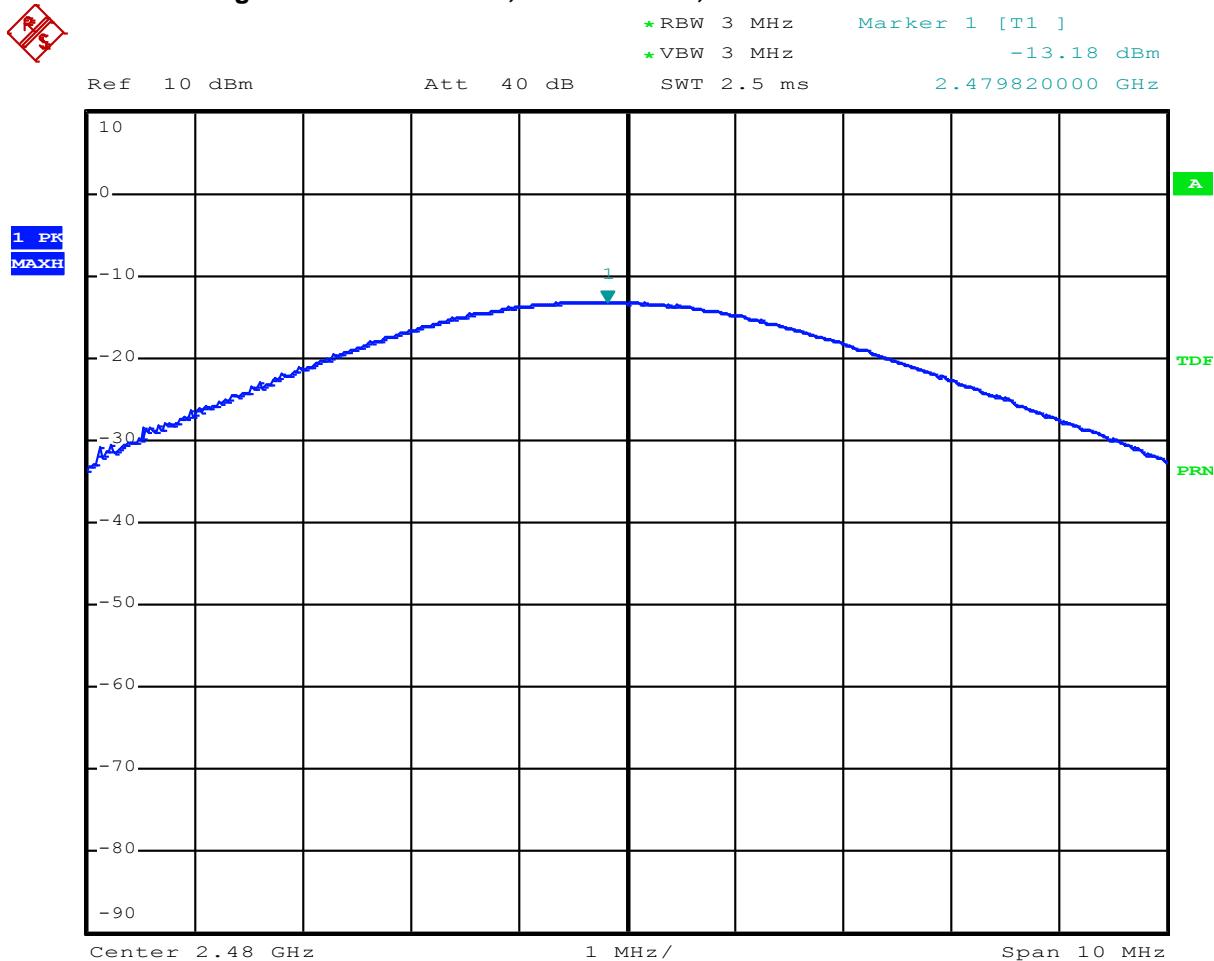

## High Channel 2480 MHz, Data rate DH3, O/P Power = -13.11 dBm

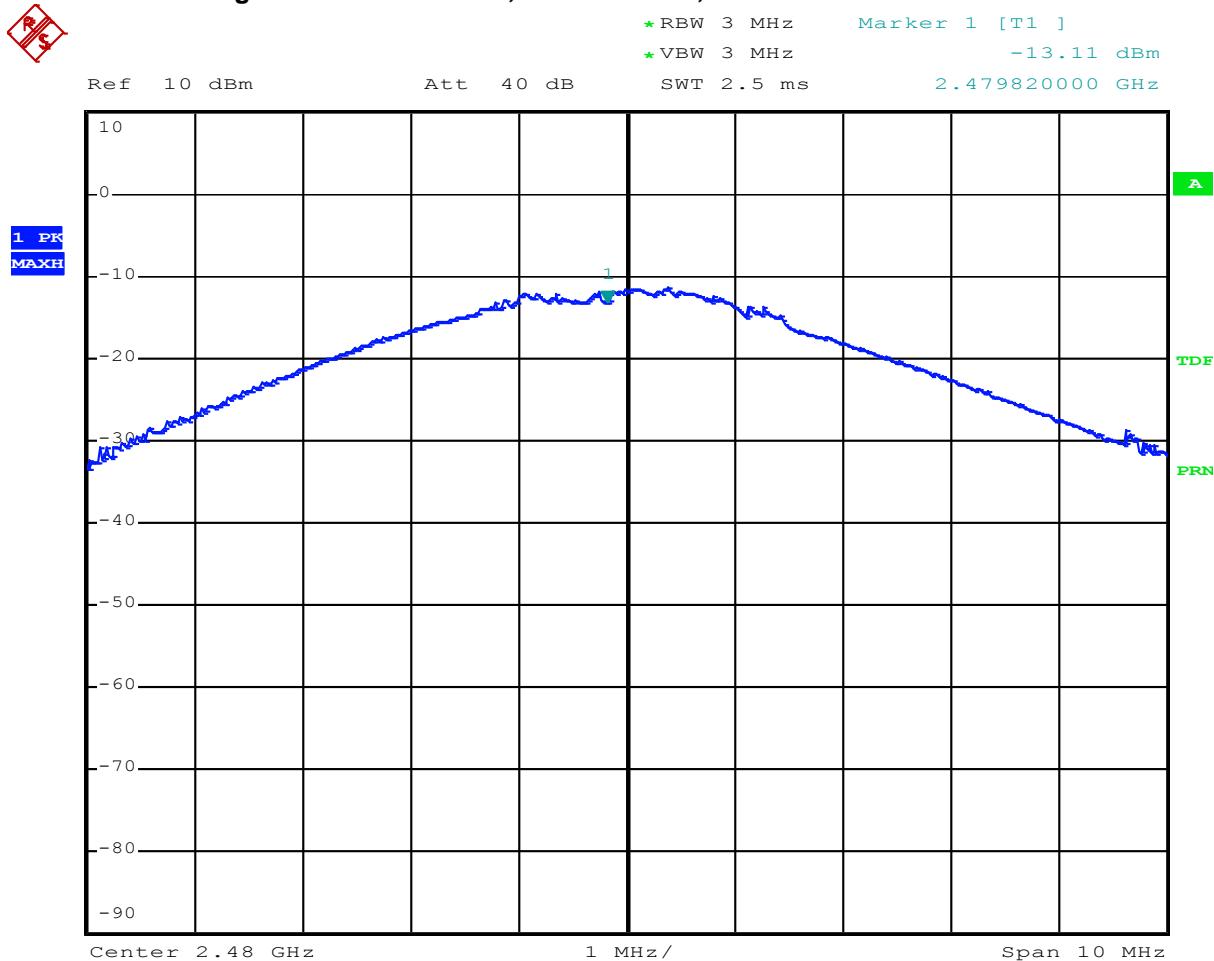

## High Channel 2480 MHz, Data rate DH1, O/P Power = -13.02 dBm

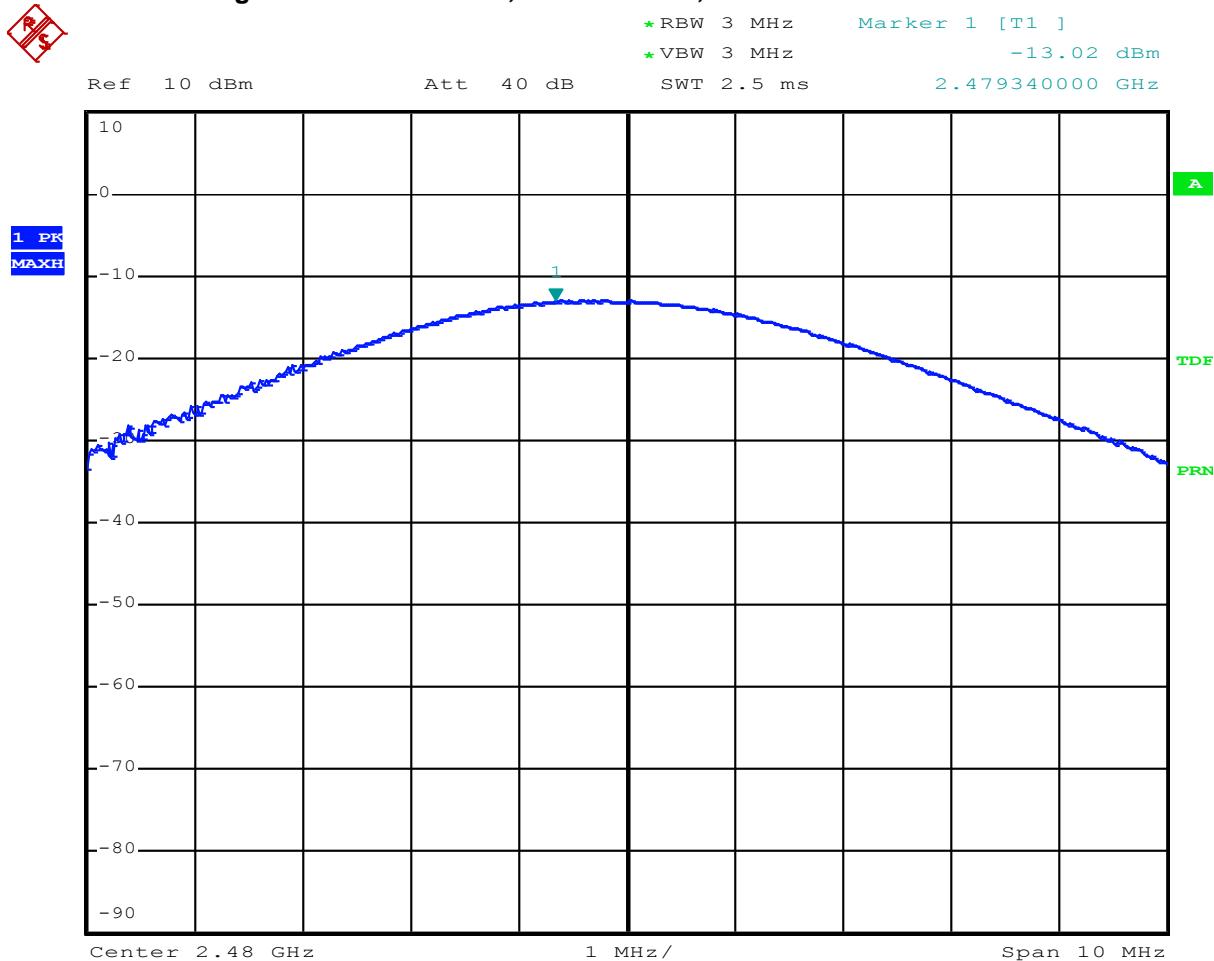

**Human RF Exposure/SAR Exemption**

Maximum measured output power is 0.0671429 mW @ 2402 MHz

**FCC SAR Exemption per KDB 447498**

a) For 100 MHz to 6 GHz and *test separation distances*  $\leq$  50 mm, the 1-g and 10-g *SAR test exclusion thresholds* are determined by the following:

$$[(\text{max. power of channel, including tune-up tolerance, mW}) / (\text{min. test separation distance, mm})] \cdot [\sqrt{f_{(\text{GHz})}}] \leq 3.0 \text{ for 1-g SAR, and } \leq 7.5 \text{ for 10-g extremity SAR,}^{30} \text{ where}$$

- $f_{(\text{GHz})}$  is the RF channel transmit frequency in GHz

$$= (0.0671429/5) * (\sqrt{2.402})$$

$$= 0.0208121 < 3.0 \text{ (below the limit SAR Exempt per FCC)}$$

**RSS 102 SAR Exemption**

**Table 1: SAR evaluation – Exemption limits for routine evaluation based on frequency and separation distance<sup>4,5</sup>**

Frequency (MHz)	Exemption Limits (mW)				
	At separation distance of $\leq$ 5 mm	At separation distance of 10 mm	At separation distance of 15 mm	At separation distance of 20 mm	At separation distance of 25 mm
≤300	71 mW	101 mW	132 mW	162 mW	193 mW
450	52 mW	70 mW	88 mW	106 mW	123 mW
835	17 mW	30 mW	42 mW	55 mW	67 mW
1900	7 mW	10 mW	18 mW	34 mW	60 mW
2450	4 mW	7 mW	15 mW	30 mW	52 mW
3500	2 mW	6 mW	16 mW	32 mW	55 mW
5800	1 mW	6 mW	15 mW	27 mW	41 mW

The exemption limits in Table 1 are based on measurements and simulations of half-wave dipole antennas at separation distances of 5 mm to 25 mm from a flat phantom, providing a SAR value of approximately 0.4 W/kg for 1 g of tissue. For low frequencies (300 MHz to 835 MHz), the exemption limits are derived from a linear fit. For high frequencies (1900 MHz and above), the exemption limits are derived from a third order polynomial fit.

**The measured maximum output power “0.0671429 mW” is less than the limit @ 5mm separation distance (4 mW) specified in the above table, hence the device is SAR exempt.**

Test Personnel: Naga Suryadevara N.S.  
 Supervising/Reviewing Engineer:  
 (Where Applicable) N/A  
 Product Standard: FCC Part 15 Subpart C  
(15.247) and RSS-247  
 Input Voltage: 12 VDC

Test Date: 08/24/2016

Limit Applied: See test report section 6.3

Pretest Verification: Yes

Ambient Temperature: 22 °C

Relative Humidity: 44 %

Atmospheric Pressure: 1003 mbars

Deviations, Additions, or Exclusions: None

## 7 20 dB and Occupied (99%) Bandwidth

### 7.1 Method

Tests are performed in accordance with FCC Part 15 Subpart C (15.247) and RSS 247.

**TEST SITE:** EMC Lab – Intertek Lake Forest CA

**The EMC Lab** has one Semi-anechoic Chamber and one Shielded Chamber. AC Mains Power is available at 120, 230, and 277 Single Phase; 208, 380, and 440 3-Phase. Large reference ground-planes are installed in the general lab area to facilitate EMC work not requiring a shielded environment.

### 7.2 Test Equipment Used:

Asset	Description	Manufacturer	Model	Serial	Cal Date	Cal Due
001001'	Barometer/Humidity Control	Omega	iBTHX-W	0440775	04/22/2016	04/22/2017
000690'	Spectrum Analyzer, 9 KHz - 40 GHz	Rohde & Schwarz	FSP40	100027	01/11/2016	01/11/2017
CBLHF20 12-5M-1'	5m 9kHz-40GHz Coaxial Cable - SET 1	Huber & Suhner	SF102	252676001	02/09/2016	02/09/2017

### Software Utilized:


Name	Manufacturer	Version
None		

### 7.3 Results:

The sample tested was found to Comply.


Frequency	Data Rate	20 dB Bandwidth
2402	DH1	604 kHz
2441	DH3	636 kHz
2480	DH1	680 kHz

Frequency	Data Rate	Occupied Bandwidth
2402	DH1	980 kHz
2441	DH3	980 kHz
2480	DH1	968 kHz

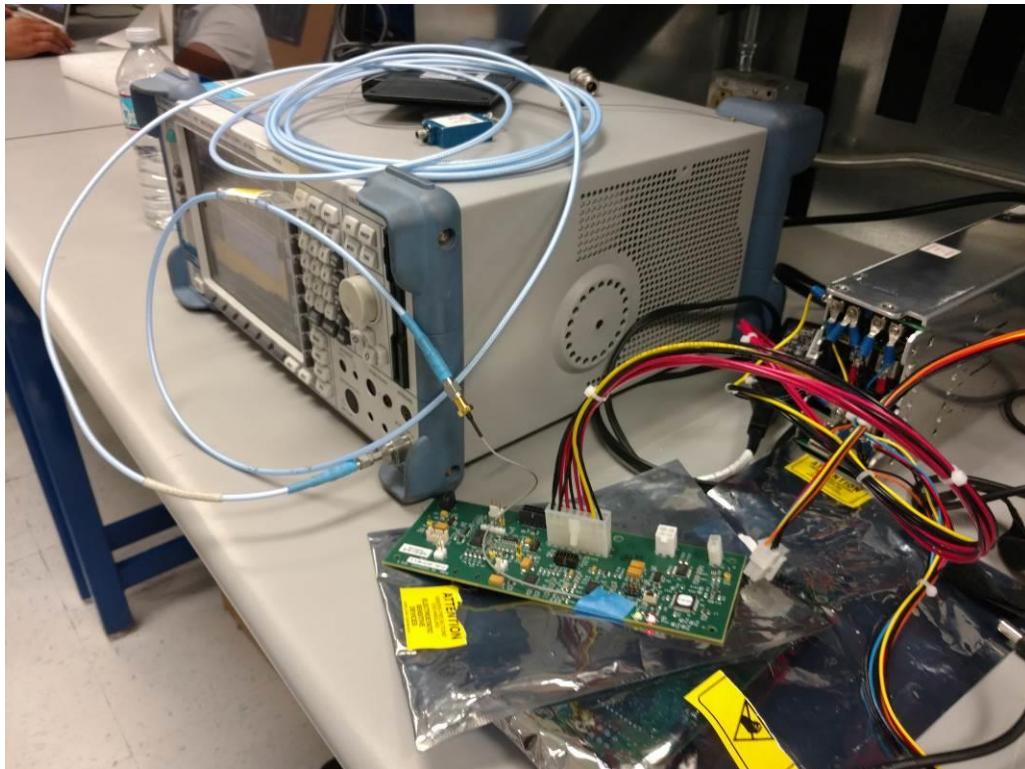
**7.4 Setup Photographs:**

## 7.5 Plots/Data:


### Low Channel 2402 MHz, Data rate DH1, Occupied Bandwidth = 980 kHz

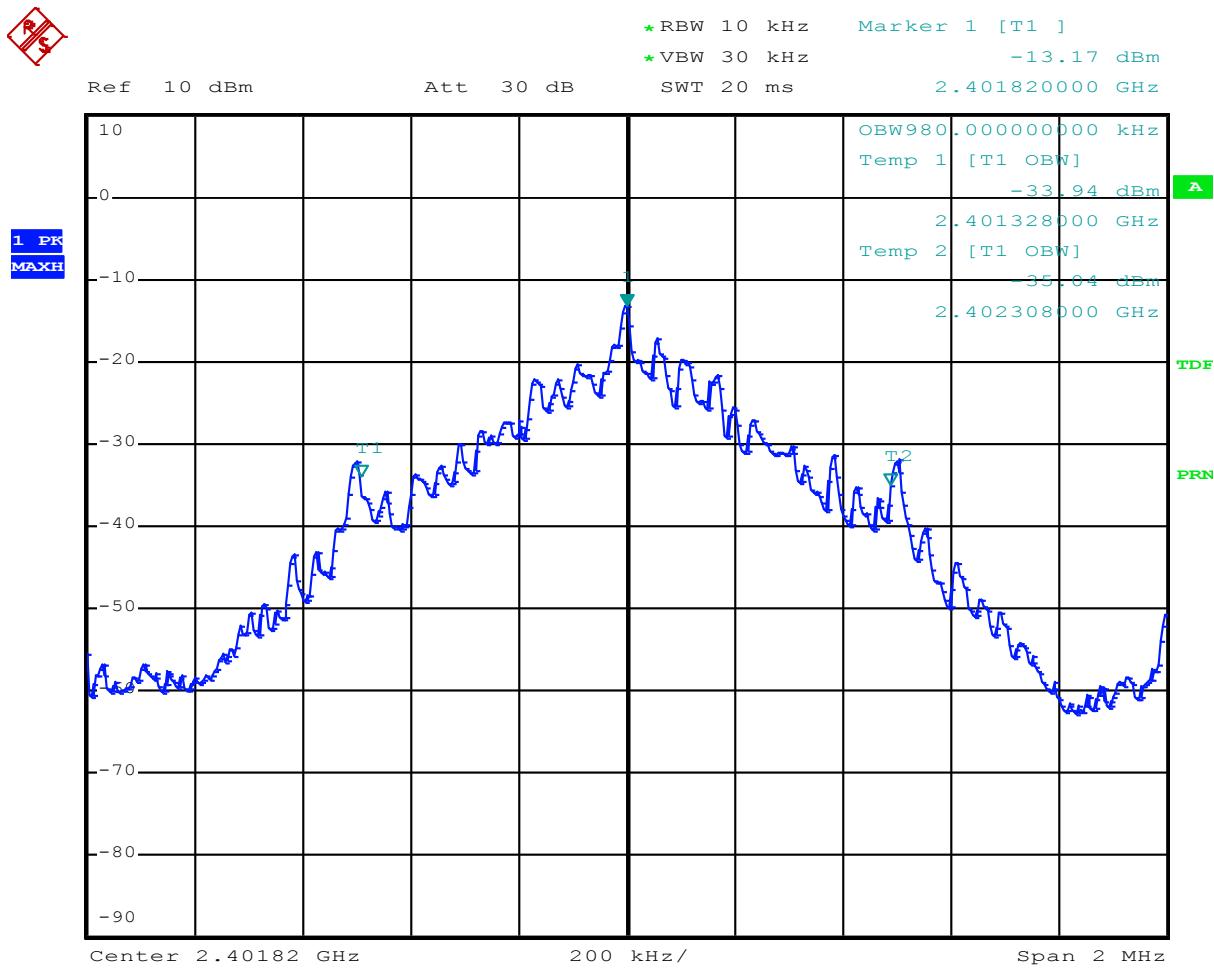


## Low Channel 2402 MHz, Data rate DH1, 20 dB Bandwidth = 604 kHz

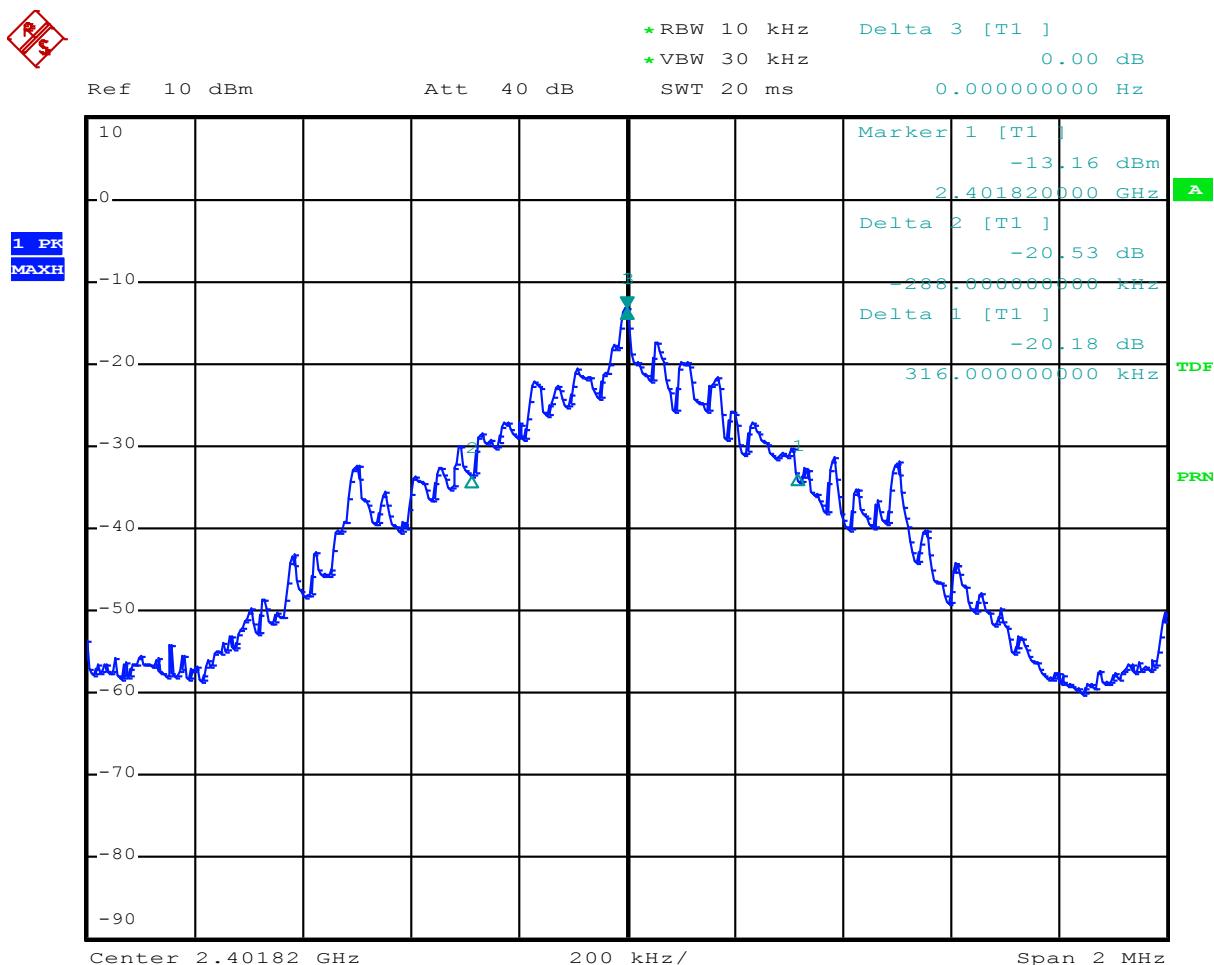


## Mid Channel 2441 MHz, Data rate DH3, Occupied Bandwidth = 980 kHz

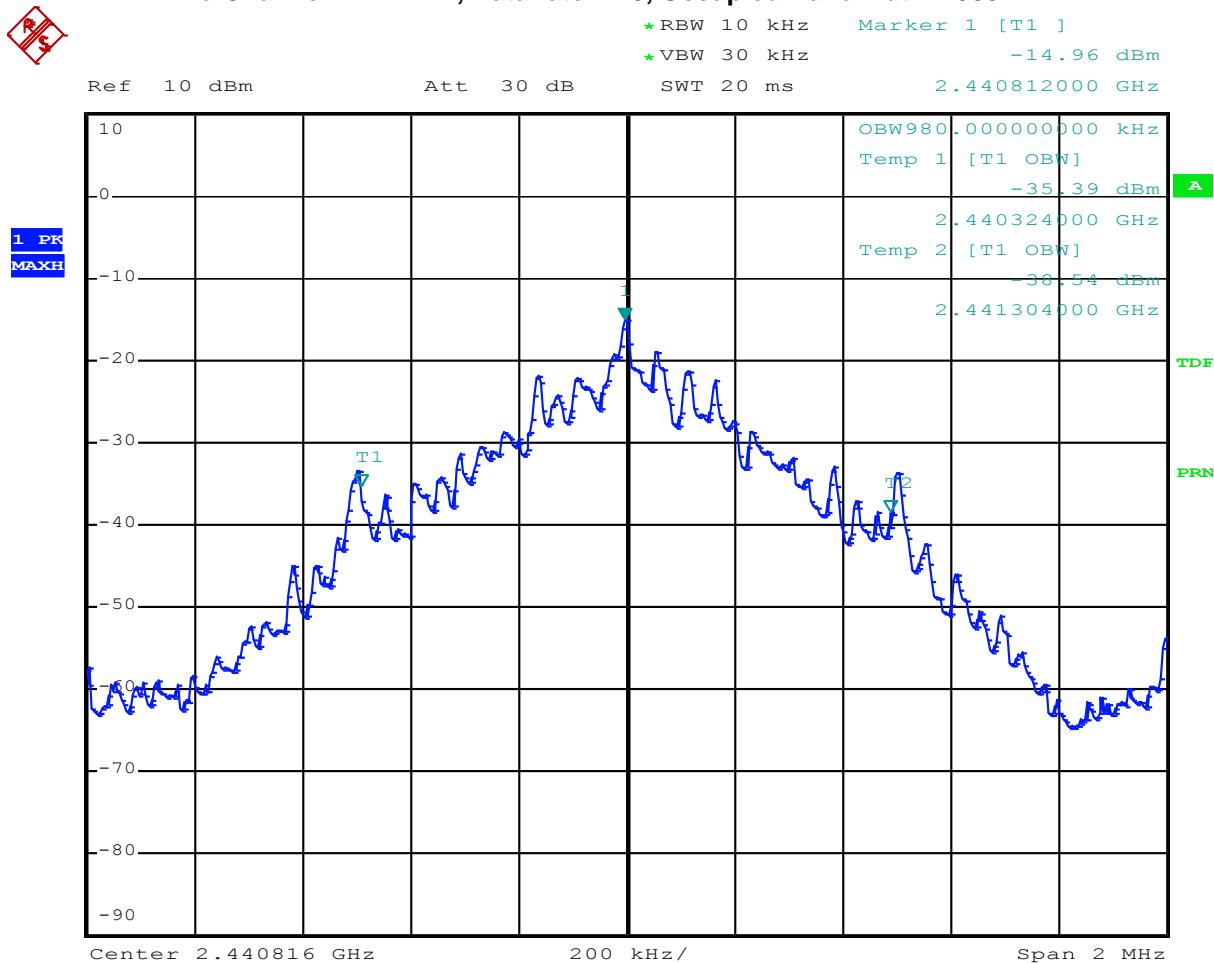


## Mid Channel 2441 MHz, Data rate DH3, 20dB Bandwidth = 636 kHz

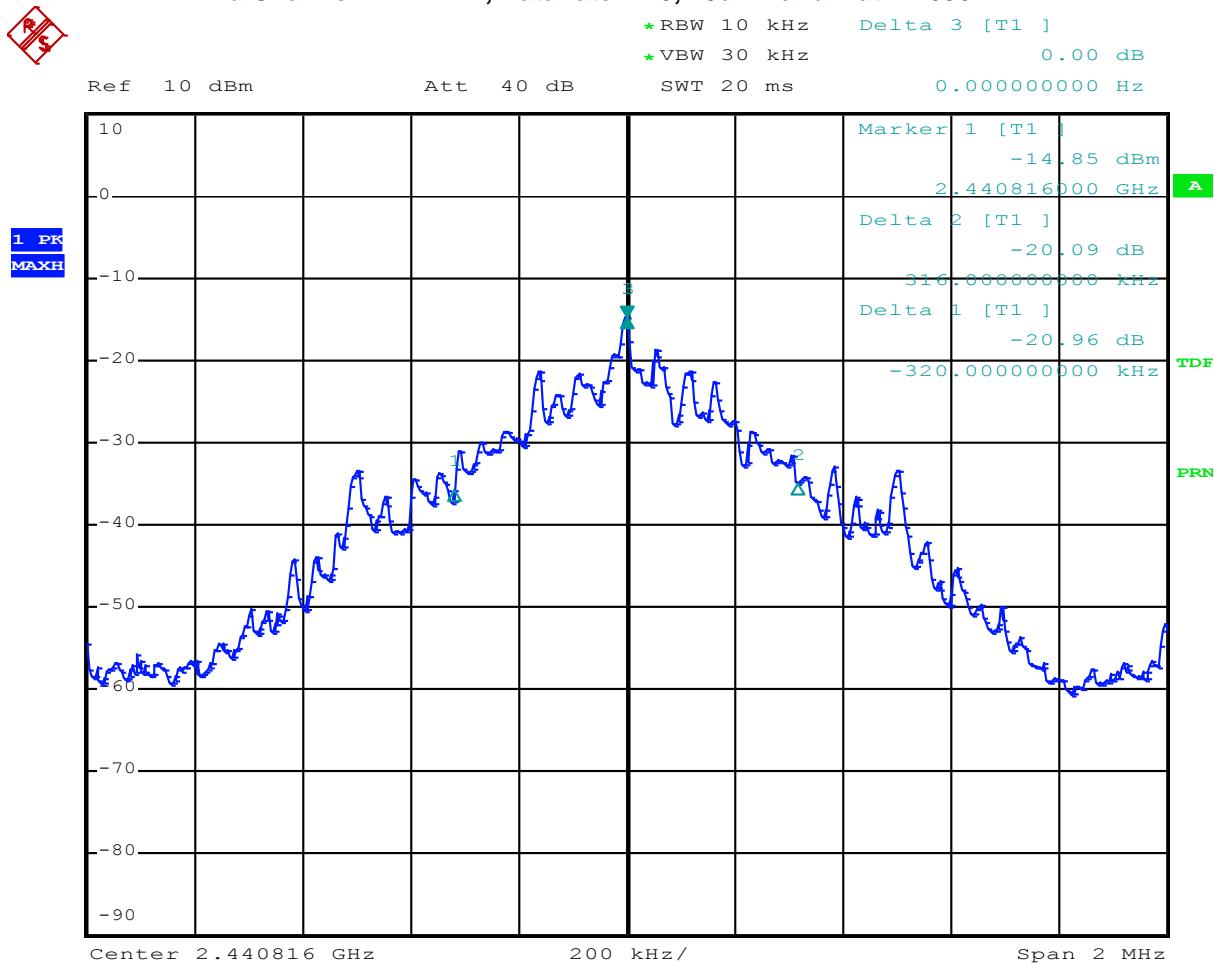

## High Channel 2480 MHz, Data rate DH1, Occupied Bandwidth = 968 kHz

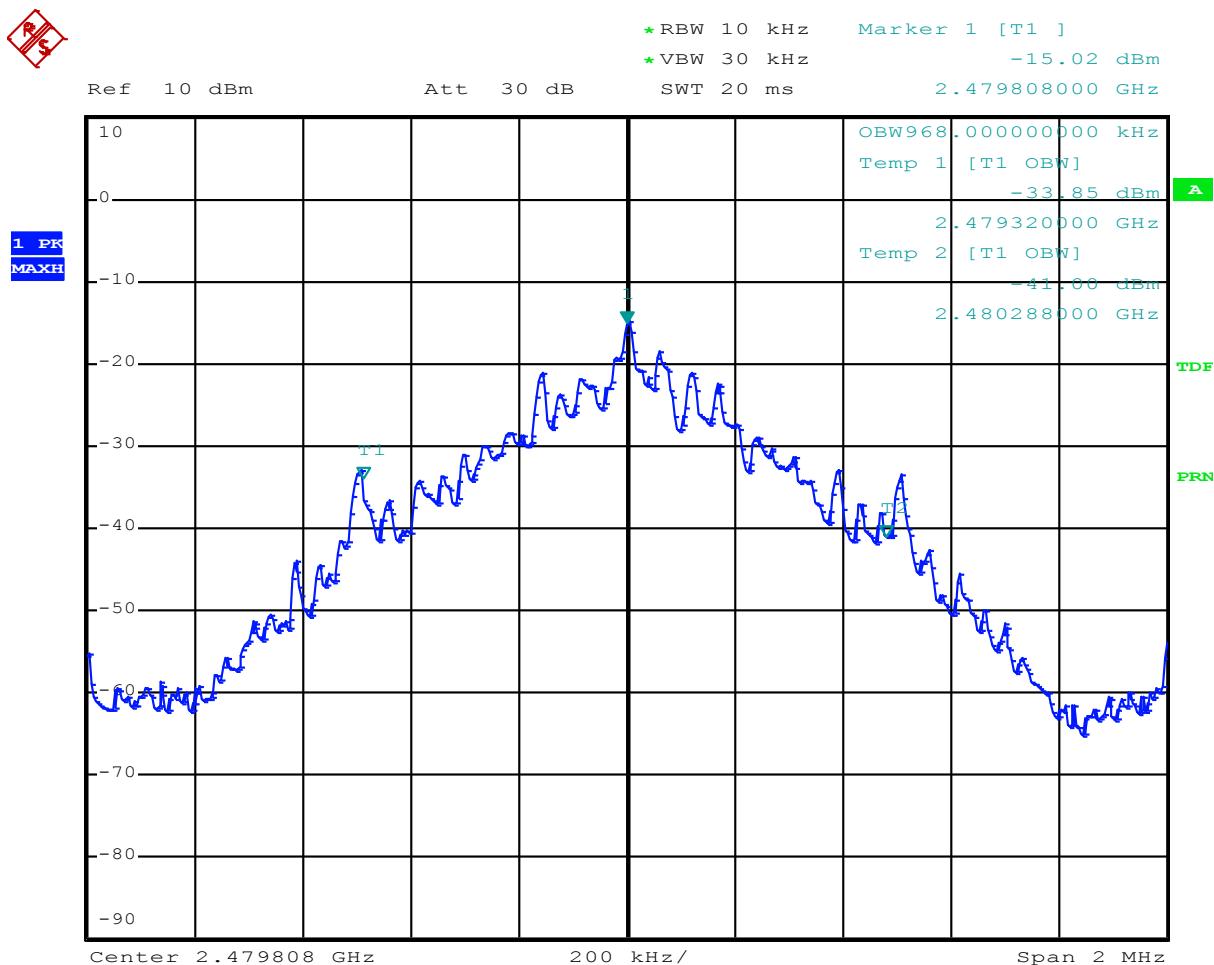

## High Channel 2480 MHz, Data rate DH1, 20 dB Bandwidth = 680 kHz

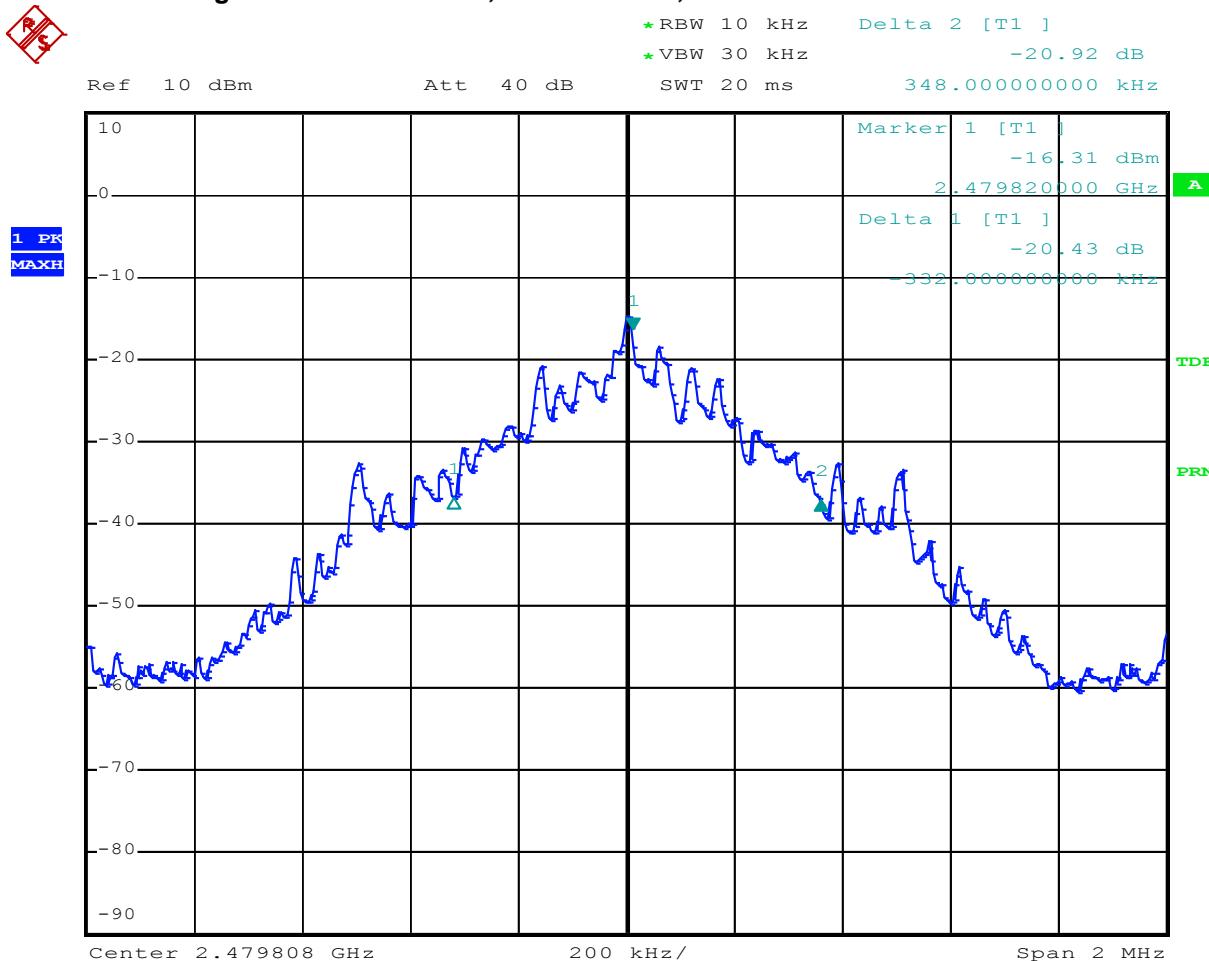

Test Personnel: Naga Suryadevara N.S  
 Supervising/Reviewing  
 Engineer:  
 (Where Applicable) N/A  
 Product Standard: FCC Part 15 Subpart C  
 (15.247) and RSS-247  
 Input Voltage: 12 VDC (System input 120  
 VAC 60 Hz)

Test Date: 08/24/2016

Limit Applied: See test report section 7.3

Ambient Temperature: 22 °C

Pretest Verification: Yes

Relative Humidity: 44 %

Atmospheric Pressure: 1003 mbars

Deviations, Additions, or Exclusions: None

## 8 Channel Separation

### 8.1 Method

Tests are performed in accordance with FCC Part 15 Subpart C (15.247) and RSS 247.

**TEST SITE:** EMC Lab – Intertek Lake Forest CA

**The EMC Lab** has one Semi-anechoic Chamber and one Shielded Chamber. AC Mains Power is available at 120, 230, and 277 Single Phase; 208, 380, and 440 3-Phase. Large reference ground-planes are installed in the general lab area to facilitate EMC work not requiring a shielded environment.

### 8.2 Test Equipment Used:

Asset	Description	Manufacturer	Model	Serial	Cal Date	Cal Due
001001'	Barometer/Humidity Control	Omega	iBTHX-W	0440775	04/22/2016	04/22/2017
000690'	Spectrum Analyzer, 9 KHz - 40 GHz	Rohde & Schwarz	FSP40	100027	01/11/2016	01/11/2017
CBLHF20 12-5M-1'	5m 9kHz-40GHz Coaxial Cable - SET 1	Huber & Suhner	SF102	252676001	02/09/2016	02/09/2017


### Software Utilized:

Name	Manufacturer	Version
None		


### 8.3 Results:

The sample tested was found to Comply. Systems shall have hopping channel carrier frequencies that are separated by 25 kHz or two-thirds of the 20-dB bandwidth of the hopping channel, whichever is greater.

The measured channel frequency separation is 1.002 MHz.

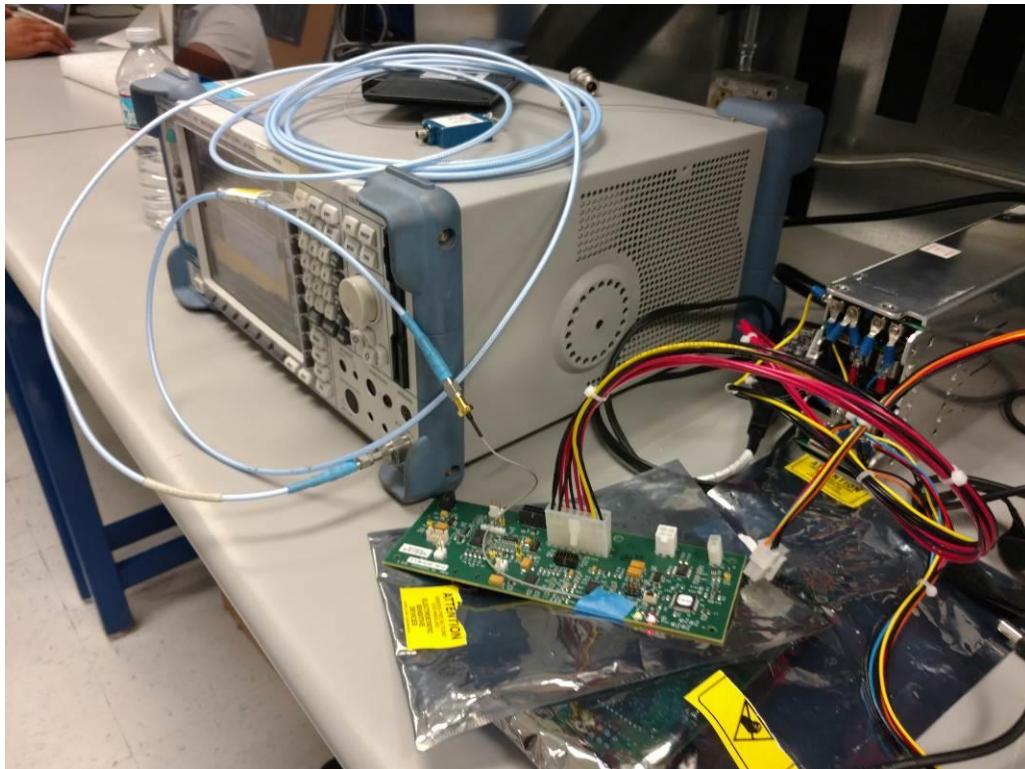**8.4 Setup Photographs:**

## 8.5 Plots/Data:

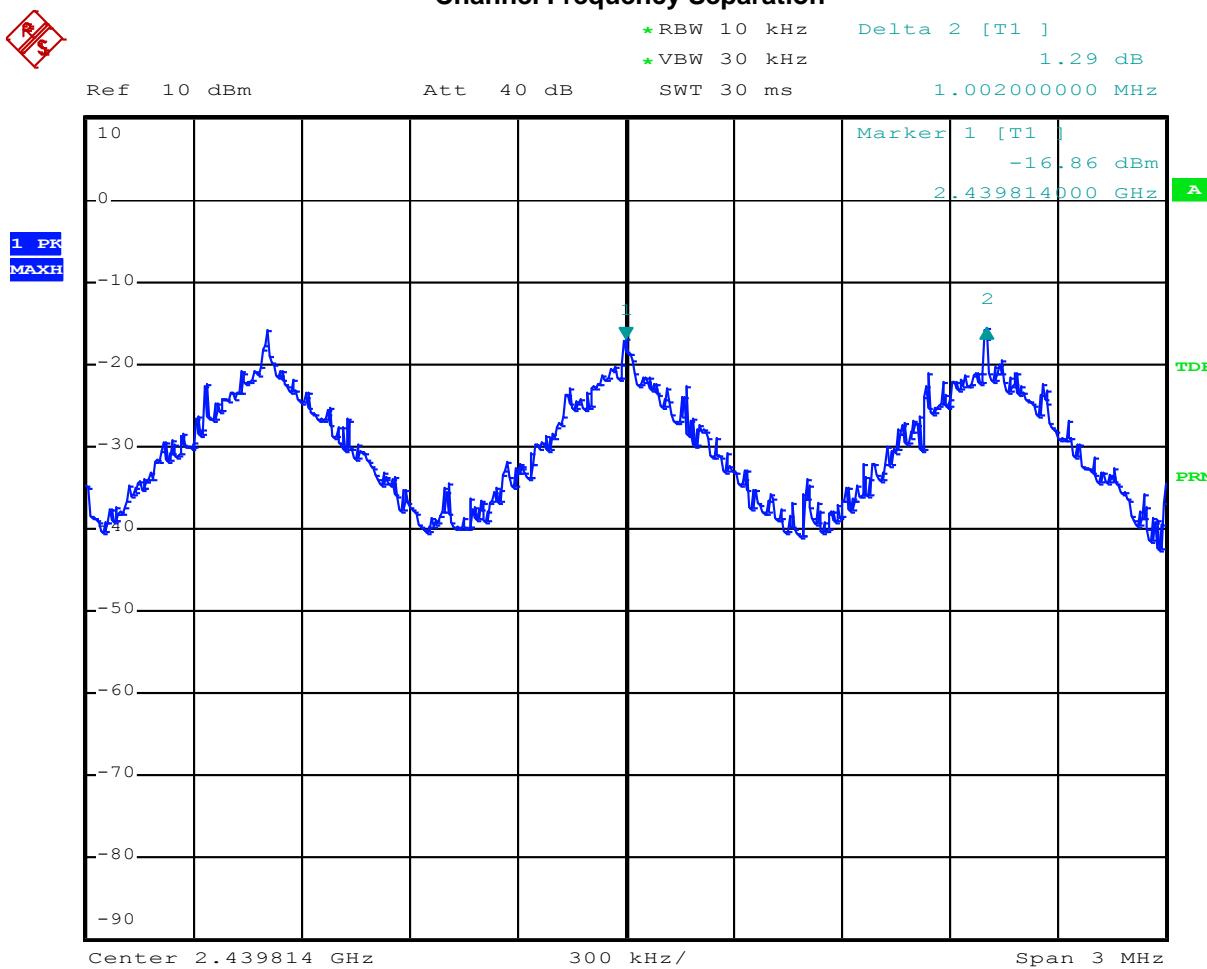

Test Personnel: Naga Suryadevara N5  
 Supervising/Reviewing  
 Engineer:  
 (Where Applicable) N/A  
 Product Standard: FCC Part 15 Subpart C  
(15.247) and RSS-247  
 Input Voltage: 12 VDC (System input 120 VAC 60 Hz)

Test Date: 08/24/2016

Limit Applied: See test report section 8.3

Pretest Verification: Yes

Ambient Temperature: 22 °C

Relative Humidity: 44 %

Atmospheric Pressure: 1003 mbars

Deviations, Additions, or Exclusions: None

## 9 Number of Hopping Channels

### 9.1 Method

Tests are performed in accordance with FCC Part 15 Subpart C (15.247) and RSS 247.

**TEST SITE:** EMC Lab – Intertek Lake Forest CA

**The EMC Lab** has one Semi-anechoic Chamber and one Shielded Chamber. AC Mains Power is available at 120, 230, and 277 Single Phase; 208, 380, and 440 3-Phase. Large reference ground-planes are installed in the general lab area to facilitate EMC work not requiring a shielded environment.

### 9.2 Test Equipment Used:

Asset	Description	Manufacturer	Model	Serial	Cal Date	Cal Due
001001'	Barometer/Humidity Control	Omega	iBTHX-W	0440775	04/22/2016	04/22/2017
000690'	Spectrum Analyzer, 9 KHz - 40 GHz	Rohde & Schwarz	FSP40	100027	01/11/2016	01/11/2017
CBLHF20 12-5M-1'	5m 9kHz-40GHz Coaxial Cable - SET 1	Huber & Suhner	SF102	252676001	02/09/2016	02/09/2017


### Software Utilized:

Name	Manufacturer	Version
None		


### 9.3 Results:

The sample tested was found to Comply. Systems operating in the 2400-2483.5 MHz band shall use at least 15 hopping channels.

The System has 79 hopping channels.

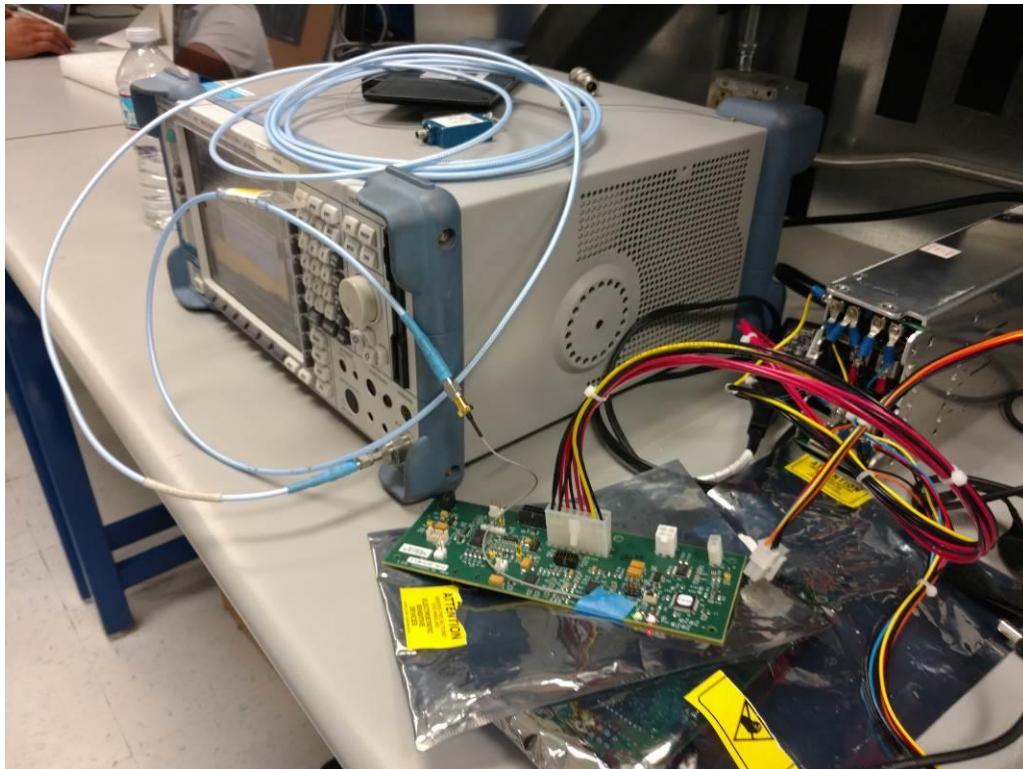**9.4 Setup Photographs:**

## 9.5 Plots/Data:

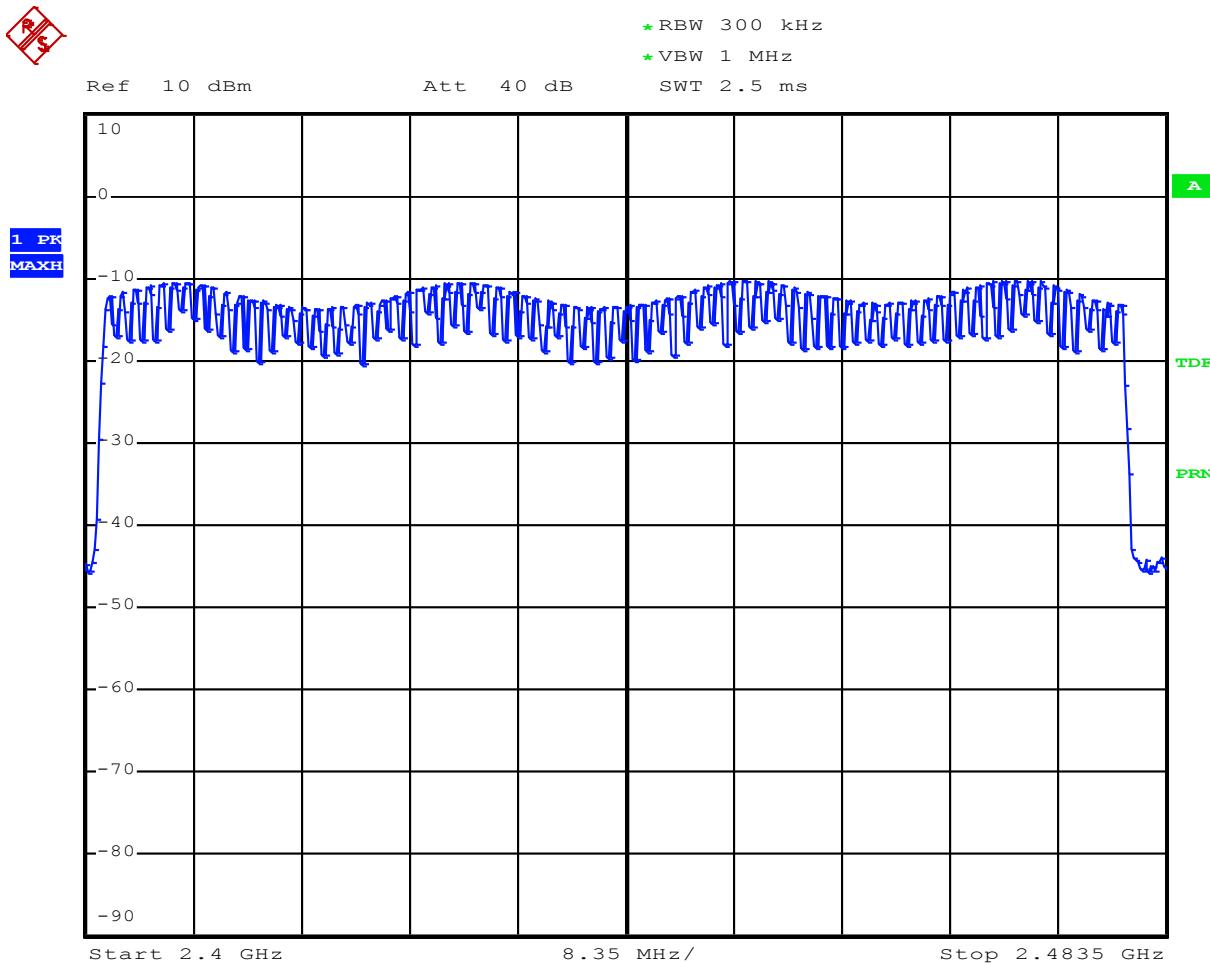

Test Personnel: Naga Suryadevara N.5  
 Supervising/Reviewing  
 Engineer:  
 (Where Applicable) N/A  
 Product Standard: FCC Part 15 Subpart C  
(15.247) and RSS-247  
 Input Voltage: 12 VDC (System input 120  
VAC 60 Hz)

Test Date: 08/24/2016

Limit Applied: See test report section 9.3

Ambient Temperature: 22 °C

Pretest Verification: Yes

Relative Humidity: 44 %

Atmospheric Pressure: 1003 mbars

Deviations, Additions, or Exclusions: None

## 10 Average Channel Occupancy Time

### 10.1 Method

Tests are performed in accordance with FCC Part 15 Subpart C (15.247) and RSS 247.

**TEST SITE:** EMC Lab – Intertek Lake Forest CA

**The EMC Lab** has one Semi-anechoic Chamber and one Shielded Chamber. AC Mains Power is available at 120, 230, and 277 Single Phase; 208, 380, and 440 3-Phase. Large reference ground-planes are installed in the general lab area to facilitate EMC work not requiring a shielded environment.

### 10.2 Test Equipment Used:

Asset	Description	Manufacturer	Model	Serial	Cal Date	Cal Due
001001'	Barometer/Humidity Control	Omega	iBTHX-W	0440775	04/22/2016	04/22/2017
000690'	Spectrum Analyzer, 9 KHz - 40 GHz	Rohde & Schwarz	FSP40	100027	01/11/2016	01/11/2017
CBLHF20 12-5M-1'	5m 9kHz-40GHz Coaxial Cable - SET 1	Huber & Suhner	SF102	252676001	02/09/2016	02/09/2017

### Software Utilized:


Name	Manufacturer	Version
None		


### 10.3 Results:

The sample tested was found to Comply. For systems operating in the 2400-2483.5 MHz band, the average time of occupancy on any channel shall not be greater than 0.4 second within a period of 0.4 second multiplied by the number of hopping channels employed


Since the radio employs 79 channels, Occupancy time was calculated during the period of  $0.4 * 79 = 31.6$  sec.

Occupancy Time (see plots in section 9.5) =  $0.00282 * 13 * 10 = 0.3666$  sec

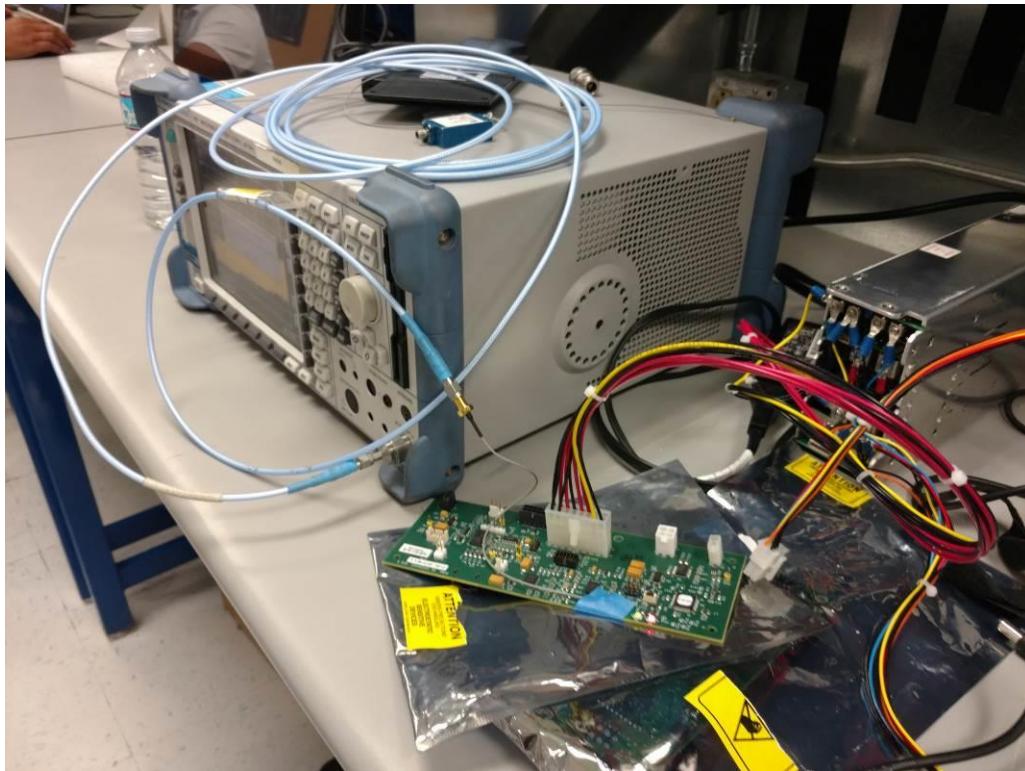**10.4 Setup Photographs:**

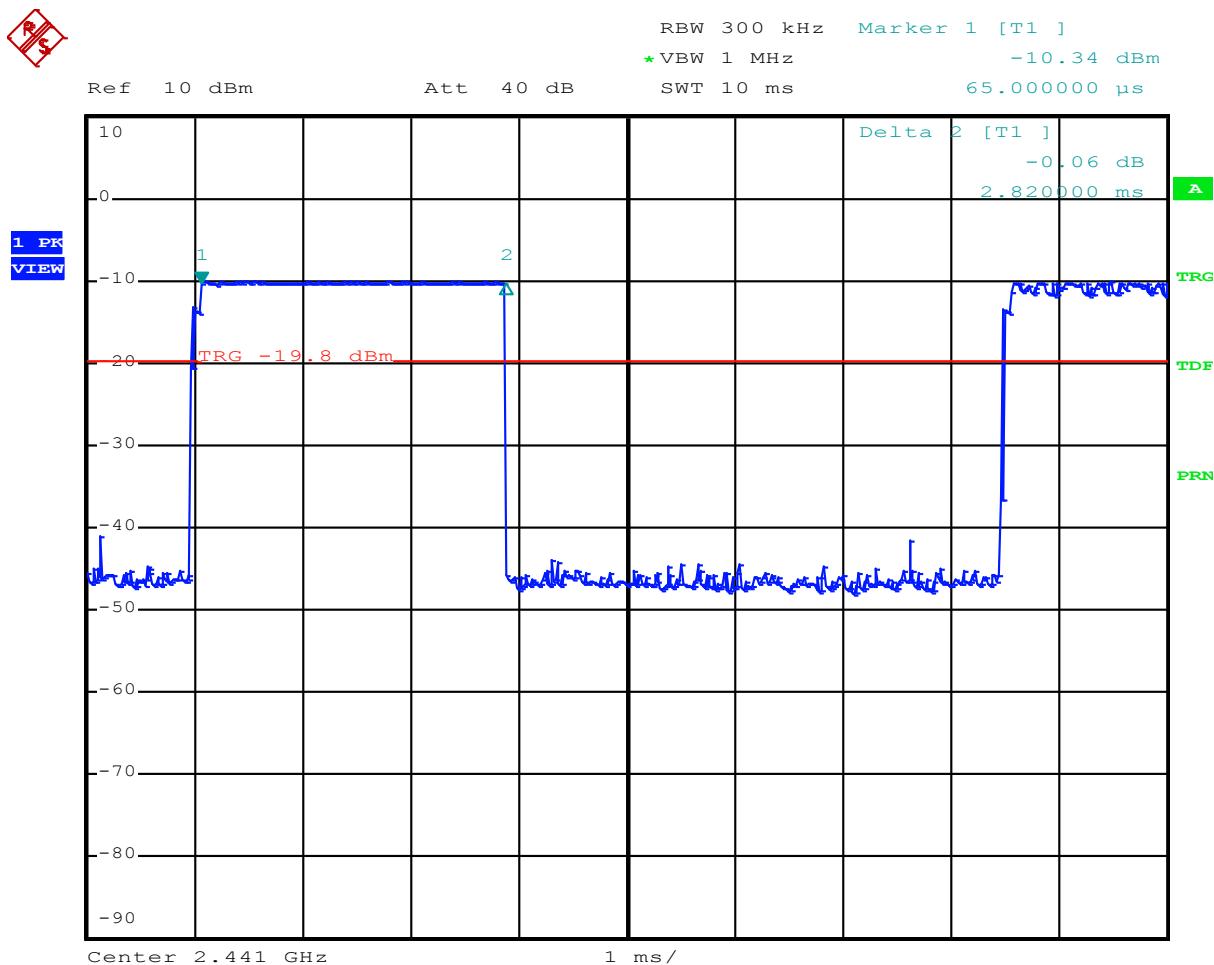**10.5 Plots/Data:**

RS

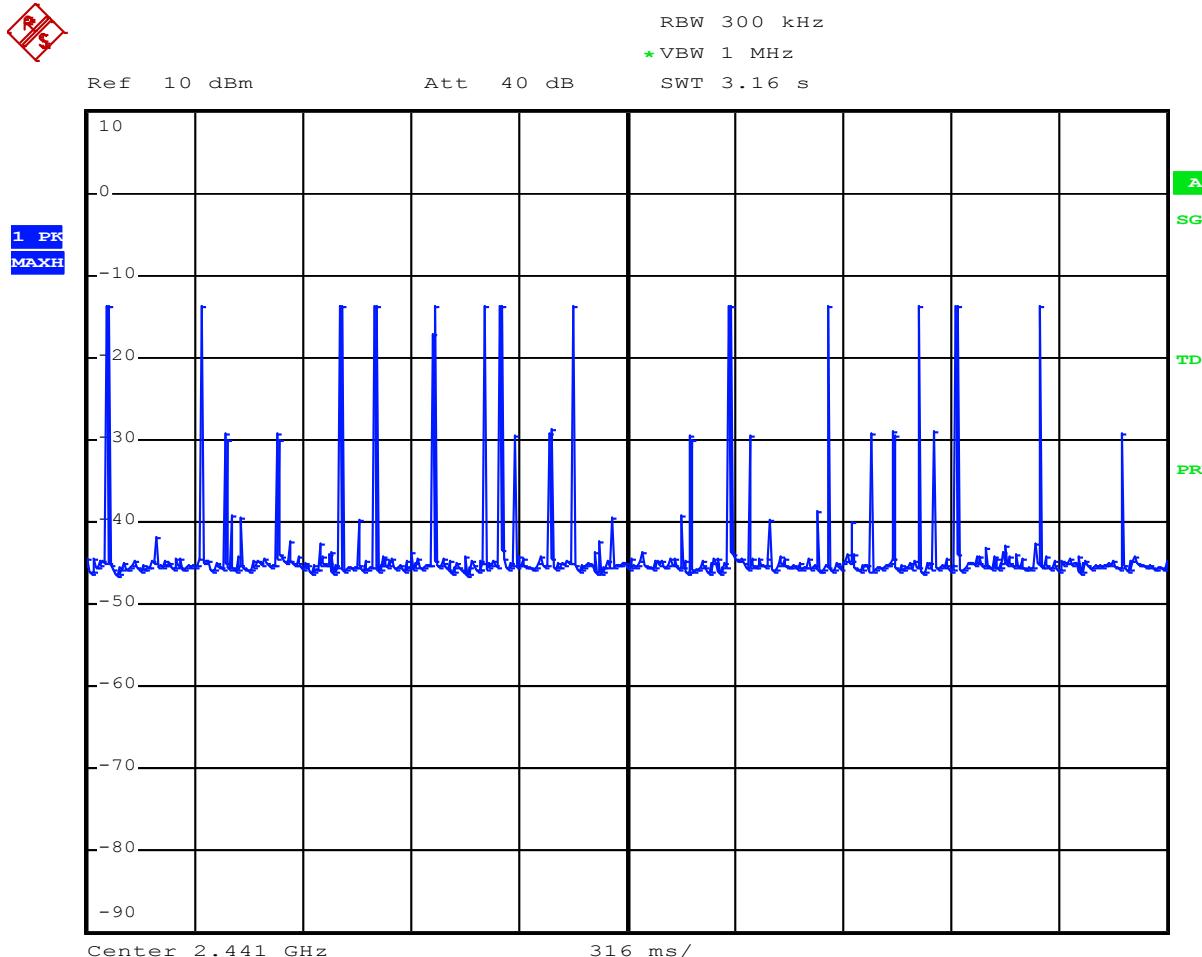

Test Personnel: Naga Suryadevara N.5  
 Supervising/Reviewing  
 Engineer:  
 (Where Applicable) N/A  
 Product Standard: FCC Part 15 Subpart C  
(15.247) and RSS-247  
 Input Voltage: 12 VDC (System input 120  
VAC 60 Hz)

Test Date: 08/24/2016

Limit Applied: See test report section 10.3

Ambient Temperature: 22 °C

Pretest Verification: Yes

Relative Humidity: 44 %

Atmospheric Pressure: 1003 mbars

Deviations, Additions, or Exclusions: None

## 11 Out of Band and Band Edge Conducted Emissions

### 11.1 Method

Tests are performed in accordance with FCC Part 15 Subpart C (15.247) and RSS 247.

**TEST SITE:** EMC Lab – Intertek Lake Forest CA

**The EMC Lab** has one Semi-anechoic Chamber and one Shielded Chamber. AC Mains Power is available at 120, 230, and 277 Single Phase; 208, 380, and 440 3-Phase. Large reference ground-planes are installed in the general lab area to facilitate EMC work not requiring a shielded environment.

### 11.2 Test Equipment Used:

Asset	Description	Manufacturer	Model	Serial	Cal Date	Cal Due
001001'	Barometer/Humidity Control	Omega	iBTHX-W	0440775	04/22/2016	04/22/2017
000690'	Spectrum Analyzer, 9 KHz - 40 GHz	Rohde & Schwarz	FSP40	100027	01/11/2016	01/11/2017
CBLHF20 12-5M-1'	5m 9kHz-40GHz Coaxial Cable - SET 1	Huber & Suhner	SF102	252676001	02/09/2016	02/09/2017


### Software Utilized:


Name	Manufacturer	Version
None		

### 11.3 Results:


The sample tested was found to Comply. In any 100 kHz bandwidth outside the EUT pass-band, the RF power shall be at least 20 dB below that of the maximum in-band 100 kHz emission.

All emissions measured were 20 dB below fundamental as indicated in the plots in sections 11.5.

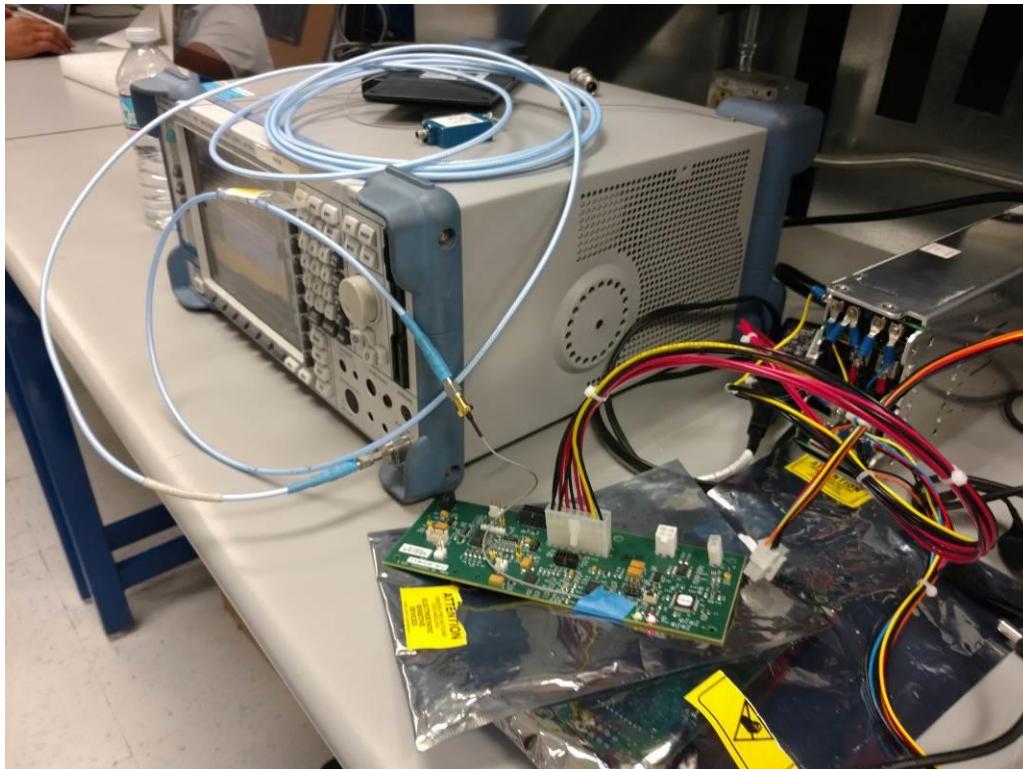
**11.4 Setup Photographs:**

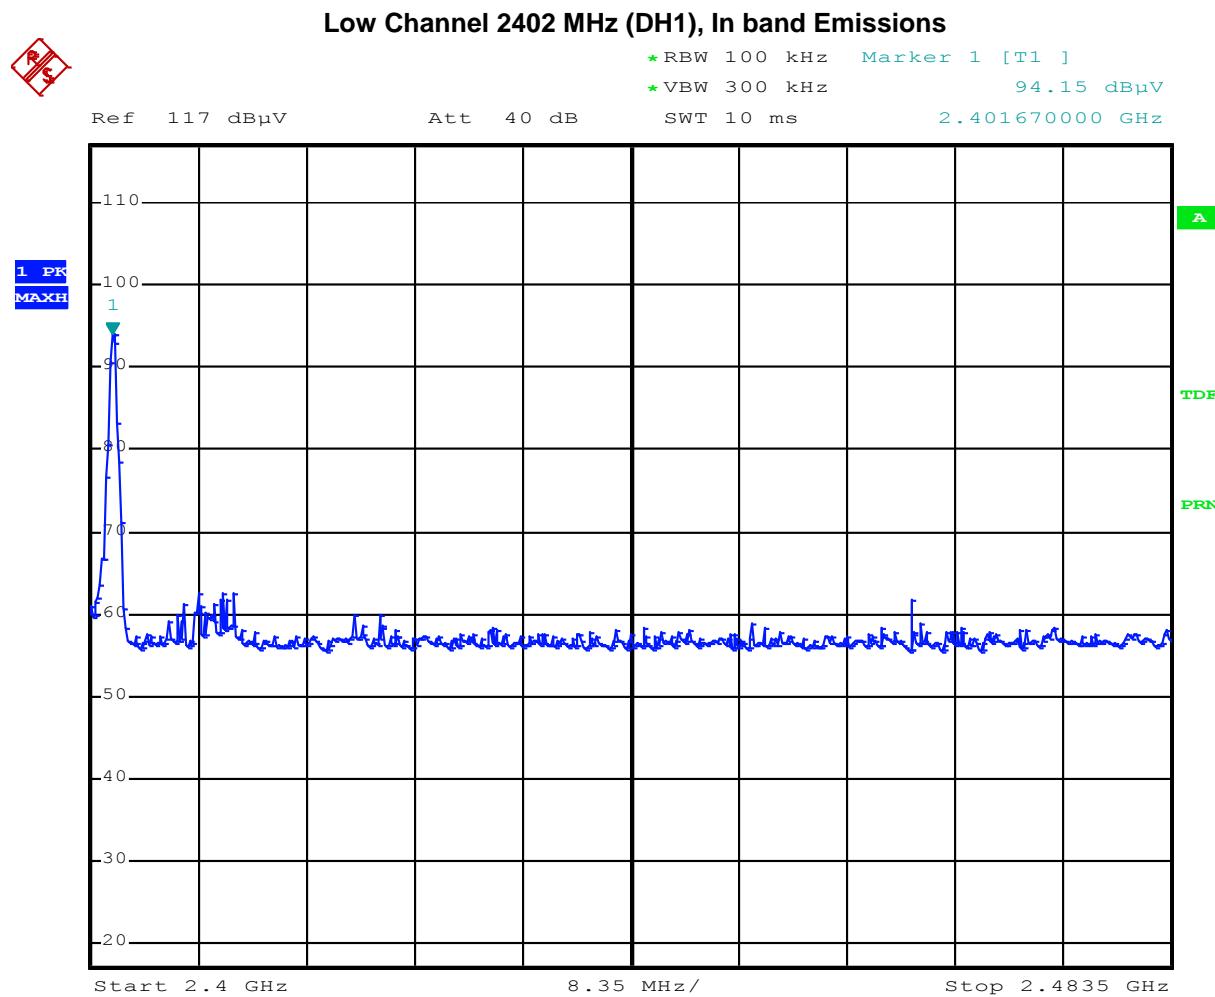**11.5 Plots/Data:**


## Low Channel 2402 MHz (DH1), Out of band Emissions 30 MHz – 2.4 GHz

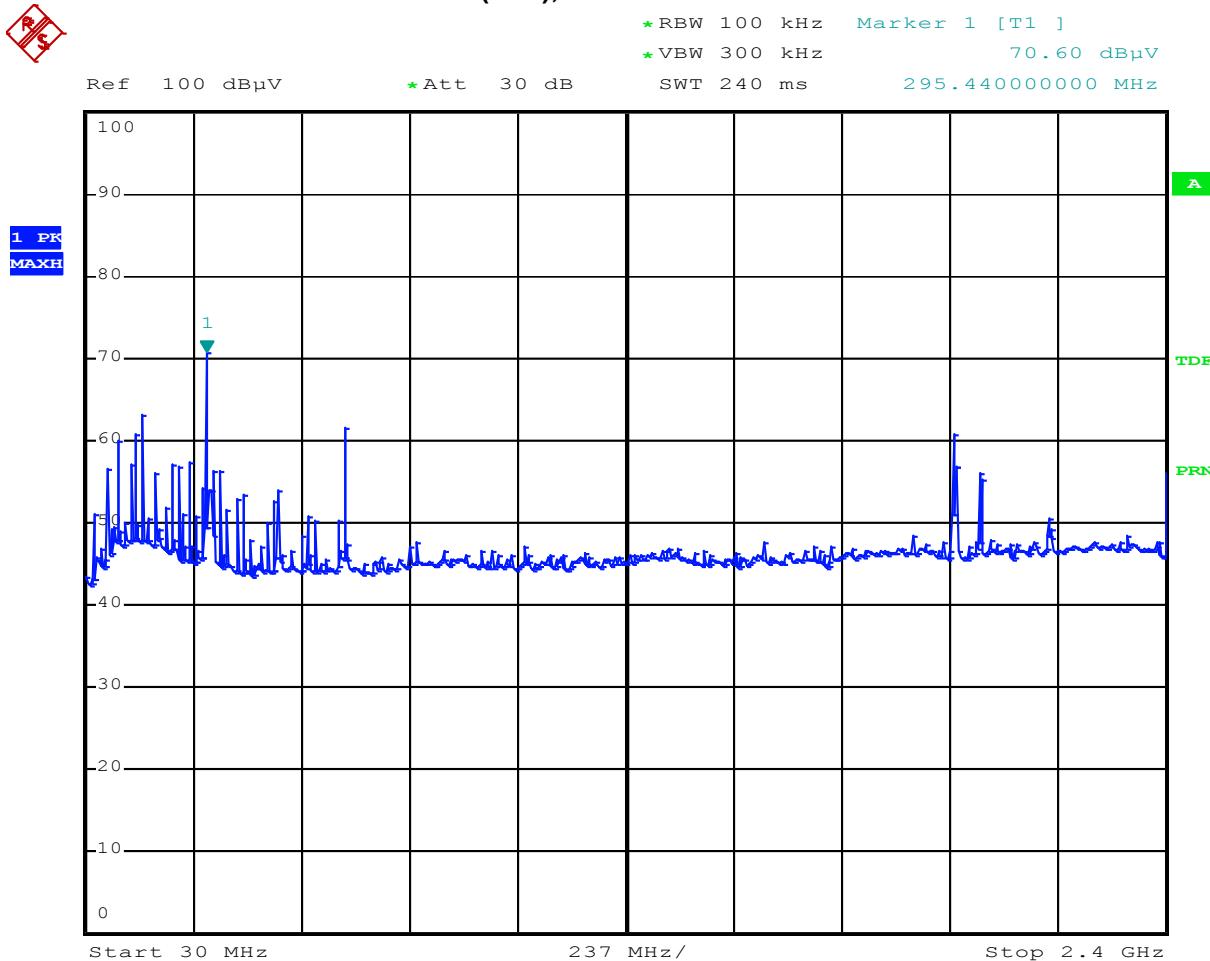


## Low Channel 2402 MHz (DH1), Out of band Emissions 2.4835 - 10 GHz

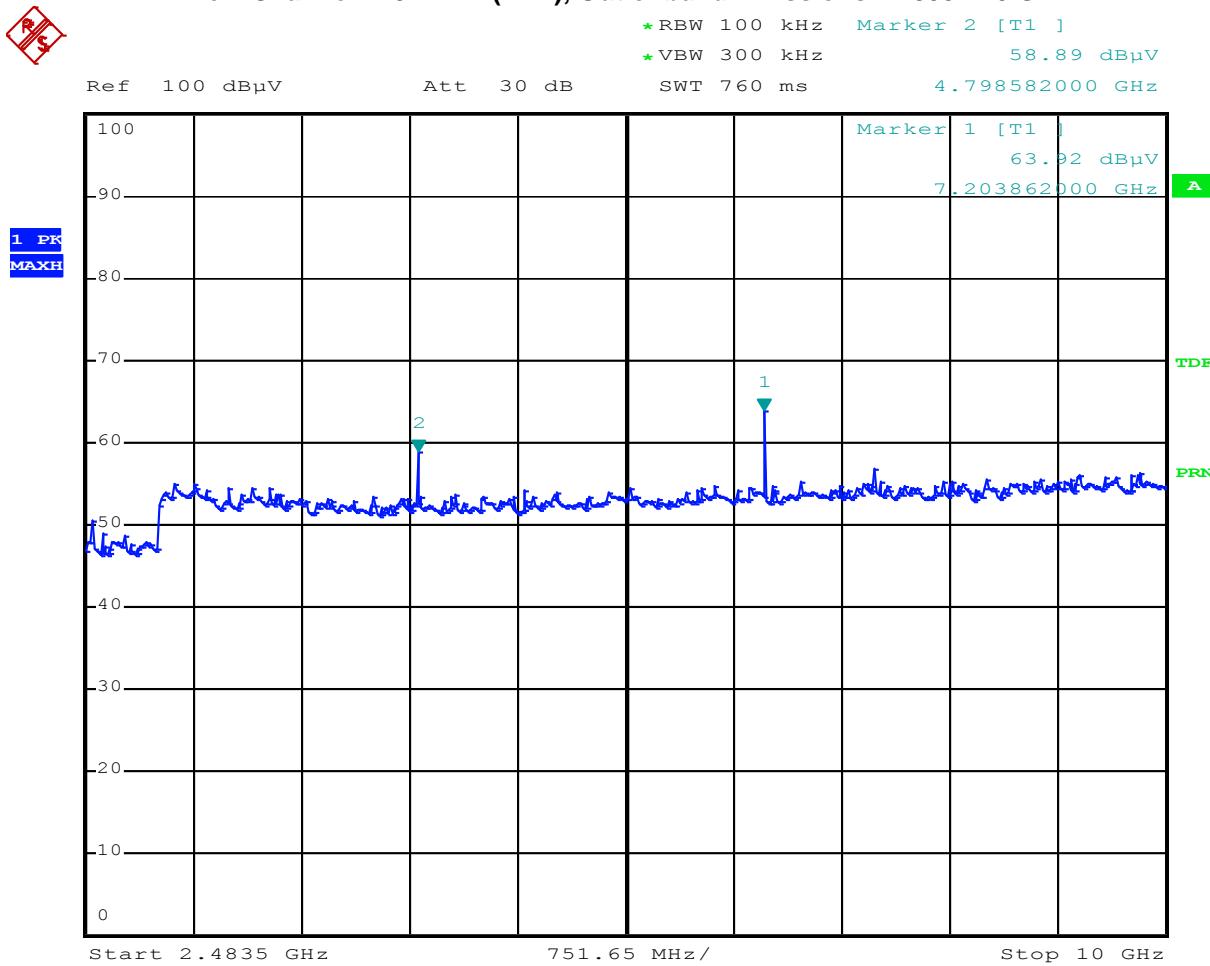


## Low Channel 2402 MHz(DH1), Out of band Emissions 10 - 25 GHz

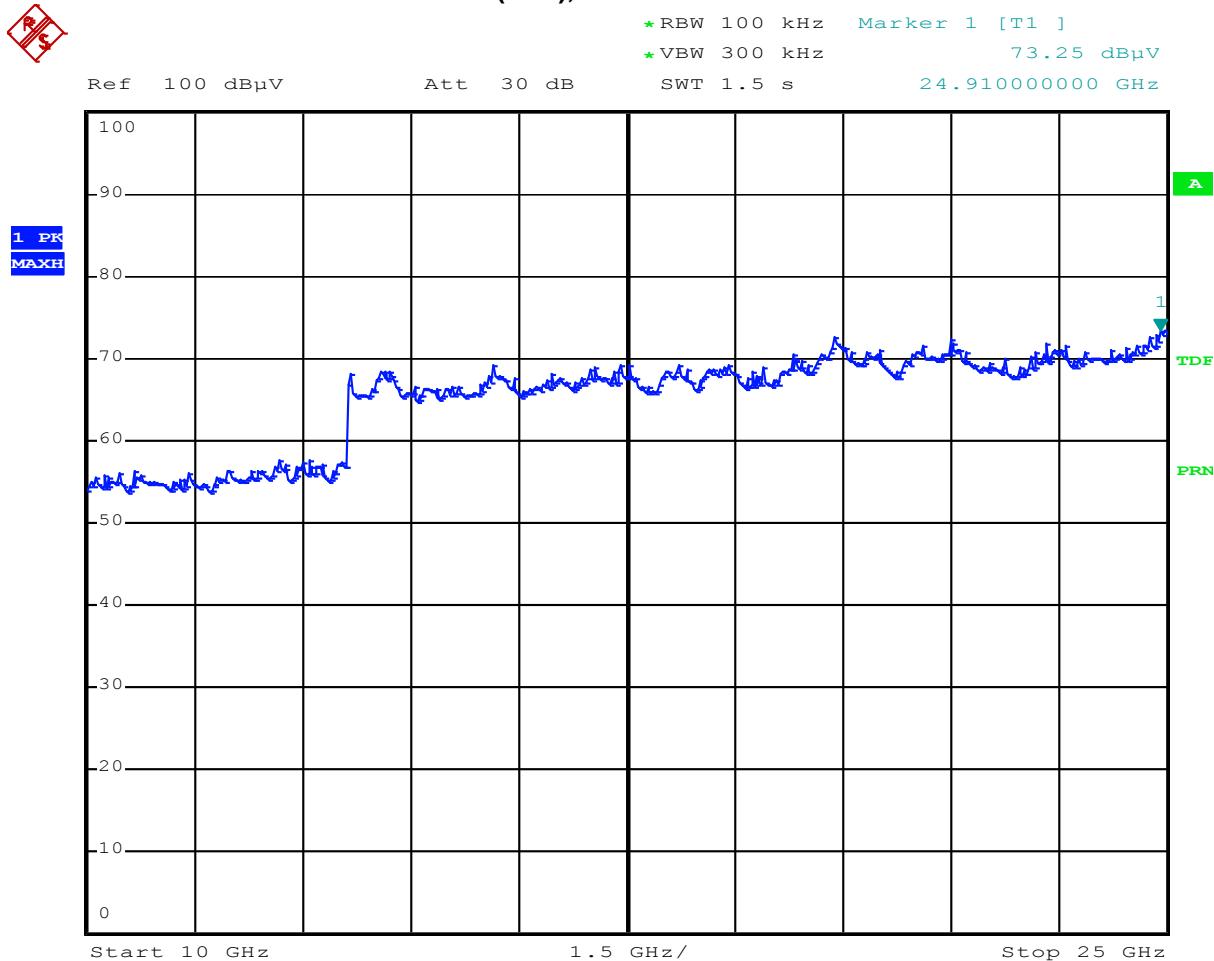


## Mid Channel 2441 MHz (DH3), In band Emissions

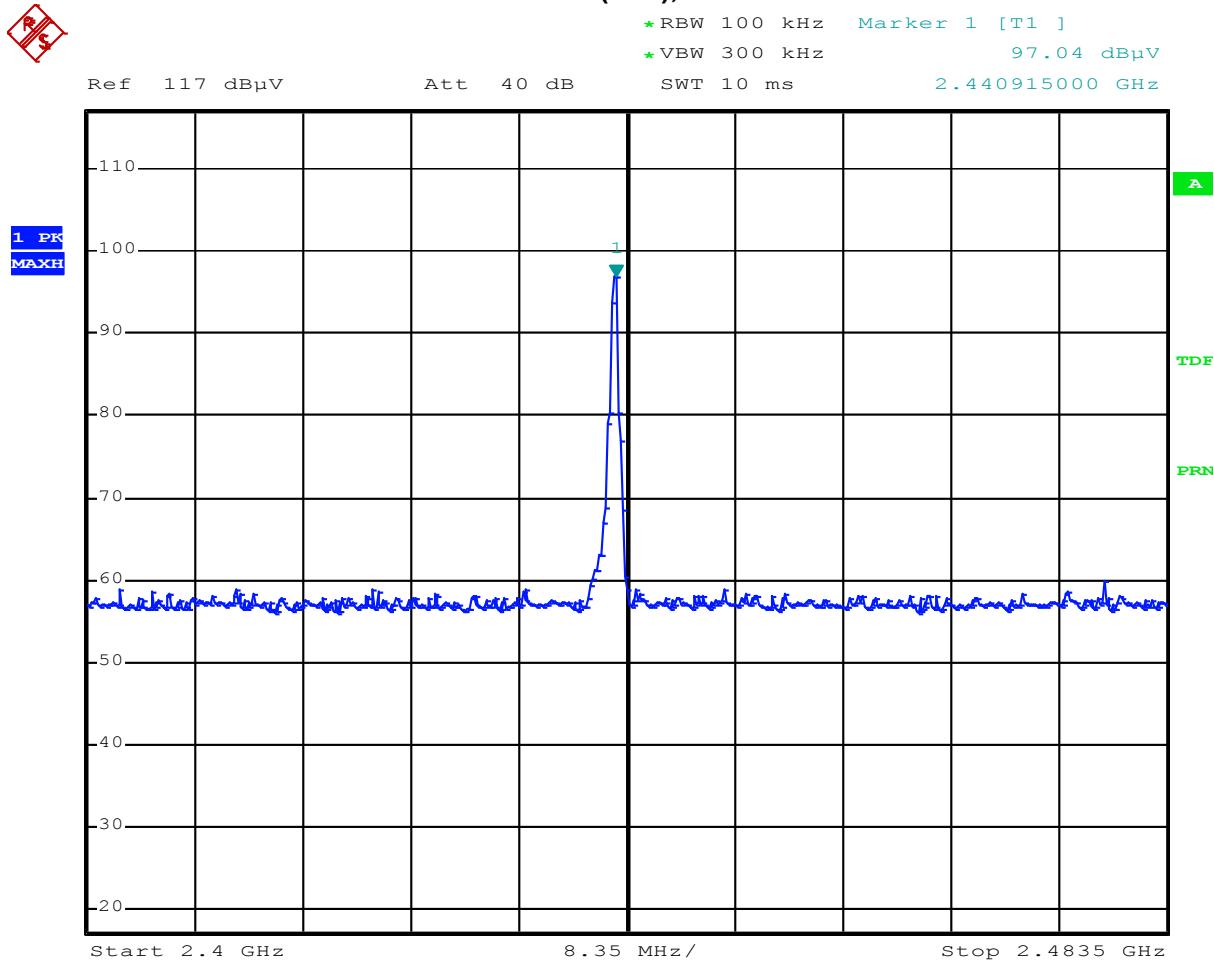


## Mid Channel 2441 MHz (DH3), Out of band Emissions 30 MHz – 2.4 GHz

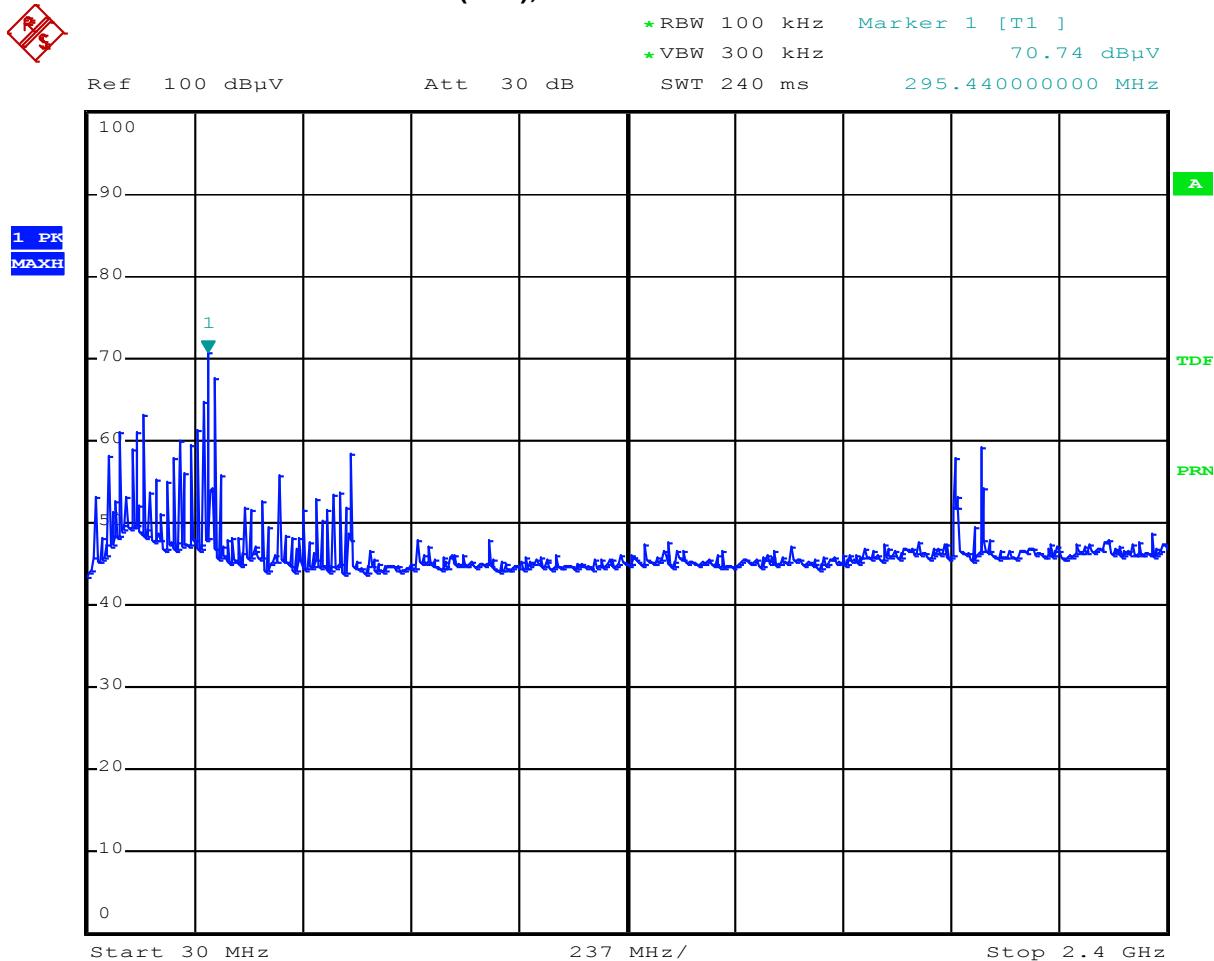


## Mid Channel 2441 MHz (DH3), Out of band Emissions 2.4835 – 10 GHz

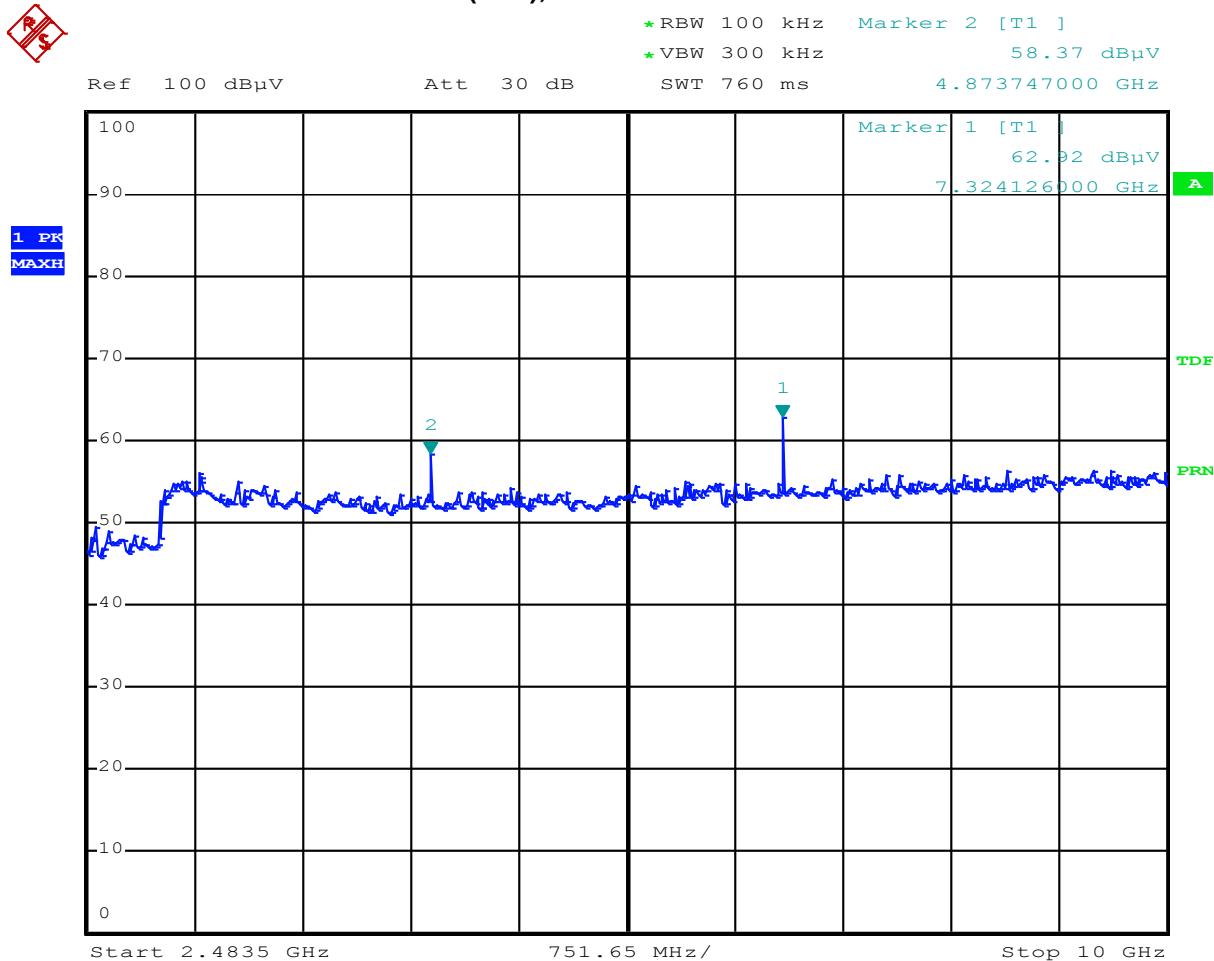


## Mid Channel 2441 MHz (DH3), Out of band Emissions 10 – 25 GHz

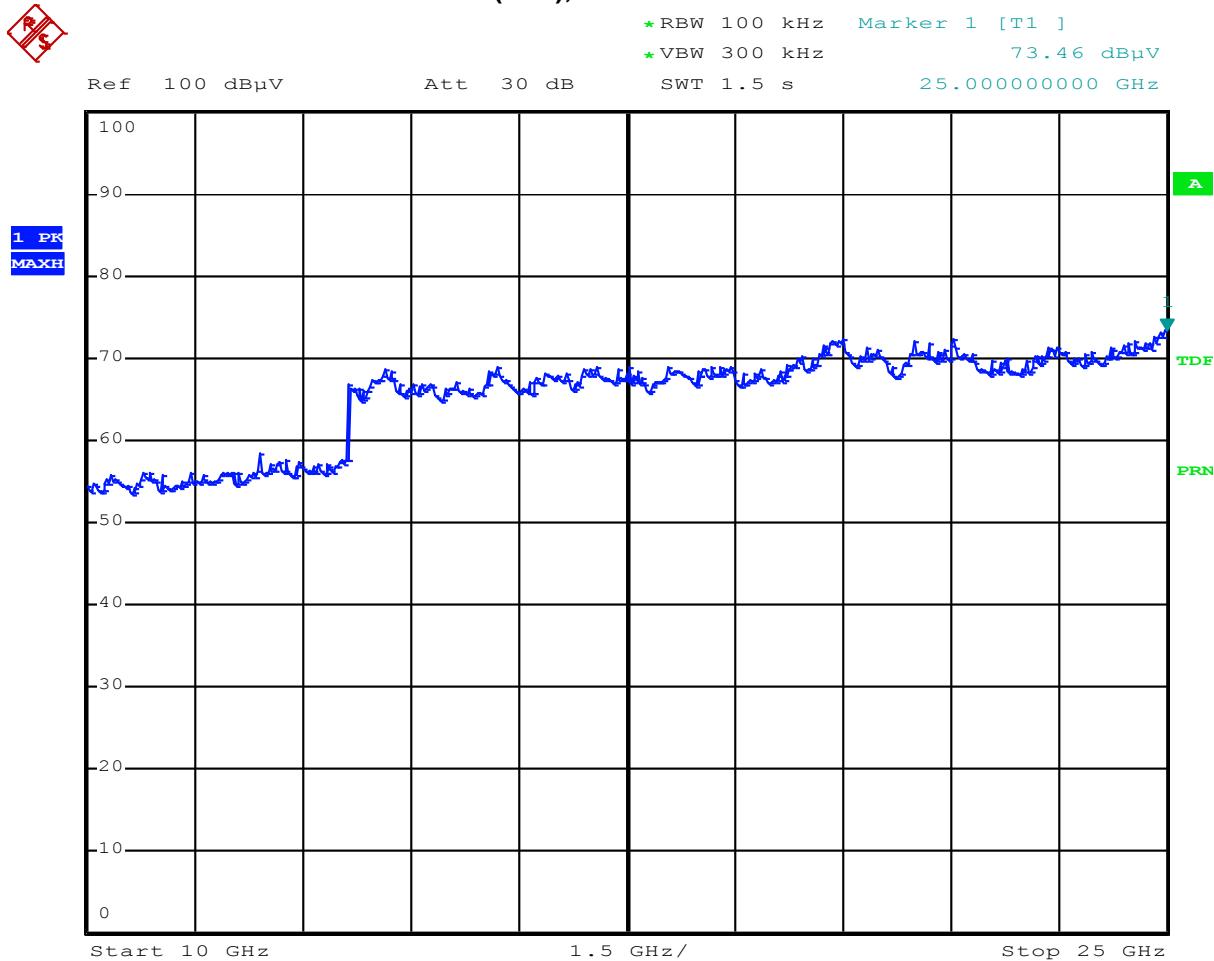


## High Channel 2480 MHz (DH1), In band Emissions

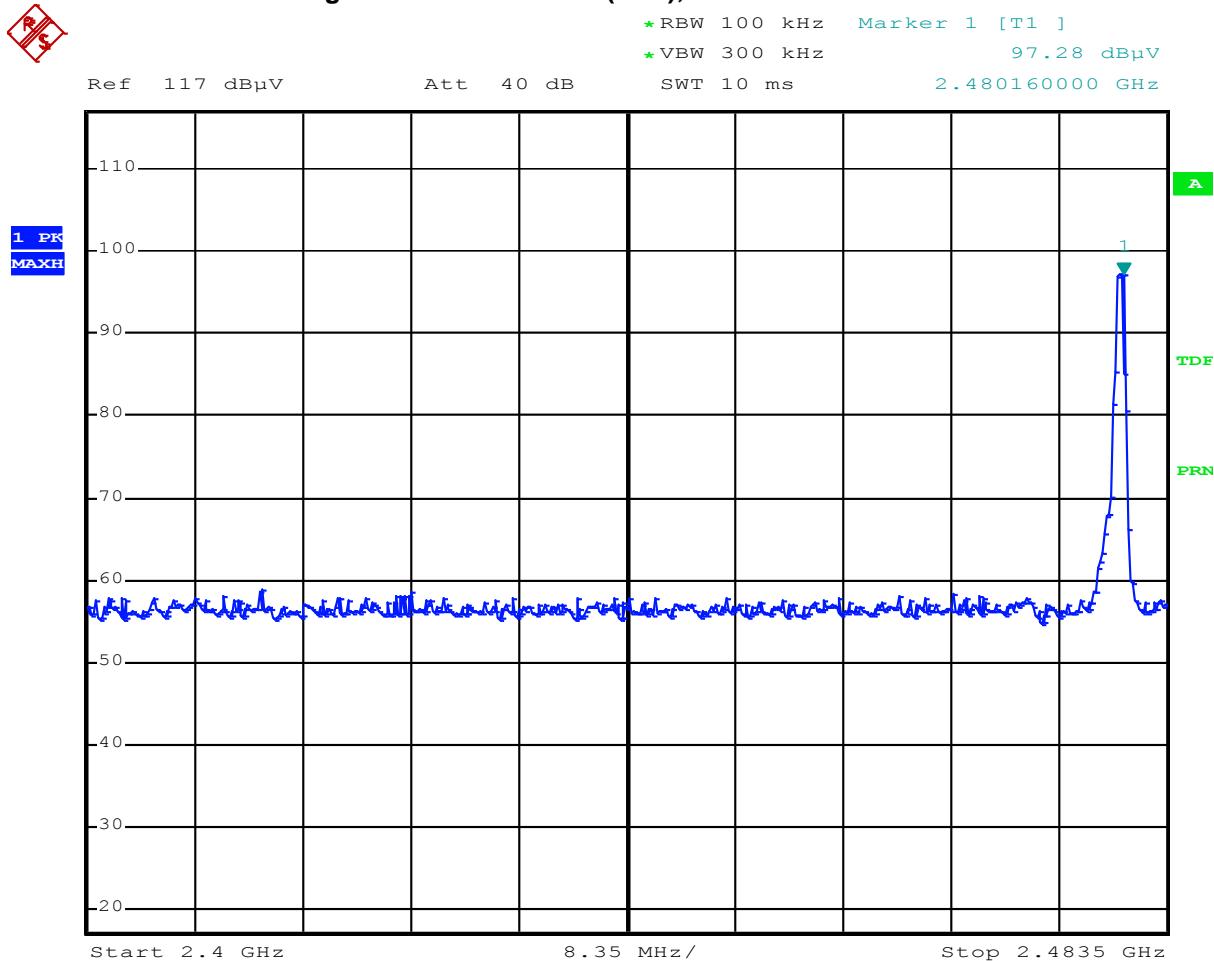


## High Channel 2480 MHz (DH1), Out of band Emissions 30 MHz – 2.4 GHz

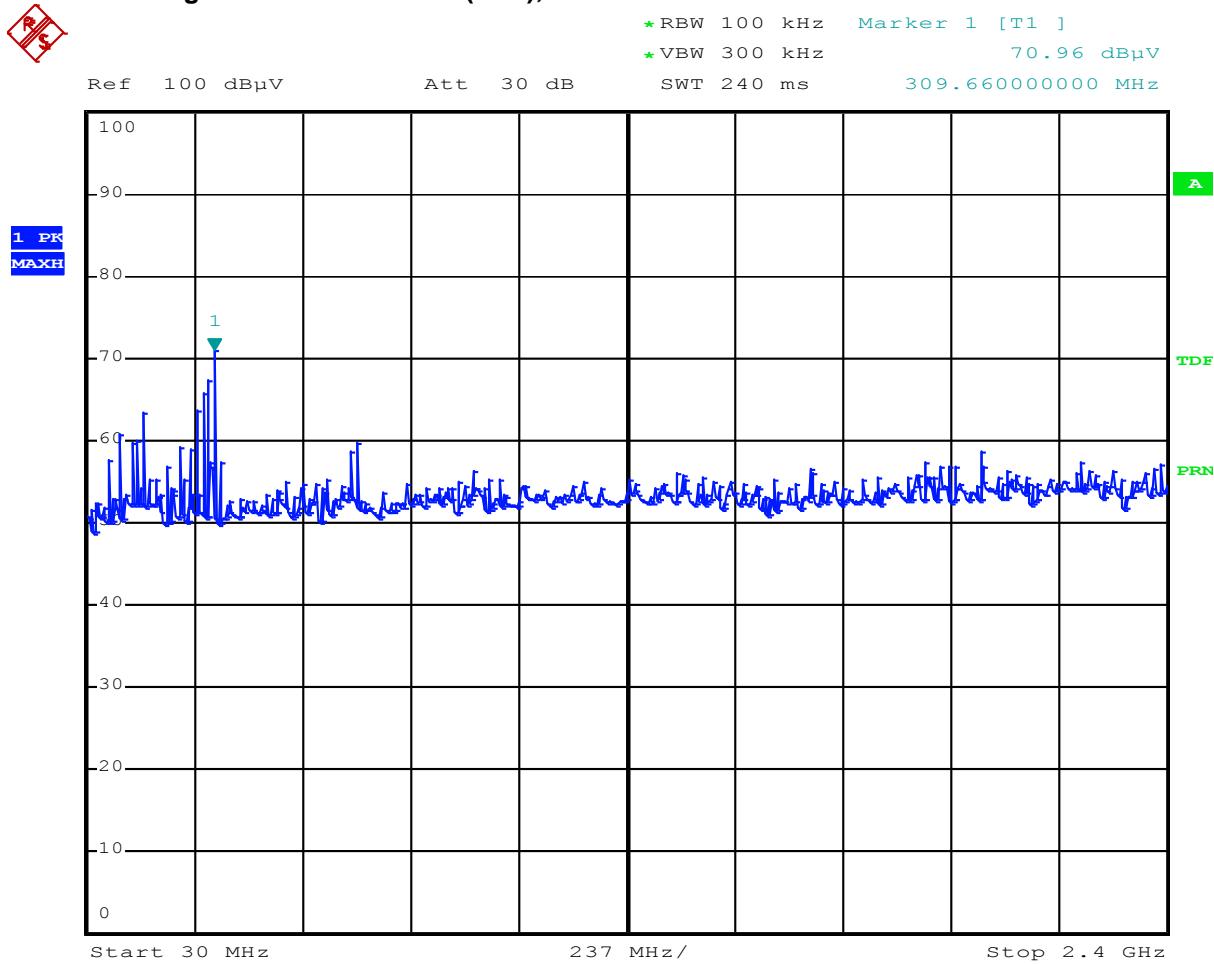


**High Channel 2480 MHz (DH1), Out of band Emissions 2.4835 – 10 GHz**

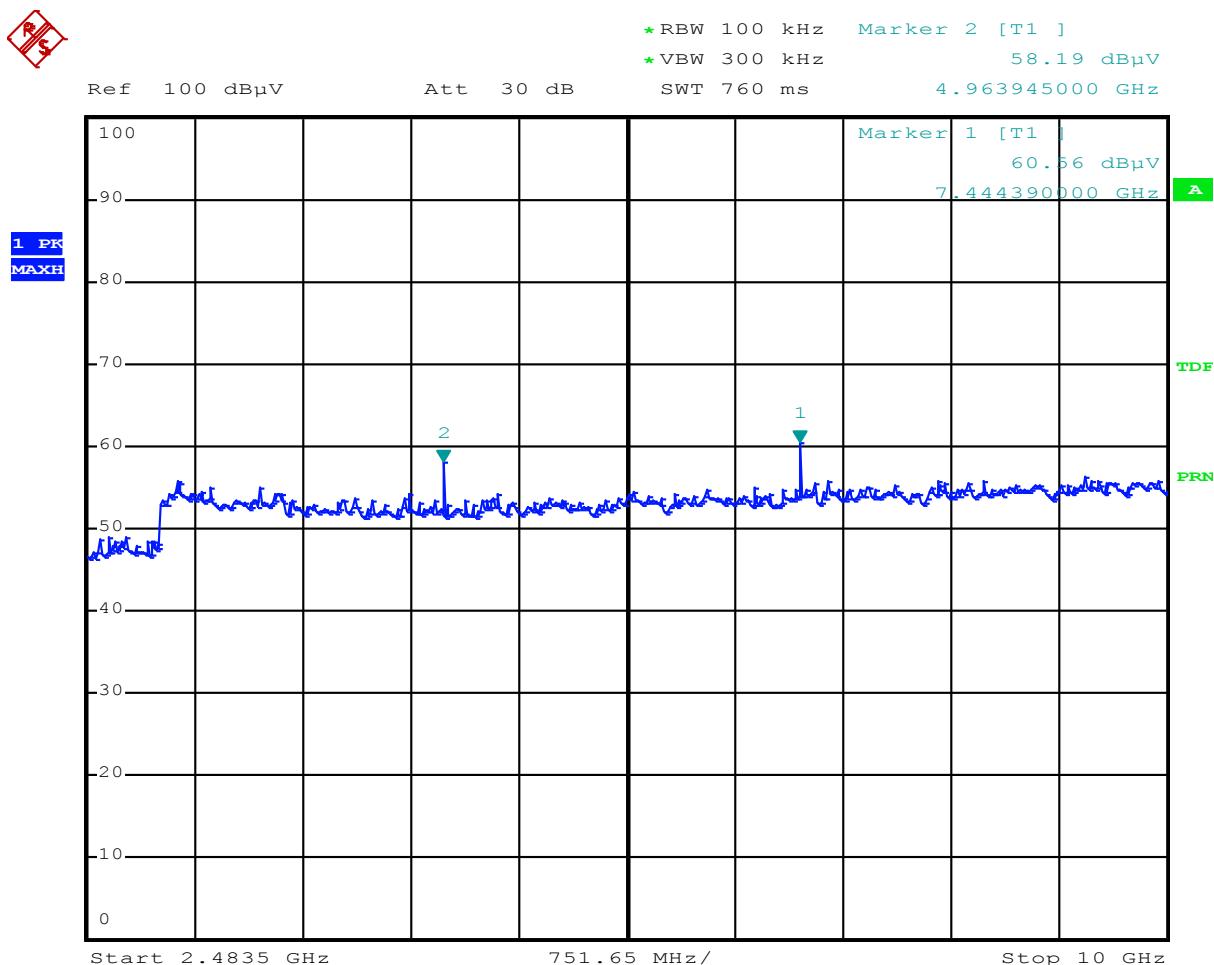


## High Channel 2480 MHz (DH1), Out of band Emissions 10 – 25 GHz

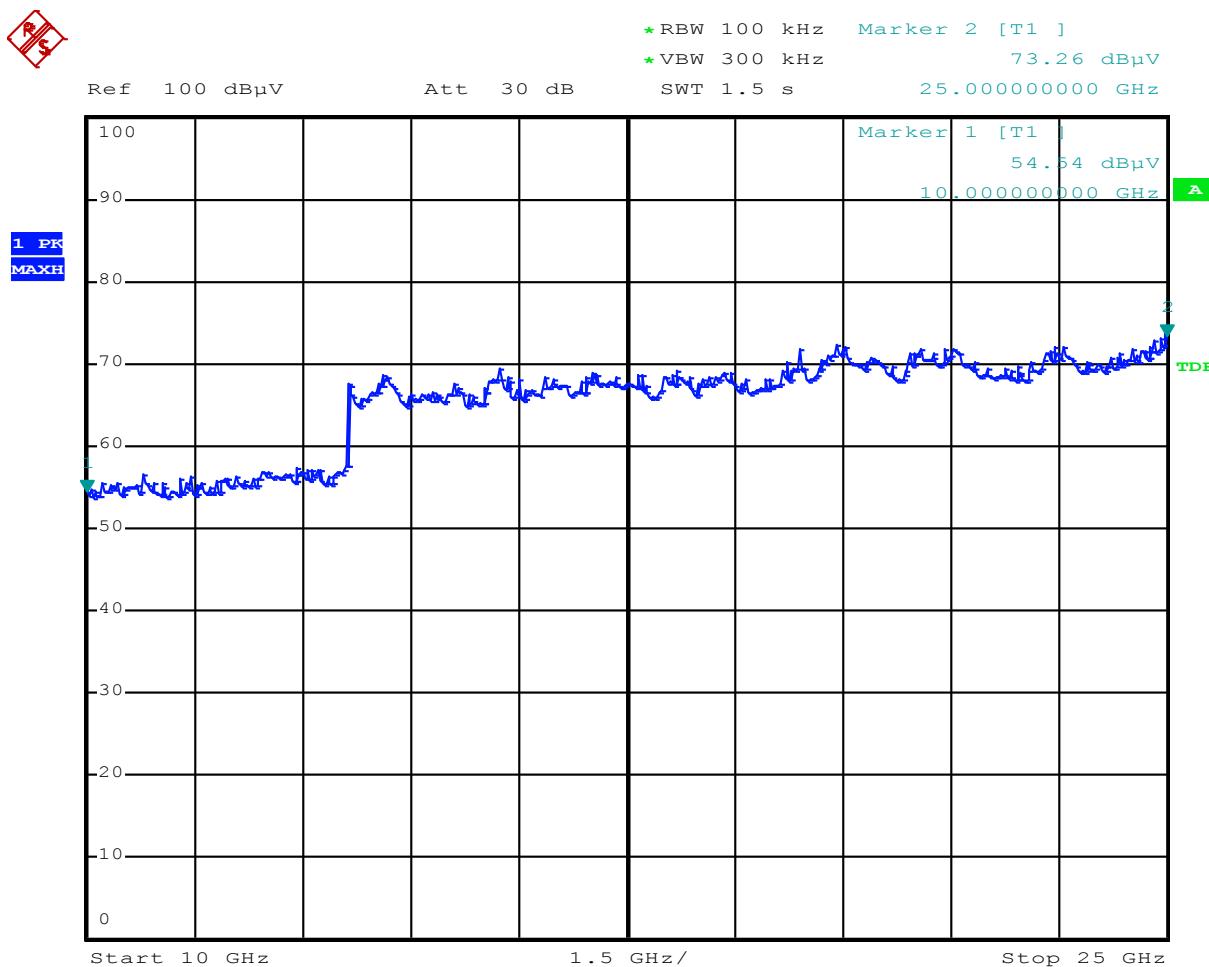


## Emissions on Low Band Edge, Tx fixed to Low Channel 2402 MHz (DH1)

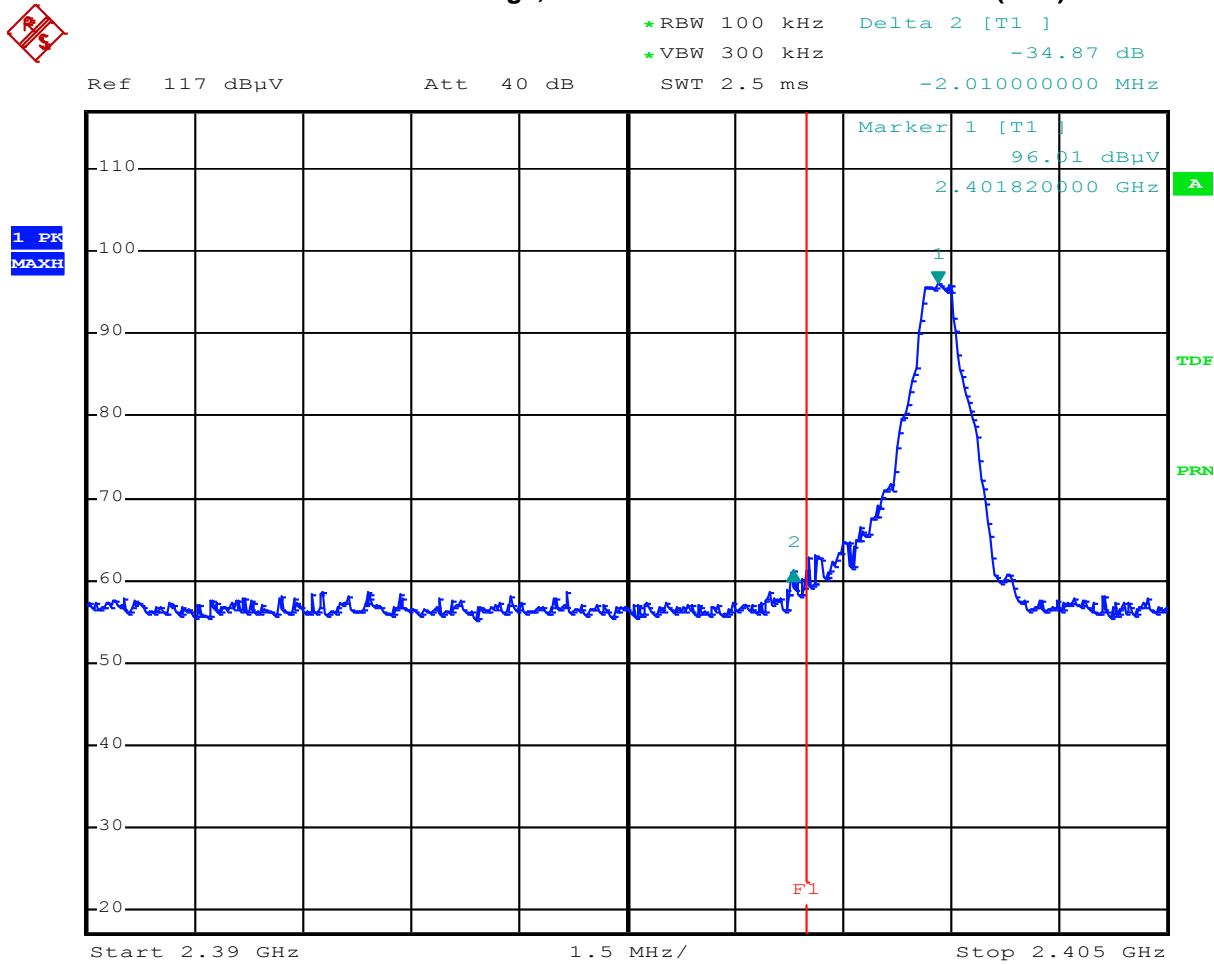


## Emissions on Low Band Edge, Hopping

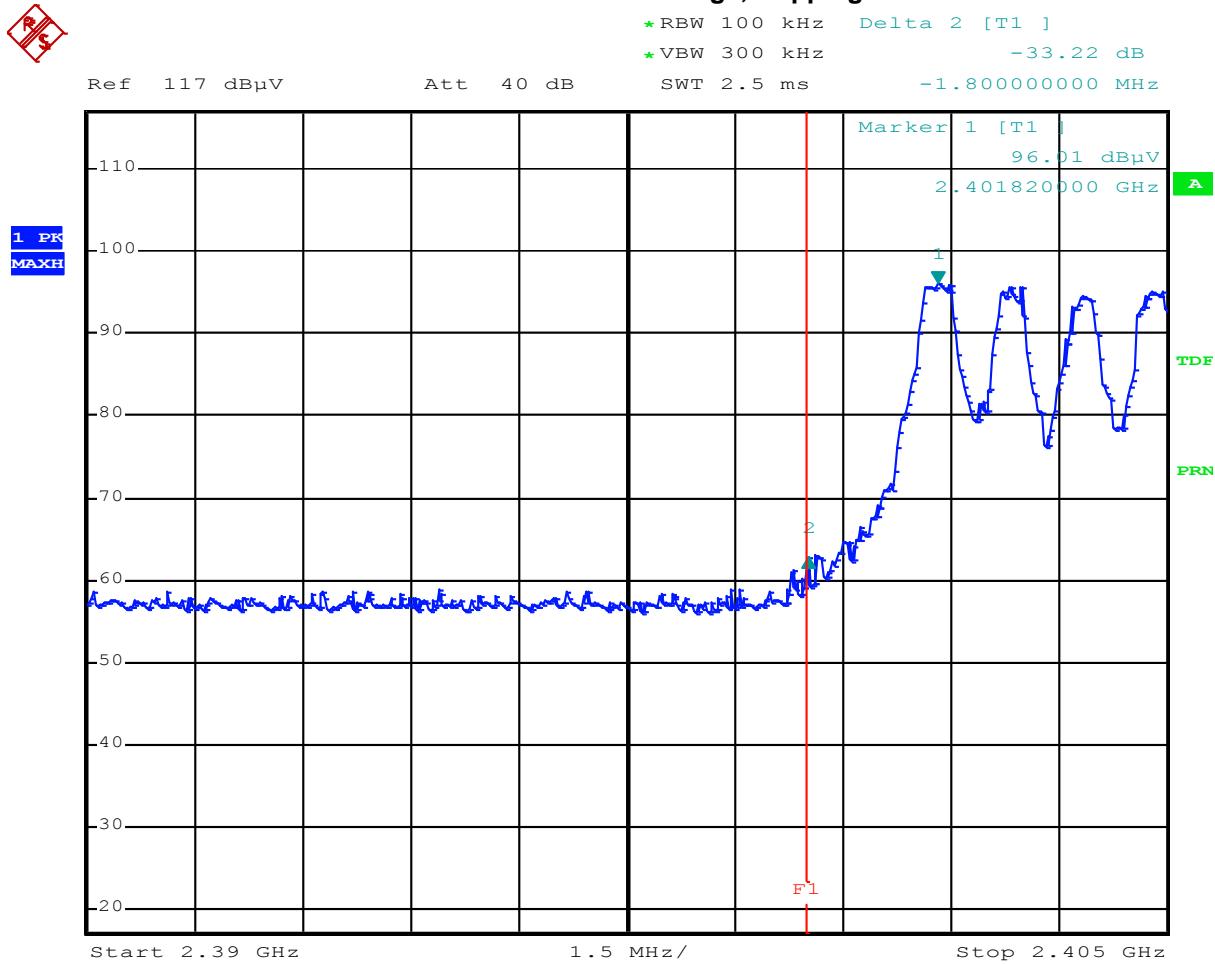

## Emissions on High Band Edge, Tx fixed to High Channel 2480 MHz (DH1)

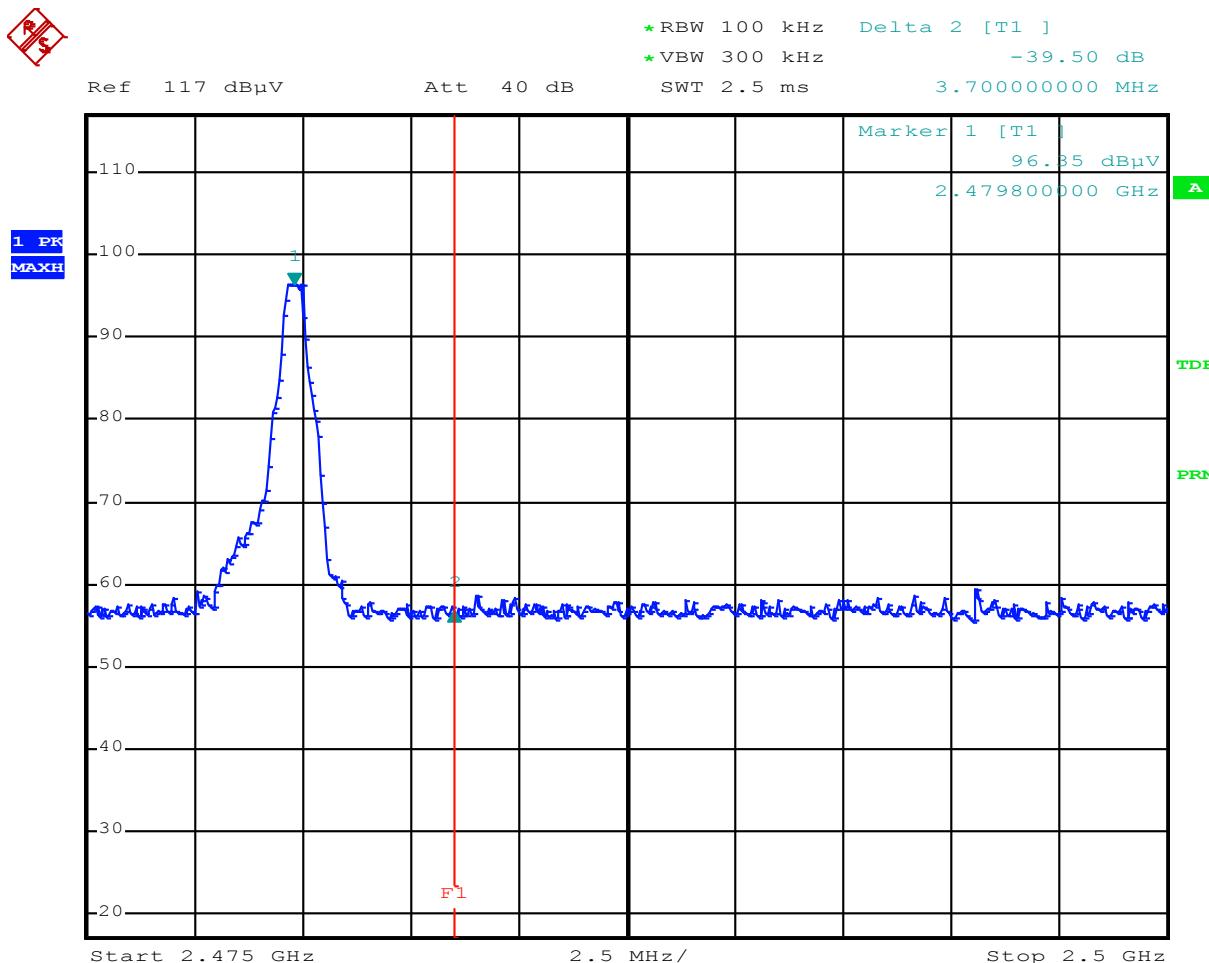

## Emissions on High Band Edge, Hopping

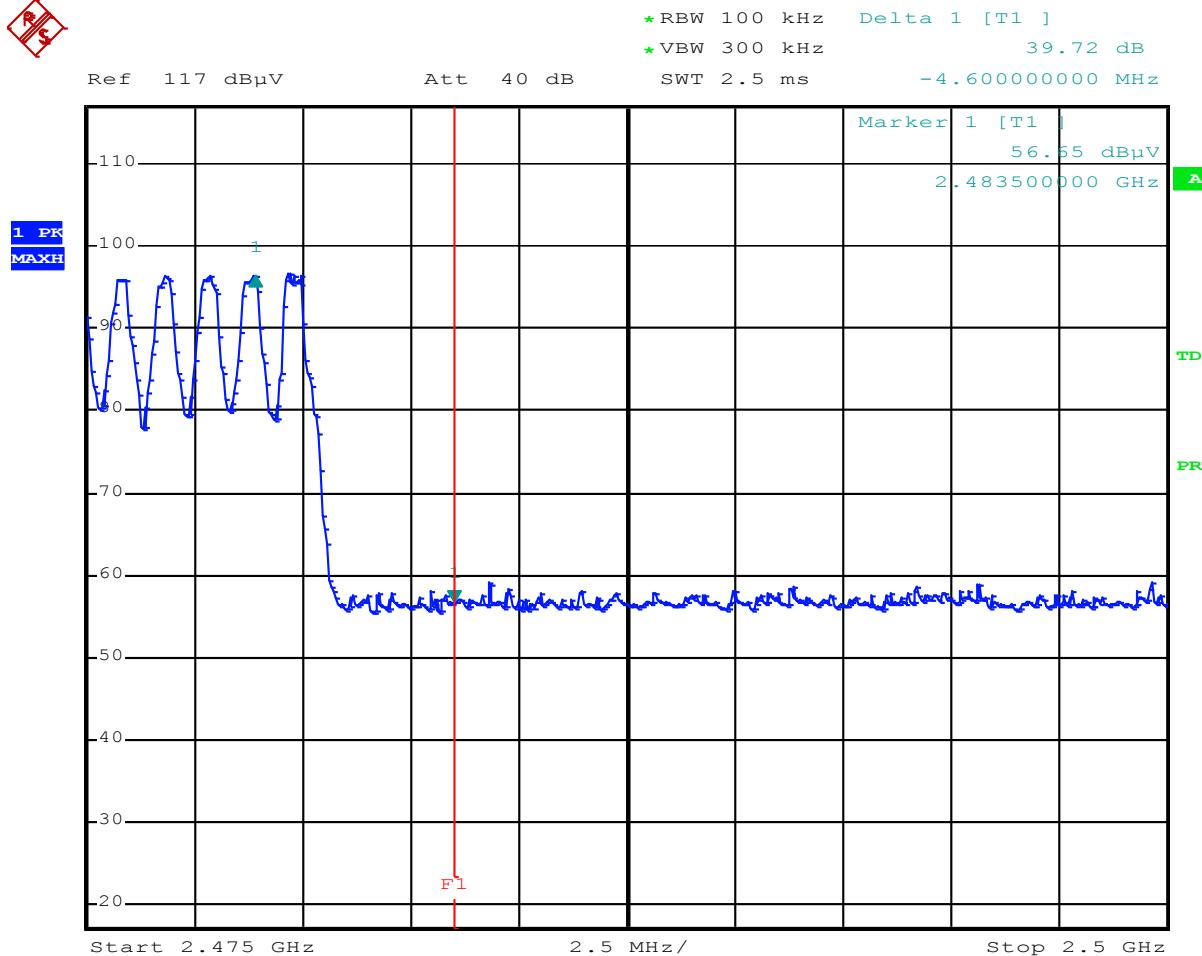

Test Personnel: Naga Suryadevara N:5  
 Supervising/Reviewing  
 Engineer:  
 (Where Applicable) N/A  
 Product Standard: FCC Part 15 Subpart C  
 (15.247) and RSS-247  
 Input Voltage: 12 VDC (System input 120  
 VAC 60 Hz)

Test Date: 08/24/2016

Limit Applied: See test report section 11.3

Ambient Temperature: 22 °C

Pretest Verification: Yes

Relative Humidity: 44 %

Atmospheric Pressure: 1003 mbars

Deviations, Additions, or Exclusions: None

## 12 Transmitter Spurious Emissions

### 12.1 Method

Tests are performed in accordance with FCC Part 15 Subpart C (15.247) and RSS 247.

**TEST SITE:** 3m Semi-Anechoic Chamber at Intertek Lake Forest CA

Radiated emission measurements are performed in a 3 meter Semi-Anechoic Chamber. The chamber is a shielded enclosure used to control and maintain a predictable EMI environment within the test region. A lining of RF absorbing material (Absorber) and other anechoic materials are installed over all interior wall and ceiling surfaces as to completely shroud exposed metallic components and disrupt reflective properties. The ground plane is an exposed RF reflective surface. The turntable is flush mounted, 2 meters in diameter, and remotely controlled. The antenna mast can be positioned at 3 meters away from the turntable. The antenna mast is remote controlled and can lower/raise an antenna between 1 – 4 meters. The antenna mast can also rotate between horizontal and vertical polarizations.

#### Measurement Uncertainty

Measurement	Frequency Range	Expanded Uncertainty (k=2)	Ucispr
Radiated Emissions, 10m	30-1000 MHz	4.5 dB	6.3 dB
Radiated Emissions, 3m	1-18 GHz	4.7 dB	5.2 dB
Radiated Emissions, 1m	18-40 GHz	4.5 dB	-

As shown in the table above our radiated emissions  $U_{lab}$  is less than the corresponding  $U_{CISPR}$  reference value in CISPR 16-4-2 Table 1, hence the compliance of the product is only based on the measured value, and no measurement uncertainty correction is required, based on CISPR 22 and CISPR 11 (for 2006 and later revisions) Clause 11.

#### Sample Calculation

The field strength is calculated by adding the Antenna Factor and Cable Factor, and subtracting the Amplifier Gain (if any) from the measured reading. The basic equation with a sample calculation is as follows:

$$FS = RA + AF + CF - AG$$

Where  $FS$  = Field Strength in  $\text{dB}\mu\text{V}/\text{m}$

$RA$  = Receiver Amplitude (including preamplifier) in  $\text{dB}\mu\text{V}$

$CF$  = Cable Attenuation Factor in dB

$AF$  = Antenna Factor in dB

$AG$  = Amplifier Gain in dB

In the following table(s), the reading shown on the data table reflects the preamplifier gain. An example for the calculations in the following table is as follows.

Assume a receiver reading of 52.0  $\text{dB}\mu\text{V}$  is obtained. The antenna factor of 7.4 dB and cable factor of 1.6 dB is added. The amplifier gain of 29 dB is subtracted, giving a field strength of 32  $\text{dB}\mu\text{V}/\text{m}$ . This value in  $\text{dB}\mu\text{V}/\text{m}$  was converted to its corresponding level in  $\mu\text{V}/\text{m}$ .

$$RA = 52.0 \text{ dB}\mu\text{V}$$

$$AF = 7.4 \text{ dB}/\text{m}$$

$$CF = 1.6 \text{ dB}$$

AG = 29.0 dB  
 FS = 32 dB $\mu$ V/m

To convert from dB $\mu$ V to  $\mu$ V or mV the following was used:

UF =  $10^{(NF/20)}$  where UF = Net Reading in  $\mu$ V  
 NF = Net Reading in dB $\mu$ V

**Example:**

FS = RA + AF + CF - AG = 52.0 + 7.4 + 1.6 - 29.0 = 32.0  
 UF =  $10^{(32 \text{ dB}\mu\text{V}/20)}$  = 39.8  $\mu$ V/m

**12.2 Test Equipment Used:**


Asset	Description	Manufacturer	Model	Serial	Cal Date	Cal Due
001001'	Barometer/Humidity Control	Omega	IBTHX-W	0440775	04/22/2016	04/22/2017
001093'	Double Ridge Guide Horn Antenna	A.H. Systems Inc.	SAS-571	1513	02/12/2016	02/12/2017
000880'	Horn Antenna, 10-40 GHZ	ETS Lindgren	3116C	00153521	11/09/2015	11/09/2016
001517'	RF Cable 30Mhz - 18Ghz	Rohde & Schwarz	TSPR-B7	101528	07/01/2016	07/01/2017
001518'	RF Cable 30Mhz - 18Ghz	Rohde & Schwarz	TSPR-B7	101529	07/01/2016	07/01/2017
000690'	Spectrum Analyzer, 9 KHz - 40 GHz	Rohde & Schwarz	FSP40	100027	01/11/2016	01/11/2017
001147'	Bilog Antenna	TESEQ GmbH	CBL 6112D	32852	10/28/2015	10/28/2016
001135'	Amplifier	Miteq	AMF-6D-00501800-24-	1685147	04/15/2016	04/15/2017
001140'	EMI Test Receiver	Rohde & Schwarz	ESC17	100825	02/22/2016	02/22/2017
001568'	Preamplifier 10 KHz - 1 GHz	Rohde & Schwarz	TS-PR1	102061	12/02/2015	12/02/2016
CBLH20 12-5M-1'	5m 9kHz-40GHz Coaxial Cable - SET 1	Huber & Suhner	SF102	252676001	02/09/2016	02/09/2017


**Software Utilized:**

Name	Manufacturer	Version
None		

**12.3 Results:**

The sample tested was found to Comply.

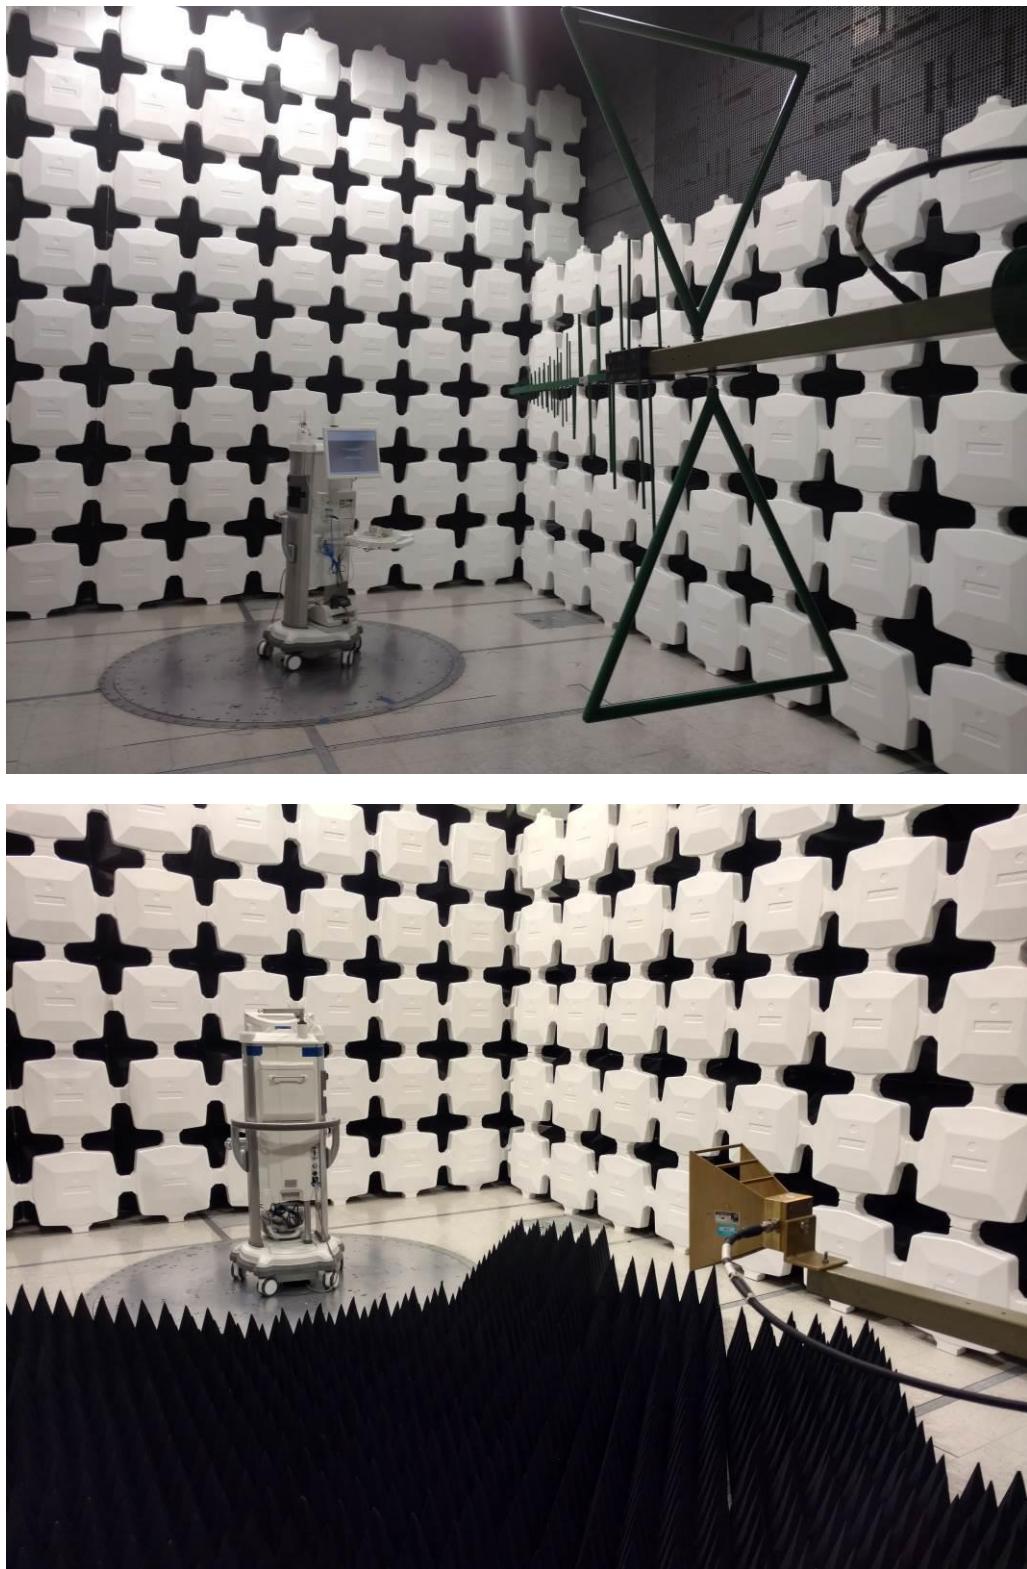**12.4 Setup Photographs:**

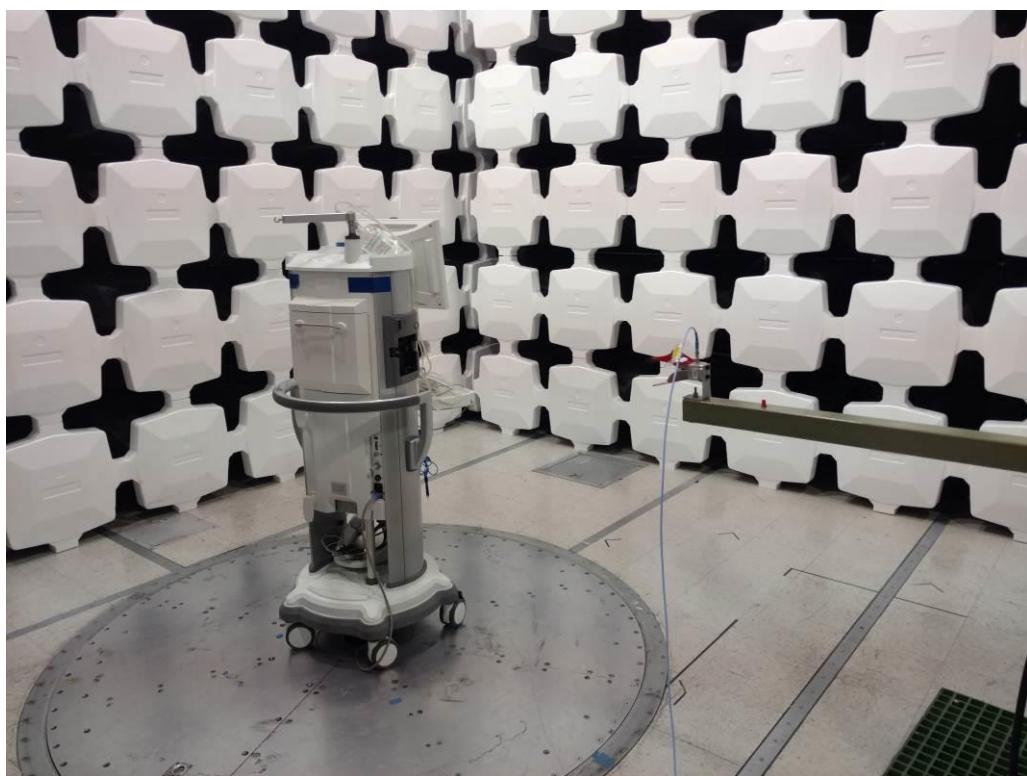

**12.5 Plots/Data:****Device Operating in Transmit mode, 30 MHz – 1 GHz**

Intertek

**Transmitter Spurious Emissions**

Company: Abbott Medical Optics, Inc.	Antenna & Cables: LF	Bands: LF									
Model #: GUI Board	Antenna: BlagAntenna1147Horizontal(10-28-2015).txt	BlagAntenna1147horizontal(10-28-2015).txt									
Serial #: 131121003	Cable(s): 01517and01518.txt	NONE.									
Engineers: Naga Suryadevara	Barometer: 1001	Filter: NONE									
Project #: G102675709	Date(s): 08/24/16										
Standard: FCC Part 15 Subpart C	Temp/Humidity/Pressure: 26.2/50/990										
Receiver: R&S ESCI7 02/22/2017	Limit Distance (m): 3										
PreAmp: DATA 001568.txt	Test Distance (m): 3										
PreAmp Used? (Y or N): Y	Voltage/Frequency:	Frequency Range: 30-1000 MHz									
Net = Reading (dBuV/m) + Antenna Factor (dB1/m) + Cable Loss (dB) - Preamp Factor (dB) - Distance Factor (dB)											
Peak: PK Quasi-Peak: QP Average: AVG RMS: RMS; NF = Noise Floor, RB = Restricted Band; Bandwidth denoted as RBW/VBW											
Detector	Ant.	Pol.	Frequency	Antenna	Cable	Pre-amp	Distance				
Type	(V/H)		MHz	Reading	Factor	Loss	Factor	Net	Limit	Margin	Bandwidth
QP	V		80.012	54.46	13.10	0.57	30.04	0.00	38.09	40.00	-1.91
QP	H		80.012	49.11	13.10	0.57	30.04	0.00	32.74	40.00	-7.26
QP	H		143.984	53.59	16.80	0.82	29.88	0.00	41.34	43.50	-2.16
QP	V		143.984	54.59	16.80	0.82	29.88	0.00	42.34	43.50	-1.16
QP	H		341.632	43.48	19.90	1.31	29.66	0.00	35.04	46.00	-10.96
QP	V		341.632	45.28	19.90	1.31	29.66	0.00	36.84	46.00	-9.16
QP	V		408.400	39.84	22.20	1.48	29.76	0.00	33.76	46.00	-12.24
QP	H		408.400	37.71	22.20	1.48	29.76	0.00	31.63	46.00	-14.37
QP	V		599.080	26.28	24.70	1.80	30.15	0.00	22.63	46.00	-23.37
QP	H		599.080	31.10	24.70	1.80	30.15	0.00	27.45	46.00	-18.55
QP	V		973.980	41.62	27.10	2.32	29.32	0.00	41.72	54.00	-12.28
QP	H		973.980	43.11	27.10	2.32	29.32	0.00	43.21	54.00	-10.79

## Device Operating in Transmit mode, 1 GHz – 25 GHz

Intertek

## Transmitter Spurious Emissions

Company: Abbott Medical

Model #: GUI Board

Serial #: 131121003

Engineers: Naga Suryadevara

Project #: G102675709

Date(s): 08/25/16

Antenna &amp; Cables: HF Bands: HF

Antenna: 1093H.txt 1093V.txt

Cable(s): 001517.txt NONE.

Location: 3m Chamber Barometer:

Filter: REA004

Standard: FCC Part 15 Subpart C

Temp/Humidity/Pressure: 24/48/1003

Receiver: R&amp;S ESCI7 02/22/2017

Limit Distance (m): 3

PreAmp: preamp1135.txt

Test Distance (m): 3

PreAmp Used? (Y or N): Y Voltage/Frequency: Frequency Range: 1-25 GHz

Net = Reading (dBuV/m) + Antenna Factor (dB1/m) + Cable Loss (dB) - Preamp Factor (dB) - Distance Factor (dB)

Peak: PK Quasi-Peak: QP Average: AVG RMS: RMS; NF = Noise Floor, RB = Restricted Band; Bandwidth denoted as RBW/VBW

Detector Type	Ant. Pol. (V/H)	Frequency MHz	Reading dB(uV)	Antenna Factor dB(1/m)	Cable Loss dB	Pre-amp Factor dB	Distance Factor dB	Net dB(uV/m)	Limit dB(uV/m)	Margin dB	REA004 Bandwidth	FCC
TX = 2402 MHz												
PK	V	2392.000	43.24	28.04	-2.02	0.00	0.00	69.26	74.00	-4.74	1/3 MHz	
AVG	V	2392.000	22.77	28.04	-2.02	0.00	0.00	48.79	54.00	-5.21	1/3 MHz	
PK	V	4804.000	69.24	32.93	-3.11	43.41	0.00	55.65	74.00	-18.35	1/3 MHz	RB
AVG	V	4804.000	59.12	32.93	-3.11	43.41	0.00	45.53	54.00	-8.47	1/3 MHz	RB
PK	H	7206.000	59.18	36.50	-3.40	43.35	0.00	48.92	74.00	-25.08	1/3 MHz	
AVG	H	7206.000	54.12	36.50	-3.40	43.35	0.00	43.86	54.00	-10.14	1/3 MHz	
PK	V	9608.000	49.12	38.36	-4.47	43.63	0.00	39.38	74.00	-34.62	1/3 MHz	
AVG	V	9608.000	43.45	38.36	-4.47	43.63	0.00	33.71	54.00	-20.29	1/3 MHz	
PK	V	12010.000	51.10	40.23	-4.58	45.34	0.00	41.40	74.00	-32.60	1/3 MHz	RB
AVG	V	12010.000	45.55	40.23	-4.58	45.34	0.00	35.85	54.00	-18.15	1/3 MHz	RB
PK	H	14412.000	48.32	41.03	-5.47	43.74	0.00	40.14	74.00	-33.86	1/3 MHz	
AVG	H	14412.000	38.18	41.03	-5.47	43.74	0.00	30.00	54.00	-24.00	1/3 MHz	
No emissions detected above this frequency												
TX = 2441 MHz												
PK	V	4882.000	61.24	33.10	-3.14	43.33	0.00	47.87	74.00	-26.14	1/3 MHz	RB
AVG	V	4882.000	52.18	33.10	-3.14	43.33	0.00	38.81	54.00	-15.20	1/3 MHz	RB
PK	V	7323.000	57.12	36.86	-3.48	42.99	0.00	47.50	74.00	-26.50	1/3 MHz	RB
AVG	V	7323.000	55.37	36.86	-3.48	42.99	0.00	45.75	54.00	-8.25	1/3 MHz	RB
PK	V	9764.000	53.19	38.50	-4.51	43.73	0.00	43.44	74.00	-30.56	1/3 MHz	
AVG	V	9764.000	48.48	38.50	-4.51	43.73	0.00	38.73	54.00	-15.27	1/3 MHz	
No emissions detected above this frequency												
TX = 2480 MHz												
PK	V	2483.500	44.12	28.34	-2.06	0.00	0.00	70.39	74.00	-3.61	1/3 MHz	RB
AVG	V	2483.500	25.18	28.34	-2.06	0.00	0.00	51.45	54.00	-2.55	1/3 MHz	RB
PK	V	4960.000	65.39	33.20	-3.17	43.32	0.00	52.10	74.00	-21.90	1/3 MHz	RB
AVG	V	4960.000	59.17	33.20	-3.17	43.32	0.00	45.88	54.00	-8.12	1/3 MHz	RB
PK	V	7440.000	56.28	36.83	-3.56	42.70	0.00	46.85	74.00	-27.15	1/3 MHz	RB
AVG	V	7440.000	51.19	36.83	-3.56	42.70	0.00	41.76	54.00	-12.24	1/3 MHz	RB
PK	V	9920.000	53.87	38.66	-4.54	43.76	0.00	44.23	74.00	-29.77	1/3 MHz	
AVG	V	9920.000	45.99	38.66	-4.54	43.76	0.00	36.35	54.00	-17.65	1/3 MHz	
PK	H	12400.000	49.89	39.97	-4.74	45.31	0.00	39.81	74.00	-34.19	1/3 MHz	RB
AVG	H	12400.000	44.21	39.97	-4.74	45.31	0.00	34.13	54.00	-19.87	1/3 MHz	RB
No emissions detected above this frequency												

Test Personnel: Naga Suryadevara N.S  
Supervising/Reviewing  
Engineer:  
(Where Applicable) N/A  
Product Standard: FCC Part 15 Subpart C  
(15.247) and RSS-247  
12 VDC (System input 120  
Input Voltage: VAC 60 Hz)

Pretest Verification w/  
Ambient Signals or  
BB Source: Yes

Test Date: 08/24/2016  
08/25/2016

Limit Applied: As specified

Ambient Temperature: 26.2, 24 °C

Relative Humidity: 50, 48 %

Atmospheric Pressure: 990, 1003 mbars

Deviations, Additions, or Exclusions: None

## 13 Receiver Spurious Emissions

### 13.1 Method

Tests are performed in accordance with FCC Part 15.209 and ICES 003.

**TEST SITE:** 3m Semi-Anechoic Chamber at Intertek Lake Forest CA

Radiated emission measurements are performed in a 3 meter Semi-Anechoic Chamber. The chamber is a shielded enclosure used to control and maintain a predictable EMI environment within the test region. A lining of RF absorbing material (Absorber) and other anechoic materials are installed over all interior wall and ceiling surfaces as to completely shroud exposed metallic components and disrupt reflective properties. The ground plane is an exposed RF reflective surface. The turntable is flush mounted, 2 meters in diameter, and remotely controlled. The antenna mast can be positioned at 3 meters away from the turntable. The antenna mast is remote controlled and can lower/raise an antenna between 1 – 4 meters. The antenna mast can also rotate between horizontal and vertical polarizations.

#### Measurement Uncertainty

Measurement	Frequency Range	Expanded Uncertainty (k=2)	Ucispr
Radiated Emissions, 10m	30-1000 MHz	4.5 dB	6.3 dB
Radiated Emissions, 3m	1-18 GHz	4.7 dB	5.2 dB
Radiated Emissions, 1m	18-40 GHz	4.5 dB	-

As shown in the table above our radiated emissions  $U_{lab}$  is less than the corresponding  $U_{CISPR}$  reference value in CISPR 16-4-2 Table 1, hence the compliance of the product is only based on the measured value, and no measurement uncertainty correction is required, based on CISPR 22 and CISPR 11 (for 2006 and later revisions) Clause 11.

#### Sample Calculation

The field strength is calculated by adding the Antenna Factor and Cable Factor, and subtracting the Amplifier Gain (if any) from the measured reading. The basic equation with a sample calculation is as follows:

$$FS = RA + AF + CF - AG$$

Where  $FS$  = Field Strength in  $\text{dB}\mu\text{V}/\text{m}$

$RA$  = Receiver Amplitude (including preamplifier) in  $\text{dB}\mu\text{V}$

$CF$  = Cable Attenuation Factor in dB

$AF$  = Antenna Factor in dB

$AG$  = Amplifier Gain in dB

In the following table(s), the reading shown on the data table reflects the preamplifier gain. An example for the calculations in the following table is as follows.

Assume a receiver reading of 52.0  $\text{dB}\mu\text{V}$  is obtained. The antenna factor of 7.4 dB and cable factor of 1.6 dB is added. The amplifier gain of 29 dB is subtracted, giving a field strength of 32  $\text{dB}\mu\text{V}/\text{m}$ . This value in  $\text{dB}\mu\text{V}/\text{m}$  was converted to its corresponding level in  $\mu\text{V}/\text{m}$ .

$$RA = 52.0 \text{ dB}\mu\text{V}$$

$$AF = 7.4 \text{ dB}/\text{m}$$

$$CF = 1.6 \text{ dB}$$

AG = 29.0 dB  
 FS = 32 dB $\mu$ V/m

To convert from dB $\mu$ V to  $\mu$ V or mV the following was used:

UF =  $10^{(NF/20)}$  where UF = Net Reading in  $\mu$ V  
 NF = Net Reading in dB $\mu$ V

**Example:**

FS = RA + AF + CF - AG = 52.0 + 7.4 + 1.6 - 29.0 = 32.0  
 UF =  $10^{(32 \text{ dB}\mu\text{V}/20)}$  = 39.8  $\mu$ V/m

**13.2 Test Equipment Used:**


Asset	Description	Manufacturer	Model	Serial	Cal Date	Cal Due
001001'	Barometer/Humidity Control	Omega	IBTHX-W	0440775	04/22/2016	04/22/2017
001093'	Double Ridge Guide Horn Antenna	A.H. Systems Inc.	SAS-571	1513	02/12/2016	02/12/2017
000880'	Horn Antenna, 10-40 GHZ	ETS Lindgren	3116C	00153521	11/09/2015	11/09/2016
001517'	RF Cable 30Mhz - 18Ghz	Rohde & Schwarz	TSPR-B7	101528	07/01/2016	07/01/2017
001518'	RF Cable 30Mhz - 18Ghz	Rohde & Schwarz	TSPR-B7	101529	07/01/2016	07/01/2017
000690'	Spectrum Analyzer, 9 KHz - 40 GHz	Rohde & Schwarz	FSP40	100027	01/11/2016	01/11/2017
001147'	Bilog Antenna	TESEQ GmbH	CBL 6112D	32852	10/28/2015	10/28/2016
001135'	Amplifier	Miteq	AMF-6D-00501800-24-	1685147	04/15/2016	04/15/2017
001140'	EMI Test Receiver	Rohde & Schwarz	ESC17	100825	02/22/2016	02/22/2017
001568'	Preamplifier 10 KHz - 1 GHz	Rohde & Schwarz	TS-PR1	102061	12/02/2015	12/02/2016
CBLH20 12-5M-1'	5m 9kHz-40GHz Coaxial Cable - SET 1	Huber & Suhner	SF102	252676001	02/09/2016	02/09/2017


**Software Utilized:**

Name	Manufacturer	Version
None		

**13.3 Results:**

The sample tested was found to Comply.

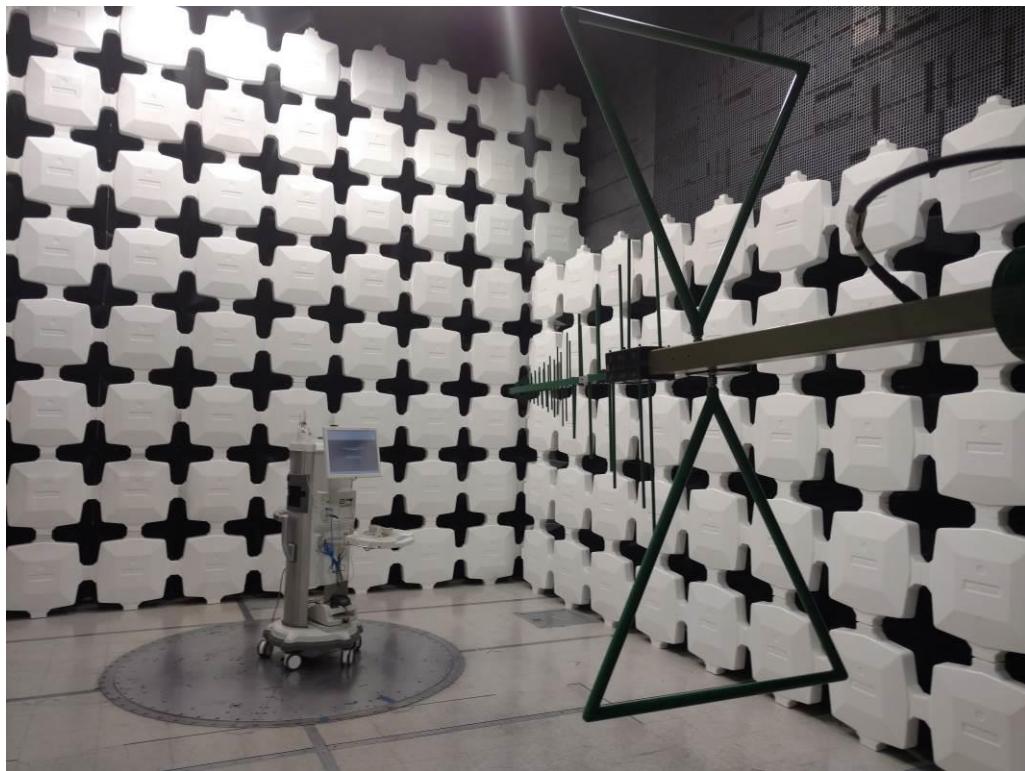**13.4 Setup Photographs:**

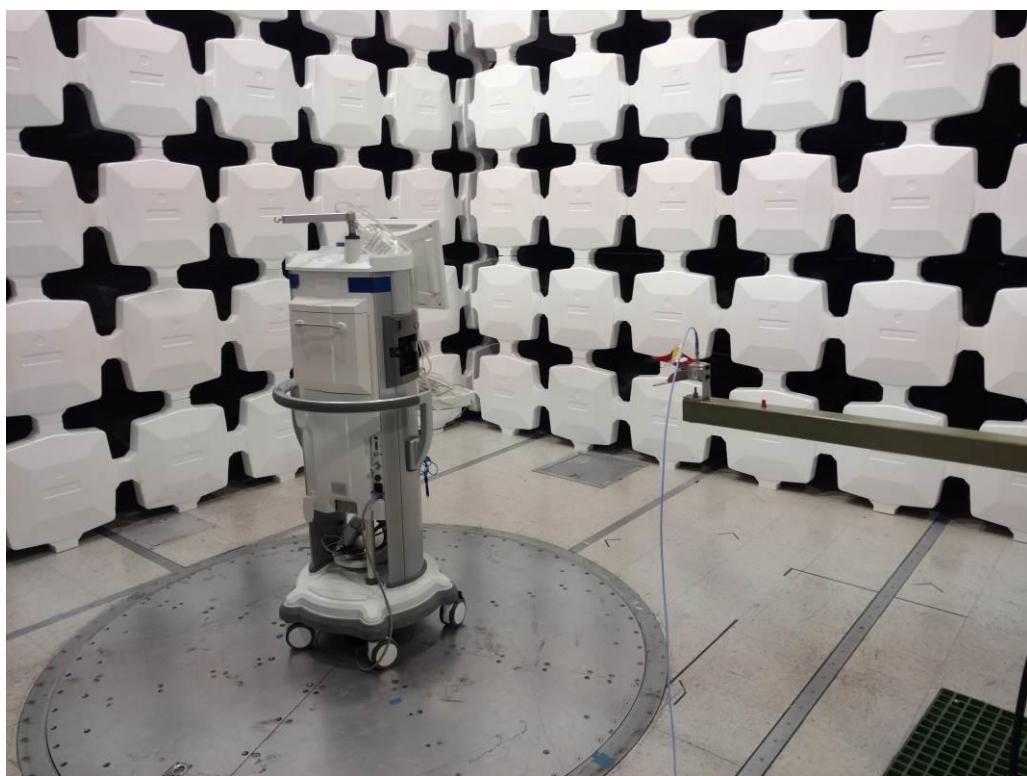

**13.5 Plots/Data:****Device Operating in Receive mode, 30 MHz – 1 GHz**

Intertek											
Rx Mode Emissions											
Company: Abbott Medical Optics, Inc.								Antenna & Cables:	LF	Bands: LF	
Model #: GUI Board								Antenna:	B1ogAntenna1147Horizontal(10-28-2015).txt	B1ogAntenna1147Horizontal(10-28-2015).txt	
Serial #: 131121003								Cable(s):	01517and01518.txt	NONE.	
Engineers: Naga Suryadevara			Location:	3 m chamber				Barometer:	1001	Filter:	NONE
Project #: G102675709		Date(s): 08/24/16						Temp/Humidity/Pressure:	26.2/50/990		
Standard: FCC 15.109											
Receiver: R&S ESCI7 02/22/2017		Limit Distance (m):	3								
PreAmp: DATA 001568.txt		Test Distance (m):	3								
PreAmp Used? (Y or N):	Y	Voltage/Frequency:						Frequency Range:	30-1000 MHz		
Net = Reading (dBuV/m) + Antenna Factor (dB1/m) + Cable Loss (dB) - Preamp Factor (dB) - Distance Factor (dB)											
Peak: PK Quasi-Peak: QP Average: AVG RMS: RMS; NF = Noise Floor, RB = Restricted Band; Bandwidth denoted as RBW/VBW											
Detector	Ant.	Pol.	Frequency	Reading	Antenna	Cable	Pre-amp	Distance			
Type	(V/H)		MHz	dB(uV)	Factor	Loss	Factor	Factor	Net	Limit	Margin
QP	V		80.012	54.46	13.10	0.57	30.04	0.00	38.09	40.00	-1.91
QP	H		80.012	49.11	13.10	0.57	30.04	0.00	32.74	40.00	-7.26
QP	H		143.984	53.59	16.80	0.82	29.88	0.00	41.34	43.50	-2.16
QP	V		143.984	54.59	16.80	0.82	29.88	0.00	42.34	43.50	-1.16
QP	H		341.632	43.48	19.90	1.31	29.66	0.00	35.04	46.00	-10.96
QP	V		341.632	45.28	19.90	1.31	29.66	0.00	36.84	46.00	-9.16
QP	V		408.400	39.84	22.20	1.48	29.76	0.00	33.76	46.00	-12.24
QP	H		408.400	37.71	22.20	1.48	29.76	0.00	31.63	46.00	-14.37
QP	V		599.080	26.28	24.70	1.80	30.15	0.00	22.63	46.00	-23.37
QP	H		599.080	31.10	24.70	1.80	30.15	0.00	27.45	46.00	-18.55
QP	V		973.980	41.62	27.10	2.32	29.32	0.00	41.72	54.00	-12.28
QP	H		973.980	43.11	27.10	2.32	29.32	0.00	43.21	54.00	-10.79

## Device Operating in Receive mode, 1 GHz – 25 GHz

## Intertek

## Rx Mode Emissions

Company: Abbott Medical  
 Model #: GUI Board  
 Serial #: 131121003  
 Engineers: Naga Suryadevara  
 Project #: G102675709 Date(s): 08/25/16  
 Standard: FCC 15.109  
 Receiver: R&S ESCI7 02/22/2017 Limit Distance (m): 3  
 PreAmp: preamp1135.txt Test Distance (m): 3  
 PreAmp Used? (Y or N): Y Voltage/Frequency: Frequency Range: 1-25 GHz  
 Net = Reading (dBuV/m) + Antenna Factor (dB1/m) + Cable Loss (dB) - Preamp Factor (dB) - Distance Factor (dB)  
 Peak: PK Quasi-Peak: QP Average: AVG RMS: RMS; NF = Noise Floor, RB = Restricted Band; Bandwidth denoted as RBW/VBW

Detector Type	Ant. Pol. (V/H)	Frequency MHz	Reading dB(uV)	Antenna Factor dB(1/m)	Cable Loss dB	Pre-amp Factor dB	Distance Factor dB	Net dB(uV/m)	Limit dB(uV/m)	Margin dB	REA004 Bandwidth
Receive mode											
PK	V	1331.310	59.21	24.48	-1.46	44.99	0.00	37.24	74.00	-36.76	1/3 MHz
AVG	V	1331.310	45.41	24.48	-1.46	44.99	0.00	23.44	54.00	-30.56	1/3 MHz
PK	H	2385.780	60.15	28.01	-2.02	44.73	0.00	41.40	74.00	-32.60	1/3 MHz
AVG	H	2385.780	55.19	28.01	-2.02	44.73	0.00	36.44	54.00	-17.56	1/3 MHz
PK	V	4348.210	56.28	31.96	-2.87	43.37	0.00	41.99	74.00	-32.01	1/3 MHz
AVG	V	4348.210	48.17	31.96	-2.87	43.37	0.00	33.88	54.00	-20.12	1/3 MHz
PK	V	8795.190	49.45	38.00	-4.27	42.38	0.00	40.80	74.00	-33.20	1/3 MHz
AVG	V	8795.190	42.12	38.00	-4.27	42.38	0.00	33.47	54.00	-20.53	1/3 MHz
PK	H	15534.320	51.17	40.32	-5.54	43.57	0.00	42.38	74.00	-31.62	1/3 MHz
AVG	H	15534.320	39.08	40.32	-5.54	43.57	0.00	30.29	54.00	-23.71	1/3 MHz

Test Personnel: Naga Suryadevara N5

Test Date: 08/24/2016

08/25/2016

Supervising/Reviewing

Engineer:  
(Where Applicable) N/ALimit Applied: FCC 15.109 Class BProduct Standard: FCC Part 15 (15.209) and  
ICES 00312 VDC (System input 120  
VAC 60 Hz)Ambient Temperature: 26.2, 24 °CInput Voltage: 12 VDC (System input 120  
VAC 60 Hz)Relative Humidity: 50, 48 %Pretest Verification w/  
Ambient Signals or  
BB Source: YesAtmospheric Pressure: 990, 1003 mbars

Deviations, Additions, or Exclusions: None

**14 Revision History**

Revision Level	Date	Report Number	Prepared By	Reviewed By	Notes
0	09/07/2016	102675709BOX-001	N5	MFM <i>HJF</i>	Original Issue
1	10/04/2016	102675709BOX-001	N5	MFM <i>HJF</i>	Updated model name
2	11/11/2016	102675709BOX-001	N5	MFM <i>HJF</i>	Updated antenna gain ,RF exposure calculation and added measurement uncertainty value for 18- 40 GHz.
3	11/21/2016	102675709BOX-001	N5	MFM <i>HJF</i>	Added SAR exemption Calculation