

802 N. Twin Oaks Valley Road, Suite 105 • San Marcos, CA 92069 • U.S.A. TEL (760) 471-2100 • FAX (760) 471-2121 http://www.rfexposurelab.com

# CERTIFICATE OF COMPLIANCE SAR EVALUATION

Juniper Systems Dates of Test: Jul. 23-26, 2014; Jan. 30 & Apr. 28, 2015 1132 West 1700 North Test Report Number: SAR.20140710 Logan, UT 84321 Revision D

FCC ID: VSF23545, VSF23795 & VSF24243

IC Certificate: 7980A-23545, 7980A-23795 & 7980A-24243

Model(s): Allegro<sup>2</sup>

Contains WLAN Module: LS Research Model TiWi-R2
Contains Cellular Module: Gemalto Model PH8-P
Contains Sensus Module: Sensus Model AR5002

Test Sample: Engineering Unit Same as Production

Serial Number: AG2B096 & AB2B274
Equipment Type: Wireless Handheld Computer
Classification: Portable Transmitter Next to Body

TX Frequency Range: 824 – 849 MHz; 1850 – 1910 MHz; 2412 – 2462 MHz; 952 MHz; 902 – 928 MHz

Frequency Tolerance: ± 2.5 ppm

Maximum RF Output: 850 MHz (GPRS) – 33.81 dBm, 850 MHz (WCDMA) – 23.39 dBm, 1900 MHz (GPRS) – 30.87 dBm, 1900 MHz (WCDMA) – 23.79 dBm,

1900 MHz (GPRS) = 30.87 dBm, 1900 MHz (WCDMA) = 23.79 dBm, 2450 MHz (b) = 19.72 dBm, 2450 MHz (a) = 19.65 dBm, 2450 MHz (p.20) = 1

2450 MHz (b) - 19.72 dBm, 2450 MHz (g) - 19.65 dBm, 2450 MHz (n20) - 19.41 dBm, 2450 MHz (n40) - 19.26 dBm, 952 MHz - 24.42 dBm, 915 MHz - 0.32 dBm Conducted

Signal Modulation: GMSK, 8PSK, WCDMA, DSSS, OFDM, DSB-AM

Antenna Type: PIFA Antenna & Internal Antenna

Application Type: Certification

FCC Rule Parts: Part 2, 22, 24, 15C, 15E, 101

KDB Test Methodology: KDB 447498 D01 v05r02, KDB 248227 v01r02, KDB 941225 D01 v02, KDB 941225 D03 v01

Industry Canada: RSS-102, Safety Code 6
Maximum SAR Value: 1.28 W/kg Reported

Simultaneous SAR: 0.04 Distance Ratio Calculated Value

Separation Distance: 0 mm

This wireless mobile and/or portable device has been shown to be compliant for localized specific absorption rate (SAR) for uncontrolled environment/general exposure limits specified in ANSI/IEEE Std. C95.1-1992 and had been tested in accordance with the measurement procedures specified in IEEE 1528-2013 and IEC 62209-2:2010 (See test report).

I attest to the accuracy of the data. All measurements were performed by myself or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

RF Exposure Lab, LLC certifies that no party to this application is subject to a denial of Federal benefits that includes FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 853(a).



# **Table of Contents**

1. Introduction	3
SAR Definition [5]	4
2. SAR Measurement Setup	5
Robotic System	5
System Hardware	5
System Electronics	6
Probe Measurement System	6
3. Probe and Dipole Calibration	14
4. Phantom & Simulating Tissue Specifications	15
Head & Body Simulating Mixture Characterization	
5. ANSI/IEEE C95.1 – 1992 RF Exposure Limits [2]	
Uncontrolled Environment	
Controlled Environment	16
6. Measurement Uncertainty	17
7. System Validation	18
Tissue Verification	18
Test System Verification	
8. SAR Test Data Summary	
Procedures Used To Establish Test Signal	
Device Test Condition	
SAR Data Summary – 835 MHz Body	
SAR Data Summary – 1900 MHz Body	
SAR Data Summary – 2450 MHz Body 802.11b	
SAR Data Summary – 900 MHz Body	
SAR Data Summary – Simultaneous Evaluation	
9. Test Equipment List	
10. Conclusion	
11. References	
Appendix A – System Validation Plots and Data	
Appendix B – SAR Test Data Plots	
Appendix C – SAR Test Setup Photos	
Appendix D – Probe Calibration Data Sheets	
Appendix E – Dipole Calibration Data Sheets	
Appendix F – Phantom Calibration Data Sheets	130



### 1. Introduction

This measurement report shows compliance of the Juniper Systems Model Allegro<sup>2</sup> FCC ID: VSF23545, VSF23795 & VSF24243 with FCC Part 2, 1093, ET Docket 93-62 Rules for mobile and portable devices and IC Certificate: 7980A-23545, 7980A-23795 & 7980A-24243 with RSS102 & Safety Code 6. The FCC have adopted the guidelines for evaluating the environmental effects of radio frequency radiation in ET Docket 93-62 on August 6, 1996 to protect the public and workers from the potential hazards of RF emissions due to FCC regulated portable devices. [1], [6]

The test results recorded herein are based on a single type test of Juniper Systems Model Allegro<sup>2</sup> and therefore apply only to the tested sample.

The test procedures, as described in ANSI C95.1 – 1999 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz [2], ANSI C95.3 – 2002 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields [3], IEEE Std.1528 – 2003 Recommended Practice [4], and Industry Canada Safety Code 6 Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz were employed.

The following table indicates all the wireless technologies operating in the Allegro<sup>2</sup> wireless handheld computer. The table also shows the tolerance for the power level for each mode.

Band	Technology	Class	3GPP Nominal Power dBm	Setpoint Nominal Power dBm	Tolerance dBm	Lower Tolerance dBm	Upper Tolerance dBm
WLAN – 2.4 GHz	802.11bgn	N/A	N/A	18	±2	16.0	20.0
Band 5	GSM	10	33.0	33.0	±1.0	29.0	34.0
Band 5	EDGE	10	28.0	28.0	±1.0	27.0	29.0
Band 5	WCDMA	3	22.0	22.0	±1.5	20.5	23.5
Band 2	GSM	10	28.5	30.0	±1.0	29.0	31.0
Band 2	EDGE	10	26.0	26.0	±1.0	25.0	27.0
Band 2	WCDMA	3	22.0	22.5	±1.5	21.0	24.0
952 MHz	DSB-FM	N/A	N/A	23.42	+1/-6	18.42	24.42
915 MHz	DSSS	N/A	N/A	0	+1/-3	-3.0	1.0



# **SAR Definition [5]**

Specific Absorption Rate is defined as the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dV) of a given density ( $\rho$ ).

$$SAR = \frac{d}{dt} \left( \frac{dW}{dm} \right) = \frac{d}{dt} \left( \frac{dW}{\rho dV} \right)$$

SAR is expressed in units of watts per kilogram (W/kg). SAR can be related to the electric field at a point by

$$SAR = \frac{\sigma \mid E \mid^2}{\rho}$$

where:

 $\sigma$  = conductivity of the tissue (S/m)

 $\rho$  = mass density of the tissue (kg/m<sup>3</sup>)

E = rms electric field strength (V/m)



# 2. SAR Measurement Setup

# **Robotic System**

These measurements are performed using the DASY52 automated dosimetric assessment system. The DASY52 is made by Schmid & Partner Engineering AG (SPEAG) in Zurich, Switzerland and consists of high precision robotics system (Staubli), robot controller, Intel Core2 computer, near-field probe, probe alignment sensor, and the generic twin phantom containing the brain equivalent material. The robot is a six-axis industrial robot performing precise movements to position the probe to the location (points) of maximum electromagnetic field (EMF) (see Fig. 2.1).

# **System Hardware**

A cell controller system contains the power supply, robot controller teach pendant (Joystick), and a remote control used to drive the robot motors. The PC consists of the HP Intel Core2 computer with Windows XP system and SAR Measurement Software DASY52, A/D interface card, monitor, mouse, and keyboard. The Staubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit that performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. is connected to the Electro-optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC plug-in card.

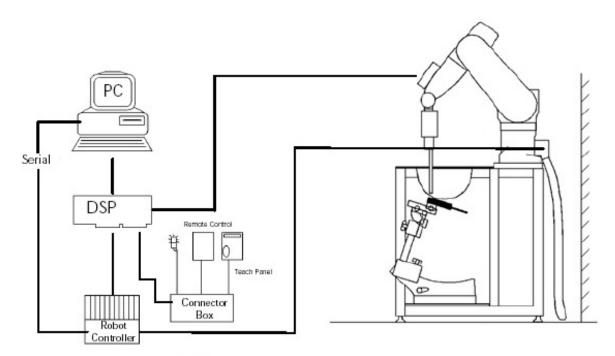


Figure 2.1 SAR Measurement System Setup



# **System Electronics**

The DAE4 consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer. The system is described in detail in.

# **Probe Measurement System**

The SAR measurements were conducted with the dosimetric probe EX3DV4, designed in the classical triangular configuration (see Fig. 2.2) and optimized for dosimetric evaluation. The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multi fiber line ending at the front of the probe tip. (see Fig. 2.3) It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY52 software reads the reflection during a software approach and looks for the maximum using a 2nd order fitting. The approach is stopped at reaching the maximum.



**DAE System** 



### **Probe Specifications**

**Calibration:** In air from 10 MHz to 6.0 GHz

In brain and muscle simulating tissue at Frequencies of 450 MHz, 835 MHz, 1750 MHz, 1900 MHz, 2450 MHz, 2600 MHz, 3500 MHz, 5200

MHz, 5300 MHz, 5600 MHz, 5800 MHz

Frequency: 10 MHz to 6 GHz

Linearity: ±0.2dB (30 MHz to 6 GHz)

Dynamic: 10 mW/kg to 100 W/kg

Range: Linearity: ±0.2dB

**Dimensions:** Overall length: 330 mm

Tip length: 20 mm


Body diameter: 12 mm

Tip diameter: 2.5 mm

Distance from probe tip to sensor center: 1 mm

Application: **SAR Dosimetry Testing** 

Compliance tests of wireless device



A - BEAM

**Figure 2.2 Triangular Probe Configurations** 



Figure 2.3 Probe Thick-Film Technique



#### **Probe Calibration Process**

### **Dosimetric Assessment Procedure**

Each probe is calibrated according to a dosimetric assessment procedure described in with accuracy better than +/- 10%. The spherical isotropy was evaluated with the procedure described in and found to be better than +/-0.25dB. The sensitivity parameters (Norm X, Norm Y, Norm Z), the diode compression parameter (DCP) and the conversion factor (Conv F) of the probe is tested.

#### **Free Space Assessment**

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies below 1 GHz, and in a waveguide above 1GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity at the proper orientation with the field. The probe is then rotated 360 degrees until the three channels show the maximum reading. The power density readings equates to 1 mW/cm<sup>2</sup>.

### Temperature Assessment \*

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium, correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor based temperature probe is used in conjunction with the E-field probe

$$SAR = C \frac{\Delta T}{\Delta t}$$

$$SAR = \frac{\left|E\right|^2 \cdot \sigma}{\rho}$$

where: where:

 $\Delta t$  = exposure time (30 seconds),  $\sigma$  = simulated tissue conductivity,

C = heat capacity of tissue (brain or muscle),  $\rho$  = Tissue density (1.25 g/cm<sup>3</sup> for brain tissue)

 $\Delta T$  = temperature increase due to RF exposure.

SAR is proportional to  $\Delta T$  /  $\Delta t$  , the initial rate of tissue heating, before thermal diffusion takes place.

Now it's possible to quantify the electric field in the simulated tissue by equating the thermally derived SAR to the E- field;




Figure 2.4 E-Field and Temperature Measurements at 900MHz




Figure 2.5 E-Field and Temperature Measurements at 1800MHz



### **Data Extrapolation**

The DASY52 software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given like below:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$
 with  $V_i$  = compensated signal of channel i (i=x,y,z) 
$$U_i = \text{input signal of channel i}$$
 (i=x,y,z) 
$$cf = \text{crest factor of exciting field}$$
 (DASY parameter) 
$$dcp_i = \text{diode compression point}$$
 (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes: with  $V_i$  = compensated signal of channel i (i = x,y,z) Norm<sub>i</sub> = sensor sensitivity of channel i (i = x,y,z)  $\mu V/(V/m)^2$  for E-field probes ConvF = sensitivity of enhancement in solution E<sub>i</sub> = electric field strength of channel i in V/m

The RSS value of the field components gives the total field strength (Hermetian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

 $SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$  with SAR = local specific absorption rate in W/g = total field strength in V/m = conductivity in [mho/m] or [Siemens/m]  $\rho$  = equivalent tissue density in g/cm<sup>3</sup>

The power flow density is calculated assuming the excitation field to be a free space field.

 $P_{prox} = \frac{E_{tot}^2}{3770}$  with  $P_{pwe} = \text{equivalent power density of a plane wave in W/cm}^2$  = total electric field strength in V/m



### Scanning procedure

- The DASY installation includes predefined files with recommended procedures for measurements and system check. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.
- The "reference" and "drift" measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. +/- 5 %.
- The highest integrated SAR value is the main concern in compliance test applications. These values can mostly be found at the inner surface of the phantom and cannot be measured directly due to the sensor offset in the probe. To extrapolate the surface values, the measurement distances to the surface must be known accurately. A distance error of 0.5mm could produce SAR errors of 6% at 1800 MHz. Using predefined locations for measurements is not accurate enough. Any shift of the phantom (e.g., slight deformations after filling it with liquid) would produce high uncertainties. For an automatic and accurate detection of the phantom surface, the DASY5 system uses the mechanical surface detection. The detection is always at touch, but the probe will move backward from the surface the indicated distance before starting the measurement.
- The "area scan" measures the SAR above the DUT or verification dipole on a parallel plane to the surface. It is used to locate the approximate location of the peak SAR with 2D spline interpolation. The robot performs a stepped movement along one grid axis while the local electrical field strength is measured by the probe. The probe is touching the surface of the SAM during acquisition of measurement values. The scan uses different grid spacings for different frequency measurements. Standard grid spacing for head measurements in frequency ranges 2GHz is 15 mm in x and y- dimension. For higher frequencies a finer resolution is needed, thus for the grid spacing is reduced according the following table:

Area scan grid spacing for different frequency ranges					
Frequency range Grid spacing					
≤ 2 GHz	≤ 15 mm				
2 – 4 GHz	≤ 12 mm				
4 – 6 GHz	≤ 10 mm				

Grid spacing and orientation have no influence on the SAR result. For special applications where the standard scan method does not find the peak SAR within the grid, e.g. mobile phones with flip cover, the grid can be adapted in orientation. Results of this coarse scan are shown in annex B.



• A "zoom scan" measures the field in a volume around the 2D peak SAR value acquired in the previous "coarse" scan. It uses a fine meshed grid where the robot moves the probe in steps along all the 3 axis (x,y and z-axis) starting at the bottom of the Phantom. The grid spacing for the cube measurement is varied according to the measured frequency range, the dimensions are given in the following table:

Zoom scan grid spacing and volume for different frequency ranges						
Ereguency range	Grid spacing	Grid spacing	Minimum zoom			
Frequency range	for x, y axis	for z axis	scan volume			
≤ 2 GHz	≤ 8 mm	≤ 5 mm	≥ 30 mm			
2 – 3 GHz	≤ 5 mm	≤ 5 mm	≥ 28 mm			
3 – 4 GHz	≤ 5 mm	≤ 4 mm	≥ 28 mm			
4 – 5 GHz	≤ 4 mm	≤ 3 mm	≥ 25 mm			
5 – 6 GHz	≤ 4 mm	≤ 2 mm	≥ 22 mm			

DASY is also able to perform repeated zoom scans if more than 1 peak is found during area scan. In this document, the evaluated peak 1g and 10g averaged SAR values are shown in the 2D-graphics in annex B. Test results relevant for the specified standard (see section 3) are shown in table form in section 7.



### **Spatial Peak SAR Evaluation**

The spatial peak SAR - value for 1 and 10 g is evaluated after the Cube measurements have been done. The basis of the evaluation are the SAR values measured at the points of the fine cube grid consisting of all points in the three directions x, y and z. The algorithm that finds the maximal averaged volume is separated into three different stages.

- The data between the dipole center of the probe and the surface of the phantom are extrapolated. This data cannot be measured since the center of the dipole is 1 to 2.7 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is about 1 mm (see probe calibration sheet). The extrapolated data from a cube measurement can be visualized by selecting 'Graph Evaluated'.
- The maximum interpolated value is searched with a straight-forward algorithm. Around this maximum the SAR values averaged over the spatial volumes (1g or 10 g) are computed using the 3d-spline interpolation algorithm. If the volume cannot be evaluated (i.e., if a part of the grid was cut off by the boundary of the measurement area) the evaluation will be started on the corners of the bottom plane of the cube.
- All neighbouring volumes are evaluated until no neighbouring volume with a higher average value is found.

### **Extrapolation**

The extrapolation is based on a least square algorithm [W. Gander, Computermathematik, p.168-180]. Through the points in the first 3 cm along the z-axis, polynomials of order four are calculated. These polynomials are then used to evaluate the points between the surface and the probe tip. The points, calculated from the surface, have a distance of 1 mm from each other.

#### Interpolation

The interpolation of the points is done with a 3d-Spline. The 3d-Spline is composed of three one-dimensional splines with the "Not a knot"-condition [W. Gander, Computermathematik, p.141-150] (x, y and z -direction) [Numerical Recipes in C, Second Edition, p.123ff].

#### **Volume Averaging**

At First the size of the cube is calculated. Then the volume is integrated with the trapezoidal algorithm. 8000 points (20x20x20) are interpolated to calculate the average.

#### **Advanced Extrapolation**

DASY uses the advanced extrapolation option which is able to compensate boundary effects on Efield probes.



### **SAM PHANTOM**

The SAM Twin Phantom V4.0 is constructed of a fiberglass shell integrated in a wooden table. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90% of all users. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. (see Fig. 2.6)

### **Phantom Specification**

**Phantom:** SAM Twin Phantom (V4.0) **Shell Material:** Vivac Composite

Thickness:  $2.0 \pm 0.2 \text{ mm}$ 



Figure 2.6 SAM Twin Phantom

#### **Device Holder for Transmitters**

In combination with the SAM Twin Phantom V4.0 the Mounting Device (see Fig. 2.7), enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation point is the ear opening. The devices can be easily, accurately, and repeat ably be positioned according to the FCC, CENELEC, IEC and IEEE specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).



**Figure 2.7 Mounting Device** 

Note: A simulating human hand is not used due to the complex anatomical and geometrical structure of the hand that may produce infinite number of configurations. To produce the worst-case condition (the hand absorbs antenna output power), the hand is omitted during the tests.



# 3. Probe and Dipole Calibration

See Appendix D and E.



# 4. Phantom & Simulating Tissue Specifications

## **Head & Body Simulating Mixture Characterization**

The head and body mixtures consist of the material based on the table listed below. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the desired tissue. Body tissue parameters that have not been specified in P1528 are derived from the issue dielectric parameters computed from the 4-Cole-Cole equations.

Table 4.1 Typical Composition of Ingredients for Tissue

Ingredients		Simulating Tissue					
		835 MHz Body	900 MHz Body	1900 MHz Body	2450 MHz Body		
Mixing Percentage							
Water		52.50	52.50	69.91	73.20		
Sugar		45.00	45.00	0.00	0.00		
Salt		1.40	1.40	0.13	0.10		
HEC		1.00	1.00	0.00	0.00		
Bactericide		0.10	0.10	0.00	0.00		
DGBE		0.00	0.00 0.00		26.70		
Dielectric Constant	Target	55.20	55.00	53.30	52.70		
Conductivity (S/m)	Target	0.97	1.05	1.52	1.95		



# 5. ANSI/IEEE C95.1 – 1992 RF Exposure Limits [2]

#### **Uncontrolled Environment**

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

### **Controlled Environment**

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

**Table 5.1 Human Exposure Limits** 

	UNCONTROLLED ENVIRONMENT General Population (W/kg) or (mW/g)	CONTROLLED ENVIROMENT Professional Population (W/kg) or (mW/g)
SPATIAL PEAK SAR <sup>1</sup> Head	1.60	8.00
SPATIAL AVERAGE SAR <sup>2</sup> Whole Body	0.08	0.40
SPATIAL PEAK SAR <sup>3</sup> Hands, Feet, Ankles, Wrists	4.00	20.00

<sup>&</sup>lt;sup>1</sup> The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

<sup>&</sup>lt;sup>2</sup> The Spatial Average value of the SAR averaged over the whole body.

<sup>&</sup>lt;sup>3</sup> The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.



# 6. Measurement Uncertainty

Measurement uncertainty table is not required per KDB 865664 D01 v01 section 2.8.2 page 12. SAR measurement uncertainty analysis is required in the SAR report only when the highest measured SAR in a frequency band is  $\geq$  1.5 W/kg for 1-g SAR. The equivalent ratio (1.5/1.6) should be applied to extremity and occupational exposure conditions. The highest reported value is less than 1.5 W/kg. Therefore, the measurement uncertainty table is not required.



# 7. System Validation

### **Tissue Verification**

**Table 7.1 Measured Tissue Parameters** 

	Table III measured ilegae i arametere							
		835 MHz Body		1900 MHz Body		2450 MHz Body		
Date(s)		Jul.	24, 2014	Jul. 23, 2014		Jul. 25, 2014		
Liquid Temperature (°C)	20.0	Target	Measured	Target	Measured	Target	Measured	
Dielectric Constant: ε		55.20	54.37	53.30	53.17	52.70	52.77	
Conductivity: σ		0.97	0.98	1.52	1.54	1.95	1.92	
		900 N	/IHz Body	900 N	/IHz Body			
Date(s)		Jan.	30, 2015	Apr. 28, 2015				
Liquid Temperature (°C)	20.0	Target	Measured	Target	Measured			
Dielectric Constant: ε		55.00	54.99	55.00	55.39			
Conductivity: σ		1.05	1.06	1.05	1.06			

See Appendix A for data printout.

# **Test System Verification**

Prior to assessment, the system is verified to the  $\pm 10\%$  of the specifications at the test frequency by using the system kit. Power is normalized to 1 watt. (Graphic Plots Attached)

**Table 7.2 System Dipole Validation Target & Measured** 

	Test Frequency	Targeted SAR <sub>1g</sub> (W/kg)	Measure SAR <sub>1g</sub> (W/kg)	Tissue Used for Verification	Deviation Target and Fast SAR to SAR (%)	Plot Number
24-Jul-2014	835 MHz	9.51	9.43	Body	- 0.84	1
23-Jul-2014	1900 MHz	40.20	40.20	Body	+ 0.00	2
25-Jul-2014	2450 MHz	51.50	51.20	Body	- 0.58	3
30-Jan-2015	900 MHz	10.70	10.90	Body	+ 1.87	4
28-Apr-2015	900 MHz	10.70	10.70	Body	+ 0.00	5

See Appendix A for data plots.5




Figure 7.1 Dipole Validation Test Setup



# 8. SAR Test Data Summary See Measurement Result Data Pages

See Appendix B for SAR Test Data Plots. See Appendix C for SAR Test Setup Photos.

### **Procedures Used To Establish Test Signal**

The device was either placed into simulated transmit mode using the manufacturer's test codes or the actual transmission is activated through a base station simulator or similar equipment. See data pages for actual procedure used in measurement.

### **Device Test Condition**

In order to verify that the device was tested at full power, conducted output power measurements were performed before and after each SAR measurement to confirm the output power unless otherwise noted. If a conducted power deviation of more than 5% occurred, the test was repeated. The power drift of each test is measured at the start of the test and again at the end of the test. The drift percentage is calculated by the formula ((end/start)-1)\*100 and rounded to three decimal places. The drift percentage is calculated into the resultant SAR value on the data sheet for each test.

The EUT was tested on all sides except the front of the device where the antenna was within 25 mm of that side. All measurements were conducted with the side of the device in direct contact with the phantom.


The Bluetooth transmitter does not simultaneously transmit with the WiFi transmitter, but can transmit simultaneous with the WWAN. The WiFi can also transmit simultaneously with the WWAN. The 900 MHz transmitter can transmit simultaneously with the WiFi and Cellular or the BT and Cellular. The table on page 33 below shows the simultaneous configurations. The WiFi/BT and WWAN hotspots are a minimum of 110 mm separation. The 900 MHz and WWAN hotspots are a minimum of 90 mm separation. Simultaneous transmission is evaluated on page 33.

The data rates used when evaluating the WiFi transmitter were the lowest data rates for each mode. The device was operating at its maximum output power at the lowest data rate for all measurements.

The device was on a minimum of 10 cm of Styrofoam during each test. The following is a pictorial drawing of the locations.



### **Location Diagram**

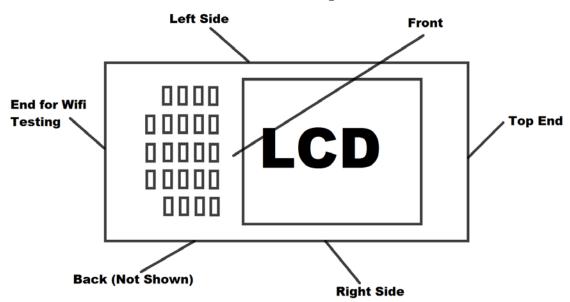



Band	Mode	Bandwidth (MHz)	Channel	Frequency (MHz)	Data Rate	Antenna	Power (dBm)
			1	2412			19.64
	802.11b	20	6	2437	1 Mbps	Main	19.72
			11	2462			19.67
		2.11g 20	1	2412	6 Mbps	Main	16.59
	802.11g		6	2437			19.65
2450 MHz			11	2462			19.54
			1	2412	HT4	Main	19.32
	802.11n	20	6	2437			19.41
			11	2462			19.37
			3	2422	HT4	Main	19.19
	802.11n	11n 40	6	2437			19.26
			9	2452			19.22

Band	Channel	Frequency (MHz)	Power (dBm)
952 MHz	1	956.3	23.46
	2	952.8	23.51

Band	Channel	Frequency (MHz)	Power (dBm)
915 MHz	1	903.08	0.12
	2	915	0.32
	3	927.69	0.08



3GPP Release	Cellular Band IdBmi		Sub-Test (See Table	MPR		
Version		4132	4183	4233	` Below)	
99	WCDMA	23.37	23.39	23.29	-	-
6		23.31	23.30	23.18	1	0
6	HSDPA	23.34	23.32	23.23	2	0
6	порга	22.91	22.89	22.76	3	0.5
6		22.86	22.91	22.72	4	0.5
6		23.32	23.31	23.21	1	0
6		21.41	21.49	21.32	2	2
6	HSUPA	22.46	22.40	22.39	3	1
6		21.38	21.36	21.27	4	2
6		23.29	23.31	23.22	5	0

3GPP Release	Mode	PCS Band [dBm]			Sub-Test (See Table	MPR
Version		9262	9400	9538	` Below)	
99	WCDMA	23.72	23.79	23.64	-	-
6		23.65	23.71	23.59	1	0
6	HSDPA	23.61	23.74	23.60	2	0
6	порга	23.19	23.26	23.12	3	0.5
6		23.26	23.33	23.07	4	0.5
6		23.64	23.72	23.58	1	0
6		21.85	21.81	21.76	2	2
6	HSUPA	22.69	22.74	22.63	3	1
6		21.77	21.82	21.63	4	2
6		23.69	23.76	23.61	5	0

**Sub-Test Setup for Release 6 HSDPA** 

Sub-Test	βc	$\beta_{d}$	B <sub>c</sub> / β <sub>d</sub>	$\beta_{hs}$	
1	2/15	15/15	2/15	4/15	
2	12/15	15/15	15/15	24/15	
3	15/15	8/15	15/8	30/15	
4	15/15	4/15	15/4	30/15	
$\Delta_{\text{ack}}$ , $\Delta_{\text{nack}}$ and $\Delta_{\text{cqi}} = 8$					

**Sub-Test Setup for Release 6 HSUPA** 

Sub-Test	$eta_{c}$	$\beta_{d}$	B <sub>c</sub> / β <sub>d</sub>	$\beta_{hs}$	B <sub>ec</sub>	$B_{ed}$	MPR	AG Index	E-TFCI
1	11/15	15/15	11/15	22/15	209/225	1039/225	0.0	20	75
2	6/15	15/15	6/15	12/15	12/15	94/75	2.0	12	67
3	15/15	9/15	15/9	30/15	30/15	47/15	1.0	15	92
4	2/15	15/15	2/15	4/15	2/15	56/15	2.0	17	71
5	15/15	15/15	15/15	30/15	24/15	134/15	0.0	21	81
$\Delta_{ack}$ , $\Delta_{nack}$ at	$nd \Delta_{cai} = 8$	3							



GPRS-GMSK/1 slot					
Band	Channel	Peak Power	Frame Average		
	128	33.76	24.73		
Cellular	190	33.81	24.78		
	251	33.67	24.64		
PCS	512	30.78	21.75		
	661	30.87	21.84		
	810	30.81	21.78		

	GPRS-GMSK/2 slot					
Band Channel Peak Fra Power Ave						
	128	31.75	25.73			
Cellular	190	31.79	25.77			
	251	31.72	25.70			
	512	28.59	22.57			
PCS	661	28.64	22.62			
	810	28.55	22.53			

	GPRS-GMSK/3 slot				
Band	Channel	Peak Power	Frame Average		
	128	28.81	24.55		
Cellular	190	28.86	24.60		
	251	28.77	24.51		
PCS	512	25.67	21.41		
	661	25.71	21.45		
	810	25.63	21.37		

GPRS-GMSK/4 slot					
Band	Channel	Peak Power	Frame Average		
	128	27.59	24.58		
Cellular	190	27.66	24.65		
	251	27.62	24.61		
PCS	512	24.69	21.68		
	661	24.78	21.77		
	810	24.72	21.71		

EDGE-8PSK/1 slot					
Band	Channel	Peak Power	Frame Average		
	128	27.76	18.73		
Cellular	190	27.89	18.86		
	251	27.82	18.79		
PCS	512	26.56	17.53		
	661	26.68	17.65		
	810	26.63	17.60		

	EDGE-8P	SK/2 slot		
Band	Channel	Peak Power	Frame Average	
	128	24.46	18.44	
Cellular	190	24.51	18.49	
	251	24.44	18.42	
	512	23.68	17.66	
PCS	661	23.75	17.73	
	810	23.79	17.77	

EDGE-8PSK/3 slot				
Band Channel Peak Power			Frame Average	
	128	22.21	17.95	
Cellular	190	22.36	18.10	
	251	22.45	18.19	
	512	21.49	17.23	
PCS	661	21.56	17.30	
	810	21.47	17.21	

EDGE-8PSK/4 slot					
Band	Frame Average				
	128	21.67	18.66		
Cellular	190	21.82	18.81		
	251	21.87	18.86		
PCS	512	20.79	17.78		
	661	20.67	17.66		
	810	20.83	17.82		



Figure 8.1 Test Reduction Table - 835 MHz Band 5

rigaro ori roccittodaction			<del></del>	
Band/	Technology	Side	Required	Tested/
Frequency (MHz)			Channel	Reduced
			128	Reduced <sup>1</sup>
		Back	190	Tested
			251	Reduced <sup>1</sup>
	GPRS – 2		128	Reduced <sup>1</sup>
	Slot	Left	190	Tested
	Siot		251	Reduced <sup>1</sup>
		Right	128	Reduced <sup>1</sup>
			190	Tested
			251	Reduced <sup>1</sup>
Band 5	All other slo	Reduced <sup>2</sup>		
824-849 MHz		Back	4132	Reduced <sup>1</sup>
			4183	Tested
			4233	Reduced <sup>1</sup>
			4132	Reduced <sup>1</sup>
	WCDMA	Left	4183	Tested
			4233	Reduced <sup>1</sup>
			4132	Reduced <sup>1</sup>
		Right	4183	Tested
			4233	Reduced <sup>1</sup>
	HSDF	A and HSL	JPA	Reduced <sup>3</sup>

Reduced<sup>1</sup> – When the mid channel is 3 dB below the limit, the remaining channels are not required per KDB 447498 D01 v05r02 section 4.3.3 page 14.

Reduced<sup>2</sup> – When the conducted power in this mode is less than 0.25 dB higher than the tested mode, testing is not required per KDB 941225 D03 v01.

Reduced<sup>3</sup> – When the conducted power in this mode is less than 0.25 dB higher than the tested mode, testing is not required per KDB 941225 D02 v02r02.



Figure 8.2 Test Reduction Table - 1900 MHz Band 2

Band/ Frequency (MHz)	Technology	Side	Required Channel	Tested/ Reduced
			512	Tested
		Back	661	Tested
			810	Tested
	CDDC 2		512	Reduced <sup>1</sup>
	GPRS – 2	Left	661	Tested
	Slot		810	Reduced <sup>1</sup>
			512	Reduced <sup>1</sup>
		Right	661	Tested
			810	Reduced <sup>1</sup>
Band 2	All other slo	Reduced <sup>2</sup>		
1850-1910 MHz			9262	Tested
		Back	9400	Tested
			9538	Tested
			9262	Reduced <sup>1</sup>
	WCDMA	Left	9400	Tested
			9538	Reduced <sup>1</sup>
			9262	Reduced <sup>1</sup>
		Right	9400	Tested
			9538	Reduced <sup>1</sup>
	HSDF	PA and HSU	JPA	Reduced <sup>3</sup>

Reduced<sup>1</sup> – When the mid channel is 3 dB below the limit, the remaining channels are not required per KDB 447498 D01 v05r02 section 4.3.3 page 14.

Reduced<sup>2</sup> – When the conducted power in this mode is less than 0.25 dB higher than the tested mode, testing is not required per KDB 941225 D03 v01.

Reduced<sup>3</sup> – When the conducted power in this mode is less than 0.25 dB higher than the tested mode, testing is not required per KDB 941225 D02 v02r02.



Figure 8.3 Test Reduction Table – 2.4 GHz Main

Mode	Side	Required Channel	Tested/Reduced
		1 – 2412 MHz	Reduced <sup>1</sup>
	Back	6 – 2437 MHz	Tested
		11 – 2462 MHz	Reduced <sup>1</sup>
		1 – 2412 MHz	Reduced <sup>1</sup>
802.11b	Left	6 – 2437 MHz	Tested
		11 – 2462 MHz	Reduced <sup>1</sup>
		1 – 2412 MHz	Reduced <sup>1</sup>
	Right	6 – 2437 MHz	Tested
		11 – 2462 MHz	Reduced <sup>1</sup>
		1 – 2412 MHz	Reduced <sup>2</sup>
	Back	6 – 2437 MHz	Reduced <sup>2</sup>
		11 – 2462 MHz	Reduced <sup>2</sup>
		1 – 2412 MHz	Reduced <sup>2</sup>
802.11g	Left	6 – 2437 MHz	Reduced <sup>2</sup>
		11 – 2462 MHz	Reduced <sup>2</sup>
		1 – 2412 MHz	Reduced <sup>2</sup>
	Right	6 – 2437 MHz	Reduced <sup>2</sup>
		11 – 2462 MHz	Reduced <sup>2</sup>
		1 – 2412 MHz	Reduced <sup>2</sup>
	Back	6 – 2437 MHz	Reduced <sup>2</sup>
		11 – 2462 MHz	Reduced <sup>2</sup>
		1 – 2412 MHz	Reduced <sup>2</sup>
802.11n	Left	6 – 2437 MHz	Reduced <sup>2</sup>
		11 – 2462 MHz	Reduced <sup>2</sup>
		1 – 2412 MHz	Reduced <sup>2</sup>
	Right	6 – 2437 MHz	Reduced <sup>2</sup>
		11 – 2462 MHz	Reduced <sup>2</sup>

Reduced¹ – When the mid channel is 3 dB below the limit, the remaining channels are not required per KDB 447498 D01 v05r01 section 4.3.3 page 14.

Reduced<sup>2</sup> – When the conducted power in this mode is less than 0.25 dB higher than the b mode, testing is not required per KDB 248227 page 5.



Figure 8.4 Test Reduction Table – 900 MHz

Band/ Frequency (MHz)	Technology	Side	Required Channel	Tested/ Reduced
		Back	1	Tested
952 MHz	DSB-AM	Left	1	Tested
		Right	1	Tested
			1	Reduced <sup>1</sup>
		Back	2	Tested
			3	Reduced <sup>1</sup>
			1	Reduced <sup>1</sup>
915 MHz	DSSS	Left	2	Tested
			3	Reduced <sup>1</sup>
			1	Reduced <sup>1</sup>
		Right	2	Tested
			3	Reduced <sup>1</sup>

Reduced¹ – When the mid channel is 3 dB below the limit, the remaining channels are not required per KDB 447498 D01 v05r02 section 4.3.3 page 14.



# SAR Data Summary – 835 MHz Body

MEASUREMENT RESULTS										
Plot	Gap	Position	Frequ	iency	Modulation	End Power	Measured	Reported		
	Cup	1 03111011	MHz	Ch.		(dBm)	SAR (W/kg)	SAR (W/kg)		
1		Back	836.6	190		31.79	0.405	0.43		
		Left	836.6	190	GMSK	31.79	0.228	0.24		
	0 mm	Right	836.6	190		31.79	0.126	0.13		
2	0 mm	Back	836.6	4183		23.39	0.390	0.40		
		Left	836.6	4183	WCDMA	23.39	0.224	0.23		
		Right	836.6	4183		23.39	0.125	0.13		

Body
1.6 W/kg (mW/g)
averaged over 1 gram

Battery is fully charged for all t	ests.		
Power Measured		□ERP	□EIRP
SAR Measurement			
Phantom Configuration	Left Head	⊠Eli4	Right Head
SAR Configuration	Head	$\boxtimes$ Body	
Test Signal Call Mode	Test Code	⊠Base Station Simular	tor
Test Configuration	☐With Belt Clip	☐Without Belt Clip	⊠N/A
Tissue Depth is at least 15.0 cm	1		
	Power Measured SAR Measurement Phantom Configuration SAR Configuration Test Signal Call Mode Test Configuration	SAR Measurement Phantom Configuration SAR Configuration Test Signal Call Mode  Left Head Head Test Code	Power Measured  SAR Measurement  Phantom Configuration  SAR Configuration  Test Signal Call Mode  Test Configuration  With Belt Clip  DERP  ERP  ERP  EI14  SAR Configuration  Head  Body  Test Code  Base Station Simulation  With Belt Clip



# SAR Data Summary – 1900 MHz Body

MEA	MEASUREMENT RESULTS										
Plot	Gap	Position	Freque	ency	Modulation	End Power	Measured	Reported			
	Cup		MHz	Ch.	Modulation	(dBm)	SAR (W/kg)	SAR (W/kg)			
3		Back	1850.2	512		28.59	1.12	1.23			
			1880.0	661	GMSK	28.64	1.09	1.18			
			1909.8	810		28.55	0.889	0.99			
		Left	1880.0	661		28.64	0.0441	0.05			
		Right	1880.0	661		28.64	0.0548	0.06			
4	0 mm		1852.4	9262		23.72	1.20	1.28			
		Back	1880.0	9400		23.79	1.06	1.11			
			1907.6	9538	WCDMA	23.64	0.861	0.94			
		Left	1880.0	9400		23.79	0.0448	0.05			
		Right	1880.0	9400		23.79	0.0932	0.10			
		Repeat	1852.4	9262	WCDMA	23.72	1.13	1.21			

Body
1.6 W/kg (mW/g)
averaged over 1 gram

1.	Battery is fully charged for all	tests.		
	Power Measured		□ERP	□EIRP
2.	SAR Measurement			
	Phantom Configuration	Left Head	⊠Eli4	Right Head
	SAR Configuration	Head	$\boxtimes$ Body	-
3.	Test Signal Call Mode	☐Test Code	⊠Base Station Simula	ator
4.	Test Configuration	☐With Belt Clip	☐Without Belt Clip	$\sum N/A$

5. Tissue Depth is at least 15.0 cm



# SAR Data Summary – 2450 MHz Body 802.11b

ME	MEASUREMENT RESULTS										
Plot	Gap	Position Frequency Modulation		Modulation	End Power Measured SAR		Reported SAR				
	Gap	Position	MHz	Ch.	Woddiation	(dBm)	(W/kg)	(W/kg)			
		Back	2437	6	DSSS	19.72	0.117	0.13			
5		Right	2437	6	DSSS	19.72	0.137	0.15			
	0 mm	End	2437	6	DSSS	19.72	0.171	0.18			
	Ullilli	Back	2440	39	GFSK	7.83	0.0082	0.01			
		Right	2440	39	GFSK	7.83	0.0103	0.01			
		End	2440	39	GFSK	7.83	0.0128	0.01			

Body
1.6 W/kg (mW/g)
averaged over 1 gram

1.	Battery is fully charged for a	ıll tests.		
	Power Measured	⊠Conducted	□ERP	☐EIRP
2.	SAR Measurement			
	Phantom Configuration	Left Head	⊠Eli4	Right Head
	SAR Configuration	Head	$\boxtimes$ Body	
3.	Test Signal Call Mode	⊠Test Code	☐Base Station Sim	ulator
4.	Test Configuration	☐With Belt Clip	Without Belt Clip	N/A
5.	Tissue Depth is at least 15.0	cm		



# SAR Data Summary – 900 MHz Body

MEA	MEASUREMENT RESULTS										
Plot	Gap	Position	Frequ	iency	Modulation	End Power	Measured	Reported			
1 100	G	1 00111011	MHz Ch.	Ch.	Modulation	(dBm)	SAR (W/kg)	SAR (W/kg)			
6		Back	952	1		23.51	0.0929	0.92			
		Left	952	1	DSB-AM	23.51	0.0536	0.53			
	0 mm	Right	952	1		23.51	0.0556	0.55			
	0 mm	Back	915	2		0.32	0.0166	0.02			
		Left	915	2	DSSS	0.32	0.0188	0.02			
		Right	915	2		0.32	0.0235	0.03			

Body 1.6 W/kg (mW/g) averaged over 1 gram

1.	Battery is fully charged for all t	ests.		
	Power Measured		□ERP	□EIRP
2.	SAR Measurement			
	Phantom Configuration	Left Head	⊠Eli4	Right Head
	SAR Configuration	Head	$\boxtimes$ Body	
3.	Test Signal Call Mode	Test Code	<b>⊠</b> Base Station Simula	tor
4.	Test Configuration	☐With Belt Clip	☐Without Belt Clip	$\square N/A$
5.	Tissue Depth is at least 15.0 cm	ı		

Jay M. Moulton Vice President

Note: The measured value was first scaled to the maximum power tolerance and then that value was scaled to 100% duty cycle.



# **SAR Data Summary – Simultaneous Evaluation**

# MEASUREMENT RESULTS

												I
Freque	ency	Modulation	Frequ	ency	Modulation			Modulation	SAR₁	SAR <sub>2</sub>	SAR <sub>3</sub>	SAR
MHz	Ch.	modulation	MHz	Ch.		MHz	Ch.	modulation	<b>0</b> 7 (	07 11 12	0, (3	Total
836.6	190	GMSK	2437	6	DSSS	952	1	DSB-AM	0.43	0.18	0.92	1.53
836.3	4183	WCDMA	2437	6	DSSS	952	1	DSB-AM	0.40	0.18	0.92	1.50
1850.2	512	GMSK	2437	6	DSSS	952	1	DSB-AM	1.23	0.18	0.92	2.33
1852.4	9262	WCDMA	2437	6	DSSS	952	1	DSB-AM	1.28	0.18	0.92	2.38
836.6	190	GMSK	2440	39	GFSK	952	1	DSB-AM	0.43	0.01	0.92	1.36
836.3	4183	WCDMA	2440	39	GFSK	952	1	DSB-AM	0.40	0.01	0.92	1.33
1850.2	512	GMSK	2440	39	GFSK	952	1	DSB-AM	1.23	0.01	0.92	2.16
1852.4	9262	WCDMA	2440	39	GFSK	952	1	DSB-AM	1.28	0.01	0.92	2.21

Body
1.6 W/kg (mW/g)
averaged over 1 gram

The worst case simultaneous with the 952 MHz transmitter is with the Cellular transmitter. The sum of the two transmitters does not meet the limit. Therefore, the simultaneous evaluation is based on the distance ratio in KDB447498 section 4.3.2 3). The calculation for the worst case configuration (WCDMA 1900 MHz and 952 MHz) is shown below.

 $(SAR_1 + SAR_2)^{1.5}/R_i \le 0.04$ 

 $(1.28+0.92)^{1.5}/90 = 0.036$  rounded to two digits is 0.04. Therefore, the simultaneous evaluation meets the requirements of KDB 447498 section 4.3.2 3).

Simultaneous Transmit Table					
Transmitter	Cellular (WWAN)	WiFi (WLAN)	Bluetooth	915/952 MHz	
Cellular (WWAN)	N/A	Yes	Yes	Yes	
WiFi (WLAN)	Yes	N/A	No	Yes	
Bluetooth	Yes	No	N/A	Yes	
952 MHz	Yes	Yes	Yes	N/A	



# 9. Test Equipment List

**Table 9.1 Equipment Specifications** 

Туре	Calibration Due Date	Calibration Done Date	Serial Number
Staubli Robot TX60L	N/A	N/A	F07/55M6A1/A/01
Measurement Controller CS8c	N/A	N/A	1012
ELI4 Flat Phantom	N/A	N/A	1065
Device Holder	N/A	N/A	N/A
Data Acquisition Electronics 4	04/10/2015	04/10/2014	1217
Data Acquisition Electronics 4	08/12/2015	08/12/2014	759
SPEAG E-Field Probe EX3DV4	01/28/2015	01/28/2014	3311
SPEAG E-Field Probe EX3DV4	08/18/2015	08/18/2014	3693
SPEAG E-Field Probe EX3DV4	01/23/2016	01/23/2015	3833
Speag Validation Dipole D835V2	12/03/2014	12/03/2012	4d089
Speag Validation Dipole D1900V2	12/06/2014	12/06/2012	5d116
Speag Validation Dipole D2450V2	12/04/2014	12/04/2012	829
Speag Validation Dipole D900V2	12/03/2015	12/03/2012	1d044
Agilent N1911A Power Meter	03/24/2016	03/24/2015	GB45100254
Agilent N1922A Power Sensor	06/25/2015	06/25/2014	MY45240464
Advantest R3261A Spectrum Analyzer	03/26/2017	03/26/2015	31720068
Agilent (HP) 8350B Signal Generator	03/26/2017	03/26/2015	2749A10226
Agilent (HP) 83525A RF Plug-In	03/26/2017	03/26/2015	2647A01172
Agilent (HP) 8753C Vector Network Analyzer	03/26/2017	03/26/2015	3135A01724
Agilent (HP) 85047A S-Parameter Test Set	03/26/2017	03/26/2015	2904A00595
Agilent (HP) 8960 Base Station Sim.	03/31/2017	03/31/2015	MY48360364
Anritsu MT8820C	07/29/2015	07/29/2014	6201176199
Agilent 778D Dual Directional Coupler	N/A	N/A	MY48220184
MiniCircuits BW-N20W5+ Fixed 20 dB	N/A	N/A	N/A
Attenuator			
MiniCircuits SPL-10.7+ Low Pass Filter	N/A	N/A	R8979513746
Aprel Dielectric Probe Assembly	N/A	N/A	0011
Body Equivalent Matter (835 MHz)	N/A	N/A	N/A
Body Equivalent Matter (1900 MHz)	N/A	N/A	N/A
Body Equivalent Matter (2450 MHz)	N/A	N/A	N/A
Body Equivalent Matter (900 MHz)	N/A	N/A	N/A



# 10. Conclusion

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the FCC/IC. These measurements are taken to simulate the RF effects exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The tested device complies with the requirements in respect to all parameters subject to the test. The test results and statements relate only to the item(s) tested.

Please note that the absorption and distribution of electromagnetic energy in the body is a very complex phenomena that depends on the mass, shape, and size of the body; the orientation of the body with respect to the field vectors; and, the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because innumerable factors may interact to determine the specific biological outcome of an exposure to electromagnetic fields, any protection guide shall consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables.



### 11. References

- [1] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radio Frequency Radiation, August 1996
- [2] ANSI/IEEE C95.1 1992, American National Standard Safety Levels with respect to Human Exposure to Radio Frequency Electromagnetic Fields, 300kHz to 100GHz, New York: IEEE, 1992.
- [3] ANSI/IEEE C95.3 1992, IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields RF and Microwave, New York: IEEE, 1992.
- [4] International Electrotechnical Commission, IEC 62209-2 (Edition 1.0), Human Exposure to radio frequency fields from hand-held and body mounted wireless communication devices Human models, instrumentation, and procedures Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz), March 2010.
- [5] IEEE Standard 1528 2013, IEEE Recommended Practice for Determining the Peak-Spatial Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communication Devices: Measurement Techniques, June 2013.
- [6] Industry Canada, RSS 102e, Radio Frequency Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands), March 2010.
- [7] Health Canada, Safety Code 6, Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz, 2009.



# Appendix A – System Validation Plots and Data

RF Exposure Lab

```
Test Result for UIM Dielectric Parameter
Thu 24/Jul/2014
Freq Frequency(GHz)
FCC_eH FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon
FCC_sH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma
FCC_eB FCC Limits for Body Epsilon
FCC_sB FCC Limits for Body Sigma
Test_e Epsilon of UIM
Test s Sigma of UIM
******************
* value interpolated
***************
Test Result for UIM Dielectric Parameter
Wed 23/Jul/2014
Freq Frequency(GHz)
FCC_eH FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon
FCC_sH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma
FCC_eB FCC Limits for Body Epsilon
FCC_sB FCC Limits for Body Sigma
Test_e Epsilon of UIM
Test_s Sigma of UIM
*****************
```

\* value interpolated



```
Test Result for UIM Dielectric Parameter
Fri 25/Jul/2014
Freq Frequency(GHz)
FCC_eH FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon
FCC_sH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma
FCC_eB FCC Limits for Body Epsilon
FCC_sB FCC Limits for Body Sigma
Test_e Epsilon of UIM
Test_s Sigma of UIM
***************
            FCC_eB FCC_sB Test_e Test_s
52.75 1.91 52.85 1.88
52.748 1.912 52.846 1.882*
2.4100
2.4120
               52.748 1.912 52.846 1.882*
52.74 1.92 52.83 1.89
52.73 1.93 52.81 1.90
52.716 1.937 52.796 1.907*
52.71 1.94 52.79 1.91
52.70 1.95 52.77 1.92
52.69 1.96 52.75 1.93
2.4200
2.4300
2.4370
2.4400
2.4500
2.4600

      2.4620
      52.686 1.964 52.746 1.932*

      2.4700
      52.67 1.98 52.73 1.94

      2.4800
      52.66 1.99 52.71 1.95

* value interpolated
Test Result for UIM Dielectric Parameter
Fri 30/Jan/2015
Freq Frequency(GHz)
FCC_eH Limits for Head Epsilon
FCC_sH Limits for Head Sigma
FCC_eB Limits for Body Epsilon
FCC_sB Limits for Body Sigma
Test_e Epsilon of UIM
Test_s Sigma of UIM
****************
Freq FCC_eB FCC_sB Test_e Test_s
Freq FCC_sB FCC_sB Test_e Test_

0.8900 55.03 1.04 55.01 1.05

0.9000 55.00 1.05 54.99 1.06

0.9100 55.00 1.06 54.96 1.07

0.9200 54.99 1.06 54.93 1.08

0.9300 54.97 1.07 54.90 1.09

0.9400 54.95 1.07 54.88 1.10

0.9500 54.93 1.08 54.85 1.11

0.9520 54.926 1.08 54.844 1.11*

0.9600 54.91 1.08 54.82 1.11
```

<sup>\*</sup> value interpolated



<sup>\*</sup> value interpolated



# RF Exposure Lab

### Plot 1

DUT: Dipole 835 MHz D835V2; Type: D835V2; Serial: D835V2 - SN:4d089

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: MSL835; Medium parameters used: f = 835 MHz;  $\sigma$  = 0.98 S/m;  $\varepsilon_r$  = 54.37;  $\rho$  = 1000 kg/m<sup>3</sup>

Phantom section: Flat Section

Test Date: Date: 7/24/2014; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: ES3DV3 - SN3311; ConvF(6.04, 6.04, 6.04); Calibrated: 1/28/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1217; Calibrated: 4/10/2014 Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1065

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7164)

#### **Procedure Notes:**

**835 MHz/Verification/Area Scan (5x11x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 1.18 W/kg

835 MHz/Verification/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 31.227 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 1.47 W/kg


SAR(1 g) = 0.943 W/kg; SAR(10 g) = 0.619 W/kg

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 1.19 W/kg

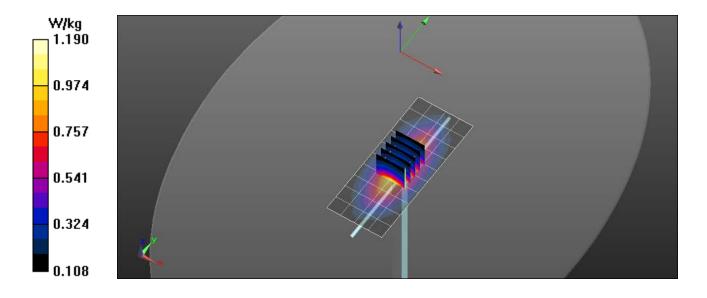



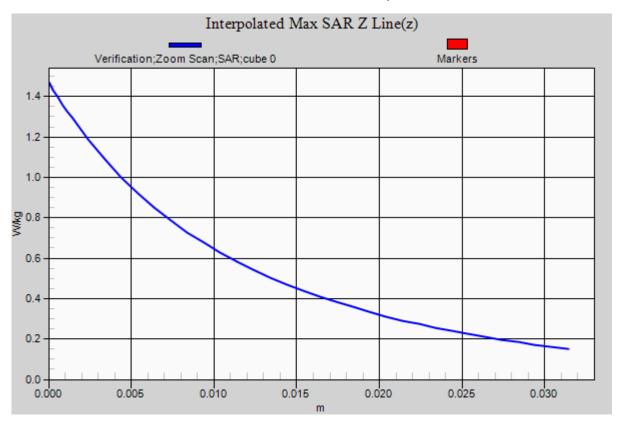



# RF Exposure Lab

### Plot 2

DUT: Dipole 1900 MHz D1900V2; Type: D1900V2; Serial: D1900V2 - SN:5d116

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: MSL1900; Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.54 S/m;  $\varepsilon_r$  = 53.17;  $\rho$  = 1000 kg/m<sup>3</sup>

Phantom section: Flat Section

Test Date: Date: 7/23/2014; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: ES3DV3 - SN3311; ConvF(4.68, 4.68, 4.68); Calibrated: 1/28/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1217; Calibrated: 4/10/2014 Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1065

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7164)

#### **Procedure Notes:**


**1900 MHz/Verification/Area Scan (5x7x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 5.44 W/kg

1900 MHz/Verification/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 31.227 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 7.22 W/kg

SAR(1 g) = 4.02 W/kg; SAR(10 g) = 2.1 W/kg Maximum value of SAR (measured) = 5.77 W/kg

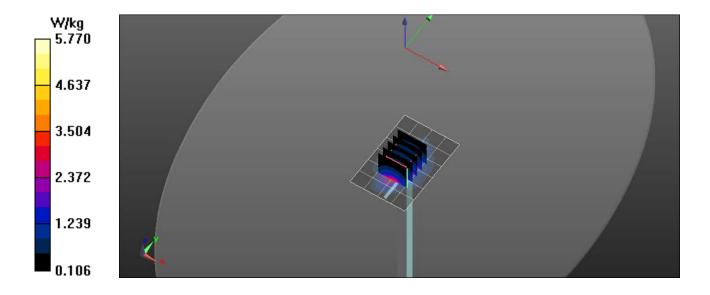



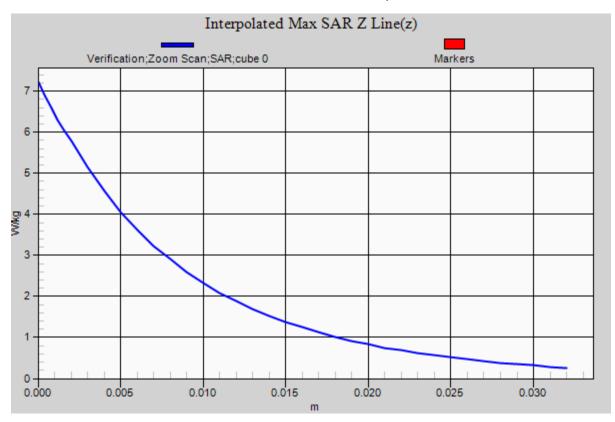



# RF Exposure Lab

### Plot 3

DUT: Dipole 2450 MHz D2450V2; Type: D2450V2; Serial: D2450V2 - SN: 829

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL2450; Medium parameters used: f = 2450 MHz;  $\sigma = 1.92 \text{ S/m}$ ;  $\epsilon_r = 52.77$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Test Date: Date: 7/25/2014; Ambient Temp: 23 °C; Tissue Temp: 21 °C Probe: ES3DV3 – SN3311; ConvF(4.29, 4.29, 4.29); Calibrated: 1/28/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1217; Calibrated: 4/10/2014 Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1065

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7164)

#### **Procedure Notes:**


**Body Verification/2450 MHz/Area Scan (61x101x1):** Interpolated grid: dx=1.200 mm, dy=1.200 mm Maximum value of SAR (interpolated) = 8.92 W/kg

Body Verification/2450 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Reference Value = 53.359 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 11.04 W/kg

**SAR(1 g) = 5.12 W/kg; SAR(10 g) = 2.37 W/kg** Maximum value of SAR (measured) = 8.79 W/kg

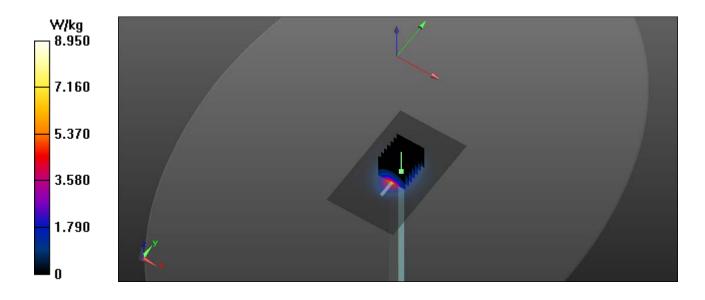



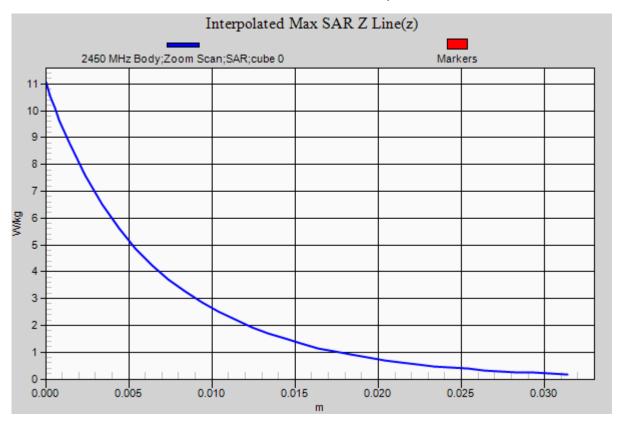



# RF Exposure Lab

### Plot 4

DUT: Dipole 900 MHz D900V2; Type: D900V2; Serial: D900V2 - SN: 1d044

Communication System: CW; Frequency: 900 MHz; Duty Cycle: 1:1

Medium: MSL900; Medium parameters used (interpolated): f = 900 MHz;  $\sigma = 1.11 \text{ mho/m}$ ;  $\epsilon_r = 54.844$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Test Date: Date: 1/30/2015; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 - SN3693; ConvF(8.7, 8.7, 8.7); Calibrated: 8/18/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1217; Calibrated: 4/10/2014 Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1065

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

#### **Procedure Notes:**

900 MHz Body/Verification/Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 1.16 W/kg

900 MHz Body/Verification/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 33.207 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 1.68 W/kg


SAR(1 g) = 1.09 W/kg; SAR(10 g) = 0.693 W/kg

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 1.48 W/kg

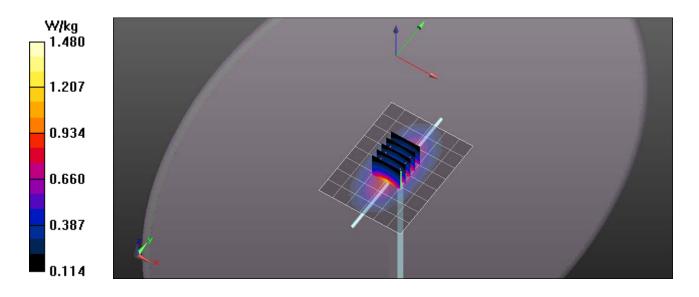



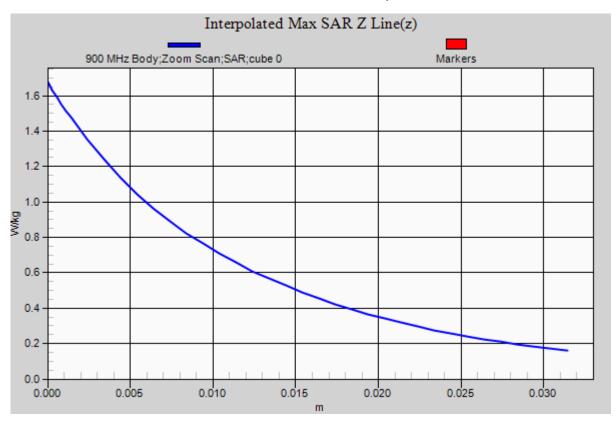



# RF Exposure Lab

### Plot 5

DUT: Dipole 900 MHz D900V2; Type: D900V2; Serial: D900V2 - SN: 1d044

Communication System: CW; Frequency: 900 MHz; Duty Cycle: 1:1

Medium: MSL900; Medium parameters used: f = 900 MHz;  $\sigma = 1.06$  mho/m;  $\epsilon_r = 55.39$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Test Date: Date: 4/28/2015; Ambient Temp: 23° C; Tissue Temp: 21° C Probe: EX3DV4 - SN3833; ConvF(8.51, 8.51, 8.51); Calibrated: 1/23/2015;

Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn759; Calibrated: 8/12/2014 Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1251

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

#### **Procedure Notes:**


**Verification/900 MHz Body/Area Scan (41x101x1):** Interpolated grid: dx=1.500 mm, dy=1.500 mm Maximum value of SAR (interpolated) = 1.15 W/kg

Verification/900 MHz Body/Zoom Scan (5x5x5)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=8mm


Reference Value = 33.828 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 1.591 mW/g

SAR(1 g) = 1.07 mW/g; SAR(10 g) = 0.695 mW/g Maximum value of SAR (measured) = 1.16 W/kg

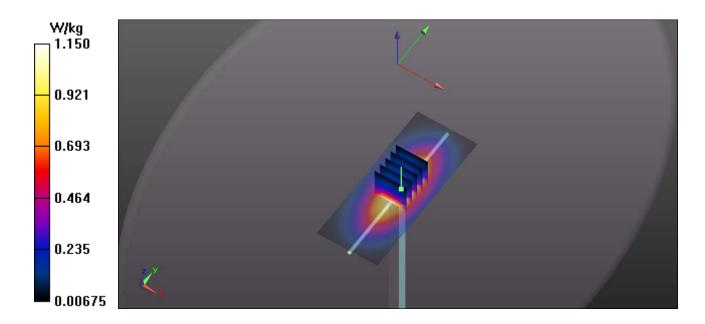



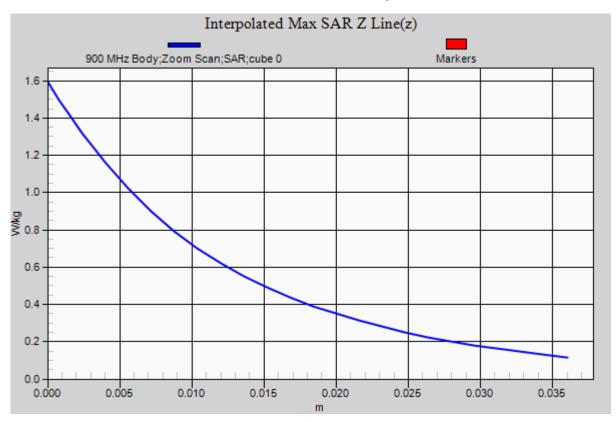



## **Appendix B – SAR Test Data Plots**



# **RF Exposure Lab**

### Plot 1

DUT: Allegro<sup>2</sup>; Type: Handheld Computer; Serial: AG2B096

Communication System: GPRS 2-Slot (GMSK); Frequency: 836.6 MHz; Duty Cycle: 1:4.00037

Medium: MSL835; Medium parameters used (interpolated): f = 836.6 MHz;  $\sigma = 0.982 \text{ S/m}$ ;  $\epsilon_r = 54.375$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Test Date: Date: 7/24/2014; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: ES3DV3 - SN3311; ConvF(6.04, 6.04, 6.04); Calibrated: 1/28/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1217; Calibrated: 4/10/2014 Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1065

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7164)

#### **Procedure Notes:**

850 MHz GPRS/Back Mid/Area Scan (11x7x1): Measurement grid: dx=15mm, dy=15mm

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 0.418 W/kg

850 MHz GPRS/Back Mid/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 21.265 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 0.669 W/kg

SAR(1 g) = 0.405 W/kg; SAR(10 g) = 0.243 W/kg

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 0.446 W/kg

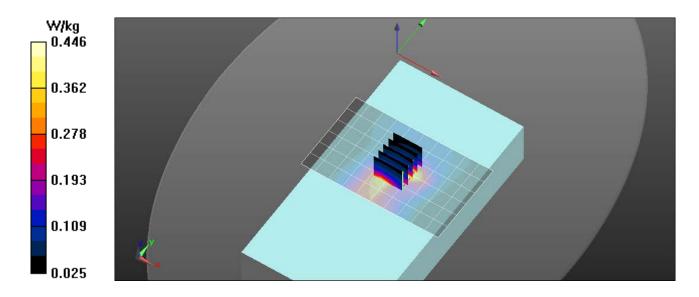



# RF Exposure Lab

### Plot 2

DUT: Allegro<sup>2</sup>; Type: Handheld Computer; Serial: AG2B096

Communication System: UMTS (WCDMA); Frequency: 836.6 MHz; Duty Cycle: 1:1

Medium: MSL835; Medium parameters used (interpolated): f = 836.6 MHz;  $\sigma$  = 0.982 S/m;  $\epsilon_r$  = 54.375;  $\rho$  = 1000 kg/m<sup>3</sup>

Phantom section: Flat Section

Test Date: Date: 7/24/2014; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: ES3DV3 - SN3311; ConvF(6.04, 6.04, 6.04); Calibrated: 1/28/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1217; Calibrated: 4/10/2014 Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1065

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7164)

#### **Procedure Notes:**

850 MHz WCDMA/Back Mid/Area Scan (11x7x1): Measurement grid: dx=15mm, dy=15mm

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 0.398 W/kg

850 MHz WCDMA/Back Mid/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 20.113 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 0.639 W/kg

SAR(1 g) = 0.390 W/kg; SAR(10 g) = 0.236 W/kg

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 0.427 W/kg

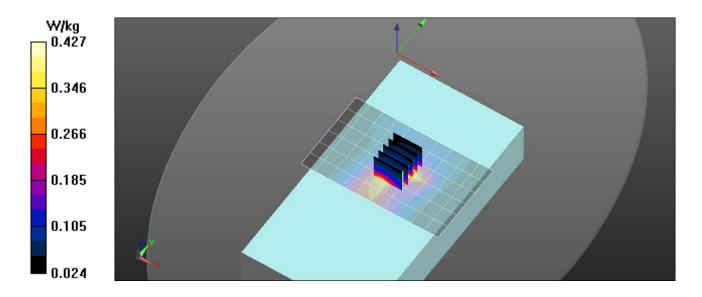



# RF Exposure Lab

### Plot 3

DUT: Allegro<sup>2</sup>; Type: Handheld Computer; Serial: AG2B096

Communication System: GPRS 2-Slot (GMSK); Frequency: 1850.2 MHz; Duty Cycle: 1:4.00037

Medium: MSL1900; Medium parameters used (interpolated): f = 1850.2 MHz;  $\sigma = 1.49$  S/m;  $\epsilon_r = 53.27$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Test Date: Date: 7/23/2014; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: ES3DV3 - SN3311; ConvF(4.68, 4.68, 4.68); Calibrated: 1/28/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1217; Calibrated: 4/10/2014 Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1065

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7164)

#### **Procedure Notes:**

1900 MHz GPRS/Back Low/Area Scan (11x7x1): Measurement grid: dx=15mm, dy=15mm

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 1.20 W/kg

1900 MHz GPRS/Back Low/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 19.937 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 1.89 W/kg

SAR(1 g) = 1.12 W/kg; SAR(10 g) = 0.617 W/kg

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 1.21 W/kg

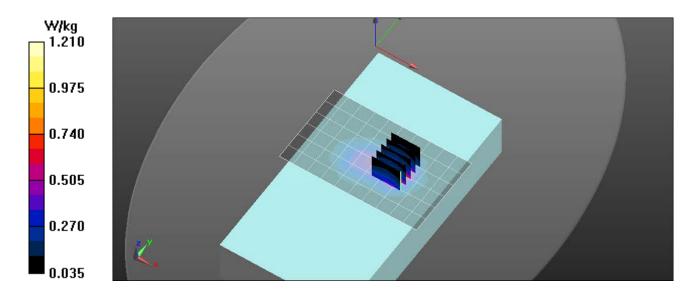



# **RF Exposure Lab**

### Plot 4

DUT: Allegro<sup>2</sup>; Type: Handheld Computer; Serial: AG2B096

Communication System: UMTS (WCDMA); Frequency: 1852.4 MHz; Duty Cycle: 1:1

Medium: MSL1900; Medium parameters used (interpolated): f = 1852.4 MHz;  $\sigma = 1.492$  S/m;  $\varepsilon_r = 53.265$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Test Date: Date: 7/23/2014; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: ES3DV3 - SN3311; ConvF(4.68, 4.68, 4.68); Calibrated: 1/28/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1217; Calibrated: 4/10/2014 Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1065

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7164)

#### **Procedure Notes:**

1900 MHz WCDMA/Back Low/Area Scan (11x7x1): Measurement grid: dx=15mm, dy=15mm

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 1.15 W/kg

1900 MHz WCDMA/Back Low/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 16.815 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 1.94 W/kg

SAR(1 g) = 1.2 W/kg; SAR(10 g) = 0.682 W/kg

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 1.31 W/kg

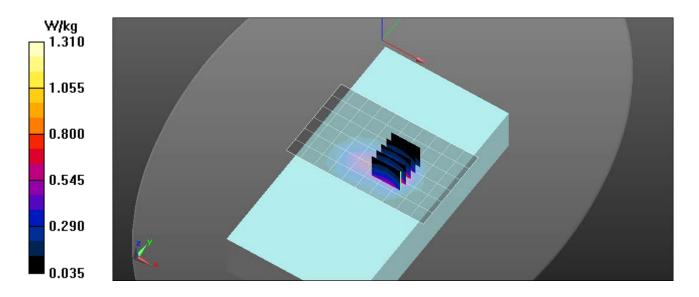



# RF Exposure Lab

### Plot 5

DUT: Allegro<sup>2</sup>; Type: Handheld Computer; Serial: AG2B096

Communication System: WiFi 802.11b (DSSS, 1 Mbps); Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL2450; Medium parameters used (interpolated): f = 2437 MHz;  $\sigma = 1.907$  S/m;  $\epsilon_r = 52.796$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Test Date: Date: 7/25/2014; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: ES3DV3 - SN3311; ConvF(4.29, 4.29, 4.29); Calibrated: 1/28/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1217; Calibrated: 4/10/2014 Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1065

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7164)

#### **Procedure Notes:**

2450 MHz Body/Bottom End Mid/Area Scan (9x15x1): Measurement grid: dx=12mm, dy=12mm

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 0.173 W/kg

2450 MHz Body/Bottom End Mid/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Reference Value = 8.890 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 0.317 W/kg

SAR(1 g) = 0.171 W/kg; SAR(10 g) = 0.092 W/kg

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 0.189 W/kg

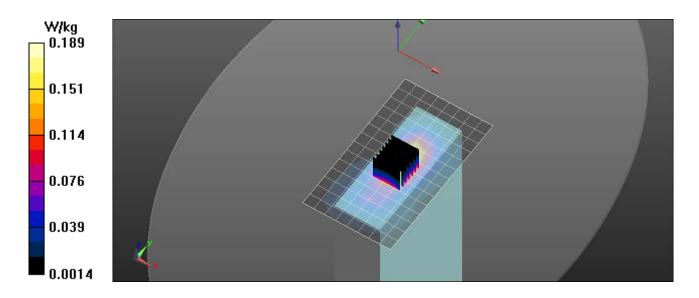



# **RF Exposure Lab**

### Plot 1

DUT: Allegro 2; Type: Handheld Computer; Serial: AB2B274

Communication System: FM; Frequency: 952 MHz; Duty Cycle: 1:8.30042

Medium: MSL900; Medium parameters used (interpolated): f = 952 MHz;  $\sigma = 1.11$  S/m;  $\epsilon_r = 54.844$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Test Date: Date: 1/30/2015; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 - SN3693; ConvF(8.7, 8.7, 8.7); Calibrated: 8/18/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection) Electronics: DAE4 Sn1217; Calibrated: 4/10/2014 Phantom: ELI v4.0; Type: QDOVA001BB; Serial: 1065

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

#### **Procedure Notes:**

900 MHz/Back Mid/Area Scan (11x7x1): Measurement grid: dx=15mm, dy=15mm

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 0.126 W/kg

900 MHz/Back Mid/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 5.907 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 0.151 W/kg

SAR(1 g) = 0.0929 W/kg; SAR(10 g) = 0.0517 W/kg

Info: Interpolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 0.133 W/kg

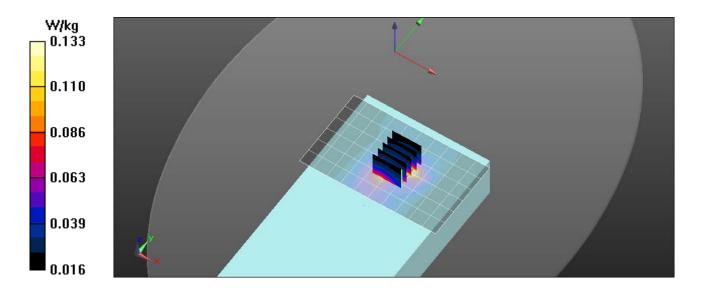



## **Appendix C – SAR Test Setup Photos**



**Test Position Back 0 mm Gap** 





Test Position Left 0 mm Gap





**Test Position Right 0 mm Gap** 





**Front of Device** 





**Back of Device** 





Battery





**Antenna Locations** 



## **Appendix D – Probe Calibration Data Sheets**



### **Calibration Laboratory of** Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





S

C

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura **Swiss Calibration Service** 

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

**RF Exposure Lab** 

Certificate No: ES3-3311\_Jan14/2

## CALIBRATION CERTIFICATE (Replacement of No: ES3-3311

Object

ES3DV3 - SN:3311

Calibration procedure(s)

QA CAL-01.v9, QA CAL-12.v9, QA CAL-23.v5, QA CAL-25.v6 Calibration procedure for dosimetric E-field probes

Calibration date:

January 28, 2014

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	04-Apr-13 (No. 217-01733)	Apr-14
Power sensor E4412A	MY41498087	04-Apr-13 (No. 217-01733)	Apr-14
Reference 3 dB Attenuator	SN: S5054 (3c)	04-Apr-13 (No. 217-01737)	Apr-14
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-13 (No. 217-01735)	Apr-14
Reference 30 dB Attenuator	SN: S5129 (30b)	04-Apr-13 (No. 217-01738)	Apr-14
Reference Probe ES3DV2	SN: 3013	30-Dec-13 (No. ES3-3013_Dec13)	Dec-14
DAE4	SN: 660	13-Dec-13 (No. DAE4-660_Dec13)	Dec-14
	ID.	Check Date (in house)	Scheduled Check
Secondary Standards	ID	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
RF generator HP 8648C  Network Analyzer HP 8753E	US3642U01700 US37390585	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

Signature Function Name Laboratory Technicia Jeton Kastrati Calibrated by: **Technical Manager** Katja Pokovic Approved by:

Issued: April 18, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Page 1 of 11 Certificate No: ES3-3311\_Jan14/2

### **Calibration Laboratory of**

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid NORMx,y,z sensitivity in free space

ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty\_cycle) of the RF signal modulation dependent linearization parameters

Polarization  $\phi$   $\phi$  rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e.,  $\vartheta = 0$  is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

## Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

## Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization θ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is
  implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
  in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: ES3-3311\_Jan14/2 Page 2 of 11

January 28, 2014 ES3DV3 - SN:3311

# Probe ES3DV3

SN:3311

Manufactured: July 5, 2011

Calibrated:

January 28, 2014

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

January 28, 2014 ES3DV3-SN:3311

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3311

**Basic Calibration Parameters** 

Basic Cambration Farai	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^A$	1,27	1.07	0.47	± 10.1 %
DCP (mV) <sup>B</sup>	103.4	100.7	96.8	

**Modulation Calibration Parameters** 

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc⁻ (k=2)
0	CW		0.0	0.0	1.0	0.00	161.7	±3.3 %
	0,,	Y	0.0	0.0	1.0		190.3	
		-   z	0.0	0.0	1.0		160.4	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>&</sup>lt;sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ES3DV3- SN:3311 January 28, 2014

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3311

## Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
150	52.3	0.76	7.46	7.46	7.46	0.07	1.30	± 13.3 %
220	49.0	0.81	7.35	7.35	7.35	0.06	1.30	± 13.3 %
300	45.3	0.87	7.36	7.36	7.36	0.14	1.70	± 13.3 %
450	43.5	0.87	7.05	7.05	7.05	0.24	2.90	± 13.3 %
600	42.7	0.88	6.88	6.88	6.88	0.15	1.74	± 13.3 %
750	41.9	0.89	6.46	6.46	6.46	0.80	1.16	± 12.0 %
900	41.5	0.97	6.17	6.17	6.17	0.80	1.15	± 12.0 %
1640	40.3	1.29	5.36	5.36	5.36	0.80	1.14	± 12.0 %
1750	40.1	1.37_	5.25	5.25	5.25	0.80	1.17	± 12.0 %
1900	40.0	1.40	5.15	5.15	5.15	0.80	1.20	± 12.0 %
2450	39.2	1.80	4.61	4.61	4.61	0.68	1.42	± 12.0 %
2600	39.0	1.96	4.41	4.41	4.41	0.80	1.27	± 12.0 %

<sup>&</sup>lt;sup>c</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Certificate No: ES3-3311\_Jan14/2

F At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

the ConvF uncertainty for indicated target tissue parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

January 28, 2014 ES3DV3-SN:3311

# DASY/EASY - Parameters of Probe: ES3DV3 - SN:3311

## Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>C</sup>	Parameter De Relative Permittivity F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
150	61.9	0.80	7.27	7.27	7.27	0.08	1.30_	± 13.3 %
220	59.4	0.88	7.08	7.08	7.08	0.05	1.30	± 13.3 %
300	58.2	0.92	7.42	7.42	7.42	0.13	1.30	± 13.3 %
450	56.7	0.94	7.23	7.23	7.23	0.14	2.21	± 13.3 %
600	56.1	0.95	6.60	6.60	6.60	0.05	1.30	± 13.3 %
750	55.5	0.96	6.16	6.16	6.16	0.50	1.45	± 12.0 %
900	55.0	1.05	6.04	6.04	6.04	0.80	1.13	± 12.0 %
1640	53.8	1.40	5.21	5.21	5.21	0.50	1.53	± 12.0 %
1750	53.4	1.49	4.88	4.88	4.88	0.74	1.29	± 12.0 %
1900	53.3	1.52	4.68	4.68	4.68	0.72	1.34	± 12.0 %
2450	52.7	1.95	4.29	4.29	4.29	0.80	1.19	± 12.0 %
2600	52.5	2.16	4.08	4.08	4.08	0.80	1.04	± 12.0 %

<sup>&</sup>lt;sup>c</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>f</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to

Certificate No: ES3-3311\_Jan14/2


At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of

the ConvF uncertainty for indicated target tissue parameters.

Galpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

January 28, 2014 ES3DV3-SN:3311


# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

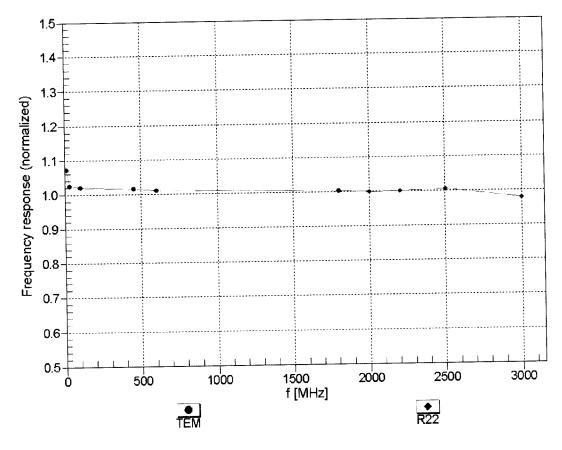


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

January 28, 2014

# Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

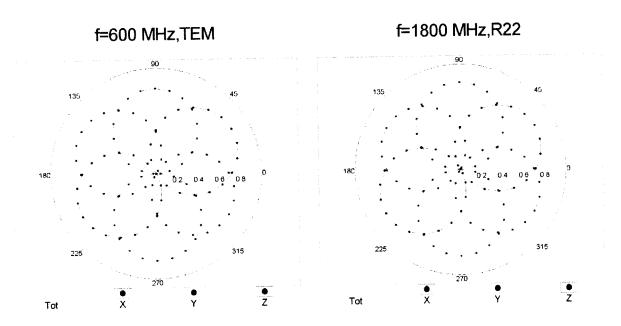


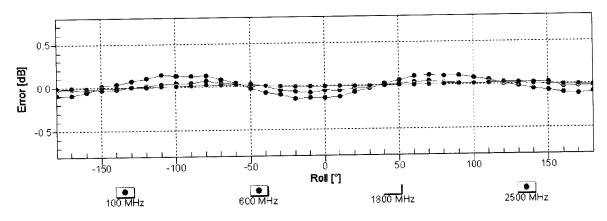


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

ES3DV3- SN:3311 January 28, 2014

## Dynamic Range f(SAR<sub>head</sub>) (TEM cell , f = 900 MHz)

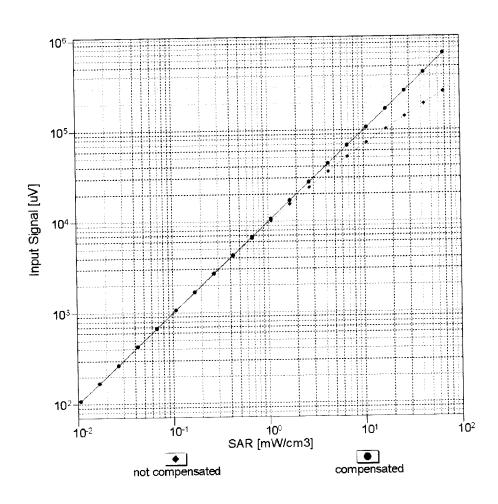


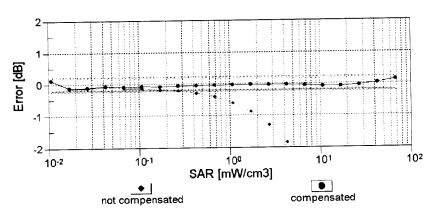


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

January 28, 2014

# **Conversion Factor Assessment**

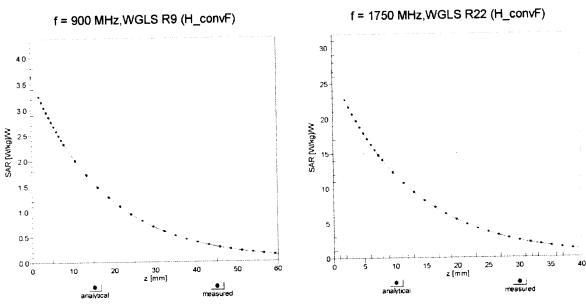

Deviation from Isotropy in Liquid Error (φ, θ), f = 900 MHz

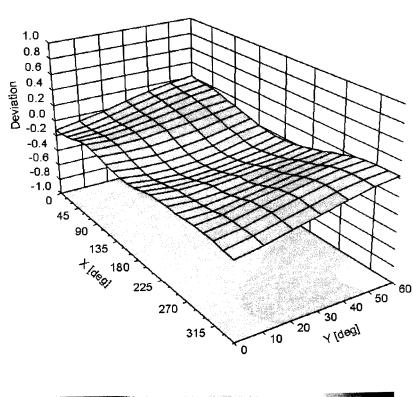

ES3DV3- SN:3311 January 28, 2014

# DASY/EASY - Parameters of Probe: ES3DV3 - SN:3311

#### **Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	-119.6
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm



#### Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

RF Exposure Lab

Certificate No: EX3-3693\_Aug14

Accreditation No.: SCS 108

# CALIBRATION CERTIFICATE

Object

EX3DV4 - SN:3693

Calibration procedure(s)

QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,

**QA CAL-25.v6** 

Calibration procedure for dosimetric E-field probes

Calibration date:

August 21, 2014

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

D. Otan danda	ID	Cal Date (Certificate No.)	Scheduled Calibration
Primary Standards	GB41293874	03-Apr-14 (No. 217-01911)	Apr-15
Power meter E4419B		03-Apr-14 (No. 217-01911)	Apr-15
Power sensor E4412A	MY41498087		Apr-15
Reference 3 dB Attenuator	SN: S5054 (3c)	03-Apr-14 (No. 217-01915)	<del></del>
Reference 20 dB Attenuator	SN: S5277 (20x)	03-Apr-14 (No. 217-01919)	Apr-15
Reference 30 dB Attenuator	SN: S5129 (30b)	03-Apr-14 (No. 217-01920)	Apr-15
Reference Probe ES3DV2	SN: 3013	30-Dec-13 (No. ES3-3013_Dec13)	Dec-14
DAE4	SN: 660	13-Dec-13 (No. DAE4-660_Dec13)	Dec-14
	I.D.	Check Date (in house)	Scheduled Check
Secondary Standards	ID	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
RF generator HP 8648C	US3642U01700		In house check: Oct-14
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-13)	III House Check. Oct 14

Name

Function

Signature

Calibrated by:

Jeton Kastrati

Laboratory Technician

Approved by:

Katja Pokovic

**Technical Manager** 

issued: August 21, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: EX3-3693\_Aug14 Page 1 of 11

#### **Calibration Laboratory of**

Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage C Servizio svizzero di taratura S **Swiss Calibration Service** 

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

tissue simulating liquid TSL sensitivity in free space NORMx,y,z sensitivity in TSL / NORMx,y,z ConvF

diode compression point **DCP** 

crest factor (1/duty\_cycle) of the RF signal CF modulation dependent linearization parameters A, B, C, D

φ rotation around probe axis Polarization φ

 $\vartheta$  rotation around an axis that is in the plane normal to probe axis (at measurement center), Polarization 9

i.e.,  $\vartheta = 0$  is normal to probe axis

information used in DASY system to align probe sensor X to the robot coordinate system Connector Angle

# Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

## Methods Applied and Interpretation of Parameters:

- NORMx, y, z: Assessed for E-field polarization 9 = 0 (f  $\leq 900$  MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E2-field uncertainty inside TSL (see below ConvF).
- $NORM(f)x,y,z = NORMx,y,z * frequency_response$  (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Page 2 of 11 Certificate No: EX3-3693\_Aug14

EX3DV4 - SN:3693

# Probe EX3DV4

SN:3693

Manufactured: Repaired:

Calibrated:

April 22, 2009

July 28, 2014

August 21, 2014

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3693

**Basic Calibration Parameters** 

<b>Basic Calibration Para</b>	meters		07	Unc (k=2)
	Sensor X	Sensor Y	Sensor Z	
2)A	0.40	0.33	0.36	± 10.1 %
Norm (μV/(V/m) <sup>2</sup> ) <sup>A</sup>	100.0	102.0	108.0	
DCP (mV) <sup>B</sup>	100.0			

**Modulation Calibration Parameters** 

Modula UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc <sup>⊨</sup> (k=2)
	CW	-	0.0	0.0	1.0	0.00	138.5	±3.3 %
	CW		0.0	0.0	1.0		143.3	
		Z	0.0	0.0	1.0		136.9	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A The uncertainties of NormX,Y,Z do not affect the E2-field uncertainty inside TSL (see Pages 5 and 6).

Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

August 21, 2014

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3693

# Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Parameter De Relative Permittivity F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
150	52.3	0.76	10.67	10.67	10.67	0.00	1.00	± 13.3 %
220	49.0	0.81	10.45	10.45	10.45	0.00	1.00	± 13.3 %
450	43.5	0.87	9.63	9.63	9.63	0.15	1.85	± 13.3 %
750	41.9	0.89	8.99	8.99	8.99	0.80	0.50	± 12.0 %
835	41.5	0.90	8.89	8.89	8.89	0.67	0.63	± 12.0 %
900	41.5	0.97	8.77	8.77	8.77	0.60	0.68	± 12.0 %
1750	40.1	1.37	7.63	7.63	7.63	0.76	0.55	± 12.0 %
1900	40.0	1.40	7.38	7.38	7.38	0.49	0.71	± 12.0 %
2450	39.2	1.80	6.91	6.91	6.91	0.58	0.68	± 12.0 %
2600	39.0	1.96	6.70	6.70	6.70	0.33	0.89	± 12.0 %
5200	36.0	4.66	5.00	5.00	5.00	0.35	1.80	± 13.1 %
5300	35.9	4.76	4.81	4.81	4.81	0.35	1.80	± 13.1 %
5500	35.6	4.96	4.87	4.87	4.87	0.35	1.80	± 13.1 %
5600	35.5	5.07	4.55	4.55	4.55	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.45	4.45	4.45	0.40	1.80	± 13.1 %

<sup>&</sup>lt;sup>c</sup> Frequency validity above 300 MHz of  $\pm$  100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to  $\pm$  50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is  $\pm$  10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to  $\pm$  110 MHz.

validity can be extended to  $\pm$  110 MHz.

Fat frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Certificate No: EX3-3693\_Aug14

the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

August 21, 2014

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3693

Calibration Parameter Determined in Body Tissue Simulating Media

	Parameter De Relative Permittivity F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
f (MHz) <sup>c</sup>	61.9	0.80	10.45	10.45	10.45	0.00	1.00	± 13.3 %
220	60.2	0.86	9.98	9.98	9.98	0.00	1.00	± 13.3 %
450	56.7	0.94	9.90	9.90	9.90	0.10	1.50	± 13.3 %
750	55.5	0.96	8.88	8.88	8.88	0.80	0.50	± 12.0 %
835	55.2	0.97	8.89	8.89	8.89	0.80_	0.50	± 12.0 %
900	55.0	1.05	8.70	8.70	8.70	0.80	0.62	± 12.0 %
1750	53.4	1.49	7.42	7.42	7.42	0.62	0.66	± 12.0 %
1900	53.3	1.52	7.15	7.15	7.15	0.55	0.71	± 12.0 %
2450	52.7	1.95	6.87	6.87	6.87	0.80	0.54	± 12.0 %
2600	52.5	2.16	6.74	6.74	6.74	0.80	0.50	± 12.0 %
5200	49.0	5.30	4.24	4.24	4.24	0.45	1.90	± 13.1 %
5300	48.9	5.42	4.06	4.06	4.06	0.45	1.90	± 13.1 %
5500	48.6	5.65	3.89	3.89	3.89	0.45	1.90	± 13.1 %
5600	48.5	5.77	3.65	3.65	3.65	0.50	1.90	± 13.1 %
5800	48.2	6.00	3.90	3.90	3.90	0.50	1.90	± 13.1 %

<sup>&</sup>lt;sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency

validity can be extended to  $\pm$  110 MHz. F At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.


Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is

Certificate No: EX3-3693\_Aug14

always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


August 21, 2014 EX3DV4-SN:3693


# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

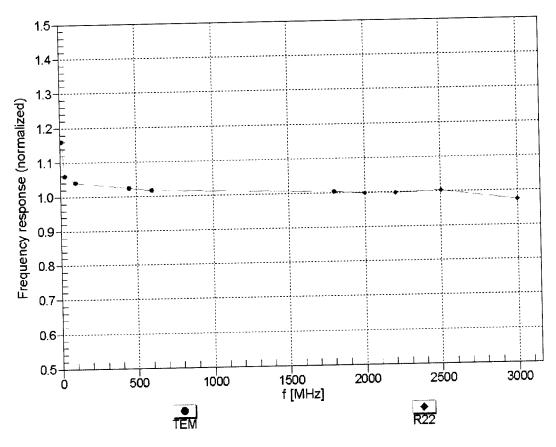

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


# Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

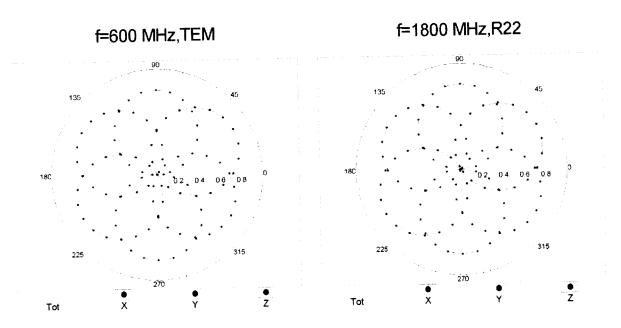


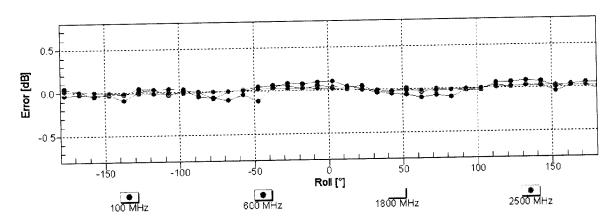

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

# Dynamic Range f(SAR<sub>head</sub>) (TEM cell , f<sub>eval</sub>= 1900 MHz)

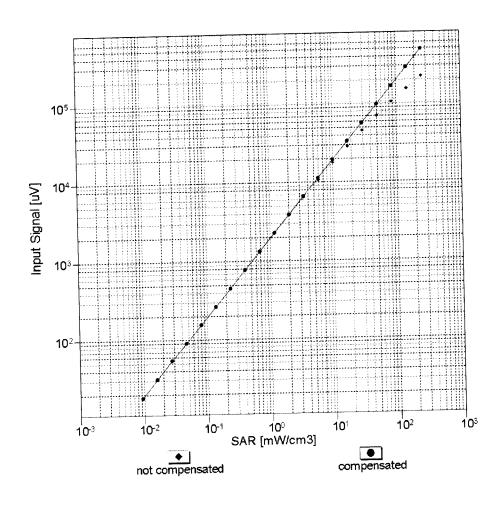


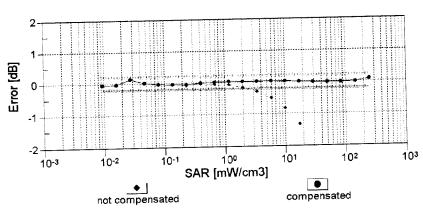


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

August 21, 2014

# **Conversion Factor Assessment**

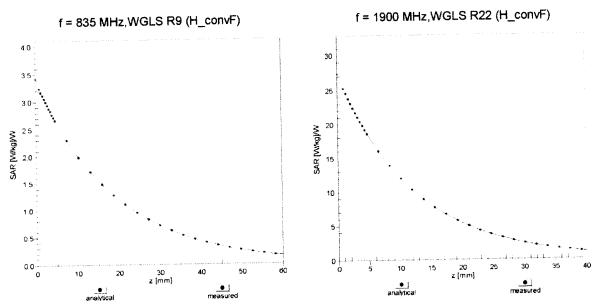

Deviation from Isotropy in Liquid Error (φ, θ), f = 900 MHz

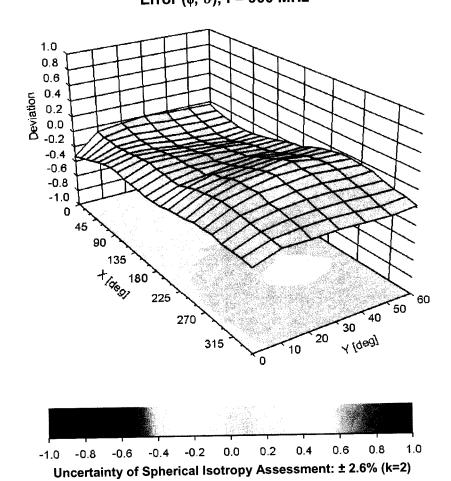

EX3DV4- SN:3693 August 21, 2014

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3693

#### **Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	-67.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

#### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

RF Exposure Lab

Certificate No: EX3-3833\_Jan15

#### **CALIBRATION CERTIFICATE**

Object

EX3DV4 - SN:3833

Calibration procedure(s)

QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,

**QA CAL-25.v6** 

Calibration procedure for dosimetric E-field probes

Calibration date:

January 23, 2015

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	Primary Standards ID		Scheduled Calibration
Power meter E4419B	GB41293874	03-Apr-14 (No. 217-01911)	Apr-15
Power sensor E4412A	MY41498087	03-Apr-14 (No. 217-01911)	Apr-15
Reference 3 dB Attenuator	SN: S5054 (3c)	03-Apr-14 (No. 217-01915)	Apr-15
Reference 20 dB Attenuator	SN: S5277 (20x)	03-Apr-14 (No. 217-01919)	Apr-15
Reference 30 dB Attenuator	SN: S5129 (30b)	03-Apr-14 (No. 217-01920)	Apr-15
Reference Probe ES3DV2	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
DAE4	SN: 660	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

Calibrated by:

Name

Function

Cluadio Leubler

Laboratory Technician

Signature

Approved by:

Katja Pokovic

Technical Manager

Issued: January 26, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX3-3833\_Jan15 Page 1 of 11

#### **Calibration Laboratory of**

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty\_cycle) of the RF signal modulation dependent linearization parameters

Polarization  $\varphi$   $\varphi$  rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e.,  $\vartheta = 0$  is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

#### Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization θ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: EX3-3833\_Jan15 Page 2 of 11

January 23, 2015 EX3DV4 - SN:3833

# Probe EX3DV4

SN:3833

Calibrated:

Manufactured: November 7, 2011 January 23, 2015

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

January 23, 2015 EX3DV4-SN:3833

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3833

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^A$	0.47	0.49	0.35	± 10.1 %
DCP (mV) <sup>B</sup>	101.8	100.3	103.5	

#### **Modulation Calibration Parameters**

UID	Communication System Name	Communication System Name A dB	B dB√μV	С	D dB	VR mV	Unc <sup>±</sup> (k=2)	
0	CW	X	0.0	0.0	1.0	0.00	131.5	±3.5 %
		Υ	0.0	0.0	1.0		133.2	
		Z	0.0	0.0	1.0		131.7	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A The uncertainties of NormX,Y,Z do not affect the E2-field uncertainty inside TSL (see Pages 5 and 6).

Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:3833 January 23, 2015

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3833

#### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
150	52.3	0.76	11.02	11.02	11.02	0.00	1.00	± 13.3 %
220	49.0	0.81	10.50	10.50	10.50	0.00	1.00	± 13.3 %
300	45.3	0.87	10.41	10.41	10.41	0.10	1.25	± 13.3 %
450	43.5	0.87	9.34	9.34	9.34	0.16	1.40	± 13.3 %
600	42.7	0.88	9.41	9.41	9.41	0.10	1.10	± 13.3 %
750	41.9	0.89	8.98	8.98	8.98	0.35	0.98	± 12.0 %
900	41.5	0.97	8.51	8.51	8.51	0.34	0.99	± 12.0 %
1640	40.3	1.29	7.50	7.50	7.50	0.23	1.08	± 12.0 %
1750	40.1	1.37	7.42	7.42	7.42	0.49	0.70	± 12.0 %
1900	40.0	1.40	7.29	7.29	7.29	0.57	0.62	± 12.0 %
2450	39.2	1.80	6.58	6.58	6.58	0.41	0.76	± 12.0 %
5200	36.0	4.66	4.62	4.62	4.62	0.35	1.80	± 13.1 %
5300	35.9	4.76	4.44	4.44	4.44	0.35	1.80	± 13.1 %
5500	35.6	4.96	4.18	4.18	4.18	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.03	4.03	4.03	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.12	4.12	4.12	0.40	1.80	± 13.1 %

<sup>&</sup>lt;sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

F At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is

<sup>&</sup>lt;sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3833 January 23, 2015

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3833

#### Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
150	61.9	0.80	11.21	11.21	11.21	0.00	1.00	± 13.3 %
220	60.2	0.86	10.20	10.20	10.20	0.00	1.00	± 13.3 %
300	58.2	0.92	10.29	10.29	10.29	0.06	1.15	± 13.3 %
450	56.7	0.94	10.02	10.02	10.02	0.08	1.12	± 13.3 %
600	56.1	0.95	9.37	9.37	9.37	0.10	1.10	± 13.3 %
750	55.5	0.96	8.75	8.75	8.75	0.24	1.32	± 12.0 %
900	55.0	1.05	8.51	8.51	8.51	0.41	0.88	± 12.0 %
1640	53.8	1.40	7.64	7.64	7.64	0.31	0.95	± 12.0 %
1750	53.4	1.49	7.18	7.18	7.18	0.34	0.93	± 12.0 %
1900	53.3	1.52	7.04	7.04	7.04	0.60	0.67	± 12.0 %
2450	52.7	1.95	6.69	6.69	6.69	0.80	0.57	± 12.0 %
5200	49.0	5.30	3.92	3.92	3.92	0.45	1.90	± 13.1 %
5300	48.9	5.42	3.81	3.81	3.81	0.45	1.90	± 13.1 %
5500	48.6	5.65	3.52	3.52	3.52	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.47	3.47	3.47	0.50	1.90	± 13.1 %
5800	48.2	6.00	3.57	3.57	3.57	0.50	1.90	± 13.1 %

Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


At frequencies below 3 GHz, the validity of tiesue parameters (a and =) can be releved to ± 100 MHz.

F At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the CopyE uncertainty for indicated target fissue parameters

the ConvF uncertainty for indicated target tissue parameters.

Galpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

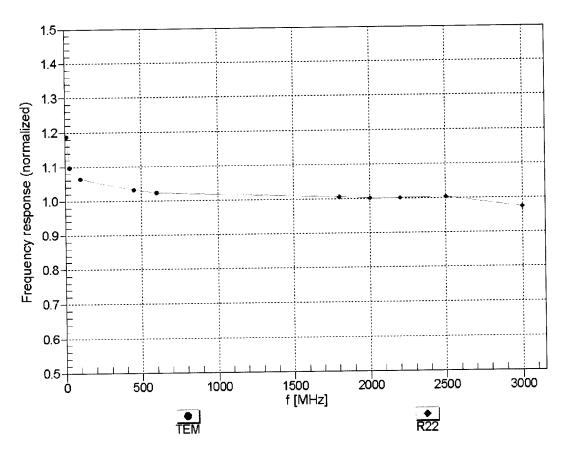



Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

# Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

f=600 MHz,TEM


f=1800 MHz,R22

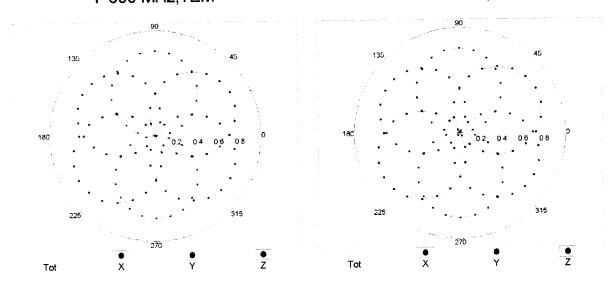


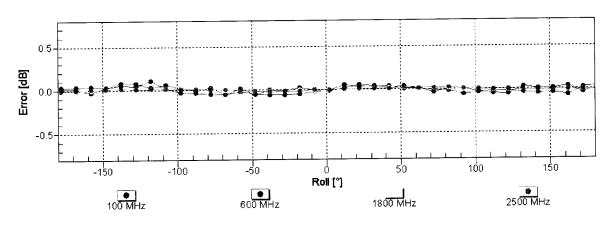

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

# Dynamic Range f(SAR<sub>head</sub>) (TEM cell , f<sub>eval</sub>= 1900 MHz)

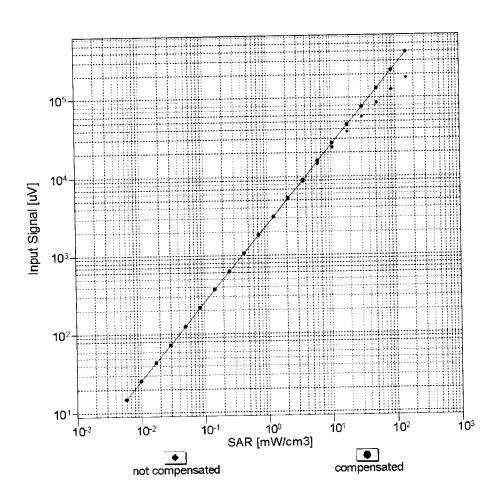


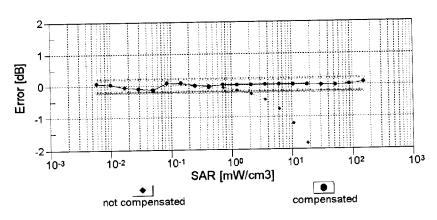


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

January 23, 2015

# **Conversion Factor Assessment**

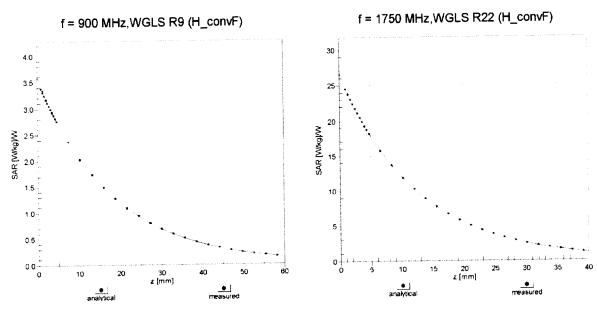

Deviation from Isotropy in Liquid Error (φ, θ), f = 900 MHz

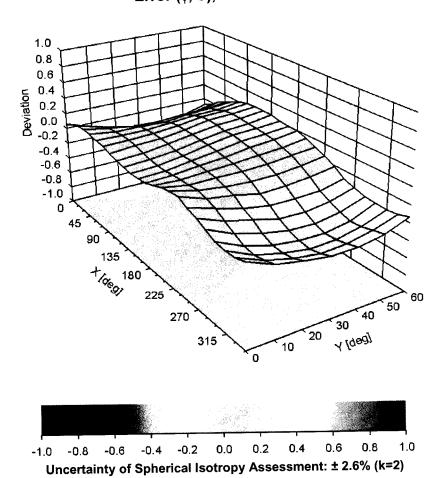

EX3DV4- SN:3833 January 23, 2015

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3833

#### **Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	12.2
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Page 11 of 11



Report Number: SAR.20140710

# **Appendix E – Dipole Calibration Data Sheets**

#### **Calibration Laboratory of**

Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage C Servizio svizzero di taratura S **Swiss Calibration Service** 

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

**RF Exposure Lab** Client

Certificate No: D835V2-4d089\_Dec12

Accreditation No.: SCS 108

#### CALIBRATION CERTIFICATE

Object D835V2 - SN: 4d089

Calibration procedure(s) QA CAL-05.v8

Calibration procedure for dipole validation kits above 700 MHz

December 03, 2012 Calibration date:

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	01-Nov-12 (No. 217-01640)	Oct-13
Power sensor HP 8481A	US37292783	01-Nov-12 (No. 217-01640)	Oct-13
Reference 20 dB Attenuator	SN: 5058 (20k)	27-Mar-12 (No. 217-01530)	Apr-13
Type-N mismatch combination	SN: 5047.3 / 06327	27-Mar-12 (No. 217-01533)	Apr-13
Reference Probe ES3DV3	SN: 3205	30-Dec-11 (No. ES3-3205_Dec11)	Dec-12
DAE4	SN: 601	27-Jun-12 (No. DAE4-601_Jun12)	Jun-13
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-12)	In house check: Oct-13
	Name	Function	Signature
Calibrated by:	Israe El-Naouq	Laboratory Technician	Israu Endanie
Approved by:	Katja Pokovic	Technical Manager	28 las

Issued: December 3, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D835V2-4d089\_Dec12

Page 1 of 8

#### **Calibration Laboratory of**

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossarv:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### **Additional Documentation:**

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.3
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, $dy$ , $dz = 5 mm$	
Frequency	835 MHz ± 1 MHz	***

#### **Head TSL parameters**

The following parameters and calculations were applied.

<u> </u>	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.92 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.38 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.36 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.55 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.12 W/kg ± 16.5 % (k=2)

#### **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.5 ± 6 %	0.99 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

## SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.42 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.51 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.59 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.27 W/kg ± 16.5 % (k=2)

Certificate No: D835V2-4d089\_Dec12 Page 3 of 8

#### **Appendix**

#### **Antenna Parameters with Head TSL**

Impedance, transformed to feed point	51.7 Ω - 2.5 jΩ
Return Loss	- 30.5 dB

#### **Antenna Parameters with Body TSL**

Impedance, transformed to feed point	47.4 Ω - 4.8 jΩ
Return Loss	- 25.0 dB

#### **General Antenna Parameters and Design**

and the second s	
Electrical Delay (one direction)	1.391 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	October 17, 2008

Certificate No: D835V2-4d089\_Dec12 Page 4 of 8

#### **DASY5 Validation Report for Head TSL**

Date: 03.12.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d089

Communication System: CW; Frequency: 835 MHz

Medium parameters used: f = 835 MHz;  $\sigma = 0.92$  mho/m;  $\varepsilon_r = 41.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

• Probe: ES3DV3 - SN3205; ConvF(6.07, 6.07, 6.07); Calibrated: 30.12.2011;

• Sensor-Surface: 3mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn601; Calibrated: 27.06.2012

• Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

• DASY52 52.8.3(988); SEMCAD X 14.6.7(6848)

## Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 56.782 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.58 W/kg

SAR(1 g) = 2.38 W/kg; SAR(10 g) = 1.55 W/kg


Maximum value of SAR (measured) = 2.79 W/kg

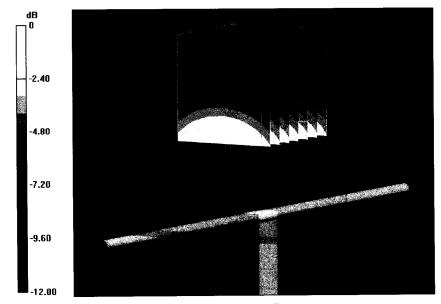

0 dB = 2.79 W/kg = 4.46 dBW/kg

Certificate No: D835V2-4d089\_Dec12 Page 5 of 8

## Impedance Measurement Plot for Head TSL

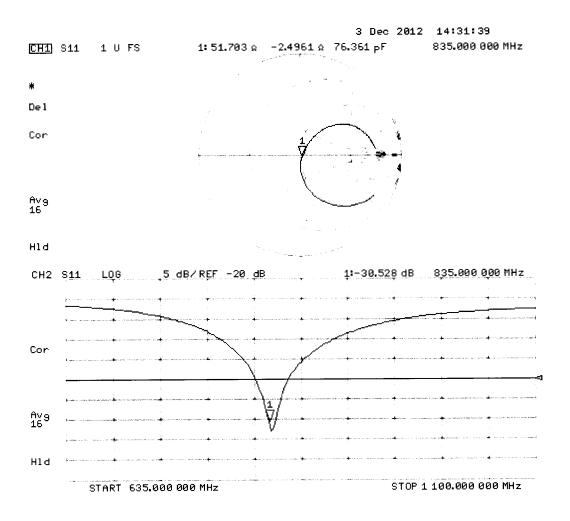

#### **DASY5 Validation Report for Body TSL**

Date: 03.12.2012

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d089** 

Communication System: CW; Frequency: 835 MHz

Medium parameters used: f = 835 MHz;  $\sigma = 0.99$  mho/m;  $\varepsilon_r = 54.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

• Probe: ES3DV3 - SN3205; ConvF(6.02, 6.02, 6.02); Calibrated: 30.12.2011;

• Sensor-Surface: 3mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn601; Calibrated: 27.06.2012

Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

• DASY52 52.8.3(988); SEMCAD X 14.6.7(6848)

## Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 55.384 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.54 W/kg

SAR(1 g) = 2.42 W/kg; SAR(10 g) = 1.59 W/kg


Maximum value of SAR (measured) = 2.82 W/kg

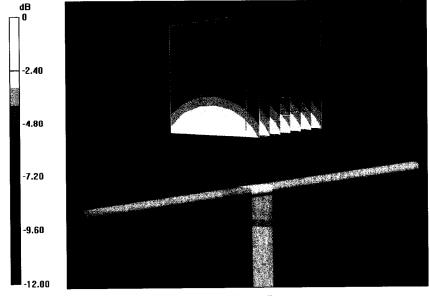

0 dB = 2.82 W/kg = 4.50 dBW/kg

Certificate No: D835V2-4d089\_Dec12 Page 7 of 8

#### **Impedance Measurement Plot for Body TSL**

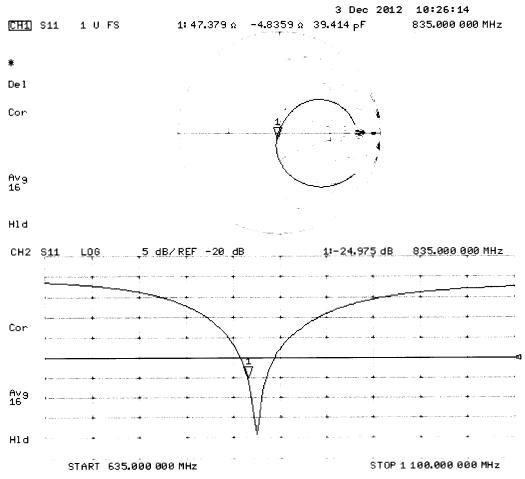

#### **Extended Calibration**

Usage of SAR dipoles calibrated less than 2 years ago but more than 1 year ago were confirmed in maintaining return loss (< -20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r03.

D835V2 SN: 4d089 - Head						
Date of Measurement	Return Loss (dB)	Δ%	Impedance (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ
12/3/2012	-30.5		51.7		-2.5	
12/4/2013	-28.7	-5.9	52.4	0.7	-1.5	1.0
12/4/2014	-29.2	-4.3	50.7	-1.0	-1.2	1.3

D835V2 SN: 4d089 - Body						
Date of Measurement	Return Loss (dB)	Δ%	Impedance (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ
12/3/2012	-25.0		47.4		-4.8	
12/4/2013	-24.6	-1.6	48.2	0.8	-5.2	-0.4
12/4/2014	-26.7	6.8	46.3	-1.1	-3.7	1.1

## **Calibration Laboratory of**

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

**RF Exposure Lab** 

Accreditation No.: SCS 108

Certificate No: D900V2-1d044\_Dec12

# **CALIBRATION CERTIFICATE**

Object

D900V2 - SN: 1d044

Calibration procedure(s)

**QA CAL-05.v8** 

Calibration procedure for dipole validation kits above 700 MHz

Calibration date:

December 03, 2012

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	01-Nov-12 (No. 217-01640)	Oct-13
Power sensor HP 8481A	US37292783	01-Nov-12 (No. 217-01640)	Oct-13
Reference 20 dB Attenuator	SN: 5058 (20k)	27-Mar-12 (No. 217-01530)	Apr-13
Type-N mismatch combination	SN: 5047.3 / 06327	27-Mar-12 (No. 217-01533)	Apr-13
Reference Probe ES3DV3	SN: 3205	30-Dec-11 (No. ES3-3205_Dec11)	Dec-12
DAE4	SN: 601	27-Jun-12 (No. DAE4-601_Jun12)	Jun-13
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-12)	In house check: Oct-13
Network Analyzer HP 8753E	0007000000004200	,,	

Calibrated by:

Name Israe El-Naouq Function

Laboratory Technician

Approved by:

Katja Pokovic

Technical Manager

Man & Jacoure

Issued: December 3, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D900V2-1d044\_Dec12

Page 1 of 8

#### **Calibration Laboratory of**

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage

Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF

sensitivity in TSL / NORM x,y,z

N/A

not applicable or not measured

# Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### **Additional Documentation:**

d) DASY4/5 System Handbook

# Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

# **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.3
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, $dy$ , $dz = 5 mm$	
Frequency	900 MHz ± 1 MHz	

#### **Head TSL parameters**

The following parameters and calculations were applied.

ne following parameters and calculations were appli	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.2 ± 6 %	0.94 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.62 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	10.7 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.69 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.88 W/kg ± 16.5 % (k=2)

#### **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.0	1.05 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.3 ± 6 %	1.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

## SAR result with Body TSL

Condition	
250 mW input power	2.66 W/kg
normalized to 1W	10.8 W/kg ± 17.0 % (k=2)
	250 mW input power

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.72 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.99 W/kg ± 16.5 % (k=2)

Certificate No: D900V2-1d044\_Dec12 Page 3 of 8

### **Appendix**

#### **Antenna Parameters with Head TSL**

Impedance, transformed to feed point	50.9 Ω - 4.3 jΩ
Return Loss	- 27.2 dB

### **Antenna Parameters with Body TSL**

Impedance, transformed to feed point	46.6 Ω - 6.8 jΩ
Return Loss	- 22.1 dB

### **General Antenna Parameters and Design**

1.411 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	September 26, 2006

Certificate No: D900V2-1d044\_Dec12

### **DASY5 Validation Report for Head TSL**

Date: 03.12.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN: 1d044

Communication System: CW; Frequency: 900 MHz

Medium parameters used: f = 900 MHz;  $\sigma = 0.94$  mho/m;  $\varepsilon_r = 41.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

### DASY52 Configuration:

• Probe: ES3DV3 - SN3205; ConvF(5.97, 5.97, 5.97); Calibrated: 30.12.2011;

• Sensor-Surface: 3mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn601; Calibrated: 27.06.2012

Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

• DASY52 52.8.3(988); SEMCAD X 14.6.7(6848)

## Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 56.736 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.93 W/kg

SAR(1 g) = 2.62 W/kg; SAR(10 g) = 1.69 W/kg


Maximum value of SAR (measured) = 3.07 W/kg

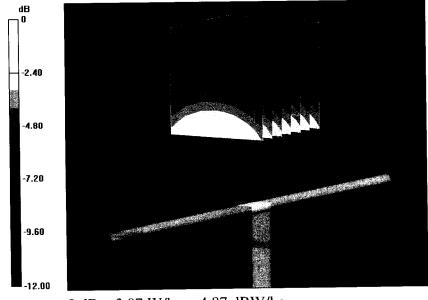

0 dB = 3.07 W/kg = 4.87 dBW/kg

Certificate No: D900V2-1d044\_Dec12 Page 5 of 8

### Impedance Measurement Plot for Head TSL

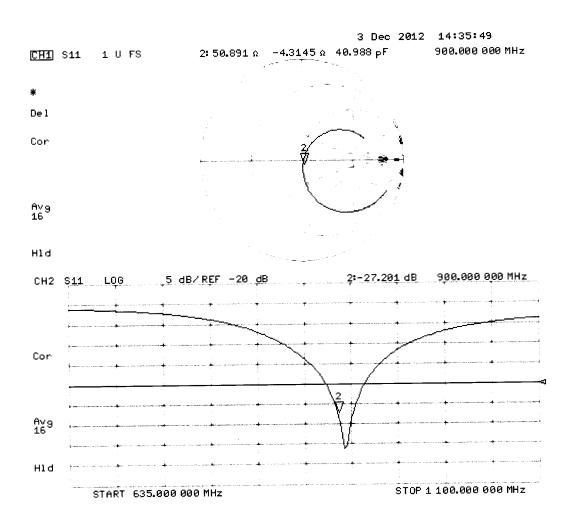

### **DASY5 Validation Report for Body TSL**

Date: 03.12.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN: 1d044

Communication System: CW; Frequency: 900 MHz

Medium parameters used: f = 900 MHz;  $\sigma = 1.02 \text{ mho/m}$ ;  $\varepsilon_r = 54.3$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

• Probe: ES3DV3 - SN3205; ConvF(5.94, 5.94, 5.94); Calibrated: 30.12.2011;

• Sensor-Surface: 3mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn601; Calibrated: 27.06.2012

Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

• DASY52 52.8.3(988); SEMCAD X 14.6.7(6848)

## Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 56.736 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 4.03 W/kg


SAR(1 g) = 2.66 W/kg; SAR(10 g) = 1.72 W/kg

Maximum value of SAR (measured) = 3.11 W/kg

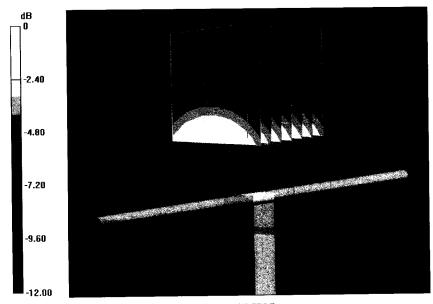

0 dB = 3.11 W/kg = 4.93 dBW/kg

#### **Impedance Measurement Plot for Body TSL**

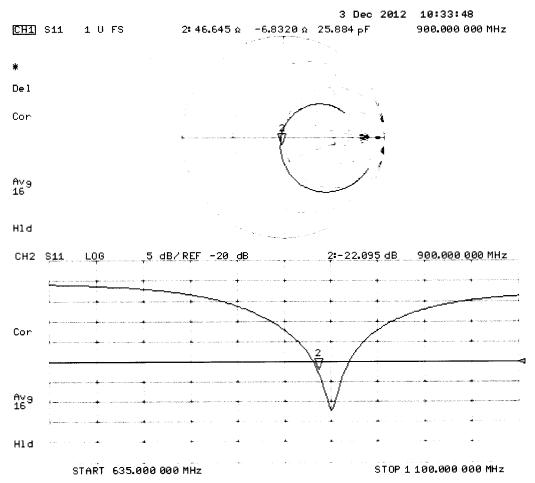

#### **Extended Calibration**

Usage of SAR dipoles calibrated less than 2 years ago but more than 1 year ago were confirmed in maintaining return loss (< -20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r03.

D900V2 SN: 1d044 - Head						
Date of Measurement	Return Loss (dB)	Δ%	Impedance Real (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ
12/3/2012	-27.2		50.9		4.3	
12/4/2013	-26.5	-2.6	51.6	-0.7	3.5	0.8
12/4/2014	-28.6	5.1	51.3	0.4	3.9	-0.4

D900V2 SN: 1d044 - Body						
Date of Measurement	Return Loss (dB)	Δ%	Impedance Real (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ
12/3/2012	-22.1		46.6		-6.8	
12/4/2013	-23.4	5.9	45.2	1.4	-5.9	-0.9
12/4/2014	-22.6	2.3	47.3	0.7	-6.4	0.4

## Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S

C

S

Accreditation No.: SCS 108

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura **Swiss Calibration Service** 

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

**RF Exposure Lab** Client

Certificate No: D1900V2-5d116\_Dec12

### CALIBRATION CERTIFICATE

D1900V2 - SN: 5d116 Object

QA CAL-05.v8 Calibration procedure(s)

Calibration procedure for dipole validation kits above 700 MHz

Calibration date:

December 06, 2012

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	01-Nov-12 (No. 217-01640)	Oct-13
Power sensor HP 8481A	US37292783	01-Nov-12 (No. 217-01640)	Oct-13
Reference 20 dB Attenuator	SN: 5058 (20k)	27-Mar-12 (No. 217-01530)	Apr-13
Type-N mismatch combination	SN: 5047.3 / 06327	27-Mar-12 (No. 217-01533)	Apr-13
Reference Probe ES3DV3	SN: 3205	30-Dec-11 (No. ES3-3205_Dec11)	Dec-12
	SN: 601	27-Jun-12 (No. DAE4-601_Jun12)	Jun-13
DAE4	314. 001	27 Odi: 12 (110: 5712 1 00: _0)	
	ID #	Check Date (in house)	Scheduled Check
Secondary Standards	1	•	Scheduled Check In house check: Oct-13
Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	ID#	Check Date (in house)	

Calibrated by:

Name Israe El-Naouq **Function** 

Laboratory Technician

Approved by:

Katja Pokovic

**Technical Manager** 

Issued: December 6, 2012

Moran El Dacong

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D1900V2-5d116\_Dec12

Page 1 of 8

### **Calibration Laboratory of**

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF

sensitivity in TSL / NORM x,y,z not applicable or not measured

N/A r

Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)",

February 2005

c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

### **Additional Documentation:**

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.3
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

### **Head TSL parameters**

The following parameters and calculations were applied.

The following parameters and calculations were app.	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.38 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.97 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.1 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.24 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.0 W/kg ± 16.5 % (k=2)

#### **Body TSL parameters**

The following parameters and calculations were applied.

Ų,	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.2 ± 6 %	1.52 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

## SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.1 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	40.2 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.31 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.2 W/kg ± 16.5 % (k=2)

Certificate No: D1900V2-5d116\_Dec12 Page 3 of 8

### **Appendix**

#### **Antenna Parameters with Head TSL**

Impedance, transformed to feed point	$51.4 \Omega + 6.6 j\Omega$
Return Loss	- 23.5 dB

### **Antenna Parameters with Body TSL**

Impedance, transformed to feed point	$47.4~\Omega + 6.7~j\Omega$
Return Loss	- 22.7 dB

### **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.202 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	August 21, 2009

Certificate No: D1900V2-5d116\_Dec12 Page 4 of 8

### **DASY5 Validation Report for Head TSL**

Date: 06.12.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d116

Communication System: CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz;  $\sigma = 1.38$  mho/m;  $\varepsilon_r = 39.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

### DASY52 Configuration:

• Probe: ES3DV3 - SN3205; ConvF(5.01, 5.01, 5.01); Calibrated: 30.12.2011;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 27.06.2012

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

DASY52 52.8.3(988); SEMCAD X 14.6.7(6848)

# Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 97.363 V/m; Power Drift = 0.07 dB

Peak SAR (extrapolated) = 17.9 W/kg


SAR(1 g) = 9.97 W/kg; SAR(10 g) = 5.24 W/kg

Maximum value of SAR (measured) = 12.3 W/kg

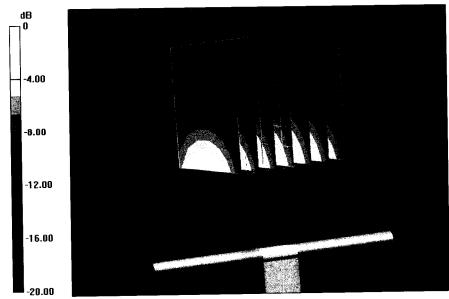

0 dB = 12.3 W/kg = 10.90 dBW/kg

## Impedance Measurement Plot for Head TSL

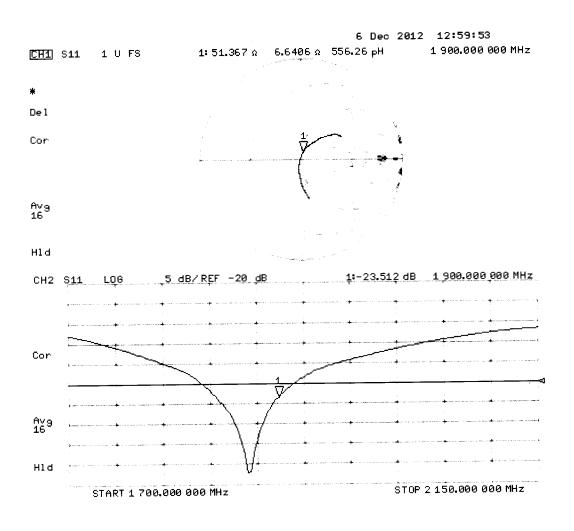

### **DASY5 Validation Report for Body TSL**

Date: 06.12.2012

Test Laboratory: SPEAG, Zurich, Switzerland

### DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d116

Communication System: CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz;  $\sigma = 1.52$  mho/m;  $\varepsilon_r = 52.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

### DASY52 Configuration:

• Probe: ES3DV3 - SN3205; ConvF(4.62, 4.62, 4.62); Calibrated: 30.12.2011;

• Sensor-Surface: 3mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn601; Calibrated: 27.06.2012

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

• DASY52 52.8.3(988); SEMCAD X 14.6.7(6848)

## Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.415 V/m; Power Drift = 0.07 dB

Peak SAR (extrapolated) = 17.7 W/kg

SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.31 W/kg


Maximum value of SAR (measured) = 12.7 W/kg

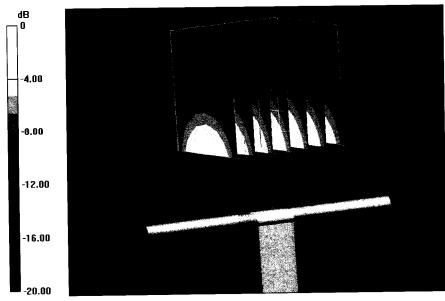

0 dB = 12.7 W/kg = 11.04 dBW/kg

Certificate No: D1900V2-5d116\_Dec12 Page 7 of 8

### Impedance Measurement Plot for Body TSL

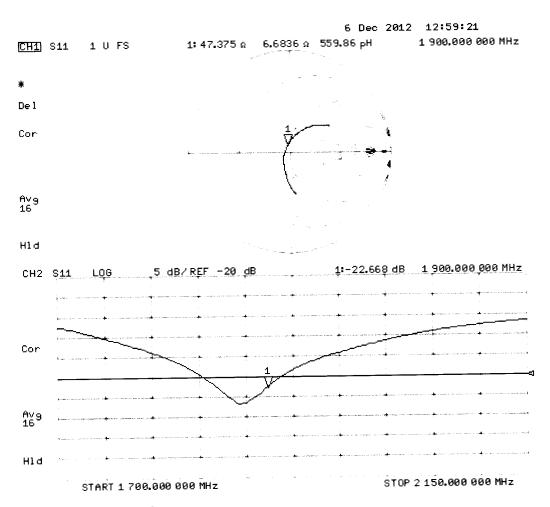

### **Extended Calibration**

Usage of SAR dipoles calibrated less than 2 years ago but more than 1 year ago were confirmed in maintaining return loss (< -20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r03.

D1900V2 SN: 5d116 - Head						
Date of Measurement	Return Loss (dB)	Δ%	Impedance (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ
12/6/2012	-23.5		51.4		6.6	
12/6/2013	-23.6	0.4	51.0	-0.4	6.1	-0.5
12/6/2014	-22.7	-3.4	50.5	-0.9	6.7	0.1

D1900V2 SN: 5d116 - Body						
Date of Measurement	Return Loss (dB)	Δ%	Impedance (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ
12/6/2012	-22.7		47.4		6.7	
12/6/2013	-21.9	-3.5	46.9	-0.5	5.8	-0.9
12/6/2014	-22.9	0.9	45.4	-2.0	6.1	-0.6

#### Calibration Laboratory of Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage C Servizio svizzero di taratura S **Swiss Calibration Service** 

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

**RF Exposure Lab** 

Accreditation No.: SCS 108

Certificate No: D2450V2-829\_Dec12

## CALIBRATION CERTIFICATE

Object

D2450V2 - SN: 829

Calibration procedure(s)

QA CAL-05.v8

Calibration procedure for dipole validation kits above 700 MHz

Calibration date:

December 04, 2012

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}$ C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

D. L Ohandarda	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Primary Standards	GB37480704	01-Nov-12 (No. 217-01640)	Oct-13
Power meter EPM-442A		01-Nov-12 (No. 217-01640)	Oct-13
Power sensor HP 8481A	US37292783	27-Mar-12 (No. 217-01530)	Apr-13
Reference 20 dB Attenuator	SN: 5058 (20k)		Apr-13
Type-N mismatch combination	SN: 5047.3 / 06327	27-Mar-12 (No. 217-01533)	Dec-12
Reference Probe ES3DV3	SN: 3205	30-Dec-11 (No. ES3-3205_Dec11)	Jun-13
DAE4	SN: 601	27-Jun-12 (No. DAE4-601_Jun12)	Juli-10
O L Obsession	ID#	Check Date (in house)	Scheduled Check
Secondary Standards	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
Power sensor HP 8481A	1	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	18-Oct-01 (in house check Oct-12)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-0ct-01 (III House cheek det 12)	
	Name	Function	Signature

Calibrated by:

Leif Klysner

Laboratory Technician

Approved by:

Katja Pokovic

**Technical Manager** 

Issued: December 4, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D2450V2-829\_Dec12

Page 1 of 8

### **Calibration Laboratory of**

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage

Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

# Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

### **Additional Documentation:**

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-829\_Dec12 Page 2 of 8

### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

ASY system configuration, as far as not DASY Version	DASY5	V52.8.3
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, $dy$ , $dz = 5 mm$	
Frequency	2450 MHz ± 1 MHz	

### **Head TSL parameters**

The following parameters and calculations were applied.

he following parameters and calculations were appli	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.2 ± 6 %	1.84 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.7 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	53.9 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.33 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	25.1 W/kg ± 16.5 % (k=2)

## **Body TSL parameters**

The following parameters and calculations were applied.

he following parameters and calculations were appli	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	50.7 ± 6 %	2.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.2 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	51.5 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.08 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	24.0 W/kg ± 16.5 % (k=2)
SAR for nominal Body 13L parameters		

Page 3 of 8 Certificate No: D2450V2-829\_Dec12

### **Appendix**

### **Antenna Parameters with Head TSL**

Impedance, transformed to feed point	53.1 $\Omega$ + 4.2 j $\Omega$
Return Loss	- 25.9 dB

### Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.7 Ω + 5.1 jΩ
Return Loss	- 25.9 dB

### **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.158 ns
Liectrical Delay (one direction)	

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### **Additional EUT Data**

Manufactured by	SPEAG
	December 11, 2008
Manufactured on	

Certificate No: D2450V2-829\_Dec12 Page 4 of 8

## **DASY5 Validation Report for Head TSL**

Date: 04.12.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 829

Communication System: CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz;  $\sigma = 1.84$  mho/m;  $\varepsilon_r = 38.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

### DASY52 Configuration:

• Probe: ES3DV3 - SN3205; ConvF(4.45, 4.45, 4.45); Calibrated: 30.12.2011;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 27.06.2012

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

• DASY52 52.8.3(988); SEMCAD X 14.6.7(6848)

# Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.1 V/m; Power Drift = 0.05 dB


Peak SAR (extrapolated) = 28.3 W/kg

SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.33 W/kg

Maximum value of SAR (measured) = 17.8 W/kg

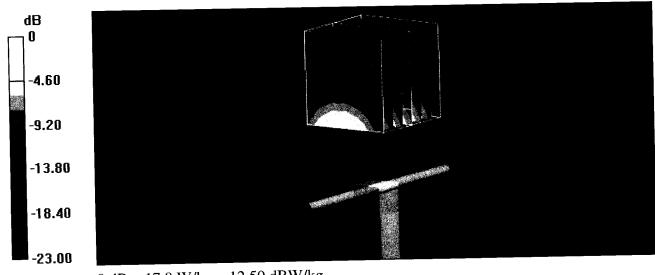

## Impedance Measurement Plot for Head TSL

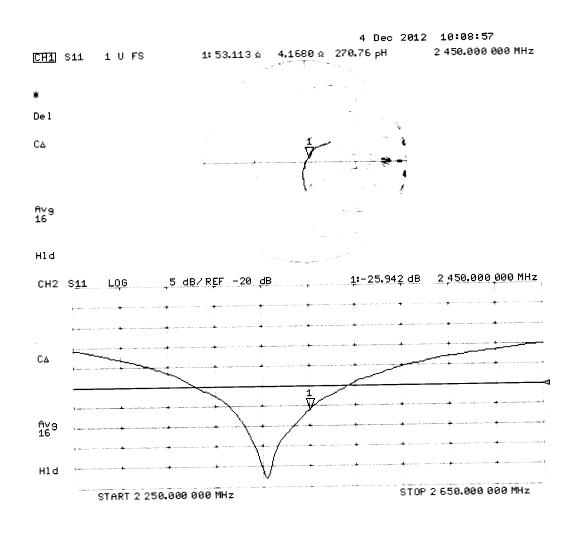

### **DASY5 Validation Report for Body TSL**

Date: 04.12.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 829

Communication System: CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz;  $\sigma = 2.02$  mho/m;  $\varepsilon_r = 50.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

### DASY52 Configuration:

• Probe: ES3DV3 - SN3205; ConvF(4.26, 4.26, 4.26); Calibrated: 30.12.2011;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 27.06.2012

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

• DASY52 52.8.3(988); SEMCAD X 14.6.7(6848)

# Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.1 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 27.4 W/kg


SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.08 W/kg

Maximum value of SAR (measured) = 17.5 W/kg

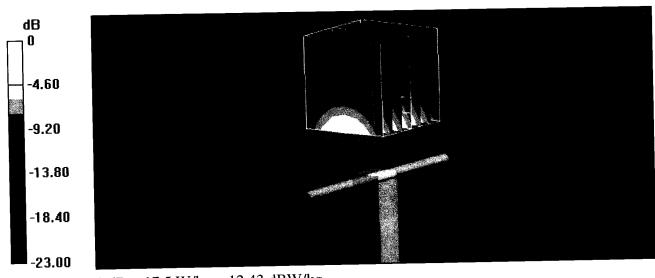

0 dB = 17.5 W/kg = 12.43 dBW/kg

### Impedance Measurement Plot for Body TSL

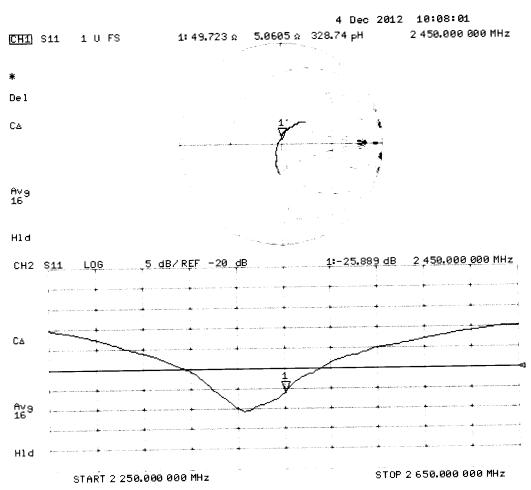

### **Extended Calibration**

Usage of SAR dipoles calibrated less than 2 years ago but more than 1 year ago were confirmed in maintaining return loss (< -20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r03.

D2450V2 SN: 829 - Head						
Date of Measurement	Return Loss (dB)	Δ%	Impedance (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ
12/4/2012	-25.9		53.1		4.2	
12/5/2013	-26.5	2.3	52.6	-0.5	3.8	-0.4
12/5/2014	-24.6	-5.0	51.6	-1.5	4.9	0.7

D2450V2 SN: 829 - Body						
Date of Measurement	Return Loss (dB)	Δ%	Impedance (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ
12/4/2012	-25.9		49.7		5.1	
12/5/2013	-26.2	1.2	48.5	-1.2	4.6	-0.5
12/4/2014	-24.6	-5.0	47.6	-2.1	5.9	0.8



Report Number: SAR.20140710

## **Appendix F – Phantom Calibration Data Sheets**

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 info@speag.com, http://www.speag.com

#### Certificate of Conformity / First Article Inspection

Item	Oval Flat Phantom ELI 4.0
Type No	QD OVA 001 B
Series No	1003 and higher
Manufacturer	Untersee Composites
	Knebelstrasse 8
	CH-8268 Mannenbach, Switzerland

#### Tests

Complete tests were made on the prototype units QD OVA 001 AA 1001, QD OVA 001 AB 1002, pre-series units QD OVA 001 BA 1003-1005 as well as on the series units QD OVA 001 BB, 1006 ff.

Test	Requirement	Details	Units tested
Material	Compliant with the standard	Bottom plate:	all
thickness	requirements	2.0mm +/- 0.2mm	
Material	Dielectric parameters for required	< 6 GHz: Rel. permittivity = 4	Material
parameters	frequencies	+/-1, Loss tangent ≤ 0.05	sample
Material	The material has been tested to be	DGBE based simulating	Equivalent
resistivity	compatible with the liquids defined in	liquids.	phantoms,
	the standards if handled and cleaned	Observe Technical Note for	Material
	according to the instructions.	material compatibility.	sample
Shape	Thickness of bottom material,	Bottom elliptical 600 x 400 mm	Prototypes,
	Internal dimensions,	Depth 190 mm,	Sample
	Sagging	Shape is within tolerance for	testing
	compatible with standards from	filling height up to 155 mm,	
	minimum frequency	Eventual sagging is reduced or	
		eliminated by support via DUT	

#### **Standards**

- [1] CENELEC EN 50361-2001, « Basic standard for the measurement of the Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz – 3 GHz) », July 2001
- [2] IEEE 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques, December 2003
- [3] IEC 62209 1, "Specific Absorption Rate (SAR) in the frequency range of 300 MHz to 3 GHz Measurement Procedure, Part 1: Hand-held mobile wireless communication devices", February 2005
- [4] IEC 62209 2, Draft, "Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices Human models, Instrumentation and Procedures Part 2: Procedure to determine the Specific Absorption Rate (SAR) in the head and body for 30 MHz to 6 GHz Handheld and Body-Mounted Devices used in close proximity to the Body.", February 2005
- [5] OET Bulletin 65, Supplement C, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields", Edition January 2001

Based on the tests above, we certify that this item is in compliance with the standards [1] to [5] if operated according to the specific requirements and considering the thickness. The dimensions are fully compliant with [4] from 30 MHz to 6 GHz. For the other standards, the minimum lower frequency limit is limited due to the dimensional requirements ([1]: 450 MHz, [2]: 300 MHz, [3]: 800 MHz, [5]: 375 MHz) and possibly further by the dimensions of the DUT.

Date

28.4.2008

Signature / Stamp

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9709, Fax+41,44 245 9779 info@speag.com; http://www.speag.com