

Contents

10.APPENDIX	62
10.1 Photographs of Test Setup.....	62
10.2 Photographs of the EUT	65

10.APPENDIX

10.1 Photographs of Test Setup



Fig.1 Photograph of the SAR measurement System

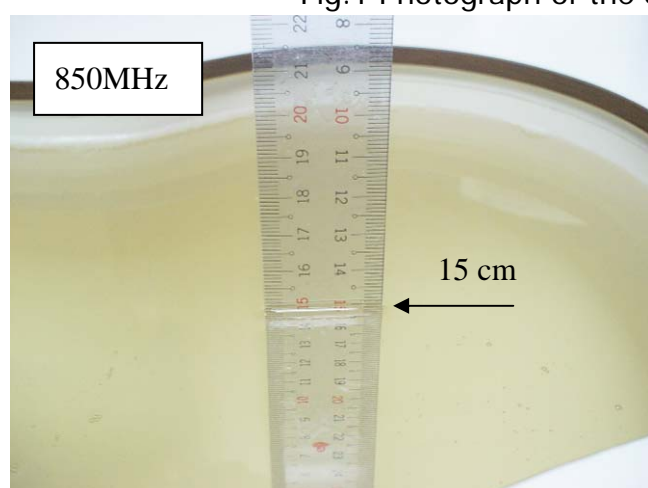


Fig.2.1 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Left-head Side

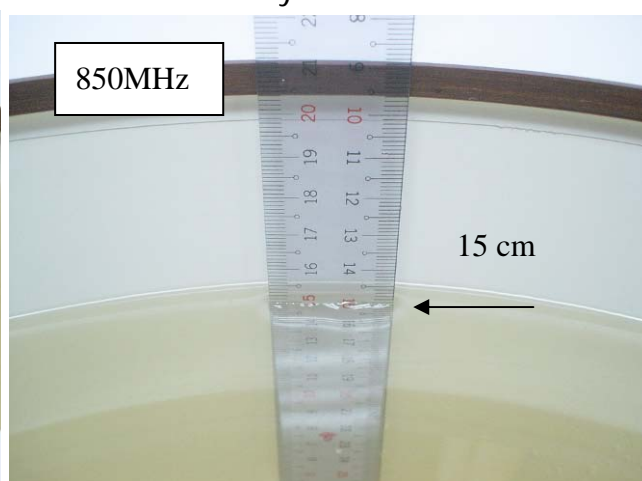


Fig.2.2 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

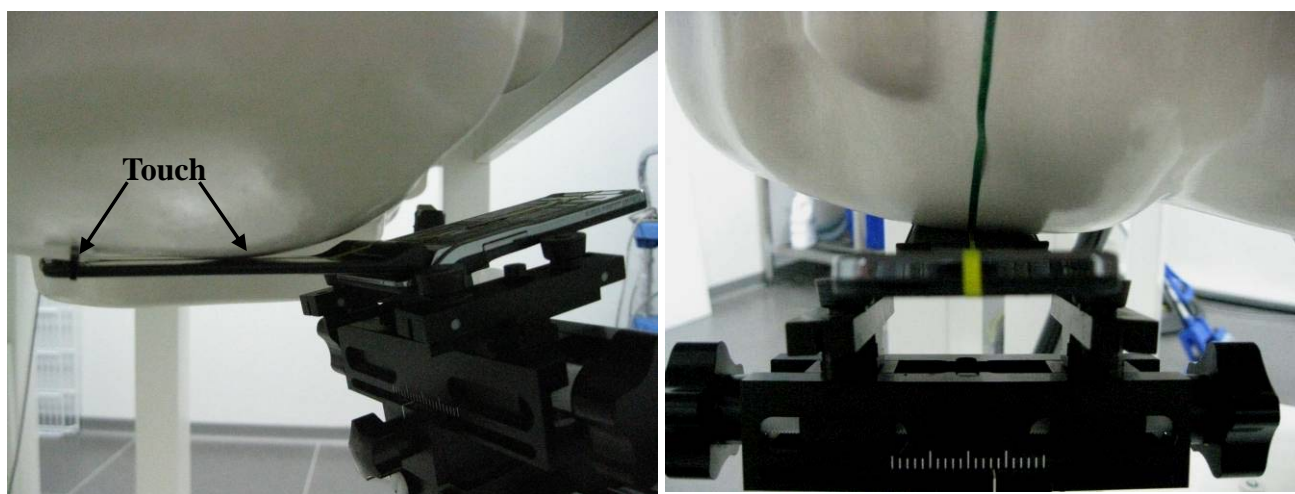


Fig.3 Right Head Section / Cheek-Touch Position

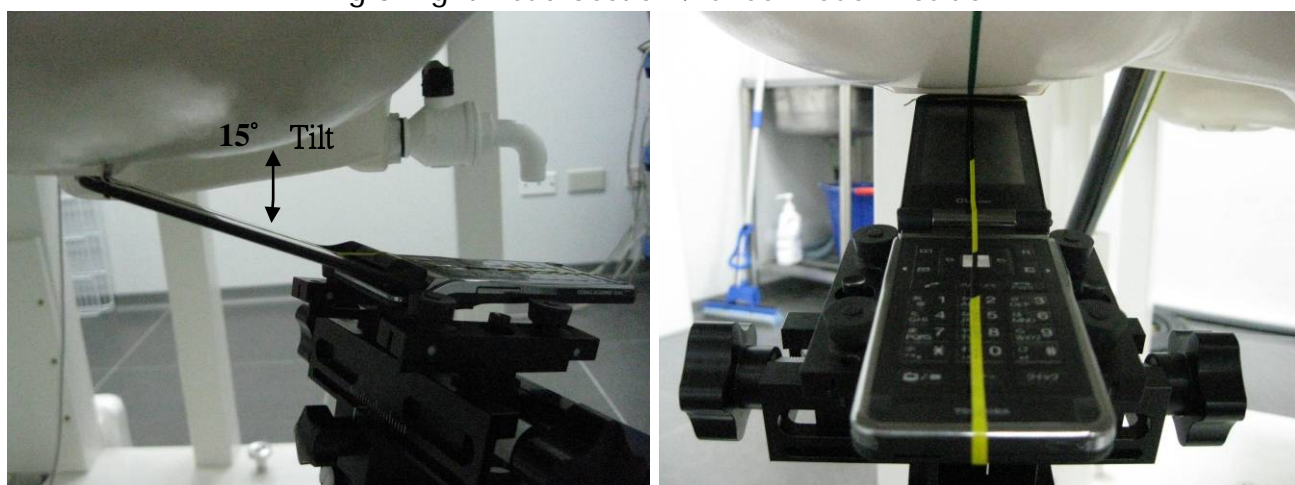


Fig.4 Right Head Section / Ear-Tilt Position(15°)

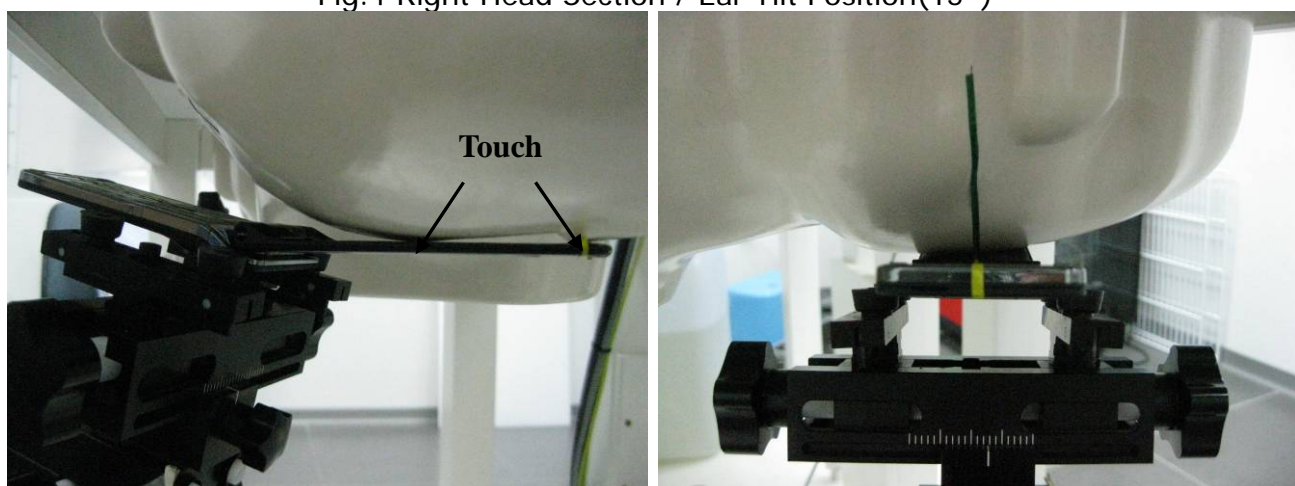


Fig.5 Left Head Section / Cheek-Touch Position

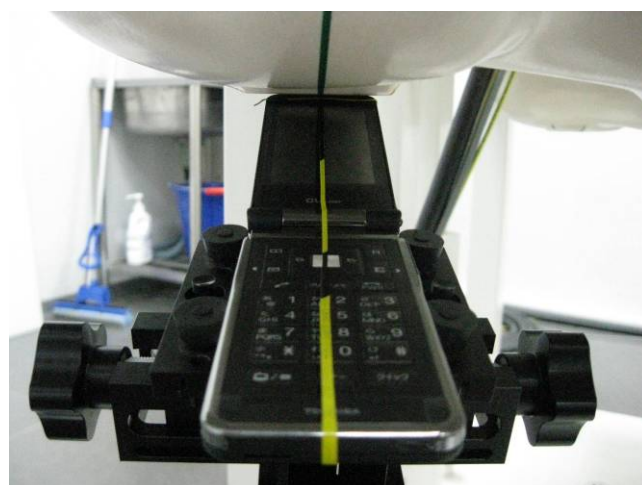
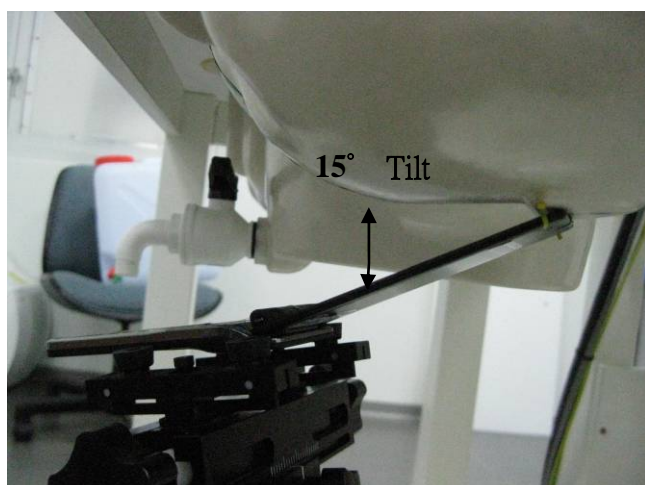


Fig.6 Left Head Section / Ear-Tilt Position(15°)

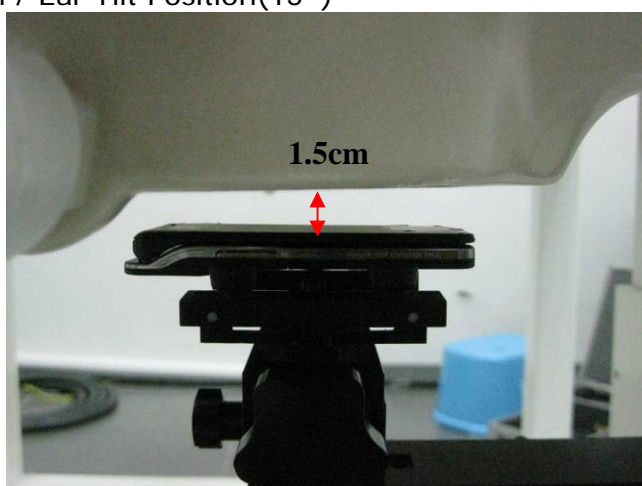
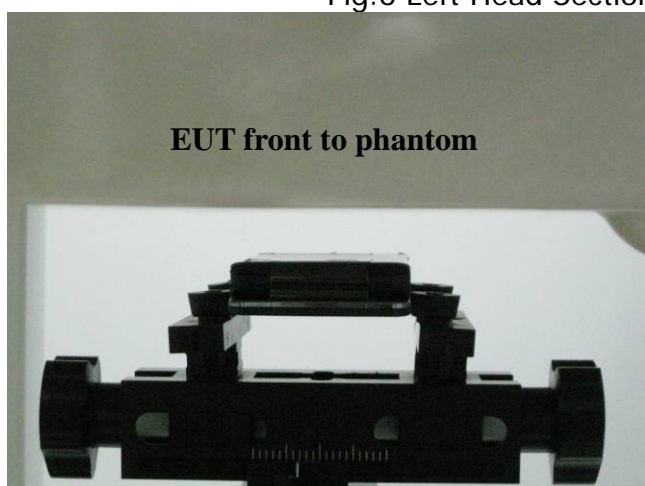


Fig.7 Body worn- EUT front to flat phantom and distance between flat phantom and mobile phone is 1.5 cm

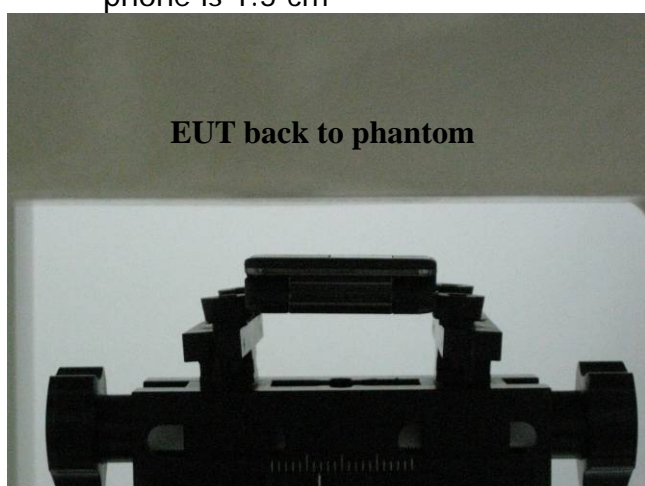


Fig.8 Body worn- EUT back to flat phantom and distance between flat phantom and mobile phone is 1.5 cm

10.2 Photographs of the EUT



Fig.9 Front view of device



Fig.10 Back view of device

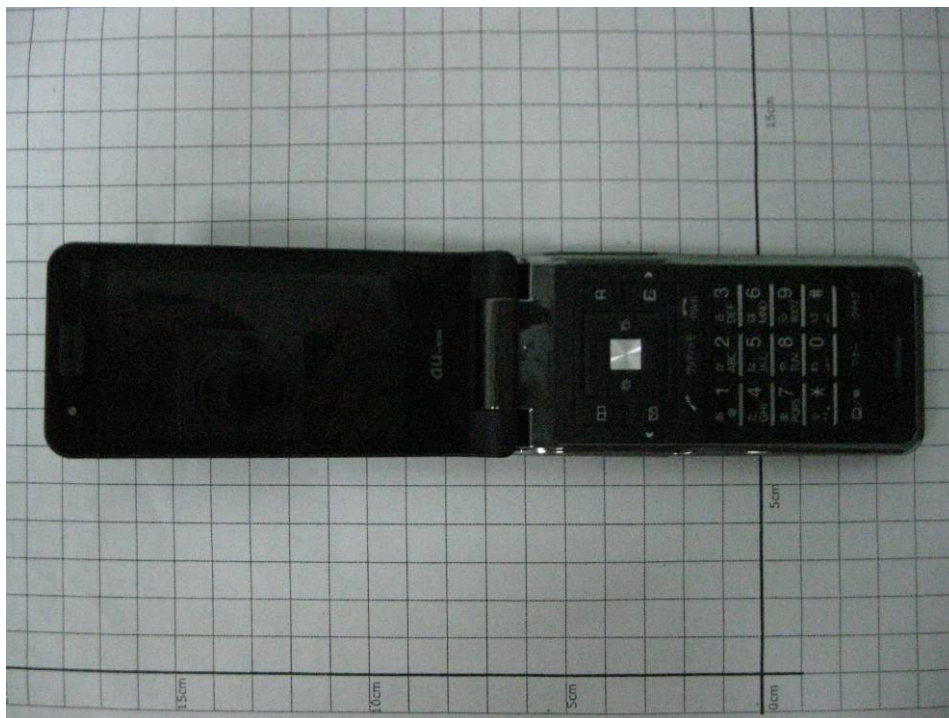


Fig.11 Open view of device



Fig.12 Right side view of device



Fig.13 Left side view of device



Fig.14 Front view of Battery



Fig.15 Back view of Battery

End of Report