

ISED CABid: ES1909
 Lab. Company Number: 4621A

Test Report No:
 74801RRF.004

Test Report

USA FCC Part 15.209

CANADA RSS-Gen, RSS-210

(*) Identification of item tested	RIE - Receiver In the Ear Hearing Aid
(*) Trademark	ReSound, Beltone
(*) Model and /or type reference	DURR1
Other identification of the product	FCC ID: X26DURR1 IC: 6941C-DURR1
(*) Features	BLE(1 & 2 MBit+Proximity), MI, Magnetic charging @135k, rechargeable battery HW version: C6.0DREHYB,V1.D,C6.0 SW version: Dooku3
Manufacturer	GN Hearing A/S Lautrupbjerg 7, 2750 Ballerup, Denmark
Test method requested, standard	USA FCC Part 15.209 (10-1-20 Edition): Radiated emission limits; general requirements. CANADA RSS-Gen Issue 5 Amendment 2 (Feb. 2021) General Requirements for Compliance of Radio Apparatus. CANADA RSS-210 Issue 10 Amendment 1 (April 2020). Licence-Exempt Radio Apparatus: Category I Equipment. ANSI C63.10-2013: American National Standard for Testing Unlicensed Wireless Devices.
Summary	IN COMPLIANCE
Approved by (name / position & signature)	José Manuel Gómez Galván EMC Consumer & RF Lab. Manager
Date of issue	2023-07-06
Report template No.	FDT08_24 (* "Data provided by the client")

Index

Competences and guarantees	3
General conditions	3
Uncertainty	3
Data provided by the client.....	3
Usage of samples	4
Test sample description	4
Identification of the client.....	5
Testing period and place.....	5
Document history	5
Environmental conditions	5
Remarks and comments	6
Testing verdicts.....	7
Summary	7
Appendix A: Test results	8
INDEX.....	9
TEST CONDITIONS.....	10
Occupied Bandwidth.....	12
General field strength and Transmitter emission limits	13

Competences and guarantees

DEKRA Testing and Certification is a testing laboratory accredited by the National Accreditation Body (ENAC - Entidad Nacional de Acreditación) to perform the tests indicated in the Certificate No. 51/LE 147.

DEKRA Testing and Certification is an FCC-recognized accredited testing laboratory with appropriate scope of accreditation that covers the performed tests in this report.

DEKRA Testing and Certification is an ISED-recognized accredited testing laboratory, CABid: ES1909, Company Number: 4621A, with the appropriate scope of accreditation that covers the performed tests in this report.

In order to assure the traceability to other national and international laboratories, DEKRA Testing and Certification has a calibration and maintenance program for its measurement equipment.

DEKRA Testing and Certification guarantees the reliability of the data presented in this report, which is the result of the measurements and the tests performed to the item under test on the date and under the conditions stated on the report and it is based on the knowledge and technical facilities available at DEKRA Testing and Certification at the time of performance of the test.

DEKRA Testing and Certification is liable to the client for the maintenance of the confidentiality of all information related to the item under test and the results of the test.

The results presented in this Test Report apply only to the particular item under test established in this document.

IMPORTANT: No parts of this report may be reproduced or quoted out of context, in any form or by any means, except in full, without the previous written permission of DEKRA Testing and Certification.

General conditions

1. This report is only referred to the item that has undergone the test.
2. This report does not constitute or imply on its own an approval of the product by the Certification Bodies or competent Authorities.
3. This document is only valid if complete; no partial reproduction can be made without previous written permission of DEKRA Testing and Certification S.A.U.
4. This test report cannot be used partially or in full for publicity and/or promotional purposes without previous written permission of DEKRA Testing and Certification S.A.U. and the Accreditation Bodies.

Uncertainty

Uncertainty (factor $k=2$) was calculated according to the DEKRA Testing and Certification S.A.U. internal document PODT000.

Data provided by the client

The following data has been provided by the client:

1. Information relating to the description of the sample ("Identification of the item tested", "Trademark", "Model and/or type reference tested").
2. The sample model DURR1 consists of a hearing aid that features a sound amplification of the sound received by the microphone.

DEKRA Testing and Certification S.A.U. declines any responsibility with respect to the information provided by the client and that may affect the validity of result.

Usage of samples

Samples undergoing test have been selected by: The client.

Id	Control Number	Description	Model	Serial No.	Date of Reception	Application
S/01	74801E_69.1	RIE - Receiver In the Ear Hearing Aid	DURR1	2300802980	2023-04-19	Equipment Under Test
S/02	74801E_58.1	RIE - Receiver In the Ear Hearing Aid	DURR1	2300803037	2023-04-19	Element Under Test

Notes referenced to samples during the project:

Id	Type
S/01	Sample used for Conducted tests.
S/02	Sample used for Radiated tests.

Test sample description

Ports..... :	Port name and description	Cable				
		Specified max length [m]	Attached during test	Shielded	Coupled to patient ⁽³⁾	
	-	-	-	-	-	
Supplementary information to the ports..... :	-					
Rated power supply	Voltage and Frequency		Reference poles			
			L1	L2	L3	N
	AC:					
	X	DC: 3.7 V rechargeable battery				
Rated Power	3.7V, 18.5mAh					
Clock frequencies..... :	CPU XTAL: 32MHz					
Other parameters	N/A					
Software version	Dooku3					
Hardware version	C6.0DREHYB,V1.D,C6.0					
Dimensions in cm (W x H x D)	up to 0.7 x 1.2 x 2.7					
Mounting position	Table top equipment					
	Wall/Ceiling mounted equipment					
	Floor standing equipment					
	Hand-held equipment					
	X	Other: Receiver in the ear, HA behind the ear				
Modules/parts..... :	Module/parts of test item		Type	Manufacturer		
	Dundee		DURR1	GN Hearing A/S		
	Description		Type	Manufacturer		

Accessories (not part of the test item)	Charger	C-1	GN Hearing A/S
	Charger	C-2	GN Hearing A/S
	Charger	C-3	GN Hearing A/S
	Power adapter, type: A806A-050100U-EU1	-	Aohai Technology
	Power adapter, type: A18A-50100U-US2	-	Aohai Technology
Documents as provided by the applicant.....	Description	File name	Issue date
	See ftp-server	-	-

⁽³⁾ Only for Medical Equipment

Identification of the client

GN HEARING A/S
 Lautrupbjerg 7, 2750 Ballerup, Denmark

Testing period and place

Test Location	DEKRA Testing and Certification S.A.U.
Date (start)	2022-05-03
Date (finish)	2022-05-30

Document history

Report number	Date	Description
74801RRF.004	2023-07-06	First release.

Environmental conditions

In the control chamber, the following limits were not exceeded during the test:

Temperature	Min. = 15 °C Max. = 35 °C
Relative humidity	Min. = 20 % Max. = 75 %

In the semi-anechoic chamber, the following limits were not exceeded during the test:

Temperature	Min. = 15 °C Max. = 35 °C
Relative humidity	Min. = 20 % Max. = 75 %

In the chamber for conducted measurements, the following limits were not exceeded during the test:

Temperature	Min. = 15 °C Max. = 35 °C
Relative humidity	Min. = 20 % Max. = 75 %

Remarks and comments

The tests have been performed by the technical personnel: Antonio Manuel Sánchez, Daniel Mejías.

Used instrumentation:

Conducted Measurements:

Equipment	Model	Manufacturer	Next Calibration
SHIELDED ROOM	-	SIEPEL	N/A
SIGNAL AND SPECTRUM ANALYZER 2Hz-50GHz	FSW50	ROHDE AND SCHWARZ	2023-07
DC Power Supply 30V/3A 90W	GPS-3030D	GW INSTEK	N/A
EMC/RF Testing SW	WMS32	ROHDE AND SCHWARZ	N/A

Radiated Measurements:

Equipment	Model	Manufacturer	Next Calibration
Semianechoic Absorber Lined Chamber	P29419	ALBATROSS PROJECTS GMBH	2026-01
Shielded Room	P29419	ALBATROSS PROJECTS GMBH	N/A
ACTIVE LOOP ANTENNA 9 kHz-30 MHz	FMZB 1519B	SCHWARZBECK	2025-12
EMI Test Receiver 7 GHz	ESR7	ROHDE AND SCHWARZ	2023-07
Hybrid Biconical/Log Antenna	JB6	SUNOL SCIENCES CORPORATION	2023-10
EMC/RF Testing SW	EMC32	ROHDE AND SCHWARZ	N/A

Testing verdicts

Not applicable:	N/A
Pass:	P
Fail:	F
Not measured:	N/M

Summary

1. SRD 10.66 MHz:

FCC PART 15.209 / RSS-Gen, RSS-210 PARAGRAPH		
Requirement – Test case	Verdict	Remark
Occupied bandwidth	P	
FCC 15.209 (a) / RSS-Gen 8.9, RSS-210 7.2 strength and emission limits	P	General field Transmitter
<u>Supplementary information and remarks:</u> None.		

Appendix A: Test results

INDEX

TEST CONDITIONS	10
Occupied Bandwidth	12
FCC 15.209 (a) / RSS-Gen 8.9, RSS-210 7.2 General field strength and Transmitter emission limits.	13

TEST CONDITIONS

(*) Declared by the Applicant

POWER SUPPLY (*):

Vnominal: 3.7 Vdc
Type of Power Supply: Rechargeable battery.

ANTENNA (*):

Maximum Declared Antenna Gain: N/A

TEST FREQUENCIES (*):

Nominal Operating Frequency: 10.66 MHz

Test setup

CONDUCTED MEASUREMENTS:

The equipment under test EUT was set up in a shielded room and connected to the spectrum analyzer through an RF cable.



RADIATED MEASUREMENTS:

All radiated tests were performed in a semi-anechoic chamber. The measurement antenna is situated at a distance of 3 m (Loop antenna for the range 9 kHz to 30 MHz and Bilog antenna for the range 30 MHz to 200 MHz).


For radiated emissions in the range 9 kHz to 30 MHz performed at a distance closer than the distance specified in the standard, an inverse proportionality factor of 40 dB per decade is used to normalize the measured data for determining compliance.

The equipment under test was set up on a non-conductive platform above the ground plane and its situation and orientation were varied to find the maximum radiated emission. It was also rotated 360°.


In the range between 9 kHz and 30 MHz the measurements were made in the three different orientation planes of the loop antenna to determine the maximum received field.

Measurements above 30 MHz up to 200 MHz were made in both horizontal and vertical planes of polarization and the measuring antenna height was varied from 1 to 4 meters to find the maximum radiated emission.

Radiated measurements setup $f < 30$ MHz:

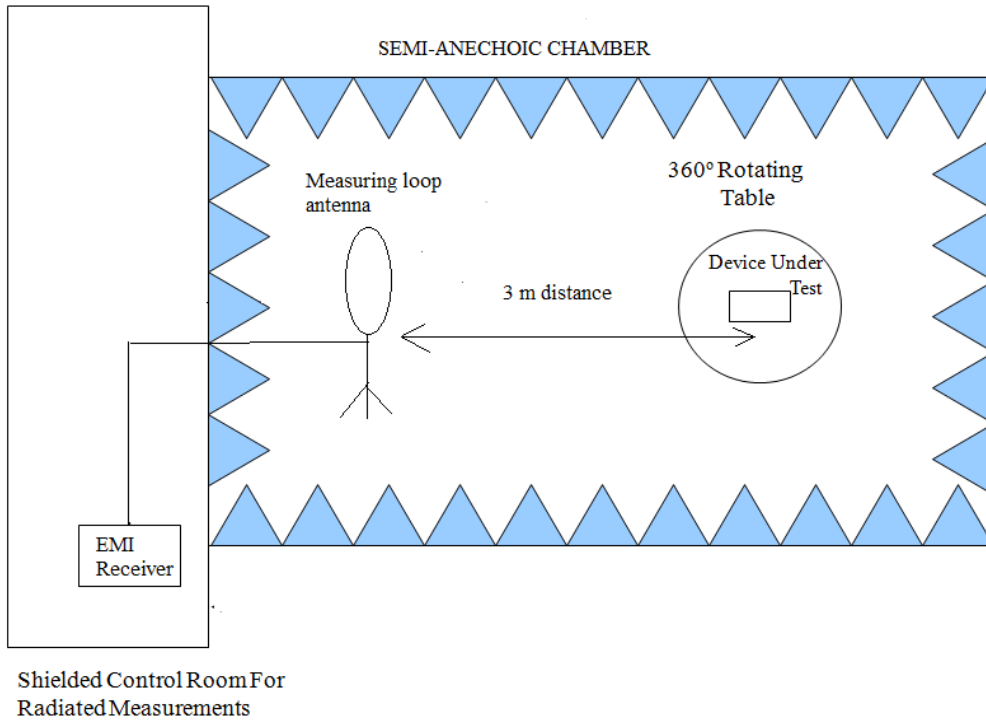

Radiated measurements setup $f > 30$ MHz up to 200 MHz:

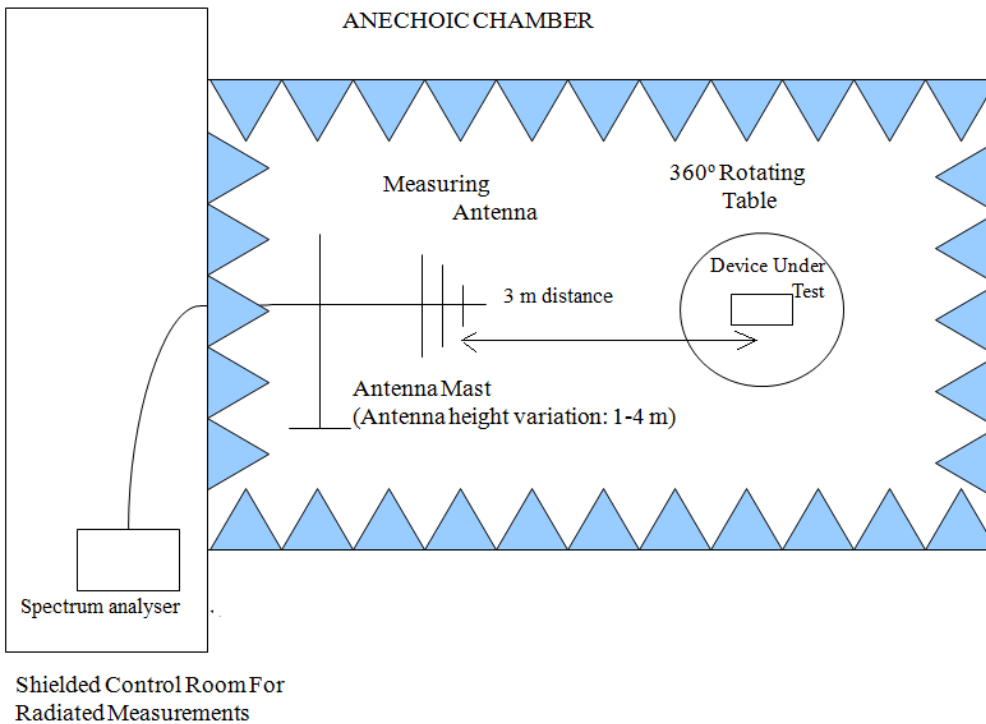


Occupied Bandwidth

Results

99% Bandwidth (MHz)	2.955151189
Measurement uncertainty (kHz)	< ±1.42

Attachments

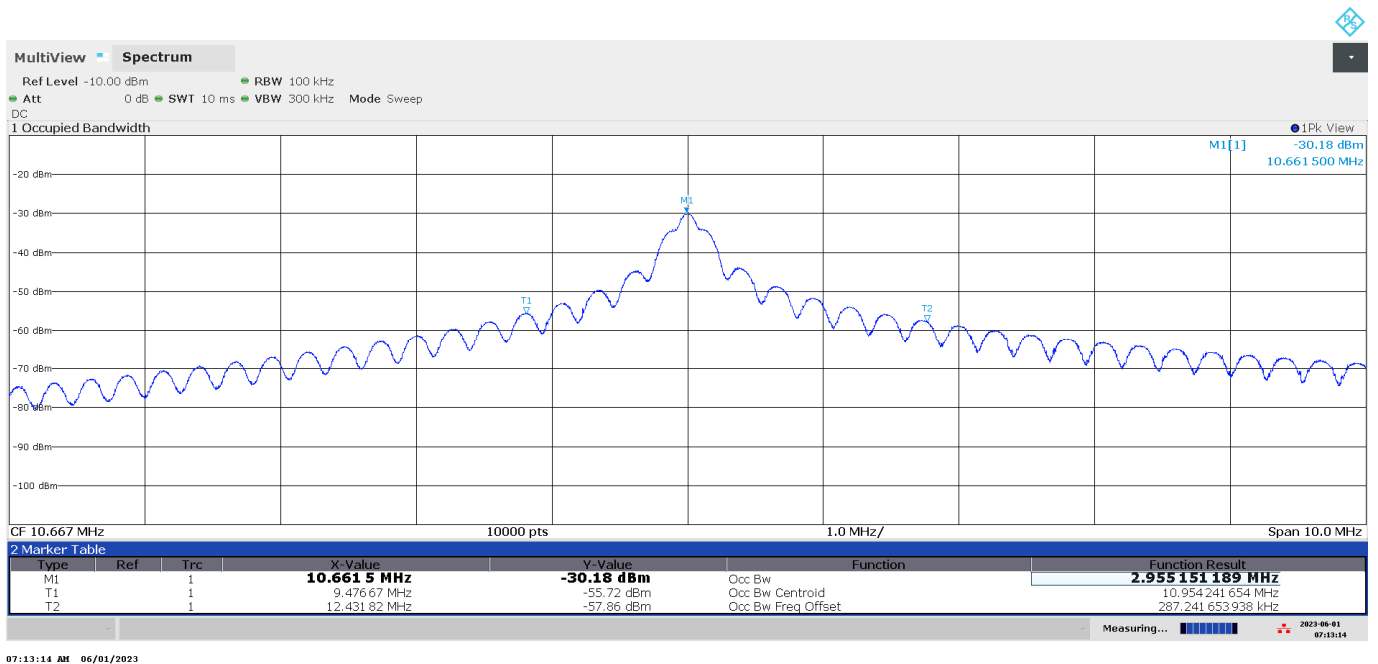

General field strength and Transmitter emission limits

Limits

The emissions from an intentional radiator shall not exceed the field strength levels specified in the following table (see §15.205(c) / RSS-Gen):

Frequency Range (MHz)	Field strength ($\mu\text{V/m}$)	Field strength ($\text{dB}\mu\text{V/m}$)	Magnetic field strength (H-Field) ($\mu\text{A/m}$)	Measurement distance (m)
0.009 - 0.490	2400/F(kHz)	-	6.37/ F(kHz)	300
0.490 - 1.705	24000/F(kHz)	-	63.7/ F(kHz)	30
1.705 - 30.0	30	29.54	0.08	30
30 - 88	100	40	-	3
88 - 216	150	43.5	-	3
216 - 960	200	46	-	3
Above 960	500	54	-	3

Additionally, the level of any transmitter unwanted emission shall not exceed the level of the transmitter's fundamental emission.

Results

All tests were performed in a semi-anechoic chamber at a distance of 3 m, except the measurement of the fundamental emission which was performed at a distance of 1 m due to its extremely low emission level. The maximum peak value of the fundamental emission was measured as the worst case.

The spectrum was inspected from 9 kHz to 200 MHz for spurious signals search.

The field strength is calculated by adding correction factor to the measured level from the spectrum analyser. This correction factor includes antenna factor and cable loss.

Fundamental emission:

E ($\text{dB}\mu\text{V/m}$) measured at 1 m (Peak value)	+43.65
E ($\text{dB}\mu\text{V/m}$) extrapolated to 30 m (40 dB/decade)	-15.43
Equivalent level ($\text{dB}\mu\text{A/m}$) at 30 m	-66.93
Measurement uncertainty (dB)	< ± 3.08

Verdict

Pass

Frequency range 9 kHz - 30 MHz:

No spurious frequencies detected at less than 20 dB below the limit.

Measurement uncertainty (dB) < ± 3.08

Frequency range 30 - 200 MHz:

No spurious frequencies detected at less than 20 dB below the limit.


Measurement uncertainty (dB) < ± 5.15

Verdict

Pass


Attachments

- FUNDAMENTAL EMISSION

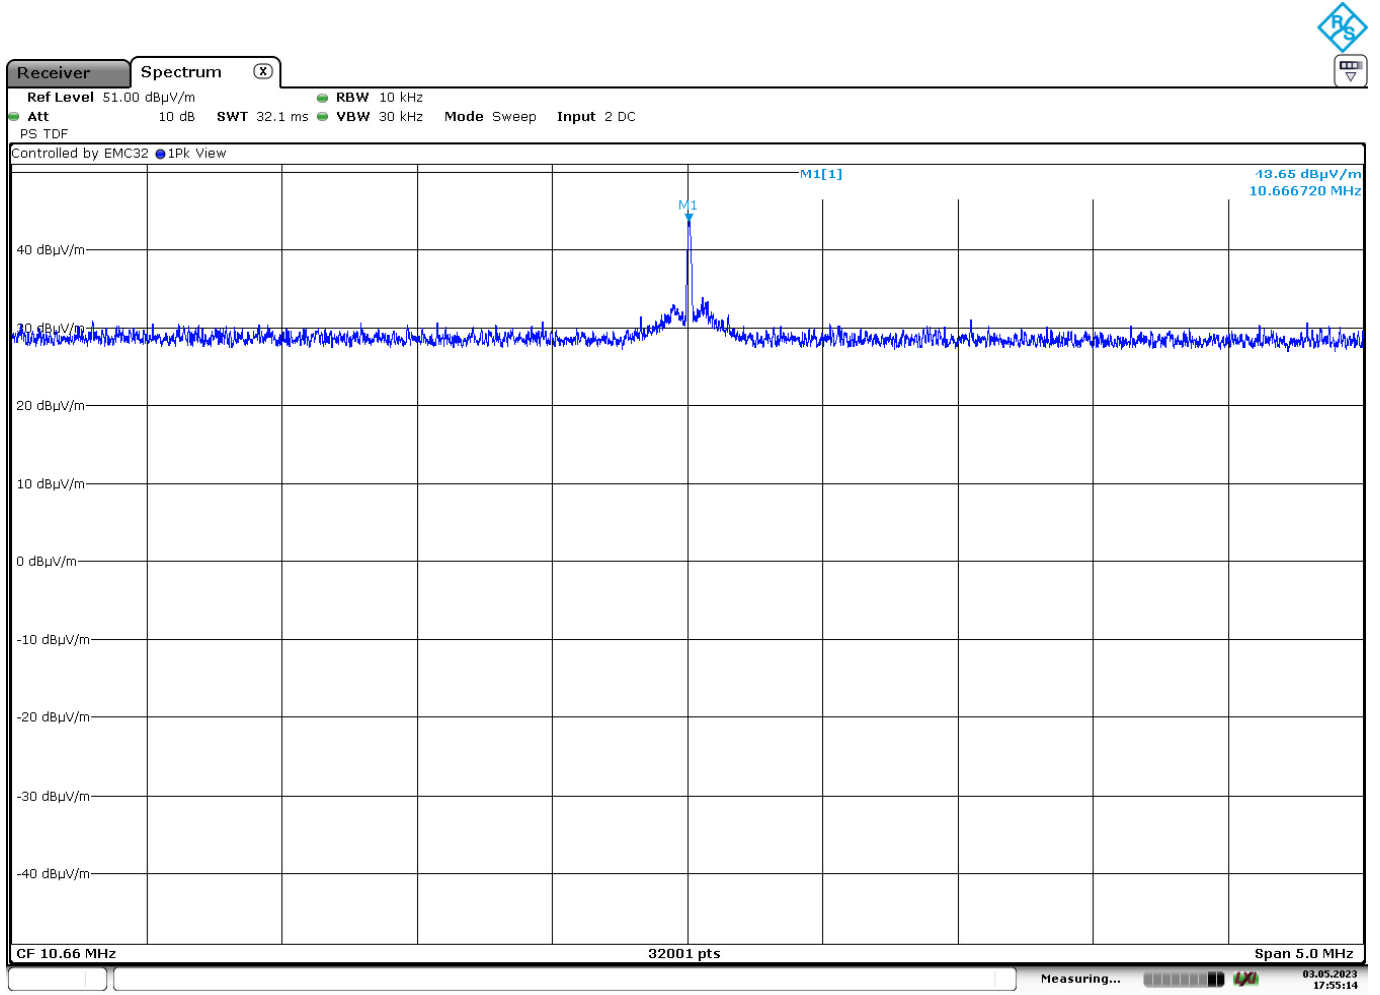

Date: 3.MAY.2023 17:55:14

FREQUENCY RANGE 9 kHz - 30 MHz:

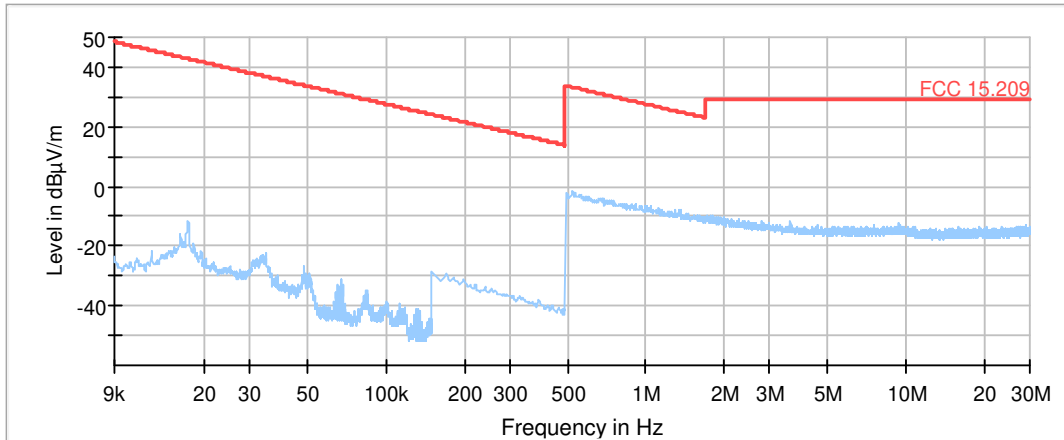


◆ Preview Result 1-PK+ Final_Result PK+
 ◆ FCC 15.225 RSE and Mask Final_Result QPK

Note: The scan is performed with a peak detector.

Resolution bandwidth:
 200 Hz for $9 \text{ kHz} \leq f \leq 150 \text{ kHz}$
 9 kHz for $150 \text{ kHz} \leq f \leq 30 \text{ MHz}$

FREQUENCY RANGE 30 - 200 MHz:

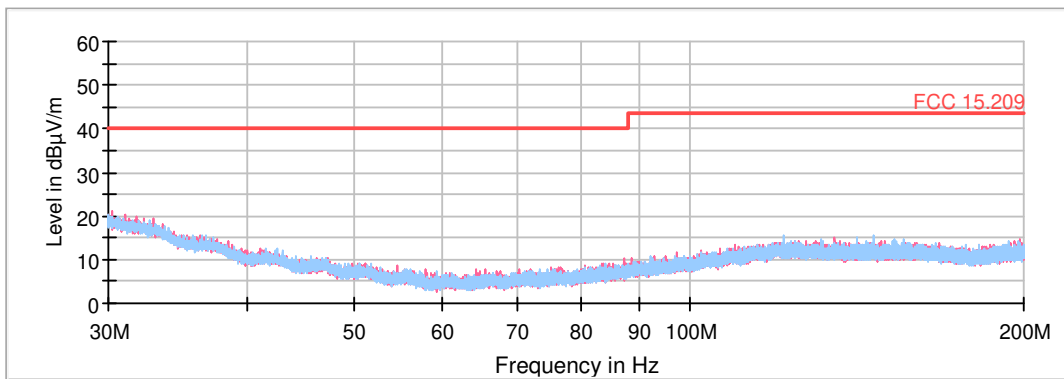

◆ Preview Result 1V-PK+ Final_Result QPK
 ◆ Preview Result 1H-PK+ Final_Result PK+
 ◆ FCC 15.225 QPK

Note: The scan is performed with a peak detector.

Resolution bandwidth:
 100 kHz