

TEST REPORT**Report Number: 3195108LEX-001**
Project Number: 3195108**Evaluation of Model Number: Pronto-7 Pulse CO Oximeter****FCCID: X44PRONTO7****IC ID: 7362C-PRONTO7**

Tested to the SAR Criteria in
FCC OET Bulletin 65, Supplement C (Edition 01-01)
Industry Canada RSS-102 Issue 3

For
Masimo Labs

Test Performed by:

Intertek
731 Enterprise Drive
Lexington, KY 40510

Test Authorized by:

Masimo Labs
30 Fairbanks Suite 100
Irvine, CA 92618

Prepared By: Jason Centers **Date:** 1/17/2010

Jason Centers, Senior Project Engineer

Approved By: Bryan C. Taylor **Date:** 1/17/2010

Bryan Taylor, Team Leader – Engineering

This report is for the exclusive use of Intertek's Client and is provided pursuant to the agreement between Intertek and its Client. Intertek's responsibility and liability are limited to the terms and conditions of the agreement. Intertek assumes no liability to any party, other than to the Client in accordance with the agreement, for any loss, expense or damage occasioned by the use of this report. Only the Client is authorized to copy or distribute this report and then only in its entirety. Any use of the Intertek name or one of its marks for the sale or advertisement of the tested material, product or service must first be approved in writing by Intertek. The observations and test results in this report are relevant only to the sample tested. This report by itself does not imply that the material, product, or service is or has ever been under an Intertek certification program.



TABLE OF CONTENTS

1.0 DOCUMENT HISTORY	4
2.0 REFERENCES.....	5
3.0 INTRODUCTION.....	6
MODIFICATIONS MADE TO TEST SAMPLE	6
4.0 TEST SITE DESCRIPTION.....	7
MEASUREMENT EQUIPMENT.....	8
MEASUREMENT TRACEABILITY	8
MEASUREMENT UNCERTAINTY	9
5.0 JOB DESCRIPTION.....	10
6.0 SYSTEM VERIFICATION	15
SYSTEM VALIDATION.....	15
TISSUE SIMULATING LIQUID DESCRIPTION AND VALIDATION	16
7.0 EVALUATION PROCEDURES	18
TEST POSITIONS:	18
REFERENCE POWER MEASUREMENT:	18
COARSE SCAN:	18
ZOOM SCAN:	18
DATA EXTRAPOLATION:	19
REFERENCE POWER MEASUREMENT:	19
RF AMBIENT ACTIVITY:.....	19
8.0 TEST CONFIGURATION.....	20
9.0 CRITERIA.....	24
10.0 TABULAR TEST RESULTS	25
CONDUCTED POWER MEASUREMENTS	25
BODY MODE SAR TEST RESULTS.....	25
11.0 GRAPHICAL SAR SCAN RESULTS.....	28
12.0 DIPOLE VALIDATION SCANS.....	51
13.0 PROBE CERTIFICATE.....	57
14.0 DIPOLE CERTIFICATE	68

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

15.0 PHANTOM CERTIFICATE77

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

1.0 DOCUMENT HISTORY

Revision/ Project Number	Writer Initials	Date	Change
1.0 /3195108	JC	1/17/2010	Original document
2.0 /3195108	JC	3/12/2010	Updated conducted power measurements per ANSI C63.10:2009

2.0 REFERENCES

- [1] ANSI, *ANSI/IEEE C95.1-1991: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3kHz to 300 GHz*, The Institute of electrical and Electronics Engineers, Inc., New York, NY 10017, 1992
- [2] Federal Communications Commission, “Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields”, Supplement C (Edition 01-01) to OET Bulletin 65 (Edition 97-01), FCC, Washington, D.C. 20554, 1997
- [3] Thomas Schmid, Oliver Egger, and Niels Kuster, “Automated E-field scanning system for dosimetric assessments”, *IEEE Transaction on Microwave Theory and Techniques*, vol. 44, pp. 105-113, Jan. 1996.
- [4] Niels Kuster, Ralph Kastle, and Thomas Schmid, “Dosimetric evaluation of mobile communications equipment with known precision”, *IEICE Transactions on Communications*, vol. E80-B, no. 5, pp.645-652, May 1997.
- [5] NIS81, NAMAS, “The treatment of uncertainty in EMC measurement”, Tech. Rep., NAMAS Executive, National Physical Laboratory, Teddington, Middlesex, England, 1994.

- [6] Barry N. Taylor and Chris E. Kuyatt, “Guidelines for evaluating and expressing the uncertainty of NIST measurement results”, Tech. Rep., National Institute of Standards and Technology, 1994.
- [7] Federal Communications Commission, “SAR Measurement Procedures for 802.11 a/b/g Transmitters”
- [8] Federal Communications Commission, KDB 648474 – “SAR Evaluation Considerations for Handsets with Multiple Transmitters and Antennas”.
- [9] Federal Communications Commission, KDB 447498 – “Mobile and Portable Device RF Exposure Procedures and Equipment Authorization Policies”.
- [10] ANSI, *ANSI/IEEE C63.10-2009: American National Standard for Testing Unlicensed Wireless Devices*.

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

3.0 INTRODUCTION

At the request of Masimo Labs, the Pulse CO Oximeter was evaluated for SAR in accordance with the requirements for RF Exposure compliance testing defined in FCC OET Bulletin 65, Supplement C (Edition 01-01). Testing was performed at the Intertek facility in Lexington, Kentucky from 1/5/2010 to 1/16/2010.

For the evaluation, the dosimetric assessment system DASY4 was used. The phantom employed was the "SAM Twin Phantom". The total uncertainty for the evaluation of the spatial peak SAR values averaged over a cube of 1g tissue mass had been assessed for this system to be $\pm 21.9\%$.

The Pronto-7 was tested at the maximum output power measured by Intertek. Maximum output power measurements are tabulated under **Heading 11.0 - Tabular Test Results**.

The maximum spatial peak SAR value for the sample device averaged over 1g was found to be:

Phantom	Mode	Setup Details	Worst Case Extrapolated SAR _{1g} mW/g
Flat Section (Body Mode)	Ch 11 - 802.11b, 5.5Mbps Data Rate	Front against phantom	1.45
Flat Section (Body Mode)	Ch 39 - Bluetooth	Front against phantom	0.003

Table 1: Maximum Measured SAR

Based on the worst-case data presented above, the Pulse CO Oximeter was found to be **compliant** with the 1.6 mW/g requirement defined in OET Bulletin 65, Supplement C (Edition 01-01) for general population / uncontrolled exposure.

Modifications made to test sample

Intertek implemented no modifications.

4.0 TEST SITE DESCRIPTION

The SAR test site located at 731 Enterprise Drive, Lexington KY 40510 is comprised of the SPEAG model DASY 4 automated near-field scanning system, which is a package, optimized for dosimetric evaluation of mobile radios [3]. This system is installed in an ambient-free shielded chamber. The ambient temperature is controlled to $22.2 \pm 2^{\circ}\text{C}$. Because the HVAC operates as a closed system, the relative humidity remains constant at $50 \pm 5\%$. During the SAR evaluations, the RF ambient conditions are monitored continuously for signals that might interfere with the test results. The tissue simulating liquid is also stored in this area in order to keep it at the same constant ambient temperature as the room.



Figure 1: Intertek SAR Test Site

Measurement Equipment

The following major equipment/components were used for the SAR evaluations:

SAR Measurement System			
Equipment	Specifications	S/N #	Cal. Due
Robot	Stäubli RX60L	597412-01	N/A
	Repeatability: $\pm 0.025\text{mm}$ Accuracy: 0.806×10^{-3} degree Number of Axes: 6		
E-Field Probe	EX3DV3	3516	12/15/2010
	Frequency Range: 10MHz to 6GHz Probe Linearity: ± 0.2 dB (30MHz to 6GHz) Length: 337 mm Distance between the probe tip and the dipole center: 1 mm Tip Diameter: 2.5 mm Calibration: 835, 900, 1750, 1900, 2450, 5200, 5800MHz for head & body tissue simulating liquid		
Data Acquisition	DAE4	358	4/17/2010
	Measurement Range: $1\mu\text{V}$ to $>200\text{mV}$ Input offset Voltage: $< 1\mu\text{V}$ (with auto zero) Input Resistance: 200 M		
Phantom	SAM Twin V4.0	TP-1243	N/A
Complies with IEEE P1528-2003	Type SAM Twin, Homogenous Shell Material: Fiberglass Thickness: 2 ± 0.2 mm Capacity: 20 liter Size of the flat section: approx. 320 x 230 mm		
Device holder	Non-conductive holder supplied with DASY4, dielectric constant less than 5.0	N/A	N/A
Network Analyzer	Agilent 8753A	3018	2/5/2010
	Frequency Range: 30KHz – 3.0 GHz		
Signal Generator	ESG-D3000A	2038	10/19/2010
	Frequency Range: 10MHz – 3 GHz		
Spectrum Analyzer	Rohde & Schwarz FSP 7	1164.4391.07	8/17/2010
	Frequency Range: 9KHz – 7 GHz		

Table 2: Test Equipment Used for SAR Evaluation

Measurement Traceability

All measurements described in this report are traceable to National Institute of Standards and Technology (NIST) standards or appropriate national standards.

Measurement Uncertainty

The Table below includes the uncertainty budget suggested by the IEEE Std 1528-2003 and determined by SPEAG for the DASY4 measurement System

Error Description	Uncertainty Value	Prob. Dist.	Div.	c_i	$c_i(10g)$	Std.Unc. (1g)	Std.Unc. (10g)	$(v_i)_{v_{eff}}$
				(1g)	(10g)			
Measurement System								
Probe Calibration	±5.9%	N	1	1	1	±5.9%	±5.9%	∞
Axial Isotropy	±4.7%	R	$\sqrt{3}$	0.7	0.7	±1.9%	±1.9%	∞
Hemispherical Isotropy	±9.6%	R	$\sqrt{3}$	0.7	0.7	±3.9%	±3.9%	∞
Boundary Effect	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	∞
Linearity	±4.7%	R	$\sqrt{3}$	1	1	±2.7%	±2.7%	∞
System Detection Limits	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	∞
Readout Electronics	±0.3%	N	1	1	1	±0.3%	±0.3%	∞
Response Time	±0.8%	R	$\sqrt{3}$	1	1	±0.5%	±0.5%	∞
Integration Time	±2.6%	R	$\sqrt{3}$	1	1	±1.5%	±1.5%	∞
RF Ambient Conditions	±3.0%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%	∞
Probe Positioner	±0.4%	R	$\sqrt{3}$	1	1	±0.2%	±0.2%	∞
Probe Positioning	±2.9%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%	∞
Max. SAR Eval.	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	∞
Test sample Related								
Device Positioning	±2.9%	N	1	1	1	±2.9%	±2.9%	145
Device Holder	±3.6%	N	1	1	1	±3.6%	±3.6%	5
Power Drift	±5.0%	R	$\sqrt{3}$	1	1	±2.9%	±2.9%	∞
Phantom and Tissue Parameters								
Phantom Uncertainty	±4.0%	R	$\sqrt{3}$	1	1	±2.3%	±2.3%	∞
Liquid Conductivity (target)	±5.0%	R	$\sqrt{3}$	0.64	0.43	±1.8%	±1.2%	∞
Liquid Conductivity (meas.)	±2.5%	N	1	0.64	0.43	±1.6%	±1.1%	∞
Liquid Permittivity (target)	±5.0%	R	$\sqrt{3}$	0.6	0.49	±1.7%	±1.4%	∞
Liquid Permittivity (meas.)	±2.5%	N	1	0.6	0.49	±1.5%	±1.2%	∞
Combined Standard Uncertainty						±10.9%	±10.7%	387
Expanded STD Uncertainty						±21.9%	±21.4%	

Notes.

1. Worst Case uncertainty budget for DASY4 assessed according to IEEE 1528. The budget is valid for the frequency range 300 MHz – 3 GHz and represents a worst-case analysis. For specific tests and configurations, the uncertainty could be considerably smaller.

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

5.0 JOB DESCRIPTION

At the request of Masimo Labs, the Pronto-7 was evaluated to the requirements defined in OET Bulletin 65, Supplement C. The Pronto-7 Pulse CO-Oximeter is used to simultaneously and non-invasively measure total hemoglobin (SpHb), pulse rate (PR) and perfusion index (PI).

Test sample	
Manufacturer	Masimo Labs
Model Number	Pronto-7
Serial Number	Not Labeled
Receive Date	1/5/2010
Device Received Condition	Good condition production unit
Device Category	Portable
RF Exposure Category	General Population/Uncontrolled Environment
Frequency Band	2.4GHz ISM Band
Mode(s) of Operation	802.11b/g, Bluetooth
Duty Cycle	100% (Test Commands)
Maximum Output Power	802.11: 23.2 dBm (peak - conducted) Bluetooth: -9.93 dbm (EIRP)
Test Channels	802.11b – Ch1 (2412MHz), Ch2 (2417MHz), Ch 6 (2437MHz), Ch 11 (2462MHz) Bluetooth – Ch 39 (2441 MHz)
Antenna Type	Bluetooth – Internal ceramic antenna 802.11b/g – $\frac{1}{2}\lambda$ dipole, 2dBi gain
Antenna Separation Distance	1.6 mm
Test sample Accessories	
Battery type	Rechargeable Li-Ion
Belt clip	None
Cables	Masimo PDC-SC (Clip Spot Check Sensor)
Antennas	Internal
Contact Information	
Contact Name	Sean Merritt
Phone Number	(949) 900-6614
Fax Number	(949) 900-6901
Email Address	smerritt@masimolabs.com

Table 3: Product Information

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Test Sample Pictures:

Photographs of the test sample and its accessories are shown in Figure 2 through Figure 5.

Figure 2: Front of Test Sample



Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Figure 3: Back of Test Sample



Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Figure 4: Left Side of Test Sample



Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Figure 5: Right of Test Sample



Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

6.0 SYSTEM VERIFICATION

System Validation

Prior to the assessment, the system was verified to be within $\pm 10\%$ of the specifications by using the system validation kit. The validation was performed at 2450 MHz using muscle simulating tissue. The results from the daily dipole validation are shown in Table 4.

Figure 6: System Verification Setup

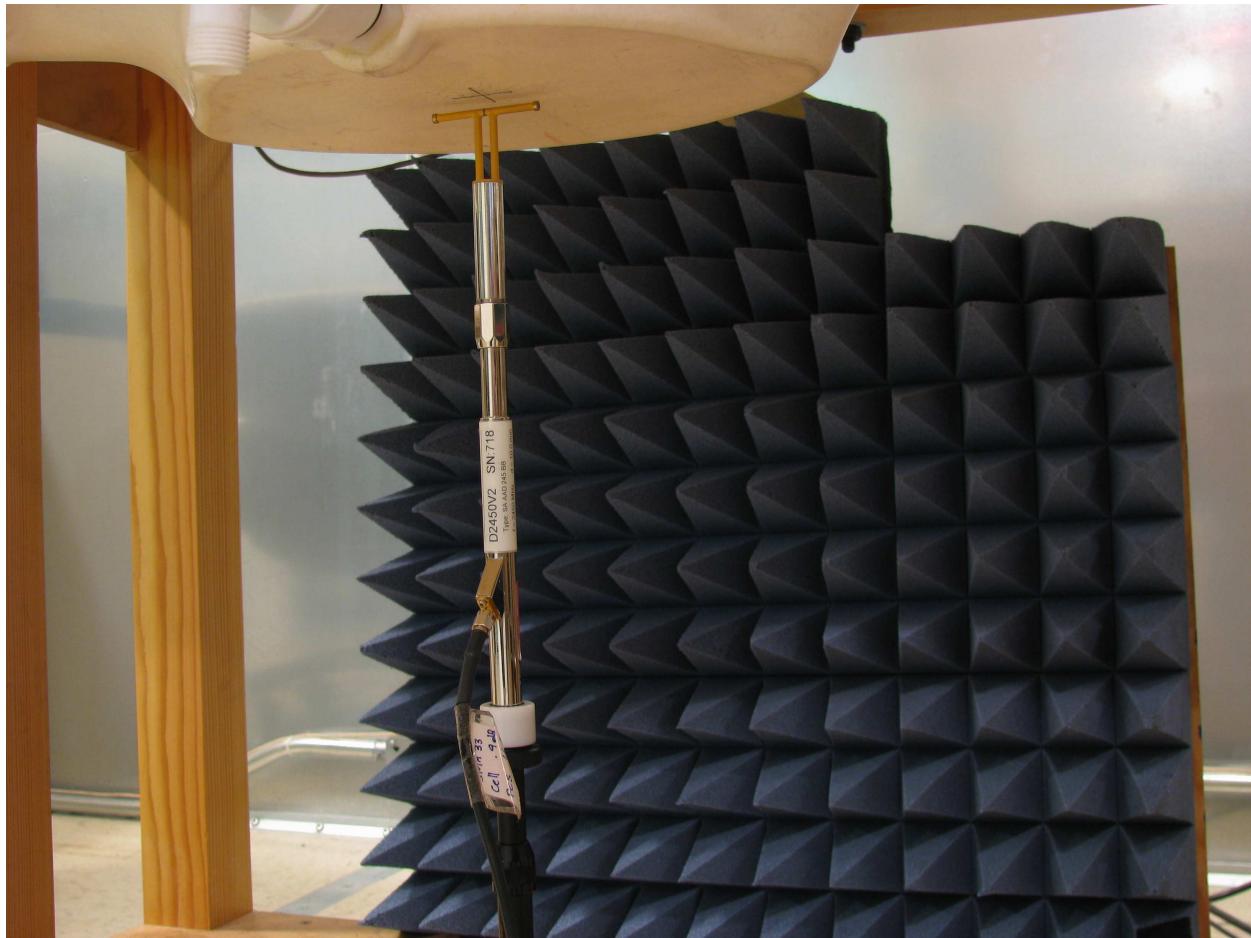


Table 4: Dipole Validation

Reference Dipole Validation								
Frequency Measure (MHz)	Dipole Type	Dipole Serial Number	Fluid Type	Dipole Power Input	Cal. Lab SAR (1g)	Measured SAR (1g)	% Error SAR (1g)	Date
2450	D2450	718	2450 MSL	1W	50.2	48.20	3.98	1/6/2010
2450	D2450	718	2450 MSL	1W	50.2	47.60	5.18	1/8/2010
2450	D2450	718	2450 MSL	1W	50.2	54.40	8.37	1/10/2010

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Tissue Simulating Liquid Description and Validation

The dielectric parameters were verified to be within 5% of the target values each day prior to assessment. The dielectric parameters (ϵ_r , σ) and temperature on each day of testing are shown in Table 5 and Table 6. A recipe for the tissue simulating fluid used is shown in Table 7.

Table 5: Dielectric Parameter Validation

Body Tissue Parameters								
Frequency Measure (MHz)	Dielectric Constant Target	Dielectric Constant Measure	Dielectric % Deviation	Imaginary Part	Conductivity Target	Conductivity Measure	Conductivity % Deviation	Date
2412	52.75	52.06	1.31	14.78	1.91	1.98	3.77	1/6/2010
2437	52.72	51.98	1.40	14.85	1.94	2.01	3.71	
2450	52.7	51.91	1.50	14.87	1.95	2.03	3.87	
2462	52.68	51.88	1.52	14.98	1.97	2.05	4.08	

The % deviation should be below 5%.

Body Tissue Parameters								
Frequency Measure (MHz)	Dielectric Constant Target	Dielectric Constant Measure	Dielectric % Deviation	Imaginary Part	Conductivity Target	Conductivity Measure	Conductivity % Deviation	Date
2412	52.75	51.27	2.81	14.5	1.91	1.94	1.80	1/8/2010
2437	52.72	51.2	2.88	14.7	1.94	1.99	2.66	
2450	52.7	51.1	3.04	14.84	1.95	2.02	3.66	
2462	52.68	51	3.19	14.91	1.97	2.04	3.60	

The % deviation should be below 5%.

Body Tissue Parameters								
Frequency Measure (MHz)	Dielectric Constant Target	Dielectric Constant Measure	Dielectric % Deviation	Imaginary Part	Conductivity Target	Conductivity Measure	Conductivity % Deviation	Date
2412	52.75	51.67	2.05	14.62	1.91	1.96	2.64	1/10/2010
2437	52.72	51.42	2.47	14.75	1.94	2.00	3.01	
2450	52.7	51.3	2.66	14.8	1.95	2.02	3.38	
2462	52.68	51.21	2.79	14.92	1.97	2.04	3.66	

The % deviation should be below 5%.

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Table 6: Temperature Validation

Date	Ambient Temperature(°C)	Muscle Simulating Liquid Temperature (°C) f=2450MHz
1/6/2010	22.3	21.9
1/8/2010	22.5	21.8
1/10/2010	22.3	22.1

Table 7: Tissue Simulating Fluid Recipe

TYPICAL COMPOSITION OF INGREDIENTS FOR LIQUID TISSUE PHANTOMS, Supplement C Edition 01-01 to OET Bulletin 65 Edition 97-01, Page 36. (450MHz to 2450 MHz data only)												
Ingredient (% by weight)	f (MHz)											
	450		835		915		1900		2450		5500	
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body
Water	38.56	51.16	41.45	52.4	41.05	56	54.9	70.45	62.7	68.64	65.53	78.67
Salt (NaCl)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.36	0.5	0	0	0
Sugar	56.32	46.78	56	45	56.5	41.76	0	0	0	0	0	0
HEC	0.98	0.52	1	1	1	1.21	0	0	0	0	0	0
Bactericide	0.19	0.05	0.1	0.1	0.1	0.27	0	0	0	0	0	0
Triton X-100	0	0	0	0	0	0	0	0	36.8	0	17.235	10.665
DGBE	0	0	0	0	0	0	44.92	29.18	0	31.37	0	0
DGHE	0	0	0	0	0	0	0	0	0	0	17.235	10.665
Dielectric Constant	43.42	58	42.54	56.1	42	56.8	39.9	53.3	39.8	52.7		
Conductivity (S/m)	0.85	0.83	0.91	0.95	1	1.07	1.42	1.52	1.88	1.95		

7.0 EVALUATION PROCEDURES

Prior to any testing, the appropriate fluid was used to fill the phantom to a depth of 15 cm \pm 0.2cm. The fluid parameters were verified and the dipole validation was performed as described in the previous sections.

Test Positions:

The Device was positioned against the SAM and flat phantom using the exact procedure described in Supplement C Edition 01 – 01 of Federal Communications Commission, “Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields”, OET Bulletin 65, FCC, Washington, D.C. 20554, 1997.

Reference Power Measurement:

The measurement probe was positioned at a fixed location above the reference point. A power measurement was made with the probe above this reference position so it could be used for the assessing the power drift later in the test procedure.

Coarse Scan:

A coarse area scan with a horizontal grid spacing of 15 x 15 mm was performed in order to find the approximate location of the peak SAR value. This scan was performed with the measurement probe at a constant height in the simulating fluid. A two dimensional spline interpolation algorithm was then used to determine the peaks and gradients within the scanned area.

Zoom Scan:

A zoom scan was performed around the approximate location of the peak SAR as determined from the coarse scan. The zoom scan was comprised of a measurement volume of 30 x 30 x 30 mm based on 7 x 7 x 7 points. On the basis of this data set, the spatial peak SAR value was evaluated with the following procedure:

Data Extrapolation:

Since the center of the dipoles in the measurement probe are 1 mm away from the tip of the probe, and the distance between the surface and the lowest measurement point is 2 mm the data at the surface was extrapolated. The extrapolation was based on a least square algorithm. A polynomial of the fourth order was calculated through the points in the Z-axes. This polynomial was then used to evaluate the points between the surface and the probe tip.

The maximum interpolated value was searched with a straightforward sorting algorithm. Around this maximum, the SAR values averaged over the spatial volumes (1g or 10g) were computed using a 3-D spline interpolation algorithm. The 3-D spline is composed of three one-dimensional splines with the “Not a knot” condition (in x, y and z directions). The volume was integrated with a trapezoidal algorithm. 1000 points (10 x 10 x 10) were interpolated to calculate the average.

All neighboring volumes were evaluated until no neighboring volume with a higher average value was found.

Reference Power Measurement:

The probe was positioned at precisely the same reference point and the reference power measurement was repeated. The difference between the initial reference power and the final one is referred to as the power drift

RF Ambient Activity:

During the entire SAR evaluation, the RF ambient activity was monitored using a spectrum analyzer with an antenna connected to it. The spectrum analyzer was tuned to the frequency of measurement and with one trace set to max hold mode. In this way, it was possible to determine if at any point during the SAR measurement there was an interfering ambient signal. If an ambient signal was detected, then the SAR measurement was repeated.

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001


Model Number: Pronto-7X44PRONTO7

8.0 TEST CONFIGURATION

For the purpose of this evaluation, the Pronto-7 was considered to be a device that could be operated when held against the body. All SAR scans were performed with a freshly charged battery installed.

The test channels and operating modes were selected using software based test commands. The device was positioned against the bottom of the phantom with zero clearance during the evaluation. Each side of the device was scanned to determine the worst case exposure. Photographs of the Pronto-7, as positioned for testing, is shown in Figure 7 through Figure 10.

Figure 7: Device Positioning for SAR Scans – Front

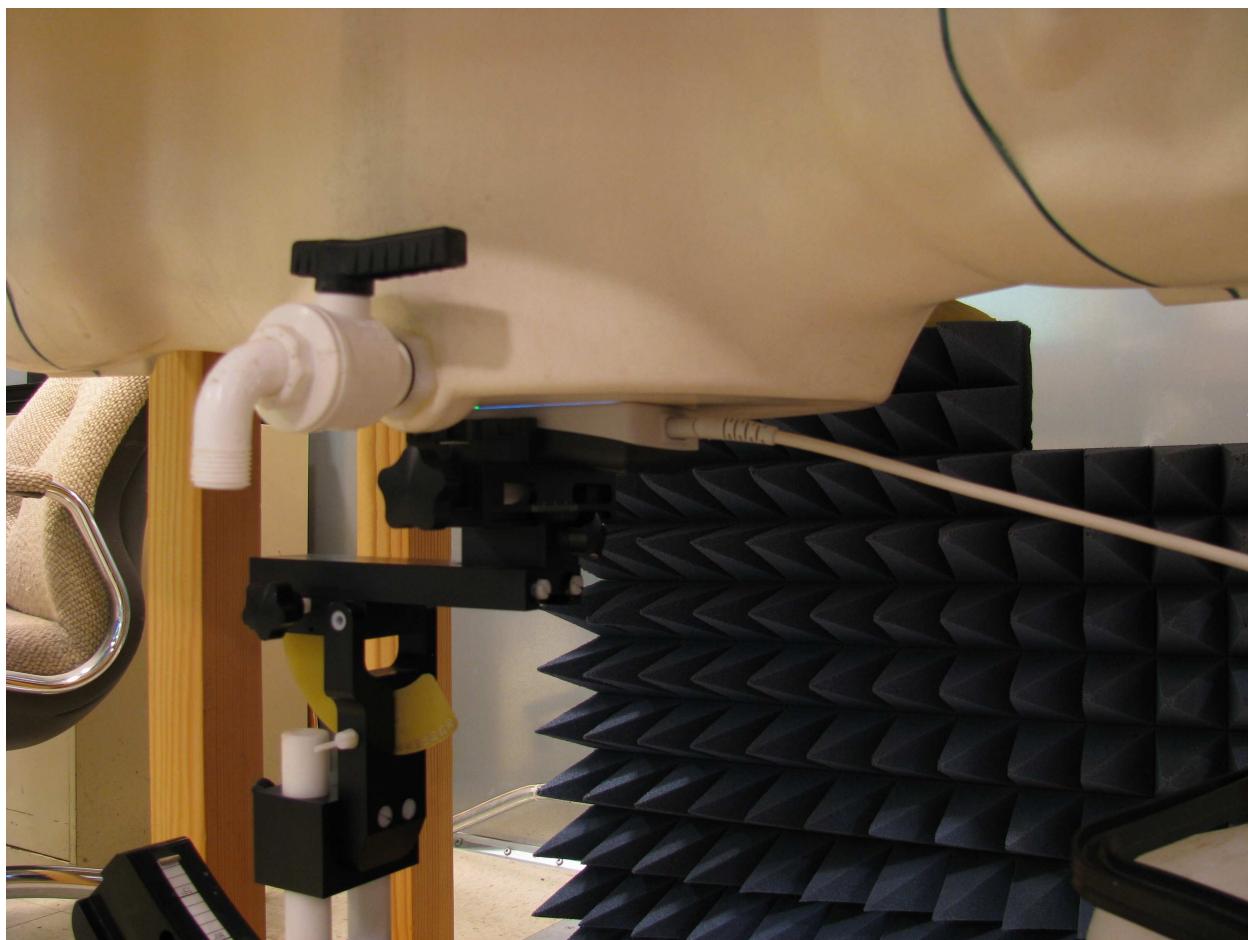


Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Figure 8: Device Positioning for SAR Scans – Back




Figure 9: Device Positioning for SAR Scans – Left Side

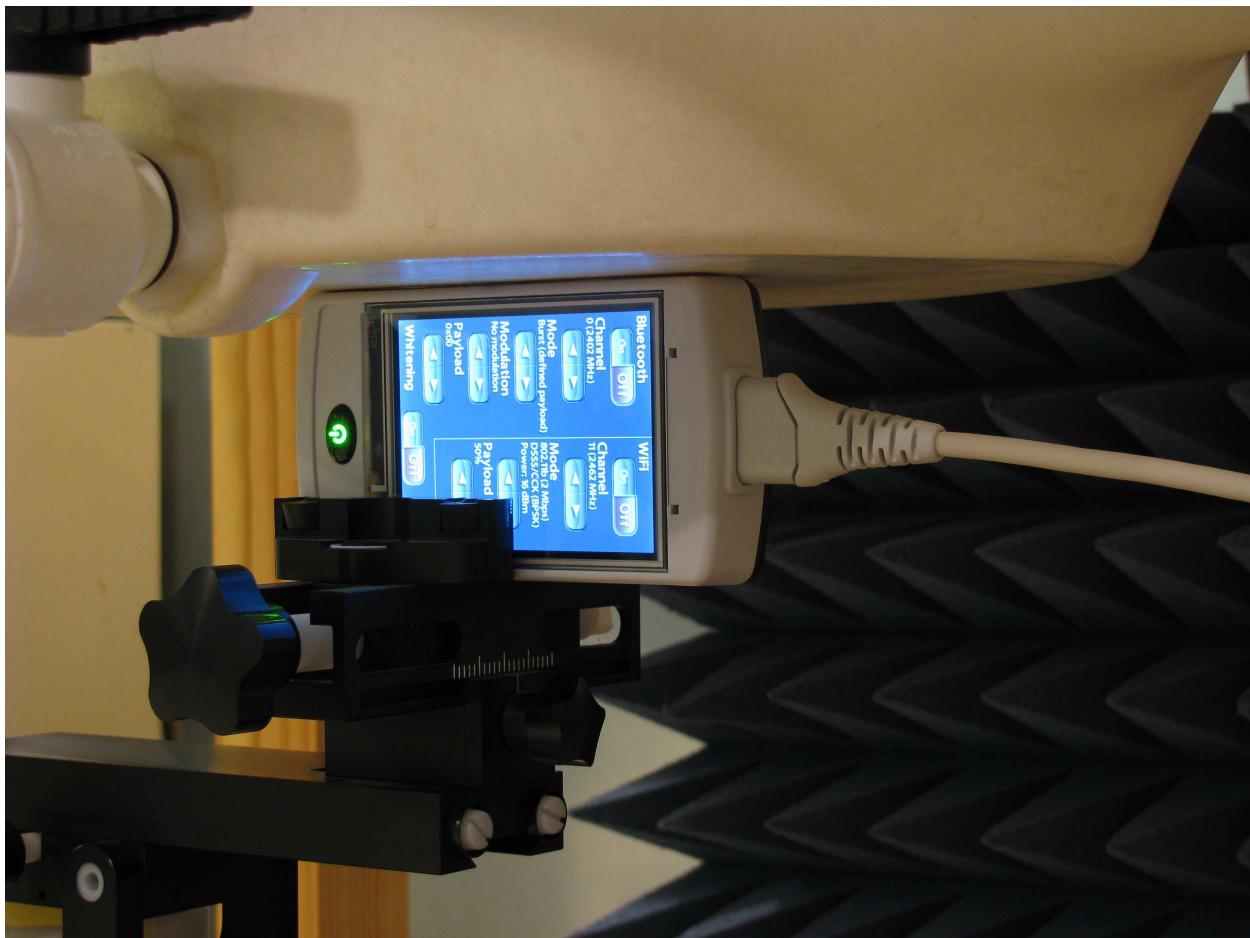

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Figure 10: Device Positioning for SAR Scans – Right Side

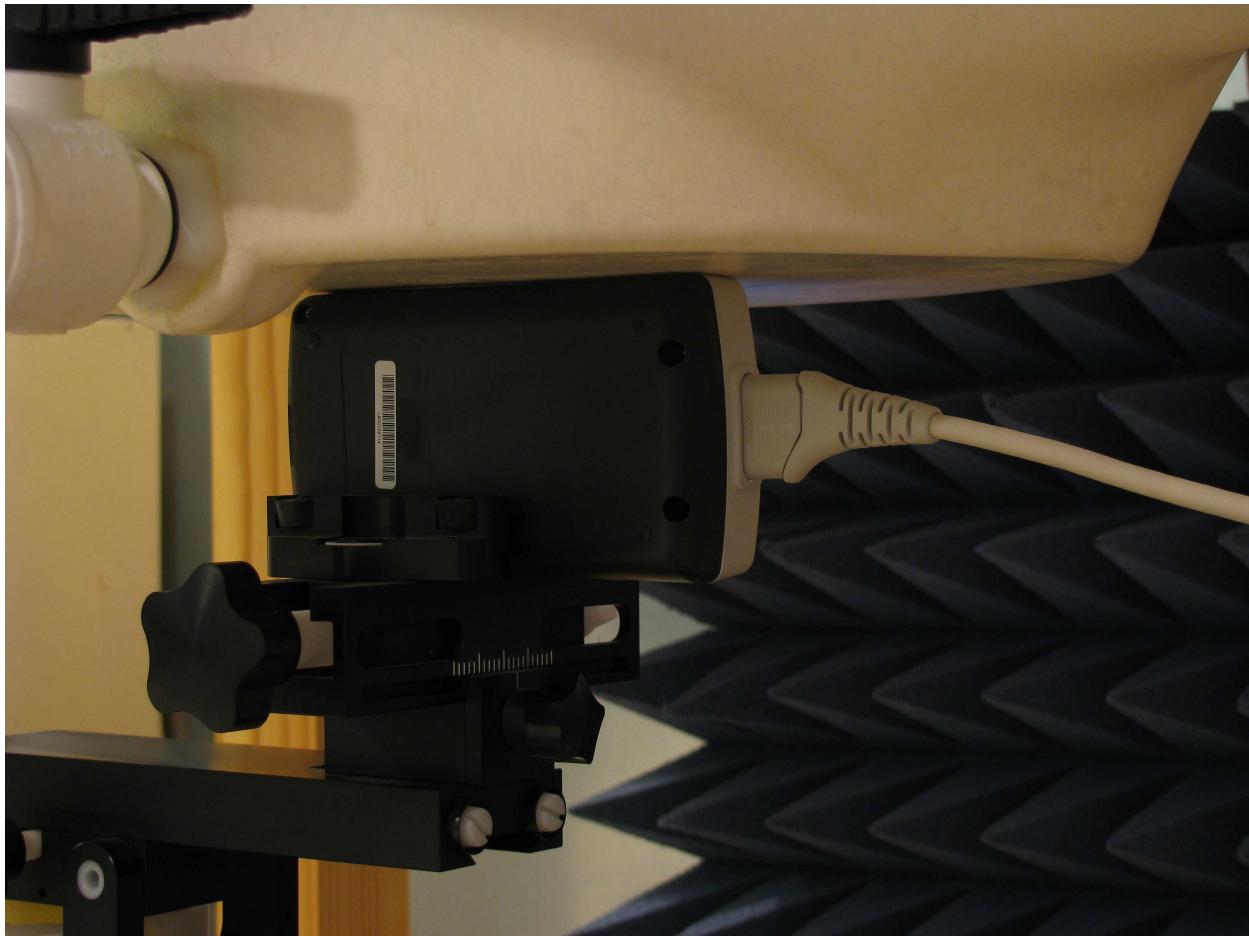

9.0 CRITERIA

The following FCC limits for SAR apply to devices operating in the General Population/Uncontrolled Exposure environment:

Exposure (General Population/Uncontrolled Exposure environment)	SAR (W/kg)
Average over the whole body	0.08
Spatial Peak (1g)	1.60
Spatial Peak for hands, wrists, feet and ankles (10g)	4.00

10.0 TABULAR TEST RESULTS

The results on the following page(s) were obtained when the device was transmitting at maximum output power. Detailed measurement data and plots, which reveal information about the location of the maximum SAR with respect to the device, are referenced under **Heading 12.0 - Graphical SAR Scan Results**.

Conducted Power Measurements

The conducted power measurements for the Pronto-7 were performed in accordance to ANSI C63.19:2009 Section 6.10.2.1 using the channel integration method. The measurements were performed using the channel power function of the spectrum analyzer in peak and average detection mode. Cable loss was accounted for within the test set by offsetting the readings by the appropriate amount.

Table 8: Conducted Output Power Results – 802.11b/g

Channel	Frequency (MHz)	Modulation	Data Rate	Peak Conducted Output Power (dBm)	Avg Conducted Output Power (dBm)
1	2412	BPSK	1 Mbps	23.25	14.41
		BPSK	5.5 Mbps	22.88	15.71
		CCK	11 Mbps	22.41	15.14
		64 QAM	54 Mbps	18.94	5.97
6	2437	BPSK	1 Mbps	24.67	15.06
		BPSK	5.5 Mbps	24.92	18.23
		CCK	11 Mbps	24.86	16.72
		64 QAM	54 Mbps	19.81	6.82
11	2462	BPSK	1 Mbps	24.46	15.26
		BPSK	5.5 Mbps	23.52	17.26
		CCK	11 Mbps	23.82	16.16
		64 QAM	54 Mbps	18.52	5.51

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Table 9: EIRP Results – Bluetooth

TX Channel	Polarity	Axis	TX Frequency (MHz)	Device Reading (dBuV)	Sub. Reading (dBuV)	Cable Loss (dB)	Tx Antenna Gain (dBi)	Signal Generator Output (dBm)	EIRP (dBm)
Low	V	X	2402	42.69	61.46	4.1	9.4	0	-13.47
Mid	V	X	2441	42.27	61.54	4.1	9.4	0	-13.97
High	V	X	2480	43.42	61.07	4.1	9.4	0	-12.35
Low	H	X	2402	45.67	64.09	4.1	9.4	0	-13.12
Mid	H	X	2441	45.72	64.27	4.1	9.4	0	-13.25
High	H	X	2480	44.08	63.72	4.1	9.4	0	-14.34
Low	V	Y	2402	45.73	61.46	4.1	9.4	0	-10.43
Mid	V	Y	2441	43.56	61.54	4.1	9.4	0	-12.68
High	V	Y	2480	41.94	61.07	4.1	9.4	0	-13.83
Low	H	Y	2402	48.17	64.09	4.1	9.4	0	-10.62
Mid	H	Y	2441	49.04	64.27	4.1	9.4	0	-9.93
High	H	Y	2480	47.37	63.72	4.1	9.4	0	-11.05
Low	V	Z	2402	43.96	61.46	4.1	9.4	0	-12.2
Mid	V	Z	2441	41.39	61.54	4.1	9.4	0	-14.85
High	V	Z	2480	42.87	61.07	4.1	9.4	0	-12.9
Low	H	Z	2402	47.44	64.09	4.1	9.4	0	-11.35
Mid	H	Z	2441	47.39	64.27	4.1	9.4	0	-11.58
High	H	Z	2480	45.8	63.72	4.1	9.4	0	-12.62

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Body Mode SAR Test Results

During the test, the RF output power of the test sample varied by a small amount due to heat and battery output power variations in the device. The device was scanned on each side for the 802.11 and Bluetooth transmitter to find the worse case SAR. The front of the device was identified as the worse case side. A scan was performed at each data rate in b-mode to find the worse case mode. A SAR measurement was made at the low, mid, and high channels with the device transmitting in the worse case orientation and data mode. Since the output power in 802.11g mode was less than the 802.11b mode, no scans were required for that mode. The sum of the worse case 1-g SAR values from the 802.11b and Bluetooth scans were less than the 1.6mW/g limit.

Table 10: Body Mode SAR Results – 802.11b/g Mode

Flat Phantom; 99% Duty Cycle						
Mode/Channel	Data Rate	Freq. (MHz)	Position	SAR Drift (dB)	Measured 1-g SAR (mW/g)	Meas. 10g-SAR (mw/g)
802.11b - Ch. 6	1Mbps	2437	Back	2.650	0.017	0.009
802.11b - Ch. 6	1Mbps	2437	Left Side	0.376	0.008	0.004
802.11b - Ch. 6	1Mbps	2437	Right Side	0.235	0.027	0.014
802.11b - Ch. 6	1Mbps	2437	Front	0.546	0.457	0.175
802.11b - Ch. 6	2Mbps	2437	Front	0.074	1.080	0.403
802.11b - Ch. 6	5.5Mbps	2437	Front	0.055	1.220	0.466
802.11b - Ch. 6	11Mbps	2437	Front	-0.210	0.667	0.258
802.11b - Ch. 1	5.5Mbps	2412	Front	0.095	0.612	0.240
802.11b - Ch. 2	5.5Mbps	2417	Front	0.170	1.020	0.397
802.11b - Ch. 11	5.5Mbps	2462	Front	-0.198	1.450	0.534
FCC Limit = 1.6mW/g (General Population / Uncontrolled Exposure)						

Table 11: Body Mode SAR Results – Bluetooth Mode

Flat Phantom; 99% Duty Cycle						
Mode/Channel	Data Rate	Freq. (MHz)	Position	SAR Drift (dB)	Measured 1-g SAR (mW/g)	Meas. 10g-SAR (mw/g)
Ch39	Continuous	2441	Front	0.158	0.003	0.001
Ch39	Continuous	2441	Left Side	9.760	0.003	0.001
Ch39	Continuous	2441	Right Side	***	***	***
Ch39	Continuous	2441	Back	3.510	0.001	0.000
FCC Limit = 1.6mW/g (General Population / Uncontrolled Exposure)						
*** The right side is opposite the Bluetooth antenna. No measurable SAR.						

11.0 GRAPHICAL SAR SCAN RESULTS

Date/Time: 1/6/2010 2:15:36 PM

Test Laboratory: Intertek ETL Semko

File Name: [CH 6 802.11b Scan Back Side.da4](#)**DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified****Program Name: Different Test Procedures (Left-Hand Side)**

Communication System: 802.11b/g; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 2437 \text{ MHz}$; $\sigma = 2.01 \text{ mho/m}$; $\epsilon_r = 52$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Cube7x7x7 - Flat Phantom/Area Scan (12x20x1): Measurement grid: $dx=10\text{mm}$, $dy=10\text{mm}$

Maximum value of SAR (measured) = 0.021 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: $dx=7\text{mm}$, $dy=7\text{mm}$, $dz=7\text{mm}$

Reference Value = 1.05 V/m; Power Drift = 2.65 dB

Peak SAR (extrapolated) = 0.032 W/kg

SAR(1 g) = 0.017 mW/g; SAR(10 g) = 0.00941 mW/g


Maximum value of SAR (measured) = 0.023 mW/g

Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: $dx=20\text{mm}$, $dy=20\text{mm}$, $dz=20\text{mm}$

Maximum value of SAR (measured) = 0.004 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

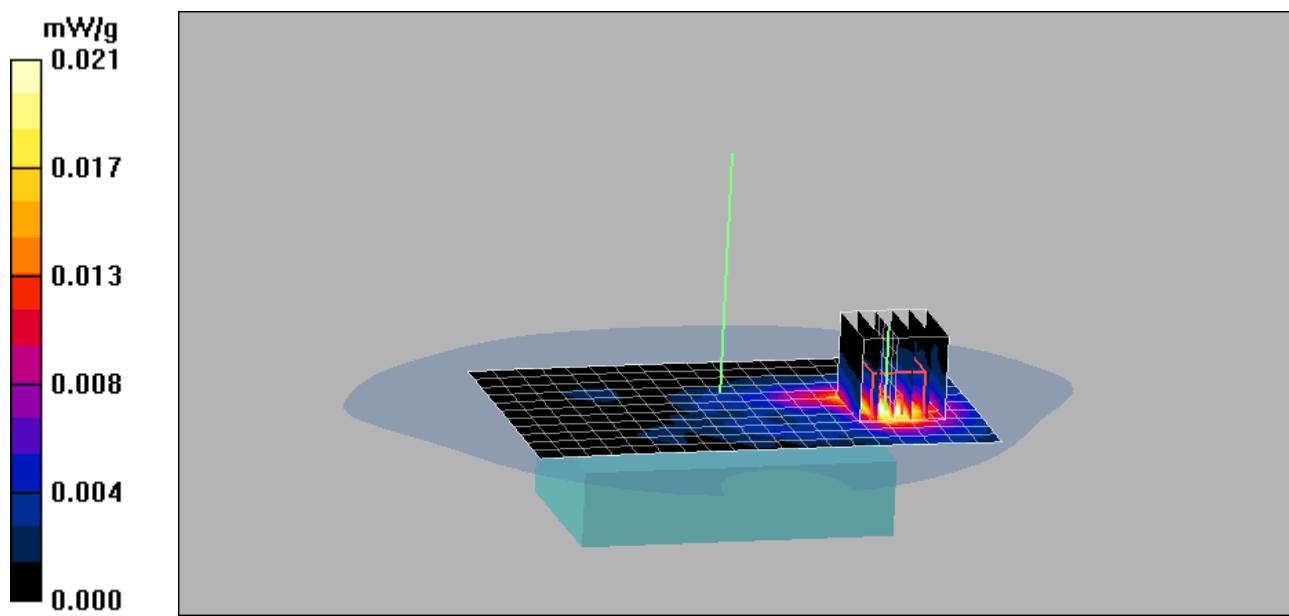

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/6/2010 2:51:26 PM

Test Laboratory: Intertek ETL Semko
File Name: [CH 6 802.11b Scan Left Side.da4](#)

DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified
Program Name: Different Test Procedures (Left-Hand Side)

Communication System: 802.11b/g; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437 \text{ MHz}$; $\sigma = 2.01 \text{ mho/m}$; $\epsilon_r = 52$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186


Cube7x7x7 - Flat Phantom/Area Scan (12x20x1): Measurement grid: $dx=10\text{mm}$, $dy=10\text{mm}$
Maximum value of SAR (measured) = 0.009 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: $dx=7\text{mm}$, $dy=7\text{mm}$, $dz=7\text{mm}$
Reference Value = 1.50 V/m; Power Drift = 0.376 dB
Maximum value of SAR (measured) = 0.011 mW/g

Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: $dx=20\text{mm}$, $dy=20\text{mm}$, $dz=20\text{mm}$
Maximum value of SAR (measured) = 0.006 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

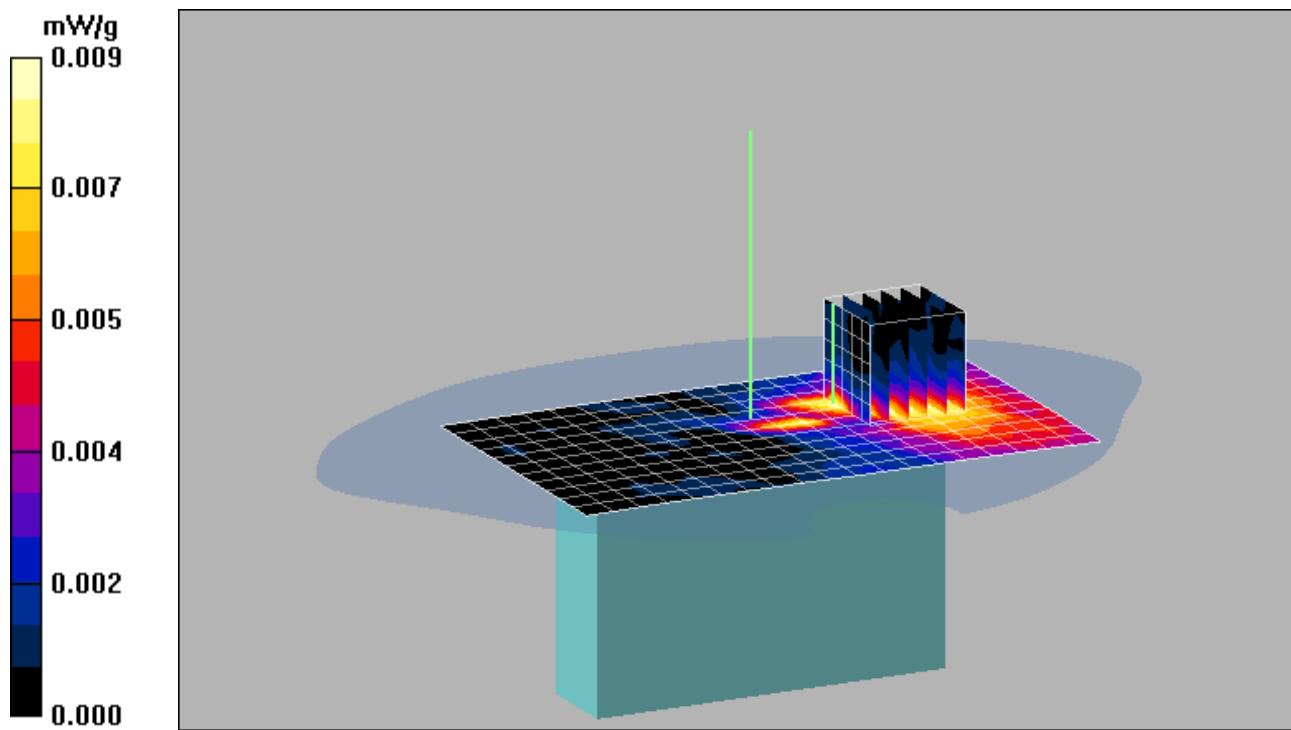

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/6/2010 3:52:10 PM

Test Laboratory: Intertek ETL Semko
File Name: [CH 6 802.11b Scan Right Side.da4](#)

DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified
Program Name: Different Test Procedures (Left-Hand Side)

Communication System: 802.11b/g; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437$ MHz; $\sigma = 2.01$ mho/m; $\epsilon_r = 52$; $\rho = 1000$ kg/m³
Phantom section: Flat Section


DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Cube7x7x7 - Flat Phantom/Area Scan (12x20x1): Measurement grid: dx=10mm, dy=10mm
Maximum value of SAR (measured) = 0.037 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: dx=7mm, dy=7mm, dz=7mm
Reference Value = 0.897 V/m; Power Drift = 0.235 dB
Maximum value of SAR (measured) = 0.039 mW/g

Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: dx=20mm, dy=20mm, dz=20mm
Maximum value of SAR (measured) = 0.002 mW/g

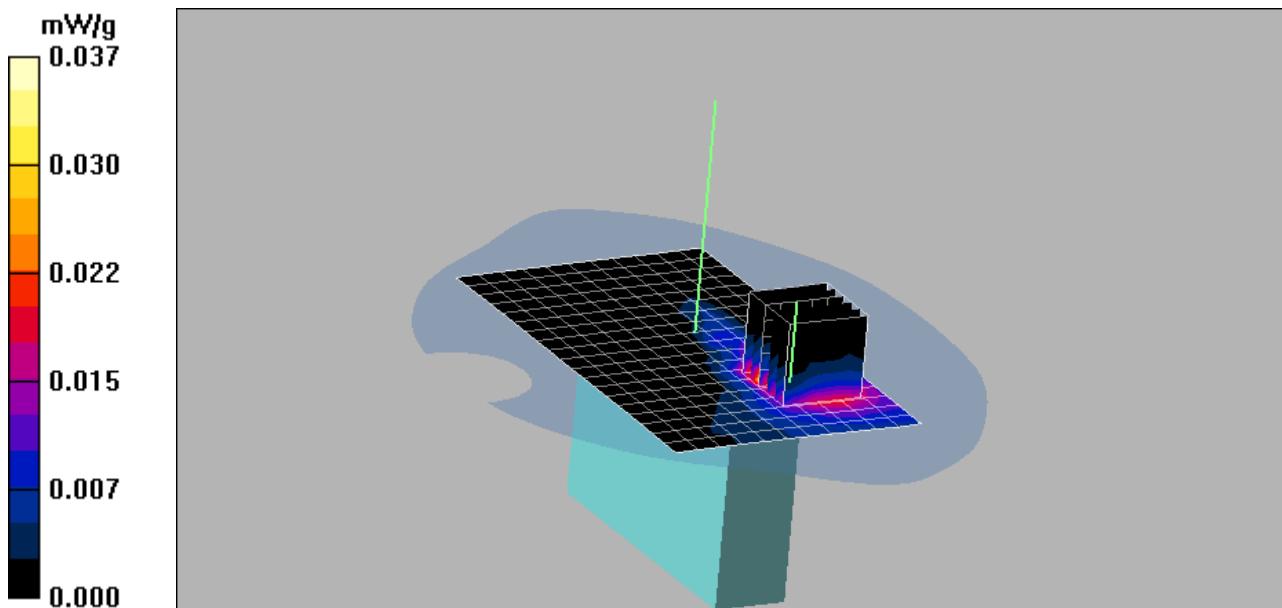

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/6/2010 4:29:49 PM

Test Laboratory: Intertek ETL Semko
File Name: [CH 6 802.11b Scan Front Side.da4](#)

DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified
Program Name: Different Test Procedures (Left-Hand Side)

Communication System: 802.11b/g; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437 \text{ MHz}$; $\sigma = 2.01 \text{ mho/m}$; $\epsilon_r = 52$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186


Cube7x7x7 - Flat Phantom/Area Scan (12x20x1): Measurement grid: $dx=10\text{mm}$, $dy=10\text{mm}$
Maximum value of SAR (measured) = 0.482 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: $dx=7\text{mm}$, $dy=7\text{mm}$, $dz=7\text{mm}$
Reference Value = 0.929 V/m; Power Drift = 0.546 dB
Peak SAR (extrapolated) = 1.14 W/kg
SAR(1 g) = 0.457 mW/g; SAR(10 g) = 0.175 mW/g
Maximum value of SAR (measured) = 0.664 mW/g

Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: $dx=20\text{mm}$, $dy=20\text{mm}$, $dz=20\text{mm}$
Maximum value of SAR (measured) = 0.002 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

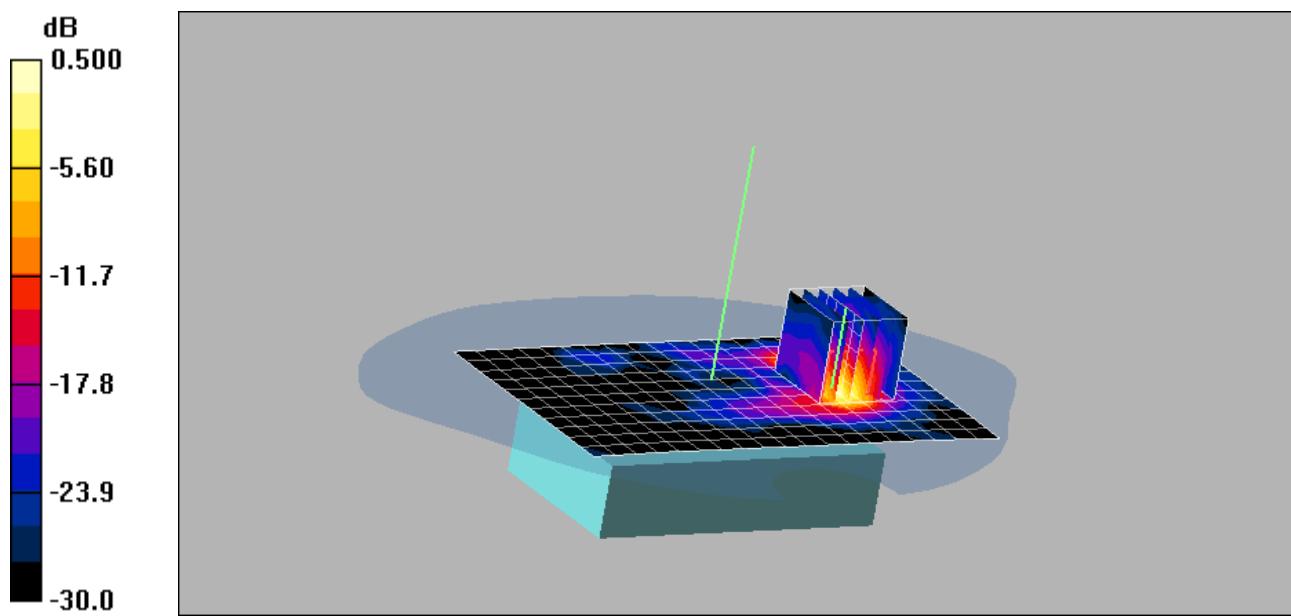

0 dB = 0.482mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/6/2010 5:13:10 PM

Test Laboratory: Intertek ETL Semko
File Name: [CH 6 802.11b 2Mbps Scan Front Side.da4](#)

DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified
Program Name: Different Test Procedures (Left-Hand Side)

Communication System: 802.11b/g; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437 \text{ MHz}$; $\sigma = 2.01 \text{ mho/m}$; $\epsilon_r = 52$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186


Cube7x7x7 - Flat Phantom/Area Scan (12x20x1): Measurement grid: $dx=10\text{mm}$, $dy=10\text{mm}$
Maximum value of SAR (measured) = 1.04 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: $dx=7\text{mm}$, $dy=7\text{mm}$, $dz=7\text{mm}$
Reference Value = 1.42 V/m; Power Drift = 0.074 dB
Peak SAR (extrapolated) = 2.78 W/kg
SAR(1 g) = 1.08 mW/g; SAR(10 g) = 0.403 mW/g
Maximum value of SAR (measured) = 1.65 mW/g

Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: $dx=20\text{mm}$, $dy=20\text{mm}$, $dz=20\text{mm}$
Maximum value of SAR (measured) = 0.004 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

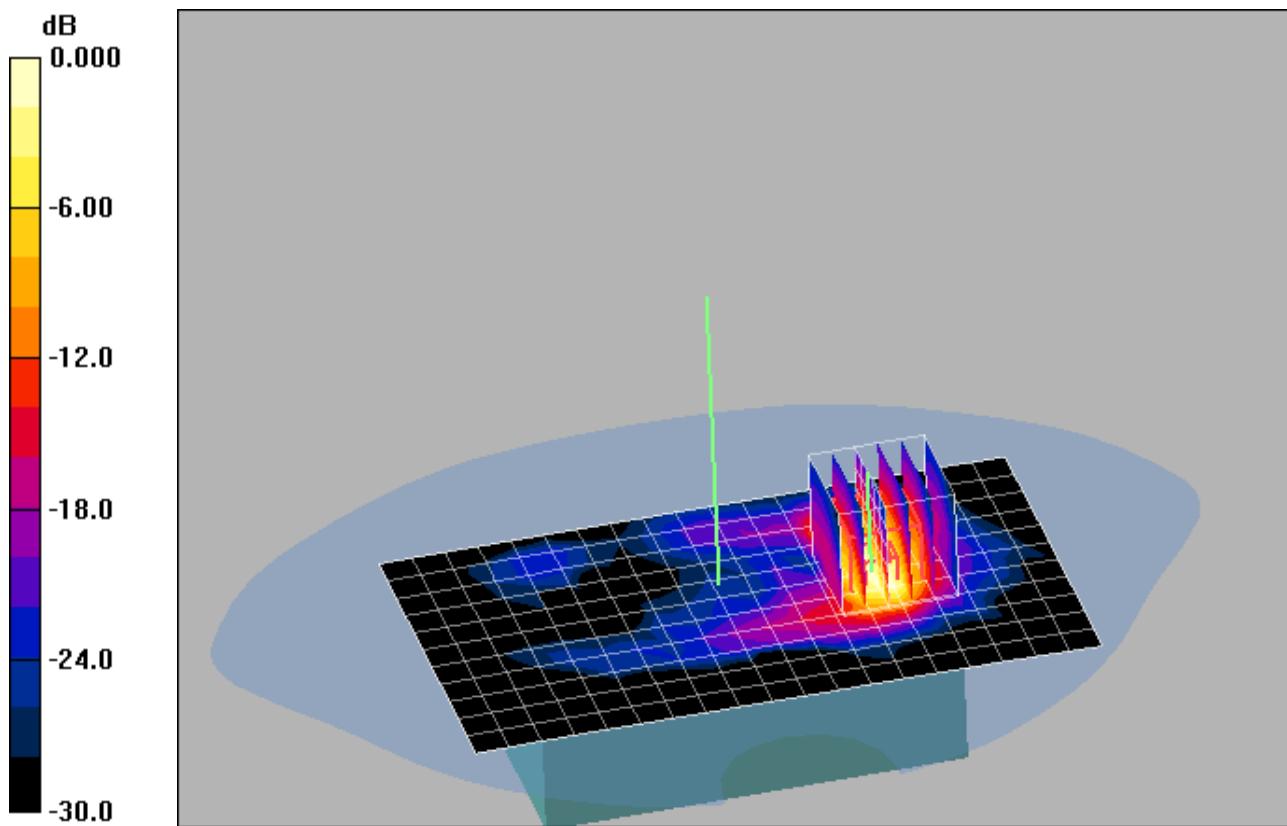

0 dB = 1.04mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/6/2010 5:42:31 PM

Test Laboratory: Intertek ETL Semko
File Name: [CH 6 802.11b 5.5 Mbps Scan Front Side.da4](#)

DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified
Program Name: Different Test Procedures (Left-Hand Side)

Communication System: 802.11b/g; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437$ MHz; $\sigma = 2.01$ mho/m; $\epsilon_r = 52$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186


Cube7x7x7 - Flat Phantom/Area Scan (12x20x1): Measurement grid: dx=10mm, dy=10mm
Maximum value of SAR (measured) = 1.37 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: dx=7mm, dy=7mm, dz=7mm
Reference Value = 1.63 V/m; Power Drift = 0.055 dB
Peak SAR (extrapolated) = 3.06 W/kg
SAR(1 g) = 1.22 mW/g; SAR(10 g) = 0.466 mW/g
Maximum value of SAR (measured) = 1.81 mW/g

Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: dx=20mm, dy=20mm, dz=20mm
Maximum value of SAR (measured) = 0.007 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

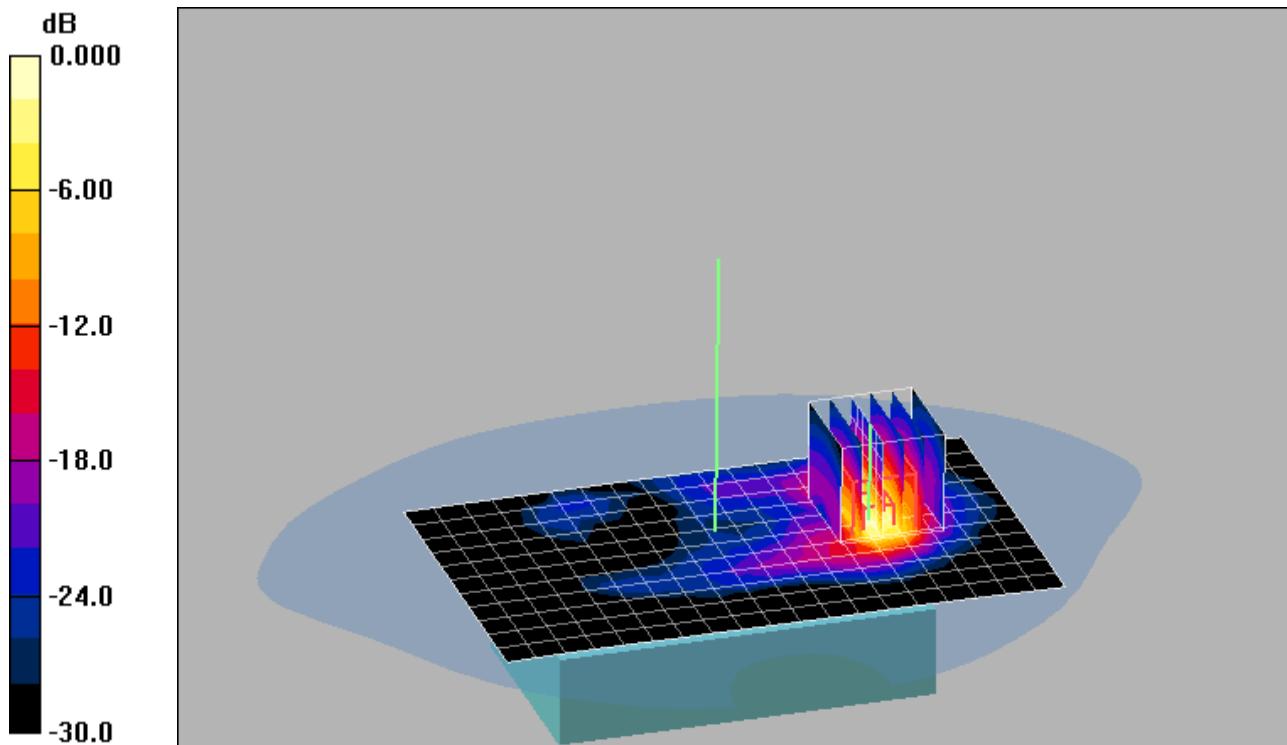

0 dB = 1.81mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/6/2010 10:40:01 PM

Test Laboratory: Intertek ETL Semko
File Name: [CH 6 802.11b 11 Mbps Scan Front Side.da4](#)

DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified
Program Name: Different Test Procedures (Left-Hand Side)

Communication System: 802.11b/g; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437 \text{ MHz}$; $\sigma = 2.01 \text{ mho/m}$; $\epsilon_r = 52$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186


Cube7x7x7 - Flat Phantom/Area Scan (12x20x1): Measurement grid: $dx=10\text{mm}$, $dy=10\text{mm}$
Maximum value of SAR (measured) = 1.01 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: $dx=7\text{mm}$, $dy=7\text{mm}$, $dz=7\text{mm}$
Reference Value = 1.23 V/m; Power Drift = -0.210 dB
Peak SAR (extrapolated) = 1.56 W/kg
SAR(1 g) = 0.667 mW/g; SAR(10 g) = 0.258 mW/g
Maximum value of SAR (measured) = 0.998 mW/g

Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: $dx=20\text{mm}$, $dy=20\text{mm}$, $dz=20\text{mm}$
Maximum value of SAR (measured) = 0.004 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

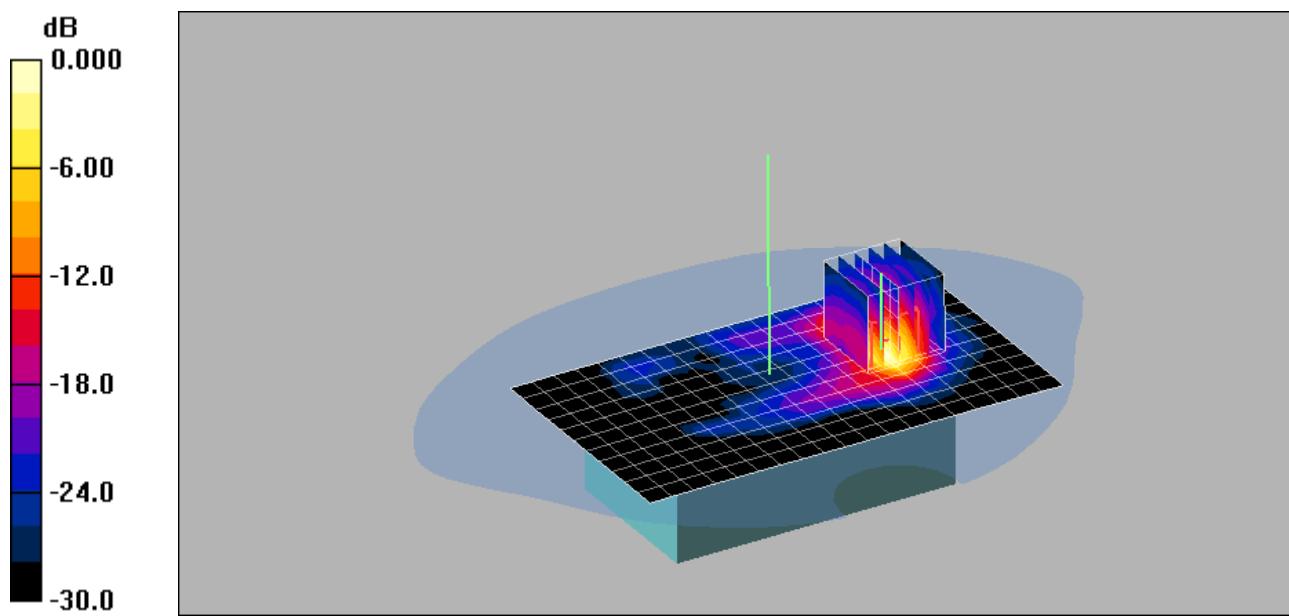

0 dB = 0.998mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/6/2010 11:16:54 PM

Test Laboratory: Intertek ETL Semko
File Name: [CH 11 802.11b 5.5 Mbps Scan Front Side.da4](#)

DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified
Program Name: Different Test Procedures (Left-Hand Side)

Communication System: 802.11b/g; Frequency: 2462 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2462 \text{ MHz}$; $\sigma = 2.05 \text{ mho/m}$; $\epsilon_r = 51.9$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186


Cube7x7x7 - Flat Phantom/Area Scan (12x20x1): Measurement grid: $dx=10\text{mm}$, $dy=10\text{mm}$
Maximum value of SAR (measured) = 1.89 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: $dx=7\text{mm}$, $dy=7\text{mm}$, $dz=7\text{mm}$
Reference Value = 1.84 V/m; Power Drift = -0.198 dB
Peak SAR (extrapolated) = 3.73 W/kg
SAR(1 g) = 1.45 mW/g; SAR(10 g) = 0.534 mW/g
Maximum value of SAR (measured) = 2.13 mW/g


Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: $dx=20\text{mm}$, $dy=20\text{mm}$, $dz=20\text{mm}$
Maximum value of SAR (measured) = 0.007 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

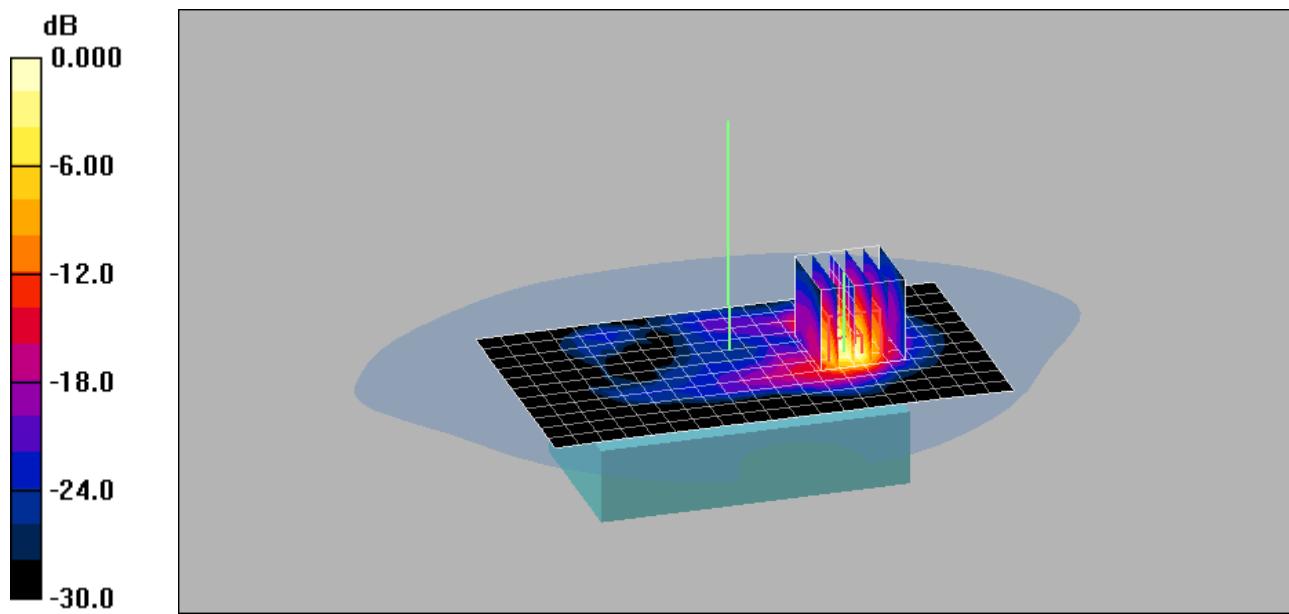

0 dB = 1.89mW/g

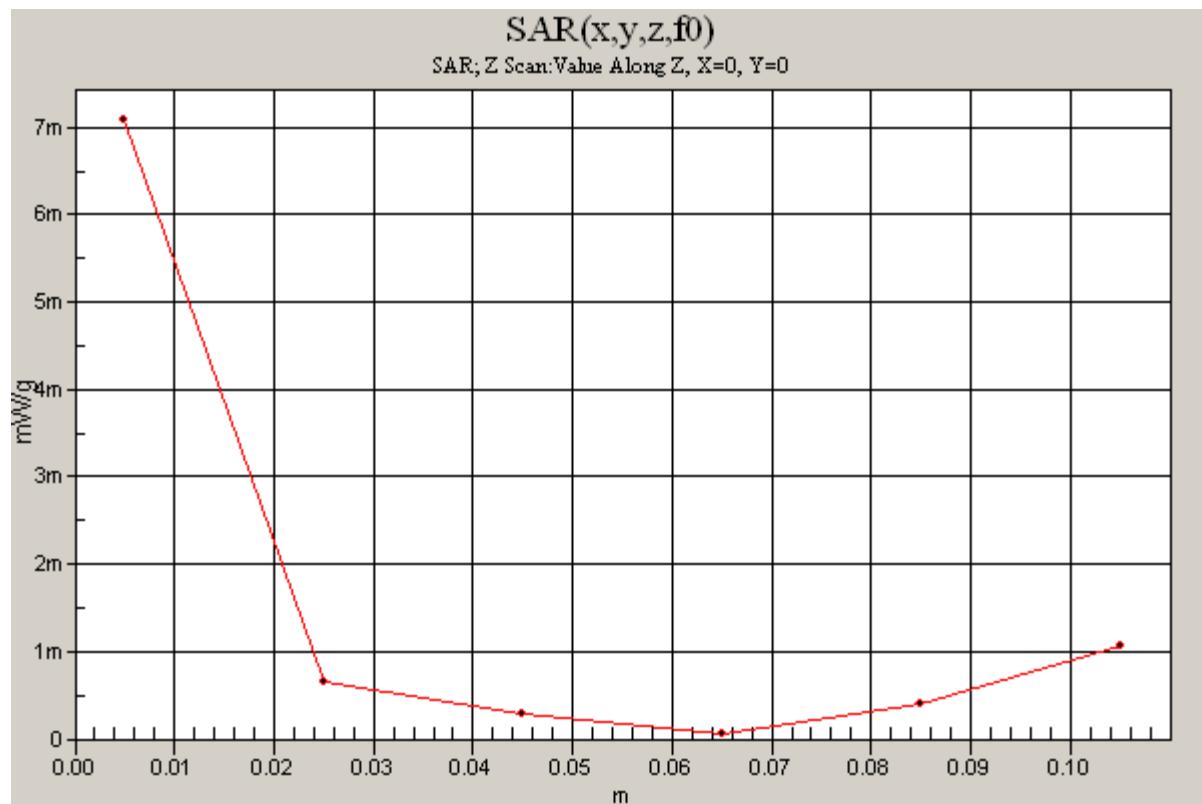

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/6/2010 11:50:21 PM

Test Laboratory: Intertek ETL Semko
File Name: [CH 1 802.11b 5.5 Mbps Scan Front Side.da4](#)

DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified
Program Name: Different Test Procedures (Left-Hand Side)

Communication System: 802.11b/g; Frequency: 2412 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2412 \text{ MHz}$; $\sigma = 1.98 \text{ mho/m}$; $\epsilon_r = 52.1$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186


Cube7x7x7 - Flat Phantom/Area Scan (12x20x1): Measurement grid: $dx=10\text{mm}$, $dy=10\text{mm}$
Maximum value of SAR (measured) = 0.849 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: $dx=7\text{mm}$, $dy=7\text{mm}$, $dz=7\text{mm}$
Reference Value = 1.20 V/m; Power Drift = 0.095 dB
Peak SAR (extrapolated) = 1.50 W/kg
SAR(1 g) = 0.612 mW/g; SAR(10 g) = 0.240 mW/g
Maximum value of SAR (measured) = 0.917 mW/g

Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: $dx=20\text{mm}$, $dy=20\text{mm}$, $dz=20\text{mm}$
Maximum value of SAR (measured) = 0.004 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

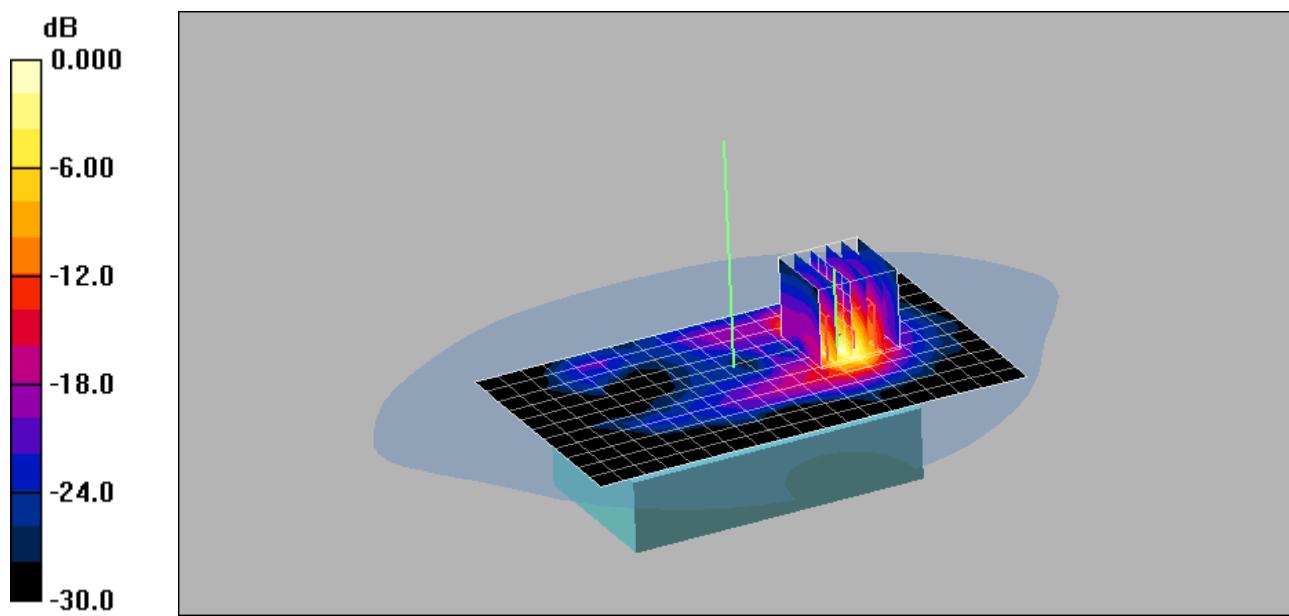

0 dB = 0.849mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/10/2010 5:39:53 PM

Test Laboratory: Intertek ETL Semko

File Name: [CH 2 802.11b 5.5 Mbps Scan Front Side DUT antenna centered in phantom.da4](#)

DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified

Program Name: Different Test Procedures (Left-Hand Side)

Communication System: 802.11b/g; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 2462 \text{ MHz}$; $\sigma = 2.04 \text{ mho/m}$; $\epsilon_r = 51.2$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Cube7x7x7 - Flat Phantom/Area Scan (12x13x1): Measurement grid: $dx=10\text{mm}$, $dy=10\text{mm}$
Maximum value of SAR (measured) = 0.953 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: $dx=7\text{mm}$, $dy=7\text{mm}$, $dz=7\text{mm}$

Reference Value = 18.8 V/m; Power Drift = 0.170 dB

Peak SAR (extrapolated) = 2.51 W/kg

SAR(1 g) = 1.02 mW/g; SAR(10 g) = 0.397 mW/g


Maximum value of SAR (measured) = 1.49 mW/g

Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: $dx=20\text{mm}$, $dy=20\text{mm}$, $dz=20\text{mm}$

Maximum value of SAR (measured) = 0.795 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

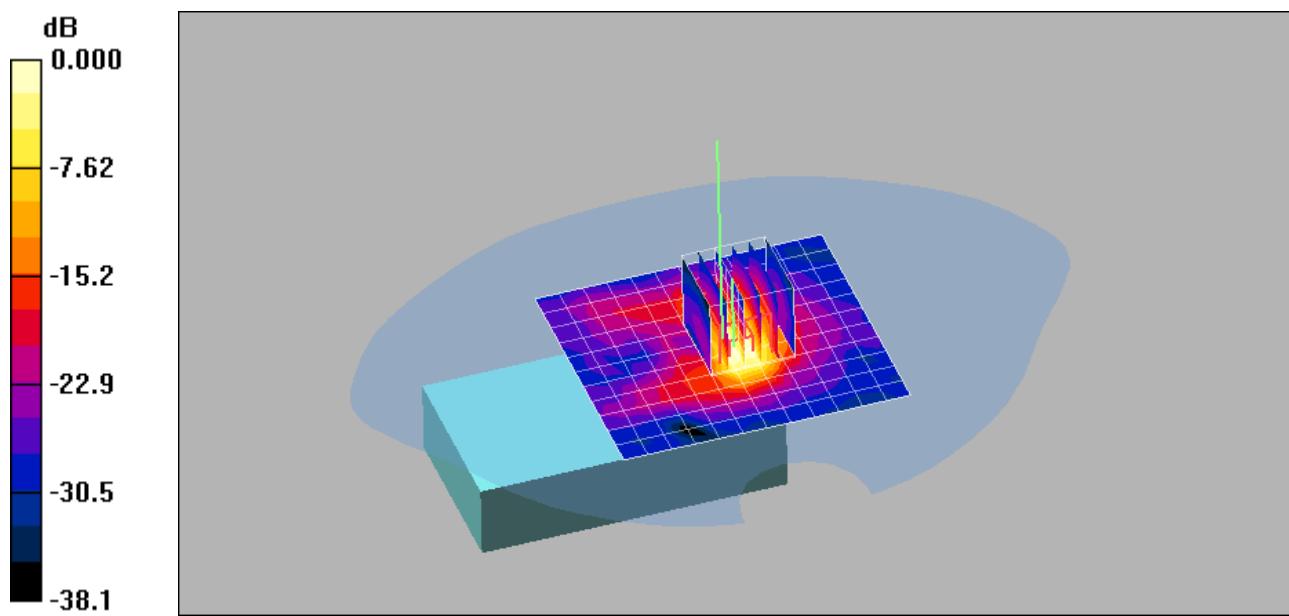

0 dB = 0.953mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/8/2010 11:28:23 AM

Test Laboratory: Intertek ETL Semko
File Name: [CH 39 Bluetooth Front Side.da4](#)

DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified
Program Name: Different Test Procedures (Left-Hand Side)

Communication System: Bluetooth; Frequency: 2441 MHz; Duty Cycle: 1:1
Medium parameters used (interpolated): $f = 2441$ MHz; $\sigma = 2$ mho/m; $\epsilon_r = 51.2$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Cube7x7x7 - Flat Phantom/Area Scan (12x20x1): Measurement grid: dx=10mm, dy=10mm

Info: Interpolated medium parameters used for SAR evaluation.
Maximum value of SAR (measured) = 0.003 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: dx=7mm, dy=7mm, dz=7mm

Reference Value = 0.316 V/m; Power Drift = 0.158 dB

Peak SAR (extrapolated) = 0.008 W/kg

SAR(1 g) = 0.00246 mW/g; SAR(10 g) = 0.000649 mW/g


Info: Interpolated medium parameters used for SAR evaluation.
Maximum value of SAR (measured) = 0.004 mW/g

Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: dx=20mm, dy=20mm, dz=20mm

Info: Interpolated medium parameters used for SAR evaluation.
Maximum value of SAR (measured) = 0.001 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

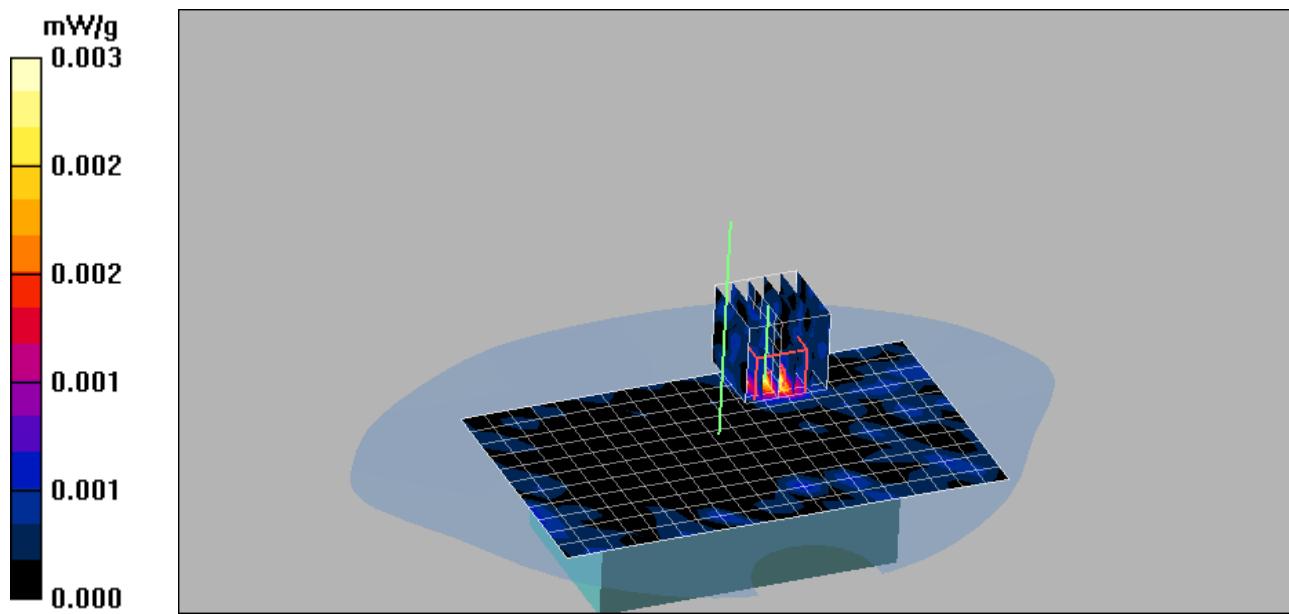

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/8/2010 1:20:15 PM

Test Laboratory: Intertek ETL Semko
File Name: CH 39 Bluetooth Left Side.da4

DUT: Masimo Labs G1; Type: Not Specified; Serial: Not Specified
Program Name: Different Test Procedures (Left-Hand Side)

Communication System: Bluetooth; Frequency: 2441 MHz; Duty Cycle: 1:1
Medium parameters used (interpolated): $f = 2441$ MHz; $\sigma = 2$ mho/m; $\epsilon_r = 51.2$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 2.7mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Cube7x7x7 - Flat Phantom/Area Scan (7x20x1): Measurement grid: dx=10mm, dy=10mm

Info: Interpolated medium parameters used for SAR evaluation.
Maximum value of SAR (measured) = 0.003 mW/g

Cube7x7x7 - Flat Phantom/Zoom Scan (6x6x6)/Cube 0: Measurement grid: dx=7mm, dy=7mm, dz=7mm

Reference Value = 0.198 V/m; Power Drift = 9.76 dB

Peak SAR (extrapolated) = 0.007 W/kg

SAR(1 g) = 0.0025 mW/g; SAR(10 g) = 0.000904 mW/g


Info: Interpolated medium parameters used for SAR evaluation.
Maximum value of SAR (measured) = 0.004 mW/g

Cube7x7x7 - Flat Phantom/Z Scan (1x1x6): Measurement grid: dx=20mm, dy=20mm, dz=20mm

Info: Interpolated medium parameters used for SAR evaluation.
Maximum value of SAR (measured) = 0.001 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

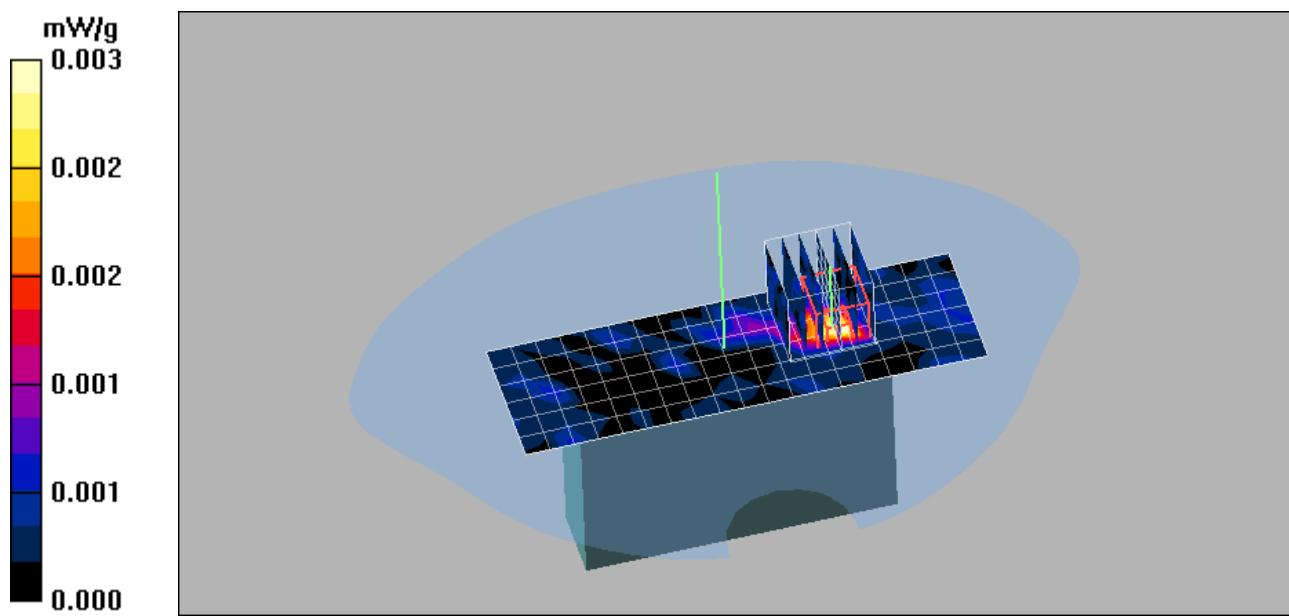

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

12.0 DIPOLE VALIDATION SCANS

Date/Time: 1/6/2010 1:40:56 PM

Test Laboratory: Intertek ETL Semko
File Name: [Dipole Validation 1_6_2010.da4](#)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:718
Program Name: System Performance Check at 2450 MHz

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 2.03$ mho/m; $\epsilon_r = 51.9$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186



d=10mm, Pin=10mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (measured) = 0.365 mW/g

d=10mm, Pin=10mW/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 15.9 V/m; Power Drift = -0.017 dB
Peak SAR (extrapolated) = 104.2 W/kg
SAR(1 g) = 48.2 mW/g; SAR(10 g) = 21.8 mW/g
Normalized to target power = 1 W and actual power = 0.01 W
Maximum value of SAR (measured) = 55.1 mW/g

d=10mm, Pin=10mW/Z Scan (1x1x6): Measurement grid: dx=20mm, dy=20mm, dz=20mm
Maximum value of SAR (measured) = 0.582 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

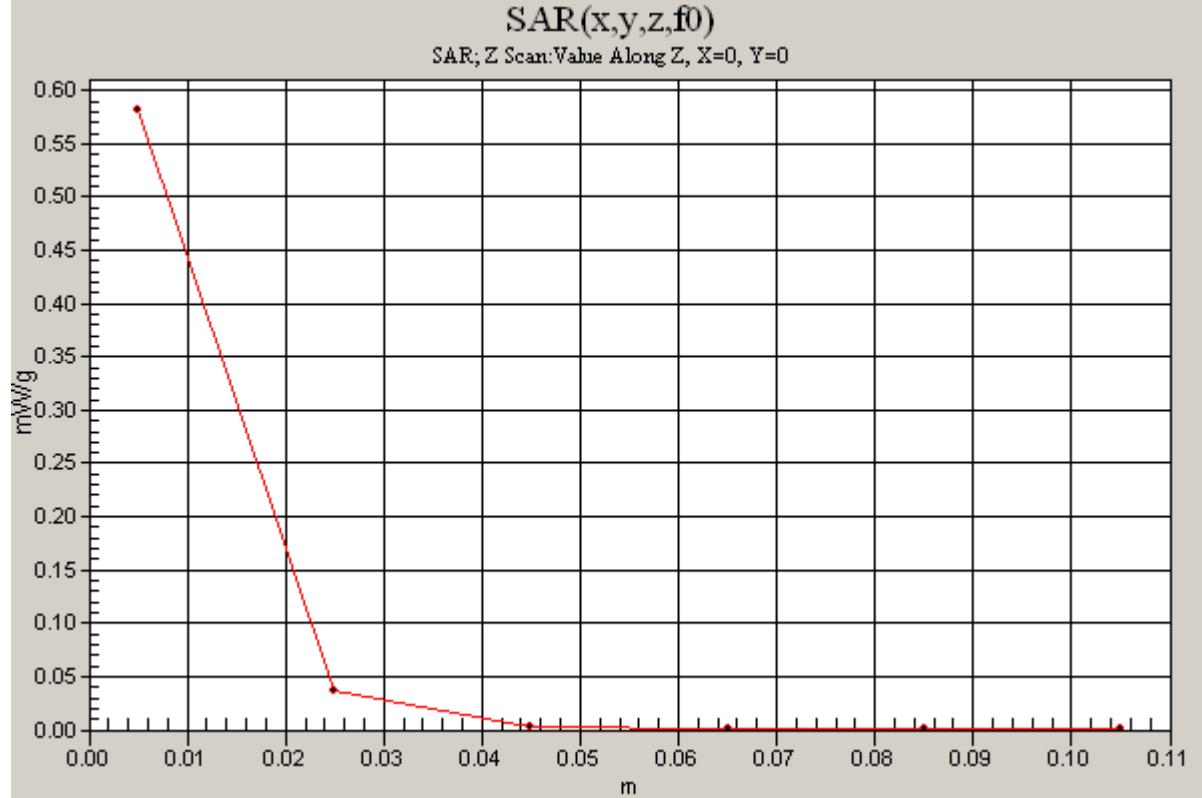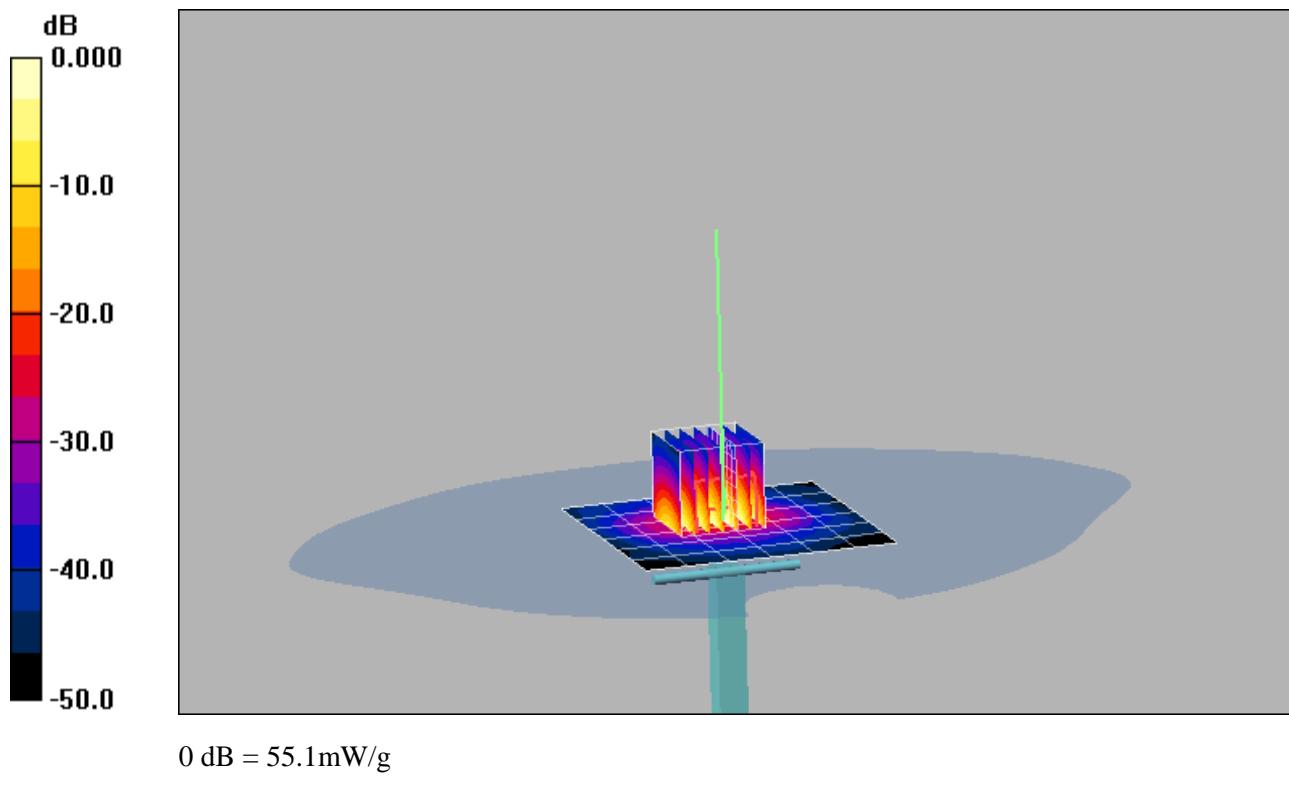

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/8/2010 10:23:22 AM

Test Laboratory: Intertek ETL Semko
File Name: [Dipole Validation 1_8_2010.da4](#)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:718
Program Name: System Performance Check at 2450 MHz

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450 \text{ MHz}$; $\sigma = 2.02 \text{ mho/m}$; $\epsilon_r = 51.1$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

d=10mm, Pin=10mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (measured) = 0.377 mW/g


d=10mm, Pin=10mW/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 16.2 V/m; Power Drift = 0.068 dB
Peak SAR (extrapolated) = 99.5 W/kg

SAR(1 g) = 47.6 mW/g; SAR(10 g) = 21.7 mW/g
Normalized to target power = 1 W and actual power = 0.01 W
Maximum value of SAR (measured) = 53.9 mW/g


d=10mm, Pin=10mW/Z Scan (1x1x6): Measurement grid: dx=20mm, dy=20mm, dz=20mm
Maximum value of SAR (measured) = 0.589 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

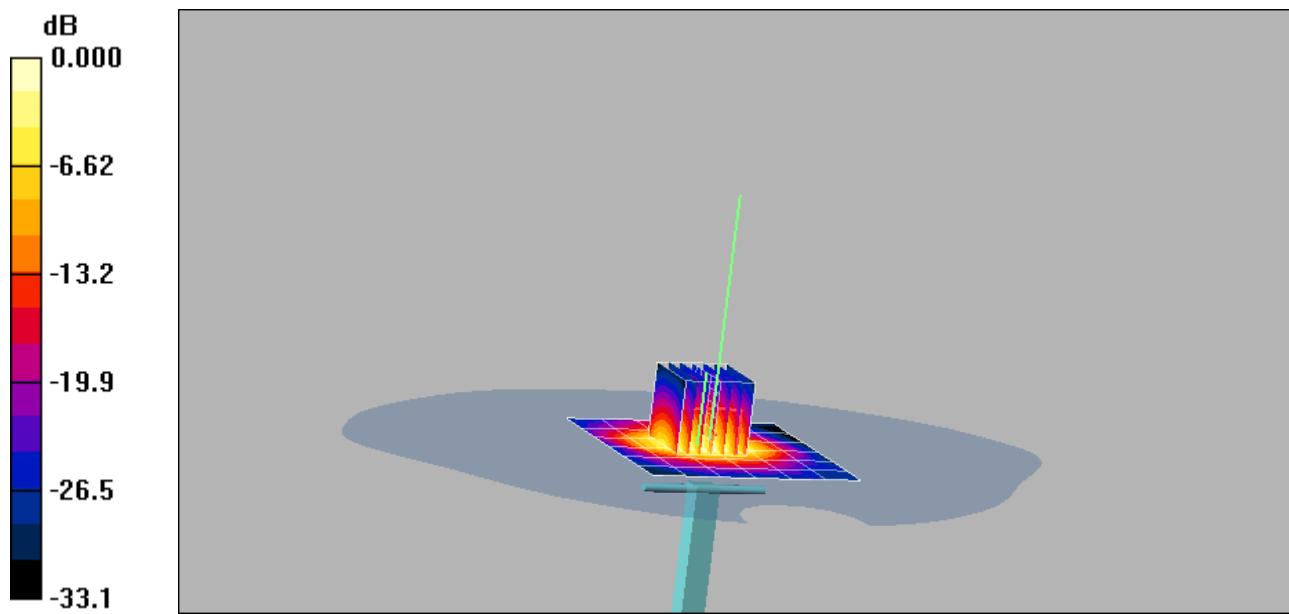

0 dB = 0.377mW/g

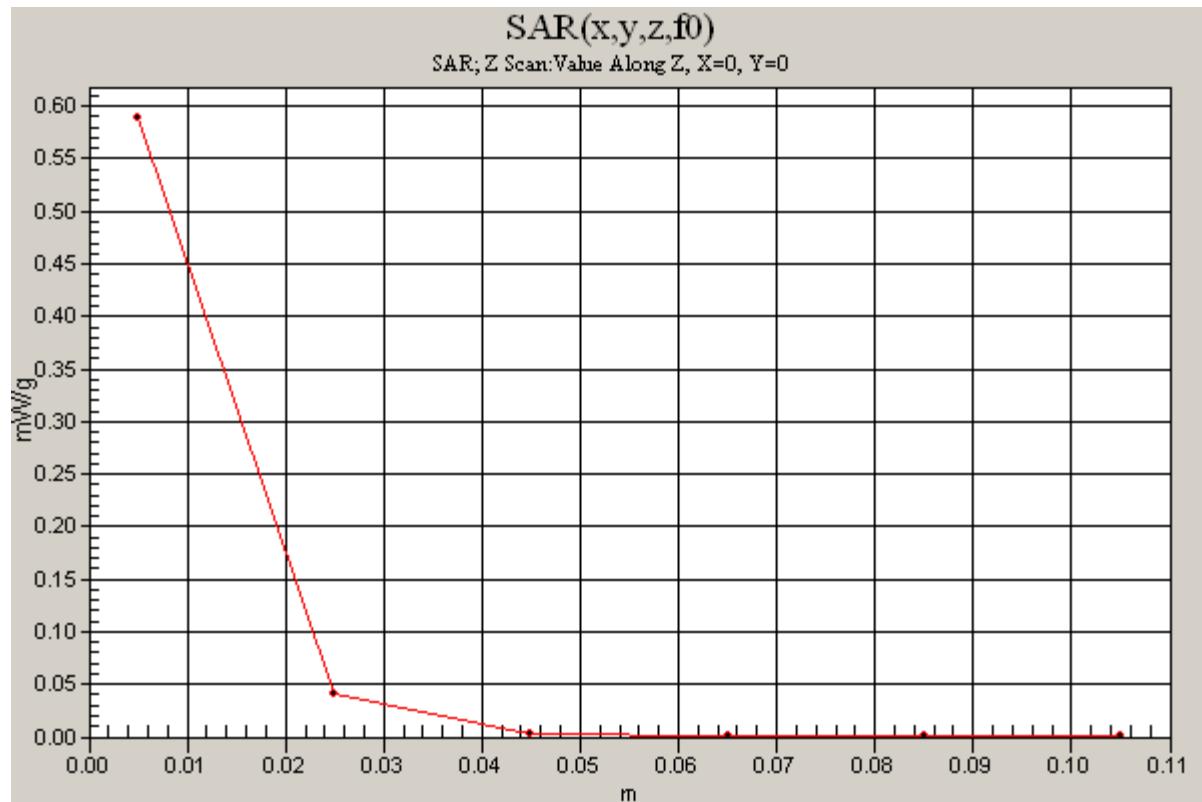

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Date/Time: 1/10/2010 10:36:50 AM

Test Laboratory: Intertek ETL Semko
File Name: [Dipole Validation 1_10_2010.da4](#)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:718
Program Name: System Performance Check at 2450 MHz

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 2.02$ mho/m; $\epsilon_r = 51.3$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 - SN3516; ConvF(8.22, 8.22, 8.22); Calibrated: 12/15/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection) Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE4 Sn358; Calibrated: 4/17/2009
- Phantom: SAM with CRP; Type: SAM; Serial: TP-1243
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

d=10mm, Pin=10mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (measured) = 0.427 mW/g


d=10mm, Pin=10mW/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 16.7 V/m; Power Drift = 0.093 dB
Peak SAR (extrapolated) = 114.5 W/kg

SAR(1 g) = 54.4 mW/g; SAR(10 g) = 24.8 mW/g
Normalized to target power = 1 W and actual power = 0.01 W
Maximum value of SAR (measured) = 61.7 mW/g


d=10mm, Pin=10mW/Z Scan (1x1x6): Measurement grid: dx=20mm, dy=20mm, dz=20mm
Maximum value of SAR (measured) = 0.624 mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

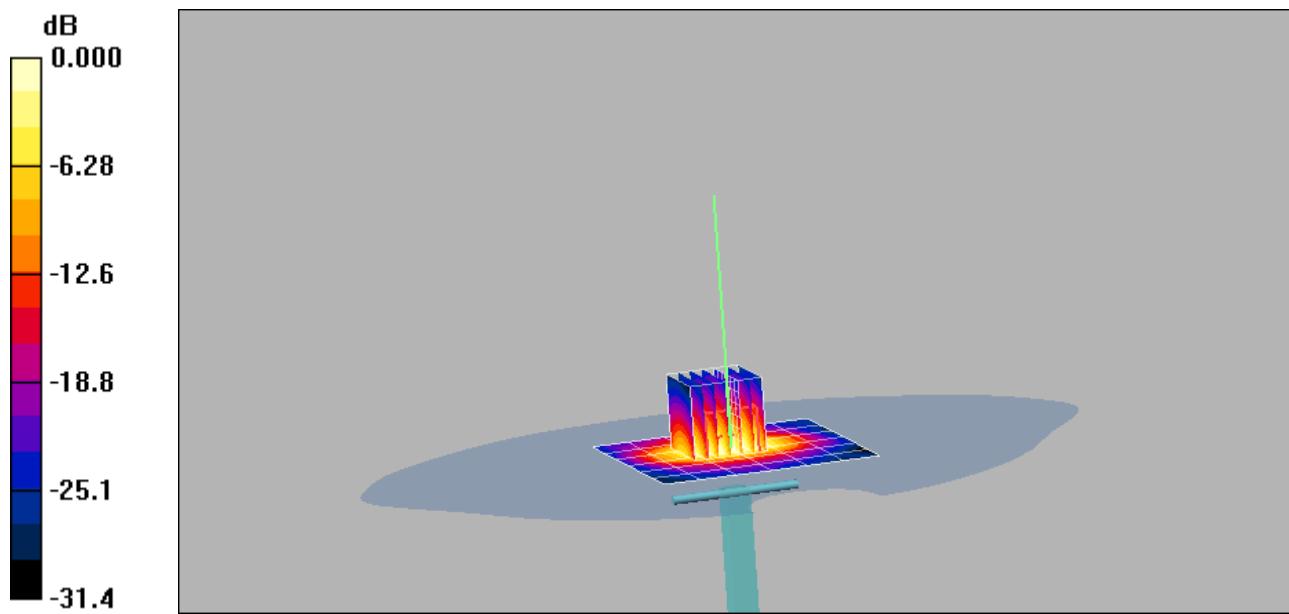

0 dB = 0.427mW/g

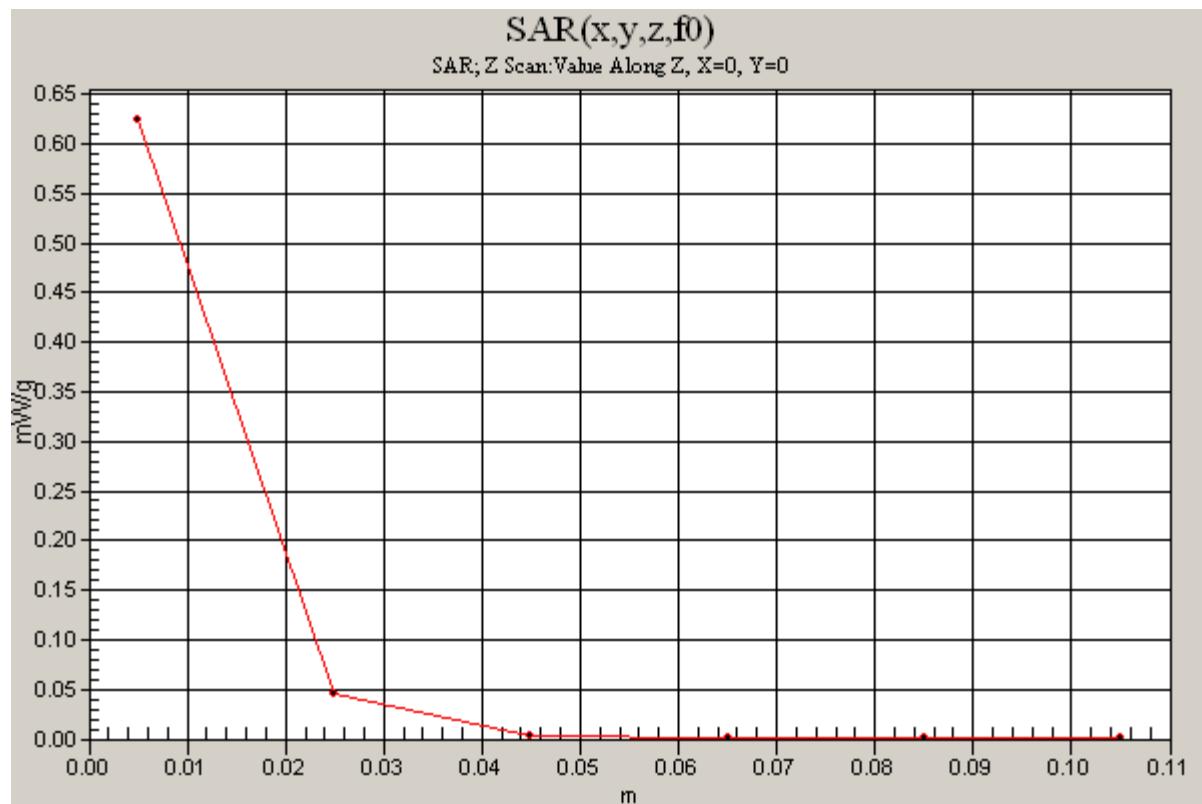

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

13.0 PROBE CERTIFICATE

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client **Intertek**

Certificate No: EX3-3516_Dec09

CALIBRATION CERTIFICATE

Object	EX3DV3 - SN:3516																																																		
Calibration procedure(s)	QA CAL-01.v6, QA CAL-14.v3, QA CAL-23.v3 and QA CAL-25.v2 Calibration procedure for dosimetric E-field probes																																																		
Calibration date:	December 15, 2009																																																		
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter E4419B</td> <td>GB41293874</td> <td>1-Apr-09 (No. 217-01030)</td> <td>Apr-10</td> </tr> <tr> <td>Power sensor E4412A</td> <td>MY41495277</td> <td>1-Apr-09 (No. 217-01030)</td> <td>Apr-10</td> </tr> <tr> <td>Power sensor E4412A</td> <td>MY41498087</td> <td>1-Apr-09 (No. 217-01030)</td> <td>Apr-10</td> </tr> <tr> <td>Reference 3 dB Attenuator</td> <td>SN: S5054 (3c)</td> <td>31-Mar-09 (No. 217-01026)</td> <td>Mar-10</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: S5086 (20b)</td> <td>31-Mar-09 (No. 217-01028)</td> <td>Mar-10</td> </tr> <tr> <td>Reference 30 dB Attenuator</td> <td>SN: S5129 (30b)</td> <td>31-Mar-09 (No. 217-01027)</td> <td>Mar-10</td> </tr> <tr> <td>Reference Probe ES3DV2</td> <td>SN: 3013</td> <td>2-Jan-09 (No. ES3-3013_Jan09)</td> <td>Jan-10</td> </tr> <tr> <td>DAE4</td> <td>SN: 660</td> <td>29-Sep-09 (No. DAE4-660_Sep09)</td> <td>Sep-10</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>RF generator HP 8648C</td> <td>US3642U01700</td> <td>4-Aug-99 (in house check Oct-09)</td> <td>In house check: Oct-11</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>US37390585</td> <td>18-Oct-01 (in house check Oct-09)</td> <td>In house check: Oct10</td> </tr> </tbody> </table> <p>Calibrated by: Katja Pokovic Function: Technical Manager Signature: </p> <p>Approved by: Niels Kuster Function: Quality Manager Signature: </p> <p>Issued: December 16, 2009</p>				Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Power meter E4419B	GB41293874	1-Apr-09 (No. 217-01030)	Apr-10	Power sensor E4412A	MY41495277	1-Apr-09 (No. 217-01030)	Apr-10	Power sensor E4412A	MY41498087	1-Apr-09 (No. 217-01030)	Apr-10	Reference 3 dB Attenuator	SN: S5054 (3c)	31-Mar-09 (No. 217-01026)	Mar-10	Reference 20 dB Attenuator	SN: S5086 (20b)	31-Mar-09 (No. 217-01028)	Mar-10	Reference 30 dB Attenuator	SN: S5129 (30b)	31-Mar-09 (No. 217-01027)	Mar-10	Reference Probe ES3DV2	SN: 3013	2-Jan-09 (No. ES3-3013_Jan09)	Jan-10	DAE4	SN: 660	29-Sep-09 (No. DAE4-660_Sep09)	Sep-10	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Oct-09)	In house check: Oct-11	Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-09)	In house check: Oct10
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																																																
Power meter E4419B	GB41293874	1-Apr-09 (No. 217-01030)	Apr-10																																																
Power sensor E4412A	MY41495277	1-Apr-09 (No. 217-01030)	Apr-10																																																
Power sensor E4412A	MY41498087	1-Apr-09 (No. 217-01030)	Apr-10																																																
Reference 3 dB Attenuator	SN: S5054 (3c)	31-Mar-09 (No. 217-01026)	Mar-10																																																
Reference 20 dB Attenuator	SN: S5086 (20b)	31-Mar-09 (No. 217-01028)	Mar-10																																																
Reference 30 dB Attenuator	SN: S5129 (30b)	31-Mar-09 (No. 217-01027)	Mar-10																																																
Reference Probe ES3DV2	SN: 3013	2-Jan-09 (No. ES3-3013_Jan09)	Jan-10																																																
DAE4	SN: 660	29-Sep-09 (No. DAE4-660_Sep09)	Sep-10																																																
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																																																
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Oct-09)	In house check: Oct-11																																																
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-09)	In house check: Oct10																																																

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization ϕ	ϕ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- $NORM_{x,y,z}$: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). $NORM_{x,y,z}$ are only intermediate values, i.e., the uncertainties of $NORM_{x,y,z}$ does not effect the E²-field uncertainty inside TSL (see below ConvF).
- $NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response$ (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- $DCP_{x,y,z}$: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- $A_x, y, z; B_x, y, z; C_x, y, z; VR_x, y, z$: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to $NORM_{x,y,z} * ConvF$ whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical Isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

EX3DV3 SN:3516

December 15, 2009

Probe EX3DV3

SN:3516

Manufactured:	March 8, 2004
Last calibrated:	November 13, 2008
Recalibrated:	December 15, 2009

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

EX3DV3 SN:3516

December 15, 2009

DASY - Parameters of Probe: EX3DV3 SN:3516

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μ V/(V/m) ²) ^A	0.86	0.77	0.62	\pm 10.1%
DCP (mV) ^B	92.7	94.5	93.6	

Modulation Calibration Parameters

UID	Communication System Name	PAR		A dB	B dBuV	C	VR mV	Unc ^E (k=2)
10000	CW	0.00	X Y Z	0.00 0.00 0.00	0.00 0.00 0.00	1.00 1.00 1.00	300 300 300	\pm 1.5%

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL. (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the maximum deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

EX3DV3 SN:3516

December 15, 2009

DASY - Parameters of Probe: EX3DV3 SN:3516

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz]	Validity [MHz] ^c	Permittivity	Conductivity	ConvF X	ConvF Y	ConvF Z	Alpha	Depth Unc (k=2)
835	± 50 / ± 100	41.5 ± 5%	0.90 ± 5%	10.65	10.65	10.65	0.67	0.65 ± 11.0%
900	± 50 / ± 100	41.5 ± 5%	0.97 ± 5%	10.35	10.35	10.35	0.63	0.66 ± 11.0%
1750	± 50 / ± 100	40.1 ± 5%	1.37 ± 5%	9.27	9.27	9.27	0.40	0.72 ± 11.0%
1900	± 50 / ± 100	40.0 ± 5%	1.40 ± 5%	9.00	9.00	9.00	0.52	0.67 ± 11.0%
2450	± 50 / ± 100	39.2 ± 5%	1.80 ± 5%	8.15	8.15	8.15	0.30	0.88 ± 11.0%
5200	± 50 / ± 100	36.0 ± 5%	4.66 ± 5%	5.32	5.32	5.32	0.40	1.80 ± 13.1%
5800	± 50 / ± 100	35.3 ± 5%	5.27 ± 5%	4.67	4.67	4.67	0.45	1.80 ± 13.1%

^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

EX3DV3 SN:3516

December 15, 2009

DASY - Parameters of Probe: EX3DV3 SN:3516**Calibration Parameter Determined in Body Tissue Simulating Media**

f [MHz]	Validity [MHz] ^c	Permittivity	Conductivity	ConvF X	ConvF Y	ConvF Z	Alpha	Depth Unc (k=2)
835	± 50 / ± 100	55.2 ± 5%	0.97 ± 5%	10.54	10.54	10.54	0.59	0.70 ± 11.0%
900	± 50 / ± 100	55.0 ± 5%	1.05 ± 5%	10.32	10.32	10.32	0.58	0.72 ± 11.0%
1750	± 50 / ± 100	53.4 ± 5%	1.49 ± 5%	9.16	9.16	9.16	0.45	0.79 ± 11.0%
1900	± 50 / ± 100	53.3 ± 5%	1.52 ± 5%	8.71	8.71	8.71	0.34	0.86 ± 11.0%
2450	± 50 / ± 100	52.7 ± 5%	1.95 ± 5%	8.22	8.22	8.22	0.30	0.95 ± 11.0%
5200	± 50 / ± 100	49.0 ± 5%	5.30 ± 5%	4.18	4.18	4.18	0.60	1.80 ± 13.1%
5800	± 50 / ± 100	48.2 ± 5%	6.00 ± 5%	3.84	3.84	3.84	0.60	1.80 ± 13.1%

^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001


Model Number: Pronto-7X44PRONTO7

EX3DV3 SN:3516

December 15, 2009

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

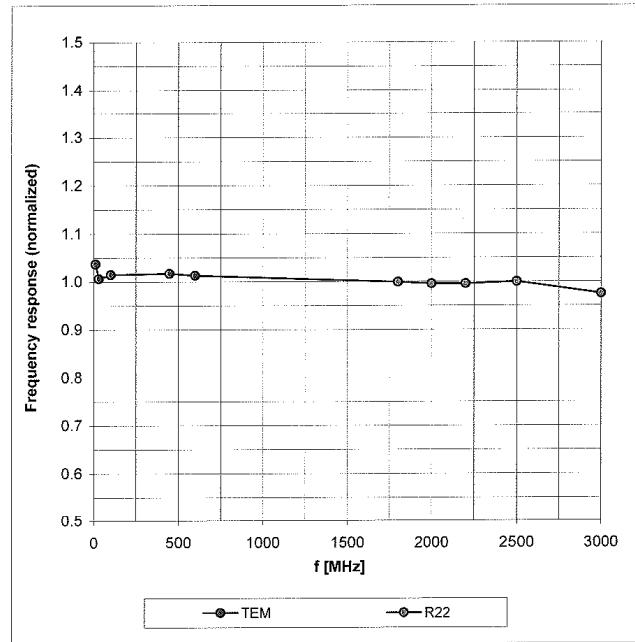



Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

EX3DV3 SN:3516

December 15, 2009

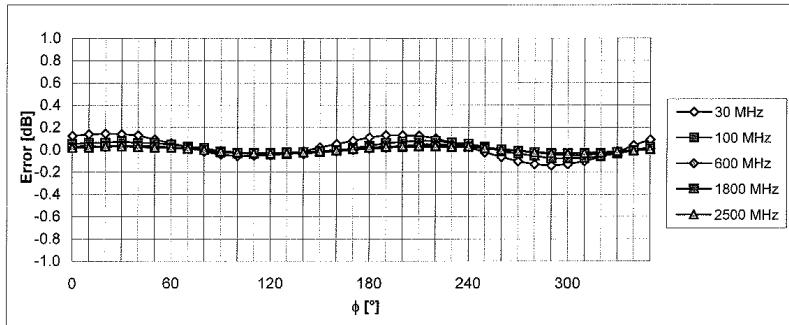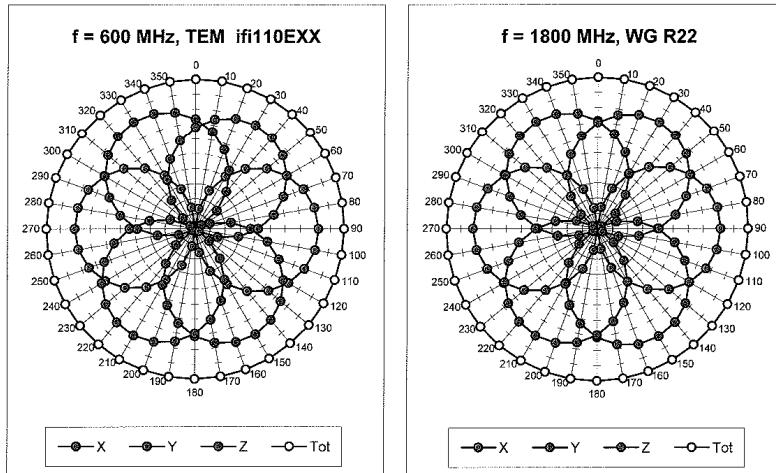Receiving Pattern (ϕ), $\vartheta = 0^\circ$ Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)


Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

EX3DV3 SN:3516

December 15, 2009

Dynamic Range f(SAR_{head})
(Waveguide R22, f = 1800 MHz)

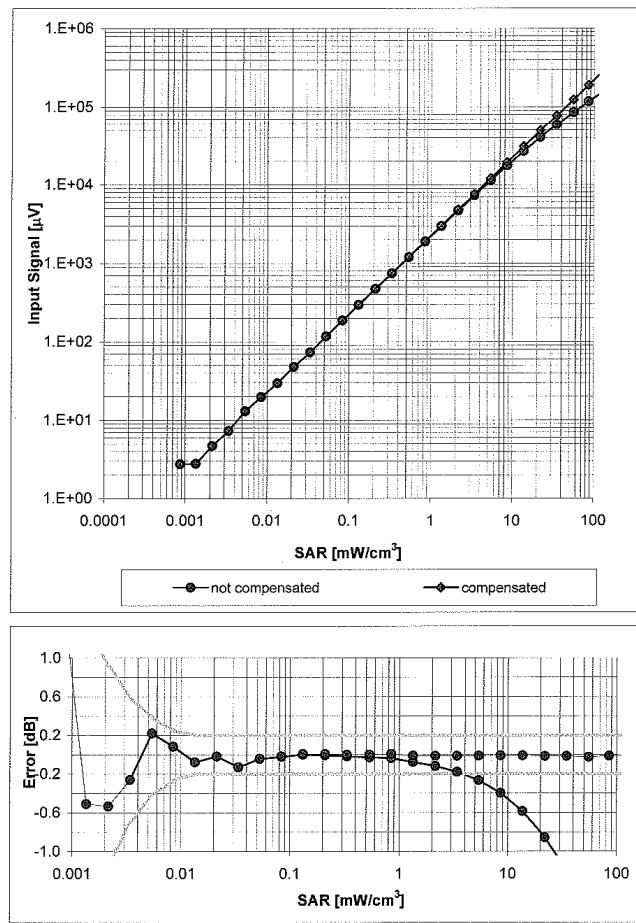

Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)


Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7


EX3DV3 SN:3516

December 15, 2009

Conversion Factor Assessment

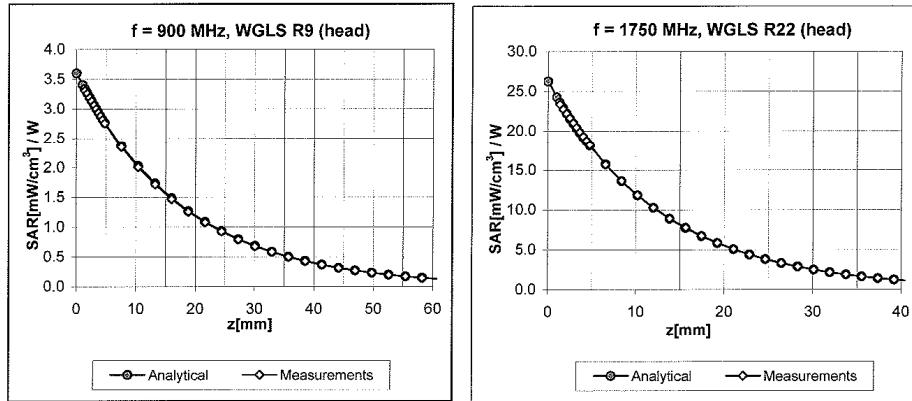

Deviation from Isotropy in HSL

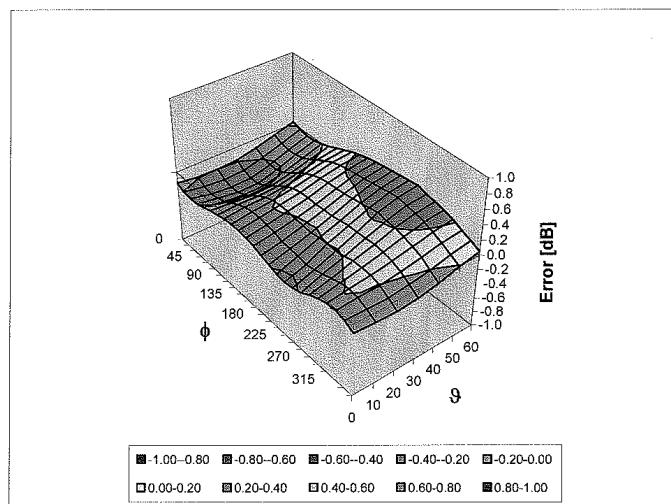Error (ϕ, θ), $f = 900 \text{ MHz}$ Uncertainty of Spherical Isotropy Assessment: $\pm 2.6\%$ ($k=2$)

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

EX3DV3 SN:3516

December 15, 2009

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

14.0 DIPOLE CERTIFICATE

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Intertek**

Certificate No: **D2450V2-718_Dec09**

CALIBRATION CERTIFICATE

Object **D2450V2 - SN: 718**

Calibration procedure(s) **QA CAL-05.v7**
Calibration procedure for dipole validation kits

Calibration date: **December 10, 2009**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-09 (No. 217-01086)	Oct-10
Power sensor HP 8481A	US37292783	06-Oct-09 (No. 217-01086)	Oct-10
Reference 20 dB Attenuator	SN: 5086 (20g)	31-Mar-09 (No. 217-01025)	Mar-10
Type-N mismatch combination	SN: 5047.2 / 06327	31-Mar-09 (No. 217-01029)	Mar-10
Reference Probe ES3DV3	SN: 3205	26-Jun-09 (No. ES3-3205_Jun09)	Jun-10
DAE4	SN: 601	07-Mar-09 (No. DAE4-601_Mar09)	Mar-10

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-09)	In house check: Oct-10

Calibrated by: Name **Jeton Kastrati** Function **Laboratory Technician** Signature

Approved by: Name **Katja Pokovic** Function **Technical Manager** Signature

Issued: December 16, 2009

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.3 ± 6 %	1.82 mho/m ± 6 %
Head TSL temperature during test	(21.4 ± 0.2) °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.4 mW / g
SAR normalized	normalized to 1W	53.6 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	53.3 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	6.31 mW / g
SAR normalized	normalized to 1W	25.2 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	25.2 mW / g ± 16.5 % (k=2)

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.6 ± 6 %	2.01 mho/m ± 6 %
Body TSL temperature during test	(21.5 ± 0.2) °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.7 mW / g
SAR normalized	normalized to 1W	50.8 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	50.2 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	5.82 mW / g
SAR normalized	normalized to 1W	23.3 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	23.2 mW / g ± 16.5 % (k=2)

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$54.2 \Omega + 2.8 j\Omega$
Return Loss	- 26.3 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$50.1 \Omega + 4.5 j\Omega$
Return Loss	- 26.9 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.147 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	September 10, 2002

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

DASY5 Validation Report for Head TSL

Date/Time: 09.12.2009 12:32:31

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:718

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U11 BB

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.82$ mho/m; $\epsilon_r = 39.4$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 26.06.2009
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57


Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 100.3 V/m; Power Drift = 0.052 dB

Peak SAR (extrapolated) = 27.3 W/kg

SAR(1 g) = 13.4 mW/g; SAR(10 g) = 6.31 mW/g


Maximum value of SAR (measured) = 17.1 mW/g

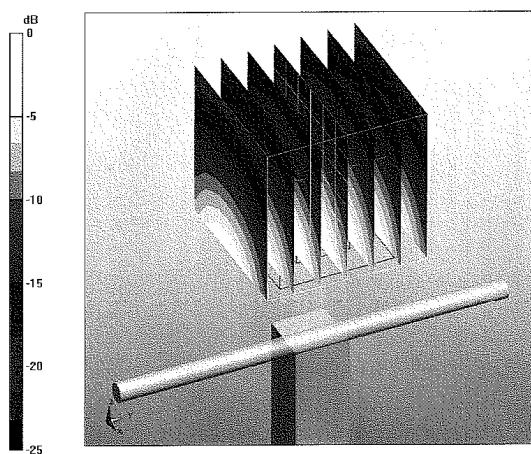

0 dB = 17.1mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

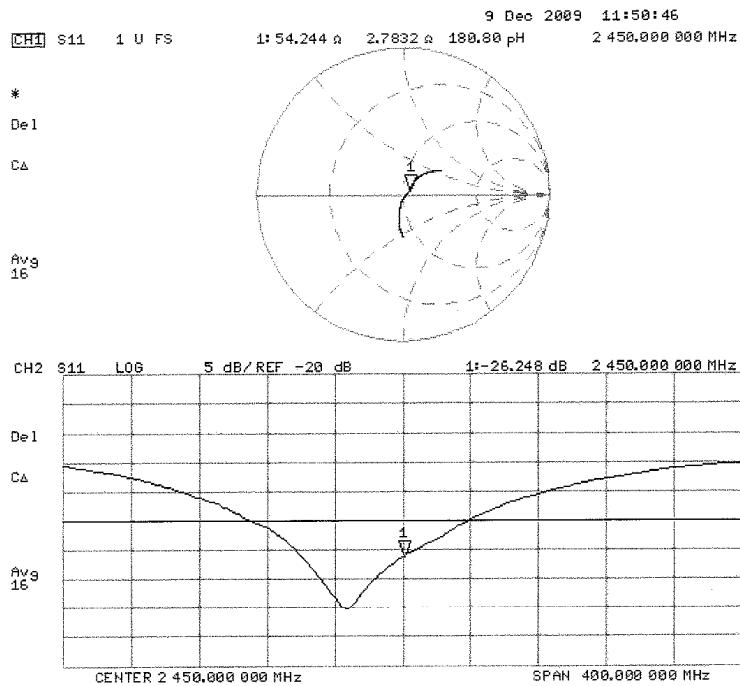Impedance Measurement Plot for Head TSL

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

DASY5 Validation Report for Body

Date/Time: 10.12.2009 13:47:28

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:718

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U10 BB

Medium parameters used: $f = 2450$ MHz; $\sigma = 2.01$ mho/m; $\epsilon_r = 53.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.31, 4.31, 4.31); Calibrated: 26.06.2009
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57


Pin250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94 V/m; Power Drift = 0.051 dB

Peak SAR (extrapolated) = 27.1 W/kg

SAR(1 g) = 12.7 mW/g; SAR(10 g) = 5.82 mW/g

Maximum value of SAR (measured) = 16.8 mW/g

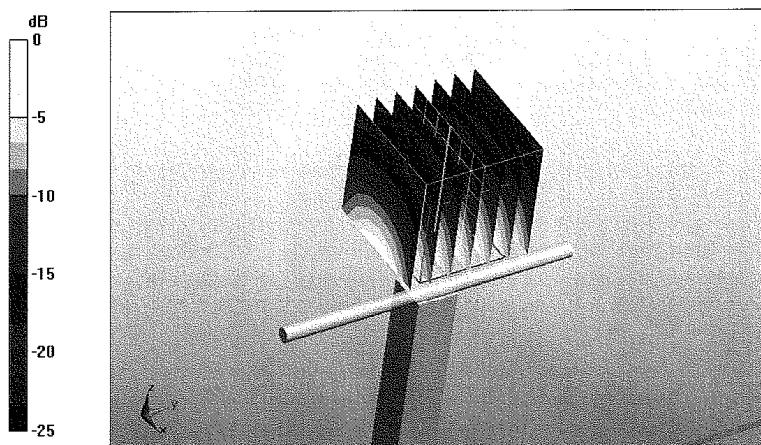


0 dB = 16.8mW/g

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

Impedance Measurement Plot for Body TSL

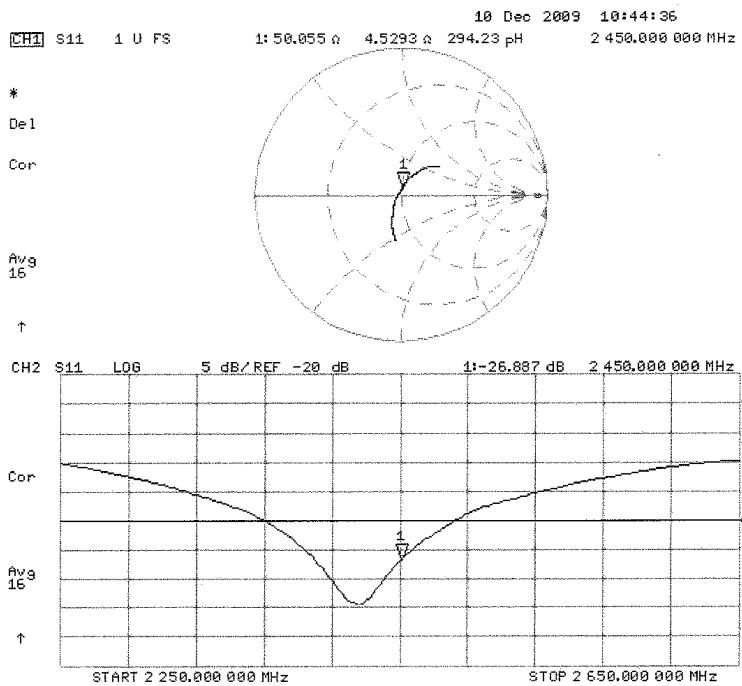

Evaluation For:Masimo Labs
Report Number: 3195108LEX-001

Model Number: Pronto-7X44PRONTO7

15.0 PHANTOM CERTIFICATE

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Certificate of conformity / First Article Inspection

Item	SAM Twin Phantom V4.0
Type No.	QD 000 P40 BA
Series No.	TP-1002 and higher
Manufacturer / Origin	Untersee Composites Hauptstr. 69 CH-8559 Fruthwilen Switzerland

Tests

The series production process used allows the limitation to test of first articles. Complete tests were made on the pre-series Type No. QD 000 P40 AA, Serial No. TP-1001 and on the series first article Type No. QD 000 P40 BA, Serial No. TP-1006. Certain parameters have been retested using further series units (called samples).

Test	Requirement	Details	Units tested
Shape	Compliance with the geometry according to the CAD model.	IT'IS CAD File (*)	First article, Samples
Material thickness	Compliant with the requirements according to the standards	2mm +/- 0.2mm in specific areas	First article, Samples
Material parameters	Dielectric parameters for required frequencies	200 MHz – 3 GHz Relative permittivity < 5 Loss tangent < 0.05	Material sample TP 104-5
Material resistivity	The material has been tested to be compatible with the liquids defined in the standards	Liquid type HSL 1800 and others according to the standard	Pre-series, First article

Standards

- [1] CENELEC EN 50381
- [2] IEEE P1528-200x draft 6.5
- [3] IEC PT 62209 draft 0.9

(*) The IT'IS CAD file is derived from [2] and is also within the tolerance requirements of the shapes of [1] and [3].

Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of SAR measurements specified in standard [1] and draft standards [2] and [3].

Date 18.11.2001

Signature / Stamp