



MEASUREMENT REPORT

FCC PART 15.225


FCC ID: XBG-CL2203

APPLICANT: AVALUE TECHNOLOGY INCORPORATION

Application Type: Certification

Product: Medical Bedside Terminal

Model No.: Medi-View-156, Medi-View-185

Trademark: 

FCC Classification: (DXX) Part 15 Low Power Communication Device Transmitter

FCC Rule Part(s): Part 15.225

Test Procedure(s): ANSI C63.10-2013

Received Date: November 16, 2018

Test Date: November 22, 2018 ~ April 5 ,2020

Tested By : *Fran Chen*
 (Fran Chen)

Reviewed By : *Paddy Chen*
 (Paddy Chen)

Approved By : *Chenz Ker*
 (Chenz Ker)



The test results only relate to the tested sample.

This equipment has been shown to be capable of compliance with the applicable technical standards as indicated in the measurement report and was tested in accordance with the measurement procedures specified in ANSI C63.10-2013. Test results reported herein relate only to the item(s) tested.

The test report shall not be reproduced except in full without the written approval of MRT Technology (Taiwan) Co., Ltd.

Revision History

Report No.	Version	Description	Issue Date	Note
1811TW3101-U1	1.0	Original Report	2020-04-05	

CONTENTS

Description	Page
§2.1033 General Information	5
1. INTRODUCTION	6
1.1. Scope.....	6
1.2. MRT Test Location.....	6
2. PRODUCT INFORMATION	7
2.1. Equipment Description.....	7
2.2. Test Mode.....	7
2.3. Test Software.....	8
2.4. Test Configuration.....	8
2.5. EMI Suppression Device(s)/Modifications.....	8
2.6. Labeling Requirements.....	8
3. DESCRIPTION of TEST	9
3.1. Evaluation Procedure.....	9
3.2. AC Line Conducted Emissions.....	9
3.3. Radiated Emissions.....	10
4. ANTENNA REQUIREMENTS	11
5. TEST EQUIPMENT CALIBRATION DATE	12
6. MEASUREMENT UNCERTAINTY	13
7. TEST RESULT	14
7.1. Summary.....	14
7.2. Field Strength of Fundamental Emissions Measurement.....	15
7.2.1. Test Limit.....	15
7.2.2. Test Procedure used.....	15
7.2.3. Test Setup.....	16
7.2.4. Test Result.....	17
7.3. Radiated Spurious Emissions Measurement.....	19
7.3.1. Test Limit.....	19
7.3.2. Test Procedure Used.....	19
7.3.3. Test Setup.....	21
7.3.4. Test Result.....	22
7.4. 20dB Bandwidth Measurement.....	30
7.4.1. Test Limit.....	30
7.4.2. Test Procedure Used.....	30

7.4.3.	Test Setting.....	30
7.4.4.	Test Setup	30
7.4.5.	Test Result.....	31
7.5.	Frequency Stability Measurement	33
7.5.1.	Test Limit	33
7.5.2.	Test Procedure Used	33
7.5.3.	Test Setup	34
7.5.4.	Test Result.....	35
7.6.	AC Conducted Emissions Measurement	36
7.6.1.	Test Limit	36
7.6.2.	Test Setup	36
7.6.3.	Test Result.....	37
8.	CONCLUSION	41

§2.1033 General Information

Applicant:	AVALUE TECHNOLOGY INCORPORATION
Applicant Address:	7F, 228, Lian-cheng Road, Zhonghe Dist., New Taipei City 235, Taiwan
Manufacturer:	AVALUE TECHNOLOGY INCORPORATION
Manufacturer Address:	7F, 228, Lian-cheng Road, Zhonghe Dist., New Taipei City 235, Taiwan
Test Site:	MRT Technology (Taiwan) Co., Ltd
Test Site Address:	No. 38, Fuxing Second Rd., Guishan Dist., Taoyuan City 333, Taiwan (R.O.C)
MRT FCC Registration No.:	291082
FCC Rule Part(s):	Part 15.225
Model No.:	Medi-View-156, Medi-View-185
Test Device Serial No.:	N/A <input type="checkbox"/> Production <input checked="" type="checkbox"/> Pre-Production <input type="checkbox"/> Engineering

Test Facility / Accreditations

1. MRT facility is a FCC registered (Reg. No. 291082) test facility with the site description report on file and is designated by the FCC as an Accredited Test Firm.
2. MRT facility is an IC registered (MRT Reg. No. 21723) test laboratory with the site description on file at Industry Canada.
3. MRT Lab is accredited to ISO 17025 by the Taiwan Accreditation Foundation (TAF Cert. No. 3261) in EMC, Telecommunications and Radio testing for FCC (Designation Number: TW3261), Industry Taiwan, EU and TELEC Rules.


1. INTRODUCTION

1.1. Scope

Measurement and determination of electromagnetic emissions (EMC) of radio frequency devices including intentional and/or unintentional radiators for compliance with the technical rules and regulations of the Federal Communications Commission and the Industry Canada Certification and Engineering Bureau.


1.2. MRT Test Location

The map below shows the location of the MRT LABORATORY, its proximity to the Taoyuan City. These measurement tests were conducted at the MRT Technology (Taiwan) Co., Ltd. Facility located at No.38, Fuxing 2nd Rd., Guishan Dist., Taoyuan City 33377, Taiwan (R.O.C).

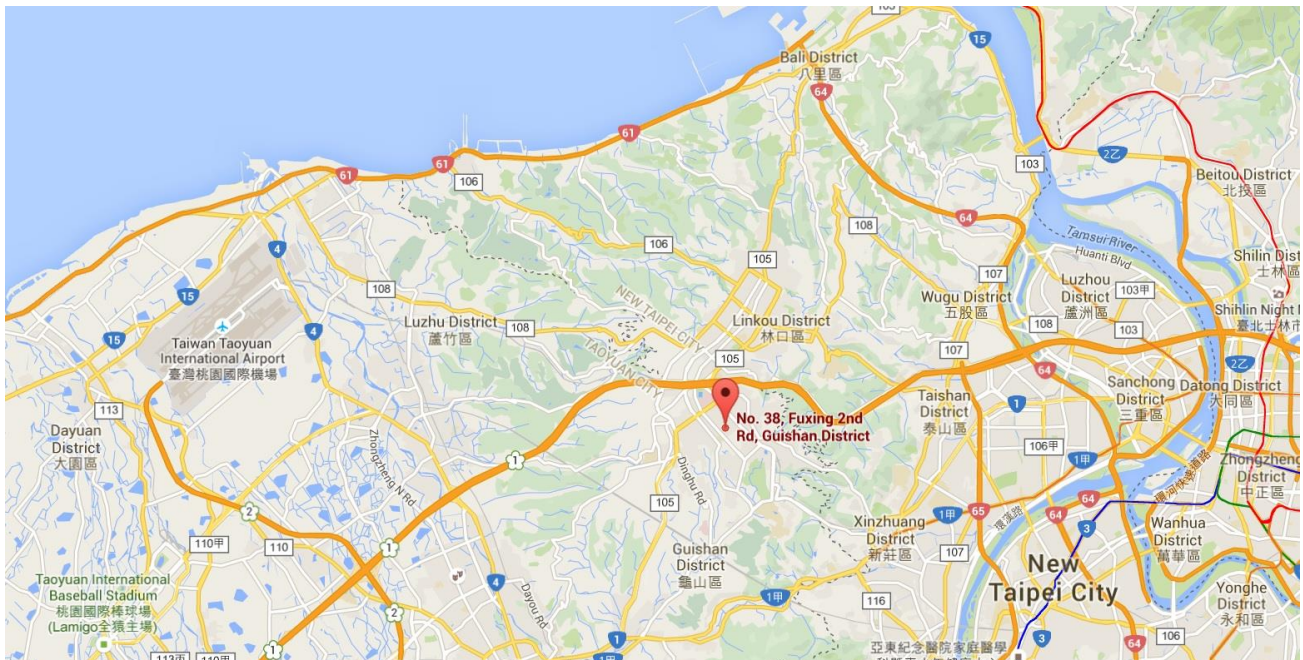

2. PRODUCT INFORMATION

2.1. Equipment Description

Product Name	Medical Bedside Terminal
Trademark	
Model No.	Medi-View-156, Medi-View-185
Module	Synnix / CL-2303M-AV
Antenna Type	Loop Antenna
NFC Specification	13.56MHz
Modulation	ASK
Power Adapter	Brand: EDAC Model No: EA10953E-190 Input: AC 100-240V~2.5A, 50-60Hz Output: DC 19V, 4.73A Cable Out: Non-shielded, 1.5m with Core*1

Note:

Model Difference: The difference of models only for Panel Size (Medi-View-156: 15" / Medi-View-185: 18"), the other hardware was the same.

2.2. Test Mode

Test Mode	Mode 1: Transmit by NFC with Medi-View-185 Mode 2: Transmit by NFC with Medi-View-156
-----------	--

2.3. Test Software

N/A.

2.4. Test Configuration

The **Medical Bedside Terminal**. ANSI C63.10-2013 was used to reference the appropriate EUT setup for radiated spurious emissions testing and AC line conducted testing.

2.5. EMI Suppression Device(s)/Modifications

No EMI suppression device(s) were added and/or no modifications were made during testing.

2.6. Labeling Requirements

Per 2.1074 & 15.19; Docket 95-19

The label shall be permanently affixed at a conspicuous location on the device; instruction manual or pamphlet supplied to the user and be readily visible to the purchaser at the time of purchase. However, when the device is so small wherein placement of the label with specified statement is not practical, only the FCC ID must be displayed on the device per Section 15.19(a)(5). Please see attachment for FCC ID label and label location.

3. DESCRIPTION of TEST

3.1. Evaluation Procedure

The measurement procedures described in the American National Standard for Testing Unlicensed Wireless Devices (ANSI C63.10-2013) were used in the measurement of the **Medical Bedside Terminal**.

Deviation from measurement procedure.....None

3.2. AC Line Conducted Emissions

The line-conducted facility is located inside an 9'x4'x3' shielded enclosure. A 1m x 2m wooden table 80cm high is placed 40cm away from the vertical wall and 80cm away from the sidewall of the shielded room. Two 10kHz-30MHz, 50Ω/50uH Line-Impedance Stabilization Networks (LISNs) are bonded to the shielded room floor. Power to the LISNs is filtered by external high-current high-insertion loss power line filters. These filters attenuate ambient signal noise from entering the measurement lines. These filters are also bonded to the shielded enclosure.

The EUT is powered from one LISN and the support equipment is powered from the second LISN. All interconnecting cables more than 1 meter were shortened to a 1 meter length by non-inductive bundling (serpentine fashion) and draped over the back edge of the test table. All cables were at least 40cm above the horizontal reference ground-plane. Power cables for support equipment were routed down to the second LISN while ensuring that that cables were not draped over the second LISN.

Sufficient time for the EUT, support equipment, and test equipment was allowed in order for them to warm up to their normal operating condition. The RF output of the LISN was connected to the receiver and exploratory measurements were made to determine the frequencies producing the maximum emission from the EUT. The receiver was scanned from 150kHz to 30MHz. The detector function was set to peak mode for exploratory measurements while the bandwidth of the analyzer was set to 9kHz. The EUT, support equipment, and interconnecting cables were arranged and manipulated to maximize each emission. Each emission was also maximized by varying: power lines, the mode of operation or data exchange speed, or support equipment which determined the worst-case emission. Once the worst case emissions have been identified, the one EUT cable configuration/arrangement and mode of operation that produced these emissions are used for final measurements on the same test site. The analyzer is set to CISPR quasi-peak and average detectors with a 9kHz resolution bandwidth for final measurements.

An extension cord was used to connect to a single LISN which powered by EUT. The extension cord was calibrated with LISN, the impedance and insertion loss are compliance with the requirements as stated in ANSI C63.10-2013.

Line conducted emissions test results are shown in Section 7.6.

3.3. Radiated Emissions

The radiated test facilities consisted of an indoor 3 meter semi-anechoic chamber used for final measurements and exploratory measurements, when necessary. The measurement area is contained within the semi-anechoic chamber which is shielded from any ambient interference. For measurements above 1GHz absorbers are arranged on the floor between the turn table and the antenna mast in such a way so as to maximize the reduction of reflections. For measurements below 1GHz, the absorbers are removed. A MF Model 210SS turntable is used for radiated measurement. It is a continuously rotatable, remote controlled, metallic turntable and 2 meters (6.56 ft.) in diameter. The turn table is flush with the raised floor of the chamber in order to maintain its function as a ground plane. An 80cm high PVC support structure is placed on top of the turntable.

For all measurements, the spectrum was scanned through all EUT azimuths and from 1 to 4 meter receive antenna height using a broadband antenna from 30MHz up to the upper frequency shown in 15.33(b)(1) depending on the highest frequency generated or used in the device or on which the device operates or tunes. For frequencies above 1GHz, linearly polarized double ridge horn antennas were used. For frequencies below 30MHz, a calibrated loop antenna was used. When exploratory measurements were necessary, they were performed at 1 meter test distance inside the semi-anechoic chamber using broadband antennas, broadband amplifiers, and spectrum analyzers to determine the frequencies and modes producing the maximum emissions. Sufficient time for the EUT, support equipment, and test equipment was allowed in order for them to warm up to their normal operating condition. The test set-up for frequencies below 1GHz was placed on top of the 0.8 meter high, 1 x 1.5 meter table; and test set-up for frequencies 1-40GHz was placed on top of the 1.5 meter high, 1 x 1.5 meter table. The EUT, support equipment, and interconnecting cables were arranged and manipulated to maximize each emission. Appropriate precaution was taken to ensure that all emissions from the EUT were maximized and investigated. The system configuration, clock speed, mode of operation or video resolution, if applicable, turntable azimuth, and receive antenna height was noted for each frequency found.

Final measurements were made in the semi-anechoic chamber using calibrated, linearly polarized broadband and horn antennas. The test setup was configured to the setup that produced the worst case emissions. The spectrum analyzer was set to investigate all frequencies required for testing to compare the highest radiated disturbances with respect to the specified limits. The turntable containing the EUT was rotated through 360 degrees and the height of the receive antenna was varied 1 to 4 meters and stopped at the azimuth and height producing the maximum emission. Each emission was maximized by changing the orientation of the EUT through three orthogonal planes and changing the polarity of the receive antenna, which produced the worst-case emissions. According to 3dB Beam-Width of horn antenna, the horn antenna should be always directed to the EUT when rising height.

Radiated Emissions test results are shown in Section 7.2 & 7.3 .

4. ANTENNA REQUIREMENTS

Excerpt from §15.203 of the FCC Rules/Regulations:

“An intentional radiator antenna shall be designed to ensure that no antenna other than that furnished by the responsible party can be used with the device. The use of a permanently attached antenna or of an antenna that uses a unique coupling to the intentional radiator shall be considered sufficient to comply with the provisions of this section.”

- The antenna of **Medical Bedside Terminal** is **permanently attached**.
- There are no provisions for connection to an external antenna.

Conclusion:

The **Medical Bedside Terminal** unit complies with the requirement of §15.203.

5. TEST EQUIPMENT CALIBRATION DATE

Conducted Emissions – SR2

Instrument	Manufacturer	Type No.	Asset No.	Cali. Interval	Cali. Due Date
Two-Line V-Network	R&S	ENV216	MRTTWA00019	1 year	2021/3/26
Cable	Rosnol	N1C50-RG400-B 1C50-500CM	MRTTWE00013	1 year	2020/6/18
EMI Test Receiver	R&S	ESR3	MRTTWA00009	1 year	2021/3/25

Radiated Emissions – AC1

Instrument	Manufacturer	Type No.	Asset No.	Cali. Interval	Cali. Due Date
Broadband TRILOG Antenna	SCHWARZBECK	VULB 9162	MRTTWA00001	1 year	2020/6/4
EMI Test Receiver	R&S	ESR3	MRTTWA00009	1 year	2021/3/25
Active Loop Antenna	Schwarzbeck	FMZB 1519B	MRTTWA00002	1 year	2020/4/29
Broadband Horn antenna	SCHWARZBECK	BBHA 9120D	MRTTWA00003	1 year	2020/4/22
Breitband Hornantenna	Schwarzbeck	BBHA 9170	MRTTWA00004	1 year	2020/4/23
Broadband Amplifier	Schwarzbeck	BBV 9721	MRTTWA00006	1 year	2020/4/24
Broadband Preampfier	SCHWARZBECK	BBV 9718	MRTTWA00005	1 year	2020/4/24
Cable	HUBERSUHNER	SF106	MRTTWA00010	1 year	2020/4/22
Cable	Rosnol	K1K50-UP0264- K1K50-4M	MRTTWA00012	1 year	2020/6/18

Conducted Test Equipment – SR2

Instrument	Manufacturer	Type No.	Asset No.	Cali. Interval	Cali. Due Date
Spectrum Analyzer	KEYSIGHT	N9010A	MRTTWA00012	1 year	2020/10/2
USB Wideband Power Sensor	KEYSIGHT	U2021XA	MRTTWA00015	1 year	2021/3/26

Test Software

Software	Version	Function
e3	9.160520a	EMI Test Software
EMI	V3	EMI Test Software

6. MEASUREMENT UNCERTAINTY

Where relevant, the following test uncertainty levels have been estimated for tests performed on the EUT as specified in CISPR 16-4-2. This uncertainty represents an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of $k = 2$.

AC Conducted Emission Measurement – SR2	
Measuring Uncertainty for a Level of Confidence of 95% ($U=2Uc(y)$): 150kHz~30MHz: 2.42dB	
Conducted Measurement– SR1	
Measuring Uncertainty for a Level of Confidence of 95% ($U=2Uc(y)$): 1.3dB	
Radiated Emission Measurement – AC1	
Measuring Uncertainty for a Level of Confidence of 95% ($U=2Uc(y)$):	
Horizontal:	9K~30MHz: 4.14dB
	30MHz~1GHz: 4.22dB
	1GHz~40GHz: 4.05dB
Vertical:	9K~30MHz: 4.14dB
	30MHz~1GHz: 3.37dB
	1GHz~40GHz: 4.08dB

7. TEST RESULT

7.1. Summary

Product Name: Medical Bedside Terminal

FCC Classification: (DXX) Part 15 Low Power Communication Device Transmitter

FCC Part Section(s)	Test Description	Test Limit	Test Condition	Test Result	Reference
15.225 (a)(b)(c)	Field Strength of Fundamental Emissions	FCC 15.225 limits	Radiated	Pass	Section 7.2
15.225(d)	Radiated Spurious Emissions	FCC 15.209 limits		Pass	Section 7.3
2.1049	20dB Bandwidth	N/A	Conducted	Pass	Section 7.4
15.225(e)	Frequency Stability	within $\pm 0.01\%$ of the operating frequency		Pass	Section 7.5
15.207	AC Conducted Emissions 150kHz - 30MHz	FCC 15.207 limits	Line Conducted	Pass	Section 7.6

Notes:

- 1) All modes of operation and data rates were investigated. For radiated emission test, every axis (X, Y, Z) was also verified (When applicable). The test results shown in the following sections represent the worst case emissions.
- 2) The analyzer plots shown in this section were all taken with a correction table loaded into the analyzer. The correction table was used to account for the losses of the cables and attenuators used as part of the system to connect the EUT to the analyzer at all frequencies of interest.
- 3) All antenna port conducted emissions testing was performed on a test bench with the antenna port of the EUT connected to the spectrum analyzer through calibrated cables and attenuators.

7.2. Field Strength of Fundamental Emissions Measurement

7.2.1. Test Limit

FCC Part 15.225 Limits				
Frequency (MHz)	Field Strength ($\mu\text{V/m}$) at 30m	Field Strength ($\text{dB}\mu\text{V/m}$) at 30m	Field Strength ($\text{dB}\mu\text{V/m}$) at 10m	Field Strength ($\text{dB}\mu\text{V/m}$) at 3m
1.705 – 13.110	30	29.5	48.58	69.5
13.110 – 13.410	106	40.5	59.98	80.5
13.410 – 13.553	334	50.5	69.58	90.5
13.553 – 13.567	15848	84	103.08	124
13.567 – 13.710	334	50.5	69.58	90.5
13.710 – 14.010	106	40.5	59.98	80.5
14.010 – 30.000	30	29.5	48.58	69.5

7.2.2. Test Procedure used

ANSI C63.10-2013 - Section 11.12.2.3 (quasi-peak measurements)

ANSI C63.10-2013 - Section 11.12.2.4 (peak power measurements)

ANSI C63.10-2013 - Section 11.12.2.5 (average power measure)

Test Setting


1. Analyzer center frequency was set to the frequency of the radiated spurious emission of interest
2. RBW = as specified in Table 1
3. VBW $\geq 3 \times$ RBW
4. Detector = Peak
5. Trace mode = max hold
6. Sweep = auto couple
7. Allow the trace was allowed to stabilize

Table 1 - RBW as a function of frequency

Frequency	RBW
9 kHz ~ 150 kHz	200 Hz ~ 300 Hz
0.15 MHz ~ 30 MHz	9 kHz ~ 10 kHz


7.2.3. Test Setup

9kHz ~ 30MHz Test Setup:

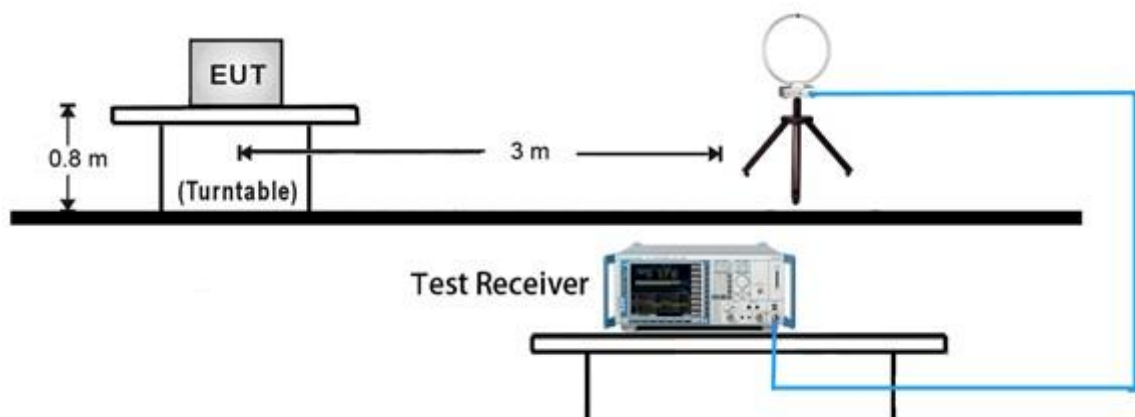

7.2.4. Test Result

EUT	Medical Bedside Terminal	Date of Test	2020/3/22
Factor	FMZB 1519B	Temp. / Humidity	25°C / 57%
Polarity	--	Site / Test Engineer	AC1 / Peter
Test Mode	Mode1	Test Voltage	AC 120V/60Hz

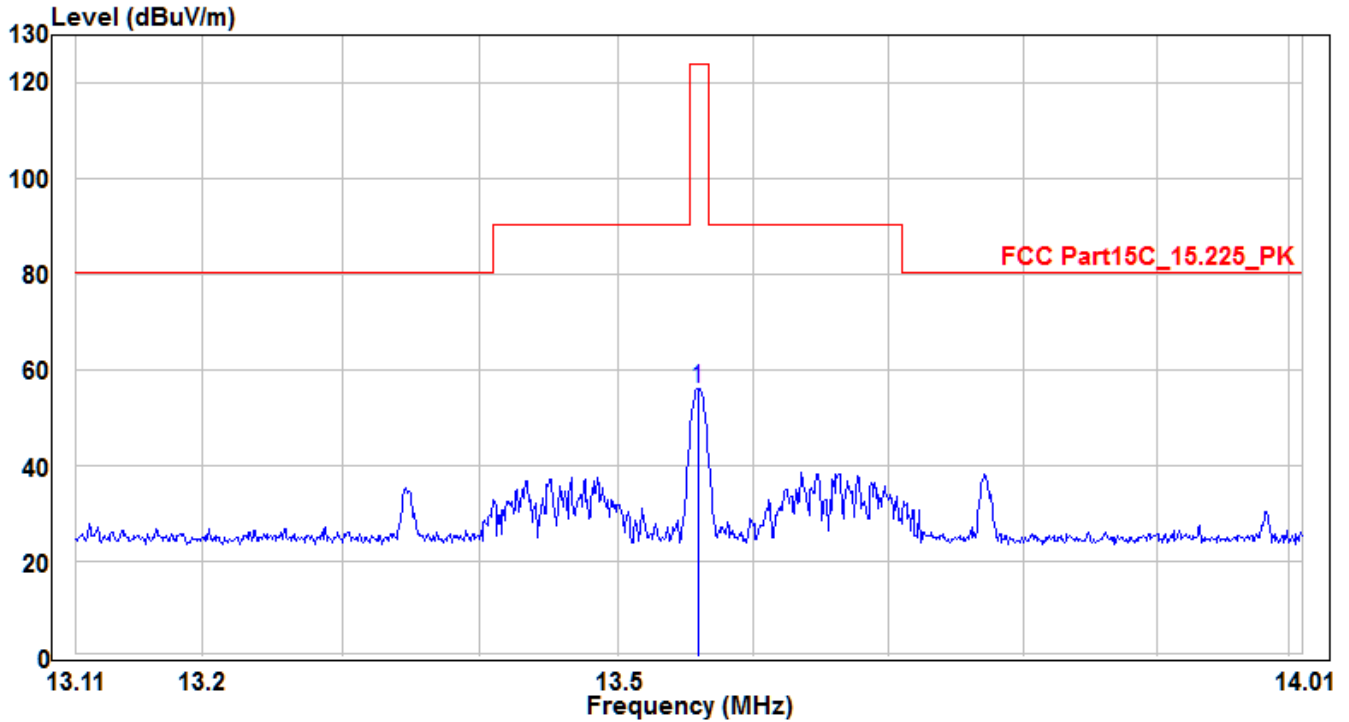


No	Frequency (MHz)	Reading (dBUV)	C.F (dB)	Measurement (dBUV/m)	Margin (dB)	Limit (dBUV)	Height (cm)	Angle (deg)	Remark (QP/PK/AV)
1	*	35.09	21.17	56.26	-67.74	124	100	400	Peak

Note:

- "*", means this data is the worst emission level.
- C.F (Correction Factor) = Antenna Factor (dB)+ Cable Loss (dB)
- Measurement (dBUV/m) = Reading(dBUV) + C.F (Correction Factor)

EUT	Medical Bedside Terminal	Date of Test	2020/3/22
Factor	FMZB 1519B	Temp. / Humidity	25°C / 57%
Polarity	--	Site / Test Engineer	AC1 / Peter
Test Mode	Mode2	Test Voltage	AC 120V/60Hz

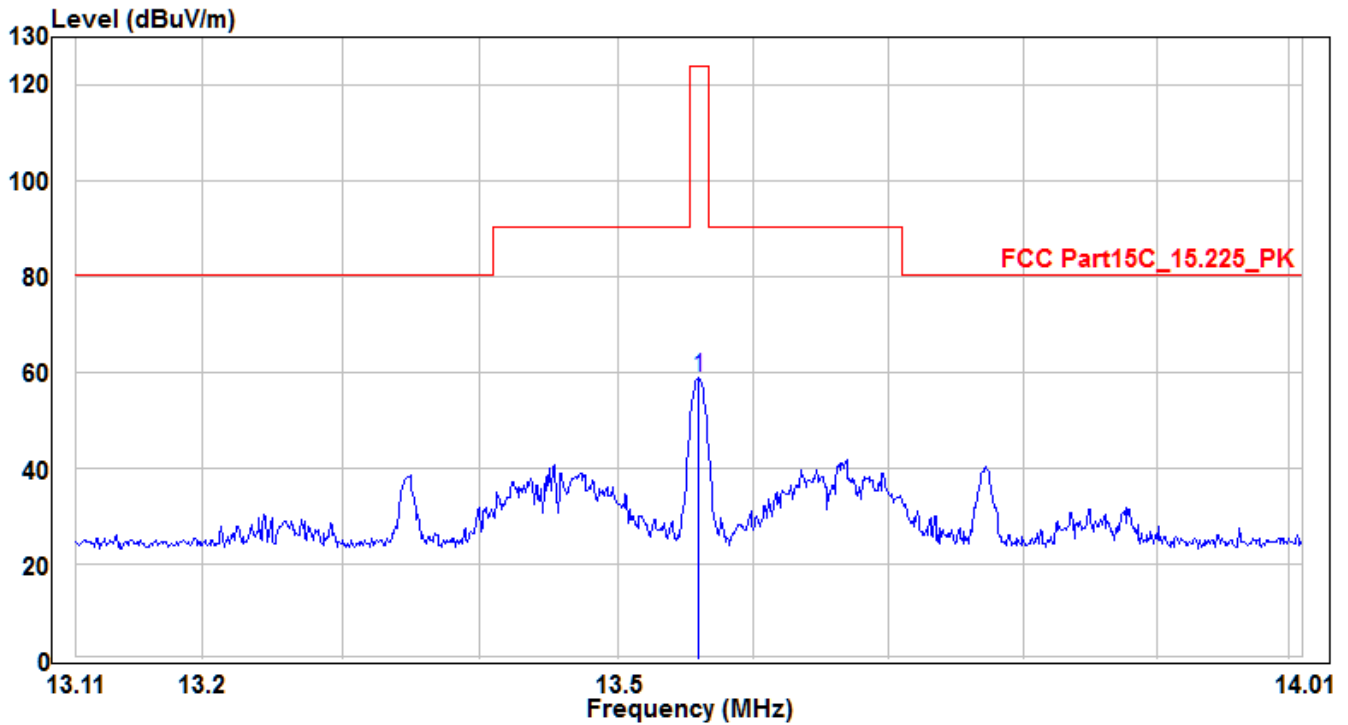

No	Frequency (MHz)	Reading (dBuV)	C.F (dB)	Measurement (dBuV/m)	Margin (dB)	Limit (dBuV)	Height (cm)	Angle (deg)	Remark (QP/PK/AV)
1	*	37.7	21.17	58.87	-65.13	124	100	400	Peak

Note:

1. " *", means this data is the worst emission level.
2. C.F (Correction Factor) = Antenna Factor (dB)+ Cable Loss (dB)
3. Measurement (dBuV/m) = Reading(dBuV) + C.F (Correction Factor)

7.3. Radiated Spurious Emissions Measurement

7.3.1. Test Limit

All out of band emissions appearing in a restricted band as specified in Section 15.225 of the Title 47 CFR must not exceed the limits shown in Table per Section 15.209.

FCC Part 15 Subpart C Paragraph 15.209		
Frequency [MHz]	Field Strength [V/m]	Measured Distance [Meters]
0.009 - 0.490	2400/F (kHz)	300
0.490 - 1.705	24000/F (kHz)	30
1.705 - 30	30	30
30 - 88	100	3
88 - 216	150	3
216 - 960	200	3
Above 960	500	3

Note : The emission limits shown in the above table are based on measurements employing a CISPR quasi-peak detector except for the frequency bands 9-90 kHz, 110-490 kHz and above 1000 MHz. Radiated emission limits in these three bands are based on measurements employing an average detector.

7.3.2. Test Procedure Used

ANSI C63.10-2013 - Section 11.12.2.3 (quasi-peak measurements)

ANSI C63.10-2013 - Section 11.12.2.4 (peak power measurements)

ANSI C63.10-2013 - Section 11.12.2.5 (average power measurements)

Test Setting**Peak Power Measurement**


1. Analyzer center frequency was set to the frequency of the radiated spurious emission of interest
2. RBW = as specified in Table 1
3. VBW = 3 × RBW
4. Detector = peak
5. Sweep time = auto couple

Table 1 - RBW as a function of frequency


Frequency	RBW
9 kHz ~ 150 kHz	200 Hz ~ 300 Hz
0.15 MHz ~ 30 MHz	9 kHz ~ 10 kHz
30 MHz ~ 1000 MHz	100 kHz ~ 120 kHz
> 1000 MHz	1 MHz

7.3.3. Test Setup

9kHz ~ 30MHz Test Setup:

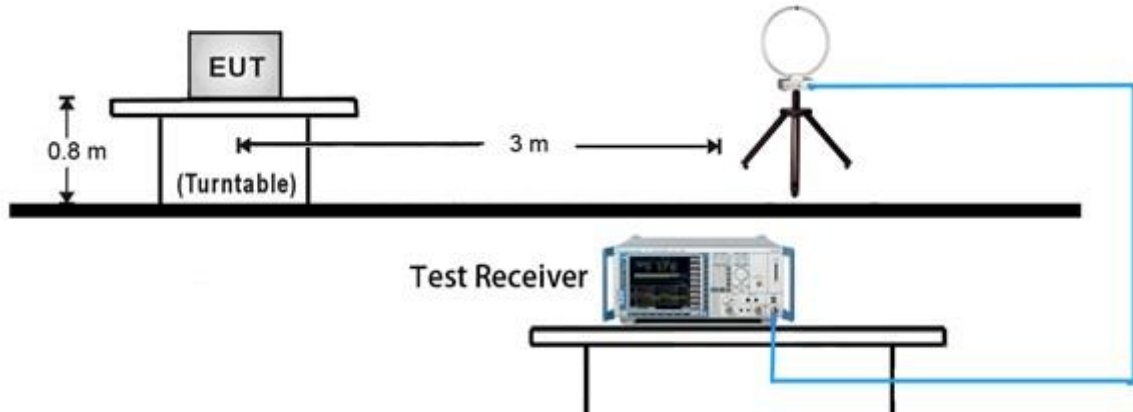


30MHz ~ 1GHz Test Setup:

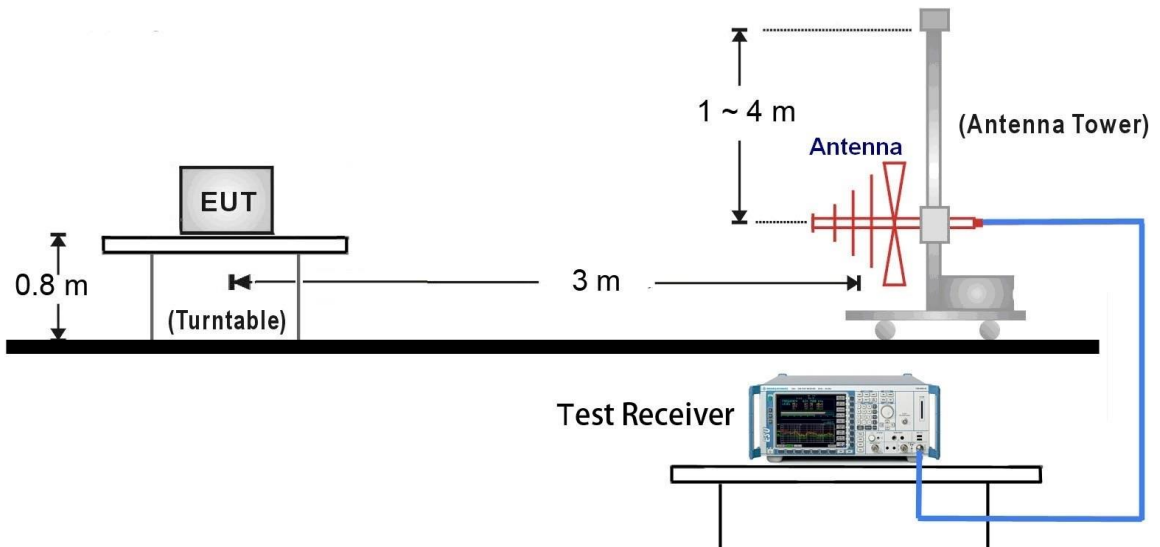

7.3.4. Test Result

EUT	Medical Bedside Terminal	Date of Test	2020/3/22
Factor	FMZB 1519B	Temp. / Humidity	25°C / 57%
Polarity	--	Site / Test Engineer	AC1 / Peter
Test Mode	Mode1	Test Voltage	AC 120V/60Hz

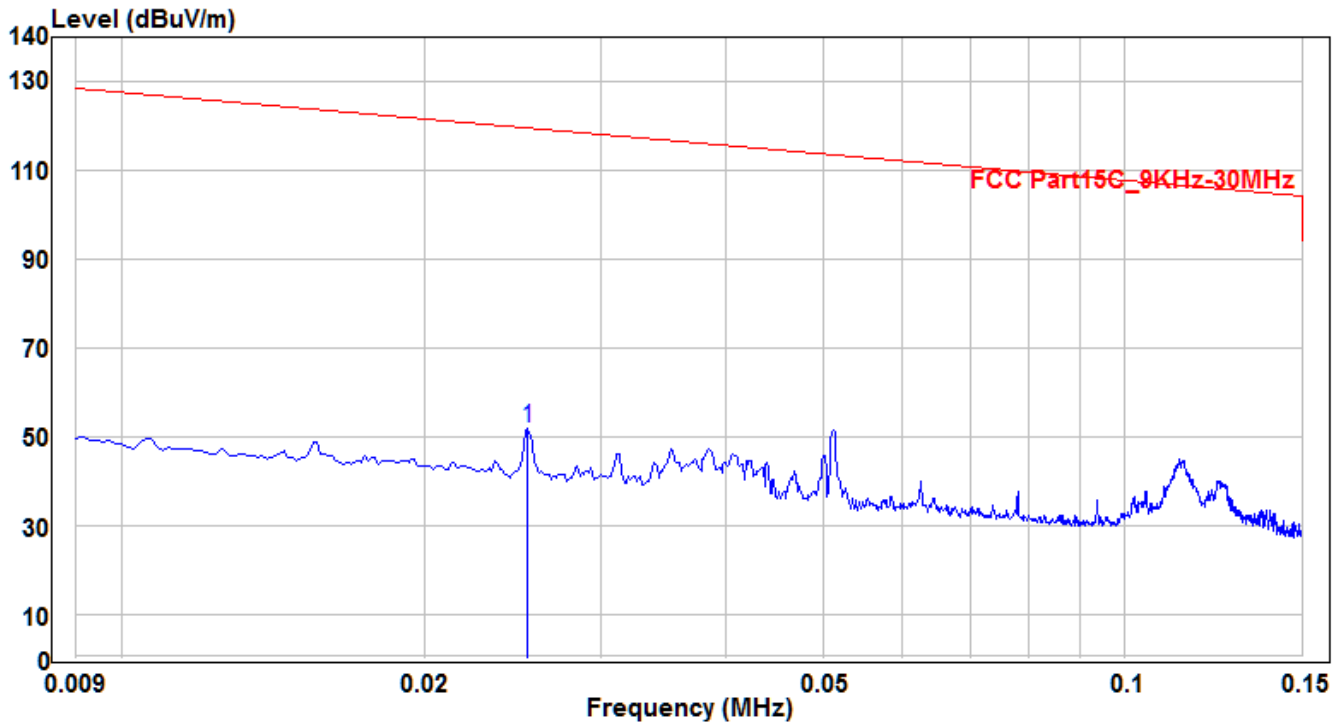


No	Frequency (MHz)	Reading (dBuV)	C.F (dB)	Measurement (dBuV/m)	Margin (dB)	Limit (dBuV)	Height (cm)	Angle (deg)	Remark (QP/PK/AV)
1	*	31.89	20.02	51.91	-67.6	119.51	100	400	Peak

Note:

1. " *", means this data is the worst emission level.
2. C.F (Correction Factor) = Antenna Factor (dB)+ Cable Loss (dB)
3. Measurement (dBuV/m) = Reading(dBuV) + C.F (Correction Factor)

EUT	Medical Bedside Terminal	Date of Test	2020/3/22
Factor	FMZB 1519B	Temp. / Humidity	25°C / 57%
Polarity	--	Site / Test Engineer	AC1 / Peter
Test Mode	Mode1	Test Voltage	AC 120V/60Hz

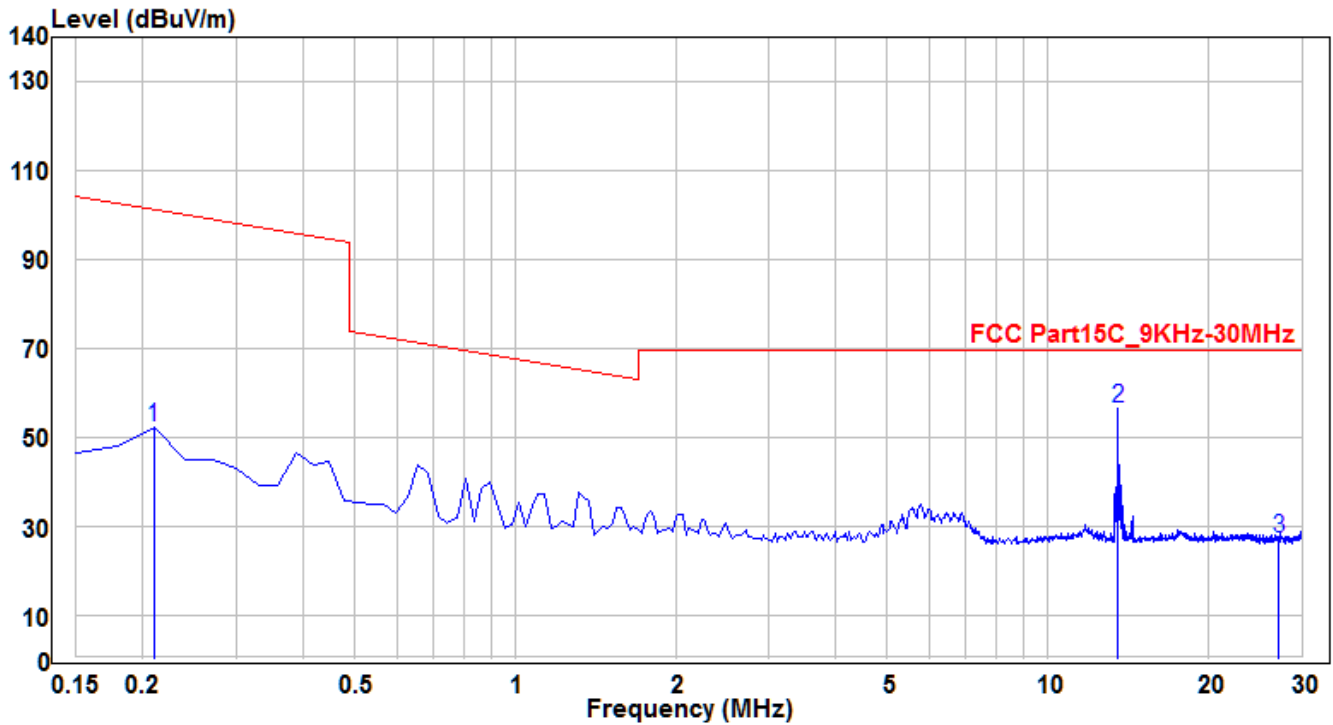


No	Frequency (MHz)	Reading (dBuV)	C.F (dB)	Measurement (dBuV/m)	Margin (dB)	Limit (dBuV)	Height (cm)	Angle (deg)	Remark (QP/PK/AV)
1	0.2097	33.71	18.79	52.5	-48.67	101.17	100	400	Peak
2	13.553	35.36	21.17	56.53	-12.97	69.5	100	400	Peak
3	27.12	5.61	21.73	27.34	-42.16	69.5	100	400	Peak
4	0.2097	33.71	18.79	52.5	-48.67	101.17	100	400	Peak
5	* 13.553	35.36	21.17	56.53	-12.97	69.5	100	400	Peak
6	27.12	5.61	21.73	27.34	-42.16	69.5	100	400	Peak

Note:

1. " *", means this data is the worst emission level.
2. C.F (Correction Factor) = Antenna Factor (dB)+ Cable Loss (dB)
3. Measurement (dBuV/m) = Reading(dBuV) + C.F (Correction Factor)

EUT	Medical Bedside Terminal	Date of Test	2020/3/22
Factor	FMZB 1519B	Temp. / Humidity	25°C / 57%
Polarity	--	Site / Test Engineer	AC1 / Peter
Test Mode	Mode2	Test Voltage	AC 120V/60Hz

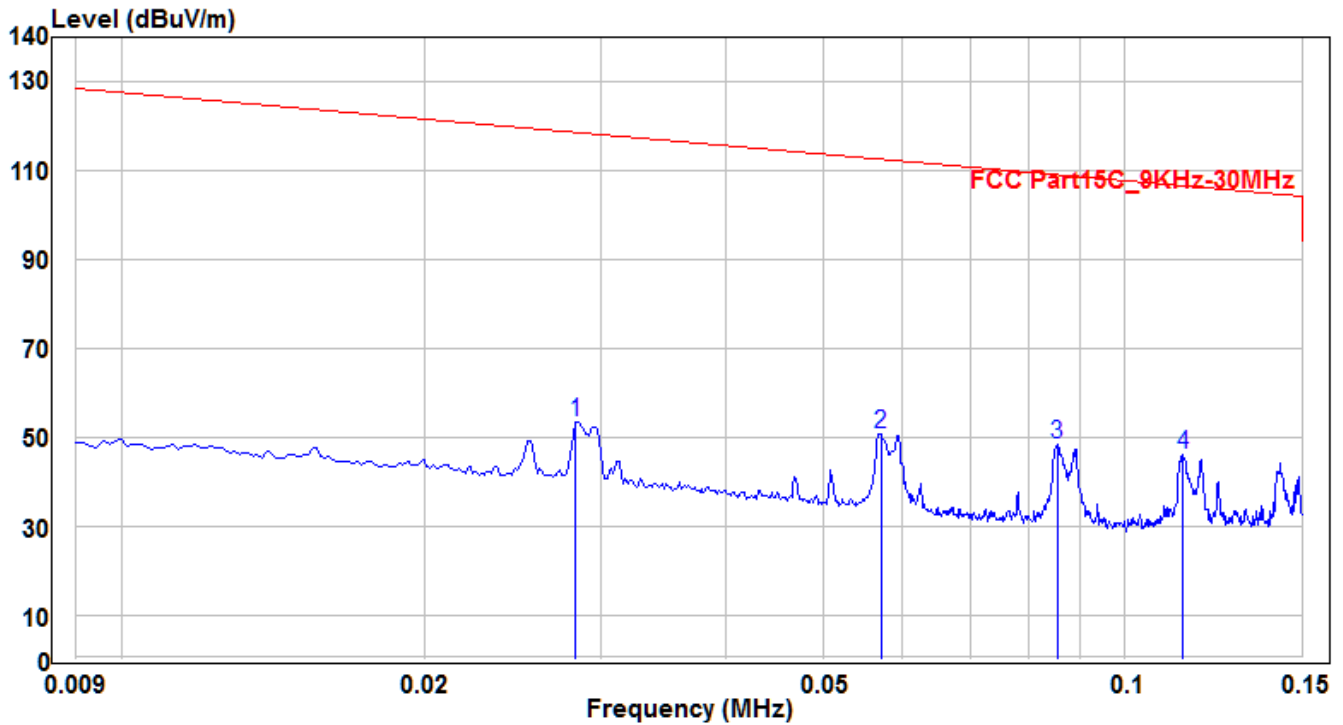


No	Frequency (MHz)	Reading (dBuV)	C.F (dB)	Measurement (dBuV/m)	Margin (dB)	Limit (dBuV)	Height (cm)	Angle (deg)	Remark (QP/PK/AV)
1	0.02832	33.18	20.14	53.32	-65.23	118.55	100	400	Peak
2	0.05708	31.48	19.37	50.85	-61.62	112.47	100	400	Peak
3	0.08556	29.86	18.8	48.66	-60.29	108.95	100	400	Peak
4	* 0.11419	27.79	18.55	46.34	-60.11	106.45	100	400	Peak

Note:

1. " *", means this data is the worst emission level.
2. C.F (Correction Factor) = Antenna Factor (dB)+ Cable Loss (dB)
3. Measurement (dBuV/m) = Reading(dBuV) + C.F (Correction Factor)

EUT	Medical Bedside Terminal	Date of Test	2020/3/22
Factor	FMZB 1519B	Temp. / Humidity	25°C / 57%
Polarity	--	Site / Test Engineer	AC1 / Peter
Test Mode	Mode2	Test Voltage	AC 120V/60Hz

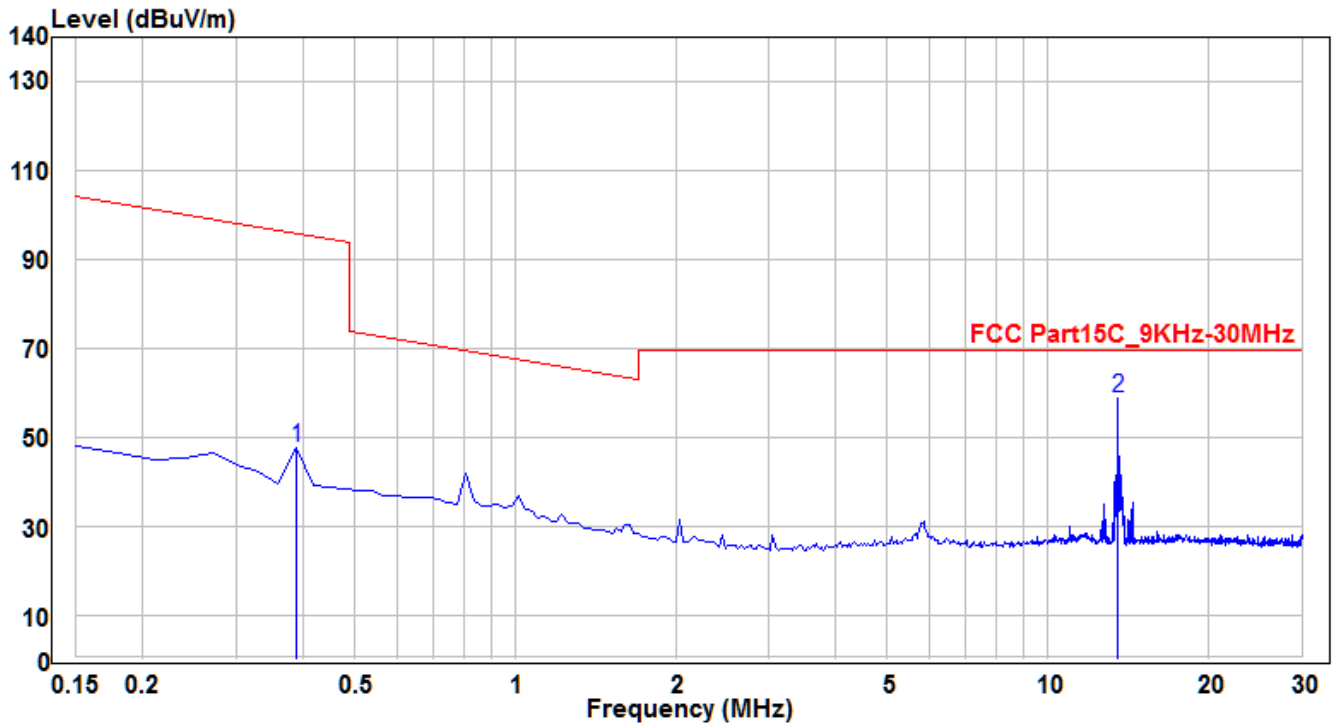


No	Frequency (MHz)	Reading (dBuV)	C.F (dB)	Measurement (dBuV/m)	Margin (dB)	Limit (dBuV)	Height (cm)	Angle (deg)	Remark (QP/PK/AV)
1	0.3888	28.71	19.03	47.74	-48.07	95.81	100	400	Peak
2	*	37.77	21.17	58.94	-10.56	69.5	100	400	Peak

Note:

1. " *", means this data is the worst emission level.
2. C.F (Correction Factor) = Antenna Factor (dB)+ Cable Loss (dB)
3. Measurement (dBuV/m) = Reading(dBuV) + C.F (Correction Factor)

EUT	Medical Bedside Terminal	Date of Test	2020/3/22
Factor	VULB 9162	Temp. / Humidity	25°C / 57%
Polarity	Horizontal	Site / Test Engineer	AC1 / Peter
Test Mode	Mode1	Test Voltage	AC 120V/60Hz

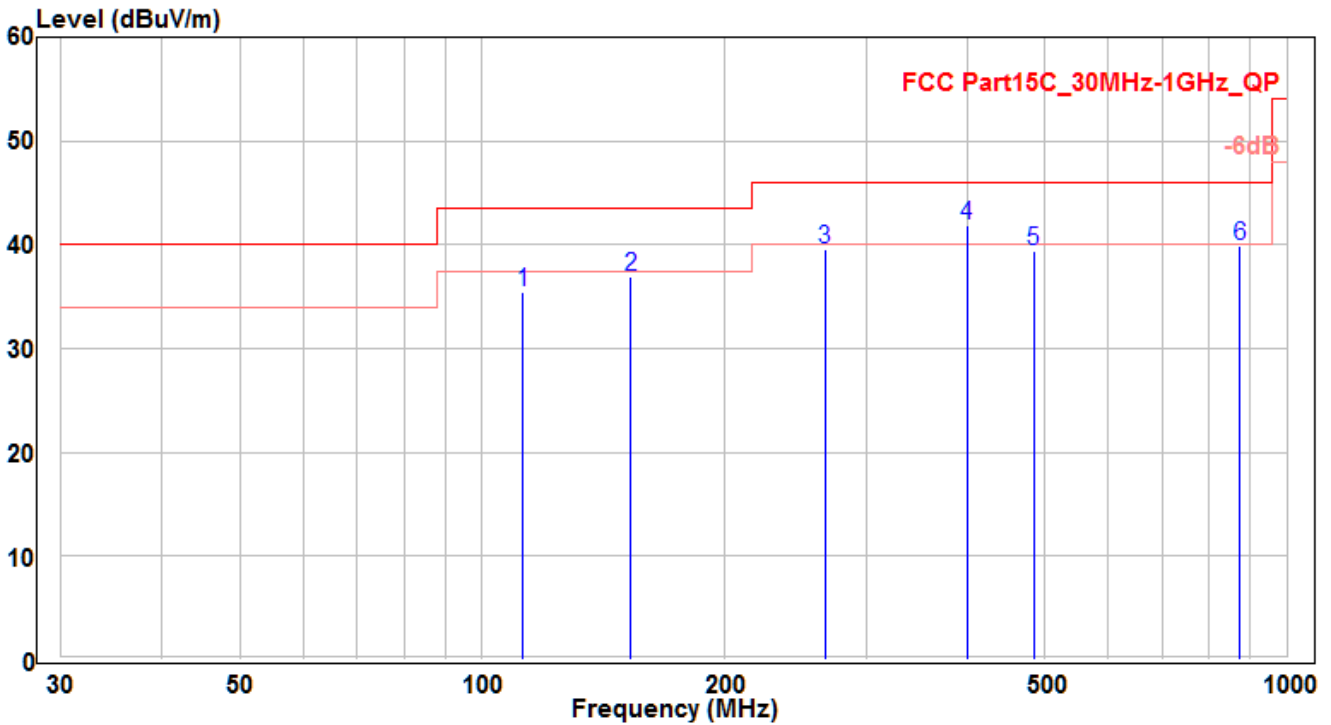


No	Frequency (MHz)	Reading (dBuV)	C.F (dB)	Measurement (dBuV/m)	Margin (dB)	Limit (dBuV)	Height (cm)	Angle (deg)	Remark (QP/PK/AV)
1	112.48	16.56	18.9	35.46	-8.04	43.5	110	145	QP
2	152.948	21.2	15.81	37.01	-6.49	43.5	155	360	QP
3	266.65	18.83	20.66	39.49	-6.51	46	130	85	QP
4	* 399.994	17.88	23.96	41.84	-4.16	46	120	110	QP
5	485.082	13.76	25.56	39.32	-6.68	46	100	60	QP
6	875.022	8.61	31.33	39.94	-6.06	46	110	240	QP

Note:

1. " *", means this data is the worst emission level.
2. C.F (Correction Factor) = Antenna Factor (dB)+ Cable Loss (dB)
3. Measurement (dBuV/m) = Reading(dBuV) + C.F (Correction Factor)

EUT	Medical Bedside Terminal	Date of Test	2020/3/22
Factor	VULB 9162	Temp. / Humidity	25°C / 57%
Polarity	Vertical	Site / Test Engineer	AC1 / Peter
Test Mode	Mode1	Test Voltage	AC 120V/60Hz

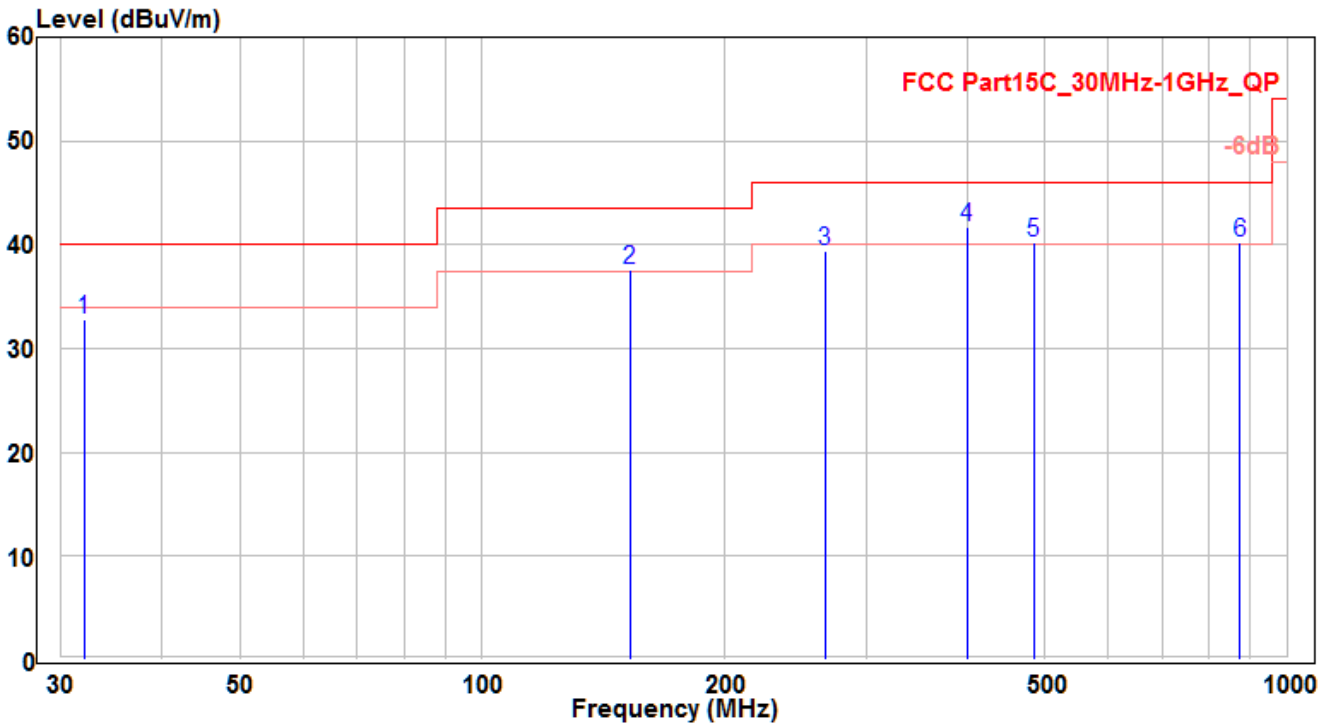


No	Frequency (MHz)	Reading (dBUV)	C.F (dB)	Measurement (dBUV/m)	Margin (dB)	Limit (dBUV)	Height (cm)	Angle (deg)	Remark (QP/PK/AV)
1	32.031	14.58	18.26	32.84	-7.16	40	100	40	QP
2	152.735	21.82	15.8	37.62	-5.88	43.5	140	85	QP
3	266.65	18.81	20.66	39.47	-6.53	46	120	370	QP
4	* 399.994	17.8	23.96	41.76	-4.24	46	120	150	QP
5	485.082	14.69	25.56	40.25	-5.75	46	100	165	QP
6	875.022	8.82	31.33	40.15	-5.85	46	100	375	QP

Note:

- "*" means this data is the worst emission level.
- C.F (Correction Factor) = Antenna Factor (dB)+ Cable Loss (dB)
- Measurement (dBUV/m) = Reading(dBUV) + C.F (Correction Factor)

EUT	Medical Bedside Terminal	Date of Test	2020/3/22
Factor	VULB 9162	Temp. / Humidity	25°C / 57%
Polarity	Horizontal	Site / Test Engineer	AC1 / Peter
Test Mode	Mode2	Test Voltage	AC 120V/60Hz

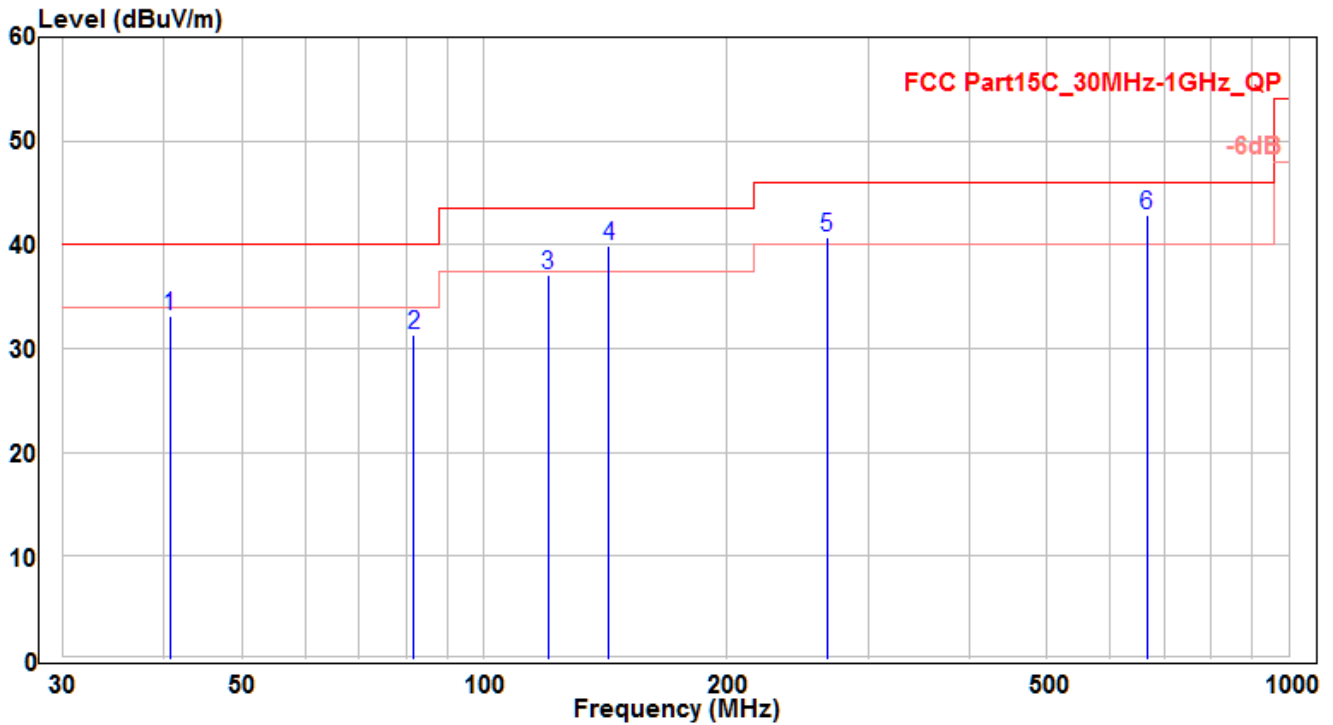


No	Frequency (MHz)	Reading (dBuV)	C.F (dB)	Measurement (dBuV/m)	Margin (dB)	Limit (dBuV)	Height (cm)	Angle (deg)	Remark (QP/PK/AV)
1	40.67	12.31	20.89	33.2	-6.8	40	200	150	QP
2	81.743	16.8	14.48	31.28	-8.72	40	240	225	QP
3	119.998	19.16	17.94	37.1	-6.4	43.5	110	265	QP
4	142.793	24.31	15.64	39.95	-3.55	43.5	100	45	QP
5	266.65	20.11	20.66	40.77	-5.23	46	150	375	QP
6	* 666.684	14.19	28.68	42.87	-3.13	46	135	250	QP

Note:

- "*", means this data is the worst emission level.
- C.F (Correction Factor) = Antenna Factor (dB)+ Cable Loss (dB)
- Measurement (dBuV/m) = Reading(dBuV) + C.F (Correction Factor)

EUT	Medical Bedside Terminal	Date of Test	2020/3/22
Factor	VULB 9162	Temp. / Humidity	25°C / 57%
Polarity	Vertical	Site / Test Engineer	AC1 / Peter
Test Mode	Mode2	Test Voltage	AC 120V/60Hz

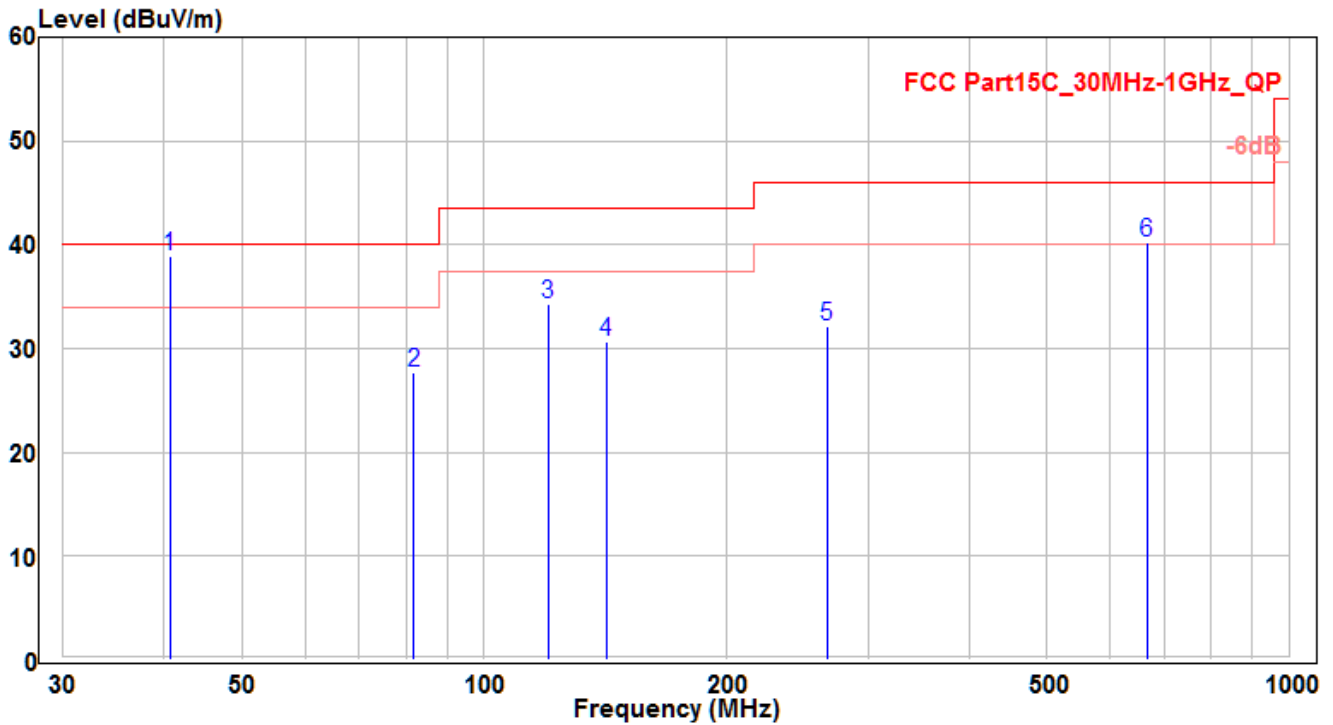

No		Frequency (MHz)	Reading (dBuV)	C.F (dB)	Measurement (dBuV/m)	Margin (dB)	Limit (dBuV)	Height (cm)	Angle (deg)	Remark (QP/PK/AV)
1	*	40.67	18	20.89	38.89	-1.11	40	100	280	QP
2		81.743	13.3	14.48	27.78	-12.22	40	200	-40	QP
3		119.998	16.43	17.94	34.37	-9.13	43.5	120	240	QP
4		141.853	15	15.64	30.64	-12.86	43.5	105	390	QP
5		266.65	11.52	20.66	32.18	-13.82	46	145	350	QP
6		666.684	11.5	28.68	40.18	-5.82	46	165	110	QP

Note:

1. " *", means this data is the worst emission level.
2. C.F (Correction Factor) = Antenna Factor (dB)+ Cable Loss (dB)
3. Measurement (dBuV/m) = Reading(dBuV) + C.F (Correction Factor)

7.4. 20dB Bandwidth Measurement

7.4.1. Test Limit

N/A


7.4.2. Test Procedure Used

KDB 789033 D02v01r01 – Section C.1

7.4.3. Test Setting

1. The analyzers' automatic bandwidth measurement capability was used to perform the 26dB bandwidth measurement. The "X" dB bandwidth parameter was set to $X = 26$. The automatic bandwidth measurement function also has the capability of simultaneously measuring the 99% occupied bandwidth. The bandwidth measurement was not influenced by any intermediated power nulls in the fundamental emission.
2. RBW = approximately 1% of the emission bandwidth.
3. VBW $\geq 3 \times$ RBW.
4. Detector = Peak.
5. Trace mode = max hold.


7.4.4. Test Setup

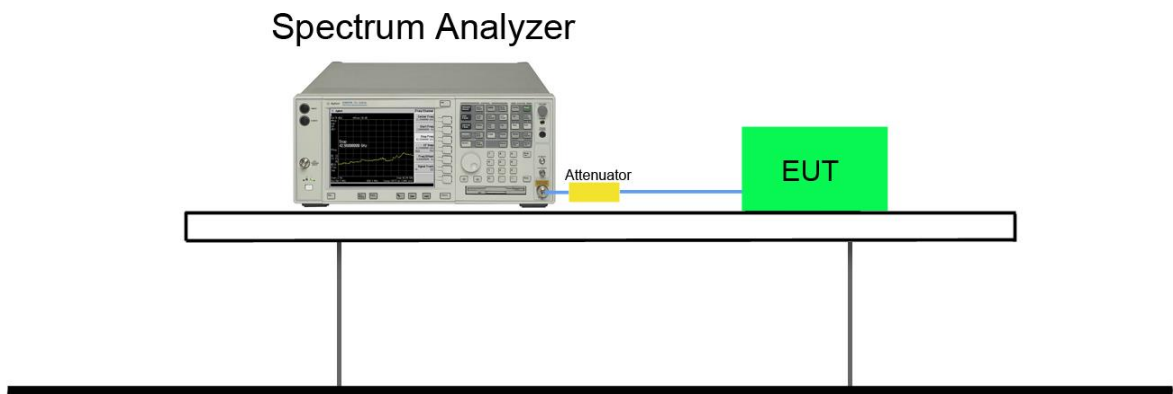

7.4.5. Test Result

Test Mode	Frequency (MHz)	20dB Bandwidth (kHz)	99% Bandwidth (kHz)
NFC (Mode 1)	13.65	2.70	2.36

NFC 13.56MHz 20dB Bandwidth & 99% Bandwidth

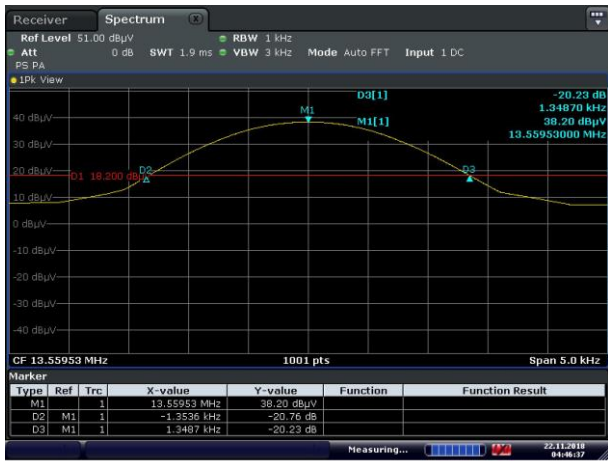

Date: 22.NOV.2016 04:46:37



Date: 22.NOV.2016 04:47:43

Test Mode	Frequency (MHz)	20dB Bandwidth (kHz)	99% Bandwidth (kHz)
NFC (Mode 2)	13.65	2.63	2.32



7.5. Frequency Stability Measurement

7.5.1. Test Limit

Manufactures of U-NII devices are responsible for ensuring frequency stability such that an emission is maintained within the band of operation under all conditions of normal operation as specified in the user's manual.

7.5.2. Test Procedure Used

Frequency Stability Under Temperature Variations:


The equipment under test was connected to an external AC or DC power supply and input rated voltage. RF output was connected to a frequency counter or spectrum analyzer via feed through attenuators. The EUT was placed inside the temperature chamber. Set the spectrum analyzer RBW low enough to obtain the desired frequency resolution and measure EUT 20°C operating frequency as reference frequency. Turn EUT off and set the chamber temperature to highest. After the temperature stabilized for approximately 30 minutes recorded the frequency. Repeat step measure with 10°C decreased per stage until the lowest temperature reached.

Frequency Stability Under Voltage Variations:

Set chamber temperature to 20°C. Use a variable AC power supply / DC power source to power the EUT and set the voltage to rated voltage. Set the spectrum analyzer RBW low enough to obtain the desired frequency resolution and recorded the frequency.

Reduce the input voltage to specify extreme voltage variation ($\pm 15\%$) and endpoint, record the maximum frequency change.

7.5.3. Test Setup

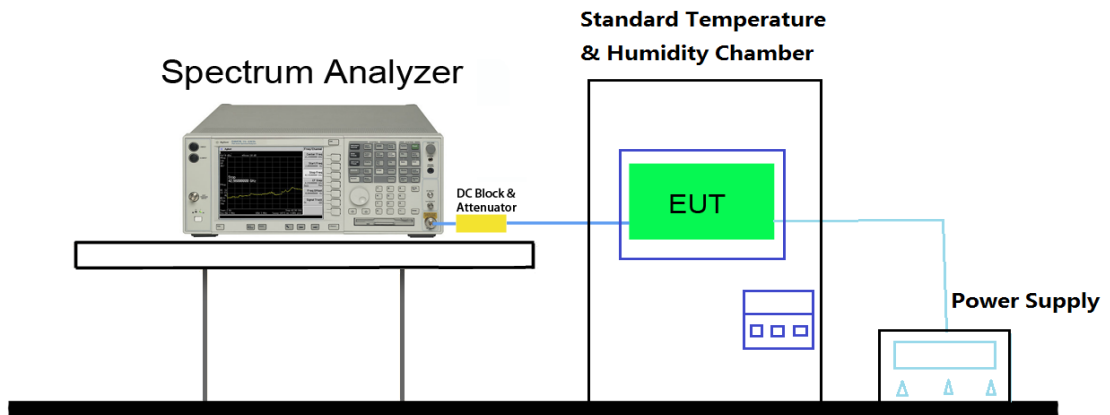

7.5.4. Test Result

Test Engineer	Peter	Temperature	-20 ~ 50°C
Test Time	2020/03/03	Relative Humidity	58%RH

NFC 13.56MHz Frequency Stability					
Temperature vs. Frequency Stability					
Voltage (%)	Power (VAC)	Temp (°C)	Frequency (MHz)	Frequency Tolerance (ppm)	Limit (ppm)
100%	120V/60Hz	- 20	13.5595	-36.8732	±100
		- 10	13.5596	-29.4985	±100
		0	13.5596	-29.4985	±100
		+ 10	13.5596	-29.4985	±100
		+ 20 (Ref)	13.5596	-29.4985	±100
		+ 30	13.5596	-29.4985	±100
		+ 40	13.5595	-36.8732	±100
		+ 50	13.5595	-36.8732	±100
Test Result			PASS		
Voltage vs. Frequency Stability					
Voltage (%)	Power (VAC)	Temp (°C)	Frequency (MHz)	Frequency Tolerance (ppm)	Limit (ppm)
100%	120V/60Hz	+ 20	13.5595	-36.8732	±100
115%	138V/60Hz	+ 20	13.5596	-29.4985	±100
85%	102V/60Hz	+ 20	13.5595	-36.8732	±100
Test Result			PASS		

Note:

Frequency Tolerance (ppm) = {[Measured Frequency (Hz) – Declared Frequency (Hz)] / Declared Frequency (Hz)} *10⁶.

7.6. AC Conducted Emissions Measurement


7.6.1. Test Limit

FCC Part 15 Subpart C Paragraph 15.207 Limits		
Frequency (MHz)	QP (dBuV)	AV (dBuV)
0.15 - 0.50	66 - 56	56 - 46
0.50 - 5.0	56	46
5.0 - 30	60	50

Note 1: The lower limit shall apply at the transition frequencies.


Note 2: The limit decreases linearly with the logarithm of the frequency in the range 0.15MHz to 0.5MHz.

7.6.2. Test Setup

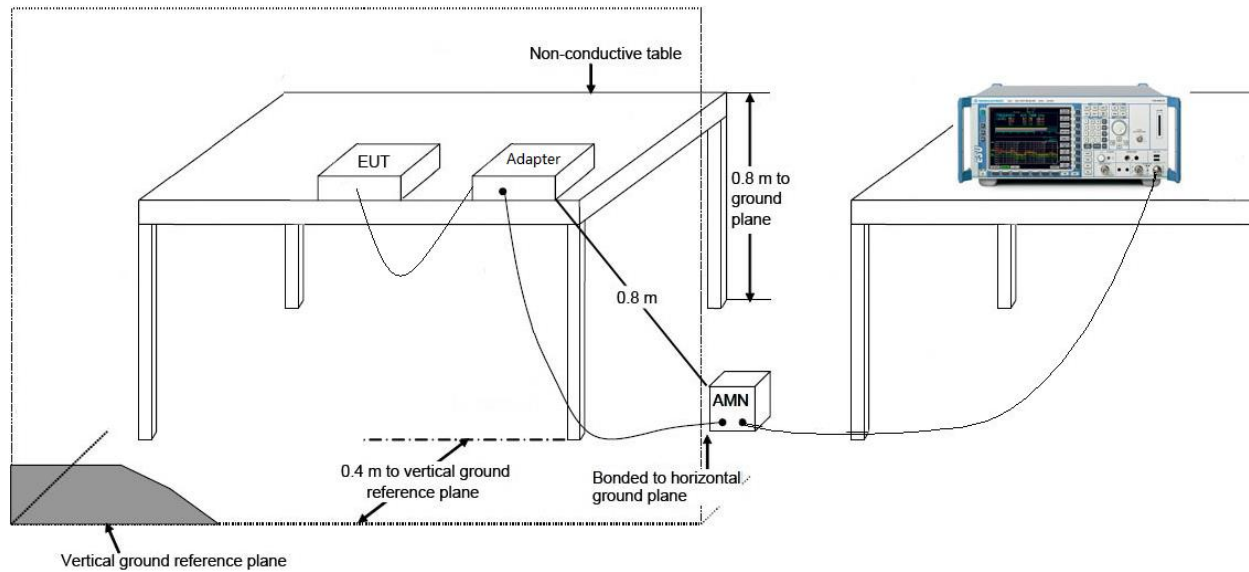

7.6.3. Test Result

EUT	Medical Bedside Terminal	Date of Test	2020/3/19
Factor	CE_ENV216-L1 (Filter ON)	Temp. / Humidity	24°C / 68%
Polarity	Line1	Site / Test Engineer	SR2 / Peter
Test Mode	Mode1	Test Voltage	AC 120V/60Hz

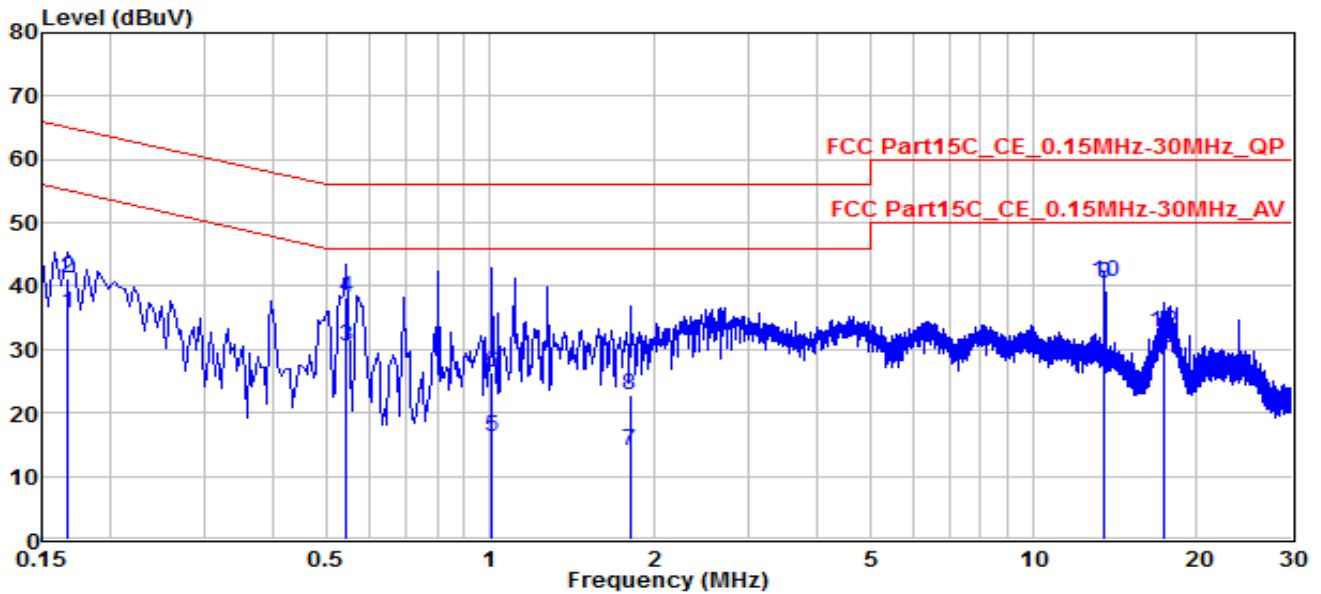


No	Frequency (MHz)	Reading (dBUV)	C.F (dB)	Measurement (dBUV)	Margin (dB)	Limit (dBUV)	Remark (QP/PK/AV)
1	0.168	25.48	10.13	35.61	-19.45	55.06	Average
2	0.168	31.05	10.13	41.18	-23.88	65.06	QP
3	0.54596	20.52	10.09	30.61	-15.39	46	Average
4	0.54596	27.99	10.09	38.08	-17.92	56	QP
5	1.009	6.36	9.89	16.25	-29.75	46	Average
6	1.009	16.45	9.89	26.34	-29.66	56	QP
7	1.81	4.17	9.87	14.04	-31.96	46	Average
8	1.81	12.92	9.87	22.79	-33.21	56	QP
9	* 13.559	30.38	9.92	40.3	-9.7	50	Average
10	* 13.559	30.81	9.92	40.73	-19.27	60	QP
11	17.334	18.51	9.96	28.47	-21.53	50	Average
12	17.334	22.84	9.96	32.8	-27.2	60	QP

Note:

1. " *", means this data is the worst emission level.
2. C.F (Correction Factor) = Factor (dB)+ Cable Loss (dB)
3. Measurement (dBUV) = Reading(dBUV)+ C.F (Correction Factor)

EUT	Medical Bedside Terminal	Date of Test	2020/3/19
Factor	CE_ENV216-N (Filter ON)	Temp. / Humidity	24°C / 68%
Polarity	Neutral	Site / Test Engineer	SR2 / Peter
Test Mode	Mode1	Test Voltage	AC 120V/60Hz

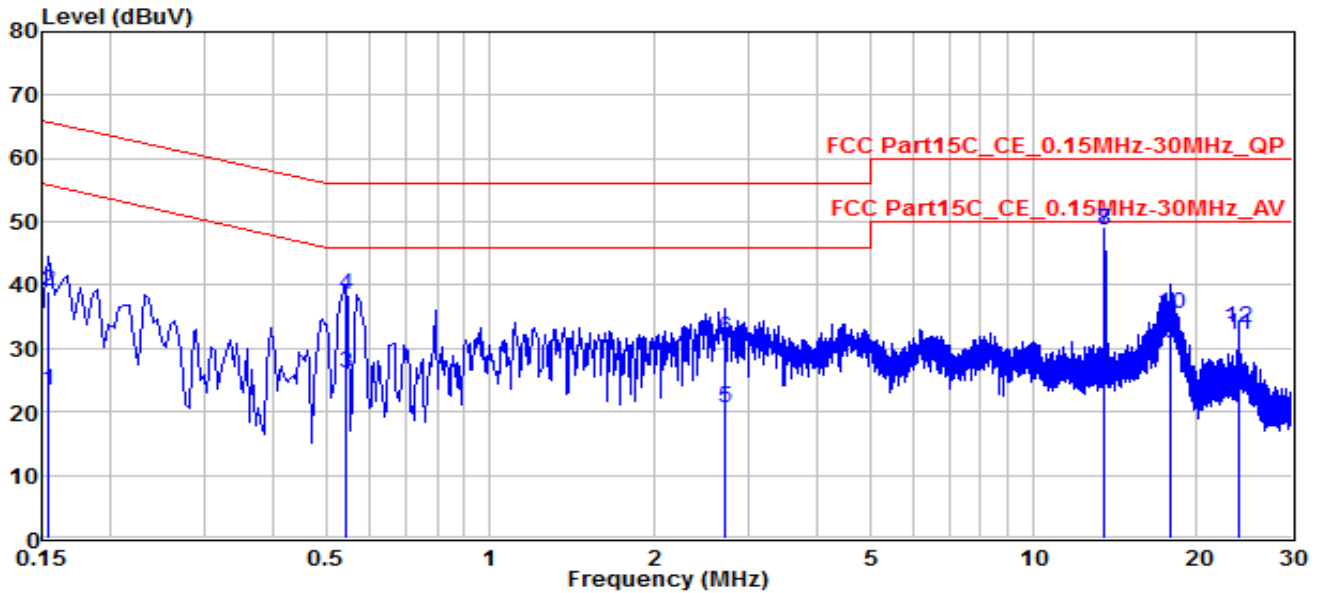


No	Frequency (MHz)	Reading (dBuV)	C.F (dB)	Measurement (dBuV)	Margin (dB)	Limit (dBuV)	Remark (QP/PK/AV)
1	0.1545	13.54	9.95	23.49	-32.26	55.75	Average
2	0.1545	29.15	9.95	39.1	-26.65	65.75	QP
3	0.54596	15.88	10.11	25.99	-20.01	46	Average
4	0.54596	28.36	10.11	38.47	-17.53	56	QP
5	2.706	10.67	9.83	20.5	-25.5	46	Average
6	2.706	21.85	9.83	31.68	-24.32	56	QP
7	*	13.559	9.94	48.65	-1.35	50	Average
8	*	13.559	9.94	48.66	-11.34	60	QP
9	17.86	20.65	10.02	30.67	-19.33	50	Average
10	17.86	25.38	10.02	35.4	-24.6	60	QP
11	23.818	22.09	10.1	32.19	-17.81	50	Average
12	23.818	23.11	10.1	33.21	-26.79	60	QP

Note:

- "*", means this data is the worst emission level.
- C.F (Correction Factor) = Factor (dB)+ Cable Loss (dB)
- Measurement (dBuV) = Reading(dBuV)+ C.F (Correction Factor)

EUT	Medical Bedside Terminal	Date of Test	2020/3/19
Factor	CE_ENV216-L1 (Filter ON)	Temp. / Humidity	24°C / 68%
Polarity	Line1	Site / Test Engineer	SR2 / Peter
Test Mode	Mode2	Test Voltage	AC 120V/60Hz

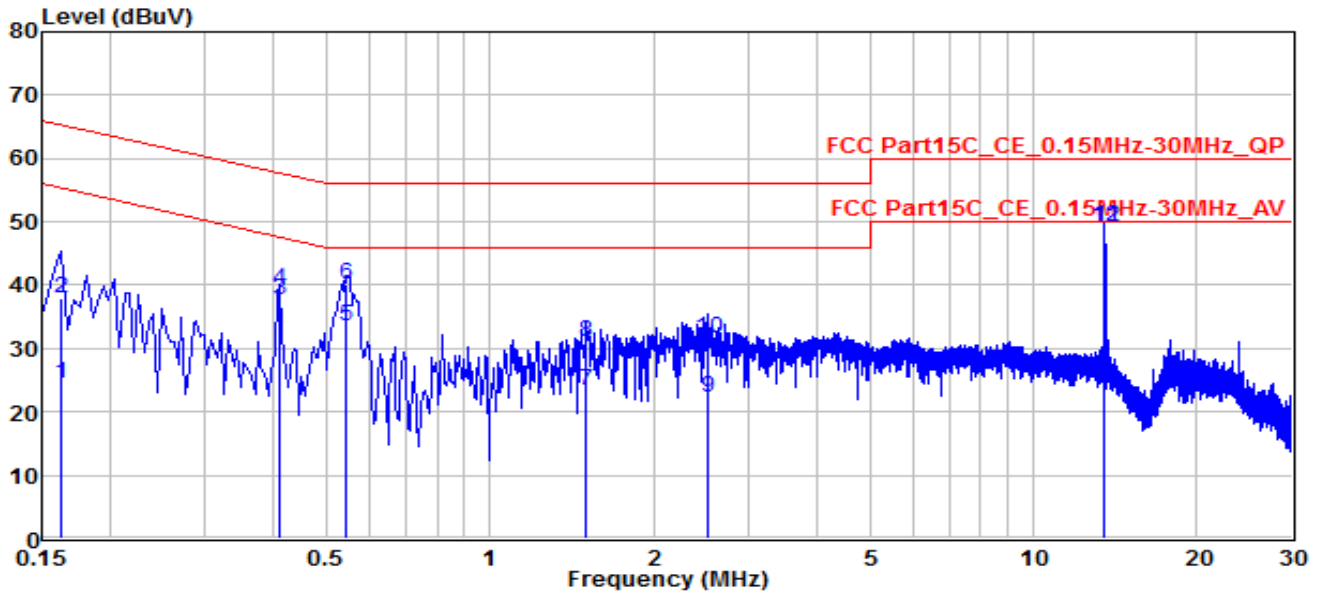


No	Frequency (MHz)	Reading (dBuV)	C.F (dB)	Measurement (dBuV)	Margin (dB)	Limit (dBuV)	Remark (QP/PK/AV)
1	0.1635	14.37	10.12	24.49	-30.79	55.28	Average
2	0.1635	27.94	10.12	38.06	-27.22	65.28	QP
3	0.41097	27.49	10.05	37.54	-10.09	47.63	Average
4	0.41097	29.28	10.05	39.33	-18.3	57.63	QP
5	0.54596	23.55	10.09	33.64	-12.36	46	Average
6	0.54596	30.09	10.09	40.18	-15.82	56	QP
7	1.504	13.41	9.88	23.29	-22.71	46	Average
8	1.504	21.29	9.88	31.17	-24.83	56	QP
9	2.521	12.51	9.85	22.36	-23.64	46	Average
10	2.521	21.8	9.85	31.65	-24.35	56	QP
11	* 13.559	39.24	9.92	49.16	-0.84	50	Average
12	* 13.559	39.26	9.92	49.18	-10.82	60	QP

Note:

- "*", means this data is the worst emission level.
- C.F (Correction Factor) = Factor (dB)+ Cable Loss (dB)
- Measurement (dBuV) = Reading(dBuV)+ C.F (Correction Factor)

EUT	Medical Bedside Terminal	Date of Test	2020/3/19
Factor	CE_ENV216-N (Filter ON)	Temp. / Humidity	24°C / 68%
Polarity	Neutral	Site / Test Engineer	SR2 / Peter
Test Mode	Mode2	Test Voltage	AC 120V/60Hz

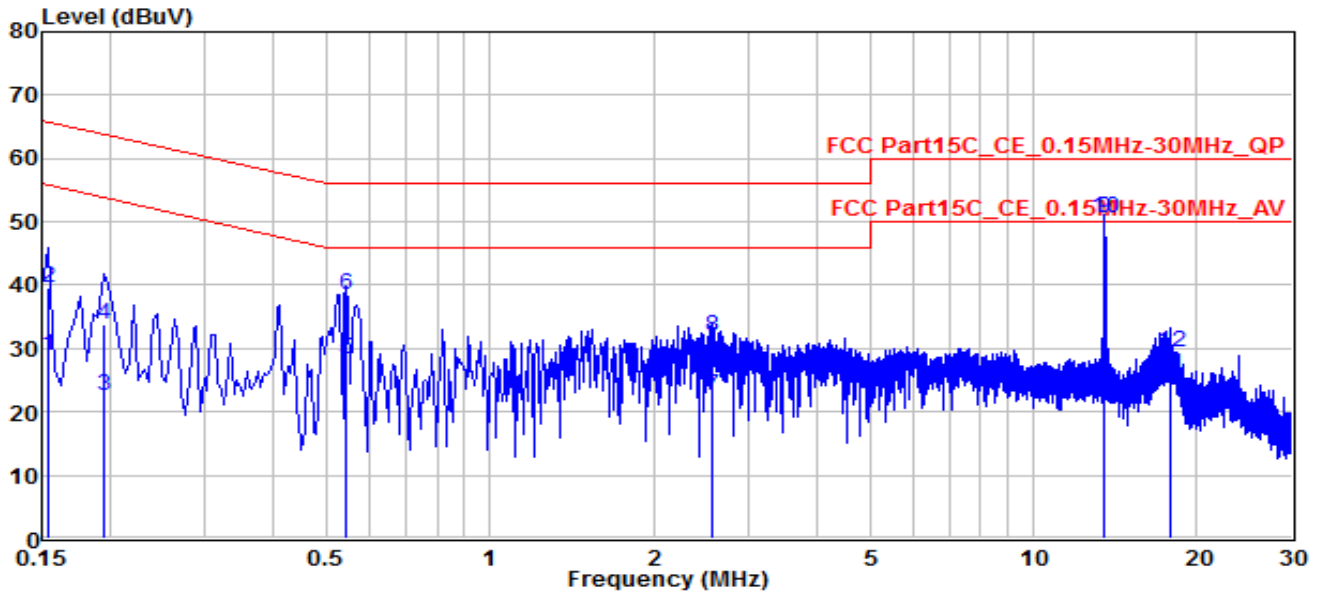

No	Frequency (MHz)	Reading (dBuV)	C.F (dB)	Measurement (dBuV)	Margin (dB)	Limit (dBuV)	Remark (QP/PK/AV)
1	0.1545	18.94	9.95	28.89	-26.86	55.75	Average
2	0.1545	29.61	9.95	39.56	-26.19	65.75	QP
3	0.195	12.64	9.95	22.59	-31.23	53.82	Average
4	0.195	23.94	9.95	33.89	-29.93	63.82	QP
5	0.54596	18.13	10.11	28.24	-17.76	46	Average
6	0.54596	28.24	10.11	38.35	-17.65	56	QP
7	2.557	12.63	9.84	22.47	-23.53	46	Average
8	2.557	22.02	9.84	31.86	-24.14	56	QP
9	*	13.559	9.94	49.63	-0.37	50	Average
10	*	13.559	9.94	49.61	-10.39	60	QP
11	17.86	15.76	10.02	25.78	-24.22	50	Average
12	17.86	19.37	10.02	29.39	-30.61	60	QP

Note:

- "*", means this data is the worst emission level.
- C.F (Correction Factor) = Factor (dB)+ Cable Loss (dB)
- Measurement (dBuV) = Reading(dBuV)+ C.F (Correction Factor)

8. CONCLUSION

The data collected relate only the item(s) tested and show that the **Medical Bedside Terminal** is in compliance with Part 15.225 of the FCC Rules.

————— The End —————