


75.00 mm

25.00 mm

Panel PC Hardware System

Model:K959T

DC Input:19V  6.32A

SN



MEDICAL-GENERAL MEDICAL EQUIPMENT AS TO ELECTRICAL SHOCK,FIRE AND MECHANICAL HAZARDS ONLY IN ACCORDANCE WITH ANSI/AAMI ES 60601-1(2005)+AMD1(2012) AND CAN/CSA-C22.2 No.60601-1:14

RoHS



Class I equipment



*This device complies with part 15 of the FCC rules. Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received, including interference that may cause undesired operation.*

FLYTECH TECHNOLOGY CO.,LTD

Contains FCC ID:PD99260NG


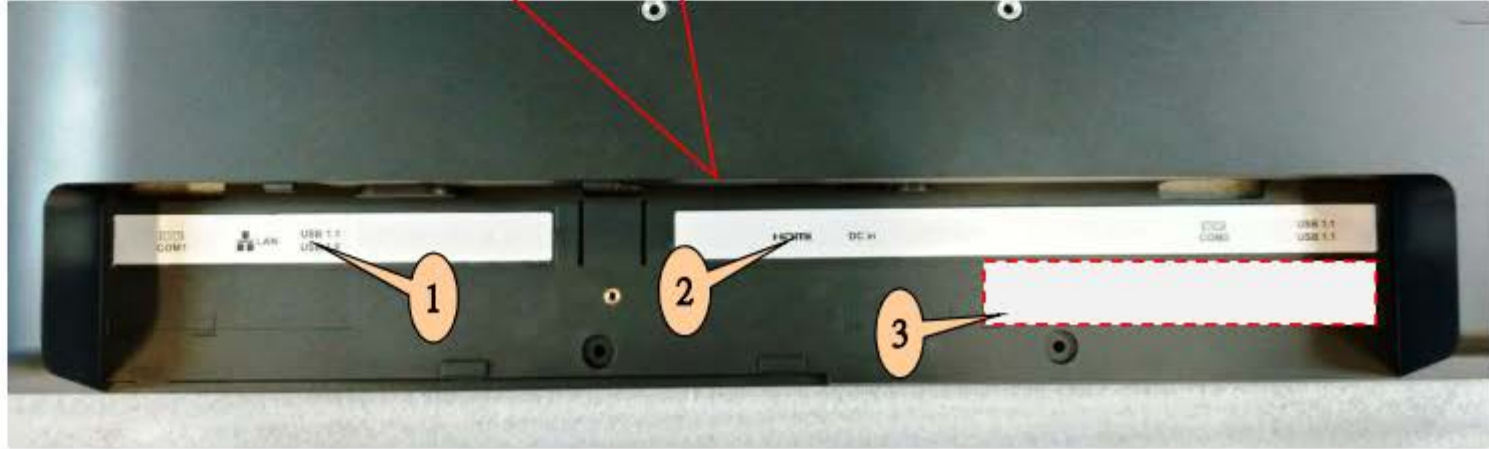
FCC ID:XHM-TME22D87UO

Address:No.168,Sing-ai Rd.,Neihu District,Taipei City 11494,Taiwan

P/N:3LEK9590008X

MADE IN TAIWAN

印刷字體黑色,尺寸公差 $\pm 0.3\text{mm}$,材質四維PO32B

適用機種		K959T+D87U		版本	F	作業項目	背蓋加工	作業站別	背蓋加工	日期	110/3/31	頁次	27 / 53
組裝物件	項次	料號	品名	數量	作業圖示順序								
	{1}	3LCK95900010	LABEL I/O CONNECTOR 131*15mm	1									
	{2}	3LCK95900020	LABEL I/O CONNECTOR 215*15mm	1									
	{3}		安規LABEL	1									
	{4}	3LW045010010	LABEL WARN NON ISOLATED PORTS 45*8mm	1									
作業內容及順序													
1. 將LABEL{1}{2}{3}{4}貼於背蓋													
工具													