


Head 5-6GHz					
Date of Measurement	Frequency (MHz)	Return Loss (dB)	Delta (%)	Impedance	Delta(ohm)
2017.11.27	5200	-9.69	-	25.64	-
2017.11.27	5400	-10.98	-	84.04	-
2017.11.27	5600	-13.52	-	36.63	-
2017.11.27	5800	-13.34	-	47.82	-
2019.11.26	5200	-9.70	-0.23	27.66	2.02
2019.11.26	5400	-11.02	-0.93	84.54	0.50
2019.11.26	5600	-13.34	4.23	36.02	-0.61
2019.11.26	5800	-13.49	0.69	51.67	3.85

The return loss is <math><-20\text{dB}</math>, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data>

Head 5-6GHz

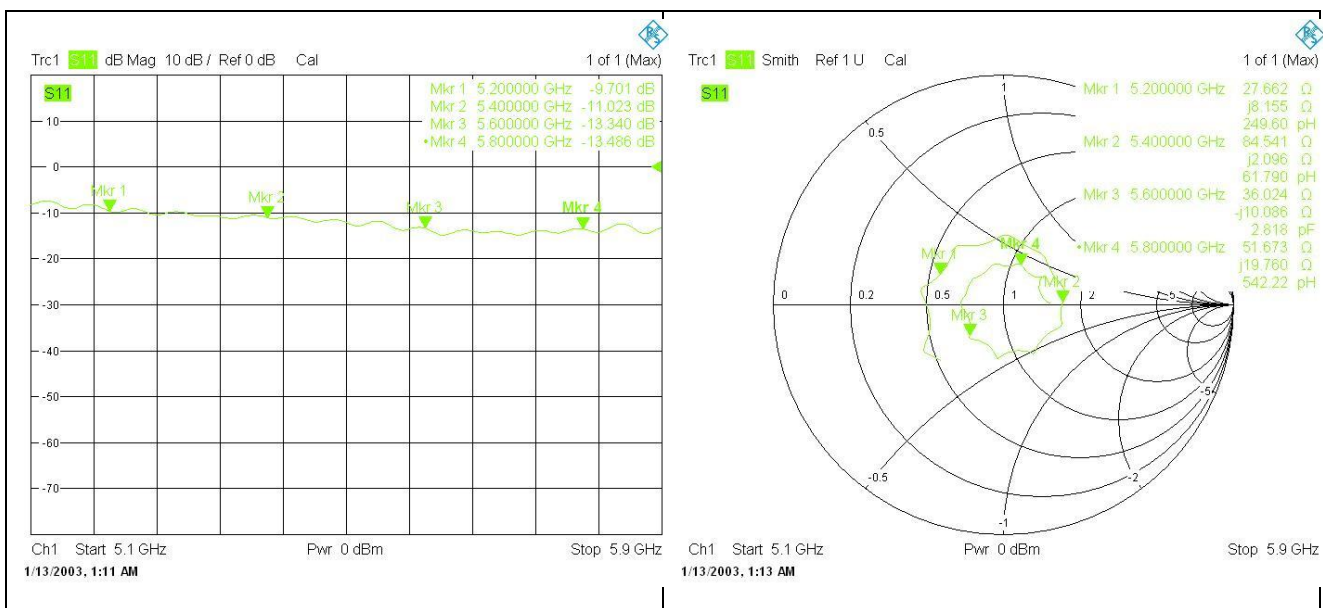

Body 5-6GHz					
Date of Measurement	Frequency (MHz)	Return Loss (dB)	Delta (%)	Impedance	Delta(ohm)
2017.11.27	5200	-8.86	-	23.97	-
2017.11.27	5400	-9.91	-	92.64	-
2017.11.27	5600	-11.72	-	32.59	-
2017.11.27	5800	-11.90	-	48.49	-
2019.11.26	5200	-8.63	5.44	24.83	0.86
2019.11.26	5400	-10.31	-9.65	92.19	-0.45
2019.11.26	5600	-11.88	-3.75	32.81	0.22
2019.11.26	5800	-11.63	6.41	52.91	4.42

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data>

Body 5-6GHz

