

Ref: CR-280-5-08-SATB-B

Page: 1/6 | Issue: B | Date: 2009/10/05

### **DIPOLE 1800 MHZ CALIBRATION REPORT**

Prepared By: LUC Jérôme, SATIMO

Project Description: SAR TEST BENCH

Prepared For (End User): Shenzhen Morlab Communication Technology

This document is issued by SATIMO, in confidence and is not to be reproduced in whole or in part without the prior written permission. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or in part without the prior written permission of SATIMO.



Ref: CR-280-5-08-SATB-B

Page: 2/6 Issue: B Date: 2009/10/05

#### **DIPOLE 1800 MHz CALIBRATION REPORT**

**DATE**: 19/02/2009

REFERENCE: SN 36/08 DIPF101

**OBJECT: COMOSAR IEEE REFERENCE DIPOLE** 

**MANUFACTURER: SATIMO** 

SERIAL NUMBER: SN 36/08 DIPF101

**CUSTOMER:** Shenzhen Morlab Communication Technology

**CONTRACT**: PF2130108b\_SAR\_Morlab

DATE OF CALIBRATION: 23/09/2009

#### **WARRANTY:**

This Calibration certificate may not be reproduced other than in full. Calibration certificates without signature and seal are not valid. This documentation contains property information which is protected by copyright. All right are reserved. No part of this document may be photocopied, reproduced without the prior written agreement of SATIMO. SATIMO shall not be liable for errors contained herein or for incidental or consequential in connection with the furnishing, performance or use of this material. Warranty doesn't apply to Normal wear, Normal tear, Improper use, Improper maintain, Improper installation.

Date

2009/10/05

SAR TEAM MANAGER


SATIMO Bretagne
Technopôle Brest Iroise
Zone du Vernis
225 rue Pierre Rivoalon
29200 BREST



Ref: CR-280-5-08-SATB-B

### PRODUCT DESCRIPTION





Dimension: L=72 mm/ h=41.7 mm / d=3.6 mm

### **CALIBRATION TEST EQUIPMENT**

TYPE	IDENTIFICATION	DATE OF CALIBRATION
Vector Network Analyzer	HP8753D (SN: 5410A08882)	10-05-2009


### **MEASUREMENT PROCEDURE**

We placed the dipole under the flat part of SAM phantom fill with 1800 MHz head liquid.




Ref: CR-280-5-08-SATB-B

Page: 4/6 Issue: B Date: 2009/10/05

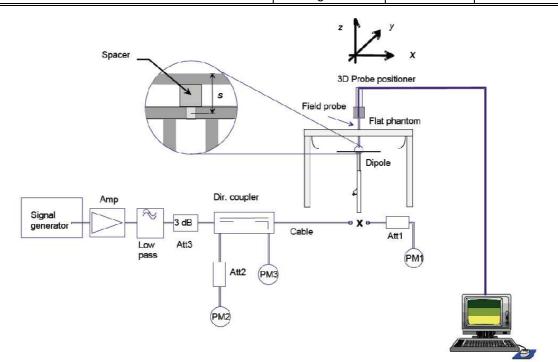

Calibration was performed according to IEEE Std P1528-2003 and OET bulletin 65 Supplement C (Ed. 01-01)

### VSWR at 1800 MHz: -25.09 dB

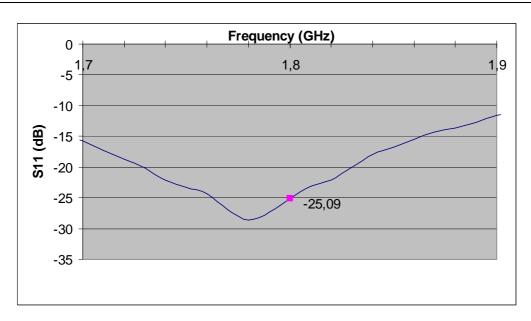



Ref: CR-280-5-08-SATB-B

Page: 5/6 Issue: B Date: 2009/10/05

### **SAR MEASUREMENT EQUIPEMENT**

Voltmeter	Keithley (2000, SN:1000572)	Date of calibration: 01-07-2009
Signal generator	Rohde&Schwarz (SML_03, SN:101868)	Date of calibration: 15-11-2008
Power amplifier	Nuclétudes (ALB216, SN:10800)	Date of calibration: 24-10-2008
Power meter	Rohde&Schwarz (NRVD, SN:101066)	Date of calibration: 04-07-2009
Probe	SATIMO Bretagne (SN:EP37)	Date of calibration: 19-06-2009
	CF (35.35,34.93,37.42)	

#### **SAR MEASUREMENT CONDITION**

Software	OpenSAR V3	
Phantom	SATIMO Bretagne (SN: SN_20_07_SAM42)	
Liquid	SATIMO Bretagne (Last Calibration: 19 09 08) Head Liquid Values: eps': 39,80 sigma: 1,45	
Distance between the center of the dipole and the liquid (set with a spacer)	10 mm	
Area scan resolution	dx=8mm/dy=8mm	
Zoom scan resolution	dx=8mm/dy=8m/dz=5mm	
Frequency	1800 MHz	
Input power	30 dBm	
Expanded uncertainty (K=1)	8.09%	

### SAR MEASUREMENT RESULT

	10g	1g
SAR measured Liquid : HL Input power : 1W	20,05 W/Kg + 1,24 %	39,32 W/Kg + 3,20 %



Ref: CR-280-5-08-SATB-B

Page: 6/6 | Issue: B | Date: 2009/10/05

#### **SAR MEASUREMENT PLOTS**

