

System Check_Head_750MHz

DUT: D750V3-1107

Communication System: CW ; Frequency: 750.0 ; Duty Cycle: 1:1
Medium: HSL_750_221213. Medium parameters used: $f=750.0$ MHz; $\sigma=0.886$ S/m; $\epsilon_r=42.7$
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(10.45, 10.45, 10.45); Calibrated: 2022-01-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2022-11-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926
- UID: CW, 0--
- MAIA: Area Scan: N/A; Zoom Scan: N/A


Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.412 W/kg; SAR (10g) = 0.273 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 0.418 W/kg; SAR (8g) = 0.285 W/kg; SAR (10g) = 0.270 W/kg

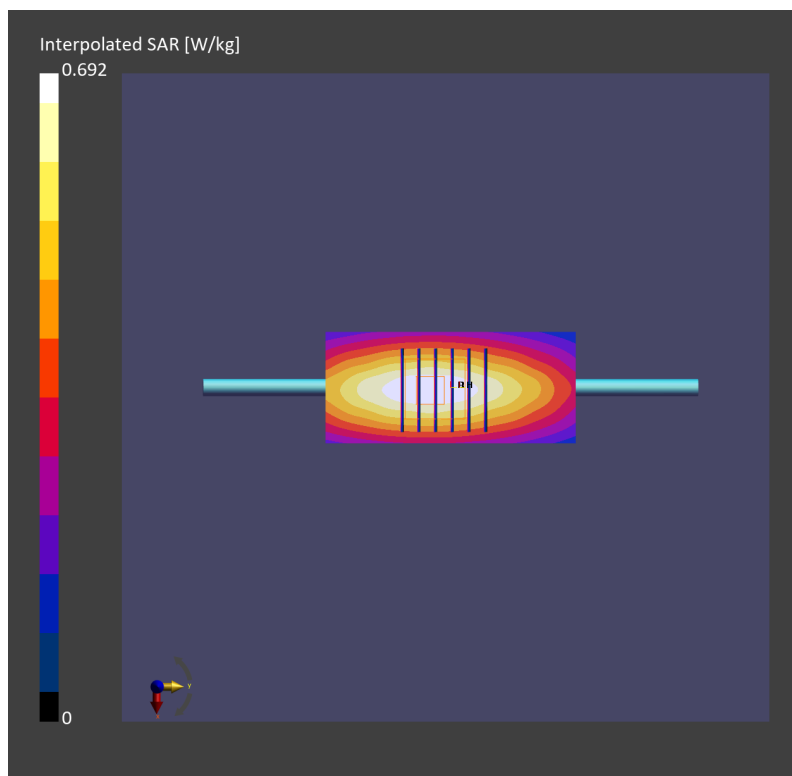

System Check_Head_835MHz

DUT: D835V2-4d167


Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1
Medium: HSL_850_221213 Medium parameters used: $f= 835.0$ MHz; $\sigma= 0.908$ S/m; $\epsilon_r = 42.2$
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(10.21, 10.21, 10.21); Calibrated: 2022-01-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2022-11-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 0.508 W/kg; SAR (10g) = 0.329 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 0.516 W/kg; SAR (8g) = 0.345 W/kg; SAR (10g) = 0.326 W/kg

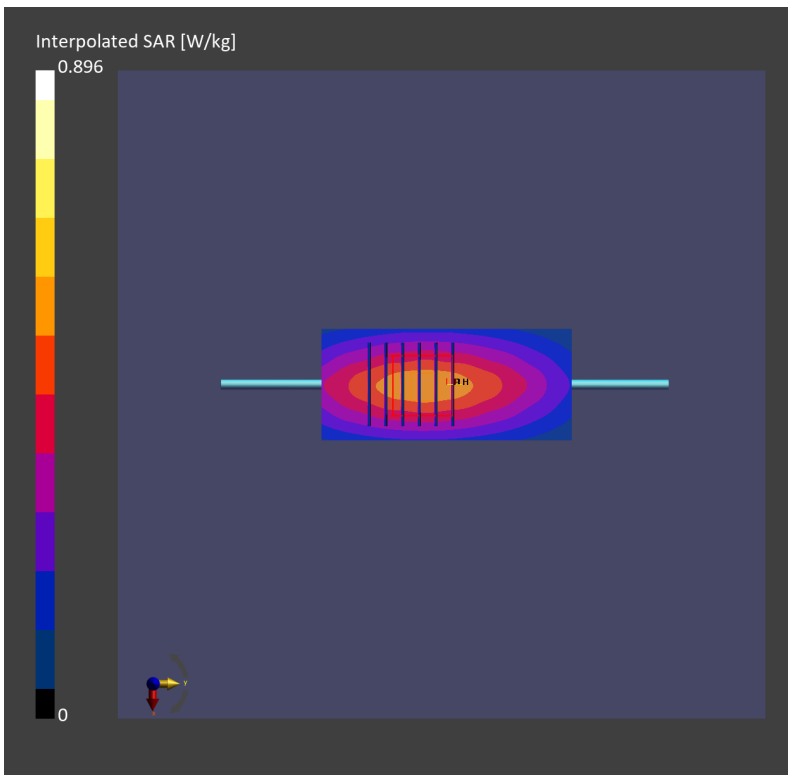

System Check_Head_1750MHz

DUT: D1750V2-1112

Communication System: CW; Frequency: 1750.0 ; Duty Cycle: 1:1
Medium: HSL_1750_221211 Medium parameters used: $f=1750.0$ MHz; $\sigma=1.38$ S/m; $\epsilon_r=41.0$
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.0, 9.0, 9.0); Calibrated: 2022-01-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2022-11-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926
- UID: CW
- MAIA: Area Scan: N/A; Zoom Scan: N/A


Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.65 W/kg; SAR (10g) = 0.877 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.03 dB

SAR (1g) = 1.67 W/kg; SAR (8g) = 0.959 W/kg; SAR (10g) = 0.885 W/kg;

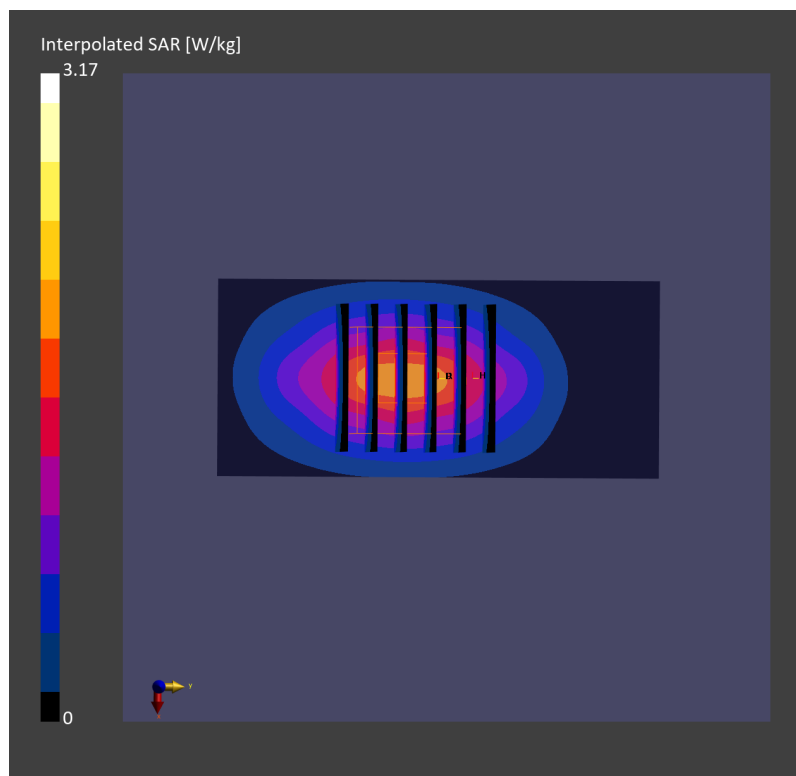

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093


Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1
Medium:HSL_1900_221211 Medium parameters used: $f=1900.0$ MHz; $\sigma=1.46$ S/m; $\epsilon_r=39.5$
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.49, 8.49, 8.49); Calibrated: 2022-01-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2022-11-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.84 W/kg; SAR (10g) = 0.975 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 1.88 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.979 W/kg

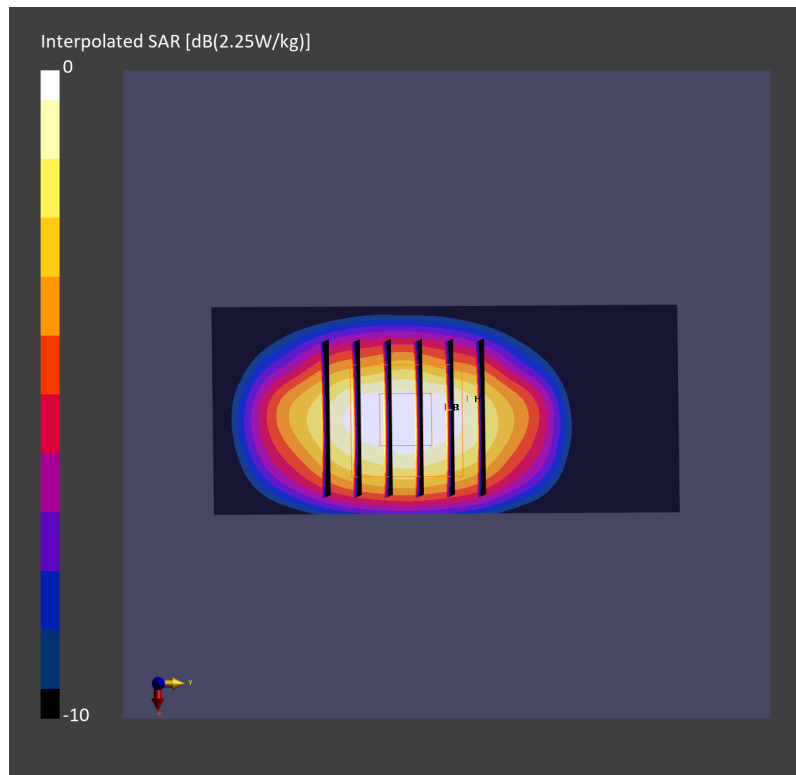

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: CW; Frequency: 2600.0 ; Duty Cycle: 1:1
Medium: HSL_2600_221212 Medium parameters used: $f=2600.0$ MHz; $\sigma=1.93$ S/m; $\epsilon_r=38.0$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.82, 7.82, 7.82); Calibrated: 2022-01-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2022-11-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926
- UID: CW
- MAIA: Area Scan: N/A; Zoom Scan: N/A

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.39 W/kg; SAR (10g) = 1.06 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.14 dB
SAR (1g) = 2.53 W/kg; SAR (8g) = 1.20 W/kg; SAR (10g) = 1.18 W/kg;

