

Compliance Testing Model Uni SAR Report

Prepared By:

James F. Stack, Jr.

Remcom, Inc.

21 July 2011

1. Introduction

This SAR computation modeling is performed to show compliance to radio frequency exposure limits as defined in 47 CFR Part 1, section 1.1307 and in 47 CFR Part 2, section 2.1093. The usage of the equipment is uncontrolled, therefore the limit for partial-body SAR is 1.6 W/kg, as averaged over any 1 g cubical tissue volume. The whole-body limit for average SAR is 0.08 W/kg.

2. Scope

This report scope illustrates compliance as required in 47 CFR Part 95, section 95.603(f) for the Compliance Testing Model S4 SAR Report.

3. Summary

The maximum SAR values were computed and listed in Table 1.

Whole-body average SAR	4.684e-10 W/kg
Partial-body maximum 1g average SAR	8.883e-10 W/kg

Table 1 Computed SAR levels summary

4. Method and Simulation Parameters

XFDTD version 7.2.0.5, developed by Remcom, Inc. (1), was used for the simulations. The software uses the Finite Difference Time-Domain (FDTD) method for electromagnetic calculation, as described in (2).

4.1. Model and Material Details

A CAD model of the parts relevant to antenna operation of the implanted device was imported into XFDTD as shown in Figure 1. The device was situated within a biological flat phantom that was 445.788 mm long (in the y-direction), 297.192 mm wide (in the x-direction), and 150 mm in depth (z-direction), as shown in Figure 2. The dimensions of the flat phantom were set based on specifications as defined in section D.9.2 (Experimental Body Phantom) of (3).

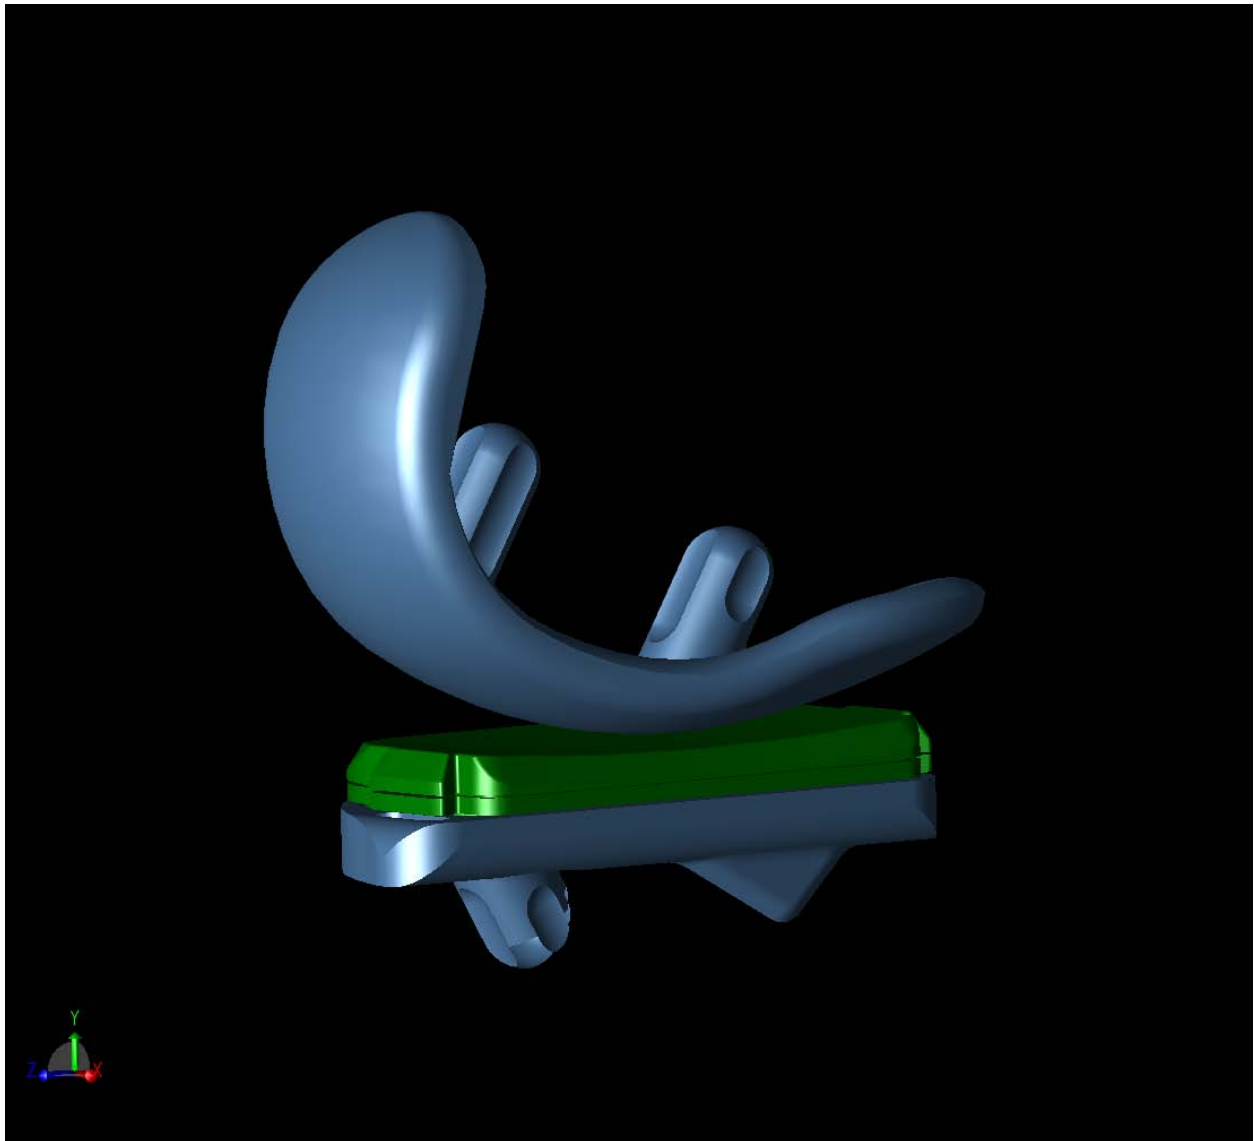


Figure 1 Device CAD file as displayed in XFtdt

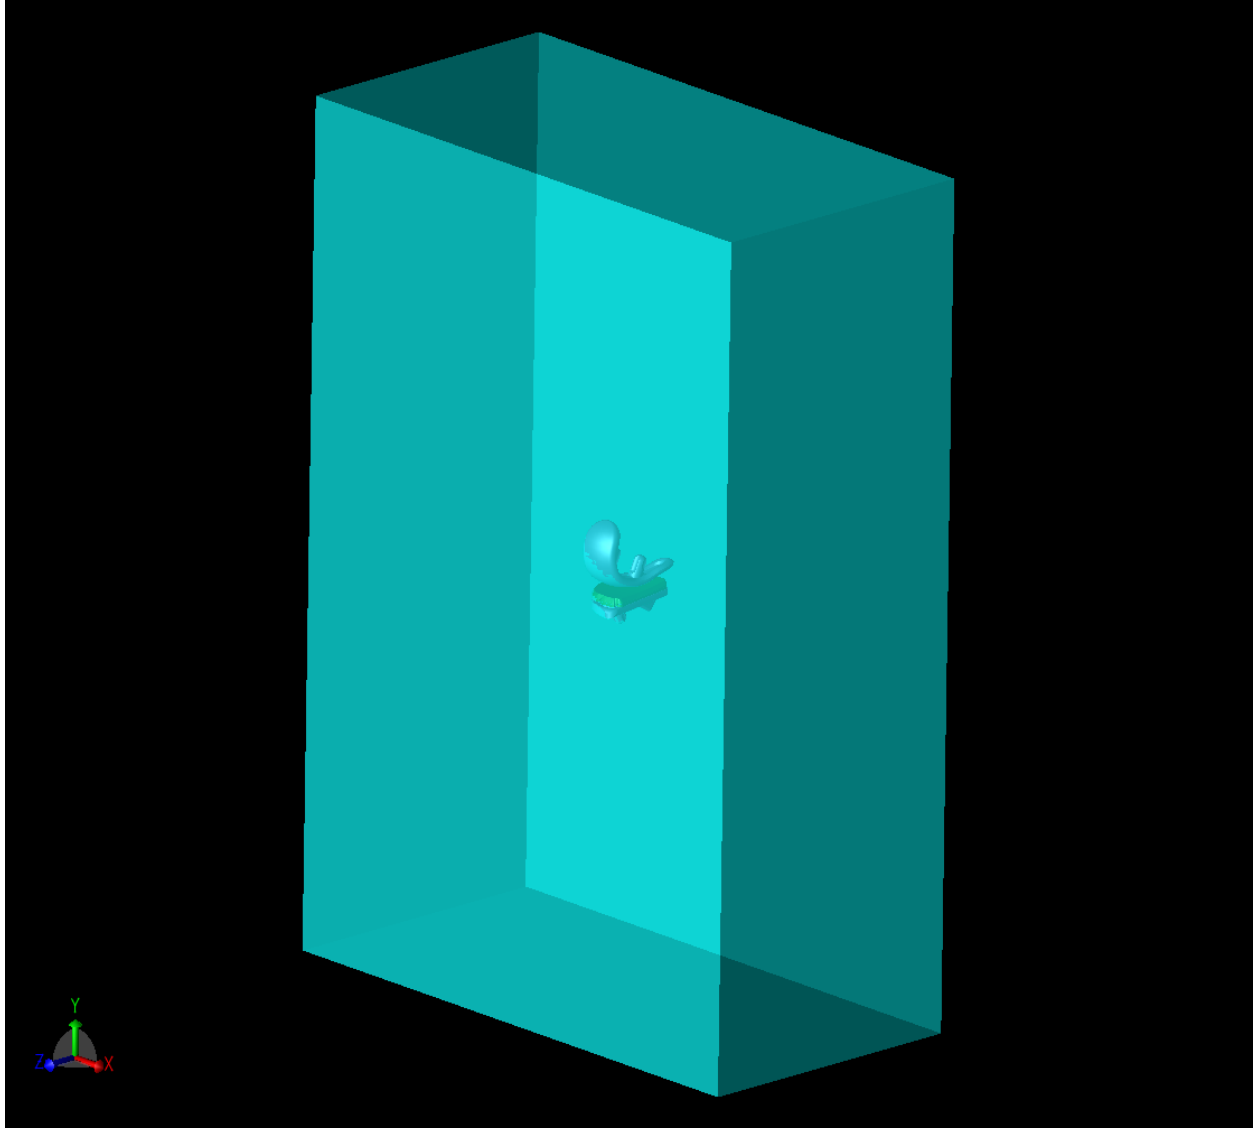


Figure 2 Device placed in flat phantom with XYZ coordinate axis shown

In order to provide a worst-case SAR analysis (with no losses in the conducting elements as would be seen in a real metal conductor), Perfect Electrical Conductor (PEC) was used on all conductive parts of the device. All dielectric materials were modeled as lossless. The flat phantom was modeled using electrical parameters as described in Appendix C of (4). Since the device is intended to be implanted into a human knee, the tissue dielectric properties for the body were used. Linear interpolation was performed to generate property values for the target frequency of 403.5 MHz. The dielectric material parameters used are listed in Table 2.

Material	Relative Permittivity	Conductivity	Density
PEC	0	Infinite	n/a
Accura 90 (SLA Plastic)	3	0	n/a
AP 8535R	3.4	0	n/a
Bayer Makrolon (Polycarbonate)	3	0	n/a
LOCTITE 3972 (Glue)	3	0	n/a
Polyurethane Foam	2	0	n/a
Rogers PORON 4701-30 (Si Foam)	1.75	0	n/a
Flat Phantom	57.165	0.9338 S/m	1,000 kg/m ³

Table 2 Dielectric properties of materials used in the simulations

4.2. Gridding Parameters

The user must define the grid size according to limits determined by the highest frequency to be considered as well as the geometry of the object being simulated. At an operating frequency of 403.5 MHz, the largest cell size supported is 74 mm. This maximum size, however, was not used as it would not adequately resolve the geometry of the objects in the simulation. The maximum cell size used in this simulation was 9.8 mm. The software will support multiple cell sizes within a single project. A cell size of 0.6 mm was chosen for the cells comprising the device, and a finer cell sizes were employed near the radiating element. Additionally, fixed points were used so that grid lines were placed along edges and other important parts of the geometry so that the size of the object was adequately represented by the cells.

To further resolve the antenna, XF's XACT feature was used on the radiating element. XACT is a subcellular modeling technique capable of accurately capturing curved surfaces that pass through a traditional FDTD grid (1).

The grid sizes used are summarized in Table 3. Figure 3 and Figure 4 display the grid lines as viewed in two of the principle plans. Figure 5 demonstrates how XACT captures the curves of the antenna through the rectangular FDTD grid.

Grid Region	Cell Size	Electrical Size (in freespace)
Base cell size	9.8 mm	0.0132* λ
Device cell size	0.6 mm	8.076e-4* λ
PCB cell size	0.127 mm	1.71e-4* λ
Antenna Trace cell size (vertical)	0.018 mm	2.43e-5* λ

Table 3 Summary of cell sizes used in the simulations

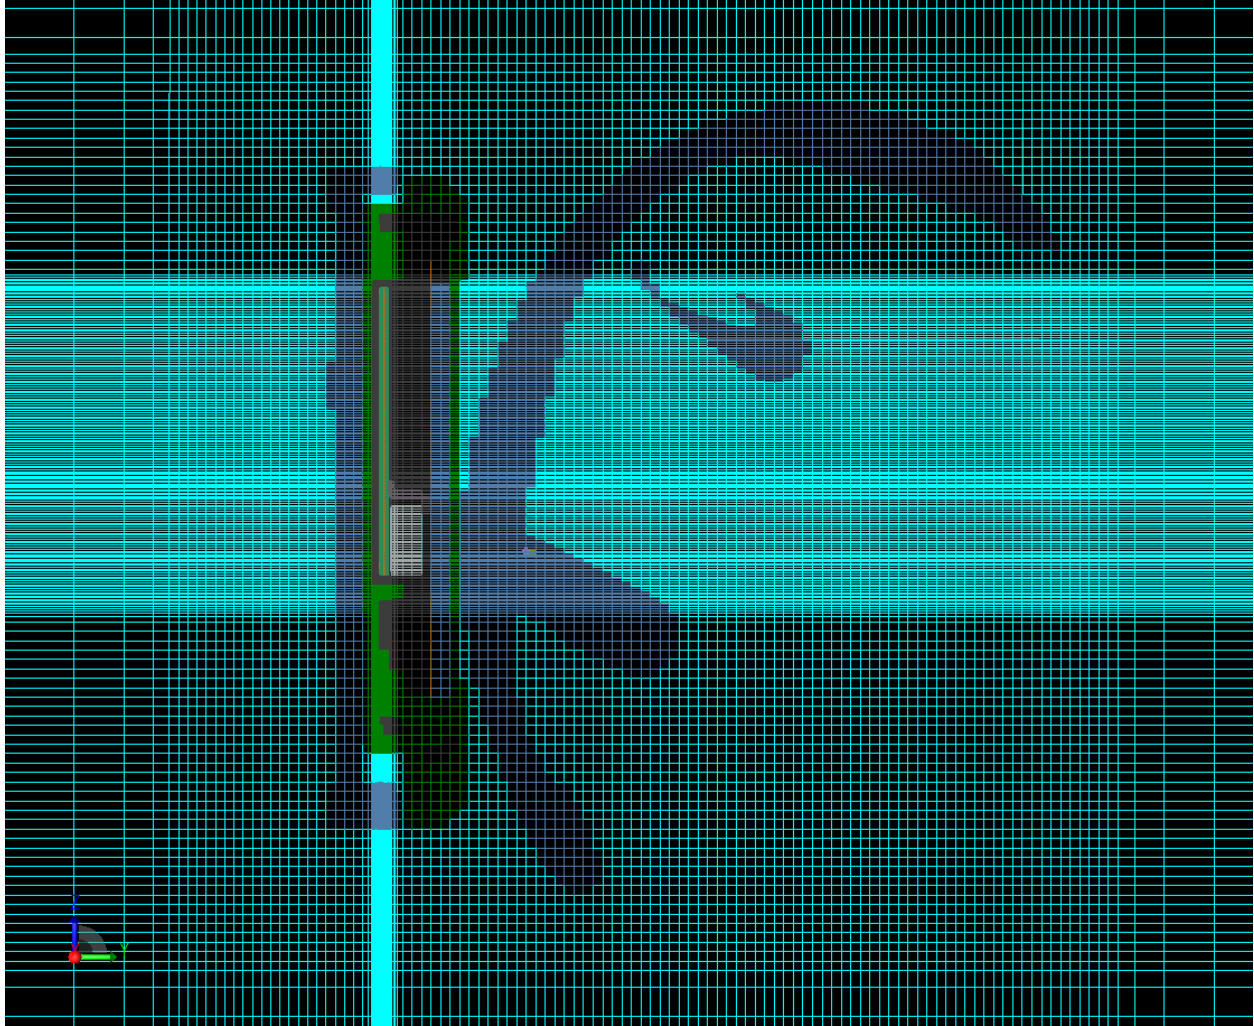


Figure 3 FDTD grid lines in YZ plane

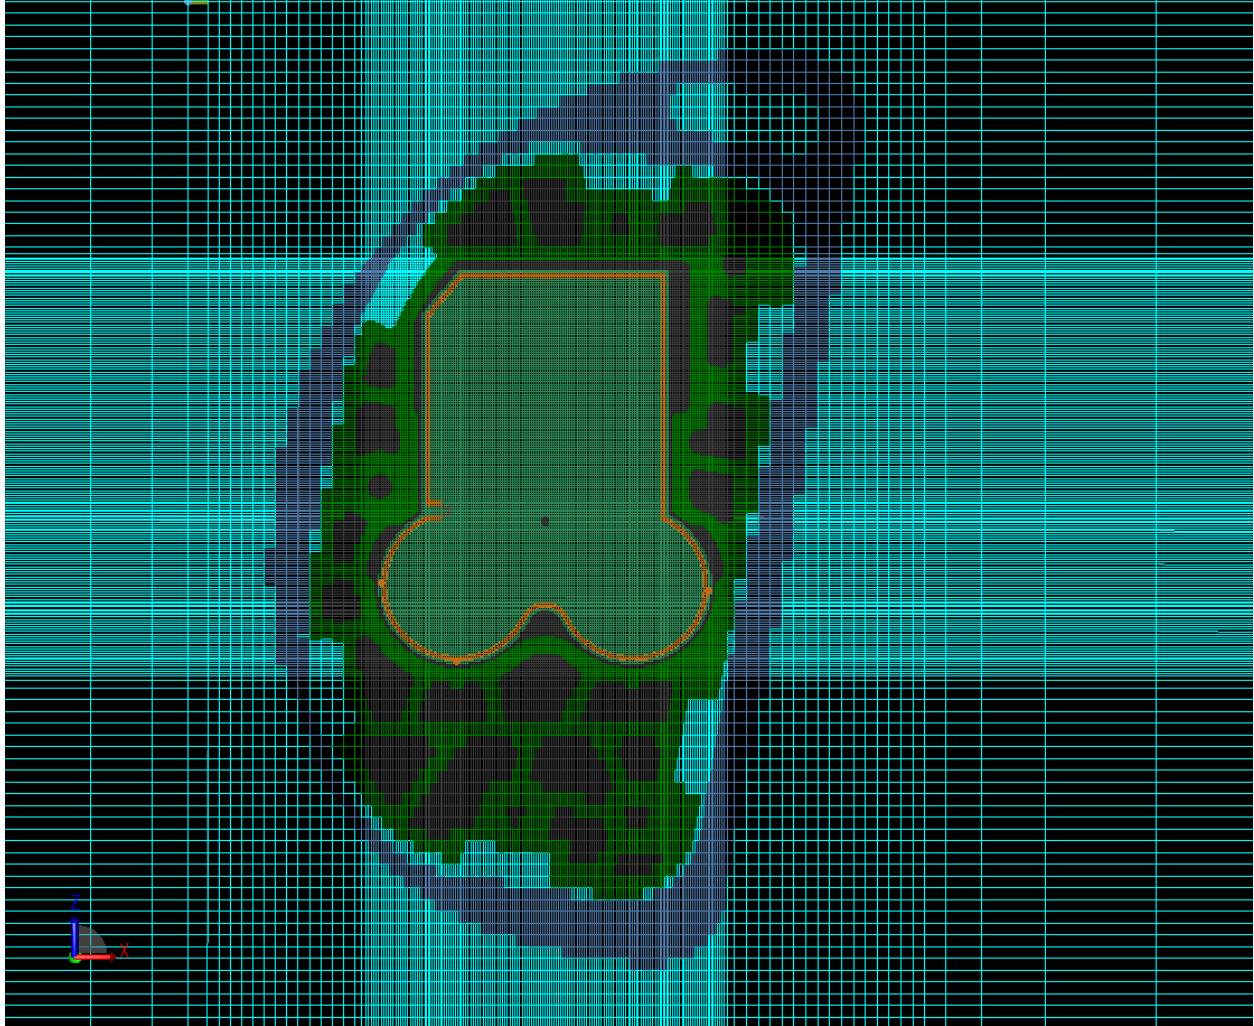


Figure 4 FDTD grid lines in ZX plane

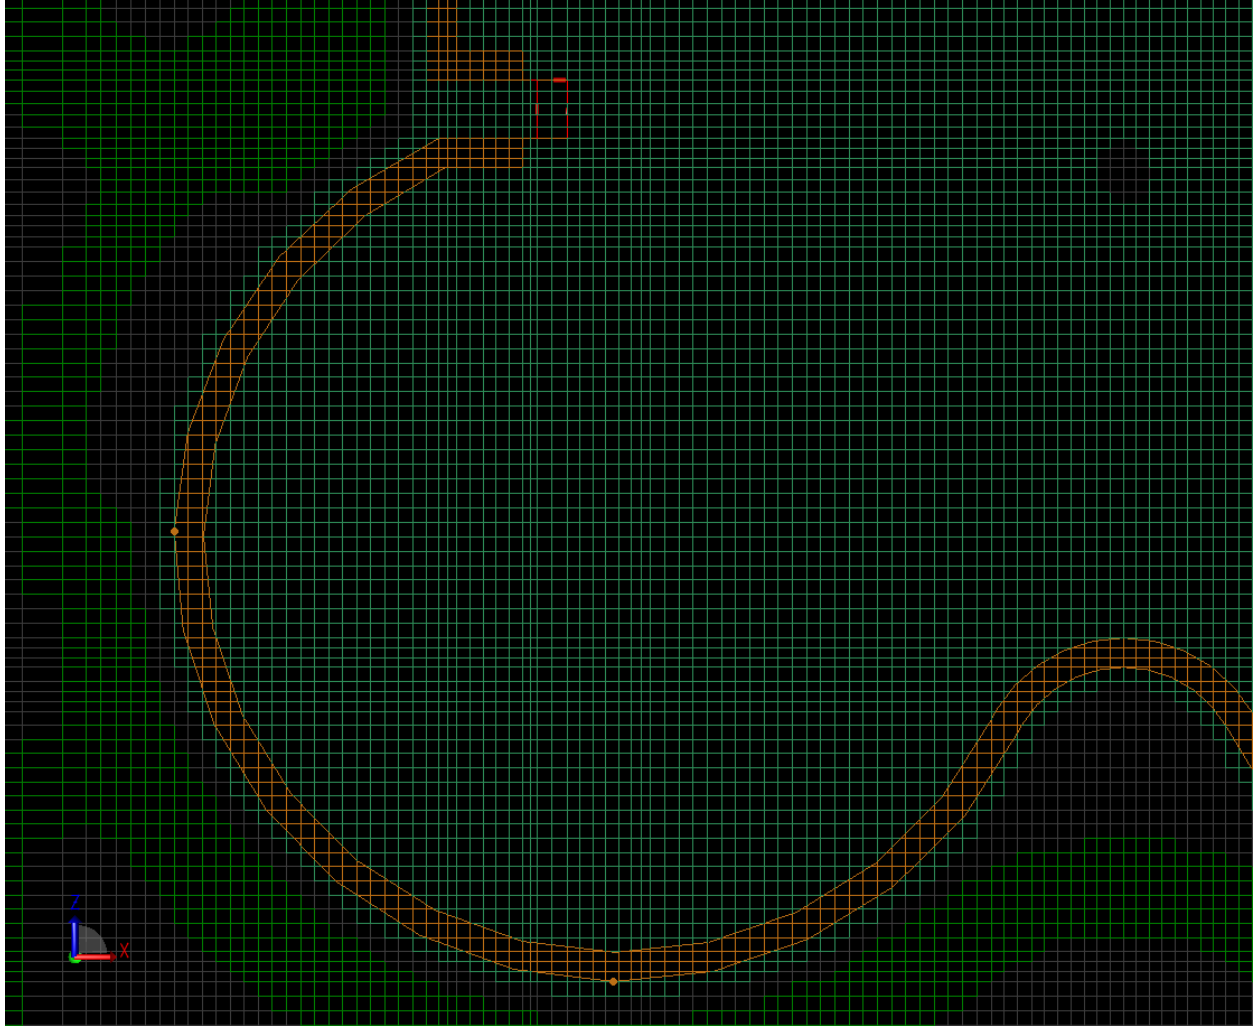


Figure 5 Close-up view of portion of the antenna with XACT enabled

The base FDTD grid sizes listed above were chosen using experience and best practices for modeling such devices. The grid sizes chosen were validated by running additional simulations using sizes 0.5 and then 0.25 times the device cell sizes and verifying that the results remained the same to within a small tolerance.

4.3. Description of Simulated Device

The implantable medical device that was simulated is shown in Figure 1. The CAD model was used for the simulation and thus was representative of the device. All relevant parts of the device were included in the model.

4.4. Input Power and Source Excitation

In order to calculate the worst-case SAR values, the waveform used to excite the antenna was a 1 V peak-to-peak sinusoid (therefore 100% duty cycle) at 403.5 MHz. An initial simulation found the input impedance of the antenna (while in the device and embedded in the flat phantom

material) to be $0 + j67.7 \Omega$. An impedance-matching network was then used to feed the device. The components comprising the voltage source and matching network were fed between the leads to the loop antenna, as shown in Figure 6. This matching circuit was used solely for the purpose of ensuring that a meaningful amount of energy was introduced into the simulation space for later scaling. After the simulation was completed, the available power was scaled within the software to 1 mW (0 dBm), with the SAR values automatically scaled accordingly. This scaled power represents the maximum amount of power that could be delivered to the antenna assuming a perfect impedance match.

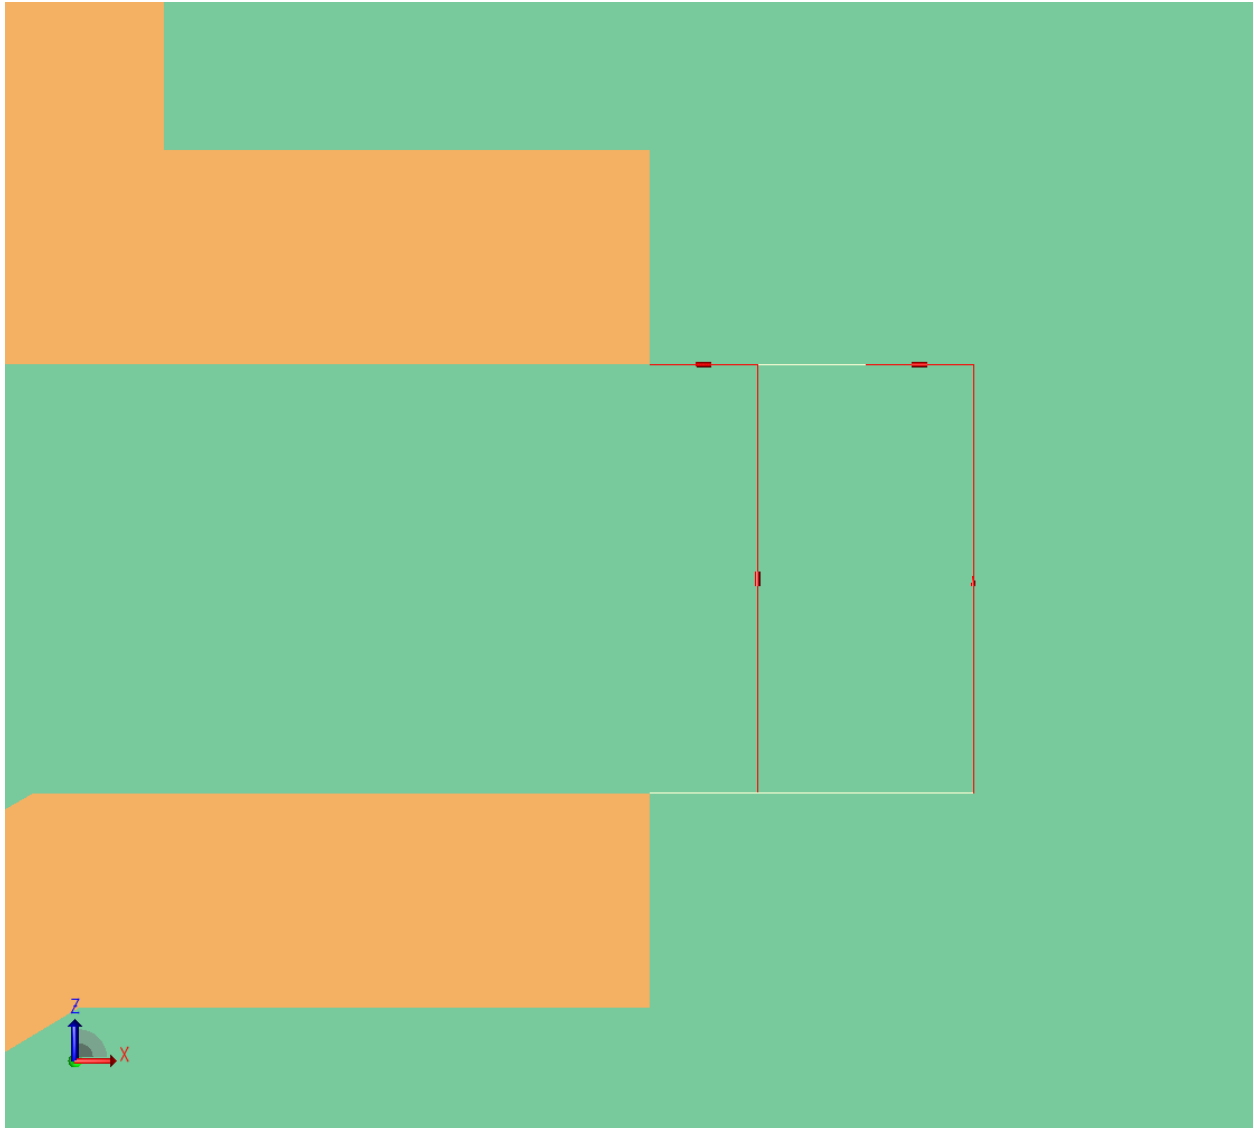


Figure 6 Voltage source (red cone) and matching network (red cylinders) used to feed the device

5. Worst-Case SAR Analysis / Results

The device was modeled in the middle of the frequency band since there was little expected difference between the upper and lower bounds. The software calculates whole body SAR and partial-body SAR using the method compliant with (3).

The worst-case average SAR values were calculated and found to be $4.68\text{e-}10$ W/kg for whole-body averaged SAR and $8.88\text{e-}10$ W/kg for partial-body 1g averaged SAR, also shown in Table 1. This worst-case analysis neglects the effects of material losses, mismatch loss, and waveform duty cycle that will further reduce the final averaged SAR.

The SAR results at the initial device cell size showed significant variation from the average value given by the half and quarter cell sizes; however, all simulations demonstrated averaged SAR values over nine orders of magnitude below the acceptable threshold. A set of additional simulations using one-eighth of the initial cell sizes was attempted but required too much memory to be completed in any reasonable amount of time as a result of the small nature of the device. The simulations indicate that the electrically-small loop antenna is functioning as a pure inductor. Thus, the electromagnetic fields are strong very close to the antenna but do not propagate significantly beyond the device.

The results of the individual simulations are summarized in Table 4. A graphical representation of the 1g SAR results scaled to a net input power of 0 dBm is presented in Figure 7.

Cell Size	1g Averaged SAR	Whole Body Average SAR
Full	$3.34\text{e-}10$ W/kg	$5.44\text{e-}14$ W/kg
Half	$7.46\text{e-}10$ W/kg	$4.10\text{e-}10$ W/kg
Quarter	$8.88\text{e-}10$ W/kg	$4.68\text{e-}10$ W/kg

Table 4 Summary of SAR results

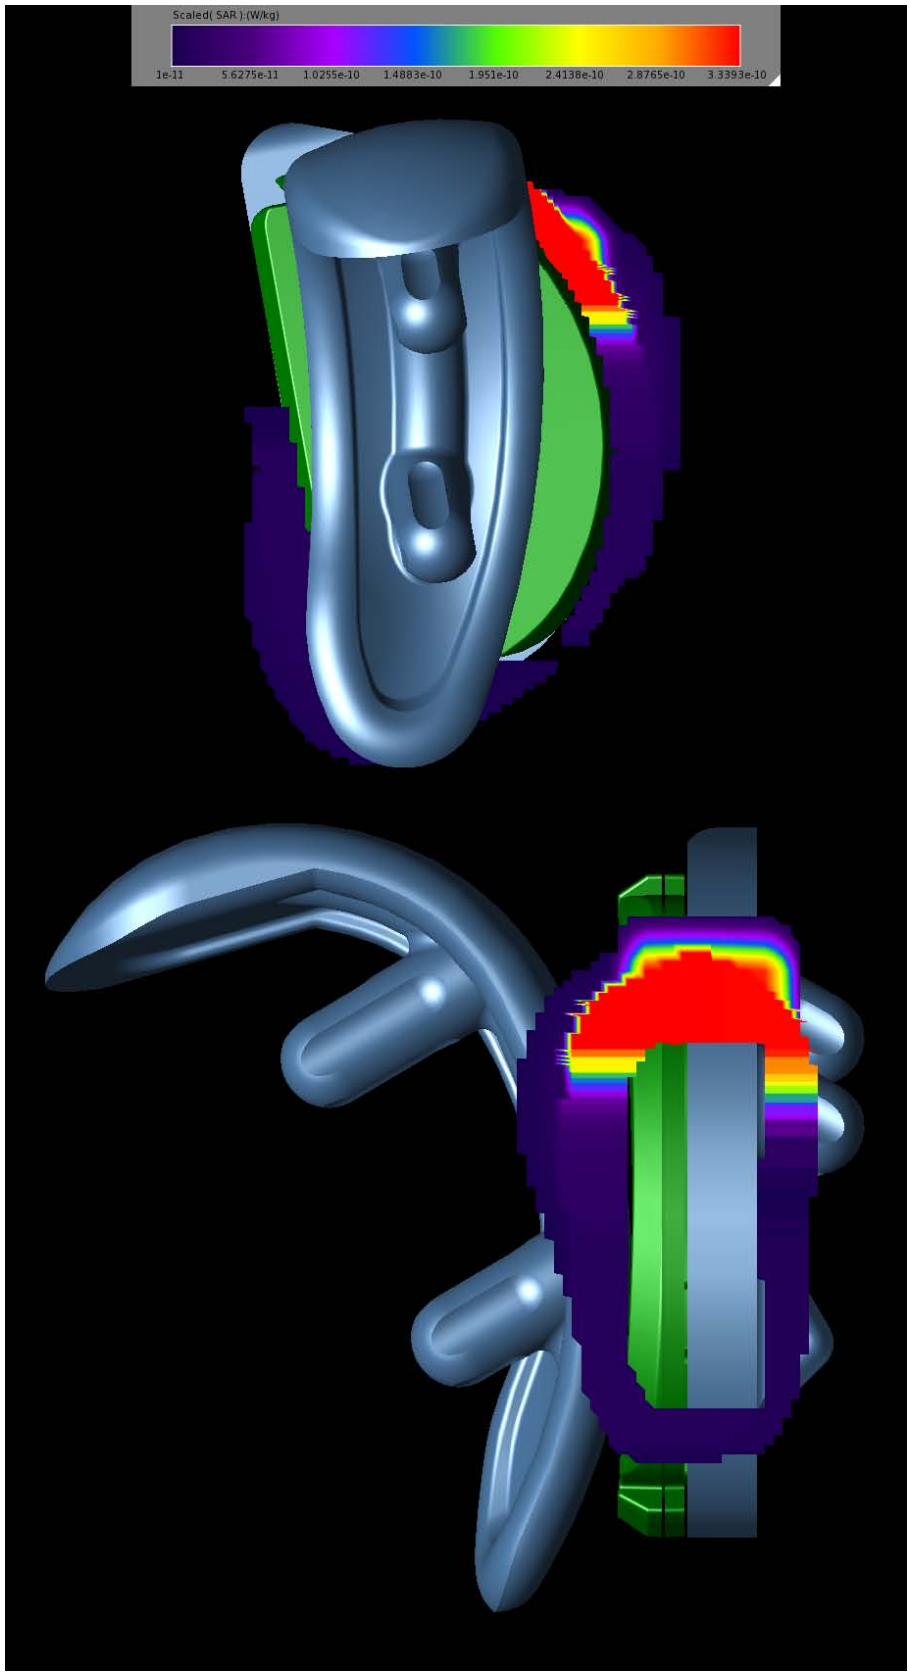


Figure 7 Graphical Display of 1g Averaged SAR Results

6. Compliance

The results shown in Section 5 are below the limit for whole-body SAR and partial-body SAR.

7. OET 65C

These sections will satisfy the OET 65C document (4). Information will be provided either in the section or referenced elsewhere in the document.

7.1. Computational Resources

System Specifications				
Processors:	(2) Intel Xeon 5660			
GPU:	(6) NVIDIA Tesla C2070			
RAM:	48GB			
Operating System:	CentOS 5.5 x86_64			
Simulation Specifications				
	Number of Cells (MCells)	RAM Required (GB)	Time Step Duration (us)	Time Steps to Convergence
Device at Full Cell Size:	17.4	1.1	3.24e-8	400,100
Device at Half Cell Size:	75.9	4.2	1.94e-8	800,100
Device at Quarter Cell Size:	464.5	24.6	9.69e-14	1,600,100

Table 5 System and Simulation Computational Resources

7.2. FDTD Algorithm Implementation and Validation

See Section 4.

7.3. Computational Parameters

See Section 4.

7.4. Phantom Implementation and Validation

See Section 4.

7.5. Tissue Dielectric Parameters

See Section 4.

7.6. Transmitter Model Implementation and Validation

See Section 4.

7.7. Test Device Positioning

Device was positioned in the middle of the flat phantom.

7.8. Steady State Termination Procedures

The simulation was terminated when the software auto-convergence detector indicated at least -40 dB of convergence.

7.9. Computing Peak SAR from Field Components

See Section 5.

7.10. One Gram Averaged SAR Procedures

See Section 5.

7.11. Total Computational Uncertainty

It is estimated that the total uncertainty is below 10%.

7.12. Test Results for Determining SAR Compliance

See Section 5.

8. References

1. Remcom, Inc. [Online] www.Remcom.com.
2. **Kunz, K. S. and Luebbers, R. J.** *The Finite Difference Time Domain Method for Electromagnetics*. New York : CRC Press, 1993.
3. **Committee, P1528.1 Working Group of the IEEE/ICES/TC34/SC2.** *IEEE P1528.1™/D1.00 Draft Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body from Wireless Communications Devices, 30 MHz - 6 GHz: General Requirements for using the Finite Difference Time Domain*. 2010. (16 December 2010 revision)
4. *FCC OET Bulletin 65, supplement C*.