

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY/EASY – Parameters of Probe: EX3DV4 – SN:3767

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	41.9	0.89	9.99	9.99	9.99	0.16	1.21	± 12.7%
835	41.5	0.90	9.61	9.61	9.61	0.14	1.42	± 12.7%
900	41.5	0.97	9.64	9.64	9.64	0.19	1.24	± 12.7%
1450	40.5	1.20	8.60	8.60	8.60	0.11	1.37	± 12.7%
1750	40.1	1.37	8.32	8.32	8.32	0.26	0.98	± 12.7%
1900	40.0	1.40	8.13	8.13	8.13	0.22	1.08	± 12.7%
2000	40.0	1.40	8.10	8.10	8.10	0.26	1.03	± 12.7%
2300	39.5	1.67	7.87	7.87	7.87	0.62	0.66	± 12.7%
2450	39.2	1.80	7.62	7.62	7.62	0.66	0.67	± 12.7%
2600	39.0	1.96	7.45	7.45	7.45	0.47	0.82	± 12.7%
3300	38.2	2.71	7.19	7.19	7.19	0.38	1.04	± 13.9%
3500	37.9	2.91	6.95	6.95	6.95	0.44	0.97	± 13.9%
3700	37.7	3.12	6.73	6.73	6.73	0.44	1.00	± 13.9%
3900	37.5	3.32	6.63	6.63	6.63	0.35	1.35	± 13.9%
4100	37.2	3.53	6.56	6.56	6.56	0.35	1.25	± 13.9%
4400	36.9	3.84	6.35	6.35	6.35	0.30	1.56	± 13.9%
4600	36.7	4.04	6.27	6.27	6.27	0.35	1.48	± 13.9%
4800	36.4	4.25	6.29	6.29	6.29	0.35	1.60	± 13.9%
4950	36.3	4.40	5.94	5.94	5.94	0.35	1.55	± 13.9%
5200	36.0	4.66	5.55	5.55	5.55	0.40	1.45	± 13.9%
5300	35.9	4.76	5.35	5.35	5.35	0.40	1.40	± 13.9%
5500	35.6	4.96	5.05	5.05	5.05	0.45	1.40	± 13.9%
5600	35.5	5.07	4.97	4.97	4.97	0.50	1.33	± 13.9%
5800	35.3	5.27	4.92	4.92	4.92	0.45	1.40	± 13.9%


^C Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency up to 6 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


Certificate No:J23Z60239

Page 4 of 9



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62304633-2117
 E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

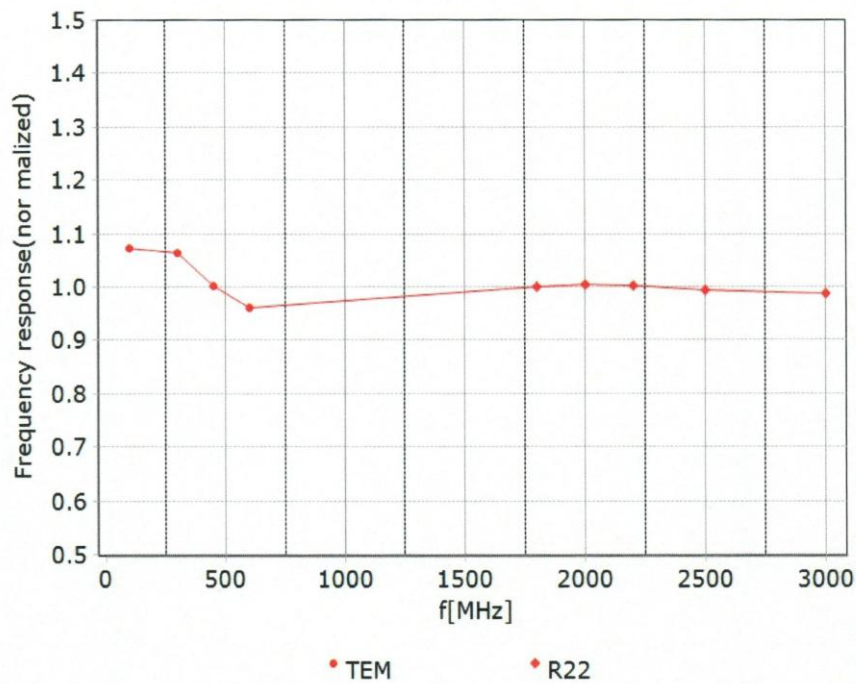

Uncertainty of Frequency Response of E-field: $\pm 7.4\%$ ($k=2$)






Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62304633-2117
 E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Receiving Pattern (Φ), $\theta=0^\circ$

f=600 MHz, TEM

f=1800 MHz, R22

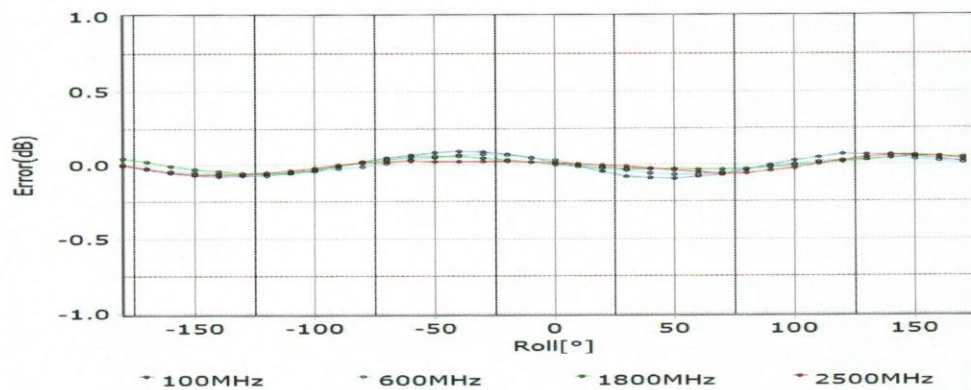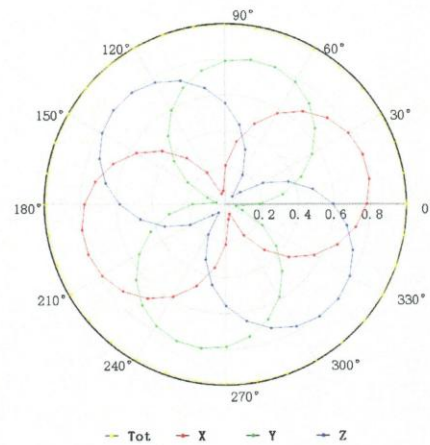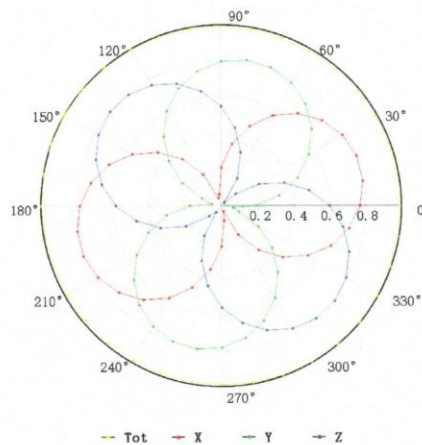

Uncertainty of Axial Isotropy Assessment: $\pm 1.2\%$ ($k=2$)



Certificate No: J23Z60239

Page 6 of 9



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62304633-2117
 E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Dynamic Range f(SAR_{head}) (TEM cell, f = 900 MHz)

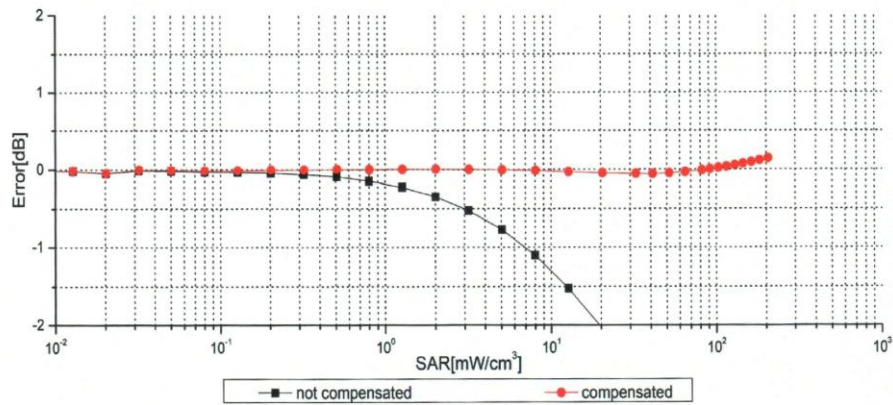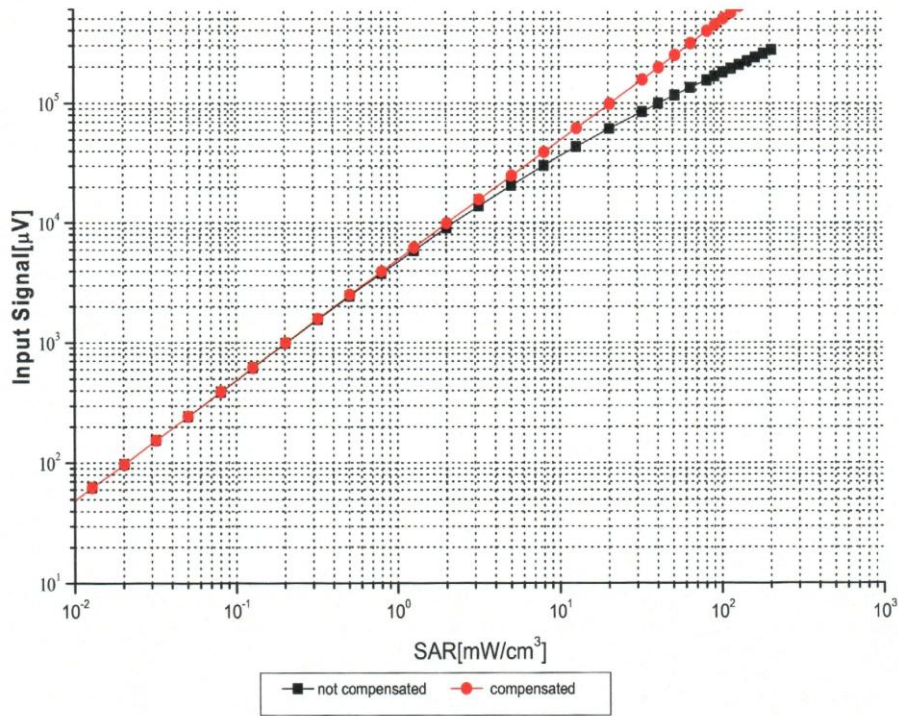

Uncertainty of Linearity Assessment: $\pm 0.9\%$ ($k=2$)

Certificate No:J23Z60239

Page 7 of 9





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>


Conversion Factor Assessment

f=750 MHz,WGLS R9(H_convF)

f=1750 MHz,WGLS R22(H_convF)

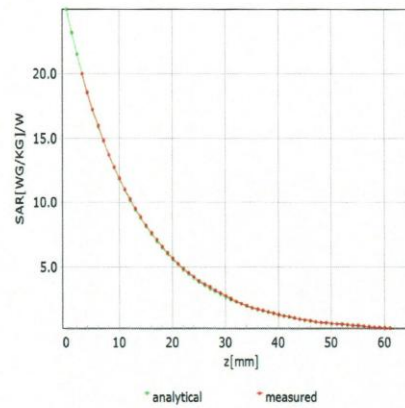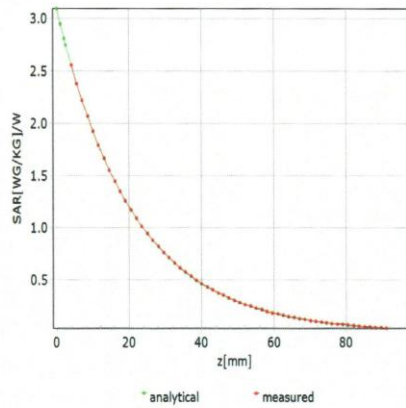


Deviation from Isotropy in Liquid

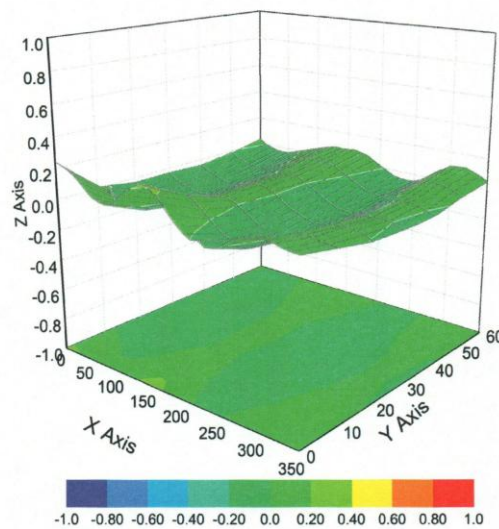

Uncertainty of Spherical Isotropy Assessment: $\pm 3.2\%$ ($k=2$)

Certificate No:J23Z60239

Page 8 of 9



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY/EASY – Parameters of Probe: EX3DV4 – SN:3767

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	151.2
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	9mm
Tip Diameter	2.5mm
Probe Tip to Sensor X Calibration Point	1mm
Probe Tip to Sensor Y Calibration Point	1mm
Probe Tip to Sensor Z Calibration Point	1mm
Recommended Measurement Distance from Surface	1.4mm