
### Impedance Measurement Plot for Body TSL

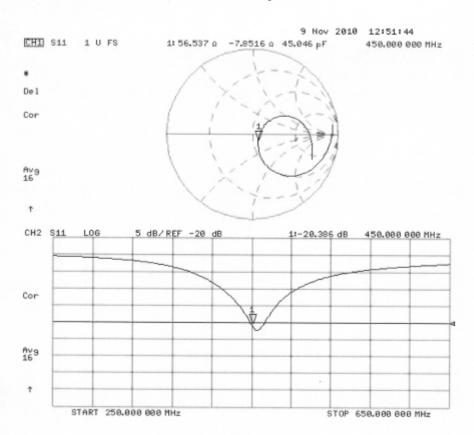

Report No. RXA1206-0320SAR

Page 82 of 108

### **ANNEX F: DAE4 Calibration Certificate**

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerlscher Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

TA-SH (Auden)

Certificate No: DAE4-871\_NoV11

Accreditation No.: SCS 108

| CALIBRATION C                          |                                      |                                                                                                          | are all                   |
|----------------------------------------|--------------------------------------|----------------------------------------------------------------------------------------------------------|---------------------------|
|                                        |                                      | Haracon y Hilling and Charles and Annah day ( Hilling                                                    |                           |
| Object                                 | DAE4 - SD 000 D                      | 04 BJ - SN: 871                                                                                          |                           |
| Calibration procedure(s)               | QA CAL-06.v23<br>Calibration process | lure for the data acquisition electron                                                                   | nics (DAE)                |
| Calibration date:                      | November 22, 20                      |                                                                                                          |                           |
| l .                                    |                                      | nal standards, which realize the physical units of<br>bbability are given on the following pages and are | · ·                       |
| All calibrations have been conducted   | ed in the closed laboratory          | r facility: environment temperature (22 ± 3)°C and                                                       | humidity < 70%.           |
| Calibration Equipment used (M&TE       | Ecritical for calibration)           |                                                                                                          |                           |
| Primary Standards                      | ID#                                  | Cal Date (Certificate No.)                                                                               | Scheduled Calibration     |
| Keithley Multimeter Type 2001          | SN: 0810278                          | 28-Sep-11 (No:11450)                                                                                     | Sep-12                    |
| Secondary Standards                    | ID#                                  | Check Date (in house)                                                                                    | Scheduled Check           |
| Calibrator Box V1.1                    | SE UMS 006 AB 1004                   | 08-Jun-11 (in house check)                                                                               | In house check: Jun-12    |
|                                        |                                      |                                                                                                          |                           |
| Calibrated by:                         | Name<br>Andrea Guntir                | Function<br>Technician                                                                                   | Signature                 |
| Approved by:                           | Fin Bomholt                          | R&D Director : iV                                                                                        | Muus                      |
| This calibration certificate shall not | be reproduced except in t            | full without written approval of the laboratory.                                                         | Issued: November 22, 2011 |

Certificate No: DAE4-871\_Nov11

Report No. RXA1206-0320SAR

Page 83 of 108

#### **Calibration Laboratory of**

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

#### Glossary

DAE

data acquisition electronics

Connector angle

information used in DASY system to align probe sensor X to the robot

coordinate system.

#### **Methods Applied and Interpretation of Parameters**

Multilateral Agreement for the recognition of calibration certificates

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - Power consumption: Typical value for information. Supply currents in various operating modes.

Report No. RXA1206-0320SAR

Page <u>84 of 108</u>

#### **DC Voltage Measurement**

A/D - Converter Resolution nominal

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | x                    | Y                    | Z                    |
|---------------------|----------------------|----------------------|----------------------|
| High Range          | 404.749 ± 0.1% (k=2) | 404.733 ± 0.1% (k=2) | 405.174 ± 0.1% (k=2) |
| Low Range           | 3.98175 ± 0.7% (k=2) | 3.93601 ± 0.7% (k=2) | 3.96830 ± 0.7% (k=2) |

#### **Connector Angle**

| Connector Angle to be used in DASY system | 90.0 ° ± 1 ° |
|-------------------------------------------|--------------|

#### **Appendix**

1. DC Voltage Linearity

| High Range |         | Reading (μV) | Difference (μV) | Error (%) |
|------------|---------|--------------|-----------------|-----------|
| Channel X  | + Input | 199991.9     | -0.91           | -0.00     |
| Channel X  | + Input | 20000.28     | 0.48            | 0.00      |
| Channel X  | - Input | -19998.51    | 0.59            | -0.00     |
| Channel Y  | + Input | 200003.0     | 1.24            | 0.00      |
| Channel Y  | + Input | 19999.67     | 0.17            | 0.00      |
| Channel Y  | - Input | -20000.04    | -0.34           | 0.00      |
| Channel Z  | + Input | 200010.1     | -0.11           | -0.00     |
| Channel Z  | + Input | 19999.33     | -0.07           | -0.00     |
| Channel Z  | - Input | -20001.45    | -0.85           | 0.00      |

| Low Range |         | Reading (μV) | Difference (μV) | Error (%) |
|-----------|---------|--------------|-----------------|-----------|
| Channel X | + Input | 2000.0       | 0.05            | 0.00      |
| Channel X | + Input | 199.81       | -0.09           | -0.04     |
| Channel X | - Input | -199.63      | 0.37            | -0.19     |
| Channel Y | + Input | 1999.9       | -0.22           | -0.01     |
| Channel Y | + Input | 198.81       | -1.19           | -0.59     |
| Channel Y | - Input | -201.62      | -1.72           | 0.86      |
| Channel Z | + Input | 2000.4       | 0.48            | 0.02      |
| Channel Z | + Input | 199.30       | -0.70           | -0.35     |
| Channel Z | - Input | -200.86      | -1.06           | 0.53      |

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Common mode<br>Input Voltage (mV) | High Range<br>Average Reading (μV) | Low Range<br>Average Reading (μV) |
|-----------|-----------------------------------|------------------------------------|-----------------------------------|
| Channel X | 200                               | 14.43                              | 13.13                             |
|           | - 200 -                           | -12.22                             | -13.72                            |
| Channel Y | 200                               | -10.07                             | -9.78                             |
|           | - 200                             | 9.61                               | 8.66                              |
| Channel Z | 200                               | -0.56                              | -0.83                             |
|           | - 200                             | -0.01                              | 0.11                              |

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Input Voltage (mV) | Channel X (μV) | Channel Y (μV) | Channel Z (μV) |
|-----------|--------------------|----------------|----------------|----------------|
| Channel X | 200                | -              | 3.08           | 0.09           |
| Channel Y | 200                | 3.19           | -              | 4.59           |
| Channel Z | 200                | 0.90           | -0.06          | -              |

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 15920            | 15519           |
| Channel Y | 16179            | 17567           |
| Channel Z | 15791            | 15270           |

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input  $10M\Omega$ 

|           | Average (μV) | min. Offset (μV) | max. Offset (μV) | Std. Deviation<br>(μV) |
|-----------|--------------|------------------|------------------|------------------------|
| Channel X | 0.03         | -1.16            | 2.66             | 0.46                   |
| Channel Y | -0.63        | -3.22            | 0.29             | 0.46                   |
| Channel Z | -0.87        | -2.03            | 0.28             | 0.46                   |

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

|           | Zeroing (kOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 200            | 200              |
| Channel Y | 200            | 200              |
| Channel Z | 200            | 200              |

8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9              |
| Supply (- Vcc) | -7.6              |

9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.01             | +6            | +14               |
| Supply (- Vcc) | -0.01             | -8            | -9                |

## **ANNEX G: The EUT Appearances and Test Configuration**



Picture 3-1: EUT

Report No. RXA1206-0320SAR

Page 88 of 108



Picture 3-2: Thicker Battery

Report No. RXA1206-0320SAR

Page 89 of 108



Picture 3-3: Thinner Battery





Picture 3-4: Belt



Picture 3-5: Earphone 1



Picture 3-6: Earphone 2

Report No. RXA1206-0320SAR

Page 93 of 108



Picture 3-7: Pocket and Leather



Picture 3-8: Accessory 1



Picture 3-9: Audio Accessory 2



Picture 3-10: Audio Accessory 3




Picture 3-11: Audio Accessory 4




Picture 3-12: Audio Accessory 5

Picture 3: Constituents of the sample

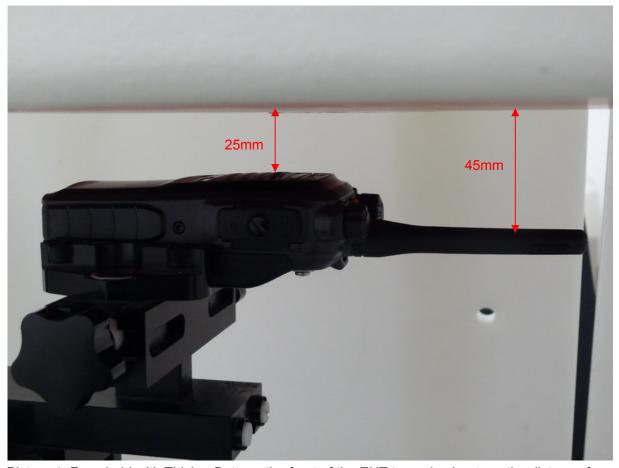

Picture 4: Face-held with Thicker Battery, the front of the EUT towards phantom, the distance from EUT Antenna to the bottom of the Phantom is 45mm

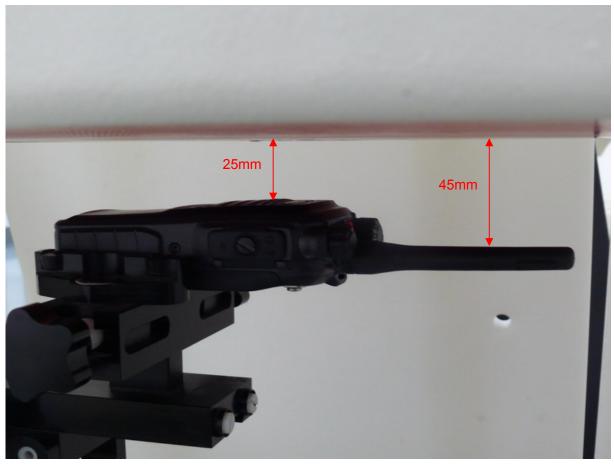

Picture 5: Face-held with Thinner Battery, the front of the EUT towards phantom, the distance from EUT Antenna to the bottom of the Phantom is 45mm





Picture 6: Body-worn with Thinner Battery, Belt and Accessory 1, the front of the EUT towards ground, the distance from EUT Antenna to the bottom of the Phantom is 26mm





Picture 7: Body-worn with Thinner Battery, Belt, Accessory 1 and Earphone 1, the front of the EUT towards ground, the distance from EUT Antenna to the bottom of the Phantom is 26mm





Picture 8: Body-worn with Thinner Battery, Belt, Accessory 1 and Earphone 2, the front of the EUT towards ground, the distance from EUT Antenna to the bottom of the Phantom is 26mm





Picture 9: Body-worn with Thinner Battery, Belt and Audio Accessory 2, the front of the EUT towards ground, the distance from EUT Antenna to the bottom of the Phantom is 26mm



Picture 10: Body-worn with Thinner Battery, Belt and Audio Accessory 3, the front of the EUT towards ground, the distance from EUT Antenna to the bottom of the Phantom is 26mm






Picture 11: Body-worn with Thinner Battery, Belt and Audio Accessory 4, the front of the EUT towards ground, the distance from EUT Antenna to the bottom of the Phantom is 26mm





Picture 12: Body-worn with Thinner Battery, Belt and Audio Accessory 5, the front of the EUT towards ground, the distance from EUT Antenna to the bottom of the Phantom is 26mm

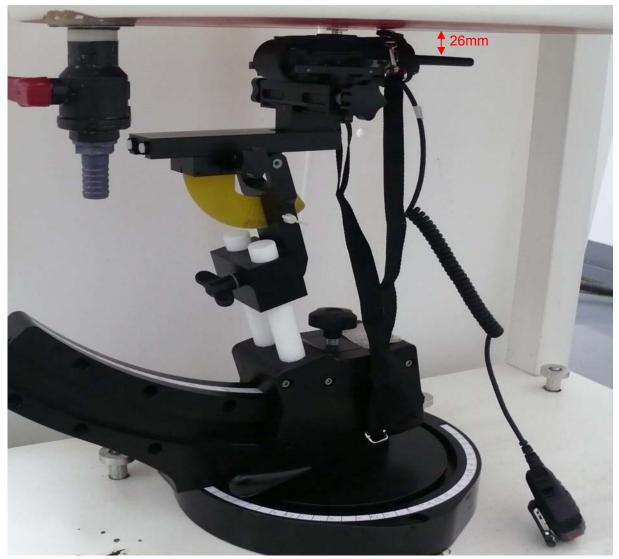



Picture 13: Body-worn with Thinner Battery, Pocket and Accessory 1, the front of the EUT towards ground, the distance from EUT Antenna to the bottom of the Phantom is 26mm





Picture 14: Body-worn with Thinner Battery, Pocket, Leather and Accessory 1, the front of the EUT towards ground, the distance from EUT Antenna to the bottom of the Phantom is 37mm





Picture 15: Body-worn with Thicker Battery, Belt and Accessory 1, the front of the EUT towards ground, the distance from EUT Antenna to the bottom of the Phantom is 24mm