Report No. RZA2010-1332SAR-R1

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.2 Ω + 1.9 jΩ	
Return Loss	- 27.1 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.1 Ω + 5.2 jΩ	
Return Loss	- 25.7 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.144 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	July 05, 2002

DASY5 Validation Report for Head TSL

Date/Time: 17.02.2010 13:12:38

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:712


Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: HSL U11 BB Medium parameters used: f = 2450 MHz; σ = 1.77 mho/m; ϵ_r = 38.7; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 26.06.2009
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.1 V/m; Power Drift = 0.032 dBPeak SAR (extrapolated) = 27.2 W/kg SAR(1 g) = 13.3 mW/g; SAR(10 g) = 6.24 mW/gMaximum value of SAR (measured) = 17.1 mW/g

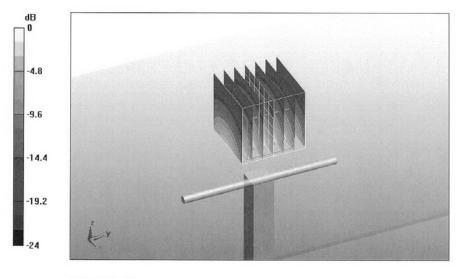


0 dB = 17.1 mW/g

Certificate No: D2450V2-712_Feb10

Page 6 of 9

Report No. RZA2010-1332SAR-R1

Impedance Measurement Plot for Head TSL

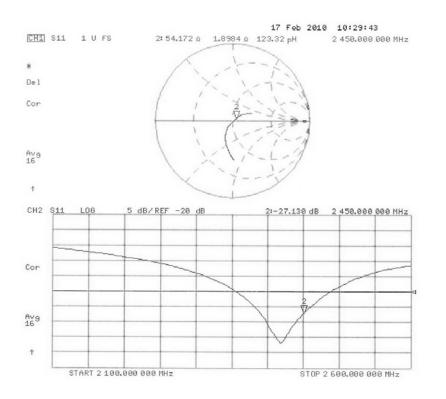

Page 7 of 9

Report No. RZA2010-1332SAR-R1

DASY5 Validation Report for Body

Date/Time: 19.02.2010 13:05:49

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:712


Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: MSL U10 BB Medium parameters used: f = 2450 MHz; σ = 2.01 mho/m; ϵ_r = 51.8; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.31, 4.31, 4.31); Calibrated: 26.06.2009
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

Pin250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 94.5 V/m; Power Drift = 0.015 dB Peak SAR (extrapolated) = 29.5 W/kg

SAR(1 g) = 13 mW/g; SAR(10 g) = 5.97 mW/g Maximum value of SAR (measured) = 17 mW/g

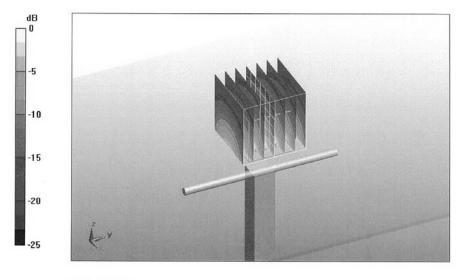


0 dB = 17 mW/g

Certificate No: D2450V2-712_Feb10

Page 8 of 9

Page 135 of 151

Impedance Measurement Plot for Body TSL

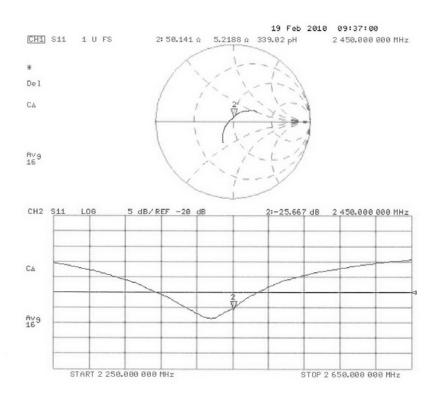

Report No. RZA2010-1332SAR-R1

ANNEX H: DAE4 Calibration Certificate

eughausstrasse 43, 8004 Zuric		The fold with the second secon	S Swiss Calibration Service
Accredited by the Swiss Accredita	e is one of the signatories	to the EA	ation No.: 3CS 106
Aultilateral Agreement for the reclient TA – SH (Aude			te No: DAE4-871_Nov09
CALIBRATION			
Object	DAE4 - SD 000 D	04 BJ - SN: 871	
Calibration procedure(s)	QA CAL-06.v12 Calibration proced	lure for the data acquisition e	electronics (DAE)
	November 11, 200	99	
This calibration certificate docum The measurements and the unce	nents the traceability to natio ertainties with confidence pro	nal standards, which realize the physic obability are given on the following page facility: environment temperature (22 :	es and are part of the certificate.
This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M&	nents the traceability to natio ertainties with confidence pro cted in the closed laboratory TE critical for calibration)	nal standards, which realize the physic obability are given on the following page facility: environment temperature (22 :	es and are part of the certificate. ± 3)°C and humidity < 70%.
This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards	nents the traceability to natio ertainties with confidence pro cted in the closed laboratory	nal standards, which realize the physic bbability are given on the following page	es and are part of the certificate.
This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001	nents the traceability to natio ertainties with confidence pro cted in the closed laboratory TE critical for calibration) ID # SN: 0810278	nal standards, which realize the physic obability are given on the following page facility: environment temperature (22 : <u>Cal Date (Certificate No.)</u> 1-Oct-09 (No: 9055)	es and are part of the certificate. ± 3)°C and humidity < 70%. <u>Scheduled Calibration</u> Oct-10
The measurements and the unce	nents the traceability to natio ertainties with confidence pro- cted in the closed laboratory TE critical for calibration) ID # SN: 0810278 ID #	nal standards, which realize the physic obability are given on the following page facility: environment temperature (22 : Cal Date (Certificate No.)	es and are part of the certificate. ± 3)°C and humidity < 70%. Scheduled Calibration
This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards	nents the traceability to natio ertainties with confidence pro- cted in the closed laboratory TE critical for calibration) ID # SN: 0810278 ID #	nal standards, which realize the physic obability are given on the following page facility: environment temperature (22 : <u>Cal Date (Certificate No.)</u> 1-Oct-09 (No: 9055) Check Date (in house)	es and are part of the certificate. ± 3)°C and humidity < 70%. <u>Scheduled Calibration</u> Oct-10 <u>Scheduled Check</u> In house check: Jun-10
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards	hents the traceability to natio ertainties with confidence pro- cted in the closed laboratory TE critical for calibration) ID # SN: 0810278 ID # SE UMS 006 AB 1004	nal standards, which realize the physic obability are given on the following page facility: environment temperature (22 : <u>Cal Date (Certificate No.)</u> 1-Oct-09 (No: 9055) <u>Check Date (in house)</u> 05-Jun-09 (in house check)	es and are part of the certificate. ± 3)°C and humidity < 70%. Scheduled Calibration Oct-10 Scheduled Check

Report No. RZA2010-1332SAR-R1

Page 137 of 151

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst C Service suisse d'étalonnage Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

S

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE Connector angle data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a
 result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - *Power consumption:* Typical value for information. Supply currents in various operating modes.

Report No. RZA2010-1332SAR-R1

DC Voltage Measurement

A/D - Converter Resol	ution nominal				
High Range:	1LSB =	6.1µV ,	full range =	-100+300 mV	
Low Range:	1LSB =	61nV ,	full range =	-1+3mV	
DASY measurement p	arameters: Aut	o Zero Time: 3	sec; Measuring	time: 3 sec	

Calibration Factors	x	Y	Z
High Range	404.813 ± 0.1% (k=2)	404.794 ± 0.1% (k=2)	405.237 ± 0.1% (k=2)
Low Range	$3.98191 \pm 0.7\%$ (k=2)	3.98417 ± 0.7% (k=2)	3.98912 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system	90.0 ° ± 1 °
---	--------------

Page 3 of 5

Report No. RZA2010-1332SAR-R1

Page 139 of 151

Appendix

1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	199994.0	1.84	0.00
Channel X + Input	19999.85	0.05	0.00
Channel X - Input	-19997.97	1.83	-0.01
Channel Y + Input	200010.3	-3.71	-0.00
Channel Y + Input	19999.12	-0.48	-0.00
Channel Y - Input	-20000.18	-0.78	0.00
Channel Z + Input	200010.2	-2.80	-0.00
Channel Z + Input	19998.54	-0.86	-0.00
Channel Z - Input	-19999.82	0.00	0.00

Low Range		Reading (µV)	Difference (µV)	Error (%)
Channel X	+ Input	2000.3	0.22	0.01
Channel X	+ Input	200.20	0.30	0.15
Channel X	- Input	-199.89	0.21	-0.10
Channel Y	+ Input	1999.8	-0.13	-0.01
Channel Y	+ Input	200.06	-0.04	-0.02
Channel Y	- Input	-200.43	-0.73	0.36
Channel Z	+ Input	1999.5	-0.57	-0.03
Channel Z	+ Input	199.58	-0.72	-0.36
Channel Z	- Input	-201.11	-1.01	0.51

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (µV)
Channel X	200	13.79	12.75
	- 200	-12.26	-13.72
Channel Y	200	-11.82	-11.47
	- 200	10.67	10.68
Channel Z	200	-1.08	-1.35
	- 200	0.32	0.12

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (µV)	Channel Z (μV)
Channel X	200	-	3.36	1.06
Channel Y	200	1.52		3.59
Channel Z	200	2.55	1.41	-

Certificate No: DAE4-871_Nov09

Report No. RZA2010-1332SAR-R1

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15928	16288
Channel Y	16188	15745
Channel Z	15790	16219

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input $10M\Omega$

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	0.06	-3.43	1.18	0.52
Channel Y	-0.71	-2.66	0.96	0.57
Channel Z	-0.95	-1.94	0.04	0.41

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.1999	204.4
Channel Y	0.1999	203.6
Channel Z	0.1999	203.8

8. Low Battery Alarm Voltage (verified during pre test)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (verified during pre test)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.0	+6	+14
Supply (- Vcc)	-0.01	-8	-9

ANNEX I: The EUT Appearances and Test Configuration



a: Slide Open





c: Battery



d: Adapter

Report No. RZA2010-1332SAR-R1



e: Earphone

Picture 7: Constituents of EUT



Picture 8: Left Hand Touch Cheek Position (Slide Open)



Picture 9: Left Hand Touch Cheek Position (Slide Close)



Picture 10: Left Hand Tilt 15 Degree Position (Slide Open)



Picture 11: Left Hand Tilt 15 Degree Position (Slide Close)



Picture 12: Right Hand Touch Cheek Position (Slide Open)



Picture 13: Right Hand Touch Cheek Position (Slide Close)



Picture 14: Right Hand Tilt 15 Degree Position (Slide Open)



Picture 15: Right Hand Tilt 15 Degree Position (Slide Open)



Picture 16: Body, The EUT display towards ground, the distance from handset to the bottom of the Phantom is 15mm (The spacer was removed during testing, Slide Open)



Picture 17: Body, The EUT display towards ground, the distance from handset to the bottom of the Phantom is 15mm (The spacer was removed during testing, Slide Close)



Picture 18: Body, The EUT display towards phantom, the distance from handset to the bottom of the Phantom is 15mm (The spacer was removed during testing, Slide Open)



Picture 19: Body, The EUT display towards phantom, the distance from handset to the bottom of the Phantom is 15mm (The spacer was removed during testing, Slide Close)



Picture 20: Body with earphone, The EUT display towards ground, the distance from handset to the bottom of the Phantom is 15mm (Slide Open)



Picture 21: Body with earphone, The EUT display towards ground, the distance from handset to the bottom of the Phantom is 15mm (Slide Close)

ANNEX J: Schematic Diagram of Antenna

