

Appendix D





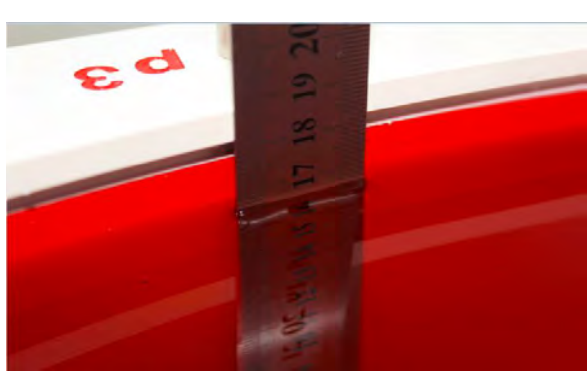

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details


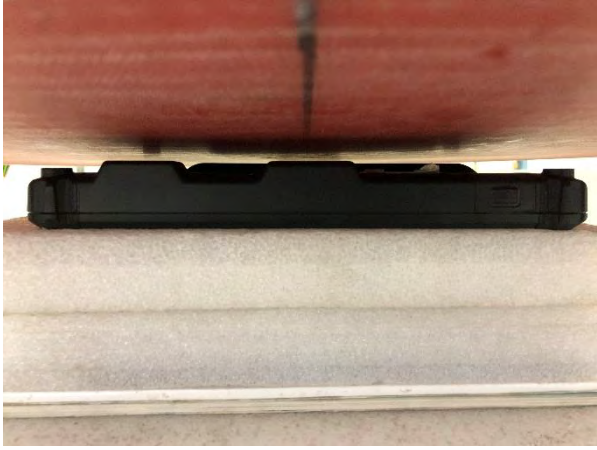
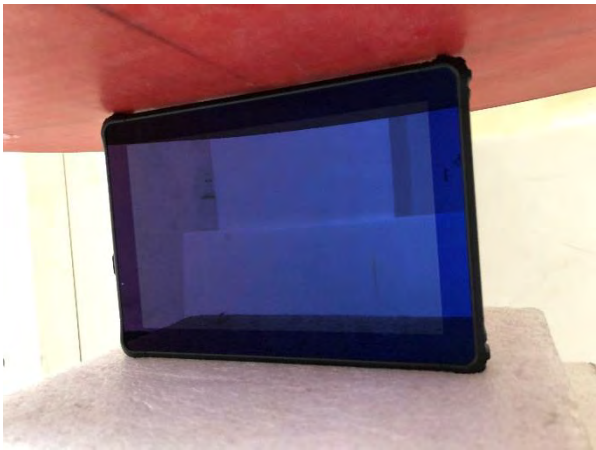



1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Head 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1800</p>	<p>Photo 4: Tissue Simulant Liquid for Head 1900</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Head 5GHz</p>
	

3. Photographs of EUT test position

<p>Photo 7: Bottom Face 0mm</p>	<p>Photo 8: Bottom Face 4mm</p>
	
<p>Photo 9: Edge 1 0mm</p>	<p>Photo 10: Edge 3 0mm</p>
	
<p>Photo 11: Edge 2 0mm</p>	<p>Photo 12: Edge 2 4mm</p>
	

4. EUT Constructional Details







<p align="center">Photo 13: Front View</p>	<p align="center">Photo 14: Back View</p>
	
<p align="center">Photo 15: Left View</p>	<p align="center">Photo 16: Right View</p>
	
<p align="center">Photo 17: Top View</p>	<p align="center">Photo 18: Bottom View</p>
	

Photo 19: Back View

