

ENERGYA DR 3440 ENERGYA VR 3140

IMPLANT MANUAL

Implantable cardioverter defibrillator DF4 DR & VR models



Intended audience


This manual is intended for use by professionals trained or experienced in device implant and/or follow-up procedures.

Training for users


The following instructions for use are for informational purpose only. Each medical professional is responsible for their medical training and experience and should apply the following instructions according to the best clinical practices and patient condition.

Reminder

Battery depletion

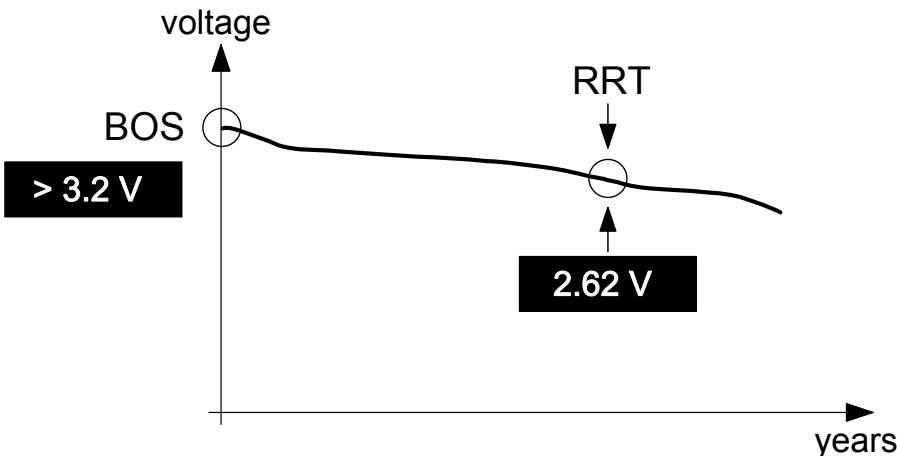

Leads connection - ENERGYA DR 3440 model - DF4

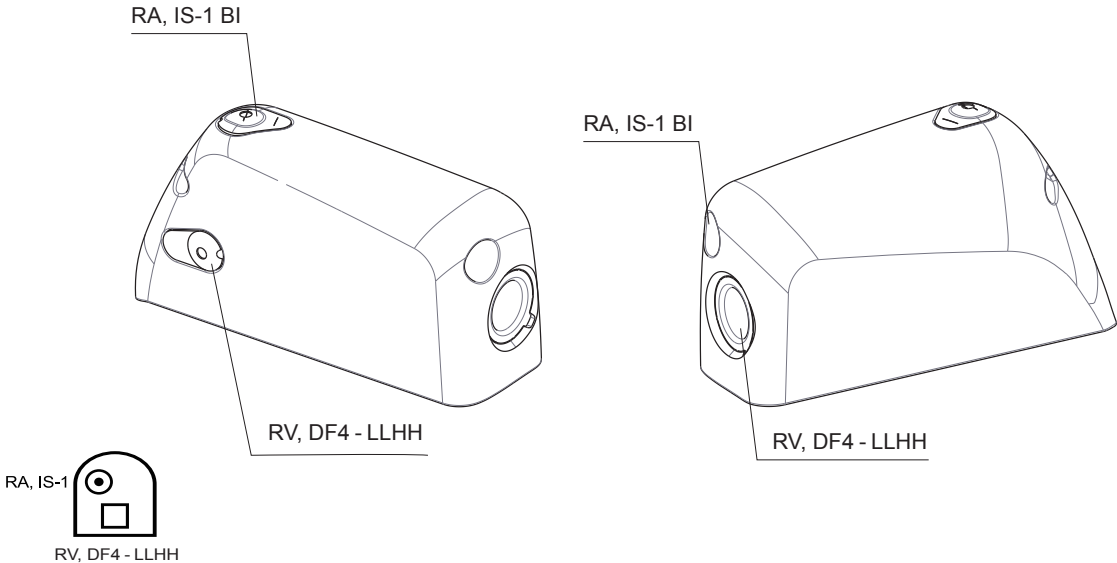

Leads connection - ENERGYA VR 3140 model - DF4

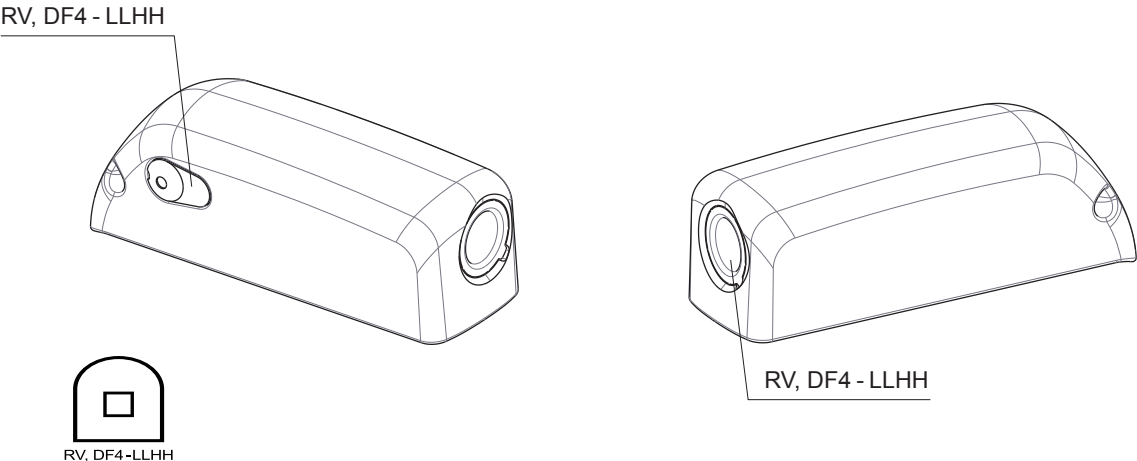


TABLE OF CONTENTS

1.	GENERAL DESCRIPTION AND COMPATIBLE DEVICES	8
2.	INTENDED PURPOSE AND TARGETED POPULATION	10
2.1.	Intended purpose	10
2.2.	Indications	10
2.3.	Targeted population	10
2.4.	Intended users.....	10
3.	CONTRAINDICATIONS.....	11
3.1.	Contraindication for patient implantation	11
3.2.	Contraindication for use under medical environments	11
3.3.	Adverse events, risks and side-effects	11
4.	WARNINGS AND PRECAUTIONS.....	14
4.1.	Warnings to patients.....	14
4.2.	Risks related to medical environment	15
4.3.	Sterilization, storage and handling	17
4.4.	Implantation and device programming	17
4.5.	Lead evaluation and lead connection.....	18
4.6.	Generator explant and disposal	19
5.	ADVERSE EVENTS.....	20
5.1.	Defender study.....	20
5.2.	SafeR (AAI <> DDD) study (for DR model only)	21
6.	CLINICAL STUDIES	23
6.1.	Defender study.....	23
6.2.	SafeR (AAI <> DDD) study (for DR model only)	25
7.	PATIENT INFORMATION.....	28
8.	PATIENT SELECTION AND TREATMENT.....	29
8.1.	Individualization of treatment.....	29
8.2.	Specific patient populations.....	29
9.	PATIENT COUNSELING INFORMATION.....	31
10.	DECLARATION OF CONFORMITY	32
11.	PHYSICIAN GUIDELINES	33
11.1.	Physician training	33
11.2.	Directions for use	33
11.3.	Maintaining device quality	33
12.	HOW SUPPLIED.....	34
12.1.	Sterility.....	34
12.2.	Warranty and replacement policy.....	34

13. DEVICE DESCRIPTION	35
14. IMPLANT PROCEDURE.....	38
14.1. Necessary equipment.....	38
14.2. Packaging.....	38
14.3. Optional equipment	39
14.4. Opening the package	39
14.5. Prior to implantation	40
14.6. Device placement.....	40
14.7. Choosing the type of lead.....	41
14.8. Shock configuration (+ -> -).....	41
14.9. Measurement of thresholds at implant	42
14.10. Leads connection	42
14.11. Device implantation	44
14.12. Tests and programming	44
15. SPECIAL MODES	45
15.1. MRI mode.....	45
15.2. Safety mode (nominal values).....	45
15.3. Magnet mode	45
15.4. Response in the presence of disturbance	46
15.5. Detection characteristics in the presence of electromagnetic fields.....	46
15.6. Protection against short-circuits	47
16. MAIN FUNCTIONS	48
16.1. Automatic lead measurements.....	48
16.2. Automatic Pacing Threshold Adaptation	48
16.3. Atrial tachyarrhythmia management (for DR model only)	49
16.4. Ventricular tachyarrhythmia management.....	50
16.5. Pacing	51
16.6. Sensing	51
16.7. Rate response	52
16.8. Lead Parameters Evaluation (LPE).....	53
16.9. Electrophysiological study (EPS)	54
16.10. Follow-up function	54
16.11. Remote Monitoring function	54
17. PATIENT FOLLOW-UP	57
17.1. Follow-up recommendations	57
17.2. Holter Function	57
17.3. Recommended Replacement Time (RRT)	58
17.4. Explantation.....	59
17.5. Defibrillator identification	59
18. PHYSICAL CHARACTERISTICS	61

18.1. Materials used	61
19. ELECTRICAL CHARACTERISTICS	62
19.1. Table of delivered shock energy and voltage	62
19.2. Battery	63
19.3. Longevity	63
19.4. Radio equipment emission	66
19.5. Conformity to standards for safety and electromagnetic compatibility	67
20. PROGRAMMABLE PARAMETERS	68
20.1. Antibradycardia pacing	68
20.2. Ventricular tachyarrhythmia detection	72
20.3. Ventricular tachyarrhythmia therapies	73
20.4. Remote alerts and warnings	77
21. NON PROGRAMMABLE PARAMETERS	80
22. LIMITED WARRANTY	81
23. PATENTS	82
24. EXPLANATION OF SYMBOLS	83

1. GENERAL DESCRIPTION AND COMPATIBLE DEVICES

ENERGYA DR / ENERGYA VR are implantable cardioverter defibrillators for the recognition and treatment of ventricular tachycardia and fibrillation, in patients with spontaneous or inducible tachyarrhythmias.

ENERGYA DR is an implantable dual-chamber cardioverter defibrillator.

ENERGYA VR is an implantable single-chamber cardioverter defibrillator.

Both devices are equipped with an accelerometer to allow adaptation of pacing to suit the patient's activity.

Both devices can be programmed and interrogated with a compatible MicroPort dedicated programmer, using a compatible MicroPort dedicated programming head for bi-directional telemetry.

For detailed information about the compatibility of programming devices and implantable patient devices, please refer to the Device-Compatibility-Matrix that is available at www.microportmanuals.com.

This device features Bluetooth®⁽¹⁾ Low Energy (BLE) wireless technology which enables:

- Remote monitoring of patients who have the compatible MicroPort SMARTVIEW CONNECT Monitor installed at home,
- wireless interrogation and device programming by a compatible MicroPort SMARTTOUCH programmer.

Data communication security:

Bluetooth communication system

Data including sensitive information is encrypted by the device before it is sent over the BLE channel.

Inductive telemetry communication system

The MicroPort CRM inductive telemetry communication system (used by the SMARTTOUCH programmer for the device interrogation and programming) uses short-range communication that protects sensitive information such as patient and device data.

Lead system:

The lead system used with this device must provide sensing, pacing to the right ventricle, appropriate defibrillation to the heart, sensing and pacing to the right atrium (for DR model only). The lead-device system compatibility is verified with MicroPort leads but has not been tested with non-MicroPort leads. Using non-MicroPort leads may lead to adverse events including oversensing or undersensing of cardiac activity, potentially leading to inappropriate therapy delivery. It is recommended to check the leads user's manual, especially in the case of leads with new technologies.

Devices and compatible lead connections are listed in the table below:

3440 Model	3140 Model
Atrium: IS-1 bipolar. Ventricle: DF4.	Ventricle: DF4.

Therapeutic and diagnostic functions:

Both devices provide a range of therapeutic and diagnostic functions:

- high energy shocks
- atrial tachyarrhythmia prevention (for DR model only)
- automatic lead measurements
- advanced diagnostic functions
- automatic adjustment of atrial sensitivity (for DR model only) and of ventricular sensitivity
- automatic adjustment of atrial pacing (atrial autothreshold in DR model only) and of ventricular pacing (ventricular autothreshold)
- AutoMRI
- high energy shocks (42 J) for enhanced safety

Usage environment:

The device is intended to be used in the following environments:

- In-clinic for implantation and post-surgical patient follow-up;
- After implantation, patient can resume a normal life considering restriction provided in the patient information booklet;
- During MRI examination under the considerations described in MRI Solutions addendum available on www.microportmanuals.com.

⁽¹⁾*The Bluetooth® word mark is a registered trademark of Bluetooth SIG, Inc. Any use of the word mark by MicroPort CRM is under license.*

2. INTENDED PURPOSE AND TARGETED POPULATION

2.1. INTENDED PURPOSE

Intended medical purpose of ENERGYA DR / ENERGYA VR:

ENERGYA DR / ENERGYA VR are dual and single chambers implantable cardioverter defibrillators (ICD) used in combination with pacing and defibrillating lead(s).

The devices sense and record the electrical activity of the patient's heart using the electrodes of the implanted atrial (for DR models only) and right ventricular leads and analyze the heart rhythm based on selectable detection parameters. The devices automatically detect ventricular tachyarrhythmias (VT/VF) and provide treatment with defibrillation, cardioversion, and antitachycardia pacing therapies through the delivery of shocks and electrical impulses. The devices also respond to bradycardia by providing atrial and/or ventricular pacing.

Intended purpose of the Screwdriver:

The screwdriver is a non-implantable accessory of MicroPort CRM pacemaker, defibrillator or resynchronisation therapy device. It is intended to tighten (untighten) the lead connector inside the header of the implantable device with screws, during implantation (explantation) procedure.

2.2. INDICATIONS

For further details please refer to “2008 ACCF/AHA/HRS Guidelines for Device-Based Therapy of Cardiac Rhythm Abnormalities” and its 2012 Focused Update or “2017 AHA/ACC/HRS Guidelines for management of patients with ventricular arrhythmias and the prevention of sudden cardiac death” or “2022 ESC Guidelines for management of patients with ventricular arrhythmias and the prevention of sudden cardiac death”.

2.3. TARGETED POPULATION

The population targeted for the device is the patient population for which the device is indicated excluding the pediatric patients.

Particular care should be taken with the implantation of devices in pregnant women with respect to the imaging technology used during the implant procedure.

2.4. INTENDED USERS

The intended users are professionals trained or experienced in device implant and/or follow-up procedures.

3. CONTRAINDICATIONS

3.1. CONTRAINDICATION FOR PATIENT IMPLANTATION

Implantation of ENERGY DR / ENERGY VR are contraindicated in patients:

- whose ventricular tachyarrhythmias may have transient or reversible causes such as: acute myocardial infarction, digitalis intoxication, drowning, electrocution, electrolyte imbalance, hypoxia, sepsis, or unstable ischemic episodes,
- who present incessant tachyarrhythmia,
- who have an internal pacemaker,
- whose primary disorder is bradyarrhythmias, or atrial tachyarrhythmias.

The use of the dual-chamber pacing mode from ENERGY DR is contraindicated in patients with chronic refractory atrial tachyarrhythmias.

3.2. CONTRAINDICATION FOR USE UNDER MEDICAL ENVIRONMENTS

Internal pacemaker:

Use of the defibrillator is contraindicated in cardiac implantable pacemaker patients.

Radiation therapy:

Betatrons are contraindicated.

Refer to the MRI Solutions document for MRI-related contraindications.

3.3. ADVERSE EVENTS, RISKS AND SIDE-EFFECTS

Based on the literature and on pulse generator and/or lead implant experience, the following list includes the possible adverse events associated with implantation of ICD systems:

Events	Possible adverse effects
Procedure related	
Clotting disorder	Pocket hematoma, bleeding, formation of clots, may necessitate reintervention
Contamination, inflammation	Pocket infection, endocarditis, septicaemia may become necessary to perform surgical intervention, to remove the device and/or the lead
Fibrotic tissue formation	Pain, risk of hematoma and infection at the time of replacement
Introduction of air (with subclavian approach)	Air embolism
Poor lead/defibrillator connection	Intermittent or continuous loss of pacing and/or sensing
Others	Adverse reaction to the procedure
	Pneumothorax linked to subclavian access
	Thrombosis
	Thrombotic embolism
	Venous occlusion

3. CONTRAINDICATIONS

Events	Possible adverse effects
	Venous trauma (e.g., perforation, dissection, erosion, rupture)
	Tissue necrosis
Pocket related	
Clotting disorder	Pocket hematoma, bleeding, formation of clots, may necessitate reintervention
Contamination, inflammation	Pocket infection, endocarditis, septicaemia may become necessary to perform surgical intervention, to remove the device and/or the lead
Fibrotic tissue formation	Risk of hematoma and infection at the time of replacement
Skin erosion by the defibrillator with possible protrusion/extrusion of the casing	Generally linked to infection and/or hematoma, necessitates re-intervention and to change the site of implantation
Others	Venous trauma (e.g., perforation, dissection, erosion, rupture)
	Tissue necrosis
Device related	
Casing migration	Pain, discomfort
Component failure	Complications and mortality due to inability to detect arrhythmia and to deliver appropriate and intended therapy, surgical intervention to remove/replace the device
Failure to convert an induced arrhythmia	Life-threatening arrhythmia
Myopotential sensing	Oversensing
Sensing circuit inhibition, reversion to backup mode, or other failures due to electromagnetic interference	Inappropriate functioning
Others	Tachyarrhythmias, which include acceleration of arrhythmias (caused by the device) and early, recurrent atrial fibrillation
Leads related	
Arrhythmia at implantation	Extrasystoles, tachycardia, ventricular/atrial fibrillation
Cardiac perforation	Intermittent or continuous loss of pacing and/or sensing
	Muscle or phrenic (for DR model only) stimulation
	Cardiac tamponade, fluid accumulation
Conductor coil fracture	Inability to pace, sense, defibrillate
Contamination, inflammation	Pocket infection, endocarditis, septicaemia may become necessary to perform surgical intervention, to remove the device and/or the lead
Lead displacement, migration, conductor fracture or incorrect lead implantation	Intermittent or continuous loss of pacing and/or sensing
Lead insulation rupture or abrasion	Pectoral and other muscular stimulation, sudden fall in impedance, loss of efficacy of pacing, early battery depletion
Lead tip deformation and/or breakage by overtorquing	Intermittent or continuous loss of pacing and/or sensing
Myocardial trauma	Chest pain, cardiac wall perforation, arrhythmias, formation of clot at injury site, bleeding, embolism, pericardial effusion or rub, endocarditis

Events	Possible adverse effects
Threshold elevation	Loss of capture
Phrenic Stimulation	Pain, discomfort
Others	Heart block
	Valvular damage
	Tachyarrhythmias, which include acceleration of arrhythmias (caused by the device) and early, recurrent atrial fibrillation
General	
Frequent shocks	Psychological intolerance to an ICD system (despite medical management): - Dependency - Depression - Fear of premature battery depletion - Fear of shocking while conscious - Fear that shocking capability may be lost - Imagined shocking (phantom shock) - Fear of device malfunction
Inappropriate therapy (e.g., shocks and antitachycardia pacing [ATP] where applicable, pacing)	Psychological intolerance to an ICD system (despite medical management): - Dependency - Depression - Fear of premature battery depletion - Fear of shocking while conscious - Fear that shocking capability may be lost - Imagined shocking (phantom shock) - Fear of device malfunction
Shock	Pain experienced during or after delivery of therapy
Others	Cardiac death
	Electrolyte imbalance/dehydration
	Pain, inesthetic scar
	Vasovagal syncope
	Stroke
	Worsening heart failure
Long term	
Prolonged exposure to fluoroscopic radiation	<i>No data available</i>



NOTE: Any serious incident in relation to the device should be reported to MicroPort CRM and the local Competent Authority.

4. WARNINGS AND PRECAUTIONS

4.1. WARNINGS TO PATIENTS

The patient should be warned of the potential risks of defibrillator malfunction if exposed to external magnetic, electrical, or electromagnetic signals.

These potential interference sources may cause conversion to inhibited mode (because of noise detection), erratic delivery of VT or VF therapies, nominal programming, or much more rarely, irreversible damage to the device's circuits.

The main sources of high magnitude disturbance are: powerful radiofrequency equipment (radar), industrial motors and transformers, induction furnaces, resistance welding / arc-welding equipment and high power loudspeakers.

Electrical Isolation:

Do not permit the patient to contact grounded equipment that could produce hazardous leakage current. Ensuing arrhythmia induction could result in the patient's death.

Electronic Article Surveillance (EAS) and RadioFrequency Identification equipment (RFID)

Patients should be advised to walk directly through and not lean against or linger near Electronic Article Surveillance (EAS) systems such as retail theft prevention systems, security gates, entry control systems, or tag readers including Radio Frequency IDentification equipment (RFID). These systems may be found at the entrances and exits of stores, libraries, banks, etc...and may interact with pulse generators. It is unlikely that these systems affect cardiac function when the patient walks through them at a normal pace. If patients do experience symptoms near these systems, they should promptly move away and inform their doctor.

Work environment:

The patient's work environment may be an important source of disturbances. In that case, specific recommendations may be required.

High voltage power transmission lines:

High voltage power transmission lines may generate enough disturbances to interfere with defibrillator operation if approached too closely.

Communication equipment:

Communication equipment such as microwave transmitters, linear power amplifiers, or high-power amateur transmitters may generate enough disturbances to interfere with defibrillator operation if approached too closely.

Home appliances:

Home appliances that are in good working order and properly grounded do not usually produce enough disturbances to interfere with defibrillator operation. However, there are reports of device interferences caused by electric hand tools or electric razors used directly over the device implant site. Patient should also avoid using induction ovens and cookers.

Pressure variations:

Repeated exposure to pressure variations are not recommended outside the following limits:

- skin diving (diving to a depth of 10 m (33ft) max, equivalent to 2 ATA),
- scuba diving (diving to a depth of 20 m (66 ft) max, equivalent to 3 ATA),
- hiking, skiing or driving to high altitude (up to 4 267 m (14 000 ft) max),



NOTE: Air travel in pressurized aircrafts is allowed (typical cabin pressurization is equivalent to 2 438 m (8 000 ft)).

Wireless devices:

The functioning of the implant can be disturbed when a wireless device emitting radiofrequency or magnetic field is placed in its vicinity. It is recommended to maintain a minimum distance of 15 cm (6 inches) between both.



CAUTION: Do not tap sharply on the ICD can after implant, because the ICD's sensing circuits can detect this as P-waves (for DR model only) or R-waves, and such oversensing could result in inappropriate pacing, inhibition, or therapy. Normal activities after implant do not result in such oversensing.

4.2. RISKS RELATED TO MEDICAL ENVIRONMENT

It is advisable to carefully monitor defibrillator operation prior to and after any medical treatment/procedure during which an electrical current from an external source passes through the patient's body or the patient body is exposed to external electromagnetic radiation.

Magnetic Resonance Imaging:

When implanted in combination with MR Conditional lead(s), the defibrillation system constitutes an MR conditional system under specific conditions. When these conditions are not met, MRI is contraindicated.



NOTE: Refer to the MRI Solutions manual for the complete instructions for use available at www.microportmanuals.com.

Radiofrequency ablation:

A radiofrequency ablation procedure in a patient with a generator may cause device malfunction or damage. RF ablation risks may be minimized by:

1. Deactivating ATP and shock therapies.
2. Avoiding direct contact between the ablation catheter and the implanted lead or generator.
3. Positioning the ground, placing it so that the current pathway does not pass through or near the device, i.e. place the ground plate under the patient's buttocks or legs.
4. Having external defibrillation equipment available.

Electrocautery or diathermy device:

Diathermy and electrocautery equipment should not be used. If such devices must be used:

1. Keep the current path and ground plate as far away from the device and the lead(s) as possible (a minimum of 15 cm [6 inches]).
2. Before procedure, deactivate ATP and shock therapies.
3. During the procedure, keep the electrocautery device as far as possible from the cardiac defibrillator. Set it at minimum intensity. Use it briefly.
4. After the procedure, check for proper implant function. The device should never be exposed directly to the diathermy source.

Left Ventricular Assistant Device (LVAD):

When implanting an ICD in a patient implanted with a LVAD, it is recommended to place the device as far as possible from the LVAD, as the LVAD may disturb device interrogation. When interrogating the device the programmer head should be kept as far away from the LVAD as possible.

External defibrillation:

ENERGYA DR / ENERGYA VR are protected from external defibrillation shocks.

1. Before external defibrillation, deactivate ATP and shock therapies.
2. During external defibrillation, it is advisable to avoid placing the defibrillating paddles directly over the casing or over the lead(s). The defibrillating paddles should preferably be placed in an anteroposterior position.
3. Avoid any direct contact between the defibrillation paddles and the conductive parts of the implanted leads or casing of the implanted device.
4. After external defibrillation, check for proper device function.

Radiation therapy:

Avoid exposure to ionizing radiation. If high doses of radiation therapy cannot be avoided, the defibrillator should be protected from direct exposure with a protection shield. ATP and shock therapies should be disabled during exposure and proper device function should be checked regularly afterwards. Resulting damage may not be immediately detectable. If irradiation of tissues close to the implantation site is necessary, it is recommended that the cardiac defibrillator be moved. As a safety measure, an external defibrillator should be immediately available.

Lithotripsy:

Lithotripsy may permanently damage the device if it is at the focal point of the lithotripsy beam. If lithotripsy must be used, keep the defibrillator at least 2.5 to 5 cm (1-2 inches) away from the focal point of the lithotripsy beam.

Diagnostic ultrasound (echography):

The defibrillator is not affected by ultrasound imaging devices.

Transcutaneous Electrical Nerve Stimulation (TENS):

TENS may interfere with defibrillator function. If necessary, the following measures may reduce interference:

1. Place the TENS electrodes as close together as possible and as far as possible from the pulse generator and leads.
2. Monitor cardiac activity during TENS use.

Scales with body fat monitors and electronic muscle stimulators:

A patient with an implanted ENERGYA DR / ENERGYA VR should not use these devices.

Surgical procedure:

For safety reasons, it is preferable to turn OFF Rate Response prior to any surgical procedure on the defibrillator patient.

Hyperbaric or hyperoxia therapy:

Elevated pressures due to hyperbaric or hyperoxia therapy may damage the pulse generator when above 3.0 ATA (300 kPa). Under simulated conditions, tests have shown the device is able to deliver continuous pacing. Shock delivery was not part of the scope.

4.3. STERILIZATION, STORAGE AND HANDLING**Resterilization:**

Do not resterilize and re-implant explanted ICDs.

"Use by" Date:

A "Use by" date is printed on the outer storage package and on the sterile package. Do not implant the device after this date because the battery may have reduced longevity and sterility may be affected. It should be returned to MicroPort.

If package is damaged:

Do not use the device or accessories if the packaging is wet, punctured, opened or damaged because the integrity of the sterile packaging may be compromised. Return the device to the manufacturer.

Device Storage:

Store the device in a clean area, away from magnets, kits containing magnets, and sources of electromagnetic disturbance to avoid device damage. Store the device between 0 - 50 °C (32 - 122 °F). Temperatures outside the specified range may damage the device.

Equilibration:

Allow the device to reach room temperature before programming or implanting the device because rapid temperature changes may affect initial device function.

4.4. IMPLANTATION AND DEVICE PROGRAMMING

Use only a MicroPort programmer to communicate with the device.

Do not inadvertently position any magnet over the ICD; this suspends tachyarrhythmia detection and treatment.

Replace the device when the RRT (Recommended Replacement Time*) point (defined by a battery voltage of 2.62 ± 0.01 V) is reached.

Program device parameters such as sensitivity threshold and VT and VF detection intervals as specified in the device manuals.

Lead System:

Do not use a lead system other than those with demonstrated compatibility because undersensing cardiac activity and failure to deliver necessary therapy may result.

In situations where an ICD and a pacemaker are implanted in the same patient, interaction testing should be completed. If the interaction between the ICD and the pacemaker cannot be resolved through repositioning of the leads or reprogramming of either the pacemaker or the ICD, the pacemaker should not be implanted (or should be explanted if previously implanted).

Failure to properly insert the torque screwdriver into the perforation at an angle perpendicular to the connector receptacle may result in damage to the sealing system and its self-sealing properties.

In the event of a warning on low shock impedance, and after lead replacement or reconnection: it is recommended to check the system integrity (sensing and pacing thresholds and the impedance of the shock electrodes)

It is recommended that a safety margin of at least 10 J be demonstrated between the effective shock energy and maximum programmable energy. Carefully confirm that true ventricular fibrillation has been induced because the DFT for ventricular tachycardia or flutter may be lower.

The defibrillator should be implanted with the engraved side facing outwards in order to facilitate telemetric communication with the programming head and to display the radiographic identification correctly.

*: corresponds to ERI (Elective Replacement Indicator) previously used.

4.5. LEAD EVALUATION AND LEAD CONNECTION

ENERGYA DR has one IS-1, and one DF4 connector ports.

ENERGYA VR has one DF4 connector port.

IS-1 refers to the international standard whereby leads and generators from different manufacturers are assured a basic fit (ISO 5841-1:2000).

DF4 refers to the international standard for defibrillation lead connectors (ISO 27186:2020).

Use only DF4-LLHH or DF4-LLHO standard lead connector types according to ISO 27186:2020.

Use only IS4-LLLL standard lead connector type according to ISO 27186:2020.

Do not tie a ligature directly to the lead body, tie it too tightly, or otherwise create excessive strain at the insertion site as this may damage the lead. Use the lead stabilizer to secure the lead lateral to the venous entry site.

Do not immerse the lead(s) in mineral oil, silicone oil, or any other liquid.

Do not grip the lead with surgical instruments.

Do not use excessive force or surgical instruments to insert a stylet into a lead.

Use ventricular transvenous leads with caution in patients with either a mechanical or bioprosthetic tricuspid valvular prosthesis.

Use the correct suture sleeve (when needed), to immobilize the lead(s) and protect it against damage from ligatures.

Never implant the system with a lead system that has a measured shock impedance of less than 30 ohms. A protection circuit in the defibrillator prevents shock delivery when impedance is too low. If the shock impedance is less than 30 ohms, reposition the lead system to allow a greater distance between the electrodes.

Do not kink leads. Kinking leads may cause additional stress on the leads, possibly resulting in lead fracture.

Do not insert a lead connector pin into the connector block without first visually verifying that the setscrews are sufficiently retracted. Do not tighten the setscrews unless a lead connector pin is inserted because it could damage the connector block.

Lead electrodes in contact during a cardioversion or defibrillation therapy will cause current to bypass the heart, possibly damaging the ICD and the lead(s). While the ICD is connected to the lead, make sure that the metal portions of any electrodes do not touch each other.

If a pacing lead is abandoned rather than removed, it must be capped to ensure that it is not a pathway for currents to or from the heart.

If a thoracotomy is required to place epicardial patches, it should be done during a separate procedure to reduce the risk of morbidity and mortality.

Do not place the patch lead over nerve tissue as this may cause nerve damage.

Place the patch lead with the conducting coil side facing the heart to ensure delivery of energy to the heart.

Place the sutures well outside the coil of the patch lead or in the area between the coils to avoid possible coil fracture.

If counter shock is unsuccessful using external paddles, adjust the external paddle position (e.g., anterior-lateral to anterior-posterior) and be sure that the external paddle is not positioned over the patch.

Do not fold, alter, or remove any portion of the patch as it may compromise electrode function or longevity.

If a header port is unused on the generator, the port must be plugged to protect the generator.

4.6. GENERATOR EXPLANT AND DISPOSAL

Interrogate the device, and program shock therapy off prior to explanting, cleaning or shipping the device to prevent unwanted shocks.

Return all explanted generators and leads to the manufacturer.

Never incinerate the device due to the potential for explosion. The device must be explanted before cremation.

5. ADVERSE EVENTS

Clinical data presented in this section are from the Defender and SafeR (AAI <> DDD) clinical studies (for DR model only).

ENERGYA DR / ENERGYA VR is similar in design and function to the Defender devices.

For the DR model only, SafeR (AAI <> DDD) operation in ENERGYA is similar to that in the Symphony pacemaker.

The data provided are applicable to ENERGYA DR / ENERGYA VR.

5.1. DEFENDER STUDY

Clinical study of Defender IV DR 612 included 60 devices implanted in 60 patients, 38 in Europe (37 patients followed for a minimum of 3 months), and 22 in the U.S. (IDE G970282/S15) with a total device exposure of 228.7 and 30.3 device months, respectively. No deaths, serious adverse experiences or complications were judged to be device-related, as determined by the investigator. The following tables summarize the safety data for this study.

There was 1 death in the study that was classified as arrhythmic. The cause of death was recurrent VT/VF which occurred 19 days post implant.

In the following tables, complications are defined as adverse device effect, which cannot be treated or resolved by simple adjustments (e.g. reprogramming) and requires intervention.



NOTE: The company classified as complications those adverse device effects that were treated with surgery or with external defibrillation of a ventricular cardiac event.

Observations are defined as symptomatic or asymptomatic clinical events with potential adverse device effects that do not require intervention or can be corrected by simple adjustments.



NOTE: The company classified as observations those adverse device effects that were treated with programming changes, medication, or other method that was not classified as a complication.

Two of the 38 Defender IV DR 612 patients in Europe (37 patients followed for a minimum of 3 months) experienced a total of three complications, including device failures and replacements. Fourteen of the 38 Defender IV DR 612 patients experienced a total of 18 observations. Complications and observations are reported in Tables 1 and 2. It should be noted that a patient can have more than one observation or complication. There were no observations or complications in the U.S.

Table 1: Summary of European Clinical Complications

(Including Device Failures and Replacements)

All complications, 2 of 38 Defender IV DR 612 patients in Europe

Event	# of Patients	% of Patients	# of Events	Events/100 Device-Years*
Hematoma	1	2.6	1	5.2
Ventricular lead migration/dislodgment	2	5.3	2	10.5

* There were 228.7 device months in this study.

Table 2: Summary of European Clinical Complications

(Including Patient Complaints)

All complications, 14 of 38 Defender IV DR 612 patients in Europe

Event	# of Patients*	% of Patients	# of Events	Events/100 Device-Years**
Change in ventricular sensing threshold	1	2.6	1°	5.2
Device reset***	1	2.6	1°	5.2
Inappropriate therapy for EMI	1	2.6	1°	5.2
Pneumothorax	1	2.6	1°	5.2
Pocket hematoma	2	5.3	2°	10.5
Pocket infection/hematoma	1	2.6	1°	5.2
Pocket infection from previous pacemaker	1	2.6	1°	5.2
Prolonged implant procedure	1	2.6	1	5.2
Sensor acceleration during telemetry***	1	2.6	1	5.2
Shock for VT in VF Zone	1	2.6	1°	5.2
Slow VT not converted by ATP therapy	1	2.6	2°	10.5
Unsatisfactory sensing threshold test***	2	5.3	2	10.5
Ventricular oversensing	3	7.9	3	15.7

* A patient can have more than one observation.

** There were 228.7 device months in this study.

***These observations would not have happened with the currently marketed device and programmer.

°Investigator indicated that Defender IV DR did not cause or contribute to the event.

5.2. SAFER (AAI <> DDD) STUDY (FOR DR MODEL ONLY)

Clinical study of the SafeR (AAI <> DDD) included 45 Symphony 2550 devices implanted in 45 patients. No serious adverse events were device- or feature-related. There were no deaths in the study.

Table 1: Summary of Symphony safety data during study

	Patients		Number of events	
	Number of patients	% of patients	Number of events	Events per device year ^(a)
Deaths	0	0	0	0
Explants	0	0	0	0
Serious pacemaker related events outside the use of SafeR (AAI <> DDD)	0	0	0	0

5. ADVERSE EVENTS

	Patients		Number of events	
	Number of patients	% of patients	Number of events	Events per device year ^(a)
Non-serious pacemaker related events outside the use of SafeR (AAI <> DDD)	0	0	0	0
Serious events due to the use of SafeR (AAI <> DDD)	0	0	0	0
Non-serious events related due to the use SafeR (AAI <> DDD)	13	28.9	15	3.2
Serious non-pacemaker related events	6	13.3	9	1.9
Non-serious non-pacemaker related events	8	17.8	8	1.7

^(a) 4.74 device years

Non-serious events due to the use of SafeR 2 (AAI <> DDD) included: delay in switching on 2nd degree AV block, inappropriate classification of a PAC, disagreement between markers and recorded EGM, atrial pacing above the maximum rate, recycling on an R-wave in a refractory period, and disagreement in the statistics for switches to DDD. No patient symptoms were associated with these events.

6. CLINICAL STUDIES

Clinical data presented in this section are from the Defender and SafeR (AAI <> DDD) clinical studies (for DR model only).

ENERGYA DR / ENERGYA VR is similar in design and function to the Defender devices.

For the DR model only, SafeR (AAI <> DDD) operation in ENERGYA is similar to that in the Symphony pacemaker.

The data provided are applicable to ENERGYA DR / ENERGYA VR.

6.1. DEFENDER STUDY

Objectives:

The primary objectives of this study were to demonstrate a complication free rate (CFR) comparable to that of historical controls, to demonstrate, using a chronotropic assessment exercise protocol (CAEP), a rate response proportional to and appropriate for the level of exercise, and to evaluate and report the incidence of adverse events.

Materials:

Each patient received one Defender IV DR 612 defibrillator, an atrial pacing and sensing lead, and a Medtronic, Angeion, or Biotronik defibrillation lead in the U.S. or any commercially available defibrillator lead outside the U.S.

Methods:

Investigators selected patients who survived at least one episode of cardiac arrest (manifested by loss of consciousness) presumably due to a ventricular tachyarrhythmia or exhibited recurrent, poorly tolerated, sustained ventricular tachycardia (VT). The protocol required evaluation of performance and adverse events at pre-discharge, one month, three months, six months, and (in the U.S.) every three months thereafter. At the one-month visit, eligible patients performed a chronotropic assessment exercise protocol (CAEP) maximal exercise test.

Study Population.

The table below summarizes inclusions.

Region	Date of first implant	Date of last implant	Data cut-off date	Number of centers	Number of patients
US	14-Dec-99	08-Mar-00	14-Mar-00	6	22
Europe	04-May-99	26-Jul-99	14-Apr-00	11	38
All	04-May-99	08-Mar-00	14-Apr-00 (Eur), 14-Mar-00 (US)	17	60

6.1.1. Complication-free rate

Only European patients followed for at least 3 months:

Symbol	Parameter	Defender IV DR 612
N	Overall number of patients	37
Pe*N	Number of successes	35

Symbol	Parameter	Defender IV DR 612
Pe	Observed experimental proportion	0.95
Ps	Null hypothesis success rate	0.76
ES	Estimated standard error of Pe	0.04
z'	Test statistic ⁽¹⁾	4.75
p	Associated p-value	< 0,0001

(1) Statistical test: $z' = (Pe - Ps) / SE$ where $SE = \sqrt{Pe(1 - Pe) / N}$

6.1.2. Rate response

European patients only:

GROUP	Number of patients included	Mean slope %SRR on %MR	STD of slopes %SRR on %MR	SE of mean slope %SRR on %MR	Lower 95% CI	Upper 95% CI
Europe	20	0.77	0.17	0.04	0.69	0.84
Small Centers	9	0.79	0.18	0.06	0.67	0.91
Large Centers	11	0.75	0.15	0.05	0.66	0.84
Males	17	0.77	0.16	0.04	0.70	0.85
Females	3	0.73	0.22	0.13	0.47	0.98

SRR: Sensor Rate Reserve

MR: Metabolic Reserve

STD: Standard Deviation

SE: Standard Error

CI: Confidence Interval

6.1.3. Adverse events

Event US (N=22)	Number of events*	Number of patients	Percent of patients
Intent to treat but did not	0	0	0.0
Non-device related death	0	0	0.0
Explant	0	0	0.0
Complication	0	0	0.0
Observation	0	0	0.0
Serious non-related other than death	1	1	4.5

Event Europe (N=38)	Number of events*	Number of patients	Percent of patients
Intent to treat but did not	0	0	0.0
Non-device related death	1	1	2.6
Explant	1	1	2.6
Complication	3	2	5.3

Event Europe (N=38)	Number of events*	Number of patients	Percent of patients
Observation	18	14	36.8
Serious non-related other than death	12	7	18.4

Event All (N=60)	Number of events*	Number of patients	Percent of patients
Intent to treat but did not	0	0	0.0
Non-device related death	1	1	1.7
Explant	1	1	1.7
Complication	3	2	3.3
Observation	18	14	23.3
Serious non-related other than death	13	8	13.3

* A patient can have more than one complication, observation, or serious adverse event, not device-related.

Device Failures and Replacements:

No device failures or replacements occurred with Defender IV DR 612 during the study.

6.2. SAFER (AAI <> DDD) STUDY (FOR DR MODEL ONLY)

SafeR (AAI <> DDD) mode in ENERGYA is similar to that in Symphony.

The differences in SafeR (AAI <> DDD) mode between the two devices are:

- To prevent long RR intervals during VT/VF, SafeR (AAI <> DDD) has no effect during VT/VF therapy, electrophysiologic studies, and post-shock recovery.
- The maximum acceptable AV delay for first degree AV block varies as a function of pacing rate.
- ENERGYA requires a ventricular sensed event to atrial paced event (RA) interval of at least 100 ms. Therefore, the device lengthens the atrial escape interval so that it ends at least 102 ms after the ventricular event.
- During atrial fibrillation episode, pause criterion is fixed to 2s to avoid long bradycardia episodes in switching to DDD mode.

Despite these differences, the data collected on Symphony devices are applicable to ENERGYA because the principles of SafeR (AAI <> DDD) operation did not change. The criteria for switching from AAI to DDD (or vice versa) did not change. The device's method for evaluating the presence of AV conduction did not change.

Methods:

All patients were implanted with a Symphony Model 2550 dual-chamber rate-responsive pacemaker with SafeR (AAI <> DDD) mode. A variety of marketed atrial and ventricular pacing leads were used. The pacemaker was programmed and interrogated via bi-directional telemetry using a MicroPort dedicated programmer and a CPR3 programming head.

The study's routine evaluation consisted of enrollment, pre-discharge evaluation, and a scheduled follow-up visit at one month. At pre-discharge, a 24-hour Holter recording was performed and pacemaker memory was read. At one month, pacemaker memory was read. Investigators also documented adverse events.

Patients studied:


A total of 45 patients from 12 centers had Symphony 2550 pacemakers with SafeR (AAI <> DDD). Of these, 14 (31 %) were female and 31 (69 %) were male. Mean patient age ($\pm$ SD) was 74 ± 9 years.

Primary indications for implant were: 1st degree AV block (11.1 %), 2nd degree AV block (6.7 %), 3rd degree AV block (22.2 %), sinus node dysfunction (62.2 %) or other (6.7 %).

Effectiveness results:

To determine the effectiveness of SafeR (AAI <> DDD) mode, the percentage of ventricular pacing provided over one month was recorded from pacemaker memory.

Thirty-five patients contributed data to evaluate the percentage of ventricular pacing provided with SafeR (AAI <> DDD). Twenty-nine patients had 1 % or less ventricular pacing and six patients had a range of 28-97 % ventricular pacing. The graph below shows the distribution of ventricular pacing observed in patients with and without AV block as a primary indication for implant.

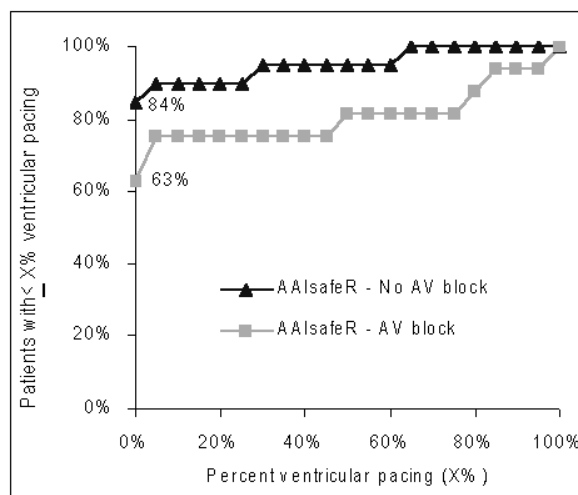

The graph shows that many patients programmed to SafeR (AAI <> DDD) had less than 1% ventricular pacing:

- 84 % of patients without AV block at implant.
- 63 % of patients with AV block at implant.

In a representative reference group⁽¹⁾ of patients programmed to DDD, none had less than 1 % ventricular pacing and only 10 % had less than 90 % ventricular pacing regardless of AV block indication at implant.

The actual reduction of ventricular pacing that SafeR (AAI <> DDD) provides in an individual will depend on the amount of time that the patient spends in AV block. SafeR (AAI <> DDD) cannot and should not provide any decrease in ventricular pacing while the patient is in AV block.

⁽¹⁾ Pioger G, Jauvert G, Nitzsché R, Pozzan J, Laure H, Zigelman M, Leny G, Vandrell M, Ritter P, and Cazeau S. Incidence and predictive factors of atrial fibrillation in paced patients. *PACE*, 28, Supp 1: S137-141; January 2005. This was a prospective observational study of 377 patients with a functionally similar device programmed to DDD. The primary indications for implant were: AV block (49 %), sinus node disease (16 %), brady-tachy syndrome (5 %), AV block + sinus node disease (19 %), AV block + brady-tachy syndrome (6 %), and brady-tachy syndrome + sinus node disease (5 %).

Adverse events

Clinical study of the SafeR (AAI <> DDD) included 45 Symphony 2550 devices implanted in 45 patients. No serious adverse events were device- or feature-related. There were no deaths in the study. Table 1 summarizes the safety data for this study.

Table 1: Summary of Symphony safety data during study

	Patients		Number of events	
	Number of patients	% of patients	Number of events	Events per device year ^(a)
Deaths	0	0	0	0
Explants	0	0	0	0
Serious pacemaker related events outside the use of SafeR (AAI <> DDD)	0	0	0	0
Non-serious pacemaker related events outside the use of SafeR (AAI <> DDD)	0	0	0	0
Serious events due to the use of SafeR (AAI <> DDD)	0	0	0	0
Non-serious events related due to the use of SafeR (AAI <> DDD)	13	28.9	15	3.2
Serious non-pacemaker related events	6	13.3	9	1.9
Non-serious non-pacemaker related events	8	17.8	8	1.7

^(a) 4.74 device years

Non-serious events due to the use of SafeR 2 (AAI <> DDD) included: delay in switching on 2nd degree AV block, inappropriate classification of a PAC, disagreement between markers and recorded EGM, atrial pacing above the maximum rate, recycling on an R-wave in a refractory period, and disagreement in the statistics for switches to DDD. No patient symptoms were associated with these events.

7. PATIENT INFORMATION

Information for the patient is available in the patient booklet, contained in the outer storage package. Please inform him/her that the document is also available on the website: www.microportpatients.com, this web link is displayed on the device implant card.

Additional copies can be obtained by contacting your MicroPort representative.

This information should be given to each patient with their first ICD and offered to the patient on each return visit or as deemed appropriate.

8. PATIENT SELECTION AND TREATMENT

8.1. INDIVIDUALIZATION OF TREATMENT

Exercise stress testing:

If the patient's condition permits, use exercise stress testing to:

- Determine the maximum rate of the patient's normal rhythm,
- Identify any supraventricular tachyarrhythmias,
- Identify exercise-induced tachyarrhythmias.

The maximum exercise rate or the presence of supraventricular tachyarrhythmias may influence selection of programmable parameters. Holter monitoring or other extended ECG monitoring also may be helpful.



CAUTION: To avoid inappropriate therapy during an exercise stress test, do not reprogram any parameter during the test. When a parameter is reprogrammed, algorithm forces acceleration to "ventricular". During conducted sinus tachycardia within the programmed Tachy zone, the device detects a 1:1 fast rhythm. Assuming that acceleration was set to ventricular by reprogramming, the device may identify this as a VT, and may immediately apply the corresponding therapy.

Electrophysiologic (EP) testing:

EP testing may be useful for ICD candidates.

EP testing may identify the classifications and rates of all the ventricular and atrial arrhythmias, whether spontaneous or during EP testing.

Drug resistant supraventricular tachyarrhythmias (SVTs):

Drug resistant supraventricular tachyarrhythmias (SVTs) may initiate frequent unwanted device therapy.

A careful choice of programming options is necessary for such patients.

Antiarrhythmic drug therapy:

If the patient is being treated with antiarrhythmic or cardiac drugs, the patient should be on a maintenance drug dose rather than a loading dose at the time of ICD implantation. If changes to drug therapy are made, repeated arrhythmia inductions are recommended to verify ICD detection and conversion. The ICD also may need to be reprogrammed.

Changes in a patient's antiarrhythmic drug or any other medication that affects the patient's normal cardiac rate or conduction can affect the rate of tachyarrhythmias and/or efficacy of therapy.

Direct any questions regarding the individualization of patient therapy to MicroPort's representative.

8.2. SPECIFIC PATIENT POPULATIONS

Pregnancy:

If there is a need to image the device, care should be taken to minimize radiation exposure to the fetus and the mother.

Nursing Mothers:

Although appropriate biocompatibility testing has been conducted for this implant device, there has been no quantitative assessment of the presence of leachables in breast milk.

Pediatric Patients:

This device has not been studied in patients younger than 18 years of age.

Geriatric Patients:

Most of the patients receiving this device in clinical studies were over the age of 60 years.

Handicapped and Disabled Patients:

Special care is needed in using this device for patients using an electrical wheel chair or other electrical (external or implanted) devices.

9. PATIENT COUNSELING INFORMATION

The physician should consider the following points in counseling the patient about this device:

- Persons administering CPR may experience tingling on the patient's body surface when the patient's ICD system delivers a shock.
- Advise patients to carry MicroPort ID cards and/or ID bracelets documenting their ICD system.

10. DECLARATION OF CONFORMITY

Federal Communication Commission Interference Statement 47 CFR Section 15.19 and 15.105(b)

FCC ID: YSGIS1BLE

This FCC ID is applicable for ENERGYA VR 3140 and ENERGYA DR 3440.

ENERGYA pacemaker is featuring Bluetooth Low Energy communication capability. Using a standard Bluetooth Low Energy component not initially intended for use in life support applications, MicroPort CRM has fully qualified that Bluetooth Low Energy communication to comply with implantable medical devices intended use and safety requirements.

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna of the radio or television.
- Increase the separation between the equipment and receiver.
- Consult the dealer or an experienced radio/TV technician for help.

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

FCC Interference Statement 47 CFR Section 15.21 - No Unauthorized Modifications



CAUTION:

This equipment may not be modified, altered, or changed in any way without signed written permission from MicroPort. Unauthorized modification may void the equipment authorization from the FCC and will void the MicroPort warranty.

Identification of the equipment according to Section 95.1217(a)

This transmitter is authorized by rule under the Medical Device Radiocommunication Service (in part 95 of the FCC Rules) and must not cause harmful interference to stations operating in the 400.150-406.00 MHz band in the Meteorological Aids (i.e., transmitters and receivers used to communicate weather data), the Meteorological Satellite, or the Earth Exploration Satellite Services and must accept interference that may be caused by such stations, including interference that may cause undesired operation. This transmitter shall be used only in accordance with the FCC Rules governing the Medical Device Radiocommunication Service. Analog and digital voice communications are prohibited. Although this transmitter has been approved by the Federal Communications Commission, there is no guarantee that it will not receive interference or that any particular transmission from this transmitter will be free from interference.

11. PHYSICIAN GUIDELINES

11.1. PHYSICIAN TRAINING

Physicians should be familiar with sterile pulse generator implant procedure and familiar with follow-up evaluation and management of patients with an implantable defibrillator (or referral to such a physician).

11.2. DIRECTIONS FOR USE

ICD operating characteristics should be verified at the time of implantation and recorded in the patient file. Complete the *Patient Registration Form* and return it to MicroPort, as it provides necessary information for warranty purposes and patient tracking.

Additional programming instructions can be found by accessing Online Help (click the “?” on the screen) on the MicroPort dedicated programmer. Paper copies of Online Help can be obtained by contacting your MicroPort representative.

11.3. MAINTAINING DEVICE QUALITY

This device is **FOR SINGLE USE ONLY**. Do not resterilize and reimplant explanted ICDs.

Do not implant the device when:

- It has been dropped on a hard surface because this could have damaged pulse generator components.
- Its storage package has been pierced or altered, because this could have rendered it non-sterile.
- It has been stored or transported outside the environmental temperature limits: 32 °F (0 °C) to 122 °F (50 °C) as an electrical reset condition may occur.
- "Use by" date has expired, because this can adversely affect pulse generator longevity or sterility.

12. HOW SUPPLIED

12.1. STERILITY

The ENERGYA defibrillators are supplied one per package in a sterile package.

12.2. WARRANTY AND REPLACEMENT POLICY

MicroPort warrants its defibrillators. Refer to the section "Warranty" for additional information. Please see the following labeling sections for information concerning the performance of this device: Indications, Contraindications, Warnings and Precautions, and Adverse Events.

13. DEVICE DESCRIPTION

The ENERGYA DR / ENERGYA VR ICD device and programming system. The programming system includes the MicroPort dedicated programmer⁽¹⁾ with the SmartTouch programming software connected to a CPR4 programming head. The programming system is configured and furnished by MicroPort.

The ENERGYA DR / ENERGYA VR can serve as a defibrillation electrode (active housing) with a total surface area of 63 cm².

The ENERGYA DR / ENERGYA VR is designed to recognize and treat slow or fast VT and VF by continuously monitoring atrial and ventricular activity to identify persistent ventricular arrhythmias and to deliver appropriate therapies. ENERGYA DR / ENERGYA VR features the PARAD/PARAD+ algorithm, which is specifically designed to differentiate ventricular tachycardias from fast rhythms of supraventricular origin. PARAD/PARAD+ continuously monitors R-R interval stability, searches for long cycles, assesses the degree of P-R association, evaluates sudden onset and determines the chamber of arrhythmia acceleration.

For the VR model only, the ENERGYA DR / ENERGYA VR is designed to recognize and treat slow or fast VT and VF by continuously monitoring ventricular activity to identify persistent ventricular arrhythmias and to deliver appropriate therapies. ENERGYA DR / ENERGYA VR features DISCRIMINATION algorithm, which is specifically designed to differentiate ventricular tachycardias from fast rhythms of supraventricular origin. DISCRIMINATION continuously monitors R-R interval stability, searches for long cycles and evaluates sudden onset.

In addition to the advanced detection scheme (for DR model only), ENERGYA DR / ENERGYA VR offers programmable dual or single-chamber pacing therapy (DDD, DDI, VVI or SafeR (AAI <> DDD) modes) with or without rate-responsive capabilities (DDDR, DDIR, VVIR, DDD/DDIR and SafeR-R (AAIR <> DDDR) modes) using an acceleration sensor. An automatic AV delay algorithm as well as a mode switching function are available.

In addition to the advanced detection scheme (for VR model only), ENERGYA DR / ENERGYA VR offers programmable single-chamber pacing therapy with or without rate-responsive capabilities using an acceleration sensor.

ENERGYA DR / ENERGYA VR offers tiered therapy. Therapies can be programmed independently in each zone:

- in the Slow VT and VT zones: two ATP programs, up to two shocks with programmable energy and up to four shocks with maximum energy can be programmed;
- in the VF zone: one ATP program, up to two shocks with programmable energy and up to four shocks with maximum energy can be programmed.

When the rhythm changes from one zone to another, the device delivers the therapy programmed in this zone, starting with the same or more aggressive program for the zone. The ATP program in the VF zone will only be applied if the VT coupling interval is longer than the programmed fast VT cycle length.

The ENERGYA DR / ENERGYA VR offers biphasic shocks with a maximum stored energy of 42 J. The shock configuration (electrodes used to apply the shock) can be chosen by programming one of the following combinations: can and one coil, can and two coils, two coils only.

Other features are as follows:

- Automatic ventricular sensitivity control
- Non-committed shocks
- Electrophysiological studies (EPS) with real-time markers or electrograms:
 - Programmer-controlled VT induction sequences,
 - Programmer-controlled VF inductions (30 Hz rapid pacing or shock on T),
 - Programmable electrogram vectors (A / RV coil-CAN / SVC coil-CAN /RV coil-SVC coil /A ring-CAN / RV tip-CAN / RV ring-CAN) and RV EGM for DR model,
 - Programmable electrogram vectors (RV coil-CAN / SVC coil-CAN /RV coil-SVC coil /RV tip-CAN / RV ring-CAN) and RV EGM for VR model,
 - Real-time annotations displayed with the markers and indicating the majority rhythm,
 - Manual ATP sequences,
 - Manual shocks.
- Rescue shock
- Follow-up tests:
 - Pacing lead impedance,
 - Coil impedance,
 - Capacitor charge time,
 - Pacing threshold tests.
- Data storage:
 - Therapy History Report,
 - Statistics (pace/sense, therapy, shocks, and battery voltage),
 - Up to 16 complete Holter records with event logs, marker channel notation, and electrogram records.

The ENERGY DR 3440 connector head has two ports:

- Atrial “IS-1” port: performs atrial bipolar pace/sense,
- RV “DF4” port: performs right ventricular bipolar pace/sense, port for RV/SVC defibrillation coils.

The ENERGY VR 3140 connector head has one port:

- RV “DF4” port: performs right ventricular bipolar pace/sense, port for RV/SVC defibrillation coils.

For the DR model, the atrial port is compatible with the IS-1 standard and the quadripolar right ventricular port is compatible with the DF4 standard.

Distal lead terminal connections are secured with set-screws accessed via self-sealing silicone plugs. All lead connections pass through the header into the device via feedthroughs.

Programming System:

The MicroPort programmer is used in conjunction with specific programmer software to interrogate and program the implanted device at implant and during patient follow-up procedures.

Remote Monitoring:

ENERGYA DR / ENERGYA VR is also equipped with the wireless Bluetooth Low Energy communication technology which enables to remotely monitor the patients who have the MicroPort SMARTVIEW CONNECT monitor installed at home.

⁽¹⁾*The software bill of materials is available upon request.*

14. IMPLANT PROCEDURE

14.1. NECESSARY EQUIPMENT

Implantation of ENERGYA DR / ENERGYA VR requires the following equipment:

- MicroPort SMARTTOUCH programmer, equipped with the SMARTVIEW software interface and inductive telemetry head,
- pacing system analyzer, as well as its sterile connecting cables, to evaluate the pacing and sensing thresholds,
- a ventricular pacing and defibrillation lead with corresponding introducers,
- physiological signal monitor capable of displaying simultaneously the surface ECG and arterial pressure,
- an external defibrillator with sterile external paddles,
- sterile cover for the telemetry head.

Implantation of ENERGYA DR also requires the following equipment:

- an atrial pacing lead with corresponding introducers.



NOTE: In case you are implanting a DF4 lead, please verify its compatibility with standard alligator clips; please refer to the lead user's manual for more details.

14.2. PACKAGING

14.2.1. Contents

ENERGYA DR / ENERGYA VR and its accessories are ethylene oxide sterilized and hermetically sealed in two-ply clear packaging meeting international requirements.

The sterile packaging contains:

- The defibrillator
- A ratcheting screwdriver intended to be used with ENERGYA devices only to tighten the set screws of the device header once the lead(s) pin(s) are inserted

As delivered, ENERGYA DR / ENERGYA VR are programmed to as-shipped values that are different from nominal values (see Chapter “Programmable Parameters” for details).

The non-sterile packaging contains:

- Leads connection leaflet
- Patient implant card
- Implant registration form
- Return envelope
- Patient booklet
- Website leaflet

14.3. OPTIONAL EQUIPMENT

The following equipment may be required during implantation of ENERGYA DR / ENERGYA VR:

- an IS-1 insulating plug to close the atrial port (for DR model only)
- Sterile water to clean traces of blood. Any parts cleaned with sterile water must be thoroughly dried
- Mineral oil to lubricate if necessary
- A lead cap to isolate a lead which is not used

14.4. OPENING THE PACKAGE

Before opening the package, check the "Use by" date printed on the labels on the box and on the sterile package. Defibrillators that have not been implanted by the end of the "Use by" date should be returned to MicroPort.

Interrogate the device:

- if a warning is displayed, do not implant the device and contact your MicroPort representative.
- if battery voltage is below 3V, and if the last reforming/charge occurred more than one week ago, do not implant the device. Otherwise, wait for one more week before checking the voltage.



NOTE : The battery voltage can decrease before the expiration date is reached. However, the battery voltage should be equal to or higher than 3V at the time of implant.

When using the inductive wand, devices **MUST NOT** be interrogated and/or programmed within the vicinity of other devices.

Also check the integrity of the sterile package. The sterility of the contents is no longer guaranteed if the package has been pierced or altered. If the defibrillator is no longer sterile, it should be returned in its packaging to MicroPort. Any re-sterilization of the unit is at the discretion of MicroPort.

Open the sterile package within the sterile field and carefully remove the device (see Figure – *Opening the sterile package*).

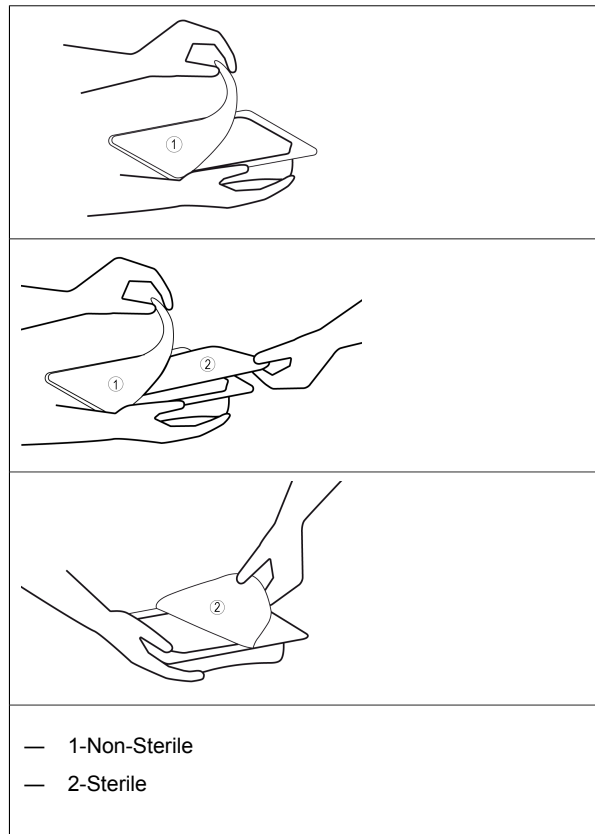


Figure - Opening the sterile package

14.5. PRIOR TO IMPLANTATION

Use the programmer to verify the defibrillator can be interrogated before implantation.

Verify all shock therapies are disabled in order to avoid accidental discharge during implantation.

It is not advisable to program the Smoothing function before implantation, since the defibrillator may detect noise and pace at a rate higher than the programmed basic rate.



CAUTION:

Do not shake or tap sharply on the ICD package with the ICD inside, because the ICD's sensing circuits can interpret this as P-waves (for DR model only) or R-waves and record these as an arrhythmia episode.

High voltage capacitors charge performed on ICD without connected leads using wireless telemetry can generate false P-waves (for DR model only) or R-waves detection.

14.6. DEVICE PLACEMENT

The pocket should be prepared in the left pectoral position, either subcutaneously or submuscularly. Subcutaneous device implantation is recommended for optimal RF communication efficacy.

Implantation in an abdominal position is not advisable.

In its final position, the defibrillator should be no more than 4 cm (1.6 in) below the skin's surface.

14.7. CHOOSING THE TYPE OF LEAD

The defibrillator should be connected to:

ENERGYA DR should be connected to:

- one bipolar atrial sensing/pacing lead
- one right ventricular lead with bipolar sensing/pacing electrodes and one or two defibrillation coils

ENERGYA VR should be connected to:

- one right ventricular lead with bipolar sensing/pacing electrodes and one or two defibrillation coils

The choice of lead(s) and their configuration is left to the implanting physician's judgment.

The lead-device system compatibility is verified with MicroPort leads but has not been tested with non-MicroPort leads. Using non-MicroPort leads may lead to adverse events including oversensing or undersensing of cardiac activity, leading to inappropriate therapy delivery.



NOTE 1: Please note that, DF-1 standard compliant lead is not compatible with DF4 connector. In the reverse, DF4 standard compliant lead is not compatible with DF-1 connector. In case of defibrillator replacement, Choose the appropriate device compatible with DF-1 or DF4 leads. For any other lead type that require an adaptor for this device, please contact your MicroPort representative for any information on lead / connector compatibility question.

NOTE2 (for DR model only): In the event that no atrial lead is implanted, the atrial port should be plugged with IS-1 insulating plug and a single chamber mode (VVI-VVIR) should be programmed. PARAD and PARAD+ should not be used.

NOTE3: In the event of a warning on a low shock impedance, and after lead replacement or reconnection: it is recommended to check the system integrity (sensing and pacing thresholds and the impedance of the shock electrodes).

NOTE4: The use of a high polarization ventricular lead interferes with normal operation of the Ventricular Autothreshold function.

Connectors:

ENERGYA DR 3440:

The pacing/sensing atrial connector is compatible with the IS-1 standard and the quadripolar right ventricular connector is compatible with the DF4 standard.

ENERGYA VR 3140:

The quadripolar right ventricular connector is compatible with the DF4 standard.


14.8. SHOCK CONFIGURATION (+ -> -)

The shock configuration is the energy pathway between the defibrillation electrodes. If an atrial coil (SVC) is present, the shock configuration can be programmed for bi-directional shocks.

Programming:

When active case and atrial coil (SVC) are both programmed to Yes, the shock configuration can be programmed to:

- RV to Case (or Case to RV),
- or RV to SVC (or SVC to RV),
- or RV to Case+SVC (or Case+SVC to RV).

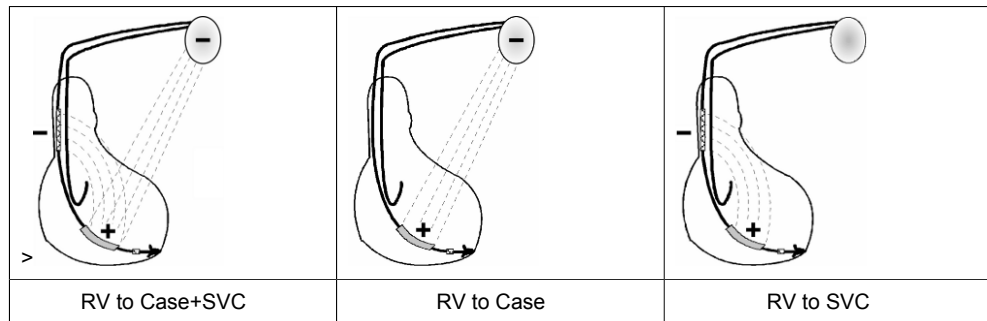

The polarity of shock is determined by the parameter itself.

14.9. MEASUREMENT OF THRESHOLDS AT IMPLANT

Pacing and sensing thresholds and pacing impedances should be measured at implant. In case of values outside the indicative thresholds below, lead-connector compatibility should be further verified.

Pacing thresholds:

Acute thresholds should be lower than 1 V (or 2 mA) for a 0.35 ms pulse width, in the ventricle and in the atrium (for DR model only).

Sensing thresholds:

For appropriate ventricular sensing, the amplitude of the R-wave should be greater than 5 mV.

For appropriate atrial sensing (for DR model only), the amplitude of the P-wave should be greater than 2 mV.

Pacing impedance measurements:

Ventricular and atrial (for DR model only) pacing impedances should range from 200 to 3000 ohms (refer to the lead characteristics, especially if high impedance leads are used).

Please refer to the leads user manuals for more details on the expected electrical performances of the leads.

14.10. LEADS CONNECTION

For DR model only: Implant the ventricular lead, then the atrial lead.

For VR model only: Implant the ventricular lead.

Each lead must be connected to the corresponding connector port. The position of each connector is indicated on the casing.

**CAUTION:**


Tighten only the distal connector block.

To connect each lead, proceed as follows:

1. Clean the lead terminal pins thoroughly, if necessary (device replacement).
2. Lubricate the lead terminal pins with sterile water, if necessary.
3. Do not insert a lead connector pin into the connector block without first visually verifying that the lead port is not obstructed.
4. Insert the screwdriver into the pre-inserted screw socket of the appropriate port (in order to allow excess air to bleed out and to make the insertion of the lead pin easier).
5. Insert the lead pin all the way into the port (check that the pin protrudes beyond the distal connector block).
6. Tighten, check the tightness and ensure the lead pin still protrudes beyond the distal connector block, and has not moved.

**CAUTION:**

1. Do not tighten the pre-inserted screws when there is no lead (this could damage the connector).
2. Do not loosen the screws before inserting the connector (subsequent risk of being unable to reinsert the screw).
3. When mineral oil or sterile water is used to make lead insertion easier, the screwdriver should remain inserted into the pre-inserted screw socket when checking the tightness. As a matter of fact, when the lead port is filled with a liquid, the physics piston effect can give the feeling the lead is properly tightened.
4. One single set screw is located on the side of the connection header.
5. Use only the screwdriver provided with the defibrillator. Keep the screwdriver's shaft perpendicular to the plane of the defibrillator (see figure below).
6. Removing the screwdriver: to avoid all risk of loosening screws during removal, hold the screwdriver by its metal part and not by the handle.

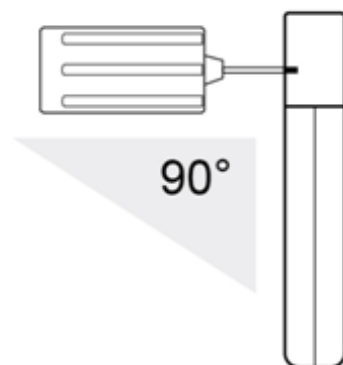

WARNING: Ensure that the screwdriver's tip is fully inserted in the setscrew; otherwise the screwdriver can damage the setscrew and prevent connection with or disconnection from the lead.

To ensure full insertion, push the screwdriver's hex tip smoothly into the setscrew until it reaches the bottom of the hex chamber in the screw, which can be felt as a solid metallic contact. Do not implant the defibrillator if there is no feeling of solid metallic contact. Do not implant the defibrillator if the wrench does not click when attempting to tighten the setscrew on the lead pin.

14.11. DEVICE IMPLANTATION

ENERGYA DR / ENERGYA VR should be implanted with the identification engraved side facing outwards for optimal communication with the programming head and radiographic identification.

In order to prevent lead damage or dislodgement, it is important to loosely coil the leads and place them in a manner that minimizes lead tension, twisting, sharp angles, and pressure.

The following factors should be considered in placing any excess of lead length:

1. recommendations/warnings of the (other) associated leads,
2. patient anatomy, and
3. pulse generator size and motion.

Suture the casing connector to the muscle using the hole provided for this purpose, in order to avoid potential migration of the device into the pectoral muscle.

14.12. TESTS AND PROGRAMMING

During the implant testing procedure:

It is recommended that a safety margin of at least 10 J be demonstrated between the effective shock energy and maximum programmable energy.

Enable shock therapies, then program the defibrillator.

Verify that the defibrillation shock impedance for each shock delivered is within the range of 30 to 150 ohms. Check the lead-connector compatibility if the values are outside these boundaries.

Save the programming data on the programmer's hard disk and on an external storage device (if desired).

Resuscitation Availability:

Do not perform device testing unless an external defibrillator is available and medical personnel skilled in cardiopulmonary resuscitation (CPR) are present.

Disable the ICD During Handling:

Program Shock Therapy to OFF to prevent the user from receiving an unexpected electrical shock delivered by the device during either system implantation, replacement or post-mortem removal surgical procedures.



CAUTION: It is recommended to reset the memory data and statistics once the device is implanted.

15. SPECIAL MODES

15.1. MRI MODE

The MRI mode is an asynchronous mode (VOO or OOO for the VR model; DOO, VOO or OOO for the DR model) which is triggered either manually or upon detection of a magnetic field.

The MRI Mode is intended to be applied during MRI examination. When MRI Mode is activated (Auto or Manual), the magnet mode is ineffective.



NOTE: Refer to the MRI Solutions manual for the complete instructions for use available at www.microportmanuals.com.

15.2. SAFETY MODE (NOMINAL VALUES)

Nominal values may be rapidly restored by pressing the following button on the programming head or programmer keyboard:



or via the Emergency button on the SMARTVIEW screen.

In safety mode, the defibrillator operates with the nominal parameters values in the table of programmable parameters.

15.3. MAGNET MODE

When the magnet is applied:

- ventricular antiarrhythmia functions are inhibited (detection of rhythm disturbances, charging, and therapy),
- AVD paced/sensed offset is set to 0 (for DR model only),
- RV amplitude is set to 6V,
- RA amplitude is set to 6V (for DR model only),
- RV width is set to 1ms,
- RA width is set to 1ms (for DR model only),
- the following functions are disabled:
 - For ENERGYA DR & VR: Smoothing.
 - For ENERGYA DR (only): ventricular arrhythmia prevention, Mode Switch, Anti-PMT.

When the magnet is removed:

- arrhythmia detection algorithms and sequential therapies are reinitialized,
- therapies start with the least aggressive program for each area.

The antiarrhythmia functions inhibition is extended after magnet removal if a charge occurred just before the application of the magnet in order to ease the communication between the device and the programmer.

The other parameters remain at their programmed value.

15.4. RESPONSE IN THE PRESENCE OF DISTURBANCE


If the defibrillator senses electrical noise at a frequency above 16 Hz, it switches to an asynchronous mode at the basic rate. The programmed mode is restored as soon as the noise is no longer detected.

Ventricular pacing may also be inhibited by ventricular noise. It can be restored by setting the parameter “V pacing on noise” to “On”.

15.5. DETECTION CHARACTERISTICS IN THE PRESENCE OF ELECTROMAGNETIC FIELDS

Per Clause 27.4 of Standard EN 45502-2-2, detection in the presence of electromagnetic fields is characterized as follows:

— Differential mode:

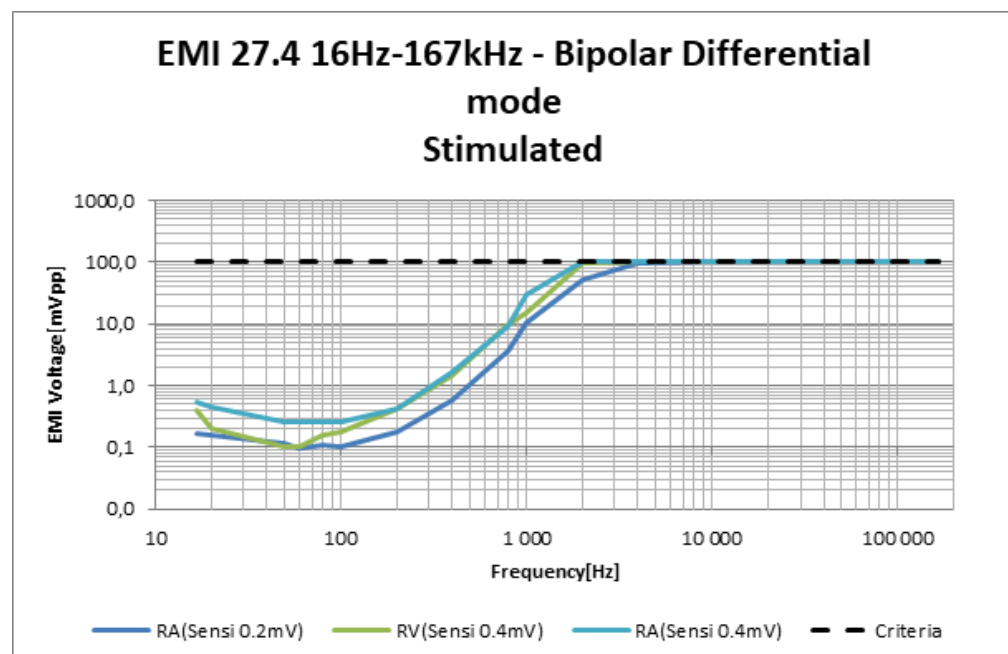

NOTE: RA channel for DR model only.

— Common mode rejection ratio:

CMRR (channel vs frequency)	16.6 Hz	50 Hz	60 Hz	100 Hz
Atrial channel	≥75 dB	76 dB	79 dB	74 dB
Ventricular channel	≥68 dB	≥79 dB	≥79 dB	≥75 dB

NOTE: Atrial for DR model only.

For atrial sensitivity settings below **0.4mV**, ENERGIA DR may detect noise lower than the level specified in clause 27.5.1 of standard EN 45502-2-2 for frequencies below 200 Hz.

For ventricular sensitivity settings below **0.6mV**, the ICD may detect noise lower than the level specified in clause 27.5.1 of standard EN 45502-2-2 for frequencies below 200 Hz.

15.6. PROTECTION AGAINST SHORT-CIRCUITS

The defibrillator can undergo a short-circuit if the anode and cathode are not adequately separated.

In this case, the shock is aborted and a warning will indicate that a short circuit (shock impedance < 20 ohms) was detected during the last shock. The device may be damaged compromising ability to provide shock therapy.

16. MAIN FUNCTIONS

16.1. AUTOMATIC LEAD MEASUREMENTS

Automatic pacing lead impedance measurement:

A lead impedance measurement is automatically performed on atrial (for DR model only) and ventricular leads every 6 hours. The daily mean impedance is stored for each chamber.

Automatic coil impedance measurement:

A coil impedance measurement is automatically performed on defibrillation coil(s) once per day. The coil impedance is stored for each coil.

Automatic sensing measurement:

The amplitude of P (for DR model only) and R waves are automatically measured at each cycle. Every 8.5 minutes, the amplitude of the last 8 P and R detections are averaged and stored.

16.2. AUTOMATIC PACING THRESHOLD ADAPTATION

The Autothreshold function allows automatic adjustment of the pacing amplitude, according to a pacing threshold test performed by the device at regular interval:

- For the Right Ventricular Autothreshold (RVAT): every 6 hours
- For the Right Atrial (RAAT) Autothresholds (for DR model only): once a day (programmable "Start Time")

When the Autothreshold function is programmed to "Monitor"

The device determines and stores the pacing threshold but the programmed pacing amplitude is unchanged.

When the Autothreshold function is programmed to "Auto"

The device determines the pacing threshold and programs the pacing amplitude accordingly.

For the Right Atrial (RAAT) (for DR model only) and the Right Ventricular (RVAT) Autothresholds: the pacing amplitude is set to twice the pacing threshold (programmable for A and RV) but never:

- below the "Minimum Amplitude" (programmable for A and RV),
- above the "Maximum Amplitude" (5V for A and 6V for RV).

If the device is not able to determine the pacing threshold, the pacing amplitude is forced to a safe amplitude (either the programmable "Safety Amplitude" or the non programmable "Maximum Amplitude").

Programming constraints:

1. The Autothreshold function is temporarily disabled if the cardiac rhythm is above a limit rate:
 - For Right Ventricular Autothreshold, 95bpm in DDD(R)/SafeR(R), 85bpm in VVI(R)/DDI(R)
 - For Right Atrial Autothreshold, 80 bpm (programmable)
 2. When the Autothreshold function is programmed, the programmable right atrial and right ventricular pulse width are limited to 0.5 ms.
 3. Autothreshold functions are not available in asynchronous mode (OOO, VOO, DOO)
 4. Right Atrial Autothreshold is not available in the following modes: VVI(R), DDI(R).
- Please note that DOO mode is available in DR model only.



WARNING: Certain drugs can greatly increase the pacing threshold. The Autothreshold function should be used with caution, properly adjusting the minimal amplitude.

16.3. ATRIAL TACHYARRHYTHMIA MANAGEMENT (FOR DR MODEL ONLY)

Atrial tachyarrhythmia prevention:

Algorithm designed to increase the pacing rate to overdrive and stabilize the sinus rate and therefore reduce ectopic activity of the patient. This algorithm is designed to prevent atrial tachyarrhythmias and avoid the circumstances of their onset.

Mode Switch:

This function is designed to limit the acceleration and variation of ventricular rate in the presence of atrial arrhythmia.

16.4. VENTRICULAR TACHYARRHYTHMIA MANAGEMENT

FOR ENERGIA DR:

Ventricular tachyarrhythmia prevention:

A set of algorithms designed to reduce ventricular ectopic activity of the patient and that can be used to avoid the circumstances of ventricular tachyarrhythmia onset.

Ventricular tachyarrhythmia detection:

The defibrillator analyzes all ventricular events sensed in the detection zone(s). The device classifies each ventricular event according to programmable rate criteria into one of the three following zones: Slow VT, VT, VF.

Ventricular tachyarrhythmia treatment:

The device only applies the programmed therapy for a given category (VF or VT) when:

- the majority is reached (see 13. Programmable parameters),
- the persistence is reached (see 13. Programmable parameters),
- it finds the last ventricular cycle in that category.

Arrhythmia discrimination algorithm PARAD and PARAD+ (P And R based Arrhythmia Detection):

PARAD is the algorithm used to discriminate sinus tachycardias (ST) and supraventricular tachycardias (SVT) from ventricular tachycardias (VT).

PARAD+ is based on the PARAD algorithm but additionally takes into account the “AF detect” discrimination criteria: the occurrence of a “long ventricular cycle” characteristic for AF patients which is an additional arrhythmia classification criterion to improve identification of atrial fibrillation and avoid inappropriate shocks.

FOR ENERGIA VR:

Arrhythmia discrimination algorithm Stability/Acceleration and Stability+/Acceleration:

Stability/Acceleration is the algorithm used to discriminate sinus tachycardias (ST) and supraventricular tachycardias (SVT) from ventricular tachycardias (VT).

Stability+/Acceleration is based on the Stability/Acceleration algorithm but additionally takes into account the “AF detect” discrimination criteria: the occurrence of a ‘long ventricular cycle’ characteristic for AF patients which is an additional arrhythmia classification criterion to improve identification of atrial fibrillation and avoid inappropriate shocks.

FOR ALL MODELS:

Automatic adjustment of tachycardia therapies (“Autoswitch ATP”):

This feature enables the device to apply the last successful therapy (ATP only) first, therefore changing the sequence of ATP programs if necessary.

Fast VT treatment:

Applies detection criteria on fast ventricular tachycardia that are different from those of the VT zone, as well as different therapies. The fast VT zone is included in the VF zone: its lower limit is determined by the programmed value for the VF zone and its upper limit by the programmed value for the fast VT zone.

Polarity alternation on Max shock:

Reverses the programmed polarity of every second shock set at maximum energy. The number, type, and energy of shocks is independently programmable by detection zone.

Defibrillation threshold (DFT):

Be aware that the changes in the patient's condition, drug regimen, and other factors may change the defibrillation threshold (DFT) which may result in non-conversion of the arrhythmia post-operatively. Successful conversion of ventricular fibrillation or ventricular tachycardia during arrhythmia conversion testing is no assurance that conversion will occur post-operatively.



WARNING: When the pacing mode is programmed to DOO, VOO or OOO, the device does not perform sensing in either atrial and/or right ventricular chamber and tachyarrhythmias therapies (Shocks and ATP) are automatically deactivated. Consequently, tachyarrhythmias cannot be detected nor treated. Use DOO, VOO and OOO mode with caution, only under medical personnel supervision. When leaving DOO, VOO or OOO mode, reactivate the tachyarrhythmias therapies (Shocks and ATP).

Please note that DOO mode is available in DR model only.

16.5. PACING**BTO (Brady Tachy Overlap):**

ENERGYA DR: Corrects chronotropic atrial incompetence by allowing pacing in the slow VT zone, without affecting arrhythmia detection specificity.

ENERGYA VR: Allows pacing in the slow VT zone, without affecting arrhythmia detection specificity.

Post-shock mode:

After any automatic shock therapy, the post-shock mode makes it possible to apply a pacing mode other than the standard antibradycardia pacing mode and/or with different pacing parameters.

SafeR (AAI <> DDD) mode (for DR model only):

Is intended to minimize deleterious effects of ventricular pacing. The defibrillator functions in AAI mode, and temporarily switches to DDD mode upon the occurrence of AVB III, AVB II, AVB I and ventricular pause.

Anti-PMT protection (for DR model only):

Is intended to protect the patient from Pacemaker-Mediated Tachycardia (PMT) without reducing atrial sensing capability of the device.

16.6. SENSING**Automatic Refractory Periods:**

Optimize sensing and make the implant programming easier. These periods are composed of a minimal Refractory Period and a triggerable Refractory Period. The duration of the refractory periods lengthens automatically as needed.

Committed period (for DR model only):

In DDI or DDD modes, the committed period is a non-programmable 95 ms ventricular relative refractory period that starts with atrial pacing. If a ventricular event is sensed during the committed period, but outside the blanking period, the ventricle is paced at the end of the committed period. The committed period prevents inappropriate ventricular inhibition if crosstalk occurs.

Protection against noise:

Allows the distinction between ventricular noise and ventricular fibrillation. If the device senses ventricular noise, the ventricular sensitivity is decreased until noise is no longer detected. Ventricular pacing can be inhibited to avoid a potential paced T-wave.

Automatic sensitivity control:

Optimizes arrhythmia detection and avoids late detection of T-waves and over-detection of wide QRS waves. The device automatically adjusts the ventricular sensitivity based on the measured ventricular amplitude. The sensitivity value will be lowered in case of VF suspicion.



WARNING: When the pacing mode is programmed to DOO, VOO or OOO, the device does not perform sensing in either atrial and/or right ventricular chamber and tachyarrhythmias therapies (Shocks and ATP) are automatically deactivated. Consequently, tachyarrhythmias cannot be detected nor treated. Use DOO, VOO and OOO mode with caution, only under medical personnel supervision. When leaving DOO, VOO or OOO mode, reactivate the tachyarrhythmias therapies (Shocks and ATP).

Please note that DOO mode is available in DR model only.

16.7. RATE RESPONSE

The rate response function enables the device to adjust the pacing rate based on the patient's physical activity.

The defibrillator is equipped with an accelerometer (G), which measures changes in the patient's anteroposterior acceleration: a rapid response may thus be obtained at the start of exertion and the end of exertion can be detected immediately.

The rate response is activated through the pacing mode and can be programmed as follow:

- Automatic rate response ("RR Auto" option). The pacing rate is constantly adapted to the patient's physical activity.
- Manual rate response ("RR Fixed" option). In that case, manual programming of the patient's physical activity determines the pacing rate applied, based on the sensor signal.

For the DR model only, rate response is inactive during fallback mode switching (DDD/DDIR mode) if the patient is in sinus rhythm. It becomes active during atrial arrhythmia.



WARNING: Use the Rate Response function with caution in cases of:

1. Severe coronary insufficiency.
 2. Severe aortic stenosis.
 3. Myocardial function compromised by undue accelerations of the pacing rate.
-

Programming at implant:

"Learn" and "RR Auto" should not be programmed prior to implant so as not to distort autocalibration.

Surgical procedure:

For safety reasons, it is preferable to deprogram the Rate Response function before any surgical procedure on the defibrillator patient.

Programming requirement:

For the DR model only, the DDD/DDIR mode (rate response during fallback mode switching) is accessible only if fallback mode switching is programmed.



NOTE: To protect the patient from inadequate prolonged pacing at high rates, if the patient is paced at Max Rate for a large number of cycles, rate responsive pacing automatically and gradually returns to Basic Rate as long as the rest conditions are not met.

16.8. LEAD PARAMETERS EVALUATION (LPE)

The Lead Parameters Evaluation (LPE) is a multi-settings algorithm that aims to assess the integrity of the Right Ventricular defibrillation lead. This algorithm evaluates several settings according to different timescales. Those settings are chosen to be indicative of a lead issue (lead dislodgment, insulation breach, etc.). The different timescales are chosen to reflect the potential lead issue through different manner.

Each day, LPE analyzes the following settings:

- Electrical Settings:
 - RV Impedance
 - Coil Continuity
 - RV Pacing threshold
 - RV Sensing amplitude
- Rhythmic Settings:
 - Number of not treated VF
 - Number of short ventricular intervals (i.e. short cycle $\leq$ 180 ms)

LPE analyzes these settings according to the following timescales:

- Short-term: Comparison of a daily value versus a limit
- Mid-term (applicable only for electric settings): Variation between the daily value and the average value of the previous week

Then, each day, LPE can thus raise an alert during the night following the event occurrence based on the following triggers:

1. 1 abnormal electrical setting for 3 days in a row,
2. 2 abnormal settings in a 7 days window (1 of the setting shall necessarily be an electrical one).

The alert is labelled as a critical red alert and as such a 7 day-inhibition period is applied to avoid this recurrent alert to be sent every day. After 7 days without an in-clinic follow-up, if the device still detects the alert, the alert will be sent for the second time. The alert can only be sent two times maximum between two in-clinic follow-ups.

16.9. ELECTROPHYSIOLOGICAL STUDY (EPS)

EPS V function enables the physician to perform VF induction, VT induction and to deliver ventricular manual ATP and ventricular manual shocks.

Physician can stop the test at any time.

16.10. FOLLOW-UP FUNCTION

Storage of memory data:

AIDA (Automatic Interpretation for Diagnosis Assistance) software provides access up to 6 months of patient follow-up with day by day data collection.

EGM and Markers are recorded on:

- Ventricular tachyarrhythmia episodes on RV and one programmable EGM channel (by default: A in DR model, RVcoil - CAN in VR model)
- Atrial tachyarrhythmia episodes on A and RV EGM channels (for DR model only)
- Switch from AAI to DDD (SafeR mode) episodes on A and RV EGM channels (for DR model only)
- High RA (for DR model only) or RV threshold episodes on A (for DR model only), RV and RVcoil - CAN EGM channels

Diagnosis and Display:

Graphic display of:

- A (for DR model only) and RV sensing,
- A (for DR model only) and RV leads impedance,
- RV and SVC coils continuity,
- A (for DR model only) and RV threshold,
- battery voltage

over time.

On DR model only, automatic diagnosis of AV conduction with graphic displays.

Alerts / Warnings:

The device routinely performs security self-checks and technical measurements to ensure system integrity. When system integrity is found to be at risk outside a follow-up, alerts are stored in the device memory. When system integrity is found to be at risk during a follow-up, the information is managed by a warning (pop-up message) to immediately notify the user. For example, the following types of events can trigger a warning or an alert: technical problem during a shock, lead impedance or shock continuity measurements out-of-range, battery depletion, etc.

16.11. REMOTE MONITORING FUNCTION

Remote monitoring enables the automatic remote transmission of implant data to the physician thanks to the wireless Bluetooth Low Energy communication ability of the implant in order to provide a comprehensive report to the physician about device functioning and patient cardiac status without having the patient physically in the clinic.

The data is transmitted from the implant to the SMARTVIEW CONNECT monitor, a small transmitter placed in the patient's home.

Implant data are first transmitted to the SMARTVIEW CONNECT monitor via Bluetooth Low Energy. Data are then routed through the mobile network to a protected remote server. This server is responsible for transforming the implant data into a comprehensive report that can be consulted by the physician on a dedicated website. The server also sends notifications to the physician via SMS, email or fax when a new transmission report is available.

16.11.1. SMARTVIEW CONNECT Monitor

The SMARTVIEW CONNECT monitor is a small device equipped with an Bluetooth Low Energy transmission module to communicate with the implant and a modem to export data through the internet.

The SMARTVIEW CONNECT monitor is delivered to the patient who has to install it at home. Preferably the SMARTVIEW CONNECT monitor will be placed on the nightstand of the patient, as close as possible to the side of the bed where the patient usually sleeps. The SMARTVIEW CONNECT monitor needs to be connected to the power plug. The scheduled transmissions, as well as alert transmissions (see below) are done during the night when the patient is asleep next to the SMARTVIEW CONNECT monitor without any intervention from the patient.

16.11.2. Transmission trigger

There are 3 different triggers for a remote transmission:

- the **remote follow-up transmission** is scheduled by the physician to occur regularly (according to the programming).
- the **alert transmission** will take place when the implant has recorded an abnormal events. The list of abnormal event is available in a following paragraph. Alert conditions are checked daily.
- the **on-demand follow-up transmission** is triggered by the patient himself through the use of a specific button on the SMARTVIEW CONNECT monitor.

16.11.3. Data transmitted

The data transmitted are identical to the data available during a standard interrogation with the dedicated programmer. All counters, histograms, IEGMs and diagnosis available in the device are transmitted containing (not an exhaustive list):

- programmed parameters
- information on patient and system implanted
- battery status
- lead status (brady leads and defibrillation coils)
- pacing counters and mean heart rate (brady)
- atrial and ventricular arrhythmia counters and episodes
- ventricular arrhythmia counters and episodes
- ventricular therapy counters

Data are presented in the form of 2 reports to the physician: the first one contains a summary of major counters, histograms, warnings and diagnosis. The second one presents the most important IEGM episodes automatically selected based on the degree of severity for the patient.

16.11.4. User website

On the website, the physician is able to:

- consult and schedule the remote follow-ups of their patient
- configure additional ways of being notified of alerts (for instance by SMS, fax or e-mail)
- consult, print and export patient reports

16.11.5. Alert system

The following set of alert triggers can be independently programmed ON/OFF by the physician using the dedicated programmer and can trigger an alert transmission:

- Low or high lead impedance (A, V)
- High threshold (A,RV)
- Abnormal coil impedance (shock lead)
- Low or high shock impedance
- Inefficient high energy shock
- RV Lead Parameters Evaluation (LPE)
- All shocks programmed OFF
- Shock treated VT/VF
- ATP treated VT/VF
- Suspicion of noise on the V lead
- AF occurrence (for DR model only)
- Fast V rate during AF (for DR model only)
- MRI notifications

The following set of alert triggers (system alerts) cannot be deactivated when the Remote monitoring is programmed “On” and can trigger an alert transmission:

- Battery depletion – RRT
- Device reset
- Excessive charge time (>25s)
- System integrity



WARNING: The use of remote monitoring does not replace regular follow-up. Therefore, when using remote monitoring, the time period between follow-ups visits may not be extended.

The device uses BLE technology with authenticated pairing with the SMARTVIEW CONNECT monitor, and data encryption for secure communication.

An excessive BLE usage is an indicator for a possible cyberattack. In this case, the BLE communication may be automatically forced to off. In such event, a warning will appear on the programmer during a follow-up visit to acknowledge the physician.

17. PATIENT FOLLOW-UP

17.1. FOLLOW-UP RECOMMENDATIONS

Before the patient is discharged and at each subsequent follow-up visit, it is advisable to:

- check the occurrence of system warnings
- check the battery status,



NOTES:

If the last reforming, charge or shock occurred during the week preceding the interrogation, the last battery value may be still impacted by the event. One week post event, the battery will recover its steady state value.

Automatic capacitor charging may affect communication between the device and the programmer.

Exiting the programming session before the patient leaves reduces battery consumption and maximizes cybersecurity protection.

- check the integrity of the pacing and defibrillation leads,
- check for proper sensing (sensitivity, crosstalk) and pacing ; set the pacing amplitude to twice the pacing threshold,
- interrogate the implant memories (AIDA),
- check the efficacy of the therapies delivered,
- keep a printout of programmed parameters, test results, and memory data,
- reset the memory data and statistics,

These operations should be performed by medical personnel in an appropriate care unit, with resuscitation equipment present.

It is recommended that a routine follow-up examination be done one month after discharge, and then every three months until the device nears the replacement date.

Refer to the online help for a description of displayed warnings, and the necessity to contact MicroPort for an evaluation.

Implant software update:

The implant provides a secured software update.

In case a new implant software is downloaded in the device memory through the programmer, a warning message could be displayed by the programmer to inform the user and give the correct instructions to follow.



CAUTION: If any issue during Implant Software download, you should contact your MicroPort representative for examination.

17.2. HOLTER FUNCTION

The Holter records markers and EGM on RV and on 1 programmable channel: A (for DR model only), RV coil – CAN, SVC coil – CAN, RV coil - SVC coil, RA ring – CAN (for DR model only), RV tip – CAN, RV ring – CAN:

- Up to 10 episodes and 5 min EGM on significant events: AV block switch (for DR model only), high pacing threshold.
- Up to 16 tachyarrhythmia episodes as well as the therapy history.

Stored Tachyarrhythmia Episodes:

ENERGYA DR / ENERGYA VR store up to 16 episodes (VF, VT, Slow VT, SVT/ST, non-sustained) with a total of 25.6 min of high resolution EGM.

For each episode four levels of details are presented:

- Tachogram (to visualize RR, PP, PR and RP intervals)
- Event log for the entire episode:
 - For DR model: PARAD/PARAD+ analysis for each majority,
 - For VR model: Arrhythmia Discrimination analysis for each majority,
 - Delivered therapies,
- Markers: Atrial and ventricular markers, sensed, paced and in relative refractory periods (atrial markers are only available in DR model),
- EGM: onset and detection of the arrhythmia, on two therapies, and the return to slow rhythm by recording electrogram.

Therapy history

For each arrhythmia detection, each therapy delivered (either automatically or during an electrophysiological study) and at the end of each arrhythmia, ENERGYA DR / ENERGYA VR record the type of majority rhythm, the number of ATP sequences delivered, the energy and the number of shocks delivered.

17.3. RECOMMENDED REPLACEMENT TIME (RRT)

Recommended Replacement Time (RRT)⁽¹⁾ is controlled by: battery voltage equal to $2.62\text{ V} \pm 0.01\text{ V}$



CAUTION: The defibrillator should be replaced as soon as the Recommended Replacement Time (RRT) point is reached.

Between the RRT and the EOS (End of Service)⁽²⁾, the device can still function more than 3 months under the following conditions:

- 100% atrial and biventricular pacing in DDD mode, 500 ohms, with as-shipped settings, 42J shock delivery per month or
- No pacing, sensors OFF and 42J shock delivery every 2 weeks.

For both ENERGY VR and DR, once the Recommended Replacement Time (RRT) point has been reached, the device operates normally, except that the charge time increases. Under normal conditions (and without programmer use) the charge times are as follows:

	Shock energy (J)	Charge time (sec)
BOS ⁽³⁾	42	10 ($\pm$ 3)
RRT ⁽¹⁾	42	15 ($\pm$ 3)
EOS ⁽²⁾	42	20 ($\pm$ 5)

⁽¹⁾Recommended Replacement Time (RRT) corresponds to Elective Replacement Indicators (ERI) previously used.

⁽²⁾End of Service (EOS) corresponds to End of Life (EOL) previously used.

⁽³⁾Beginning of Service (BOS) corresponds to Beginning of Life (BOL) previously used.

17.4. EXPLANTATION

The defibrillator should be explanted in the following cases:

- The Recommended Replacement Time (RRT) point is reached
- Confirmed malfunction
- Burial of the patient (for environmental reasons, the local regulation may require the explantation of the devices containing a battery supply)
- Cremation of the patient (the defibrillator may explode if placed in an incinerator)

The explanted defibrillator should not be reused in another patient.

All explanted defibrillators must be disposed of as medical waste according to applicable local regulations and should be returned to MicroPort, carefully cleaned of all traces of contamination. Cleaning may be done by immersing them in an aqueous sodium hypochlorite containing at least 1% chlorine, followed by rinsing copiously with water. In case of return, please contact your local MicroPort representative.

The defibrillator should be protected against mechanical impact and the temperature variations that may occur during shipping.


Before explantation, it is advisable to:

- Print out all programmed parameters, statistics and Holter function report,
- Save Patient data on floppy disk or hard disk,
- Disable shock therapies (VT and VF) to avoid any risk of untimely shock.

17.5. DEFIBRILLATOR IDENTIFICATION


The defibrillator can be interrogated and programmed via telemetry, using the programming head interfaced with the MicroPort dedicated programmer.

Position the programming head over the telemetry antenna located in the upper part of the device, in order to communicate effectively via telemetry (see diagram below).



The device can be non-invasively identified as follows:

1. Take an x-ray to identify the name of the manufacturer and defibrillators range (X-ray ID is SEA for MicroPort ICD and CRT-D).



2. Interrogate the device using the MicroPort dedicated programmer. The model and serial number of the device are automatically displayed. The first figure in the serial number corresponds to the last figure in the year of manufacture.

18. PHYSICAL CHARACTERISTICS

3440 MODEL:

Dimensions	72.3 x 54.3 x 11.1 mm
Weight	86 g
Volume	33 cm ³
Active surface area of casing	62.8cm ²
Connector	Atrium: IS-1 bipolar. Ventricle: DF4.

3140 MODEL:


Dimensions	65.8 x 54.3 x 11.1 mm
Weight	84 g
Volume	31.2 cm ³
Active surface area of casing	62.9cm ²
Connector	Ventricle: DF4.

18.1. MATERIALS USED

Active surface area of casing	99% pure titanium
Connectors	Polyurethane* and silicone elastomer*

*Medical-grade materials that have undergone "in vitro" and "in vivo" qualifications.

19. ELECTRICAL CHARACTERISTICS

Atrial input impedance (for DR model only)	80 kilohms $\pm$ 40 %
Ventricular input impedance	80 kilohms $\pm$ 30 %
D.C. capacitance	149 μ F $\pm$ 8 %
Capacitor reformation	No reformation required
Rate limit	192 ppm $\pm$ 10 ppm
Pacing waveform	
Defibrillation waveform	

19.1. TABLE OF DELIVERED SHOCK ENERGY AND VOLTAGE

The relationship between stored energies, maximum voltages and delivered energies (at 37°C, 50 ohm load) for the minimum, low, mean and maximum programmed energy values is as follows:

Stored energy (J)	0.5	10	20	34	42
V1 (Volt)	71	332	471	617	686
V2 (Volt)	35	167	235	309	342
Delivered E: Phase 1 (J)	0.32	6.94	14.0	23.8	29.6
Delivered E: Phase 2 (J)	0.08	1.75	3.4	6.0	7.4
Delivered E: Total (J)	0.4	8.7	17.4	30	37

Tolerances are 12% for voltage (25% at 0.5 J) and 30% for energy.

19.2. BATTERY

Manufacturer	Greatbatch
Type	Quasar High Rate (QHR)
Model	GB 3070
Number of batteries	1
Total capacity	2192 mAh
Usable capacity	Between BOS and RRT: 1530 mAh. Between BOS and EOS: 1910 mAh.
Voltage	BOS: 3.24 V. RRT: 2.62 V. EOS: 2.5 V.

19.3. LONGEVITY

For the DR model:

The longevitys are calculated by taking into account 6 months storage with the following conditions:

- Basic rate: 60 ppm
- EGM: ON
- 2 battery reformings per year (at 34J), replaced by shocks if any
- Remote monitoring: ON, daily check, 4 follow-ups and 5 full alert reports per year
- RF telemetry: ON, 45min at implantation + 15min at discharge + 15min for in-clinic quarterly follow-ups

Longevity projection at 500 Ω pacing impedance:

Mode	DDD	DDD	DDD	DDD	DDD	SafeR	-
A pacing (%)	100	100	15	15	15	30	0
V pacing (%)	100	100	1	15	1	6	0
Pacing amplitude (V)	3.5	3.5	3.5	4.5	2.5	2.5	-
Pulse width (ms)	0.35	0.35	0.35	0.50	0.35	0.35	-
Sensor	OFF	ON	OFF	OFF	OFF	OFF	OFF
Max shocks (42J) per year	4	4	4	4	0	4	4
Longevity (years)	8.8	8.6	13.6	12.0	17.8	13.5	14.3


Longevity projection at 600 Ω pacing impedance:

Mode	DDD	DDD	DDD	DDD	DDD	SafeR	-
A pacing (%)	100	100	15	15	15	30	0
V pacing (%)	100	100	1	15	1	6	0
Pacing amplitude (V)	3.5	3.5	3.5	4.5	2.5	2.5	-
Pulse width (ms)	0.35	0.35	0.35	0.50	0.35	0.35	-
Sensor	OFF	ON	OFF	OFF	OFF	OFF	OFF
Max shocks (42J) per year	4	4	4	4	0	4	4
Longevity (years)	9.3	9.1	13.7	12.3	17.9	13.6	14.3


Longevity projection at 700 Ω pacing impedance:

Mode	DDD	DDD	DDD	DDD	DDD	SafeR	-
A pacing (%)	100	100	15	15	15	30	0
V pacing (%)	100	100	1	15	1	6	0
Pacing amplitude (V)	3.5	3.5	3.5	4.5	2.5	2.5	-
Pulse width (ms)	0.35	0.35	0.35	0.35	0.35	0.35	-
Sensor	OFF	ON	OFF	OFF	OFF	OFF	OFF
Max shocks (42J) per year	4	4	4	4	0	4	4
Longevity (years)	9.8	9.5	13.8	12.5	18.0	13.7	14.3

The mean longevity as a function of shocks delivered at maximum energy, with and without pacing, is as follows:

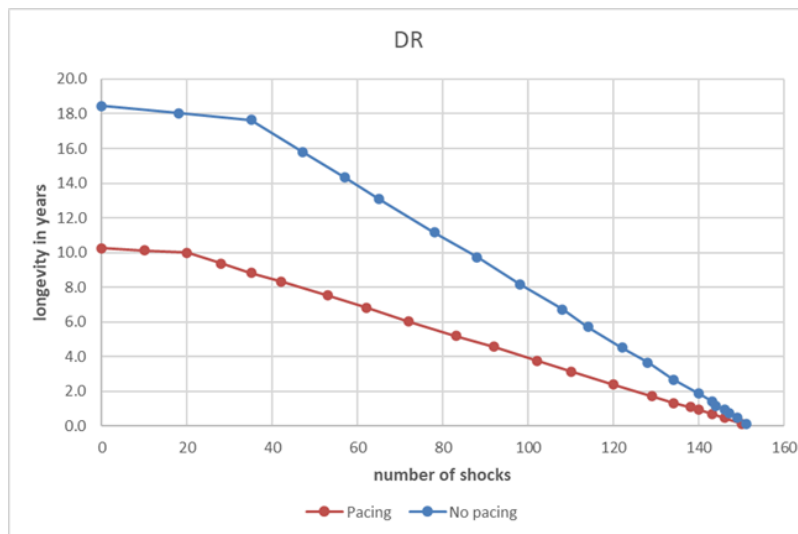

The mean longevity as a function of yearly remote follow-ups⁽¹⁾, with and without pacing, is as follows:

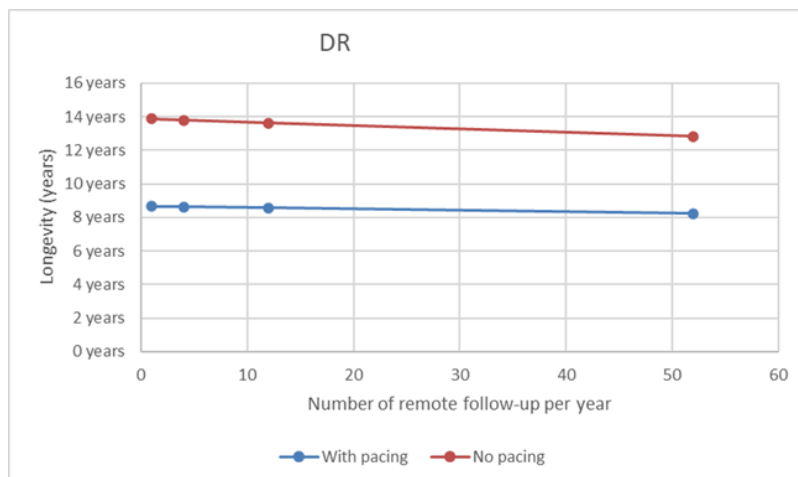

⁽¹⁾An excessive number of remote follow-ups can have a non-negligible impact on device longevity.

1h of additional RF programming session reduces the device longevity from 3 to 10 days depending on the device functioning mode (no pacing, 100% pacing, number of shocks per year, sensors, ...).

For VR model:

The longevity are calculated by taking into account 6 months storage with the following conditions:

- Mode: VVI
- EGM: ON
- 2 battery reformings per year (at 34J), replaced by shocks if any
- Remote monitoring: ON, daily check, 4 follow-ups and 5 full alert reports per year
- RF telemetry: ON, 45min at implantation + 15min at discharge + 15min for in-clinic quarterly follow-ups

Longevity projection at 500 Ω pacing impedance:

Basic Rate (ppm)	60	60	60	60	60	40	60
V pacing (%)	100	100	1	15	15	6	0
Pacing amplitude (V)	3.5	3.5	3.5	4.5	2.5	2.5	-
Pulse width (ms)	0.35	0.35	0.35	0.50	0.35	0.35	-
Sensor	OFF	ON	OFF	OFF	OFF	OFF	OFF
Max shocks (42J) per year	4	4	4	4	0	4	4
Longevity (years)	11.2	10.8	14.7	13.4	18.5	14.6	14.7


Longevity projection at 600 Ω pacing impedance:

Basic Rate (ppm)	60	60	60	60	60	40	60
V pacing (%)	100	100	1	15	15	6	0
Pacing amplitude (V)	3.5	3.5	3.5	4.5	2.5	2.5	-
Pulse width (ms)	0.35	0.35	0.35	0.50	0.35	0.35	-
Sensor	OFF	ON	OFF	OFF	OFF	OFF	OFF
Max shocks (42J) per year	4	4	4	4	0	4	4
Longevity (years)	11.6	11.2	14.7	13.5	18.6	14.6	14.7


Longevity projection at 700 Ω pacing impedance:

Basic Rate (ppm)	60	60	60	60	60	40	60
V pacing (%)	100	100	1	15	15	6	0
Pacing amplitude (V)	3.5	3.5	3.5	4.5	2.5	2.5	-
Pulse width (ms)	0.35	0.35	0.35	0.50	0.35	0.35	-
Sensor	OFF	ON	OFF	OFF	OFF	OFF	OFF
Max shocks (42J) per year	4	4	4	4	0	4	4
Longevity (years)	11.9	11.5	14.7	13.7	18.6	14.6	14.7

The mean longevity as a function of shocks delivered at maximum energy, with and without pacing, is as follows:

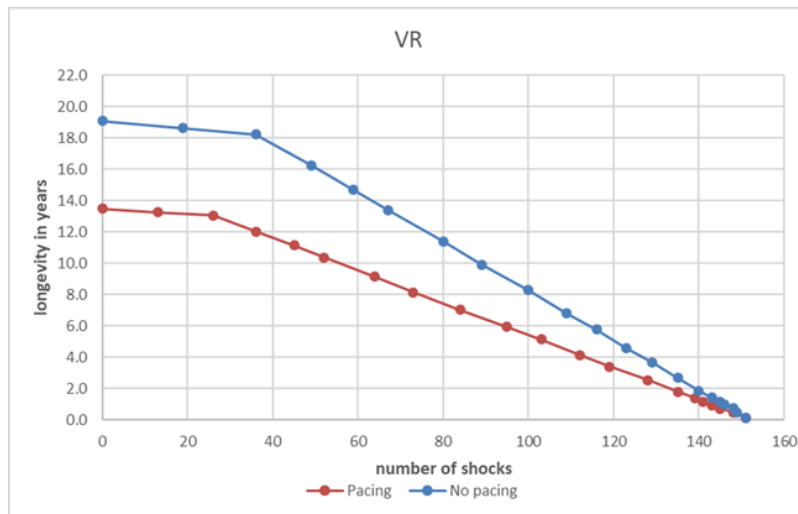

The mean longevity as a function of yearly remote follow-ups⁽¹⁾, with and without pacing, is as follows:

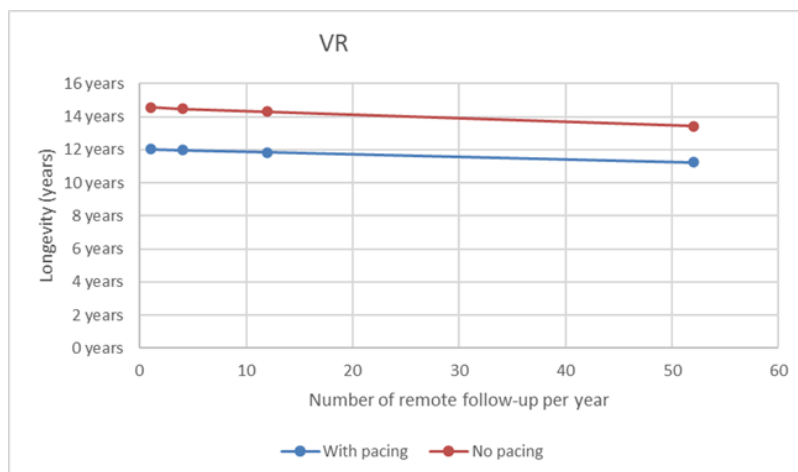

⁽¹⁾An excessive number of remote follow-ups can have a non-negligible impact on device longevity.

1h of additional RF programming session reduces the device longevity from 3 to 10 days depending on the device functioning mode (no pacing, 100% pacing, number of shocks per year, sensors, ...).

19.4. RADIO EQUIPMENT EMISSION

Radio Equipment	Transmitter Frequency Bands Maximal Power	Receiver Frequency Bands
Bluetooth Low Energy™ ® RF telemetry (ISM Band)	Bluetooth Low Energy 4.2 2400-2483.5 MHz -21.6 dBm max implanted	Bluetooth Low Energy 4.2 2400-2483.5 MHz

Radio Equipment	Transmitter Frequency Bands Maximal Power	Receiver Frequency Bands
Inductive Telemetry	Slow mode: 8kHz, Fast mode: 16kHz Simulated Worst Case (16kHz) in continuous communication, -7.4 dBμA max at 10m	Slow mode: Frequency ~30kHz modulation pulsed, Fast mode: Frequency ~70 kHz modulation pulsed.

19.5. CONFORMITY TO STANDARDS FOR SAFETY AND ELECTROMAGNETIC COMPATIBILITY

ENERGYA DR / ENERGYA VR defibrillators conform to the following standards for active implantable medical devices for safety and electromagnetic compatibility:

- ISO 14117
- EN 45502-1
- EN 45502-2-2
- ISO 14708-1
- ISO 14708-6

20. PROGRAMMABLE PARAMETERS

Measured at 37 °C under a 500 ohm load.



NOTE: The Nominal values are programmed in case of Safety mode or proposed as default values in case of reprogramming after a Safety Mode.

20.1. ANTIBRADYCARDIA PACING

Basic parameters	Models	Values	Nominal value	"As shipped" value
Mode	DR	VVI-VVIR-DDD-DDDR-DDD/DDIR-DDI-DDIR-SafeR (AAI <=> DDD)-SafeR-R (AAIR <=> DDDR)-DOO-VOO-OOO	VVI	SafeR (AAI <=> DDD)
Mode	VR	VVI-VVIR-VOO-OOO	VVI	VVI
Basic rate (ppm) ⁽¹⁾	DR	From 30 to 90 by steps of 5 (± 4 %)	60	60
Basic rate (ppm) ⁽¹⁾	VR	From 30 to 90 by steps of 5 (± 4 %)	60	40
Maximum rate (ppm)	DR, VR	From 100 to 145 by steps of 5 (± 6 %)	120	120
Rate hysteresis (%)	DR, VR	0-5-10-20-35 (± 18 ms)	0	0
Rest AV delay (ms)	DR	30-40-45-55-65-70-80-85-95-100-110-115-125-135-140-150-155-165-170-180-190-195-205-210-220-225-235-250 (± 19 ms)	155	155
Exercise AV delay (ms)	DR	30-40-45-55-65-70-80-85-95-100-110-115-125-135-140-150-155-165-170-180-190-195-205-210-220-225-235-250 (± 19 ms)	80	80
AVD Paced/Sensed Offset (ms)	DR	0-10-15-25-30-40-45-55-65-70-80-85-95-100-110-115-125 (± 1 ms)	65	65

(1) The corresponding periods are (in ms):
2000-1714-1500-1333-1200-1091-1000-923-857-800-750-706-667 ms.

Special features	Models	Values	Nominal value	"As shipped" value
Rate smoothing	DR, VR	OFF-Very Slow-Slow-Medium-Fast	OFF	OFF
Mode Switch	DR	ON-OFF	ON	ON
Mode Switch Rate (ppm)	DR	From 30 to 90 by steps of 5	60	60
Anti-PMT protection	DR	Termin-Reprog	Reprog	Reprog

Pacing/Sensing	Models	Values	Nominal value	"As shipped" value
Atrial sensitivity (mV) ⁽¹⁾	DR	From 0.2 to 4 by steps of 0.2 (± 50 %)	0.4	0.4
Atrial amplitude (V) ⁽²⁾	DR	1-1.5-2-2.5-3-3.5-4-4.5-5-6 (± 20 %)	5	3.5
Atrial pulse width (ms)	DR	0.12-0.25-0.35-0.5-0.6-0.75-0.85 -1 (± 10 %)	0.35	0.35
Ventricular sensitivity (mV) ⁽¹⁾	DR, VR	From 0.4 to 4 by steps of 0.2 (± 50 %)	0.4	0.4
Ventricular amplitude (V) ⁽²⁾	DR, VR	1-1.5-2-2.5-3-3.5-4-4.5-5-6 (± 20 %)	5	3.5
Ventricular pulse width (ms)	DR, VR	0.12-0.25-0.35-0.5-0.6-0.75-0.85 -1 (± 10 %)	0.35	0.35

(1) Values are measured using a positive and negative triangular signal of 2/13 ms.

(2) The correlation between the programmed amplitudes, the stored amplitudes and the mid-pulse delivered amplitudes under a 500 ohm load are given in the following table:

Programmed amplitude (V)	Stored amplitude (V)	Mid-pulse delivered amplitude (V)	Programmed amplitude (V)	Stored amplitude (V)	Mid-pulse delivered amplitude (V)
1	1.11	0.94	3.5	3.65	3.09
1.5	1.63	1.38	4	4.2	3.55
2	2.1	1.78	4.5	4.69	3.97
2.5	2.6	2.2	5	5.25	4.44
3	3.15	2.67	6	6.3	5.33

Ventricular arrhythmia algorithms	Models	Values	Nominal value	"As shipped" value
PVC pause suppression	DR	Yes-No	No	No

Atrial arrhythmia algorithms	Models	Values	Nominal value	"As shipped" value
Overdrive	DR	Yes-No	No	No
Maximum Overdrive rate (ppm)	DR	80-90-100-110-130	100	100

Rate responsive parameters	Models	Values	Nominal value	"As shipped" value
Sensor choice	DR, VR	G	G	G
Rate response mode	DR, VR	Learn-RR auto-RR fixed-No	No	No
Physical activity	DR, VR	Very low-Low-Medium-High-Very high	Medium	Medium

Post-shock mode	Models	Values	Nominal value	"As shipped" value
Mode	DR	OFF-VVI-DDI-DDD	DDD	DDD
Mode	VR	OFF-VVI	VVI	VVI
Duration	DR, VR	10s-20s-30s-1min-2min-3min-4min-5min	20s	20s
Basic rate (ppm)	DR, VR	From 50 to 90 by steps of 5 ($\pm 4\%$)	80	80
Rest AV delay (ms)	DR	30-40-45-55-65-70-80-85-95-100-110-115-125-135-140-150-155-165-170-180-190-195-205-210-220-225-235-250 (± 19 ms)	155	155
Exercise AV delay (ms)	DR	30-40-45-55-65-70-80-85-95-100-110-115-125-135-140-150-155-165-170-180-190-195-205-210-220-225-235-250 (± 19 ms)	80	80
AVD Paced/Sensed Offset (ms)	DR	0-10-15-25-30-40-45-55-65-70-80-85-95-100-110-115-125 (± 1 ms)	65	65
A amplitude (V)	DR	1-1.5-2-2.5-3-3.5-4-4.5-5-6 ($\pm 20\%$)	6	6
A pulse width (ms)	DR	0.12-0.25-0.35-0.5-0.6-0.75-0.85-1 ($\pm 10\%$)	1	1
V amplitude (V)	DR, VR	1-1.5-2-2.5-3-3.5-4-4.5-5-6 ($\pm 20\%$)	6	6
V pulse width (ms)	DR, VR	0.12-0.25-0.35-0.5-0.6-0.75-0.85-1 ($\pm 10\%$)	1	1

Autothreshold Parameters	Models	Values	Nominal value	"As shipped" value
Right Atrial Autothreshold	DR	Auto-OFF-Monitoring	OFF	OFF
Right Atrial Amplitude Safety Margin	DR	X1.5-X2-X2.5-X3	X2	X2
Right Atrial Minimum Amplitude (V)	DR	1-1.5-2-2.5-3-3.5	1.5	1.5
Right Atrial Safety Amplitude (V)	DR	2-2.5-3-3.5-4-4.5-5	3.5	3.5
Right Atrial Maximum Rate (ppm)	DR	100-110-120	110	110
Right Atrial Autothreshold Start Time	DR	00am-01am-02am-12pm	02am	02am
Right Ventricular Autothreshold	DR, VR	Auto-OFF-Monitoring	OFF	OFF
Right Ventricular Amplitude Safety Margin	DR, VR	X1.5-X2-X2.5-X3	X2	X2
Right Ventricular Minimum Amplitude (V)	DR, VR	1-1.5-2-2.5-3-3.5	2.5	2.5
Right Ventricular Safety Amplitude (V)	DR, VR	2-2.5-3-3.5-4-4.5-5-6	3.5	3.5

Refractory periods	Models	Values	Nominal value	"As shipped" value
Atrial refractory period post ventricular sensing (ms)	DR	45-65-80-95-110-125-140-155 (± 16 ms)	45	45
Atrial refractory period post ventricular pacing (ms)	DR	80-95-110-125-140-155 (± 4 ms)	80	80

Sensitivity margins	Models	Values	Nominal value	"As shipped" value
Atrial post pacing/sensing margin (mV)	DR	From 0 to 1 by steps of 0.2	0.4	0.4
Ventricular post pacing margin (mV)	DR, VR	From 0 to 2 by steps of 0.2	0.8	0.8

Response to noise	Models	Values	Nominal value	"As shipped" value
Automatic sensitivity on noise	DR, VR	ON-OFF	ON	ON
V pacing on noise	DR, VR	ON-OFF	OFF	OFF

SafeR parameters	Models	Values	Nominal value	"As shipped" value
AVB I switch	DR	Rest+Exercise-Exercise	Exercise	Rest+Exercise
Max. pause (s)	DR	2-3-4	2	2
Long PR: max (ms)	DR	From 200 to 500 by steps of 50	450	450
Long PR: min (ms)	DR	From 200 to 500 by steps of 50	250	250

MRI Mode parameters	Models	Values	Nominal value	"As shipped" value
MRI Mode	DR, VR	Auto-Manual-OFF	OFF	OFF
MRI Pacing Mode	DR	DOO-VOO-OOO	DOO	DOO
MRI Pacing Mode	VR	VOO-OOO	VOO	VOO
MRI Pacing Rate (ppm) ⁽¹⁾	DR, VR	50-55-60-65-70-75-80-85-90-95-100-105-110-115-120 (± 2 ppm)	80	80
MRI Monitoring Period (h)	DR, VR	Auto:2h-4h-6h-12h-1 day-2 days-3 days-7 days-10 days Manual:2h-4h-6h-12h-1 day-2 days	1 day	Auto:1 day Manual:12 h

(1) Default pacing rate is 20 ppm over programmed basic rate.

20.2. VENTRICULAR TACHYARRHYTHMIA DETECTION

Therapy zones	Models	Values	Nominal value	"As shipped" value
Slow VT detection zone	DR, VR	Slow VT ON-Slow VT OFF	Slow VT OFF	Slow VT OFF
VT detection zone	DR, VR	VT ON-VT OFF	VT OFF	VT OFF
Fast VT / VF detection zone	DR, VR	Fast VT+VF ON-VF ON	VF ON	VF ON
Slow VT rate (lower limit) (ppm)	DR, VR	From 100 to 200 by steps of 5	190	190
VT rate (lower limit) (ppm)	DR, VR	130-135-140-145-150-155-160-165-170-175-180-185-190-195-200-210-220-230	190	190
VF rate (lower limit) (ppm)	DR, VR	150-155-160-165-170-175-180-185-190-195-200-210-220-230-240	190	190
Fast VT rate (upper limit) (ppm)	DR, VR	155-160-165-170-175-180-185-190-195-200-210-220-230-240-255	190	190
Slow VT persistence (cycles)	DR, VR	4-6-8-12-16-20-30-50-100-200	20	20
VT persistence (cycles)	DR, VR	4-6-8-12-16-20-30-50-100-200	20	20
VF persistence (cycles)	DR, VR	From 4 to 20 by steps of 1	12	12

Detection criteria	Models	Values	Nominal value	"As shipped" value
Slow VT and VT detection criteria	DR	Rate Only-Stability-Stability+-Stability/Acc-Stability+/Acc-PARAD-PARAD+	PARAD	PARAD+
Slow VT and VT detection criteria	VR	Rate Only-Stability-Stability+-Stability/Acc-Stability+/Acc	Stability/Acc	Stability+/Acc
Fast VT detection criteria	DR, VR	Rate+Stability-Rate Only	Rate+Stability	Rate+Stability
Majority: (X/Y), Y (cycles)	DR, VR	8-12-16	8	8
Majority: (X/Y), X (%)	DR, VR	65-70-75-80-90-95-100	75	75
Window of RR stability for Slow VT and VT (ms)	DR, VR	30-45-65-80-95-110-125	65	65
Window of RR stability for fast VT (ms)	DR, VR	30-45-65	30	30
Acceleration (%)	DR	6-13-19-25-31-38-44-50	25	25
Acceleration (%)	VR	6-13-19-25-31-38-44-50	19	19
Long cycle persistence extension (cycles)	DR, VR	From 0 to 16 by steps of 1	10	10
Long cycle gap (ms)	DR, VR	15-30-45-65-80-95-110-125-140-155-170-190-205	170	170
Atrial monitoring	DR	Yes-No	Yes	Yes

20.3. VENTRICULAR TACHYARRHYTHMIA THERAPIES

Common parameters	Models	Values	Nominal value	"As shipped" value
Enable ATP therapy	DR, VR	Yes-No	No	No
Enable shock therapy	DR, VR	Yes-No	Yes	No
Polarity alternation (42J)	DR, VR	Yes-No	Yes	Yes
Atrial coil (SVC) present	DR, VR	Yes-No	(1)	Yes
Shock configuration (+ --> -)	DR, VR	Case to RV-SVC to RV-Case + SVC to RV-RV to Case-RV to SVC-RV to Case + SVC	RV to Case	RV to Case
Autoswitch ATP	DR, VR	Yes-No	Yes	Yes
Active case	DR, VR	Yes-No	(1)	Yes

(1) Value depending on the previous programming

20.3.1. Therapy parameters in slow VT zone

ATP 1 program	Models	Values	Nominal value	"As shipped" value
ATP program	DR, VR	OFF-Burst-Burst+Scan-Ramp-Ramp+Scan	OFF	OFF
Number of sequences	DR, VR	1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	3	3
Cycles in first sequence	DR, VR	1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	8	8
Cycles added per sequence	DR, VR	0-1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	0	0
Coupling interval (%)	DR, VR	50-55-60-65-70-75-80-85-90-95	80	80
Ramp decrement (per cycle) (ms)	DR, VR	0-4-8-12-16-20-30-40-50-60	0	0
Scan decrement (per sequence) (ms)	DR, VR	0-4-8-12-16-20-30-40-50-60	8	8
Time limit (min)	DR, VR	0.5-1-1.5-2-2.5-3-3.5-4	2	2
Minimum cycle length (ms)	DR, VR	95-110-125-140-155-170-190-205-220-235-250-265-280-295-310	220	220

ATP 2 program	Models	Values	Nominal value	"As shipped" value
ATP program	DR, VR	OFF-Burst-Burst+Scan-Ramp-Ramp+Scan	OFF	OFF
Number of sequences	DR, VR	1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	3	3
Cycles in first sequence	DR, VR	1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	6	6
Cycles added per sequence	DR, VR	0-1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	1	1
Coupling interval (%)	DR, VR	50-55-60-65-70-75-80-85-90-95	85	85
Ramp decrement (per cycle) (ms)	DR, VR	0-4-8-12-16-20-30-40-50-60	8	8
Scan decrement (per sequence) (ms)	DR, VR	0-4-8-12-16-20-30-40-50-60	0	0
Time limit (min)	DR, VR	0.5-1-1.5-2-2.5-3-3.5-4	2	2
Minimum cycle length (ms)	DR, VR	95-110-125-140-155-170-190-205-220-235-250-265-280-295-310	220	220

Shock program	Models	Values	Nominal value	"As shipped" value
Shock 1 (J)	DR, VR	OFF-0.5-0.8-1-1.3-1.5-2-2.5-3-3.5-4-5-6-7-8-9-10-12-14-16-18-20-22-24-26-28-30-32-34-42	OFF	OFF
Shock 2 (J)	DR, VR	OFF-0.5-0.8-1-1.3-1.5-2-2.5-3-3.5-4-5-6-7-8-9-10-12-14-16-18-20-22-24-26-28-30-32-34-42	OFF	OFF
Number of Max. Shock (42 J)	DR, VR	OFF-1-2-3-4	OFF	OFF

20.3.2. Therapy parameters in VT zone

ATP 1 program	Models	Values	Nominal value	"As shipped" value
ATP program	DR, VR	OFF-Burst-Burst+Scan-Ramp-Ramp+Scan	Burst+Scan	Burst+Scan
Number of sequences	DR, VR	1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	3	3
Cycles in first sequence	DR, VR	1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	8	8
Cycles added per sequence	DR, VR	0-1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	0	0
Coupling interval (%)	DR, VR	50-55-60-65-70-75-80-85-90-95	80	80
Ramp decrement (per cycle) (ms)	DR, VR	0-4-8-12-16-20-30-40-50-60	0	0
Scan decrement (per sequence) (ms)	DR, VR	0-4-8-12-16-20-30-40-50-60	8	8
Time limit (min)	DR, VR	0.5-1-1.5-2-2.5-3-3.5-4	2	2
Minimum cycle length (ms)	DR, VR	95-110-125-140-155-170-190-205-220-235-250-265-280-295-310	220	220

ATP 2 program	Models	Values	Nominal value	"As shipped" value
ATP program	DR, VR	OFF-Burst-Burst+Scan-Ramp-Ramp+Scan	Ramp	Ramp
Number of sequences	DR, VR	1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	3	3
Cycles in first sequence	DR, VR	1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	6	6
Cycles added per sequence	DR, VR	0-1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	1	1
Coupling interval (%)	DR, VR	50-55-60-65-70-75-80-85-90-95	85	85
Ramp decrement (per cycle) (ms)	DR, VR	0-4-8-12-16-20-30-40-50-60	8	8
Scan decrement (per sequence) (ms)	DR, VR	0-4-8-12-16-20-30-40-50-60	0	0
Time limit (min)	DR, VR	0.5-1-1.5-2-2.5-3-3.5-4	2	2
Minimum cycle length (ms)	DR, VR	95-110-125-140-155-170-190-205-220-235-250-265-280-295-310	220	220

Shock program	Models	Values	Nominal value	"As shipped" value
Shock 1 (J)	DR, VR	OFF-0.5-0.8-1-1.3-1.5-2-2.5-3-3.5-4-5-6-7-8-9-10-12-14-16-18-20-22-24-26-28-30-32-34-42	OFF	OFF
Shock 2 (J)	DR, VR	OFF-0.5-0.8-1-1.3-1.5-2-2.5-3-3.5-4-5-6-7-8-9-10-12-14-16-18-20-22-24-26-28-30-32-34-42	OFF	OFF
Number of Max. Shock (42 J)	DR, VR	OFF-1-2-3-4	4	4

20.3.3. Therapy parameters in fast VT / VF zone

ATP 1 program	Models	Values	Nominal value	"As shipped" value
ATP program	DR, VR	OFF-Burst-Burst+Scan-Ramp-Ramp+Scan	Burst	Burst
Number of sequences	DR, VR	1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	1	1
Cycles in first sequence	DR, VR	1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	8	8
Cycles added per sequence	DR, VR	0-1-2-3-4-5-6-7-8-9-10-11-12-13-14-15	0	0
Coupling interval (%)	DR, VR	50-55-60-65-70-75-80-85-90-95	80	80
Ramp decrement (per cycle) (ms)	DR, VR	0-4-8-12-16-20-30-40-50-60	0	0
Scan decrement (per sequence) (ms)	DR, VR	0-4-8-12-16-20-30-40-50-60	0	0
Time limit (s)	DR, VR	10-20-30-60-90-120	30	30
Minimum cycle length (ms)	DR, VR	95-110-125-140-155-170-190-205-220-235-250-265-280-295-310	205	205

Shock program	Models	Values	Nominal value	"As shipped" value
Shock 1 (J)	DR, VR	OFF-0.5-0.8-1-1.3-1.5-2-2.5-3-3.5-4-5-6-7-8-9-10-12-14-16-18-20-22-24-26-28-30-32-34-42	OFF	OFF
Shock 2 (J)	DR, VR	OFF-0.5-0.8-1-1.3-1.5-2-2.5-3-3.5-4-5-6-7-8-9-10-12-14-16-18-20-22-24-26-28-30-32-34-42	OFF	OFF
Number of Max. Shock (42 J)	DR, VR	1-2-3-4	4	4

20.4. REMOTE ALERTS AND WARNINGS

The device routinely performs security self-checks and technical measurements to ensure system integrity. When system integrity is found to be at risk outside a follow-up, alerts are stored in the device memory. When system integrity is found to be at risk during a follow-up, the information is managed by a warning (pop-up message) to immediately notify the user. For example, the following types of events can trigger a warning or an alert: technical problem during a shock, pacing lead impedance or coil impedance measurements out-of-range, battery depletion, etc. The Remote tab presents an overview of all the alerts managed by the device.

General parameter	Models	Values	Nominal value	"As shipped" value
Remote monitoring ⁽¹⁾	DR, VR	ON-OFF	ON	OFF

(1) Remote monitoring is turned on automatically if Shocks are programmed ON.

When Remote monitoring is programmed "On", the following System Alerts are automatically activated:

- "Battery depletion – RRT"
- "Device reset"
- "Excessive charge time (>25s)"
- "System integrity"

Lead Alerts	Models	Values	Nominal value	"As shipped" value
Abnormal A lead impedance	DR	ON-OFF	ON	ON
Abnormal A lead low limit (Ohm)	DR	200-250-300-350-400-450-500	200	200
Abnormal A lead high limit (Ohm)	DR	1500-1750-2000-2500-3000	3000	3000
Abnormal V lead impedance	DR, VR	ON-OFF	ON	ON
Abnormal V lead low limit (Ohm)	DR, VR	200-250-300-350-400-450-500	200	200
Abnormal V lead high limit (Ohm)	DR, VR	1500-1750-2000-2500-3000	3000	3000
Abnormal RV coil impedance	DR, VR	ON-OFF	ON	ON
Abnormal SVC coil impedance	DR, VR	ON-OFF	ON	ON
Abnormal Shock impedance ⁽¹⁾	DR, VR	ON-OFF	ON	ON
Atrial Autothreshold	DR	ON-OFF	ON	ON
Atrial Autothreshold High Limit (V)	DR	1-1.25-1.5-1.75-2-2.25-2.5-3-3.5-4	2	2
Right Ventricular Autothreshold	DR, VR	ON-OFF	ON	ON
Right Ventricular Autothreshold High Limit (V)	DR, VR	1-1.25-1.5-1.75-2-2.25-2.5-3-3.5-4-4.5-5	2.5	2.5
RV Lead Parameters Evaluation (LPE)	DR, VR	ON-OFF	ON	ON

(1) Normal impedance range [20 Ohm-200 Ohm]

Clinical status	Models	Values	Nominal value	"As shipped" value
V oversensing	DR, VR	ON-OFF	ON	ON
V oversensing limit (nb of episodes)	DR, VR	1-2-3-4-5-6	2	2
AT/AF burden	DR	ON-OFF	ON	ON
AF burden daily limit 1 (h)	DR	6 min-15 min-30 min-1h-3h-6h-12h-24h	6 min	6 min
AF burden daily limit 2 (h)	DR	OFF-15 min-30 min-1h-3h-6h-12h-24h	6h	6h
AF burden daily limit 3 (h)	DR	OFF-30 min-1h-3h-6h-12h-24h	24h	24h
Fast V Rate during AT/AF	DR	ON-OFF	OFF	OFF
Fast V Rate limit (ppm)	DR	80-90-100-110-120	100	100
Fast V Duration limit (h)	DR	0.5-1-3-6-12-24	1	1

Therapy information	Models	Values	Nominal value	"As shipped" value
Shock disabled	DR, VR	ON-OFF	ON	ON
Shocks delivered	DR, VR	OFF-All shocks-Inefficient shock-Inefficient max shock	All shocks	All shocks
ATP delivered	DR, VR	ON-OFF	ON	ON

Other alerts	Models	Values	Nominal value	"As shipped" value
MRI notifications	DR, VR	ON-OFF	ON	ON
Asynchronous mode	DR, VR	ON-OFF	ON	ON

21. NON PROGRAMMABLE PARAMETERS

Interval	Models	Values
Committed period (ms)	DR	95 (± 5 ms)

Atrial refractory periods	Models	Values
Post atrial sensing (ms)	DR	47 (± 16 ms)
Post atrial pacing (ms)	DR	109 (± 4 ms)

Ventricular refractory periods	Models	Values
Post ventricular sensing (ms)	DR, VR	95 (± 16 ms)
Post ventricular pacing (ms)	DR, VR	220 (± 4 ms)
Post atrial pacing (blanking) (ms)	DR	16 (± 3 ms)

Tachycardia criteria	Models	Values
Window of PR association (ms)	DR	63 (± 1 ms)

Therapies	Models	Values
Waveform ⁽¹⁾	DR, VR	Constant tilt (50% - 50%)
Stored energy for the Max. shock (J)	DR, VR	42
Pacing amplitude during ATP therapies	DR, VR	7 V (Actual value at 300 ms: 5.3 V)

- (1) The device has 50% tilt in each phase thus delivers 94% of stored energy. Each phase is limited to 10 ms duration.

Pacing/Sensing	Models	Values
A pacing polarity	DR	Bipolar
A sensing polarity	DR	Bipolar
RV pacing polarity	DR, VR	Bipolar
RV sensing polarity	DR, VR	Bipolar

Autothreshold Parameters	Models	Values
A Max Amplitude (V)	DR	5
RV Max Amplitude (V)	DR, VR	6
RV Max Rate (ppm)	DR, VR	100
RV Start Time	DR, VR	00am-06am-12pm-06pm

22. LIMITED WARRANTY

ENERGYA implantable cardioverter defibrillator is the result of highly advanced research and all components have been selected after exhaustive testing.


The terms of the limited warranty are available upon request from your MicroPort representative.

23. PATENTS




The ENERGYA model described in this manual is covered by the following US patents:

7 065 402, 7 072 716, 7 076 297, 7 113 826, 7 142 924, 7 164 946, 7 251 526, 7 366 566,
7 400 922, 7 953 483, 8 064 992, 8 043 225, 7 792 582, 8 798 748, 7 890 168, 8 195 293,
7 966 068, 8 768 464, 8 874 209, 8 554 313, 8 214 036, 8 233 981, 8 554 319, 7 966 065,
8 253 279, 8 874 210, 8 219 193, 8 391 976, 8 855 764, 8 359 096, 8 494 629, 8 359 091,
8 489 188, 8 712 526, 8 862 230, 8 641 436, 8 718 765, 8 798 771, 8 868 170, 8 678 843 ,
8 694 098, 8 938 286, 8 874 212, 9 014 805, 9 014 806, 9 026 210, 9 084 899, 9 089 284,
9 089 711, 9 186 500, 9 205 267, 9 227 049, 9 247 888, 9 259 581, 9 272 146, 9 272 149, 9
283 393, 9 314 636, 8 805 486, 9 504 835, 9 446 256, 9 498 630, 9 474 456, 9 668 659, 9
668 660, 9 700 727, 9 943 693, 10 016 168, 10 441 797.

83

General symbols	Explanation of symbols	General symbols	Explanation of symbols
	Use by		Temperature limitation
	Date of manufacture		Screwdriver
	Manufacturer		Basic rate
	Catalogue number		Instructions for use on the website
	Serial number	microportmanuals.com	
	Implantable device uncoated		This icon is used to call your attention to a particularly important point.
	Unique device identifier		This icon alerts you to a hazard that may result in equipment damage or personal injury. Carefully read the instructions provided with this icon.
	Double entry package with external single sterile barrier system		
	Federal Communications commission		
	Package content	Defibrillator symbols	Explanation of symbols
	Sterile package content		ICD (CRT-D, RA, RV, LV)
	Open here		ICD (dual chamber, RA, RV)
	Do not use if the package is damaged		ICD (single chamber, RV)
	Do not reuse		CRT-D DF-1 connectors
	Do not resterilize		DR DF-1 connectors
	Sterilised using ethylene oxide		VR DF-1 connectors
			CRT-D DF-1 connectors

24. EXPLANATION OF SYMBOLS

Defibrillator symbols	Explanation of symbols	Defibrillator symbols	Explanation of symbols
	DR DF-1 connectors		High voltage DF-1 connector compatible with DF-1 standard compliant lead
	VR DF-1 connectors		High voltage DF4 connector compatible with DF4-LLHO or DF4-LLHH standard compliant lead
	CRT-D DF4 (IS-1) connectors		Low voltage IS4 connector compatible with IS4-LLLL standard compliant lead
	DR DF4 (IS-1) connectors		Bluetooth
	VR DF4 connector		MR Conditional and Full Body
	CRT-D DF4 (IS4) connectors		MR Conditional
	Shocks		Full Body
	ATP Anti-tachycardia pacing, RV, LV		DF-1 defibrillating connector insulating plug
	ATP Anti-tachycardia pacing, RV		
	High voltage		

Last revision date of this manual: 2024-03



MicroPort CRM S.r.l.
Via Crescentino s.n.
13040 Saluggia (VC)
Italy
Tel: +39 0161 487095
US Phone: 877.663.7674

www.microport.com

FOR US ONLY - CAUTION: FEDERAL LAW RESTRICTS THIS DEVICE TO SALE BY OR ON THE ORDER OF A PHYSICIAN

2024-03
UA15188A

