



Report No.: RZA1011-1731SAR



# OET 65

# TEST REPORT

|                     |  |
|---------------------|--|
| <b>Product Name</b> | USB Wifi Adaptor                                       |
| <b>Model</b>        | 3E,2E;<br>GWF-3E31,3E32,3E33,2E31,2E32,2E33;<br>WU-150 |
| <b>FCC ID</b>       | YWTWF2EXX3EXX  |
| <b>Client</b>       | Shenzhen Ogemray Technology Co.,Ltd                    |

**TA Technology (Shanghai) Co., Ltd.**



## GENERAL SUMMARY

|                              |   |              |   |
|------------------------------|---|--------------|---|
| <b>Product Name</b>          | USB Wifi Adaptor  | <b>Model</b> | 3E,2E;<br>GWF-3E31,3E32,3<br>E33,2E31,2E32,2E<br>33; WU-150 |
| <b>FCC ID</b>                | YWTWF2EXX3EXX   |              |   |
| <b>Report No.</b>            | RZA1011-1731SAR   |              |   |
| <b>Client</b>                | Shenzhen Ogemray Technology Co.,Ltd   |              |   |
| <b>Manufacturer</b>          | Shenzhen Ogemray Technology Co.,Ltd   |              |   |
| <b>Reference Standard(s)</b> | <p><b>IEEE Std C95.1, 1999:</b> IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz.</p> <p><b>SUPPLEMENT C Edition 01-01 to OET BULLETIN 65 Edition 97-01 June 2001 including DA 02-1438, published June 2002:</b> Evaluating Compliance with FCC Guidelines for Human Exposure to Radio frequency Electromagnetic Fields Additional Information for Evaluation Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radio frequency Emissions.</p> <p><b>KDB 248227 D01 SAR meas for 802 11 a b g v01r02:</b> SAR Measurement Procedures for 802.11a/b/g Transmitters.</p> <p><b>KDB 447498 D02 SAR Procedures for Dongle Xmtr v02:</b> SAR Measurement Procedures for USB Dongle Transmitters.</p> |              |   |
| <b>Conclusion</b>            | <p>This portable wireless equipment has been measured in all cases requested by the relevant standards. Test results in Chapter 7 of this test report are below limits specified in the relevant standards.</p> <p>General Judgment: <b>Pass</b></p> <p style="text-align: right;">(Stamp) </p> <p style="text-align: right;"><b>Date of issue: November 8<sup>th</sup> 2010</b></p>   |              |   |
| <b>Comment</b>               | The test result only responds to the measured sample.   |              |   |

Approved by 杨伟中  
Yang Weizhong

Revised by 凌敏宝  
Ling Minbao

Performed by 刘军  
Liu Jun

## TABLE OF CONTENT

|  |    |
|--|----|
| 1. General Information .....   | 5  |
| 1.1. Notes of the Test Report.....   | 5  |
| 1.2. Testing Laboratory .....  | 5  |
| 1.3. Applicant Information .....   | 6  |
| 1.4. Manufacturer Information.....   | 6  |
| 1.5. Information of EUT.....   | 7  |
| 1.6. The Maximum SAR <sub>1g</sub> Values and Power of each tested Mode..... | 8  |
| 1.7. Test Date .....   | 8  |
| 2. Operational Conditions during Test .....                                  | 9  |
| 2.1. General Description of Test Procedures .....                            | 9  |
| 2.2. Position of Module in Portable Devices.....                             | 10 |
| 2.3. Picture of Host Product .....   | 11 |
| 3. SAR Measurements System Configuration .....                               | 13 |
| 3.1. SAR Measurement Set-up .....  | 13 |
| 3.2. DASY4 E-field Probe System .....  | 14 |
| 3.2.1. EX3DV4 Probe Specification .....                                      | 14 |
| 3.2.2. E-field Probe Calibration .....                                       | 15 |
| 3.3. Other Test Equipment .....  | 15 |
| 3.3.1. Device Holder for Transmitters .....                                  | 15 |
| 3.3.2. Phantom .....   | 16 |
| 3.4. Scanning Procedure .....  | 16 |
| 3.5. Data Storage and Evaluation .....                                       | 18 |
| 3.5.1. Data Storage.....   | 18 |
| 3.5.2. Data Evaluation by SEMCAD .....                                       | 18 |
| 3.6. System Check.....   | 21 |
| 3.7. Equivalent Tissues.....   | 22 |
| 4. Laboratory Environment.....   | 22 |
| 5. Characteristics of the Test.....  | 23 |
| 5.1. Applicable Limit Regulations.....                                       | 23 |
| 5.2. Applicable Measurement Standards .....                                  | 23 |
| 6. Conducted Output Power Measurement .....                                  | 24 |
| 6.1. Summary .....   | 24 |
| 6.2. Conducted Power Results .....   | 24 |
| 7. Test Results .....  | 25 |
| 7.1. Dielectric Performance.....   | 25 |
| 7.2. System Check.....   | 25 |
| 7.3. Summary of Measurement Results.....                                     | 26 |
| 7.3.1. 802.11b.....  | 26 |
| 7.3.2. 802.11g/n.....  | 26 |
| 8. Measurement Uncertainty .....   | 27 |
| 9. Main Test Instruments .....   | 28 |

**TA Technology (Shanghai) Co., Ltd.**  
**Test Report**

Report No. RZA1011-1731SAR

Page 4 of 65

---

|   |    |
|---|----|
| ANNEX A: Test Layout .....                                | 29 |
| ANNEX B: System Check Results .....                       | 30 |
| ANNEX C: Graph Results .....                              | 31 |
| ANNEX D: Probe Calibration Certificate .....              | 38 |
| ANNEX E: D2450V2 Dipole Calibration Certificate .....     | 49 |
| ANNEX F: DAE4 Calibration Certificate .....               | 58 |
| ANNEX G: The EUT Appearances and Test Configuration ..... | 63 |

## **1. General Information**

### **1.1. Notes of the Test Report**

**TA Technology (Shanghai) Co., Ltd.** guarantees the reliability of the data presented in this test report, which is the results of measurements and tests performed for the items under test on the date and under the conditions stated in this test report and is based on the knowledge and technical facilities available at TA Technology (Shanghai) Co., Ltd. at the time of execution of the test.

**TA Technology (Shanghai) Co., Ltd.** is liable to the client for the maintenance by its personnel of the confidentiality of all information related to the items under test and the results of the test. This report only refers to the item that has undergone the test.

This report standalone does not constitute or imply by its own an approval of the product by the certification Bodies or competent Authorities. This report cannot be used partially or in full for publicity and/or promotional purposes without previous written approval of **TA Technology (Shanghai) Co., Ltd.** and the Accreditation Bodies, if it applies.

### **1.2. Testing Laboratory**

Company: TA Technology (Shanghai) Co., Ltd.  
Address: No.145, Jintang Rd, Tangzhen Industry Park, Pudong  
City: Shanghai  
Post code: 201201  
Country: P. R. China  
Contact: Yang Weizhong  
Telephone: +86-021-50791141/2/3  
Fax: +86-021-50791141/2/3-8000  
Website: <http://www.ta-shanghai.com>  
E-mail: [yangweizhong@ta-shanghai.com](mailto:yangweizhong@ta-shanghai.com)

**TA Technology (Shanghai) Co., Ltd.**  
**Test Report**

Report No. RZA1011-1731SAR

Page 6 of 65

---

**1.3. Applicant Information**

Company: Shenzhen Ogemray Technology Co.,Ltd  
Address: 3/F,No.9 Bldg.Minxing Industrial Park.Minkang Rd.Minzhi St.Baoan District.Shenzhen  
City: Shenzhen  
Postal Code: /  
Country: China  
Telephone: 0755-29500315  
Fax: 0755-29500309

**1.4. Manufacturer Information**

Company: Shenzhen Ogemray Technology Co.,Ltd  
Address: 3/F,No.9 Bldg.Minxing Industrial Park.Minkang Rd.Minzhi St.Baoan District.Shenzhen  
City: Shenzhen  
Postal Code: /  
Country: China  
Telephone: 0755-29500315  
Fax: 0755-29500309

**TA Technology (Shanghai) Co., Ltd.**  
**Test Report**

Report No. RZA1011-1731SAR

Page 7 of 65

**1.5. Information of EUT**

**General Information**

|  |   |                |
|--|---|----------------|
| Device Type:                           | Portable Device                               |                |
| Exposure Category:                     | Uncontrolled Environment / General Population |                |
| Product Name:                          | USB Wifi Adaptor                              |                |
| IMEI:                                  | /   |                |
| Hardware Version:                      | /   |                |
| Software Version:                      | /   |                |
| Antenna Type:                          | Internal Antenna                              |                |
| Device Operating Configurations:       |   |                |
| Supporting Mode(s):                    | 802.11b/g/n;                                  |                |
| Operating Frequency Range(s):          | Band  | Tx (MHz)       |
|  | 802.11b/g/n                                   | 2412 ~ 2462MHz |
| Test Channel:<br>(Low - Middle - High) | 1-6-11 (802.11b/g/n)                          |                |
| Used Host Products:                    | IBM T61<br>Lenovo Y-450                       |                |

# TA Technology (Shanghai) Co., Ltd.

## Test Report

Report No. RZA1011-1731SAR

Page 8 of 65

Equipment Under Test (EUT) is USB Wifi Adaptor. During SAR test of the EUT, it was connected to a portable computer. SAR is tested for 802.11b in this report. SAR is not required for 802.11g/n channels when the maximum average output power is less than 0.25dB higher than that measured on the corresponding 802.11b channels. The EUT has a WIFI antenna that is used for Tx/Rx. the EUT is not supported the MIMO facition.

The measurements were performed in combination with two host products (IBM T61 and Lenovo Y-450). IBM T61 laptop has horizontal USB slot, Lenovo Y-450 laptop has vertical USB slot.

The sample undergoing test was selected by the Client.

Components list please refer to documents of the manufacturer.

### 1.6. The Maximum SAR<sub>1g</sub> Values and Power of each tested Mode

#### Body Worn Configuration

| Mode    | Channel | Position   | Separation distance | SAR <sub>1g</sub> (W/kg) |
|---------|---------|------------|---------------------|--------------------------|
| 802.11b | 11      | Front Side | 5mm                 | <b>0.401</b>             |

#### Maximum Power

| Mode    | Max Power (dBm) |
|---------|-----------------|
| 802.11b | <b>24.14</b>    |
| 802.11g | <b>19.73</b>    |
| 802.11n | <b>18.67</b>    |

### 1.7. Test Date

The test is performed on November 6, 2010.



## 2. Operational Conditions during Test

### 2.1. General Description of Test Procedures

For the 802.11b/g SAR body tests, a communication link is set up with the test mode software for WIFI mode test. The Absolute Radio Frequency Channel Number (ARFCN) is allocated to 1, 6 and 11 respectively in the case of 2450 MHz. During the test, at the each test frequency channel, the EUT is operated at the RF continuous emission mode. Each channel should be tested at the lowest data rate in each mode.

802.11b/g operating modes are tested independently according to the service requirements in each frequency band. 802.11b/g modes are tested on channels 1,6 and 11; however, if output power reduction is necessary for channels 1 and /or 11 to meet restricted band requirements the highest output channels closest to each of these channels must be tested instead.

SAR is not required for 802.11g channels when the maximum average output power is less than 0.25dB higher than that measured on the corresponding 802.11b channels. When the maximum average output channel in each frequency band is not included in the “default test channels”, the maximum channel should be tested instead of an adjacent “default test channels”, these are referred to as the “required test channels” and are illustrated in table 1.

Then The Absolute Radio Frequency Channel Number (ARFCN) is firstly allocated to 2437 respectively in the case of 802.11b/g.

**Table 1: “Default Test Channels”**

| Mode      | GHz   | Channel         | Turbo Channel | “Default Test Channels” |         |      |  |
|-----------|-------|-----------------|---------------|-------------------------|---------|------|--|
|           |       |                 |               | 15.247                  |         | UNII |  |
|           |       |                 |               | 802.11b                 | 802.11g |      |  |
| 802.11b/g | 2.412 | 1 <sup>#</sup>  |               | √                       | *       |      |  |
|           | 2.437 | 6               | 6             | √                       | *       |      |  |
|           | 2.462 | 11 <sup>#</sup> |               | √                       | *       |      |  |

Note: <sup>#</sup>=when output power is reduced for channel 1 and /or 11to meet restricted band requirements the highest out put channels closet to each of these channels should be tested.

√= “default test channels”

\* =possible 802.11g channels with maximum average output 0.25dB>=the “default test channels”

## **2.2. Position of Module in Portable Devices**

The measurements were performed in combination with two host products (IBM T61 and Lenovo Y-450). IBM T61 laptop has horizontal USB slot, Lenovo Y-450 laptop has vertical USB slot.

A test distance of 5mm or less, according to KDB 447498 D02, should be considered for the orientation that can satisfy such requirements.

For each channel, the EUT is tested at the following 4 test positions:

- Test Position 1: The EUT is connected to the portable computer with horizontal USB slot. The back side of the EUT towards the bottom of the flat phantom. The distance from back side of the EUT to the bottom of the flat phantom is 5mm. (ANNEX G Picture 5)
- Test Position 2: The EUT is connected to the portable computer through a 19 cm USB cable. The front side of the EUT towards the bottom of the flat phantom. The distance from front side of the EUT to the bottom of the flat phantom is 5mm. (ANNEX G Picture 6)
- Test Position 3: The EUT is connected to the portable computer through a 19 cm USB cable. The left side of the EUT towards the bottom of the flat phantom. The distance from left side of the EUT to the bottom of the flat phantom is 5mm. (ANNEX G Picture 7)
- Test Position 4: The EUT is connected to the portable computer with vertical USB slot. The right side of the EUT towards the bottom of the flat phantom. The distance from right side of the EUT to the bottom of the flat phantom is 5mm. (ANNEX G Picture 8)

### 2.3. Picture of Host Product

During the test, IBM T61 and Lenovo Y-450 laptop were used as an assistant to help to setup communication. (See Picture 1)



Picture 1-a: IBM T61 Close



Picture 1-b: IBM T61 Open



Picture 1-c: Lenovo Y-450 Close



Picture 1-d: Lenovo Y-450 Open



Picture 1-e: IBM T61 with horizontal USB slot



Picture 1-f: Lenovo Y-450 with Vertical USB slot



Picture 1-g: a 19 cm USB cable


**Picture 1: Computer as a test assistant**

### 3. SAR Measurements System Configuration

#### 3.1. SAR Measurement Set-up

The DASY4 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Stäubli RX family) with controller and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e. an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronic (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- A unit to operate the optical surface detector which is connected to the EOC.
- The Electro-Optical Coupler (EOC) performs the conversion from the optical into a digital electric signal of the DAE. The EOC is connected to the DASY4 measurement server.
- The DASY4 measurement server, which performs all real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operation. A computer operating Windows 2003
- DASY4 software and SEMCAD data evaluation software.
- Remote control with teach panel and additional circuitry for robot safety such as warning lamps, etc.
- The generic twin phantom enabling the testing of left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- System validation dipoles allowing to validate the proper functioning of the system.

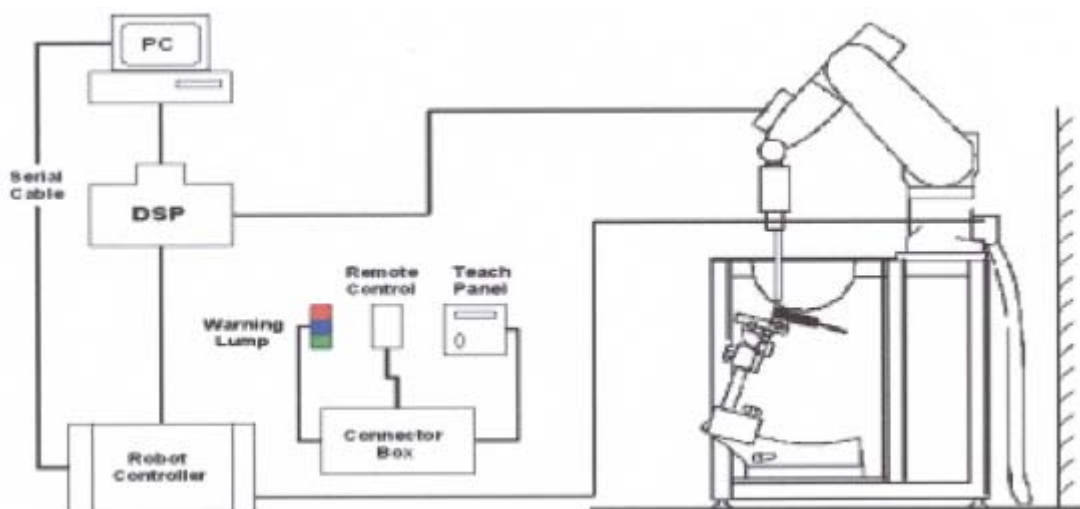

**Figure 1. SAR Lab Test Measurement Set-up**

### 3.2. DASY4 E-field Probe System

The SAR measurements were conducted with the dosimetric probe EX3DV4 (manufactured by SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation.

#### 3.2.1. EX3DV4 Probe Specification

|               |  |
|---------------|--|
| Construction  | Symmetrical design with triangular core<br>Built-in shielding against static charges<br>PEEK enclosure material (resistant to organic solvents, e.g., DGBE)  |
| Calibration   | ISO/IEC 17025 calibration service available  |
| Frequency     | 10 MHz to > 6 GHz<br>Linearity: $\pm 0.2$ dB<br>(30 MHz to 6 GHz)  |
| Directivity   | $\pm 0.3$ dB in HSL (rotation around probe axis)<br>$\pm 0.5$ dB in tissue material (rotation normal to probe axis)  |
| Dynamic Range | 10 $\mu$ W/g to > 100 mW/g Linearity:<br>$\pm 0.2$ dB (noise: typically < 1 $\mu$ W/g)   |
| Dimensions    | Overall length: 330 mm (Tip: 20 mm) Tip diameter: 2.5 mm (Body: 12 mm) Typical distance from probe tip to dipole centers: 1 mm   |
| Application   | High precision dosimetric measurements in any exposure scenario (e.g., very strong gradient fields). Only probe which enables compliance testing for frequencies up to 6 GHz with precision of better 30%. |



Figure 2. EX3DV4 E-field Probe



Figure 3. EX3DV4 E-field probe

### 3.2.2. E-field Probe Calibration

Each probe is calibrated according to a dosimetric assessment procedure with accuracy better than  $\pm 10\%$ . The spherical isotropy was evaluated and found to be better than  $\pm 0.25\text{dB}$ . The sensitivity parameters (NormX, NormY, NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested.

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies below 1 GHz, and in a wave guide above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$\text{SAR} = C \frac{\Delta T}{\Delta t}$$

Where:  $\Delta t$  = Exposure time (30 seconds),  
C = Heat capacity of tissue (brain or muscle),  
 $\Delta T$  = Temperature increase due to RF exposure.  
Or

$$\text{SAR} = \frac{|E|^2 \sigma}{\rho}$$

Where:  
 $\sigma$  = Simulated tissue conductivity,  
 $\rho$  = Tissue density (kg/m<sup>3</sup>).

### 3.3. Other Test Equipment

#### 3.3.1. Device Holder for Transmitters

**Construction:** Simple but effective and easy-to-use extension for Mounting Device that facilitates the testing of larger devices according to IEC 62209-2 (e.g., laptops, cameras, etc.) It is lightweight and fits easily on the upper part of the Mounting Device in place of the phone positioner. The extension is fully compatible with the Twin SAM, ELI4 and SAM v6.0 Phantoms.

**Material:** POM, Acrylic glass, Foam

### 3.3.2. Phantom

The Generic Twin Phantom is constructed of a fiberglass shell integrated in a wooden Figure. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90% of all users. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot.

|                 |                                 |
|-----------------|---------------------------------|
| Shell Thickness | 2±0.1 mm                        |
| Filling Volume  | Approx. 20 liters               |
| Dimensions      | 810 x 1000 x 500 mm (H x L x W) |
| Available       | Special                         |



**Figure 4. Generic Twin Phantom**

### 3.4. Scanning Procedure

The DASY4 installation includes predefined files with recommended procedures for measurements and validation. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.

- The “reference” and “drift” measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT’s output power and should vary max.  $\pm 5\%$ .
- The “surface check” measurement tests the optical surface detection system of the DASY4 system by repeatedly detecting the surface with the optical and mechanical surface detector and comparing the results. The output gives the detecting heights of both systems, the difference between the two systems and the standard deviation of the detection repeatability. Air bubbles or refraction in the liquid due to separation of the sugar-water mixture gives poor repeatability (above  $\pm 0.1\text{mm}$ ). To prevent wrong results tests are only executed when the liquid is free of air bubbles. The difference between the optical surface detection and the actual surface depends on the probe and is specified with each probe. (It does not depend on the surface reflectivity or the probe angle to the surface within  $\pm 30^\circ$ .)
- Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values before running a detailed measurement around the hot spot. Before starting the area scan a grid spacing of 10 mm x 10 mm is set. During the scan the distance of the probe to the phantom remains



unchanged.

After finishing area scan, the field maxima within a range of 2 dB will be ascertained.

- **Zoom Scan**

Zoom Scans are used to estimate the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The default Zoom Scan is done by 7x7x7 points within a cube whose base is centered around the maxima found in the preceding area scan.

- **Spatial Peak Detection**

The procedure for spatial peak SAR evaluation has been implemented and can determine values of masses of 1g and 10g, as well as for user-specific masses. The DASY4 system allows evaluations that combine measured data and robot positions, such as:

- maximum search
- extrapolation
- boundary correction
- peak search for averaged SAR

During a maximum search, global and local maxima searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard's method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation. Extrapolation routines require at least 10 measurement points in 3-D space.

They are used in the Zoom Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the modified Quadratic Shepard's method for extrapolation. For a grid using 7x7x7 measurement points with 5mm resolution amounting to 343 measurement points, the uncertainty of the extrapolation routines is less than 1% for 1g and 10g cubes.

- A Z-axis scan measures the total SAR value at the x-and y-position of the maximum SAR value found during the cube 7x7x7 scan. The probe is moved away in z-direction from the bottom of the SAM phantom in 5mm steps.

### 3.5. Data Storage and Evaluation

#### 3.5.1. Data Storage

The DASY4 software stores the acquired data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension “.DA4”. The software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of incorrect parameter settings. For example, if a measurement has been performed with a wrong crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be re-evaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type ([V/m], [A/m], [°C], [mW/g], [mW/cm<sup>2</sup>], [dBrel], etc.). Some of these units are not available in certain situations or show meaningless results, e.g., a SAR output in a lossless media will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

#### 3.5.2. Data Evaluation by SEMCAD

The SEMCAD software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

|                    |                           |  |
|--------------------|---------------------------|--|
| Probe parameters:  | - Sensitivity             | Normi, a <sub>i0</sub> , a <sub>i1</sub> , a <sub>i2</sub> |
|                    | - Conversion factor       | ConvF <sub>i</sub>   |
|                    | - Diode compression point | Dcp <sub>i</sub>   |
| Device parameters: | - Frequency               | f  |
|                    | - Crest factor            | cf   |
| Media parameters:  | - Conductivity            |  |
|                    | - Density                 |  |

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY4 components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics.

**TA Technology (Shanghai) Co., Ltd.**  
**Test Report**

If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot c f / d c p_i$$

With  $V_i$  = compensated signal of channel i (i = x, y, z)

$U_i$  = input signal of channel i (i = x, y, z)

$cf$  = crest factor of exciting field (DASY parameter)

$dcp_i$  = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes:  $E_i = (V_i / Norm_i \cdot ConvF)^{1/2}$

H-field probes:  $H_i = (V_i)^{1/2} \cdot (a_{i0} + a_{i1} f + a_{i2} f^2) / f$

With  $V_i$  = compensated signal of channel i (i = x, y, z)

$Norm_i$  = sensor sensitivity of channel i (i = x, y, z)  
[mV/(V/m)<sup>2</sup>] for E-field Probes

$ConvF$  = sensitivity enhancement in solution

$a_{ij}$  = sensor sensitivity factors for H-field probes

$f$  = carrier frequency [GHz]

$E_i$  = electric field strength of channel i in V/m

$H_i$  = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = (E_x^2 + E_y^2 + E_z^2)^{1/2}$$

The primary field data are used to calculate the derived field units.

$$SAR = (E_{tot}^2 \cdot \dots) / (\dots \cdot 1000)$$

with  $SAR$  = local specific absorption rate in mW/g

**$E_{tot}$**  = total field strength in V/m

$\sigma$  = conductivity in [mho/m] or [Siemens/m]

$\rho$  = equivalent tissue density in g/cm<sup>3</sup>

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid. The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = E_{tot}^2 / 3770 \quad \text{or} \quad P_{pwe} = H_{tot}^2 \cdot 37.7$$

with  $P_{pwe}$  = equivalent power density of a plane wave in mW/cm<sup>2</sup>

**$E_{tot}$**  = total electric field strength in V/m

**$H_{tot}$**  = total magnetic field strength in A/m

### 3.6. System Check

The manufacturer calibrates the probes annually. Dielectric parameters of the tissue simulants were measured every day using the dielectric probe kit and the network analyzer. A system check measurement was made following the determination of the dielectric parameters of the simulant, using the dipole validation kit. A power level of 250 mW was supplied to the dipole antenna, which was placed under the flat section of the twin SAM phantom. The system check results (dielectric parameters and SAR values) are given in the Table 6.

System check results have to be equal or near the values determined during dipole calibration with the relevant liquids and test system ( $\pm 10\%$ ).

System check is performed regularly on all frequency bands where tests are performed with the DASY4 system.

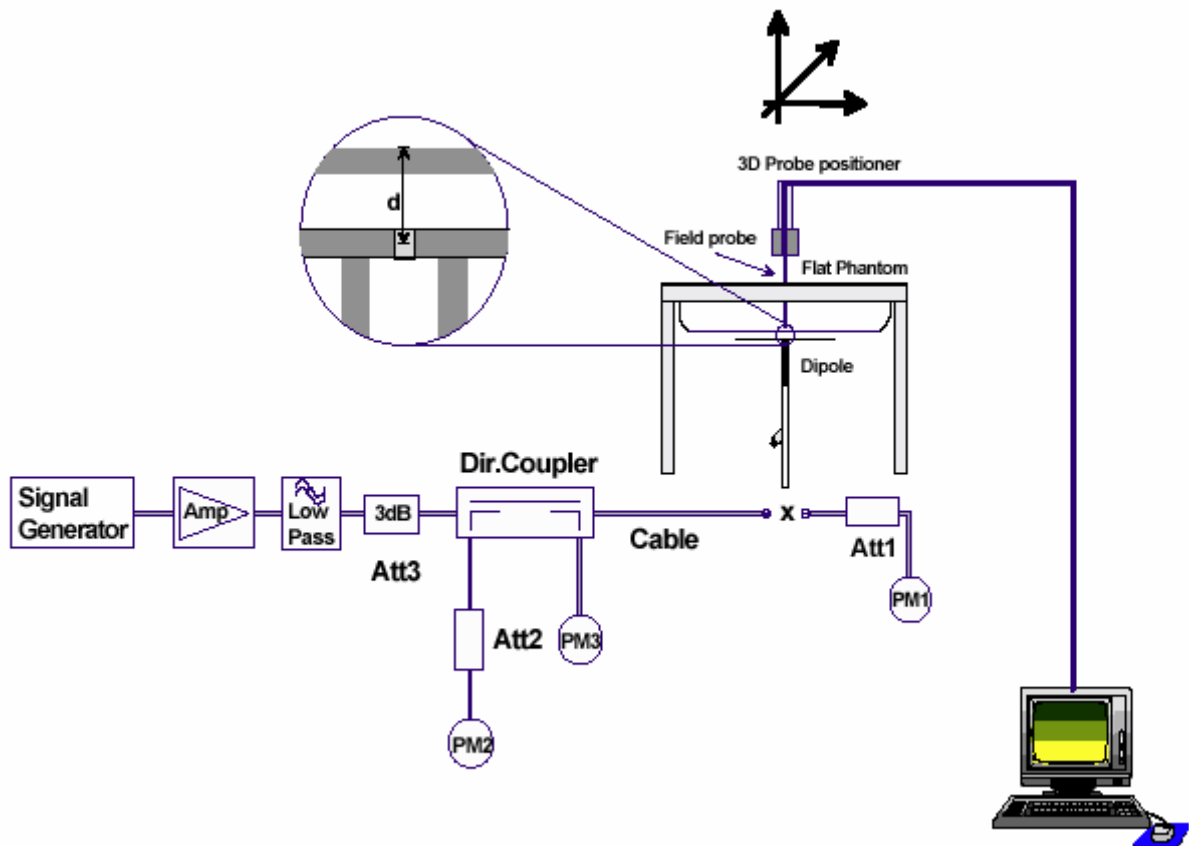


Figure 5. System Check Set-up

### 3.7. Equivalent Tissues

The liquid is consisted of water, sugar, salt, Glycol monobutyl, Preventol and Cellulose. The liquid has previously been proven to be suited for worst-case. The Table 2 shows the detail solution. It's satisfying the latest tissue dielectric parameters requirements proposed by IEC62209-2.

**Table 2: Composition of the Body Tissue Equivalent Matter**

| MIXTURE%                              | FREQUENCY(Body) 2450MHz |                  |               |
|---------------------------------------|-------------------------|------------------|---------------|
| Water                                 | 73.2                    |                  |               |
| Glycol                                | 26.7                    |                  |               |
| Salt                                  | 0.1                     |                  |               |
| Dielectric Parameters<br>Target Value | f=2450MHz               | $\epsilon=52.70$ | $\sigma=1.95$ |

## 4. Laboratory Environment

**Table 3: The Ambient Conditions during Test**

|   |                           |
|---|---------------------------|
| Temperature   | Min. = 20°C, Max. = 25 °C |
| Relative humidity   | Min. = 30%, Max. = 70%    |
| Ground system resistance  | < 0.5 $\Omega$            |
| Ambient noise is checked and found very low and in compliance with requirement of standards.    |                           |
| Reflection of surrounding objects is minimized and in compliance with requirement of standards. |                           |

## **5. Characteristics of the Test**

### **5.1. Applicable Limit Regulations**

**IEEE Std C95.1, 1999:** IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz.

### **5.2. Applicable Measurement Standards**

**SUPPLEMENT C Edition 01-01 to OET BULLETIN 65 Edition 97-01 June 2001 including DA 02-1438, published June 2002:** Evaluating Compliance with FCC Guidelines for Human Exposure to Radio frequency Electromagnetic Fields Additional Information for Evaluation Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radio frequency Emissions.

**KDB 248227 D01 SAR meas for 802 11 a b g v01r02:** SAR Measurement Procedures for 802.11a/b/g Transmitters.

**KDB 447498 D02 SAR Procedures for Dongle Xmtr v02:** SAR Measurement Procedures for USB Dongle Transmitters.

## 6. Conducted Output Power Measurement

### 6.1. Summary

The following procedures had been used to prepare the EUT for the SAR test. The client provided a special driver and program, which enable engineer to control the frequency and output power of the module.

### 6.2. Conducted Power Results

**Table 4: Conducted Power Measurement Results**

| Wifi                 |        | Conducted Power (dBm) |           |            |
|----------------------|--------|-----------------------|-----------|------------|
|                      |        | Channel 1             | Channel 6 | Channel 11 |
| <b>802.11 b</b>      | Before | 24.14                 | 22.16     | 23.21      |
|                      | After  | 24.12                 | 22.15     | 23.20      |
| <b>802.11 g</b>      | Before | 19.23                 | 19.52     | 19.73      |
| <b>802.11 n(H20)</b> | Before | 18.67                 | 18.49     | 18.26      |
| <b>802.11 n(H40)</b> | Before | 18.27                 | 18.19     | 18.16      |

Note: 1. SAR is not required for 802.11g/n channels when the maximum average output power is less than 0.25dB higher than that measured on the corresponding 802.11b channels.



## 7. Test Results

### 7.1. Dielectric Performance

**Table 5: Dielectric Performance of Body Tissue Simulating Liquid**

| Frequency         | Description                    | Dielectric Parameters  |                      | Temp<br>°C |
|-------------------|--------------------------------|------------------------|----------------------|------------|
|                   |                                | $\epsilon_r$           | $\sigma(\text{s/m})$ |            |
| 2450MHz<br>(body) | Target value<br>±10% window    | 52.70<br>50.07 — 55.34 | 1.95<br>1.85 — 2.05  | /          |
|                   | Measurement value<br>2010-11-6 | 51.83                  | 1.92                 | 21.5       |

### 7.2. System Check

**Table 6: System Check for Body Tissue Simulating Liquid**

| Frequency | Description                      | SAR(W/kg)         |                   | Dielectric Parameters |                      | Temp<br>°C |
|-----------|----------------------------------|-------------------|-------------------|-----------------------|----------------------|------------|
|           |                                  | 10g               | 1g                | $\epsilon_r$          | $\sigma(\text{s/m})$ |            |
| 2450MHz   | Recommended value<br>±10% window | 5.97<br>5.37—6.57 | 13<br>11.7 — 14.3 | 51.8                  | 2.01                 | /          |
|           | Measurement value<br>2010-11-6   | 6.46              | 14.00             | 51.83                 | 1.92                 | 21.5       |

Note: 1. The graph results see ANNEX B.

2. Target Values used derive from the calibration certificate and 250 mW is used as feeding power to the Calibrated dipole.

**TA Technology (Shanghai) Co., Ltd.**  
**Test Report**

**7.3. Summary of Measurement Results**

**7.3.1. 802.11b**

**Table 7: SAR Values (802.11b)**

| Limit of SAR            |         | 10 g Average              | 1g Average  | Power Drift      | Graph Results |
|-------------------------|---------|---------------------------|-------------|------------------|---------------|
|                         |         | 2.0 W/kg                  | 1.6 W/kg    | ± 0.21 dB        |               |
| Test Case Of Body       |         | Measurement Result (W/kg) |             | Power Drift (dB) |               |
| Different Test Position | Channel | 10 g Average              | 1 g Average |                  |               |
| <b>IBM T61</b>          |         |                           |             |                  |               |
| Test Position 1         | Middle  | 0.114                     | 0.227       | -0.013           | Figure 7      |
| Test Position 2         | High    | 0.198                     | 0.401       | -0.028           | Figure 8      |
|                         | Middle  | 0.150                     | 0.308       | 0.067            | Figure 9      |
|                         | Low     | 0.191                     | 0.394       | 0.138            | Figure 10     |
| <b>Lenovo Y-450</b>     |         |                           |             |                  |               |
| Test Position 3         | Middle  | 0.056                     | 0.109       | -0.092           | Figure 11     |
| Test Position 4         | Middle  | 0.026                     | 0.063       | -0.066           | Figure 12     |

Note: 1. The value with blue color is the maximum SAR Value of each test band.

2. The SAR test shall be performed at the high, middle and low frequency channels of each operating mode. If the SAR measured at mid-band channel for each test configuration is at least 3.0 dB (< 0.8W/kg) lower than the SAR limit, testing at the high and low channels is optional.
3. Upper and lower frequencies were measured at the worst case.

**7.3.2. 802.11g/n**

SAR is not required for 802.11g/n channels when the maximum average output power is less than 0.25dB higher than that measured on the corresponding 802.11b channels.

**TA Technology (Shanghai) Co., Ltd.**  
**Test Report**

Report No. RZA1011-1731SAR

Page 27 of 65

**8. Measurement Uncertainty**

| No.                 | source  | Type | Uncertainty Value (%) | Probability Distribution | k          | c <sub>i</sub> | Standard uncertainty u <sub>i</sub> (%) | Degree of freedom V <sub>eff</sub> or v <sub>i</sub> |
|---------------------|---|------|-----------------------|--------------------------|------------|----------------|---|--|
| 1                   | System repetivity   | A    | 0.5                   | N                        | 1          | 1              | 0.5                                     | 9  |
| Measurement system  |   |      |                       |                          |            |                |   |  |
| 2                   | probe calibration   | B    | 5.9                   | N                        | 1          | 1              | 5.9                                     | ∞  |
| 3                   | axial isotropy of the probe   | B    | 4.7                   | R                        | $\sqrt{3}$ | $\sqrt{0.5}$   | 1.9                                     | ∞  |
| 4                   | Hemispherical isotropy of the probe   | B    | 9.4                   | R                        | $\sqrt{3}$ | $\sqrt{0.5}$   | 3.9                                     | ∞  |
| 6                   | boundary effect   | B    | 1.9                   | R                        | $\sqrt{3}$ | 1              | 1.1                                     | ∞  |
| 7                   | probe linearity   | B    | 4.7                   | R                        | $\sqrt{3}$ | 1              | 2.7                                     | ∞  |
| 8                   | System detection limits   | B    | 1.0                   | R                        | $\sqrt{3}$ | 1              | 0.6                                     | ∞  |
| 9                   | readout Electronics   | B    | 1.0                   | N                        | 1          | 1              | 1.0                                     | ∞  |
| 10                  | response time   | B    | 0                     | R                        | $\sqrt{3}$ | 1              | 0                                       | ∞  |
| 11                  | integration time  | B    | 4.32                  | R                        | $\sqrt{3}$ | 1              | 2.5                                     | ∞  |
| 12                  | noise   | B    | 0                     | R                        | $\sqrt{3}$ | 1              | 0                                       | ∞  |
| 13                  | RF Ambient Conditions   | B    | 3                     | R                        | $\sqrt{3}$ | 1              | 1.73                                    | ∞  |
| 14                  | Probe Positioner Mechanical Tolerance   | B    | 0.4                   | R                        | $\sqrt{3}$ | 1              | 0.2                                     | ∞  |
| 15                  | Probe Positioning with respect to Phantom Shell                                 | B    | 2.9                   | R                        | $\sqrt{3}$ | 1              | 1.7                                     | ∞  |
| 16                  | Extrapolation, interpolation and Integration Algorithms for Max. SAR Evaluation | B    | 3.9                   | R                        | $\sqrt{3}$ | 1              | 2.3                                     | ∞  |
| Test sample Related |   |      |                       |                          |            |                |   |  |
| 17                  | -Test Sample Positioning  | A    | 2.9                   | N                        | 1          | 1              | 2.9                                     | 5  |
| 18                  | -Device Holder Uncertainty  | A    | 4.1                   | N                        | 1          | 1              | 4.1                                     | 5  |
| 19                  | -Output Power Variation - SAR drift measurement                                 | B    | 5.0                   | R                        | $\sqrt{3}$ | 1              | 2.9                                     | ∞  |
| Physical parameter  |   |      |                       |                          |            |                |   |  |

**TA Technology (Shanghai) Co., Ltd.**  
**Test Report**

Report No. RZA1011-1731SAR

Page 28 of 65

|  |  |  |     |   |            |      |      |          |
|--|--|--|-----|---|------------|------|------|----------|
| 20   | -phantom                                       | B  | 4.0 | R | $\sqrt{3}$ | 1    | 2.3  | $\infty$ |
| 21   | -liquid conductivity (deviation from target)   | B  | 5.0 | R | $\sqrt{3}$ | 0.64 | 1.8  | $\infty$ |
| 22   | -liquid conductivity (measurement uncertainty) | B  | 5.0 | N | 1          | 0.64 | 3.2  | $\infty$ |
| 23   | -liquid permittivity (deviation from target)   | B  | 5.0 | R | $\sqrt{3}$ | 0.6  | 1.7  | $\infty$ |
| 24   | -liquid permittivity (measurement uncertainty) | B  | 5.0 | N | 1          | 0.6  | 3.0  | $\infty$ |
| Combined standard uncertainty                      |  | $u_c = \sqrt{\sum_{i=1}^{21} c_i^2 u_i^2}$ |     |   |            |      | 12.0 |          |
| Expanded uncertainty (confidence interval of 95 %) |  | $u_e = 2u_c$                               |     | N | k=2        | 24.0 |      |          |


## 9. Main Test Instruments

**Table 8: List of Main Instruments**


| No. | Name                   | Type           | Serial Number | Calibration Date         | Valid Period |
|-----|------------------------|----------------|---------------|--------------------------|--------------|
| 01  | Network analyzer       | Agilent 8753E  | US37390326    | September 13, 2010       | One year     |
| 02  | Dielectric Probe Kit   | Agilent 85070E | US44020115    | No Calibration Requested |              |
| 03  | Power meter            | Agilent E4417A | GB41291714    | March 13, 2010           | One year     |
| 04  | Power sensor           | Agilent 8481H  | MY41091316    | March 26, 2010           | One year     |
| 05  | Signal Generator       | HP 8341B       | 2730A00804    | September 13, 2010       | One year     |
| 06  | Amplifier              | IXA-020        | 0401          | No Calibration Requested |              |
| 07  | Validation Kit 2450MHz | D2450V2        | 712           | February 19, 2010        | One year     |
| 09  | BTS                    | E5515C         | MY48360988    | December 4, 2009         | One year     |
| 10  | E-field Probe          | EX3DV4         | 3661          | December 30, 2009        | One year     |
| 11  | DAE                    | DAE4           | 871           | November 11, 2009        | One year     |

\*\*\*END OF REPORT BODY\*\*\*

## ANNEX A: Test Layout

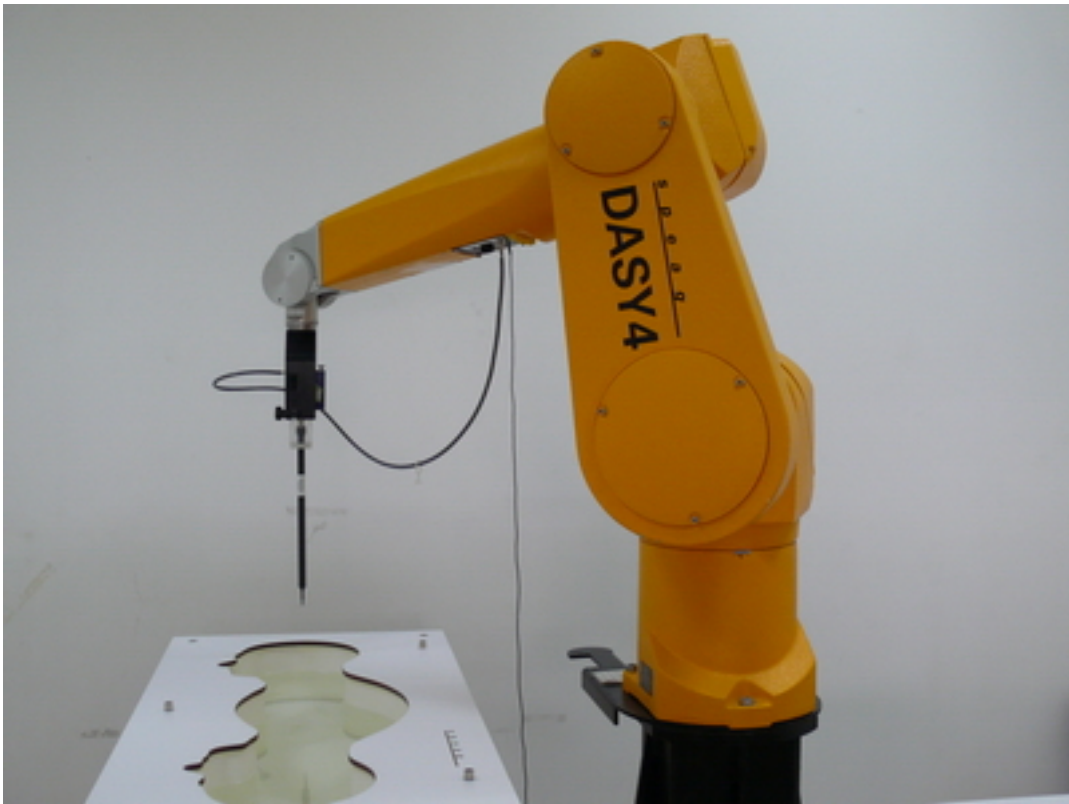

Picture 2: Specific Absorption Rate Test Layout

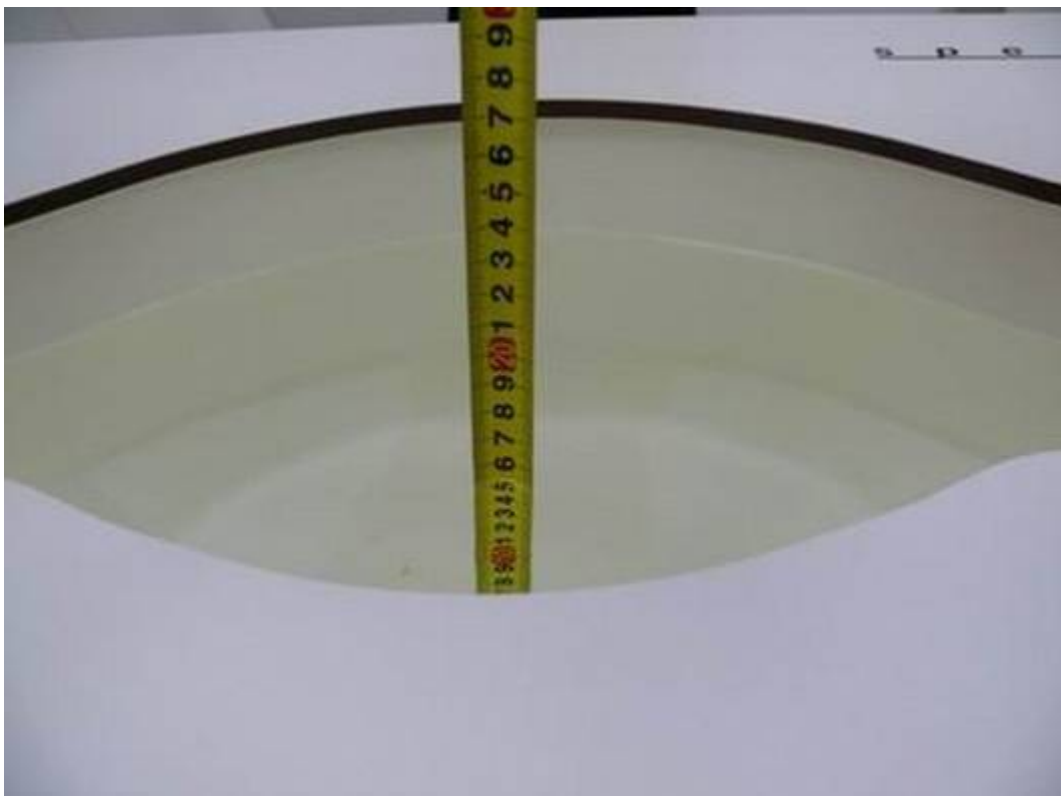

Picture 3: Liquid depth in the flat Phantom (2450 MHz, 15.2cm depth)

## ANNEX B: System Check Results

### System Performance Check at 2450 MHz

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 712

Date/Time: 11/6/2010 9:12:36 AM

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.92$  mho/m;  $\epsilon_r = 51.83$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.3 °C      Liquid Temperature: 21.5 °C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3661; ConvF(7.34, 7.34, 7.34); Calibrated: 12/30/2009

Electronics: DAE4 Sn871; Calibrated: 11/11/2009

Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

**d=10mm, Pin=250mW/Area Scan (71x71x1):** Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 21.5 mW/g


**d=10mm, Pin=250mW/Zoom Scan (7x7x7) /Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 71.0 V/m; Power Drift = 0.011 dB

Peak SAR (extrapolated) = 28.2 W/kg

**SAR(1 g) = 14.0 mW/g; SAR(10 g) = 6.46 mW/g**

Maximum value of SAR (measured) = 19.8 mW/g

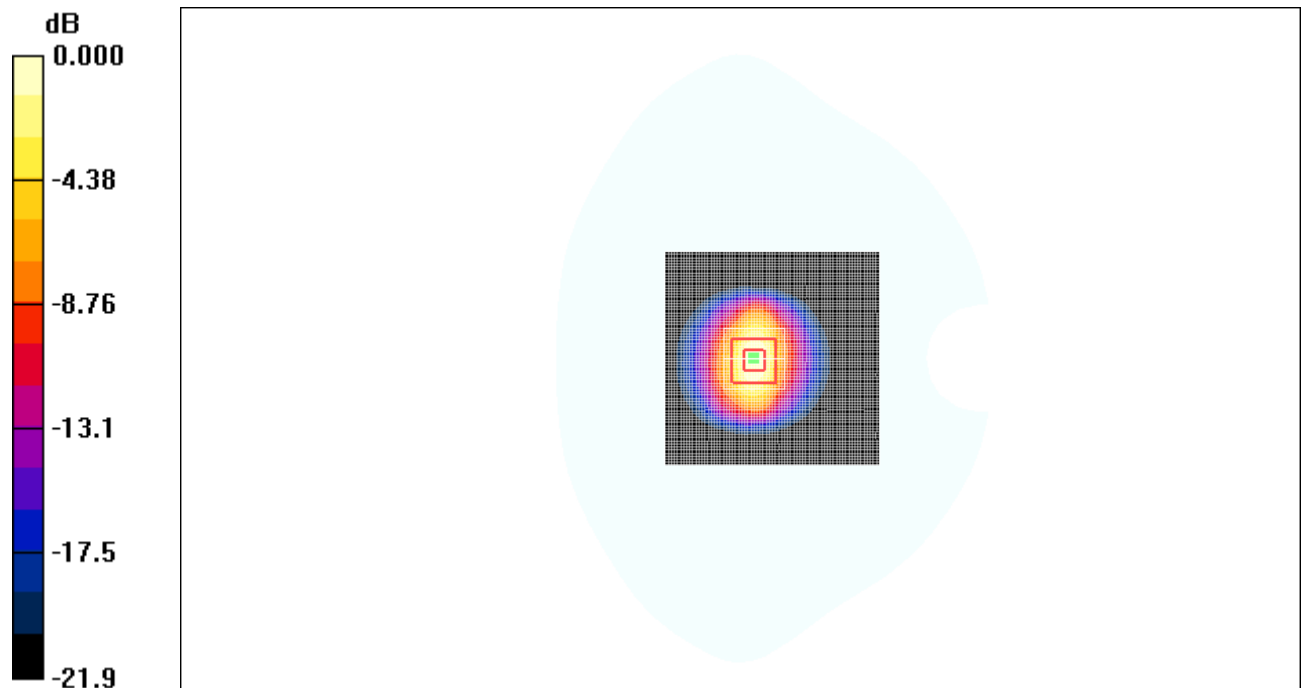

0 dB = 19.8mW/g

Figure 6 System Performance Check 2450MHz 250mW

## ANNEX C: Graph Results

### 802.11b with IBM T61 Test Position 1 Middle

Date/Time: 11/6/2010 12:12:09 PM

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated):  $f = 2437$  MHz;  $\sigma = 1.91$  mho/m;  $\epsilon_r = 51.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.3 °C      Liquid Temperature: 21.5°C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3661; ConvF(7.34, 7.34, 7.34); Calibrated: 12/30/2009

Electronics: DAE4 Sn871; Calibrated: 11/11/2009

Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

**Test Position 1 Middle/Area Scan (41x101x1):** Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.277 mW/g

**Test Position 1 Middle/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 9.63 V/m; Power Drift = -0.013 dB

Peak SAR (extrapolated) = 0.438 W/kg

**SAR(1 g) = 0.227 mW/g; SAR(10 g) = 0.114 mW/g**

Maximum value of SAR (measured) = 0.258 mW/g

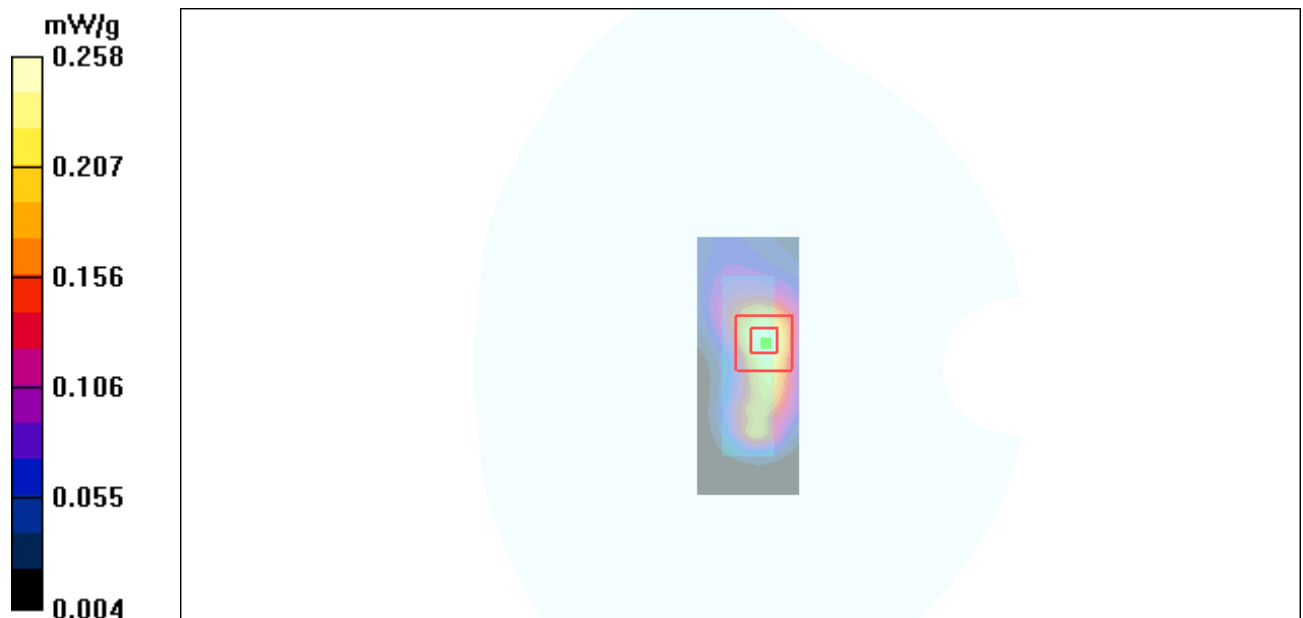


Figure 7 802.11b with IBM T61 Test Position 1 Channel 6

### 802.11b with IBM T61 Test Position 2 High

Date/Time: 11/6/2010 1:34:44 PM

Communication System: 802.11b; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 2462$  MHz;  $\sigma = 1.94$  mho/m;  $\epsilon_r = 51.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.3 °C      Liquid Temperature: 21.5°C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3661; ConvF(7.34, 7.34, 7.34); Calibrated: 12/30/2009

Electronics: DAE4 Sn871; Calibrated: 11/11/2009

Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

**Test Position 2 High/Area Scan (41x101x1):** Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.458 mW/g


**Test Position 2 High/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 15.3 V/m; Power Drift = -0.028 dB

Peak SAR (extrapolated) = 0.808 W/kg

**SAR(1 g) = 0.401 mW/g; SAR(10 g) = 0.198 mW/g**

Maximum value of SAR (measured) = 0.455 mW/g

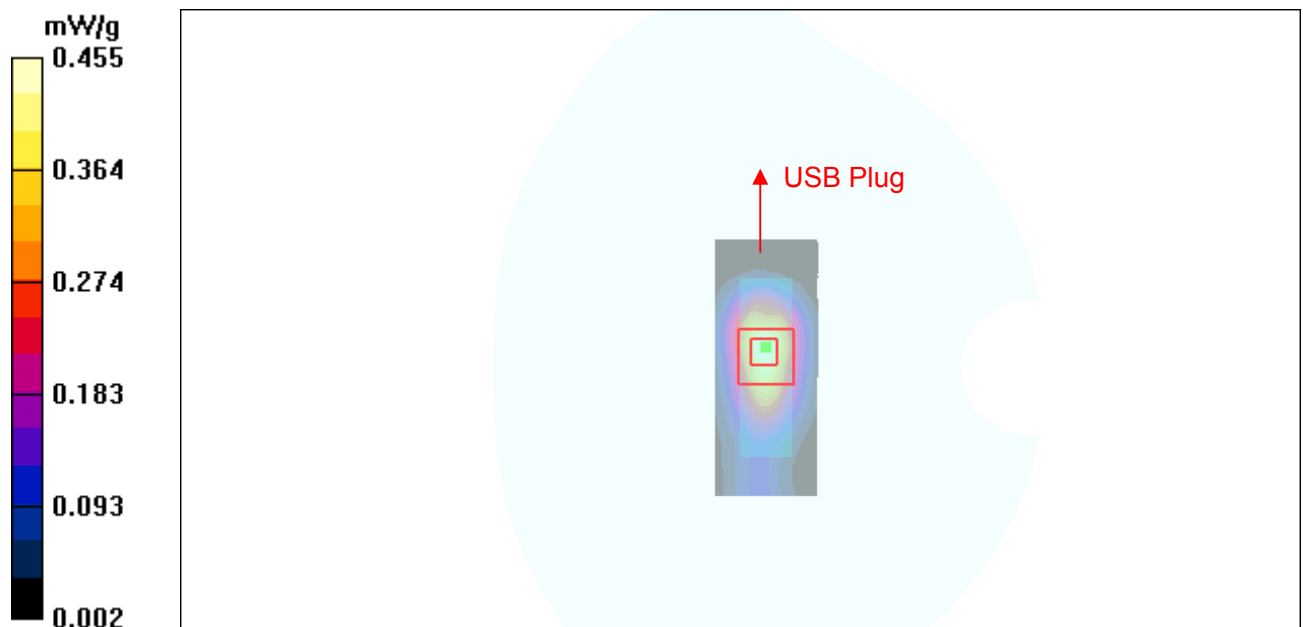



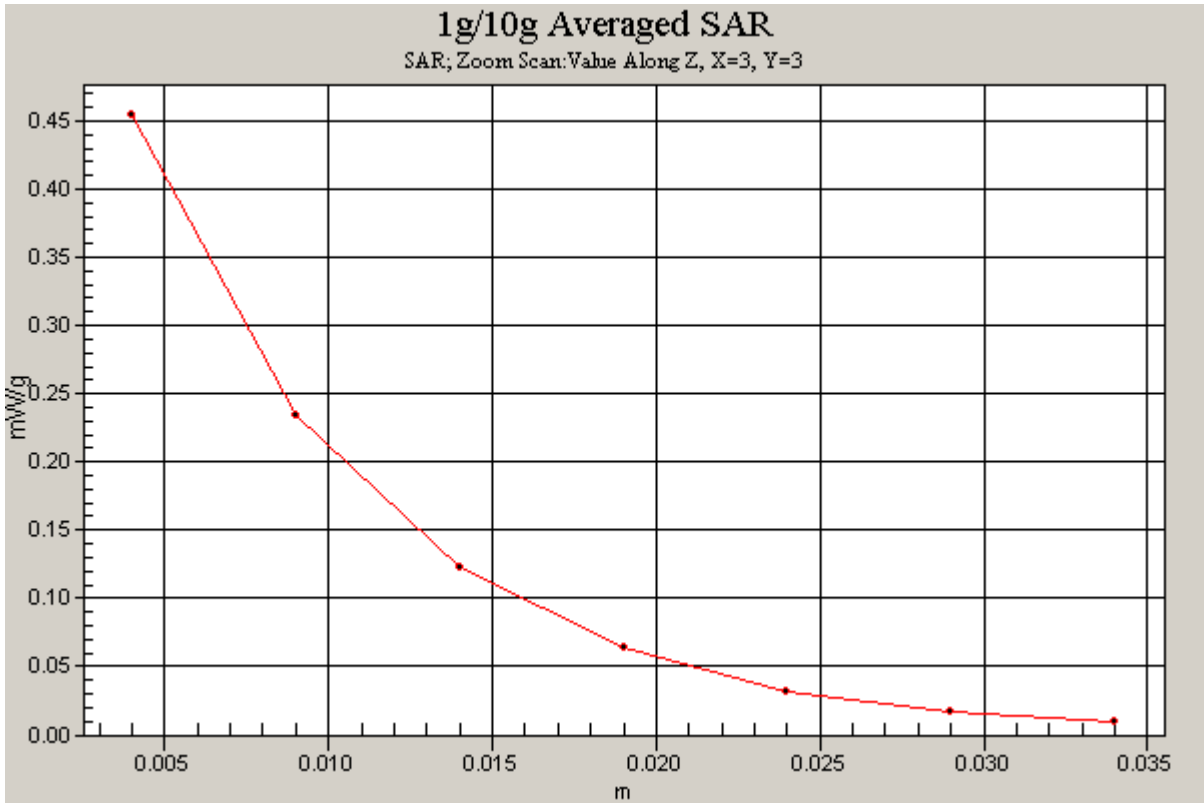


Figure 8 802.11b with IBM T61 Test Position 2 Channel 11

**802.11b with IBM T61 Test Position 2 Middle**

Date/Time: 11/6/2010 1:08:02 PM

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated):  $f = 2437$  MHz;  $\sigma = 1.91$  mho/m;  $\epsilon_r = 51.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.3 °C      Liquid Temperature: 21.5 °C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3661; ConvF(7.34, 7.34, 7.34); Calibrated: 12/30/2009

Electronics: DAE4 Sn871; Calibrated: 11/11/2009

Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

**Test Position 2 Middle/Area Scan (41x101x1):** Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.395 mW/g

**Test Position 2 Middle/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 15.1 V/m; Power Drift = 0.067 dB

Peak SAR (extrapolated) = 0.625 W/kg

**SAR(1 g) = 0.308 mW/g; SAR(10 g) = 0.150 mW/g**

Maximum value of SAR (measured) = 0.350 mW/g

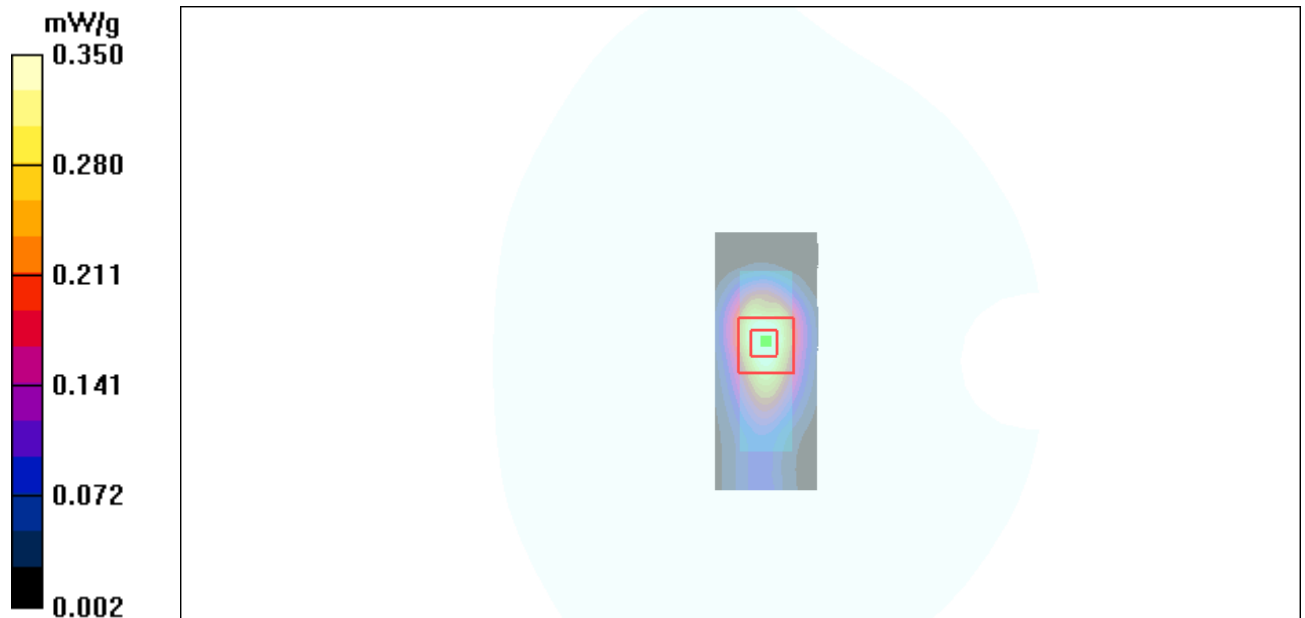


Figure 9 802.11b with IBM T61 Test Position 2 Channel 6

**802.11b with IBM T61 Test Position 2 Low**

Date/Time: 11/6/2010 1:52:39 PM

Communication System: 802.11b; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 2412$  MHz;  $\sigma = 1.88$  mho/m;  $\epsilon_r = 51.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.3 °C      Liquid Temperature: 21.5°C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3661; ConvF(7.34, 7.34, 7.34); Calibrated: 12/30/2009

Electronics: DAE4 Sn871; Calibrated: 11/11/2009

Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

**Test Position 2 Low/Area Scan (41x101x1):** Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.439 mW/g

**Test Position 2 Low/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 14.2 V/m; Power Drift = 0.138 dB

Peak SAR (extrapolated) = 0.799 W/kg

**SAR(1 g) = 0.394 mW/g; SAR(10 g) = 0.191 mW/g**

Maximum value of SAR (measured) = 0.452 mW/g

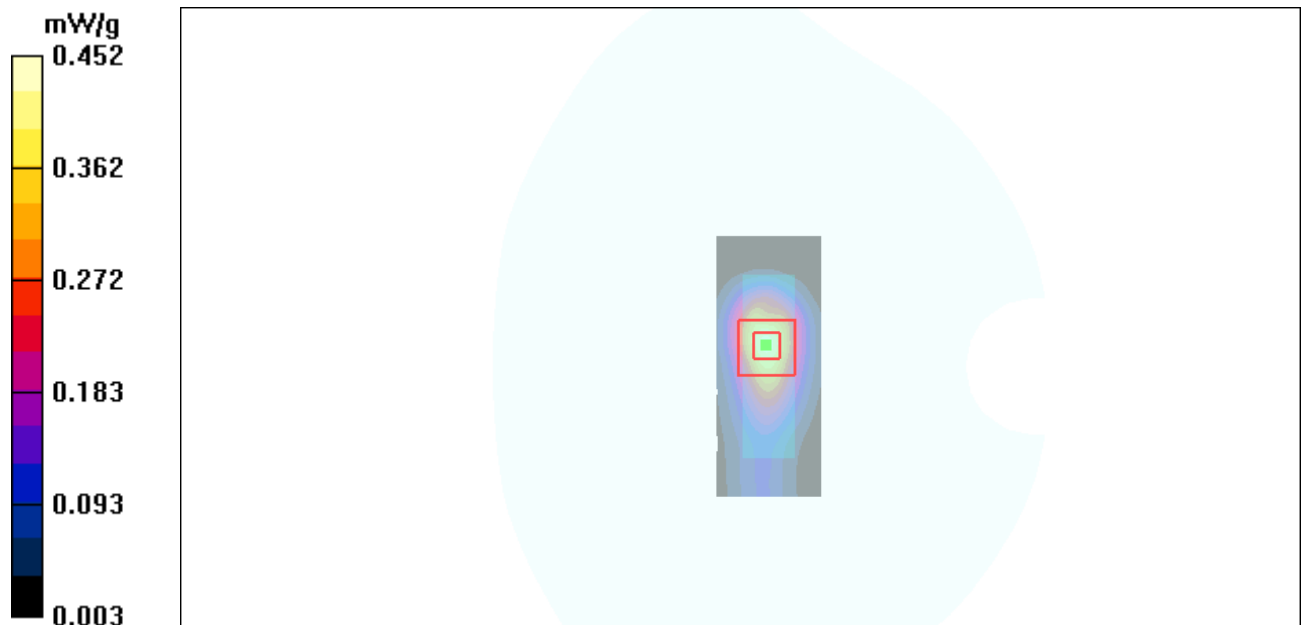


Figure 10 802.11b with IBM T61 Test Position 2 Channel 1

**802.11b with Lenovo Y-450 Test Position 3 Middle**

Date/Time: 11/6/2010 11:41:38 AM

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated):  $f = 2437$  MHz;  $\sigma = 1.91$  mho/m;  $\epsilon_r = 51.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.3 °C      Liquid Temperature: 21.5°C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3661; ConvF(7.34, 7.34, 7.34); Calibrated: 12/30/2009

Electronics: DAE4 Sn871; Calibrated: 11/11/2009

Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

**Test Position 3 Middle/Area Scan (41x101x1):** Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.132 mW/g

**Test Position 3 Middle/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 8.41 V/m; Power Drift = -0.092 dB

Peak SAR (extrapolated) = 0.210 W/kg

**SAR(1 g) = 0.109 mW/g; SAR(10 g) = 0.056 mW/g**

Maximum value of SAR (measured) = 0.121 mW/g

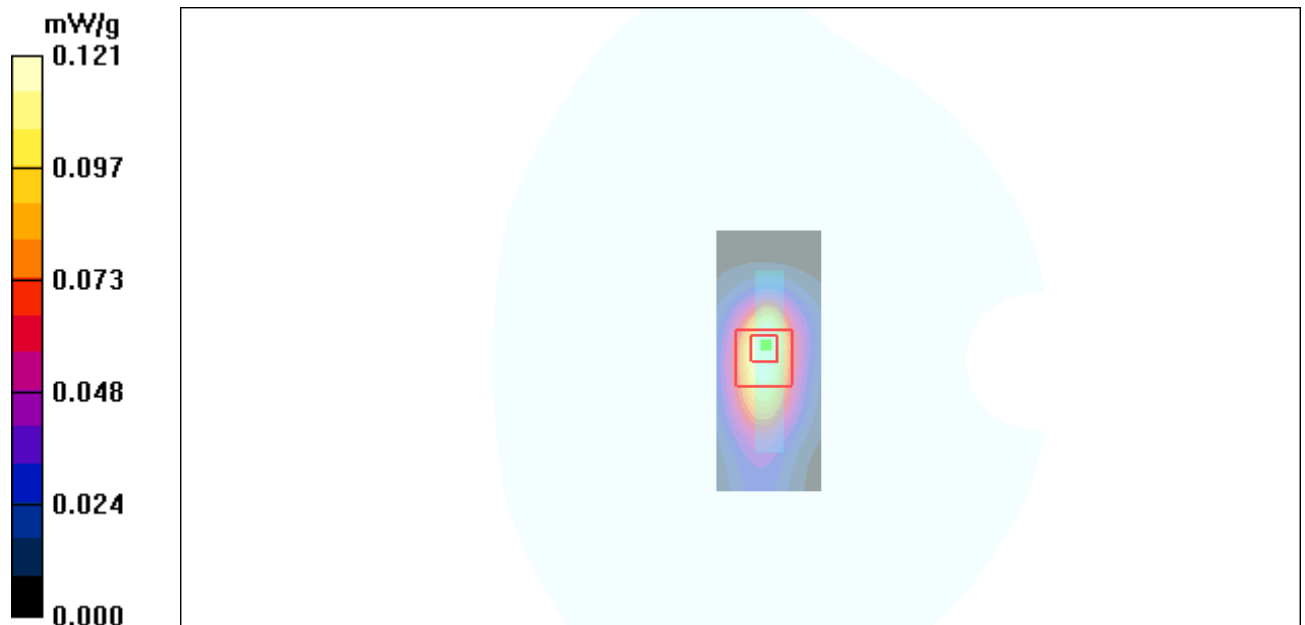


Figure 11 802.11b with Lenovo Y-450 Test Position 3 Channel 6

**802.11b with Lenovo Y-450 Test Position 4 Middle**

Date/Time: 11/6/2010 10:50:24 AM

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated):  $f = 2437$  MHz;  $\sigma = 1.91$  mho/m;  $\epsilon_r = 51.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.3 °C      Liquid Temperature: 21.5 °C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3661; ConvF(7.34, 7.34, 7.34); Calibrated: 12/30/2009

Electronics: DAE4 Sn871; Calibrated: 11/11/2009

Phantom: SAM000 T01; Type: SAM V4.0; Serial: TP-1246

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

**Test Position 4 Middle/Area Scan (41x101x1):** Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.080 mW/g

**Test Position 4 Middle/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 4.24 V/m; Power Drift = -0.066 dB

Peak SAR (extrapolated) = 0.148 W/kg

**SAR(1 g) = 0.063 mW/g; SAR(10 g) = 0.026 mW/g**

Maximum value of SAR (measured) = 0.075 mW/g

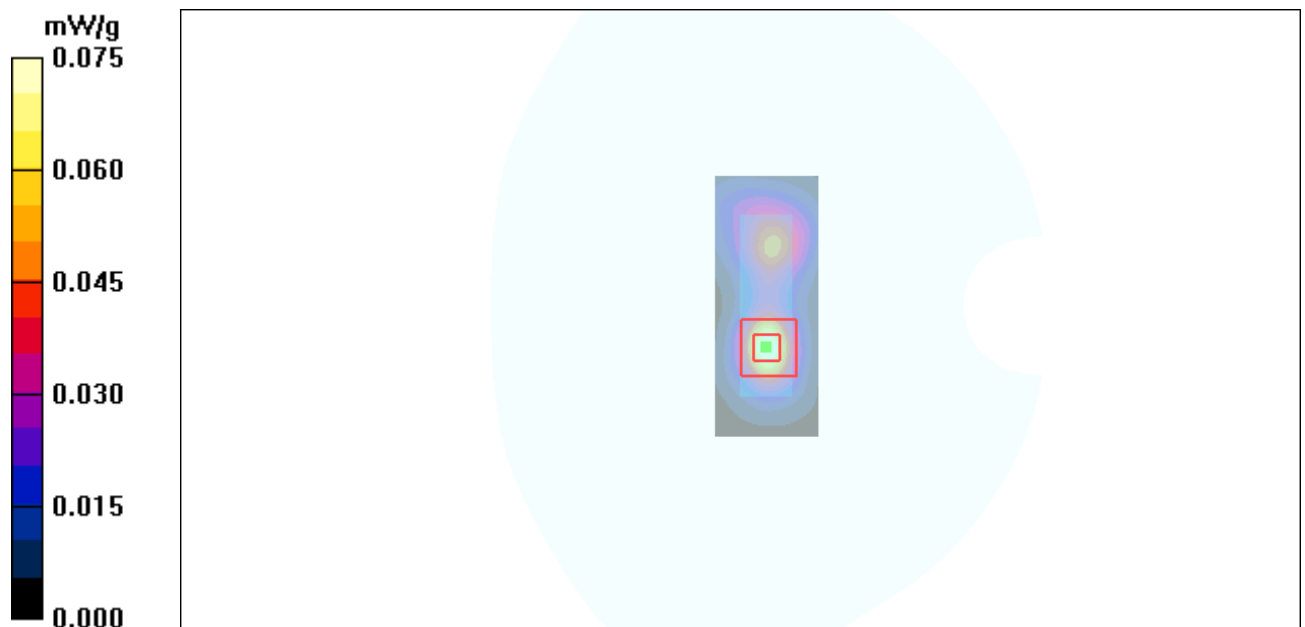


Figure 12 802.11b with Lenovo Y-450 Test Position 4 Channel 6

# TA Technology (Shanghai) Co., Ltd. Test Report

Report No. RZA1011-1731SAR

Page 38 of 65

## ANNEX D: Probe Calibration Certificate

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Auden**

Certificate No: **EX3-3661\_Dec09**

| <b>CALIBRATION CERTIFICATE</b>   |  |                                      |                        |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
|--|--|--------------------------------------|------------------------|-------------------|------|----------------------------|-----------------------|--------------------|------------|--------------------------|--------|---------------------|------------|--------------------------|--------|---------------------|------------|--------------------------|--------|---------------------------|----------------|---------------------------|--------|----------------------------|-----------------|---------------------------|--------|----------------------------|-----------------|---------------------------|--------|------------------------|----------|-------------------------------|--------|------|---------|--------------------------------|--------|---------------------|------|-----------------------|-----------------|-----------------------|--------------|----------------------------------|------------------------|---------------------------|------------|-----------------------------------|-----------------------|
| Object   | EX3DV4 - SN:3661   |                                      |                        |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Calibration procedure(s)   | QA CAL-01.v6, QA CAL-14.v3, QA CAL-23.v3 and QA CAL-25.v2<br>Calibration procedure for dosimetric E-field probes |                                      |                        |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Calibration date:  | December 30, 2009  |                                      |                        |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).<br/>The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 30%;">Primary Standards</th> <th style="width: 15%;">ID #</th> <th style="width: 30%;">Cal Date (Certificate No.)</th> <th style="width: 25%;">Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter E4419B</td> <td>GB41293874</td> <td>1-Apr-09 (No. 217-01030)</td> <td>Apr-10</td> </tr> <tr> <td>Power sensor E4412A</td> <td>MY41495277</td> <td>1-Apr-09 (No. 217-01030)</td> <td>Apr-10</td> </tr> <tr> <td>Power sensor E4412A</td> <td>MY41498087</td> <td>1-Apr-09 (No. 217-01030)</td> <td>Apr-10</td> </tr> <tr> <td>Reference 3 dB Attenuator</td> <td>SN: S5054 (3c)</td> <td>31-Mar-09 (No. 217-01026)</td> <td>Mar-10</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: S5086 (20b)</td> <td>31-Mar-09 (No. 217-01028)</td> <td>Mar-10</td> </tr> <tr> <td>Reference 30 dB Attenuator</td> <td>SN: S5129 (30b)</td> <td>31-Mar-09 (No. 217-01027)</td> <td>Mar-10</td> </tr> <tr> <td>Reference Probe ES3DV2</td> <td>SN: 3013</td> <td>2-Jan-09 (No. ES3-3013_Jan09)</td> <td>Jan-10</td> </tr> <tr> <td>DAE4</td> <td>SN: 880</td> <td>29-Sep-08 (No. DAE4-880_Sep08)</td> <td>Sep-10</td> </tr> </tbody> </table><br><table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 30%;">Secondary Standards</th> <th style="width: 15%;">ID #</th> <th style="width: 30%;">Check Date (in house)</th> <th style="width: 25%;">Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>RF generator HP 8648C</td> <td>US3642U01700</td> <td>4-Aug-99 (in house check Oct-09)</td> <td>In house check: Oct-11</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>US37390585</td> <td>18-Oct-01 (in house check Oct-09)</td> <td>In house check: Oct10</td> </tr> </tbody> </table> |  |                                      |                        | Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration | Power meter E4419B | GB41293874 | 1-Apr-09 (No. 217-01030) | Apr-10 | Power sensor E4412A | MY41495277 | 1-Apr-09 (No. 217-01030) | Apr-10 | Power sensor E4412A | MY41498087 | 1-Apr-09 (No. 217-01030) | Apr-10 | Reference 3 dB Attenuator | SN: S5054 (3c) | 31-Mar-09 (No. 217-01026) | Mar-10 | Reference 20 dB Attenuator | SN: S5086 (20b) | 31-Mar-09 (No. 217-01028) | Mar-10 | Reference 30 dB Attenuator | SN: S5129 (30b) | 31-Mar-09 (No. 217-01027) | Mar-10 | Reference Probe ES3DV2 | SN: 3013 | 2-Jan-09 (No. ES3-3013_Jan09) | Jan-10 | DAE4 | SN: 880 | 29-Sep-08 (No. DAE4-880_Sep08) | Sep-10 | Secondary Standards | ID # | Check Date (in house) | Scheduled Check | RF generator HP 8648C | US3642U01700 | 4-Aug-99 (in house check Oct-09) | In house check: Oct-11 | Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (in house check Oct-09) | In house check: Oct10 |
| Primary Standards  | ID #   | Cal Date (Certificate No.)           | Scheduled Calibration  |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Power meter E4419B   | GB41293874   | 1-Apr-09 (No. 217-01030)             | Apr-10                 |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Power sensor E4412A  | MY41495277   | 1-Apr-09 (No. 217-01030)             | Apr-10                 |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Power sensor E4412A  | MY41498087   | 1-Apr-09 (No. 217-01030)             | Apr-10                 |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Reference 3 dB Attenuator  | SN: S5054 (3c)   | 31-Mar-09 (No. 217-01026)            | Mar-10                 |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Reference 20 dB Attenuator   | SN: S5086 (20b)  | 31-Mar-09 (No. 217-01028)            | Mar-10                 |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Reference 30 dB Attenuator   | SN: S5129 (30b)  | 31-Mar-09 (No. 217-01027)            | Mar-10                 |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Reference Probe ES3DV2   | SN: 3013   | 2-Jan-09 (No. ES3-3013_Jan09)        | Jan-10                 |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| DAE4   | SN: 880  | 29-Sep-08 (No. DAE4-880_Sep08)       | Sep-10                 |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Secondary Standards  | ID #   | Check Date (in house)                | Scheduled Check        |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| RF generator HP 8648C  | US3642U01700   | 4-Aug-99 (in house check Oct-09)     | In house check: Oct-11 |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Network Analyzer HP 8753E  | US37390585   | 18-Oct-01 (in house check Oct-09)    | In house check: Oct10  |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Calibrated by:   | Name<br><b>Katja Pokovic</b>   | Function<br><b>Technical Manager</b> | Signature<br>          |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Approved by:   | Name<br><b>Niels Kuster</b>  | Quality Manager                      |                        |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| Issued: December 30, 2009  |  |                                      |                        |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory.  |  |                                      |                        |                   |      |                            |                       |                    |            |                          |        |                     |            |                          |        |                     |            |                          |        |                           |                |                           |        |                            |                 |                           |        |                            |                 |                           |        |                        |          |                               |        |      |         |                                |        |                     |      |                       |                 |                       |              |                                  |                        |                           |            |                                   |                       |

Certificate No. EX3-3661\_Dec09

Page 1 of 11

# TA Technology (Shanghai) Co., Ltd.

## Test Report

Report No. RZA1011-1731SAR

Page 39 of 65

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary:

|                       |   |
|-----------------------|---|
| TSL                   | tissue simulating liquid  |
| NORM <sub>x,y,z</sub> | sensitivity in free space   |
| ConvF                 | sensitivity in TSL / NORM <sub>x,y,z</sub>  |
| DCP                   | diode compression point   |
| CF                    | crest factor (1/duty_cycle) of the RF signal  |
| A, B, C               | modulation dependent linearization parameters   |
| Polarization $\phi$   | $\phi$ rotation around probe axis   |
| Polarization $\theta$ | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\theta = 0$ is normal to probe axis |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not effect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: In a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

EX3DV4 SN:3661

December 30, 2009

# Probe EX3DV4

## SN:3661

|               |                   |
|---------------|-------------------|
| Manufactured: | October 20, 2008  |
| Calibrated:   | December 30, 2009 |

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)



# TA Technology (Shanghai) Co., Ltd.

## Test Report

EX3DV4 SN:3661

December 30, 2009

### DASY - Parameters of Probe: EX3DV4 SN:3661

#### Basic Calibration Parameters

|   | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|---|----------|----------|----------|-----------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 0.46     | 0.52     | 0.48     | ± 10.1%   |
| DCP (mV) <sup>B</sup>                                     | 89.4     | 91.4     | 90.5     |           |

#### Modulation Calibration Parameters

| UID   | Communication System Name | PAR  |   | A<br>dB | B<br>dBuV | C    | VR<br>mV | Unc <sup>C</sup><br>(k=2) |
|-------|---------------------------|------|---|---------|-----------|------|----------|---------------------------|
| 10000 | CW                        | 0.00 | X | 0.00    | 0.00      | 1.00 | 300      | ± 1.5%                    |
|       |                           |      | Y | 0.00    | 0.00      | 1.00 | 300      |                           |
|       |                           |      | Z | 0.00    | 0.00      | 1.00 | 300      |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter; uncertainty not required.

<sup>C</sup> Uncertainty is determined using the maximum deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4 SN:3661

December 30, 2009

### DASY - Parameters of Probe: EX3DV4 SN:3661

#### Calibration Parameter Determined in Head Tissue Simulating Media

| f [MHz] | Validity [MHz] <sup>c</sup> | Permittivity | Conductivity | ConvF X | ConvF Y | ConvF Z | Alpha | Depth Unc (k=2) |
|---------|-----------------------------|--------------|--------------|---------|---------|---------|-------|-----------------|
| 835     | ± 50 / ± 100                | 41.5 ± 5%    | 0.90 ± 5%    | 9.34    | 9.34    | 9.34    | 0.69  | 0.64 ± 11.0%    |
| 900     | ± 50 / ± 100                | 41.5 ± 5%    | 0.97 ± 5%    | 9.06    | 9.06    | 9.06    | 0.72  | 0.64 ± 11.0%    |
| 1750    | ± 50 / ± 100                | 40.1 ± 5%    | 1.37 ± 5%    | 8.19    | 8.19    | 8.19    | 0.59  | 0.63 ± 11.0%    |
| 1950    | ± 50 / ± 100                | 40.0 ± 5%    | 1.40 ± 5%    | 7.77    | 7.77    | 7.77    | 0.83  | 0.56 ± 11.0%    |
| 2450    | ± 50 / ± 100                | 39.2 ± 5%    | 1.80 ± 5%    | 7.22    | 7.22    | 7.22    | 0.35  | 0.83 ± 11.0%    |
| 5200    | ± 50 / ± 100                | 36.0 ± 5%    | 4.66 ± 5%    | 5.01    | 5.01    | 5.01    | 0.45  | 1.75 ± 13.1%    |
| 5500    | ± 50 / ± 100                | 35.6 ± 5%    | 4.96 ± 5%    | 4.38    | 4.38    | 4.38    | 0.48  | 1.75 ± 13.1%    |
| 5800    | ± 50 / ± 100                | 35.3 ± 5%    | 5.27 ± 5%    | 4.26    | 4.26    | 4.26    | 0.45  | 1.75 ± 13.1%    |

<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

EX3DV4 SN:3661

December 30, 2009

### DASY - Parameters of Probe: EX3DV4 SN:3661

#### Calibration Parameter Determined in Body Tissue Simulating Media

| f [MHz] | Validity [MHz] <sup>c</sup> | Permittivity | Conductivity | ConvF X | ConvF Y | ConvF Z | Alpha | Depth Unc (k=2) |
|---------|-----------------------------|--------------|--------------|---------|---------|---------|-------|-----------------|
| 835     | ± 50 / ± 100                | 55.2 ± 5%    | 0.97 ± 5%    | 9.24    | 9.24    | 9.24    | 0.54  | 0.73 ± 11.0%    |
| 900     | ± 50 / ± 100                | 55.0 ± 5%    | 1.05 ± 5%    | 8.97    | 8.97    | 8.97    | 0.53  | 0.72 ± 11.0%    |
| 1750    | ± 50 / ± 100                | 53.4 ± 5%    | 1.49 ± 5%    | 7.93    | 7.93    | 7.93    | 0.67  | 0.65 ± 11.0%    |
| 1950    | ± 50 / ± 100                | 53.3 ± 5%    | 1.52 ± 5%    | 7.60    | 7.60    | 7.60    | 0.60  | 0.69 ± 11.0%    |
| 2450    | ± 50 / ± 100                | 52.7 ± 5%    | 1.95 ± 5%    | 7.34    | 7.34    | 7.34    | 0.26  | 1.12 ± 11.0%    |
| 5200    | ± 50 / ± 100                | 49.0 ± 5%    | 5.30 ± 5%    | 4.59    | 4.59    | 4.59    | 0.46  | 1.75 ± 13.1%    |
| 5500    | ± 50 / ± 100                | 48.6 ± 5%    | 5.65 ± 5%    | 4.11    | 4.11    | 4.11    | 0.46  | 1.75 ± 13.1%    |
| 5800    | ± 50 / ± 100                | 48.2 ± 5%    | 6.00 ± 5%    | 4.12    | 4.12    | 4.12    | 0.48  | 1.75 ± 13.1%    |


<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

EX3DV4 SN:3661

December 30, 2009

### Frequency Response of E-Field

(TEM-Cell: ifi110 EXX, Waveguide: R22)

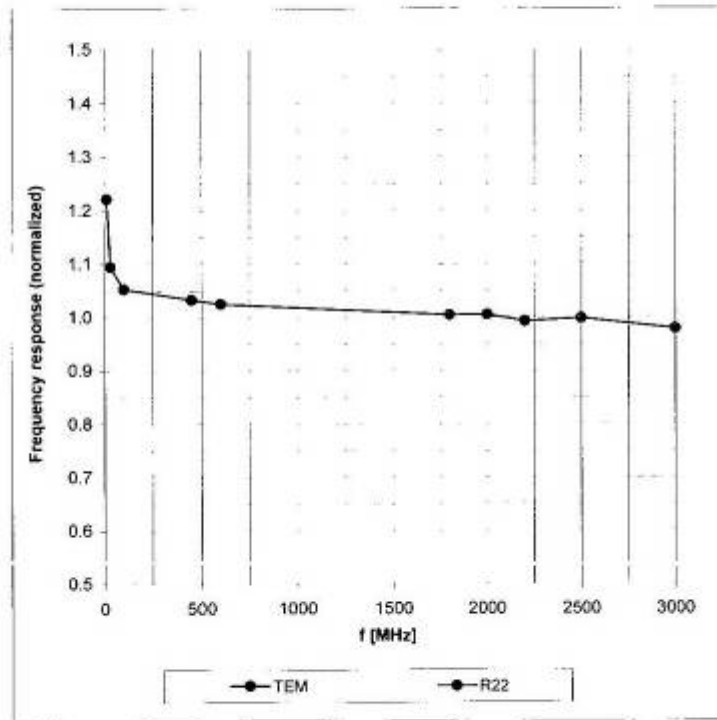



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)

# TA Technology (Shanghai) Co., Ltd. Test Report

EX3DV4 SN:3661

December 30, 2009

## Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

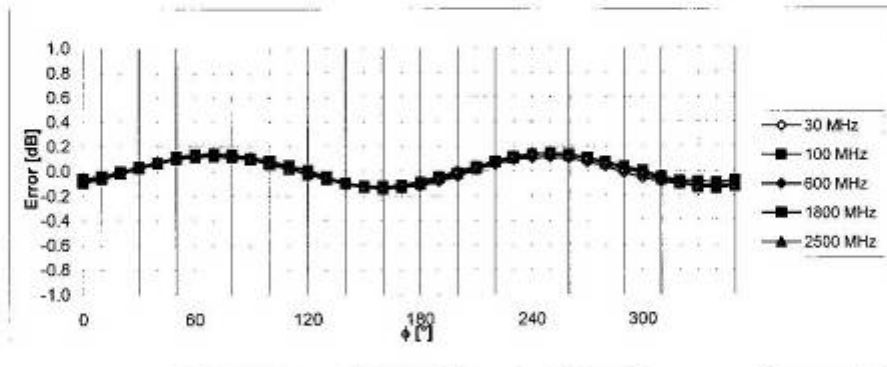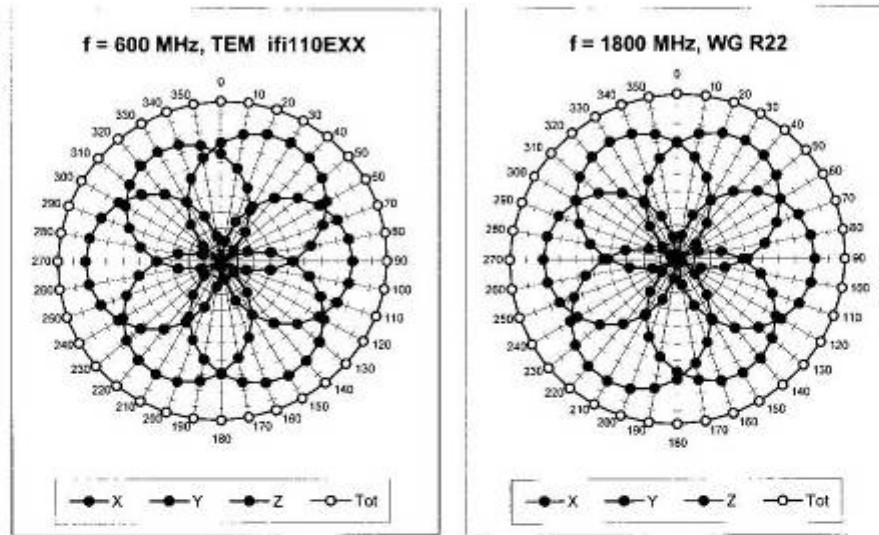


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)

EX3DV4 SN:3661

December 30, 2009

**Dynamic Range f(SAR<sub>head</sub>)**  
(Waveguide R22, f = 1800 MHz)

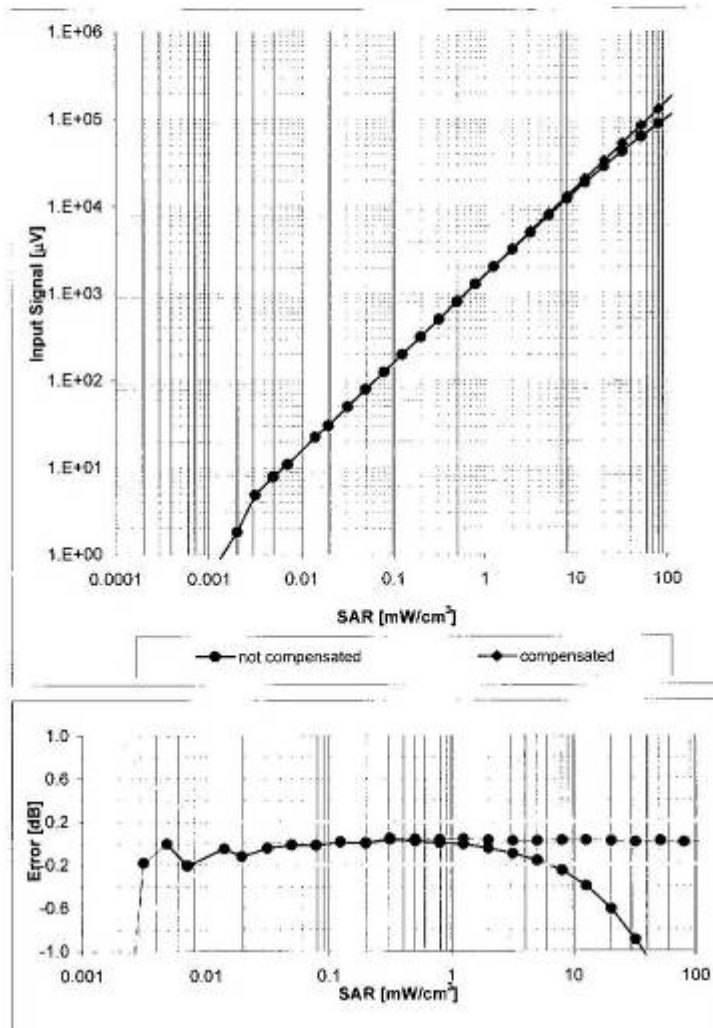


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

EX3DV4 SN:3661


December 30, 2009

### Conversion Factor Assessment

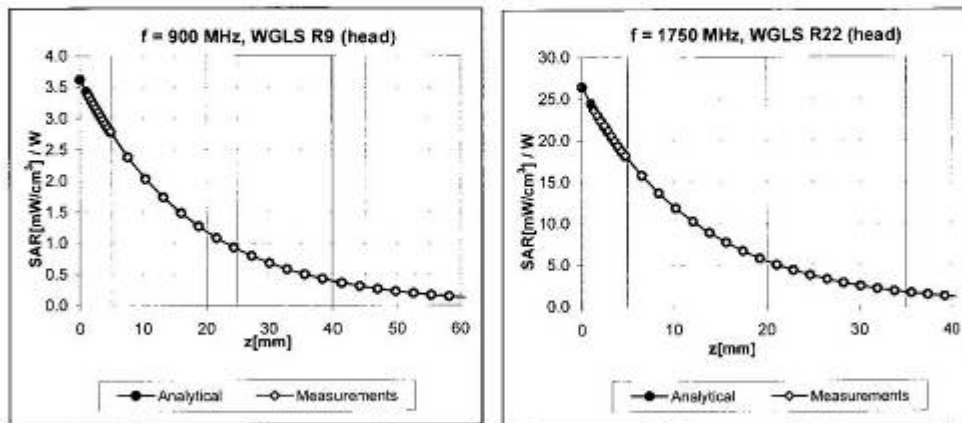

### Deviation from Isotropy in HSL

Error ( $\phi, \theta$ ), f = 900 MHz

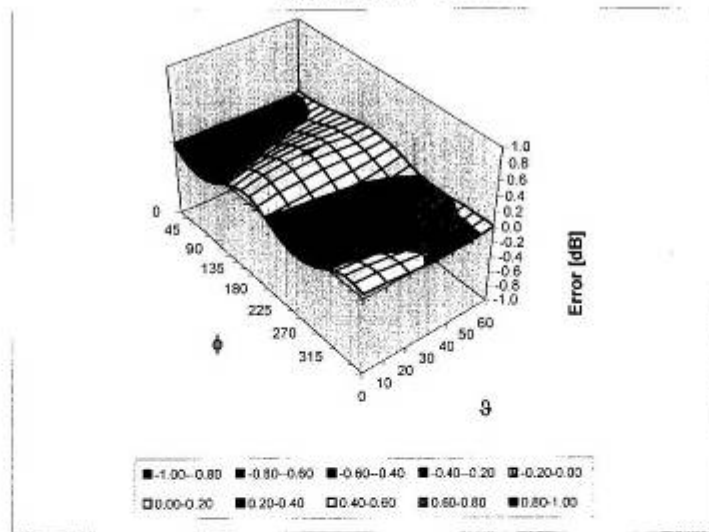

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  (k=2)

**TA Technology (Shanghai) Co., Ltd.**  
**Test Report**

Report No. RZA1011-1731SAR

Page 48 of 65

EX3DV4 SN:3661

December 30, 2009

**Other Probe Parameters**

|   |                |
|---|----------------|
| Sensor Arrangement                            | Triangular     |
| Connector Angle (°)                           | Not applicable |
| Mechanical Surface Detection Mode             | enabled        |
| Optical Surface Detection Mode                | disabled       |
| Probe Overall Length                          | 337 mm         |
| Probe Body Diameter                           | 10 mm          |
| Tip Length                                    | 9 mm           |
| Tip Diameter                                  | 2.5 mm         |
| Probe Tip to Sensor X Calibration Point       | 1 mm           |
| Probe Tip to Sensor Y Calibration Point       | 1 mm           |
| Probe Tip to Sensor Z Calibration Point       | 1 mm           |
| Recommended Measurement Distance from Surface | 2 mm           |



# TA Technology (Shanghai) Co., Ltd. Test Report

Report No. RZA1011-1731SAR

Page 49 of 65

## ANNEX E: D2450V2 Dipole Calibration Certificate

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **ATL (Auden)**

Certificate No: **D2450V2-712\_Feb10**

| <b>CALIBRATION CERTIFICATE</b>  |  |                                   |                           |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
|---|--|-----------------------------------|---------------------------|-------------------|------|----------------------------|-----------------------|----------------------|------------|---------------------------|--------|-----------------------|------------|---------------------------|--------|----------------------------|----------------|---------------------------|--------|-----------------------------|--------------------|---------------------------|--------|------------------------|----------|--------------------------------|--------|------|---------|--------------------------------|--------|---------------------|------|-----------------------|-----------------|-----------------------|------------|-----------------------------------|------------------------|-------------------------|--------|----------------------------------|------------------------|---------------------------|------------------|-----------------------------------|------------------------|
| Object  | D2450V2 - SN: 712  |                                   |                           |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Calibration procedure(s)  | QA CAL-05.v7<br>Calibration procedure for dipole validation kits |                                   |                           |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Calibration date:   | February 19, 2010  |                                   |                           |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).<br/>The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 30%;">Primary Standards</th> <th style="width: 15%;">ID #</th> <th style="width: 35%;">Cal Date (Certificate No.)</th> <th style="width: 20%;">Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter EPM-442A</td> <td>GB37480704</td> <td>06-Oct-09 (No. 217-01086)</td> <td>Oct-10</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>US37292763</td> <td>06-Oct-09 (No. 217-01086)</td> <td>Oct-10</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: 5086 (20g)</td> <td>31-Mar-09 (No. 217-01025)</td> <td>Mar-10</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 5047.2 / 06327</td> <td>31-Mar-09 (No. 217-01029)</td> <td>Mar-10</td> </tr> <tr> <td>Reference Probe ES3DV3</td> <td>SN: 3205</td> <td>26-Jun-09 (No. ES3-3205_Jun09)</td> <td>Jun-10</td> </tr> <tr> <td>DAE4</td> <td>SN: 601</td> <td>07-Mar-09 (No. DAE4-601_Mar09)</td> <td>Mar-10</td> </tr> </tbody> </table><br><table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 30%;">Secondary Standards</th> <th style="width: 15%;">ID #</th> <th style="width: 35%;">Check Date (in house)</th> <th style="width: 20%;">Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power sensor HP 8481A</td> <td>MY41092317</td> <td>18-Oct-02 (in house check Oct-09)</td> <td>In house check: Oct-11</td> </tr> <tr> <td>RF generator R&amp;S SMT-06</td> <td>100005</td> <td>4-Aug-99 (in house check Oct-09)</td> <td>In house check: Oct-11</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>US37390585 S4206</td> <td>18-Oct-01 (in house check Oct-09)</td> <td>In house check: Oct-10</td> </tr> </tbody> </table> |  |                                   |                           | Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration | Power meter EPM-442A | GB37480704 | 06-Oct-09 (No. 217-01086) | Oct-10 | Power sensor HP 8481A | US37292763 | 06-Oct-09 (No. 217-01086) | Oct-10 | Reference 20 dB Attenuator | SN: 5086 (20g) | 31-Mar-09 (No. 217-01025) | Mar-10 | Type-N mismatch combination | SN: 5047.2 / 06327 | 31-Mar-09 (No. 217-01029) | Mar-10 | Reference Probe ES3DV3 | SN: 3205 | 26-Jun-09 (No. ES3-3205_Jun09) | Jun-10 | DAE4 | SN: 601 | 07-Mar-09 (No. DAE4-601_Mar09) | Mar-10 | Secondary Standards | ID # | Check Date (in house) | Scheduled Check | Power sensor HP 8481A | MY41092317 | 18-Oct-02 (in house check Oct-09) | In house check: Oct-11 | RF generator R&S SMT-06 | 100005 | 4-Aug-99 (in house check Oct-09) | In house check: Oct-11 | Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-09) | In house check: Oct-10 |
| Primary Standards   | ID #   | Cal Date (Certificate No.)        | Scheduled Calibration     |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Power meter EPM-442A  | GB37480704   | 06-Oct-09 (No. 217-01086)         | Oct-10                    |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Power sensor HP 8481A   | US37292763   | 06-Oct-09 (No. 217-01086)         | Oct-10                    |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Reference 20 dB Attenuator  | SN: 5086 (20g)   | 31-Mar-09 (No. 217-01025)         | Mar-10                    |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Type-N mismatch combination   | SN: 5047.2 / 06327   | 31-Mar-09 (No. 217-01029)         | Mar-10                    |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Reference Probe ES3DV3  | SN: 3205   | 26-Jun-09 (No. ES3-3205_Jun09)    | Jun-10                    |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| DAE4  | SN: 601  | 07-Mar-09 (No. DAE4-601_Mar09)    | Mar-10                    |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Secondary Standards   | ID #   | Check Date (in house)             | Scheduled Check           |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Power sensor HP 8481A   | MY41092317   | 18-Oct-02 (in house check Oct-09) | In house check: Oct-11    |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| RF generator R&S SMT-06   | 100005   | 4-Aug-99 (in house check Oct-09)  | In house check: Oct-11    |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-09) | In house check: Oct-10    |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Calibrated by:  | Name<br>Jeton Kastrati   | Function<br>Laboratory Technician | Signature<br>             |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| Approved by:  | Name<br>Katja Pokovic  | Function<br>Technical Manager     | Signature<br>             |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
|   |  |                                   | Issued: February 19, 2010 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory.   |  |                                   |                           |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                       |            |                                   |                        |                         |        |                                  |                        |                           |                  |                                   |                        |

# TA Technology (Shanghai) Co., Ltd.

## Test Report

Report No. RZA1011-1731SAR

Page 50 of 65

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary:

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

### Additional Documentation:

- DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

# TA Technology (Shanghai) Co., Ltd.

## Test Report

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                           |             |
|------------------------------|---------------------------|-------------|
| DASY Version                 | DASY5                     | V5.2        |
| Extrapolation                | Advanced Extrapolation    |             |
| Phantom                      | Modular Flat Phantom V4.9 |             |
| Distance Dipole Center - TSL | 10 mm                     | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm         |             |
| Frequency                    | 2450 MHz ± 1 MHz          |             |

### Head TSL parameters

The following parameters and calculations were applied.

|                                  | Temperature     | Permittivity | Conductivity     |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters      | 22.0 °C         | 39.2         | 1.80 mho/m       |
| Measured Head TSL parameters     | (22.0 ± 0.2) °C | 38.5 ± 6 %   | 1.76 mho/m ± 6 % |
| Head TSL temperature during test | (21.0 ± 0.2) °C | ----         | ----             |

### SAR result with Head TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                                   |
|---|--------------------|-----------------------------------|
| SAR measured  | 250 mW input power | 13.3 mW / g                       |
| SAR normalized  | normalized to 1W   | 53.2 mW / g                       |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | <b>53.5 mW / g ± 17.0 % (k=2)</b> |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                                   |
|---|--------------------|-----------------------------------|
| SAR measured  | 250 mW input power | 6.24 mW / g                       |
| SAR normalized  | normalized to 1W   | 25.0 mW / g                       |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | <b>25.0 mW / g ± 16.5 % (k=2)</b> |

# TA Technology (Shanghai) Co., Ltd. Test Report

### Body TSL parameters

The following parameters and calculations were applied.

|                                  | Temperature     | Permittivity | Conductivity     |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters      | 22.0 °C         | 52.7         | 1.95 mho/m       |
| Measured Body TSL parameters     | (22.0 ± 0.2) °C | 51.7 ± 6 %   | 2.00 mho/m ± 6 % |
| Body TSL temperature during test | (21.2 ± 0.2) °C | ----         | ----             |

### SAR result with Body TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                                   |
|---|--------------------|-----------------------------------|
| SAR measured  | 250 mW input power | 13.0 mW / g                       |
| SAR normalized  | normalized to 1W   | 52.0 mW / g                       |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | <b>51.1 mW / g ± 17.0 % (k=2)</b> |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                                   |
|---|--------------------|-----------------------------------|
| SAR measured  | 250 mW input power | 5.97 mW / g                       |
| SAR normalized  | normalized to 1W   | 23.9 mW / g                       |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | <b>23.7 mW / g ± 16.5 % (k=2)</b> |

# TA Technology (Shanghai) Co., Ltd.

## Test Report

### Appendix

#### Antenna Parameters with Head TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $54.2 \Omega + 1.9 j\Omega$ |
| Return Loss                          | - 27.1 dB                   |

#### Antenna Parameters with Body TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $50.1 \Omega + 5.2 j\Omega$ |
| Return Loss                          | - 25.7 dB                   |

#### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1,144 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

|                 |               |
|-----------------|---------------|
| Manufactured by | SPEAG         |
| Manufactured on | July 05, 2002 |

**DASY5 Validation Report for Head TSL**

Date/Time: 17.02.2010 13:12:38

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:712**

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U11 BB

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.77$  mho/m;  $\epsilon_r = 38.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY5 Configuration:**

- Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 26.06.2009
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

**Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7)/Cube 0: Measurement**


grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.1 V/m; Power Drift = 0.032 dB

Peak SAR (extrapolated) = 27.2 W/kg


**SAR(1 g) = 13.3 mW/g; SAR(10 g) = 6.24 mW/g**

Maximum value of SAR (measured) = 17.1 mW/g

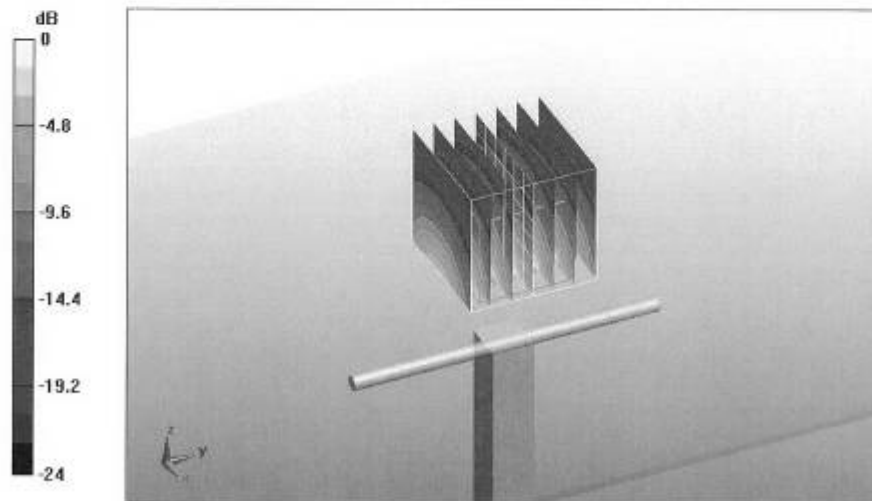

0 dB = 17.1mW/g

Impedance Measurement Plot for Head TSL

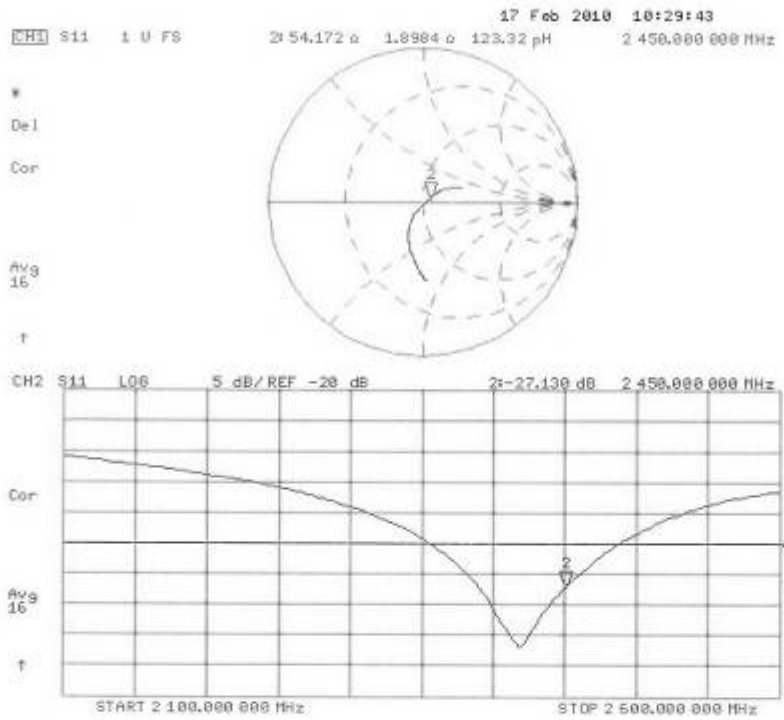

**DASY5 Validation Report for Body**

Date/Time: 19.02.2010 13:05:49

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:712**

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U10 BB

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 2.01$  mho/m;  $\epsilon_r = 51.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.31, 4.31, 4.31); Calibrated: 26.06.2009
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

**Pin250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7)/Cube 0: Measurement**


grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.5 V/m; Power Drift = 0.015 dB

Peak SAR (extrapolated) = 29.5 W/kg

**SAR(1 g) = 13 mW/g; SAR(10 g) = 5.97 mW/g**


Maximum value of SAR (measured) = 17 mW/g

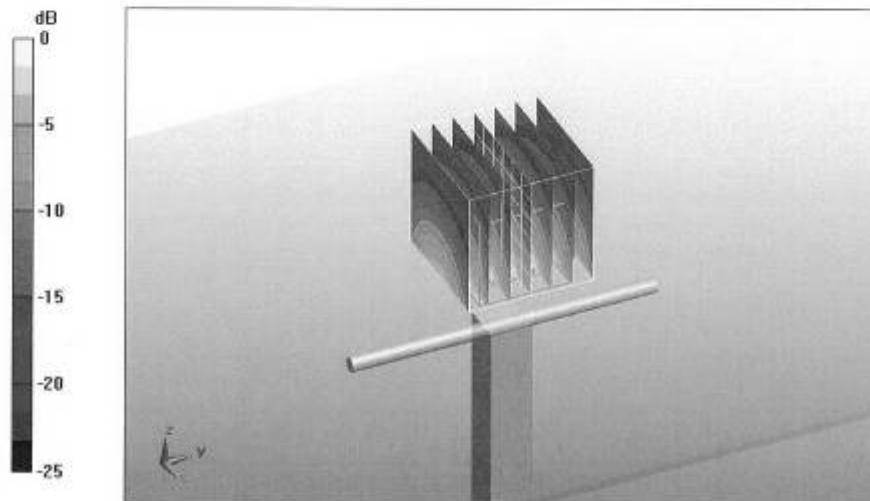

0 dB = 17mW/g



Impedance Measurement Plot for Body TSL

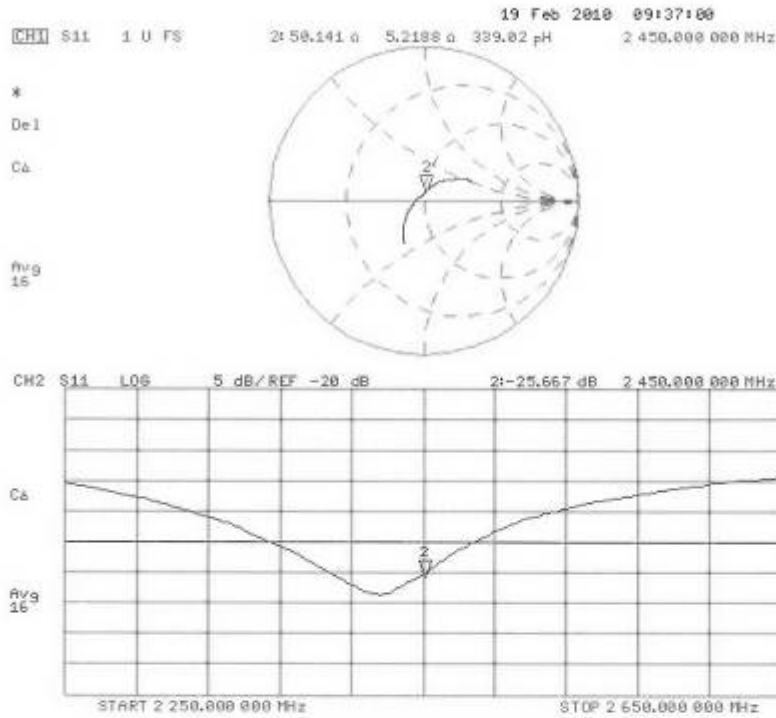

# TA Technology (Shanghai) Co., Ltd. Test Report

Report No. RZA1011-1731SAR

Page 58 of 65

## ANNEX F: DAE4 Calibration Certificate

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **TA - SH (Auden)**

Certificate No: **DAE4-871\_Nov09**

### CALIBRATION CERTIFICATE

Object: **DAE4 - SD 000 D04 BJ - SN: 871**

Calibration procedure(s): **QA CAL-06.v12  
Calibration procedure for the data acquisition electronics (DAE)**

Calibration date: **November 11, 2009**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards             | ID #               | Cal Date (Certificate No.) | Scheduled Calibration  |
|-------------------------------|--------------------|----------------------------|------------------------|
| Keithley Multimeter Type 2001 | SN: 081027B        | 1-Oct-09 (No: 9055)        | Oct-10                 |
| Secondary Standards           | ID #               | Check Date (in house)      | Scheduled Check        |
| Calibrator Box V1.1           | SE UMS 006 AB 1004 | 05-Jun-09 (in house check) | In house check: Jun-10 |

|                |                              |                                     |               |
|----------------|------------------------------|-------------------------------------|---------------|
| Calibrated by: | Name<br><b>Andrea Guntli</b> | Function<br><b>Technician</b>       | Signature<br> |
| Approved by:   | Name<br><b>Fin Bomholt</b>   | Function<br><b>R&amp;D Director</b> | Signature<br> |

Issued: November 11, 2009

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary

**DAE** data acquisition electronics  
**Connector angle** information used in DASY system to align probe sensor X to the robot coordinate system.

### Methods Applied and Interpretation of Parameters

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - **DC Voltage Measurement Linearity:** Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - **Common mode sensitivity:** Influence of a positive or negative common mode voltage on the differential measurement.
  - **Channel separation:** Influence of a voltage on the neighbor channels not subject to an input voltage.
  - **AD Converter Values with inputs shorted:** Values on the internal AD converter corresponding to zero input voltage
  - **Input Offset Measurement:** Output voltage and statistical results over a large number of zero voltage measurements.
  - **Input Offset Current:** Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - **Input resistance:** DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - **Low Battery Alarm Voltage:** Typical value for information. Below this voltage, a battery alarm signal is generated.
  - **Power consumption:** Typical value for information. Supply currents in various operating modes.

**TA Technology (Shanghai) Co., Ltd.**  
**Test Report**

**DC Voltage Measurement**

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 $\mu$ V , full range = -100...+300 mV

Low Range: 1LSB = 61nV , full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X                        | Y                        | Z                        |
|---------------------|--------------------------|--------------------------|--------------------------|
| High Range          | 404.813 $\pm$ 0.1% (k=2) | 404.794 $\pm$ 0.1% (k=2) | 405.237 $\pm$ 0.1% (k=2) |
| Low Range           | 3.98191 $\pm$ 0.7% (k=2) | 3.98417 $\pm$ 0.7% (k=2) | 3.98912 $\pm$ 0.7% (k=2) |

**Connector Angle**

|   |                                    |
|---|------------------------------------|
| Connector Angle to be used in DASY system | 90.0 $^{\circ}$ $\pm$ 1 $^{\circ}$ |
|---|------------------------------------|

# TA Technology (Shanghai) Co., Ltd.

## Test Report

### Appendix

#### 1. DC Voltage Linearity

| High Range        | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-------------------|---------------------------|------------------------------|-----------|
| Channel X + Input | 199994.0                  | 1.84                         | 0.00      |
| Channel X + Input | 19999.85                  | 0.05                         | 0.00      |
| Channel X - Input | -19997.97                 | 1.83                         | -0.01     |
| Channel Y + Input | 200010.3                  | -3.71                        | -0.00     |
| Channel Y + Input | 19999.12                  | -0.48                        | -0.00     |
| Channel Y - Input | -20000.18                 | -0.78                        | 0.00      |
| Channel Z + Input | 200010.2                  | -2.80                        | -0.00     |
| Channel Z + Input | 19998.54                  | -0.86                        | -0.00     |
| Channel Z - Input | -19999.82                 | 0.00                         | 0.00      |

| Low Range         | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-------------------|---------------------------|------------------------------|-----------|
| Channel X + Input | 2000.3                    | 0.22                         | 0.01      |
| Channel X + Input | 200.20                    | 0.30                         | 0.15      |
| Channel X - Input | -199.89                   | 0.21                         | -0.10     |
| Channel Y + Input | 1999.8                    | -0.13                        | -0.01     |
| Channel Y + Input | 200.06                    | -0.04                        | -0.02     |
| Channel Y - Input | -200.43                   | -0.73                        | 0.36      |
| Channel Z + Input | 1999.5                    | -0.57                        | -0.03     |
| Channel Z + Input | 199.58                    | -0.72                        | -0.36     |
| Channel Z - Input | -201.11                   | -1.01                        | 0.51      |

#### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Common mode Input Voltage (mV) | High Range Average Reading ( $\mu\text{V}$ ) | Low Range Average Reading ( $\mu\text{V}$ ) |
|-----------|--------------------------------|--|---|
| Channel X | 200                            | 13.79  | 12.75                                       |
|           | - 200                          | -12.26                                       | -13.72                                      |
| Channel Y | 200                            | -11.82                                       | -11.47                                      |
|           | - 200                          | 10.67  | 10.68                                       |
| Channel Z | 200                            | -1.08  | -1.35                                       |
|           | - 200                          | 0.32   | 0.12  |

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Input Voltage (mV) | Channel X ( $\mu\text{V}$ ) | Channel Y ( $\mu\text{V}$ ) | Channel Z ( $\mu\text{V}$ ) |
|-----------|--------------------|-----------------------------|-----------------------------|-----------------------------|
| Channel X | 200                | -                           | 3.36                        | 1.06                        |
| Channel Y | 200                | 1.52                        | -                           | 3.59                        |
| Channel Z | 200                | 2.55                        | 1.41                        | -                           |

# TA Technology (Shanghai) Co., Ltd.

## Test Report

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 15928            | 16288           |
| Channel Y | 16188            | 15745           |
| Channel Z | 15790            | 16219           |

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

|           | Average ( $\mu$ V) | min. Offset ( $\mu$ V) | max. Offset ( $\mu$ V) | Std. Deviation ( $\mu$ V) |
|-----------|--------------------|------------------------|------------------------|---------------------------|
| Channel X | 0.06               | -3.43                  | 1.18                   | 0.52                      |
| Channel Y | -0.71              | -2.66                  | 0.96                   | 0.57                      |
| Channel Z | -0.95              | -1.94                  | 0.04                   | 0.41                      |

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance

|           | Zeroing (MOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 0.1999         | 204.4            |
| Channel Y | 0.1999         | 203.6            |
| Channel Z | 0.1999         | 203.8            |

#### 8. Low Battery Alarm Voltage (verified during pre test)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9              |
| Supply (- Vcc) | -7.6              |

#### 9. Power Consumption (verified during pre test)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.0              | +6            | +14               |
| Supply (- Vcc) | -0.01             | -8            | -9                |

**ANNEX G: The EUT Appearances and Test Configuration**



Picture 4: Constituents of the EUT




Picture 5: Test position 1



Picture 6: Test position 2



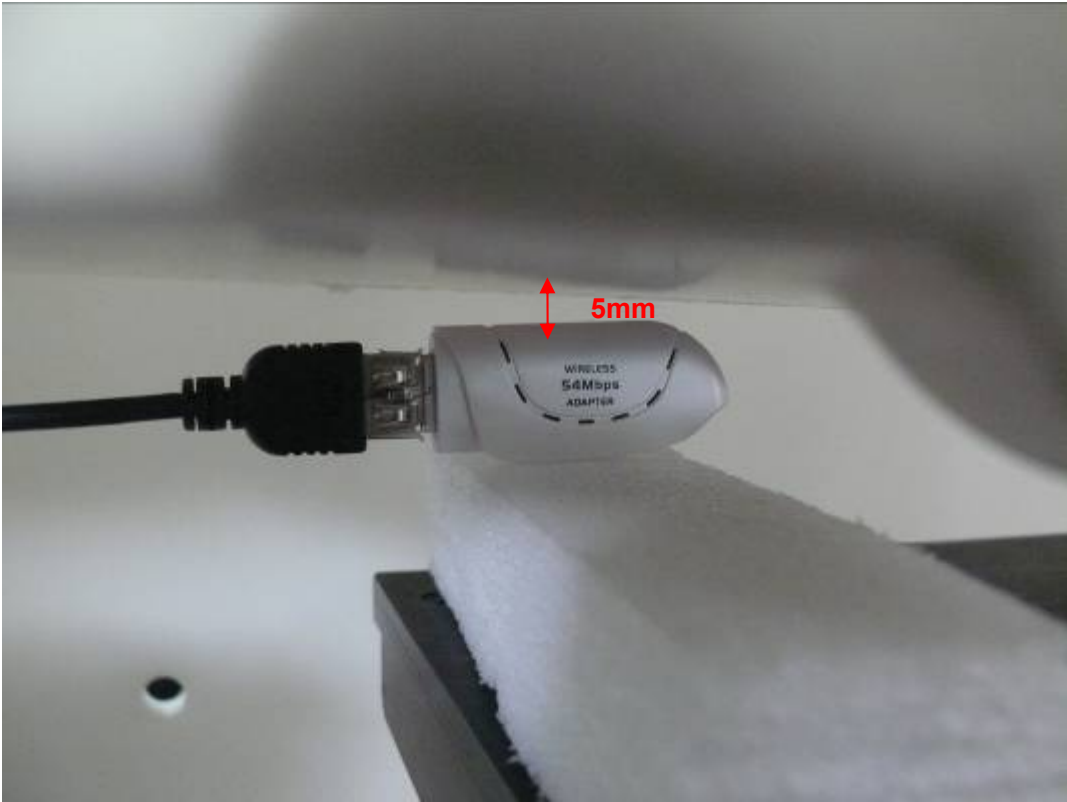

Picture 7: Test Position 3



Picture 8: Test Position 4

Remark: This six model devices have the some software and hardware version, and noly the change of the housing, colour, via the validation, the white model that have been tested is the worst case.