



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Code of Federal Regulations 47 Part 15 – Radio Frequency Devices

Subpart F – Ultra-Wideband Operation

Section 15.519

Technical Requirements for hand held UWB systems

THE FOLLOWING **MEETS** THE ABOVE TEST SPECIFICATION

Formal Name: URP Radio Board

Kind of Equipment: UWB Radio

FCC ID Number: YYJ-5406102

Frequency Range: 3168 - 4752 MHz, 6336 – 7920 MHz

Test Configuration: Hand-held transceiver tested table-top in worst case configuration of three orthogonal planes.

Model Number(s): 5436008 rev3, 5436008-2 rev1

Model(s) Tested: 5436008-2 rev1

Serial Number(s): 11100098

Date of Tests: May 23 – 27, 2011

Test Conducted For: GE Medical Systems, LLC
3000 N. Grandview Blvd
Mailstop W622
Waukesha, WI 53188

NOTICE: “This test report relates only to the items tested and must not be used by the client to claim product endorsement by NVLAP or any agency of the U.S. Government”. Please see the "Description of Test Sample" page listed inside of this report.

© Copyright 1983 - 2011 D.L.S. Electronic Systems, Inc.

COPYRIGHT NOTICE

This report must not be reproduced (except in full), without the approval of D.L.S. Electronic Systems, Inc.



166 South Carter, Genoa City, WI 53128

Company:
Model Tested:
Report Number:
Project Number:

GE Medical Systems, LLC
5436008-2 rev1
17001
4679

SIGNATURE PAGE

Report By:

A handwritten signature in black ink that reads "Adam D. Alger". The signature is fluid and cursive.

Adam Alger
Test Engineer
June 20, 2011

Reviewed By:

A handwritten signature in black ink that reads "William Stumpf". The signature is fluid and cursive.

William Stumpf
OATS Manager

Approved By:

A handwritten signature in black ink that reads "Brian J. Mattson". The signature is fluid and cursive.

Brian Mattson
General Manager



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Table of Contents

i. Cover Page1
ii. Signature Page2
iii. Table of Contents3
iv. NVLAP Certificate of Accreditation4
1.0 Summary of Test Report5
2.0 Introduction5
3.0 Test Facilities5
4.0 Description of Test Sample6
5.0 Test Equipment7
6.0 Test Arrangements8
7.0 Test Conditions8
8.0 Modifications Made To EUT For Compliance8
9.0 Additional Descriptions9
10.0 Results9
11.0 Conclusion9
Appendix A – Test Photos10
Appendix B – Measurement Data19
1.0 Fundamental Emission Bandwidth – 10 dB 19
2.0 Radiated Spurious Emissions below 960 MHz 26
3.0 Radiated / RF Conducted Spurious Emissions above 960 MHz 27
4.0 Radiated Fundamental Emissions in band 3100 to 10600 MHz 34
5.0 Radiated Spurious Emissions in GPS Band 37



166 South Carter, Genoa City, WI 53128

Company:
Model Tested:
Report Number:
Project Number:

GE Medical Systems, LLC
5436008-2 rev1
17001
4679

United States Department of Commerce
National Institute of Standards and Technology



Certificate of Accreditation to ISO/IEC 17025:2005

NVLAP LAB CODE: 100276-0

D.L.S. Electronic Systems, Inc.
Wheeling, IL

is accredited by the National Voluntary Laboratory Accreditation Program for specific services,
listed on the Scope of Accreditation, for:

ELECTROMAGNETIC COMPATIBILITY AND TELECOMMUNICATIONS

This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2005.
This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality
management system (refer to joint ISO-IAC-IAF Communiqué dated January 2009).



2010-10-01 through 2011-09-30

Effective dates

Jolly A. Buce
For the National Institute of Standards and Technology

NVLAP-01C (REV. 2009-01-28)



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
 Model Tested: 5436008-2 rev 1
 Report Number: 17001
 Project Number: 4679

1.0 Summary of Test Report

It was determined that the GE Medical Systems, LLC URP Radio Board, Model 5436008-2 rev 1, complies with the requirements of CFR 47 Part 15 Subpart F Section 15.519.

Subpart F Applicable Technical Requirements Tested:

Section	Description	Procedure	Note	Compliant?
15.519 (b)	Fundamental Emission Bandwidth – 10dB	ANSI C63.4-2009 & ANSI C63.10-2009	1	Yes
15.519 (c) / 15.209	Radiated Spurious Emissions below 960 MHz	ANSI C63.4-2009 & ANSI C63.10-2009	1	Yes
15.519 (c)	Radiated / RF Conducted Spurious Emissions above 960 MHz	ANSI C63.4-2009 & ANSI C63.10-2009	1,2	Yes
15.519 (c) & (e)	Radiated Fundamental Emissions in band 3100 to 10600 MHz	ANSI C63.4-2009 & ANSI C63.10-2009	1	Yes
15.519 (d)	Radiated Spurious Emissions in GPS band	ANSI C63.4-2009 & ANSI C63.10-2009	1	Yes

Note 1: Radiated emission measurement tested in 3 orthogonal planes.

Note 2: RF antenna port conducted emissions.

2.0 Introduction

On May 23 – 27, 2011 the URP Radio Board, Model 5436008-2 rev 1, as provided from GE Medical Systems, LLC was tested to the requirements of CFR 47 Part 15 Subpart C Section 15.519. To meet these requirements, the procedures contained within this report were performed by personnel of D.L.S Electronic Systems, Inc.

3.0 Test Facilities

D.L.S. Electronic Systems, Inc. is a full service EMC/Safety Testing Laboratory accredited to ISO 17025. NVLAP Certificate and Scope can be viewed at <http://www.dlsemc.com/certificate>. Our facilities are registered with the FCC, Industry Canada, and VCCI.

Wisconsin Test Facility:

D.L.S. Electronic Systems, Inc.
 166 S. Carter Street
 Genoa City, Wisconsin 53128

Wheeling Test Facility:

D.L.S. Electronic Systems, Inc.
 1250 Peterson Drive
 Wheeling, IL 60090



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

4.0 Description of Test Sample

Description:

URP Radio Board acts like a Wireless USB Device using the UWB protocol. The device is used to transfer large medical images.

Type of Equipment / Frequency Range:

Handheld / MHz

Band Group	Band ID	Lower Frequency	Center Frequency	Upper Frequency
1	1	3168	3432	3696
	2	3696	3960	4224
	3	4224	4488	4752
3	7	6336	6600	6864
	8	6864	7128	7392
	9	7392	7656	7920

Physical Dimensions of Equipment Under Test:

Length: 62 mm x Width: 91 mm x Height:10 mm

Power Source:

USB powered (5 VDC)

Internal Frequencies:

66 MHz

Type of Modulation(s) / Antenna Type:

QPSK, DCM / Mitsumi Isotropic Ceramic Chip Antenna DCA-E05

Description of Circuit Board(s) / Part Number:

URP Radio Board	5436008-2 rev 1
URP Radio Board	5436008-2 rev 2
URP Radio Board	5436008-3 rev 1



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
 Model Tested: 5436008-2 rev1
 Report Number: 17001
 Project Number: 4679

5.0 Test Equipment

A list of the equipment used can be found in the table below. All primary equipment was calibrated against known reference standards with a verified traceable path to NIST.

D.L.S. Wisconsin –Site 3 / G1

Description	Manufacturer	Model Number	Serial Number	Frequency Range	Cal Dates	Cal Due Dates
G1 Emissions 30-1000 MHz						
Receiver	Rohde & Schwarz	ESI 40	837808/005	20 Hz – 40 GHz	7/10	7/11
Preamplifier	Rohde & Schwarz	TS-PR10	032001/003	9 kHz – 1 GHz	1/11	1/12
Antenna	EMCO	3104C	9810-4849	20 MHz – 200 MHz	2/10	2/12
Antenna	EMCO	3146	1604	200 MHz – 1 GHz	8/10	8/12
Site 3 Emissions – 1-40 GHz						
Receiver	Rohde & Schwarz	ESI 40	837808/005	20 Hz – 40 GHz	7/10	7/11
Preamp	Ciao	CA118-4010	101	1GHz-18GHz	1/11	1/12
Horn Antenna	EMCO	3115	9903-5731	1-18GHz	6/09	6/11
Signal Generator	Rhode & Schwarz	SMR40	100092	1-40 GHz	1/11	1/12
Horn Antenna	EMCO	3115	9502-4451	1-18GHz	4/11	4/13
Preamp	Miteq	AMF-8B-180265-40-10P-H/S	438727	18GHz-26GHz	8/10	8/11
Horn Antenna	EMCO	3116	2549	18 – 40GHz	8/10	8/11
Preamp	R&S	TS-PR40	052002/025	26GHz-40GHz	8/10	8/11
Receiver	Rohde & Schwarz	ESI 40	837808/005	20 Hz – 40 GHz	7/10	7/11
Preamp	Ciao	CA118-4010	101	1GHz-18GHz	1/11	1/12
Horn Antenna	EMCO	3115	9903-5731	1-18GHz	6/09	6/11



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

6.0 Test Arrangements

Emissions Measurement Arrangement:

All emissions measurements were performed at D.L.S. Electronic Systems, Inc. and set up according to ANSI C63.4-2009 and ANSI C63.10-2009, unless otherwise noted. Description of procedures and measurements can be found in Appendix B – Measurement Data. See Appendix A for additional photos of the test set up.

Unless otherwise noted, the bandwidth of the measuring receiver / analyzer used during testing is shown below.

Frequency Range	Bandwidth (-6 dB)
10 to 150 kHz	200 Hz
150 kHz to 30 MHz	9 kHz
30 MHz to 1 GHz	120 kHz
Above 1 GHz	1 MHz

7.0 Test Conditions

Test Conditions recorded during test:

Temperature and Humidity:

65°F at 25% RH

8.0 Modifications Made To EUT For Compliance

None noted at time of test.



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

9.0 Additional Descriptions

The client has been informed of the operational limits defined in FCC 47 CFR Section 15.519 (a).

AC Mains Line conducted was not performed because the the UWB radio is powered by a PC USB port.

Using a PC with proprietary software, the UWB radio was connected through a USB cable and configured for continuous transmit. The software allowed the user to configure the radio settings to achieve compliant levels and determine worst case data rate settings.

TX Rate: 53
TX Payload: 4095
TX IFS: 10 us

Final Transmitter Power Settings:

Band Group 1			
	TFC 5	TFC 6	TFC 7
TPC	3	4	4
C1	20	30	20
C2	05		

Band Group 3			
	TFC 5	TFC 6	TFC 7
TPC	6	7	4
D1	01		
D2	01		

10.0 Results

Measurements were performed in accordance with ANSI C63.4-2009 and ANSI C63.10-2009. Graphical and tabular data can be found in Appendix B at the end of this report.

11.0 Conclusion

The URP Radio Board, Model 5436008-2 rev 1, as provided from GE Medical Systems, LLC tested on May 23 - 27, 2011 **meets** the requirements of CFR 47 Part 15 Subpart F Section 15.519.



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Appendix A – Test Photos

Photo Information and Test Setup:


Items: URP Radio Board 5436008-2 rev 1
Antenna: Mitsumi Isotropic Ceramic Chip Antenna DCA-E05
20 meter USB cable with ferrites

Radiated Emissions – Y – Worst Case Position




Appendix A

Radiated Emissions – Y Position

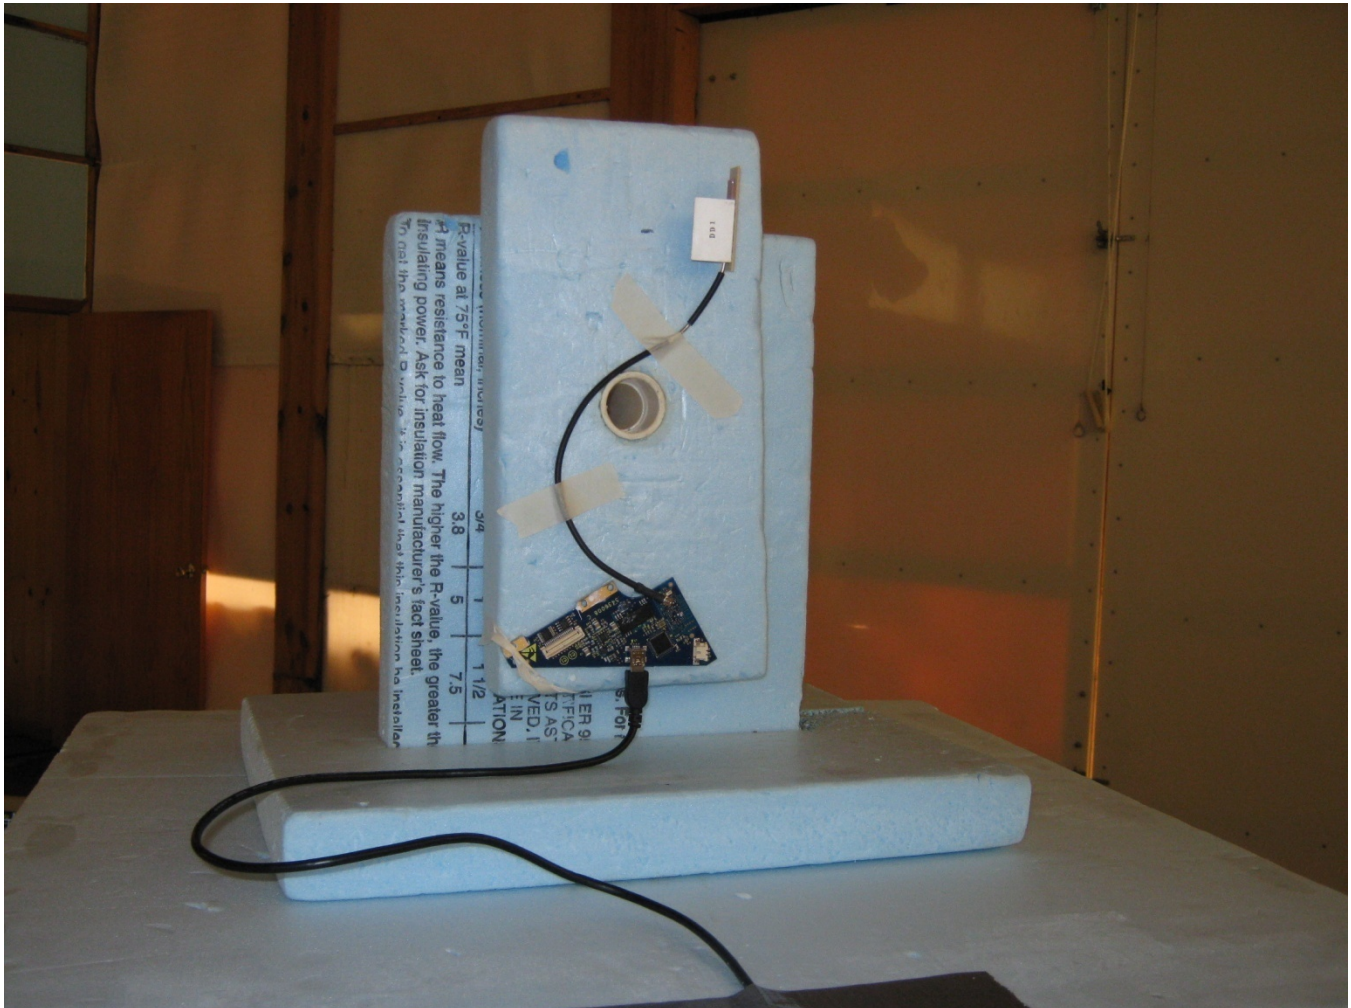

Appendix A

Radiated Emissions – Y Position

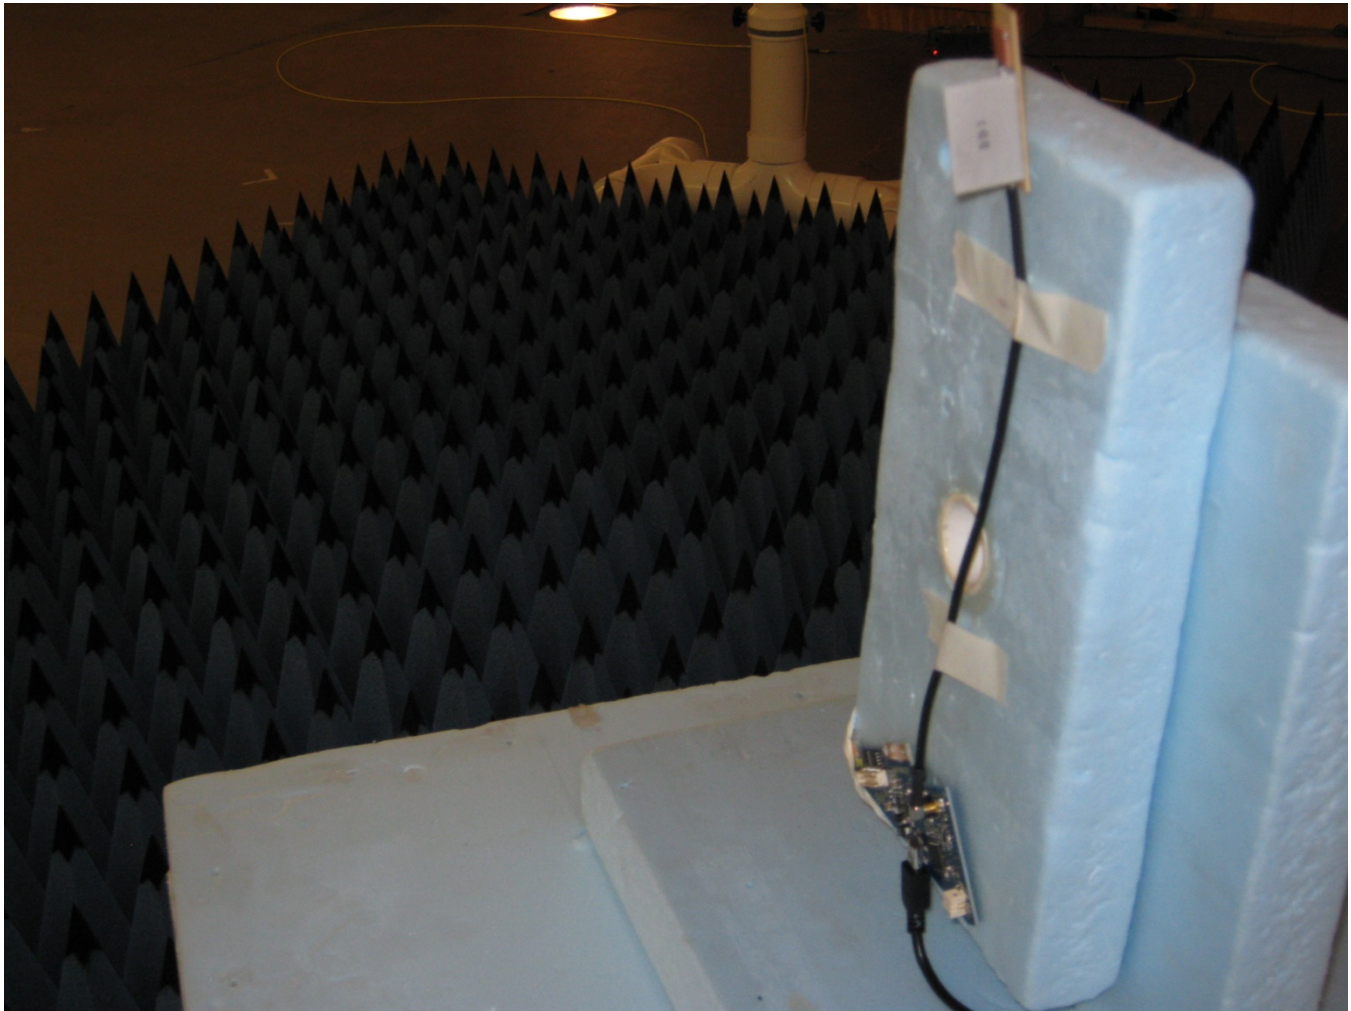




166 South Carter, Genoa City, WI 53128

Company:
Model Tested:
Report Number:
Project Number:

GE Medical Systems, LLC
5436008-2 rev1
17001
4679


Appendix A

Radiated Emissions – Y Position

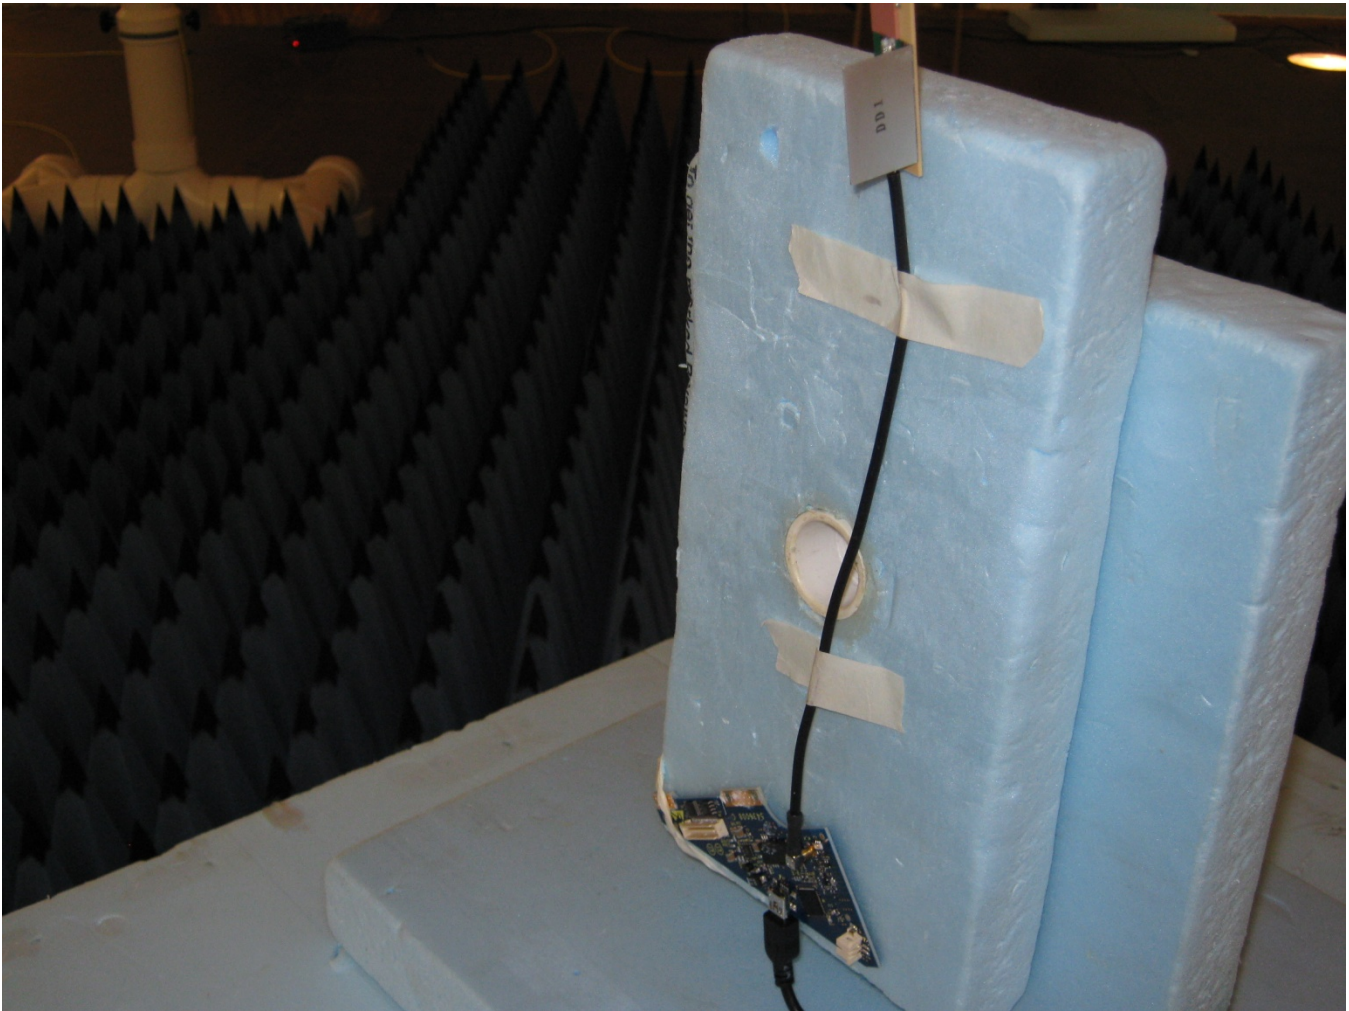


Appendix A

Radiated Emissions – Y Position

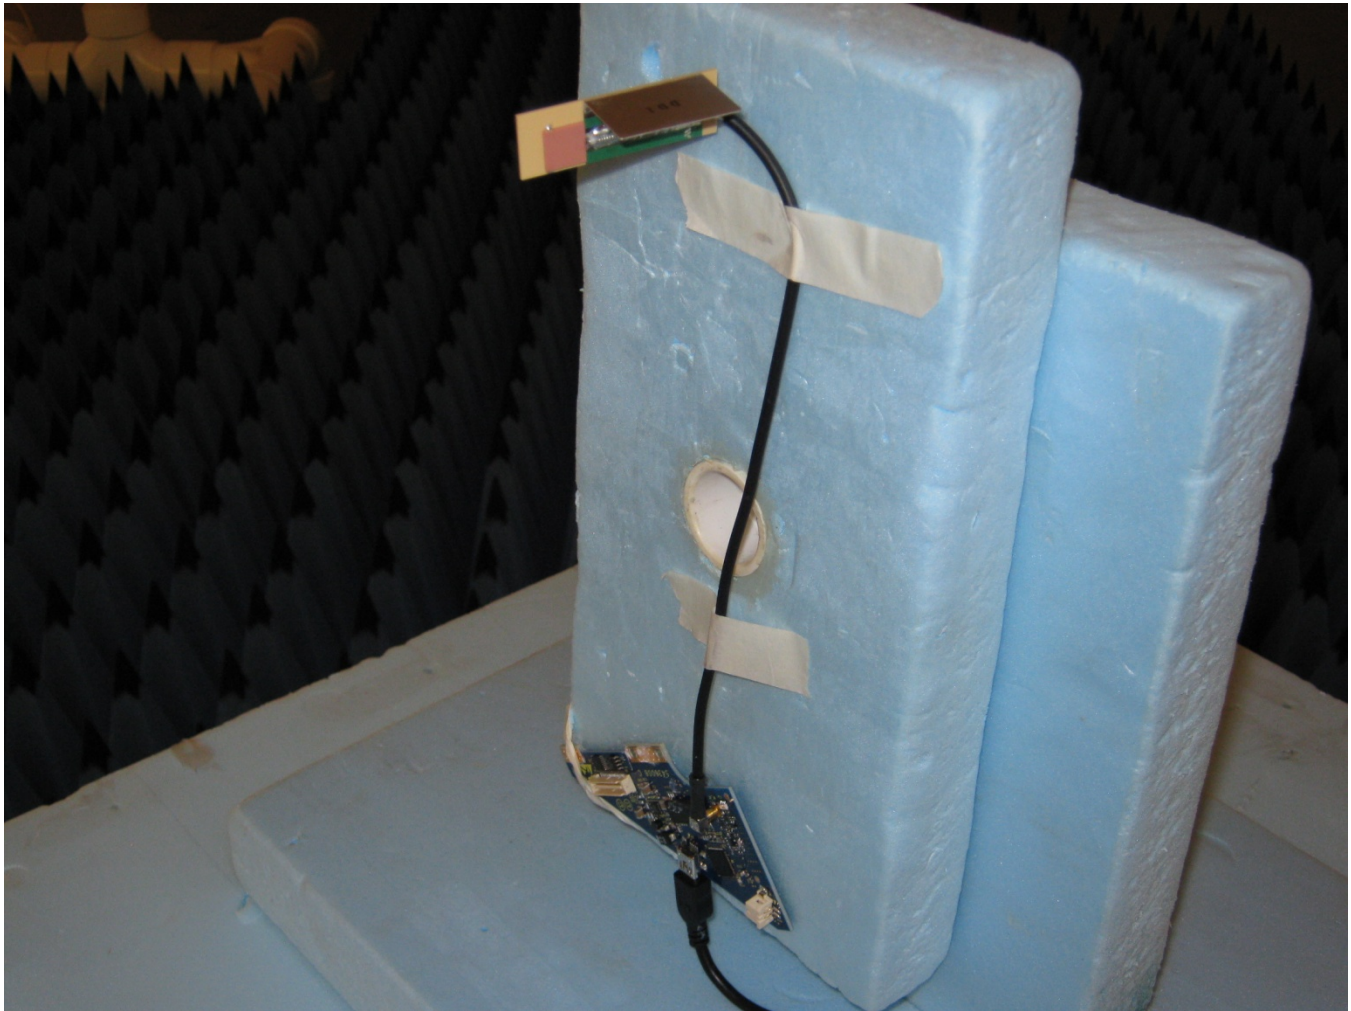


Appendix A

Radiated Emissions – Z Position

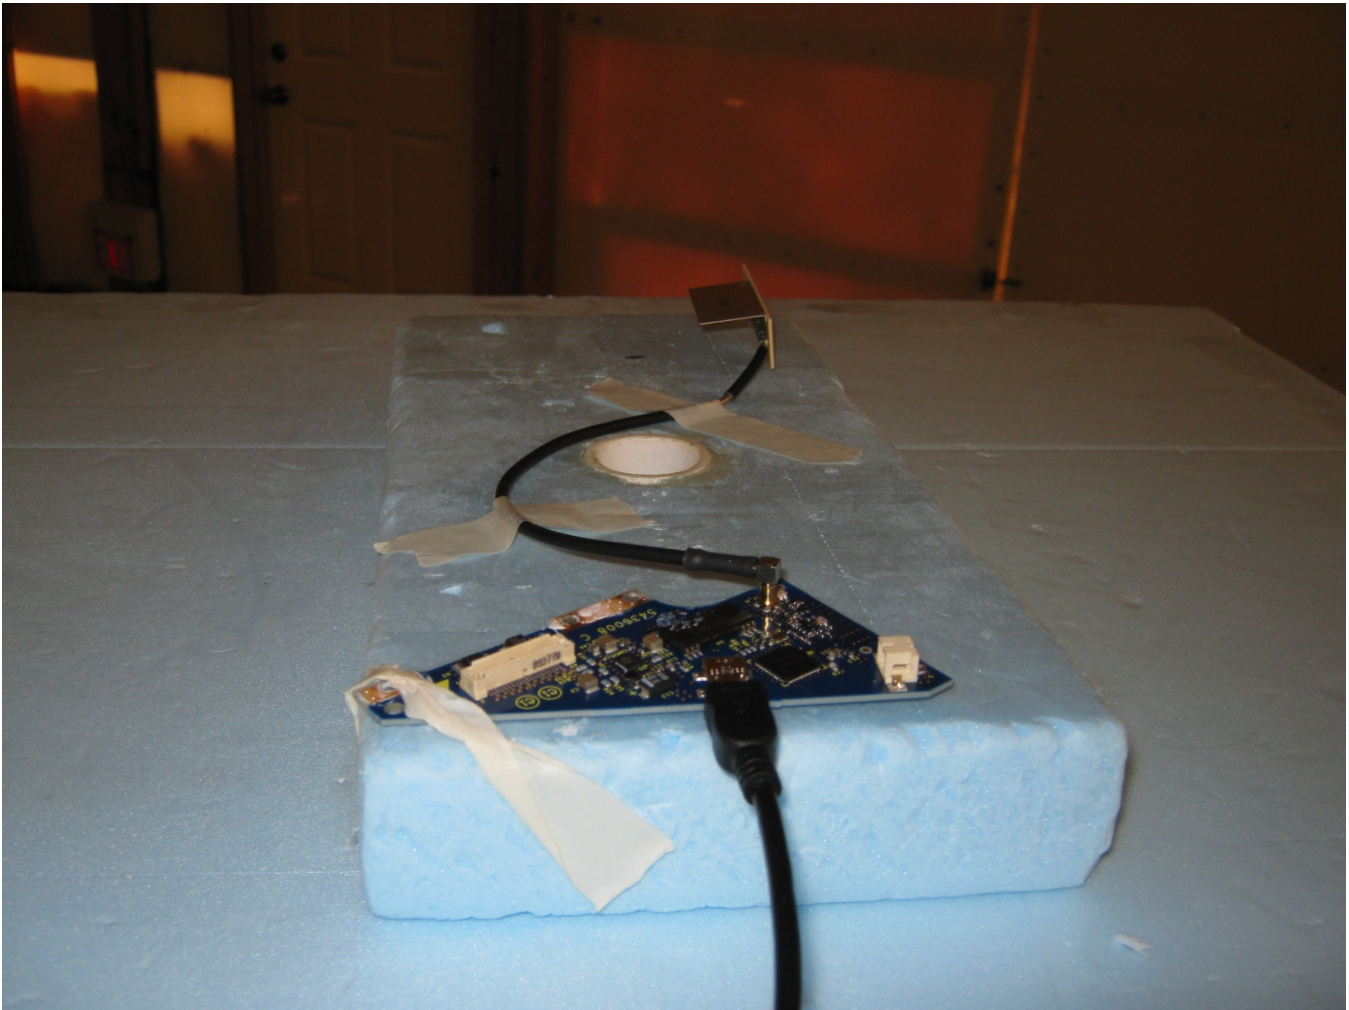


Appendix A

Radiated Emissions – Z Position

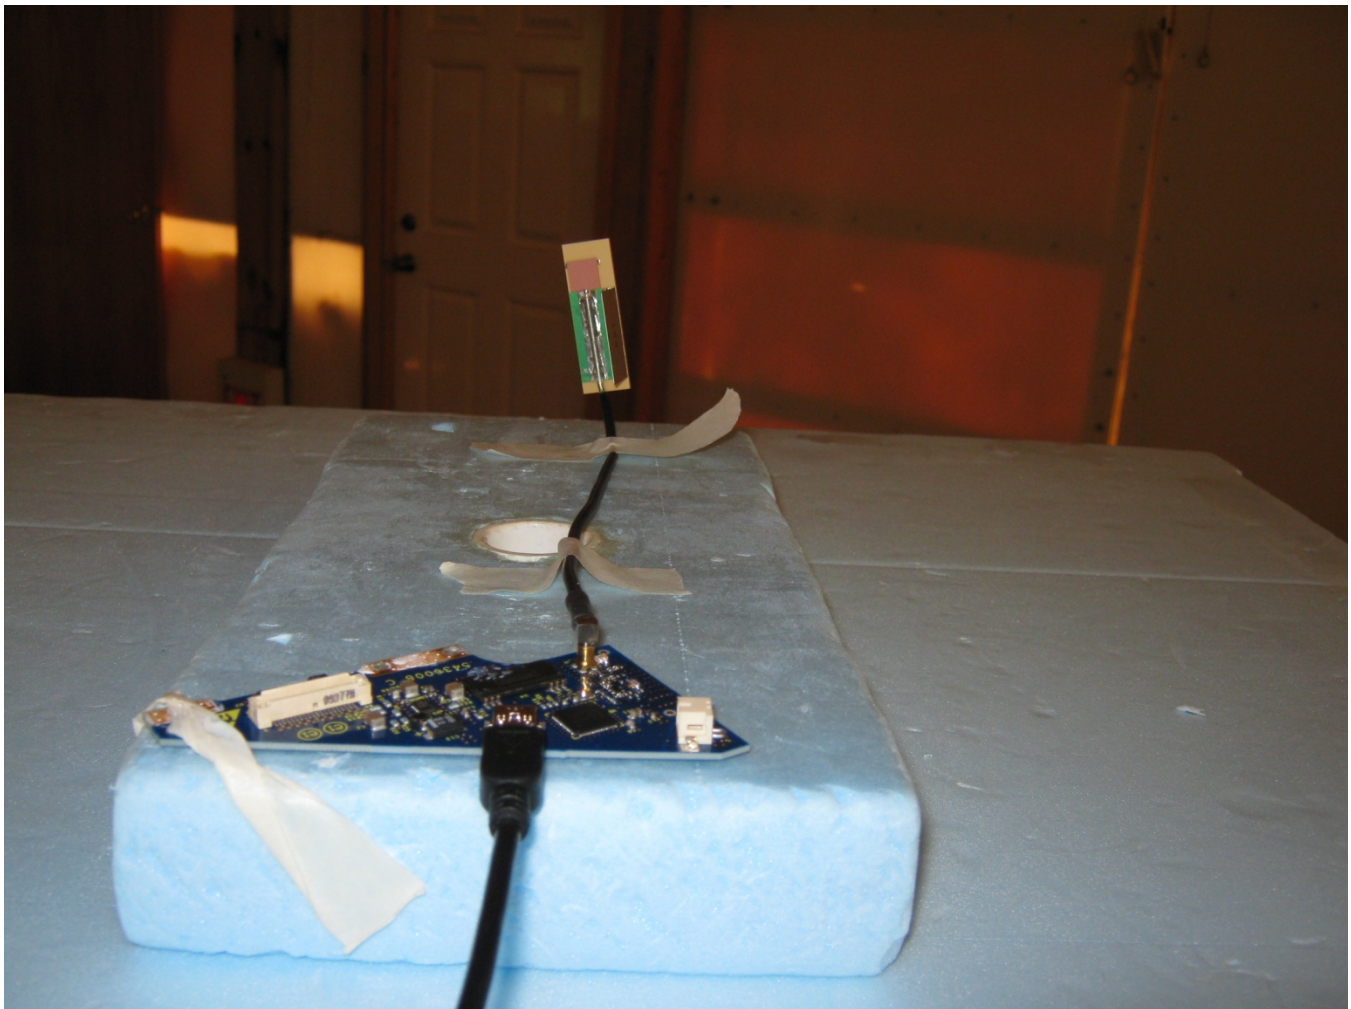

Appendix A

Radiated Emissions – X Position

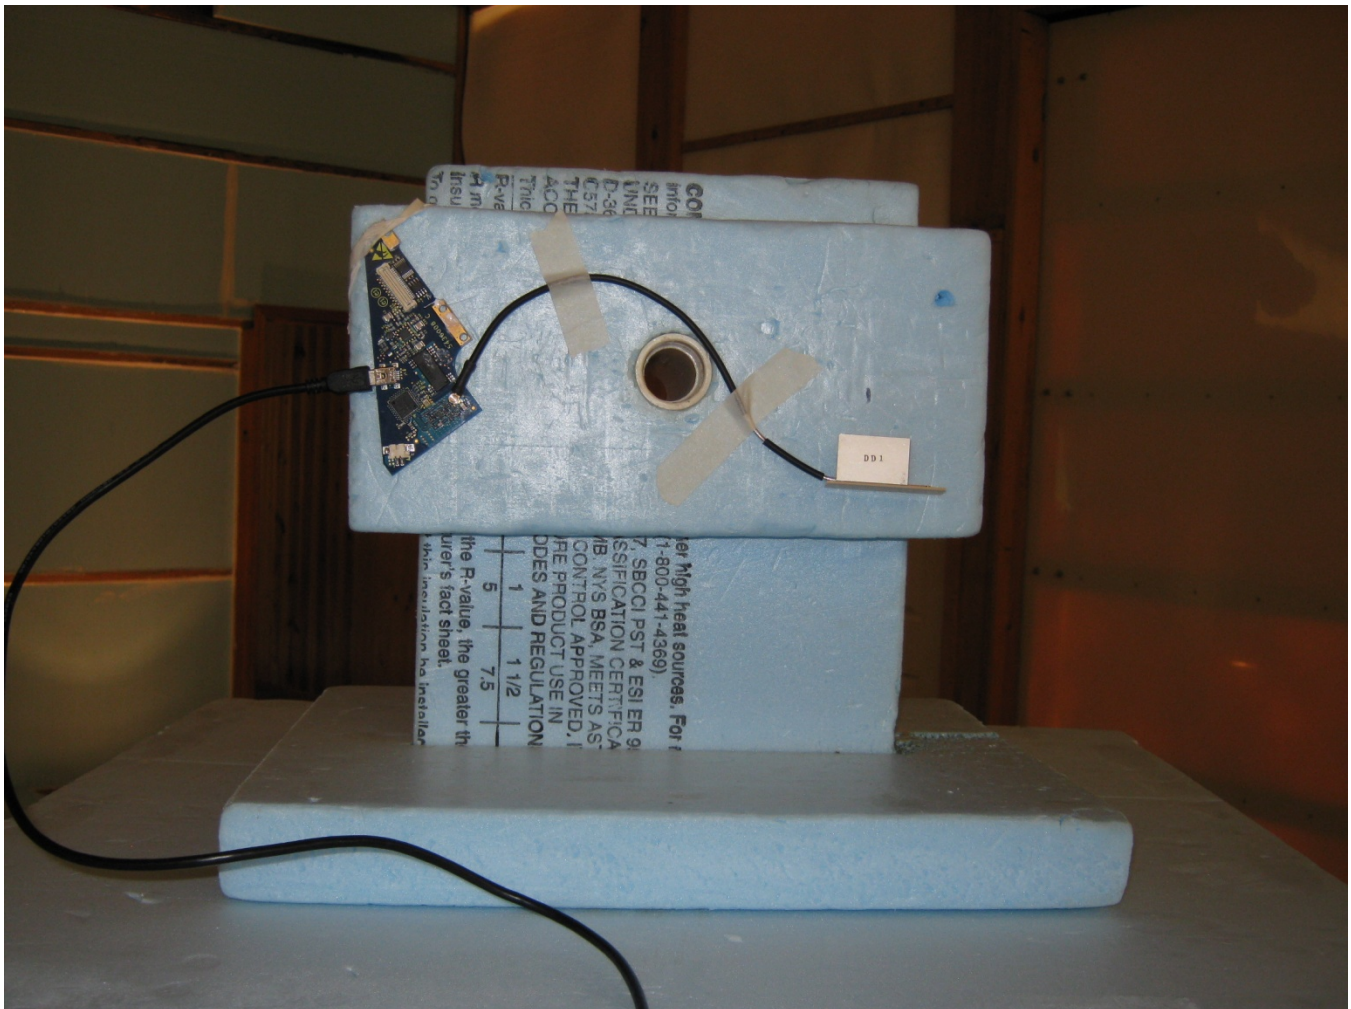



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Appendix B – Measurement Data

1.0 Fundamental Emission Bandwidth – 10 dB

Rule Part:

Section 15.519 (b)

Test Procedure:

ANSI C63.4-2009 and ANSI C63.10-2009

Limit:

Contained between 3100 MHz and 10,600 MHz

Results:

Compliant:

Band ID	10 dB bandwidth
1	510.3 MHz
2	510.3 MHz
3	509.2 MHz
7	510.3 MHz
8	510.3 MHz
9	512.5 MHz

Sample Equation(s):

None

Notes:

This was a radiated emissions measurement. The maximum field strength of the emission was determined and the bandwidth was measured from the points at 10 dB down from the highest radiated emission, as based on the complete transmission system including the antenna.




166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
 Model Tested: 5436008-2 rev1
 Report Number: 17001
 Project Number: 4679

Band Group 1
 Band # 1



Ref Lvl	Marker 1 [T1 ndB]	RBW	1 MHz	RF Att	10 dB
87 dB*	ndB 10.00 dB	VBW	3 MHz		
	BW 510.32064128 MHz	SWT	500 ms	Unit	dBµV/m

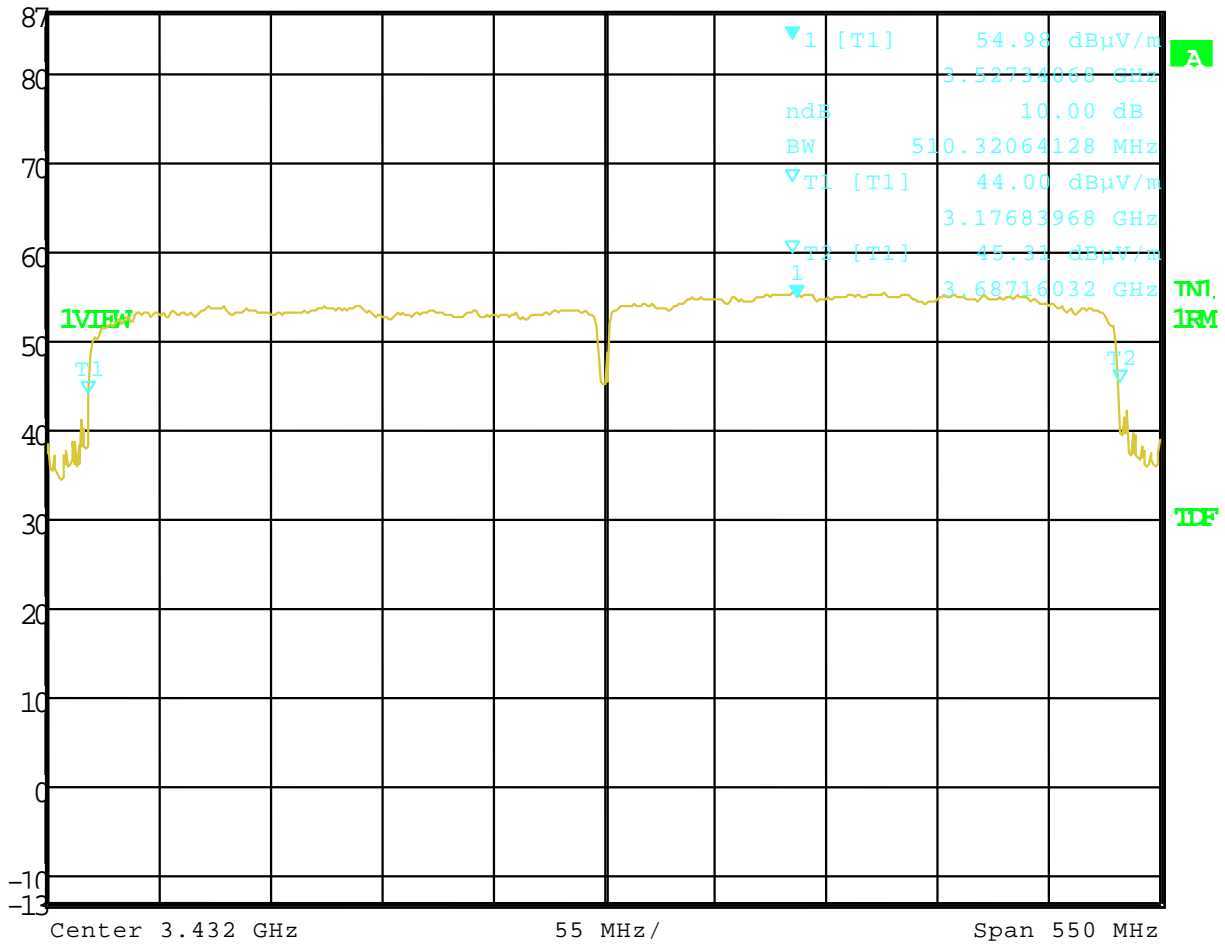

Date: 23.MAY.2011 13:27:42




166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
 Model Tested: 5436008-2 rev1
 Report Number: 17001
 Project Number: 4679

Band Group 1
 Band # 2



Delta 1 [T1] RBW 1 MHz RF Att 10 dB
 Ref Lvl 0.99 dB VBW 3 MHz
 87 dB* 510.32064128 MHz SWT 500 ms Unit dBμV/m

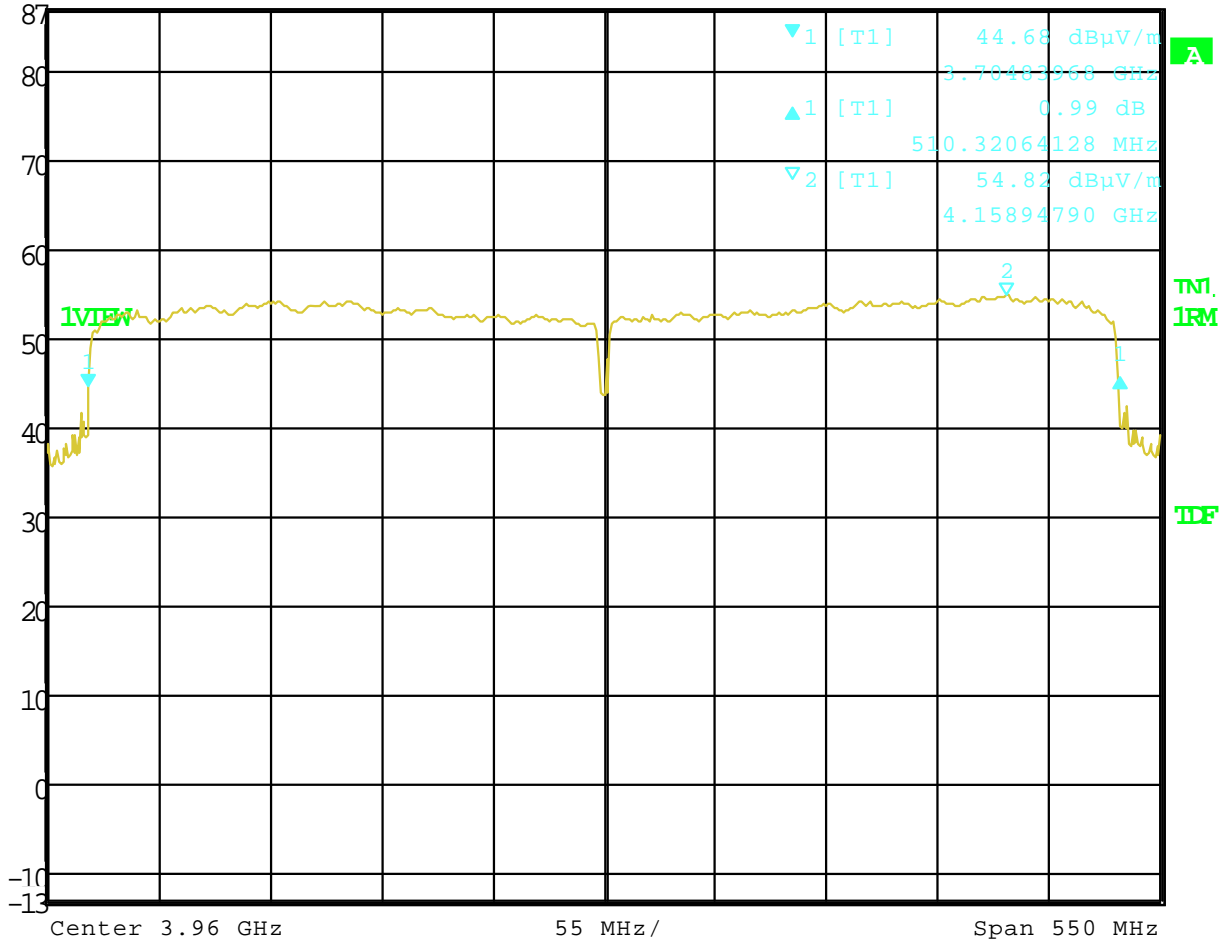

Date: 23.MAY.2011 13:40:19




166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
 Model Tested: 5436008-2 rev1
 Report Number: 17001
 Project Number: 4679

Band Group 1
 Band # 3



Ref Lvl	87 dB*	Marker 1 [T1 ndB]	ndB	10.00 dB	RBW	1 MHz	RF Att	10 dB	
		BW	509.21843687 MHz	VBW	3 MHz	SWT	500 ms	Unit	dBµV/m

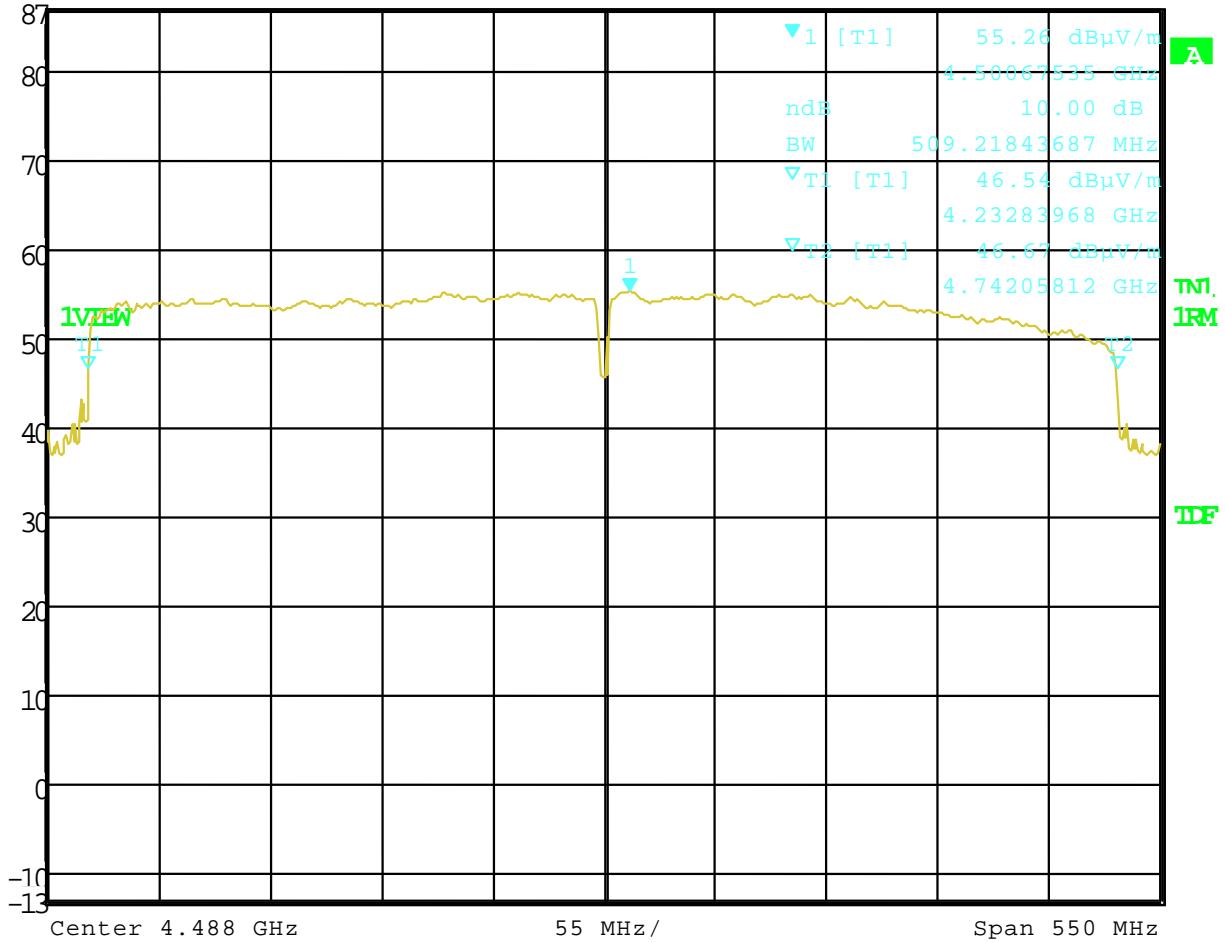

Date: 23.MAY.2011 13:49:10




166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Band Group 3
Band # 9



Ref Lvl	87 dB*	Marker 1 [T1 ndB]	ndB	10.00 dB	RBW	1 MHz	RF Att	10 dB	
		BW	512.52505010 MHz	VBW	3 MHz	SWT	500 ms	Unit	dBµV/m

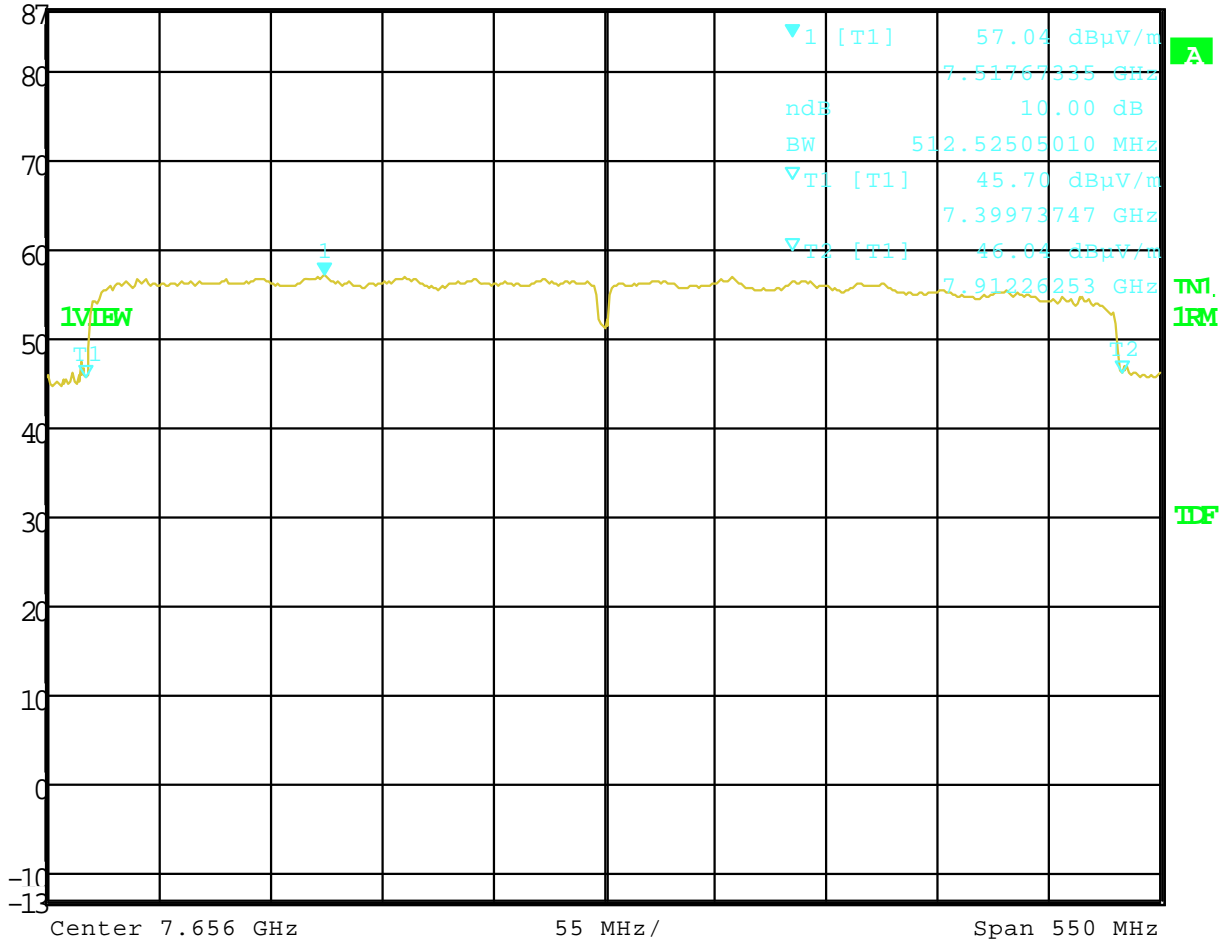

Date: 23.MAY.2011 12:24:41



166 South Carter, Genoa City, WI 53128


Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Band Group 3

Band # 8



Ref Lvl	Marker 1 [T1 ndB]	RBW	1 MHz	RF Att	10 dB
87 dB*	ndB 10.00 dB	VBW	3 MHz		
	BW 510.32064128 MHz	SWT	500 ms	Unit	dBµV/m

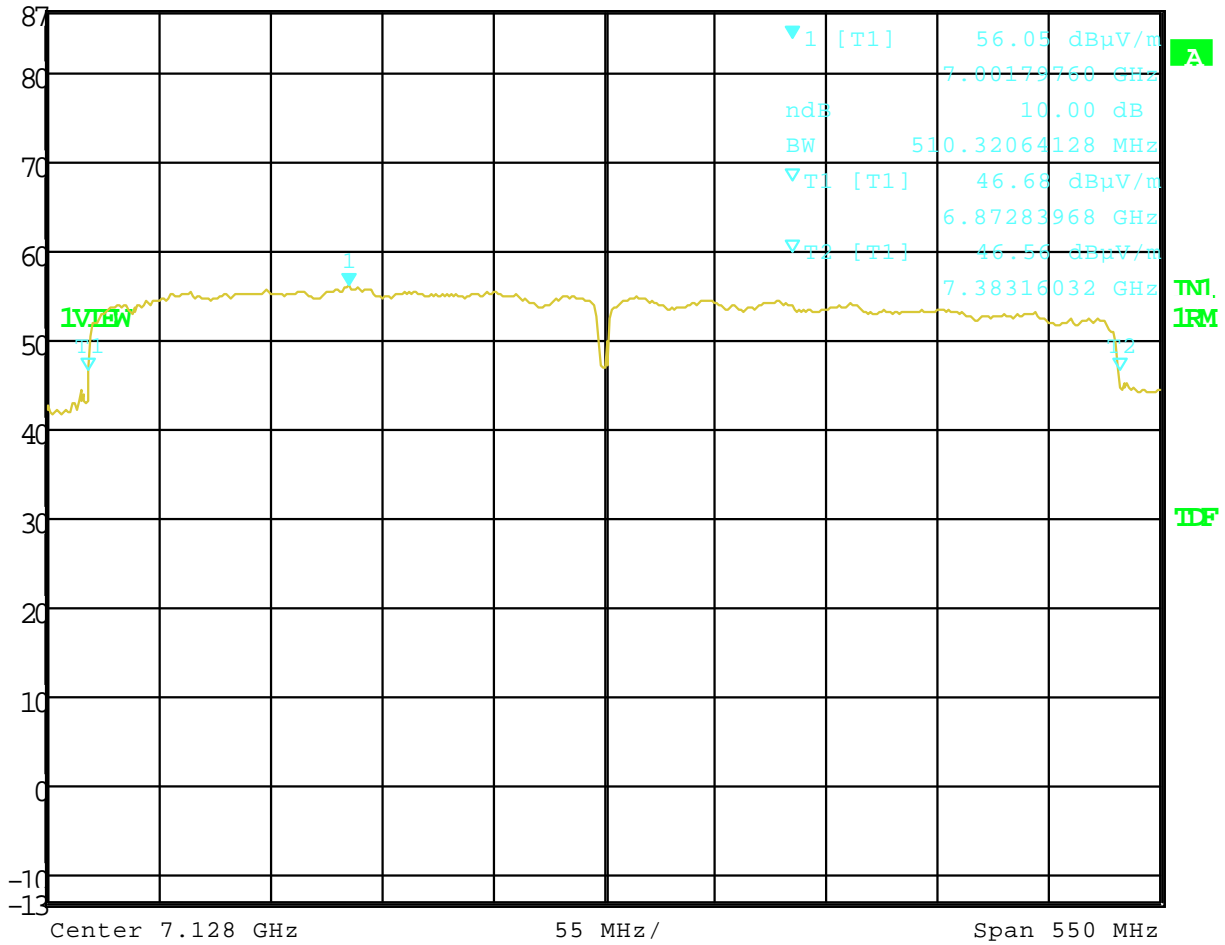

Date: 23.MAY.2011 12:35:17




166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Band Group 3
Band # 7



Ref Lvl	Marker 1 [T1 ndB]	RBW	1 MHz	RF Att	10 dB
87 dB*	ndB 10.00 dB	VBW	3 MHz		
	BW 510.32064128 MHz	SWT	500 ms	Unit	dBµV/m

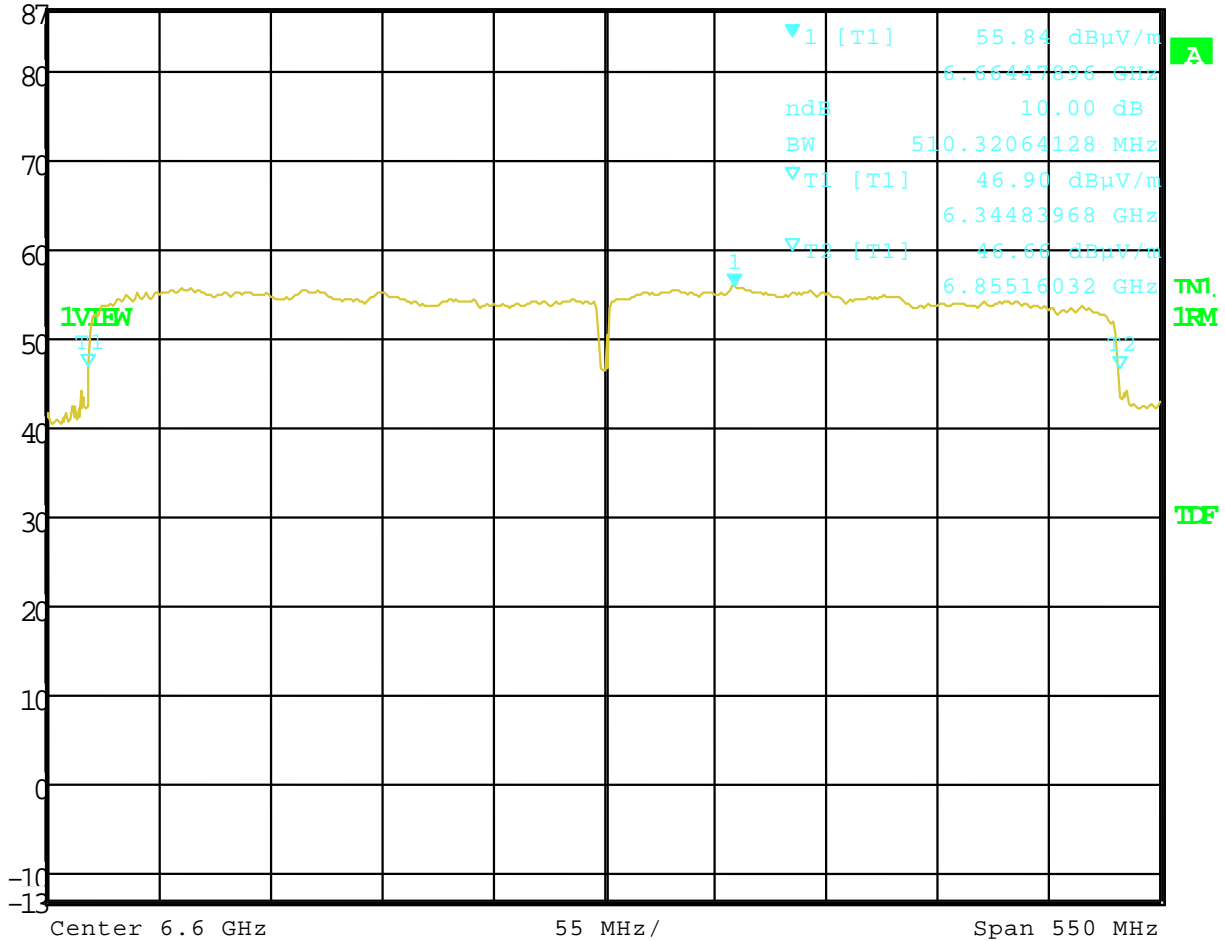

Date: 25.MAY.2011 12:03:18



166 South Carter, Genoa City, WI 53128

Company:
Model Tested:
Report Number:
Project Number:

GE Medical Systems, LLC
5436008-2 rev1
17001
4679

Appendix B

2.0 Radiated Spurious Emissions below 960 MHz

Rule Part:

15.519 (c)

Test Procedure:

ANSI C63.4-2009 and ANSI C63.10-2009

Limit:

15.209

Results:

Compliant

Sample Equation(s):

None

Notes:

Test distance 3 meter. No emissions detected within 20 dB of limit associated with UWB transmission.



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Appendix B

3.0 Radiated / RF Conducted Spurious Emissions above 960 MHz

Rule Part:

15.519 (c)

Test Procedure:

ANSI C63.4-2009 and ANSI C63.10-2009

Limit:

Average limit with resolution bandwidth of 1 MHz

Frequency (MHz)	EIRP in dBm
960 – 1610	-75.3
1610 – 1990	-63.3
1990 – 3100	-61.3
3100 – 10600	-41.3
Above 10600	-61.3

Results:

Compliant

Sample Equation(s):

See data

Notes:

Radiated emissions tested at 3 meter distance 1-10 GHz, 1 meter distance 10-18 GHz and 0.5 meter distance 18-40 GHz maximized in vertical and horizontal polarizations. No spurious radiated emissions were found associated with UWB transmission. The antenna port was connected directly to the analyzer through appropriate adapter and investigated for spurious emissions. No spurious conducted emissions were detected.




166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Radiated Spurious

10 – 18 GHz @ 1 meter – Maximized in vertical and horizontal polarizations – no emissions found

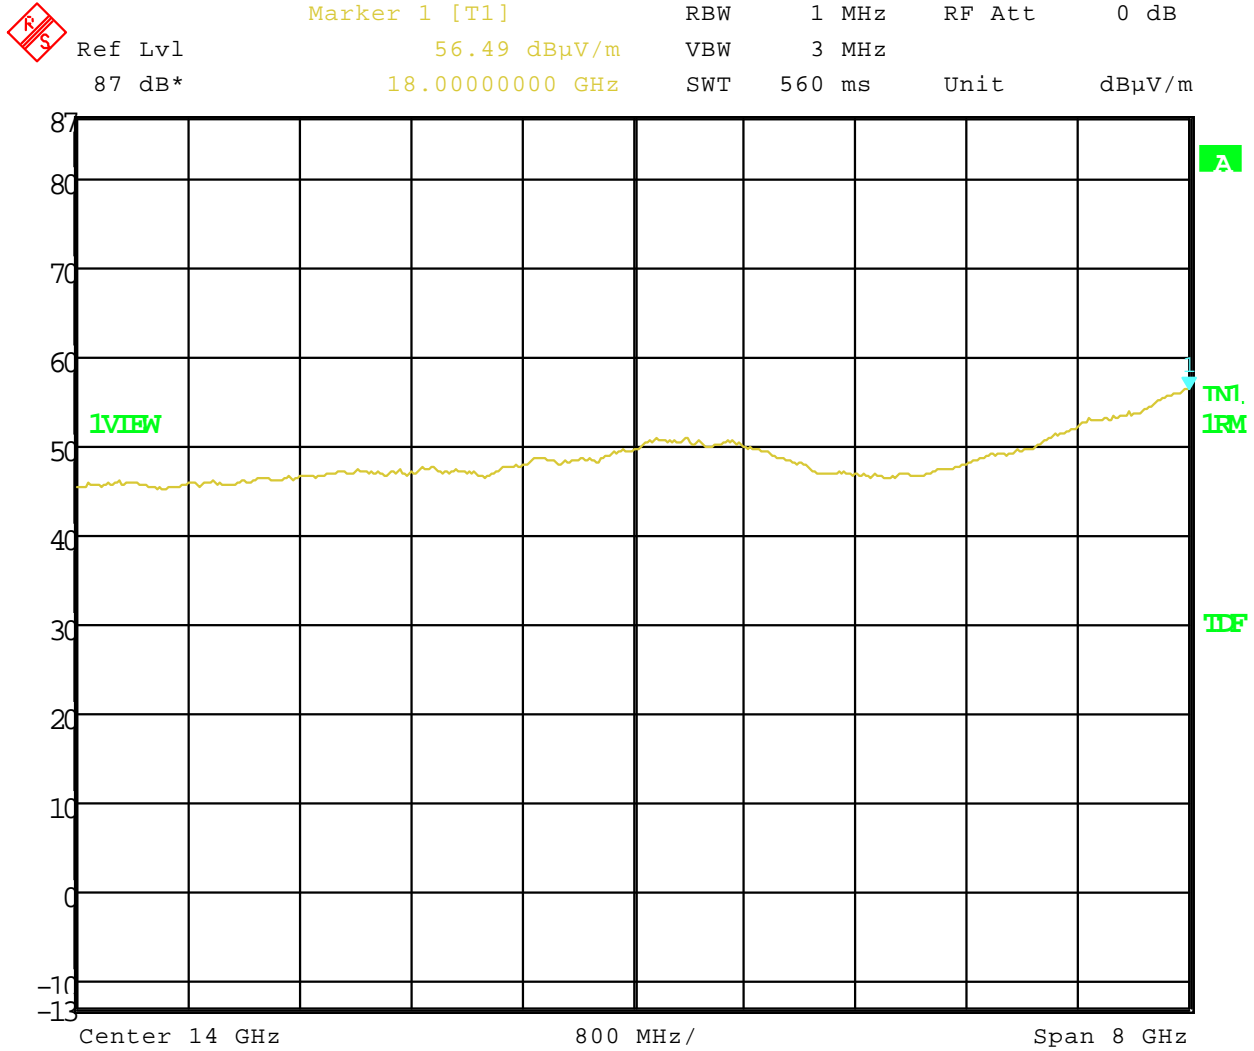

Date: 31.MAY.2011 13:25:20




166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Radiated Spurious

18 – 26.5 GHz @ 0.5 meter – Maximized in vertical and horizontal polarizations – no emissions found

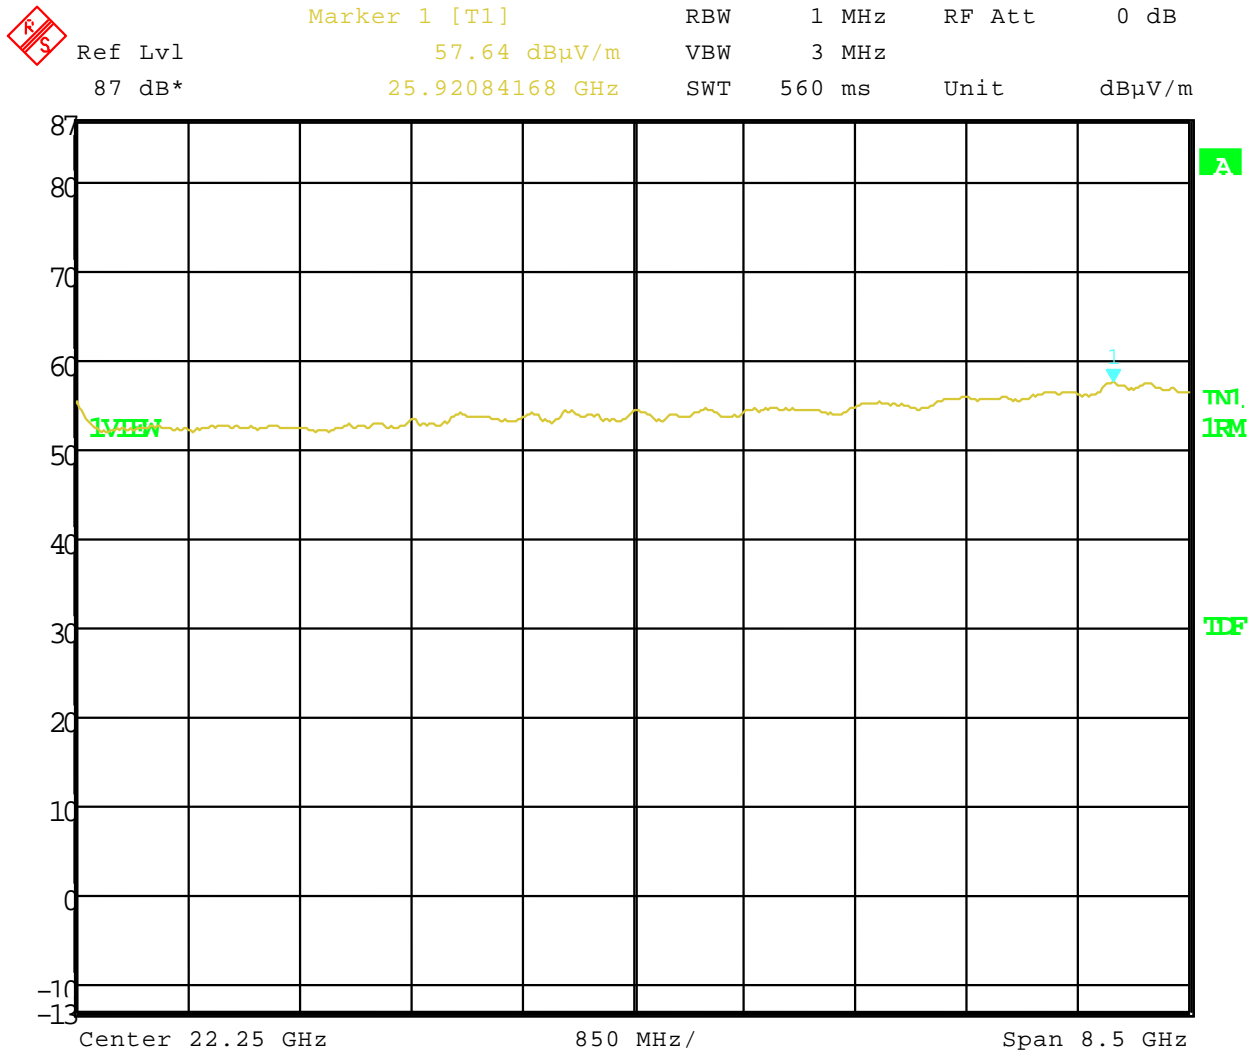

Date: 31.MAY.2011 13:51:38




166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Radiated Spurious

26.5 – 40 GHz @ 0.5 meter – Maximized in vertical and horizontal polarizations – no emissions found

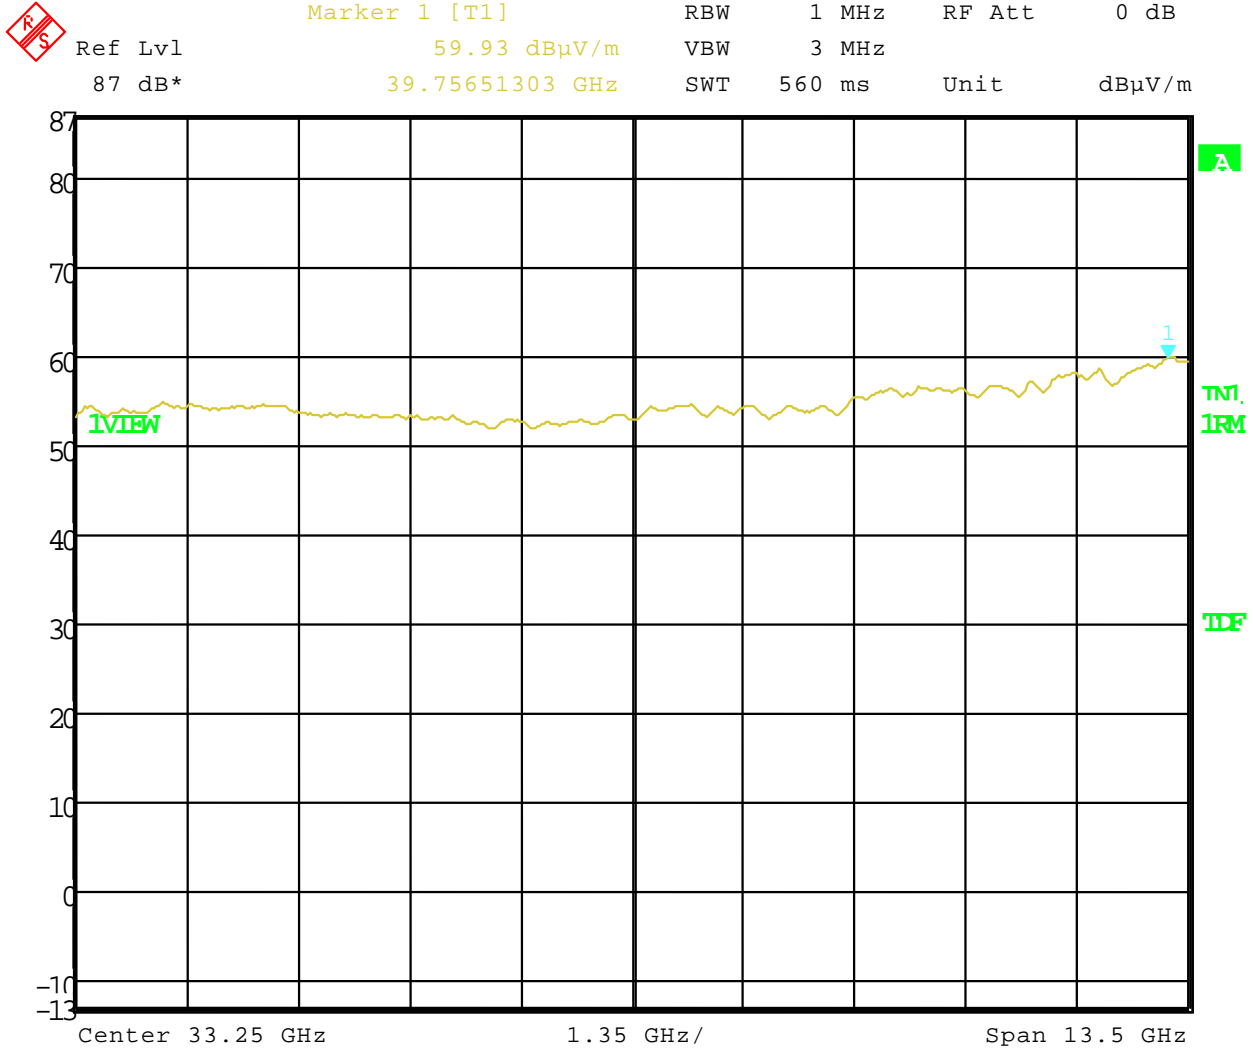

Date: 31.MAY.2011 14:06:00



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679


Conducted Spurious

10 – 26.5 GHz



Ref Lvl
-20 dBm

RBW 1 MHz RF Att 0 dB
VBW 3 MHz
SWT 500 ms Unit dBm

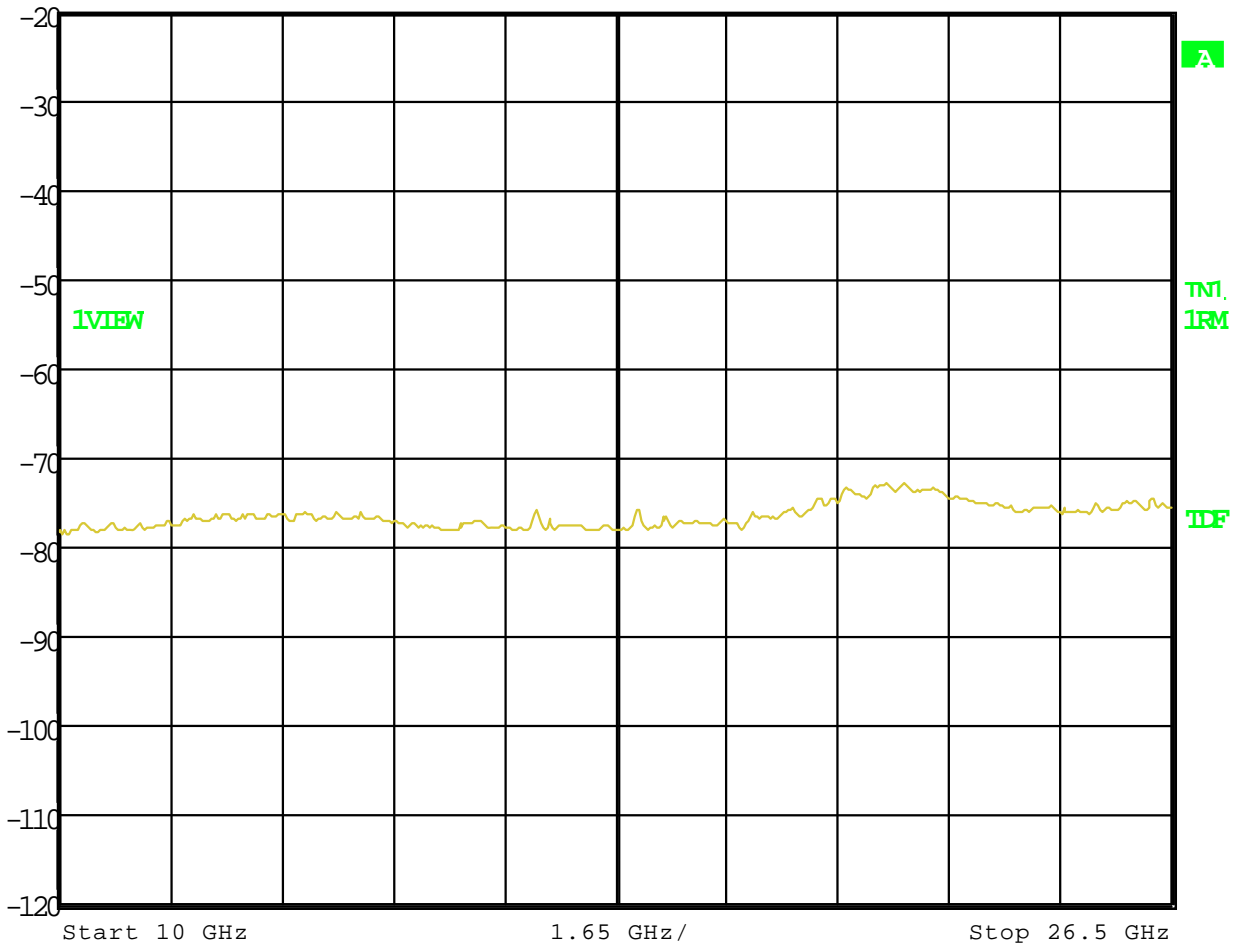

Date: 6.JUN.2011 11:45:30



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679


Conducted Spurious

26.5 – 40GHz



Ref Lvl
-20 dBm

RBW 1 MHz RF Att 0 dB
VBW 3 MHz
SWT 500 ms Unit dBm

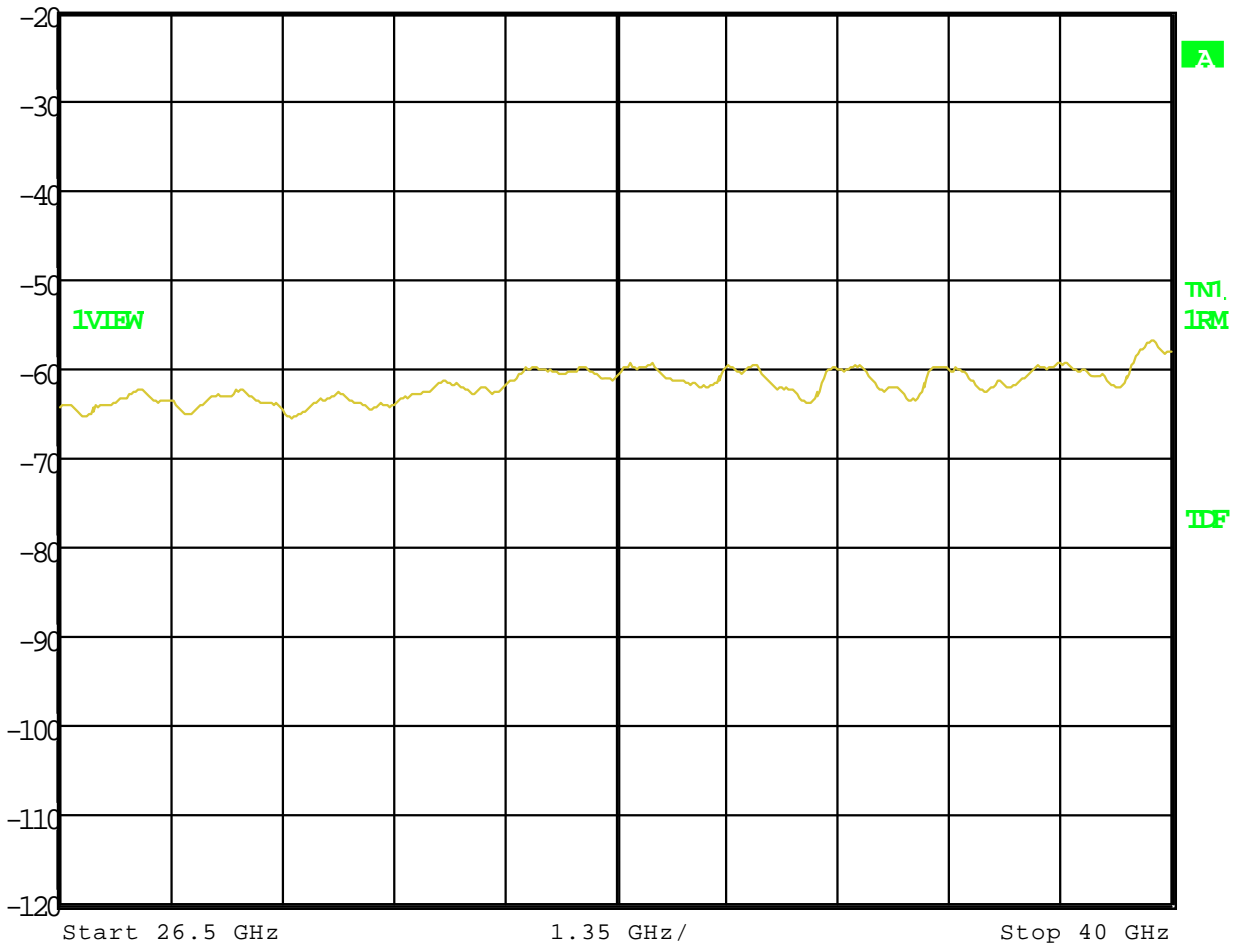

Date: 6 JUN. 2011 11:46:11




166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Conducted Spurious

30 – 1000 MHz

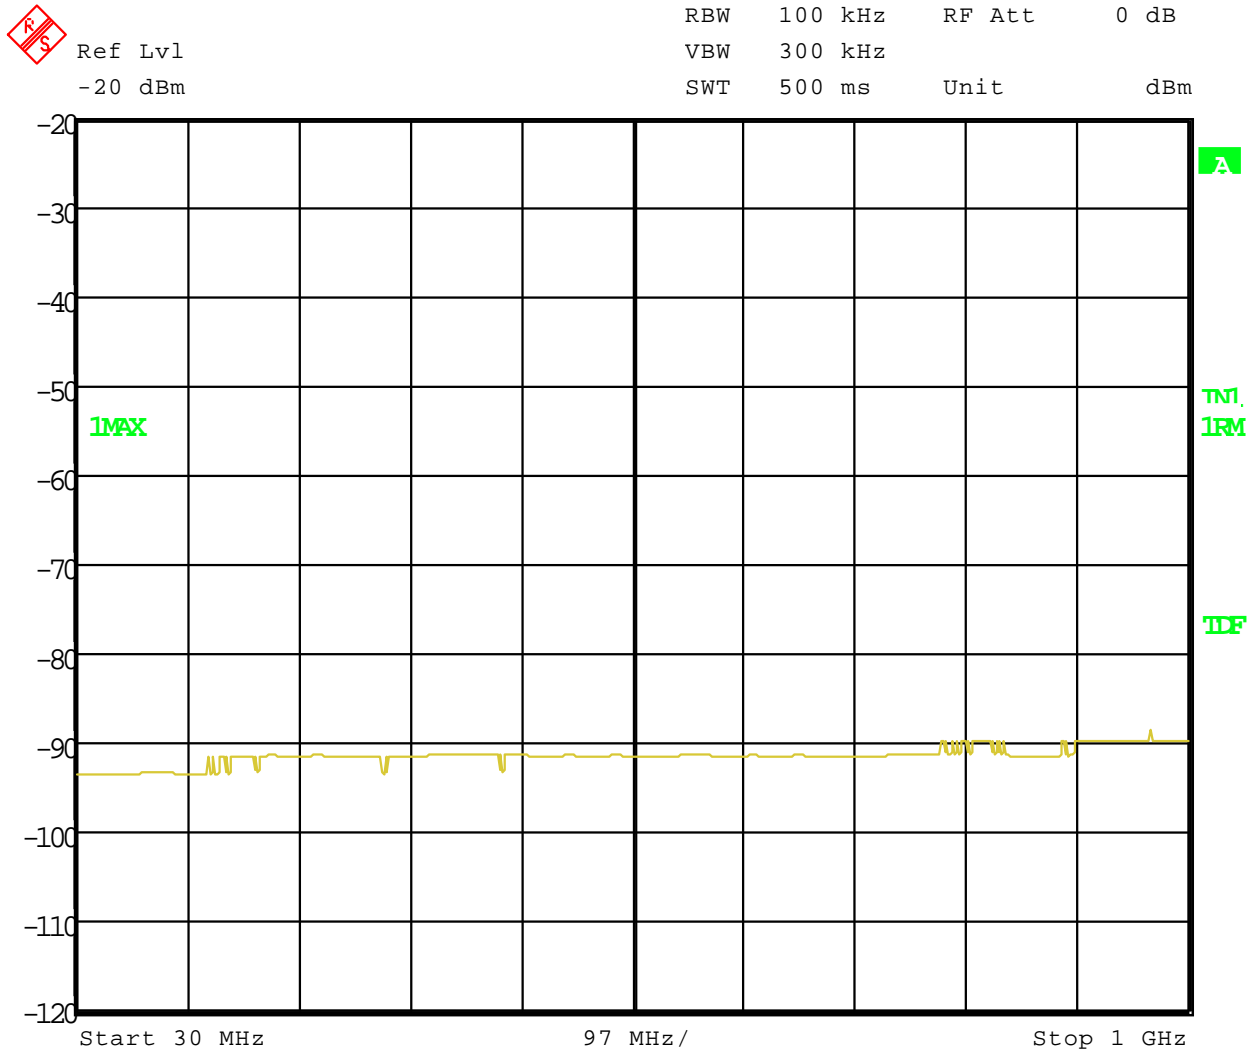

Date: 6.JUN.2011 12:05:23



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Appendix B

4.0 Radiated Fundamental Emissions in band 3100 to 10600 MHz

Rule Part:

15.519 (c) & (e)

Test Procedure:

ANSI C63.4-2009 and ANSI C63.10-2009

Limit:

EIRP in dBm
Average: -41.3
Peak: -24.4*

Results:

Compliant

Sample Equation(s):

See data

Notes:

*As per 15.521(g), limit adjusted by $20\log(\text{RBW}/50)$ dBm where RBW is the resolution bandwidth in MHz that is employed.

EUT investigated for worst case orientation and maximized in vertical and horizontal polarization. The maximum emission was then recorded. The EUT was replaced by an antenna connected to a signal generator. The level of the signal generator was set to match the maximum emission recorded from the EUT. Once corrected for antenna gain and cable loss the EIRP was compared to the limit.



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
 Model Tested: 5436008-2 rev1
 Report Number: 17001
 Project Number: 4679

Band Group 1

DLS Electronic Systems, Inc.												
Company: GE Healthcare												
Operator: Adam A												
Date of test: 5-23-2011												
Temperature: 70 deg. F												
Humidity: 61% R.H.												
	Average	Peak										
Detector	RMS (linear)	Peak						Antenna to EUT Distance:		3 m		
RBW	1 MHz	3 MHz						Floor to EUT Height:		80 cm		
VBW	3 MHz	3 MHz						Antenna Scan Height*:		1 - 4 m		
Sweep	500 ms (1 ms per point)							* EUT to remain in antenna 3dB beamwidth				
Span	550 MHz							RF Absorber lined floor				
EIRP = Signal generator output + cable loss + antenna gain												

Model: 98 (Band Group 1)

Band #	Frequency (GHz)	Measurement Antenna Polarization	Limit Type	Field Strength of EUT (dBμV/m)	Antenna Height (m)	Table Azimuth (deg)	Level of Gen. when field strength equals that of EUT (dBm)	Cable loss between Gen. and Subst. Antenna (dB)	Gain of subst. antenna (dBi)	Strength of emission [EIRP] (dBm)	Limit (dBm)	Margin (dB)
1	3.525	Vertical	Average	55.38	1.0	40	-50.9	-2.21	9.91	-43.20	-41.3	1.9
			Peak	66.80			-40.3			-32.60	-24.4	8.2
2	4.158	Vertical	Average	55.11	1.3	355	-51.3	-2.36	10.39	-43.27	-41.3	2.0
			Peak	66.80			-40.6			-32.57	-24.4	8.2
3	4.500	Vertical	Average	55.26	1.2	15	-51.8	-2.48	10.85	-43.43	-41.3	2.1
			Peak	66.80			-41.5			-33.13	-24.4	8.7



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
 Model Tested: 5436008-2 rev1
 Report Number: 17001
 Project Number: 4679

Band Group 3

DLS Electronic Systems, Inc.												
Company: GE Healthcare												
Operator: Adam A												
Date of test: 5-23-2011												
Temperature: 70 deg. F												
Humidity: 61% R.H.												
	Average	Peak										
Detector	RMS (linear)	Peak							Antenna to EUT Distance:	3 m		
RBW	1 MHz	3 MHz							Floor to EUT Height:	80 cm		
VBW	3 MHz	3MHz							Antenna Scan Height*:	1 - 4 m		
Sweep	500 ms (1 ms per point)								* EUT to remain in antenna 3dB beamwidth			
Span	550 MHz								RF Absorber lined floor			
EIRP = Signal generator output + cable loss + antenna gain												
Model: 98 (Band Group 3)												
Band #	Frequency (GHz)	Measurement Antenna Polarization	Limit Type	Field Strength of EUT (dBµV/m)	Antenna Height (m)	Table Azimuth (deg)	Level of Gen. when field strength equals that of EUT (dBm)	Cable loss between Gen. and Subst. Antenna (dB)	Gain of subst. antenna (dBi)	Strength of emission [EIRP] (dBm)	Limit (dBm)	Margin (dB)
7	6.664	Horizontal	Average	55.84	1.2	170	-52.0	-3.10	12.06	-43.04	-41.3	1.7
			Peak	68.01			-41.7			-32.74	-24.4	8.3
8	7.001	Vertical	Average	56.05	1.3	85	-51.8	-3.30	12.00	-43.10	-41.3	1.8
			Peak	67.44			-41.9			-33.20	-24.4	8.8
9	7.517	Vertical	Average	57.04	1.2	350	-50.7	-3.34	11.23	-42.81	-41.3	1.5
			Peak	68.74			-40.5			-32.61	-24.4	8.2



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

Appendix B

5.0 Radiated Spurious Emissions in GPS Band

Rule Part:

15.519 (d)

Test Procedure:

ANSI C63.4-2009 and ANSI C63.10-2009

Limit:

Average limit with resolution bandwidth of no less than 1 kHz

Frequency (MHz)	EIRP in dBm
1164 – 1240	-85.3
1559 – 1610	-85.3

Results:

Compliant

Sample Equation(s):

15.519 (e) limit @ 1 meter: $-85.3 + 95.2 + 20\log(3/1)$

15.209 limit @ 1 meter: 63.54 dBμV/m

Notes:

EUT tested at 1 meter distance.

EUT was set in standby mode with no UWB transmission. The EUT was then placed in transmit mode and no emissions were observed. (Emission from associated equipment not related to the function of the UWB transmission.)




166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

GPS BAND 1.164 – 1.240 GHz Digital Device Emission



Ref Lvl	Marker 1 [T1]	RBW	10 kHz	RF Att	10 dB
87 dB*	10.53 dB μ V/m	VBW	10 kHz		
	1.20009619 GHz	SWT	1.9 s	Unit	dB μ V/m

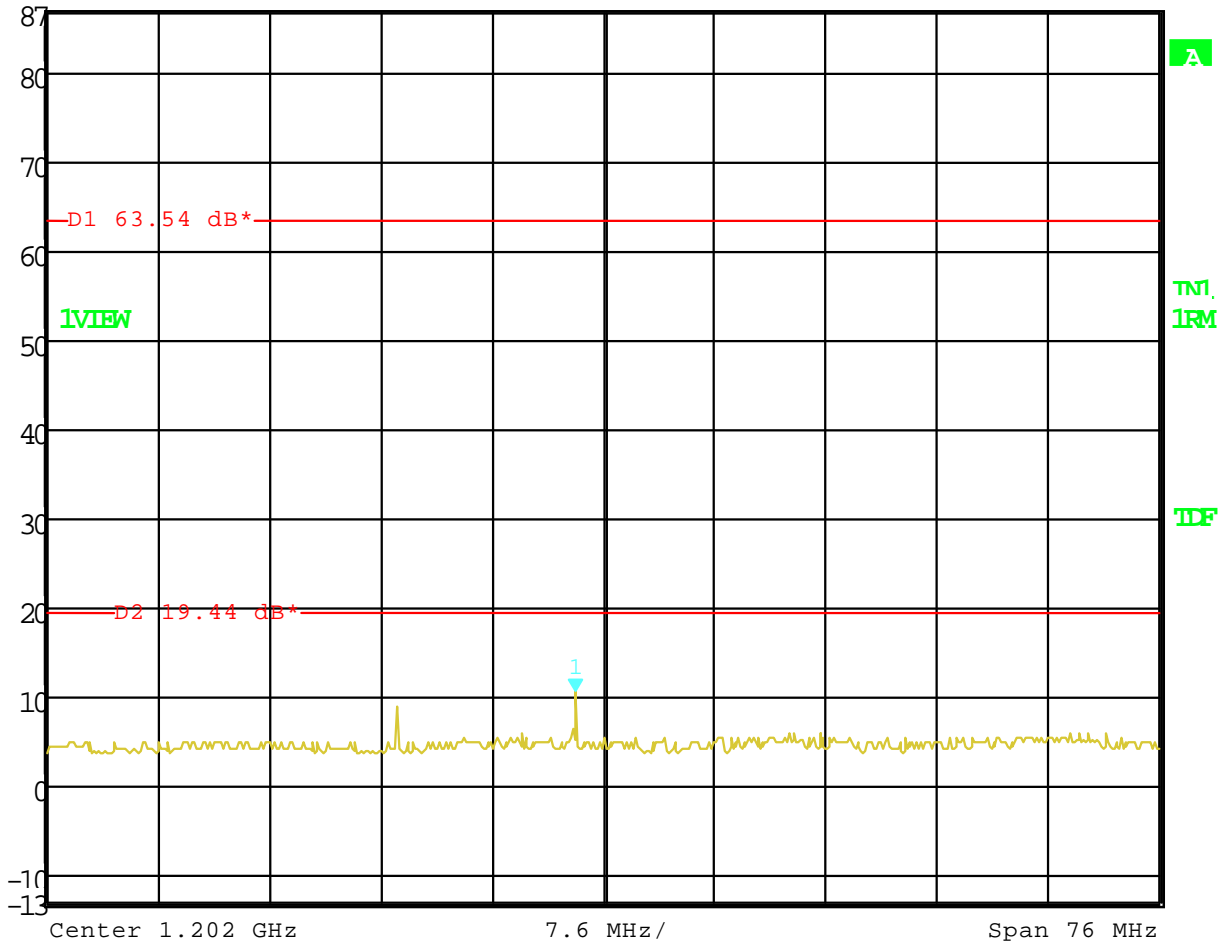

Date: 27.MAY.2011 08:43:52




166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
 Model Tested: 5436008-2 rev1
 Report Number: 17001
 Project Number: 4679

GPS BAND 1.559 – 1.61 GHz
 Digital Device Emission



Ref Lvl	Marker 1 [T1]	RBW	10 kHz	RF Att	10 dB
87 dB*	19.33 dB μ V/m	VBW	10 kHz		
	1.58404008 GHz	SWT	1.3 s	Unit	dB μ V/m

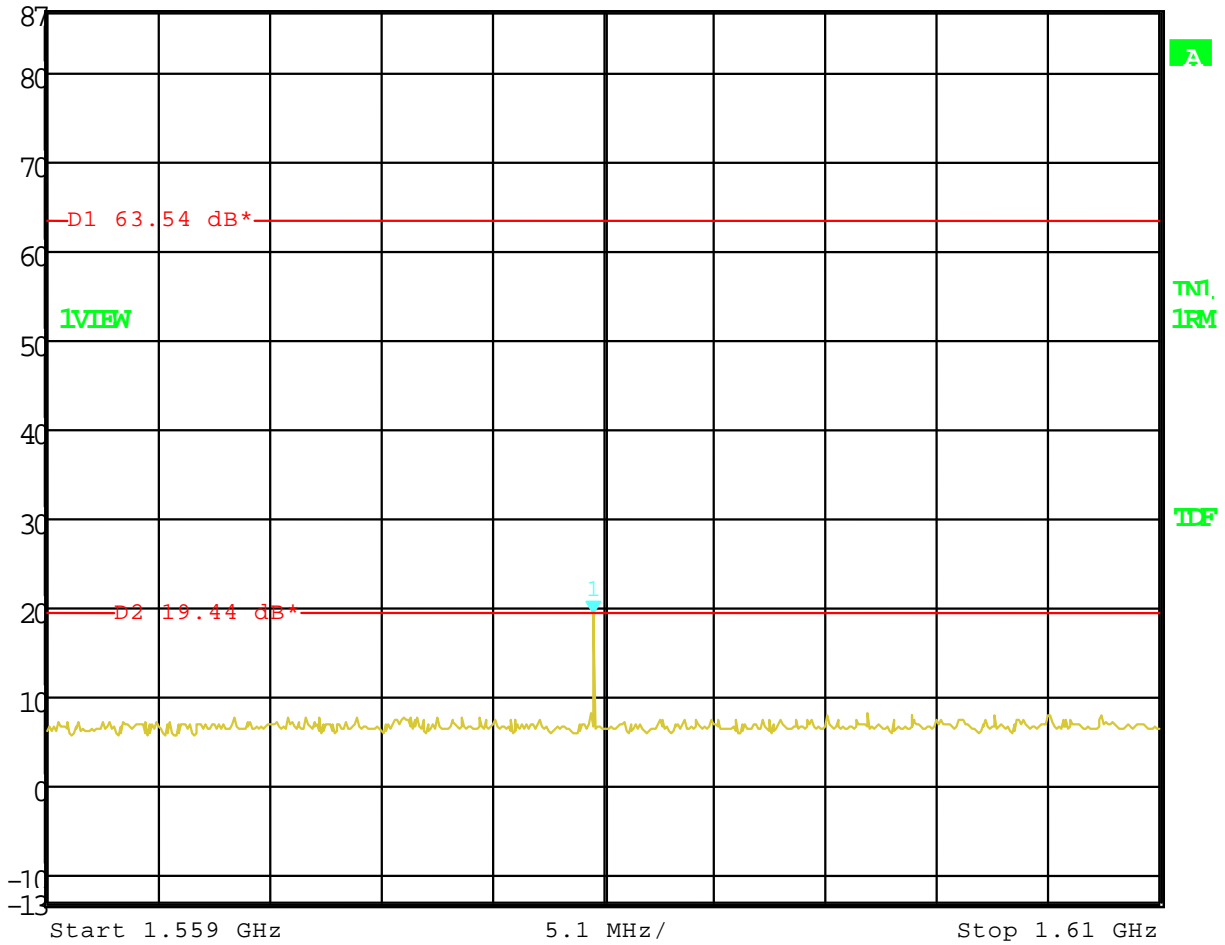

Date: 27.MAY.2011 08:46:03



166 South Carter, Genoa City, WI 53128

Company: GE Medical Systems, LLC
Model Tested: 5436008-2 rev1
Report Number: 17001
Project Number: 4679

END OF REPORT

Revision #	Date	Comments	By
1.0	6-20-2011	Preliminary Release	AA
1.1	6-21-2011	Minor typo fixes	AA
1.2	6-22-2011	Updated description pg 6 / name w- "Board"	JS