


Company: GE Medical Systems, LLC
Model: URP Radio Board
Setup Photos


Radiated Emissions – Y – Worst Case Position



Radiated Emissions – Y Position (2)

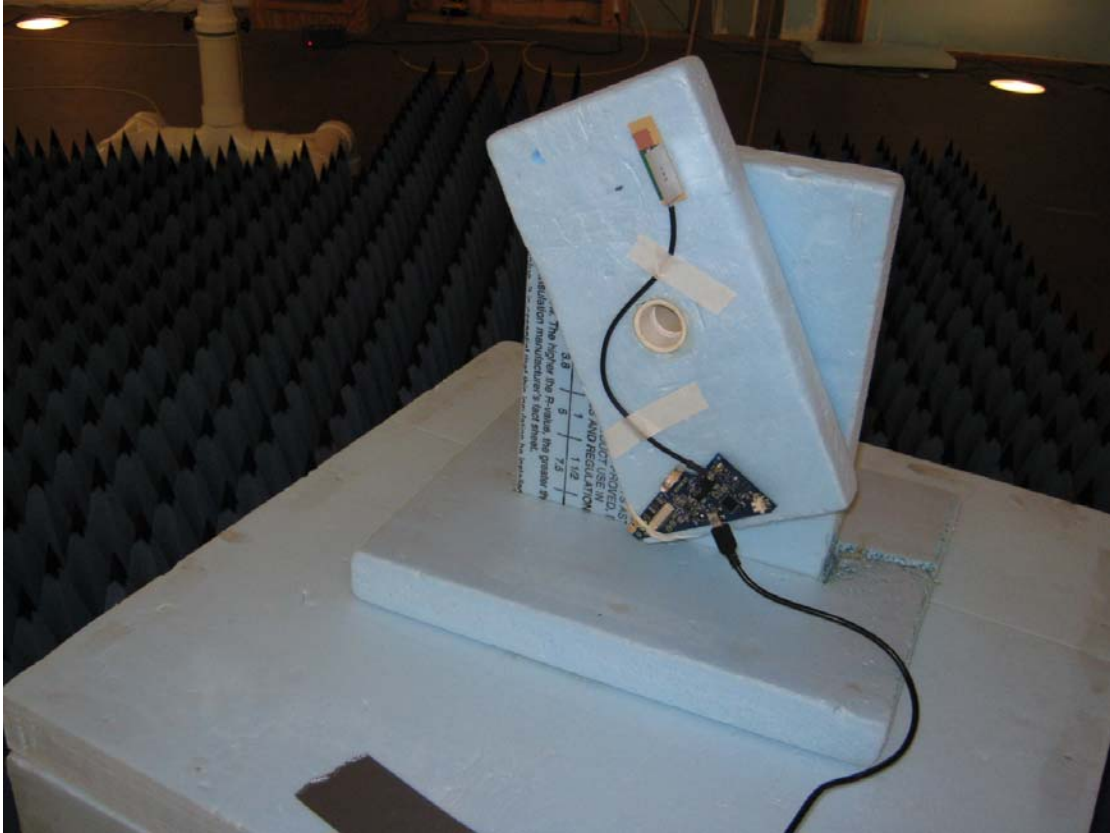


Radiated Emissions – Y Position (3)

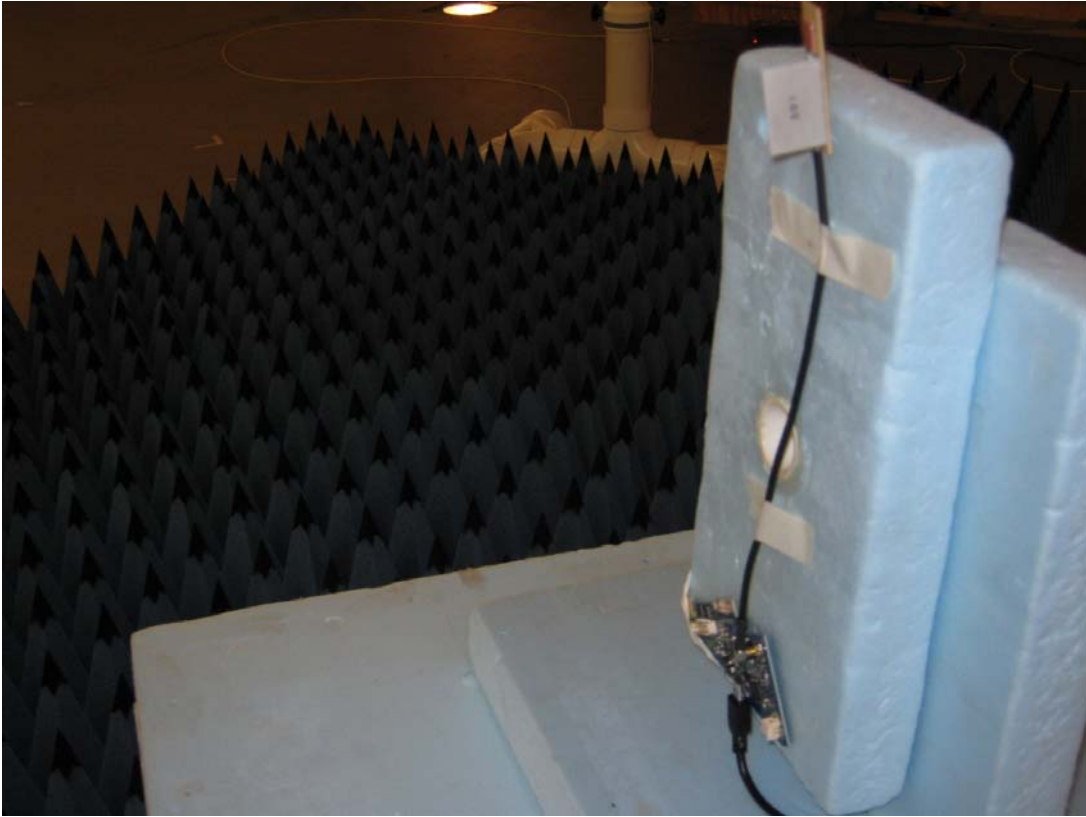


Radiated Emissions – Y Position (4)




Radiated Emissions – Y Position (5)

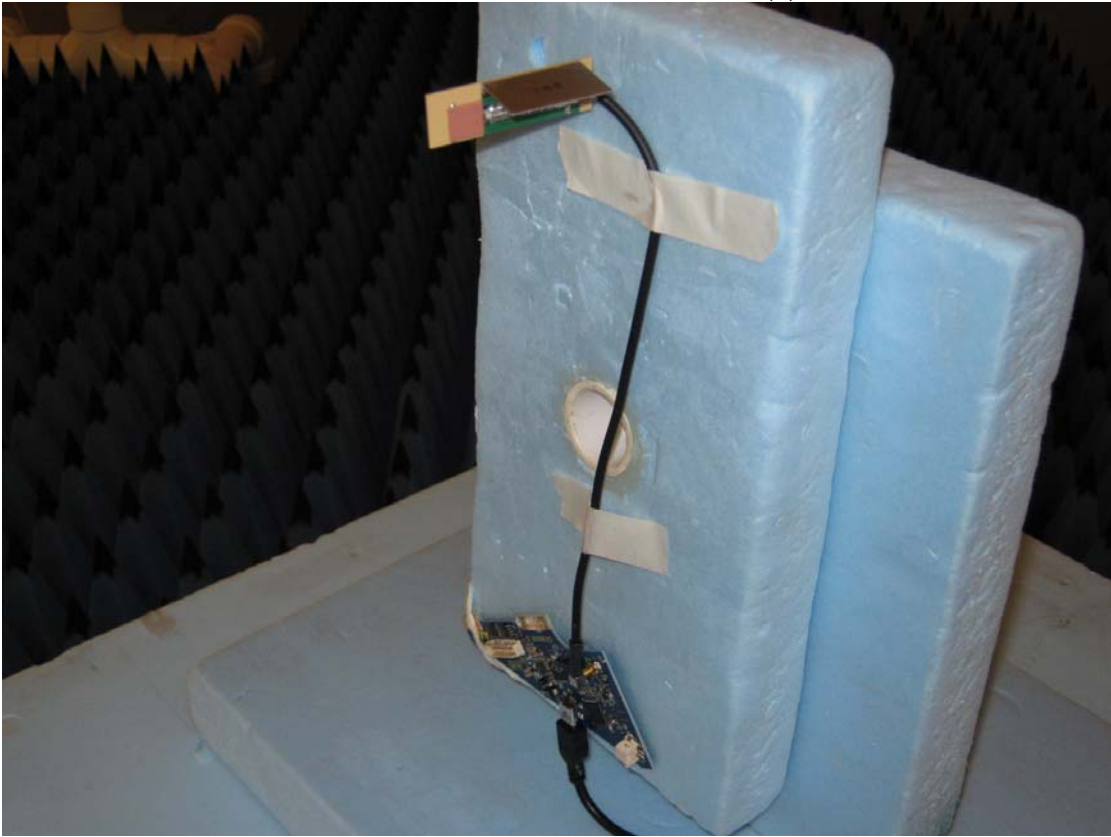


Radiated Emissions – Z Position

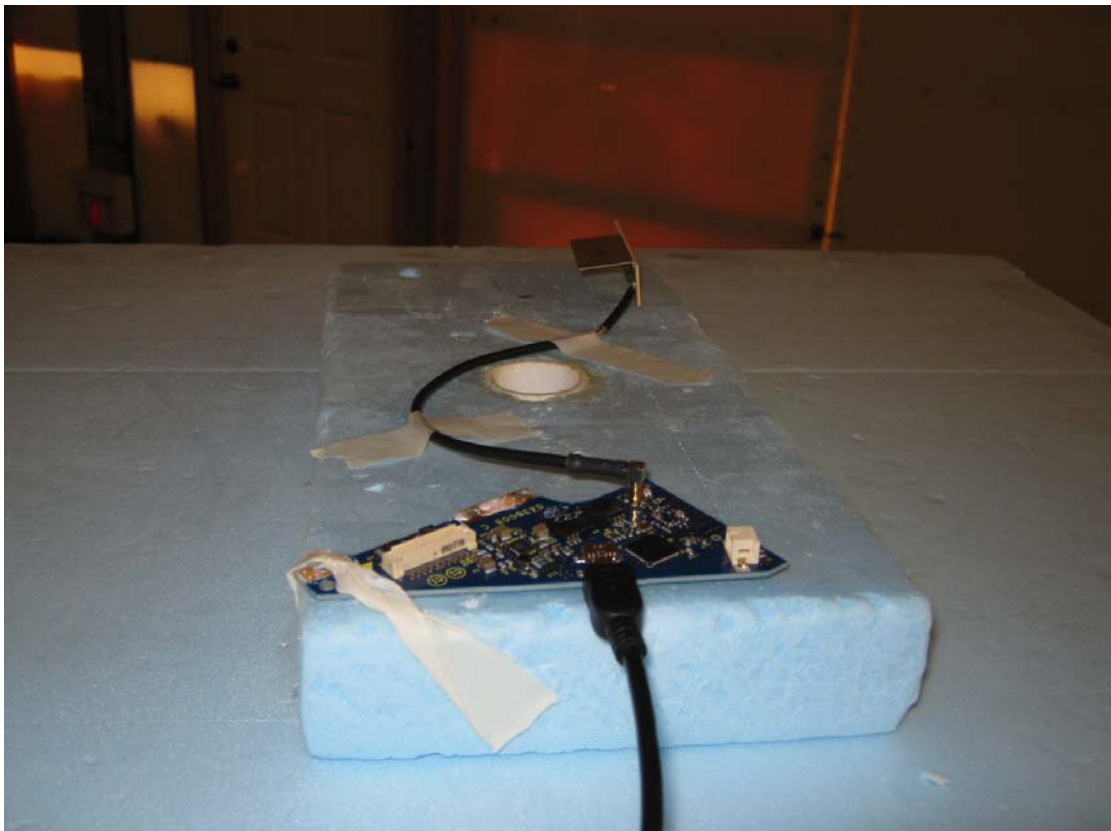

Radiated Emissions – Z Position (2)

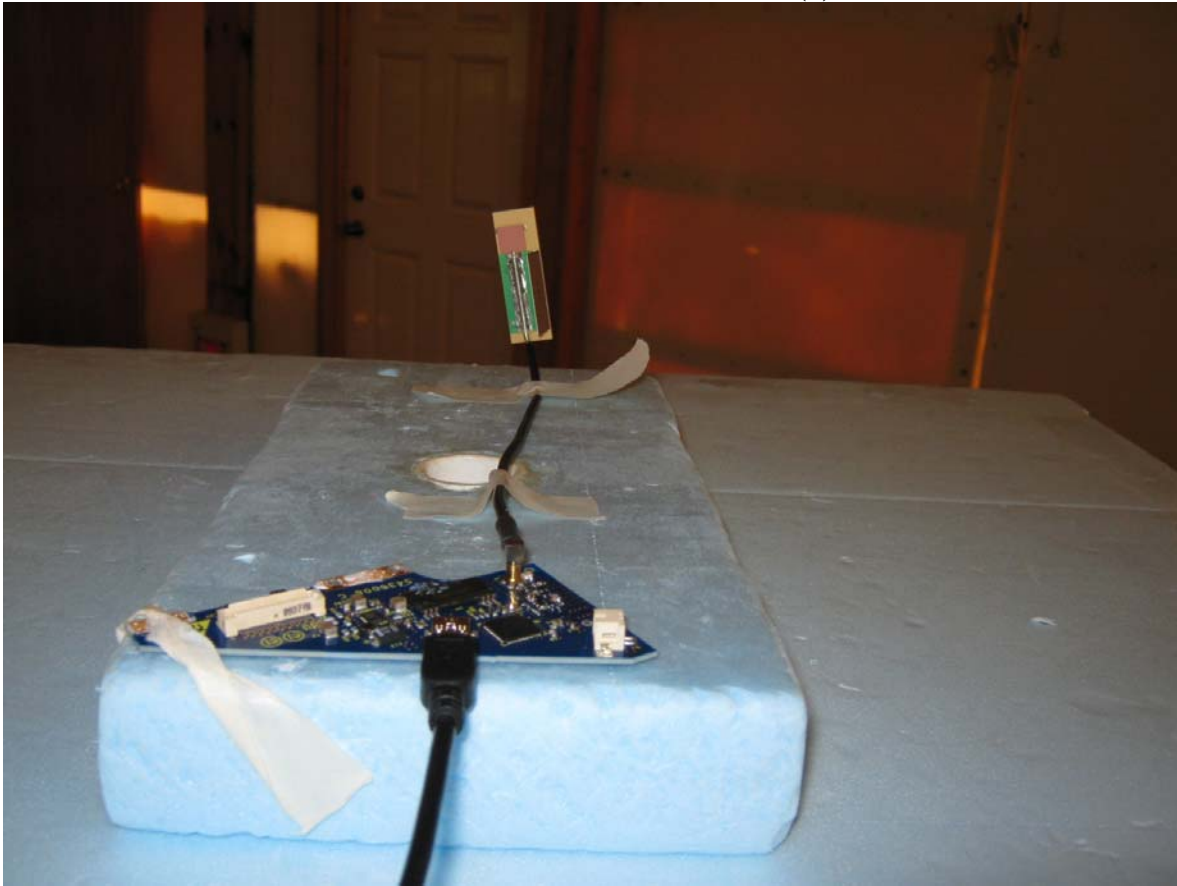

Radiated Emissions – X Position

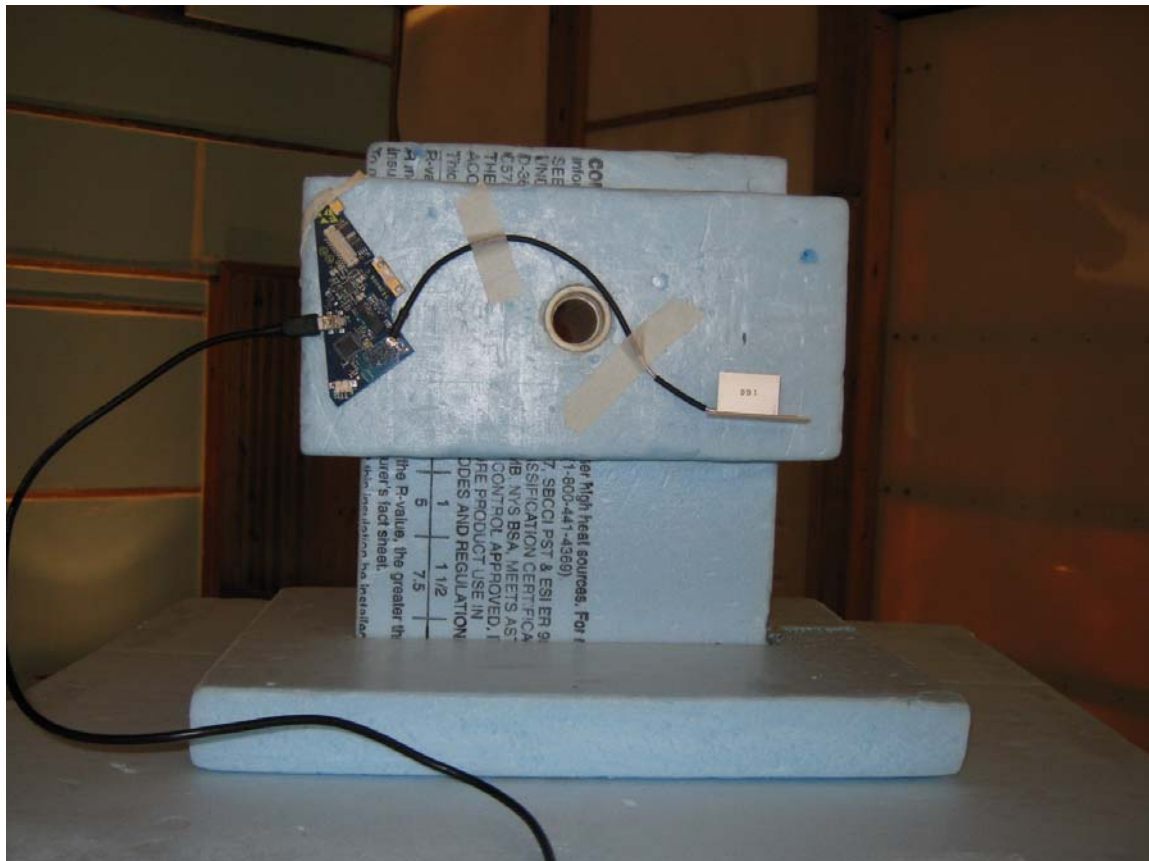

Radiated Emissions – X Position (2)

