

DUT and SAR Set-up Photos

Overview

Wi-Fi Radio location




Note: Plastic patient rails on sides have been removed to allow positioning of the DUT as close as possible to phantom.

Side View of the DUT – Close up at patient surface




Top View of the DUT

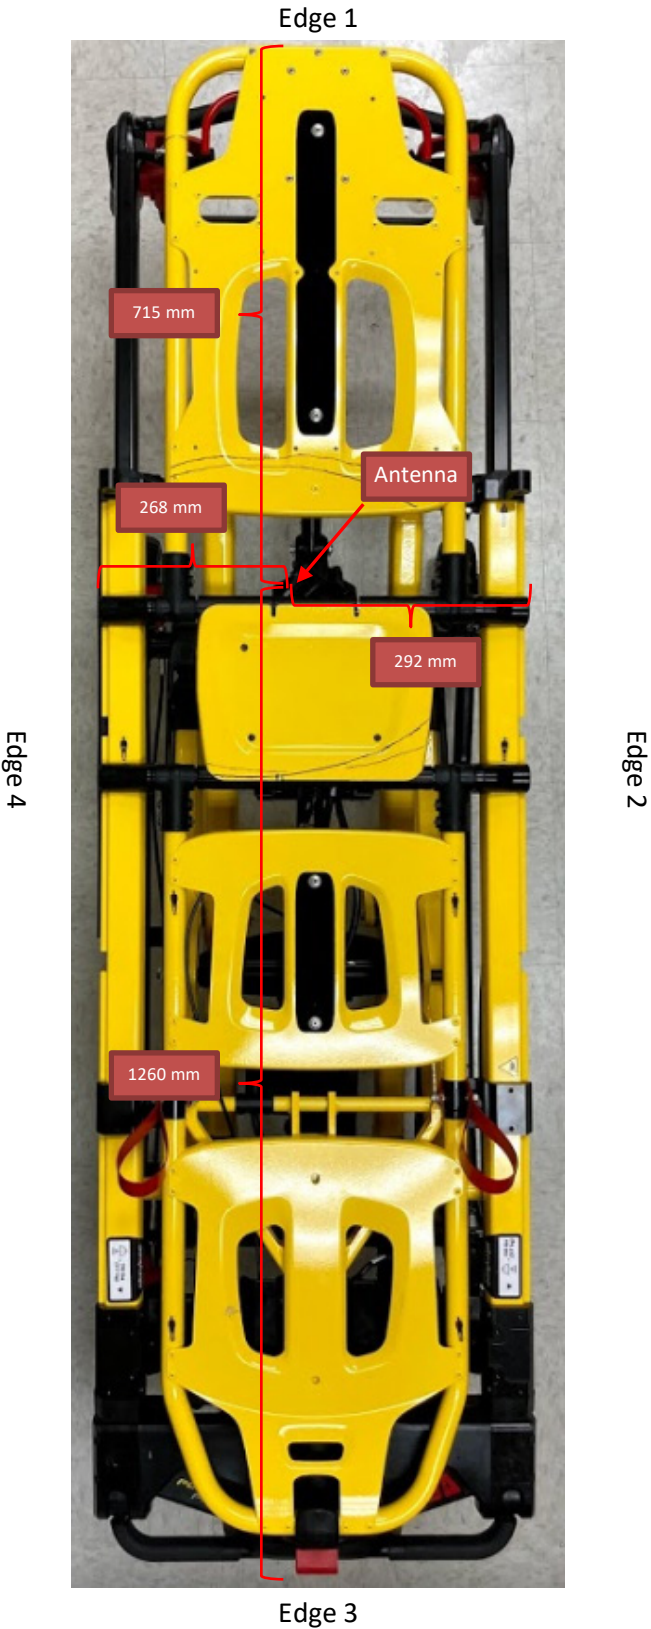

Setup Photos

Phantom Placement

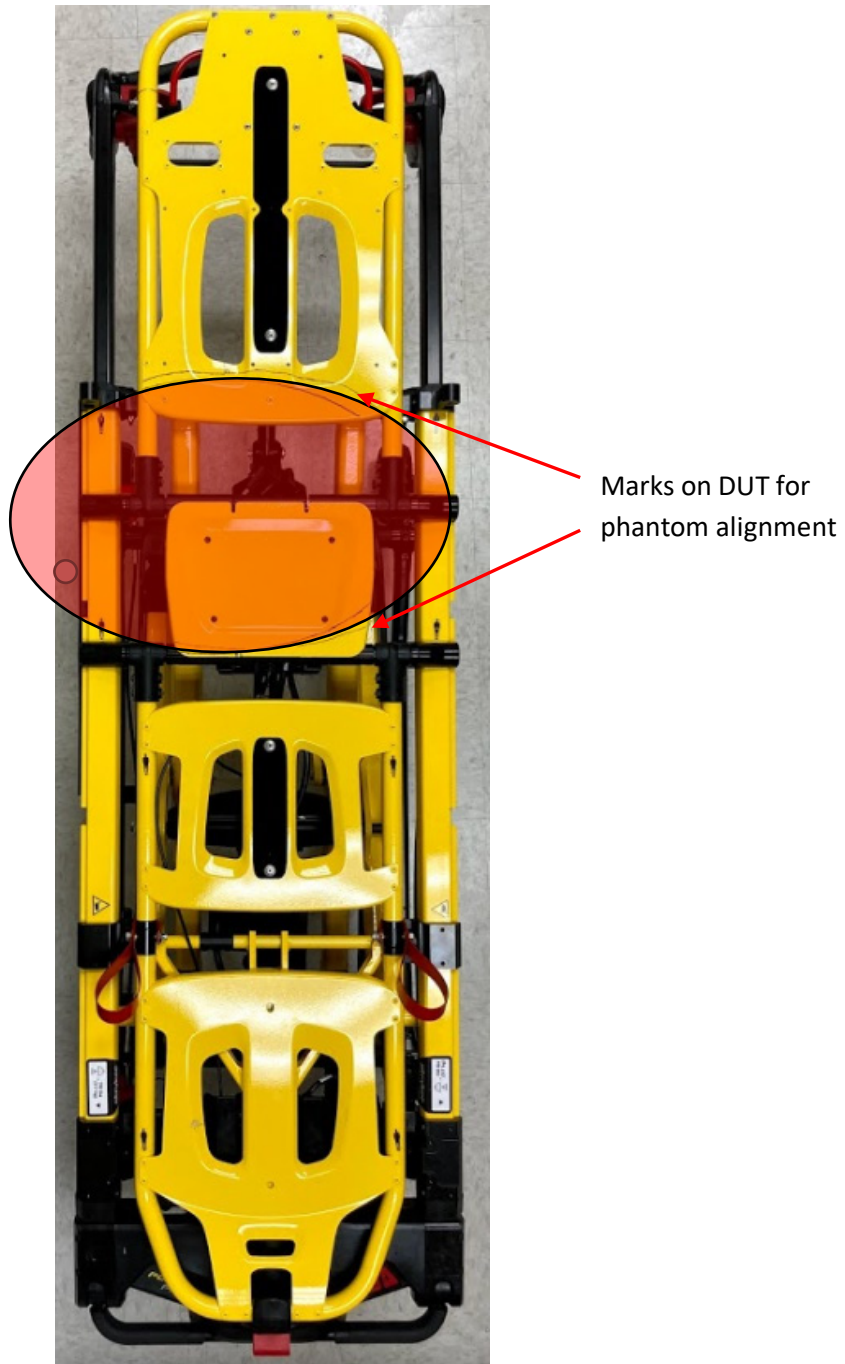

WiFi Exposure Conditions

Flat Phantom Touch - Side



Flat Phantom Touch – End

