

# NCL CALIBRATION LABORATORIES

Calibration File No: DC-1203  
Project Number: SPTB-ALSAS-5566

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Validation Dipole  
2450MHz Head & Body

Manufacturer: APREL Laboratories

Part number: ALS-D-2450-S-2

Frequency: 2450MHz

Serial No: 220-00762

Customer: SPORTON

Calibrated: 20<sup>th</sup> February 2011  
Released on: 25<sup>h</sup> February 2011

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

303 Terry Fox Drive, Suite 102  
Kanata, Ontario  
CANADA K2K 3J1

Division of APREL  
TEL: (613) 435-8300  
FAX: (613) 435-8306

# NCL Calibration Laboratories

Division of APREL Inc.

---

## Conditions

Dipole 220-00762 was a new dipole taken from stock.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C

**Temperature of the Tissue:** 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



-----  
**Stuart Nicol**



-----  
**C. Teodorian**

## Primary Measurement Standards

<b>Instrument</b>	<b>Serial Number</b>	<b>Cal due date</b>
Power meter Anritsu MA2408A	245025437	Nov.4, 2010
Power Sensor Anritsu MA2481D	103555	Nov 4, 2010
Attenuator HP 8495A (70dB)	1944A10711	Sept. 14, 2010
Network Analyzer Anritsu MT8801C	MB11855	Feb. 8, 2011

## Secondary Measurement Standards

Signal Generator Agilent E4438C -506	MY55182336	June 7, 2011
--------------------------------------	------------	--------------

## Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

### Mechanical Dimensions


**Length:** 51.5 mm  
**Height:** 30.4 mm

### Electrical Specification 2450MHz

Tissue Type	Return Loss:	Impedance:	SWR:
Head	-36.573	50.472	1.032U
Body	-28.075	51.272	1.083U

### System Validation Results

Tissue	Frequency	1 Gram	10 Gram	Peak
Head	2450 MHz	52.456	23.603	108.940
Body	2450 MHz	52.592	24.461	104.910

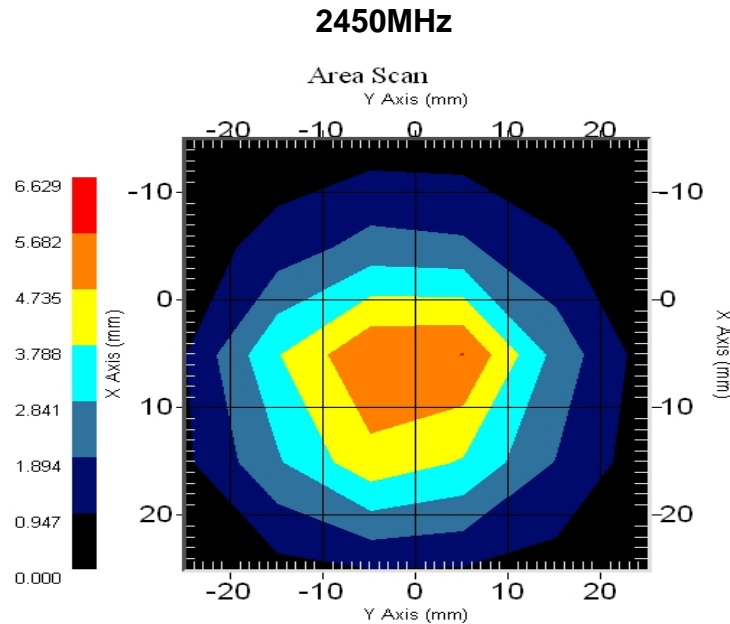

## Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole 220-00762. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-030 130 MHz to 26 GHz E-Field Probe Serial Number 215.

## References

- o IEEE Standard 1528 (2003) including Amendment 1  
IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
- o EN 62209-1 (2006)  
Human Exposure to RF Fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures-Part 1: Procedure to measure the Specific Absorption Rate (SAR) for hand-held mobile wireless devices
- o IEC 62209-2 Ed. 1.0 (2010-03)  
Human exposure to RF fields from hand-held and body-mounted wireless devices - Human models, instrumentation, and procedures - Part 2: specific absorption rate (SAR) for wireless communication devices (30 MHz - 6 GHz)
- o TP-D01-032-E020-V2 E-Field probe calibration procedure
- o D22-012-Tissue dielectric tissue calibration procedure
- o D28-002-Dipole procedure for validation of SAR system using a dipole
- o IEEE 1309 Draft Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9kHz to 40GHz

## Conditions

Dipole 220-00762 was a new dipole taken from stock.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 20 °C +/- 0.5°C

**Electrical Calibration**


**Electrical Specification 2450MHz**

Tissue Type	Measured Epsilon	Measured Sigma
Head	37.87	1.82
Body	50.84	1.92

**Head Tissue**

S11 FORWARD REFLECTION

LOG MAGNITUDE      REF=-20.000 dB      5.000 dB/DIV

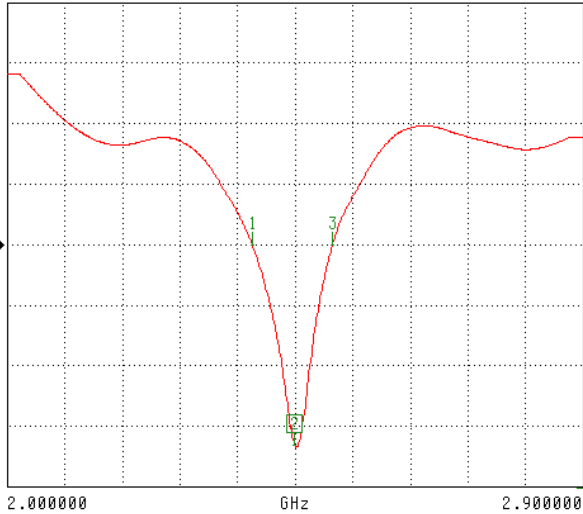

CH 1 - S11  
5.0584 mm REF  
0.000 dB OFFSET  
0.00° OFFSET

MARKER 2  
2.450000 GHz  
-36.573 dB

MARKER TO MAX  
MARKER TO MIN


1 2.383480 GHz  
-20.030 dB  
3 2.509320 GHz  
-20.028 dB

MARKER READOUT  
FUNCTIONS

**Body Tissue**

S11 FORWARD REFLECTION

LOG MAGNITUDE      REF=-20.000 dB      5.000 dB/DIV

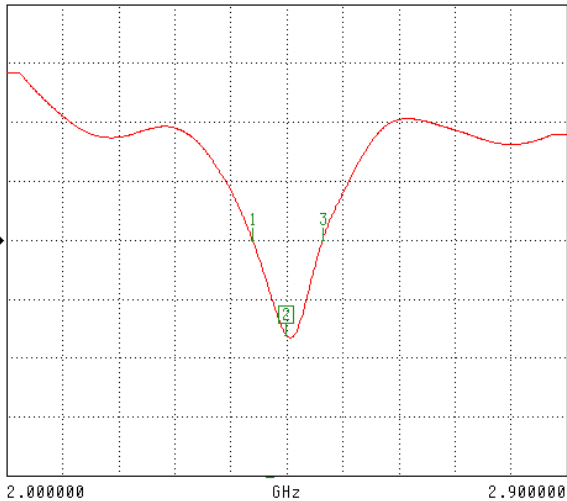

CH 1 - S11  
5.0584 mm REF  
0.000 dB OFFSET  
0.00° OFFSET

MARKER 2  
2.450000 GHz  
-28.075 dB

MARKER TO MAX  
MARKER TO MIN

1 2.395270 GHz  
-20.001 dB  
3 2.508330 GHz  
-20.031 dB


MARKER READOUT  
FUNCTIONS

**Electrical Specification 2450MHz  
Impedance**

Tissue Type	Measured Epsilon	Measured Sigma
Head	37.87	1.82
Body	50.84	1.92

**Head Tissue**

S11 FORWARD REFLECTION  
IMPEDANCE

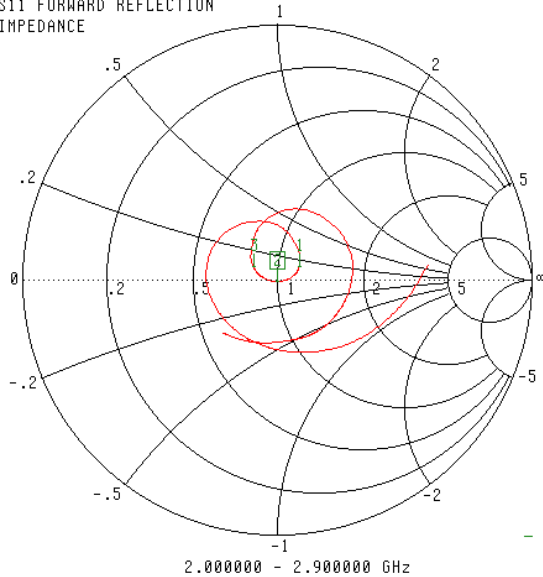

CH 1 - S11  
5.0584 mm REF  
0.000 dB OFFSET  
0.00° OFFSET


▶ MARKER 2  
2.450000 GHz  
50.472 Ω  
-1.017 jΩ  
MARKER TO MAX  
MARKER TO MIN

- 1 2.383400 GHz  
59.587 Ω  
5.641 jΩ
- 3 2.509320 GHz  
41.615 Ω  
3.970 jΩ

MARKER READOUT  
FUNCTIONS

**Body Tissue**

S11 FORWARD REFLECTION  
IMPEDANCE

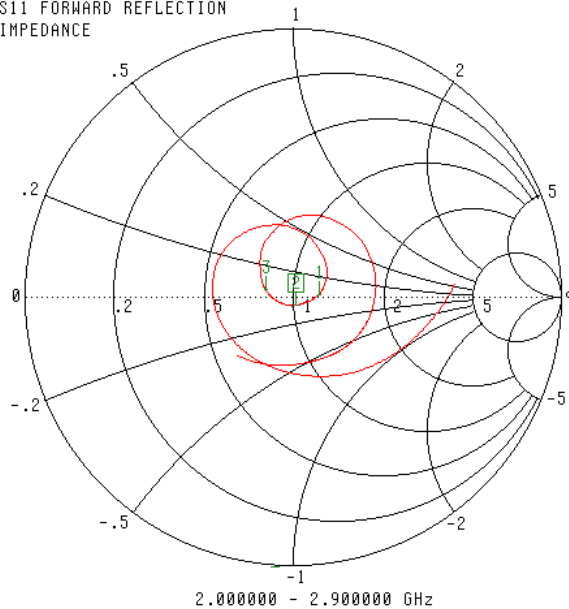

CH 1 - S11  
5.0584 mm REF  
0.000 dB OFFSET  
0.00° OFFSET

▶ MARKER 2  
2.450000 GHz  
51.272 Ω  
-3.639 jΩ

MARKER TO MAX  
MARKER TO MIN

- 1 2.395270 GHz  
61.141 Ω  
771.973 jΩ
- 3 2.508330 GHz  
41.037 Ω  
1.882 jΩ


MARKER READOUT  
FUNCTIONS

**Electrical Specification 2450MHz  
Standing Wave Ratio**

Tissue Type	Measured Epsilon	Measured Sigma
Head	37.87	1.82
Body	50.84	1.92

**Head Tissue**

S11 FORWARD REFLECTION

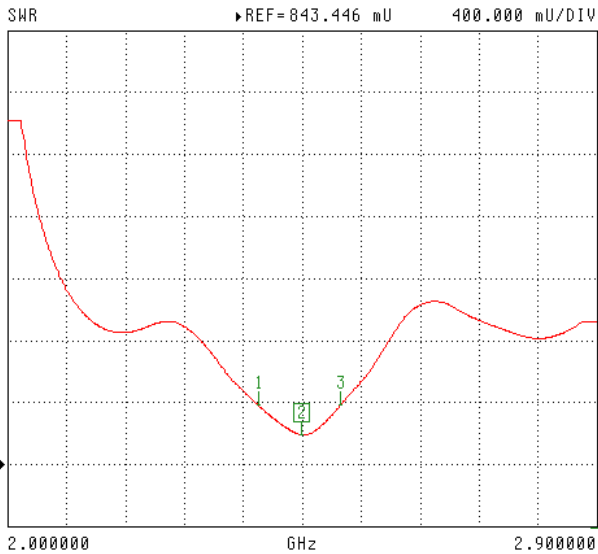

CH 1 - S11  
5.0584 mm REF  
0.000 dB OFFSET  
0.00° OFFSET

▶ MARKER 2  
2.450000 GHz  
1.032 U


MARKER TO MAX  
MARKER TO MIN

- 1 2.383480 GHz  
1.224 U
- 3 2.509320 GHz  
1.226 U

MARKER READOUT  
FUNCTIONS

**Body Tissue**

S11 FORWARD REFLECTION

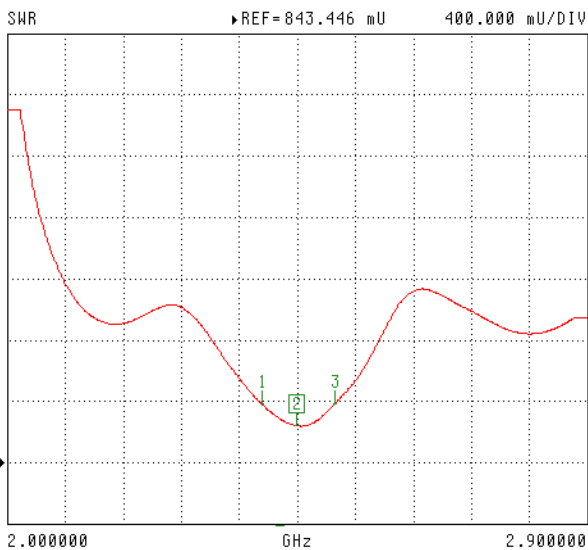

CH 1 - S11  
5.0584 mm REF  
0.000 dB OFFSET  
0.00° OFFSET

▶ MARKER 2  
2.450000 GHz  
1.083 U

MARKER TO MAX  
MARKER TO MIN

- 1 2.395270 GHz  
1.225 U
- 3 2.508330 GHz  
1.225 U

MARKER READOUT  
FUNCTIONS

## **NCL Calibration Laboratories**

---

Division of APREL Inc.

### **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2010.