





SAR TEST REPORT

No. I23Z670257-SEM02

For

SAMSUNG Electronics Co., Ltd.

Wearable device

Model Name: SM-R390

with

Hardware Version: REV1.0

Software Version: R390XXU0AWHG

FCC ID: ZCASMR390

Issued Date: 2023-9-27

Note:

The test results in this test report relate only to the devices specified in this report. This report shall not be reproduced except in full without the written approval of CTTL.

Test Laboratory:

CTTL-Telecommunication Technology Labs, CAICT

No. 52, Huayuan North Road, Haidian District, Beijing, P. R. China 100191. Tel:+86(0)10-62304633-2512, Fax:+86(0)10-62304633-2504 Email: <u>cttl_terminals@caict.ac.cn</u>, website: <u>www.caict.ac.cn</u>

REPORT HISTORY

Report Number	Revision	Issue Date	Description
I23Z70257-SEM02	Rev.0	2023-9-27	Initial creation of test report





TABLE OF CONTENT

1 TEST LABORATORY	5
1.1 INTRODUCTION & ACCREDITATION	5
1.2 TESTING LOCATION	5
1.3 TESTING ENVIRONMENT	
1.4 Project data	
1.5 Signature	
2 STATEMENT OF COMPLIANCE	6
3 CLIENT INFORMATION	7
3.1 Applicant Information	7
3.2 MANUFACTURER INFORMATION	7
4 EQUIPMENT UNDER TEST (EUT) AND ANCILLARY EQUIPMENT (AE)	8
4.1 About EUT	
4.2 INTERNAL IDENTIFICATION OF EUT USED DURING THE TEST	
4.3 INTERNAL IDENTIFICATION OF AE USED DURING THE TEST	
5 TEST METHODOLOGY	9
5.1 APPLICABLE LIMIT REGULATIONS	9
5.2 Applicable Measurement Standards	9
6 SPECIFIC ABSORPTION RATE (SAR)	10
6.1 INTRODUCTION	10
6.2 SAR DEFINITION	
7 TISSUE SIMULATING LIQUIDS	11
7.1 TARGETS FOR TISSUE SIMULATING LIQUID	
7.2 DIELECTRIC PERFORMANCE	
8 SYSTEM VERIFICATION	12
8.1 System Setup	
8.2 System Verification	
9 MEASUREMENT PROCEDURES	14
9.1 Tests to be performed	14
9.2 General Measurement Procedure	
9.3 BLUETOOTH MEASUREMENT PROCEDURES FOR SAR	
9.4 Power Drift	17
10 CONDUCTED OUTPUT POWER	17
11 TRANSMIT ANTENNA SEPARATION DISTANCES	17
12 SAR TEST RESULT	18
12.1 SAR results for BT	





13 SAR MEASUREMENT VARIABILITY	19
14 MEASUREMENT UNCERTAINTY	20
14.1 MEASUREMENT UNCERTAINTY FOR NORMAL SAR TESTS (300MHz~3GHz)	20
15 MAIN TEST INSTRUMENTS	21
ANNEX A GRAPH RESULTS	22
ANNEX B SYSTEM VERIFICATION RESULTS	23
ANNEX C SAR MEASUREMENT SETUP	24
ANNEX D POSITION OF THE WIRELESS DEVICE IN RELATION TO THE PHANTOM.	30
ANNEX E EQUIVALENT MEDIA RECIPES	32
ANNEX F SYSTEM VALIDATION	33
ANNEX G PROBE CALIBRATION CERTIFICATE	34
ANNEX H DIPOLE CALIBRATION CERTIFICATE	43
ANNEX I ACCREDITATION CERTIFICATE	49





1 Test Laboratory

1.1 Introduction & Accreditation

Telecommunication Technology Labs, CAICT is an ISO/IEC 17025:2017 accredited test laboratory under American Association for Laboratory Accreditation (A2LA) with lab code 7049.01, and is also an FCC accredited test laboratory (CN1349), and ISED accredited test laboratory (CAB identifier:CN0066). The detail accreditation scope can be found on A2LA website.

1.2 Testing Location

Location 1: CTTL(huayuan North Road)

Address:

No. 52, Huayuan North Road, Haidian District, Beijing, P. R. China 100191

1.3 Testing Environment


Normal Temperature:	15-35°C	
Extreme Temperature:	-10/+55°C	
Relative Humidity:	20-75%	

1.4 Project data

Testing Start Date:	2023-9-5
Testing End Date:	2023-9-26

1.5 Signature

Wang Tian (Prepared this test report)



Qi Dianyuan (Reviewed this test report)

Lu Bingsong Deputy Director of the laboratory (Approved this test report)





2 Statement of Compliance

The maximum results of Specific Absorption Rate (SAR) found during testing for SAMSUNG Electronics Co., Ltd. Wearable device SM-R390 are as follows:

Table 2.1: Highest Reported SAR						
Exposure	Technology	Highest Reported SAR	Limited	Equipment		
Configuration	Band	(W/kg)	(W/kg)	Class		
Limb-worn						
(Separation Distance	BT	0.09(10g)	4.0(10g)	DSS		
0mm)						

The SAR values found for the Smart Watch are below the maximum recommended levels of 1.6 W/kg as averaged over any 1g tissue according to the ANSI C95.1-1992.

The EUT battery must be fully charged and checked periodically during the test to ascertain uniform power output.

The measurement together with the test system set-up is described in annex C of this test report. A detailed description of the equipment under test can be found in chapter 4 of this test report. The highest reported SAR value is obtained at the case of **(Table 2.1)**, and the values are: **0.09** W/kg(10g) for limb-worn.





3 Client Information

3.1 Applicant Information

Company Name:	Samsung Electronics Co., Ltd.
Address/Post:	19 Chapin Rd., Building D Pine BrookNJ07058
Contact Person:	Jenni Chun
E-mail:	j1.chun@samsung.com
Telephone:	+1-201-937-4203
Fax:	

3.2 Manufacturer Information

Company Name:	Samsung Electronics Co., Ltd.
Address/Post:	Samsung R5, Maetan dong 129, Samsung ro
Address/Post.	Youngtong gu, Suwon city 443 742, Korea
Contact Person:	JP KIM
E-mail:	jp426.kim@samsung.com
Telephone:	+82-10-4376-0326
Fax:	





4 Equipment Under Test (EUT) and Ancillary Equipment (AE)

4.1 About EUT

Description:	Wearable device
Model name:	SM-R390
Operating mode(s):	BT
Tested Tx Frequency:	2402 – 2480 MHz (Bluetooth)
Test device Production information:	Production unit
Device type:	Portable device
Antenna type:	Integrated antenna

4.2 Internal Identification of EUT used during the test

EUT ID*	IMEI	HW Version	SW Version
EUT1	I23Z70257ut10a	REV1.0	R390XXU0AWHG
EUT2	I23Z70257ut24a	REV1.0	R390XXU0AWHG
EUT3	I23Z70257ut51a	REV1.0	R390XXU0AWHG

*EUT ID: is used to identify the test sample in the lab internally.

Note: It is performed to test SAR with the EUT1-3.

4.3 Internal Identification of AE used during the test

AE	Description	Model	SN	Manufacturer
ID*				
AE1	Battery	B319	١	Sunwoda
AE2	Battery	B319	\	ATL

*AE ID: is used to identify the test sample in the lab internally.





5 TEST METHODOLOGY

5.1 Applicable Limit Regulations

ANSI C95.1–1992:IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz.

It specifies the maximum exposure limit of **1.6 W/kg** as averaged over any 1 gram of tissue for portable devices being used within 20 cm of the user in the uncontrolled environment.

5.2 Applicable Measurement Standards

IEEE 1528–2013: Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques.

KDB447498 D01: General RF Exposure Guidance v06: Mobile and Portable Devices RF Exposure Procedures and Equipment Authorization Policies.

KDB648474 D04 Handset SAR v01r03: SAR Evaluation Considerations for Wireless Handsets.

KDB865664 D01SAR measurement 100 MHz to 6 GHz v01r04: SAR Measurement Requirements for 100 MHz to 6 GHz.

KDB865664 D02RF Exposure Reporting v01r02: RF Exposure Compliance Reporting and Documentation Considerations





6 Specific Absorption Rate (SAR)

6.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

6.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy ($_{dW}$) absorbed by (dissipated in) an incremental mass ($_{dm}$) contained in a volume element ($_{dv}$) of a given density ($_{\rho}$). The equation description is as below:

$$SAR = \frac{d}{dt}(\frac{dW}{dm}) = \frac{d}{dt}(\frac{dW}{\rho dv})$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$SAR = c(\frac{\delta T}{\delta t})$$

Where: C is the specific head capacity, δT is the temperature rise and δt is the exposure duration, or related to the electrical field in the tissue by

$$SAR = \frac{\sigma |E|^2}{\rho}$$

Where: σ is the conductivity of the tissue, ρ is the mass density of tissue and *E* is the RMS electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.





7 Tissue Simulating Liquids

7.1 Targets for tissue simulating liquid

Table 7.1: Targets for tissue simulating liquid


Frequency(MHz)	Liquid Type	Conductivity(o)	±10% Range	Permittivity(ε)	± 10% Range
2450	Head	1.80	1.62~1.98	39.2	35.28~43.12

7.2 Dielectric Performance

Table 7.2: Dielectric Performance of Tissue Simulating Liquid

Measurement Date (yyyy-mm-dd)	Туре	Frequency	Permittivity ٤	Drift (%)	Conductivity σ (S/m)	Drift (%)
2023-9-26	Head	2450MHz	39.83	1.61	1.832	1.78

Note: The liquid temperature is $22.0^{\rm o}{\rm C}$

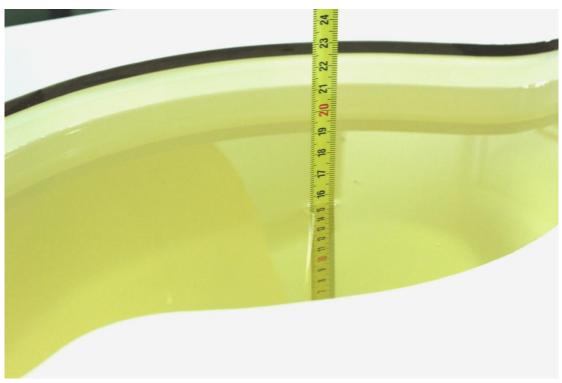

Picture 7 Liquid depth in the Flat Phantom






8 System verification

8.1 System Setup

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave that comes from a signal generator. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

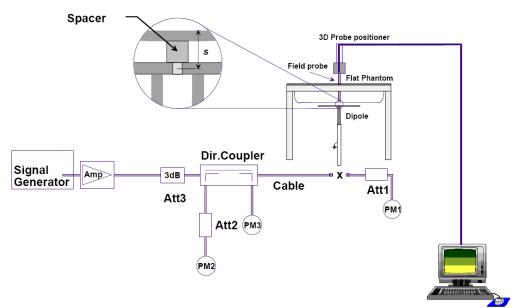

Picture 8.1 System Setup for System Evaluation



Picture 8.2 Photo of Dipole Setup





8.2 System Verification

SAR system verification is required to confirm measurement accuracy, according to the tissue dielectric media, probe calibration points and other system operating parameters required for measuring the SAR of a test device. The system verification must be performed for each frequency band and within the valid range of each probe calibration point required for testing the device.

The system verification results are required that the area scan estimated 1-g SAR is within 3% of the zoom scan 1-g SAR. The details are presented in annex B.

Measurement		Target value (W/kg)		Measured	value(W/kg)	Deviation		
Date	Frequency	10 g	1 g	10 g	1 g	10 g	1 g	
(yyyy-mm-dd)		Average	Average	Average	Average	Average	Average	
2023-9-26	2450 MHz	24.7	52.1	24.7	51.2	0.08%	-1.73%	

Table 8.1: System Verification of Head





9 Measurement Procedures

9.1 Tests to be performed

In order to determine the highest value of the peak spatial-average SAR of a handset, all device positions, configurations and operational modes shall be tested for each frequency band according to steps 1 to 3 below. A flowchart of the test process is shown in picture 9.1.

Step 1: The tests described in 9.2 shall be performed at the channel that is closest to the centre of

the transmit frequency band (f_c) for:

a) all device positions (cheek and tilt, for both left and right sides of the SAM phantom, as described in annex D),

b) all configurations for each device position in a), e.g., antenna extended and retracted, andc) all operational modes, e.g., analogue and digital, for each device position in a) and configuration in b) in each frequency band.

If more than three frequencies need to be tested according to 11.1 (i.e., $N_c > 3$), then all

frequencies, configurations and modes shall be tested for all of the above test conditions.


Step 2: For the condition providing highest peak spatial-average SAR determined in Step 1,perform all tests described in 9.2 at all other test frequencies, i.e., lowest and highest frequencies. In addition, for all other conditions (device position, configuration and operational mode) where the peak spatial-average SAR value determined in Step 1 is within3 dB of the applicable SAR limit, it is recommended that all other test frequencies shall be tested as well.

Step 3: Examine all data to determine the highest value of the peak spatial-average SAR found in Steps 1 to 2.



Preparation of system



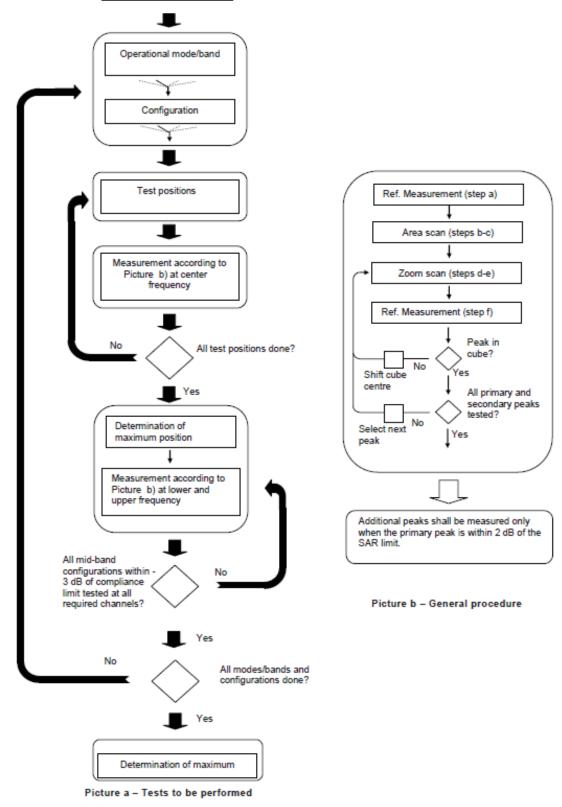

Picture 9.1Block diagram of the tests to be performed





9.2 General Measurement Procedure

The area and zoom scan resolutions specified in the table below must be applied to the SAR measurements and fully documented in SAR reports to qualify for TCB approval. Probe boundary effect error compensation is required for measurements with the probe tip closer than half a probe tip diameter to the phantom surface. Both the probe tip diameter and sensor offset distance must satisfy measurement protocols; to ensure probe boundary effect errors are minimized and the higher fields closest to the phantom surface can be correctly measured and extrapolated to the phantom surface for computing 1-g SAR. Tolerances of the post-processing algorithms must be verified by the test laboratory for the scan resolutions used in the SAR measurements, according to the reference distribution functions specified in IEEE Std 1528-2003. The results should be documented as part of the system validation records and may be requested to support test results when all the measurement parameters in the following table are not satisfied.

			\leq 3 GHz	> 3 GHz		
Maximum distance from (geometric center of pro		•	$5 \pm 1 \text{ mm}$	${\scriptstyle \frac{1}{2}\cdot\delta\cdot\ln(2)\pm0.5}~{\rm mm}$		
Maximum probe angle t normal at the measurem		xis to phantom surface	30°±1°	20°±1°		
			$\leq 2 \text{ GHz}$: $\leq 15 \text{ mm}$ 2 - 3 GHz: $\leq 12 \text{ mm}$	$\begin{array}{l} 3-4 \ GHz :\leq 12 \ mm \\ 4-6 \ GHz :\leq 10 \ mm \end{array}$		
Maximum area scan spa	itial resolutio	on: Δx _{Area} , Δy _{Area}	When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be \leq the corresponding x or y dimension of the test device with at least one measurement point on the test device.			
Maximum zoom scan spatial resolution: Δx_{Zoom} , Δy_{Zoom}			$\leq 2 \text{ GHz:} \leq 8 \text{ mm}$ 2 - 3 GHz: $\leq 5 \text{ mm}^*$	$3 - 4 \text{ GHz} \le 5 \text{ mm}^*$ $4 - 6 \text{ GHz} \le 4 \text{ mm}^*$		
	uniform grid: ∆z _{Zoom} (n)		≤ 5 mm	$\begin{array}{l} 3-4 \; \mathrm{GHz:} \leq 4 \; \mathrm{mm} \\ 4-5 \; \mathrm{GHz:} \leq 3 \; \mathrm{mm} \\ 5-6 \; \mathrm{GHz:} \leq 2 \; \mathrm{mm} \end{array}$		
Maximum zoom scan spatial resolution, normal to phantom surface	graded	$\Delta z_{Zoom}(1)$: between 1 st two points closest to phantom surface	≤ 4 mm	$3 - 4 \text{ GHz:} \le 3 \text{ mm}$ $4 - 5 \text{ GHz:} \le 2.5 \text{ mm}$ $5 - 6 \text{ GHz:} \le 2 \text{ mm}$		
Juliace	grid	∆z _{Zoom} (n>1): between subsequent points	$\leq 1.5 \cdot \Delta z_{Zoom}(n-1)$			
Minimum zoom scan volume	x, y, z	1	\geq 30 mm	$\begin{array}{l} 3-4 \ \mathrm{GHz:} \geq 28 \ \mathrm{mm} \\ 4-5 \ \mathrm{GHz:} \geq 25 \ \mathrm{mm} \\ 5-6 \ \mathrm{GHz:} \geq 22 \ \mathrm{mm} \end{array}$		
2011 for details. * When zoom scan is r	equired and	the <u>reported</u> SAR from th	ridence to the tissue medium; see te area scan based <i>1-g SAR estin</i> scan resolution may be applied,	ation procedures of KDB		

GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.





9.3 Bluetooth Measurement Procedures for SAR

Normal network operating configurations are not suitable for measuring the SAR of 802.11 transmitters in general. Unpredictable fluctuations in network traffic and antenna diversity conditions can introduce undesirable variations in SAR results. The SAR for these devices should be measured using chipset based test mode software to ensure that the results are consistent and reliable.

Chipset based test mode software is hardware dependent and generally varies among manufacturers. The device operating parameters established in a test mode for SAR measurements must be identical to those programmed in production units, including output power levels, amplifier gain settings and other RF performance tuning parameters. The test frequencies should correspond to actual channel frequencies defined for domestic use. SAR for devices with switched diversity should be measured with only one antenna transmitting at a time during each SAR measurement, according to a fixed modulation and data rate. The same data pattern should be used for all measurements.

9.4 Power Drift

To control the output power stability during the SAR test, DASY4 system calculates the power drift by measuring the E-field at the same location at the beginning and at the end of the measurement for each test position. These drift values can be found in section14 labeled as: (Power Drift [dB]). This ensures that the power drift during one measurement is within 5%.

10 Conducted Output Power

The maximum tune up of BT antenna is 9.93dBm The maximum output power of BT antenna is 10dBm.

11 Transmit Antenna Separation Distances

Please refer to the picture of antenna locations in the document: "The antenna locations of SAR test-I23Z70257"





12 SAR Test Result

B2= Battery 2 (ATL)

12.1 SAR results for BT

Test Position	Phantom position L/R/F	Frequency Band	Channel Number	Frequency (MHz)		EUT Measured Power (dBm)	Tune up (dBm)	Measured SAR 1g (W/kg)	Calculated SAR 1g (W/kg)	Measured SAR 10g (W/kg)	Calculated SAR 10g (W/kg)	Power Drift
Body	F	BT	78	2480	Rear Omm	9.7	10	0.086	0.09	0.04	0.04	0.11
Body	F	BT	39	2441	Rear Omm	9.82	10	0.092	0.10	0.042	0.04	-0.14
Body	F	BT	0	2402	Rear Omm	9.93	10	0.2	0.20	0.0928	0.09	-0.05
Body	F	BT	0	2402	Rear Omm B2	9.93	10	0.143	0.15	0.0702	0.07	0.03





13 SAR Measurement Variability

SAR measurement variability must be assessed for each frequency band, which is determined by the SAR probe calibration point and tissue-equivalent medium used for the device measurements. When both head and body tissue-equivalent media are required for SAR measurements in a frequency band, the variability measurement procedures should be applied to the tissue medium with the highest measured SAR, using the highest measured SAR configuration for that tissue-equivalent medium.

The following procedures are applied to determine if repeated measurements are required. 1) Repeated measurement is not required when the original highest measured SAR is < 0.80 W/kg; steps2) through 4) do not apply.

2) When the original highest measured SAR is \geq 0.80 W/kg, repeat that measurement once.

3) Perform a second repeated measurement only if the ratio of largest to smallest SAR for the original and first repeated measurements is > 1.20 or when the original or repeated measurement is \geq 1.45W/kg (~ 10% from the 1-g SAR limit).

4) Perform a third repeated measurement only if the original, first or second repeated measurement is \geq 1.5 W/kg and the ratio of largest to smallest SAR for the original, first and second repeated measurements is > 1.20.





14 Measurement Uncertainty

14.1 Measurement Uncertainty for Normal SAR Tests (300MHz~3GHz)

No.	Error Description	Туре	Uncertainty	Probably	Div.	(Ci)	(Ci)	Std.	Std.	Degree
110.	Life Description	турс	value	Distribution	DIV.	1g	10g	Unc.	Unc.	of
			value	Distribution		Ig	log	(1g)	(10g)	freedom
Measurement system										
1	Probe calibration	В	6.0	Ν	1	1	1	6.0	6.0	∞
2	Isotropy	B	4.7	R	$\sqrt{3}$	0.7	0.7	1.9	1.9	~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~
3	Boundary effect	B	1.0	R	$\sqrt{3}$	1	1	0.6	0.6	~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~
4	Linearity	B	4.7	R	$\sqrt{3}$	1	1	2.7	2.7	~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~
5	Detection limit	B	1.0	N	1	1	1	0.6	0.6	~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~
6	Readout electronics	B	0.3	R	$\sqrt{3}$	1	1	0.3	0.3	∞
7	Response time	B	0.8	R	$\sqrt{3}$	1	1	0.5	0.5	∞
8	Integration time	B	2.6	R	$\sqrt{3}$	1	1	1.5	1.5	∞
9	RF ambient conditions-noise	В	0	R	$\sqrt{3}$	1	1	0	0	œ
10	RFambient conditions-reflection	В	0	R	$\sqrt{3}$	1	1	0	0	~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~
11	Probe positioned mech. restrictions	В	0.4	R	$\sqrt{3}$	1	1	0.2	0.2	œ
12	Probe positioning with respect to phantom shell	В	2.9	R	$\sqrt{3}$	1	1	1.7	1.7	œ
13	Post-processing	В	1.0	R	$\sqrt{3}$	1	1	0.6	0.6	∞
			Test	sample related	ł				•	
14	Test sample positioning	А	3.3	Ν	1	1	1	3.3	3.3	71
15	Device holder uncertainty	А	3.4	Ν	1	1	1	3.4	3.4	5
16	Drift of output power	В	5.0	R	$\sqrt{3}$	1	1	2.9	2.9	∞
			Phan	tom and set-u	р					
17	Phantom uncertainty	В	4.0	R	$\sqrt{3}$	1	1	2.3	2.3	∞
18	Liquid conductivity (target)	В	5.0	R	$\sqrt{3}$	0.64	0.43	1.8	1.2	œ
19	Liquid conductivity (meas.)	А	2.06	N	1	0.64	0.43	1.32	0.89	43
20	Liquid permittivity (target)	В	5.0	R	$\sqrt{3}$	0.6	0.49	1.7	1.4	œ
21	Liquid permittivity (meas.)	А	1.6	N	1	0.6	0.49	1.0	0.8	521





Combined standard uncertainty	$u_{c}' = \sqrt{\sum_{i=1}^{21} c_{i}^{2} u_{i}^{2}}$			9.55	9.43	257
Expanded uncertainty (confidence interval of 95 %)	$u_e = 2u_c$			19.1	18.9	

15 MAIN TEST INSTRUMENTS

Table	15.1:	List of	of Main	Instruments
-------	-------	---------	---------	-------------

No.	Name	Туре	Serial Number	Calibration Date	Valid Period
01	Network analyzer	E5071C	MY46110673	January 10, 2023	One year
02	2 Power sensor NRP11		101139	January 13, 2023	One year
03	Power sensor	NRP110T	101159	January 13, 2023	One year
04	Signal Generator	E4438C	MY49071430	January 19, 2023	One year
05	Amplifier	60S1G4	0331848	No Calibration	Requested
06	BTS	CMW500	159890	January 12, 2023	One year
08	E-field Probe	SPEAG EX3DV4	7673	July 24, 2023	One year
10	DAE SPEAG DAE4		549	January 24, 2023	One year
16	Dipole Validation Kit	SPEAG D2450V2	853	July 11,2023	One year

END OF REPORT BODY





ANNEX A Graph Results

BT_ Rear 0mm

Date/Time: 9/26/2023

Electronics: DAE4 Sn549

Medium: H700-6000M

Medium parameters used (interpolated): f = 2402 MHz; σ = 1.83 S/m; ϵ_r = 39.813; ρ = 1000 kg/m³

Ambient Temperature: 23.3°C Liquid Temperature: 22.5°C

Communication System: UID 0, Bluetooth (0) Frequency: 2402 MHz Duty Cycle: 1:1

Probe: EX3DV4 - SN7673 ConvF(7.65, 7.65, 7.65)

Area Scan (81x81x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 0.412 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 10.41 V/m; Power Drift = -0.05 dB Peak SAR (extrapolated) = 0.527 W/kg SAR(1 g) = 0.200 W/kg; SAR(10 g) = 0.0928 W/kg Maximum value of SAR (measured) = 0.204 W/kg

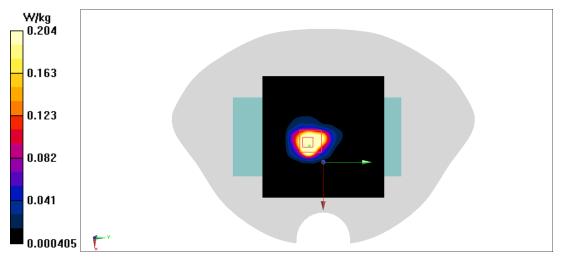


Fig A.1






ANNEX B System Verification Results

2450 MHz

Date:9/26/2023 Electronics: DAE4 Sn549 Medium: H700-6000M Medium parameters used: f = 2450 MHz; $\sigma = 1.832$ S/m; $\epsilon r = 39.83$; $\rho = 1000$ kg/m3 Ambient Temperature:23.3°C Liquid Temperature: 22.5°C Communication System: CW (0) Frequency: 2450 MHz Duty Cycle: 1:1 Probe: EX3DV4 - SN7673 ConvF(7.65, 7.65, 7.65)

Area Scan (61x61x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm Maximum value of SAR (interpolated) = 21.2 W/kg

Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 96.71 V/m; Power Drift = 0.15 dB Peak SAR (extrapolated) = 27.6 W/kg SAR(1 g) = 12.8 W/kg; SAR(10 g) = 6.18 W/kg Maximum value of SAR (measured) = 21.5 W/kg

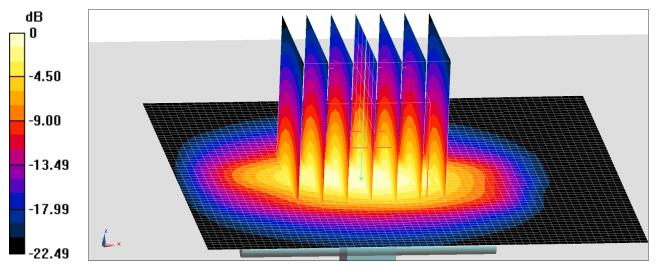

0 dB = 21.5 W/kg = 13.32 dBW/kg

Fig.B.1 validation 2450 MHz






ANNEX C SAR Measurement Setup

C.1 Measurement Set-up

The Dasy5 or DASY6 system for performing compliance tests is illustrated above graphically. This system consists of the following items:

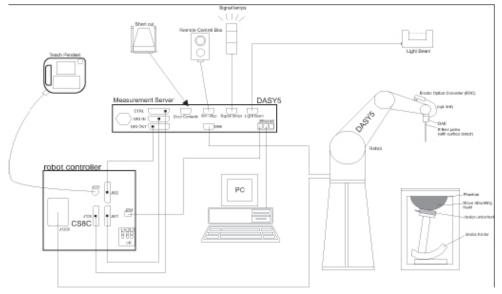

Picture C.1SAR Lab Test Measurement Set-up

- A standard high precision 6-axis robot (StäubliTX=RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- An isotropic field probe optimized and calibrated for the targeted measurement.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- A computer running WinXP and the DASY5 or DASY6 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as
- warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.





C.2 Dasy5 E-field Probe System

The SAR measurements were conducted with the dosimetric probe designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multifiber line ending at the front of the probe tip. It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY5 or DASY6 software reads the reflection durning a software approach and looks for the maximum using 2nd ord curve fitting. The approach is stopped at reaching the maximum.

Probe Specifications:

Model:	ES3DV3, EX3DV4						
Frequency	10MHz — 6.0GHz(EX3DV4)						
Range:	10MHz — 4GHz(ES3DV3)						
Calibration:	In head and body simulating tissue at						
	Frequencies from 835 up to 5800MHz						
Linearity:	± 0.2 dB(30 MHz to 6 GHz) for EX3DV4						
± 0.2 dB(30 MHz to 4 GHz) for ES3DV3							
DynamicRange: 10 mW/kg — 100W/kg							
Probe Length:	330 mm						
Probe Tip							
Length:	20 mm						
Body Diameter:	12 mm						
Tip Diameter:	2.5 mm (3.9 mm for ES3DV3)						
Tip-Center:	1 mm (2.0mm for ES3DV3)						
Application:SAF	R Dosimetry Testing						
	Compliance tests of mobile phones						
	Dosimetry in strong gradient fields						
	d Dealar						



Picture C.2Near-field Probe



Picture C.3E-field Probe

C.3 E-field Probe Calibration

Each E-Probe/Probe Amplifier combination has unique calibration parameters. A TEM cell calibration procedure is conducted to determine the proper amplifier settings to enter in the probe parameters. The amplifier settings are determined for a given frequency by subjecting the probe to a known E-field density (1 mW/cm²) using an RF Signal generator, TEM cell, and RF Power Meter.

The free space E-field from amplified probe outputs is determined in a test chamber. This calibration can be performed in a TEM cell if the frequency is below 1 GHz and inn a waveguide or





other methodologies above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees until the three channels show the maximum reading. The power density readings equates to 1 mW/cm².

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The E-field in the medium correlates with the temperature rise in the dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$SAR = C \frac{\Delta T}{\Delta t}$$

Where:

 Δt = Exposure time (30 seconds), C = Heat capacity of tissue (brain or muscle), ΔT = Temperature increase due to RF exposure.

$$SAR = \frac{\left|E\right|^2 \cdot \sigma}{\rho}$$

Where:

 σ = Simulated tissue conductivity,

 ρ = Tissue density (kg/m³).

C.4 Other Test Equipment

C.4.1 Data Acquisition Electronics(DAE)

The data acquisition electronics consist of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder with a control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information, as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE is 200 MOhm; the inputs are symmetrical and floating. Common mode rejection is above 80 dB.



PictureC.4: DAE





C.4.2 Robot

The SPEAG DASY system uses the high precision robots (DASY5: RX160L) type from Stäubli SA (France). For the 6-axis controller system, the robot controller version from Stäubli is used. The Stäubli robot series have many features that are important for our application:

- High precision (repeatability 0.02mm)
- High reliability (industrial design)
- > Low maintenance costs (virtually maintenance free due to direct drive gears; no belt drives)
- Jerk-free straight movements (brushless synchron motors; no stepper motors)
- Low ELF interference (motor control fields shielded via the closed metallic construction shields)



Picture C.5 DASY 5

C.4.3 Measurement Server

The Measurement server is based on a PC/104 CPU broad with CPU (DASY5: 400 MHz, Intel Celeron), chipdisk (DASY5: 128MB), RAM DASY5: 128MB). The necessary circuits for communication with the DAE electronic box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY I/O broad, which is directly connected to the PC/104 bus of the CPU broad.

The measurement server performs all real-time data evaluation of field measurements and surface detection, controls robot movements and handles safety operation. The PC operating system cannot interfere with these time critical processes. All connections are supervised by a watchdog, and disconnection of any of the cables to the measurement server will automatically disarm the robot and disable all program-controlled robot movements. Furthermore, the measurement server is equipped with an expansion port which is reserved for future applications. Please note that this expansion port does not have a standardized pinout, and therefore only devices provided by SPEAG can be connected. Devices from any other supplier could seriously damage the measurement server.



Picture C.6 Server for DASY 5





C.4.4 Device Holder for Phantom


The SAR in the phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source at 5mm distance, a positioning uncertainty of ± 0.5 mm would produce a SAR uncertainty of $\pm 20\%$. Accurate device positioning is therefore crucial for accurate and repeatable measurements. The positions in which the devices must be measured are defined by the standards.

The DASY device holder is designed to cope with the different positions given in the standard. It has two scales for device rotation (with respect to the body axis) and device inclination (with respect to the line between the ear reference points). The rotation centers for both scales are the ear reference point (ERP). Thus the device needs no repositioning when changing the angles. The DASY device holder is constructed of low-loss POM material having the following dielectric parameters: relative permittivity $\ell = 3$ and loss tangent $\delta = 0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.

<Laptop Extension Kit>

The extension is lightweight and made of POM, acrylic glass and foam. It fits easily on the upper part of the Mounting Device in place of the phone positioner. The extension is fully compatible with the Twin-SAM and ELI phantoms.





Picture C7-1: Device Holder

Picture C.7-2: Laptop Extension Kit

C.4.5 Phantom

The SAM Twin Phantom V4.0 is constructed of a fiberglass shell integrated in a table. The shape of the shell is based on data from an anatomical study designed to

Represent the 90th percentile of the population. The phantom enables the dissymmetric evaluation of SAR for both left and right handed handset usage, as well as body-worn usage using the flat phantom region. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. The shell phantom has a 2mm shell thickness (except the ear region where shell thickness increases to 6 mm).

Shell Thickness:	2±0. 2 mm
Filling Volume:	Approx. 25 liters
Dimensions:	810 x 1000 x 500 mm (H x L x W)
Available:	Special

©Copyright. All rights reserved by CTTL.







Picture C.8: SAM Twin Phantom






ANNEX D Position of the wireless device in relation to the phantom

D.1 Limb-worn device

A limb-worn device is a unit whose intended use includes being strapped to the arm or leg of the user while transmitting (except in idle mode). It is similar to a body-worn device. Therefore, the test positions of 6.1.4.4 also apply. The strap shall be opened so that it is divided into two parts as shown in Figure 10. The device shall be positioned directly against the phantom surface with the strap straightened as much as possible and the back of the device towards the phantom.


If the strap cannot normally be opened to allow placing in direct contact with the phantom surface, it may be necessary to break the strap of the device but ensuring to not damage the antenna.

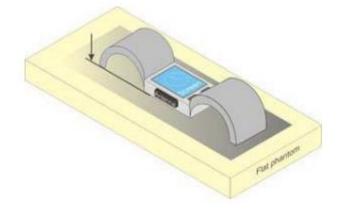

Picture D.1 Test position for limb-worn devices

D.2 Front-of-face device

A typical example of a front-of-face device is a two-way radio that is held at a distance from the face of the user when transmitting. In these cases the device under test shall be positioned at the distance to the phantom surface that corresponds to the intended use as specified by the manufacturer in the user instructions (Figure 9a). If the intended use is not specified, a separation distance of 25 mm⁵ between the phantom surface and the device shall be used.

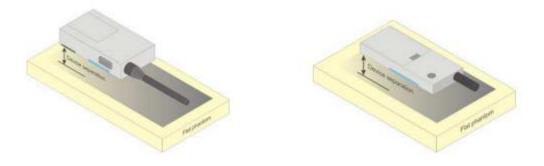


Picture D.2 Test position for front-of-face devices





D.3 DUT Setup Photos

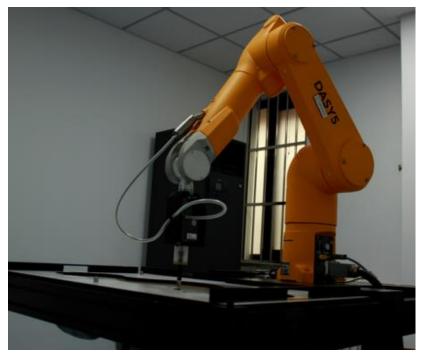

Picture D.3





ANNEX E Equivalent Media Recipes

The liquid used for the frequency range of 800-3000 MHz consisted of water, sugar, salt, preventol, glycol monobutyl and Cellulose. The liquid has been previously proven to be suited for worst-case. The Table E.1 shows the detail solution. It's satisfying the latest tissue dielectric parameters requirements proposed by the IEEE 1528 and IEC 62209.

Frequency	835Head	025Dody	1900	1900	2450	2450	5800	5800		
(MHz)	osoneau	835Body	Head	Body	Head	Body	Head	Body		
Ingredients (% by	Ingredients (% by weight)									
Water	41.45	52.5	55.242	69.91	58.79	72.60	65.53	65.53		
Sugar	56.0	45.0	١	١	١	١	١	١		
Salt	1.45	1.4	0.306	0.13	0.06	0.18	١	\		
Preventol	0.1	0.1	١	١	١	١	١	١		
Cellulose	1.0	1.0	١	١	١	١	١	١		
Glycol	1	N	44.452	29.96	41.15	27.22	N	١		
Monobutyl	١	١	44.432	29.90	41.15	21.22	١	١		
Diethylenglycol	1	N	N	1	1	1	17.24	17.24		
monohexylether	۸	١	١	λ	λ	١	17.24	17.24		
Triton X-100	١	١	١	١	١	١	17.24	17.24		
Dielectric	ε=41.5	ε=55.2	ε=40.0	ε=53.3	ε=39.2	ε=52.7	ε=35.3	ε=48.2		
Parameters										
Target Value	σ=0.90	σ=0.97	σ=1.40	σ=1.52	σ=1.80	σ=1.95	σ=5.27	σ=6.00		

TableE.1: Composition of the Tissue Equivalent Matter

Note: There are a little adjustment respectively for 750, 1750, 2600, 5200, 5300 and 5600 based on the recipe of closest frequency in table E.1.





ANNEX F System Validation

The SAR system must be validated against its performance specifications before it is deployed. When SAR probes, system components or software are changed, upgraded or recalibrated, these must be validated with the SAR system(s) that operates with such components.

Probe SN.	Liquid name	Validation date	Frequency point	Status (OK or Not)					
7673	Head 750MHz	July.27,2023	750 MHz	OK					
7673	Head 900MHz	July.27,2023	900 MHz	OK					
7673	Head 1750MHz	July.27,2023	1750 MHz	OK					
7673	Head 1900MHz	July.27,2023	1900 MHz	OK					
7673	Head 2000MHz	July.27,2023	2000 MHz	OK					
7673	Head 2300MHz	July.27,2023	2300 MHz	OK					
7673	Head 2450MHz	July.27,2023	2450 MHz	OK					
7673	Head 2600MHz	July.27,2023	2600 MHz	OK					
7673	Head 3300MHz	July.27,2023	3300 MHz	OK					
7673	Head 3500MHz	July.27,2023	3500 MHz	OK					
7673	Head 3700MHz	July.27,2023	3700 MHz	OK					
7673	Head 3900MHz	July.27,2023	3900 MHz	OK					
7673	Head 4100MHz	July.27,2023	4100 MHz	OK					
7673	Head 4200MHz	July.27,2023	4200 MHz	OK					
7673	Head 4400MHz	July.27,2023	4400 MHz	OK					
7673	Head 4600MHz	July.27,2023	4600 MHz	OK					
7673	Head 4800MHz	July.27,2023	4800 MHz	OK					
7673	Head 4950MHz	July.27,2023	4950 MHz	OK					
7673	Head 5250MHz	July.27,2023	5250 MHz	OK					
7673	Head 5600MHz	July.27,2023	5600 MHz	OK					
7673	Head 5750MHz	July.27,2023	5750 MHz	OK					

Table F.1: System Validation for 7673





ANNEX G Probe Calibration Certificate

Probe 7673 Calibration Certificate


July 24, 20 ments the traceability to	Certificate SN : 7673 4-02 Procedures for Dosimetric E-field I	ysical units of me	
EX3DV4 - FF-Z11-00 Calibration July 24, 20 ments the traceability to	4-02 Procedures for Dosimetric E-field 23 national standards, which realize the physical	ysical units of me	asurements(SI). The
EX3DV4 - FF-Z11-00 Calibration July 24, 20 ments the traceability to	4-02 Procedures for Dosimetric E-field 23 national standards, which realize the physical	ysical units of me	asurements(SI). The
FF-Z11-00 Calibration July 24, 20 ments the traceability to	4-02 Procedures for Dosimetric E-field 23 national standards, which realize the physical	ysical units of me	asurements(SI). The
FF-Z11-00 Calibration July 24, 20 ments the traceability to	4-02 Procedures for Dosimetric E-field 23 national standards, which realize the physical	ysical units of me	asurements(SI). The
Calibration July 24, 20 ments the traceability to	Procedures for Dosimetric E-field I 23 national standards, which realize the phy	ysical units of me	asurements(SI). The
Calibration July 24, 20 ments the traceability to	Procedures for Dosimetric E-field I 23 national standards, which realize the phy	ysical units of me	asurements(SI). The
July 24, 20 ments the traceability to	23 national standards, which realize the phy	ysical units of me	asurements(SI). The
ments the traceability to	national standards, which realize the phy		asurements(SI). The
			asurements(SI). The
indeo with confidence pr	submity are given on the following page		
ucted in the closed labo	ratory facility: environment temperature(2	2±3)℃ and humidi	ty<70%.
&TE critical for calibratio	n)		
ID # Ca	I Date(Calibrated by, Certificate No.) S	Scheduled Calibra	ation
101919	12-Jun-23(CTTL, No.J23X05435)		Jun-24
101547	12-Jun-23(CTTL, No.J23X05435)		Jun-24
101548	12-Jun-23(CTTL, No.J23X05435)		Jun-24
18N50W-10dB	19-Jan-23(CTTL, No.J23X00212)		Jan-25
18N50W-20dB	19-Jan-23(CTTL, No.J23X00211)		Jan-25
SN 3846	31-May-23(SPEAG, No.EX-3846_Ma	iy23)	May-24
SN 7517	27-Jan-23(SPEAG, No.EX-7517_Jan	23)	Jan-24
SN 1555	25-Aug-22(SPEAG, No.DAE4-1555_	Aug22)	Aug-23
ID #	Cal Date(Calibrated by, Certificate No	o.) Sched	uled Calibration
6201052605	12-Jun-23(CTTL, No.J23X05434)		Jun-24
MY46110673	10-Jan-23(CTTL, No.J23X00104)		Jan-24
BT0520	11-May-23(CTTL, No.J23X04061)		May-25
BT0267	11-May-23(CTTL, No.J23X04062)		May-25
	18-Jan-23(SPEAG, No.OCP-DAK3.5	-1040_Jan23)	Jan-24
SN 1040			
SN 1040	Function	Signature	The second s
SN 1040	Function SAR Test Engineer	Signature	X
SN 1040 Name		Signature	R
SN 1040 Name		Signature	N 下
SN 1040 Name Yu Zongying Lin Hao	SAR Test Engineer	Signature	A 国 山
SN 1040 Name Yu Zongying	SAR Test Engineer	Signature	大 市 市 上
	BTE critical for calibratio ID # Calibratio 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 3846 SN 7517 SN 1555 ID # 6201052605 MY46110673 SN 24010673	BTE critical for calibration) Cal Date(Calibrated by, Certificate No.) Second	ID # Cal Date(Calibrated by, Certificate No.) Scheduled Calibra 101919 12-Jun-23(CTTL, No.J23X05435) 101547 101547 12-Jun-23(CTTL, No.J23X05435) 101548 101548 12-Jun-23(CTTL, No.J23X05435) 18N50W-10dB 18N50W-10dB 19-Jan-23(CTTL, No.J23X00212) 18N50W-20dB 18N50W-20dB 19-Jan-23(CTTL, No.J23X00211) SN 3846 SN 7517 27-Jan-23(SPEAG, No.EX-3846_May23) SN 1555 SN 1555 25-Aug-22(SPEAG, No.DAE4-1555_Aug22) ID # ID # Cal Date(Calibrated by, Certificate No.) Sched 6201052605 12-Jun-23(CTTL, No.J23X005434) MY46110673 10-Jan-23(CTTL, No.J23X00104)

Certificate No: J23Z60316

Page 1 of 9







CAICT

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.cn

Glossary:

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A,B,C,D	modulation dependent linearization parameters
Polarization Φ	Φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i
	$\theta=0$ is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010

d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORMx, y, z: Assessed for E-field polarization θ=0 (f≤900MHz in TEM-cell; f>1800MHz: waveguide). NORMx, y, z are only intermediate values, i.e., the uncertainties of NORMx, y, z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x, y, z = NORMx, y, z* frequency_response (see Frequency Response Chart). This
 linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the
 frequency response is included in the stated uncertainty of ConvF.
- DCPx, y, z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- *Ax,y,z; Bx,y,z; Cx,y,z; VRx,y,z*:A,B,C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f≤800MHz) and inside waveguide using analytical field distributions based on power measurements for f >800MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from±50MHz to±100MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the
 probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No:Z22-60207

Page 2 of 9









Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.cn

DASY/EASY – Parameters of Probe: EX3DV4 – SN:7673

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm(µV/(V/m) ²) ^A	0.62	0.63	0.61	±10.0%
DCP(mV) ^B	110.3	111.1	110.2	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dBõV	С	D dB	VR mV	Unc ^E (<i>k</i> =2)
0 CW	X	0.0	0.0	1.0	0.00	198.1	±2.1%	
		Y	0.0	0.0	1.0		199.1	
	Z	0.0	0.0	1.0		193.0		

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X, Y, Z do not affect the E²-field uncertainty inside TSL (see Page 4).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainly is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No:Z22-60207

Page 3 of 9









DASY/EASY – Parameters of Probe: EX3DV4 – SN:7673

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (<i>k</i> =2)
750	41.9	0.89	10.34	10.34	10.34	0.14	1.40	±12.1%
900	41.5	0.97	9.95	9.95	9.95	0.17	1.30	±12.1%
1750	40.1	1.37	8.49	8.49	8.49	0.26	0.98	±12.1%
1900	40.0	1.40	8.07	8.07	8.07	0.24	1.07	±12.1%
2000	40.0	1.40	8.08	8.08	8.08	0.20	1.31	±12.1%
2300	39.5	1.67	7.86	7.86	7.86	0.62	0.66	±12.1%
2450	39.2	1.80	7.57	7.57	7.57	0.60	0.68	±12.1%
2600	39.0	1.96	7.31	7.31	7.31	0.65	0.65	±12.1%
3300	38.2	2.71	6.93	6.93	6.93	0.36	0.99	±13.3%
3500	37.9	2.91	6.73	6.73	6.73	0.40	0.94	±13.3%
3700	37.7	3.12	6.50	6.50	6.50	0.30	1.20	±13.3%
3900	37.5	3.32	6.44	6.44	6.44	0.30	1.50	±13.3%
4100	37.2	3.53	6.46	6.46	6.46	0.30	1.40	±13.3%
4200	37.1	3.63	6.35	6.35	6.35	0.35	1.35	±13.3%
4400	36.9	3.84	6.26	6.26	6.26	0.30	1.50	±13.3%
4600	36.7	4.04	6.10	6.10	6.10	0.35	1.50	±13.3%
4800	36.4	4.25	5.99	5.99	5.99	0.35	1.60	±13.3%
4950	36.3	4.40	5.65	5.65	5.65	0.35	1.65	±13.3%
5250	35.9	4.71	5.21	5.21	5.21	0.40	1.42	±13.3%
5600	35.5	5.07	4.71	4.71	4.71	0.40	1.50	±13.3%
5750	35.4	5.22	4.70	4.70	4.70	0.40	1.50	±13.3%

^c Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters. ^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No:Z22-60207

Page 4 of 9










Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

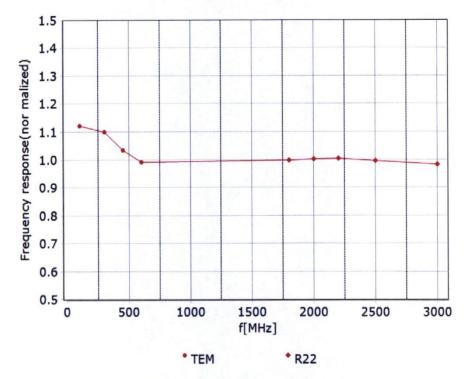

Uncertainty of Frequency Response of E-field: ±7.4% (k=2)














Receiving Pattern (Φ), θ=0°

f=600 MHz, TEM

f=1800 MHz, R22





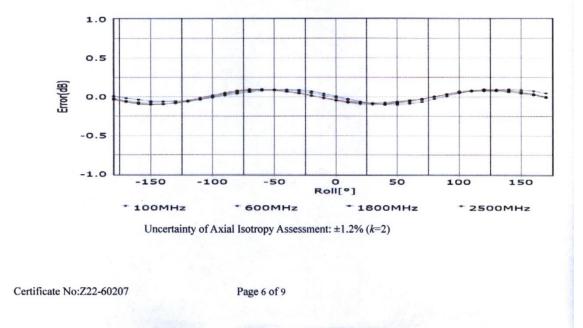






CAICT



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.cn

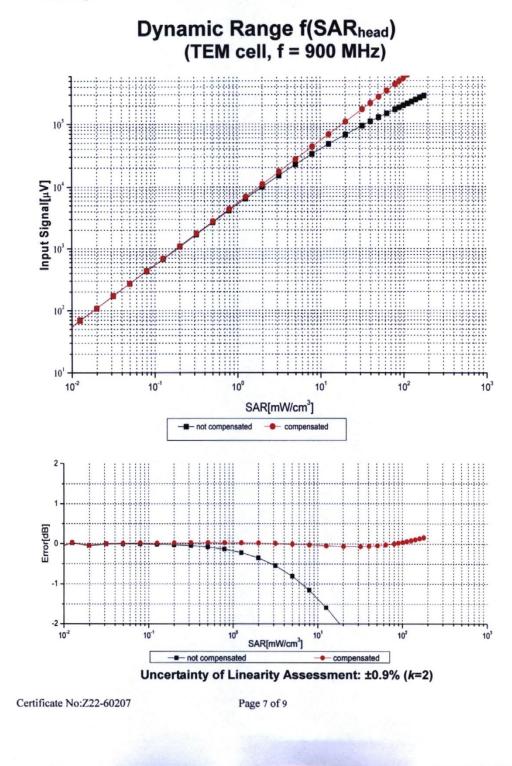











Conversion Factor Assessment

f=750 MHz,WGLS R9(H_convF)

f=1750 MHz,WGLS R22(H_convF)

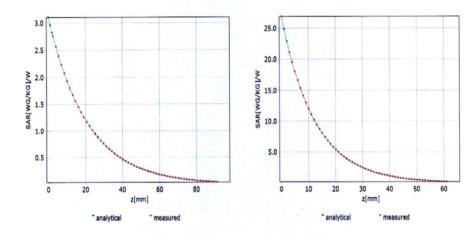

Deviation from Isotropy in Liquid

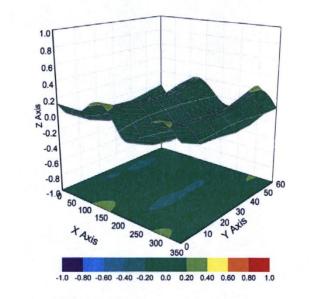

Uncertainty of Spherical Isotropy Assessment: ±3.2% (k=2)

Certificate No:Z22-60207

Page 8 of 9









DASY/EASY – Parameters of Probe: EX3DV4 – SN:7673

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	145.7
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	9mm
Tip Diameter	2.5mm
Probe Tip to Sensor X Calibration Point	1mm
Probe Tip to Sensor Y Calibration Point	1mm
Probe Tip to Sensor Z Calibration Point	1mm
Recommended Measurement Distance from Surface	1.4mm

Certificate No:Z22-60207

Page 9 of 9





ANNEX H Dipole Calibration Certificate

2450 MHz Dipole Calibration Certificate

Engineering AG Zeughausstrasse 43, 8004 Zurich Accredited by the Swiss Accreditat			S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
The Swiss Accreditation Service Multilateral Agreement for the re	is one of the signatori		Accreditation No.: SCS 0108
Client CTTL Beijing		Certificate No	D2450V2-853_Jul23
CALIBRATION C	ERTIFICAT	3	
Object	D2450V2 - SN:8	53	
Calibration procedure(s)	QA CAL-05.v12 Calibration Proce	edure for SAR Validation Source	es between 0.7-3 GHz
Calibration date:	July 11, 2023		
The measurements and the uncert	ainties with confidence p	onal standards, which realize the physical u robability are given on the following pages a ry facility: environment temperature (22 ± 3)	and are part of the certificate.
The measurements and the uncert	ainties with confidence p ad in the closed laborator	robability are given on the following pages a	and are part of the certificate.
The measurements and the uncert All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards	ainties with confidence p ad in the closed laborator	robability are given on the following pages a	and are part of the certificate.
The measurements and the uncert All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Power meter NRP2	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778	robability are given on the following pages a ry facility: environment temperature (22 ± 3)	nd are part of the certificate. °C and humidity < 70%.
The measurements and the uncert All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804)	nd are part of the certificate. °C and humidity < 70%. Scheduled Calibration
The measurements and the uncert All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245	robability are given on the following pages a ry facility: environment temperature (22 ± 3) <u>Cal Date (Certificate No.)</u> 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805)	nd are part of the certificate. °C and humidity < 70%. <u>Scheduled Calibration</u> Mar-24 Mar-24 Mar-24 Mar-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k)	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805)	nd are part of the certificate. °C and humidity < 70%. <u>Scheduled Calibration</u> Mar-24 Mar-24 Mar-24 Mar-24 Mar-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: BH9394 (20k) SN: 310982 / 06327	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810)	nd are part of the certificate. °C and humidity < 70%. <u>Scheduled Calibration</u> Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Mar-24
The measurements and the uncert All calibrations have been conducts Calibration Equipment used (M&TE Primary Standards Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k)	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805)	nd are part of the certificate. °C and humidity < 70%. <u>Scheduled Calibration</u> Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24
The measurements and the uncert All calibrations have been conducts Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22)	rC and humidity < 70%. *C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23
The measurements and the uncert All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8H9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID #	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house)	rC and humidity < 70%. *C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 Scheduled Check
The measurements and the uncert All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 8H9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22)	nd are part of the certificate. "C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24
The measurements and the uncert All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8H9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID #	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22)	nd are part of the certificate. "C and humidity < 70%. <u>Scheduled Calibration</u> Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 <u>Scheduled Check</u> In house check: Oct-24 In house check: Oct-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22)	nd are part of the certificate. "C and humidity < 70%. <u>Scheduled Calibration</u> Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Dec-23 <u>Scheduled Check</u> In house check: Oct-24 In house check: Oct-24 In house check: Oct-24 In house check: Oct-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: MY41093315	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22)	nd are part of the certificate. "C and humidity < 70%. <u>Scheduled Calibration</u> Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 <u>Scheduled Check</u> In house check: Oct-24 In house check: Oct-24
The measurements and the uncert All calibrations have been conducts Calibration Equipment used (M&TE Primary Standards Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer Agilent E8358A	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 013245 SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: WY41093315 SN: WY41093315 SN: US41080477 Name	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house check Oct-22) 07-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22)	nd are part of the certificate. *C and humidity < 70%. *C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 013245 SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: MY41093315 SN: 100972 SN: US41080477	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22)	nd are part of the certificate. "C and humidity < 70%. <u>Scheduled Calibration</u> Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Jan-24 Dec-23 <u>Scheduled Check</u> In house check: Oct-24 In house check: Oct-24
The measurements and the uncert All calibrations have been conducts Calibration Equipment used (M&TE Primary Standards Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer Agilent E8358A	ainties with confidence p ad in the closed laborator critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 013245 SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: WY41093315 SN: WY41093315 SN: US41080477 Name	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22)	nd are part of the certificate. "C and humidity < 70%. <u>Scheduled Calibration</u> Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Jan-24 Dec-23 <u>Scheduled Check</u> In house check: Oct-24 In house check: Oct-24





Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-853_Jul23

Page 2 of 6





Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.8 ± 6 %	1.85 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.3 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.1 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured	condition 250 mW input power	6.25 W/kg

Certificate No: D2450V2-853_Jul23

Page 3 of 6





Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.3 Ω + 4.2 jΩ	٦
Return Loss	- 24.8 dB	-

General Antenna Parameters and Design

Electrical Delay (one direction)	1.164 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	ODEAC
indicated by	SPEAG

Certificate No: D2450V2-853_Jul23

Page 4 of 6





DASY5 Validation Report for Head TSL

Date: 11.07.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:853


Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz; σ = 1.85 S/m; ϵ _r = 37.8; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(7.9, 7.9, 7.9) @ 2450 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 19.12.2022
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 115.1 V/m; Power Drift = 0.00 dB Peak SAR (extrapolated) = 25.8 W/kg SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.25 W/kg Smallest distance from peaks to all points 3 dB below = 9 mm Ratio of SAR at M2 to SAR at M1 = 51.7% Maximum value of SAR (measured) = 21.6 W/kg

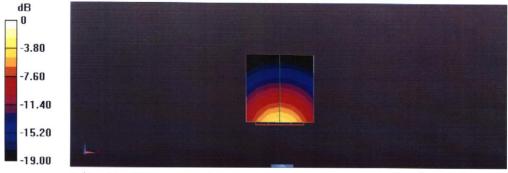

0 dB = 21.6 W/kg = 13.35 dBW/kg


Certificate No: D2450V2-853_Jul23

Page 5 of 6





Impedance Measurement Plot for Head TSL

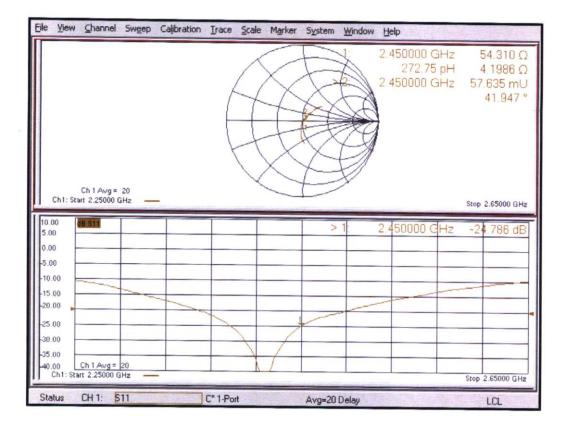

Certificate No: D2450V2-853_Jul23

Page 6 of 6





ANNEX I Accreditation Certificate





Accredited Laboratory

A2LA has accredited

TELECOMMUNICATION TECHNOLOGY LABS, CAICT

Beijing, People's Republic of China

for technical competence in the field of

Electrical Testing

This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017 General requirements for the competence of testing and calibration laboratories. This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).



Presented this 26th day of June 2023.

Mr. Trace McInturff, Vice President, Accreditation Services For the Accreditation Council Certificate Number 7049.01 Valid to July 31, 2024

For the tests to which this accreditation applies, please refer to the laboratory's Electrical Scope of Accreditation.